



US010405799B2

(12) **United States Patent**
Kumar et al.

(10) **Patent No.:** **US 10,405,799 B2**
(45) **Date of Patent:** **Sep. 10, 2019**

(54) **DEVICE FEATURES AND DESIGN**
ELEMENTS FOR LONG-TERM ADHESION

(71) Applicant: **iRhythm Technologies, Inc.**, San Francisco, CA (US)
(72) Inventors: **Uday N. Kumar**, San Francisco, CA (US); **Peter H. Livingston**, San Francisco, CA (US); **Mark J. Day**, San Francisco, CA (US); **Shena Hae Park**, San Francisco, CA (US); **William F. Willis**, San Francisco, CA (US); **William H. Righter**, San Francisco, CA (US)

(73) Assignee: **iRhythm Technologies, Inc.**, San Francisco, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 699 days.

(21) Appl. No.: **15/005,854**

(22) Filed: **Jan. 25, 2016**

(65) **Prior Publication Data**
US 2016/0135746 A1 May 19, 2016

Related U.S. Application Data

(63) Continuation of application No. 13/890,144, filed on May 8, 2013, now Pat. No. 9,241,649, which is a (Continued)

(51) **Int. Cl.**
A61B 5/0408 (2006.01)
A61B 5/04 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/6832** (2013.01); **A61B 5/0408** (2013.01); **A61B 5/0478** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC **A61B 5/04087**; **A61B 5/6832**; **A61B 5/6833**; **A61B 2560/0412**; **A61B 2560/0468**; **A61N 1/0492**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,497,079 A 6/1924 Gullborg
2,179,922 A 11/1939 Dana
(Continued)

FOREIGN PATENT DOCUMENTS

AU 2011252998 8/2015
AU 2014209376 6/2017
(Continued)

OTHER PUBLICATIONS


US 8,750,980 B2, 06/2014, Katra et al. (withdrawn)
(Continued)

Primary Examiner — Lee S Cohen
Assistant Examiner — Erin M Cardinal

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

(57) **ABSTRACT**

An electronic device for long-term adhesion to a mammal includes a housing with an electronic component. The electronic device may include a first wing and a second wing, each being integrally formed with the housing. An electrode is positioned on a bottom surface of each of the wings, the electrodes electrically connected to the electronic component. An adhesive layer is provided for adhesion to a surface of the mammal. The adhesive layer may cover a portion of the bottom surfaces of the wings but generally does not cover the electrode or a bottom surface of the housing. A method of applying an electronic device to a mammal includes removing first and second adhesive covers from first and second wings of the electronic device to (Continued)

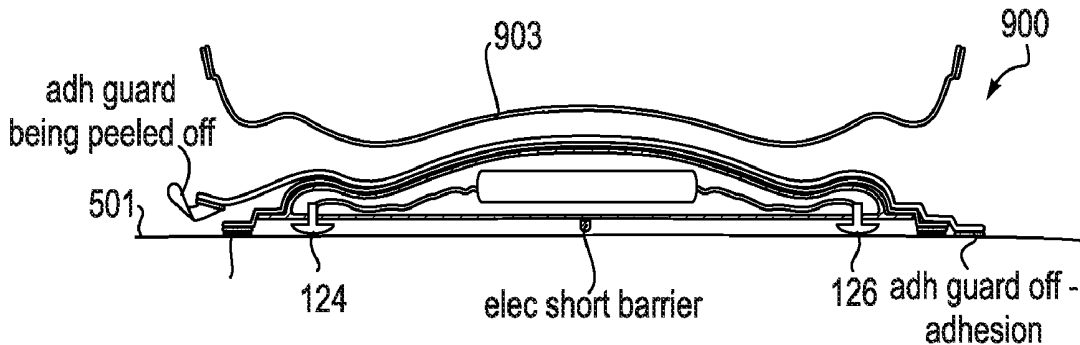

expose an electrode and an adhesive coated on a bottom surface of each wing.

19 Claims, 11 Drawing Sheets

Related U.S. Application Data

continuation of application No. 13/563,546, filed on Jul. 31, 2012, now Pat. No. 8,538,503, which is a continuation of application No. 13/106,750, filed on May 12, 2011, now Pat. No. 8,560,046.

(60) Provisional application No. 61/334,081, filed on May 12, 2010.

(51) **Int. Cl.**

A61B 5/00 (2006.01)

A61B 5/0478 (2006.01)

A61B 5/0488 (2006.01)

(52) **U.S. Cl.**

CPC *A61B 5/04085* (2013.01); *A61B 5/04087* (2013.01); *A61B 5/6833* (2013.01); *A61B 5/0488* (2013.01); *A61B 2560/0406* (2013.01); *A61B 2560/0468* (2013.01); *Y10T 156/10* (2015.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,201,645 A 5/1940 Epner
 2,311,060 A 2/1943 Lurrain
 2,500,840 A 3/1950 Lyons
 3,215,136 A 11/1965 Holter et al.
 3,547,107 A * 12/1970 Gofman A61B 5/02455
 600/382
 3,870,034 A 3/1975 James
 3,882,853 A 5/1975 Gofman
 3,911,906 A 10/1975 Reinhold
 4,023,312 A 5/1977 Stickney
 4,027,664 A 6/1977 Heavner, Jr. et al.
 4,121,573 A 10/1978 Crovella et al.
 4,123,785 A 10/1978 Cherry et al.
 4,126,126 A 11/1978 Bare
 4,202,139 A 5/1980 Hong et al.
 4,274,419 A 6/1981 Tam et al.
 4,274,420 A 6/1981 Hymes
 4,286,610 A 9/1981 Jones
 4,333,475 A 6/1982 Moreno et al.
 4,361,990 A 12/1982 Link
 4,381,792 A 5/1983 Busch
 4,438,767 A 3/1984 Nelson
 4,459,987 A 7/1984 Pangburn
 4,535,783 A 8/1985 Marangoni
 4,537,207 A 8/1985 Gilhaus
 4,572,187 A 2/1986 Schetrumpf
 4,621,465 A 11/1986 Pangburn
 4,658,826 A 4/1987 Weaver
 4,712,552 A 12/1987 Pangburn
 4,736,752 A 4/1988 Munck et al.
 4,925,453 A 5/1990 Kannankeril
 4,938,228 A 7/1990 Righter et al.
 4,981,141 A 1/1991 Segalowitz
 5,003,987 A 4/1991 Grinwald
 5,027,824 A 7/1991 Dougherty et al.
 5,082,851 A 1/1992 Appelbaum et al.
 5,086,778 A 2/1992 Mueller et al.
 5,191,891 A 3/1993 Righter
 5,205,295 A 4/1993 Del Mar et al.
 5,226,425 A 7/1993 Righter
 5,228,450 A 7/1993 Sellers
 5,230,119 A 7/1993 Woods et al.

5,289,824 A 3/1994 Mills et al.
 5,305,746 A 4/1994 Fendrock
 5,309,909 A 5/1994 Gadsby
 5,365,935 A 11/1994 Righter et al.
 5,458,141 A 10/1995 Neil
 5,483,967 A 1/1996 Ohtake
 5,489,624 A 2/1996 Kantner et al.
 5,511,553 A 4/1996 Segalowitz
 5,515,858 A 5/1996 Myllymaki
 5,536,768 A 7/1996 Kantner et al.
 5,581,369 A 12/1996 Righter et al.
 5,626,140 A 5/1997 Feldman et al.
 5,634,468 A 6/1997 Platt et al.
 5,645,063 A 7/1997 Straka
 5,645,068 A 7/1997 Mezack et al.
 5,730,143 A 3/1998 Schwarzberg
 5,749,365 A 5/1998 Magill
 5,749,367 A 5/1998 Gamlyn et al.
 5,771,524 A 6/1998 Woods et al.
 5,776,072 A 7/1998 Hsu et al.
 5,881,743 A 3/1999 Nadel
 5,931,791 A 8/1999 Saltzstein et al.
 5,941,829 A 8/1999 Saltzstein et al.
 5,957,854 A 9/1999 Besson et al.
 5,959,529 A 9/1999 Kail
 6,013,007 A 1/2000 Root et al.
 6,032,060 A 2/2000 Carim
 6,038,464 A * 3/2000 Axelgaard A61B 5/04087
 600/391
 6,038,469 A 3/2000 Karlsson et al.
 6,044,515 A 4/2000 Zygmunt
 6,093,146 A 7/2000 Filangeri
 D429,336 S 8/2000 Francis et al.
 6,102,856 A 8/2000 Groff et al.
 6,117,077 A 9/2000 Del Mar et al.
 6,132,371 A 10/2000 Dempsey et al.
 6,134,480 A 10/2000 Minogue
 6,136,008 A 10/2000 Becker et al.
 6,161,036 A 12/2000 Matsumura et al.
 6,169,915 B1 1/2001 Krumbiegel et al.
 6,178,357 B1 1/2001 Gliner et al.
 6,200,265 B1 3/2001 Walsh et al.
 6,225,901 B1 5/2001 Kail
 6,232,366 B1 5/2001 Wang et al.
 6,238,338 B1 5/2001 DeLuca et al.
 6,248,115 B1 6/2001 Halk
 6,287,252 B1 9/2001 Lugo
 6,290,707 B1 9/2001 Street
 6,315,719 B1 11/2001 Rode et al.
 6,379,237 B1 4/2002 Gordon
 6,385,473 B1 5/2002 Haines et al.
 6,389,308 B1 5/2002 Shusterman
 6,416,471 B1 7/2002 Kumar et al.
 6,434,410 B1 8/2002 Cordero et al.
 6,441,747 B1 8/2002 Khair et al.
 6,454,708 B1 9/2002 Ferguson et al.
 6,456,872 B1 9/2002 Faisandier
 6,464,815 B1 10/2002 Beaudry
 6,493,898 B1 12/2002 Woods et al.
 6,496,705 B1 12/2002 Ng et al.
 6,510,339 B2 1/2003 Kovtun et al.
 6,546,285 B1 4/2003 Owen et al.
 6,564,090 B2 5/2003 Taha et al.
 6,569,095 B2 5/2003 Eggers
 6,577,893 B1 6/2003 Besson et al.
 6,580,942 B1 6/2003 Willshire
 6,585,707 B2 7/2003 Cabiri et al.
 6,589,170 B1 7/2003 Flach et al.
 6,589,187 B1 7/2003 Dimberger et al.
 6,605,046 B1 8/2003 Del Mar et al.
 6,615,083 B2 9/2003 Kupper
 6,622,035 B1 9/2003 Merilainen
 6,626,865 B1 9/2003 Prisell
 6,656,125 B2 12/2003 Mischzynski et al.
 6,664,893 B1 12/2003 Eveland et al.
 6,665,385 B2 12/2003 Rogers et al.
 6,690,959 B2 2/2004 Thompson
 6,694,177 B2 2/2004 Eggers et al.
 6,701,184 B2 3/2004 Henkin

(56)

References Cited

U.S. PATENT DOCUMENTS

6,711,427 B1	3/2004	Ketelhohn	8,002,701 B2	8/2011	John et al.	
6,730,028 B2	5/2004	Eppstein	8,077,042 B2	12/2011	Peeters	
6,773,396 B2	8/2004	Flach et al.	8,103,333 B2	1/2012	Tran	
6,775,566 B2	8/2004	Nissila	8,108,036 B2	1/2012	Tran	
6,801,137 B2	10/2004	Eggers	8,116,841 B2	2/2012	Bly et al.	
6,801,802 B2	10/2004	Sitzman et al.	8,150,502 B2	4/2012	Kumar et al.	
6,871,089 B2	3/2005	Korzinov et al.	8,156,945 B2	4/2012	Hart	
6,871,211 B2	3/2005	Labounty et al.	8,160,682 B2	4/2012	Kumar et al.	
6,875,174 B2	4/2005	Braun et al.	D659,836 S	5/2012	Bensch et al.	
6,881,191 B2	4/2005	Oakley et al.	8,200,319 B2	6/2012	Pu et al.	
6,893,396 B2	5/2005	Schulze et al.	8,214,007 B2	7/2012	Baker et al.	
6,897,788 B2	5/2005	Khair et al.	8,244,335 B2	8/2012	Kumar et al.	
6,925,324 B2	8/2005	Shusterman	8,249,686 B2	8/2012	Libbus et al.	
6,940,403 B2	9/2005	Kail	8,261,754 B2	9/2012	Pitstick	
6,954,163 B2	10/2005	Toumazou et al.	8,265,907 B2	9/2012	Nanikashvili et al.	
6,957,107 B2	10/2005	Rogers et al.	RE43,767 E	10/2012	Eggers et al.	
6,987,965 B2	1/2006	Ng et al.	8,280,749 B2	10/2012	Hsieh et al.	
7,002,468 B2	2/2006	Eveland et al.	8,285,356 B2	10/2012	Bly et al.	
7,020,508 B2	3/2006	Stivoric et al.	8,290,129 B2	10/2012	Rogers et al.	
7,024,248 B2	4/2006	Penner et al.	8,290,574 B2	10/2012	Field et al.	
7,072,708 B1	7/2006	Andresen et al.	8,301,219 B2	10/2012	Chen et al.	
7,072,709 B2	7/2006	Xue	8,301,236 B2	10/2012	Baumann et al.	
7,076,283 B2	7/2006	Cho et al.	8,311,604 B2	11/2012	Rowlandson et al.	
7,076,287 B2	7/2006	Rowlandson	8,315,687 B2	11/2012	Cross et al.	
7,076,288 B2	7/2006	Skinner	8,315,695 B2	11/2012	Sebelius et al.	
7,076,289 B2	7/2006	Sarkar et al.	8,323,188 B2	12/2012	Tran	
7,079,977 B2	7/2006	Osorio et al.	8,326,394 B2	12/2012	Rowlandson et al.	
7,082,327 B2	7/2006	Houben	8,326,407 B2	12/2012	Linker	
7,089,048 B2	8/2006	Matsumura et al.	8,328,718 B2	12/2012	Tran	
7,099,715 B2	8/2006	Korzinov et al.	8,343,116 B2	1/2013	Ignon	
7,117,031 B2	10/2006	Lohman et al.	8,374,688 B2	2/2013	Libbus et al.	
7,120,485 B2	10/2006	Glass et al.	8,386,009 B2	2/2013	Lindberg et al.	
7,130,396 B2	10/2006	Rogers et al.	8,406,843 B2	3/2013	Tiegs et al.	
7,161,484 B2	1/2007	Tsoukalis	8,412,317 B2	4/2013	Mazar	
7,171,166 B2	1/2007	Ng et al.	8,425,414 B2	4/2013	Eveland	
7,179,152 B1	2/2007	Rhoades	8,449,471 B2	5/2013	Tran	
7,186,264 B2	3/2007	Liddicoat et al.	8,452,356 B2	5/2013	Vestel et al.	
7,193,264 B2	3/2007	Lande	8,460,189 B2	6/2013	Libbus et al.	
7,194,300 B2	3/2007	Korzinov	8,473,039 B2	6/2013	Michelson et al.	
7,206,630 B1	4/2007	Tarler	8,473,047 B2	6/2013	Chakravarthy et al.	
7,212,850 B2	5/2007	Prystowsky et al.	8,478,418 B2	7/2013	Fahey	
7,222,054 B2	5/2007	Geva	8,483,809 B2	7/2013	Kim et al.	
7,242,318 B2	7/2007	Harris	8,500,636 B2	8/2013	Tran	
7,266,361 B2	9/2007	Burdett	8,515,529 B2	8/2013	Pu et al.	
7,316,671 B2	1/2008	Lastovich et al.	8,525,673 B2	9/2013	Tran	
7,349,947 B1	3/2008	Slage et al.	8,535,223 B2	9/2013	Corroy et al.	
7,354,423 B2	4/2008	Zelickson et al.	8,538,503 B2 *	9/2013	Kumar	A61B 5/6833 600/391
7,387,607 B2	6/2008	Holt et al.	8,540,731 B2	9/2013	Kay	
7,444,177 B2	10/2008	Nazeri	8,560,046 B2 *	10/2013	Kumar	A61B 5/6833 600/392
7,477,933 B2	1/2009	Ueyama	8,562,527 B2	10/2013	Braun et al.	
7,478,108 B2	1/2009	Townsend et al.	8,571,645 B2	10/2013	Wu et al.	
7,481,772 B2	1/2009	Banet	8,591,430 B2	11/2013	Amurthur et al.	
7,482,314 B2	1/2009	Grimes et al.	8,594,763 B1	11/2013	Bibian	
7,502,643 B2	3/2009	Farringdon et al.	8,626,262 B2	1/2014	McGusty et al.	
7,539,533 B2	5/2009	Tran	8,639,319 B2	1/2014	Hugh et al.	
7,542,878 B2	6/2009	Nanikashvili	8,668,643 B2	3/2014	Kinast	
7,587,237 B2	9/2009	Korzinov et al.	8,684,900 B2	4/2014	Tran	
7,630,756 B2	12/2009	Linker	8,684,925 B2	4/2014	Amurthur et al.	
7,632,174 B2	12/2009	Gringer et al.	8,688,189 B2	4/2014	Shennib	
7,672,714 B2	3/2010	Kuo et al.	8,688,190 B2	4/2014	Libbus et al.	
7,715,905 B2	5/2010	Kurzweil et al.	8,688,202 B2	4/2014	Brockway et al.	
7,729,753 B2	6/2010	Kremliovsky et al.	8,718,742 B2	5/2014	Beck et al.	
7,733,224 B2	6/2010	Tran	8,718,752 B2	5/2014	Libbus et al.	
D621,048 S	8/2010	Severe et al.	8,731,632 B1	5/2014	Sereboff et al.	
7,815,494 B2	10/2010	Gringer et al.	8,738,118 B2	5/2014	Moon et al.	
7,841,039 B1	11/2010	Squire	8,782,308 B2	7/2014	Vlach	
7,889,070 B2	2/2011	Reeves et al.	8,790,257 B2	7/2014	Libbus et al.	
D634,431 S	3/2011	Severe et al.	8,795,174 B2	8/2014	Manicka et al.	
7,904,133 B2	3/2011	Gehman et al.	8,818,481 B2	8/2014	Bly et al.	
7,907,956 B2	3/2011	Uhlik	8,823,490 B2	9/2014	Libbus et al.	
7,907,996 B2	3/2011	Prystowsky et al.	8,838,218 B2	9/2014	Khair	
7,941,207 B2	5/2011	Korzinov	8,874,185 B2	10/2014	Sonnenborg	
7,970,450 B2	6/2011	Kroecker et al.	8,903,477 B2	12/2014	Berkner	
7,996,075 B2	8/2011	Korzinov et al.	8,903,484 B2	12/2014	Mazar	
7,996,187 B2	8/2011	Nanikashvili et al.	8,909,330 B2	12/2014	McCombie et al.	
			8,909,832 B2	12/2014	Vlach et al.	
			8,926,509 B2	1/2015	Magar et al.	

(56)		References Cited						
		U.S. PATENT DOCUMENTS						
8,945,019	B2	2/2015	Prystowsky et al.	2005/0096513	A1	5/2005	Ozguz et al.	
8,954,129	B1	2/2015	Schlegel et al.	2005/0101875	A1	5/2005	Semler et al.	
8,956,293	B2	2/2015	McCombie et al.	2005/0118246	A1	6/2005	Wong et al.	
8,968,195	B2	3/2015	Tran	2005/0119580	A1	6/2005	Eveland	
8,972,000	B2	3/2015	Manera	2005/0165323	A1	7/2005	Montgomery et al.	
8,979,755	B2	3/2015	Szydlo-Moore et al.	2005/0204636	A1	9/2005	Azar et al.	
9,014,777	B2	4/2015	Woo	2005/0277841	A1	12/2005	Shennib	
9,015,008	B2	4/2015	Geva et al.	2005/0280531	A1	12/2005	Fadem et al.	
9,017,255	B2	4/2015	Raptis et al.	2006/0030781	A1	2/2006	Shennib	
9,017,256	B2	4/2015	Gottesman	2006/0030782	A1	2/2006	Shennib	
9,021,161	B2	4/2015	Vlach et al.	2006/0047215	A1	3/2006	Newman et al.	
9,021,165	B2	4/2015	Vlach	2006/0084883	A1	4/2006	Linker	
9,026,190	B2	5/2015	Shenasa et al.	2006/0142648	A1	6/2006	Banet et al.	
9,037,223	B2	5/2015	Oral et al.	2006/0142654	A1	6/2006	Rytky	
9,044,148	B2	6/2015	Michelson et al.	2006/0149156	A1	7/2006	Cochran et al.	
9,084,548	B2	7/2015	Bouguerra	2006/0155173	A1	7/2006	Anttila et al.	
9,095,274	B2	8/2015	Fein et al.	2006/0155183	A1	7/2006	Kroecker et al.	
9,101,264	B2	8/2015	Acquista	2006/0155199	A1	7/2006	Logier et al.	
9,138,144	B2	9/2015	Geva	2006/0155200	A1	7/2006	Ng et al.	
9,149,228	B2	10/2015	Kinast	2006/0161064	A1	7/2006	Watrous et al.	
9,173,670	B2	11/2015	Sepulveda et al.	2006/0161065	A1	7/2006	Elion	
9,179,851	B2	11/2015	Baumann et al.	2006/0161066	A1	7/2006	Elion	
9,211,076	B2	12/2015	Kim	2006/0161067	A1	7/2006	Elion	
9,226,679	B2	1/2016	Balda	2006/0161068	A1	7/2006	Hastings et al.	
9,241,649	B2*	1/2016	Kumar A61B 5/6833	2006/0224072	A1	10/2006	Shennib	
9,241,650	B2	1/2016	Amirim	2006/0264767	A1	11/2006	Shennib	
15,005,854		1/2016	Kumar et al.	2007/0003695	A1	1/2007	Tregub et al.	
9,277,864	B2	3/2016	Yang et al.	2007/0010729	A1	1/2007	Virtanen	
9,282,894	B2	3/2016	Banet et al.	2007/0027388	A1	2/2007	Chou	
9,345,414	B1	5/2016	Bardy et al.	2007/0088419	A1	4/2007	Florina et al.	
9,355,215	B2	5/2016	Vlach	2007/0156054	A1	7/2007	Korzinov et al.	
9,357,939	B1	6/2016	Nosrati	2007/0225611	A1	9/2007	Kumar et al.	
9,364,150	B2	6/2016	Sebelius et al.	2007/0249946	A1	10/2007	Kumar et al.	
9,398,853	B2	7/2016	Nanikashvili	2007/0255153	A1	11/2007	Kumar et al.	
9,414,786	B1	8/2016	Brockway et al.	2007/0270678	A1	11/2007	Fadem et al.	
9,433,367	B2	9/2016	Felix et al.	2007/0293776	A1	12/2007	Korzinov et al.	
9,439,566	B2	9/2016	Arne et al.	2008/0039730	A1	2/2008	Pu et al.	
9,439,599	B2	9/2016	Thompson et al.	2008/0091089	A1	4/2008	Guillory et al.	
9,445,719	B2	9/2016	Libbus et al.	2008/0108890	A1	5/2008	Teng et al.	
9,451,890	B2	9/2016	Gitlin et al.	2008/0114232	A1	5/2008	Gazit	
9,451,975	B2	9/2016	Sepulveda et al.	2008/0139953	A1	6/2008	Baker et al.	
9,474,445	B2	10/2016	Eveland	2008/0214901	A1*	9/2008	Gehman A61B 5/0006	
9,474,461	B2	10/2016	Fisher et al.				600/391	
D773,056	S	11/2016	Vlach	2008/0275327	A1	11/2008	Faarbaek et al.	
9,492,084	B2	11/2016	Behar et al.	2008/0288026	A1	11/2008	Cross et al.	
9,504,423	B1	11/2016	Bardy et al.	2009/0048556	A1*	2/2009	Durand A61K 9/0009	
9,579,020	B2	2/2017	Libbus et al.				604/20	
9,597,004	B2	3/2017	Hughes et al.	2009/0062670	A1	3/2009	Sterling et al.	
9,615,793	B2	4/2017	Solosko et al.	2009/0073991	A1	3/2009	Landrum et al.	
9,655,518	B2	5/2017	Lin	2009/0076336	A1	3/2009	Mazar et al.	
9,706,938	B2	7/2017	Chakravarthy et al.	2009/0076340	A1	3/2009	Libbus et al.	
9,775,534	B2	10/2017	Korzinov et al.	2009/0076341	A1	3/2009	James et al.	
9,782,095	B2	10/2017	Ylostalo et al.	2009/0076342	A1	3/2009	Amurthur et al.	
9,839,363	B2	12/2017	Albert	2009/0076343	A1	3/2009	James et al.	
2001/0056262	A1	12/2001	Cabiri et al.	2009/0076344	A1	3/2009	Libbus et al.	
2002/0067256	A1	6/2002	Kail	2009/0076345	A1	3/2009	Manicka et al.	
2002/0082491	A1	6/2002	Nissila	2009/0076346	A1	3/2009	James et al.	
2002/0087167	A1	7/2002	Winitzky	2009/0076349	A1	3/2009	Libbus et al.	
2002/0180605	A1	12/2002	Ozguz et al.	2009/0076350	A1	3/2009	Bly et al.	
2003/0069510	A1	4/2003	Semler	2009/0076364	A1	3/2009	Libbus et al.	
2003/0083559	A1	5/2003	Thompson	2009/0076397	A1	3/2009	Libbus et al.	
2003/0149349	A1*	8/2003	Jensen A61B 5/02055	2009/0076341	A1	3/2009	James et al.	
			600/372	2009/0076559	A1	3/2009	Libbus et al.	
2003/0176795	A1	9/2003	Harris et al.	2009/0182204	A1	7/2009	Semler et al.	
2003/0195408	A1	10/2003	Hastings	2009/0253975	A1	10/2009	Tiegs	
2003/0199811	A1	10/2003	Sage, Jr. et al.	2009/0292194	A1	11/2009	Libbus et al.	
2003/0212319	A1	11/2003	Magill	2010/0022864	A1	1/2010	Cordero	
2004/0032957	A1	2/2004	Mansy et al.	2010/0042113	A1	2/2010	Mah	
2004/0068195	A1	4/2004	Massicotte et al.	2010/0049006	A1	2/2010	Magar et al.	
2004/0077954	A1*	4/2004	Oakley A61B 5/0006	2010/0051039	A1	3/2010	Ferrara	
			600/483	2010/0056881	A1*	3/2010	Libbus A61B 5/0402	
2004/0215091	A1	10/2004	Lohman et al.				600/301	
2004/0236202	A1	11/2004	Burton	2010/0057056	A1	3/2010	Gurtner	
2004/0254587	A1	12/2004	Park	2010/0081913	A1	4/2010	Cross et al.	
2004/0260189	A1	12/2004	Eggers et al.	2010/0145359	A1	6/2010	Keller	
				2010/0191310	A1	7/2010	Bly	
				2010/0234716	A1	9/2010	Engel	
				2010/0249625	A1	9/2010	Lin	
				2010/0268103	A1	10/2010	McNamara et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

2010/0331711	A1	12/2010	Krauss et al.
2011/0021937	A1	1/2011	Hugh et al.
2011/0087083	A1	4/2011	Poeze et al.
2011/0144470	A1*	6/2011	Mazar A61B 5/04085 600/391
2011/0160601	A1	6/2011	Wang et al.
2011/0166468	A1	7/2011	Prystowsky et al.
2011/0190650	A1	8/2011	McNair
2011/0237922	A1	9/2011	Parker, III et al.
2011/0306862	A1	12/2011	Hayes-Gill
2012/0029307	A1	2/2012	Paquet et al.
2012/0071730	A1	3/2012	Romero
2012/0071731	A1	3/2012	Gottesman
2012/0071743	A1	3/2012	Todorov et al.
2012/0083670	A1	4/2012	Rotondo et al.
2012/0088999	A1	4/2012	Bishay et al.
2012/0101396	A1	4/2012	Solosko et al.
2012/0108917	A1	5/2012	Libbus et al.
2012/0108920	A1	5/2012	Bly et al.
2012/0110226	A1	5/2012	Vlach et al.
2012/0110228	A1	5/2012	Vlach et al.
2012/0172676	A1	7/2012	Penders et al.
2012/0197150	A1	8/2012	Cao et al.
2012/0209102	A1	8/2012	Ylotalo et al.
2012/0215123	A1	8/2012	Kumar et al.
2012/0220835	A1	8/2012	Chung
2012/0259233	A1	10/2012	Chan et al.
2012/0271141	A1	10/2012	Davies
2012/0310070	A1	12/2012	Kumar et al.
2012/0323257	A1	12/2012	Sutton
2013/0046151	A1	2/2013	Bsoul et al.
2013/0085347	A1	4/2013	Manicka et al.
2013/0096395	A1	4/2013	Katra et al.
2013/0116533	A1	5/2013	Lian et al.
2013/0116585	A1	5/2013	Bouguerra
2013/0144146	A1	6/2013	Linker
2013/0150698	A1	6/2013	Hsu et al.
2013/0225938	A1	8/2013	Vlach
2013/0225967	A1	8/2013	Esposito
2013/0226018	A1	8/2013	Kumar et al.
2013/0245415	A1	9/2013	Kumar et al.
2013/0245472	A1	9/2013	Eveland
2013/0253285	A1	9/2013	Bly et al.
2013/0274584	A1	10/2013	Finlay et al.
2013/0296680	A1	11/2013	Linker
2013/0300575	A1	11/2013	Kurzweil et al.
2013/0324868	A1	12/2013	Kaib et al.
2013/0331663	A1	12/2013	Albert et al.
2013/0331665	A1	12/2013	Bly et al.
2013/0338448	A1	12/2013	Libbus et al.
2014/0012154	A1	1/2014	Mazar
2014/0058280	A1	2/2014	Cheffes et al.
2014/0094709	A1	4/2014	Korzinov et al.
2014/0100432	A1	4/2014	Golda et al.
2014/0171751	A1	6/2014	Sankman et al.
2014/0116825	A1	7/2014	Kurzweil et al.
2014/0206976	A1	7/2014	Thompson et al.
2014/0206977	A1	7/2014	Bahney et al.
2014/0275928	A1	9/2014	Acquista et al.
2014/0330136	A1	11/2014	Manicka et al.
2015/0022372	A1	1/2015	Vosch
2015/0057512	A1	2/2015	Kapoor
2015/0073252	A1	3/2015	Mazar
2015/0081959	A1	3/2015	Vlach et al.
2015/0082623	A1	3/2015	Felix et al.
2015/0087921	A1	3/2015	Felix et al.
2015/0087922	A1	3/2015	Bardy et al.
2015/0087923	A1	3/2015	Bardy et al.
2015/0087933	A1	3/2015	Gibson et al.
2015/0087948	A1	3/2015	Bishay et al.
2015/0087949	A1	3/2015	Felix et al.
2015/0087950	A1	3/2015	Felix et al.
2015/0087951	A1	3/2015	Felix et al.
2015/0088007	A1	3/2015	Bardy et al.
2015/0088020	A1	3/2015	Dreisbach et al.

2015/0094556	A1	4/2015	Geva et al.
2015/0173671	A1	6/2015	Paalasmaa et al.
2015/0238107	A1	8/2015	Acquista et al.
2015/0289814	A1	10/2015	Magar et al.
2015/0297134	A1	10/2015	Albert et al.
2015/0327781	A1	11/2015	Hernandez-Silverira et al.
2015/0351799	A1	12/2015	Sepulveda et al.
2015/0374244	A1	12/2015	Yoo et al.
2016/0022161	A1	1/2016	Khair
2016/0029906	A1	2/2016	Tompkins et al.
2016/0066808	A1	3/2016	Hijazi
2016/0113520	A1	4/2016	Manera
2016/0120433	A1	5/2016	Hughes et al.
2016/0120434	A1	5/2016	Park et al.
2016/0128597	A1	5/2016	Lin et al.
2016/0135746	A1	5/2016	Kumar et al.
2016/0157744	A1	6/2016	Wu et al.
2016/0166155	A1	6/2016	Banet et al.
2016/0192852	A1	7/2016	Bozza et al.
2016/0192855	A1	7/2016	Geva et al.
2016/0192856	A1	7/2016	Lee
2016/0198972	A1	7/2016	Lee et al.
2016/0232807	A1	8/2016	Ghaffari et al.
2016/0262619	A1	9/2016	Marcus et al.
2016/0287177	A1	10/2016	Huppert et al.
2016/0287207	A1	10/2016	Xue
2016/0296132	A1	10/2016	Bojovic et al.
2016/0302726	A1	10/2016	Chang
2016/0317048	A1	11/2016	Chan et al.
2016/0317057	A1	11/2016	Li et al.
2016/0367164	A1	12/2016	Felix et al.
2016/0374583	A1	12/2016	Cerruti et al.
2017/0065823	A1	3/2017	Kaib et al.
2017/0188872	A1	7/2017	Hughes et al.

FOREIGN PATENT DOCUMENTS

CA	2752154	8/2010
CA	2797980	11/2011
CA	2898626	7/2014
CA	2651203	9/2017
EP	01782729	5/2007
EP	1981402	10/2008
EP	2262419	12/2010
EP	2395911	12/2011
EP	2568878	3/2013
EP	2635179	9/2013
EP	2635180	9/2013
EP	2948050	12/2015
EP	2983593	2/2016
EP	3165161	5/2017
EP	3212061	9/2017
GB	2299038	9/1996
GB	2348707	10/2000
JP	08-317913	3/1996
JP	2000-126145	5/2000
JP	2001-057967	3/2001
JP	2004-121360	4/2004
JP	2007-045967	2/2007
JP	2007-097822	4/2007
JP	2007-296266	11/2007
JP	2009-525816	7/2009
JP	2011-519583	7/2011
JP	2013-521966	6/2013
JP	5203973	6/2013
JP	5559425	7/2014
JP	2014-236982	12/2014
JP	2016-504159	2/2016
JP	2013-517053	5/2016
JP	2017-136380	8/2017
JP	6198849	9/2017
KR	10-1513288	4/2015
WO	WO 1999/023943	5/1999
WO	WO 2001/016607	3/2001
WO	WO 2004/100785	11/2004
WO	WO 2005/025668	3/2005
WO	WO 2005/037946	4/2005
WO	WO 2005/084533	9/2005
WO	WO 2006/094513	9/2006

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 2007/049080	3/2007
WO	WO 2007/036748	4/2007
WO	WO 2007/063436	6/2007
WO	WO 2007/071180	6/2007
WO	WO 2007/072069	6/2007
WO	WO 2007/092543	8/2007
WO	WO 2008/005015	1/2008
WO	WO 2008/005016	1/2008
WO	WO 2008/057884	5/2008
WO	WO 2008/120154	10/2008
WO	WO 2009/074928	6/2009
WO	WO 2009/112976	9/2009
WO	WO 2009/112979	9/2009
WO	WO 2009/134826	11/2009
WO	WO 2010/104952	9/2010
WO	WO 2010/105203	9/2010
WO	WO 2010/093900	10/2010
WO	WO 2011/077097	6/2011
WO	WO 2011/143490	11/2011
WO	WO 2011/149755	12/2011
WO	WO 2012/009453	1/2012
WO	WO 2012/061509	5/2012
WO	WO 2012/061518	5/2012
WO	WO 2012/125425	9/2012
WO	WO 2012/160550	11/2012
WO	WO 2014/051563	4/2014
WO	WO 2014/116825	7/2014
WO	WO 2014/168841	10/2014
WO	WO 2016/070128	5/2016
WO	WO 2016/181321	11/2016
WO	WO 2017/039518	3/2017
WO	WO 2017/041014	3/2017

OTHER PUBLICATIONS

3M Corporation, "3M Surgical Tapes—Choose the Correct Tape" quicksheet (2004).

Del Mar et al.; The history of clinical holter monitoring; A.N.E.; vol. 10; No. 2; pp. 226-230; Apr. 2005.

Enseleit et al.; Long-term continuous external electrocardiographic recording: a review; Eurospace; vol. 8; pp. 255-266; 2006.

Hoefman et al.; Optimal duration of event recording for diagnosis of arrhythmias in patients with palpitations and light-headedness in the general practice; Family Practice; Dec. 7, 2006.

International Search Report and Written Opinion for International Application No. PCT/US2011/036335 dated Oct. 31, 2011 in 7 pages.

International Preliminary Report on Patentability for International Application No. PCT/US2011/036335 dated Nov. 13, 2012 in 5 pages.

Kennedy et al.; The history, science, and innovation of holter technology; A.N.E.; vol. 11; No. 1; pp. 85-94; 2006.

Mundt et al. "A Multiparameter Wearable Physiologic Monitoring System for Space and Terrestrial Applications" IEEE Transactions on Information Technology in Biomedicine, vol. 9, No. 3, pp. 382-384, Sep. 2005.

Reiffel et al.; Comparison of autotriggered memory loop recorders versus standard loop recorders versus 24-hour holter monitors for arrhythmia detection; Am. J. Cardiology; vol. 95; pp. 1055-1059; May 1, 2005.

Request for Reexamination of U.S. Pat. No. 7,020,508 under 35 U.S.C. §§ 311-318 and 37 C.F.R. § 1.913 as submitted Sep. 14, 2012 in 78 pages.

Scapa Medical product listing and descriptions (2008) available at <http://www.caapana.com/productlist.jsp> and <http://www.metplus.co.rs/pdf/prospekti/Samolepljivemedicinsketrake.pdf>; retrieved via WayBack Machine Sep. 24, 2012.

Ward et al.; Assessment of the diagnostic value of 24-hour ambulatory electrocardiographic monitoring; Biotelemetry Patient monitoring; vol. 7; 1980.

Ziegler et al.; Comparison of continuous versus intermittent monitoring of atrial arrhythmias; Heart Rhythm; vol. 3; No. 12; pp. 1445-1452; Dec. 2006.

Zimetbaum et al.; The evolving role of ambulatory arrhythmia monitoring in general clinic practice; Ann. Intern. Med.; vol. 130; pp. 846-8556; 1999.

Zimetbaum et al.; Utility of patient-activated cardiac event recorders in general clinical practice; The Amer. J. of Cardiology; vol. 79; Feb. 1, 1997.

* cited by examiner

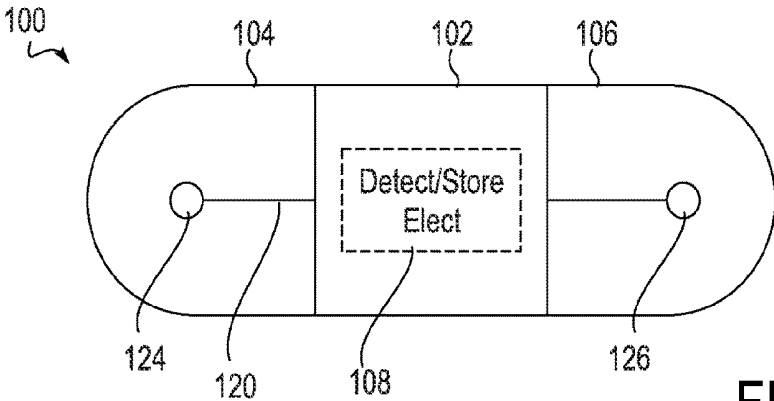


FIG. 1

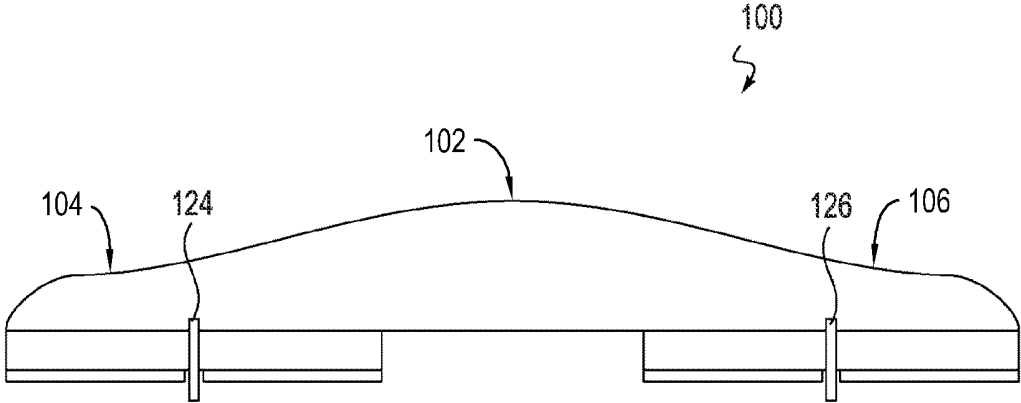


FIG. 1A

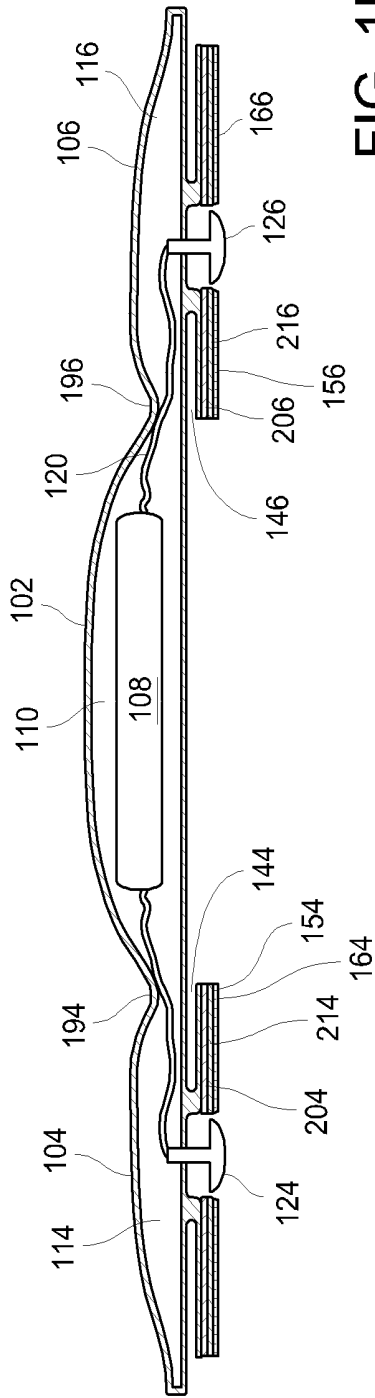


FIG. 1D

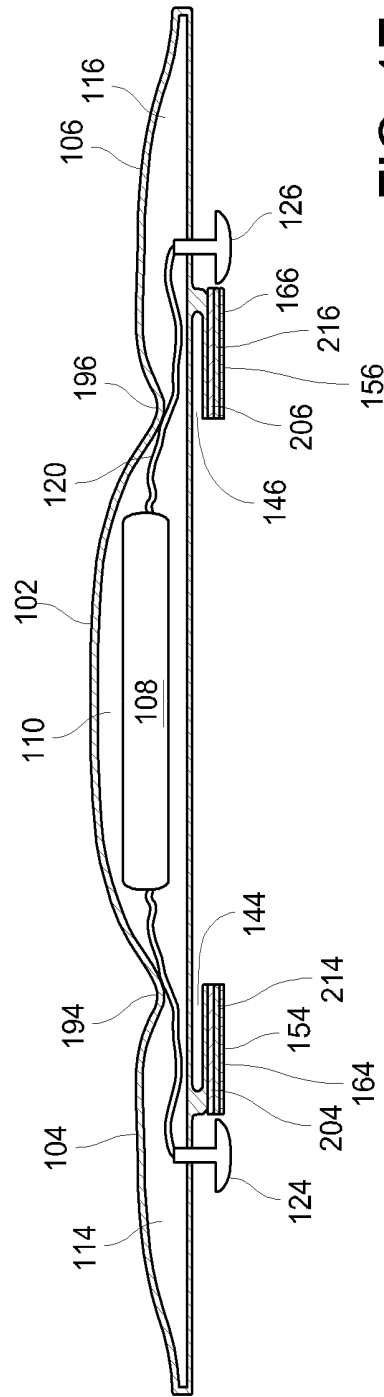


FIG. 1E

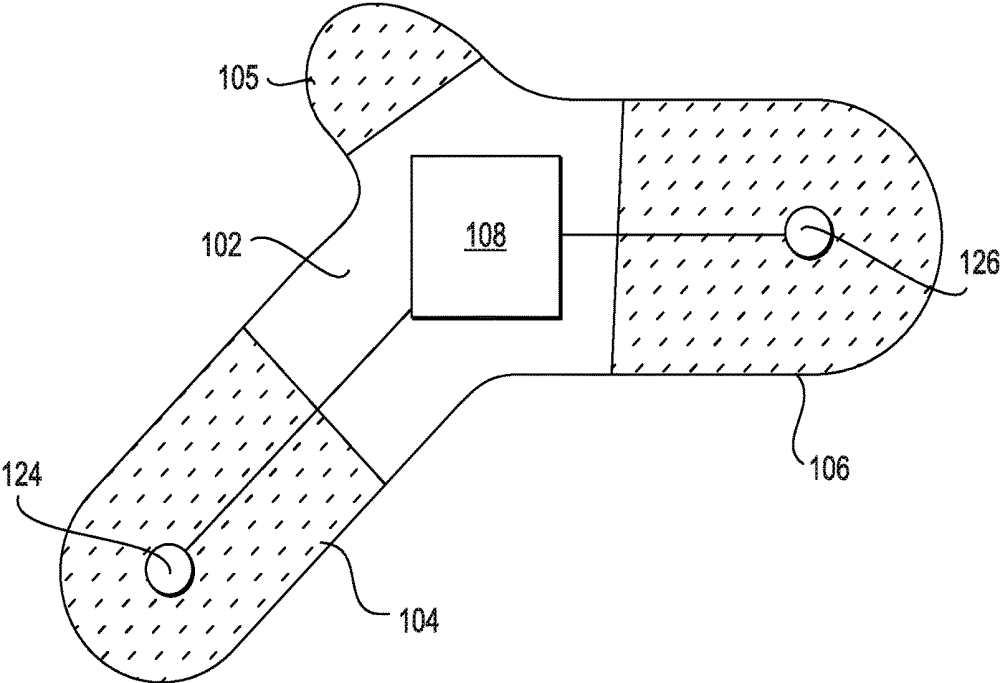


FIG. 1F

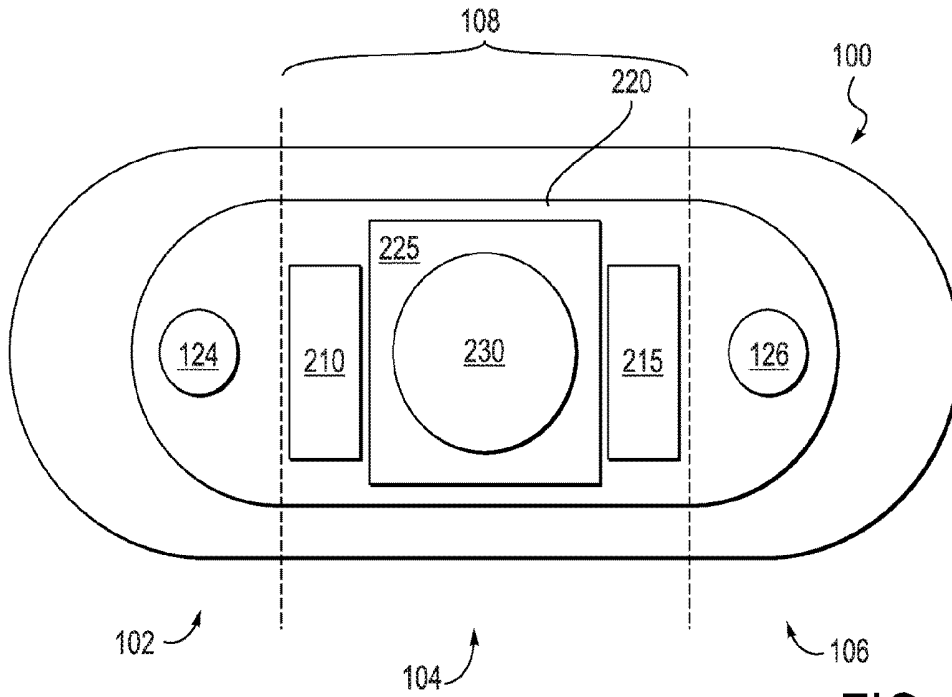


FIG. 2A

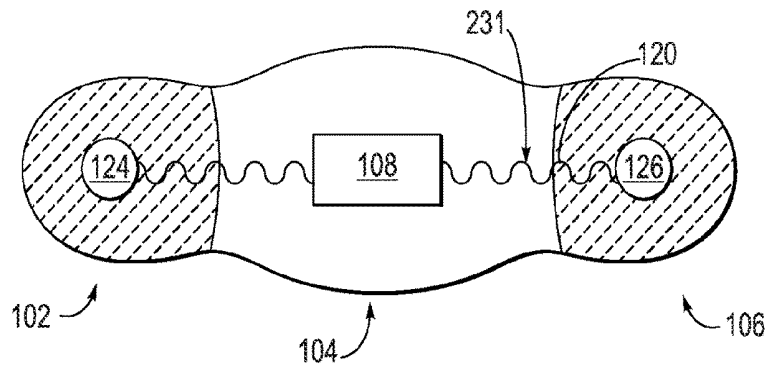


FIG. 2B

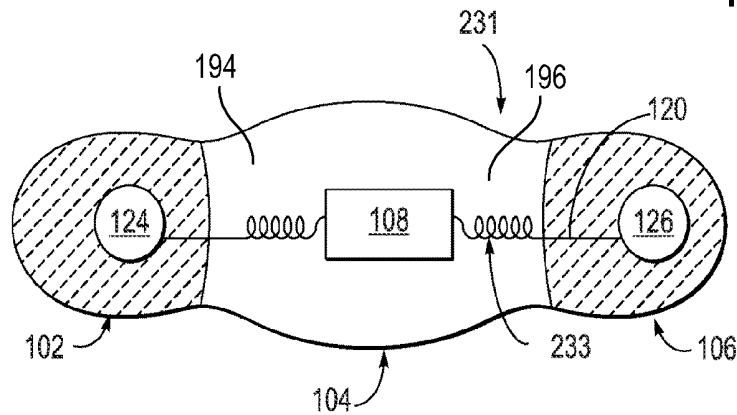


FIG. 2C

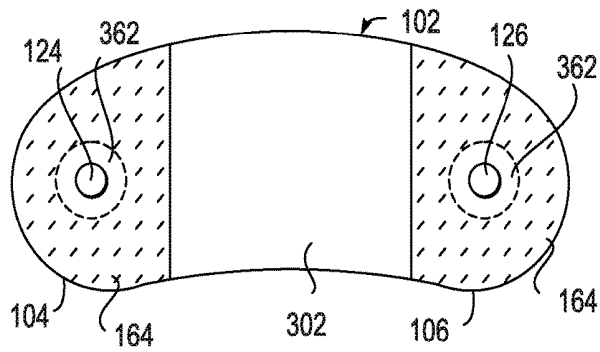


FIG. 3

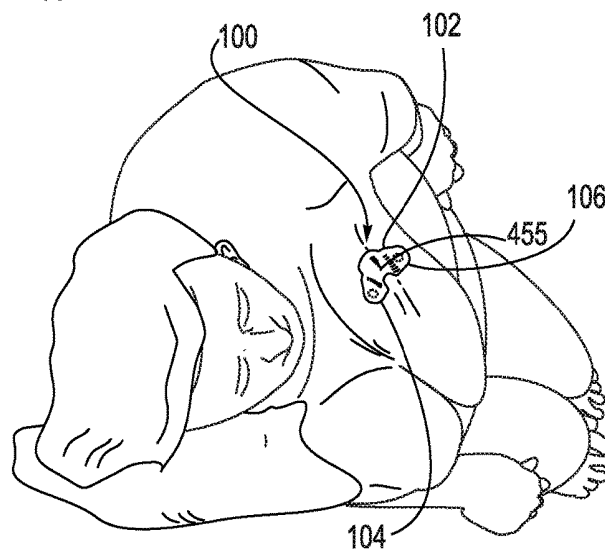


FIG. 4A

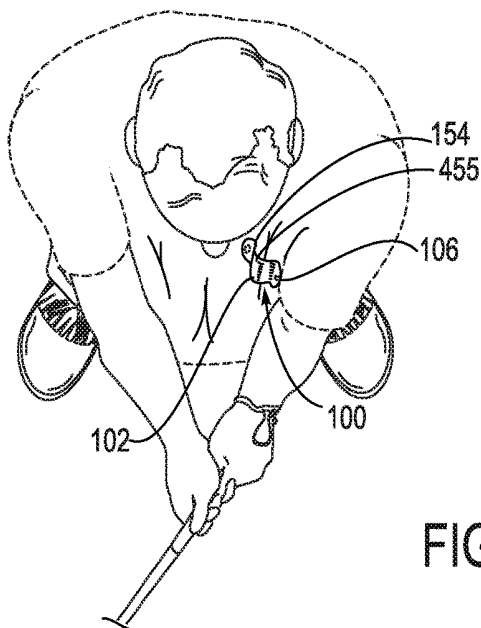


FIG. 4B

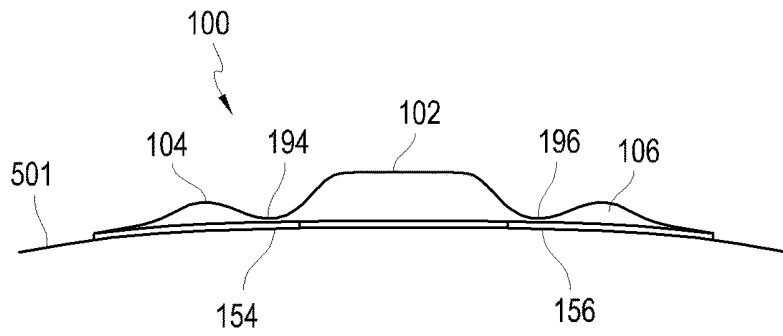


FIG. 5A

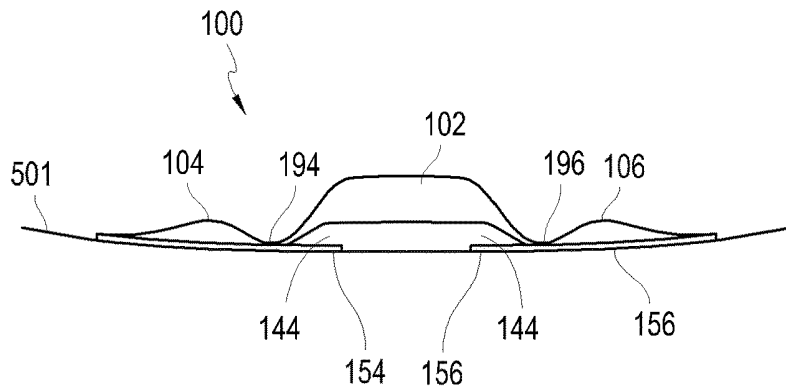


FIG. 5B

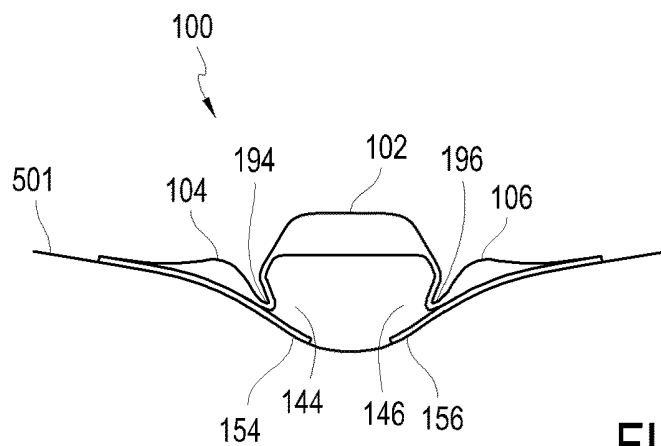
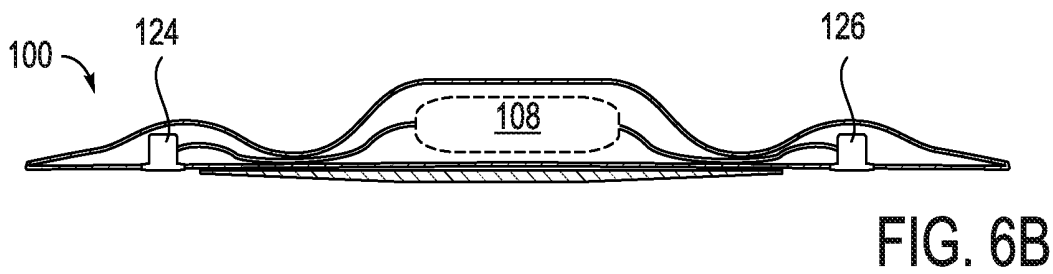
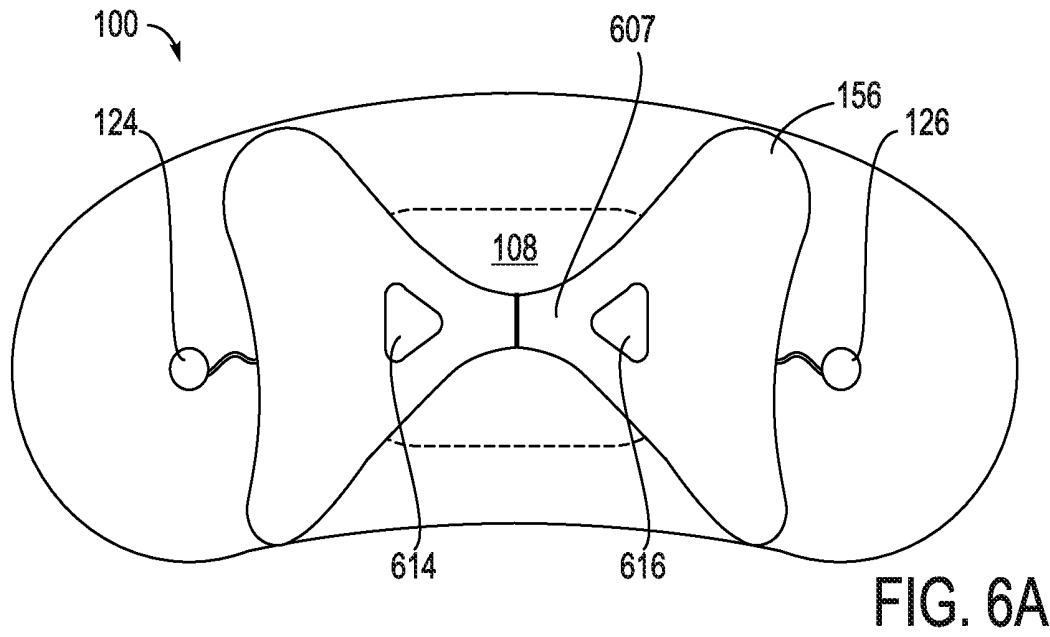


FIG. 5C



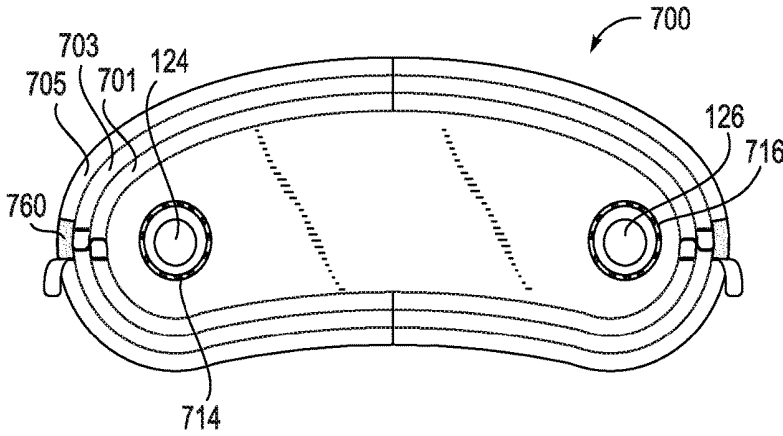


FIG. 7A

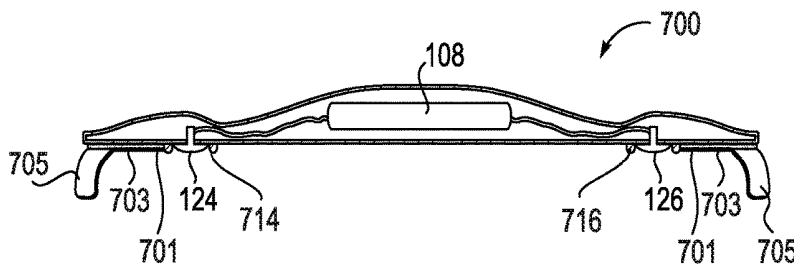


FIG. 7B

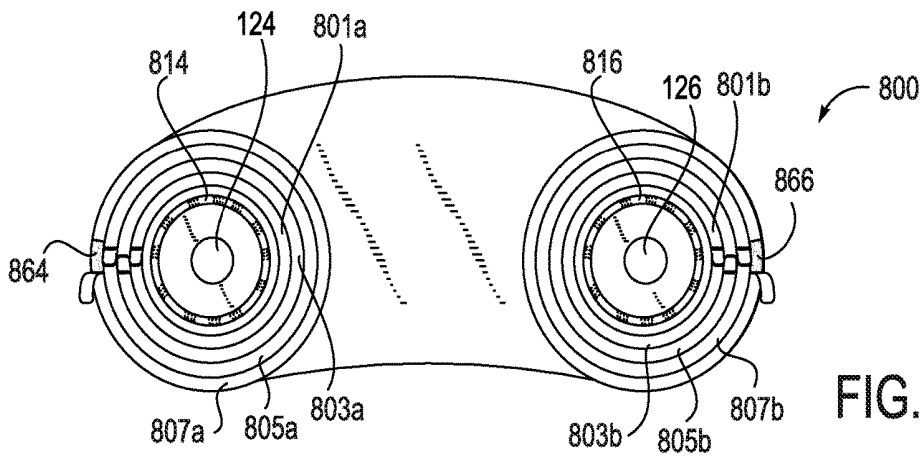


FIG. 8A

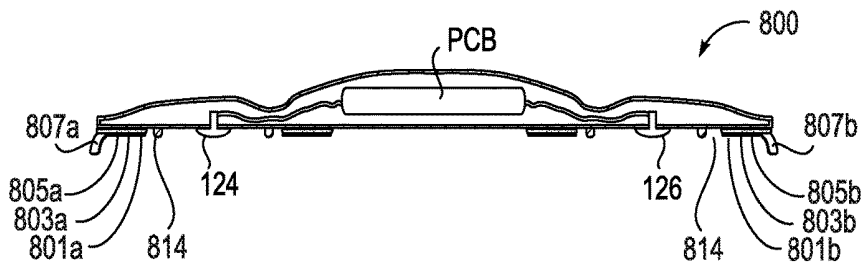


FIG. 8B

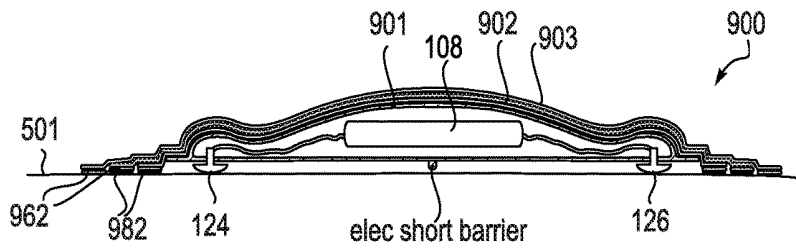


FIG. 9A

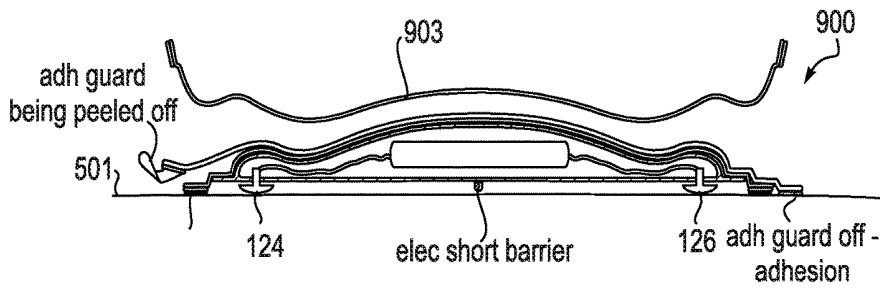


FIG. 9B

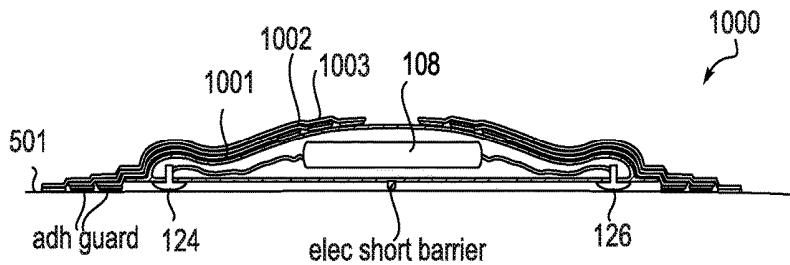


FIG. 10A

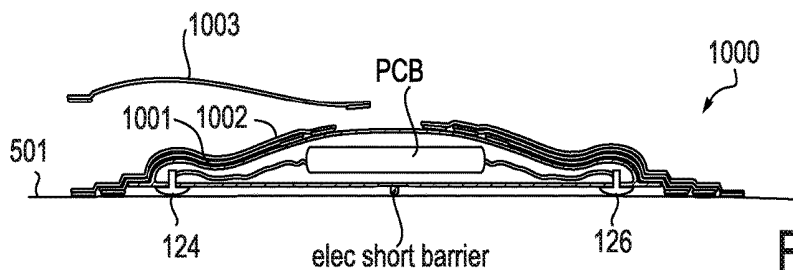


FIG. 10B

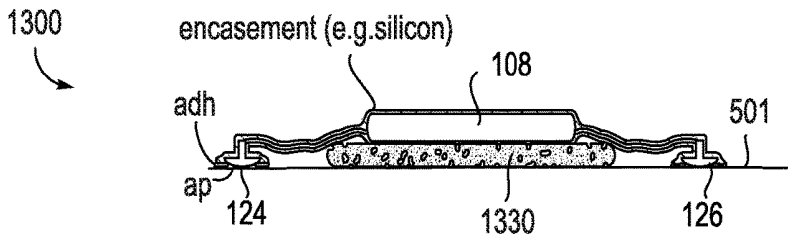


FIG. 11

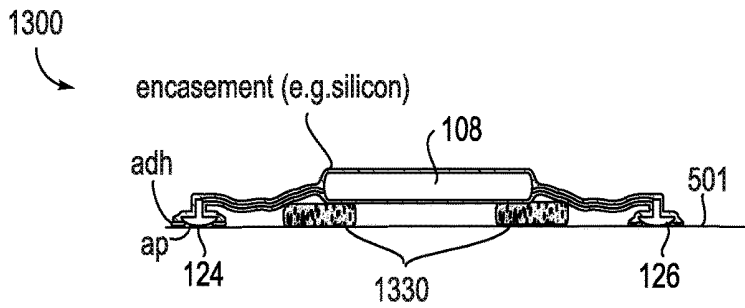


FIG. 12

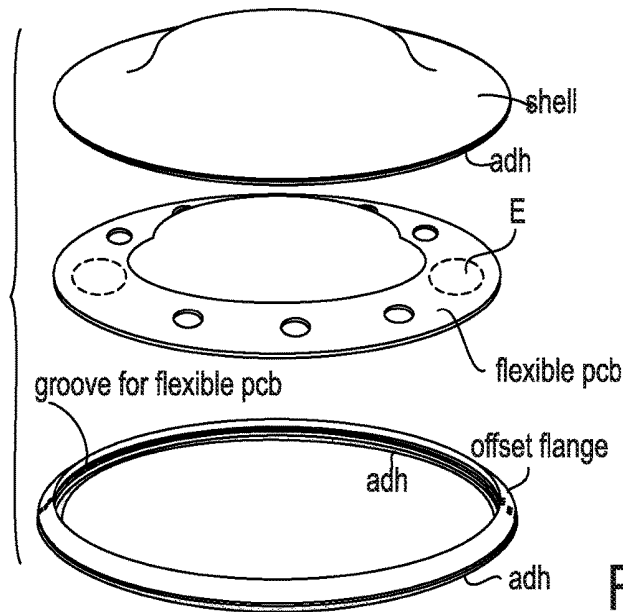


FIG. 13A

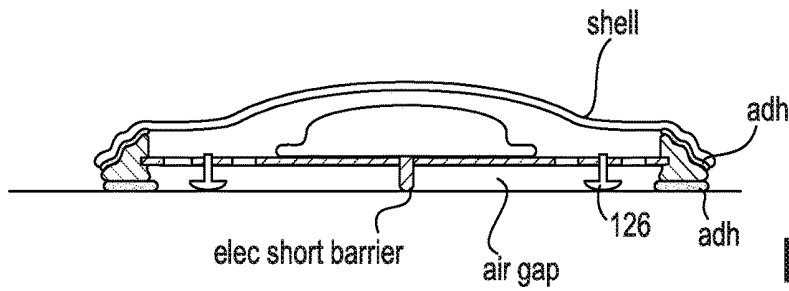


FIG. 13B

DEVICE FEATURES AND DESIGN ELEMENTS FOR LONG-TERM ADHESION

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. application Ser. No. 13/890,144, filed May 8, 2013, now U.S. Pat. No. 9,241,649, titled "Device Features and Design Elements for Long-Term Adhesion" which claims priority to U.S. application Ser. No. 13/563,546, filed Jul. 31, 2012, now U.S. Pat. No. 8,538,503 which claims priority to U.S. patent application Ser. No. 13/106,750, filed May 12, 2011, now U.S. Pat. No. 8,560,046, which claims priority to U.S. Provisional Patent Application No. 61/334,081, filed May 12, 2010, entitled "Device Features and Design Elements for Long-Term Adhesion." The aforementioned applications are all incorporated by reference as if fully set forth herein.

INCORPORATION BY REFERENCE

All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

FIELD OF THE INVENTION

This application relates to devices worn on a body for monitoring, recording, reporting and/or treating the person wearing the device. Improvements in the device design elements and functionality are disclosed for maintaining the device in contact with and operational for extended periods of time, typically longer than 24 hours.

BACKGROUND OF THE INVENTION

The ability to adhere a medical device to a human body for a long-period of time is dependent on a variety of factors. In addition to the type and nature of the adhesive chosen, another factor is the mechanical design of the device. By design, this refers to, but is not limited to, the device shape, size, weight, flexibility, and rigidity. These design elements are influenced by a number of additional factors, including, but not limited to, where on the body the device will attach and the duration of the attachment, moisture conditions in that area, movement conditions in that area, stretching and contraction in that area, interactions with external factors in that area such as clothing, and purposeful and/or inadvertent interaction between the person wearing the device and the device.

As many are typically used on the body for less than 24 hours, devices have not been designed that can withstand longer-term adhesion. Hence, there is a need to implement device features and design elements that have the ability to enhance the likelihood of adhesion of a device to a human body for 24 hours or more, while accommodating the functionality, shape, size, weight, flexibility, and rigidity of a given device.

SUMMARY

In one aspect of the invention, there is an electronic device for long-term adhesion to a mammal. The device has a housing containing an electronic component with a first wing and a second wing integrally formed with the housing.

There is an electrode positioned on a bottom surface of each of the wings with the electrodes electrically connected to the electronic component. An adhesive layer is provided for adhesion to a surface of the mammal. The adhesive layer is coated on a portion of the bottom surface of the wings. The adhesive layer is not coated on the electrode or on a bottom surface of the housing.

The electronic component in any of the devices described herein may include a processor having a memory with computer readable instructions to record signals from the first and second electrodes while the electronic device is attached to the mammal. The processor may be configured to only convert signals from the electrodes to digital signals, filter those signals and then store the signals in memory.

In another aspect, the device includes a flap connected to each of the wings. The flaps may extend below the housing. Additionally or alternatively, the adhesive layer is coated on a bottom surface of the flaps.

In another aspect, the device includes a connector segment. In one aspect, the connector segment configured to connect the flaps together. In other aspects, the connector segment is located at least partially below the housing. Still further, the connector segment is not attached to the housing.

In one alternative, the adhesive layer is coated on a bottom surface of the flap.

In still another aspect, the adhesive for adhesion to a surface of the mammal is an adhesive that can absorb fluids. In another aspect, the adhesive that can absorb fluids is a hydrocolloid adhesive. In another aspect, the adhesive for adhesion to a surface of the mammal is a pressure-sensitive adhesive. The pressure sensitive adhesive is selected from the group consisting of: a polyacrylate, a polyisobutylene, and a polysiloxane. In one alternative, the device includes a diffusion barrier between the adhesive layer and each of the wings. The device may also include an additional adhesive layer and material layer between the wing and the adhesive layer for adhesion to the mammal. The material layer is configured to prevent diffusion of adhesive components from the adhesive layer to the wing. The diffusion barrier may be made from polyester or other suitable synthetic material.

In one aspect of the device, all or substantially all of the electronic components are within the housing. In another aspect, the wing is free from electronic components. In one aspect, the wing is more flexible than the housing. In one alternative, the wings and the housing are made from the same material. In another aspect, the wings and the housing are made from different materials. In another, the wings are made from a fabric. In still another aspect, the material used to make the wings includes a synthetic fiber. In another alternative, the wing and the flap are composed of the same material.

In another alternative, the device includes a hinge portion between the housing and wing. The hinge portion is configured to allow the device to bend between the housing and the wing. In one aspect, the hinge portion exists between a rigid portion of the device and a flexible portion of the device. In one alternative, the rigid portion of the device corresponds to the portion of the housing including the electronics and the flexible portion of the device includes a wing.

In one aspect, the bottom surface of the wing and the bottom surface of the flap are contiguous. In another aspect, the bottom surfaces of the wings, the flap, and the connectors are contiguous. In still other aspects, the flaps and the connector are contiguous.

In another aspect, the connector has at least one hole extending it. The hole may have any of a number of shapes such as circular, oval, round, or triangular.

In one aspect, the housing is thicker at a center of the housing than at edges of the housing.

In another aspect of the device, the housing is unattached to the mammal when the electrodes are in contact with the mammal.

In another alternative aspect of a device for long-term adhesion to a mammal, the device includes a housing with a first wing extending laterally from the housing and a second wing extending laterally from the housing without overlapping the first wing. There is a first electrode positioned on a bottom surface of the first wing and a second electrode positioned on a bottom surface of the second wing. An electronic memory is positioned within the housing. The electronic memory is configured to receive and store electronic signals from the first and second electrodes while the electronic device is attached to the mammal. There is also an adhesive layer on a portion of a bottom surface of the first wing and the second wing. The adhesive is not on a bottom surface of the housing. When the device is worn on the mammal, only the adhesive layer(s) are attached to the mammal.

In one aspect, the portion of the bottom surface of the first wing and the second wing does not include the first and second electrodes. In one device aspect, the first wing, the second wing, and the housing are formed from the same material. In still another, the first wing, the second wing and the housing integrally form a monolithic structure. In other aspects, an angle formed by the first wing, the second wing, and the housing is between approximately 90° and 180°. In one variation, the angle is approximately 180°. In another variation, the angle is approximately 135°.

In still other embodiments, there is a first hinged portion between the first electrode and the processor and a second hinged portion between the second electrode and the housing.

In a further aspect, at least a portion of the body uncovered is not adhered to the mammal when signals from the electrodes are being recorded in memory.

In another aspect, the device includes a first flap connected to the first wing medial to the first electrode and a second flap connected to the second wing medial to the second electrode. Each flap may extend below the housing.

The device may also include a connector segment configured to connect the flaps together. In one aspect, the connector segment is located at least partially below the housing, but is not attached to the housing.

In another aspect, there is an electronic device that has a patch including a housing containing an electronic component. There is an electrode positioned on a bottom surface of the patch, the electrode electrically connected to the electronic component. There is a first adhesive strip extending around the perimeter of the patch and a second adhesive strip extending around the perimeter of the first adhesive strip. In one aspect, the first adhesive cover over the first adhesive strip and a second adhesive cover over the second adhesive strip. The first and second adhesive covers may be configured to be separably removed from the first and second adhesive strips. In one alternative, the first adhesive strip extends between the first and second adhesive covers. In another alternative, the adhesive in the first and the second adhesive strips is an adhesive that can absorb fluids. In still another aspect, the adhesive that can absorb fluids is a hydrocolloid adhesive. In one alternative, the adhesive in the first and the second adhesive is a pressure-sensitive adhesive.

In some aspects, the pressure-sensitive adhesive is a polyacrylate, a polyisobutylene, or a polysiloxane.

In one alternative, the second adhesive strip partially overlaps the first adhesive strip. In another aspect, the second adhesive strip is attached to a shell, the shell overlapping the first adhesive strip.

In still another alternative device for long-term adhesion to a mammal, the device includes a patch having a housing with an electronic component contained therein. There is an electrode positioned on a bottom surface of the patch. The electrode electrically connected to the electronic component. There is a porous foam pad configured to be positioned between the electronic component and the mammal. In one aspect, the porous foam pad comprises a biocompatible foam material. In one variation, the porous foam pad can absorb fluids. In still another aspect, the porous foam pad is attached to the housing. In another, the porous foam pad is configured to be attached to the mammal. In another request, the porous foam pad can absorb fluids.

In one aspect of a method of applying an electronic device, there is a step of removing a first adhesive cover from the first wing of the electronic device to expose an electrode and an adhesive coated on a bottom surface of a first wing. There is a step of placing the exposed electrode into contact with the mammal by adhering the adhesive coated bottom of the first wing to the mammal. There is also a step of removing a second adhesive cover from the second wing of the electronic device to expose an adhesive coated on a bottom surface of the second wing and another exposed electrode. There is also a step of placing the another exposed electrode into contact with the mammal by adhering the adhesive coated bottom of the second wing to the mammal. After performing the removing and the placing steps, the housing is unattached to the mammal, but is held in position on the mammal using the adhesive coated bottoms of the first and the second wings.

In one alternative method of attaching a device, the electronic device includes a first flap connected to the first wing and a second flap connected to the second wing. The first and second flaps each extend below the housing. The step of removing a first adhesive cover from the first wing may also include exposing an adhesive coated on a bottom surface of the first flap. The step of removing a second adhesive cover from the second wing may also include exposing an adhesive coated on a bottom surface of the second flap.

In another alternative method of attaching a device, after performing the removing and the placing steps, the housing is held in position on the mammal using only the adhesive coated bottoms of the first wing, the second wing, the first flap and the second flap.

In an alternative aspect of a method of applying an electronic device to a mammal for long-term adhesion, the method includes removing a first adhesive cover from the first wing of the electronic device to expose an electrode and an adhesive coated on a bottom surface of the first wing. There is also a step of removing a second adhesive cover from the second wing of the electronic device to expose an adhesive coated on a bottom surface of the second wing and another exposed electrode. There is a step of placing the exposed electrodes into contact with the mammal by adhering the adhesive coated on the bottom of the first and the second wings to the mammal. After performing the removing and the placing steps, the housing is unattached to the mammal, but is held in position on the mammal using the adhesive coated bottoms of the first and the second wings.

There is also provided a method of applying an electronic device to a mammal for long-term adhesion wherein the electronic device includes a patch. The patch includes an electronic component along with an electrode positioned on a bottom surface of the patch and electrically connected to the electronic component. There is a first adhesive strip extending around the perimeter of the patch and a second adhesive strip extending around the perimeter of the first adhesive strip. One aspect of a method of applying the device includes a step of removing an adhesive cover from the second adhesive strip of the electronic device. There is a step of applying pressure to the second adhesive strip to adhere the second adhesive strip to the mammal such that the electrode is in contact with the mammal. Then, after a period of time, removing an adhesive cover from the first adhesive strip of the electronic device. Next, there is the step of applying pressure to the first adhesive strip to adhere the first adhesive strip to the mammal such that the electrode remains in contact with the mammal.

In another alternative method of applying an electronic device to a mammal for long-term adhesion, the electronic device includes a patch, an electronic component, and an electrode positioned on a bottom surface of the patch and electrically connected to the electronic component. There is a first adhesive strip extending around the perimeter of the patch. The method includes a step of applying pressure to a first adhesive strip to adhere the first adhesive strip to the mammal such that the electrode is in contact with the mammal. After a period of time, placing a second adhesive strip around the perimeter of the first adhesive strip. Then there is the step of applying pressure to the second adhesive strip to adhere the second adhesive strip to the mammal such that the electrode remains in contact with the mammal.

Any of the above described devices may include additional aspects. A device may also include a first wire connecting the first electrode and the processor or an electronic memory and a second wire connecting the second electrode and the processor or an electronic memory. The first and second wires extend within the body and the first and second wings. In one aspect, the first and second wires extend within and are completely encapsulated within the body and the first and second wings. In one aspect, a conduit is provided within the body and the wings and the wires pass through the conduit. In one alternative, the conduit extends from the processor or electronic memory to an electrode so that the wire is completely within the conduit. In still other aspects of the devices described above, the first and second wires connecting the electrodes to the processor or electronics each include slack between the electrode and the processor. In one aspect, the slack is located in a portion of each wing that is configured to bend or flex. In another aspect, the slack is a portion of the wire within the wing and at least partially coiled about the first or the second electrode. In still other aspects, the slack is provided by a portion of the wire formed into a coil, a wave pattern, or a sinusoidal pattern along its length the connection point on the electronics to the connection point on the electrode.

In still other alternatives, the devices described above may be applied to any of a wide variety of conventional physiological data monitoring, recording and/or transmitting devices. Any of the improved adhesion design features and aspects may also be applied to conventional devices useful in the electronically controlled and/or time released delivery of pharmacological agents or blood testing, such as glucose monitors or other blood testing devices. Additional alternatives to the devices described may include the specific components of a particular application such as electronics,

antenna, power supplies or charging connections, data ports or connections for down loading or off loading information from the device, adding or offloading fluids from the device, monitoring or sensing elements such as electrodes, probes or sensors or any other component or components needed in the device specific function. In still other aspects, the electronic component in any of the above devices is an electronic system configured for performing, with the electronic signals of the mammal detected by the electrodes, one or more or any combination of or the following electronic functions: monitoring, recording, analyzing, or processing using one or more algorithms electronic signals from the mammal. Still further, any of the devices described above may include appropriate components such that the device is used to detect, record, process or transmit signals or information related to signals generated by a mammal to which the device is attached including but not limited to signals generated by one or more of EKG, EEG and/or EMG.

BRIEF DESCRIPTION OF THE DRAWINGS

The novel features of the invention are set forth with particularity in the claims that follow. A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are utilized, and the accompanying drawings of which:

FIG. 1 is a top view of a patch having two wings;

FIG. 1A is a representative cross-section of an embodiment of the patch in FIG. 1;

FIG. 1B is a representative cross-section of another embodiment of the patch in FIG. 1;

FIG. 1C is a representative cross-section of another embodiment of the patch in FIG. 1;

FIG. 1D is a representative cross-section of another embodiment of the patch in FIG. 1;

FIG. 1E is a representative cross-section of another embodiment of the patch in FIG. 1;

FIG. 1F is a top view of a patch having three wings illustrating an alternative electrode-electronics-electrode orientation;

FIG. 2A is a schematic drawing of the electronics contained within a patch;

FIG. 2B is a schematic drawing of a patch with wiring having slack in the form of undulations between electronics and electrodes;

FIG. 2C is a schematic drawing of a patch with wiring having slack in the form of a coil between electronics and electrodes;

FIG. 3 is the bottom view of a patch having adhesive thereon;

FIG. 4A shows a patch as worn by a person rolled to the side;

FIG. 4B shows a patch as worn by a person playing golf;

FIG. 5A shows a patch in response to a concave bend of the skin;

FIGS. 5B and 5C show a patch in response to a convex bend of the skin;

FIG. 6A is a bottom view of a patch having a connector between two flaps;

FIG. 6B is a cross-section of the patch of FIG. 6A;

FIG. 7A is a bottom view of a patch having multiple covers forming strips of adhesive;

FIG. 7B is a cross-section of the patch of FIG. 7A;

FIG. 8A is a bottom view of a patching having multiple covers forming strip of adhesive around each electrode;

FIG. 8B is a cross-section of the patch of FIG. 8A;

FIGS. 9A and 9B show a patch having multiple layers formed thereon;

FIGS. 10A and 10B show a patching having multiple layers formed thereon, each layer having multiple patches of adhesive;

FIG. 11 shows a patch having an open cell support;

FIG. 12 shows a patch having an annular open cell support;

FIG. 13A shows a patch having a protective shell thereon; and

FIG. 13B shows a cross-section of the patch of FIG. 13A.

DETAILED DESCRIPTION

The following device features and design elements can be implemented into any device being adhered to the human body for a long-period of time, typically greater than 24 hours. As an example, the following device features and design elements can be used for long-term adhesion of a cardiac rhythm monitoring patch ("patch") to the chest of a person.

Referring to FIGS. 1 and 1A, a patch 100 for long term adhesion includes a housing 102. The housing 102 can be formed from any flexible, durable material, such as a biocompatible polymer, for example silicone. The housing 102 can include electronic components 108 therein. As shown in FIG. 2, the electronics 108 can include a printed circuit board 220, a battery 225, and a communications port mounted on the printed circuit board 220. The printed circuit board 220 can include analog circuits 210, digital circuits 215, and an activation or event notation button or switch 130. The electronics 108 can be used, for example, to record continuous physiological signals from a mammal wearing the patch 100. A system for continuously recording data is described further in co-owned U.S. application Ser. No. 11/703,428, filed Feb. 6, 2007, the entire contents of which are incorporated by reference herein.

As shown in FIGS. 1 and 1A, wings 104, 106 can be connected to the housing 102. The wings 104, 106 can be integral with the housing 102 and, in some embodiments, can be formed of the same material as the housing 102. The wings 104, 106 can be more flexible than the electronic components 108, which can be substantially rigid. An electrode 124, 126 can extend through a bottom surface of each wing 104, 106. The electrodes can be positioned to detect an ECG of a mammal wearing the patch 100 for processing by the electronics 108. For example, the electrodes can be more than 2 cm apart, such as more than 3 cm apart, for example at least 6 cm apart. The electrodes 124, 126 can be integral with the wings 104, 106 so as to be inseparable from the wings 104, 106 when the patch is in use.

For a patch 100 that is entirely flexible and can conform, stretch, and adapt to the movement and conditions of the chest underneath the device, adhesive can be placed over the entire surface of the device that is in contact with the body, except for areas where sensors, electronics, or others elements such as electrodes are interacting with the body related to the functioning of the device may be incorporated. Thus, as shown in FIG. 3, an adhesive layer 166 can coat the bottom of the patch 100 for attachment to the skin. For a patch 100 in which there may be some areas that are not completely flexible and may not be able to stretch or contract (e.g., the electronics 108), adhesive may be excluded from the portion of the patch 100 underneath these areas. Thus, for example, the bottom surface 302 of the housing 102, which contains the electronics, can remain free from adhesive.

As shown in FIG. 1 A, by not coating adhesive on a bottom surface of the housing 102, the housing 102 can float above the adhered portions, allowing for increased flexibility of the patch, as will be discussed further below. Further, as shown in FIG. 3 the bottom surface of the electrodes 124, 126 can remain free of adhesive. For example, a ring 362 without adhesive can be formed around each electrode 124, 126 to separate the electrodes from the adhesive 164. The adhesive can be, for example, a pressure-sensitive adhesive, such as polyacrylate, polyisobutylene, or a polysiloxane. Alternatively, the adhesive can be a hydrocolloid which advantageously absorbs water.

The wings 104, 106 and the housing 102 can form a smooth, contiguous outer surface to the patch 100. As shown in FIG. 1 A, when viewed from the top, the housing 102 and wings 104, 106 can together form an oblong substantially oval shape. Further, the housing 102 can have a thickness that is greater than the thickness of the wings 104, 106. The housing 102 and each of the wings 104, 106 when viewed in profile, can each form a dome with a height that is greater at the center than at the ends of the respective component, i.e. some or all of the components can be tapered at the ends and/or sides.

The electronics 108 can extend along only a portion of the distance between the electrodes 104, 106. For example, the electronics can occupy less than 90% of the distance between the electrodes, for example less than 80%. By having the electronics 108 in a relatively limited space between the electrodes 124, 126, the flexibility of the patch 100 can be increased.

The housing 102 can provide a watertight enclosure 110 for electronic components 108 of the patch 100. The electronics 108 can be unattached to the housing 102 such that the electronics 108 are free to move within the watertight enclosure 110. Allowing the relatively rigid electronics 108 to move freely within the flexible housing 102 advantageously enhances the overall flexibility of the patch 100. The wings 104, 106 can each have a watertight enclosure 114, 116 formed therein, which can be contiguous with the watertight enclosure 110 of the housing 102.

Wiring 120 or other suitable electrical connections can connect the electrodes 124, 126 with the electrical components 108 of the housing. In some embodiments, as shown in FIGS. 1B-1E, the contiguous nature of the enclosure 110 and the enclosures 114, 116 allows the wiring 120 to extend within the patch 100 from the electrodes 124, 126 to the electronic components 108. In other embodiments, one or more channels, tubes, or conduits are provided between the housing 102 and the wings 104, 106, to provide space for the wiring 120. The tube or channel may be straight or curved. In use, the wire 120 positioned in the enclosures 110, 114, 116 or in the tube or channel may move relative thereto in order to remain flexible within the housing. In one aspect, the flexible channels or tubes are formed within the device housing so that the housing, as it is being stretched, does not affect the ability of the components, such as wires, that may connect more rigid structures, to move or elongate.

As shown in FIG. 1, the wire 120 is straight with a direct line of connection between the electrodes 124, 126 and the electronics 108. FIG. 1 illustrates an embodiment where the length of the wires 120 connecting the electrodes 124, 126 to electronics 108 are about the same distance as the spacing between the electrode connection point on electronics 108 and the electrodes 124, 126. FIG. 1F also illustrates a straight line type connection where wire 120 length is nearly the same as the spacing between the electronics 108 and the electrodes 124, 126. However, as a patient moves, the patch

100 flexes along with patient movement. As shown in FIGS. 4B and 5C, patch flexion may be severe and is likely to occur during long term monitoring. In order to address the possible dislocation or breakage of the wire 120, the length or shape of the wire 120 may be selected to permit patch flexion to occur with little risk of wire 120 pulling from the electrode or electronics. Numerous alternatives are possible to compensate for patch flexion. Exemplary confirmations include undulations or zig-zags 231 as shown in FIG. 2B, coils 233 as shown in FIG. 2e, or a configuration that partially or fully wraps around an electrode. In some embodiments, other components, such as the circuit board or electrodes, can alternatively or additionally contain additional length to help accommodate stretch or displacement. When the patch 100 is attached to a mammal, the slack in the wiring 120 allows the patch 100 to flex while not placing stress on the wiring 120.

While the illustrated embodiments of FIGS. 1A-1D show only two wings and show the electrodes and electronics in a direct line in an approximate 180 degree alignment of electrode 124 to electronics 108 to electrode 126, other configurations are possible. For example, as shown in FIG. 1F, the wings 104, 106 are arranged in an orientation less than 180 degrees. In the illustrated embodiment, the angle formed by the electrodes and the electronics is about 135 degrees. Other ranges are possible so long as electrode spacing is provided to permit ECG monitoring. The orientation of the wings 104, 106 to the housing 102 also illustrates the use of an additional adhesive tab 105. Tab 105 is shown as a semicircular extension of the body 102. The bottom of tab 105 can include adhesives as described herein and is used to provide additional anchoring of the patch to the patient. The tab 105 may be formed in any of a number of different shapes such as rectangles, ovals, loops or strips. Further, in some embodiments, the tab 105 can function similar to a wing, e.g., include an electrode therethrough that connects to the electronics 108.

Referring to FIGS. 1A-1D and 2B-2C, a hinge portion 194,196 in the patch 100 can extend between each electrode 124, 126 and the electronics 108. The hinge portions 194, 196 can have a thickness less than the thickness of surrounding portions of the patch 100. For example, if the hinge portions 194, 196 are in the wings 104, 106, then the thickness can be less than adjacent portions of the wings. Likewise, the hinge portions 194, 196 can have a width less than adjacent portions of the patch 100, e.g., less than adjacent portions of the wings 104, 106. Alternatively, the hinged portion can be formed by the adjunct between a rigid portion, i.e. the electronics 108, and a more flexible portion. The hinged portion allows the patch 100 to bend between the housing 102 and wings 104, 106 to compensate for any movement caused by the patient. As shown in FIGS. 2B and 2C, the slack in the wiring 120 can be placed at or proximal to the hinge portions 194, 196 to allow for bending at the hinge portions 194, 196 without pulling or breaking the wiring 120.

Referring to FIGS. 4A and 4B, having adhesive on the bottom of the patch 100 except in the areas substantially around the electrodes and directly underneath the housing 102 can create a floating section 455 over the skin of the mammal to which the patch 100 is attached. The floating section 455 can house the more rigid or less flexible electronic components while the flexible wings 104, 106 can be adhered to the skin and provide the flexibility necessary to hold the patch 100 in place. As a result of this selective use of adhesive areas and non-adhesive areas, the limitation on device flexibility imposed by the less flexible floating sec-

tion can be mitigated or reduced by hounding the floating section with one or more adhered flexible areas. The flexible sections can thus adhere to the body if the underlying portion of the body is stretched and/or contracted while the floating section is free to move above the skin, for example if the person wearing the device rolls over (as shown in FIG. 4A) or is involved in activities that can otherwise cause movement of the skin (as shown in FIG. 4B).

Referring back to FIGS. 1B-1E, each wing 104, 106 can include a material layer 214,216 between the adhesive 164, 166 and the wings 104, 106. The material layer 214,216 can be, for example, a polyester layer. The material layer 214, 216 can be attached to the patch 100 with a layer of adhesive 204,206. The adhesive 204, 206 can be the same as the adhesive 164, 166 or different. For example, the adhesive 204, 206 could be a silicone adhesive. The material layer 214 can serve as a barrier to prevent diffusion or migration of adhesive components, such as a tackifier, from the adhesive 164, 166 into the wings 104, 106 or housing 102. The material layer 214 can thus advantageously serve to maintain the strength of the adhesive 104, 106 over time.

Referring still to FIGS. 1B-1E, the patch 100 can further include a first flap 154 connected to the first wing 104 and a second flap 156 connected to the second wing 106. The flaps 154, 156 can both extend from a position on the wings 104, 106 medial to the electrodes to a position below the housing 102, such as below the electronics 108. The flaps 154, 156 can remain unattached to the housing 102. As a result, gaps 144, 146 can be formed between the flaps 154, 156 and the housing 102. The gaps can provide additional "floating" for the housing 102 and the relatively rigid components 108 contained therein.

In some embodiments, shown in FIG. 1B, the flaps 154, 156 can be attached to the wings 104, 106 with adhesive 134, 136. The adhesive 134, 136 can be the same as the adhesive 164, 166 or different. For example, the adhesive 134, 136 could be a silicone adhesive. In other embodiments, shown in FIGS. 1C-1E, the flaps 154, 156 can be integral with the wings 104, 106. For example, the flaps 154, 156 can be solvent welded to and/or formed during the molding process of the wings 104, 105 such that hinges 194, 196 form below the wings 104, 106. Additionally or alternatively, one or more of the flaps 154, 156 may be separably attached to the wings 104, 106. In wings 104, 106, shown in FIGS. 1B and 1C, the materials making up the flaps 154, 156 can extend all the way to the lateral edge of the patch 100. In other embodiments, shown in FIG. 1D, a flap can extend on each side of the electrodes, i.e. one flap can extend medially and the other laterally. In some embodiments, the lateral and medial-extending flaps are part of the same annular flap. In other embodiments, shown in FIG. 1E, the flaps and materials making up the flaps extend only from a position medial to the electrodes underneath the housing.

The Flaps 154, 156 may be positioned in virtually any relationship to the adhered flexible area such that, when attached in use, the attachment of the flap or flaps effectively counteracts the expected external forces acting on the device, specifically those forces that may dislodge the adhered flexible areas. Further, in embodiments such as that shown in FIG. 1F where there are more than two wings, there can be a flap corresponding to each additional wing.

The adhesive layers 164, 166 can coat all or a portion of the bottom of each of the flaps 154, 156. In some embodiments, the adhesive 164, 166 extends continuously from the bottom surface of the wings 104, 106 to the bottom surface of the flaps 154, 156, except for areas proximate to the electrodes 124, 126. Further, the top surface of the flaps 154,

156, i.e. the surface closest to the housing 102, can remain free of adhesive to ensure that the housing 102 remains floating. In some embodiments, the only portion of the patch 100 including adhesive for adhesion to the skin can be the flaps 154, 156.

Referring to FIGS. 5A-5C, the naps 154, 156, can provide hinge-like behavior for the patch 100. Thus, as shown in FIG. 5A, if the skin 501 is stretched or bent in a concave manner, the gaps 144, 146 between the flaps 154, 156 and the housing 102 can approach zero such that the patch 100 can sit substantially flat on the skin 501. As shown, the hinge portions 194, 196 between the housing 102 and wings 104, 106 can provide additional flexibility for concave bends by flattening as the patch 100 is stretched. In contrast, as shown in FIGS. 5B and 5C, as the skin 501 is bent in an increasingly convex manner, the gaps 144, 146 between the flaps 154, 156 and the housing 102 can increase, thereby allowing the flexible wings 104, 106 to remain adhered to the skin and the rigid housing 102 to float above skin. As shown, the hinge portions 194, 196 between the housing and the wings 104, 106 can provide additional flexibility for convex bends by folding inward as the patch 100 is bent.

When placed substantially flat on the skin 501, the patch 100 can have a height that extends no more than 2 cm off of the skin, such as no more than 1.5 cm off of the skin, when lying flat on the patient and no more than 4 cm, such as no more than 2 cm off of the skin when floating above the skin. The relatively low height of the patch 100 can enhance long-term adhesion by reducing the potential for the patch 100 to snag or rip off of the skin.

Advantageously, the flaps 154, 156 can function as anchors for adhesion that mitigates shear force. The flaps 154, 156 can provide a different direction for the acute and chronic forces being experienced by the device due to stretching, contraction, or torsion to be spread out over both the flap as well as the flexible adhesive areas. Further, by pre-aligning the orientation of the floating section, adhered flexible area and the flaps, the device may be better able to tolerate (i.e., remain attached to the body and in use) and/or tailor the interaction with the forces acting on the device in order to better withstand the acute or chronic forces being experienced by the device. Tailoring the response of the device to the expected forces is one

Because the flaps can be used to counteract forces acting on a particular device, it is to be appreciated that the dimensions, flexibility, attachment technique, and/or orientation between a flap and another component may vary depending upon the purpose of a particular flap. Accordingly, a flap may have the same or different characteristics from another flap or component of the device. In one aspect, at least one flap is more flexible than the other flaps in a particular device. In another aspect, each of the flaps has similar flexibility. In still another aspect, at least one flap is more flexible than the device component to which it is attached or from which it originates. In still another aspect, at least one flap is less flexible than the device component to which it is attached or from which it originates.

Referring to FIGS. 6A and 6B, in one embodiment, the flaps 154, 156 may be augmented by a connector segment 607 used to join the flaps together. The connector segment 607 can extend below the housing 102, but remain unattached to the housing 102. As shown in FIG. 6A, the flaps 154, 156 and the connector 607 can together form a butterfly shape. In one embodiment, the connector segment 607 and the flaps 154, 156 are formed from a single piece of material. The connector segment 607 can be made of the same material as the flaps 154, 156 or of different material. In one

embodiment, the bottom surface of the connector is covered with adhesive. In another embodiment, the bottom surface of the connector does not include any adhesive. Further, as shown in FIG. 6B, the connector segment 607 can be thicker in the middle, under the housing 102, than near the edges, i.e., closer to the electrodes. The variable thickness can help prevent the connector segment 607 from capturing moisture thereunder. The connector segment 607 can advantageously prevent the device from flipping when attached to the patient

The connector segment 607 can include one or more holes 614, 616. In some configurations, the connector segment may trap moisture and/or inadvertently stick to the body. The holes 614, 616 can advantageously minimize the potential for undesired sticking or moisture collection. The size, shape and placement of the holes mitigate or reduce the collection of moisture and/or undesired adhesive still providing a connector with sufficient structural integrity (i.e. the connector allows the flaps to be connected to one another in order to prevent them from folding). Additionally or alternatively, the connector holes could also be made to preferentially allow forces to be distributed along certain axes of the connector in order to further maximize the ability of the device to adhere long-term in the face of significant acute and chronic forces due to stretching, contraction, and torsion.

Adhesive can be selectively applied to the connector and/or naps to provide the desired body attachment locations depending upon the specific use of the device. For example, one piece of material including flaps and the connector can be adhered along two or more edges and/or with adhesive only covering certain areas. In another aspect, at least a portion of the skin-contacting surface of the unitary nap connector structure does not include any adhesive. Additionally or alternatively, the connector segment incorporating the flaps may be integral parts of the larger device housing (e.g. could be molded as part of the device housing or enclosure).

In some embodiments, the patch 100 can include one or more release liners to cover parts of the adhesive prior to adhesion. As is particular to devices having multiple adhesive areas and/or multiple adhesive components (i.e., flaps and flexible sections), the manner of applying the device may be specifically detailed in order to ensure that the device and the adhesive portions are properly engaged. In one particular aspect, the release liners are removed in a particular order to minimize the likelihood that the device adhesive is misapplied. For example, a portion of the adhesive may be exposed first and used to affix the device to the body. Thereafter, a second set of adhesive liners may be removed to expose and affix one or more flaps to the body. A stepwise adhesive exposure method may be implemented during device application such that elements, such as the one or more flaps do not fold on themselves, for example.

Breaking up the areas in which the adhesive is used to adhere the device, whether it be splitting it up to rigid areas, to create flaps, to create connector segments with holes, of any of the other techniques described above may also have benefits in terms of preventing moisture bridges that could act as conducting pathways between electrical sensing elements, such as electrodes. Bridges of moisture could short-circuit electrical connections and/or prevent the proper functioning of the device, particularly if the device has an electrical function, such as sensing via electrodes.

In some applications, a long-duration patch may experience excessive forces due to acute (quick and/or rapid) or chronic (slow and/or prolonged) contraction, stretching, or torsion. In such applications, the hinge points between a

floating rigid section and flexible adhered sections may be modified in order to align with and counteract or mitigate the predominant direction of the force acting on the patch. In some device situations or configurations, the strength and direction of the acute or chronic force may be so strong that the forces imparted on the device adhesive surfaces or components may be distributed differently in addition to or as an alternative to the hinge described above.

Further, the device construction can be made in such a way that the housing is fashioned so that the axes of the housing are structured and placed along or against the direction of various forces, possibly during certain states, such as sleeping, so that the device itself can help counteract these forces and improve long-term adhesion.

Advantageously, the patch described herein can provide long-term adhesion to the skin. Having the various flexible portions and/or hinged portions can compensate for stressed caused as the skin stretches or bends, while allowing the rigid portion to float about the skin. As a result, the devices described herein can adhere to the skin substantially continuously for more than 24 hours, such as greater than 3 days, for example, greater than 7 days, greater than 14 days, or greater than 21 days.

Another mechanism for adhering a patch to the skin long-term is described with respect to FIGS. 7-10. As shown in the embodiments of FIGS. 7-10, one or more parts of the patch are used in a temporary fashion in order to improve adhesion. The adhesive used in the embodiments described below can include a hydrocolloid or a pressure-sensitive adhesive, such as polyacrylate, polyisobutylenes, or polysiloxane.

In one embodiment, shown in FIGS. 7A and 7B, the patch 700 can be surrounded with an adhesive 760 having multiple covers 701, 703, 705 thereon that can be peeled away in a sequence to expose strips of adhesive 760 underneath. The covers 701, 703, 705 can be concentric with one another and be configured to be pulled off separately and sequentially starting from the inside of the patch 700. Each additional exposed area of adhesive 760 can increase the adhesion life of the patch 700. Although only three covers are shown in FIG. 7A, other numbers, such as 2, 4, 5, or more are possible. Further, each electrode 124, 126 of the patch 700 can include a barrier 714, 716 to protect the electrodes 124, 126 from shortage.

In another embodiment, shown in FIGS. 8A and 8B, each electrode 124, 126 can be surrounded by a patch of adhesive 864, 866. Accordingly, a set of covers 801, 803, 805, 807 can be positioned sequentially around each of the electrodes 124, 126 over the adhesive 864, 866. The covers 801, 803, 805, 807 can be concentric with one another and be configured to be pulled off sequentially starting from the inside. Each additional exposed strip of adhesive 864, 866 can increase the adhesion life of the patch 100. Although only four covers are shown in FIG. 8A, other numbers, such as 2, 3, 5, or more are possible. Further, each electrode 124, 126 of the patch 800 can include a barrier 814, 816 to protect from shortage.

Referring to FIGS. 9A-9B, in other embodiments, shells or layers 901, 902, 903 can extend over all or a portion of the patch 900. Each layer 901, 902, 903 can include a strip of adhesive 962 on the bottom surface and an adhesion guard 982 protecting the adhesive. As shown in FIG. 913, as the patch 900 is worn over a period of time, the layers 901, 902, 903 can be sequentially removed. As a new layer is exposed, the adhesive guard 982 of that layer can be peeled away such that the adhesive 962 of the new layer can be used to adhere the patch 900 to the skin. In a similar embodiment, referring

to FIGS. 10A-10B, each of the layers 1001, 1002, 1003 can include multiple portions of adhesive to help adhere the layer to both the skin and the patch itself. As with the embodiments of FIGS. 7-8, the number of layers in the embodiments of FIGS. 9 and 10 can vary. For example, there can be 2, 3, 4, or 5 or more layers.

In some embodiments, the layers or covers of the embodiments described herein can be added to the device over time to improve adhesion. Further, the multiple layers or covers of the embodiments described herein can be partially overlapped. Further, in some embodiments, the strips of adhesive can be overlapped.

Advantageously, the use of multiple covers or layers can assist in the adhesive performance of a base or core device because the added surface area or adhesive force of the combined outer layer aids in preventing layer pull away and/or may act to spread forces being experienced away from the core device by spreading those forces over a larger area.

Referring to FIGS. 11 and 12, an open cell structured support 1330 or porous foam can be used to support a more rigid or less flexible portion 1302 of the patch 1300. As shown in FIG. 11, the open cell structured support 1330 can fully fill an area below the rigid portion 1302. Alternatively, as shown in FIG. 12, the open cell structured support 1330 can be an annular shape or have some other configuration that includes spaces between adjacent portions of the support. The open cell structured support 1302 may be attached to both the skin and to the rigid portion, to only the rigid portion, or to only the skin. Because of the open cell structure of the support, the flexible movement of the skin can be absorbed by the structure entirely or partially such that the rigid portion does not impact or has a reduced impact on the ability of the device to accommodate movement and remain affixed. In addition, the open cell support may have a thickness selected to enhance patient comfort so that the more rigid portion of a device does not push against the skin. In one aspect, the open cell structure is a biocompatible foam material. In another aspect, the open cell material is positioned between an electronics module on the device and the skin when worn by a patient. The open cell support can advantageously absorb fluids to keep the electrodes from shorting.

Referring to FIG. 13, the patch can have a shell design. Adhesive can be placed on the perimeter edge of the bottom ring. The circuit board and electrode unit can be dropped into the bottom ring, and a shell can be dropped on top of the circuit board and electrode. The perimeter adhesive can create a watertight chamber therein.

The shape of a particular electronic device embodiment may vary. The shape, footprint, perimeter or boundary of the device may be a circle or circular (see FIG. 13A), an oval (see FIG. 1A, 2A), a triangle or generally triangular (see FIG. 1F) or a compound curve. Examples of a device embodiments having a compound curve shape are shown in FIGS. 2B, 2B, 3, 6A, 7A, and 8A. In some embodiments, the compound curve includes one or more concave curves and one or more convex curves. FIG. 3 illustrates a device having a convex surface along the top (where reference 102 indicates), a concave surface along the bottom and convex shaped edges around the electrodes 124, 126. FIGS. 2B and 2C illustrate a device embodiment having a convex shape on either side of the electronics 108 and around the electrodes 124, 126. The convex shapes are separated by a concave portion. The concave portion is between the convex portion on the electronics and the convex portion on the electrodes,

In some embodiments, the concave portion corresponds at least partially with a hinge, hinge region or area of reduced.

While described in the context of a heart monitor, the device adhesion improvements described herein are not so limited. The improvement described in this application may be applied to any of a wide variety of conventional physiological data monitoring, recording and/or transmitting devices. The improved adhesion design features may also be applied to conventional devices useful in the electronically controlled and/or time released delivery of pharmacological agents or blood testing, such as glucose monitors or other blood testing devices. As such, the description, characteristics and functionality of the components described herein may be modified as needed to include the specific components of a particular application such as electronics, antenna, power supplies or charging connections, data ports or connections for down loading or off loading information from the device, adding or offloading fluids from the device, monitoring or sensing elements such as electrodes, probes or sensors or any other component or components needed in the device specific function. In addition or alternatively, devices described herein may be used to detect, record, or transmit signals or information related to signals generated by a body including but not limited to one or more of EKG, EEG, and/or EMG.

What is claimed is:

1. An electronic device for long-term adhesion to a mammal, the device comprising:
 - a housing;
 - a physiologic data collection circuit contained in the housing;
 - a plurality of wings extending from the housing;
 - an electrode positioned on a bottom surface of each of the wings, the electrodes electrically connected to the physiologic data collection circuit;
 - each wing comprising a first adhesive layer positioned on a bottom surface of the wing, wherein the first adhesive layer provides adhesion to the skin of the mammal; and
 - each wing comprising a second adhesive layer functioning as an adhesion guard protecting the first adhesive layer; the second adhesive layer positioned over a top of the wing and extending horizontally outward beyond a boundary of each wing.
2. The device of claim 1, wherein the first adhesive layer is not on a bottom surface of the housing.
3. The electronic device of claim 1, wherein the wings are more flexible than the housing.
4. The electronic device of claim 1, wherein the wings and the housing are made from the same material.
5. The electronic device of claim 1, wherein the wings and the housing are made from different materials.
6. The electronic device of claim 1, further comprising a hinge portion adjacent the housing.
7. The electronic device of claim 1, further comprising a flap connected to each wing, the flaps extending below the

housing but not directly attached to a bottom surface of the housing, wherein the first adhesive layer extends onto a bottom surface of each flap.

8. The electronic device of claim 7, further comprising a connector segment configured to connect the flaps together without directly attaching to the bottom surface of the housing.
9. The electronic device of claim 1, wherein the first adhesive layer comprises an adhesive that can absorb fluids.
10. The electronic device of claim 1, wherein the first adhesive layer comprises a hydrocolloid adhesive.
11. The electronic device of claim 1, wherein the first adhesive layer comprises a pressure-sensitive adhesive.
12. The electronic device of claim 11, wherein the pressure sensitive adhesive is selected from the group consisting of a polyacrylate, a polyisobutylene and a polysiloxane.
13. The electronic device of claim 1, further comprising: an additional adhesive layer between each wing and the first adhesive layer; and a synthetic material layer between the wing and the first adhesive layer.
14. The electronic device of claim 1, wherein the physiologic data collection circuit is configured to collect cardiac rhythm data from the mammal.
15. The electronic device of claim 1, wherein each wing comprises a fabric or synthetic fiber layer.
16. The electronic device of claim 15, wherein the fabric or synthetic fiber layer is positioned over the first adhesive layer.
17. The electronic device of claim 1, further comprising a third adhesive layer positioned between the first adhesive layer and the second adhesive layer.
18. The electronic device of claim 1, wherein the second adhesive layer covers the entirety of the wing.
19. A device for monitoring cardiac rhythms of a mammal, the device comprising:
 - a floating section configured to move toward and away from the body of a mammal;
 - two skin-adhering sections extending out from the floating section;
 - an electrode integral with a bottom surface of each skin-adhering section and disposed along the bottom surface of each skin-adhering section;
 - each skin-adhering section comprising a first adhesive layer on the bottom surface of the skin-adhering section, wherein the first adhesive layer provides adhesion to the skin of the mammal; and
 - each skin-adhering section comprising a second adhesive layer functioning as an adhesion guard protecting the first adhesive layer, the second adhesive layer positioned over a top of the skin-adhering section and extending horizontally outward beyond a boundary of each skin-adhering section.

* * * * *

专利名称(译)	设备特征和设计元素，用于长期粘合		
公开(公告)号	US10405799	公开(公告)日	2019-09-10
申请号	US15/005854	申请日	2016-01-25
申请(专利权)人(译)	IRYTHM TECHNOLOGIES, INC.		
当前申请(专利权)人(译)	IRHYTHM TECHNOLOGIES, INC.		
[标]发明人	KUMAR UDAY N LIVINGSTON PETER H DAY MARK J PARK SHENA HAE WILLIS WILLIAM F RIGHTER WILLIAM H		
发明人	KUMAR, UDAY N. LIVINGSTON, PETER H. DAY, MARK J. PARK, SHENA HAE WILLIS, WILLIAM F. RIGHTER, WILLIAM H.		
IPC分类号	A61B5/00 A61B5/0408 A61B5/0478 A61B5/04 A61B5/0488 B31B50/62		
CPC分类号	A61B5/0408 A61B5/0478 A61B5/04085 A61B5/04087 A61B5/6832 A61B5/6833 A61B5/0488 A61B2560/0406 A61B2560/0468 Y10T156/10 A61B5/68335		
优先权	61/334081 2010-05-12 US		
其他公开文献	US20160135746A1		
外部链接	Espacenet		

摘要(译)

一种用于长期粘附到哺乳动物的电子装置包括具有电子元件的壳体。电子设备可包括第一机翼和第二机翼，每个机翼与壳体一体地形成。电极位于每个翼的底表面上，电极电连接到电子元件。提供粘合剂层以粘附到哺乳动物的表面。粘合剂层可以覆盖翼的底表面的一部分，但通常不覆盖电极或壳体的底表面。将电子设备应用于哺乳动物的方法包括从电子设备的第一和第二翼移除第一和第二粘合剂覆盖物以暴露电极和涂覆在每个翼的底表面上的粘合剂。

