


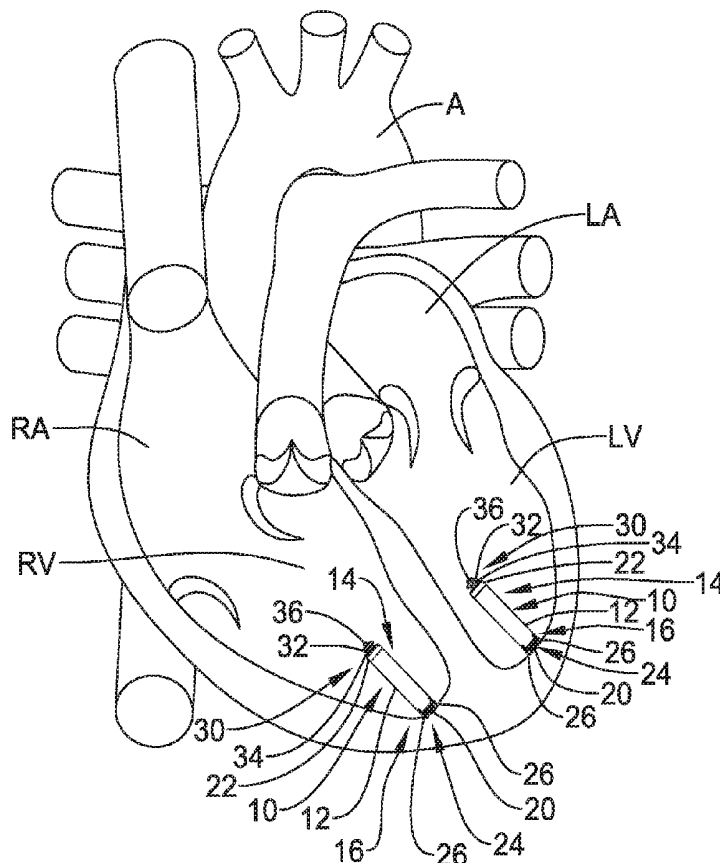

US 20180117304A1

(19) **United States**(12) **Patent Application Publication**
Koop et al.(10) **Pub. No.: US 2018/0117304 A1**(43) **Pub. Date: May 3, 2018**(54) **IMPLANTABLE MEDICAL DEVICE
DELIVERY SYSTEM WITH INTEGRATED
SENSOR**(22) Filed: **Oct. 25, 2017****Related U.S. Application Data**(71) Applicant: **CARDIAC PACEMAKERS, INC.**, St.
Paul, MN (US)(60) Provisional application No. 62/413,748, filed on Oct.
27, 2016.**Publication Classification**(72) Inventors: **Brendan Early Koop**, Ham Lake, MN
(US); **Yinghong Yu**, Shoreview, MN
(US); **Qi An**, Blaine, MN (US); **Keith
R. Maile**, New Brighton, MN (US);
Pramodsingh Hirasingh Thakur,
Woodbury, MN (US); **Bin Mi**,
Plymouth, MN (US); **Jeffrey E.
Stahmann**, Ramsey, MN (US);
Viktoria A. Averina, Shoreview, MN
(US); **Krzysztof Z. Siejko**, Maple
Grove, MN (US); **Michael J. Kane**, St.
Paul, MN (US); **Allan Charles Shuros**,
St. Paul, MN (US); **Arjun D. Sharma**,
St. Paul, MN (US); **Brian Soltis**, St.
Paul, MN (US)(51) **Int. Cl.**
A61N 1/05 (2006.01)
A61B 5/00 (2006.01)
(52) **U.S. Cl.**
CPC *A61N 1/056* (2013.01); *A61N 1/37288*
(2013.01); *A61B 5/686* (2013.01); *A61B*
5/0031 (2013.01)(57) **ABSTRACT**

A delivery and deployment device may include a handle assembly and a shaft extending distally from the handle assembly. A device containment housing may be coupled to a distal region of the shaft and may extend distally therefrom. The distal containment housing may be configured to accommodate at least a portion of the IMD therein. The IMD may, for example, be a leadless pacemaker, a lead, a neurostimulation device, a sensor or any other suitable IMD. A plurality of electrodes may be distributed about an exterior surface of the device containment housing such that at least some of the plurality of electrodes may be positioned to test a potential IMD deployment location before deploying the IMD.

(73) Assignee: **CARDIAC PACEMAKERS, INC.**, St.
Paul, MN (US)(21) Appl. No.: **15/793,149**

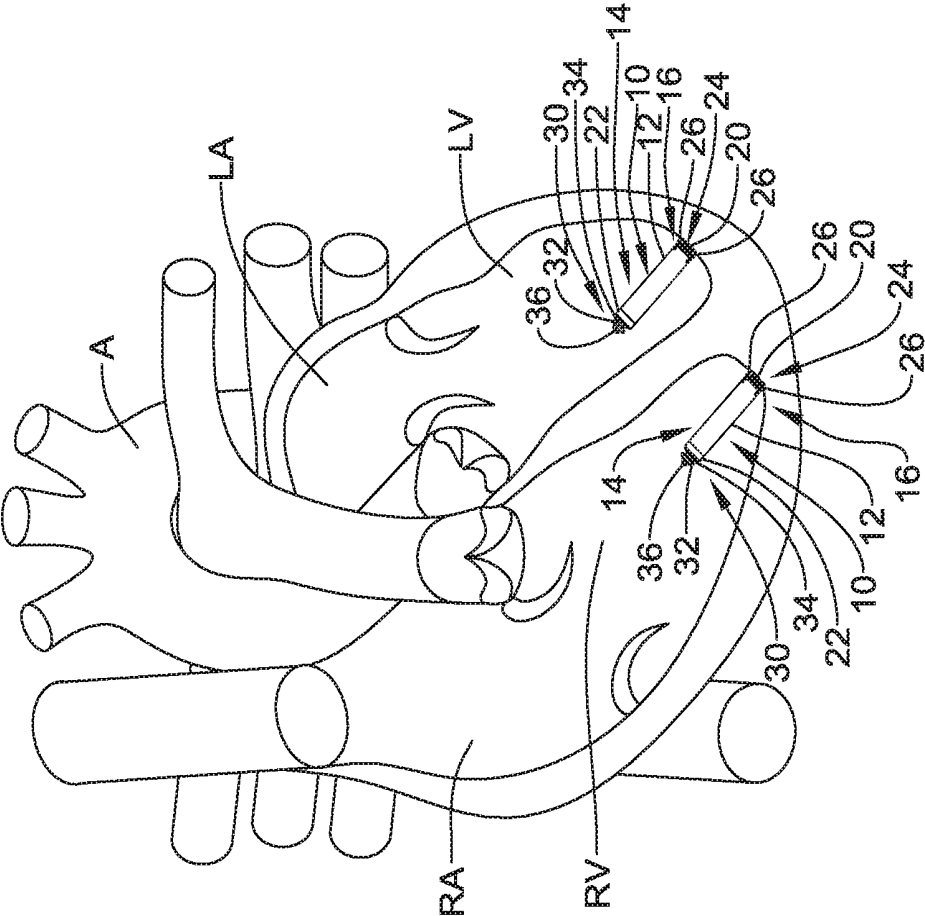


FIG. 1

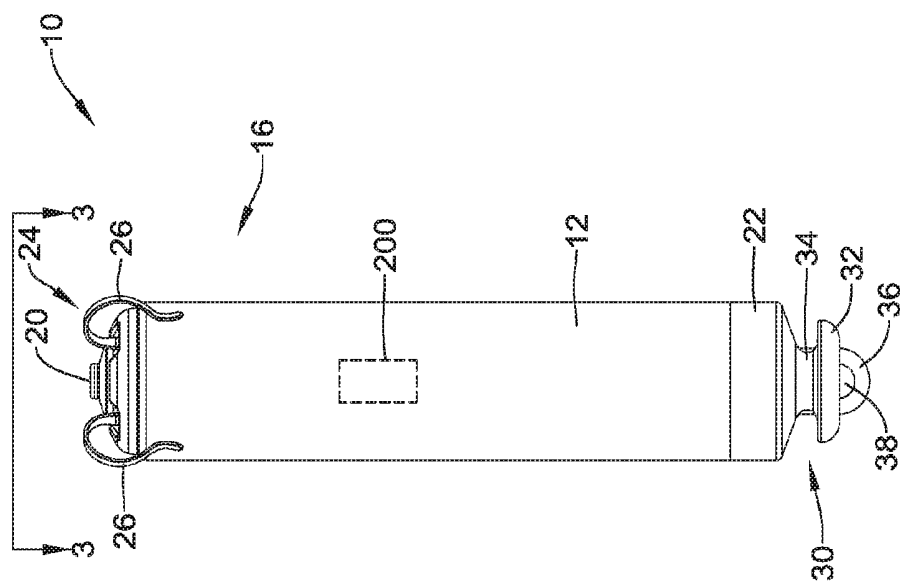


FIG. 2

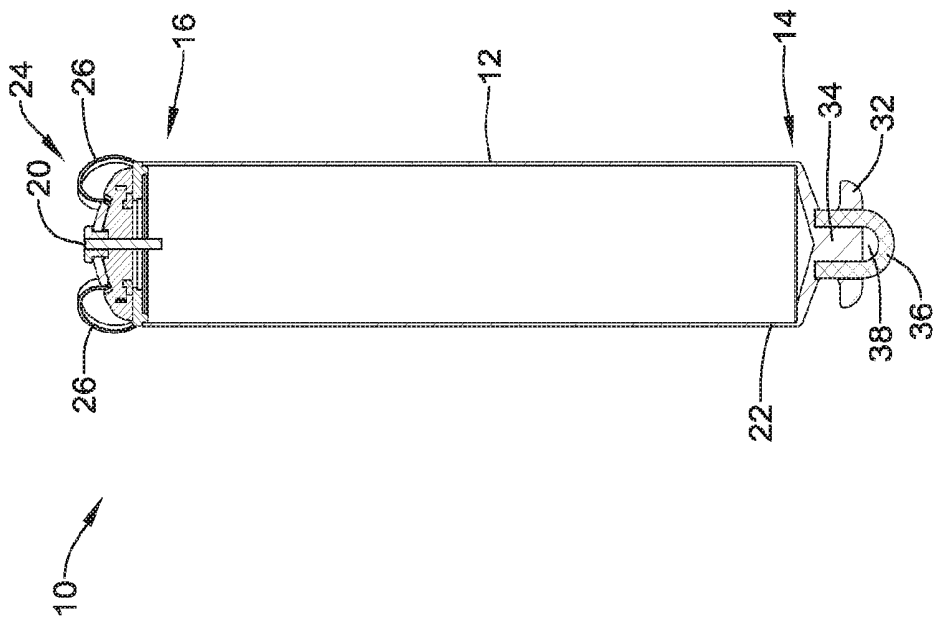


FIG. 3

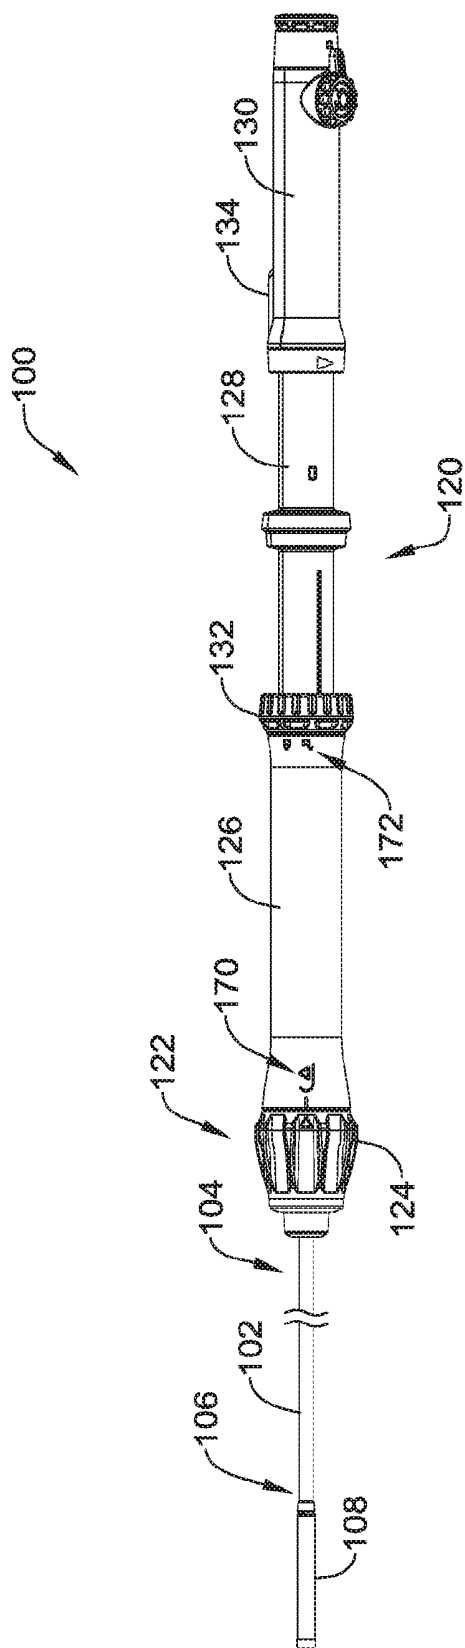


FIG. 4

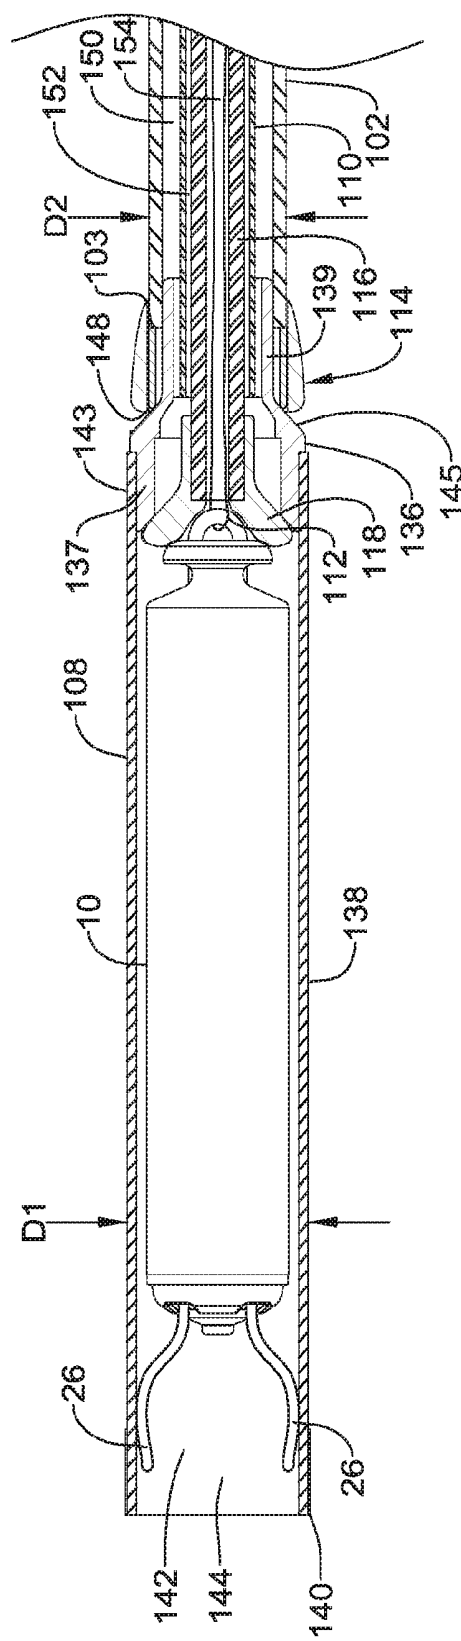
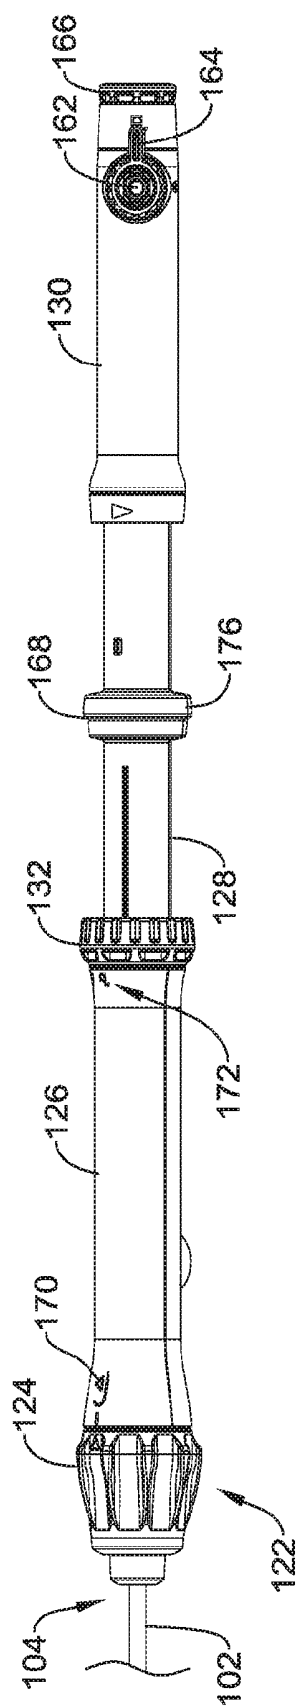


FIG. 5

COL




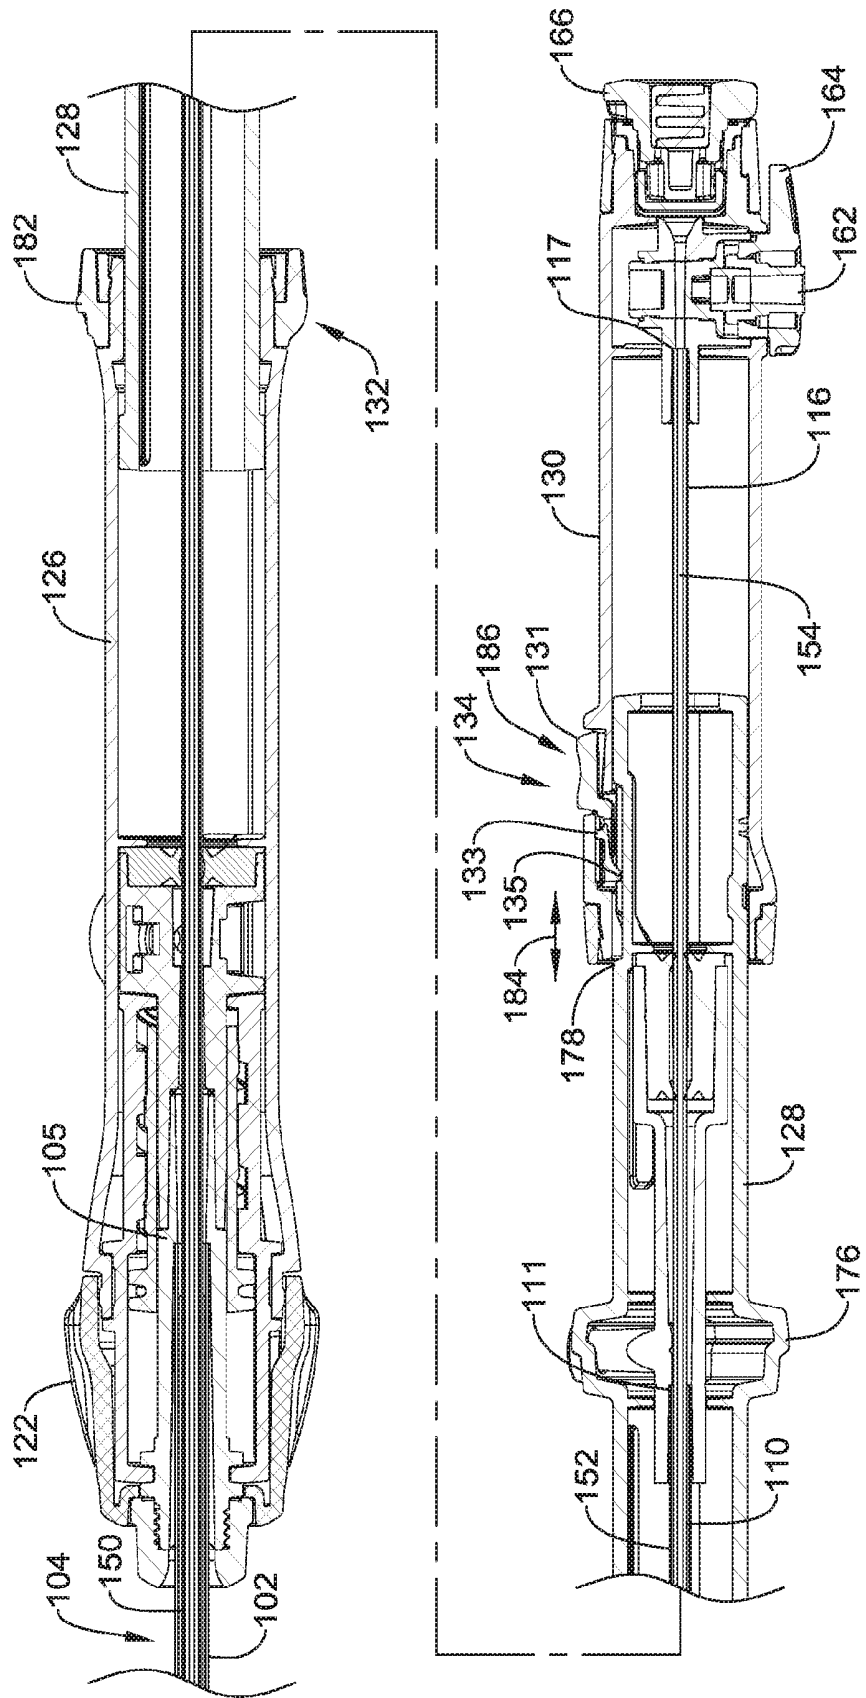


FIG. 8

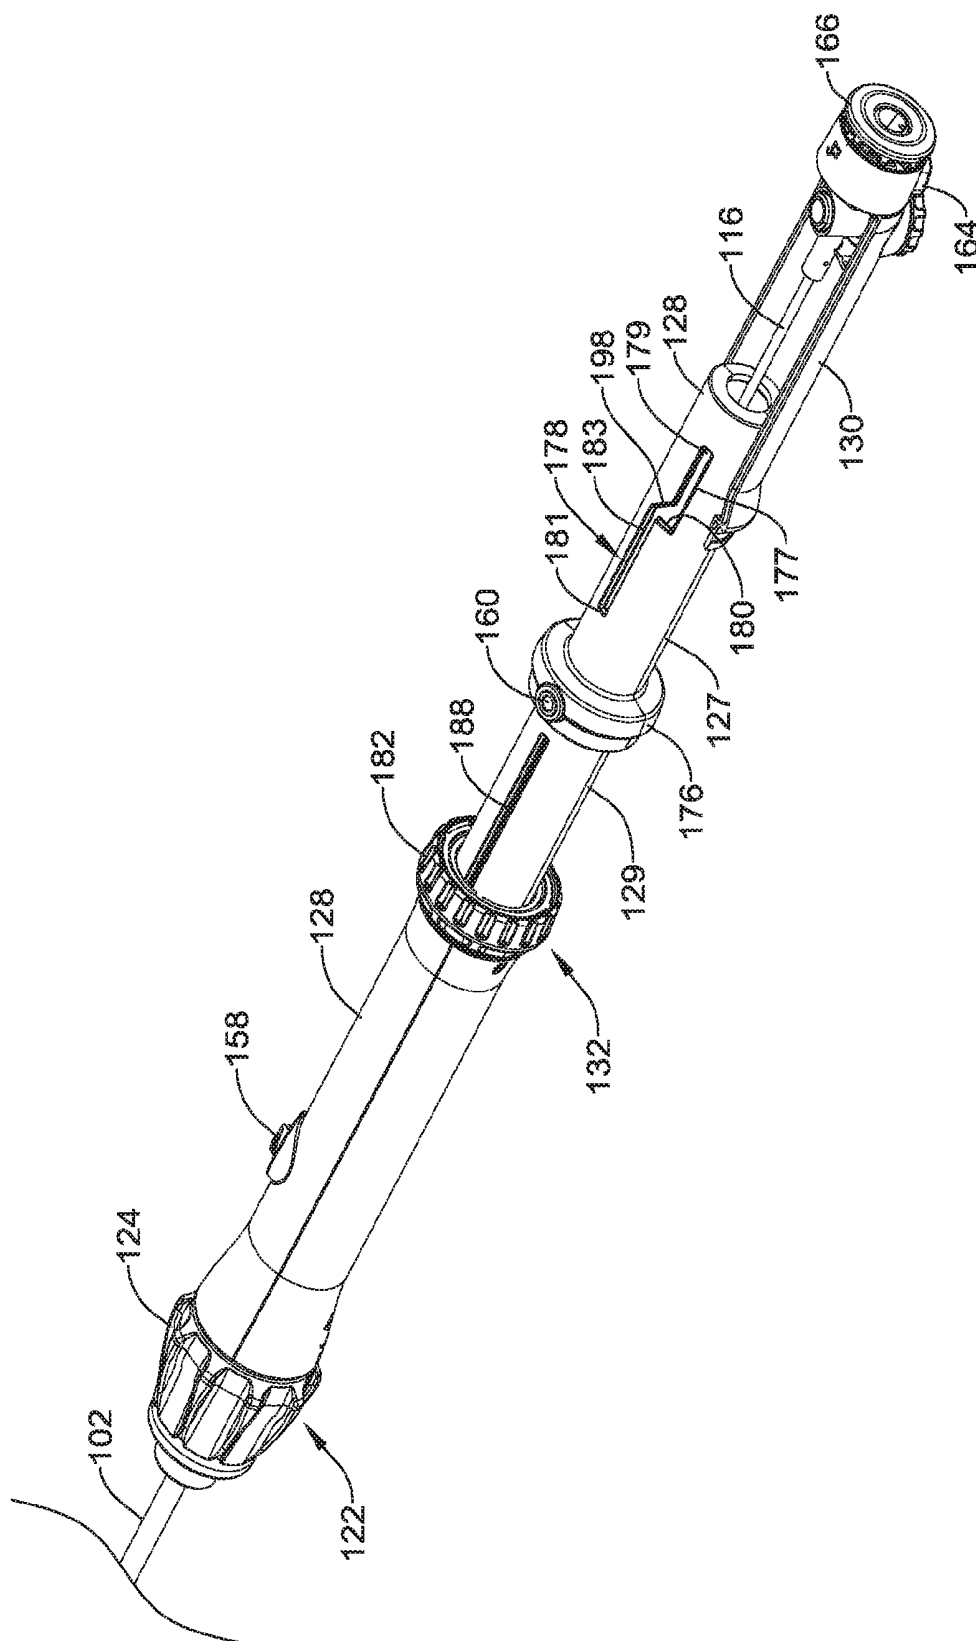

9
K
G
—
L

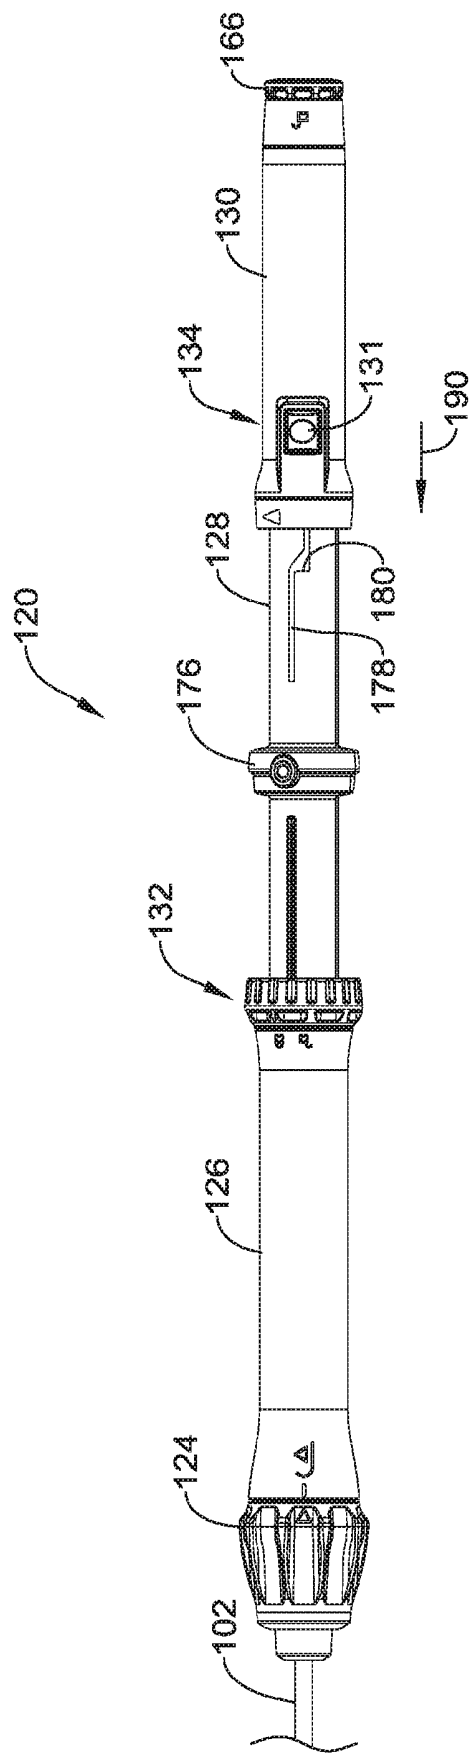
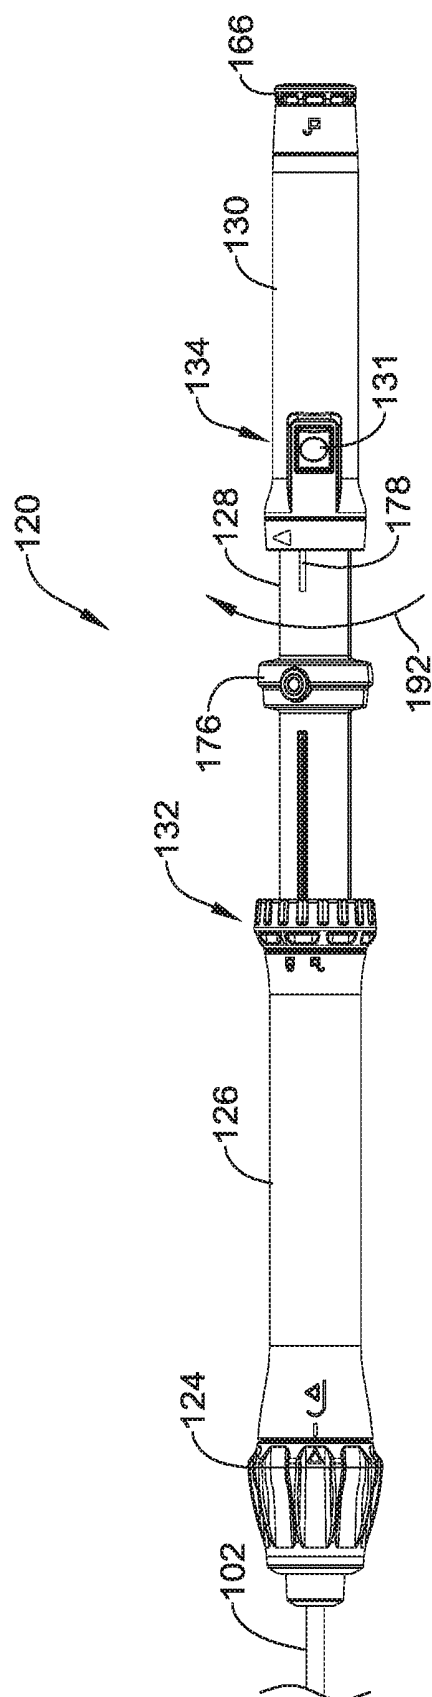
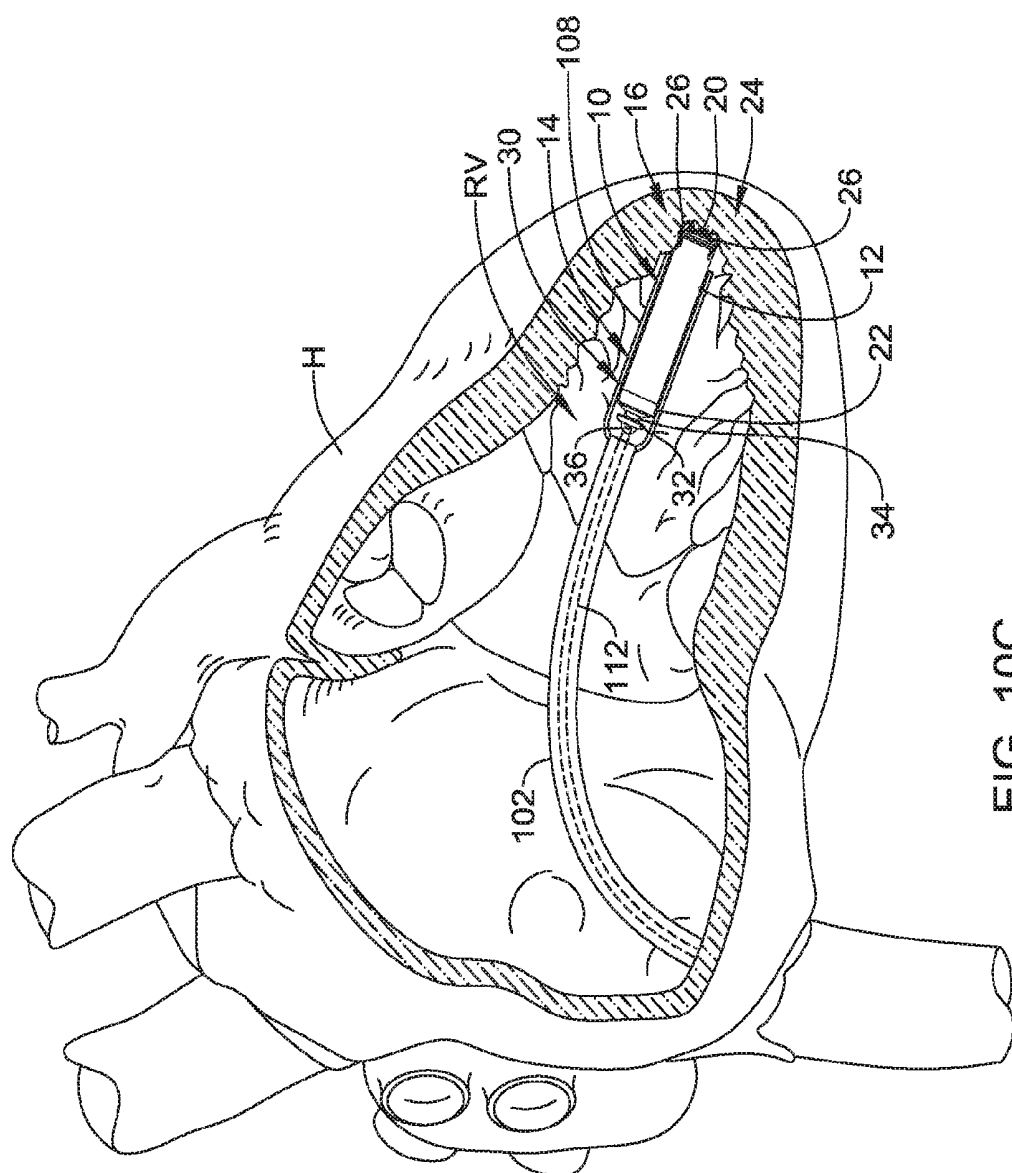


FIG. 10A

100% GLE[®]





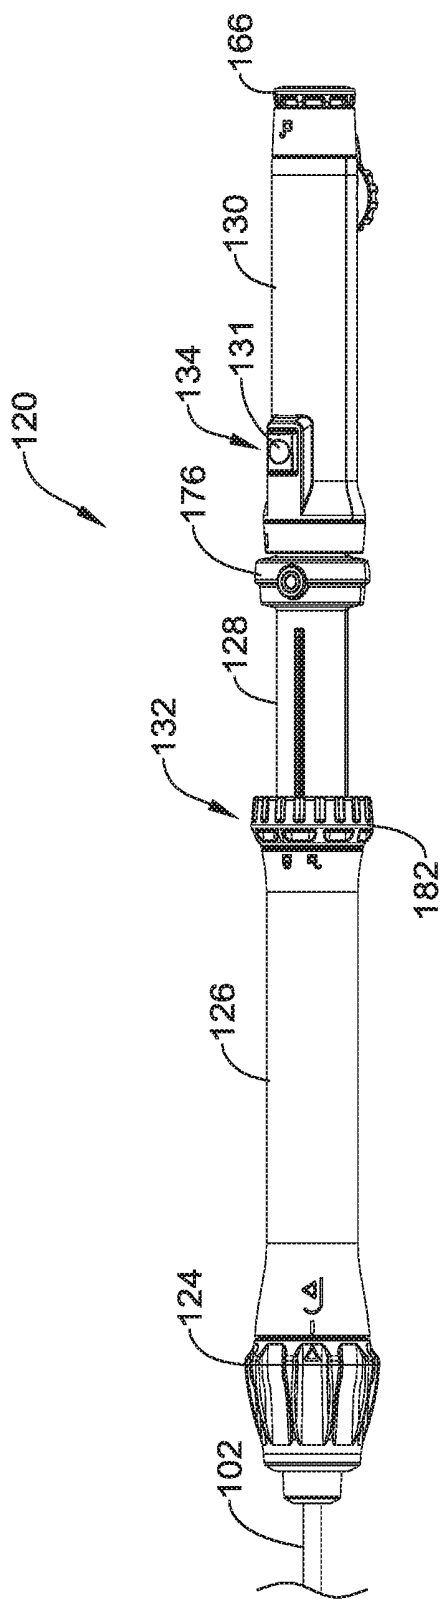


FIG. 10D

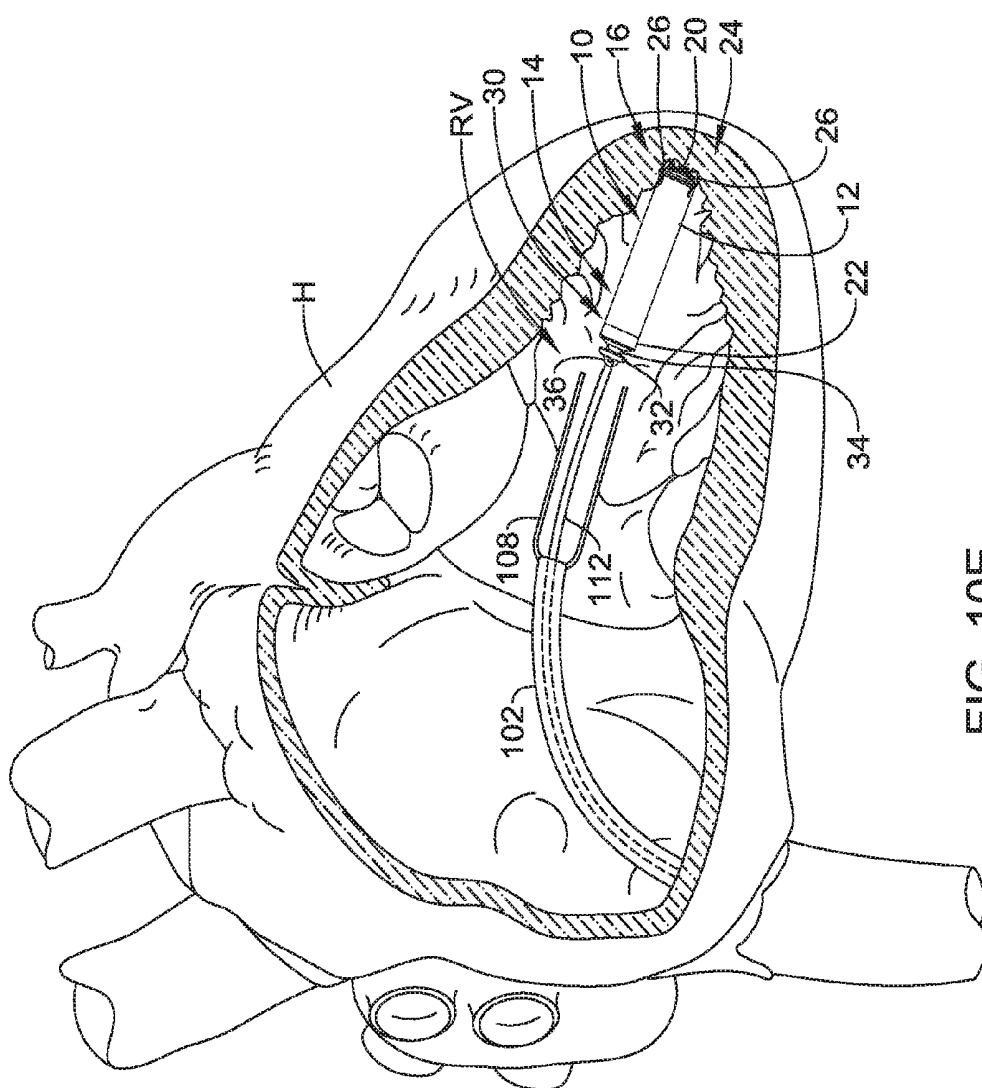

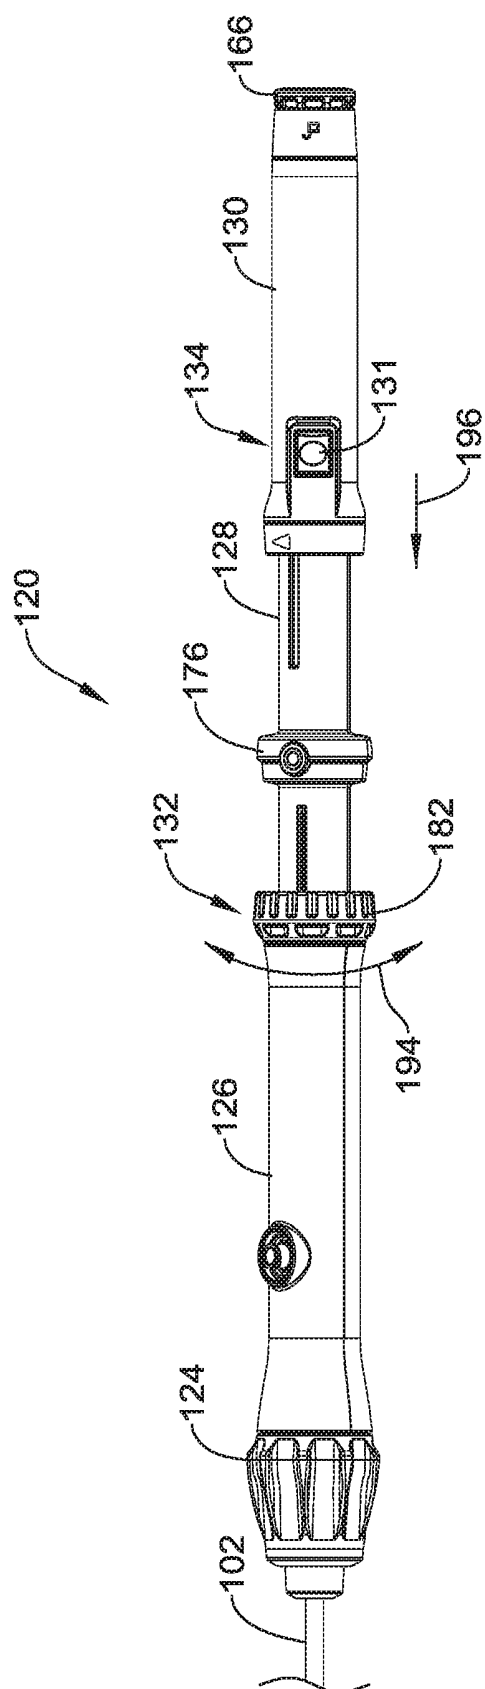

ATL 5 GLE

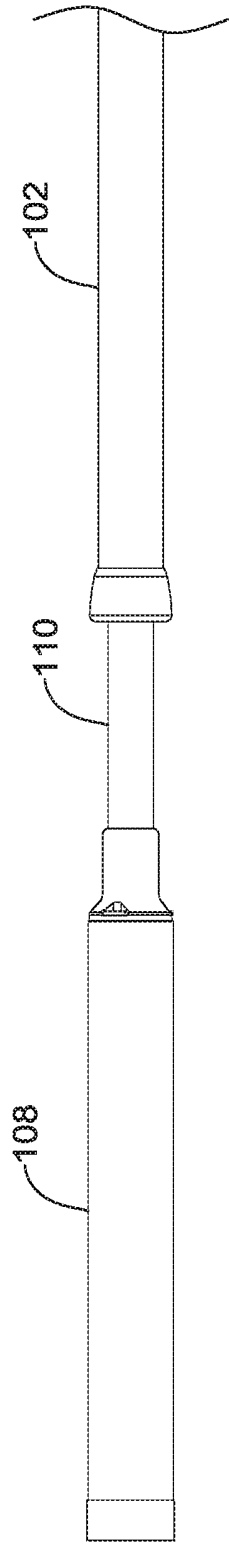


FIG. 11B

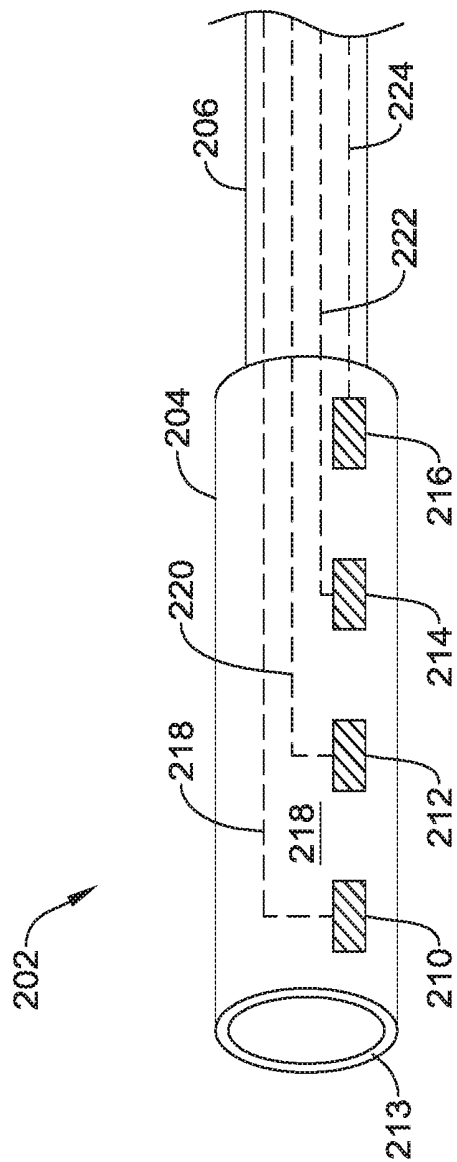


FIG. 12

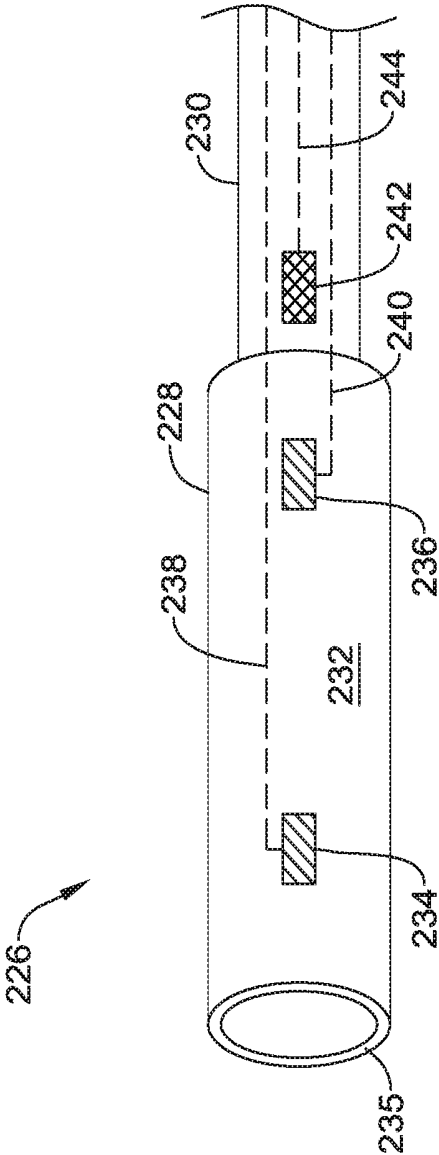


FIG. 13

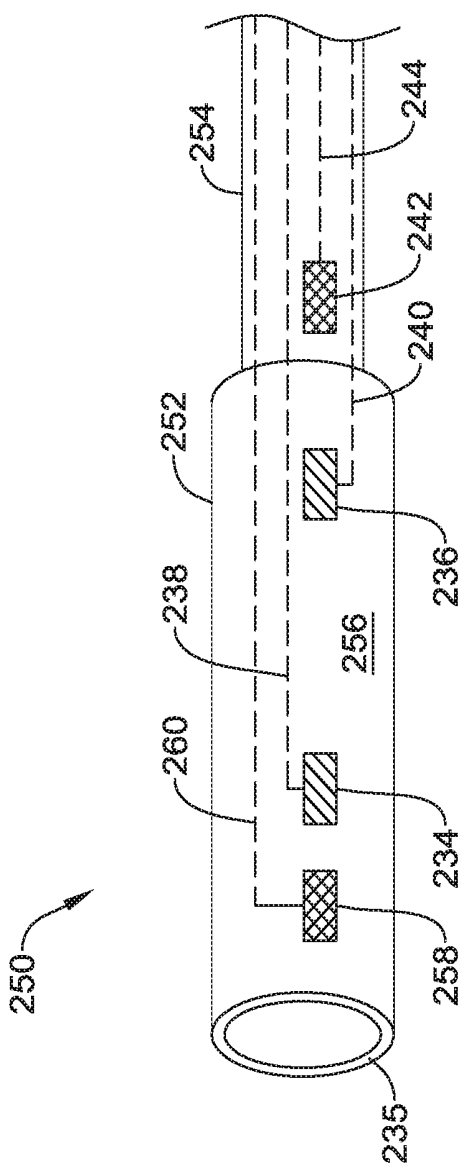


FIG. 14

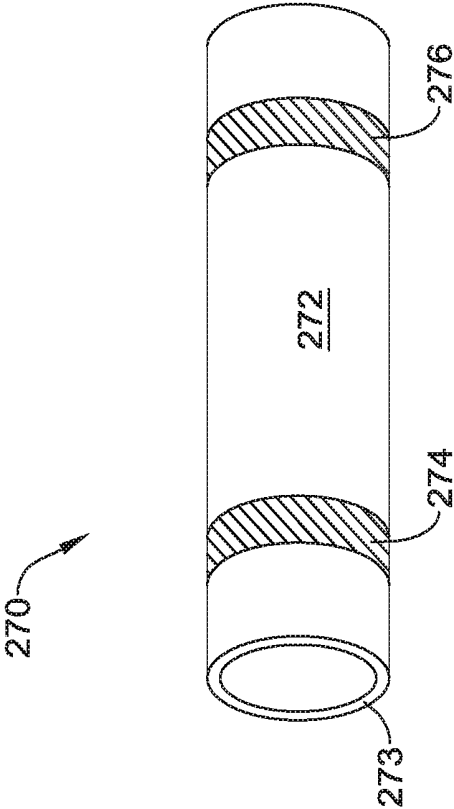


FIG. 15

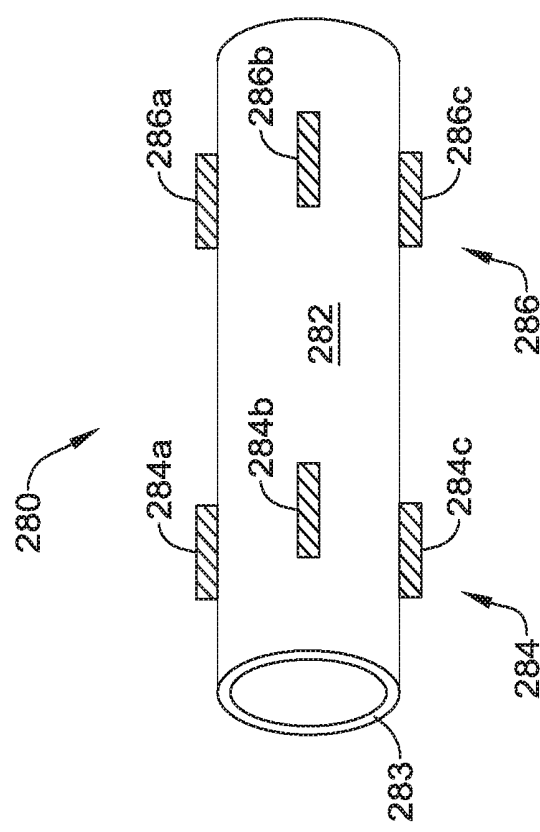


FIG. 16

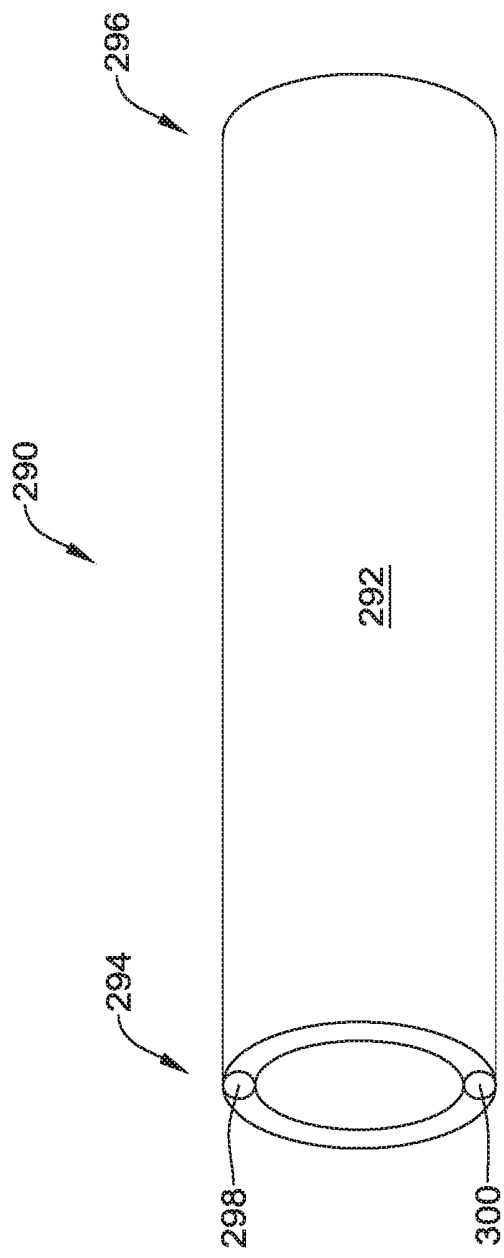


FIG. 17

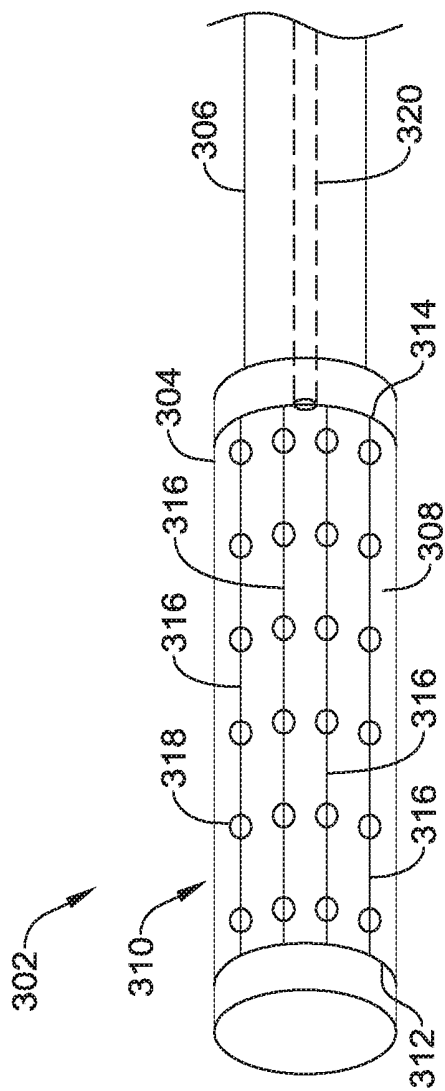


FIG. 18

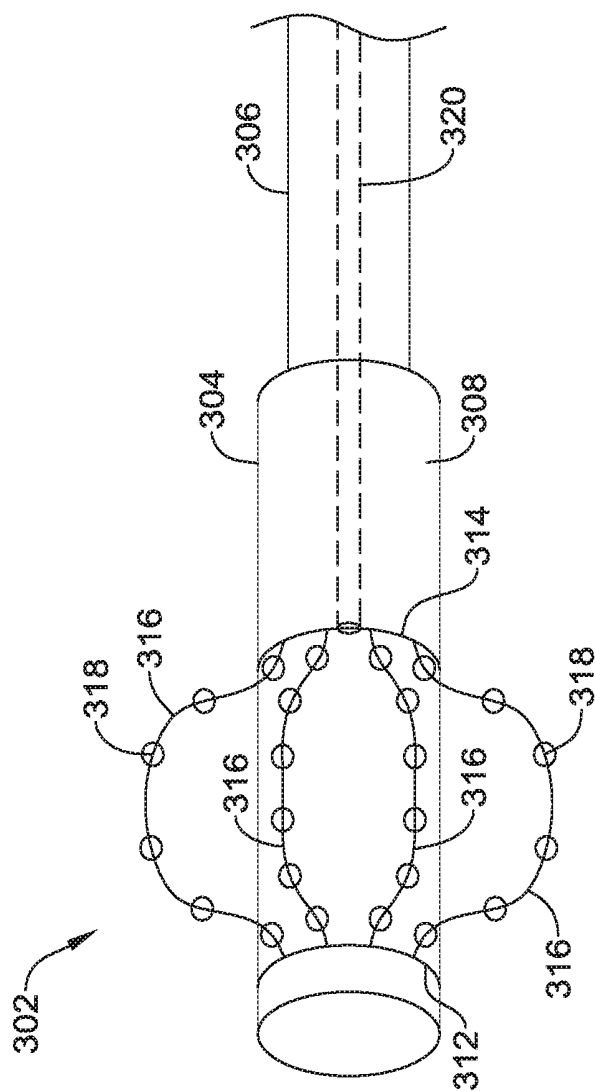


FIG. 19

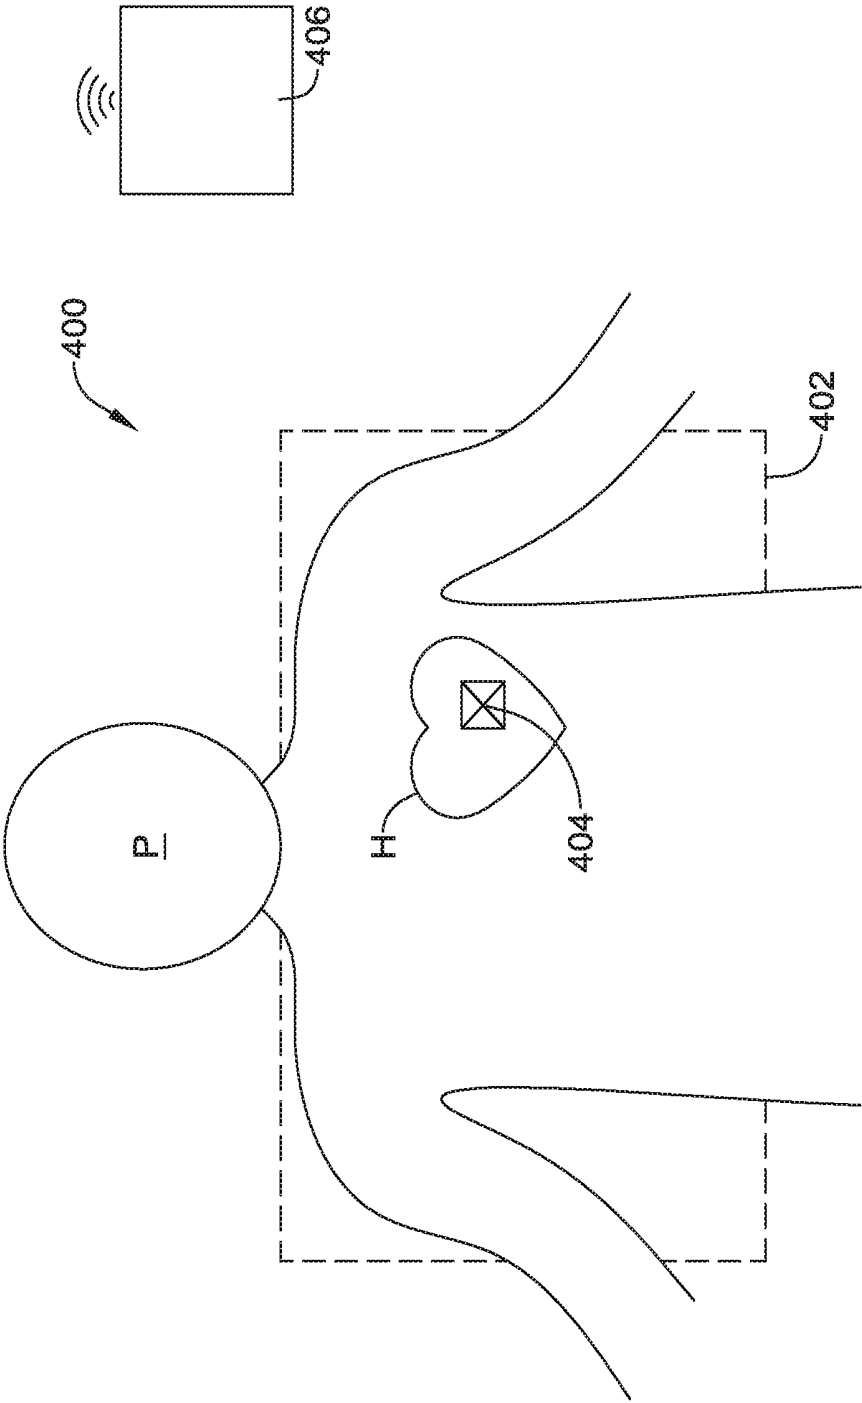


FIG. 20

**IMPLANTABLE MEDICAL DEVICE
DELIVERY SYSTEM WITH INTEGRATED
SENSOR**

**CROSS REFERENCE TO RELATED
APPLICATIONS**

[0001] This application claims the benefit of U.S. Provisional Patent Application Ser. No. 62/413,748 filed on Oct. 27, 2016, the disclosure of which is incorporated herein by reference.

TECHNICAL FIELD

[0002] The present disclosure pertains to medical devices, and methods for manufacturing and/or using medical devices. More particularly, the present disclosure pertains to leadless devices and methods, such as leadless cardiac pacing devices and methods, and delivery devices and methods for such leadless cardiac pacing devices.

BACKGROUND

[0003] A wide variety of medical devices have been developed for medical use, for example, cardiac use. Some of these devices include catheters, leads, pacemakers, and the like, and delivery devices and/or systems used for delivering such devices. These devices are manufactured by any one of a variety of different manufacturing methods and may be used according to any one of a variety of methods. Of the known medical devices, delivery systems, and methods, each has certain advantages and disadvantages. There is an ongoing need to provide alternative medical devices and delivery devices as well as alternative methods for manufacturing and using medical devices and delivery devices.

SUMMARY

[0004] This disclosure provides design, material, manufacturing method, and use alternatives for medical devices, including delivery devices.

[0005] An example delivery and deployment device that is configured to deliver an implantable medical device (IMD) to a chamber of a patient's heart and to deploy the IMD may include a handle assembly and a shaft extending distally from the handle assembly, the shaft including a distal region. A device containment housing may be coupled to the distal region of the shaft and may extend distally therefrom. The distal containment housing may be configured to accommodate at least a portion of the IMD therein. The IMD may, for example, be a leadless pacemaker, a lead, a neurostimulation device, a sensor or any other suitable IMD. A plurality of electrodes may be distributed about an exterior surface of the device containment housing such that at least some of the plurality of electrodes may be positioned to test a potential IMD deployment location before deploying the IMD. In some cases, a plurality of electrical conductors may be operably coupled with the plurality of electrodes and may extend proximally back along the shaft toward the handle assembly, the plurality of electrical conductors having proximal ends configured to be operably coupled to a testing device.

[0006] Alternatively or additionally to any of the embodiments above, the plurality of electrodes may include at least some electrodes that are radially disposed about the exterior surface of the device containment housing.

[0007] Alternatively or additionally to any of the embodiments above, the plurality of electrodes may include at least four electrodes spaced axially along the exterior surface of the device containment housing, the at least four electrodes including a first electrode, a second electrode, a third electrode and a fourth electrode. The first electrode and the fourth electrode may be spaced apart a first distance to form a stimulation dipole providing a potential difference. The second electrode and the third electrode may be spaced apart a second distance less than the first distance to provide a conductivity measurement by measuring a voltage between the second electrode and the third electrode resulting from the potential difference applied by the first electrode and the second electrode and the second electrode and the third electrode disposed between the first electrode and the fourth electrode.

[0008] Alternatively or additionally to any of the embodiments above, the plurality of electrodes may include a first electrode and a second electrode disposed on an exterior surface of the device containment housing to form a stimulation bipole.

[0009] Alternatively or additionally to any of the embodiments above, the delivery and deployment device may further include a pressure sensor configured to obtain an indication of pressure in the chamber of the patient's heart in response to a stimulating electrical pulse delivered via the first electrode and the second electrode.

[0010] Alternatively or additionally to any of the embodiments above, the pressure sensor may be disposed at or near a proximal end of the device containment housing.

[0011] Alternatively or additionally to any of the embodiments above, the delivery and deployment device may further include a first pressure sensor that is configured to obtain an indication of pressure in the chamber of the patient's heart and a second pressure sensor that is configured to obtain an indication of pressure in a different chamber of the patient's heart.

[0012] Alternatively or additionally to any of the embodiments above, the delivery and deployment device may further include an accelerometer and/or a gyroscope that is fixed relative to the device containment housing.

[0013] Alternatively or additionally to any of the embodiments above, at least some of the plurality of electrodes are disposed on an expandable assembly movably secured about an exterior of the device containment housing, the expandable assembly movable to a deployed configuration in which at least some of the plurality of electrodes contact cardiac tissue for endocardial mapping of at least part of the chamber of the patient's heart prior to IMD deployment.

[0014] Alternatively or additionally to any of the embodiments above, the delivery and deployment device further includes one or more magnet tracking sensor fixed relative to the device containment housing for tracking purposes.

[0015] An example IMD implantation device that is configured to deliver an implantable medical device (IMD) to a chamber of a patient's heart and to deploy the IMD therein may include a handle assembly and a shaft extending distally from the handle assembly, the shaft including a distal region. A device containment housing may be coupled to the distal region of the shaft and may extend distally therefrom. The distal containment housing may be configured to accommodate at least a portion of the IMD therein. A deployment member may extend through the shaft and may be configured to apply a deployment force to the IMD

in order to move the IMD from the device containment housing to deploy the IMD in the patient's heart. A plurality of electrodes may be distributed about an exterior surface of the device containment housing such that at least some of the plurality of electrodes may be positioned to test a potential IMD deployment location before deploying the IMD. A plurality of electrical conductors may be operably coupled with the plurality of electrodes and may extend proximally back along the shaft toward the handle assembly, the plurality of electrical conductors having proximal ends configured to be operably coupled to a testing device.

[0016] Alternatively or additionally to any of the embodiments above, the deployment member may be a push tube, and the IMD implantation device may further include a tether that extends distally through the push tube and is coupled to the IMD, the tether configured to be used to retrieve the IMD back into the device containment housing if an alternate deployment location is desired.

[0017] Alternatively or additionally to any of the embodiments above, the plurality of electrodes may include at least four electrodes spaced axially along the device containment housing, the at least four electrodes including a first electrode, a second electrode, a third electrode and a fourth electrode. The first electrode and the fourth electrode may be spaced apart a first distance to form a stimulation dipole providing a potential difference, wherein the fourth electrode extends to a distal end of the device containment housing. The second electrode and the third electrode may be spaced apart a second distance less than the first distance to provide a conductivity measurement by measuring a voltage between the second electrode and the third electrode resulting from the potential difference applied by the first electrode and the second electrode and the second electrode and the third electrode may be disposed between the first electrode and the fourth electrode.

[0018] Alternatively or additionally to any of the embodiments above, the plurality of electrodes may include a first electrode and a second electrode that are disposed on an exterior surface of the device containment housing to form a stimulation bipole.

[0019] Alternatively or additionally to any of the embodiments above, the IMD implantation device may further include a pressure sensor that is configured to obtain an indication of pressure in the chamber of the patient's heart in response to a stimulating electrical pulse delivered via the first electrode and the second electrode.

[0020] Alternatively or additionally to any of the embodiments above, the pressure sensor may be disposed at or near a proximal end of the device containment housing.

[0021] Alternatively or additionally to any of the embodiments above, the IMD implantation device may further include an accelerometer and/or a gyroscope that is fixed relative to the device containment housing.

[0022] An example implantation device that is configured to deliver a leadless cardiac pacemaker (LCP) to a chamber of a patient's heart and to deploy the LCP therein may include a handle assembly and a shaft that extends distally from the handle assembly, the shaft including a distal region. A device containment housing may be coupled to the distal region of the shaft and may extend distally therefrom, the device containment housing configured to accommodate the LCP therein. A deployment member may extend through the shaft and may be configured to apply a deployment force to the LCP in order to move the LCP from a distal end of the

device containment housing to deploy the LCP in the patient's heart. One or more tracking sensors may be fixed relative to the device containment housing to facilitate tracking of the device containment housing.

[0023] Alternatively or additionally to any of the embodiments above, the one or more tracking sensors may include a magnetic tracking sensor to facilitate magnet tracking of the device containment housing and/or an impedance tracking sensor to facilitate impedance tracking of the device containment housing.

[0024] Alternatively or additionally to any of the embodiments above, the implantation device may further include an LCP disposed within the device containment housing, and the LCP may include one or more LCP magnetic tracking sensors to facilitate magnet tracking of the LCP and/or one or more LCP impedance tracking sensors to facilitate impedance tracking of the LCP.

[0025] The above summary of some illustrative embodiments is not intended to describe each disclosed embodiment or every implementation of the present disclosure. The Figures, and Detailed Description, which follow, more particularly exemplify some of these embodiments.

BRIEF DESCRIPTION OF THE DRAWINGS

[0026] The disclosure may be more completely understood in consideration of the following detailed description in connection with the accompanying drawings, in which:

[0027] FIG. 1 is a plan view of an example leadless pacing device implanted within a heart;

[0028] FIG. 2 is a side view of an example implantable leadless cardiac pacing device;

[0029] FIG. 3 is a cross-sectional view of the implantable leadless cardiac pacing device of FIG. 2;

[0030] FIG. 4 is a plan view of an example delivery device for an implantable leadless cardiac pacing device;

[0031] FIG. 5 is a partial cross-sectional side view of the distal portion of the delivery device of FIG. 4;

[0032] FIG. 6 is a top view of the handle of the illustrative delivery device of FIG. 4;

[0033] FIG. 7 is a bottom view of the handle of the illustrative delivery device of FIG. 4;

[0034] FIG. 8 is a cross-section view of the handle of the illustrative delivery device of FIG. 4 taken at line 8-8 in FIG. 6;

[0035] FIG. 9 is a perspective view of the handle of the illustrative delivery device of FIG. 4 with portions removed;

[0036] FIGS. 10A-10E are schematic views illustrating the use of the illustrative delivery device to deploy an implantable leadless cardiac pacing device;

[0037] FIGS. 11A-11B are schematic views illustrating an example telescoping feature of the illustrative delivery device;

[0038] FIG. 12 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0039] FIG. 13 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0040] FIG. 14 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0041] FIG. 15 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0042] FIG. 16 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0043] FIG. 17 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0044] FIG. 18 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing;

[0045] FIG. 19 is a schematic view of a distal portion of the illustrative delivery device, showing features of the device containment housing; and

[0046] FIG. 20 is a schematic view of an illustrative imaging system.

[0047] While the disclosure is amenable to various modifications and alternative forms, specifics thereof have been shown by way of example in the drawings and will be described in detail. It should be understood, however, that the intention is not to limit the disclosure to the particular embodiments described. On the contrary, the intention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the disclosure.

DETAILED DESCRIPTION

[0048] For the following defined terms, these definitions shall be applied, unless a different definition is given in the claims or elsewhere in this specification.

[0049] All numeric values are herein assumed to be modified by the term “about,” whether or not explicitly indicated. The term “about” generally refers to a range of numbers that one of skill in the art would consider equivalent to the recited value (i.e., having the same function or result). In many instances, the terms “about” may include numbers that are rounded to the nearest significant figure.

[0050] The recitation of numerical ranges by endpoints includes all numbers within that range (e.g. 1 to 5 includes 1, 1.5, 2, 2.75, 3, 3.80, 4, and 5).

[0051] As used in this specification and the appended claims, the singular forms “a,” “an,” and “the” include plural referents unless the content clearly dictates otherwise. As used in this specification and the appended claims, the term “or” is generally employed in its sense including “and/or” unless the content clearly dictates otherwise.

[0052] It is noted that references in the specification to “an embodiment,” “some embodiments,” “other embodiments,” etc., indicate that the embodiment described may include one or more particular features, structures, and/or characteristics. However, such recitations do not necessarily mean that all embodiments include the particular features, structures, and/or characteristics. Additionally, when particular features, structures, and/or characteristics are described in connection with one embodiment, it should be understood that such features, structures, and/or characteristics may also be used connection with other embodiments whether or not explicitly described unless clearly stated to the contrary.

[0053] The following detailed description should be read with reference to the drawings in which similar structures in different drawings are numbered the same. The drawings, which are not necessarily to scale, depict illustrative embodiments and are not intended to limit the scope of the disclosure.

[0054] Cardiac pacemakers provide electrical stimulation to heart tissue to cause the heart to contract and thus pump blood through the vascular system. Conventional pacemak-

ers may include an electrical lead that extends from a pulse generator implanted subcutaneously or sub-muscularly to an electrode positioned adjacent the inside or outside wall of the cardiac chamber. As an alternative to conventional pacemakers, self-contained or leadless cardiac pacemakers have been proposed. Leadless cardiac pacemakers are small capsules that may, for example, be fixed to an intracardiac implant site in a cardiac chamber. In some cases, the small capsule may include bipolar pacing/sensing electrodes, a power source (e.g. a battery), and associated electrical circuitry for controlling the pacing/sensing electrodes, and thus may provide electrical stimulation to heart tissue and/or sense a physiological condition. The capsule may be delivered to the heart using a delivery device which may be advanced through a femoral vein, into the inferior vena cava, into the right atrium, through the tricuspid valve, and into the right ventricle. Accordingly, it may be desirable to provide delivery devices which facilitate advancement through the vasculature.

[0055] FIG. 1 illustrates example implantable leadless cardiac pacing devices 10 (e.g., a leadless pacemaker) implanted in a heart H. An illustrative implantable medical device (IMD) 10 is shown within the right ventricle RV while another IMD 10 is shown within the left ventricle LV as the IMD 10 may be configured for implantation in either ventricle, or in another chamber such as a right atrium RA or a left atrium LA. Depending on therapeutic needs, a patient may have a single IMD 10 or may have two or more IMDs 10 implanted in appropriate chambers. A side view of the illustrative implantable medical device (IMD) 10 is shown in FIG. 2 and a cross-sectional view of the illustrative IMD 10, taken at line 3-3 in FIG. 2, is illustrated in FIG. 3. The implantable medical device 10 may include a shell or housing 12 having a proximal end 14 and a distal end 16. In some instances, the IMD 10 may include a first electrode 20 positioned adjacent to the distal end 16 of the housing 12 and a second electrode 22 positioned adjacent to the proximal end 14 of the housing 12. In some cases, the housing 12 may include a conductive material and may be insulated along at least a portion of its length. A section along the proximal end 14 may be free of insulation so as to define the second electrode 22. The electrodes 20, 22 may be sensing and/or pacing electrodes to provide electro-therapy and/or sensing capabilities. The first electrode 20 may be configured to be positioned against the cardiac tissue of the heart H or may otherwise contact the cardiac tissue of the heart H while the second electrode 22 may be spaced away from the first electrode 20, and thus spaced away from the cardiac tissue.

[0056] The IMD 10 may include a pulse generator (e.g., electrical circuitry) and a power source (e.g., a battery) within the housing 12 to provide electrical signals to the electrodes 20, 22 and thus control the pacing/sensing electrodes 20, 22. In some cases, electrical communication between the pulse generator and the electrodes 20, 22 may provide electrical stimulation to heart tissue and/or sense a physiological condition.

[0057] The IMD 10 may include a fixation mechanism 24 proximate the distal end 16 of the housing 12 configured to attach the IMD 10 to a tissue wall of the heart H, or otherwise anchor the IMD 10 to the anatomy of the patient. As shown in FIG. 1, in some instances, the fixation mechanism 24 may include one or more, or a plurality of hooks or tines 26 anchored into the cardiac tissue of the heart H to attach the IMD 10 to a tissue wall. In other cases, the fixation

mechanism **24** may include one or more, or a plurality of passive tines, configured to entangle with trabeculae within the chamber of the heart **H** and/or a helical fixation anchor configured to be screwed into a tissue wall to anchor the IMD **10** to the heart **H**.

[0058] The IMD **10** may include a docking member **30** proximate the proximal end **14** of the housing **12** configured to facilitate delivery and/or retrieval of the IMD **10**. For example, the docking member **30** may extend from the proximal end **14** of the housing **12** along a longitudinal axis of the housing **12**. The docking member **30** may include a head portion **32** and a neck portion **34** extending between the housing **12** and the head portion **32**. The head portion **32** may be an enlarged portion relative to the neck portion **34**. For example, the head portion **32** may have a radial dimension from the longitudinal axis of the IMD **10** which is greater than a radial dimension of the neck portion **34** from the longitudinal axis of the IMD **10**. The docking member **30** may further include a tether retention structure **36** extending from the head portion **32**. The tether retention structure **36** may define an opening **38** configured to receive a tether or other anchoring mechanism therethrough. While the retention structure **36** is shown as having a generally “U-shaped” configuration, the retention structure **36** may take any shape which provides an enclosed perimeter surrounding the opening **38** such that a tether may be securably and releasably passed (e.g. looped) through the opening **38**. The retention structure **36** may extend through the head portion **32**, along the neck portion **34**, and to or into the proximal end **14** of the housing **12**, as is shown more clearly in FIG. **3**. The docking member **30** may be configured to facilitate delivery of the IMD **10** to the intracardiac site and/or retrieval of the IMD **10** from the intracardiac site. Other docking members **30** are contemplated.

[0059] In some cases, the IMD **10** may include one or more sensors or other devices that facilitate tracking the IMD **10** during and/or after delivery. In some cases, as schematically illustrated, the IMD **10** may include a sensor **200** that is disposed on or within the IMD **10**. In some cases, the sensor **200** may be considered to represent one or more magnetic tracking sensors that may facilitate magnetic tracking of the IMD **10** using a system such as will be described with respect to FIG. **20**. An illustrative but non-limiting example of such a system is the RHTHYMIA® system available from Boston Scientific. In some cases, the sensor **200** may be considered to represent one or more impedance tracking sensors that may facilitate impedance tracking of the IMD **10**. In some cases, the sensor **200** may be considered to represent one or more magnetic tracking sensors and one or more impedance tracking sensors, both of which may facilitate impedance tracking of the IMD **10**.

[0060] In some cases, the IMD **10** may be delivered to the heart **H** using a delivery device which may be advanced through a femoral vein, into the inferior vena cava, into the right atrium, through the tricuspid valve, and into the right ventricle. Accordingly, it will be appreciated that the delivery device may need to be navigated through relatively tortuous anatomy to deliver the IMD **10** to a suitable location. The target region for the delivery of the IMD **10** may be a portion of the right ventricle, for example, a portion of the right ventricle near the apex of the heart. The target region may also include other regions of the heart (e.g., right atrium, left atrium, or left ventricle), blood vessels, or other suitable targets. It may be desirable to

provide the delivery system with certain features that may allow for easier or better control for navigation or delivery purposes.

[0061] FIG. **4** is a plan view of an illustrative delivery device **100**, such as a catheter, that may be used to deliver the IMD **10**. It will be appreciated that the delivery device **100** is merely illustrative, as the IMD **10** may be delivered with other delivery devices that may or may not include some of the features described with respect to the delivery device **100**. As illustrated, the delivery device **100** may include an outer tubular member **102** having a proximal section **104** and a distal section **106**. An intermediate tubular member **110** may be longitudinally slidably disposed within a lumen **150** of the outer tubular member **102** (see e.g. FIG. **5**). An inner tubular member **116** may be longitudinally slidably disposed within a lumen **152** of the intermediate tubular member **110** (see e.g. FIG. **5**). A distal holding section, or device containment housing **108** may be attached to a distal end portion **114** of the intermediate tubular member **110**, as illustrated in FIG. **5**. The delivery device **100** may also include a handle assembly **120** positioned adjacent to the proximal section **104** of the outer tubular member **102**. In some instances, the outer tubular member **102** may include at least a section thereof that has an outer diameter **D2** that is less than the outer diameter **D1** of at least a portion of the device containment housing **108** (see e.g. FIG. **5**).

[0062] The handle assembly **120** may include a first or distal hub portion **126** attached to, such as fixedly attached to, the proximal end section **104** of the outer tubular member **102**, a second or intermediate hub portion **128** attached to, such as fixedly attached to, a proximal end section of the intermediate tubular member **110**, and a third or proximal hub portion **130** attached to, such as fixedly attached to, a proximal end section of the inner tubular member **116** (see e.g. FIG. **5**). The first hub portion **126**, second hub portion **128**, and third hub portion **130** may be positioned in a generally telescoping arrangement and longitudinally slidable relative to each other. As will be discussed in more detail below, each of the first hub portion **126**, the second hub portion **128**, and the third hub portion **130** may be longitudinally slidable and rotatable relative to each other such that the outer tubular member **102**, intermediate tubular member **110**, and inner tubular member **116** may be individually actuated. In some instances, it may be desirable to move the outer tubular member **102**, intermediate tubular member **110** and inner tubular member **116** simultaneously. The handle assembly **120** may include a multi-stage deployment mechanism or a first locking mechanism **134** to releasably couple the second hub portion **128** to the third hub portion **130** to prevent relative longitudinal movement therebetween, and thus prevent relative longitudinal movement between the intermediate tubular member **110** and the inner tubular member **116**, as will be discussed in more detail below. The handle assembly **120** may also include a second locking mechanism **132** to releasably couple the first hub portion **126** to the second hub portion **128** to prevent relative longitudinal movement therebetween, and thus prevent relative longitudinal movement between the outer tubular member **102** and the intermediate tubular member **110**, as will be discussed in more detail below.

[0063] The device containment housing **108** may be configured to receive the IMD **10** therein. For example, referring to FIG. **5**, which illustrates a cross-sectional view of a

distal portion of the delivery device **100**, the device containment housing **108** may define a cavity **142** for slidably receiving the IMD **10**, and may include a distal opening **144** for slidable insertion and/or extraction of the IMD **10** into and/or out of the cavity **142**. The device containment housing **108** may include a body portion **138** and a distal tip portion **140** that may be, for example, configured to be atraumatic to anatomy, such as a bumper tip. For example, as the catheter is navigated through the anatomy, the distal tip may come into contact with anatomy. Additionally, when the catheter is used to deliver the implantable medical device **10**, the tip **140** of the delivery device **100** will likely come into contact with tissue adjacent the target site (e.g. cardiac tissue of the heart).

[0064] In some cases, a hard distal tip formed of the material of the outer tubular member **102** and/or intermediate tubular member **110** may injure a vessel wall or cardiac tissue. As such, it may be desirable to provide the delivery device **100** with a softer distal tip **140** that can be introduced into the anatomy and come into contact with anatomy adjacent the target site without causing unnecessary trauma. In some cases, the distal tip **140** may be made of a material that is softer than the body portion **138** of the device containment housing **108**. In some cases, the distal tip **140** may include a material that has a durometer that is less than the durometer of the material of the body portion **138**. In some particular embodiments, the durometer of the material used in the distal tip **140** may be in the range of about 5 D to about 70 D, or for example, in the range of about 25 D to about 65 D. Additionally, the distal tip **140** may include a shape or structure that may make it less traumatic to tissue. For example, the distal tip **140** may have a distal surface, such as a tissue contacting surface, that is that is rounded or includes a curvature configured to be more atraumatic to tissue.

[0065] In some instances, all or a portion of the device containment housing **108** may include an inner surface that may be configured to resist getting caught on the fixation mechanism **24**, such as the one or more, or a plurality of hooks or tines **26** on the implantable medical device **10**. For example, the device containment housing **108** may include an inner layer or coating of harder or more lubricious material that resists force applied by the fixation mechanism **24** onto the inner surface of the device containment housing **108**. For example, the device containment housing **108** may include a multi-layered structure, and an inner layer may be made of a material that is harder than an outer layer.

[0066] The inner tubular member **116** may be disposed (e.g., slidably disposed) within a lumen **152** of the intermediate tubular member **110**. The inner tubular member **116** may be engaged by a user near or at the third hub portion **130**, and extend through a lumen **152** of the intermediate tubular member **110** and into the device containment housing **108**. A distal portion **118** of the inner tubular member **116** may be capable of engaging the IMD **10**, and the inner tubular member **116** may be used to “push” the IMD **10** out from device containment housing **108** so as to deploy and anchor the IMD **10** within a target region (e.g., a region of the heart such as the right ventricle). The inner tubular member **116** may have a lumen **154** extending from the proximal end **117** to a distal portion **118** thereof. A tether **112** or other retaining feature may be used to releasably secure the IMD **10** to the delivery device **100**. In some instances, the tether **112** may be a single or unitary length of material

that may extend from a proximal end **117** of the lumen **154**, out through the distal portion **118**, through the opening **38** of the IMD **10** and return to the proximal end **117** of the inner tubular member **116** through the lumen **154** such that both ends of the tether **112** are positioned adjacent to the third hub portion **130**. In some instances, as will be discussed in more detail below, the ends of the tether **112** may be secured within a locking feature in the third hub portion **130**.

[0067] In order to more specifically place or steer the delivery device **100** to a position adjacent to the intended target, the delivery device **100** may be configured to be deflectable or articulable or steerable. Referring to FIG. 4, for example, the outer tubular member **102** and/or intermediate tubular member **110** may include one or more articulation or deflection mechanism(s) that may allow for the delivery device **100**, or portions thereof, to be deflected, articulated, steered and/or controlled in a desired manner. For example, the outer tubular member **102** may include at least a portion thereof that can be selectively bent and/or deflected in a desired or predetermined direction. This may, for example, allow a user to orient the delivery device **100** such that the device containment housing **108** is in a desirable position or orientation for navigation or delivery of the IMD **10** to a target location. The outer tubular member **102** may be deflected, for example, along a deflection region.

[0068] A wide variety of deflection mechanisms may be used. In some example embodiments, deflection may be effected by one or more actuation members, such as pull wire(s) extending between a distal portion of the outer tubular member **102** and an actuation mechanism **122** near the proximal end of the outer tubular member **102**. As such, the one or more pull wires may extend both proximally and distally of the desired deflection or bending region or point. This allows a user to actuate (e.g., “pull”) one or more of the pull wires to apply a compression and/or deflection force to at least a portion of the outer tubular member **102** and thereby deflect or bend the outer tubular member **102** in a desired manner. In addition, in some cases the one or more wires may be stiff enough so that they can also be used to provide a pushing and/or tensioning force on the outer tubular member **102**, for example, to “push” or “straighten” the shaft into a desired position or orientation.

[0069] In some embodiments, the actuation member takes the form of a continuous wire that is looped through or otherwise coupled to a distal end region of the outer tubular member **102** so as to define a pair of wire sections. Other embodiments are contemplated, however, including embodiments where the actuation member includes one or a plurality of individual wires that are attached, for example, to a metal or metal alloy ring adjacent the distal end region of the outer tubular member **102**.

[0070] The actuation mechanism **122** may include a desired mechanism that may allow for applying tension (i.e. pulling force), or compression (i.e. pushing force), or both, on the actuation member(s). In some embodiments, the actuation mechanism **122** may include an external rotatable member **124** connected to and rotatable about the longitudinal axis of the handle assembly **120**. The rotatable member **124** may threadingly engage an internal member that is attached to the proximal end of the actuation member(s) or pull wires. When the external rotatable member **124** is rotated in a first rotational direction, the internal member translates in a first longitudinal direction, thereby applying

tension to the pull wire(s), which applies compression force to the shaft, so as to deflect the outer tubular member **102** from an initial position to a deflected position. When the external rotatable member **124** is rotated in a second rotational direction, the internal member translates in a second longitudinal direction, thereby reducing and/or releasing the tension on the pull wire(s), and allowing the outer tubular member **102** to relax back toward the initial position. Additionally, in some cases, as mentioned above, where the one or more wires may be stiff enough, rotation of the rotatable member **124** in the second rotational direction such that the internal member translates in a second longitudinal direction may apply compression to the wire(s), such that the wire(s) may apply tension to the outer tubular member **102** and “push” the outer tubular member **102** back toward an initial position, and possibly into additional positions beyond the initial position.

[0071] The one or more articulation and/or deflection mechanism(s) may also entail the outer tubular member **102** including structure and/or material that may provide for the desired degree and/or location of the deflection when the compressive or tensile forces are applied. For example, the outer tubular member **102** may include one or more sections that include structure and/or material configured to allow the shaft to bend and/or deflect in a certain way when a certain predetermined compressive and/or tensile force is applied. For example, the shaft may include one or more sections that are more flexible than other sections, thereby defining a bending or articulating region or location. Some such regions may include a number of varying or changing flexibility characteristics that may define certain bending shapes when predetermined forces are applied. Such characteristics may be achieved through the selection of materials or structure for different sections of the outer tubular member **102**.

[0072] In other embodiments, other articulation and/or deflection mechanism(s) are contemplated. For example, all or a portion of the delivery device **100**, such as the outer tubular member **102**, may be made of a shape memory material, such as a shape memory polymer and/or a shape memory metal. Such materials, when stimulated by an actuation mechanism, such as a change in temperature or the application of an electrical current, may change or move from a first shape to a second shape. As such, these material and mechanism may be used to deflect or bend the outer tubular member **102** in a desired manner. Other suitable deflection mechanism(s) that are able to deflect the delivery device **100** may also be used. Such alternative mechanisms may be applied to all other embodiments shown and/or discussed herein, and others, as appropriate.

[0073] Furthermore, the outer tubular member **102** may include one or more predefined or fixed curved portion(s) along the length thereof. In some cases, such curved sections may be configured to fit with particular anatomies or be configured for better navigation or delivery of the IMD **10**. Additionally, or alternatively, some such curved sections may be configured to allow the outer tubular member **102** to be predisposed to be bent and/or deflected in a certain direction or configuration when compression and/or tension forces are applied thereto. In some cases, the outer tubular member **102** may be a laser cut metallic tubing, a braid reinforced polymeric tubing, or other flexible tubular structure as desired.

[0074] Returning again to FIG. **5**, the device containment housing **108** may be affixed to a distal end portion **114** of the intermediate tubular member **110**. The device containment housing **108** may include a hub portion **136** and a tubular body portion **138**. In some instances, the hub portion **136** may be formed from a metal or metal alloy while the body portion **138** may be formed from a polymeric material, although this is not required. In some instances, a proximal region **143** of the body portion **138** may be heat bonded to a distal end portion **137** of the hub portion **136**, or otherwise affixed. The hub portion **136** may include a tapered intermediate region **145** disposed between a proximal end portion **139** and the distal end portion **137**.

[0075] In some cases, the outer tubular member **102** may include a metal ring or tip adjacent the distal end **103** thereof for attaching one or more pull wires thereto. In some cases, the outer tubular member **102** may further include a lubricious liner, such as, but not limited to a polytetrafluoroethylene (PTFE) liner. The proximal end portion **139** of the hub portion **136** may extend proximally into the lumen **150** of the outer tubular member **102**. In some instances, an outer surface of the proximal end portion **139** may form an interference fit with an inner surface of the outer tubular member **102**. In some cases, the outer surface of the proximal end portion **139** and the inner surface of the outer tubular member **102** may be coupled in a tapered engagement. For example, the distal end **103** of the outer tubular member **102** may flare radially outwards in the distal direction and/or the proximal end portion **139** may taper radially inward in the proximal direction. The two angled surfaces may engage as the proximal end portion **139** is proximally retracted within the outer tubular member **102**. Other coupling arrangements may be used as desired.

[0076] In some cases, as the outer tubular member **102** is bent to navigate the IMD **10** to the desired location, the proximal end portion **139** may advance distally and disengage from the inner surface of the outer tubular member **102** creating a kink point or weakened region adjacent to the bonding region **146**. Proximally retracting the intermediate tubular member **110** to bring the intermediate region **145** into contact with the outer tubular member **102** at contact point **148** and/or bringing the proximal end portion **139** into the outer tubular member **102** and fixing the intermediate tubular member **110** in this configuration may help prevent migration of the device containment housing **108** during navigation of the delivery device **100** to the desired location. Such a configuration may also place the intermediate tubular member **110** in tension while the device containment housing **108** applies a compression force on the outer tubular member **102**, as will be discussed in more detail below. As discussed above, a locking mechanism **132** in the handle assembly **120** may be utilized to releasably maintain the outer tubular member **102** and the intermediate tubular member **110** in a desired orientation.

[0077] FIG. **6** illustrates a top view of the handle assembly **120** of the delivery device **100**. FIG. **7** illustrates a bottom view of the handle assembly, approximately 180° from the view shown in FIG. **6**. The handle assembly **120** may include one or more ports **158**, **160**, **162** for delivering fluids, such as, but not limited to, a contrast and/or flushing fluid to the cavity **142** of the device containment housing **108**. The flush ports **158**, **160**, **162** may be in fluid communication with the lumens **150**, **152**, **154** of the outer, intermediate or inner tubular members **102**, **110**, **116**, as desired. For

example, the flush port 158 may be in fluid communication with the lumen 150 of the outer tubular member 102, the flush port 160 may be in fluid communication with the lumen 152 of the intermediate tubular member 110, and the flush port 162 may be in fluid communication with the lumen 154 of the inner tubular member 116.

[0078] The handle assembly 120 may further include a tether lock 164. The tether lock 164 may be actuatable between a locked and an unlocked configuration to maintain the tether 112 in a desired orientation. The ends of the tether 112 may be affixed to, secured to, or otherwise engage a tether cap 166 positioned at a proximal end of the third hub portion 130. The tether cap 166 may be removably secured to the third hub portion 130 to allow a clinician access to the ends of the tether 112. When the tether lock 164 is in the locked configuration, the tether cap 166 may not be removed from the third hub portion 130. When the tether lock 164 is in the unlocked configuration, the tether cap 166 may be removed and the ends of the tether 112 may be actuated. For example, once the IMD 10 has been implanted and its location verified, the tether 112 may be removed from the tether retention feature 36 of the IMD 10 by pulling on one of the ends until the opposite end has passed through the opening 38 such that the IMD 10 is free from the tether 112.

[0079] In some instances, the handle assembly 120 may also include visual markings, such as, but not limited to the markings illustrated at 170, 172, 174. These markings 170, 172, 174 may provide visual instructions or indications to the clinician. For example, the marking shown at 170 may be positioned proximate the rotatable member 124 of the actuation mechanism 122 to indicate that the rotatable member 124 controls deflection of the outer tubular member 102 and/or to indicate which direction the distal section 106 will deflect when the rotatable member 124 of the actuation mechanism 122 is rotated in a given direction. The markings shown at 172 may provide an indication of whether the second locking mechanism 132 is in the unlocked and/or locked configuration. Similarly, the markings shown at 174 may provide an indication of whether the tether lock 164 is in the unlocked and/or locked configuration.

[0080] FIG. 8 illustrates a cross-sectional view of the handle assembly 120 of the delivery device. As discussed above, the handle assembly 120 may include a first hub portion 126 attached to the proximal end section 104 of the outer tubular member 102, a second hub portion 128 attached to a proximal end section of the intermediate tubular member 110, and a third hub portion 130 attached to a proximal end section of the inner tubular member 116. Each of the first hub portion 126, the second hub portion 128, and the third hub portion 130 may be slidable and rotatable relative to each other such that the outer tubular member 102, intermediate tubular member 110, and inner tubular member 116 may be individually longitudinally actuated.

[0081] The inner tubular member 116 may extend distally from a proximal end 117. The proximal end 117 of the inner tubular member 116 may be positioned within or adjacent to the tether lock 164. The tether lock 164 may include a port 162 which may be in fluid communication with a lumen 154 of the inner tubular member 116. The lumen 154 may extend from the proximal end 117 to the distal portion 118 for delivering fluids, such as, but not limited to, a contrast and/or flushing fluid to the cavity 142 of the device containment housing 108. In some instances, the inner tubular

member 116 may be coupled or affixed to the third hub portion 130 adjacent the proximal end 117 of the inner tubular member 116, although this is not required. In some cases, the inner tubular member 116 may be affixed to the third hub portion 130 at any longitudinal location desired. In some instances, a tether, such as tether 112, for securing the IMD 10 to the distal portion 118 of the inner tubular member 116 may be disposed within the lumen 154 and may exit the delivery device 100 through or adjacent to tether cap 166, although this is not required.

[0082] The intermediate tubular member 110 may extend distally from a proximal end 111. The proximal end 111 of the intermediate tubular member 110 may be positioned within the second hub portion 128. The intermediate tubular member 110 may include a lumen 152 extending from the proximal end 111 to a distal end of the intermediate tubular member 110. The inner tubular member 116 may be slidably disposed within the lumen 152 of the intermediate tubular member 110. In some instances, the intermediate tubular member 110 may be coupled or affixed to the second hub portion 128 adjacent the proximal end 111 of the intermediate tubular member 110, although this is not required. In some cases, the intermediate tubular member 110 may be affixed to the second hub portion 128 at any longitudinal location desired.

[0083] The outer tubular member 102 may extend distally from a proximal end 105. The proximal end 105 of the outer tubular member 102 may be positioned within the first hub portion 126. The outer tubular member 102 may include a lumen 150 extending from the proximal end 105 to a distal end 103 of the outer tubular member 102. The intermediate tubular member 110 may be longitudinally slidably disposed within the lumen 150 of the outer tubular member 102. In some instances, the outer tubular member 102 may be coupled or affixed to the first hub portion 126 adjacent the proximal end 105 of the outer tubular member 102, although this is not required. In some cases, the outer tubular member 102 may be affixed to the first hub portion 126 at any longitudinal location desired.

[0084] In some instances, the first hub portion 126 may include a retaining ring 182 positioned adjacent to a proximal end of the first hub portion 126. In some instances, the retaining ring 182 may be rotatable about a longitudinal axis of the handle assembly 120. In some cases, the retaining ring 182 may include locking features configured to engage with other locking features of the locking mechanism 132. When the retaining ring 182 engages other features of the locking mechanism 132, longitudinal movement of the first hub portion 126 and the second hub portion 128 relative to one another may be prevented. Rotating the retaining ring 182 may disengage the retaining ring 182 from the other features of the locking mechanism 132. This may allow for longitudinal movement of the first hub portion 126 and the second hub portion 128 relative to one another, as will be described in more detail below. While the second locking mechanism 132 is described as a rotating retaining ring 182, other locking mechanisms capable of releasably securing first hub portion 126 and the second hub portion 128, and thus the outer tubular member 102 and the intermediate tubular member 110, may be used.

[0085] In some instances, the first locking mechanism 134 may include a depressible button 131. The depressible button 131 may include a first outwardly protruding portion 133 configured to engage a region of the third hub portion

130 and a second inwardly protruding portion **135** configured to engage a region of the second hub portion **128**. For example, the second protruding portion **135** may be disposed in and engage a groove or recess **178** formed in the second hub portion **128**. The engagement of the first locking mechanism **134** may prevent or reduce relative movement of the second hub portion **128** and the third hub portion **130** when the first locking mechanism **134** is not actively actuated (e.g. depressed) by a clinician. A downward force **186** may be applied to the button **131**. The force **186** may cause the first protruding portion **133** to lower and/or disengage from a surface of the third hub portion **130** and the second protruding portion **135** to raise and/or disengage from a surface of the second hub portion **128**. This may allow the third hub portion **130** to be moved longitudinally (e.g., proximally and/or distally), as shown at **184**, along a longitudinal axis of the handle assembly **120** relative to the second hub portion **128**, as will be discussed in more detail below. Longitudinal actuation of the third hub portion **130** relative to the second hub portion **128** may result in a corresponding longitudinal actuation of the inner tubular member (and hence the IMD **10**) relative to the intermediate tubular member **110** and the device containment housing **108**. Such actuation may be used to incrementally deploy the IMD **10**. FIG. **8** illustrates the second protruding portion **135** disposed in the middle of the recess **178**. However, in some cases, during advancement of the delivery device **100** to the desired treatment location, the second protruding portion **135** may be positioned at the proximal end of the recess **178** to ensure the IMD **10** is fully disposed in the device containment housing **108**. This is just an example. While the first locking mechanism **134** is described as a depressible button **131**, in some cases other locking mechanisms capable of releasably securing the second hub portion **128** and the third hub portion **130**, and thus the intermediate tubular member **110** and the inner tubular member **116**, may be used.

[0086] FIG. **9** illustrates a partial perspective view of the handle assembly **120** with portions of the third hub portion **130** removed to more clearly illustrate features of the second hub portion **128**. A proximal portion **127** of the second hub portion **128** may include a groove or recess **178** formed therein. The groove **178** may extend from a proximal end **179** to a distal end **181**. In some embodiments, groove **178** may include a proximal portion **177** and a distal portion **183** which may be circumferentially offset from one another. A hard stop **180** may be provided at a region between the proximal end **179** and the distal end **181**. The hard stop **180** may be a wall or other protrusion configured to engage the second protruding portion **135** of the first locking mechanism **134** such that in order to advance the second protruding portion **135** distally past the hard stop **180** from the proximal portion **177**, the user rotates the third hub portion **130** to align the second protruding portion **135** with the distal portion **183** of the groove **178**. This may allow the implantable medical device **10** to be incrementally deployed. During advancement of the delivery device **100** through the vasculature, the second protruding portion **135** may be disposed within the proximal portion **177** adjacent to the proximal end **179**. As discussed above, the second protruding portion **135** may engage a surface of the second hub portion **128** to prevent and/or minimize relative movement of the second and third hub portions **128**, **130** relative to one another.

[0087] The groove **178** may also include an angled region **198** between the proximal portion **177** and the distal portion **183** positioned generally opposite the hard stop **180**. When the third hub portion **130** is proximally retracted from the distal end **181** to the proximal end **179**, the angled region **198** may guide the second protruding portion **135** from the distal portion **183** of the groove **178** to the proximal portion **177** of the groove in a single fluid movement. For example, the third hub portion **130** may be proximally retracted from the distal end **181** to the proximal end **179** relative to the second hub portion **128** in a single proximal movement, if so desired, without prohibiting travel of the second protruding portion **135** from the distal portion **183** to the proximal portion **177**.

[0088] A distal portion **129** of the second hub portion **128** may include a groove or recess **188** configured to receive a mating feature disposed on the first hub portion **126**. This may allow the first hub portion **126** to be proximally retracted over the second hub portion **128**, as will be discussed in more detail below. The proximal and distal portions **127**, **129** of the second hub portion **128** may be separated by a gripping region **176** configured to provide a region for the clinician to hold.

[0089] Referring now to FIGS. **10A-10E**, a method for deploying an IMD **10** using the illustrative delivery device **100** will now be described. For simplicity, these Figures show the IMDS **10** being delivered to the right ventricle RV. The delivery device **100** may be introduced into the vasculature through the femoral vein through a previously introduced guide catheter. This is just an example. It will be appreciated that the IMD **10** may be delivered and deployed in the left ventricle LV via an intra-aortic approach through the left atrium LA, for example. The delivery device **100** may be introduced through any desired location and with or without the use of a guide catheter as desired. The delivery device **100** may be advanced through the vasculature to the desired treatment location, which, in the case of a leadless cardiac pacing device, may be a chamber of the heart. The clinician may use the actuation mechanism **122** may to deflect the distal section **106** of the outer tubular member **102** in a desired manner to facilitate advancement of the delivery device **100**. During advancement of the delivery device **100**, the handle assembly **120** may be in a fully extended configuration, as shown in FIG. **10A**. In such a configuration, the third hub portion **130** may be at its proximal-most location relative to the second hub portion **128** and the first hub portion **126** may be at its distal-most location relative to the second hub portion **128**. When the handle assembly **120** is in its fully extending configuration, the inner tubular member **116**, intermediate tubular member **110**, and the outer tubular member **102** may be oriented in the manner illustrated in FIG. **5**. The delivery device **100** can be imaged using known techniques to ensure accurate placement of the IMD **10**.

[0090] Once the distal tip portion **140** of the device containment housing **108** has been positioned adjacent to the cardiac tissue where the IMD **10** is desired, deployment of the IMD **10** can begin. The first stage of deploying the IMD **10** may enable activation of the fixation mechanism **24**. To initiate the first stage of deployment, the clinician may stabilize the first hub portion **126** relative to the patient and depress the button **131** of the first locking mechanism **134**. The clinician may then slide the third hub portion **130** distally, as shown at **190**, until the first locking mechanism

134 engages the hard stop 180 provided in the second hub portion 128 resulting in the handle assembly 120 configuration shown in FIG. 10B. Distal actuation of the third hub portion 130 may also move the inner tubular member 116 distally by the same distance. As the inner tubular member 116 advances distally, the distal portion 118 may “push” against the proximal end 14 of the implantable medical device 10. As the IMD 10 is pushed distally, the hooks 26 engage the heart tissue as shown in FIG. 10C. The IMD 10 may be distally advanced out of the device containment housing 108 to deploy the hooks or tines 26 from the device containment housing 108 to engage the hooks or tines 26 in the heart tissue while the proximal portion of the IMD 10 remains within the device containment housing 108. In some instances, the IMD 10 may be advanced distally in the range of 1 to 5 millimeters, although this is merely illustrative. This may allow the IMD 10 to be deployed while minimizing the amount of pressure applied to the heart wall. Further, the first locking mechanism 134 may prevent accidental or unintentional deployment of the IMD 10 as the button 131 must be actuated while advancing the third hub portion 130.

[0091] Referring briefly to FIGS. 11A and 11B, in some instances, it may be desirable to advance the device containment housing 108 and the intermediate tubular member 110 without advancing the outer tubular member 102 (i.e., telescoping the intermediate tubular member 110). For example, this may facilitate advancement of the delivery device 100 within the heart or maintain the position of the device containment housing 108 once it is placed against the heart wall. To distally advance or telescope the intermediate tubular member 110 relative to the outer tubular member 102, the second locking mechanism 132 may be actuated to “unlock” the first hub portion 126 and the second hub portion 128. As described above, a rotating retaining ring 182 may be rotated, as shown at 194, to move the second locking mechanism 132 from a locked to an unlocked configuration. Once the first locking mechanism has been unlocked, the clinician may distally advance 196 the second and third hub portions 128, 130 together to distally advance the device containment housing 108 as far as desired and/or needed. The actuation of the second and third hub portions 128, 130 may simultaneously move the intermediate tubular member 110 and the inner tubular member 116 as well. This may be done during advancement of the delivery device 100 through the vasculature, before initiating the first stage of deploying the IMD 10, and/or after the first stage of deploying the IMD 10 has been completed, as desired or needed.

[0092] After the first stage of deployment of the IMD 10, in which the tines or hooks 26 have been deployed from the device containment housing 108 into engagement with the heart wall, the tether 112 may be used to perform a tug test to determine if the IMD 10 is sufficiently engaged with the heart wall. In other words, the fixation of the IMD 10 (e.g. how well the hooks 26 are secured to the heart tissue) may be tested by gently tugging on the ends of the tether 112. If it is determined that the IMD 10 is sufficiently engaged with the heart wall, then the user may proceed to the second stage of deployment of the IMD 10 in which the remainder of the IMD 10 is expelled from the device containment housing 108. Otherwise, if the tug test fails and it is determined that the IMD 10 is not sufficiently engaged with the heart wall, the user may use the tether to pull (retract) the IMD 10, including the tines or hooks 26, back into the device containment housing 108 to release the implantable medical

device 10 from the heart wall. The IMD 10 may then be repositioned and the first stage of deployment repeated.

[0093] Returning to FIG. 10B, the second stage of deploying the IMD 10 may proximally retract the device containment housing 108, and thus the intermediate tubular member 110, relative to the inner tubular member 116 to fully deploy the IMD 10. Once the clinician has determined that the position of the IMD 10 is satisfactory and the fixation mechanism 24 is securely engaged with the heart tissue, the intermediate tubular member 110, including the device containment housing 108, of the delivery device 100 can be proximally retracted. To initiate the second stage of the deployment, the clinician may first rotate the third hub portion 130, as shown at 192, such that the button 131 is aligned with the distal portion 183 of the groove 178. The clinician may then stabilize the third hub portion 130 relative to the patient and proximally retract the first and second hub portions 126, 128. It should be noted that while it is possible to distally actuate the third hub portion 130 at this point, this may cause additional and unnecessary forces to be applied to the heart wall. Further, such distal movement of the third hub portion 130 may move the inner tubular member 116 (and hence the implantable medical device 10) distally rather than proximally retracting the intermediate tubular member 110 and/or the outer tubular member 102. The first and second hub portions 126, 128 may be proximally retracted until the first locking mechanism 134 engages the distal end 181 of the groove 178, resulting in the handle assembly 120 configuration shown in FIG. 10D. Such actuation of the first and second hub portions 126, 128 may fully deploy the implantable medical device 10 such that the IMD 10 is exterior of the device containment housing 108 and engaged with the heart wall, as shown in FIG. 10E.

[0094] As can be seen in FIG. 10E, the IMD 10 may still be affixed to the delivery device 100 through the tether 112. Once the clinician has verified the position of the IMD 10, the fixation of the IMD 10 and/or the electrical performance of the IMD 10, the tether 112 may be removed. In some instances, fixation of the IMD 10 (e.g. how well the hooks 26 are secured to the heart tissue) may be tested by gently tugging on the ends of the tether 112. The tether 112 may be removed by unlocking the tether lock 164, removing the tether cap 166, cutting the tether 112 at some location along its length, and pulling on one of the ends until the opposite end has passed through the opening 38 of the IMD 10 such that the IMD 10 is free from the tether 112. In some instances, the tether 112 may be affixed to a portion of the tether cap 166 (e.g. creating a loop) such that the tether 112 must be cut to allow the IMD 10 to be freed from the tether 112.

[0095] In some cases, there may be a desire to test a possible implantation site before deploying and fixating the IMD 10. In some cases, a delivery device such as the delivery device 100 may include structure or otherwise be configured to be able to electrically test a possible implantation site by delivering an electrical pulse to cardiac tissue proximate the possible implantation site and measuring a resultant cardiac parameter. If the measured cardiac parameter indicates a good implantation site, the IMD 10 may be deployed and fixated at that implantation site as discussed with respect to FIGS. 10A-10E. Otherwise, the delivery device 100 may be moved to another possible site, which can then be tested. This may be repeated until an acceptable

site is found. FIGS. 12-19 provide illustrative but non-limiting examples of how the delivery device 100 in general, and the device containment housing 108 in particular, may be modified to help in testing possible implantation sites.

[0096] FIG. 12 is a schematic diagram of a portion of an illustrative delivery device 202, which may be considered as being an example of the delivery device 100. In some cases, as illustrated, the delivery device 202 includes a device containment housing 204 extending distally from a shaft 206. In some cases, the device containment housing 204 may be considered as being an example of the device containment housing 108 while the shaft 206 may be considered as generally representing at least a portion of the intermediate tubular member 110 and the outer tubular member 102, and may in some cases be considered as extending proximally to the handle assembly 120. In some cases, as seen, the device containment housing 204 includes several electrodes that may be used in electrically testing a possible implantation site. The electrodes may, for example, be disposed on an outer surface 208 of the device containment housing 204 and in some cases may be axially and/or radially spaced apart on the outer surface 208. As shown, there is a first electrode 210, a second electrode 212, a third electrode 214 and a fourth electrode 216. In some cases, one or more of the electrodes 210, 212, 214 and 216 may extend radially at least partially about the outer surface 208.

[0097] In some cases, a first electrical connector 218 extends proximally from the first electrode 210, a second electrical connector 220 extends proximally from the second electrode 212, a third electrical connector 222 extends proximally from the third electrode 214 and a fourth electrical connector 224 extends proximally from the fourth electrode 216. In some cases, the electrical connectors 218, 220, 222 and 224 extend to the handle assembly 120 and enable a device such as but not limited to a programmer or tester to be electrically coupled to the electrodes 210, 212, 214 and 216 via the electrical connectors 218, 220, 222 and 224.

[0098] In some cases, the first electrode 210 and the fourth electrode 216 may, in combination, be considered as forming a stimulation bipole. A potential difference may be applied between the first electrode 210 and the fourth electrode 216, thereby creating a voltage therebetween. In some cases, the second electrode 212 and the third electrode 214 may be used to provide a resistance measurement by detecting a voltage between the second electrode 212 and the third electrode 214 resulting from the potential difference applied between the first electrode 210 and the fourth electrode 216. In some cases, as illustrated, the second electrode 212 and the third electrode 214 may be disposed between the first electrode 210 and the fourth electrode 216. It will be appreciated that in some cases, there may be a relationship between the detected resistance between the second electrode 212 and the third electrode 214 and the current chamber volume of the corresponding chamber of the heart when a current is applied between the first electrode 210 and the fourth electrode 216. In some cases, it may be possible, for example, to use the first electrode 210 and the third electrode 214 to stimulate and to use the second electrode 212 and the fourth electrode 216 to measure conductivity, for example. In some cases, an external electrode such as a temporary patch electrode may be worn by the patient and may for example be used as part of a stimulation circuit.

[0099] In some cases, the first electrode 210 may be smaller than the fourth electrode 216. When so provided, the first electrode 210 may be the cathode and the fourth electrode 216 may be the anode of the stimulation bipole (cathodic stimulation). While not explicitly shown, in some cases the first electrode 210 may extend over the distal end 213 of the device containment housing 204 so as to directly engage tissue when the distal end 213 of the device containment housing 204 is pushed up against a heart wall.

[0100] In some cases, conductivity values obtained via electrodes on the device containment housing 204 may, for example, be used to determine heart wall contact. For example, blood has a lower conductivity compared to tissue such as cardiac tissue. A relatively lower conductivity value may indicate a lack of tissue contact while a relatively higher conductivity value may indicate tissue contact, for example. In some cases, tissue composition may impact conductivity. For example, infarcted tissue has more collagen than healthy myocardium, and thus a conductivity value may be useful in determining whether a possible implantation site includes healthy myocardium or unhealthy myocardium, which can be important in achieving lower pacing threshold values.

[0101] FIG. 13 is a schematic diagram of a portion of an illustrative delivery device 226, which may be considered as being an example of the delivery device 100. In some cases, as illustrated, the delivery device 226 includes a device containment housing 228 extending distally from a shaft 230. In some cases, the device containment housing 228 may be considered as being an example of the device containment housing 108 while the shaft 230 may be considered as generally representing at least a portion of the intermediate tubular member 110 and the outer tubular member 102, and may in some cases be considered as extending proximally to the handle assembly 120. In some cases, as seen, the device containment housing 228 includes several electrodes that may be used in electrically testing a possible implantation site. The electrodes may, for example, be disposed on an outer surface 232 of the device containment housing 228 and in some cases may be axially and/or radially spaced apart on the outer surface 232. As shown, there is a first electrode 234 and a second electrode 236 that may function together as a stimulation bipole. While not explicitly shown, in some cases the first electrode 234 may extend over the distal end 235 of the device containment housing 228 so as to directly engage tissue when the distal end 235 of the device containment housing 228 is pushed up against a heart wall. In some cases, a first electrical connector 238 extends proximally from the first electrode 234 and a second electrical connector 240 extends proximally from the second electrode 236. In some cases, the electrical connectors 238 and 240 extend to the handle assembly 120 and enable a device such as but not limited to a programmer or tester to be electrically coupled to the electrodes 234 and 236 via the electrical connectors 238 and 240.

[0102] In some cases, a sensor 242 may be disposed on the shaft 230, near to the device containment housing 228. An electrical connector 244 may extend proximally from the sensor 242 and may extend to the handle assembly 120 and thus may be operably coupled with a programmer, tester or other device. In some cases, for example, the sensor 242 may be a pressure sensor such as a piezoelectric pressure sensor and may be configured to provide a signal representative of blood pressure within a cardiac chamber that results from a stimulation pulse applied as a potential difference

between the first electrode **234** and the second electrode **236**, for example. In some cases, the sensor **242** may instead represent an accelerometer or an acoustic sensor that can output a signal representative of cardiac performance in response to an applied stimulation pulse (e.g. heart sounds, heart wall acceleration, etc.). In some cases, the sensor **242** may represent a gyroscope that can output a signal representative of cardiac performance (e.g. twist) in response to an applied stimulation pulse. In some cases, the sensor **242** may include electronic components to amplify, filter or otherwise condition a raw sensor signal. In some cases, the sensor **242** may be a bidirectional transducer (e.g. a bidirectional acoustic transducer to facilitate ultrasound measurements).

[0103] In some cases, rather than using electrodes on the device containment housing **228** for stimulation, one or more electrodes on the IMD **10** may instead be used to stimulate cardiac tissue (provide a pacing pulse), and the electrodes **234** and **236** may instead be used to provide a resulting conductivity value. In some cases, the IMD **10** may be used to stimulate cardiac tissue and a sensor such as the sensor **242** may be used to measure a resulting cardiac parameter. In some cases, the device containment housing **228** may not include any electrodes.

[0104] In some cases, a delivery device may include two pressure sensors. As shown for example in FIG. **14**, a delivery device **250** may include a device containment housing **252** extending proximally from shaft **254**, and may be considered as being an example of the delivery device **100**. In some cases, the device containment housing **252** may be considered as being an example of the device containment housing **108** while the shaft **254** may be considered as generally representing at least a portion of the intermediate tubular member **110** and the outer tubular member **102**, and may in some cases be considered as extending proximally to the handle assembly **120**. In some cases, as seen, the device containment housing **252** has an outer surface **256** and includes the first electrode **234** and the second electrode **236**. In some cases, the first electrical connector **238** extends proximally from the first electrode **234** and the second electrical connector **240** extends proximally from the second electrode **212**.

[0105] In some cases, a sensor **242** may represent a first pressure sensor and a sensor **258** may represent a second pressure sensor. The sensor **242** is shown operably coupled to the electrical connector **244** while the sensor **258** is shown operably coupled to an electrical connector **260** that extends proximally from the sensor **258** and thus may be operably coupled with a programmer, tester or other device. In some cases, for example, the sensor **242** and the sensor **258** may each be piezoelectric pressure sensors, or other types of pressure sensors, and may each be configured to provide a signal representative of blood pressure within a cardiac chamber that results from a stimulation pulse applied as a potential difference between the first electrode **234** and the second electrode **236**, for example. In some cases, it will be appreciated that depending on the exact position of the delivery device **250** with respect to the patient's heart, the sensor **242** and the sensor **258** may see different pressure waveforms that may be useful in determining the appropriateness of a particular possible implantation site. For example, in some cases, the sensor **242** may see an atrial pressure waveform while the sensor **258** may see a ven-

tricular pressure waveform. These may be useful in determining an A-V delay, for example.

[0106] FIGS. **15** and **16** provide illustrative but non-limiting examples of electrode configurations that may, for example, be considered as showing possible electrode configurations useable with any of the device containment housings **204** (FIG. **12**), **228** (FIGS. **13**) and **252** (FIG. **14**). FIG. **15** shows a device containment housing **270** that has an outer surface **272**. A first ring electrode **274** and a second ring electrode **276** can be seen to be disposed on the outer surface **272**. It will be appreciated that by having electrodes that extend at least partially, if not entirely, around the outer surface **272**, there may be fewer issues with making tissue/blood contact regardless of rotational orientation of the device containment housing **204**. While not explicitly shown, in some cases the first ring electrode **274** may extend over the distal end **273** of the device containment housing **270** so as to directly engage tissue when the distal end **273** of the device containment housing **270** is pushed up against a heart wall. While two electrodes **274**, **276** are shown, it will be appreciated that the device containment housing **204** may include three, four or more electrodes. In some cases, the device containment housing **204** may also include one or more sensors that are configured to provide a signal representative of cardiac performance.

[0107] FIG. **16** shows a device containment housing **280** that has an outer surface **282**. A first electrode constellation **284** and a second electrode constellation **286** can be seen to be disposed on the outer surface **282**. In some cases, as illustrated, the first electrode constellation **284** includes an electrode **284a**, an electrode **284b** and an electrode **284c**. The first electrode constellation **284** may include additional electrodes not visible in this view. Similarly, the second electrode constellation **286** may include an electrode **286a**, an electrode **286b** and an electrode **286c**. The second electrode constellation **286** may include additional electrodes not visible in this view. In some cases, each of the electrodes **284a**, **284b**, **284c** may be electrically coupled together. In some instances, each of the electrodes **284a**, **284b**, **284c** may be individually addressable. While not explicitly shown, in some cases each of the electrodes **284a**, **284b**, **284c** may extend over the distal end **283** of the device containment housing **280** so as to directly engage tissue when the distal end **283** of the device containment housing **280** is pushed up against a heart wall. In some cases, each of the electrodes **286a**, **286b**, **286c** may be electrically coupled together. In some instances, each of the electrodes **286a**, **286b**, **286c** may be individually addressable.

[0108] It will be appreciated that by having electrodes that extend at least partially, if not entirely, around the outer surface **282**, there may be fewer issues with making tissue/blood contact regardless of rotational orientation of the device containment housing **280** relative to the heart H. While two electrode constellations **284**, **286** are shown, it will be appreciated that the device containment housing **280** may include three, four or more electrode constellations. In some cases, the device containment housing **280** may also include one or more sensors that are configured to provide a signal representative of cardiac performance.

[0109] FIG. **17** is a schematic illustration of a device containment housing **290** including features that may be combined with any of the device containment housings **204** (FIG. **12**), **228** (FIGS. **13**) and **252** (FIG. **14**). The illustrative device containment housing **290** includes an outer surface

292 that extends from a distal end **294** to a proximal end **296**. In some cases, the device containment housing **290** may include a vision system that enables a physician or other user to actually visualize a possible implantation site. A vision system may, for example, utilize intracardiac ultrasound, infrared imaging, direction vision, and the like. The distal end **294** includes a first visualization element **298** and a second visualization element **300**. One these elements may, for example, be or otherwise include a light source while the other element includes a camera, or a fiber optic cable and a lens operably coupled to a proximally located camera for visualization.

[0110] FIGS. **18** and **19** are schematic illustrations of a portion of a delivery device **302**, which may be considered as being an example of the delivery device **100**, with FIG. **18** showing the delivery device **302** in a delivery configuration while FIG. **19** shows the delivery device **302** in a mapping configuration. In some cases, as illustrated, the delivery device **302** may include a device containment housing **304** extending distally from a shaft **306**. In some cases, the device containment housing **304** may be considered as being an example of the device containment housing **108** while the shaft **306** may be considered as generally representing at least a portion of the intermediate tubular member **110** and the outer tubular member **102**, and may in some cases be considered as extending proximally to the handle assembly **120**. In some cases, as seen, the device containment housing **304** includes electrodes that may be used in electrically testing a possible implantation site.

[0111] In some cases, the device containment housing **304** includes an electrode assembly **310** that includes a distal ring **312** and a proximal ring **314**, with a plurality of electrode supports **316** extending between the distal ring **312** and the proximal ring **314**. Each of the plurality of electrode supports **316** include a plurality of individually addressable electrodes **318**. In some cases, the distal ring **312** is secured relative to the device containment housing **304** while the proximal ring **314** may be slidable relative to the device containment housing **304**. In some cases, a deployment member **320** may be operably coupled to the proximal ring **314** and extend proximally through the shaft **306** such that the proximal ring **314** may be moved forwards and backwards by pushing and pulling on the deployment member **320**. In other cases, the distal ring **312** may be slidable, and the deployment member **320** may instead be operably coupled to the distal ring **312**. In either case, in the deployed state, stimulation pulses (e.g. pacing pulses) may be sequentially applied to each of the plurality of individually addressable electrodes **318**, and a response may be sensed and recorded. This may help determine a suitable implantation site for the IMD. Once a suitable implantation site has been determined, the deployment member **320** may be moved to retract the electrode supports **316**, and the device containment housing **304** may be positioned over the suitable site and the IMD in the device containment housing **304** may be deployed and implanted at the site.

[0112] It will be appreciated that the electrode assembly **310** permits mapping of the endocardial surface. In some cases, this may be useful in determining or otherwise identifying intrinsic activation patterns. In some cases, mapping the endocardial surface may facilitate identification of scar tissue and possibly other damaged tissue, to be avoided when deploying the IMD **10**. It will be appreciated that while no sensors are shown as being part of the delivery

device **302**, one or more sensors such as pressure sensors, accelerometers and/or gyroscopes may be included as part of the delivery device **302** in order to gauge cardiac response to an applied stimulation via each of two or more of the individually addressable electrodes **318**, for example.

[0113] As noted with respect to FIG. **2**, in some cases the IMD **10** may include one or more magnetic tracking sensors and/or impedance tracking sensors. FIG. **20** schematically illustrates a system **400** in which a patient P, including a heart H, is placed in front of (or on top of) a magnetic field generator **402**. In some cases, a device disposed within the heart H includes a magnetic tracking sensor and/or an impedance tracking sensor **404**. In some cases, when the magnetic field generator **402** is generating a magnetic field, and the magnetic tracking sensor **404** within the device is turned on, the magnetic tracking sensor **404** is able to determine its location relative to the magnetic field lines, and to communicate this information for display on a monitor **406**. When a current generator (not shown) provides current to the body (e.g. via two or more electrode patches), an impedance tracking sensor within the device may be able to determine its location relative to the electric field lines, and to communicate this information for display on a monitor **406**. In some cases, both magnetic tracking and impedance tracking may be used to identify and track the location of the device. In some cases, the device including the magnetic tracking sensor and/or an impedance tracking sensor **404** may be a leadless cardiac pacemaker (LCP) or other intracardially implanted device, and the system **400** may provide an indication of the location of the device within the body. In some cases, the device including the magnetic tracking sensor and/or impedance tracking sensor **404** may instead be a delivery device, and the magnetic tracking sensor and/or an impedance tracking sensor **404** may provide an indication of the location of the delivery device. In some cases, the magnetic tracking sensor and/or impedance tracking sensor **404** may not only provide location (X, Y, Z), but may also provide pitch, yaw, velocity, acceleration, twist, and/or other parameters related to the device's position.

[0114] As illustrated, the system **400** may be a structure that the patient P lies on, or perhaps stands in front of. In some cases, it is contemplated that the magnetic field generator **402** may be incorporated into a wearable vest that may be used for ambulatory measurements. In some cases, information provided by the system **400** may be used to help guide initial implantation and to verify fixation of the device (such as the IMD **10**). In some cases, the data provided may be used for determining rate response sensor calibration, as otherwise heart motion can interfere with detecting physical movement of the patient. In some cases, a co-implanted device such as but not limited to a subcutaneous implantable cardioverter-defibrillator (SICD) may be used to generate the magnetic field and/or electric field (e.g. current). In some cases, the SICD may inject a current, which may be detected by the IMD **10** and this information may be used to improve location detection via impedance tracking.

[0115] The delivery device **100**, **202**, **226**, **250**, **302**, or components thereof, may be made from a metal, metal alloy, polymer (some examples of which are disclosed below), a metal-polymer composite, ceramics, combinations thereof, and the like, or other suitable material. Some examples of suitable polymers may include polytetrafluoroethylene (PTFE), ethylene tetrafluoroethylene (ETFE), fluorinated ethylene propylene (FEP), polyoxymethylene (POM, for

example, DELRIN® available from DuPont), polyether block ester, polyurethane (for example, Polyurethane 85A), polypropylene (PP), polyvinylchloride (PVC), polyether-ester (for example, ARNITEL® available from DSM Engineering Plastics), ether or ester based copolymers (for example, butylene/poly(alkylene ether) phthalate and/or other polyester elastomers such as HYTREL® available from DuPont), polyamide (for example, DURETHAN® available from Bayer or CRISTAMID® available from Elf Atochem), elastomeric polyamides, block polyamide/ethers, polyether block amide (PEBA, for example available under the trade name PEBAX®), ethylene vinyl acetate copolymers (EVA), silicones, polyethylene (PE), Marlex high-density polyethylene, Marlex low-density polyethylene, linear low density polyethylene (for example REXELL®), polyester, polybutylene terephthalate (PBT), polyethylene terephthalate (PET), polytrimethylene terephthalate, polyethylene naphthalate (PEN), polyetheretherketone (PEEK), polyimide (PI), polyetherimide (PEI), polyphenylene sulfide (PPS), polyphenylene oxide (PPO), poly paraphenylene terephthalamide (for example, KEVLAR®), polysulfone, nylon, nylon-12 (such as GRILAMID® available from EMS American Grilon), perfluoro(propyl vinyl ether) (PFA), ethylene vinyl alcohol, polyolefin, polystyrene, epoxy, polyvinylidene chloride (PVdC), poly(styrene-*b*-isobutylene-*b*-styrene) (for example, SIBS and/or SIBS 50A), polycarbonates, ionomers, biocompatible polymers, other suitable materials, or mixtures, combinations, copolymers thereof, polymer/metal composites, and the like. In some embodiments the polymer can be blended with a liquid crystal polymer (LCP). For example, the mixture can contain up to about 6 percent LCP.

[0116] Some examples of suitable metals and metal alloys include stainless steel, such as 304V, 304L, and 316LV stainless steel; mild steel; nickel-titanium alloy such as linear-elastic and/or super-elastic nitinol; other nickel alloys such as nickel-chromium-molybdenum alloys (e.g., UNS: N06625 such as INCONEL® 625, UNS: N06022 such as HASTELLOY® C-22®, UNS: N10276 such as HASTELLOY® C276®, other HASTELLOY® alloys, and the like), nickel-copper alloys (e.g., UNS: N04400 such as MONEL® 400, NICKELVAC® 400, NICORROS® 400, and the like), nickel-cobalt-chromium-molybdenum alloys (e.g., UNS: R30035 such as MP35-N® and the like), nickel-molybdenum alloys (e.g., UNS: N10665 such as HASTELLOY® ALLOY B2®), other nickel-chromium alloys, other nickel-molybdenum alloys, other nickel-cobalt alloys, other nickel-iron alloys, other nickel-copper alloys, other nickel-tungsten or tungsten alloys, and the like; cobalt-chromium alloys; cobalt-chromium-molybdenum alloys (e.g., UNS: R30003 such as ELGILOY®, PHYNOX®, and the like); platinum enriched stainless steel; titanium; combinations thereof; and the like; or any other suitable material.

[0117] In at least some embodiments, portions or all of the delivery device **100**, **202**, **226**, **250**, **302**, or components thereof, may be doped with, made of, or otherwise include a radiopaque material. Radiopaque materials are understood to be materials capable of producing a relatively bright image on a fluoroscopy screen or another imaging technique during a medical procedure. This relatively bright image aids the user of the delivery device **100**, **202**, **226**, **250**, **302** in determining its location. Some examples of radiopaque materials can include, but are not limited to, gold, platinum, palladium, tantalum, tungsten alloy, polymer material loaded with a radiopaque filler, and the like. Additionally, other radiopaque marker bands and/or coils may also be

incorporated into the design of the delivery device **100**, **202**, **226**, **250**, **302**, or components thereof, to achieve the same result.

[0118] It should be understood that this disclosure is, in many respects, only illustrative. Changes may be made in details, particularly in matters of shape, size, and arrangement of steps without exceeding the scope of the disclosure. This may include, to the extent that it is appropriate, the use of any of the features of one example embodiment being used in other embodiments. The disclosure's scope is, of course, defined in the language in which the appended claims are expressed.

What is claimed is:

1. A delivery and deployment device configured to deliver an implantable medical device (IMD) to a chamber of a patient's heart and deploy the IMD therein, the delivery and deployment device comprising:

- a handle assembly;
- a shaft extending distally from the handle assembly, the shaft including a distal region;
- a device containment housing coupled to the distal region of the shaft and extending distally therefrom, the device containment housing configured to accommodate at least part of the IMD therein;
- a plurality of electrodes distributed about an exterior surface of the device containment housing such that at least some of the plurality of electrodes may be positioned to test a potential IMD deployment location before deploying the IMD; and
- a plurality of electrical conductors operably coupled with the plurality of electrodes and extending proximally back along the shaft toward the handle assembly, the plurality of electrical conductors having proximal ends configured to be operably coupled to a testing device.

2. The delivery and deployment device of claim 1, wherein the plurality of electrodes include at least some electrodes that are radially disposed about the exterior surface of the device containment housing.

3. The delivery and deployment device of claim 1, wherein the plurality of electrodes comprise at least four electrodes spaced axially along the exterior surface of the device containment housing, the at least four electrodes including a first electrode, a second electrode, a third electrode and a fourth electrode;

the first electrode and the fourth electrode spaced apart a first distance to form a stimulation dipole providing a potential difference;

the second electrode and the third electrode spaced apart a second distance less than the first distance to provide a conductivity measurement by measuring a voltage between the second electrode and the third electrode resulting from the potential difference applied by the first electrode and the second electrode; and

the second electrode and the third electrode disposed between the first electrode and the fourth electrode.

4. The delivery and deployment device of claim 1, wherein the plurality of electrodes comprise a first electrode and a second electrode disposed on an exterior surface of the device containment housing to form a stimulation bipole.

5. The delivery and deployment device of claim 4, further comprising a pressure sensor configured to obtain an indication of pressure in the chamber of the patient's heart in response to a stimulating electrical pulse delivered via the first electrode and the second electrode.

6. The delivery and deployment device of claim 5, wherein the pressure sensor is disposed at or near a proximal end of the device containment housing.

7. The delivery and deployment device of claim 4, further comprising:

- a first pressure sensor configured to obtain an indication of pressure in the chamber of the patient's heart; and
- a second pressure sensor configured to obtain an indication of pressure in a different chamber of the patient's heart.

8. The delivery and deployment device of claim 4, further comprising an accelerometer and/or a gyroscope fixed relative to the device containment housing.

9. The delivery and deployment device of claim 1, wherein at least some of the plurality of electrodes are disposed on an expandable assembly movably secured about an exterior of the device containment housing, the expandable assembly movable to a deployed configuration in which at least some of the plurality of electrodes contact cardiac tissue for endocardial mapping of at least part of the chamber of the patient's heart prior to IMD deployment.

10. The delivery and deployment device of claim 1, further comprising one or more magnet tracking sensor fixed relative to the device containment housing for tracking purposes.

11. An IMD implantation device configured to deliver an implantable medical device (IMD) to a chamber of a patient's heart and deploy the IMD therein, the IMD implantation device comprising:

- a handle assembly;
- a shaft extending distally from the handle assembly, the shaft including a distal region;
- a device containment housing coupled to the distal region of the shaft and extending distally therefrom, the device containment housing configured to accommodate at least part of the IMD therein;
- a deployment member extending through the shaft, the deployment member configured to apply a deployment force to the IMD in order to move the IMD from the device containment housing to deploy the IMD in the patient's heart;
- a plurality of electrodes distributed about an exterior surface of the device containment housing such that at least some of the plurality of electrodes may be positioned to test a potential IMD deployment location before deploying the IMD; and
- a plurality of electrical conductors operably coupled with the plurality of electrodes and extending proximally back along the shaft toward the handle assembly, the plurality of electrical conductors having proximal ends configured to be operably coupled to a testing device.

12. The IMD implantation device of claim 11, wherein the deployment member is a push tube, and wherein the IMD implantation device further comprises:

- a tether extending distally through the push tube and coupled to the IMD, the tether configured to be used to retrieve the IMD back into the device containment housing if an alternate deployment location is desired.

13. The IMD implantation device of claim 12, wherein the plurality of electrodes comprise at least four electrodes spaced axially along the device containment housing, the at least four electrodes including a first electrode, a second electrode, a third electrode and a fourth electrode;

the first electrode and the fourth electrode are spaced apart a first distance to form a stimulation dipole providing a potential difference, wherein the fourth electrode extends to a distal end of the device containment housing;

the second electrode and the third electrode are spaced apart a second distance less than the first distance to provide a conductivity measurement by measuring a voltage between the second electrode and the third electrode resulting from the potential difference applied by the first electrode and the second electrode; and

the second electrode and the third electrode disposed between the first electrode and the fourth electrode.

14. The IMD implantation device of claim 11, wherein the plurality of electrodes comprise a first electrode and a second electrode disposed on an exterior surface of the device containment housing to form a stimulation bipole.

15. The IMD implantation device of claim 14, further comprising a pressure sensor configured to obtain an indication of pressure in the chamber of the patient's heart in response to a stimulating electrical pulse delivered via the first electrode and the second electrode.

16. The IMD implantation device of claim 15, wherein the pressure sensor is disposed at or near a proximal end of the device containment housing.

17. The IMD implantation device of claim 14, further comprising an accelerometer and/or a gyroscope fixed relative to the device containment housing.

18. An implantation device configured to deliver a leadless cardiac pacemaker (LCP) to a chamber of a patient's heart and deploy the LCP therein, the implantation device comprising:

- a handle assembly;
- a shaft extending distally from the handle assembly, the shaft including a distal region;
- a device containment housing coupled to the distal region of the shaft and extending distally therefrom, the device containment housing configured to accommodate the LCP therein;
- a deployment member extending through the shaft, the deployment member configured to apply a deployment force to the LCP in order to move the LCP from a distal end of the device containment housing to deploy the LCP in the patient's heart; and

one or more tracking sensors fixed relative to the device containment housing to facilitate tracking of the device containment housing.

19. The implantation device of claim 18, wherein the one or more tracking sensors comprise a magnetic tracking sensor to facilitate magnet tracking of the device containment housing and/or an impedance tracking sensor to facilitate impedance tracking of the device containment housing.

20. The implantation device of claim 18, further comprising an LCP disposed within the device containment housing, the LCP comprising one or more LCP magnetic tracking sensors to facilitate magnet tracking of the LCP and/or one or more LCP impedance tracking sensors to facilitate impedance tracking of the LCP.

* * * * *

专利名称(译)	具有集成传感器的植入式医疗设备输送系统		
公开(公告)号	US20180117304A1	公开(公告)日	2018-05-03
申请号	US15/793149	申请日	2017-10-25
[标]申请(专利权)人(译)	心脏起搏器股份公司		
申请(专利权)人(译)	心脏起搏器，INC.		
当前申请(专利权)人(译)	心脏起搏器，INC.		
[标]发明人	KOOP BRENDAN EARLY YU YINGHONG AN QI MAILE KEITH R THAKUR PRAMODSINGH HIRASINGH MI BIN STAHMANN JEFFREY E AVERINA VIKTORIA A SIEJKO KRZYSZTOF Z KANE MICHAEL J SHUROS ALLAN CHARLES SHARMA ARJUN D SOLTIS BRIAN		
发明人	KOOP, BRENDAN EARLY YU, YINGHONG AN, QI MAILE, KEITH R. THAKUR, PRAMODSINGH HIRASINGH MI, BIN STAHMANN, JEFFREY E. AVERINA, VIKTORIA A. SIEJKO, KRZYSZTOF Z. KANE, MICHAEL J. SHUROS, ALLAN CHARLES SHARMA, ARJUN D. SOLTIS, BRIAN		
IPC分类号	A61N1/05 A61B5/00		
CPC分类号	A61N1/056 A61B5/0031 A61B5/686 A61N1/37288 A61N1/3706 A61F2/2436 A61N1/372 A61N1/3756		
优先权	62/413748 2016-10-27 US		
外部链接	Espacenet USPTO		

摘要(译)

递送和展开装置可以包括手柄组件和从手柄组件向远侧延伸的轴。装置容纳壳体可以联接到轴的远侧区域并且可以从其远侧延伸。远端容纳壳体可构造成在其中容纳IMD的至少一部分。例如，IMD可以是无导线起搏器，导线，神经刺激设备，传感器或任何其他合适的IMD。多个电极可以围绕装置容纳壳体的外表面分布，使得多个电极中的至少一些可以被定位成在部署IMD之前测试潜在的IMD部署位置。

