



US009757530B2

(12) **United States Patent**
Nolan

(10) **Patent No.:** **US 9,757,530 B2**
(45) **Date of Patent:** ***Sep. 12, 2017**

(54) **APPARATUS AND METHOD FOR
IMPROVED ASSISTED VENTILATION**

(71) Applicant: **Colabs, Inc.**, Carmel, CA (US)

(72) Inventor: **Clay Nolan**, Carmel, CA (US)

(73) Assignee: **CoLabs, Inc.**, Carmel, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/666,244**

(22) Filed: **Mar. 23, 2015**

(65) **Prior Publication Data**

US 2015/0265790 A1 Sep. 24, 2015

Related U.S. Application Data

(63) Continuation-in-part of application No. 14/296,298, filed on Jun. 4, 2014, now Pat. No. 9,220,858, which
(Continued)

(51) **Int. Cl.**
A61M 16/04 (2006.01)
A61M 16/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61M 16/0003** (2014.02); **A61B 5/087** (2013.01); **A61B 5/6847** (2013.01); **A61M 16/0051** (2013.01); **A61M 16/0069** (2014.02); **A61M 16/04** (2013.01); **A61M 16/0411** (2014.02); **A61M 16/0463** (2013.01); **A61M 16/0475** (2014.02); **A61M 16/0486** (2014.02); **A61M 16/06** (2013.01); **A61M 16/201**

(2014.02); **A61M 16/0063** (2014.02); **A61M 16/0434** (2013.01); **A61M 16/0484** (2014.02); **A61M 16/0488** (2013.01); **A61M 16/202** (2014.02); **A61M 16/209** (2014.02);
(Continued)

(58) **Field of Classification Search**

CPC **A61M 16/04**; **A61M 16/0402**; **A61M 16/0409**; **A61M 16/0411**; **A61M 16/0413**; **A61M 16/0465**; **A61M 16/0477**; **A61M 16/0484**; **A61M 16/0486**

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,233,984 A * 11/1980 Walling **A61M 16/04**
128/207.14
4,351,330 A * 9/1982 Scarberry **A61M 16/04**
128/207.15

(Continued)

Primary Examiner — Justine Yu


Assistant Examiner — LaToya M Louis

(74) *Attorney, Agent, or Firm* — Levine Bagade Han LLP

(57) **ABSTRACT**

Devices and methods for allowing for improved assisted ventilation of a patient. The methods and devices provide a number of benefits over conventional approaches for assisted ventilation. For example, the methods and devices described herein permit blind insertion of a device that can allow ventilation regardless of whether the device is positioned within a trachea or an esophagus. In addition, the methods and device allow for timed delivery of ventilations based on a condition of a thoracic cavity to increase the amount and efficiency of blood flow during a resuscitation procedure.

22 Claims, 37 Drawing Sheets

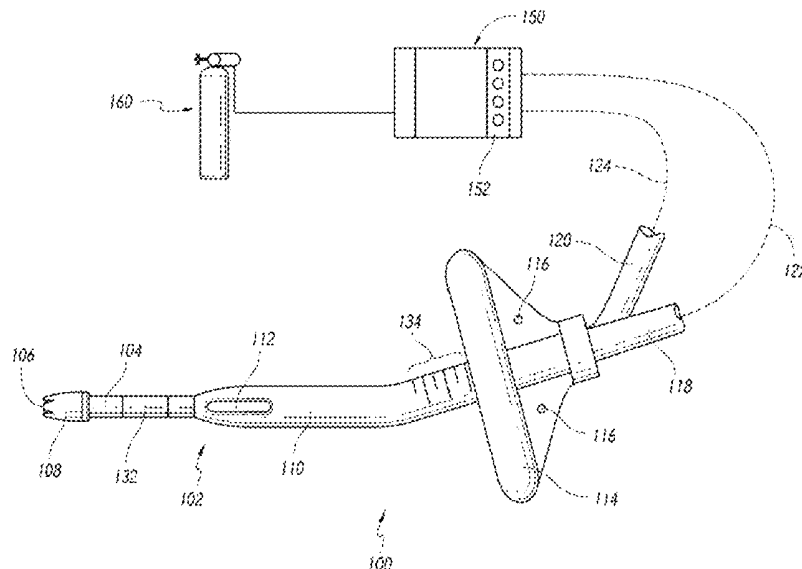

Related U.S. Application Data

is a continuation of application No. 13/659,699, filed on Oct. 24, 2012, now Pat. No. 8,776,796.

- (60) Provisional application No. 61/969,043, filed on Mar. 21, 2014, provisional application No. 61/569,169, filed on Dec. 9, 2011.

(51) **Int. Cl.**

A61M 16/06 (2006.01)

A61B 5/00 (2006.01)

A61B 5/087 (2006.01)

A61M 16/20 (2006.01)

A61N 1/39 (2006.01)

A61N 1/05 (2006.01)

A61N 1/362 (2006.01)

(52) **U.S. Cl.**

CPC *A61M 2016/003* (2013.01); *A61M 2016/0027* (2013.01); *A61M 2202/0208* (2013.01); *A61M 2205/054* (2013.01); *A61M 2205/332* (2013.01); *A61M 2205/3344* (2013.01); *A61M 2205/502* (2013.01); *A61M 2205/583* (2013.01); *A61M 2230/432* (2013.01); *A61N 1/0517* (2013.01); *A61N 1/0519* (2013.01); *A61N 1/362* (2013.01); *A61N 1/39* (2013.01)


(56) **References Cited**

U.S. PATENT DOCUMENTS

5,080,107 A * 1/1992 Teves A61B 7/023
128/207.15
5,197,463 A * 3/1993 Jeshuran A61M 16/0463
128/206.28
5,339,808 A * 8/1994 Don Michael A61M 16/04
128/200.26
5,413,558 A * 5/1995 Paradis A61B 17/12045
600/18
5,499,625 A * 3/1996 Frass A61M 16/04
128/200.26
5,785,051 A * 7/1998 Lipscher A61B 5/06
128/200.26
5,832,920 A * 11/1998 Field A61M 16/0477
128/205.12


5,885,248 A * 3/1999 Denton A61M 16/0078
604/100.03
6,155,257 A * 12/2000 Lurie A61H 31/005
128/204.18
6,202,646 B1 * 3/2001 Camodeca A61M 16/04
128/200.26
6,584,974 B1 * 7/2003 Ratner A61M 1/0072
128/205.23
6,827,695 B2 * 12/2004 Palazzolo A61B 5/04012
128/901
6,994,087 B1 * 2/2006 Smith A61M 16/0488
128/205.13
7,178,519 B2 * 2/2007 Melker A61M 16/0488
128/200.26
7,503,328 B2 * 3/2009 Kolobow A61M 16/0463
128/200.26
7,747,319 B2 * 6/2010 Freeman A61H 31/005
128/207.14
8,062,239 B2 * 11/2011 Sherman A61H 31/006
601/44
2003/0188750 A1 * 10/2003 Christopher A61M 16/0488
128/207.14
2004/0020491 A1 * 2/2004 Fortuna A61M 16/04
128/207.15
2006/0230931 A1 10/2006 Bliss et al.
2007/0221222 A1 * 9/2007 Lurie A61M 16/0078
128/204.18
2008/0029100 A1 * 2/2008 Glassenberg A61B 1/04
128/207.15
2009/0277447 A1 * 11/2009 Voss A61M 16/0051
128/204.18
2010/0051030 A1 3/2010 Richard et al.
2010/0163023 A1 * 7/2010 Singh A61M 16/04
128/200.26
2010/0204622 A1 * 8/2010 Hwang A61B 5/6831
601/41
2010/0319691 A1 * 12/2010 Lurie A61H 31/02
128/203.12
2012/0016179 A1 * 1/2012 Paradis A61H 9/0078
600/17
2012/0024292 A1 * 2/2012 Sandmore A61M 16/04
128/207.14
2013/0072830 A1 * 3/2013 Illindala A61H 11/00
601/41
2013/0085425 A1 * 4/2013 Monsieurs A61B 5/036
601/41
2013/0146051 A1 6/2013 Nolan

* cited by examiner

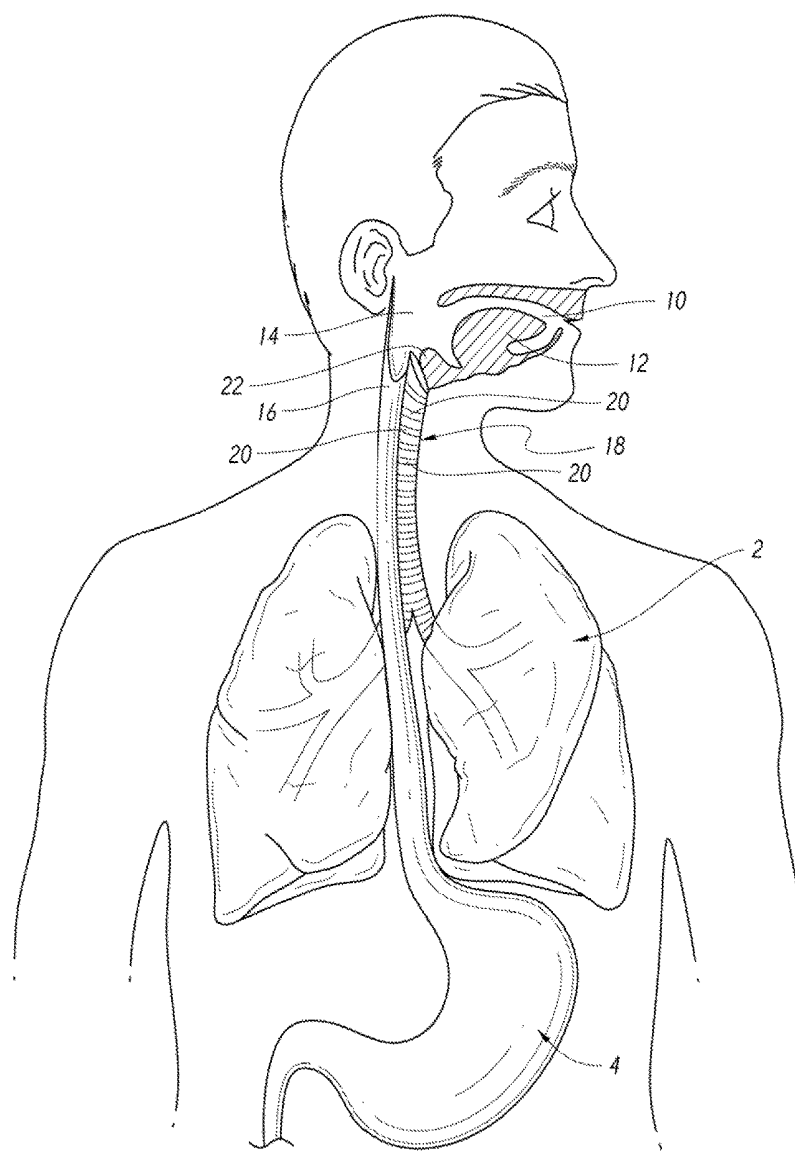


Prior Art

FIG. 1

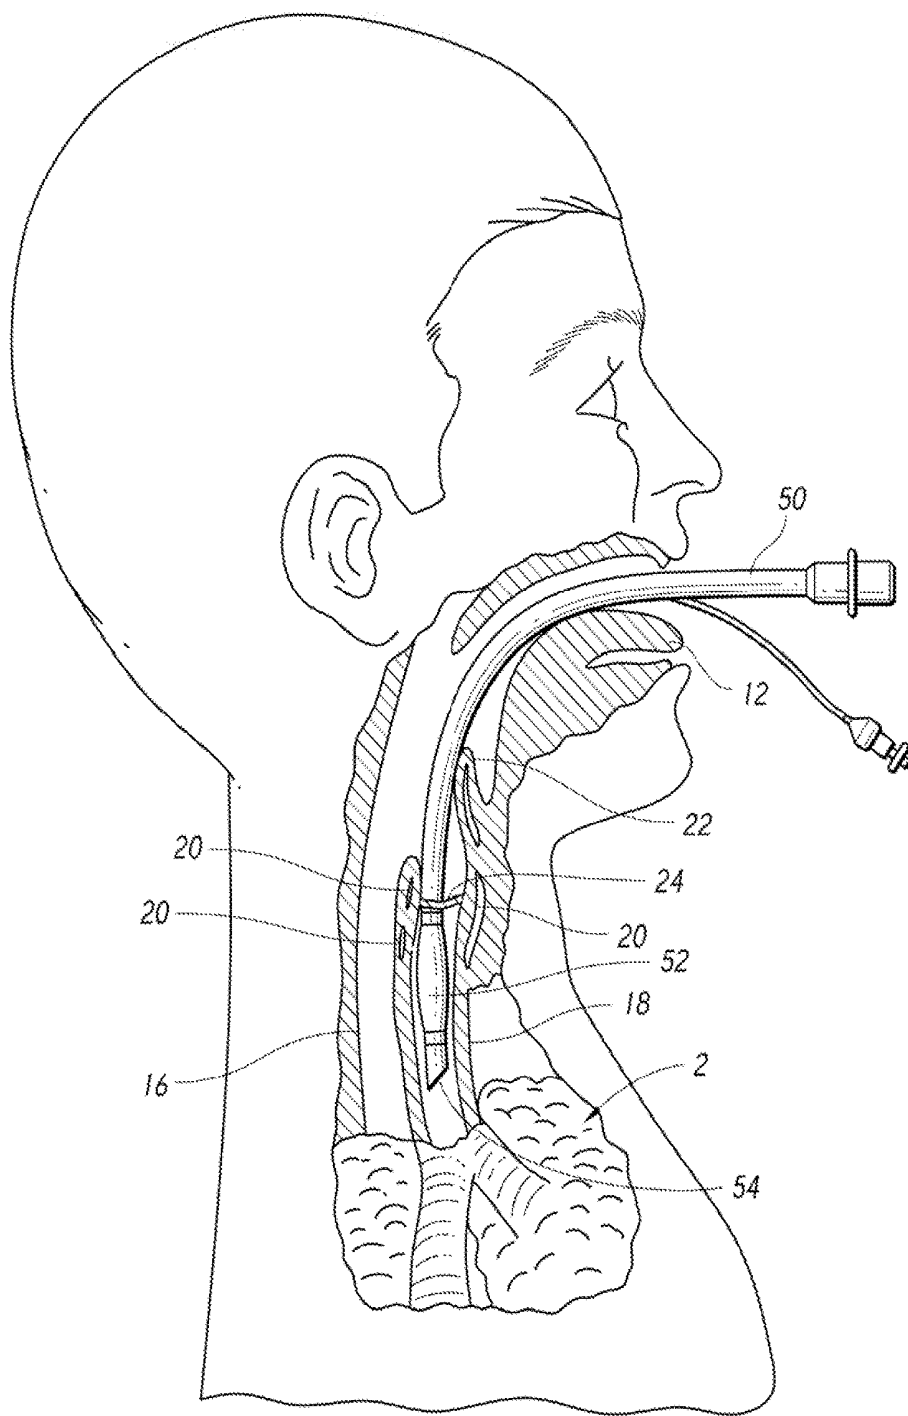

Prior Art

FIG. 2

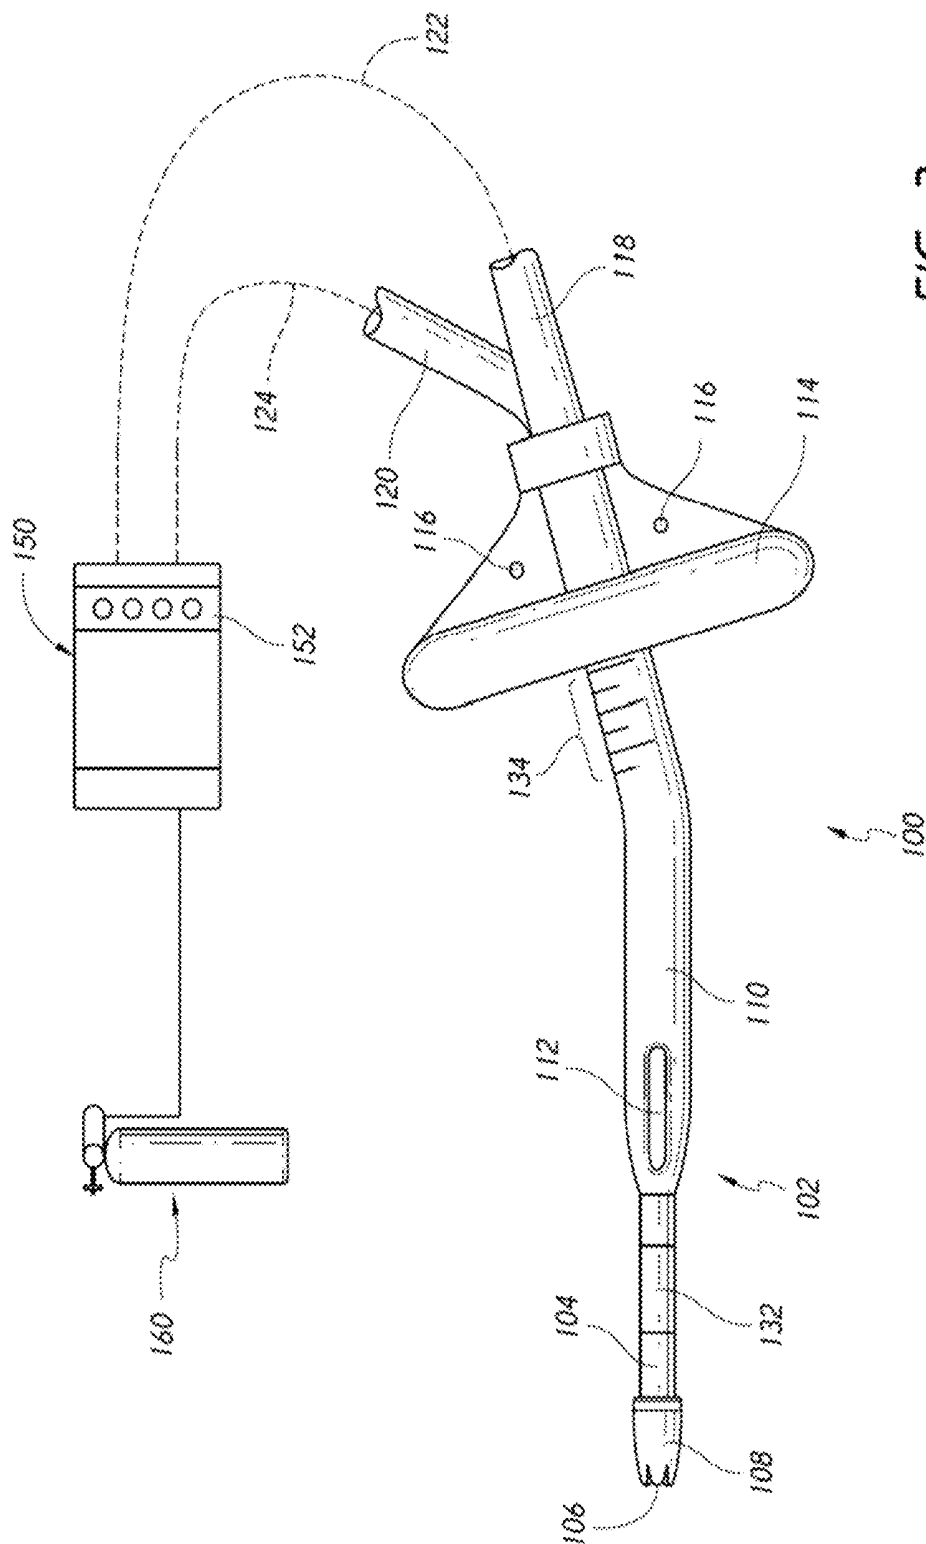

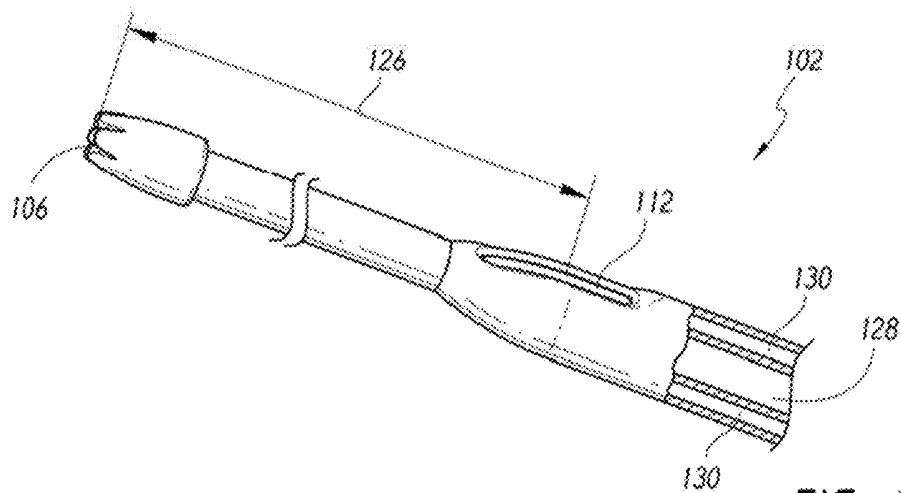


FIG. 4A

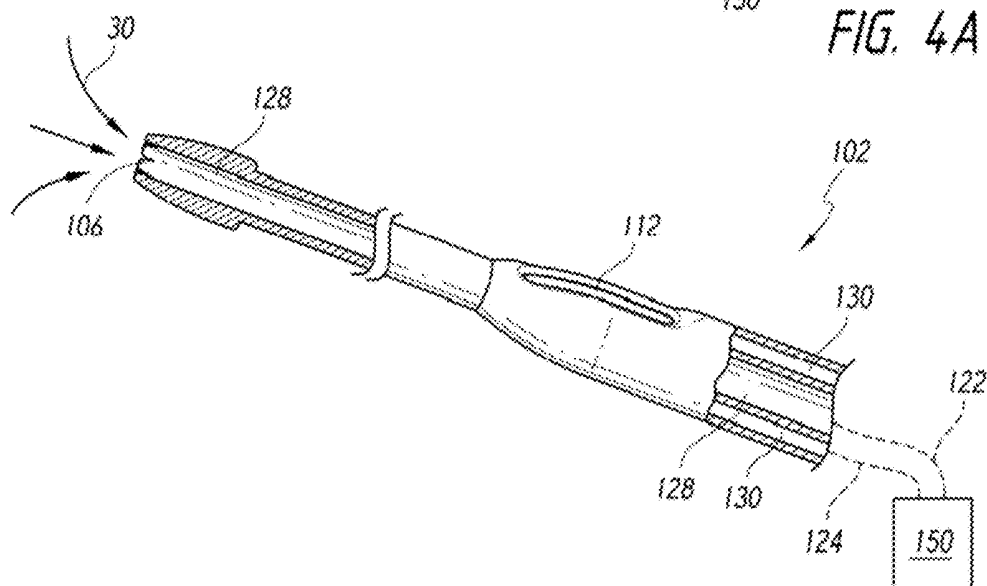


FIG. 4B

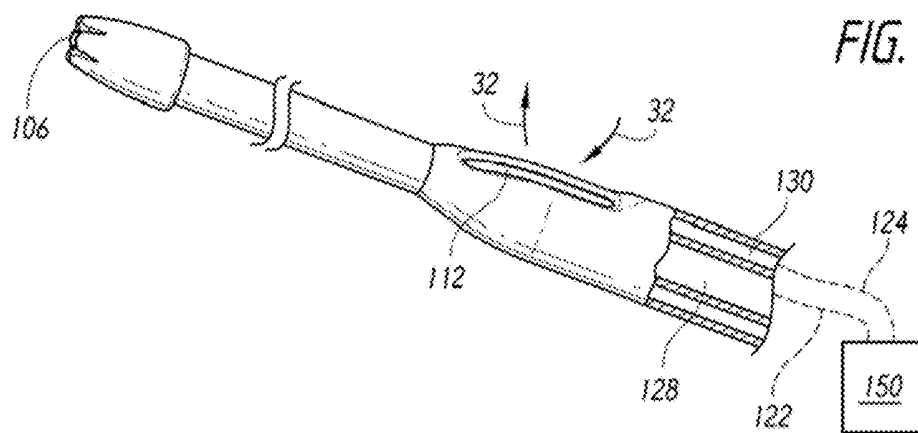


FIG. 4C

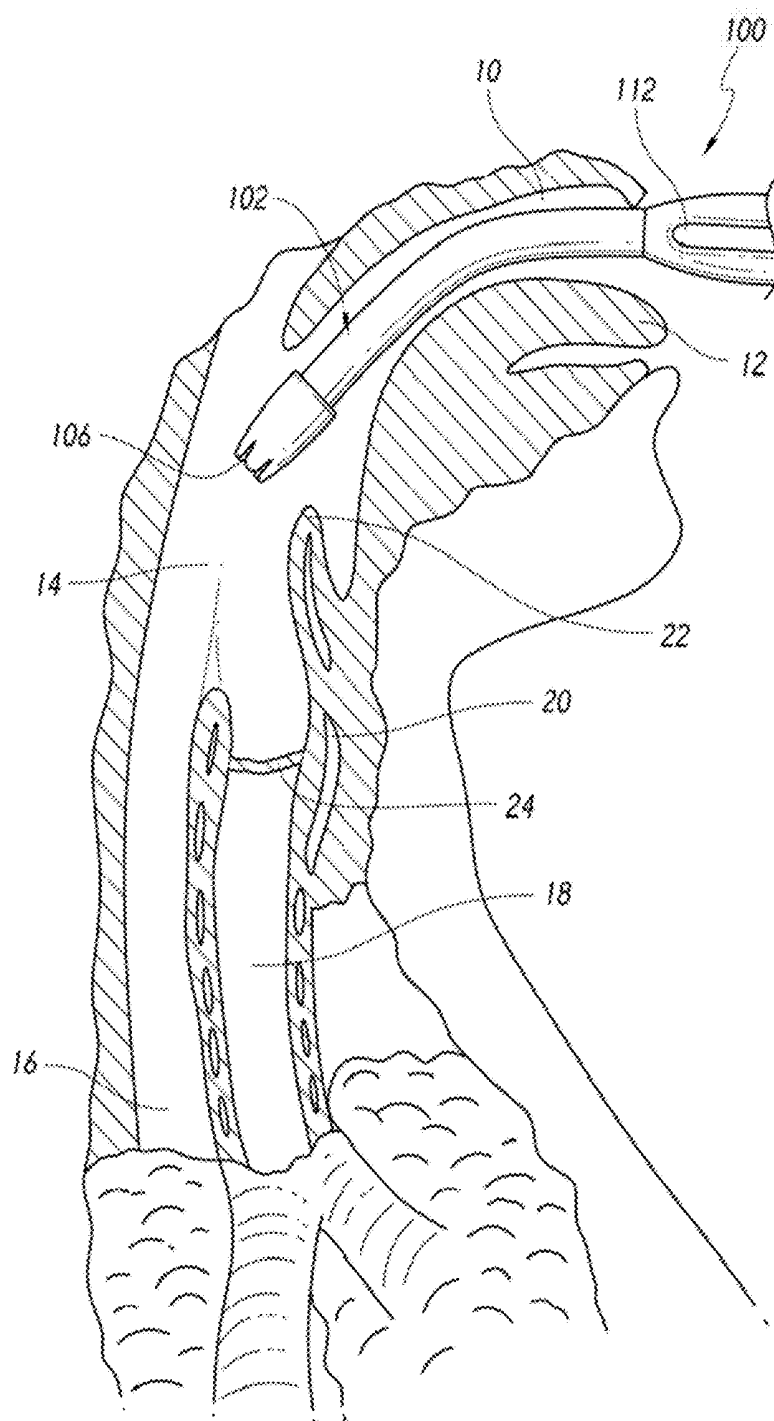


FIG. 5A

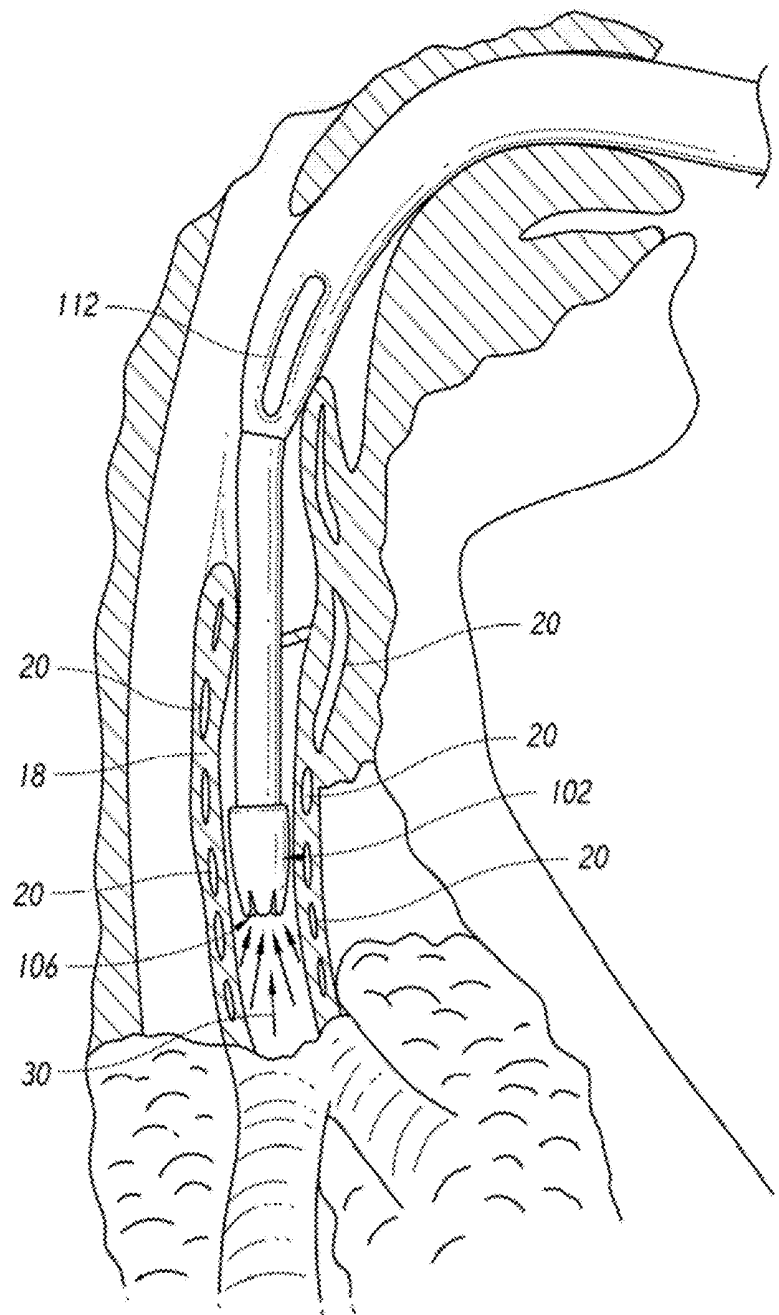


FIG. 5B

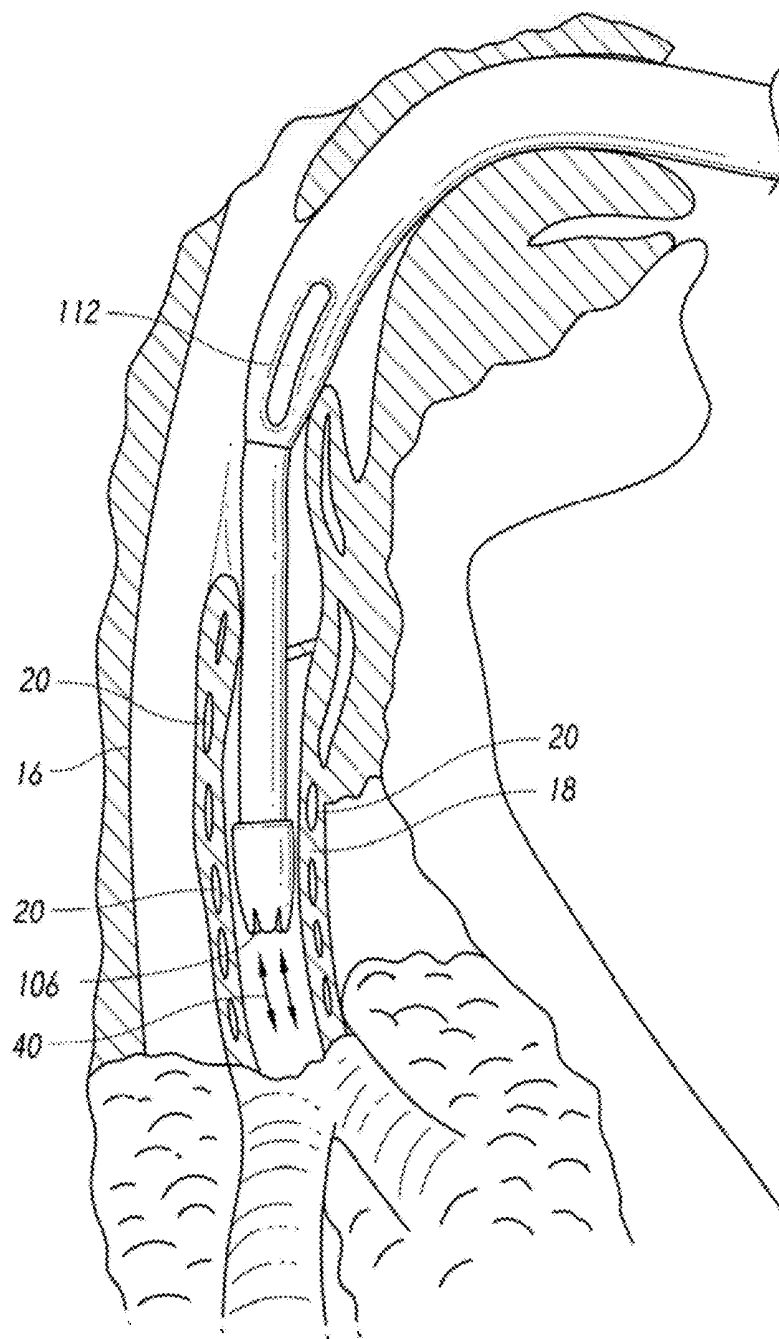


FIG. 5C

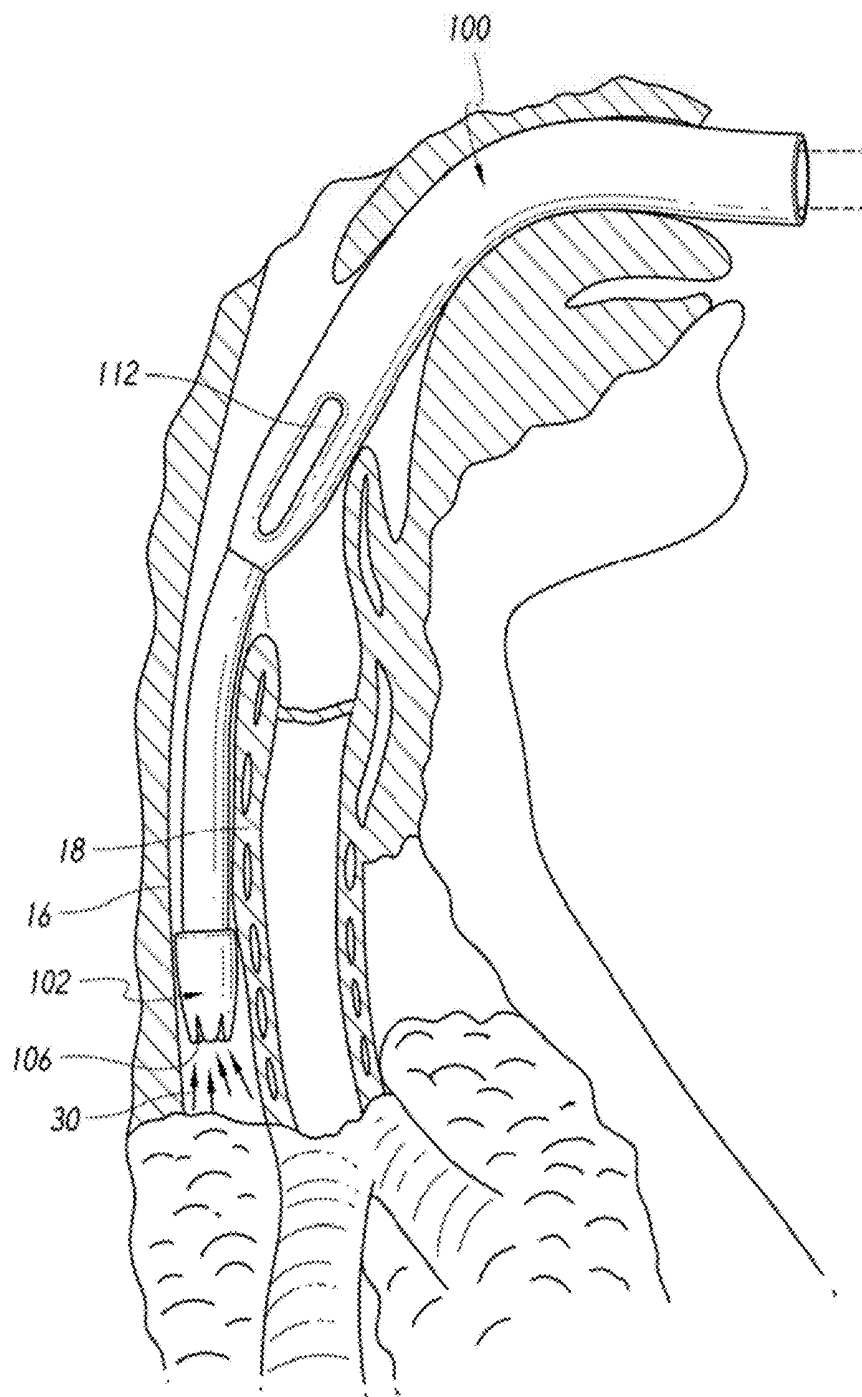


FIG. 5D

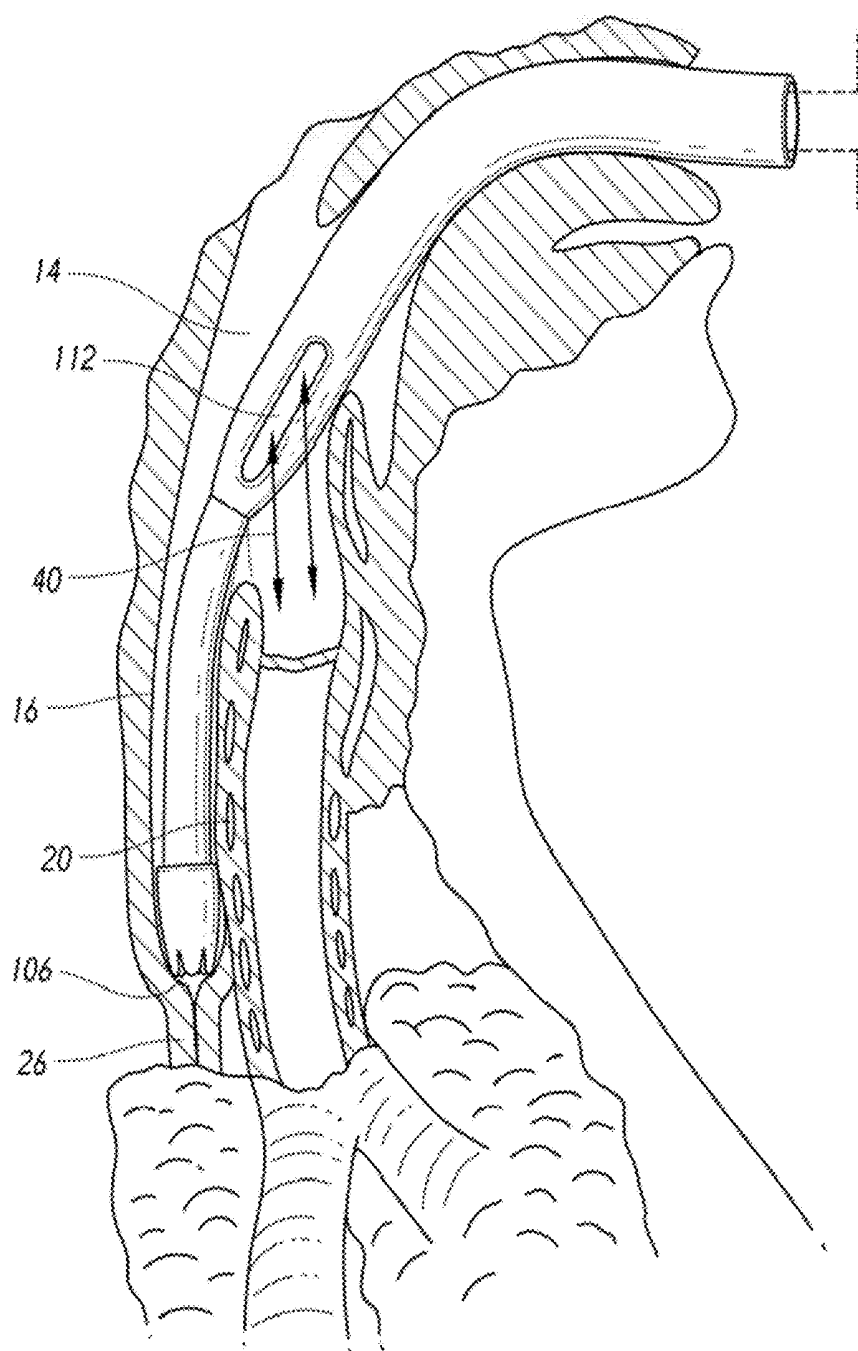


FIG. 5E

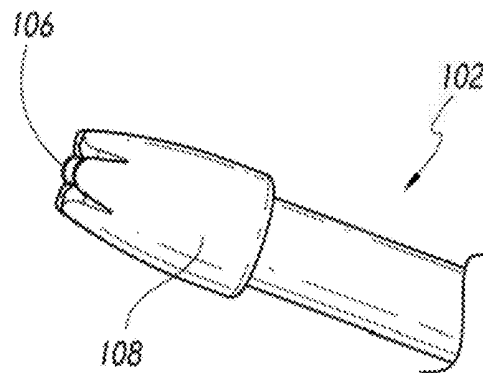


FIG. 6A

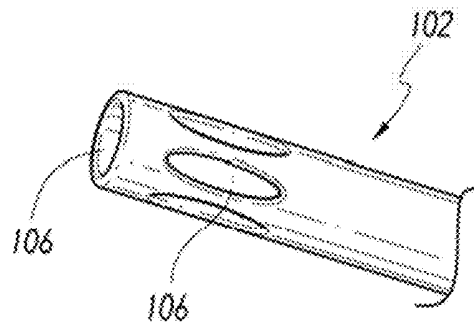


FIG. 6B

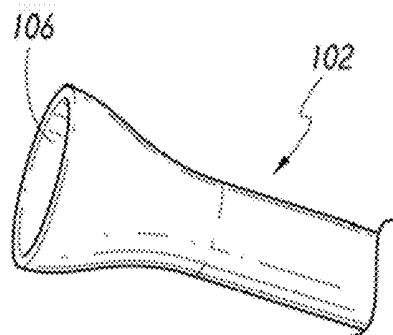


FIG. 6C

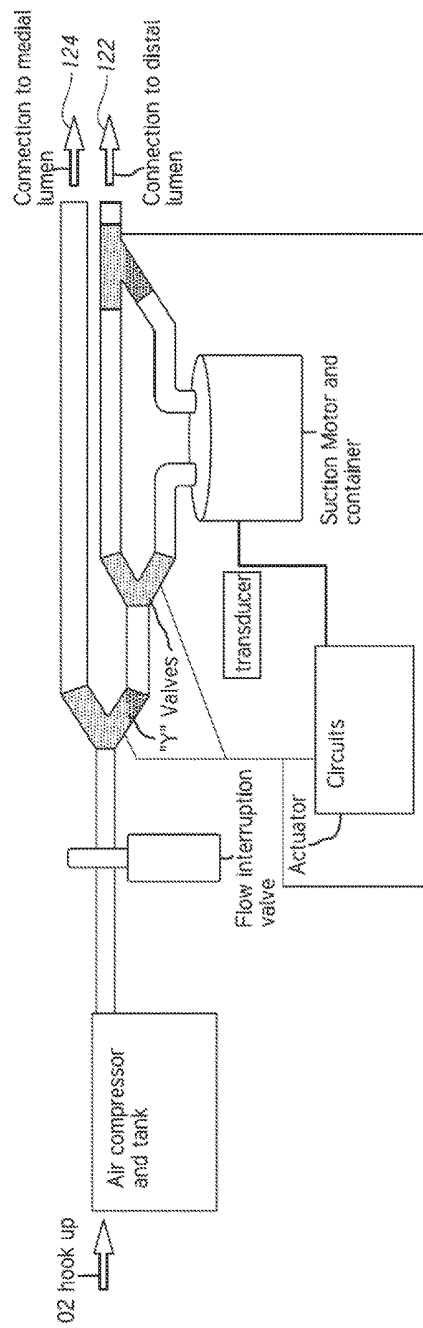


FIG. 7

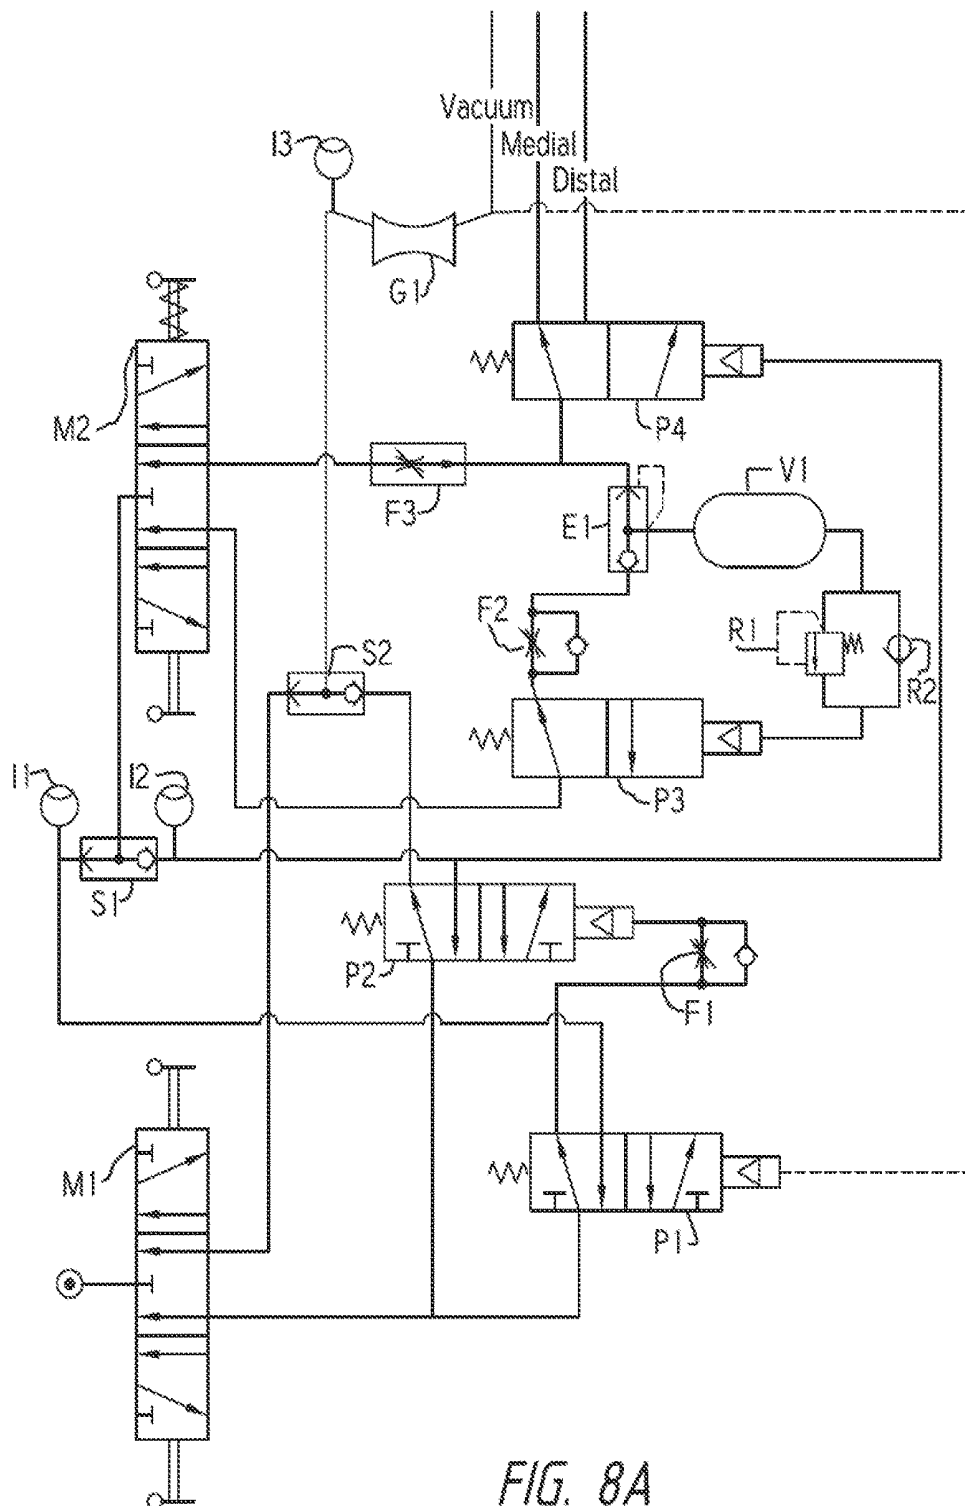




FIG. 8A

	Component	Description	Part		
1	M1	Operation Valve	Clippard TV-40P or Equiv		
2	M2	Mode Valve	TV-4DMP		
3	P1	Medial Supply Valve	MJV-4, Pilot MVA-10		
4	P2	Distal Supply Valve	MJV-4, Pilot MPA-3		
5	P3	Pulse Valve	FV-3P, Pilot MPA-10		
6	P4	Ventilation Selector Valve	FV-3P, Pilot MPA-3		
7	F1	Reset Timing Flow Control Valve	JFC-3AR		
8	F2	Pulse Timing Flow Control Valve	JFC-3AR		
9	F3	On-Demand Flow Control Valve	(10-32 threads)		
10	E1	Accumulator Quick Exhaust	MEV-2		
11	S1	Ventilation Supply Shuttle Valve	MSV-1444		
12	S2	Vacuum Supply Shuttle Valve	MSV-1444		
13	R1	Pulse Pressure Relief Valve	Smart Products, 2x15psi		
14	R2	Pulse Pilot Relief Valve	Smart Products, 0.5psi		
15	I1	Medial Ventilation Indicator	IND-3G		
16	I2	Distal Ventilation Indicator	IND-3G		
17	I3	Vacuum Indicator	IND-3G		
18	G1	Vacuum Generator	SMC		
19	V1	Pulse Accumulator	MAT-4.0		

FIG. 8B

Operational Mode	Manual Valve				Pilot Valve				Indicator			Output			
	1	2	3	4	1	2	3	4	1	2	3	V	M	D	
0	2	(any)	N/A	N/A	N/A	N/A	N/A	N/A	OFF	OFF	OFF				
1	3	(any)	N/A	N/A	N/A	N/A	N/A	N/A	OFF	OFF	ON	✓			
2	1	1	1	1	N/A	N/A	N/A	N/A	OFF	OFF	ON	✓			
3A	1	1	1	2	1	2	2	2	OFF	ON	OFF				
3B	1	1	1	2	2	2	2	2	OFF	ON	OFF			✓	Fixed Vol
4A	1	1	2	1	1	1	1	1	ON	OFF	ON	✓			
4B	1	1	2	1	2	1	1	1	ON	OFF	ON	✓	✓		Fixed Vol
5	1	2	1	2	N/A	2	2	2	OFF	ON	OFF				
6	1	3	1	2	N/A	2	2	2	OFF	ON	OFF			✓	Continuous
7	1	2	2	1	N/A	1	1	1	ON	OFF	ON	✓			
8	1	3	2	1	N/A	1	1	1	ON	OFF	ON	✓	✓		Continuous

FIG. 8C

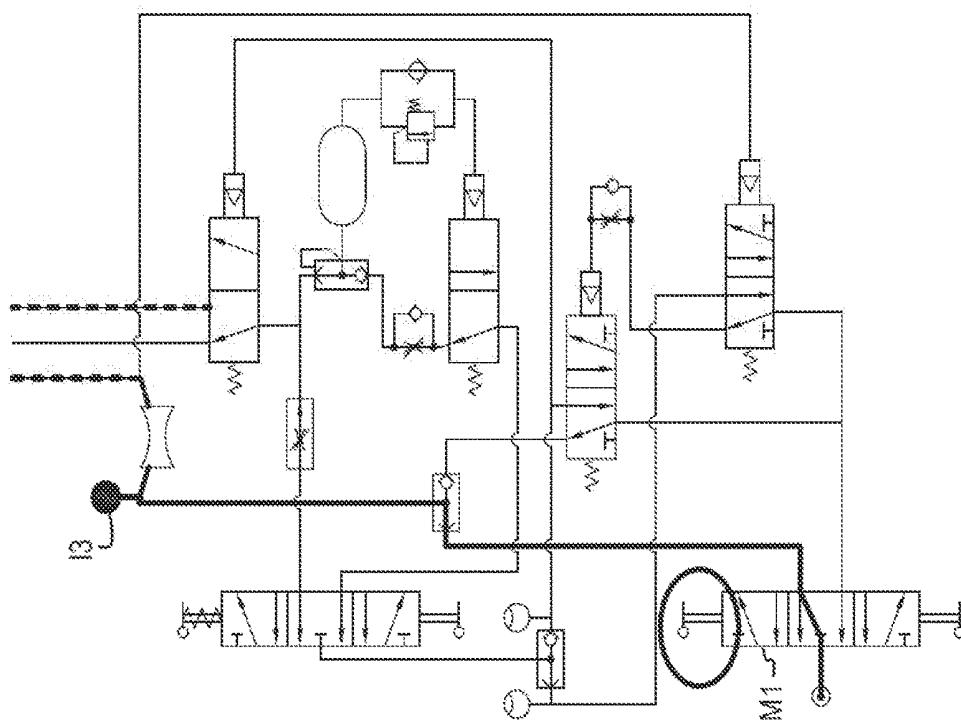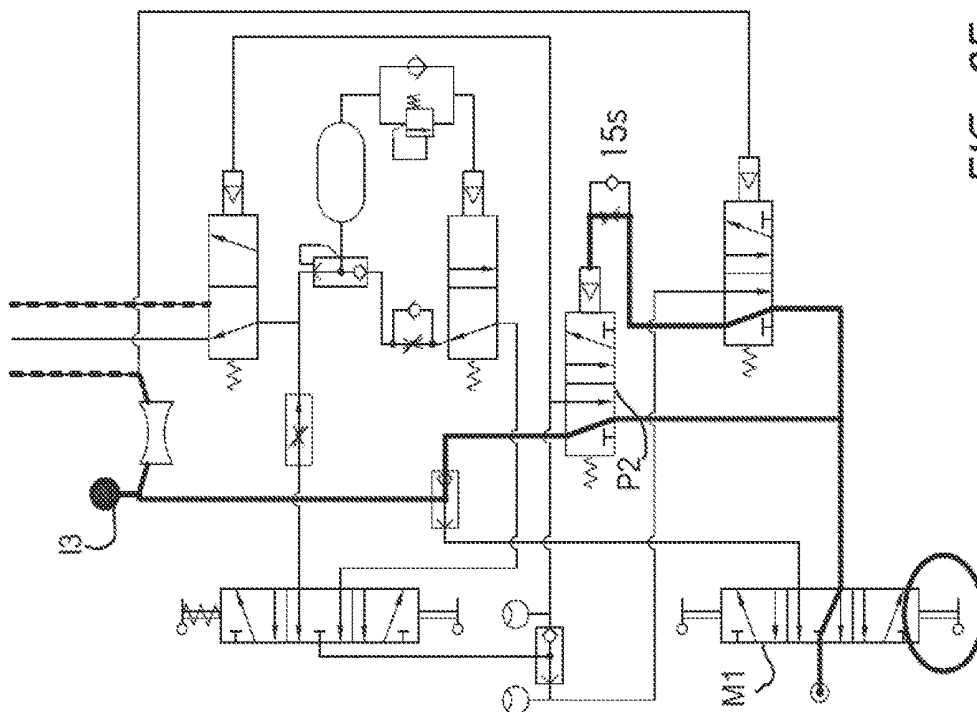

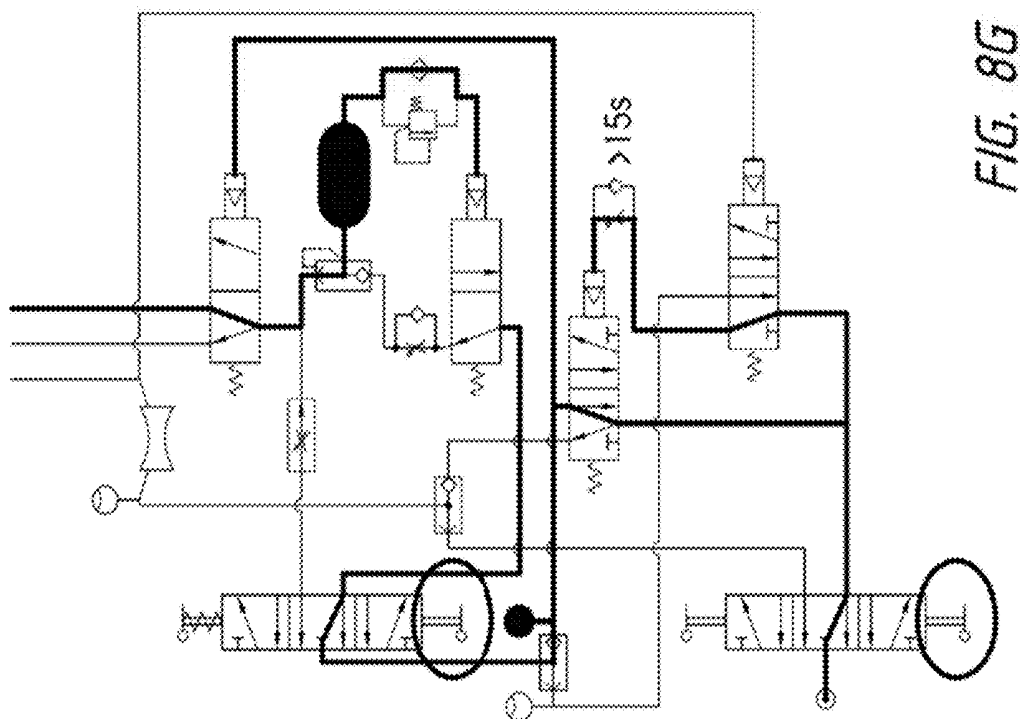


FIG. 8G


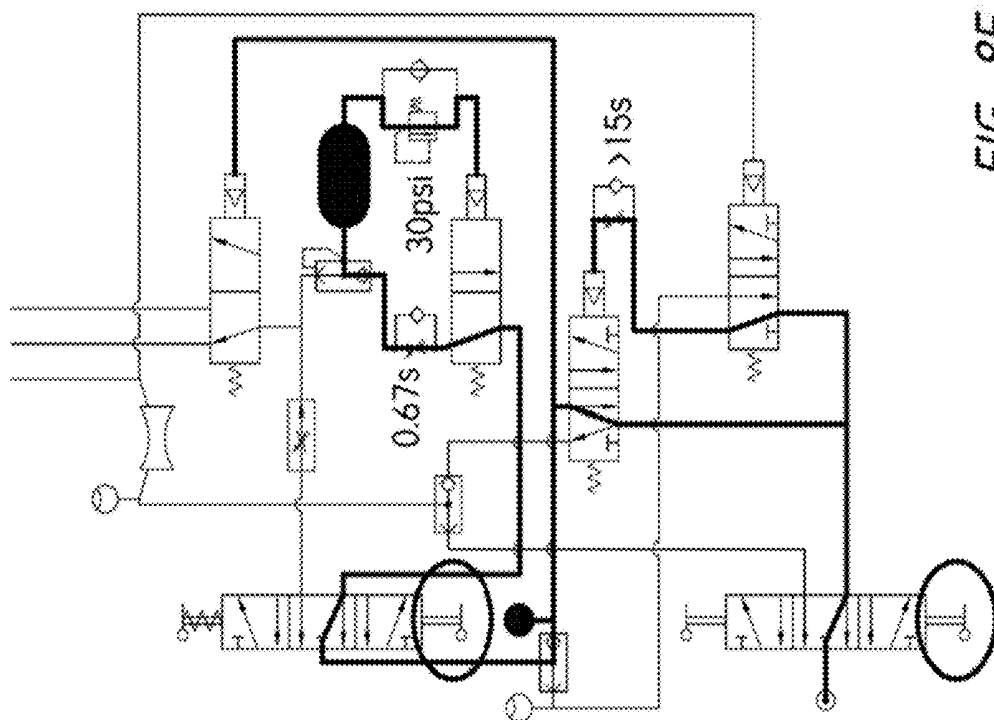


FIG. 8F

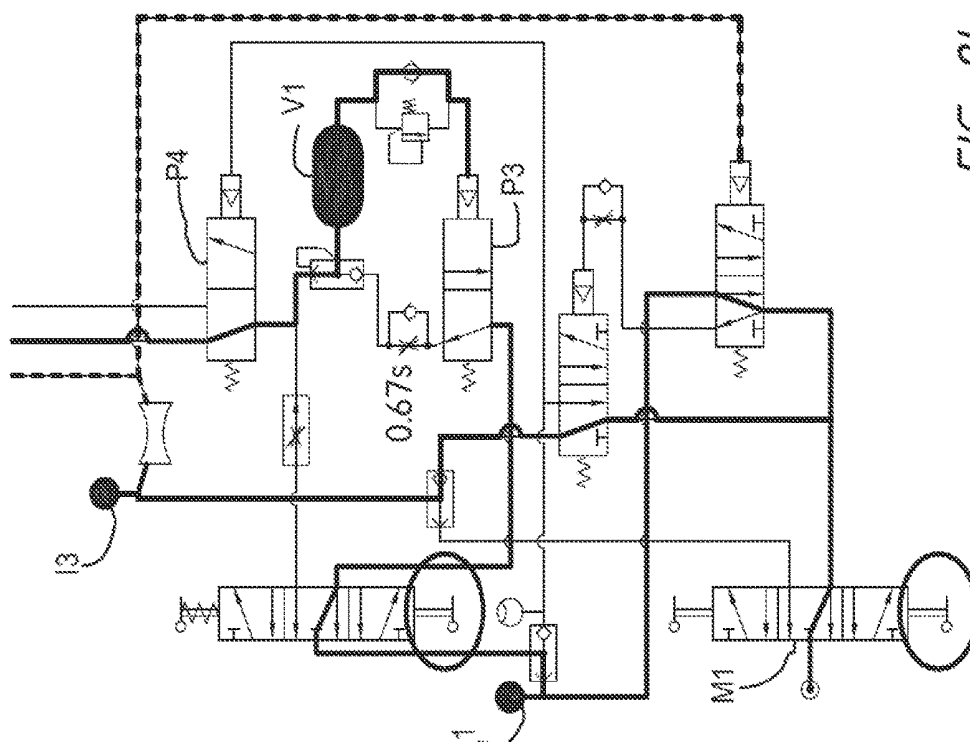

154

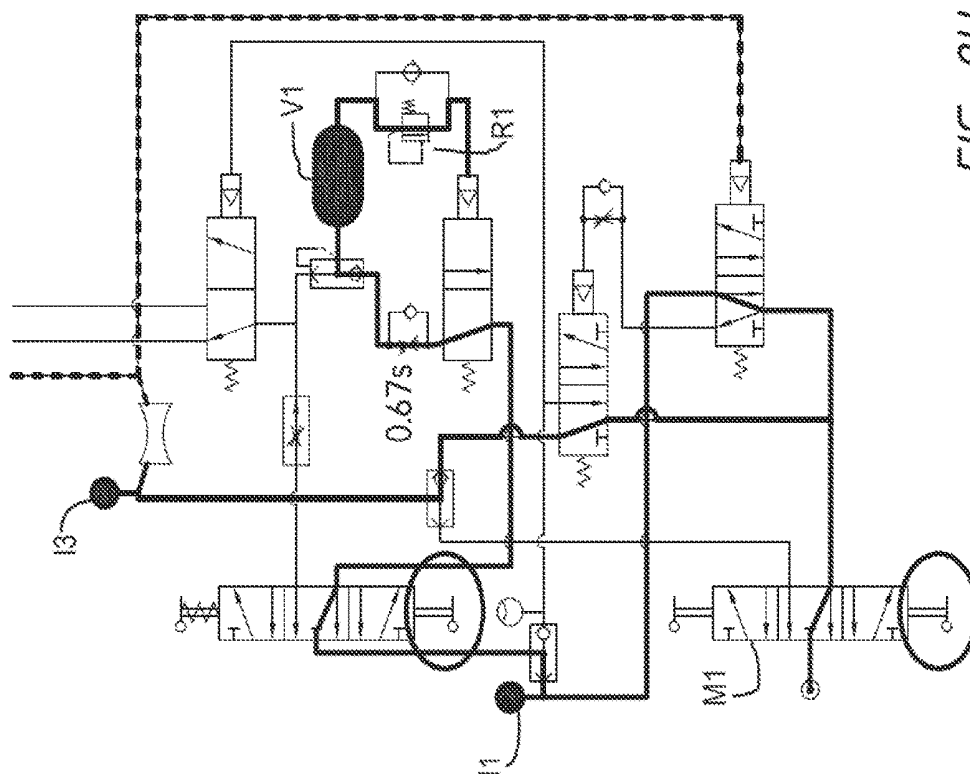


FIG. 84

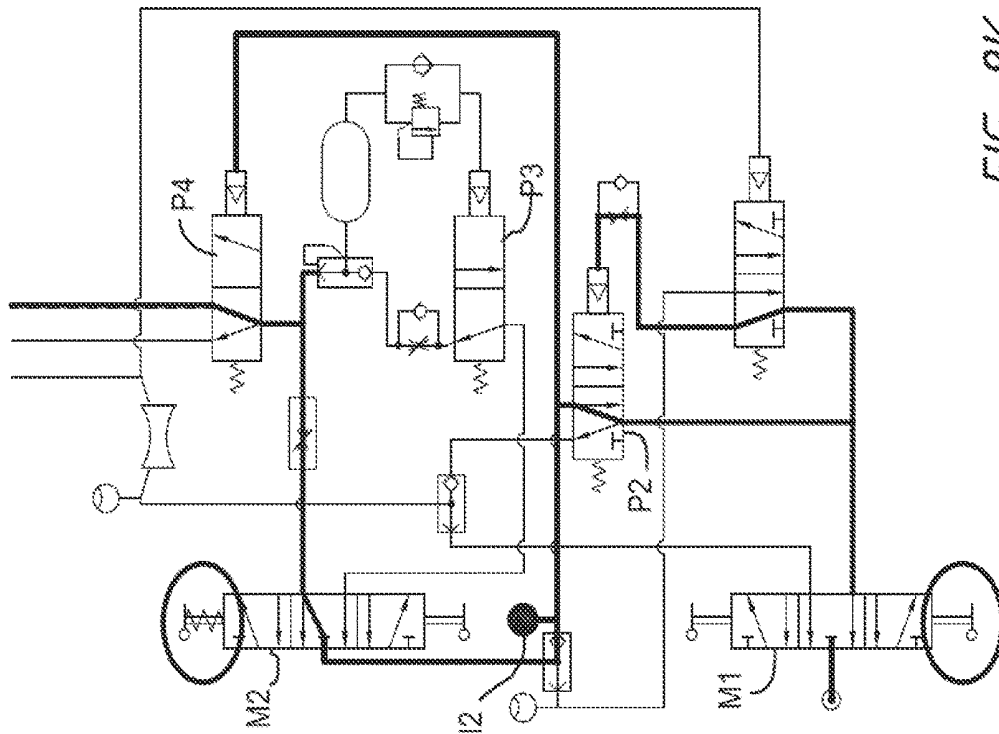


FIG. 8K

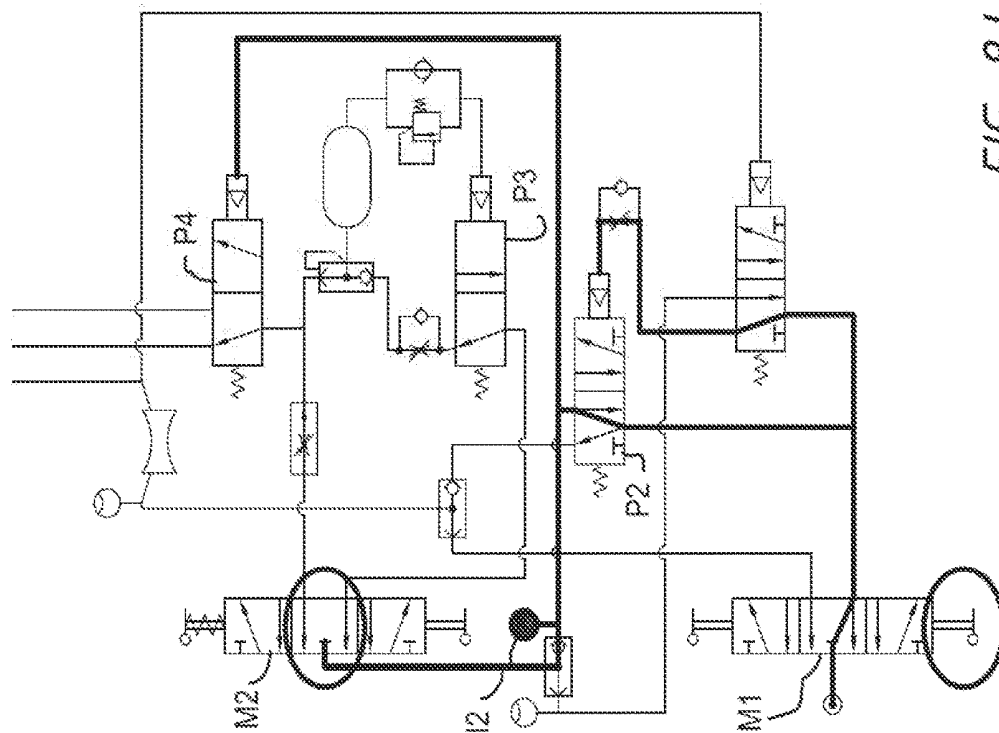


FIG. 8J

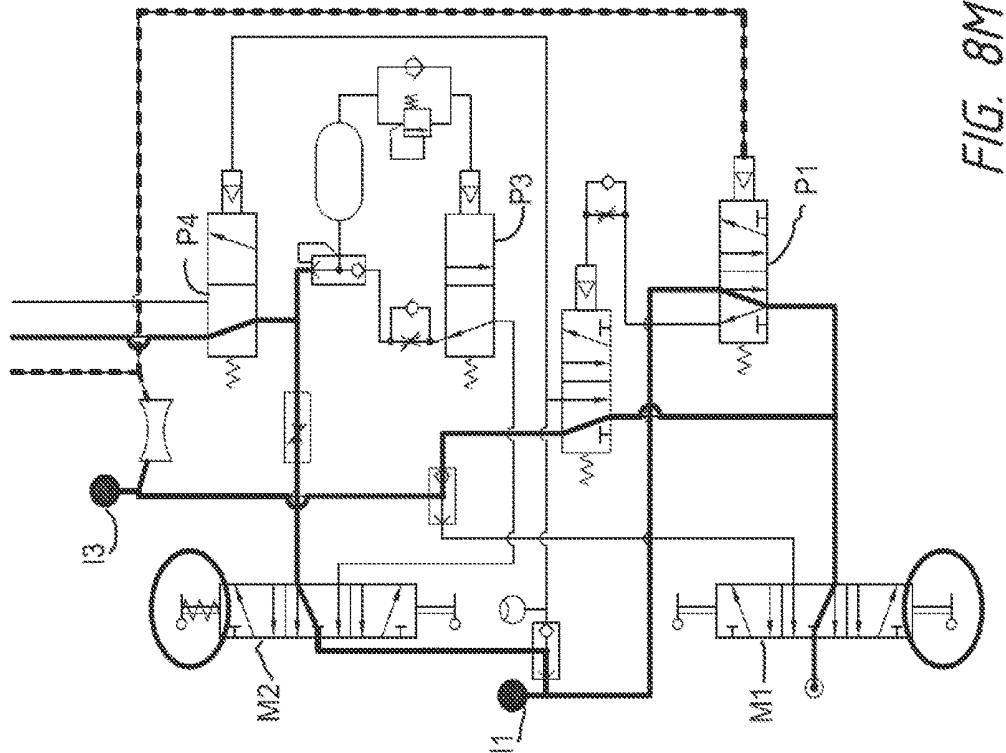


FIG. 8M

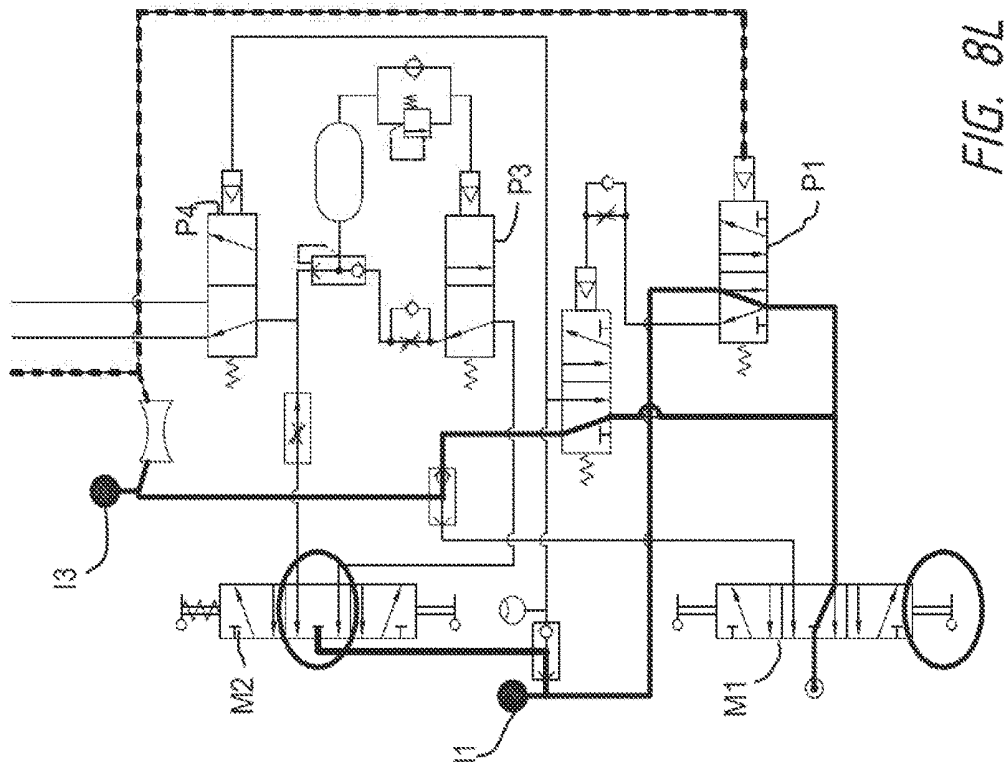


FIG. 8L

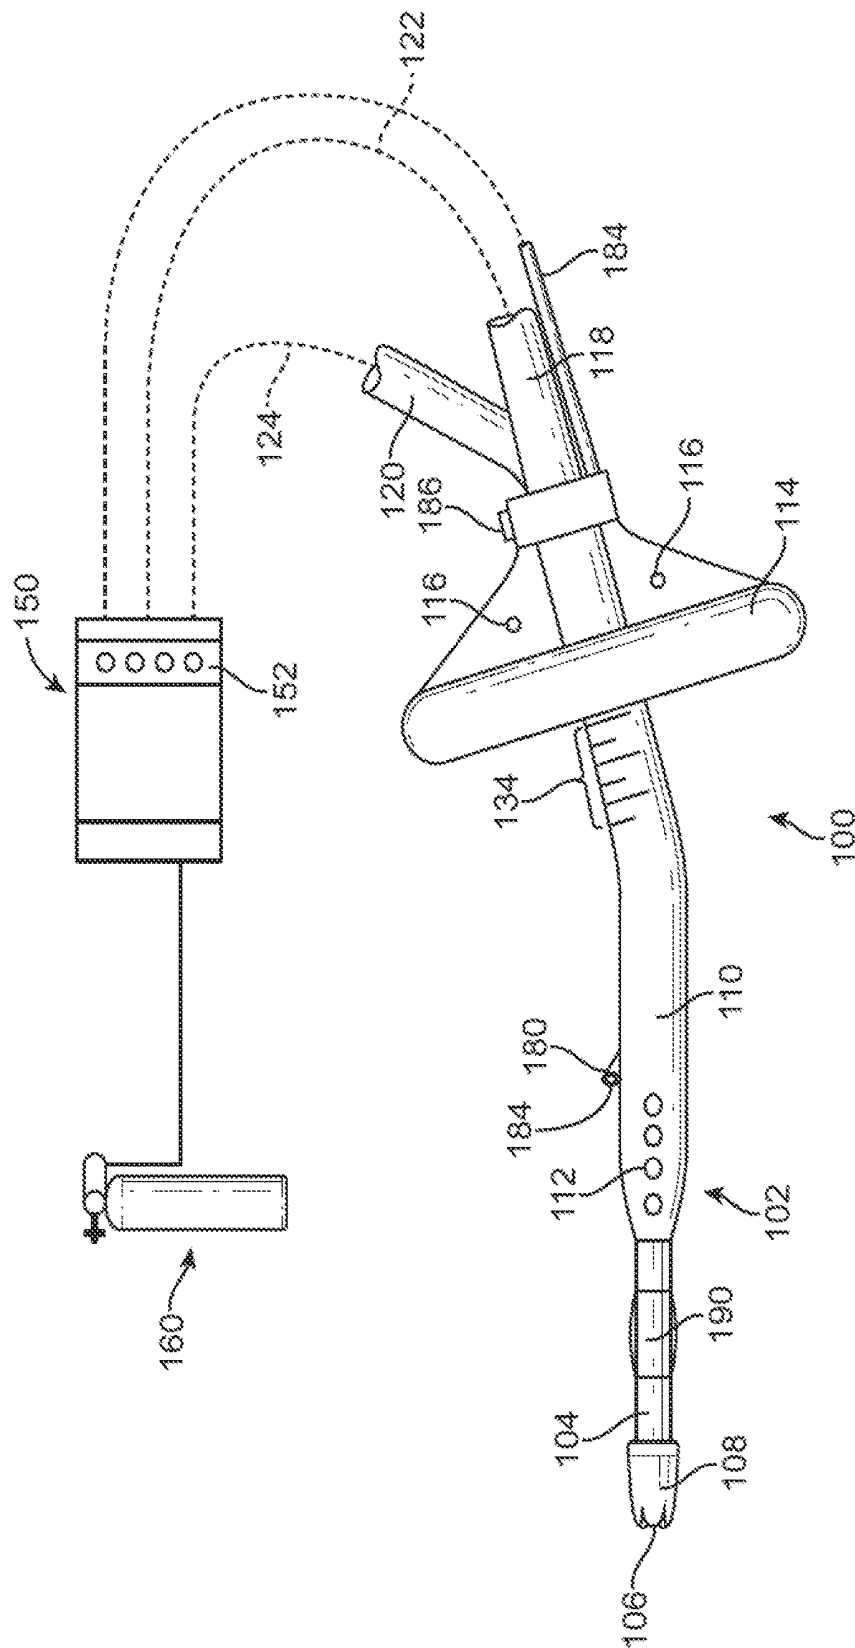


FIG. 9A

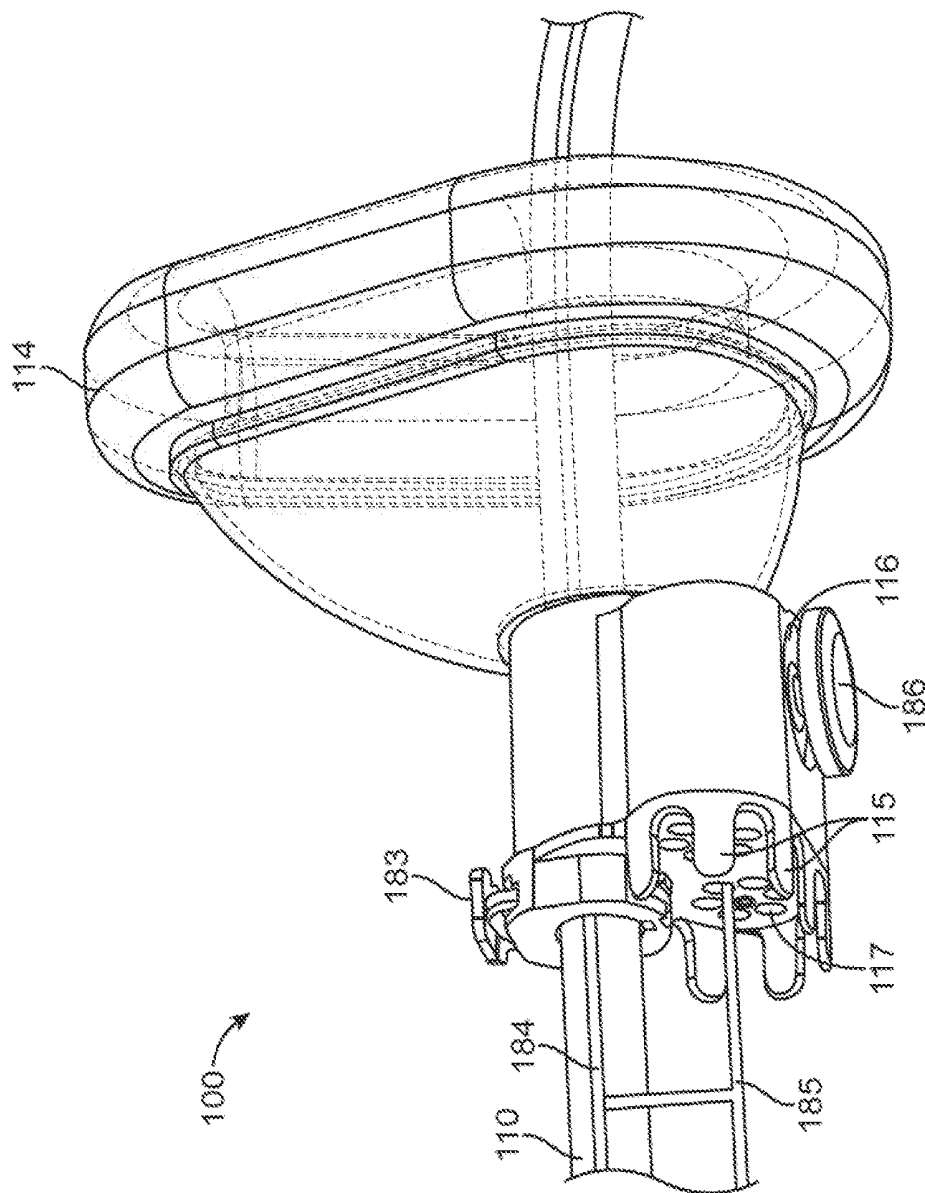


FIG. 9B

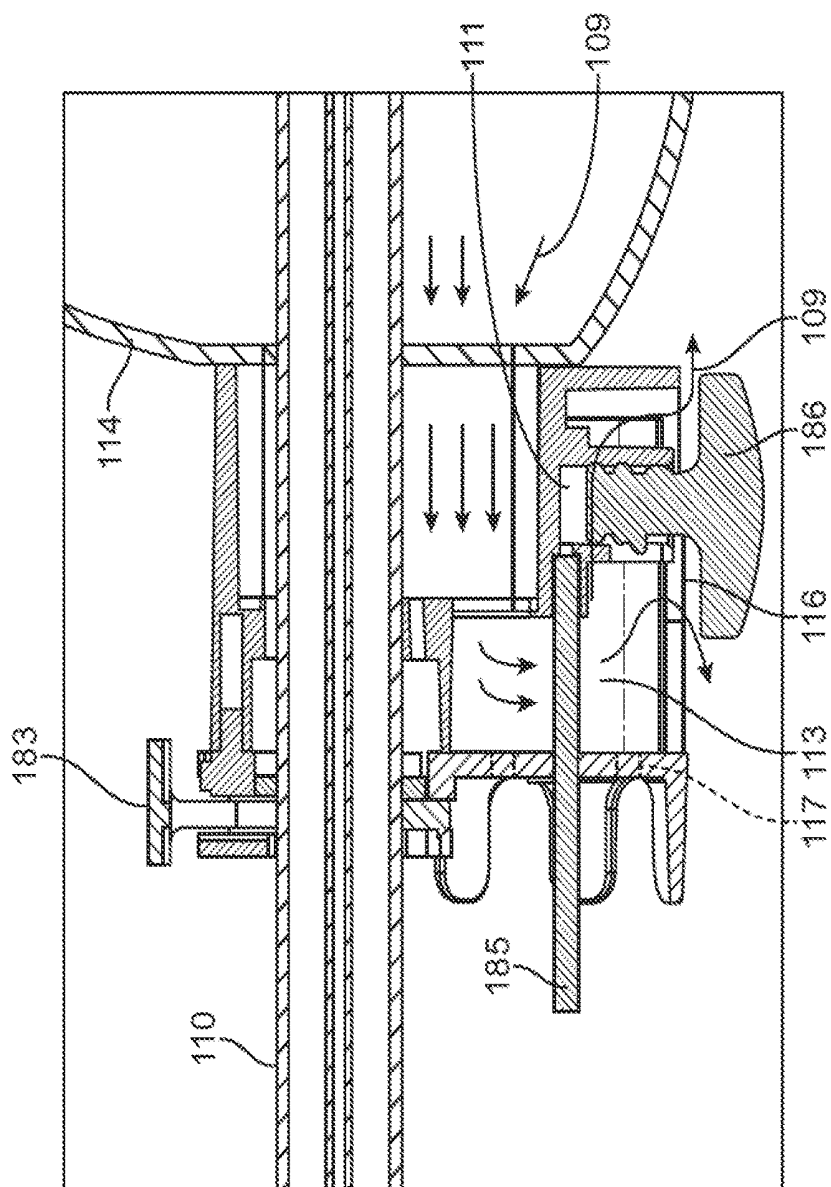


FIG. 9C

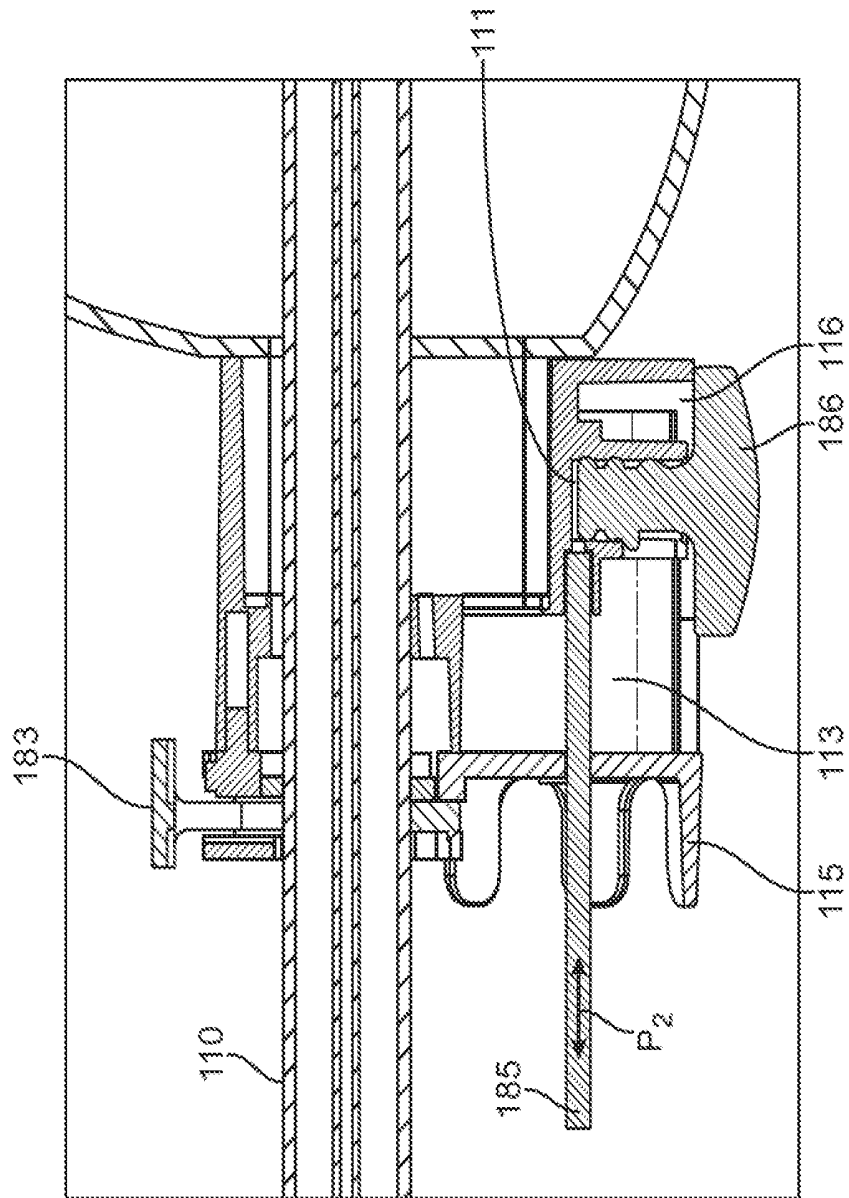


FIG. 9D

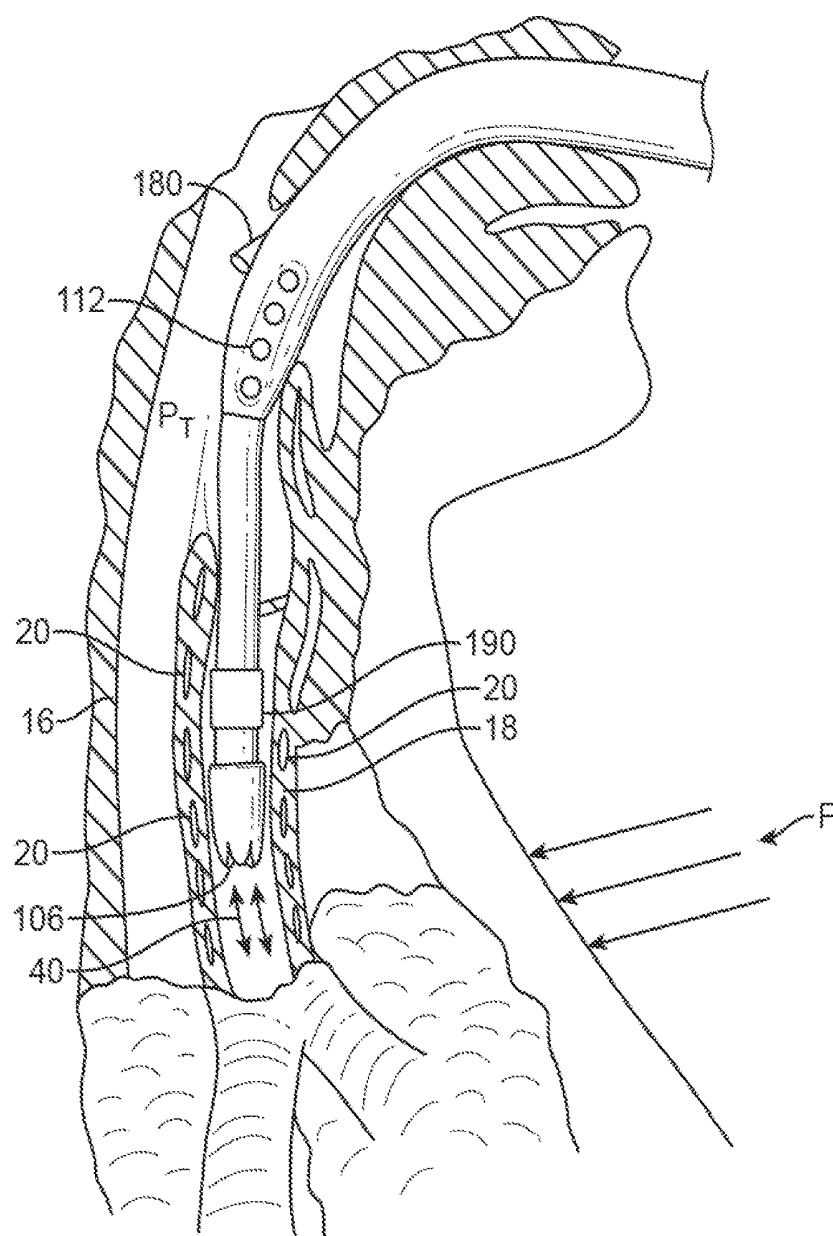


FIG. 10A

FIG. 10B

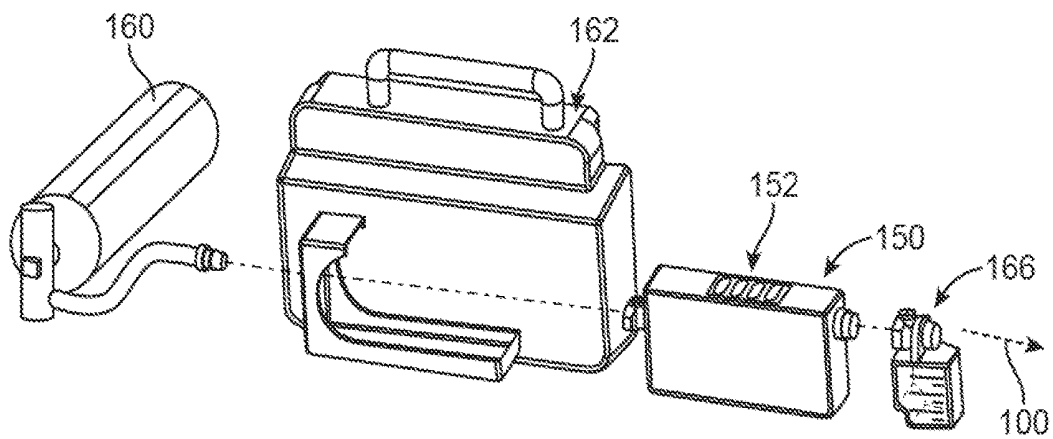


FIG. 11A

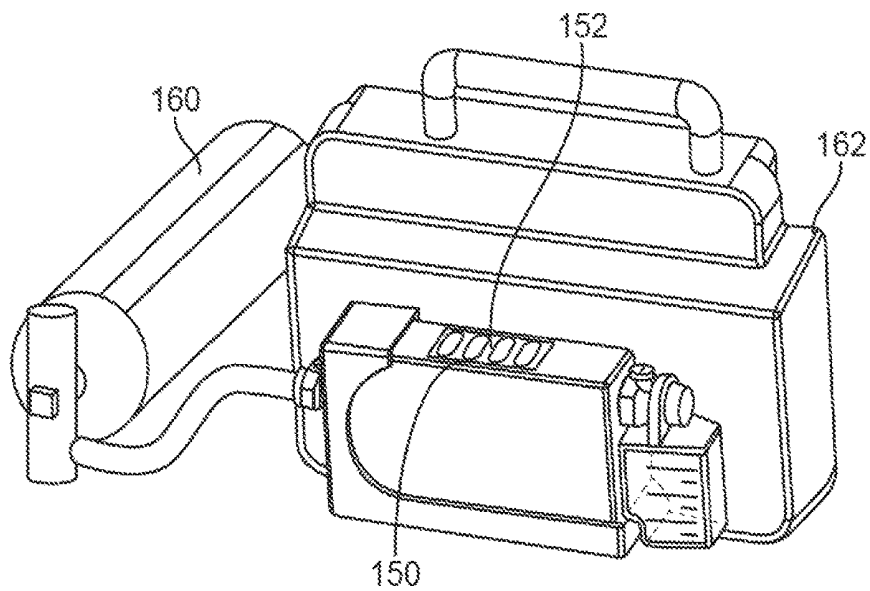


FIG. 11B

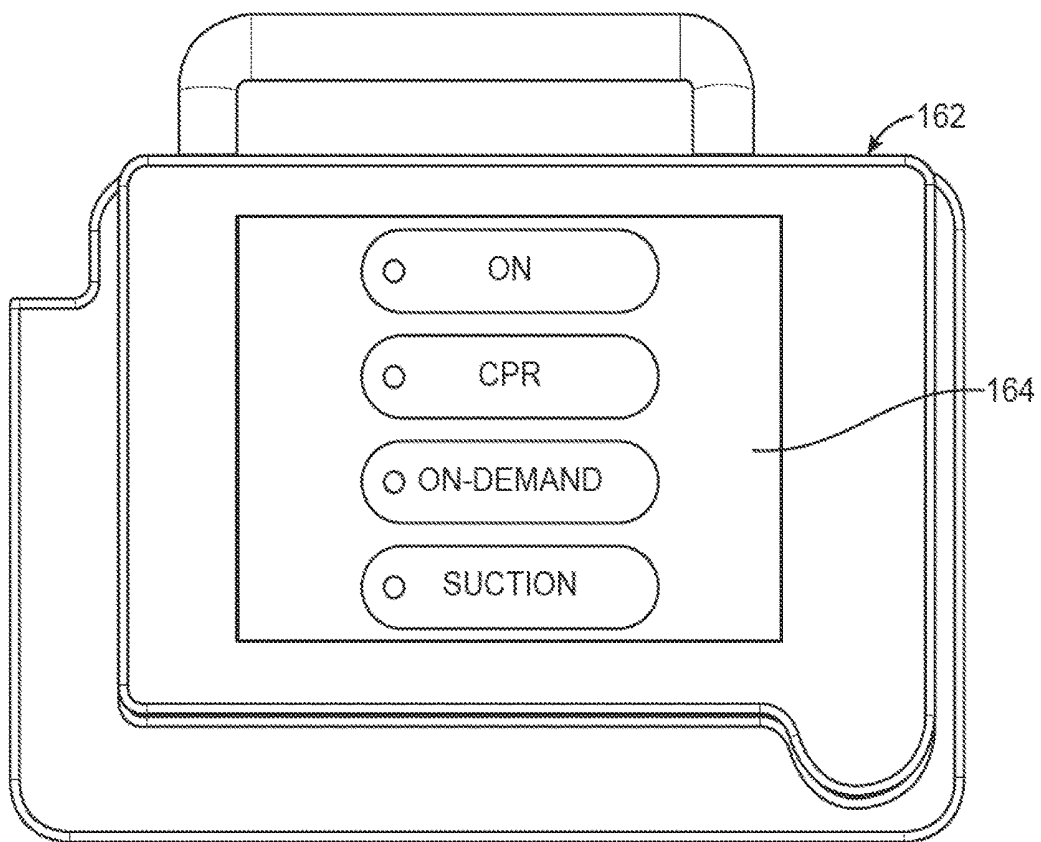


FIG. 11C

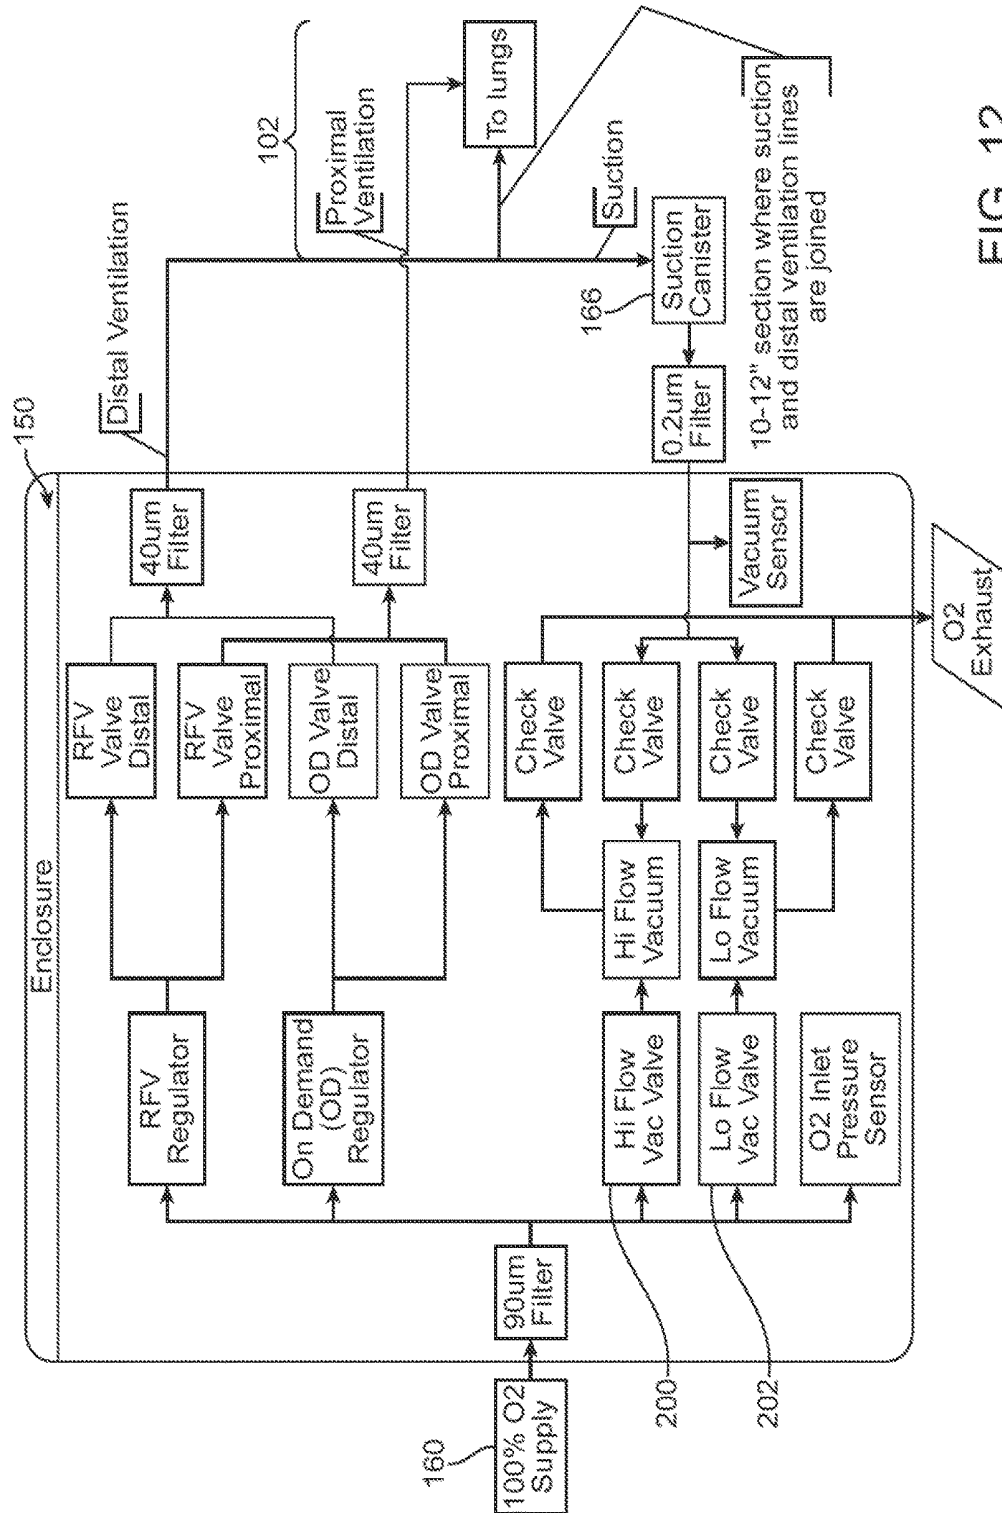


FIG. 12

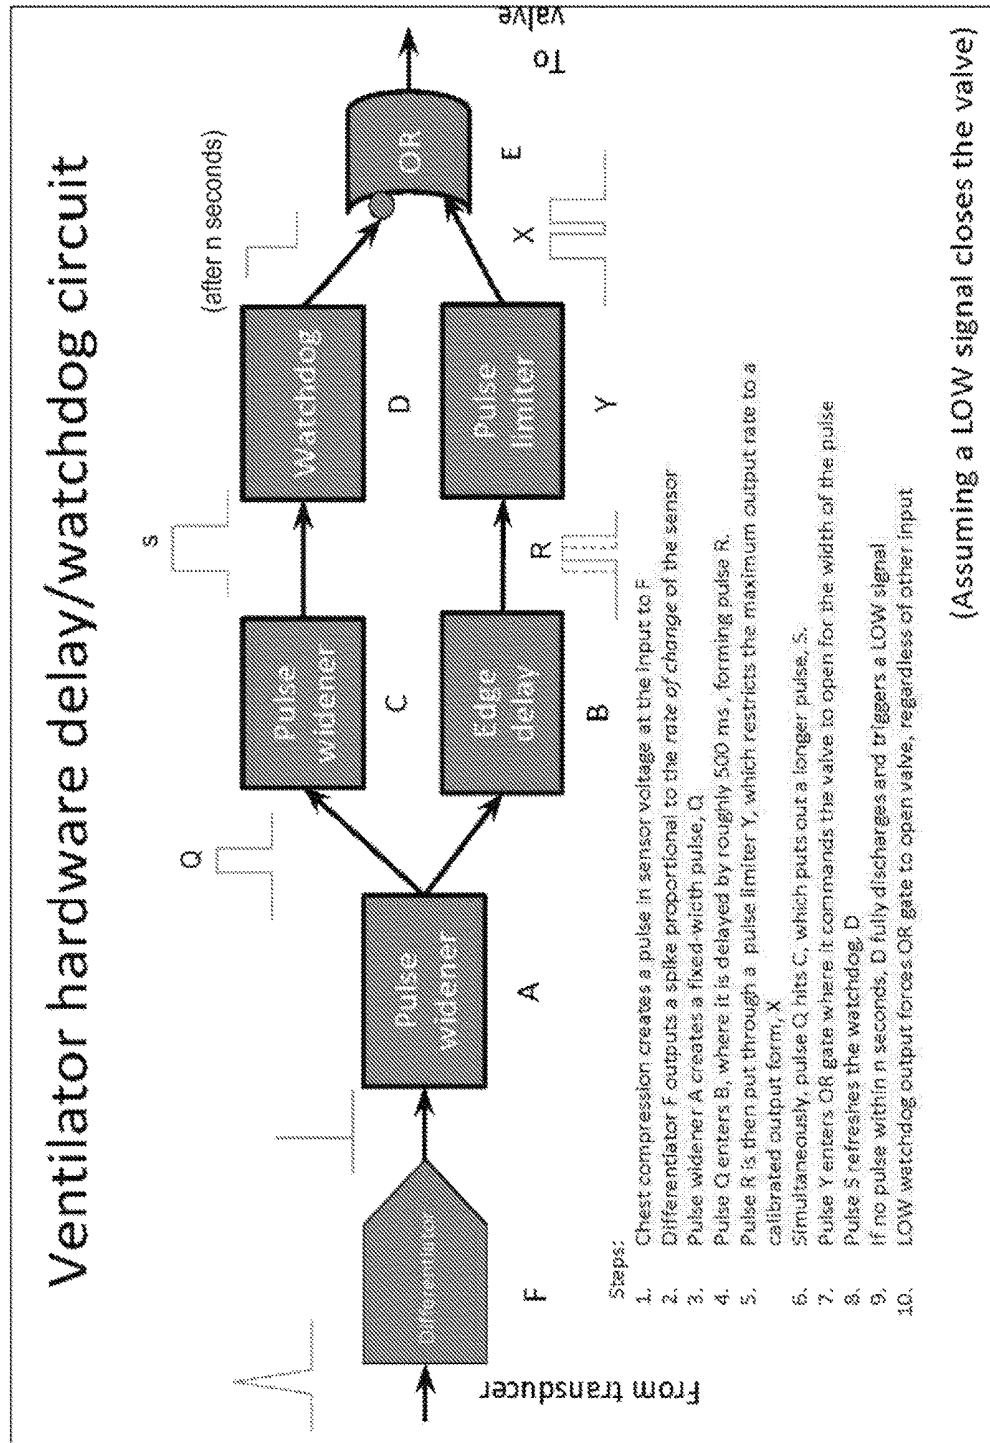


FIG. 13

Dependencies

- Amount of time valve remains open per chest compression is determined by pulse limiter Y
- Minimum spacing between valve openings is determined by pulse limiter Y
- Delay between initial compression and valve opening is determined by B
- Time before timeout is determined by C + D

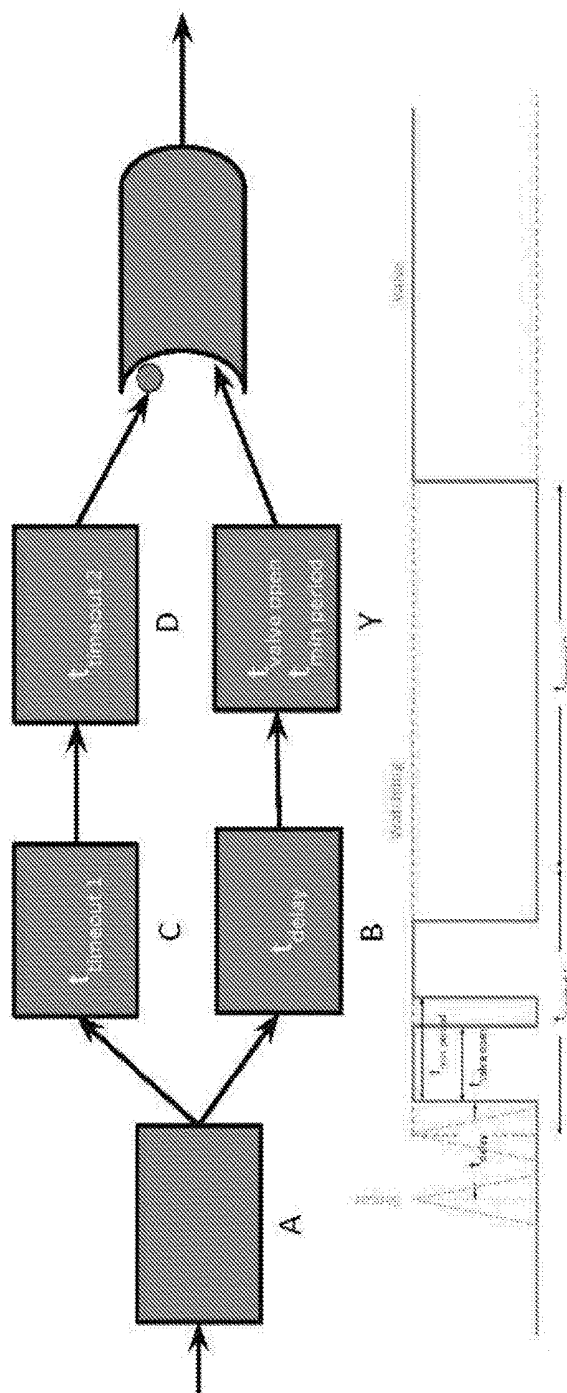


FIG. 14

Differentiator

- Given an input pulse, generates an output signal proportional to the rate of change of the input by a factor k
 - Only responds to rising edges
- Allows for exclusion of steady-state strain on sensor due to a bend in tube; extracts only transient compressions

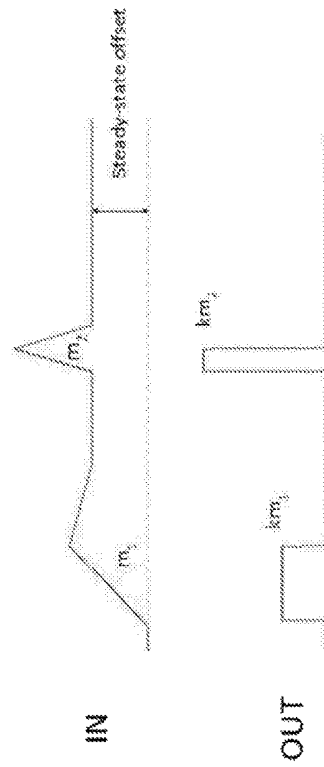


FIG. 15

Pulse widener (A & C)

- Goes HIGH when hit with a rising edge
- Stays HIGH for user-adjustable amount of time (t_1)
 - Does not extend time on if sees another rising edge when already HIGH
- Goes LOW until next rising edge

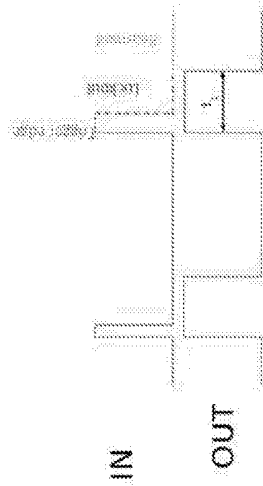


FIG. 16

Edge delay (B)

- Shifts an entire pulse by a user-adjustable amount (t_1)




FIG. 17

Pulse limiter

- Performs three operations:
 1. Generates a period-limiting pulse- this determines the maximum frequency of valve openings the system will perform
 2. Extracts the leading edge of the pulse- this ensures that the valve only fires *once* per chest compression
 3. Uses the leading edge to trigger an on-time pulse- this is tuned to allow for a full cycle of the valve
- Resulting output has a limited frequency, and a fixed on-time.
 - Frequency is limited to roughly 100 bpm
 - On time is calibrated to allow full pneumatic cycling
 - Any chest compressions performed before the end of the period limit are ignored
 - Valve opening always coincides with a chest compression, although not all chest compressions will generate a pulse (for too-fast compressions)

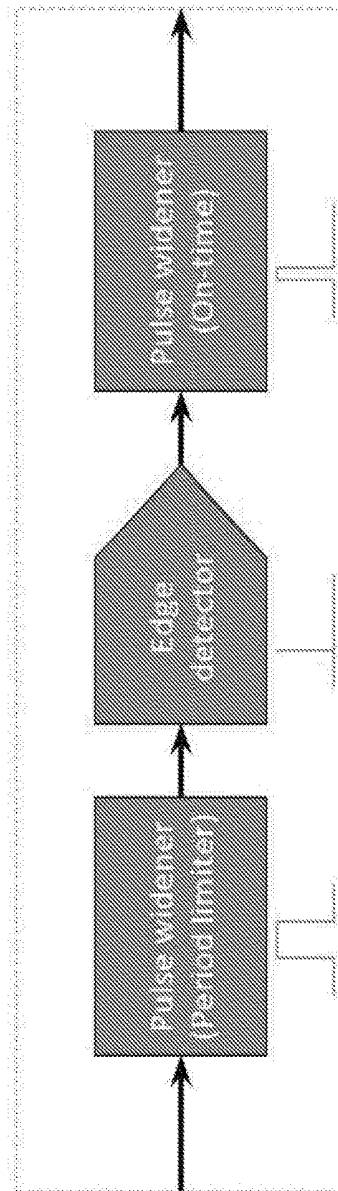


FIG. 18

Pulse limiter (2)

- Output form has two parameters:
 - Period limit
 - On time



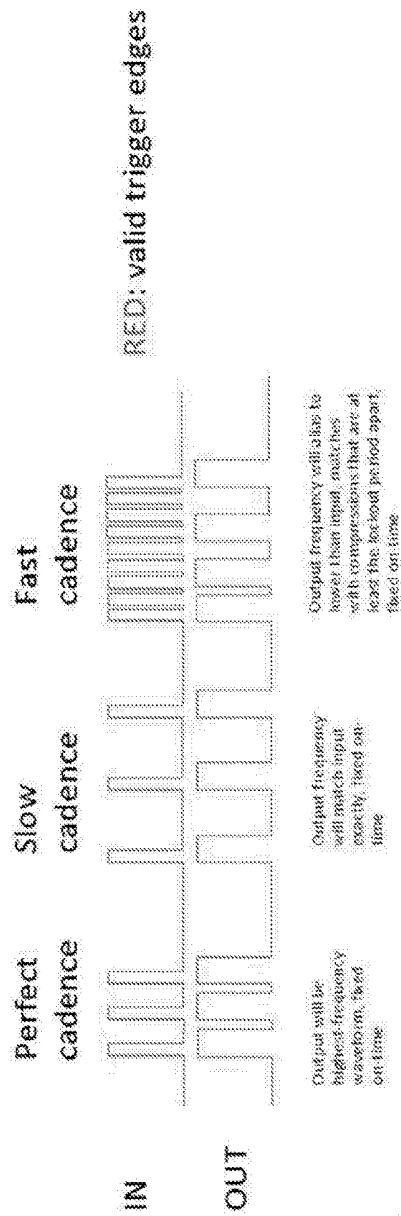


FIG. 19

Watchdog (D)

- Drains charge with a user-adjustable time constant
- A HIGH pulse will recharge the watchdog for the duration of the pulse
- Once the watchdog goes below a threshold (V_{low}), it outputs a LOW signal until recharged above another (V_{high}).

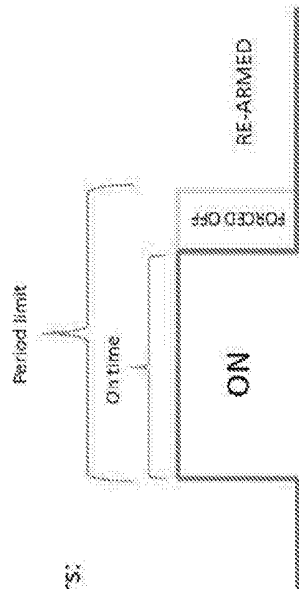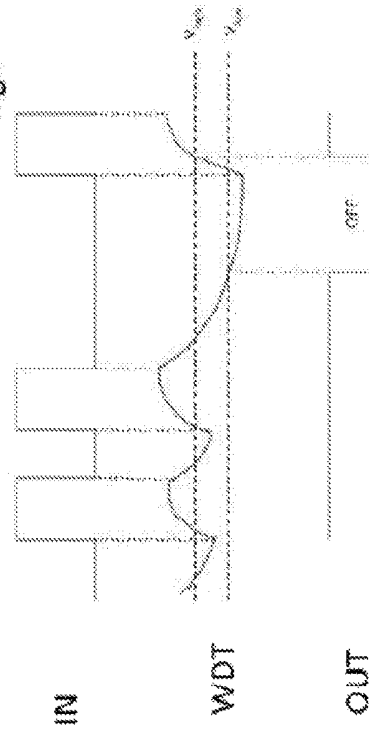

2/7/2014

FIG. 20

OR gate (E)

- Outputs a HIGH signal if either input is HIGH
- In this implementation, a LOW output closes the valve
 - The watchdog input is inverted before going into the gate

LOW	HIGH	LOW	HIGH	OPEN	Timeout
LOW	HIGH	HIGH	HIGH	OPEN	Timeout (during a chest compression- not actually possible to reach this state)
HIGH	LOW	LOW	LOW	CLOSED	Between chest compressions, not timed out
HIGH	LOW	HIGH	HIGH	OPEN	500 ms after a chest compression, opening valve to admit air, not timed out

FIG. 21

Possible improvement

Period limiter may be unnecessary; pulse widener A could perform the same function.

- Currently, widener A serves only to de-noise output of differentiator F.
- Pulse width output of A has a minimum value above what is necessary for denoising; edge delay B requires a minimum pulse width to function (acts as a low pass filter).
- There is no point in picking up spikes exiting F faster than the period limit; pulse limiter will alias them regardless.
- As such, extending the pulse width of A and removing the period limiter from the pulse limiter would be functionally identical with one fewer degree of freedom.

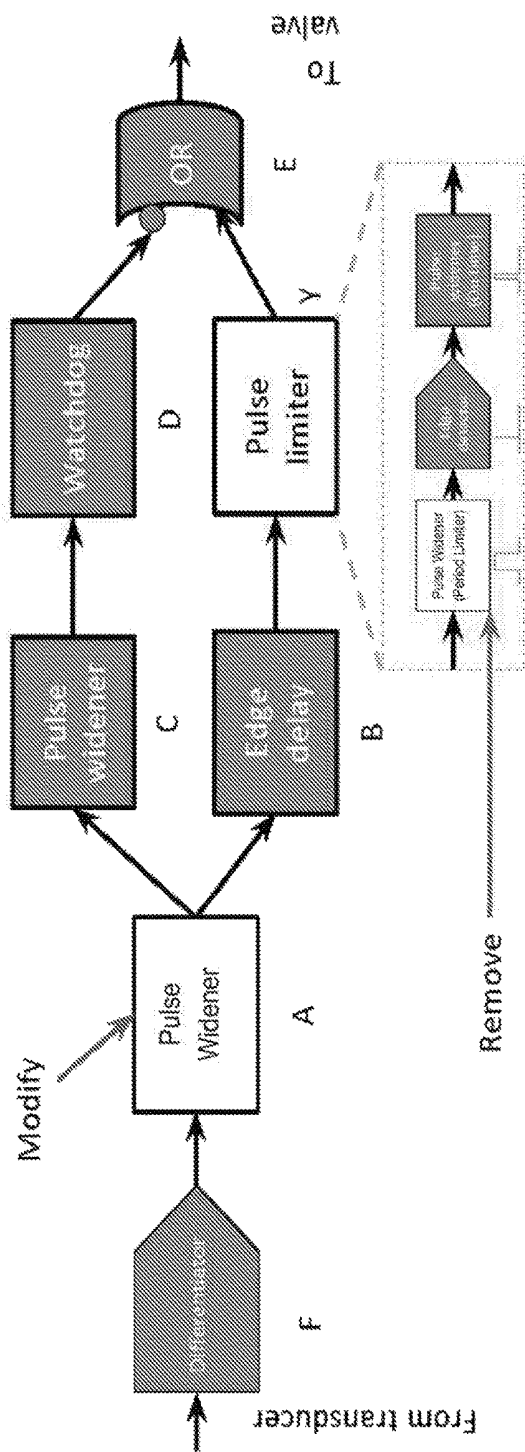


FIG. 22

APPARATUS AND METHOD FOR IMPROVED ASSISTED VENTILATION

CROSS-REFERENCE TO RELATED APPLICATIONS

The present is a non-provisional application of U.S. Provisional Application 61/969,043 filed Mar. 21, 2014 and is a continuation-in-part of U.S. patent application Ser. No. 14/296,298 filed Jun. 4, 2014 which is a continuation of U.S. patent application Ser. No. 13/659,699 filed Oct. 24, 2012 (now U.S. Pat. No. 8,776,796 issued on Jul. 15, 2014) which claims benefit to U.S. Provisional Application No. 61/569,569 filed Dec. 9, 2011, the content of each of which is incorporated herein by reference in its entirety. The present application also incorporates PCT Application No. PCT/US2015/022079 filed Mar. 23, 2015 in its entirety by reference herein.

BACKGROUND OF THE INVENTION

Intubation is the placement of a tube of an intubation device into an airway lumen of the body of a patient to provide assisted ventilation of the lungs to maintain a supply of oxygen to the blood in those cases where the patient is unable to breathe on his or her own. Intubation in cases of respiratory distress involves the placement of a tube into the trachea of the patient. Tracheal intubation also involves the positioning of an endotracheal tube into a patient's trachea through the vocal cords, so the caregiver must also be careful to avoid injuring the vocal cords. In many cases, care must be taken when intubating a patient since improper placement of the tube can result in additional harm to the patient. For example, many conventional intubation devices rely on an inflatable cuff that forms a seal against the lumen wall to maintain a position of the tube within the lumen. Over-inflation of the cuff, can cause internal bleeding in the patient. Another significant problem is that extreme care must be taken to avoid positioning the intubation tube within the esophagus rather than the trachea. In such cases, with conventional devices, the first responder or medical practitioner cannot properly ventilate the patient and the patient can suffer further injury.

Even properly trained medical caregivers and first respondent must proceed with caution during intubation to avoid misplacement of the intubation device or to avoid, unwanted insertion errors and risk of injury. Delay and/or misplacement of the endotracheal tube, such as misplacement of the endotracheal tube into the esophagus, can potentially result in neurological damage or death. Improper positioning of the endotracheal tube also can compromise airway protection or result in inadequate ventilation. It is therefore imperative to intubate a patient quickly and position the endotracheal tube correctly when a medical condition arises.

To reduce the risk of complications during intubation, the caregiver, whether a first responder, such as an emergency medical technician, paramedic, or a nurse or physician must proceed as quickly as possible yet with caution to avoid, the potential complications. In addition, a first responder must often attempt to intubate the patient in a less than desirable location, such as a bathroom, restaurant, or other area not conducive to providing proper medical treatment and care.

Assisted ventilation in cases of cardiac arrest also requires prompt and accurate placement of an intubation device within the trachea so that chest compressions can occur. In such cases, intubation allows for ventilation of the lungs and

a supply of oxygen to the blood while chest compressions provide circulation of the blood.

The American Heart Association's protocols for cardio pulmonary resuscitation (CPR) previously required pausing after every fifteen chest compressions to allow for two ventilations. The American Heart Association's 2010 protocols decreased the frequency of ventilations such that chest compressions are to be paused after every thirty compressions to allow for two ventilations. It is believed that the main reasons supporting the change in protocol are: 1) reduce the amount of intra-thoracic pressure associated with positive pressure ventilations since positive pressure ventilations decrease the efficiency of the heart; and 2) to minimize the interruptions of chest compressions to maintain constant arterial pressure. Accordingly, now most caregivers only simultaneously ventilate the patient and provide compressions if the patient is properly intubated.

FIG. 1 provides a partial view of a patient's oral cavity 10, tongue 12 and pharynx 14 where the pharynx 14 is the membrane-lined cavity at the rear of the oral cavity 10. The pharynx 14 includes openings of the esophagus 16 and trachea 18. As shown, the openings to the esophagus 16 and trachea 18 are adjacent to one another. When a medical caregiver attempts to intubate a patient, the caregiver shall attempt to position the intubation device within the trachea 18 to provide oxygen to the lungs 2. As noted above, the caregiver shall attempt to avoid positioning the intubation device within the esophagus 16 and in doing so often must proceed slowly and with caution to avoid causing undesired trauma to vocal cords or other structures within the body.

The wall of the esophagus 16 is composed of striated and smooth muscle. Since the esophagus 16 relies on peristalsis to move food downward towards the stomach, the walls of the esophagus 16 are naturally compliant and do not have any structural reinforcement. The trachea 18, on the other hand, is relatively stronger and is naturally designed not to collapse given its function of transporting air to the bronchi and lungs 2. The wall of the trachea 18 includes a number of cartilaginous semicircular rings 20 that prevent the trachea 18 from collapsing. The trachea 20 lies anteriorly to the esophagus 16 where the openings of the esophagus 16 and trachea are separated by a tiny flap, the epiglottis 22. The epiglottis 22 protects the trachea when the individual swallows food or other substances.

FIG. 2 illustrates a conventional device 50 used for intubating a patient. As shown, the device 50 is inserted through the mouth and oral cavity into the trachea 18. The caregiver must navigate the device 50 into the trachea 18 rather than the esophagus while traversing the epiglottis 22 and vocal cords 24. The caregiver must take particular care to avoid causing damage to the vocal cords 24. Once properly positioned, the caregiver can optionally inflate 52 a balloon on the device 50 to anchor the device within the trachea 18. After the caregiver confirms placement of the device 50, ventilation of the patient can take place.

Presently, the Combitube, supplied by Nellcor, is commonly used for airway management. The Combitube, also known as a double-lumen airway, is a blind insertion airway device (BIAD) used by first responders as well as in an emergency room setting. The Combitube is intended to allow for tracheal intubation of a patient in respiratory distress by use of a cuffed, double-lumen tube. The double lumen tube is inserted into the patient's airway to allow for ventilation of the patient's lungs. Inflation of the cuff allows the device to function similarly to an endotracheal tube and usually closes off the esophagus, allowing ventilation and preventing pulmonary aspiration of gastric contents.

However, placement of traditional intubation devices is very difficult due to the risk of improperly positioning the device. The risk of a device being improperly positioned can be fatal if not recognized. The conventional devices described above require positioning by an individual that is well trained in positioning such devices. Furthermore, even well trained individuals must proceed with caution when placing conventional devices.

In addition, there remains a need to improve timing of air delivery during artificial ventilations of a patient. This need especially remains where the patient is experiencing distress and requires both ventilation for oxygen and chest compression to re-establish blood circulation. Presently, if the act of artificially ventilating the individual (e.g., through assisted ventilation or mouth-to-mouth) and providing chest compressions is not timed, such as during normal CPR, normal artificial ventilation of the individual can work against the effectiveness of the compression. For instance, assisted ventilation by repeatedly delivering a large bolus of air can raise the pressure within the thoracic cavity and increase resistance by raising pressure on the heart. This back pressure can prevent the heart and lungs from filling with blood. As a result, impeding the ability of the heart and lungs to fill with blood, makes the chest compression less effective as a lower volume of blood is circulated after the compression.

There remains a need for a ventilation device and/or system that can effectively ventilate individuals and can be effectively positioned with minimal training required by the caregiver. In addition, there remains a need for such ventilation devices and methods to optimize the effect of providing assisted ventilation with chest compressions to circulate oxygenated blood within an individual.

SUMMARY OF THE INVENTION

The present disclosure includes devices and method allowing for improved assisted ventilation of a patient. The methods and devices provide a number of benefits over conventional approaches for assisted ventilation. For example, the methods and devices described herein permit blind insertion of a device that can allow ventilation regardless of whether the device is positioned within a trachea or an esophagus. Some variations of the devices and methods allow minimally trained bystanders and laypersons to place an advanced airway for assisted ventilation. The devices described herein can be designed such that a single size can accommodate a variety of patient sizes thereby reducing the number of devices of varying sizes that must be kept in inventory. Additionally, having devices that can accommodate a wide range of individuals reduces the need of a first responder to assess the anatomic features of a patient prior to acting on the patient, in patients undergoing cardiac distress, delivery of large boluses of air during CPR can result in hyperventilating the patient, which can decrease the effectiveness of CPR. Elevated intrathoracic pressure can ultimately reduce the effectiveness of chest compressions. Variations of the current, device and methods allow for controlled ventilation, which avoids hyperventilation.

In another variation, the devices described in the present disclosure allow for improved assisted ventilating an individual. For example, a variation of the method includes inserting a ventilation device into the individual by advancing a working end of the ventilation device within a body passage of the individual, where the working end includes a far opening fluidly coupled to a first lumen and a medial opening fluidly coupled to a second lumen; drawing suction through the opening and attempting to hold a vacuum

through the first lumen and the far opening for a pre-determined period of time; automatically ventilating the individual through the second lumen upon detecting the vacuum during the pre-determined period of time and maintaining suction to maintain the vacuum; and automatically ventilating the individual through the first lumen upon failure to detect the vacuum during the pre-determined period of time; where automatically ventilating the individual occurs at a pre-determined timing; measuring a condition of a thoracic cavity to determine a change in the thoracic cavity; and altering a timing of automatically ventilating of the individual upon detecting the change in the condition of the thoracic cavity.

The present disclosure also includes a system artificially ventilating an individual, the system comprising: a ventilation device configured for insertion within a respiratory opening of the individual and having a working end for positioning within a body passageway of the individual, the ventilation device having a pressure sensor configured to detect pressure changes within the body passage; and the ventilation device having a control system, configured to deliver a bolus of air into an airway the individual at a pre-determined rate until detection of the pressure change within the body passageway, whereafter the control system is configured to alter the pre-determined rate by delaying delivery of the bolus of air until the sensor detects the pressure change in the air within the body passage, where the pressure change within the body passage results from a chest compression.

Measuring the condition of the thoracic cavity can include measuring the condition of the thoracic cavity using the ventilation device or measuring a change in a compression of a chest of the patient. For example, measuring the change of the compression of the chest of the patient comprises observing a force applied to the ventilation device by the body passageway. Alternatively, measuring the change of the compression of the chest of the patient comprises observing a deflection of the chest of the patient using one or more sensors on the chest.

In an additional variation, measuring the condition of the thoracic cavity comprises measuring a state of air flow within the thoracic cavity. Such measuring can be performed using a sensor on the ventilation device and where measuring the state of air flow within the thoracic cavity comprises detecting airflow, pressure, and/or volume using the sensor. Moreover, the sensor can monitor a direction of air flow.

The timing of the artificial ventilation can be altered by using the sensor to determine when a pressure in the body passageway increases and delivering air for automatically ventilating the individual when the pressure in the body passageway increases, or at least before the decrease, the pressure of the ventilations acts like and internal chest, compression, then the recoil of the chest draws the air into the lungs.

The methods can further include providing a feedback based on measuring the condition of the thoracic cavity. Such feedback can include information regarding the compression, where the information is selected from a phase, rate, efficiency, depth, and timing. The feedback can also be based on measuring the condition of the thoracic cavity comprises measuring a quality of the chest compression by determining a change in a volume of air in the thoracic cavity. In some variation, the feedback comprises information to increase or decrease a compression applied to a chest of the patient.

Variations of the method include altering the timing of the ventilation to initiate automatic ventilating of the individual

when a pressure increases, decreases, or reaches a maximum pressure in the body passageway. The method can further comprise continuing measuring the condition of the thoracic cavity to determine the change in the thoracic cavity after altering the timing of automatically ventilating the individual and reverting to automatically ventilating the individual at the predetermined timing upon failure to detect the change in the thoracic cavity.

In an additional variation, the method can further include adjusting the ventilating device to suspend automatically ventilating the individual and manually ventilating the individual while maintaining suction to maintain the vacuum if the vacuum is detected.

The methods described herein can include a mask that is slidably positioned along the ventilation device and where the mask can be pressed against the individual with a manual actuator or trigger to isolate the respiratory opening of the individual from an external atmosphere. Typically, the mask will not be sealed against the patient during the automatic assisted ventilation. Therefore, during CPR the system is open. Sealing the mask against the patient and initiating a manual trigger can close the system and administering a bolus of air to manually ventilate the patient.

The methods described herein can further include electrically stimulating a heart of the individual using the ventilation device.

In another variation, the method of artificially ventilating an individual can comprise inserting a ventilation device within a respiratory opening of the individual and positioning a working end of tire ventilation device within a body passageway of the individual, the ventilation device having a pressure sensor configured to detect pressure changes within the body passage: delivering a bolus of air into an airway the individual at a pre-determined rate: altering the pre-determined rate by delaying delivery of the bolus of air when the sensor detects a pressure change in the air within the body passage, where the pressure change within the body passage results from a chest compression.

The method can further comprise delivering the bolus of air into the airway of the individual occurs after a pre-determined delay. In some variations, the sensor is configured to intermittently detect pressure changes within the body passageway.

In another variation, the method further comprises, after altering the pre-determined rate, the ventilation device resumes delivering the bolus of air at the pre-determined rate if the pressure sensor fails to detect a pressure range within a first period of time.

In another variation, the method for ventilating an individual includes inserting a ventilation device within a respiratory opening of the individual and advancing a working end of the ventilation device within a body passageway of the individual, where the working end includes a first opening fluidly coupled to a first lumen and a second opening fluidly coupled to a second lumen, where the second opening is located along the ventilation device proximal to the first opening; drawing suction through the first opening to induce collapse of the body passageway and maintaining the suction for a period of time; monitoring a fluid parameter to determine whether the body passageway collapses; automatically ventilating the individual through the second lumen upon detecting collapse of the body passageway and maintaining suction to maintain the collapse of the body passageway; and automatically ventilating the individual through the first lumen upon failure to detect collapse of the body passageway; wherein delivery of a bolus of air during automatically ventilating the individual occurs at a first

timing; measuring a condition of a thoracic cavity to determine a change in the thoracic cavity; and altering the timing of the delivery of the bolus of air during automatically ventilating the individual upon detecting the change in the condition thoracic cavity.

In another variation, the present disclosure includes a method for artificially ventilating an individual by coupling a ventilation device to a respiratory opening of a respiratory passage of the individual; positioning a pressure sensor in fluid communication with the respiratory passage, the pressure sensor configured to detect pressure changes within the respiratory passage; delivering a bolus of air into the respiratory passage of the individual at a pre-determined rate; and altering the pre-determined rate by delaying delivery of the bolus of air until the sensor detects a pressure change in the air within, the respiratory passage, where the pressure change within, the respiratory passage results from a chest compression. Such a method can include any device, including conventional ventilation devices.

The present disclosure also includes a system for artificially ventilating an individual using a source of oxygen, the system comprising; a ventilation device having a pressure sensor configured to detect pressure changes within the body passage, the pressure sensor being positioned on a portion of the device configured to be inserted into a body passageway of the individual; a controller configured to deliver a bolus of air into an airway the individual at a pre-determined rate, where the controller is configured to monitor the pressure sensor and upon detecting a pressure change, the controller alters the pre-determined rate by delaying delivery of the bolus of air.

The present disclosure also includes devices for ventilating an individual. In one example such a device comprises a tubular member having at least a first and second lumen, where the first lumen is fluidly coupled to a first opening located distally relative to a medial opening, where the medial opening is fluidly coupled to the second lumen, where the first opening and medial opening are each fluidly isolated within the tubular member; the tubular member being configured to measure a condition of a body lumen to determine a change in a thoracic cavity of the individual; a control system having a suction source and a gas supply lumen, the control system having a valve configured to fluidly couple the gas supply lumen to either the first lumen or to the second lumen; the control system also capable of drawing suction from the suction source through the first opening and first lumen, where the control system is configured to monitor the first lumen for a vacuum to indicate collapse of the body passageway and formation of a seal at the first opening; where the control system is further configured to selectively form a ventilation path from the supply lumen to the first lumen or second lumen by selecting the first lumen as the ventilation path if collapse of the body passageway is not detected; and selecting the second lumen as the ventilation path if collapse of the body passageway is detected; where the control system is configured to automatically ventilate the individual through the ventilation path at a first rate; and where the control system is further configured to alter the first rate upon detecting the condition of the body lumen.

The system and methods described herein can be compatible with devices that monitor the concentration or partial pressure of carbon dioxide (CO₂) in the respiratory gases (capnography). Primarily such devices are monitoring tool for use during anesthesia and intensive care that monitor expiratory CO₂ are of interest when rebreathing systems are being used. The ability to integrate the ventilation systems

described herein with such capnography systems allows for improved patient care. Furthermore, the systems and methods described herein can be compatible with equipment found in emergency vehicles such as oxygen supplies and/or power supplies. In some variations, the system of the present disclosure can also provide audio or even video (through use of a display screen) instructions to ensure proper operation in those situations where the system may be used by first responders that are not trained emergency personnel.

BRIEF DESCRIPTION OF THE DRAWINGS

The invention is best understood from the following detailed description when read in conjunction with the accompanying drawings, it is emphasized that, according to common practice, the various features of the drawings are not to-scale. On the contrary, the dimensions of the various features are arbitrarily expanded or reduced for clarity. Also for purposes of clarity, certain features of the invention may not be depicted in some of the drawings. Included in the drawings are the following figures:

FIG. 1 provides a partial view of a patient's oral cavity, tongue, pharynx as well as esophagus and trachea.

FIG. 2 illustrates one example of a conventional device as used to intubate a patient.

FIG. 3 illustrates various components of an example of an improved, ventilation system.

FIGS. 4A to 4C illustrate a partial sectional view of a working end of an improved ventilation device.

FIGS. 5A to 5E show a representation of the process of ventilating a patient using an improved ventilation device.

FIGS. 6A to 6C show additional variations of a working end of a ventilation device.

FIG. 7 illustrates a schematic of an electrically powered system,

FIG. 8A shows an example of a component schematic for a pneumatically driven system as described herein.

FIG. 8B provides a component listing for the schematic of FIG. 8A.

FIG. 8C shows a listing of various modes for the system.

FIGS. 8D to 8M illustrates various flow paths for the various modes of operation.

FIG. 9A illustrates another variation of a device useful for providing assisted ventilation with improved outcomes by monitoring a condition of the thoracic cavity.

FIGS. 9B to 9C show a partial isometric view and partial cross sectional views of the mask and trigger used to close the system and initiate manual ventilation.

FIG. 9D illustrates a condition where a trigger in the system fluidly closes by-closing the exhaust port.

FIGS. 10A and 10B illustrate examples of the working end of the device when inserted into a body passageway of an individual and monitoring a condition of the thoracic cavity.

FIGS. 11A and 11B illustrate a variation of a system for artificially ventilating an individual using a source of oxygen, such as those described herein,

FIG. 11C shows an external device being used to control the ventilator described herein.

FIG. 12 provides a schematic of a control system relying on the gas supply to provide a source for both ventilation and suction.

FIGS. 13-22 illustrate an example of the circuitry for sensing the phase, rate, depth and effectiveness of a chest

compression with a resistor placed, on the tube of an airway placed in the patient's mouth, trachea or esophagus

DETAILED DESCRIPTION OF THE INVENTION

Before the devices, systems and methods of the present invention are described, it is to be understood that this invention is not limited to particular therapeutic applications and implant sites described, as such may vary, it is also to be understood that the terminology used herein is for the purpose of describing particular embodiments only, and is not intended to be limiting, since the scope of the present invention will be limited only by the appended claims.

Unless defined otherwise, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. The terms "proximal", "distal", "near" and "far" when used indicate positions or locations relative to the user where proximal refers to a position or location closer to the user and distal refers to a position or location farther away from the user.

FIG. 3 illustrates various components of an example of an improved system according to the present disclosure. As shown, the ventilation device **100** includes a working end **102** that is inserted into a patient. The working end can include a distal tubing **104** that contains a first lumen (not shown), which extends through a distal opening **106** of the ventilation device **100** and is in fluid communication with a control unit (also called a ventilator) **150** and/or supply source **160** via one or more proximal tubes **118**. The control unit **150** can also include an apparatus designed to provide suction as well as a collection canister. In operation, the control unit **150** directs suction or applies a vacuum through a first fluid path **122**, which in turn causes a suction or negative pressure at the distal opening **106**. The source **160** can comprise oxygen, air, or any other gas that is desired, for ventilation of delivery into the lungs. The source **160** can be nested within physical construct of the controller **150**. However, the source **160** can be optional so that the controller ventilates the patient only using ambient air.

The control unit **150** maintains the device **100** in this state for a set period of time and monitors the parameters of the pressure or flow parameters within the first lumen to determine whether to ventilate through the first or second. The example illustrated in FIG. 3 also includes a hub **108** with one or more features that aid in proper functioning of the device. Such features are described in detail below. Furthermore, the distal opening **106** can include any number of ports at the distal end of the device so long as the ports are in a fluid path with the first lumen. Likewise, the medial opening **112** can comprise any number of openings as long as those openings are in fluid communication with the second lumen. In addition, variations of the device can also be inserted through a nasal opening rather than a mouth.

The ventilation device **100** further includes a proximal tubing **110** that houses a second lumen (not shown) that exits the device **100** at a medial opening **112**. As discussed below, distal opening and first lumen are fluidly isolated from the medial opening and second lumen through the working end of the device **102** to the control unit **150**. This fluid isolation allows the control unit **150** to determine which lumen to use to ventilate the patient. The control unit directs flow through a second fluid path **124** that is fluidly coupled to the second lumen and medial opening **112** when the device is positioned in the esophagus **16** rather than the trachea **18**.

The ventilation system **100** illustrated in FIG. **3** also shows an optional mask **114** with optional venting ports **116**. Variations of the system can include alternate configurations without a mask or with other such devices such as a mouth guard or any other commonly used mounting apparatus. As discussed below, the mask **114** or other mounting apparatus can be used to assist the caregiver in properly orienting the device **100** as it is inserted into the patient. Variations of the device can include a balloon, sponge or any other structure that secures the proximal region of the device to the patient to ensure that gas is directed to the lungs during inhalation. The mask (or other structure as described herein) can include a securing band, tape strip, or temporary adhesive to secure the mask in place on the patient. The mask or similar feature can be used to determine how far to advance the working end **102** into the patient. Alternatively or in combination, the device **100** can include graduated markings **134** to assist the caregiver in properly advancing the device into the patient. The mask can be slidable to adjust the length from the mask to the distal or proximal opening.

FIG. **3** also shows a representative figure of a control system **150** with a number of controls **152** that allow for various device operative sequences, manual controls, or device overrides. For example the system **150** can include manual ventilation controls so that the caregiver can manually adjust inspiration and expiration of the patient. The controls **152** can include a reset or rapid ventilation mode for performing cardio pulmonary resuscitation. The controls **150** include a continuous airflow or continuous vacuum mode that can assist in clearing debris or bodily fluids from the body passages. The controls also allow caregivers to connect the device **100** directly to an endotracheal tube if the caregiver decides to intubate. In an additional variation, the system can allow for active ventilation consisting of blowing for a period and then sucking for a period through the active lumen in order to increase ventilation efficiency. In some variations, the system is configured so that the ventilation openings, as well as other openings on the tube do not rotate relative to the mask so that caregiver can align the openings with the trachea.

The device shown in FIG. **3** can also include one or more electrodes positioned on the working end. For example, the hub **108** can serve as an electrode and apply electricity to the heart in order to defibrillate a patient out of an irregular rhythm or increase the heart rate or contractility. Additionally, one or more electrodes can be inserted on or embedded in a tube designed to be placed in the patient's mouth, esophagus or trachea. Such placement will be beneficial because it would allow the operator a more direct route of electrical stimulation of the heart compared that the current use of pads placed on the patient's chest. A tube placed in the esophagus would more easily be able to detect a pulse because of the major arteries running parallel to the esophagus. This would allow rescuers to determine a pulse without having to touch the patient, it would also allow an untrained bystander to administer CPR who was not trained on checking for pulse. In addition, the pressure sensors, as described below, can be placed on the tube that had been advanced into the patient's mouth that may be pressing against major arteries would be able to detect if there was a change in pressure.

In additional variations, the control system **150** can be integrated into one or more parts of the device body **102** rather than being a separate stand-alone box type configuration. In addition, the ventilation system **100** can be optionally configured to work with a defibrillator. Alternate variations of the system **100** can be configured to provide an

audible, visual, or tactile sensation to indicate when a caregiver should administer chest compressions.

FIG. **3** also shows the depicted variation of the device **100** as having an optional balloon **132** or other expandable member located on a working end. When used, the balloon can be positioned anywhere along the device adjacent to the distal opening **106**. Alternatively, or in combination, a balloon can be located adjacent to the medial opening.

The various tubing forming the device **100** should be sufficiently flexible so that the device can be navigated through the upper respiratory system. Alternatively, or in addition, portions of the tubing can be constructed to withstand being collapsed by the patient's mouth or teeth. In additional variations the system **100** can be designed such that the distance between the distal opening **106** is adjustable relative to the medial opening **112** and/or the mask **114** (or even moveable relative to the graduations **134**). A similar variation includes a medial opening **112** that can be adjustably positioned relative to the distal opening **106**, mask **114** and/or graduations **134**.

FIGS. **4A** to **4C** illustrate a partial sectional, view of an airway unit or working end **102** of a ventilation device **100** as described herein.

FIG. **4A** illustrates a first lumen **128** that is fluidly coupled to a distal opening **106** and a second lumen **130** that is fluidly coupled to the medial opening **112** where the first and second lumens **128** and **130** are fluidly isolated from each other as described above, FIG. **4A** also illustrates that the spacing **126** between the distal opening **106** and the medial opening **112** can be selected based on the intended patient. For example, since the medial opening **112** is intended to be positioned, in or around the pharynx when the distal opening **106** is positioned in the esophagus or trachea, the spacing **126** can be selected for an individual of average build. In most cases, the working end **102** of the ventilation device **100** will comprise a single use disposable component. Accordingly, the ventilation device **100** can include a number of disposable components having different spacing **126** between the medial **112** and distal **106** openings. For instance, the varying spacing can accommodate infants, toddlers, young children, as well as various body sizes.

FIG. **4B** illustrates a partial cross sectional view of the working end **102** of the ventilation device of FIG. **4A**. Once the device is properly positioned within the patient, the control unit **150** applies a suction or vacuum through a first fluid path **122**, then through the first lumen **128** and ultimately causing a vacuum at the distal opening **106** as denoted by arrows **30**. In additional variations, the operator or caregiver may choose to clear food or other debris from the patient by delivering air through the first lumen **128** or by attempting to use the suction at the distal opening to remove particles or other bodily fluids. The system **150** shall continue to pull a vacuum through the first lumen **130** for a period of time. If the device **100** is properly positioned within the trachea (as discussed below), the system **150** will begin to ventilate through the first lumen **128**. In other words, the system **100** will begin to cyclically deliver oxygen or other gas from the source **160** and remove carbon dioxide from the patient to properly ventilate the patient's lungs. In this situation, flow is not required through the second lumen **130** and medial opening **112**. Although FIG. **4B** shows the first lumen **128** to be located within the second lumen **130** any number of variations can be used. For example, the lumens can be concentric or parallel. Additional variations even allow for the lumens to be in fluid communication where one or more valves determine whether ventilation occurs through the distal opening or

through the medial opening. The device can include any number of safety checks to confirm placement of the device doesn't change. For example, once the device confirms placement in the trachea, it can re-perform a check to ensure that it is placed in the trachea over a pre-determined interval. Alternatively, it can perform this check on a sliding scale (e.g., 1st check at 30 second, 2nd check at 2 minutes, 3rd check at 10 minutes, etc). In an additional variation, the system is designed to provide a safety check to ensure that the suction filter is not clogged causing a misread of position. In such a case the device gives ventilation out the distal port once a vacuum is detected. This ventilation bolus can be small or large. By monitoring vacuum and determining if it is lost during the distal air bolus, the device knows that the seal was at the esophagus and resumes suctioning distally and ventilation through the proximal ports. If the vacuum is not lost during the distal air bolus the device can assume that the filter is clogged and an error signal will indicate for the operator to replace the working end of the device or to check for obstructions.

The system 150 can comprise the mechanism that ventilates and produces suction or a vacuum. Generally, the system 150 is reusable (as opposed to the working end that is generally disposable). The system 150 can be portable, affixed to an ambulance or other emergency vehicle or build within a cart or room. Variations include battery powered devices, pneumatic powered devices, or devices that require a power source (such as an AC outlet).

FIG. 4C illustrates the condition where the distal opening 106 is positioned within the esophagus. In this situation the control unit 150 directs ventilation through the second lumen 130. As shown by arrows 32, because the medial lumen 112 is fluidly coupled to the second lumen 130 ventilation 32 takes place at the medial opening 112.

FIGS. 5A to 5E show a representation of the process of ventilating a patient using a ventilation device 100 as described herein.

FIG. 5A illustrates the ventilation device 100 as a caregiver advances the device 100 into the oral cavity 10 over the tongue 12 and into the pharynx 14. At any time during the procedure, the caregiver can manually operate the device to suction fluids, food particles, or other items from the body. As described herein, the caregiver can "blindly" advance the working end 102 into the patient. As a result, the working end 102 will either end up in the esophagus 16 or trachea 18 of the patient.

FIG. 5B illustrates the condition where the caregiver advances the working end 102 into a trachea 18 of an individual. Once the caregiver places the device 100, the caregiver can initiate the control unit 150 to start the process to determine placement of the device 100. Alternatively, one or more sensors on the device can automatically trigger actuation of the control unit. In either case, the control unit draws a vacuum through the distal opening 106 for a predetermined period of time. The vacuum reduces pressure and draws air within the distal opening 106. The control unit 150 then assess a state of the device by monitoring the vacuum, airflow, or any other fluid parameter that would indicate whether the walls of the body passage, in this case the trachea 18, collapsed causing the formation of a vacuum seal. In those cases like FIG. 5B where the device is situated within the trachea, the suction 30 will have little effect on the walls of the trachea 18. As noted above, the walls of the trachea 18 are reinforced with rings of cartilage 20 that provide structural rigidity of the airway. Because the controller 150 will not detect the formation of a vacuum seal at the distal opening 106 (or within the first lumen) the system

registers the distal opening 106 as being properly positioned in the trachea 18 (rather than the esophagus 16) and, after a pre-determined period of time (e.g., 10-15 seconds), the controller ISO ceases to draw a vacuum and begins to ventilate the patient's lungs by alternating between delivery of the gas from the gas supply 160 and removing carbon dioxide. As a result, the first lumen is used, as a ventilation lumen. It will be important for the controller 150 to differentiate changes in vacuum or flow that result from suctioning of fluids or debris. In some variations of the device, the controller 150 is configured to identify formation of a seal when the vacuum builds or flow drops to a sufficient degree such that the device has formed a vacuum seal rather than suctioned fluids or a substance.

The control unit 150 can determine whether or not a seal, is formed by measuring strain on a suction motor (or similar apparatus such as a venturi device that produces a vacuum) that causes the negative pressure within the main lumen for suction. If the control unit 150 observes zero or minimal strain on the suction motor after a pre-determined time, then the control unit 150 will use the first lumen as the ventilation lumen.

FIG. 5D illustrates a state where the caregiver advances a working end 102 of the ventilation device 100 into an esophagus 16 rather than the trachea 18. Similarly to the state depicted by FIG. 5B above, once the caregiver positions the device 100, the caregiver can initiate the control unit 150 to start, the process to determine placement of the device 100. As noted above, additional variations of the device and system can include one or more sensors that can automatically trigger actuation of the control unit.

FIG. 5D depicts the state where the control unit 150 poll vacuum through the distal opening 106 for a predetermined period of time. The vacuum reduces pressure and draws air within the distal opening 106. The control unit 150 then assess a state of the device by monitoring the vacuum, airflow, or any other fluid parameter that would indicate whether the walls of the body passage, in this case the esophagus 16 collapsed. As shown, the walls partially or totally collapse resulting in formation of a vacuum seal at the distal opening 16. As noted above, muscles form the walls of the esophagus 16. There is no reinforcing structure in the esophagus as opposed to the cartilage rings in the trachea 18. The control unit can be configured to monitor the formation of a vacuum seal and if the seal remains for a predetermined period of time, the control unit 150 directs ventilation 40 in and out of the medial opening 112 as depicted in FIG. 5E. As shown and discussed above, the spacing between the distal opening 106 and medial opening 112 can be selected such that the medial opening remains in or near the pharynx 14. However, variations of the device permit the medial opening to enter the esophagus 16 so long as the opening 112 can continue to ventilate the patient.

Because the control unit 150 will not detect the formation of a vacuum seal at the distal opening 106 (or within the first lumen) the system registers the distal opening 106 as being properly positioned in the trachea 18 (rather than the esophagus 16) and, after a pre-determined period of time, the control unit 150 ceases to draw a vacuum and begins to ventilate the patient's lungs by alternating between delivery of the gas from the gas supply 160 and removing carbon dioxide. In this situation the device uses the second lumen as a ventilation lumen. One additional benefit of positioning the working end 102 of the device 100 within the esophagus 16 is that the vacuum seal produces an anchoring effect that maintains the device in position. This feature eliminates the need to secure the mask or other feature about the patient's

head, neck or face. In addition, if a caregiver inadvertently pulls the device **100** while a seal is formed, the vacuum seal is simply broken and the device releases from the esophagus **16**. This provides a safety improvement over conventional ventilation devices that rely on an expandable balloon, which if pulled, can cause trauma to the patient's airways, vocal cords, or other structures.

In certain variations, the device **100** shall cease ventilating after a period of time and produce suction through the distal opening. Such a step is considered a safety feature in the event that the working end is moved, repositioned, etc.

FIGS. **6A** to **6C** show variations of the working end **102** of a ventilation device as described herein. FIG. **6A** illustrates a hub having an opening **106** that is surrounded by a contoured surface. The contoured surface can assist reducing the chance that the distal opening **106** becomes clogged due to food particles or other fluids. This feature also assists in reducing the occurrences that the control unit misreads an opening **106** that is obstructed (with food particles or other bodily fluids) for an opening that formed a seal with the walls of the esophagus, FIGS. **6B** and **6C** illustrate additional variations of a working end **102** of a ventilation device. In these variations, the working end **102** can be fabricated with or without a hub. FIG. **6B** illustrates a straight tube having a plurality of openings **106**. FIG. **6C** illustrates a beveled end having an opening **106**.

As noted above, the device described herein can be pneumatically driven using compressed gas and valves or electrically controlled. FIG. **7** illustrates a schematic of an electrically powered device using a suction motor, air compressor and circuitry to switch between a first fluid path **122** (ultimately fluidly coupled to a distal opening) and a second fluid path **124** (ultimately fluidly coupled to a medial opening).

FIG. **8A** shows an example of a component schematic for a system as described herein that is pneumatically driven. FIG. **8B** provides a list of the components found in FIG. **8A**. The valves operate in multiple states based on the conditions discussed above. The following description illustrates an example of the different states of the components found in the component schematic of FIG. **8A**.

Medial Supply Valve **P1** (4/2):

State **1** (nominal, spring return): Controls the 15 s timing of vacuum supply through Distal Supply Valve **P2**;

State **2** (actuated): Provides supply for medial, ventilation;

Pilot Actuation: 10" Hg vacuum

Distal Supply Valve **P2** (4/2)

State **1** (nominal, spring return): Provides supply for Vacuum Generator;

State **2** (actuated): Provides Supply for Distal Ventilation;

Pilot Actuation: 40 psi from flow-controlled output of Medial Supply Valve, State **1**.

Pulse Valve **P3** (3/2 Normally Open);

State **1** (nominal, spring return): Fills Accumulator volume at flow-controlled rate until set pressure is achieved at inline Relief Valve;

State **2**; (actuated): Dumps accumulator volume to Ventilation Selector Valve through quick exhaust;

Pilot Actuation: 5 psi from output of inline Relief Valve Ventilation Selector Valve **P4** (3/2 Fully Ported);

State **1** (nominal, spring return): Routes output of Pulse Valve to Medial Ventilation Output;

State **2**; (actuated): Routes output of Pulse Valve to Distal Ventilation Output;

Pilot Actuation: 40 psi from output of Distal Supply Valve, State **2**

Operation Valve **M1** (Manual Toggle, 3 position. All Detent);

State **1** (toggle down, "ON"): Provides supply for Medial Supply Valve and Distal Supply Valve;

State **2** (toggle centered, "OFF/RESET"); Blocks supply, vents system;

State **3** (toggle up, "VACUUM"): Bypasses all valves, provides supply to Vacuum Generator.

Mode Valve **M2** (Manual Toggle, 3 position, Detent/ Detent/Momentary);

State **1** (toggle down, detent, "VENTILATE"): Provides supply for Pulse Valve and Ventilation Selector Valve;

State **2** (toggle centered, detent, "BYPASS"): Blocks supply to Pulse Valve and Ventilation Selector Valve.

State **3** (toggle up, momentary spring return, "ON-DEMAND"); Blocks supply to Pulse Valve, provides continuous flow-controlled supply to Ventilation Selector Valve

The system illustrated by the component schematic of FIG. **8A** can have a variety of modes of operation. In one example, as shown by FIG. **8C**, the system can include 8 separate modes of operations controlled by the position of various valves and the operation state of a medial supply valve.

Mode **0**, where the system is set to an Off position.

M1 set to OFF;

Main supply blocked; system vented;

FIG. **8D** shows Mode **1**, where there is a continuous vacuum applied through the system.

M1 set to VACUUM

Ventilation system bypassed; vacuum at Vacuum. Output; Vacuum indicator on

FIG. **8E** shows Mode **2**, where the system engages in placement detection;

M1 set to ON;

Vacuum at Vacuum. Output until **P2** pilot activated (15 s); Vacuum indicator

on;

In Mode **3**, the system engages in ventilation through the distal opening.

M1 set to ON; **M2** set to VENTILATE;

No vacuum detected; **P2** pilot activated; **P4** pilot activated.

FIG. **8F** shows Mode **3A**, where an accumulator fills at controlled rate (0.67 s) until inline Relief Valve activates (30 psi);

Distal Ventilation Indicator on.

FIG. **8G** shows Mode **3B**: **P3** pilot activates, closing **P3** and exhausting Accumulator volume through Quick Exhaust to **P4**; Distal Ventilation Indicator on.

Mode **4**—Medial Ventilation

M1 set to ON; **M2** set to VENTILATE

Vacuum detected; **P1** pilot activated; vacuum at Vacuum Output.

FIG. **8H** shows Mode **4A** where accumulator fills at controlled rate (0.67 s) until inline Relief Valve activates (30 psi);

Vacuum indicator on;

Medial Ventilation. Indicator on.

FIG. **8I** shows Mode **4B**: **P3** pilot activates, closing **P3** and exhausting Accumulator volume through Quick Exhaust to **P4**;

Vacuum Indicator on; Medial Ventilation Indicator on.

FIG. **8J** shows Mode **5**—Ventilation Bypass (Distal);

M1 set to ON; **M2** set to BYPASS;

No vacuum detected; **P2** pilot activated; **P4** pilot activated; supply to **P3** & **P4** blocked; Distal Ventilation Indicator on.

15

FIG. 8K shows Mode 6—On-Demand Ventilation (Distal);

M1 set to ON; M2 set to ON-DEMAND;

No vacuum detected; P2 pilot activated; P4 pilot activated; supply to P3 blocked; continuous flow-regulated flow to P4; Distal Ventilation Indicator on

FIG. 8L shows Mode 7—Ventilation Bypass (Medial);

M1 set to ON; M2 set to BYPASS;

Vacuum detected; P1 pilot activated; vacuum at Vacuum Output;

supply to P3 blocked;

Vacuum Indicator on;

Medial Ventilation Indicator on

FIG. 8M shows Mode 8—On-Demand Ventilation (Medial);

M1 set to ON; M2 set to ON-DEMAND;

Vacuum detected; P1 pilot activated; vacuum at Vacuum Output;

supply to P3 blocked;

continuous flow-regulated flow to P4; Vacuum Indicator on; Medial Ventilation Indicator on.

FIG. 9A illustrates another variation of a device useful for providing assisted ventilation with improved outcomes. The features and aspect of the illustrated example can be combined with any of the variations of the devices described herein. Moreover, the features of the devices described herein that improve the effectiveness of assisted ventilation can be used with conventional assisted ventilation devices.

As illustrated, assisted ventilation device 100 includes a working end 102 that is inserted into a patient. The working end can include a distal tubing 104 that contains a first lumen (not shown), which extends through a distal opening 106 of the ventilation device 100 and is in fluid communication with a control unit (also called a ventilator) 150 and/or supply source 160 via one or more proximal tubes 118. The control unit 150 can also include an apparatus designed to provide suction as well as a collection canister (not shown). As noted above, the device 100 can optionally include an improved control unit 150 that directs suction or applies a vacuum through a first, fluid path 122, which in turn causes a suction or negative pressure at the distal opening 106. The source 160 can comprise oxygen, air, or any other gas that is desired for ventilation of delivery into the lungs. The source 160 can be nested within physical construct of the controller 150. However, the source 160 can be optional so that the controller ventilates the patient only using ambient air. FIG. 9A also illustrates the device 100 as including features that allow the assisted ventilation device 100 to deliver ventilation in a manner that improves the efficiency of the assisted ventilation procedure.

For example, the improved device 100 can include one or more structures used to determine a change in the thoracic cavity. Such changes can include physical movement of the tissues within the thoracic cavity, the force applied to the working end 102 of the device 100, and/or the deflection of any part of the device 100. Alternatively, or in combination, a change in the thoracic cavity can comprise a change in the fluid environment of the thoracic cavity, including anybody passageways that are in fluid communication with the thoracic cavity, e.g., the airway, the esophagus, etc.

FIG. 9A illustrates the device 100 as being able to measure fluid parameters in the thoracic cavity via a sensor 180 located along a portion of the working end 102 of the device. Although the sensor 180 is illustrated on the proximal tubing 110, the sensor 180 can be positioned along any portion of the device 100 that enables monitoring of the fluid parameters of the thoracic cavity and/or body passage in

16

fluid communication with the thoracic cavity. For instance, the device 100 can include one or more sensors 180 positioned along the distal tubing 104 and/or hub 108. Moreover, variations of the device include one or more sensors positioned within the device 100.

The sensor 180 can comprise a pressure sensor, flow sensor, transducer, or similar structure. Alternatively, in additional variations, the sensor 150 can comprise a lumen or passageway having an open end positioned as described above, where the lumen or passageway extends through the device via a sensor tubing 182 that allows the actual fluid parameters to be read by the actual sensor located within the device 100, tubing 118, and/or control unit 150.

The variation illustrated in FIG. 9A also shows a sensor 150 that is not flush with the proximal tubing 110 of the device 100. As shown, the measurement surface (e.g., the actual sensor or the sensor lumen 184 can be positioned so that tissue adjacent to the device 100 does not obscure or affect the readings of the sensor. However, additional variations of the device 100 include sensors that are flush, with the device body. In addition, pressure from the device 100 (e.g., the proximal tube 118 can be used to deliver air to the sensor 180 reduce obstructions from interfering with the measurement of any fluid parameter in the body lumen.

FIG. 9A also illustrates a force detecting component, such as a strain gauge, optic fiber, transducer, or similar force/movement detecting structure that can be located anywhere along the working end 102 of the device 100. The force detecting component 190 is shown as being on the distal tubing 104, however, one or more force detecting components 190 can be positioned along any portion of the device as long as the component 190 detects a force applied to the chest via a resulting force being applied to the device through movement of the tissue displaced by assisted chest compression.

The presence of both the sensor 180 and the force detecting component 190 on a single device is for purposes of illustration only. Certain variations of the device can include any combination of force detecting component, sensor, or both.

FIG. 9A also shows the device as including a manual ventilation trigger 186. In operation, the medical caregiver can use the manual ventilation trigger 186 to manually deliver a bolus of air through the device 100. Alternatively, or in combination, the manual ventilation trigger 186 can activate the sensor 180 or force detecting component 190 to deliver a bolus of air on demand. Such a feature can be useful if the care giver has obtained a pulse and intends on delivering assisted, ventilation alone. Alternatively, the caregiver can use the manual ventilation trigger 186 to deliver a bolus of air through any part of the device in an attempt to clear bodily fluids that might otherwise obstruct the device. The manual ventilation trigger 186 can operate as the device performs the automated assisted ventilation where a bolus of air is delivered at certain period of time. Alternatively, or in combination, the manual ventilation trigger 186 can deliver a bolus of air when the ventilation device 100 (or controller 150) is placed in a manual-mode.

In certain variations of the device, when initiating the manual trigger 186, the device be programmed to maintain, ventilation through the respective opening that was selected in the automatic mode. For example, if the device is placed in the esophagus, and then switched to manual operation, the control system can maintain suction to ensure that the esophagus closes the distal opening and forms a vacuum so that manual ventilation automatically proceeds through the proximal or medial opening 112. Likewise, if the device is

positioned in the trachea, actuating the device in a manual mode will cause the bolus of air to be expelled from the distal opening of the device.

In one example, the trigger **186** comprises a hollow button, attached to the device and inline with the tubing that connects to the sensor **180**. When the button is pressed it sends an air bolus to the sensor **180** that signals the control system **150** to start assisted ventilation. The volume of air provided by the manual trigger **186** can be preset. Alternatively, air can be delivered until the caregiver releases the trigger **186** to stop the ventilation. In addition, mounting the trigger **186** mounted on the mask **114** is beneficial because it allows the caregiver to ensure the mask **114** is sealed against the patient's face with one or two hands while operating the demand ventilations.

The manual trigger **186** can also operate to with one or more one-way valves (e.g., a flap that allows exhaust of air when the trigger **186** is not pressed). This ensures that there is no excess buildup of pressure in the airway and prevents barotrauma. This also allows spontaneous breathing. When the ventilator is switched to demand ventilation mode the lungs need to be isolated from atmosphere during the inhalation period only. This can be achieved by having the demand ventilation trigger **186** mounted on a flap that is above an opening on the mask. The flap is designed to be opened with when no pressure is being applied to the button, then, once pressure is applied to the trigger the flap is sealed against the opening, closing the system and allowing air to inflate the lungs. When the button is released for exhalation the flap is conies off the mask opening allowing air to escape and lungs deflate.

FIG. 9B illustrates a variation of a portion of a device **100** showing a mask **14** having a trigger **186** that is coupled to an exhaust port **116**. In this variation, the mask **114** also includes one or more pressure release valves **117** that will crack or permit flow beyond an established pressure. Such a fail-safe presents unsafe pressurization of the airway by the device. The pressure release valves **117** can be surrounded by protrusions or features **115** that prevent objects from blocking the valves **117**. The device **100** is also shown with an adjustment control **183** that permits movement of the mask **114** along the tube **110**. FIG. 8B also illustrates a tubing **185** that couples the trigger **186** to the sensor lumen **184**. As shown, the sensor lumen **184** can be coupled with a t-fitting or other fluid coupling so that a portion of the lumen is in fluid communication with the trigger **186** as described below.

FIG. 9C illustrates a partial cross sectional view of the mask **114** and tubing **110**. As shown, when the mask is positioned against the respiratory opening of the patient (i.e., a mouth or nose), airflow from the expiratory cycle (represented by arrows **109**) flow through a portion of the mask **114** and into a chamber **113** that is in fluid communication with the exhaust lumens **117**. However, in this condition, the trigger **186** is not being pressed against the mask **114** such that the exhaust port **116** remains open allowing airflow **109** to exit the mask. Furthermore, the trigger **186** can be positioned in a shaft having a compressible air volume **111** that is in fluid communication with the tubing **185**. Accordingly, although the mask **114** is pressed against the patient, the exhaust port **116** permits the system to be open (fluidly open).

FIG. 9D illustrates a condition where the trigger is pressed or actuated (the trigger can be on a spring return or have elasticity to function as a spring return). Once actuated, the trigger **186** fluidly closes the system by closing the exhaust port **116**. The action of the trigger **186** can also be used

Initiate a manual bolus of air through the tubing **110**. For example, the trigger **186** can have one or more electrical contacts or switches in region **111** that provides a signal to the control, system to deliver a bolus of air. In an additional configuration, actuation of the trigger **186** compresses the volume of air in space **111** causing a pressure increase P_2 in tube **185**, which is coupled to the sensor lumen **184**, this increase in pressure causes the sensor lumen to perform a manual ventilation by delivering a bolus of air through the tubing **110**. Likewise, when the trigger **186** is released, the expansion in volume of region **111** creates a drop in pressure in tubing **185** as well as in the sensor lumen **184**, where the drop in pressure is registered by the sensor to stop ventilation.

In addition to the sensor **180** and/or sensor lumen **184** the device **100** can include any number of additional lumens to provide information to monitoring equipment. For example, the device can include one or more lumens that are fluidly coupleable to a capnograph device. Alternatively, or in combination, the sensor lumen **184** can also allow fluid coupling to a monitoring device. In such a case, the lumens can be coupled to one or more openings (such as **180**) located on the working end of the device.

FIG. 10A illustrates an example of the working end **102** of the device **100** when inserted into a body passageway of an individual. In this example, the device is inserted into a trachea **18**, where the device **100** detects that it is in an airway as described above. However, as shown in FIG. 10B, variations of the device **100** can also be positioned in the esophagus **16** using the process described, above, which temporally seals the esophagus **16** to deliver air to the respiratory passage **18**.

In either case, the device **100** is configured to begin assisted ventilation by delivering a bolus of air **40** at a pre-determined rate. The device **100** is configured to measure a condition of a thoracic cavity to determine a change in the thoracic cavity, either through pressure within the thoracic cavity as denoted by PT or a force F applied to the thoracic cavity via chest compressions. In the latter case, the force F applied to the chest causes movement of tissue (such as the trachea or other tissue) that can be determined by a force detecting component **190** as discussed above. The detection of a change in the thoracic cavity by measuring a fluid characteristic such as a change in pressure PT is typically measured within a body passageway (such as the trachea **18** or esophagus **16**). Such measurements can include measuring flow rate of air, volume, pressure, etc.

In one variation, the initial or pre-determine rate comprises 100 ventilations per minute (i.e., a bolus of air is delivered 100 times per minute). However, any rate of delivery is within the scope of this disclosure. Upon detecting a change in the condition of the thoracic cavity, typically due to chest compressions, the device **100** will adjust the timing and/or rate of air delivery to achieve an optimum result. For example, the system can deliver a bolus of air upon detecting the chest compression (either by the force measurement or via the fluid sensor measurement). In such a case, the bolus of air increases pressure in the thoracic cavity to serve as an internal chest compression which compresses the heart and lungs from within causing increased blood flow.

In variations of the device, the system monitors for a change in a condition of the thoracic cavity on a continuous basis, or on a delay. In either case, the system can be configured to not respond to a change in the pressure of the thoracic cavity driven by the delivery of the bolus of air. For

example, the system can ignore readings during and immediately after the delivery of the bolus of air.

The process of adjusting the delivery of a bolus of air (either by timing and/or rate) in response to a particular phase of the chest compression is intended for use during CPR. However, the assisted ventilation can be accomplished whether using a mechanical compression system or a caregiver performing manual chest compressions.

The alteration of the timing and/or rate is intended to provide a bolus of air with each or a specific number of compression and at a specific phase of the compression of the patient's chest. As noted herein, the ventilations are timed in a way that both increased the efficiency of the chest compression by increasing intrathoracic pressure during the down stroke of the chest compression, which would increase the pressure on the heart thus increasing blood flow. During the up stroke of the compression the a portion of the ventilation could still be given to allow new air enter the alveoli while allowing a portion, of the up stroke of the compression to create a negative intrathoracic pressure drawing blood back into the heart and air into the alveoli. This technique also prevents a rescuer from having to pause compressions in order give ventilations, which decreases blood flow and decreases odds of patient's survival.

When using the devices described herein, regardless of whether the device is positioned in the trachea or esophagus, the airway is always opened to the outside environment which greatly reduces, if not eliminates, the chance of barotrauma.

The data generated by the devices described herein regarding the efficiency of the compression regarding depth, rate, recoil time can be analyzed and presented via feedback to the caregiver in order to maximize the efficiency of the compressions. All of this information and be used to increase the efficiency of the compressions and therefore increase blood flow of the patient and increasing patients chance of survival. If using a mechanical compression system the cycle phase could be directly linked to the device 100.

Furthermore, the system can be configured to return to a pre-determine rate of providing the bolus of air, if at any time chest compression, stop/pause. In such a case, the system can monitor the amount of time during which a change in the thoracic cavity is not detected. If no change is detected for a pre-set time, the control unit can reset the rate of assisted ventilation to the initial rate or an alternate rate that is not dependent upon chest-compression. In addition, if the patient's pulse resumes, the system can continue to provide assisted ventilation at a pre-determined rate, volume, etc. Alternatively, the system can enter a manual mode where a caregiver can deliver assisted ventilation upon demand (e.g., using the manual trigger button). Furthermore, the system can be configured, to check for a patient's pulse and use identification of the pulse to adjust the rate of assisted ventilation or cease assisted ventilation.

The manual trigger allows the caregiver to give a controlled ventilation on demand button may be beneficial once the patient has regained a pulse eliminating the need for external chest compression. As noted above, the device 100 can still continue isolation of the lungs by collapsing the esophagus with suction and/or direct air through the proper lumen into the lungs but changes the ventilation to an air bolus given on demand given by the caregiver. The manual trigger allows the caregiver to start the flow of air to the lungs. Release of the trigger stops the flow of air to the lungs to allow the patient to exhale. Alternatively, a single actuation of the trigger can give a preset amount of air that ventilates the patient.

The system described herein can also be used with conventional rescue devices. For example, the ventilation system can be configured to work with an active chest compression device so that ventilations and chest compressions are timed to increase effectiveness of both the compression and ventilation. The coupling can be mechanical, and/or electrical. The ventilation system can also include carbon dioxide sampling so that carbon dioxide levels are outputted via a signal or gas stream to a monitor or other notification means as described herein.

FIGS. 11A and 11B illustrate a variation of a system for artificially ventilating an individual using a source of oxygen, such as those described herein. In the illustrated example, the device 100 is not shown for purposes of clarity in illustration how the control system 150 can be used as a stand-alone unit having electrical control systems having firmware can be controlled through the system interface 152, or can be Integrated or controlled with an external device (e.g., a cardiac monitor, monitor/defibrillator, or other critical care device). As shown, the control unit 150 can be mounted on the external device 162 and coupled to a source of oxygen 160. As shown in FIG. 11B, once coupled to the external device 162, the control unit 150 can be operated using the on-board controls 152 or can be controlled via the external device 162 via a wireless or wired connection. In such a case and as shown in FIG. 11G, one or more of the on-board controls 152 of the control unit 150 can be displayed on the control/display 164 of the external device 162. The variation shown in FIG. 11C illustrates controls for operating the device 100 in a CPR mode, on-demand mode, or suction mode. However, any number of items can be displayed on the control/display 164 and/or on the on-board controls 152.

For example, the device 100 can display information relating to the phase, rate, efficiency, depth, ratios of chest compression during CPR. Additionally, the device can display information for giving an operator real time feed-back on the efficiency of the assisted compressions via audible or visual feedback as well as information on whether to increase or decrease the speed of manual compressions, or whether to resume chest compressions if pulses are lost or the caregiver stops chest compression for too long.

The device 100 can also be configured with a rechargeable power supply that can be charged when coupled to an external device 162, or where the connection allows for charging the device 100 via a typical AC power source. In most cases, the control unit 150 will carry a power supply capable of powering the device for a sufficient period of operation and a sufficient stand-by period.

FIG. 12 illustrates an additional improvement to increasing the portability of the control unit 150. In this configuration, the control unit 150 relies upon the source of oxygen 160 to provide ventilation to the individual as well as to produce the vacuum described above. Accordingly, to extend the source of the oxygen, the device can employ one or more vacuum valves 200, 202 that produce a vacuum as a result of the pressurized flow of oxygen where one vacuum valve operates at a high flow to generate suction. Once a vacuum is established for a certain period of time, the system can switch to a low flow vacuum valve 202 that generates high, vacuum, with, low flow. Such a configuration extends the life of the oxygen supply.

In another variation, the devices described herein can be used to determine ventilation parameters using tubing that accommodates different sizes. For example, having a variety of working ends of different, sizes that were coordinated with a Broslow tape for pediatric applications. This way a

caregiver could simple select the size airway the Broslow tape recommended and attach, to the ventilator. The caregiver would not have to adjust the ventilation parameters because either the authentication process would signal to the ventilator the approximate size of the patient based on the airway selected. Alternatively, the airway itself would reduce the volume, pressure, suction pressure that the patient received. An example of this method would be a narrowing of the ventilation, tubing that restricted flow so the volume ventilated over a period of time was less. Another example would be an exhaust valve the dumped excess ventilation volume into the atmosphere, reducing both the volume and pressure for ventilating the patient.

Method for being able to determine the phase, rate, efficiency, depth, ratios of chest compression during CPR by detecting the bending of a tube placed in the patient's mouth, esophagus via various methods. Including but not limited to, strain gauges on tube, fiber optics, air movement sensors. A method for timing ventilations at a certain phase of the compression to maximize the efficiency of CPR while allowing adequate gas exchange. Using the technology mentioned in the method above attached the ventilator. A method for continuing ventilations after compressions are stopped or paused. A method for giving operator real time feed back on the efficiency of rescuers compressions via audible or visual feedback.

Some of the features of the systems described above include: a method for placing electrodes on the tube and pacing the heart via tube placed in the mouth, esophagus or trachea; a method for defibrillating the heart through electrodes placed on a tube in the mouth, trachea or esophagus of a patient; and a method for determining if the patient has a pulse through a tube in the patients mouth, trachea or esophagus.

FIGS. 19-28 illustrate an example of the circuitry for sensing the phase, rate, depth and effectiveness of a chest compression with a resistor placed on the tube of an airway placed in the patient's mouth, trachea or esophagus. The information can be relayed to the rescuer or used to signal a valve to time a ventilation. This is only one example of how to implement the invention described above by no way are we limiting other methods mentioned above.

The preceding merely illustrates the principles of the invention. It will be appreciated that those skilled in the art will be able to devise various arrangements which, although not explicitly described or shown herein, embody the principles of the invention and are included within its spirit and scope. Furthermore, all examples and conditional language recited herein are principally intended to aid the reader in understanding the principles of the invention and the concepts contributed by the inventors to furthering the art, and are to be construed as being without limitation to such specifically recited examples and conditions. Moreover, all statements herein reciting principles, aspects, and embodiments of the invention as well as specific examples thereof are intended to encompass both structural and functional equivalents thereof. Additionally, it is intended that such equivalents include both currently known equivalents and equivalents developed in the future, i.e., any elements developed that perform the same function, regardless of structure. The scope of the present invention, therefore, is not intended to be limited to the exemplary embodiments shown and described herein. Rather, the scope and spirit of present invention is embodied by the appended claims.

It must be noted that as used herein and in the appended claims, the singular forms "a", "an", and "the" include plural referents unless the context clearly dictates otherwise. Thus,

for example, reference to "a string" may include a plurality of such strings aid reference to "the tubular member" includes reference to one or more tubular members and equivalents thereof known to those skilled in the art, and so forth.

Where a range of values is provided, it is understood that each intervening value, to the tenth of the unit of the lower limit unless the context clearly dictates otherwise, between the upper and lower limits of that range is also specifically disclosed. Each smaller range between any stated value or intervening value in a stated range and any other stated or intervening value in that stated range is encompassed within the invention. The upper and lower limits of these smaller ranges may independently be included or excluded in the range, and each range where either, neither or both limits are included in the smaller ranges is also encompassed within the invention, subject to any specifically excluded limit in the stated range. Where the stated range includes one or both of the limits, ranges excluding either or both of those included limits are also included in the invention.

All publications mentioned herein are incorporated herein by reference to disclose and describe the methods and/or materials in connection with which the publications are cited. The publications discussed herein are provided solely for their disclosure prior to the filing date of the present application. Nothing herein is to be construed as an admission that the present invention is not entitled to antedate such publication by virtue of prior invention. Further, the dates of publication provided may be different from the actual publication dates which may need to be independently confirmed.

I claim:

1. A method of artificially ventilating an individual during chest compressions, the method comprising the steps of:
 - inserting a ventilation device within a respiratory opening of the individual and positioning a working end of the ventilation device within a body passageway of the individual, the ventilation device having a pressure sensor configured to detect pressure changes within the body passageway;
 - delivering a bolus of air into an airway of the individual at a pre-determined rate;
 - altering the pre-determined rate by delaying the delivery of the bolus of air when the sensor detects a pressure change in the air within the body passageway, where the pressure change within the body passageway resulting from the chest compressions;
 - where the working end includes a first opening fluidly coupled to a first lumen and a second opening fluidly coupled to a second lumen, where the second opening is located along the ventilation device proximal to the first opening; and
 - where inserting the ventilation device within the respiratory opening further comprises:
 - drawing suction through the first opening to induce collapse of the body passageway and maintaining the suction for a period of time;
 - monitoring a fluid parameter to determine whether the body passageway collapses;
 - automatically ventilating the individual by:
 - automatically ventilating the individual through the second lumen upon detecting collapse of the body passageway and maintaining suction during the ventilating to maintain the collapse of the body passageway; and

23

automatically ventilating the individual through the first lumen upon failure to detect collapse of the body passageway;

wherein the bolus of air is delivered during the automatically ventilating of the individual, where the automatically ventilating of the individual occurs at a first timing;

measuring a condition of a thoracic cavity to determine a change in the thoracic cavity; and

altering the timing of the delivery of the bolus of air during the automatically ventilating of the individual upon detecting the change in the condition thoracic cavity.

2. The method of claim 1, where delivering the bolus of air into the airway of the individual occurs after a pre-determined delay.

3. The method of claim 1, where the sensor is configured to intermittently detect pressure changes within the body passageway.

4. The method of claim 1, further comprising, after altering the pre-determined rate, the ventilation device resumes delivering the bolus of air at the pre-determined rate if the pressure sensor fails to detect a pressure range within a first period of time.

5. The method of claim 1, where measuring the condition of the thoracic cavity comprises measuring the condition of the thoracic cavity using the ventilation device.

6. The method of claim 1, where measuring the condition of the thoracic cavity comprises measuring a change in a compression of a chest of the individual.

7. The method of claim 6, where measuring the change of the compression of the chest of the individual comprises observing a force applied to the ventilation device by the body passageway.

8. The method of claim 6, where measuring the change of the compression of the chest of the individual comprises observing a deflection of the chest of the individual using one or more sensors on the chest.

9. The method of claim 1, where measuring the condition of the thoracic cavity comprises measuring a state of air flow within the thoracic cavity.

10. The method of claim 9, where measuring the state of air flow comprises measuring a direction of air flow.

11. The method of claim 1, where the altering the timing comprises using the pressure sensor to determine when a pressure in the body passageway increases and delivering air for automatically ventilating the individual when the pressure in the body passageway increases, decreases, or reaches a maximum pressure.

12. The method of claim 1, further comprising providing a feedback based on measuring the condition of the thoracic cavity.

13. The method of claim 12, where the feedback comprises information regarding the chest compression, where the information is selected from the group consisting of a phase, rate, efficiency, depth, and timing.

24

14. The method of claim 12, where the feedback comprises information to increase or decrease a compression applied to a chest of the individual.

15. The method of claim 1, where the altering the timing of the ventilation comprises initiating the automatically ventilating of the individual when a pressure increases in the body passageway.

16. The method of claim 15, further comprising continuing measuring the condition of the thoracic cavity to determine the change in the thoracic cavity after the altering the timing of the automatically ventilating of the individual and reverting to automatically ventilating the individual at the first timing upon failure to detect the change in the thoracic cavity.

17. The method of claim 1, further comprising adjusting the ventilating device to suspend the automatically ventilating of the individual and manually ventilating the individual while maintaining suction to maintain a vacuum.

18. The method of claim 1, further comprising a mask slidably positioned along the ventilation device.

19. The method of claim 18, further comprising sealing the mask against the individual to isolate the respiratory opening of the individual from an external atmosphere.

20. The method of claim 1, further comprising electrically stimulating, a heart of the individual using the ventilation device.

21. The method of claim 1, further comprising monitoring the individual for a pulse using a portion of the ventilation device located in the body lumen.

22. A method for ventilating an individual, the method comprising the steps of:

inserting a ventilation device into the individual by advancing a working end of the ventilation device within a body passage of the individual, where the working end includes a far opening fluidly coupled to a first lumen and a medial opening fluidly coupled to a second lumen;

drawing suction through the far opening and attempting to hold a vacuum through the first lumen and the far opening for a pre-determined period of time;

automatically ventilating the individual by:

automatically ventilating the individual through the second lumen upon detecting the vacuum during the pre-determined period of time and maintaining suction through the far opening during ventilating to maintain the vacuum; and

automatically ventilating the individual through the first lumen upon failure to detect the vacuum during the pre-determined period of time;

where the automatically ventilating of the individual occurs at a pre-determined timing;

measuring a condition of a thoracic cavity to determine a change in the thoracic cavity; and

altering a timing of the automatically ventilating of the individual upon detecting the change in the condition of the thoracic cavity.

* * * * *

专利名称(译)	用于改善辅助通气的装置和方法		
公开(公告)号	US9757530	公开(公告)日	2017-09-12
申请号	US14/666244	申请日	2015-03-23
[标]申请(专利权)人(译)	COLABS		
申请(专利权)人(译)	COLABS INC.		
当前申请(专利权)人(译)	COLABS INC.		
[标]发明人	NOLAN CLAY		
发明人	NOLAN, CLAY		
IPC分类号	A61M16/04 A61M16/00 A61M16/06 A61B5/00 A61B5/087 A61N1/39 A61N1/05 A61M16/20 A61N1/362		
CPC分类号	A61M16/0003 A61B5/087 A61B5/6847 A61M16/0051 A61M16/0069 A61M16/04 A61M16/0411 A61M16/0486 A61M16/0463 A61M16/06 A61M16/201 A61M16/0475 A61M2016/003 A61M2016/0027 A61M2202/0208 A61M2205/054 A61M2205/332 A61M2205/3344 A61M2205/502 A61M2205/583 A61M2230/432 A61N1/0517 A61N1/0519 A61N1/362 A61N1/39 A61M16/0063 A61M16/0434 A61M16/0484 A61M16/0488 A61M16/202 A61M16/209 A61M16/022 A61N1/39044		
优先权	13/659699 2014-07-15 US 61/969043 2014-03-21 US 61/569169 2011-12-09 US		
其他公开文献	US20150265790A1		
外部链接	Espacenet USPTO		

摘要(译)

用于允许改善患者的辅助通气的装置和方法。与传统的辅助通气方法相比，该方法和装置提供了许多益处。例如，本文描述的方法和装置允许盲装插入可允许通气的装置，而不管装置是否位于气管或食道内。另外，该方法和装置允许基于胸腔的状况定时输送通气，以增加复苏过程期间血流量和效率。

