



US 20180242852A1

(19) **United States**

(12) **Patent Application Publication**
Govari et al.

(10) **Pub. No.: US 2018/0242852 A1**
(43) **Pub. Date: Aug. 30, 2018**

(54) **MAPPING FORCE AND TEMPERATURE FOR A CATHETER**

A61B 5/103 (2006.01)
A61B 90/00 (2016.01)
A61B 34/20 (2016.01)

(71) Applicant: **BIOSENSE WEBSTER (ISRAEL) LTD.**, Yokneam (IL)

(52) **U.S. Cl.**
CPC *A61B 5/01* (2013.01); *A61B 2018/00821* (2013.01); *A61B 5/743* (2013.01); *A61B 2018/00815* (2013.01); *A61B 2018/00791* (2013.01); *A61B 2018/00577* (2013.01); *A61B 2018/00357* (2013.01); *A61B 2018/00029* (2013.01); *A61B 2017/00084* (2013.01); *A61B 18/1492* (2013.01); *A61B 5/6852* (2013.01); *A61B 5/103* (2013.01); *A61B 2090/065* (2016.02); *A61B 2090/064* (2016.02); *A61B 2034/2051* (2016.02); *A61B 2218/002* (2013.01); *A61B 5/015* (2013.01)

(72) Inventors: **Assaf Govari**, Haifa (IL); **Christopher Thomas Beeckler**, Brea, CA (US)

(73) Assignee: **Biosense Webster (Israel) Ltd.**, Yokneam (IL)

(21) Appl. No.: **15/966,662**

(22) Filed: **Apr. 30, 2018**

Related U.S. Application Data


(62) Division of application No. 14/058,325, filed on Oct. 21, 2013, now Pat. No. 9,980,652.


Publication Classification

(51) **Int. Cl.**
A61B 5/01 (2006.01)
A61B 5/00 (2006.01)
A61B 18/00 (2006.01)
A61B 17/00 (2006.01)
A61B 18/14 (2006.01)

(57) **ABSTRACT**

A method for displaying information, including receiving measurements, with respect to an invasive probe inside a body of a subject, of probe parameters consisting of a force exerted by the probe on tissue of the subject and temperatures measured by sensors of the probe. The method further includes, responsively to the measurements, displaying in a single map on a display screen a graphical representation of a distribution of the temperatures in a vicinity of the probe and superimposing thereon a vector representation of the force.

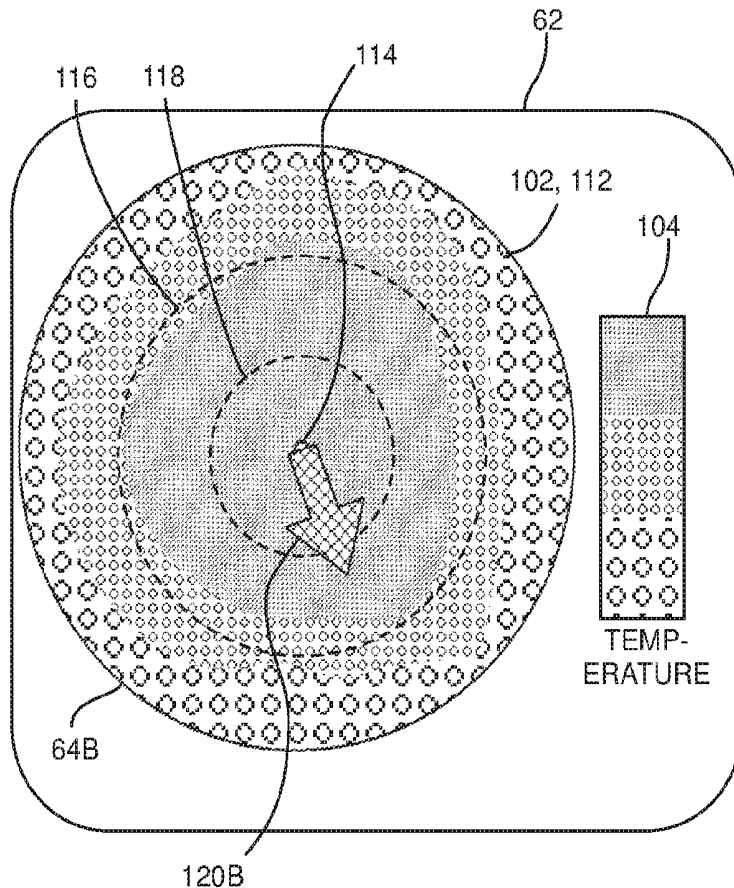

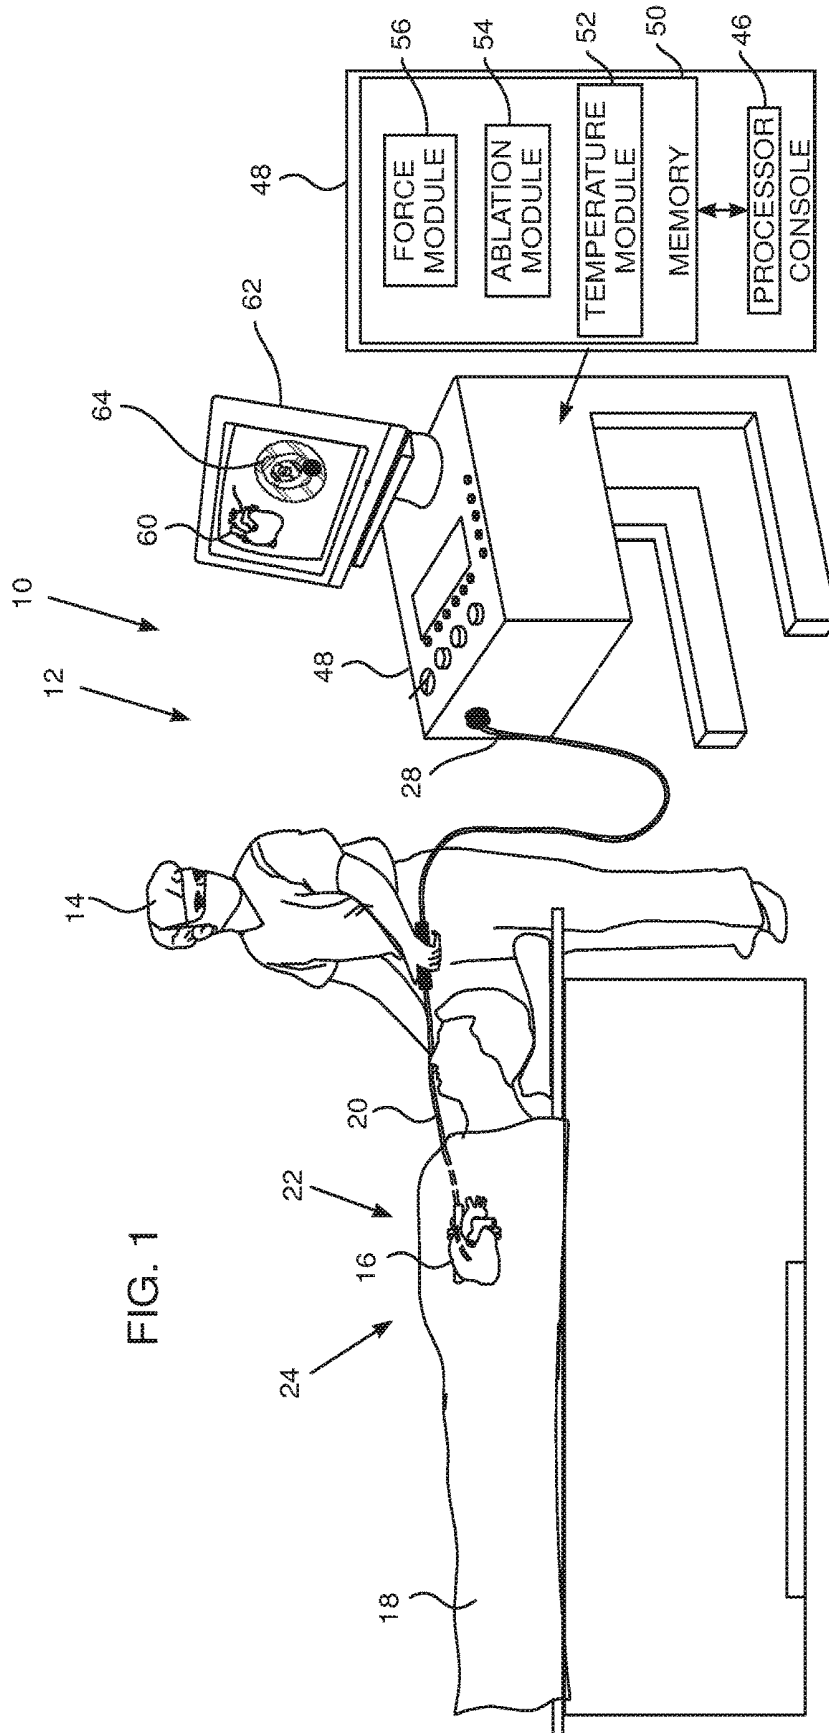

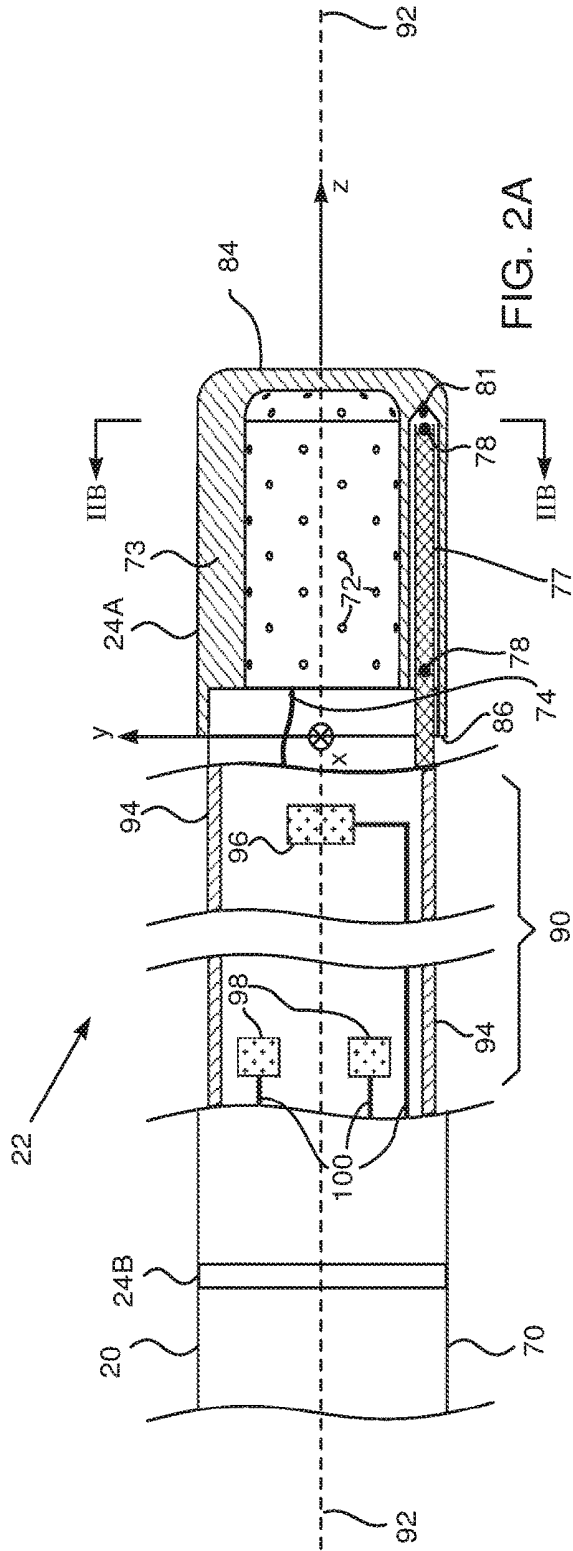


FIG. 2A

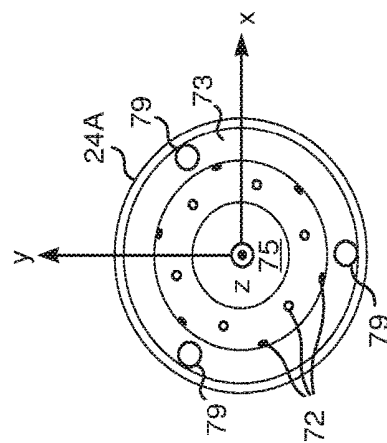


FIG. 2B

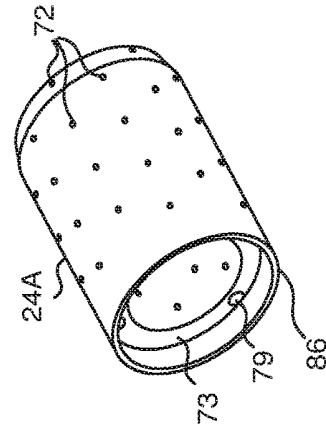


FIG. 2C

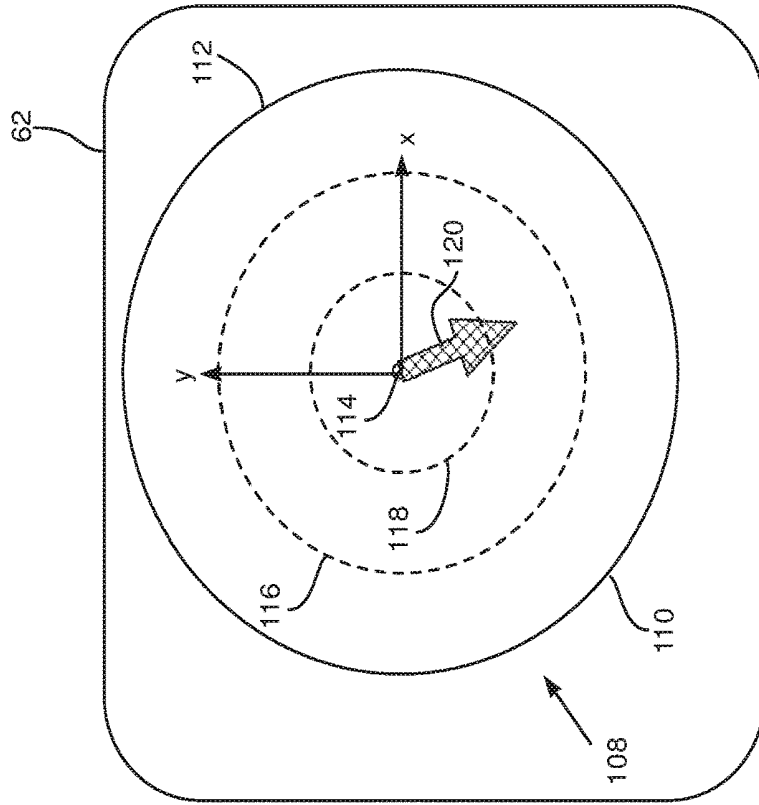


FIG. 3A

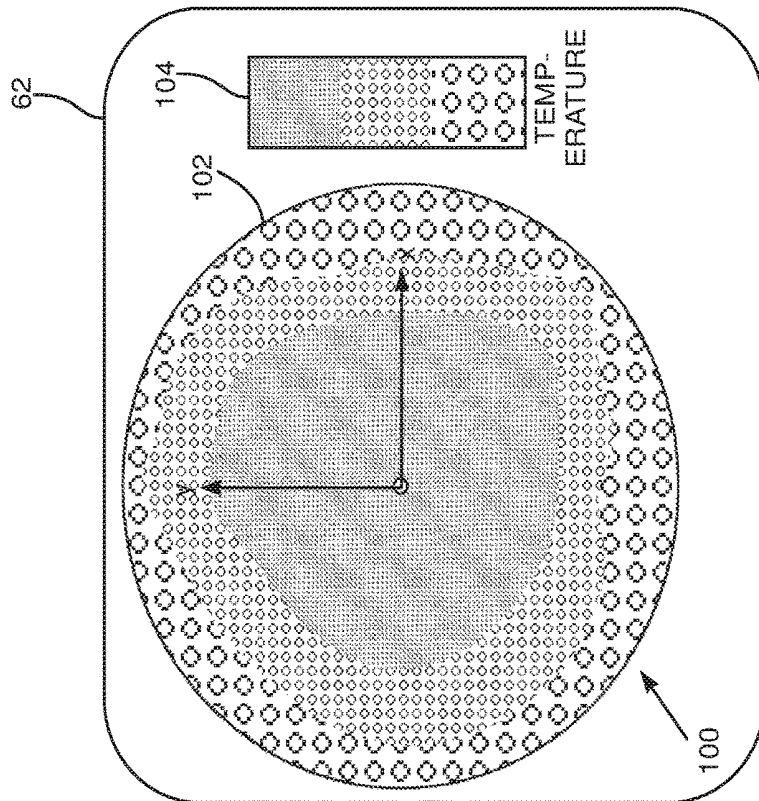


FIG. 3B

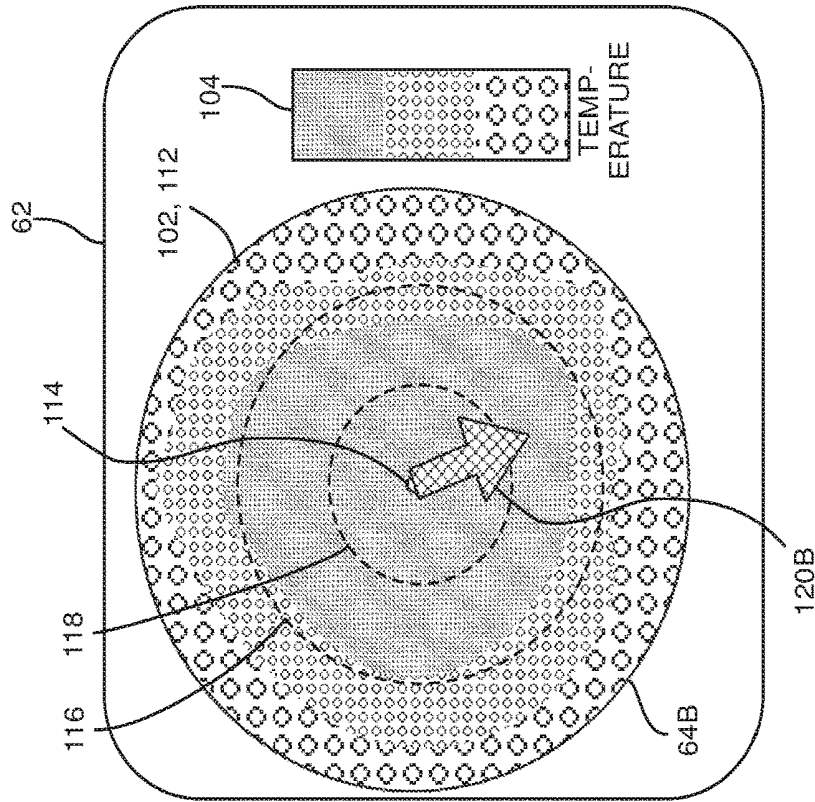


FIG. 3D

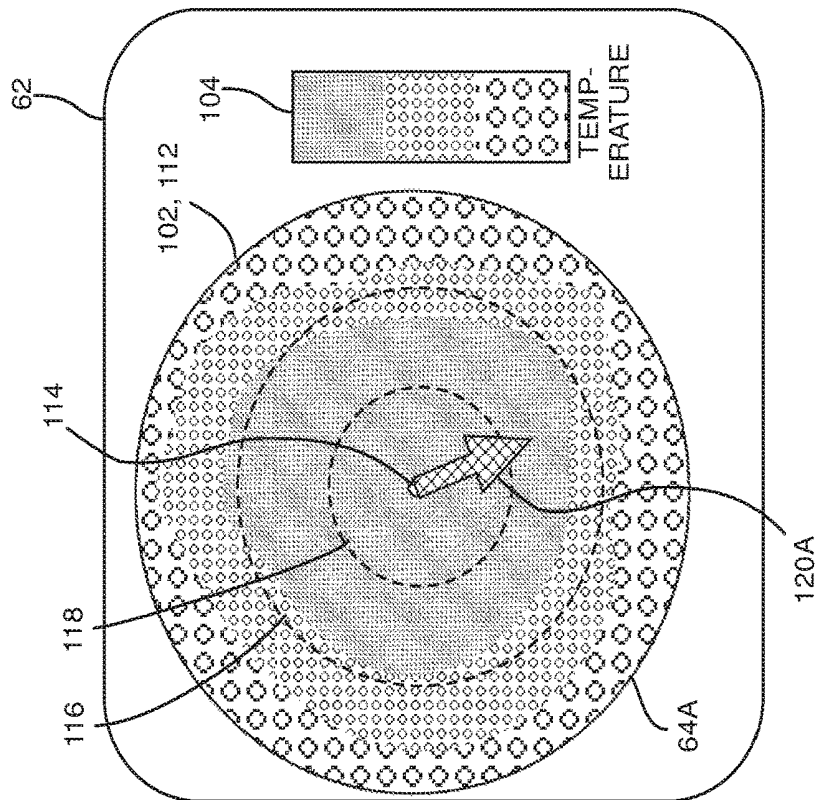


FIG. 3C

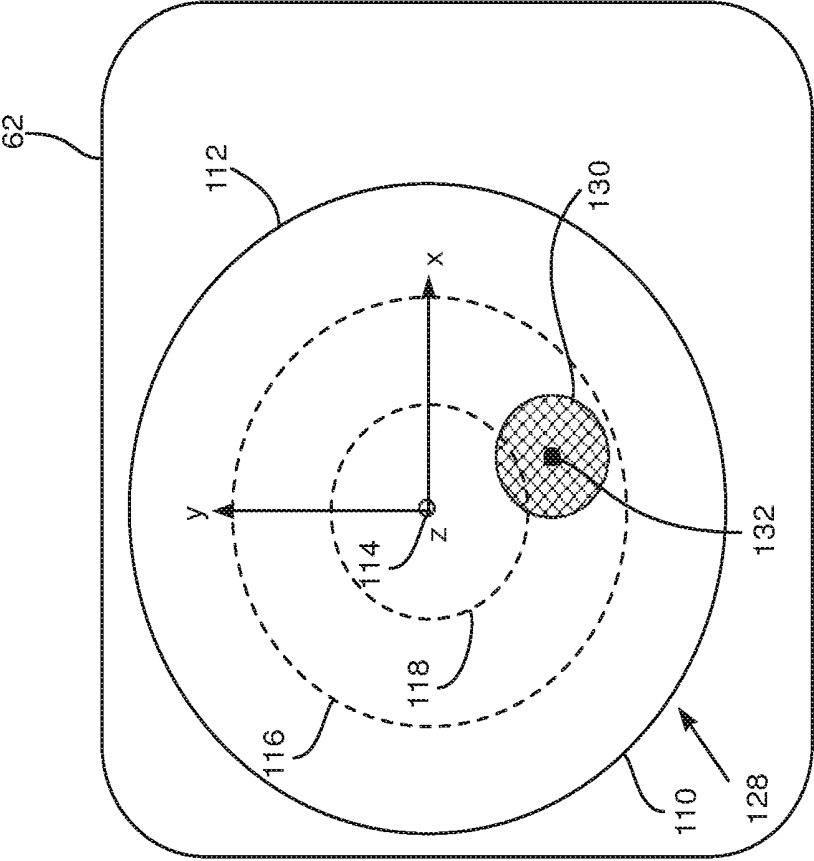
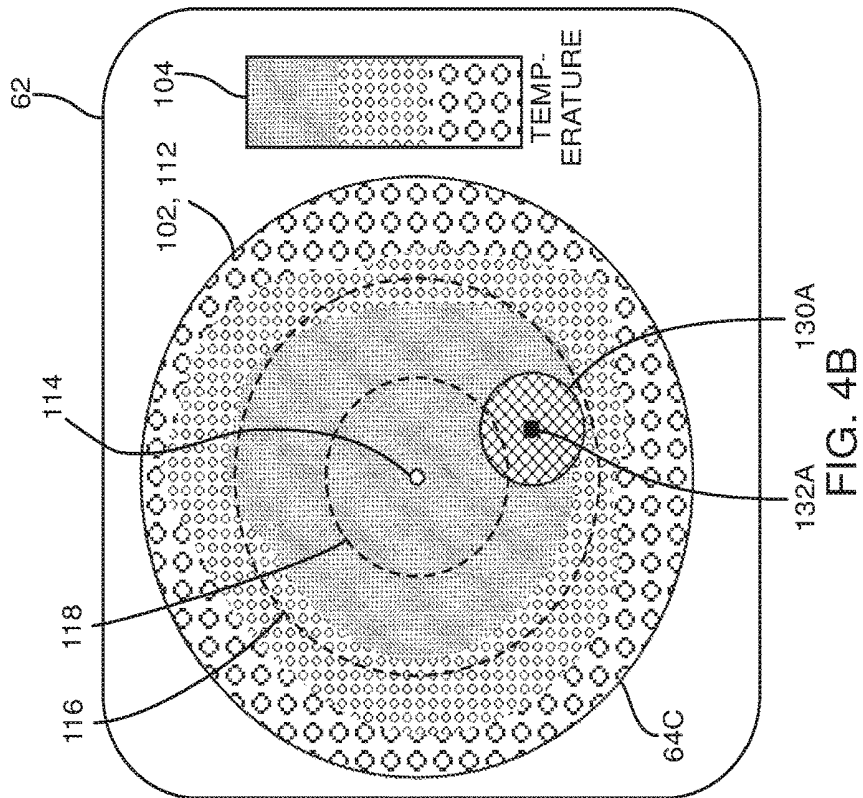
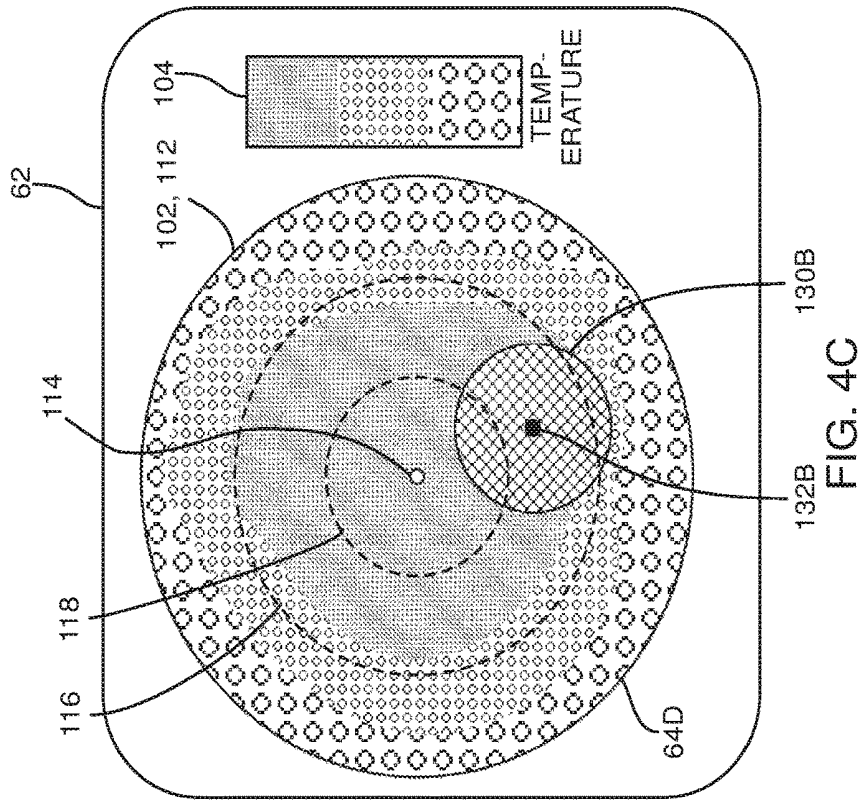


FIG. 4A



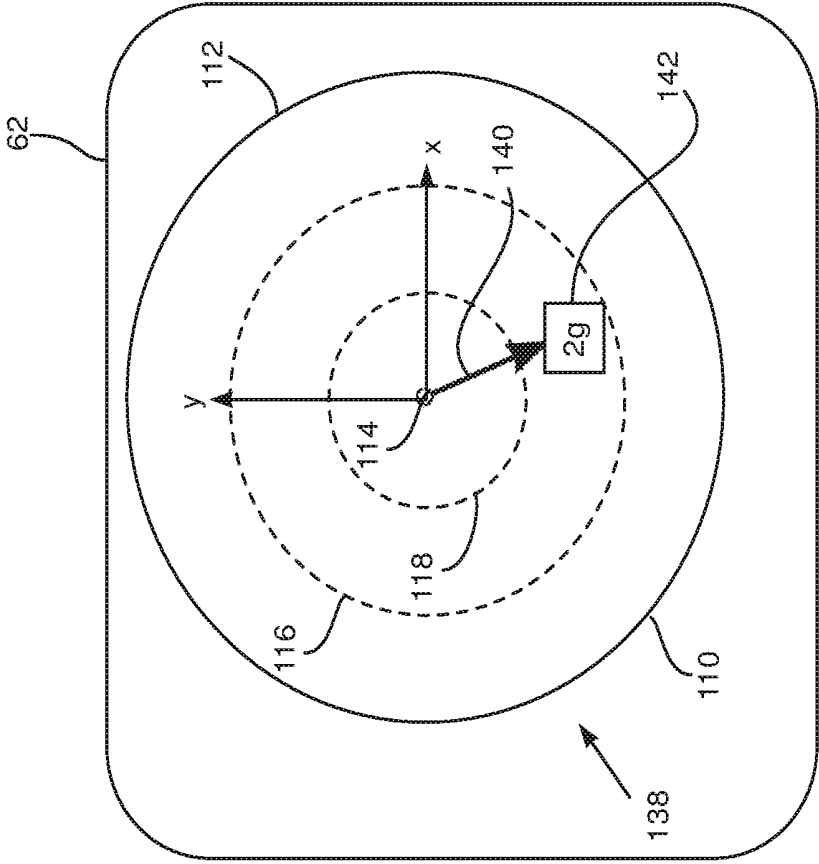


FIG. 5A

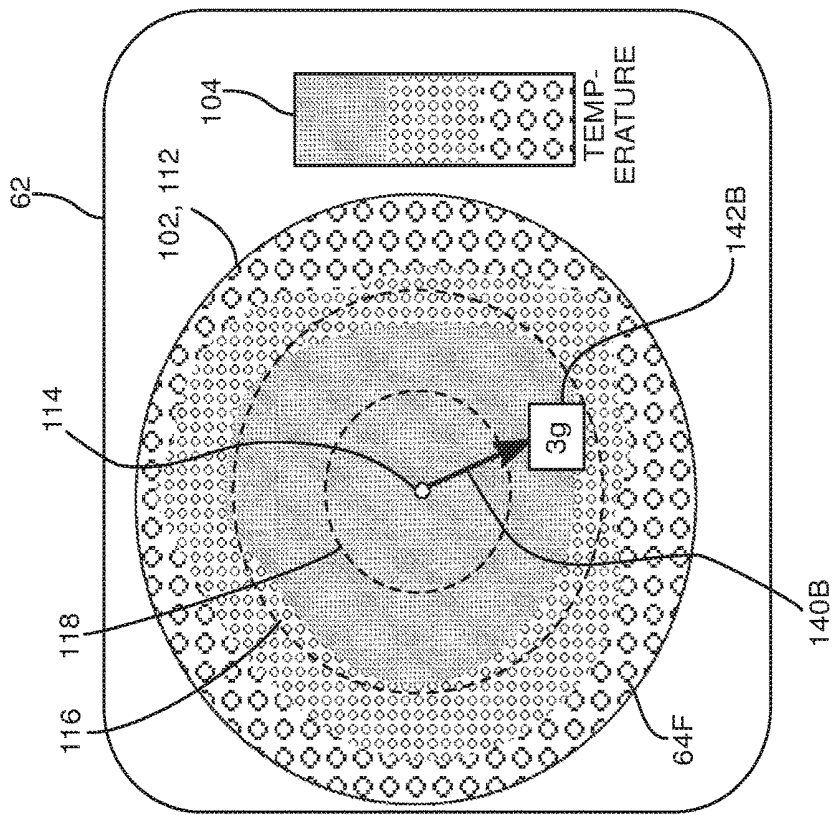


FIG. 5C

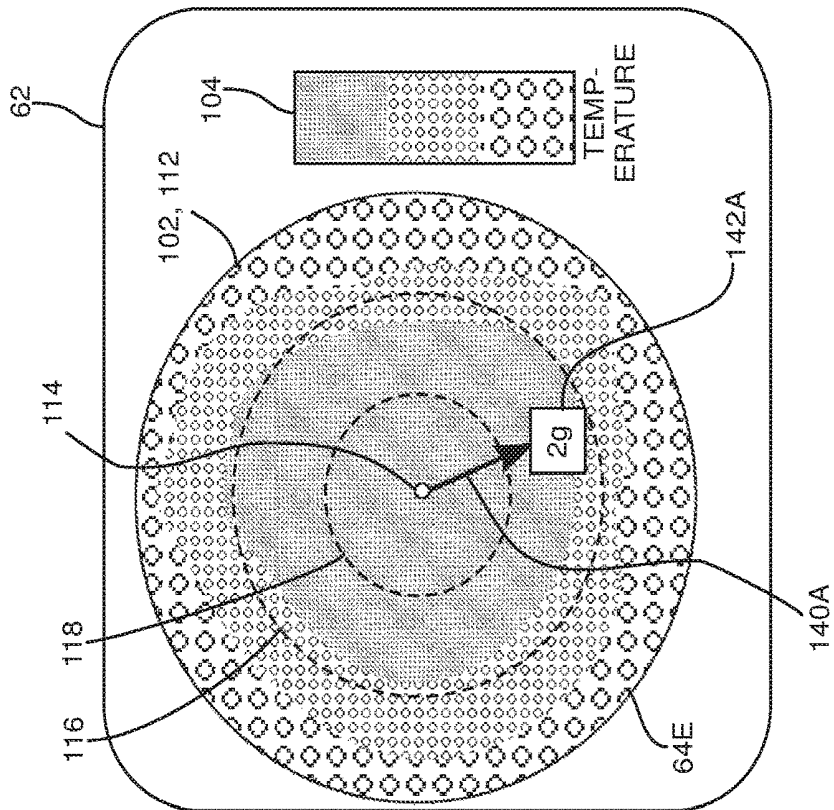


FIG. 5B

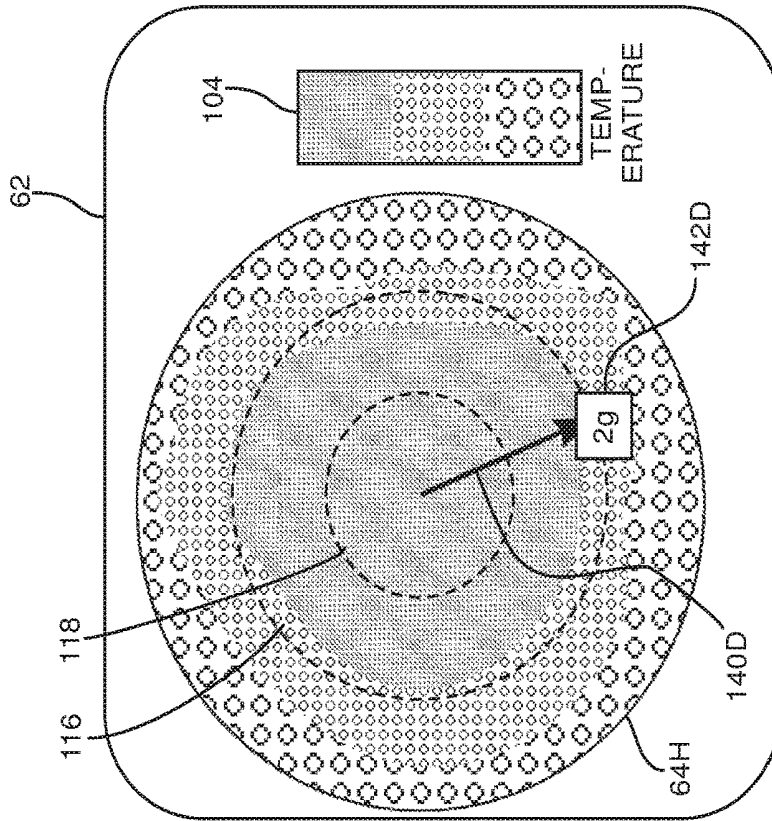


FIG. 6B

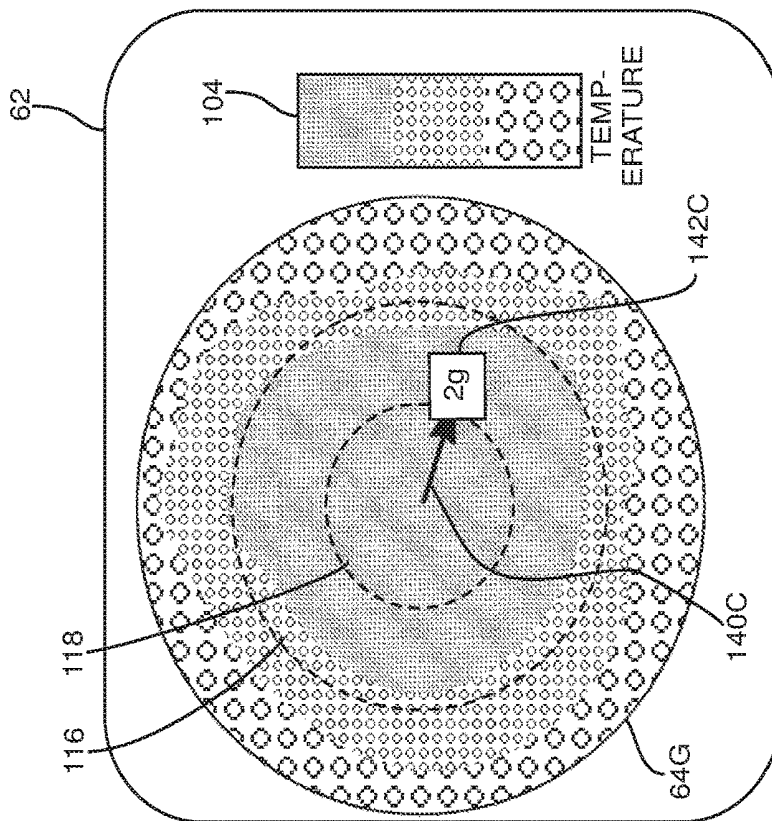


FIG. 6A

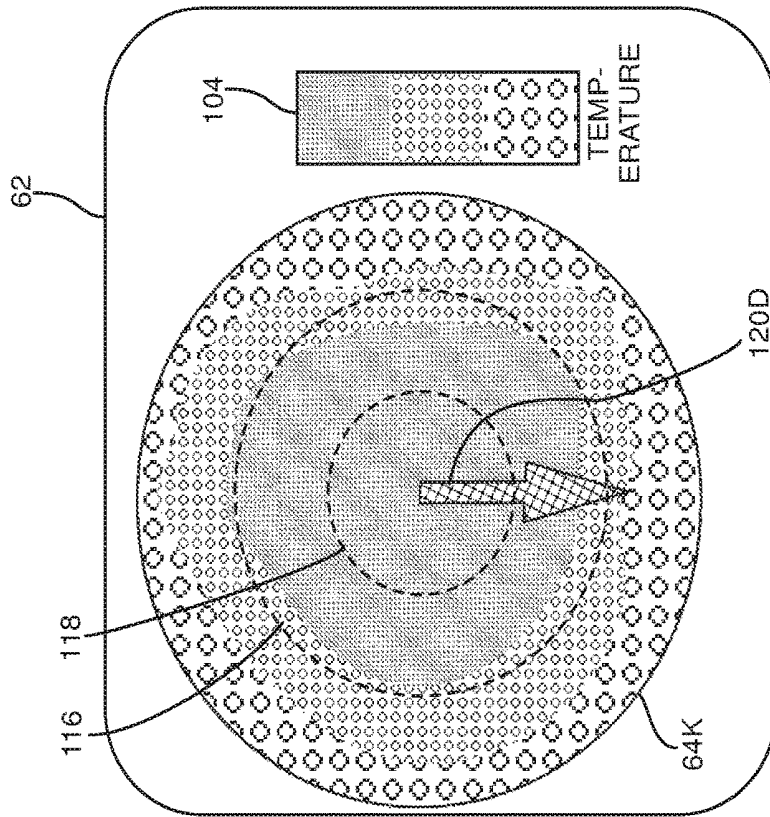


FIG. 7B

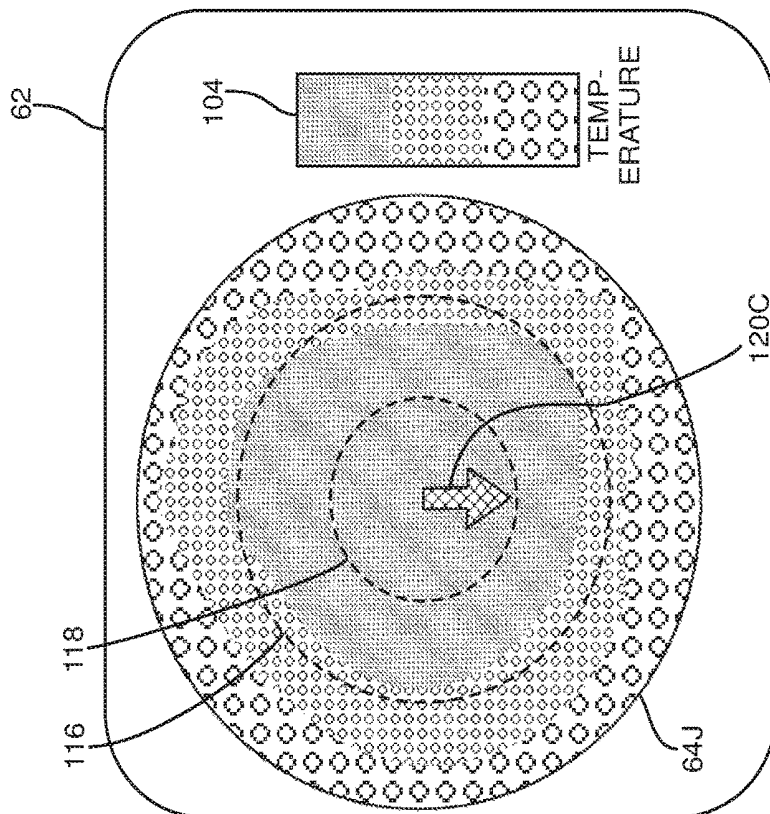


FIG. 7A

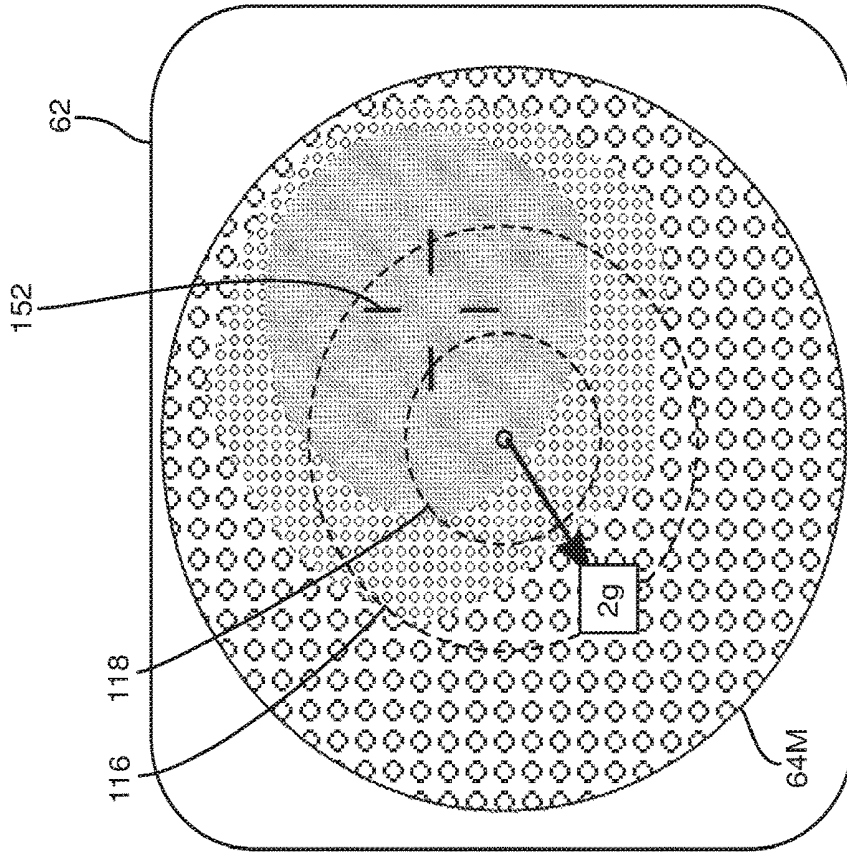


FIG. 8A

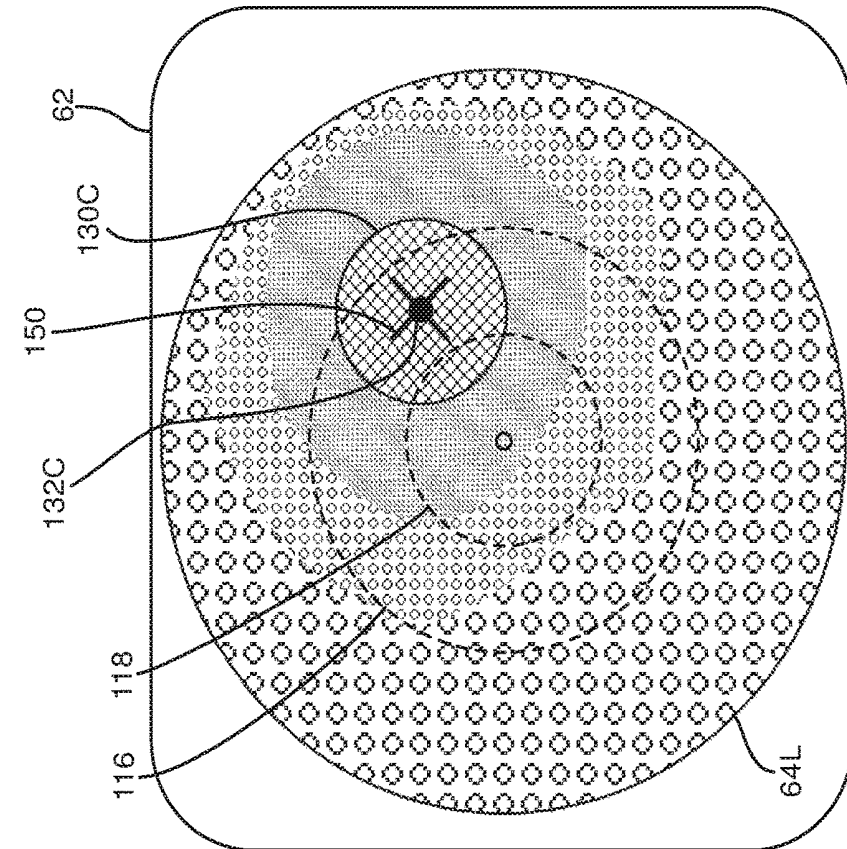


FIG. 8B

MAPPING FORCE AND TEMPERATURE FOR A CATHETER

FIELD OF THE INVENTION

[0001] The present invention relates generally to graphic displays, and specifically to displays related to the temperature and force measured by a catheter.

BACKGROUND OF THE INVENTION

[0002] PCT/US2012/059131 Patent Application to Ghafari et al., whose disclosure is incorporated herein by reference, describes an apparatus for medical diagnosis. The disclosure provides a series of screen shots of an example graphical user interface demonstrating a variety of conditions simulated with the apparatus.

[0003] U.S. Patent Application 2003/0153905 to Edwards, et al. whose disclosure is incorporated herein by reference, describes systems for ablation of hollow organs. The disclosure describes a temperature map in which the temperature data may be used to monitor and control ablation.

[0004] U.S. Patent Application 2006/0253116 to Avitall, et al. whose disclosure is incorporated herein by reference, describes catheters, systems, and methods for performing medical procedures such as tissue ablation. The disclosure describes a graphical representation of an internal anatomical structure, which may be displayed in a display window of a monitor.

[0005] U.S. Patent Application 2007/0293792 to Sliwa, et al. whose disclosure is incorporated herein by reference, describes prostate probe systems comprising either a force or pressure sensor mounted on or in a rectally insertable probe or a temperature sensor mounted on or in a rectally insertable probe, or both. The disclosure describes a thermographic or temperature mapping capability.

[0006] U.S. Patent Application 2012/0226130 to De Graff, et al. whose disclosure is incorporated herein by reference, describes systems that integrate stretchable or flexible circuitry, including arrays of active devices for enhanced sensing, diagnostic, and therapeutic capabilities. The disclosure describes a graphical presentation and mapping functionality.

[0007] U.S. Patent Application 2012/0232388 to Curra, et al. whose disclosure is incorporated herein by reference, describes ultrasound systems and methods for real-time noninvasive spatial temperature estimation. The disclosure claims that strain and spectral information can be compounded and correlated with both strain-based and spectral-based temperature calibration maps.

[0008] U.S. Patent Application 2013/0079650 to Turge-man, et al. whose disclosure is incorporated herein by reference, describes a graphic user interface for physical parameter mapping. The disclosure describes receiving a selection, from a user of a value in a parameter sub-range and displaying a candidate location for further measurement.

[0009] Endosense, of Geneva, Switzerland, produce a "Tactisys Quartz" system. The system is claimed to allow visualization of contact force between a catheter tip of the system and a heart wall.

[0010] Documents incorporated by reference in the present patent application are to be considered an integral part of the application except that to the extent any terms are defined in these incorporated documents in a manner that conflicts with the definitions made explicitly or implicitly in

the present specification, only the definitions in the present specification should be considered.

SUMMARY OF THE INVENTION

[0011] An embodiment of the present invention provides a method for displaying information, including:

[0012] receiving measurements, with respect to an invasive probe inside a body of a subject, of probe parameters consisting of a force exerted by the probe on tissue of the subject and temperatures measured by sensors of the probe; and

[0013] responsively to the measurements, displaying in a single map on a display screen a graphical representation of a distribution of the temperatures in a vicinity of the probe and superimposing thereon a vector representation of the force.

[0014] Typically, the vector representation includes a first indication of a magnitude of the force and a second indication of a force-direction of the force.

[0015] In a disclosed embodiment the vector representation includes an arrow, the first indication includes a width of the arrow, and the second indication includes a combination of a length of the arrow and a direction of the arrow.

[0016] In a further disclosed embodiment the vector representation includes an arrow and a text box associated with the arrow, the first indication includes text within the text box, and the second indication includes a combination of a length of the arrow and a direction of the arrow.

[0017] In a yet further disclosed embodiment the vector representation includes a first circle having a first center, the graphical representation of the distribution includes a second circle having a second center, the first indication includes a diameter of the first circle, and the second indication consists of a combination of a distance between the first and second centers and a direction therebetween.

[0018] In an alternative embodiment the method includes calculating a center of the graphical representation, and displaying the center in the single map.

[0019] There is further provided, according to an embodiment of the present invention embodiment of the present invention, apparatus for displaying information, including:

[0020] a probe, configured to be inserted into a body of a subject;

[0021] a force sensor attached to the probe, coupled to provide a force signal indicative of a force exerted by the probe on tissue of the subject;

[0022] temperature sensors attached to the probe, coupled to provide temperature signals of temperatures in a vicinity of the probe;

[0023] a display screen; and

[0024] a processor coupled to receive the force signal and the temperature signals, to display in a single map on the display screen a graphical representation of a distribution of the temperatures, and to superimpose thereon a vector representation of the force.

[0025] The present disclosure will be more fully understood from the following detailed description of the embodiments thereof, taken together with the drawings, in which:

BRIEF DESCRIPTION OF THE DRAWINGS

[0026] FIG. 1 is a schematic illustration of an invasive medical procedure, according to an embodiment of the present invention;

[0027] FIGS. 2A, 2B, and 2C schematically illustrate a distal end of a probe used in the procedure of FIG. 1, according to an embodiment of the present invention;

[0028] FIG. 3A is a schematic diagram illustrating a temperature distribution in the vicinity of a distal end of the probe, as displayed on a screen, according to an embodiment of the present invention;

[0029] FIG. 3B is a schematic diagram illustrating a vector representation of the force exerted by the distal end, as displayed on the screen, according to an embodiment of the present invention;

[0030] FIG. 3C and FIG. 3D are respective illustrations of a first single combined force-temperature map and a second single combined force-temperature map, according to embodiments of the present invention;

[0031] FIG. 4A is a schematic diagram illustrating a vector representation of the force exerted by distal the end 22, as displayed on the screen, according to an alternative embodiment of the present invention;

[0032] FIG. 4B and FIG. 4C are respective illustrations of single combined force-temperature maps, according to alternative embodiments of the present invention;

[0033] FIG. 5A is a schematic diagram illustrating a vector representation of the force exerted by the distal end, according to a further alternative embodiment of the present invention;

[0034] FIG. 5B and FIG. 5C are respective illustrations of single combined force-temperature maps, according to further alternative embodiments of the present invention;

[0035] FIG. 6A and FIG. 6B are respective illustrations of single combined force-temperature maps, according to disclosed embodiments of the present invention;

[0036] FIG. 7A and FIG. 7B are respective illustrations of single combined force-temperature maps, according to further disclosed embodiments of the present invention; and

[0037] FIG. 8A and FIG. 8B are respective illustrations of single combined force-temperature maps, according to yet further disclosed embodiments of the present invention.

DETAILED DESCRIPTION OF EMBODIMENTS

[0038] In the following description, like elements in the drawings are identified by like numerals, and the like elements are differentiated as necessary by appending a letter to the identifying numeral.

[0039] FIG. 1 is a schematic illustration of an invasive medical procedure 10 using apparatus 12, according to an embodiment of the present invention. The procedure is performed by a medical professional 14, and, by way of example, procedure 10 is assumed to comprise ablation of a portion of a myocardium 16 of the heart of a human patient 18. In order to perform the ablation, professional 14 inserts a probe 20 into a lumen of the patient, so that a distal end 22 of the probe enters the heart of the patient. Distal end 22 comprises electrodes 24 mounted on the outside of the distal end, the electrodes contacting respective regions of the myocardium. Probe 20 has a proximal end 28. Distal end 22 of the probe is described in more detail below with reference to FIGS. 2A and 2B. Apparatus 12 is controlled by a system processor 46, which is located in an operating console 48 of the apparatus. During the procedure, processor 46 typically tracks a location and an orientation of distal end 22 of the probe, using any method known in the art. For example, processor 46 may use a magnetic tracking method, wherein magnetic transmitters external to patient 18 generate signals

in coils positioned in the distal end. The Carto® system produced by Biosense Webster, of Diamond Bar, Calif., uses such a tracking method.

[0040] The software for processor 46 may be downloaded to the processor in electronic form, over a network, for example. Alternatively or additionally, the software may be provided on non-transitory tangible media, such as optical, magnetic, or electronic storage media. The track of distal end 22 is typically displayed on a three-dimensional representation 60 of the heart of patient 18 on a screen 62.

[0041] In order to operate apparatus 12, processor 46 communicates with a memory 50, which has a number of modules used by the processor to operate the apparatus. Thus, memory 50 comprises a temperature module 52, an ablation module 54, and a force module 56, the functions of which are described below. Memory 50 typically comprises other modules, such as a tracking module for operating the tracking method used by processor 46, and an irrigation module allowing the processor to control irrigation provided for distal end 22. For simplicity, such other modules, which may comprise hardware as well as software elements, are not illustrated in FIG. 1.

[0042] Processor 46 uses results of measurements of temperature and force, acquired by modules 52 and 56, to display on screen 62 a combined force-temperature map 64. Embodiments of force-temperature map 64 are described in more detail below.

[0043] FIGS. 2A, 2B, and 2C schematically illustrate distal end 22 of probe 20, according to an embodiment of the present invention. FIG. 2A is a sectional view along the length of the probe, FIG. 2B is a cross-sectional view along a cut IIB-IIB that is marked in FIG. 2A, and FIG. 2C is a perspective view of a section of the distal end. An insertion tube 70 extends along the length of the probe and is connected at the termination of its distal end to a conductive cap electrode 24A, which is assumed herein to be used for ablation. FIG. 2C is a schematic perspective view cap electrode 24A. Cap electrode 24A has an approximately plane conducting surface 84 at its distal end and a substantially circular edge 86 at its proximal end. Conductive cap electrode 24A is herein also termed. The ablation electrode. Proximal to ablation electrode 24A there are typically other electrodes such as electrode 24B. Typically, insertion tube 70 comprises a flexible, biocompatible polymer, while electrodes 24A, 21B comprise a biocompatible metal, such as gold or platinum, for example. Ablation electrode 24A is typically perforated by an array of irrigation apertures 72.

[0044] An electrical conductor 74 conveys radio-frequency (RF) electrical energy from ablation module 54 (FIG. 1), through insertion tube 70, to electrode 24A, and thus energizes the electrode to ablate myocardial tissue with which the electrode is in contact. Module 54 controls the level of RF power dissipated via electrode 34A. During the ablation procedure, cooling fluid flowing out through apertures 72 may irrigate the tissue under treatment. Temperature sensors 78 are mounted within conductive cap electrode 24A at locations that are arrayed around the distal tip of the probe, both axially and circumferentially. In this example, cap 24A contains six sensors, with one group in a distal location, close to the tip, and the other group in a slightly more proximal location. This distribution is shown only by way of example, however, and greater or smaller numbers of sensors may be mounted in any suitable locations within the cap. Sensors 78 may comprise thermocouples, thermistors,

or any other suitable type of miniature temperature sensor. These sensors are connected by leads **80** running through the length of insertion tube **70** to provide temperature signals to temperature module **52**.

[0045] In a disclosed embodiment cap **24A** comprises a side wall **73** that is relatively thick, on the order of 0.5 mm thick, in order to provide the desired thermal insulation between temperature sensors **78** and the cooling fluid inside a central cavity **75** of the tip. The cooling fluid exits cavity **75** through apertures **72**. Sensors **78** are mounted on rods **77**, which are fitted into longitudinal bores **79** in side wall **73**. Rods **77** may comprise a suitable plastic material, such as polyimide, and may be held in place at their distal ends by a suitable glue **81**, such as epoxy. U.S. patent application Ser. No. 13/716,578, which is incorporated herein by reference, describes a catheter having temperature sensors mounted in a similar configuration to that described above. The arrangement described above provides an array of six sensors **78**, but other arrangements, and other numbers of sensors, will be apparent to those having ordinary skill in the art, and all such arrangements and numbers are included within the scope of the present invention. Another arrangement of sensors is described in U.S. patent application Ser. No. 13/716,578, referenced above.

[0046] In addition to the temperature sensors, distal end **22** comprises a force sensor **90**, which is configured to measure the force exerted by the distal end on tissue contacted by the distal end. Force sensor **90** generates signals in response to the measured force, and the signals are transferred to force module **56**, which operates the sensor and which calculates a value for the magnitude, as well as a value for the direction, of the force exerted. The direction of the force exerted is measured with respect to an axis **92**, typically the axis of symmetry, of distal end **22**.

[0047] In the description herein, distal end **22** is assumed to define a set of xyz orthogonal axes, where axis **92** corresponds to the z axis of the set, and orthogonal x and y axes are in any convenient xy plane orthogonal to the z axis. For simplicity, the xy plane is herein assumed to correspond to the plane defined by circle **86**, the origin of the xyz axes is assumed to be the center of the circle. Force sensor **90** may comprise any convenient sensor of force or pressure known in the art. By way of example, herein force sensor **90** is assumed to operate by measuring the deflection, parallel to z axis **92** and orthogonal to the axis, i.e., in an xy plane, of a cylindrically shaped spring **94**. The deflection of spring **94** may be measured by transmitting an alternating magnetic field from a magnetic transmitter **96** located in proximity to the distal end of the spring, and measuring the received magnetic field in magnetic receivers **98** located at the proximal end of the spring. Typically transmitter **96** and receivers **98** are coils, transmitter **96** being located on axis **92**, and receivers **98** being distributed symmetrically around the axis. In force sensor **90** there are three receivers **98** (two are shown in the figure). Operating signals between force module **90** and the transmitter and the receivers are transferred by conductors **100**, and enable the force module to generate a unique value for the magnitude of a given force, as well as a unique value for the direction of the force with respect to the xyz axes of distal end **22**. Force sensors similar to force sensor **90** are described in U.S. Patent Applications 2009/0306650 to Govari et al., 2011/0130648 to Beeckler et al., and 2012/0253167 to Bonyak et al., all of which are incorporated herein by reference.

[0048] Typically, distal end **22** contains other functional components, which are outside the scope of the present disclosure and are therefore omitted for the sake of simplicity. For example, the distal end of the probe may contain steering wires, as well as sensors of other types, such as a position sensor. Probes containing components of these kinds are described, for example, in U.S. Patent Applications 2009/0306650 and 2011/0130648, referenced above.

[0049] FIG. 3A is a schematic diagram illustrating a temperature distribution in the vicinity of distal end **22**, as displayed on screen **62**, according to an embodiment of the present invention. Using measurements provided by temperature sensors **78**, as well as knowledge of the positions of the sensors with respect to each other and with respect to the xyz axes of distal end **22**, processor **46** uses temperature module **52** to generate a two-dimensional (2D) temperature map **100**. 2D map **100** is a graphical representation of the three-dimensional (3D) distribution of the temperatures of the external surface of electrode **24A**, and is assumed to be drawn as a 2D projection with respect to the xyz axes defined above for distal end **22**. Map **100** is drawn as a circular map, a bounding circle **102** of the map corresponding with edge **86** of electrode **24A**. The generation of 2D map **100** from measurements of sensors **78** typically uses interpolation and extrapolation from the measurements, as is known in the art.

[0050] As stated above, 2D map **100** is a 2D projection of a 3D distribution of temperatures. One type of projection that may be used, based on angles subtended by a line through the origin of the xyz axes to the z-axis (FIG. 2A), is described in more detail with respect to FIG. 3B, which illustrates a projection used to represent the direction of a force vector. As is assumed in the following description, the same type of projection may be used to represent the temperature distribution and the force vector. However, there is no necessity that the projections are the same, and in some embodiments the projections are different.

[0051] 2D map **100** is typically a color map showing the different temperatures of the external surface of electrode **24A**, and a legend **104** may be displayed with the map showing values of the temperatures for the different colors. (In the figures different colors are schematically illustrated by different shadings.) In some embodiments the numerical values measured by each of sensors **78** may also be displayed on map **100**. For simplicity, the display of such numerical values is not illustrated in FIG. 3A.

[0052] FIG. 3B is a schematic diagram illustrating a vector representation **108** of the force exerted by distal end **22**, as displayed on screen **62**, according to an embodiment of the present invention. As explained above force sensor **90** is able to generate signals which may be used by force module **56** and processor **46** to find a magnitude of the force exerted by distal end **22**, as well as a direction of the force. The direction of the force may be measured relative to the xyz axes of distal end **22**. Starting with a 3D vector representation of the force, the 3D direction may be represented on a 2D surface such as that of screen **62** by any convenient projection of a 3D direction. By way of example, a projection used herein is similar to a polar stereographic projection, generating a circular map **110**. Map **110** has a bounding circle **112**, which represents directions orthogonal to the z-axis referred to above. A center **114** of map **110** represents directions along the z-axis. In the exemplary projection illustrated herein, a broken circle **116** corresponds to a

direction at 60° to the z-axis, and a broken circle **118** corresponds to a direction at 30° to the z-axis. Circles representing angles to the z-axis, such as circles **116** and **118**, are also herein termed angular circles. By way of example, in the projection assumed herein a diameter of an angular circle is in direct proportion to the angle it represents, so that circles **112**, **116**, and **118** have diameters in the ratio of 3:2:1.

[0053] Representation **108** comprises a variable length arrow **120** representing the direction of the force exerted by distal end **22**, which has been drawn on map **110**. Arrow **120** has a start point corresponding with the center of circle **112**, and an end point corresponding to the angle subtended by the distal end force to the z-axis, so that a length of the arrow is a function of the angle of the force measured with respect to the z-axis. Thus in FIG. 3B, the distal end force is in a direction that is approximately 40° to the z-axis. In representation **108** arrow **120** has a direction with respect to the xy axes corresponding to a projection of a 3D representation of the force vector on the xy plane. FIG. 3B illustrates arrow **120** as subtending an angle of approximately -70° with respect to the x-axis.

[0054] In order to represent the magnitude of the force in representation **108**, in a disclosed embodiment a width of arrow **120** is varied according to the magnitude. By varying the width of the arrow, representation **108** is a complete vector representation of the magnitude and the direction of the force exerted by distal end **22**.

[0055] FIG. 3C and FIG. 3D are respective illustrations of a single combined force-temperature map **64A** and a single combined force-temperature map **64B**, according to embodiments of the present invention. In the following description, elements indicated by the same reference numerals in FIGS. 3A, 3B, 3C, and 3D are generally similar in function. Maps **64A** and **64B** are formed by having circles **102** and **112** (FIGS. 3A and 3B) the same diameter, and superimposing the resulting circular temperature map **100** and force representation **108** on each other, so as to form single maps **64A** and **64B** on screen **62**. Thus combined force-temperature map **64A** displays both the temperature distribution in the vicinity of distal end **22** and the force exerted by the distal end. For a different case, combined force-temperature map **64B** also displays the temperature distribution and the force. In both maps the force is displayed as an arrow, and a color of the arrow is selected so that the arrow is easily differentiated from the temperature distribution.

[0056] In the presentation of single map **64** on screen **62**, an operator of the system may choose to display all, some, or none of the xyz axes and the angular circles. By way of example, in the examples illustrated herein, angular circles, but not the xyz axes, are displayed.

[0057] Single maps **64A** and **64B** have the same temperature distribution, and the force is in the same direction (approximately 40° to the z-axis and -70° to the x-axis). However, the magnitudes of the force in the two maps is different, the difference being presented on screen **62** as different widths of an arrow **120A** in map **64A** and an arrow **120B** in map **64B**. Usually a width of the arrow representing the force as configured to be proportional to, and typically directly proportional to, a magnitude of the force. FIGS. 3C and 3D show that arrow **120B** (map **64B**) is wider than arrow **120A** (map **64A**). Thus, for example, the force in map **64A** may be 2 g, and the force in map **64B** may be 3 g.

[0058] FIG. 4A is a schematic diagram illustrating a vector representation **128** of the force exerted by distal end **22**, as

displayed on screen **62**, according to an alternative embodiment of the present invention. Apart from the differences described below, vector representation **128** (FIG. 4A) is generally similar to representation **108** (FIG. 3B), and elements indicated by the same reference numerals in both representations are generally similar in function and in properties.

[0059] Rather than using an arrow to represent the force exerted by distal end **22**, representation **128** uses a circle **130**. A center **132** of the circle, measured with respect to center **114** and the xy axes, represents the direction of the force exerted by the distal end. FIG. 4A has been drawn assuming the force on distal end **22** is the same as that illustrated in FIG. 3B. Thus in FIG. 4A, angular circles **116** and **118** indicate that center **132** is in a direction that is approximately 40° to the z-axis, and an imaginary line between centers **114** and **132** subtends an angle of approximately 70° with respect to the x-axis.

[0060] In order to represent the magnitude of the force in representation **128**, in a disclosed embodiment a diameter of circle **130** is varied according to the magnitude. By varying the diameter of the circle, representation **128** is a complete vector representation of the magnitude and the direction of the force exerted by distal end **22**.

[0061] FIG. 4B and FIG. 4C are respective illustrations of a single combined force-temperature map **64C** and a single combined force-temperature map **64D**, according to alternative embodiments of the present invention. In contrast to maps **64A** and **64B**, maps **64C** and **64D** are formed by superimposing temperature map **100** (FIG. 3A) and force representation **128** (FIG. 4A) on each other, and displaying the resulting combined force-temperature map on screen **62**. Thus combined force-temperature map **64C** displays both the temperature distribution in the vicinity of distal end **22** and the force exerted by the distal end. For a different case, combined force-temperature map **64D** also displays the temperature distribution and the force. In both maps the force is displayed as a circle, and a color of the circle is selected so that the circle is easily differentiated from the temperature distribution.

[0062] Single maps **64C** and **64D** have the same temperature distribution, and the force is in the same direction (approximately 40° to the z-axis and -70° to the x-axis), as is indicated by the same positions of centers **132A** and **132B** in their respective circles. However, the magnitudes of the force in the two maps is different, the difference being presented on screen **62** as different diameters of a circle **130A** in map **64C** and a circle **130B** in map **64D**. Usually a diameter of the circle representing the force is configured to be proportional to, and typically directly proportional to, a magnitude of the force. FIGS. 4B and 4C show that circle **130B** (map **64D**) has a larger diameter than circle **130A** (map **64C**). Thus, for example, the force in map **64C** may be 2 g, and the force in map **64D** may be 3 g.

[0063] FIG. 5A is a schematic diagram illustrating a vector representation **138** of the force exerted by distal end **22**, as displayed on screen **62**, according to a further alternative embodiment of the present invention. Apart from the differences described below, vector representation **138** (FIG. 5A) is generally similar to representation **108** (FIG. 3B), and elements indicated by the same reference numerals in the two representations are generally similar in function and in properties.

[0064] Rather than using a variable length arrow having a variable width (as described above for representation 108) to represent the force exerted by distal end 22, representation 138 uses a variable length arrow 140 with a constant width. Except that it is invariant with regard to width, arrow 140 is generally similar to arrow 120 (FIG. 3B), so that a length of arrow 140 is a function of the angle subtended by the force with the z-axis. FIG. 5A has been drawn assuming the force on distal end 22 is the same as that illustrated in FIG. 3B. Thus, in FIG. 5A, the end or length of arrow 140 indicates that the force is in a direction that is approximately 40° to the z-axis, and the direction of the arrow indicates that the force subtends an angle of approximately -70° with respect to the x-axis.

[0065] In order to represent the magnitude of the force in representation 138, in a disclosed embodiment a text box 142 is “attached” to arrow 140 and a value corresponding to the force magnitude is entered into the text box. By way of example, text box 142 is attached to the head of arrow 140, but in other embodiments text box 142 may be in any convenient position with respect to the arrow. Text within the text box gives a magnitude of the force, so that representation 138 is a complete vector representation of the force on distal end 22.

[0066] FIG. 5B and FIG. 5C are respective illustrations of a single combined force-temperature map 64E and a single combined force-temperature map 64F, according to further alternative embodiments of the present invention. Except for the following differences, maps 64E and 64F are generally similar to maps 64A and 64B. However, in contrast to maps 64A and 64B, maps 64E and 64F are formed by superimposing temperature map 100 (FIG. 3A) and force representation 138 (FIG. 5A) on each other, and displaying the resulting combined force-temperature map on screen 62. Thus combined force-temperature map 64E displays both the temperature distribution in the vicinity of distal end 22 and the force exerted by the distal end. For a different case, combined force-temperature map 64F also displays the temperature distribution and the force. In both maps the direction of the force is displayed as an arrow.

[0067] Single maps 64E and 64F have the same temperature distribution, and the force is in the same direction (approximately 40° to the z-axis and -70° to the x-axis), as is indicated by the same directions and lengths of arrows 140A and 140B. However, the magnitudes of the force in the two maps are different, the difference being presented on screen 62 as a text box 142A in map 64E and as a text box 142B in map 64F. Thus, for example, the force in map 64E is 2 g, and the force in map 64F is 3 g.

[0068] FIG. 6A and FIG. 6B are respective illustrations of a single combined force-temperature map 64G and a single combined force-temperature map 64H, according to embodiments of the present invention. Except for the following differences, maps 64G and 64H are generally similar to maps 64E and 64F. Maps 64E, 64F, 64G, and 64H are all combined force-temperature maps, using the embodiment illustrated in FIGS. 5A-5C, with the same temperature distribution. However, while maps 64E, 64F illustrate the force as having the same direction and a different magnitude, maps 64G, 64H illustrate the force as having the same magnitude of 2 g, but different force directions. Thus map 64G illustrates the force as subtending approximately 30° to

the z-axis, and -20° to the x-axis, and map 64H illustrates the force as subtending approximately 60° to the z-axis, and -70° to the x-axis.

[0069] FIG. 7A and FIG. 7B are respective illustrations of a single combined force-temperature map 64J and a single combined force-temperature map 64K, according to embodiments of the present invention. Except for the following differences, maps 64J and 64K are generally similar to maps 64A and 64B. Maps 64A, 64B, 64J, and 64K are all combined force-temperature maps, using the embodiment illustrated in FIGS. 3B-3D, with the same temperature distribution. However, while maps 64A, 64B illustrate the force as having the same direction and a different magnitude, shown by the different arrow widths, maps 64J, 64K illustrate the force as having the same magnitude, since arrows 120C and 120D have the same widths. However, the forces in the two maps have different directions. Thus map 64J illustrates the force as subtending approximately 30° to the z-axis, and -90° to the x-axis, and map 64K illustrates the force as subtending approximately 70° to the z-axis, and -90° to the x-axis.

[0070] By presenting the force (in magnitude and direction) together with the temperature distribution in a single map, embodiments of the present invention facilitate the ablation process performed by a physician, by enabling the physician to see the relative alignment between the force and the temperature distribution. For example, during the ablation process, the physician may desire that the force is directed to the hottest part of the temperature distribution, so that the force “aligns” with the temperature. This is typically the desired state during ablation of a single region. Alternatively, the physician may desire that the force is directed in a particular direction away from the hottest part of the temperature distribution. This is typically the desired state during ablation along a line. Embodiments of the present invention.

[0071] facilitate these types of alignment by allowing the physician to mark a “center” of the temperature, which enables the physician to compare the direction of the force, and the “direction” of the temperature distribution.

[0072] FIG. 8A and FIG. 8B are respective illustrations of a single combined force-temperature map 64L and a single combined force-temperature map 64M, according to embodiments of the present invention. The two maps have the same temperature distribution, but in map 64L the force is represented as a circle 130C with a center 132C, as described above with respect to FIG. 4A, and in map 64M the force is represented as an arrow 140C with an attached text box 142C, as described above with respect to FIG. 5A.

[0073] A center of the temperature distribution is calculated by any means known in the art. For example, the center may correspond to a weighted center of gravity of regions of the distribution, where the weights are according to the temperatures of each of the regions. In map 64L a temperature distribution center 150 is indicated by an X on the map; in map 64M a temperature distribution center 152 is indicated by cross-hairs on the map. In map 64L the force direction is shown as aligning with temperature distribution center 150, in a “bullseye” type of display, which may be the desired situation for ablation of a single region. In contrast, in map 64M the force does not align with temperature distribution center 152, and this may be the desired situation for ablation along a line.

[0074] It will be appreciated that the embodiments described above are cited by way of example, and that the present invention is not limited to what has been particularly shown and described hereinabove. Rather, the scope of the present invention includes both combinations and subcombinations of the various features described hereinabove, as well as variations and modifications thereof which would occur to persons skilled in the art upon reading the foregoing description and which are not disclosed in the prior art.

1. A method for displaying information, comprising:
receiving measurements, with respect to an invasive probe inside a body of a subject, of probe parameters comprising a force exerted by the probe on tissue of the subject and temperatures measured by sensors of the probe; and
responsively to the measurements, displaying in a single map on a display screen a graphical representation of a distribution of the temperatures in a vicinity of the probe and superimposing thereon a vector representation of the force.
2. The method according to claim 1, wherein the vector representation comprises a first indication of a magnitude of the force and a second indication of a force-direction of the force.

3. The method according to claim 2, wherein the vector representation comprises an arrow, and wherein the first indication comprises a width of the arrow, and wherein the second indication comprises a combination of a length of the arrow and a direction of the arrow.

4. The method according to claim 2, wherein the vector representation comprises an arrow and a text box associated therewith, and wherein the first indication comprises text within the text box, and wherein the second indication comprises a combination of a length of the arrow and a direction of the arrow.

5. The method according to claim 2, wherein the vector representation comprises a first circle having a first center, and wherein the graphical representation of the distribution comprises a second circle having a second center, and wherein the first indication comprises a diameter of the first circle, and wherein the second indication comprises a combination of a distance between the first and second centers and a direction therebetween.

6. The method according to claim 1, and comprising calculating a center of the graphical representation, and displaying the center in the single map.

7-12. (canceled)

* * * * *

专利名称(译)	绘制导管的力和温度		
公开(公告)号	US20180242852A1	公开(公告)日	2018-08-30
申请号	US15/966662	申请日	2018-04-30
[标]申请(专利权)人(译)	韦伯斯特生物官能(以色列)有限公司		
申请(专利权)人(译)	生物传感韦伯斯特 (以色列) LTD.		
当前申请(专利权)人(译)	生物传感韦伯斯特 (以色列) LTD.		
[标]发明人	GOVARI ASSAF BEECKLER CHRISTOPHER THOMAS		
发明人	GOVARI, ASSAF BEECKLER, CHRISTOPHER THOMAS		
IPC分类号	A61B5/01 A61B5/00 A61B5/103 A61B17/00 A61B18/00 A61B18/14 A61B34/20 A61B90/00		
CPC分类号	A61B2218/002 A61B18/1492 A61B5/103 A61B5/743 A61B2017/00084 A61B2018/00791 A61B5/6852 A61B2090/064 A61B2090/065 A61B2034/2051 A61B5/015 A61B2018/00029 A61B2018/00357 A61B2018/00577 A61B2018/00815 A61B2018/00821 A61B5/01		
外部链接	USPTO		

摘要(译)

一种用于显示信息的方法，包括接收关于受试者体内的侵入性探针的测量，探针参数包括由探针施加在受试者组织上的力和由探针的传感器测量的温度。该方法还包括，响应于测量，在显示屏上的单个图中显示探针附近的温度分布的图形表示，并在其上叠加力的矢量表示。

