



US009844426B2

(12) **United States Patent**
Atiya et al.

(10) **Patent No.:** **US 9,844,426 B2**
(45) **Date of Patent:** **Dec. 19, 2017**

(54) **DIGITAL DENTAL TRAY**

(71) Applicant: **Align Technology, Inc.**, San Jose, CA (US)

(72) Inventors: **Yossi Atiya**, Maccabim (IL); **Avi Kopelman**, Palo Alto, CA (US); **Erez Lampert**, Rehovot (IL)

(73) Assignee: **Align Technology, Inc.**, San Jose, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 167 days.

(21) Appl. No.: **14/656,523**

(22) Filed: **Mar. 12, 2015**

(65) **Prior Publication Data**

US 2016/0262856 A1 Sep. 15, 2016

(51) **Int. Cl.**

A61B 1/00 (2006.01)

A61B 1/015 (2006.01)

A61B 1/04 (2006.01)

A61B 1/06 (2006.01)

A61B 1/12 (2006.01)

(Continued)

(52) **U.S. Cl.**

CPC **A61C 9/006** (2013.01); **A61B 1/00009** (2013.01); **A61B 1/00016** (2013.01); **A61B 1/00142** (2013.01); **A61B 1/00181** (2013.01); **A61B 1/00193** (2013.01); **A61B 1/015** (2013.01); **A61B 1/04** (2013.01); **A61B 1/06** (2013.01); **A61B 1/0684** (2013.01); **A61B 1/126** (2013.01); **A61B 1/128** (2013.01); **A61B 1/24** (2013.01); **A61B 1/253** (2013.01); **A61B 5/0088** (2013.01); **A61B 5/1077** (2013.01); **A61B 5/1079** (2013.01); **A61B 5/4547** (2013.01); **A61C 9/0006** (2013.01); **A61B 5/01** (2013.01);

(Continued)

(58) **Field of Classification Search**

CPC **A61B 1/00009**; **A61B 1/00016**; **A61B 1/00142**; **A61B 1/015**; **A61B 1/04**; **A61B 1/06**; **A61B 1/126**; **A61B 1/128**; **A61B 1/24**; **A61B 1/253**; **A61C 2204/002**; **A61C 9/0006**; **A61C 9/006**
USPC **348/66**
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,589,054 B2 * 7/2003 Tingley **A61B 8/0875**
433/215
8,520,925 B2 8/2013 Duret
(Continued)

FOREIGN PATENT DOCUMENTS

DE 112012005886 T5 11/2014
WO 97/31293 A1 8/1997
WO 2008/064904 A1 6/2008

OTHER PUBLICATIONS

International Search Report and Written Opinion of the International Searching Authority for PCT Application No. PCT/IB2016/051398 dated May 31, 2016.

(Continued)


Primary Examiner — Deirdre Beasley

(74) Attorney, Agent, or Firm — Lowenstein Sandler LLP

(57) **ABSTRACT**

A digital dental tray system is described including a dental tray shaped to at least partially surround a plurality of teeth and a plurality of three-dimensional (3D) optical imaging elements attached to the dental tray. Each of the 3D optical imaging elements comprises a structured light projector to project a light pattern onto one or more teeth of the plurality of teeth and a camera to capture an image of the one or more teeth.

18 Claims, 8 Drawing Sheets

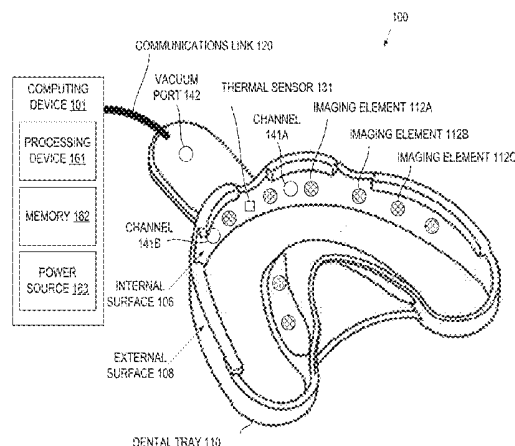

(51) **Int. Cl.**

A61B 1/24 (2006.01)
A61C 9/00 (2006.01)
A61B 1/253 (2006.01)
A61B 5/00 (2006.01)
A61B 5/107 (2006.01)
A61B 5/01 (2006.01)

(52) **U.S. Cl.**

CPC . *A61B 2560/0242* (2013.01); *A61B 2562/043*
 (2013.01); *A61C 2204/002* (2013.01)

(56)

References Cited

U.S. PATENT DOCUMENTS

9,199,574 B2 * 12/2015 Pierce H04N 17/002
 2002/0055082 A1 * 5/2002 Durbin A61C 9/00
 433/29
 2005/0143625 A1 * 6/2005 Whitmore, III ... A61B 1/00142
 600/121
 2007/0248930 A1 * 10/2007 Brawn A61N 5/0613
 433/25
 2008/0063998 A1 * 3/2008 Liang A61B 1/0638
 433/29
 2008/0090198 A1 * 4/2008 Liang A61B 1/0638
 433/29
 2008/0280260 A1 * 11/2008 Belikov A46B 11/002
 433/215
 2009/0080766 A1 * 3/2009 Daxauer G01B 11/2545
 382/154
 2010/0009313 A1 * 1/2010 Kushner A61C 5/00
 433/140
 2010/0036535 A1 * 2/2010 Feine A61C 1/0061
 700/282
 2010/0239136 A1 * 9/2010 Gandyra G01B 11/03
 382/128

2012/0064477 A1 * 3/2012 Schmitt A61C 9/0006
 433/29
 2013/0108981 A1 * 5/2013 Duret A61B 1/24
 433/30
 2013/0323673 A1 * 12/2013 Hakomori A61B 5/0261
 433/29
 2014/0146142 A1 * 5/2014 Duret H04N 13/0242
 348/47
 2014/0212841 A1 * 7/2014 Nguyen A61C 17/043
 433/92
 2014/0272765 A1 * 9/2014 Andreiko A61B 1/00006
 433/27
 2014/0277665 A1 * 9/2014 Fisker A61C 9/0006
 700/98
 2015/0064641 A1 * 3/2015 Gardner A61C 7/146
 433/3
 2015/0079534 A1 * 3/2015 Tsuji A61C 9/0006
 433/29
 2016/0242692 A1 * 8/2016 McAuliffe A61B 5/228

OTHER PUBLICATIONS

Schechner et al., "Depth from Defocus vs. Stereo: How Different Really Are They," International Journal of Computer Vision, 39(2), 2000, http://web.ee.technion.ac.il/~yoav/publications/dfd_stereot2a.pdf.
 Kapusta, Roman, "Scene reconstruction using structured light," Slovak University of Technology Bratislava Faculty of Electrical Engineering and Information Technology, Bratislava, Slovakia, Downloaded Mar. 13, 2015, <http://www.cescg.org/CESCG-2003/RKapusta/paper.pdf>.
 Greengard et al., "Depth from diffracted rotation," Optics Letters, vol. 31, No. 2, Jan. 15, 2006, http://cgm.technion.ac.il/Computer-Graphics-Multimedia/Publications/Papers/2006/2006_Depth_from_diffracted_rotation.pdf.

* cited by examiner

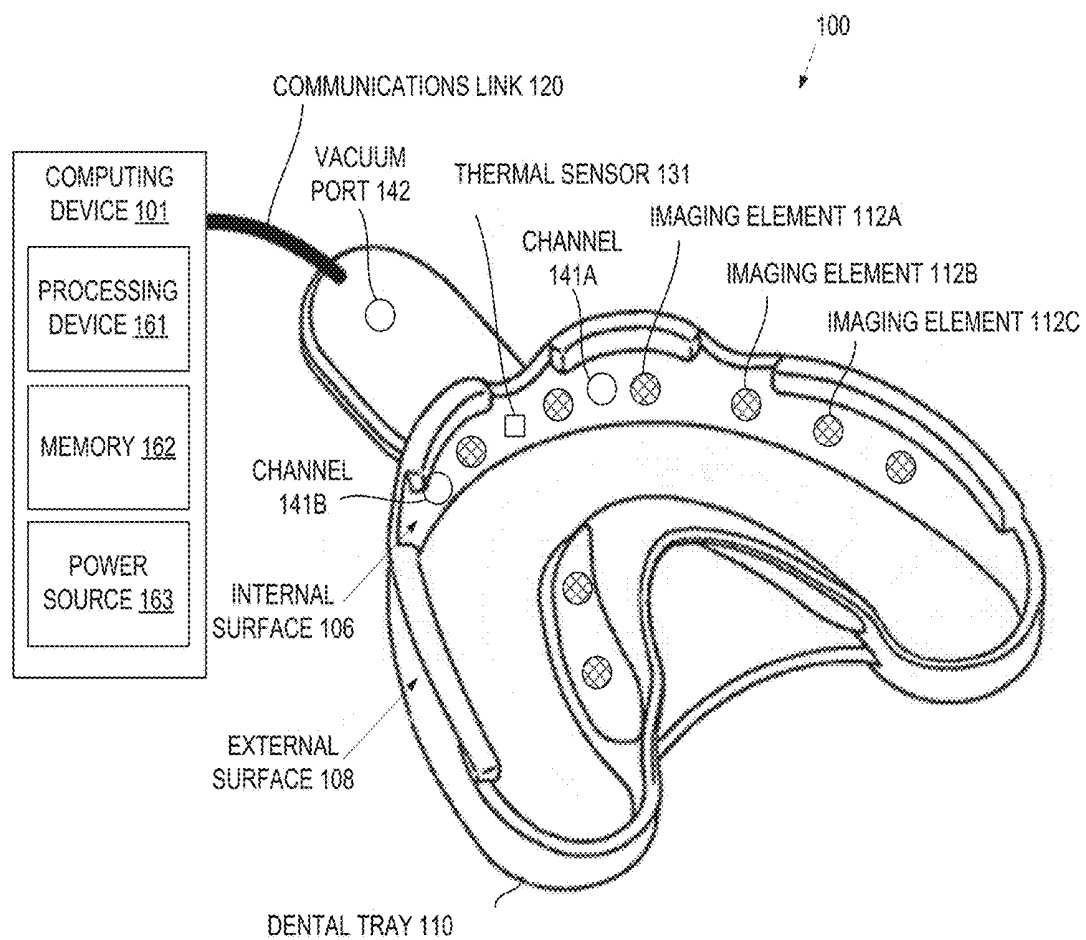


Figure 1

IMAGING ELEMENT 220

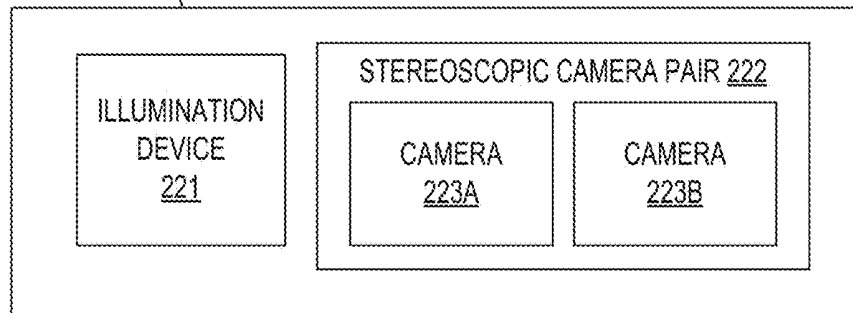


Figure 2A

IMAGING ELEMENT 230

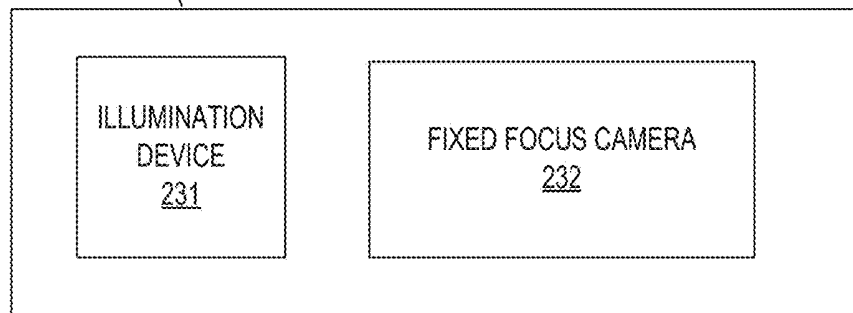


Figure 2B

IMAGING ELEMENT 240

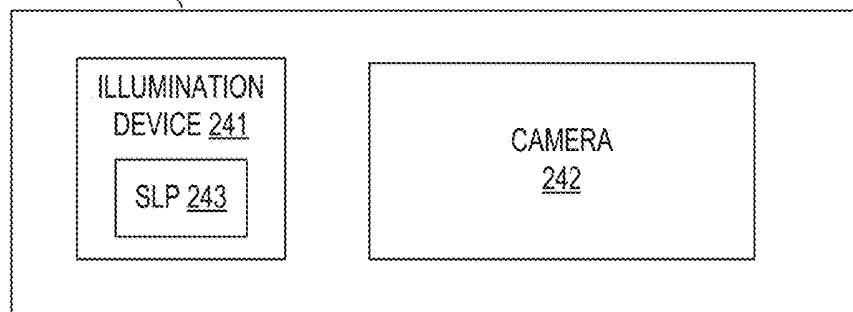


Figure 2C

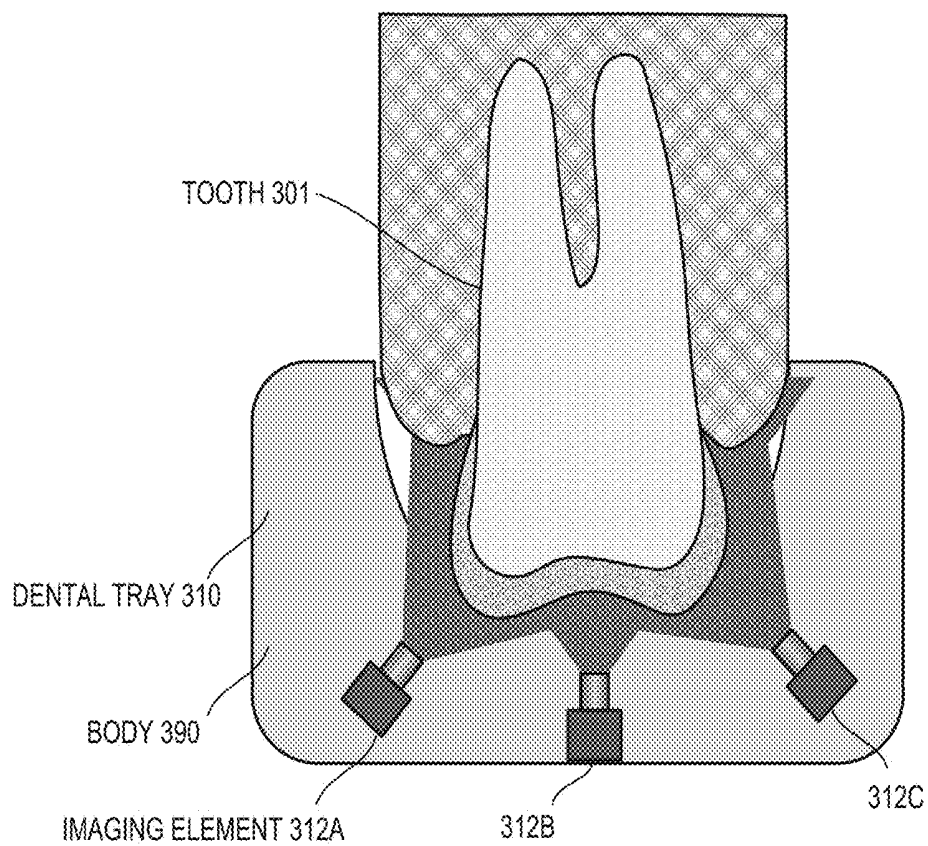


FIG. 3A

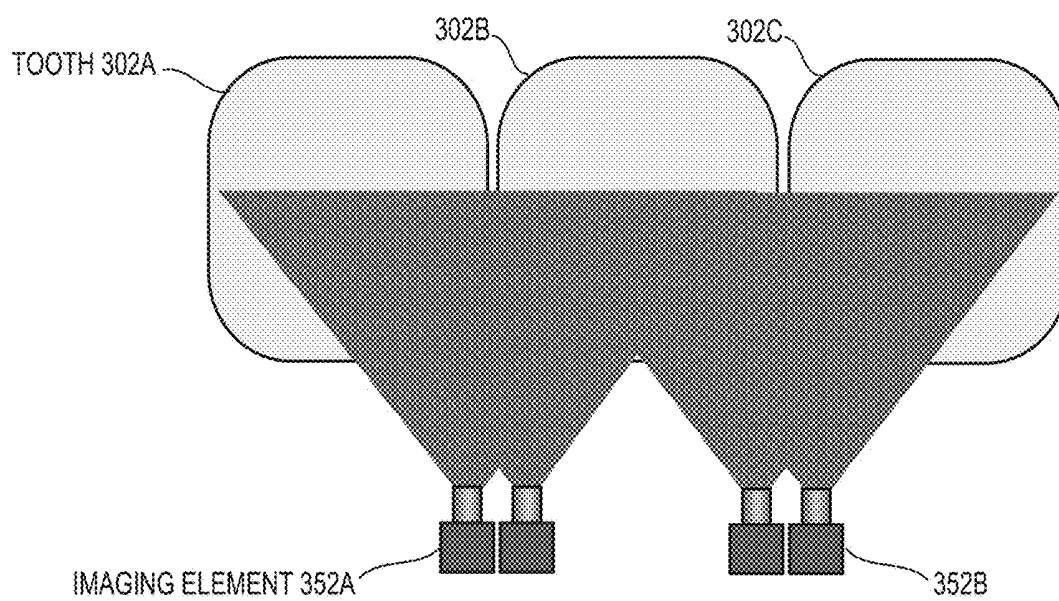


FIG. 3B

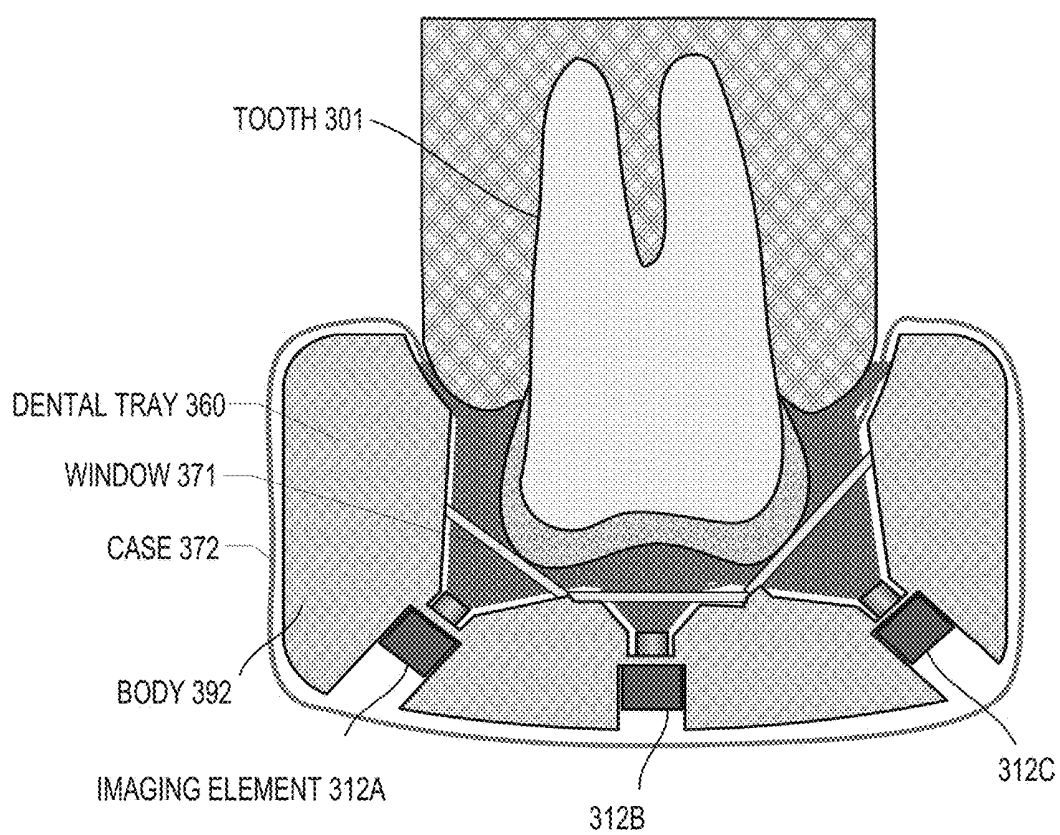


FIG. 3C

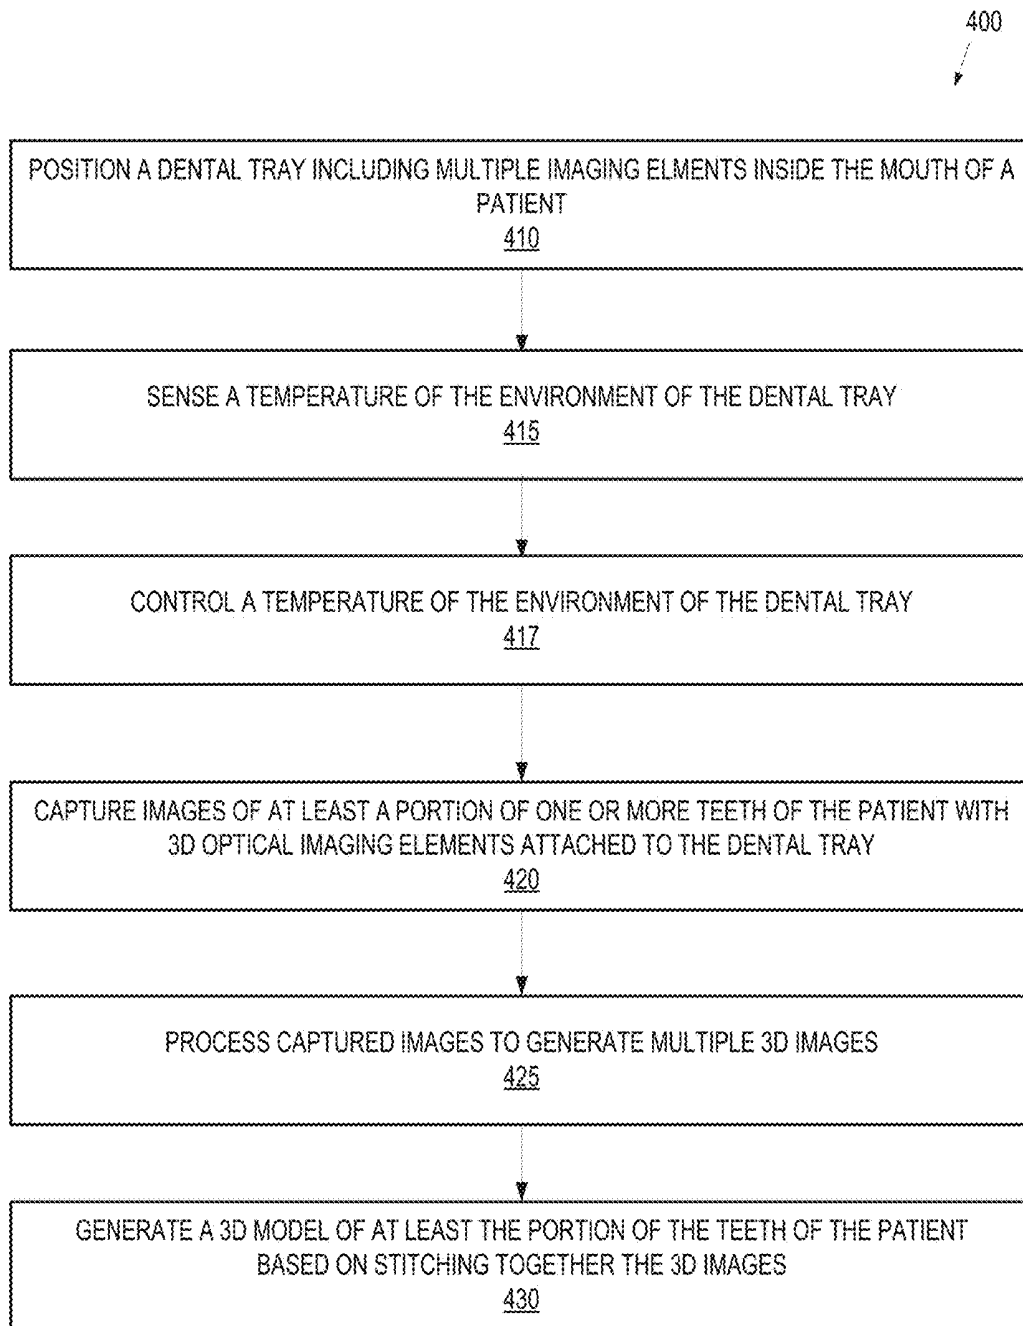


Figure 4

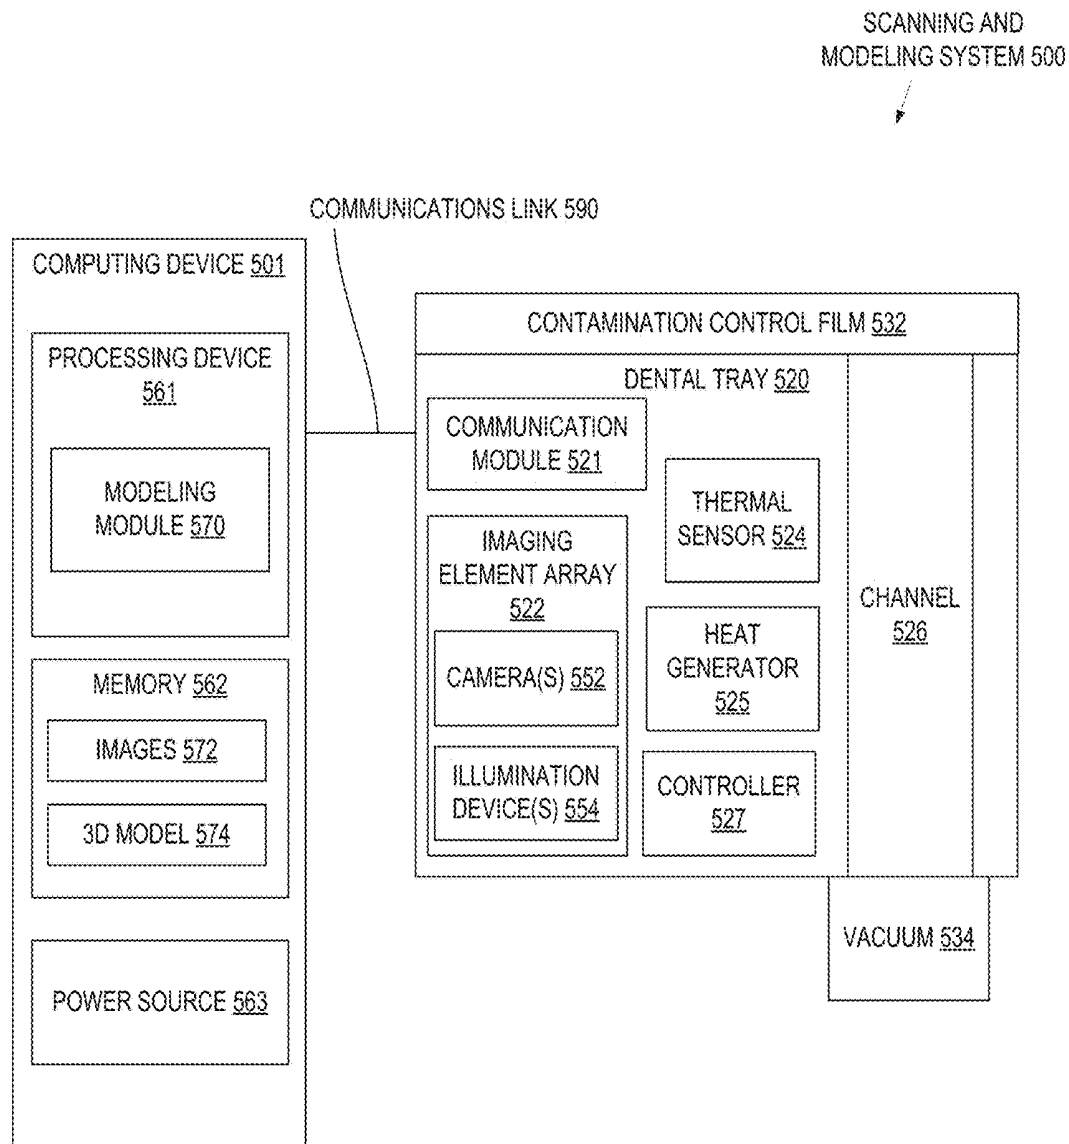


Figure 5

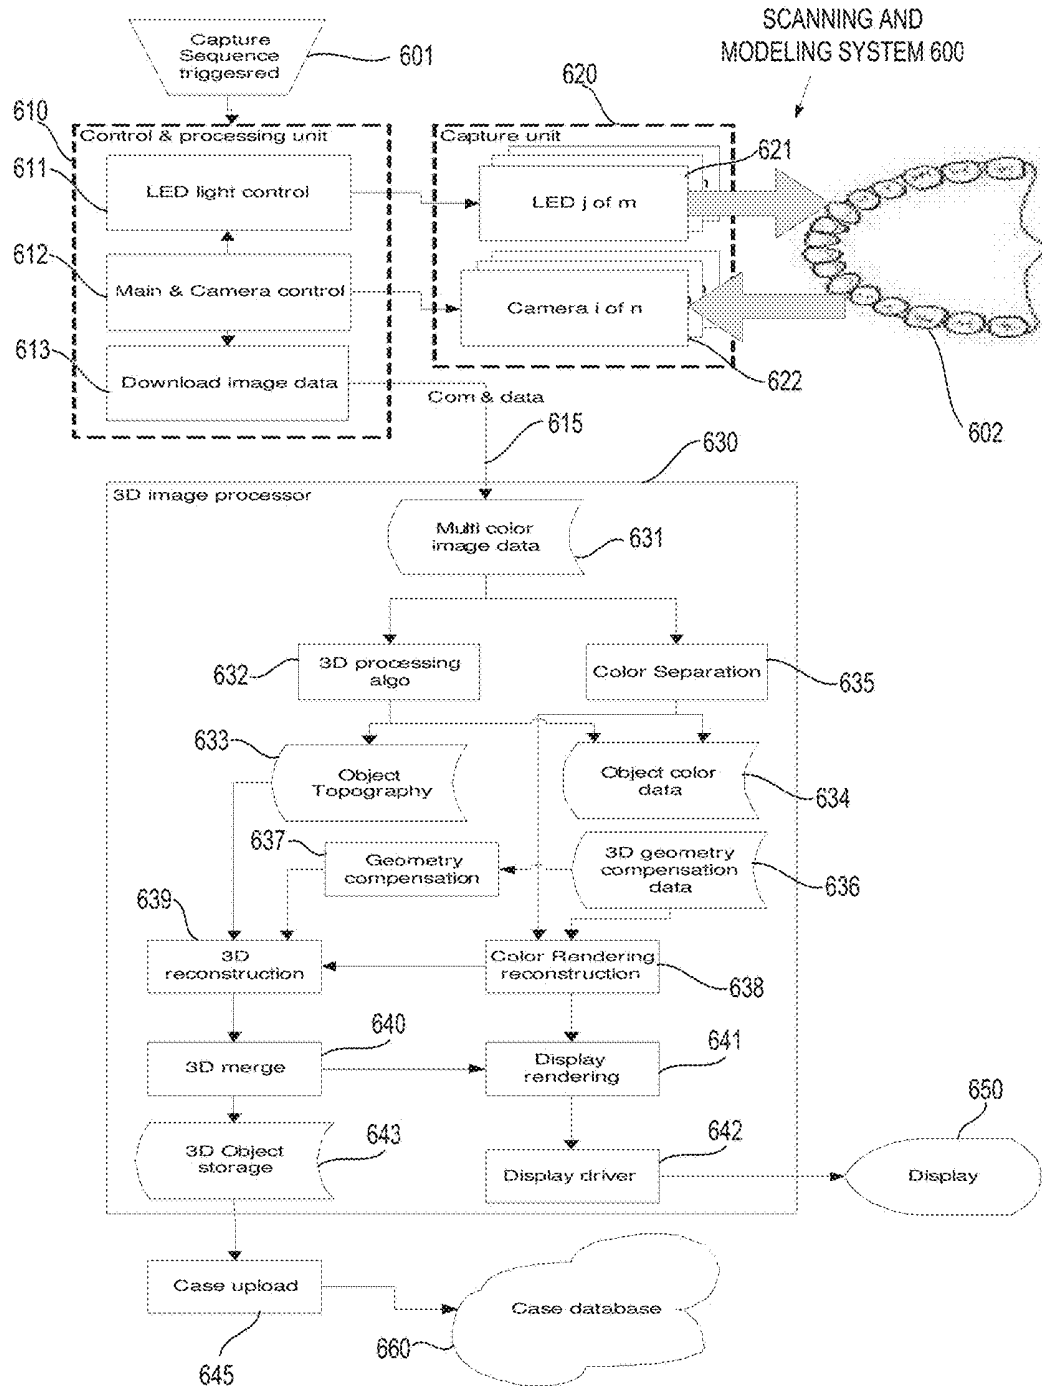


Figure 6

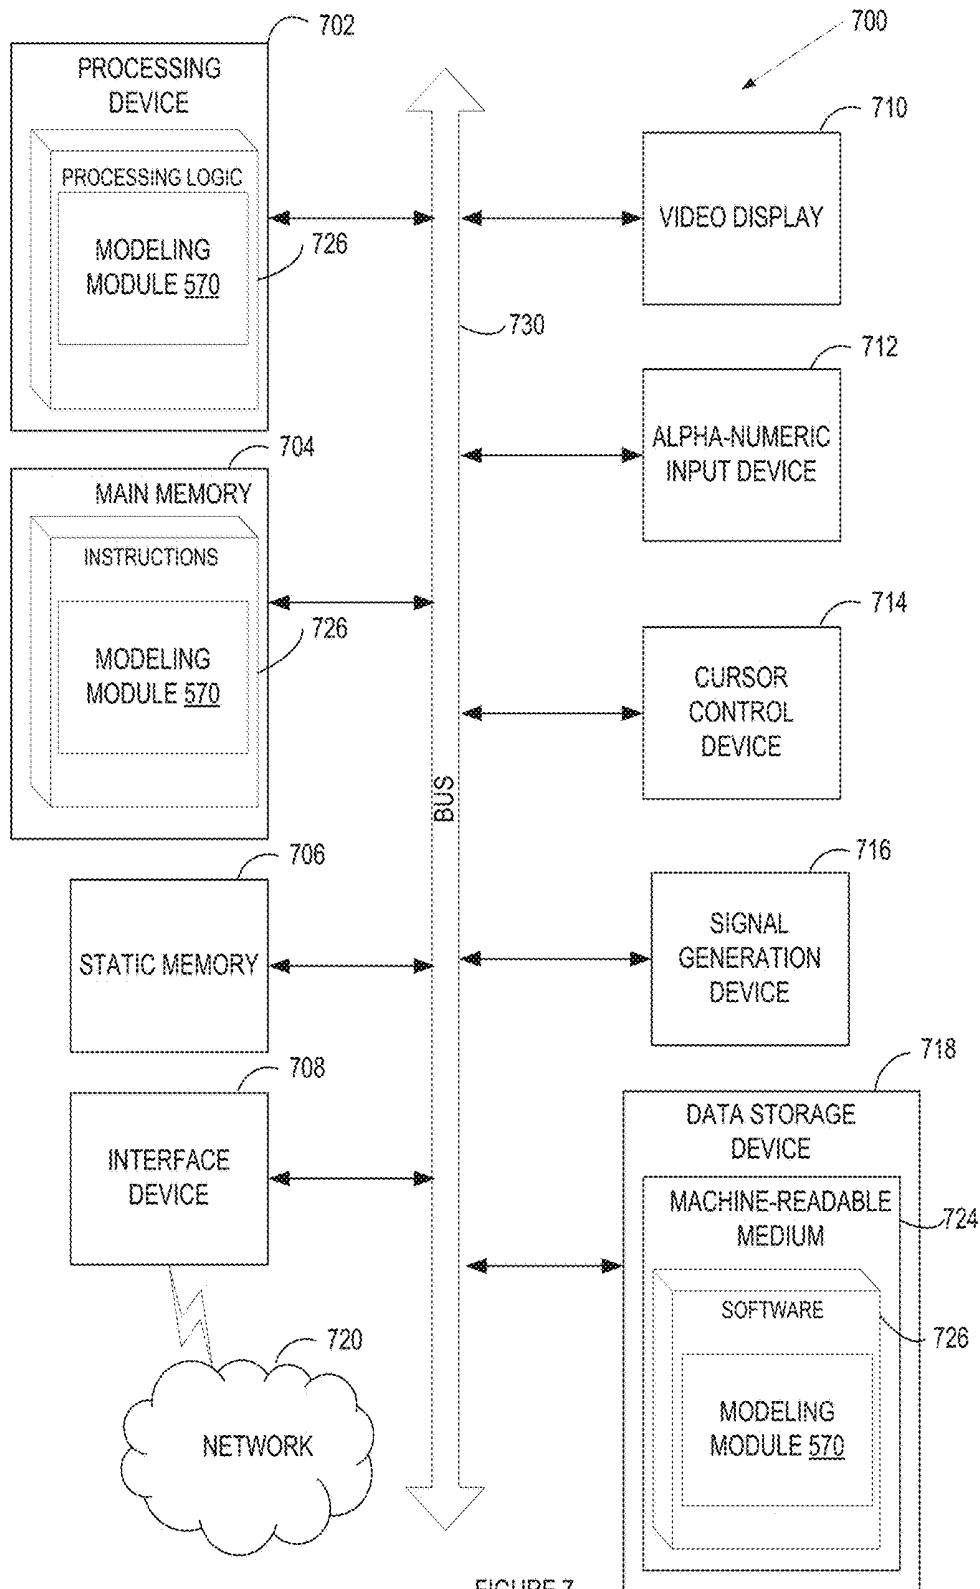


FIGURE 7

1

DIGITAL DENTAL TRAY

TECHNICAL FIELD

Embodiments of the present invention relate to the field of intraoral scanning and, in particular, to a system and method for using a digital dental tray for intraoral scanning.

BACKGROUND

In prosthodontic procedures designed to implant a dental prosthesis in the oral cavity, the dental site at which the prosthesis is to be implanted may be measured accurately and studied carefully, so that a prosthesis such as a crown, denture or bridge, for example, can be properly designed and dimensioned to fit in place. A good fit, for example, enables mechanical stresses to be properly transmitted between the prosthesis and the jaw and minimizes infection of the gums via the interface between the prosthesis and the dental site.

Some procedures call for removable prosthetics to be fabricated to replace one or more missing teeth, such as a partial or full denture, in which case the surface contours of the areas where the teeth are missing may be reproduced accurately so that the resulting prosthetic fits over the edentulous region with even pressure on the soft tissues.

In some practices, the dental site is prepared by a dental practitioner, and a positive physical model of the dental site is constructed. Alternatively, the dental site may be scanned or otherwise imaged to provide three-dimensional (3D) data of the dental site. In either case, the virtual or real model of the dental site may be sent to a dental lab that manufactures the prosthesis based on the model. However, if the model is deficient or undefined in certain areas, or if the preparation was not optimally configured for receiving the prosthesis, the design of the prosthesis may be less than optimal. For example, if the insertion path implied by the preparation for a closely-fitting coping would result in the prosthesis colliding with adjacent teeth, the coping geometry may need to be altered to avoid the collision. Further, if the area of the preparation containing a finish line lacks definition, it may not be possible to properly determine the finish line and thus the apical edge of the coping may not be properly designed. Indeed, in some circumstances, the model is rejected and the dental practitioner then re-images the dental site, or reworks the preparation, so that a suitable prosthesis may be produced.

In orthodontic procedures, it can be important to provide a model of one or both dental arches and/or a jaw of a patient. Where such orthodontic procedures are designed virtually, a virtual model of the oral cavity is also beneficial. Such a virtual model may be obtained by imaging the oral cavity directly, or by producing a physical model of the dentition, and then imaging the model with a suitable imaging device.

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention is illustrated by way of example, and not by way of limitation, in the figures of the accompanying drawings.

FIG. 1 illustrates one embodiment of a system for performing intraoral scanning using a dental tray with embedded imaging elements.

FIG. 2A illustrates one embodiment of an imaging element for generating images using a stereoscopic camera pair.

FIG. 2B illustrates one embodiment of an imaging element for generating images using a fixed focus camera.

2

FIG. 2C illustrates one embodiment of an imaging element for generating images using a structured light projector.

FIG. 3A illustrates a cross-sectional view of one embodiment of a dental tray.

FIG. 3B illustrates a side view of one embodiment of an imaging element arrangement for a dental tray.

FIG. 3C illustrates a cross-sectional view of another embodiment of a dental tray.

FIG. 4 illustrates a flow diagram for a method of generating a 3D model of teeth of a patient based on images captured by a dental tray, in accordance with embodiments of the present invention.

FIG. 5 illustrates a functional block diagram of an embodiment of a scanning and modeling system.

FIG. 6 illustrates a functional block diagram of another embodiment of a scanning and modeling system.

FIG. 7 illustrates a block diagram of an example computing device, in accordance with embodiments of the present invention.

DETAILED DESCRIPTION

Described herein is a method and apparatus for generating a three-dimensional (3D) model of a patient's teeth using a dental tray with 3D optical imaging elements (also referred to herein as a digital dental tray). In one embodiment, a dentist or other dental practitioner may generate a model of a patient's teeth by taking an impression of a dental site using an elastomeric impression material (e.g., as polyvinyl siloxanes (PVS) or polyethers (PE)) or an alginate impression material, placed in a conventional dental tray. The resulting impression may be used as a negative to generate a physical model that is scanned into a digital 3D model of the dental site. In another embodiment, a dental practitioner may use a wand-shaped intraoral scanner to capture the patient's dental topography by consecutively scanning the wand the patient's teeth. Both techniques for capturing a patient's dental topography may have drawbacks in some situations. The dental tray discussed in embodiments herein is capable of capturing a patient's dental topography without the potential drawbacks of the other discussed techniques.

In one embodiment, the dental practitioner uses a digital dental tray that does not use an impression material to create a model of a patient's teeth. The digital dental tray includes an array of 3D optical imaging elements with overlapping fields of view to capture the topography of a plurality of the patient's teeth, even all of the patient's teeth, at one time. By capturing images of all of the patient's teeth at one time, the amount of time needed to capture the topography of the dental site may be reduced. This may be convenient for both the practitioner and the patient, and may improve practitioner throughput. In particular, discomfort associated with long impression times using physical impression materials or wand-shaped scanners may be reduced. Further, such reduction in the capture time increases the accuracy and reliability of the capture. The reliability of the capture of dental site images in some embodiments may also be increased by the lack of moving parts of the dental tray and the fixed position of the 3D optical imaging elements with respect to each other.

FIG. 1 illustrates one embodiment of a system **100** for performing intraoral scanning (and potentially intraoral modelling) using a dental tray **110** (e.g., a digital dental tray) with embedded imaging elements **112A-112C**. The system **100** includes a dental tray **110** coupled by a communication link **120** to a computing device **101**. The dental tray **110**

includes an array of imaging elements **112A-112C** to generate images of one or more teeth of a patient that can be used to generate a 3D model of the patient's mouth (e.g., of a jaw and/or teeth of the patient).

The dental tray **110** is shaped to at least partially surround one or more teeth of the patient. In particular, the dental tray **110** includes an internal surface **106** that defines a tray cavity into which the patient's teeth are positioned. In one embodiment, the dental tray **110** may be shaped (as illustrated in FIG. 1) to at least partially surround both the upper teeth and the lower teeth of the patient. This may enable the imaging elements **112A-112C** of the dental tray **110** to create images usable to create a full mouth model of a patient dental site, including jaw, teeth, bite information, and so on. In another embodiment, the dental tray **110** may be shaped to at least partially surround only the upper teeth or only the lower teeth at any one time. In such an embodiment, the system **100** may be used to successively model the upper teeth in the maxilla (upper jaw) and then the lower teeth in the mandible (lower jaw) by first placing the dental tray **110** over the upper teeth and generating a first set of images and then placing the dental tray **110** over the lower teeth and generating a second set of images. In another embodiment, the dental tray **110** may be shaped to surround a quadrant portion of the patient's teeth or any or section including two or more teeth. In such an embodiment, the dental tray **110** may be positioned at a first location on an upper or lower jaw to take a first set of images, repositioned to a second location on the upper or lower jaw to take a second set of images, and so on until all desired portions of the patient's upper and/or lower jaw (and associated teeth) have been imaged.

The dental tray **110** includes an array of imaging elements **112A-112C** to generate images of the teeth of the patient, and in some instances to generate images of the jaw to which the teeth are attached. The imaging elements **112A-112C** may be three-dimensional (3D) optical imaging elements that generate images (e.g., 3D images) that may be used to generate a 3D model of the teeth of the patient. The imaging elements **112A-112C** may be embedded in the dental tray **110** or otherwise attached to the dental tray **110**, each positioned to have a field of view of a portion of one or more teeth, facing the one or more teeth when the dental tray is positioned in a patient's mouth over the patient's teeth. As described in detail below, the imaging elements **112A-112C** may be spaced and positioned such that each imaging element **112A-112C** generates images of at least a portion of one or more first teeth in a field of view of the imaging element **112A-112C** that overlaps with at least a portion of one or more second teeth in a field of view of another imaging element **112A-112C**. Although three imaging elements **112A-112C** are labelled in FIG. 1, it is to be appreciated that the dental tray **110** may include any number of imaging elements **112A-112C**.

Each imaging element **112A-112C** may generate images of the subset of the teeth in the field of view of the imaging element **112A-112C**. Each imaging element **112A-112C** may include one or more cameras and/or one or more illumination devices. In one embodiment, each imaging element **112A-112C** includes a stereoscopic camera pair and an illumination device and generates a pair of images from slightly different angles. The pair of images may be used to generate a 3D model or image of the section of teeth where the fields of view of the pair of images overlap. Such an embodiment is described more fully with reference to FIG. 2A. In another embodiment, each imaging element **112A-112C** includes a fixed focus camera and an illumination device and a 3D model may be generated using depth from

defocus principles. Such an embodiment is described more fully with reference to FIG. 2B. In another embodiment, each imaging element **112A-112C** includes a camera and a structured light projector and may be used to generate a 3D model using triangulation principles and/or a comparison of a known pattern of the structured light versus a captured pattern of the structured light as reflected off of the teeth of the patient. Such an embodiment is described more fully with reference to FIG. 2C.

The dental tray **110** (and the various components thereof, such as the imaging elements **112A-112C** or their subparts) may be connected to computing device **101** via a communications link **120**. The communications link **120** may be a wired link between the dental tray **110** and the computing device **101**, as shown. Alternatively, the communications link **120** may be a wireless connection that is established between the dental tray and computing device **101** via a wireless module (not shown) of the dental tray. The communications link **120** may allow for the transmission of a large amount of data generated by each scan. In one embodiment, approximately 50 stereo camera pairs, each capturing 4 frames, generates approximately 400 color frames that may be transmitted over the communications link **120**. Alternatively, up to approximately 50 or more fixed focus cameras or traditional cameras may each capture around 4 frames in an embodiment, resulting in approximately 200 frames that are transmitted. The communications link **120** may be a two-way communications link that allows communication from the dental tray **110** to the computing device **101** and from the computing device **101** to the dental tray **110**. The computing device **101** may provide control or instructions to the dental tray **110** via the communications link **120** and receive feedback or image data from the dental tray **110** via the communications link **120**.

The computing device **101** may include a processing device **161** for controlling the dental tray **110** and/or for processing data received from the dental tray **110**. The computing device **101** may additionally include a memory **162** to store received data, such as image data, and a power source **163** for providing power to the dental tray **110**. Alternatively, the dental tray may include its own power source, such as a rechargeable battery. For example, the dental tray **110** may include a standard or rechargeable battery if it does not have a wired link to computing device **101**. The computing device **101** may also include other components, such as those described below with respect to FIG. 7.

In one embodiment, the dental tray **110** is shaped to at least partially surround a subset of patient teeth such that the teeth are confined in a relatively enclosed volume. The teeth may therefore be isolated from the humid environment of the intraoral cavity by the dental tray **110** such that fog does not form on the internal surface **106** of the dental tray **110**. Alternatively, the dental tray **110** may not isolate the teeth from the humid environment of the intraoral cavity. Accordingly, the imaging elements **112A-112C** may have a tendency to fog over time in some embodiments. However, the dental tray **110** may further include a thermal sensor **131** configured to sense an environment (e.g., temperature) of the dental tray **110**. The thermal sensor **131** may communicate the sensed temperature via the communications link **120** to the computing device **101**. The computing device **101** (or the processing device **161** thereof) may control the temperature of the environment of the dental tray **110** based on the sensed temperature to defog the dental tray **110**, preventing the generation of fog on the dental tray **110** or removing fog that is present. Alternatively, dental tray **110**

may include a controller (not shown), which may receive the temperature measurements and determine settings for the imaging elements 112A-112C and/or heating elements therefrom. The controller may then adjust the settings of the imaging elements 112A-112C and/or heating elements to prevent the generation of fog and/or remove accumulated fog. The controller may be a programmable logic control, system on a chip (SoC), field programmable gate array, microprocessor, and/or other processing device. The processing device 161 or controller may control the temperature by controlling one or more illumination device of the imaging elements 112A-112C or any another heating element (also referred to as a heat generator) that generates heat in the environment of the dental tray 110. In one embodiment, where each camera pair has its own LED light illumination unit that consumes approximately 0.25 watts, the total power dissipation, assuming all cameras work in parallel, may be 54 times this, or approximately 13.5 watts. Some of this generated heat may be used to defog the dental tray 110. In one embodiment, the processing device 161 or controller controls the temperature by preheating the dental tray 110 to approximately body temperature prior to insertion of the dental tray into the mouth of the patient.

The dental tray 110 may have one or a plurality of channels 141A-141B through the dental tray 110 between the internal surface 106 of the dental tray and a vacuum port 142 of the external surface 108. The channels 141A-141B may be continuous spaces defined by a tubular inner surface connecting the internal surface 106 and the vacuum port 142 of the external surface 108. A disposable and transparent contamination control film (not shown) may be disposed over the internal surface 106 of the dental tray 110 prior to insertion of the dental tray into the mouth of the patient. The film may be shaped to cover the dental tray 110 or just a portion of the dental tray 110 and prevent contamination of the dental tray 110 (or a portion thereof) by exposure of the dental tray to the intraoral cavity of the patient.

The contamination control film may be thin and optically clear such that the film does not impact the imaging quality or geometry of images captured by the imaging elements 112A-112C. The film may be composed of polyvinyl chloride, polyethylene, or any other transparent material. A vacuum machine may be coupled to the vacuum port 142 to remove air from the channels 141A-141B and adhere the film to the internal surface 106 of the dental tray. In one embodiment, a tube connected to a vacuum machine is coupled to the vacuum port 142 to create a slight vacuum. The vacuum should be strong enough to cause the film to adhere to the dental tray 110, but not strong enough to deform the film or to generate holes, tears or rips in the film. The film may alternatively be adhered to the internal surface 106 by surface tension, static electricity, or any other method. Once imaging of a dental site is complete, the film may be removed and disposed of.

In one embodiment, the dental tray 110 is composed of a translucent or opaque material that can withstand disinfecting autoclave temperatures. In one embodiment, the dental tray has a rigid or semi-rigid body that may include metal and/or plastic. The imaging elements and other components may be attached to or integrated into this body. The body may be cast into (encapsulated in) a translucent material, such as polypropylene or another plastic, that can withstand disinfecting autoclave temperatures. The imaging elements 112A-112B and other components may be embedded within the dental tray 110, and may also be constructed to withstand autoclave temperatures. The dental tray 110 and its compo-

nents may be composed of autoclavable materials that are not damaged or deformed by temperatures between approximately 100° C. and 150° C.

FIG. 2A illustrates one embodiment of an imaging element 220 for generating images using a stereoscopic camera pair 222. The imaging element 221 may be one of the array of imaging elements 112A-112C of the dental tray 110 of FIG. 1. The imaging element 220 includes an illumination device 221 and a stereoscopic camera pair 222. Stereoscopic camera pairs may be advantageously allow multiple cameras in the tight space of the oral cavity given the constraints of stereo viewing angle (distance between the cameras relative to the distance to the object) and address the challenge of resolving details of the object.

The stereoscopic camera pair 222 includes a first camera 223A and a second camera 223B, each camera 223A-223B configured to generate an image of a section of the portion of the teeth at slightly different angles. In one embodiment, the stereoscopic camera pair 222 may be a Naneye stereo camera set produced by AWAIBA of Maderia, Portugal.

The images generated by each stereoscopic camera pair may be used to generate a 3D image of the section of the portion of the teeth where the fields of view of the cameras overlap. Each of the two cameras 223A-223B captures an image of the same scene, but the cameras 223A-223B are separated by a known distance. The computing device 101 may compare the images to determine parts of the image that match, but are shifted between the images. The shifted amount is called the disparity and the disparity at which objects in the image best match is used by the computing device 101, along with the known separation distance of the cameras 223A-223B, to calculate the distance of the objects from the camera pair 222. The distance information may be used to generate 3D images from 2D images, and ultimately to generate a 3D model that includes the portion of teeth in the field of view of the camera pair 222. Because multiple camera pairs 222 are in fixed relative position to each other on the dental tray, the distance information may be used to stitch together 2D images from the two cameras in the camera pair to form a full 3D image of the patient's dentition with minimum computational complexity.

The illumination device 221 may include one or more light emitting devices. The illumination device 221 may include at least one of a light emitting device placed between the cameras 223A-223B of each camera pair 222 or beside the camera pair 222. The light emitting devices may include one or more of light emitting diodes (LEDs), optical fibers connected to a light source, incandescent filaments, or any other light producing element. The illumination device 221 may be positioned to illuminate a portion of teeth of patient in a field of view of the imaging element 220. In one embodiment, the imaging element 220 does not include an illumination device 221. However, an illumination device may be included in a dental tray separate from the imaging element 220. The illumination device 221 may provide uniform, random, or structured illumination. The illumination device 221 may include one or more of a white light source or a monochrome light source of one or more possible wavelengths or colors. The illumination devices 221 for different imaging elements 220 may be of different wavelengths to distinguish between different imaging elements 220.

FIG. 2B illustrates one embodiment of an imaging element 230 for generating images using a fixed focus camera 232. The imaging element 230 may be one of the array of imaging elements 112A-112C of the dental tray 110 of FIG.

1. The imaging element **230** includes an illumination device **231** and a fixed focus camera **232**.

Like the illumination device **221** of the imaging element **220** of FIG. 2A, the illumination device **231** may include one or more light emitting devices and may be positioned to illuminate a portion of teeth of the patient in a field of view of the imaging element **230**. In one embodiment, the imaging element **230** does not include an illumination device **231**. In one embodiment, the illumination device **231** projects an illumination pattern onto the portion of the jaw such that weakly textured objects may be accurately modelled. The local blurring of the projected pattern as captured by the fixed focus camera **232** at each point may be used to determine the topography of the dental site.

The fixed focus camera **232** may be a camera with a focal length that is fixed throughout the image and, thus, a focus level that varies through the depth of interest. The fixed focus camera **232** may be configured to generate an image with embedded focus/defocus information that may be used to generate a 3D model of the portion of teeth in the field of view of the imaging element **230**.

The computing device **101** may quantify the blur or defocus of the image at various points and determine the distance of an object at the point from the fixed focus camera **232** using the following formula:

$$\psi = \frac{2\pi}{\lambda} \left(\frac{1}{z_o^f} - \frac{1}{z_o'} \right) r^2,$$

where λ is the wavelength of light, and z_o^f and z_o' are the in-focus and actual object distances from the fixed focus camera **232**, respectively, and r is a measure of the aperture of the fixed focus camera **232**.

In one embodiment, the fixed focus camera **232** takes multiple images at various focal lengths and the computing device **101** determines, for each of variety of points, the corresponding focal length at which the point is in focus. The distance of the object at the various points from the fixed focus camera **232** may be used as topography information to generate a 3D image of the portion of teeth in the field of view of the fixed focus camera **232**. These 3D images generated from images taken by the fixed focus cameras may then be combined to create a 3D model of a patient's dentition. Because multiple cameras **232** may be in fixed relative position to each other on the dental tray, the distance information and known angles between cameras may be used to stitch together 3D images generated from the images captured by the fixed focus camera to form a full 3D model of the patient's dentition.

FIG. 2C illustrates one embodiment of an imaging element **240** for generating images using a structured light projector **243**. The imaging element **240** may be one of the array of imaging elements **112A-112C** of the dental tray **110** of FIG. 1. The imaging element **240** includes an illumination device **241** and a camera **242**.

Like the illumination device **221** of the imaging element **220** of FIG. 2A, the illumination device **241** may include one or more light emitting devices and may be positioned to illuminate a portion of teeth of patient in a field of view of the imaging element **240**. The illumination device **241** includes a structured light projector **243** that projects a light pattern, such as a set of parallel lines, a grid, a pattern of dots, or any other known pattern, onto the portion of teeth in the field of view of the imaging element **240**.

The camera **242** may be any camera that generates an image within a field of view. The camera **242** may be configured to generate an image of the portion of the teeth with the light pattern of the structure light projector **243** projected upon it. The image may be used to generate a 3D model of the portion of teeth in the field of view of the imaging element **240** using triangulation principles.

The computing device **101** may generate a 3D model of the portion of teeth in the field of view of the imaging element **240** by analyzing the deformation of the light pattern caused when striking surfaces to calculate the depth and surface information of the objects in the scene. For example, the intersections of a grid pattern may be spread out upon reflection from an object convexly shaped, protruding towards the camera **242** or bunched together upon reflection from an object concavely shaped, protruding away from the camera **242**. Thus, the displacement of the intersections of a grid pattern upon reflection from an object may be used to determine the topology of the object or the distance of various points of the object to the camera **242**. Each captured image may be a 2D image. However, the differences between the structured light pattern as captured in the captured image and the known original structured light pattern are usable to convert the 2D image into a 3D image. The 3D images from multiple cameras may then be stitched together based on known offsets and angles between the cameras to form a 3D model of a jaw and/or teeth of a patient.

In one embodiment, the structured light projector **243** projects a first light pattern onto the portion of the teeth and, subsequently, a second light pattern onto the portion of the teeth. The structured light projector **243** may include two structured light projectors, one for each light pattern, or may include a single structured light projector that projects different patterns. In particular, the first light pattern and the second light pattern may be different. For example, in one embodiment, the second light pattern is a shifted version of the first light pattern. In another embodiment, the first light pattern is a first grid having a first grid spacing and the second light pattern is a second grid having a second grid spacing that is different (e.g., larger or smaller) than the first grid spacing. By dynamically changing the phase or frequency of the pattern using sequence two different structured light projectors, ambiguities in the structural reconstruction can be resolved. Thus, a first image of a tooth captured with a first structured light pattern may be combined with a second image of the tooth captured with a second structured light pattern to improve the quality and resolution of a 3D image generated from the 2D images.

FIG. 3A illustrates a cross-sectional view of one embodiment of a dental tray **310**. The dental tray **310** includes, along a cross-section, three imaging elements **312A-312C** embedded in the dental tray **310** and positioned to at least partially surround a tooth **301**. The three imaging elements **312A-312C** are encapsulated in a body **390**, which may be a translucent material, such as polypropylene or another plastic, that can withstand disinfecting autoclave temperatures, and are positioned such that a first imaging element **312A** has a field of view that includes a front of the tooth **301**, a second imaging element **312B** has a field of view that includes a bottom of the tooth **301**, and a third imaging element **312C** that includes a back of the tooth **301**. The three imaging elements **312A-312C** have overlapping fields of view such that the field of view of the first imaging element **312A** overlaps with the field of view of the second imaging element **312B** and the field of view of the second imaging element **312B** overlaps with the field of view of the

third imaging element **312C**. The three imaging elements **312A-312C** may be arranged such that their fields of view, together, include substantially all of the exposed portion of the tooth **301** (e.g., that is above the gum line).

FIG. **3B** illustrates a side view of one embodiment of an imaging element arrangement. The imaging elements **352A-352B** (illustrated as stereoscopic camera pairs) are positioned to align with interproximal gaps between teeth **302A-302C**. In other embodiments, each of the imaging elements **352A-352B** may be aligned with a center of a tooth **302A-302C**.

The imaging elements may be arranged, as illustrated in FIGS. **3A-3B**, with sufficient overlap to cover the entire set of the patient's teeth corresponding to the tray segment size. Thus, the topography of all of the patient's teeth may be captured at once, using a single snapshot of all of the imaging elements at the same time. The positioning of the imaging elements may be tailored to correspond to the tooth geometry in the respective dental zones to reduce the number of imaging elements used in the dental tray. In particular, the spacing between imaging elements may be variable such that each tooth is captured by respective imaging elements.

FIG. **3C** illustrates a cross-sectional view of another embodiment of a dental tray **360**. The dental tray **360** includes, along a cross-section, three imaging elements **312A-312C** embedded in a body **392** and positioned to at least partially surround a tooth **301**. The imaging elements **312A-312C** may be strategically retained in space by a rigid body **392** of minimal size. The dental tray **360** may be encased in a transparent case **372** that surrounds the dental tray **360**. The case **372** may be disposable or autoclavable, saving the need to subject the imaging and illumination elements to the high autoclave temperatures. Whereas the case **372** may be transparent, the body **392** may be opaque with the exception of one or more windows **371** disposed between the imaging elements **312A-312C** and the tooth **301**.

FIG. **4** illustrates a flow diagram for a method **400** of generating a 3D model of teeth of a patient, in accordance with embodiments of the present invention. The method **400** may be at least partially performed by processing logic that may comprise hardware (e.g., circuitry, dedicated logic, programmable logic, microcode, etc.), software (such as instructions run on a processing device), firmware, or a combination thereof. In one implementation, the method **400** may be at least partially performed by the system **100** of FIG. **1**. For simplicity of explanation, the method **400** is depicted and described as a series of acts. However, acts in accordance with this disclosure can occur in various orders, concurrently, and/or with other acts not presented or described herein. Furthermore, not all illustrated acts may be required to implement the method **400** in accordance with the disclosed subject matter.

The method **400** begins at block **410** with the positioning of a dental tray, such as the dental tray **110** of FIG. **1**, inside the mouth of a patient. Adjusting to different mouth sizes may be accomplished by providing a set of dental trays, each as described above, but of a different size. Thus, positioning the dental tray inside the mouth of the patient may include selecting a dental tray of an appropriate size from a set of dental trays of different sizes. The set of dental trays may include two, three, or more dental trays of different sizes.

The dental tray may be positioned to at least partially surround one or more teeth of the patient. In one embodiment, the patient bites down upon the dental tray to fix the

position of the dental tray inside the patient's mouth while images are captured, as described below with respect to block **420**.

At block **415**, the temperature of the environment of the dental tray is sensed. The temperature may be sensed using one or more thermal sensors attached to the dental tray. At block **417**, the processing logic controls the temperature of the environment of the dental tray, based on the sensed temperature, to defog the dental tray, preventing the generation of fog on the dental tray or removing fog that is present. The processing logic that controls the temperature of the dental tray may be integral with the dental tray or communicatively coupled to the dental tray. The processing logic may control the temperature by adjusting the settings of the imaging elements (e.g., intensity of illumination devices thereof) and/or heating elements to prevent the generation of fog and/or remove accumulated fog. In one embodiment, processing logic includes an ambient environment thermal sensor to sense the temperature of an environment of the dental tray (e.g., a temperature of a patient's oral cavity) and one or more additional thermal sensors to detect temperatures of the dental tray at one or more regions of the dental tray. Processing logic may set a temperature threshold based on the detected ambient temperature, and may adjust settings of the imaging elements and/or heating elements to cause the temperature at the one or more regions to approximately match the ambient temperature. Alternatively, or additionally, processing logic may include a preset temperature threshold (e.g., 98.6 degrees F.), and may adjust settings of the imaging elements and/or heating elements to cause the regions of the dental tray to reach the threshold temperature even before the dental tray is inserted into a patient's mouth.

At block **420**, 3D optical imaging elements embedded or otherwise attached to the dental tray are used to capture images of at least a portion of the teeth of the patient. Because the dental tray may lack moving parts and be relatively static when the patient bites down on the tray, proper positioning may be achieved without use of a viewfinder. However, in one embodiment, one or more of the imaging elements may provide a real-time image to verify that the dental tray is well-seated before the imaging elements capture the images used to generate a 3D model. These images may be provided to a processing device for output to a display.

The 3D optical imaging elements may include imaging elements such as those described with respect to FIGS. **2A-2C** and/or in an arrangement as described in FIGS. **3A-3B**. In particular, the 3D optical imaging elements may include one or more light sources and/or one or more cameras. The 3D optical imaging elements may include one or more of a stereoscopic camera pair, a fixed focus camera, or a camera paired with a structured light projector.

The 3D optical imaging elements may be used to simultaneously capture images of various sections of the portion of teeth of the patient in a single snapshot, significantly reducing the amount of time used to generate enough data to model the teeth of the patient and reducing the possibility that the dental tray (and the 3D optical imaging elements thereof) may shift during capture. In one embodiment, each 3D optical imaging element or grouping of 3D optical imaging elements is used sequentially to capture an image of a section of the portion of teeth. The sequential triggering of the 3D optical imaging elements may be performed to reduce heat generation and/or the bandwidth used to transmit the images from the optical imaging elements to a computing device used to generate a 3D model of the teeth

of the patient as described below with respect to block 430. In one embodiment, sets of two or more 3D optical imaging elements are used sequentially, each of the elements of the set being used simultaneously.

At block 425, the processing logic generates multiple 3D images based on the captured images (which may be captured two dimensional (2D) images with additional information usable to generate 3D images from the 2D images). The processing logic may generate a 3D image, e.g., an image including depth and/or topographic information, in a number of ways. In one embodiment, the processing logic generates a respective 3D image from the captured image or images from each imaging element. In one embodiment, the processing logic receives two images from each camera in a stereoscopic camera pair and generates a 3D image from the two images. The 3D image may be generated, as described above, by determining parts of the images that match, but are shifted between the images. The shifted amount is called the disparity and the disparity at which objects in the image best match may be used by the processing logic to calculate distance information of the 3D image. In one embodiment, the processing logic receives an image from a fixed focus camera configured such that the image focus level varies through the depth of interest, but not enough to result in a blurred image. The processing logic may quantify the blurring at various points on the image and generate depth information for the section of the portion of teeth in the field of view of the fixed focus camera based on the blurring. The distance of the blurred object point relative to the known focused object distance may be determined from the blur information by analyzing the point spread function at the object point. In particular, the further an object is from the in-focus plane, the more blurred it appears. The processing logic may use the amount of blurring to determine distance information of the 3D image. In one embodiment, the processing logic receives an image with a structured light pattern projected onto an object. The processing logic may use the amount of distortion of the light pattern introduced by the object to determine distance information of the 3D image.

At block 430, the 3D images generated are used to generate a 3D model of at least the portion of the teeth of the patient. The 3D model may be generated by stitching the 3D images together to generate a complete 3D model of at least the portion of the teeth of the patient. The 3D images from different imaging elements using different imaging modalities may be combined together to generate a 3D model of at least the portion of the teeth of the patient. Stitching the 3D images together may be relatively straightforward given the relatively fixed positions of the 3D optical imaging elements with respect to each other. Each dental tray may be used in an initial calibration procedure in which stitching and other vision reconstruction parameters are derived by measuring a known 3D object using the dental tray.

FIG. 5 illustrates a functional block diagram of an embodiment of an intraoral scanning and modeling system 500. The intraoral scanning and modeling system 500 includes a computing device 501 that generates a 3D model 574 of a patient's teeth based on images 572 captured by 3D optical imaging elements 522 embedded in or otherwise attached to a dental tray 520.

The dental tray 520 may be shaped to at least partially surround a plurality of teeth of a patient. In particular, the dental tray 520 may include an internal surface that at least partially surrounds the plurality of teeth of the patient. The dental tray 520 may surround all of the teeth of the patient,

the upper or lower teeth of the patient, a quadrant of the teeth of the patient, or any other section of the teeth of the patient including two or more teeth.

The dental tray 520 has an array of three-dimensional (3D) optical imaging elements 522 embedded in or otherwise attached to the dental tray. The 3D optical imaging elements may each include an illumination device 554 configured to illuminate one or more of the plurality of teeth and a camera 552 configured to capture an image of the one or more of the plurality of teeth.

The camera 552 may be any image capturing device and may be configured to capture color images or black-and-white images. The camera 552 may be configured to capture optical information, including information outside the visible spectrum in the infrared and/or ultraviolet regions. The illumination device 554 may include one or more light emitting devices, which may include one or more of light emitting diodes (LEDs), optical fibers connected to a light source, incandescent filaments, or any other light producing element. The illumination device 554 may include one or more of a white light source covering at least the full visible spectrum range or a monochrome source. The illumination device 554 may, for example, include a red light source, a blue light source, and a green light source.

The array of 3D optical imaging elements 522 may be arranged such that a first one or more of the plurality of teeth to be imaged by a first 3D optical imaging element of the first plurality of 3D optical imaging elements at least partially overlaps with a second one or more of the plurality of teeth to be imaged by a second 3D optical imaging element of the first plurality of 3D optical imaging elements. The array of 3D optical imaging elements 522 may include two sets of 3D optical imaging elements, wherein the first set is configured to capture images of the upper teeth of the patient and the second set is configured to capture images of the lower teeth of the patient.

In one embodiment, the 3D optical imaging elements 522 include a structured light projection optical imaging element that includes, as an illumination device 554, a structured light projector configured to project a light pattern onto one or more of the plurality of teeth, and a camera 552. The structured light projection optical imaging element may include, as an illumination device 554, two structured light projectors, each configured to project a different light pattern onto the one or more of the plurality of teeth, or a single light projector configured to project two different light patterns onto the one or more of the plurality of teeth. The first light pattern may be a first grid having a first grid spacing and the second light pattern is a second grid having a second grid spacing that is different than the first grid spacing.

In one embodiment, the 3D optical imaging elements 522 include a stereoscopic optical imaging element that includes, as a camera 552, a stereoscopic pair of cameras configured to capture images of one or more of the plurality of teeth from slightly different angles, and an illumination device 554. In one embodiment, the 3D optical imaging elements 522 include a depth-from-defocus optical imaging element that includes, as a camera 552, a fixed focus camera with a fixed focal length and, thus, a focus level that varies through the depth of interest, and an illumination device 552.

The dental tray 520 may include a communication module 521 that transmits images captured by the imaging elements 522 to the computing device 501 via a communications link 590. The communication module 521 may also be configured to receive information, such as information to control the imaging elements 522, from the computing device 501 over the communications link 590.

In one embodiment, the communication module **521** is a wired communication module. The communication module **521** may be a network adapter, a universal serial bus (USB) module, a serial communication module, a parallel communication module, and so on. The communication module **521** may transmit the captured images over a wired communications link **590**.

In one embodiment, the communication module **521** is a wireless module that establishes a wireless communications link **590** with the computing device **501**. In one embodiment, the wireless module is configured to communicate using Bluetooth. Alternatively, the wireless module may be configured to communicate using Wi-Fi, Zigbee, Internet Protocol version 6 over Low power Wireless Area Networks (6LowPAN), power line communication (PLC), or other communication protocols. The wireless module may include a processing device, a memory and/or a network adapter. The processing device of the wireless module may be a microcontroller, a digital signal processor (DSP), a programmable logic controller (PLC), a microprocessor or programmable logic device such as a field programmable gate array (FPGA) or a complex programmable logic device (CPLD). The memory of the wireless module may include a non-volatile memory (e.g., RAM) and/or a volatile memory (e.g., ROM, Flash, etc.). In one embodiment, the memory is integrated into the processing device of the wireless module.

The dental tray **520** may be coupled to or include a thermal sensor **524** that senses a temperature of an environment of the dental tray **520**. The sensed temperature may be transmitted, using the communication module **521** via the communications link **590**, to the computing device **501**. The computing device **501**, or the processing device **561** thereof may control the temperature of the environment of the dental tray **520** based on the sensed temperature to defog the dental tray **520**, either preventing the formation of fog on the dental tray **520** or removing fog that is present. Alternatively, dental tray **520** may include a controller **527** that receives the temperature information and controls the temperature of the environment of the dental tray **527**. The controller **527** may be a microcontroller, a digital signal processor (DSP), a programmable logic controller (PLC), a microprocessor or programmable logic device such as a field programmable gate array (FPGA) or a complex programmable logic device (CPLD).

The computing device **501** or controller **527** may control the temperature of the environment of the dental tray **520** in a number of ways. In one embodiment, the computer device **501** or controller **527** controls one or more illumination devices **554** of the imaging elements **522** to generate heat to defog the dental tray **520**. In one embodiment, the computer device **501** or controller **527** controls one or more heat generators **525** (also referred to as heating elements) embedded in or otherwise attached to the dental tray to generate heat in the environment of the dental tray **520**.

The dental tray **520** may have one or more channels **526** through the dental tray between an internal surface of the dental tray **520** and a vacuum port of an external surface of the dental tray **520**. A disposable and optically clear contamination control film **532** may be disposed over the internal surface of the dental tray prior to insertion of the dental tray into the mouth of the patient for intraoral scanning. The film **532** may be a thin film (e.g., approximately 0.4-0.6 millimeters thick) composed of polyvinyl chloride, polyethylene, or any other material. A vacuum machine **534** may be coupled to the vacuum port to remove air from the channels **526** and adhere the film **532** to the internal surface of the dental tray.

In one embodiment, the dental tray **520** is composed of or encased in a translucent material that can withstand disinfecting autoclave temperatures and the imaging elements **522** and other components are embedded within the dental tray **520**. The dental tray **520** may be composed of or encased in an autoclavable material that is not damaged or deformed by temperatures between approximately 100° C. and 150° C. For example, the dental tray **520** may be composed of or encased in polypropylene or another translucent plastic.

The computing device **501** may include a processing device **561** that executes a modelling module **570**. The modelling module **570** may take, as input, images **572** received from the imaging elements **522** and generate a 3D model **574** of a dental site (e.g., of an upper and lower jaw and teeth) based on the received captured images **572**. The 3D model **574** may be based on color images and, therefore, be a color 3D model. The color 3D model may be used for display, interpretation, and tooth-shading purposes to ensure that prosthetics match the natural color of the patient's teeth.

The images **572** and the resulting 3D model **574** may be stored in a memory **574** of the computing device **501**. The computing device **501** may also include a power source **563** that provides power to the computing device and/or provides power (e.g., over the communications link **590** which may also act as a power link) to the components of the dental tray **520**, such as the imaging elements **522**. Alternatively, the dental tray **520** may include its own power source (not shown), which may be a rechargeable battery, or be connected to power source separate from the computing device **501**.

The images **572**, in addition to being used to generate the 3D model **574**, may be used for dental hygiene diagnosis. A dental practitioner may view the images **572** remotely from the patient to develop a dental hygiene treatment plan that may be incorporated into a comprehensive treatment plan. In one embodiment, computer software analyzes the images to generate a dental hygiene diagnosis, expanding the access of patients to treatment initializing diagnoses.

FIG. 6 illustrates a functional block diagram of an embodiment of an intraoral scanning and modeling system **600**. In response to a command triggering a capture sequence **601**, a control and processing unit **601** controls a capture unit **620** to perform a capture sequence and capture one or more images of a patient's mouth **602**. The control and processing unit **610** may correspond to and perform at least some of the functions of the computing device **501** of FIG. 5 and the capture unit **620** may correspond to and have at least some of the features of the dental tray **520** of FIG. 5. For example, the capture unit **620** may include or be a component of a dental tray, such as an imaging element **112A-112C** of dental tray **110** of FIG. 1. Alternatively, capture unit **620** may be a dental tray, such as dental tray **110** of FIG. 1.

The control and processing unit **610** may include an LED light control module **611** that controls one or more LED lights **621** of the capture unit **620** and may also include a main and camera control module **612** that controls one or more cameras **622** of the capture unit **620**. The control and processing unit **610** may include an image data module **613** that sends communications, such as image data, via a communications bus **615** to a 3D image processor **630**. The 3D image processor **630** may also correspond to and perform at least some of the functions of the computing system **501** of FIG. 5.

The 3D image processor **630** may receive data including multiple color images **631**. The 3D image processor **630**

may include a 3D processing algorithm module **632** that performs one or more 3D processing algorithms, such as those described above with respect to FIGS. 2A-2C, to generate object topography data **633** and object color data **634** from the multiple color images **631**. The object color data **634** may also be at least partially generated by a color separation module **635** that derives object color information from the received color images **631**.

The 3D image processor may include 3D geometry compensation data **636** derived from an initial calibration of the capture unit **620** as described above. The 3D geometry compensation data **636** may include, for example, stitching and other vision reconstruction parameters. The 3D geometry compensation data **636** may further include color compensation data that is used, along with the object color data **634** to perform a color rendering reconstruction by a color rendering reconstruction module **638**. The 3D geometry compensation data **636** may be used by a geometry compensation module **637** to perform geometry compensation that, among other things, may standardize the images based on the relative positions of the cameras **622** within the capture unit **620**.

The geometry compensation may be used, along with the object topography data **633** by a 3D reconstruction module **639** to perform 3D reconstruction. The color rendering reconstruction performed by the color rendering reconstruction module **638** may also be used to assist in the 3D reconstruction performed by the 3D reconstruction module **639**.

The result of the 3D reconstruction may be used by a 3D merge module **640** to perform a 3D merge and generate a 3D model of the patient's mouth **602**. The results of the 3D merge and the results of the color rendering reconstruction may be used by a display rendering module **641** to render a color display of the model of the patient's mouth **602**. The rendering may be fed to a display driver **642** of the 3D image processor **630** which drives a display **650** to present a user with a color display of the model of the patient's mouth **602**.

The 3D merge may result in a storable 3D object **643** that may be uploaded by a case upload module **645**, e.g., a network interface, to a case database **660**, where the 3D object **643** of the model of the patient's mouth **602** is stored in association with information about the patient.

FIG. 7 illustrates a block diagram of an example computing device, in accordance with embodiments of the present invention. In alternative implementations, the machine may be connected (e.g., networked) to other machines in a LAN, an intranet, an extranet, or the Internet. The machine may operate in the capacity of a server or a client device in a client-server network environment, or as a peer machine in a peer-to-peer (or distributed) network environment. The machine may be a personal computer (PC), a tablet PC, a set-top box (STB), a Personal Digital Assistant (PDA), a cellular telephone, a web appliance, a server, a network router, switch or bridge, or any machine capable of executing a set of instructions (sequential or otherwise) that specify actions to be taken by that machine. Further, while only a single machine is illustrated, the term "machine" shall also be taken to include any collection of machines that individually or jointly execute a set (or multiple sets) of instructions to perform any one or more of the methodologies discussed herein.

The computer system **700** includes a processing device **702**, a main memory **704** (e.g., read-only memory (ROM), flash memory, dynamic random access memory (DRAM) (such as synchronous DRAM (SDRAM) or DRAM (RDRAM), etc.), a static memory **706** (e.g., flash memory,

static random access memory (SRAM), etc.), and a data storage device **718**, which communicate with each other via a bus **730**.

Processing device **702** represents one or more general-purpose processing devices such as a microprocessor, central processing unit, or the like. More particularly, the processing device may be complex instruction set computing (CISC) microprocessor, reduced instruction set computer (RISC) microprocessor, very long instruction word (VLIW) microprocessor, or processor implementing other instruction sets, or processors implementing a combination of instruction sets. Processing device **702** may also be one or more special-purpose processing devices such as an application specific integrated circuit (ASIC), a field programmable gate array (FPGA), a digital signal processor (DSP), network processor, or the like. The processing device **702** may be configured to execute the processing logic **726** for performing the operations and steps discussed herein.

The computer system **700** may further include an interface device **708** (e.g., a network adapter, wireless module, etc.) communicably coupled to a network **720** and/or to a dental tray. The computer system **700** also may include a video display unit **710** (e.g., a liquid crystal display (LCD) or a cathode ray tube (CRT)), an alphanumeric input device **712** (e.g., a keyboard), a cursor control device **714** (e.g., a mouse), and a signal generation device **716** (e.g., a speaker).

The data storage device **718** may include a machine-accessible storage medium **724** on which may be stored software **726** embodying any one or more of the methodologies of functions described herein. The software **726** may also reside, completely or at least partially, within the main memory **704** as instructions **726** and/or within the processing device **702** as processing logic **726** during execution thereof by the computer system **700**; the main memory **704** and the processing device **702** also constituting machine-accessible storage media.

The machine-readable storage medium **724** may also be used to store instructions **726** to implement the modeling module **570** and/or any one or more of the methodologies of functions described herein in a computer system, such as the system described with respect to FIG. 1, and/or a software library containing methods that call the above applications.

While the machine-accessible storage medium **724** is shown in an example implementation to be a single medium, the term "machine-accessible storage medium" should be taken to include a single medium or multiple media (e.g., a centralized or distributed database, and/or associated caches and servers) that store the one or more sets of instructions. The term "machine-accessible storage medium" shall also be taken to include any medium that may be capable of storing, encoding or carrying a set of instruction for execution by the machine and that cause the machine to perform any one or more of the methodologies of the disclosure. The term "machine-accessible storage medium" shall accordingly be taken to include, but not be limited to, solid-state memories, and optical and magnetic media.

In the foregoing description, numerous details are set forth. It may be apparent, however, that the disclosure may be practiced without these specific details. In some instances, well-known structures and devices are shown in block diagram form, rather than in detail, in order to avoid obscuring the disclosure.

Some portions of the detailed descriptions which follow are presented in terms of algorithms and symbolic representations of operations on data bits within a computer memory. These algorithmic descriptions and representations are the means used by those skilled in the data processing

arts to most effectively convey the substance of their work to others skilled in the art. An algorithm is here, and generally, conceived to be a self-consistent sequence of steps leading to a desired result. The steps are those requiring physical manipulations of physical quantities. Usually, though not necessarily, these quantities take the form of electrical or magnetic signals capable of being stored, transferred, combined, compared, and otherwise manipulated. It has proven convenient at times, principally for reasons of common usage, to refer to these signals as bits, values, elements, symbols, characters, terms, numbers, or the like.

It should be borne in mind, however, that all of these and similar terms are to be associated with the appropriate physical quantities and are merely convenient labels applied to these quantities. Unless specifically stated otherwise, as apparent from the following discussion, it is appreciated that throughout the description, discussions utilizing terms such as “receiving”, “performing”, “creating”, “registering”, “applying”, “allocating”, “merging”, “using”, or the like, refer to the action and processes of a computer system, or similar electronic computing device, that manipulates and transforms data represented as physical (electronic) quantities within the computer system’s registers and memories into other data similarly represented as physical quantities within the computer system memories or registers or other such information storage, transmission or display devices.

The disclosure also relates to an apparatus for performing the operations herein. This apparatus may be specially constructed for the required purposes, or it may comprise a general purpose computer selectively activated or reconfigured by a computer program stored in the computer. Such a computer program may be stored in a machine readable storage medium, such as, but not limited to, any type of disk including floppy disks, optical disks, CD-ROMs, and magnetic-optical disks, read-only memories (ROMs), random access memories (RAMs), EPROMs, EEPROMs, magnetic or optical cards, or any type of media suitable for storing electronic instructions, each coupled to a computer system bus.

The algorithms and displays presented herein are not inherently related to any particular computer or other apparatus. Various general purpose systems may be used with programs in accordance with the teachings herein, or it may prove convenient to construct more specialized apparatus to perform the required method steps. The required structure for a variety of these systems may appear as set forth in the description below. In addition, the disclosure is not described with reference to any particular programming language. It may be appreciated that a variety of programming languages may be used to implement the teachings of the disclosure as described herein.

The disclosure may be provided as a computer program product, or software, that may include a machine-readable medium having stored thereon instructions, which may be used to program a computer system (or other electronic devices) to perform a process according to the disclosure. A machine-readable medium includes any mechanism for storing or transmitting information in a form readable by a machine (e.g., a computer). For example, a machine-readable (e.g., computer-readable) medium includes a machine (e.g., a computer) readable storage medium (e.g., read only memory (“ROM”), random access memory (“RAM”), magnetic disk storage media, optical storage media, flash memory devices, etc.), etc.

Whereas many alterations and modifications of the disclosure may no doubt become apparent to a person of ordinary skill in the art after having read the foregoing

description, it is to be understood that any particular example shown and described by way of illustration is in no way intended to be considered limiting. Therefore, references to details of various examples are not intended to limit the scope of the claims, which in themselves recite only those features regarded as the disclosure.

What is claimed is:

1. A system comprising:

a dental tray shaped to at least partially surround a plurality of teeth;

a first plurality of three-dimensional (3D) optical imaging elements attached to the dental tray, wherein each of the first plurality of 3D optical imaging elements comprises:

an illumination device to project light onto one or more teeth of the plurality of teeth; and

a camera to capture an image of the one or more teeth;

a first thermal sensor to detect a first temperature of the dental tray;

a second thermal sensor to detect a second temperature of an oral cavity; and

a controller to:

determine that the first temperature of the dental tray is lower than the second temperature of the oral cavity;

activate the illumination device for one or more of the first plurality of 3D optical imaging elements, and

adjust the first temperature of the dental tray to cause the first temperature of the dental tray to approximately match the second temperature of the oral cavity based on optical heating caused by the illumination device for the one or more of the first plurality of 3D optical imaging elements.

2. The system of claim 1, further comprising:

a wireless module to wirelessly transmit captured images to a computing device, wherein the computing device is to generate a 3D model of the plurality of teeth based on the captured images.

3. The system of claim 1, wherein a first one or more of the plurality of teeth to be imaged by a first 3D optical imaging element of the first plurality of 3D optical imaging elements at least partially overlaps with a second one or more of the plurality of teeth to be imaged by a second 3D optical imaging element of the first plurality of 3D optical imaging elements.

4. The system of claim 1, wherein the illumination device of a first 3D optical imaging element of the first plurality of 3D optical imaging elements comprises a first structured light projector that is to project a first light pattern onto one or more of the plurality of teeth and to project a second light pattern onto the one or more of the plurality of teeth.

5. The system of claim 1, wherein the dental tray has one or more channels through the dental tray between an internal surface of the dental tray and an external vacuum port, and wherein a vacuum is to couple to the external vacuum port to remove air from the one or more channels and adhere an optically clear contamination control film to the internal surface of the dental tray.

6. The system of claim 1, further comprising a second plurality of 3D optical imaging elements attached to the dental tray, each of the second plurality of 3D optical imaging elements comprising a structured light projector configured to project a light pattern onto one or more of the plurality of teeth and a camera configured to capture an image of the one or more of the plurality of teeth, wherein the first plurality of 3D optical imaging elements is configured to capture images of an upper section of the plurality of

19

teeth and the second plurality of 3D optical imaging elements is configured to capture images of a lower section of the plurality of teeth.

7. A system comprising:

- a dental tray shaped to at least partially surround a plurality of teeth;
- a first plurality of three-dimensional (3D) optical imaging elements attached to the dental tray, each of the first plurality of 3D optical imaging elements to capture an image of one or more of the plurality of teeth with a field of view that at least partially overlaps with a field of view of another of the first plurality of 3D optical imaging elements;
- a plurality of illumination devices to project light onto the plurality of teeth;
- a first thermal sensor to sense a temperature of the dental tray;
- a second thermal sensor to sense a temperature of an oral cavity; and
- a controller to adjust a setting of the plurality of illumination devices to use optical heating to control the temperature of the dental tray, cause the temperature of the dental tray to approximately match the temperature of the oral cavity and mitigate condensation on the dental tray.

8. The system of claim 7, wherein each of the plurality of illumination devices is a component of one of the first plurality of 3D optical imaging elements, wherein each of the plurality of illumination devices is a structured light projector to project a light pattern onto one or more teeth of the plurality of teeth, and wherein each of the plurality of 3D optical imaging elements further comprises a camera to capture an image of the one or more teeth.

9. The system of claim 7, wherein a first 3D optical imaging element of the first plurality of 3D optical imaging elements comprises at least one of a stereoscopic camera pair or a fixed focus camera.

10. The system of claim 7, wherein a first camera of a first 3D optical imaging element of the first plurality of 3D optical imaging elements is to capture a color image.

11. The system of claim 7, further comprising a transmitter to transmit the captured images to a computing device, wherein the computing device is to generate a 3D model of the plurality of teeth based on the captured images.

12. A system comprising:

- a dental tray shaped to at least partially surround a plurality of teeth; and

20

a first plurality of three-dimensional (3D) optical imaging elements attached to the dental tray, each of the first plurality of 3D optical imaging elements to capture an image of one or more of the plurality of teeth with a field of view that at least partially overlaps with a field of view of another of the first plurality of 3D optical imaging elements,

wherein the dental tray comprises a plurality of channels through the dental tray between an internal surface of the dental tray and an external vacuum port, wherein the plurality of channels are to apply, at a plurality of locations on the internal surface of the dental tray, a vacuum having sufficient suction to secure an optically clear disposable contamination control film to the internal surface of the dental tray without tearing the optically clear disposable contamination control film, wherein the optically clear disposable contamination control film does not impact imaging quality or geometry of images generated by the first plurality of 3D optical imaging elements.

13. The system of claim 12, further comprising the optically clear contamination control film disposed over the internal surface of the dental tray, wherein the optically clear disposable contamination control film has a thickness of 0.4-0.6 mm.

14. The system of claim 13, wherein the optically clear disposable contamination control film comprises at least one of polyvinyl chloride or polyethylene.

15. The system of claim 13, further comprising a vacuum machine coupled to the external vacuum port to remove air from the one or more channels to cause the vacuum and adhere the optically clear disposable contamination control film to the internal surface of the dental tray.

16. The system of claim 12, wherein the dental tray comprises an autoclavable translucent material.

17. The system of claim 15, wherein the dental tray further comprises:

- a thermal sensor to sense a temperature of an environment of the dental tray; and
- a controller to control the temperature of the environment of the dental tray based on the sensed temperature to defog the dental tray.

18. The system of claim 1, wherein the controller is further to adjust an intensity of the illumination device for the one or more of the plurality of 3D optical imaging elements, wherein an adjustment of the intensity causes an adjustment in the optical heating.

* * * * *

专利名称(译)	数字牙科托盘		
公开(公告)号	US9844426	公开(公告)日	2017-12-19
申请号	US14/656523	申请日	2015-03-12
[标]申请(专利权)人(译)	阿莱恩技术有限公司		
申请(专利权)人(译)	ALIGN科技股份有限公司.		
当前申请(专利权)人(译)	ALIGN科技股份有限公司.		
[标]发明人	ATIYA YOSSI KOPELMAN AVI LAMPERT EREZ		
发明人	ATIYA, YOSSI KOPELMAN, AVI LAMPERT, EREZ		
IPC分类号	A61B1/00 A61B1/24 A61C9/00 A61B1/253 A61B5/00 A61B1/12 A61B5/107 A61B1/04 A61B1/015 A61B1/06 A61B5/01		
CPC分类号	A61C9/006 A61B1/00016 A61B1/00142 A61B1/00181 A61B1/00193 A61B1/015 A61B1/04 A61B1/06 A61B1/0684 A61B1/126 A61B1/128 A61B1/24 A61B1/253 A61B5/0088 A61B5/1077 A61B5/1079 A61B5/4547 A61C9/0006 A61B1/00009 A61C2204/002 A61B5/01 A61B2560/0242 A61B2562/043		
其他公开文献	US20160262856A1		
外部链接	Espacenet USPTO		

摘要(译)

描述了一种数字牙科托盘系统，包括成形为至少部分地围绕多个牙齿的牙托和附接到牙托的多个三维（3D）光学成像元件。每个3D光学成像元件包括结构光投影仪，用于将光图案投射到多个牙齿的一个或多个牙齿上，以及相机，以捕获一个或多个牙齿的图像。

(Continued)

18 Claims, 8 Drawing Sn

