



US 20140371618A1

(19) **United States**(12) **Patent Application Publication**
Steinhauer et al.(10) **Pub. No.: US 2014/0371618 A1**(43) **Pub. Date: Dec. 18, 2014**(54) **ANALYTICS REGARDING VENTILATED PATIENTS***A61B 5/091* (2006.01)*A61B 5/00* (2006.01)*A61M 5/172* (2006.01)(71) Applicant: **CareFusion 303, Inc.**, San Diego, CA (US)(52) **U.S. Cl.**CPC *A61M 16/0051* (2013.01); *A61B 5/4833*(2013.01); *A61M 5/172* (2013.01); *A61B**5/0816* (2013.01); *A61B 5/082* (2013.01);*A61B 5/091* (2013.01); *A61B 5/0871*(2013.01); *A61B 5/4848* (2013.01)USPC **600/532**; 600/300; 128/202.22; 600/529;


600/538

(72) Inventors: **Tom Steinhauer**, San Diego, CA (US);
Terry Lee Blansfield, Orange, CA (US);
Leonard Mulkowsky, Del Mar, CA (US);
Andres Jesus Calderon, III, San Diego, CA (US)(73) Assignee: **CareFusion 303, Inc.**, San Diego, CA (US)

(57)

ABSTRACT

A method, system and computer-readable medium are provided for determining compliance with one or more patient care rules and protocols, the method including the steps of sending infusion information from a pump to a processor pertaining to one or more drugs provided to a patient, sending ventilation information from a ventilator to the processor pertaining to ventilation provided to the patient and determining, with the processor, a variation between actual care of the patient and a set of rules and protocols associated with care of the patient at least in part based on the infusion information and the ventilation information.

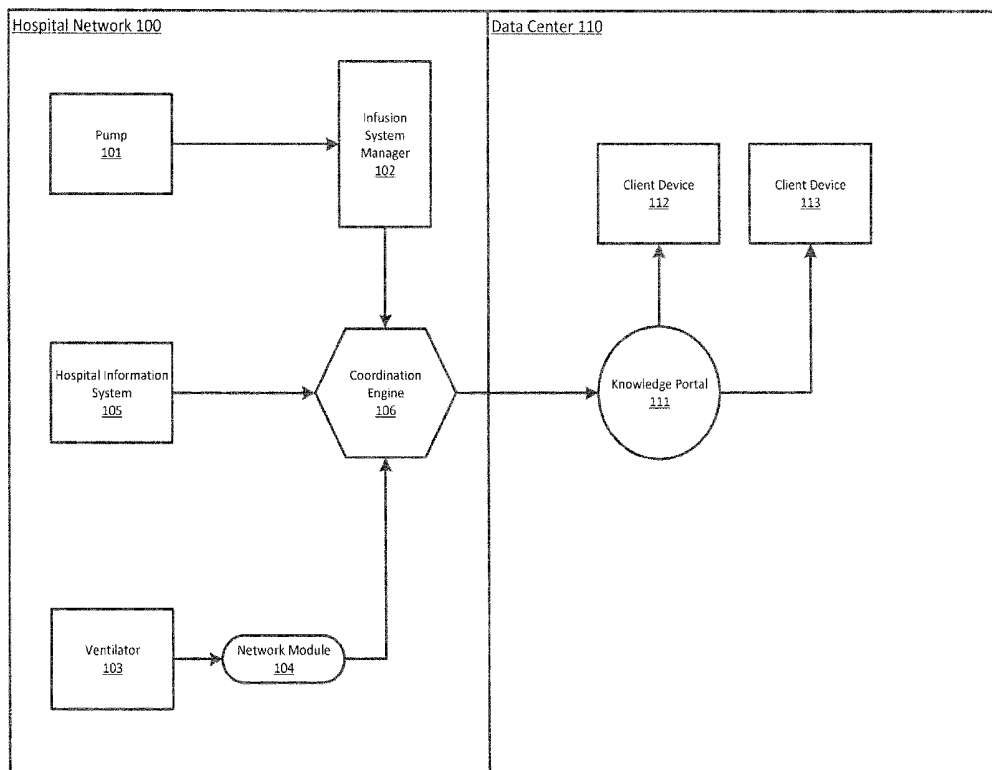(21) Appl. No.: **13/917,614**(22) Filed: **Jun. 13, 2013****Publication Classification**(51) **Int. Cl.***A61M 16/00* (2006.01)*A61B 5/087* (2006.01)*A61B 5/08* (2006.01)

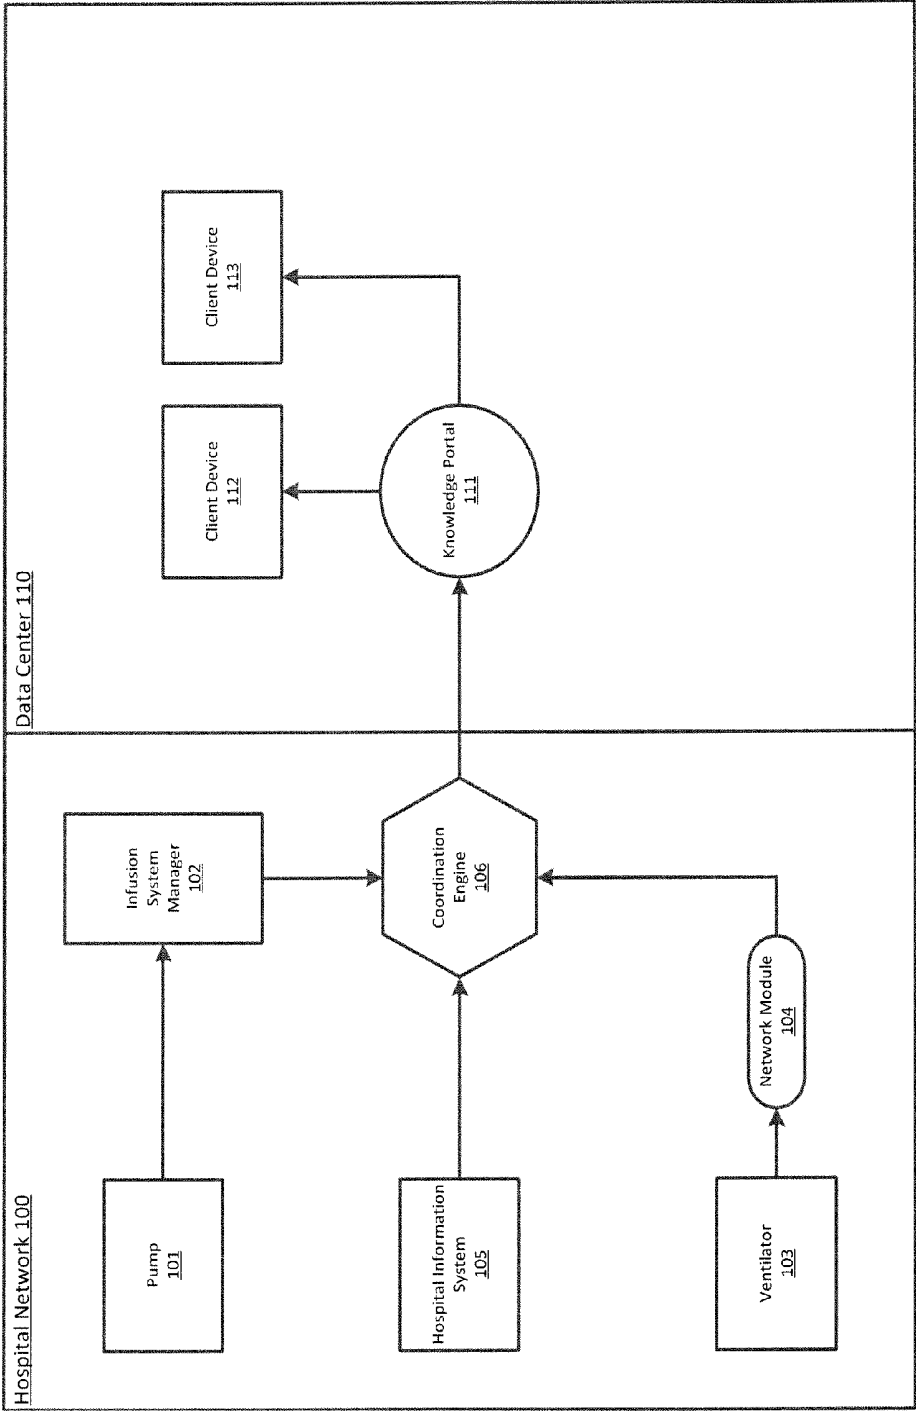


FIG. 1A

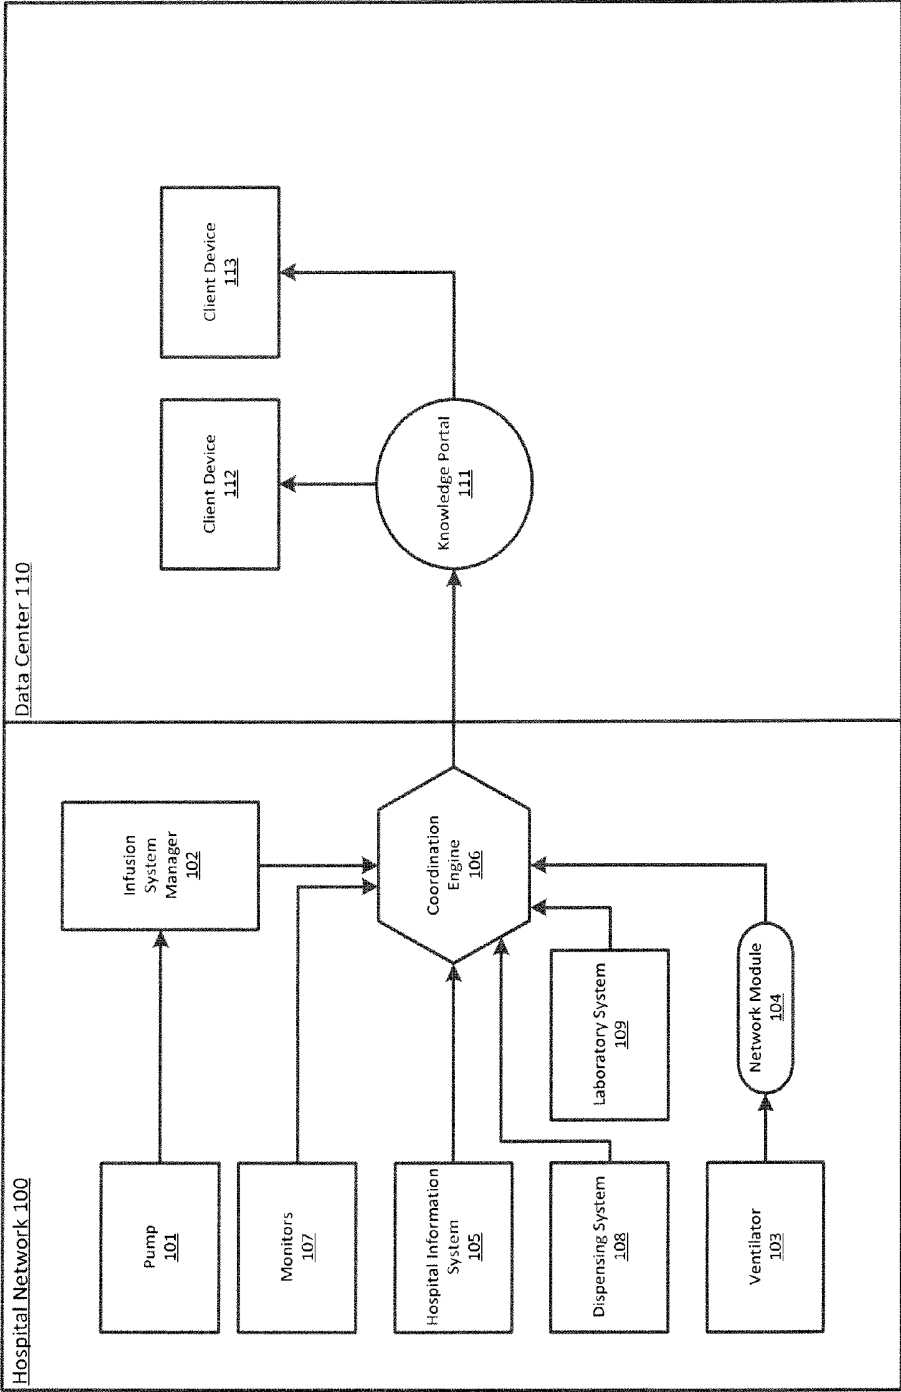


FIG. 1B

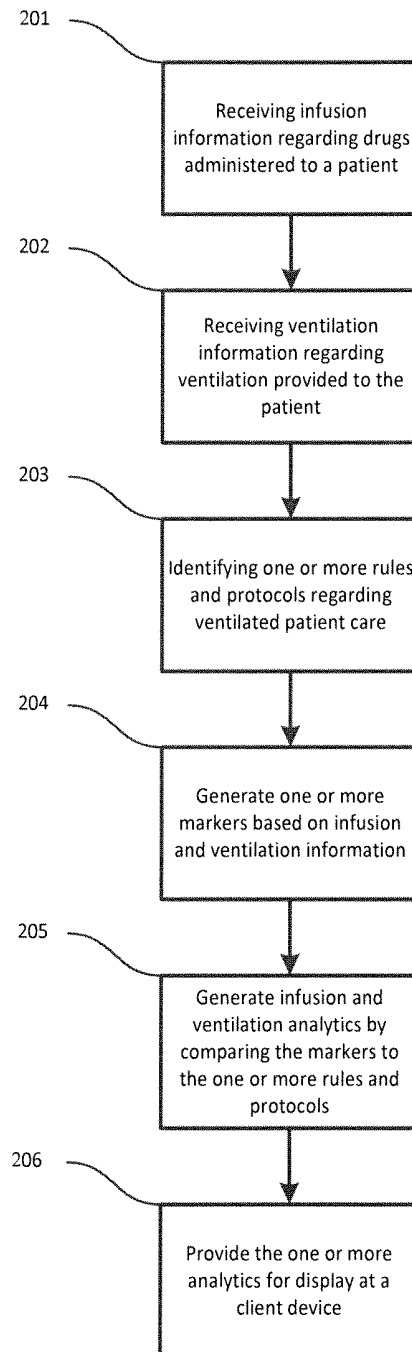


FIG. 2

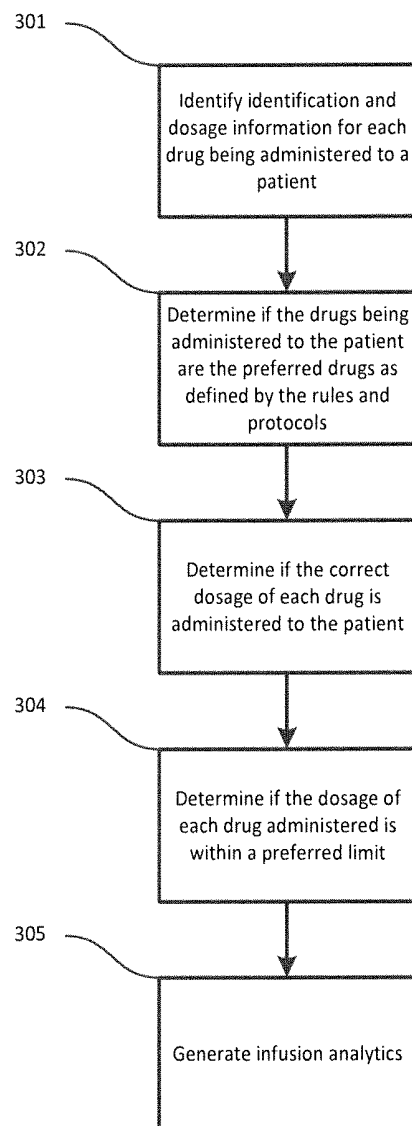


FIG. 3

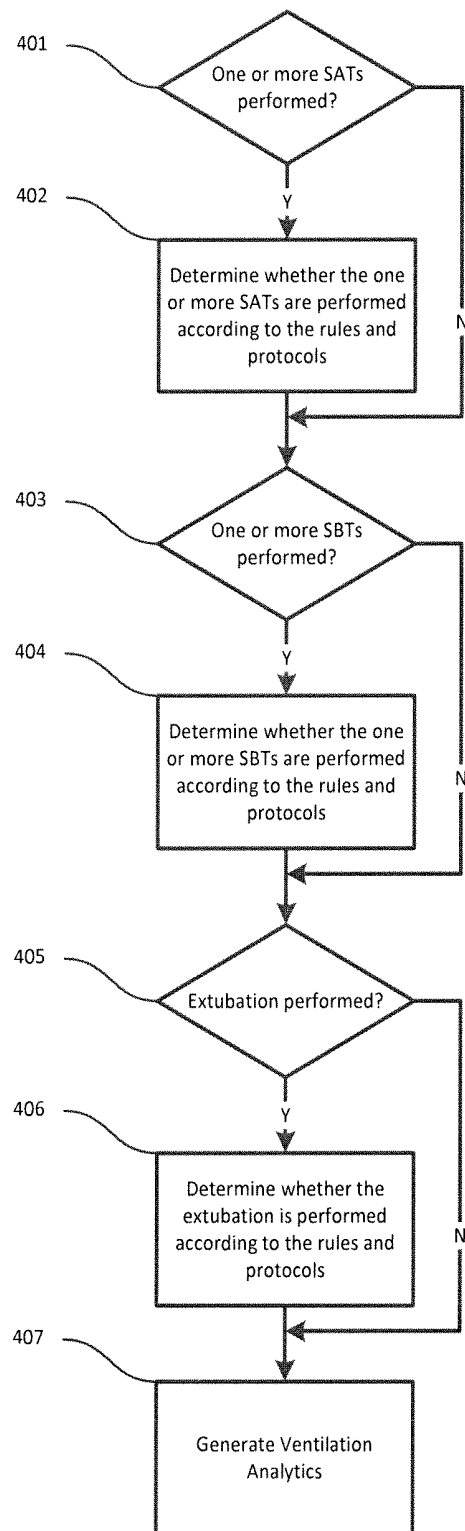


FIG. 4

500

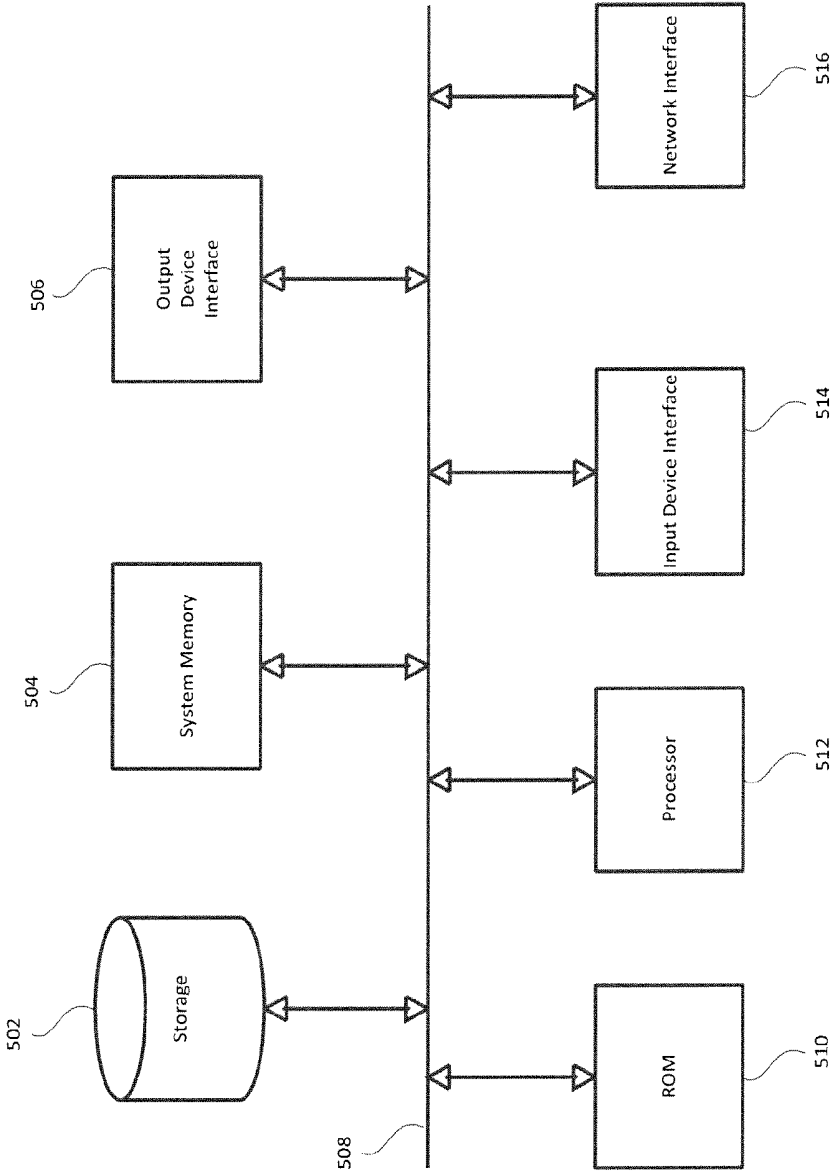


FIG. 5

ANALYTICS REGARDING VENTILATED PATIENTS

BACKGROUND

[0001] 1. Field

[0002] The present disclosure generally relates to systems and methods facilitating optimization of patient care, and, in particular, relates to monitoring of ventilated patient sedation, pain therapy and the process of weaning ventilated patients off of the ventilator.

[0003] 2. Description of the Related Art

[0004] Mechanical ventilator patients, who are intubated in a care facility, typically receive sedation and pain therapy from an infusion pump, as well as life-support from the mechanical ventilator device. Typically, a Nurse operates the infusion pump and has the overall responsibility for the patient. The ventilator is typically operated by a Respiratory Therapist.

[0005] The mechanical ventilator provides life support by assisting the patient with the inhalation of oxygen and the exhalation of CO₂ in order to maintain the necessary PaO₂, PaCO₂ and pH arterial blood levels, when the patient is unable to sustain adequate levels with their own spontaneous breathing. Positive pressure mechanical ventilators pump air with a controllable percentage of inspired oxygen (21%-100%) during the inspiratory phase of the breathing cycle. When the inspiratory phase of the breathing cycle is complete, the patient exhales through the ventilator by utilizing the natural recoil characteristics of the lungs. The volume of air that is introduced into the lungs on each cycle is the "tidal volume." This process is very invasive and introduces a high potential for complications such as baro trauma and secondary infections. Furthermore, the analgesics (or other pain medication) and sedatives commonly prescribed to such patients to provide patient comfort can themselves lead to adverse patient outcomes.

[0006] Thus, it is desirable to end the use of a mechanical ventilator as early as possible. Many of the rules and protocols for transitioning a patient off of a mechanical ventilator, or "weaning" the patient, include a series of clinical interventions including sedation and pain therapy management where the amount of sedatives and analgesics or other pain medications is reduced to awaken the patient and enable the return of their natural respiratory drive. "Spontaneous awakening trials" or "sedation vacations" where the patient is awakened as tolerated and monitored, and "spontaneous breathing trials" or "weaning trials" where the ventilator support is reduced or stopped for a period of time and the patient is monitored during the trial to identify signs of distress or difficulty. If the patient is able to successfully complete the prescribed weaning trials, "extubation" may be performed where the ventilator is removed, or the patient may be put back on full support to further prepare them for extubation.

[0007] Such interventions that facilitate a total dose reduction in analgesic and sedative medications such as the use of nurse controlled protocol guided sedation, the combination of spontaneous awakening and breathing trials, and the use of short acting medications, are associated with improved outcomes such as decreased time of mechanical ventilation and ICU length of stay. Titration of individual patients' sedation throughout their ICU admission is also managed to reduce over-sedation and side-effects, and contributes to reduced duration of mechanical ventilation and length of stay.

SUMMARY

[0008] Certain aspects of the disclosed method facilitate managing rules and protocols for ventilator patient care. In certain embodiments, a method is provided for determining compliance with one or more patient care rules and protocols. The method includes the steps of sending infusion information from a pump to a processor pertaining to one or more drugs provided to a patient, receiving ventilation information from a ventilator to the processor pertaining to ventilation provided to the patient and determining, with the processor, a variation between actual care of the patient and a set of rules and protocols associated with care of the patient at least in part based on the infusion information and the ventilation information.

[0009] In certain embodiments, a system for determining compliance with one or more patient care rules and protocols is provided. The system comprises an infusion pump providing infusion information pertaining to one or more drugs provided to a patient, a ventilator providing ventilation information pertaining to ventilation provided to the patient and a processor communicably coupled to the infusion pump and the ventilator and configured to determine a variation between actual care of the patient and a set of rules and protocols associated with care of the patient at least in part based on the infusion information and the ventilation information.

[0010] In certain embodiments, a non-transitory computer-readable medium having computer-executable instructions stored thereon for execution by a processor to perform a method of determining compliance with one or more patient care rules and protocols is provided. The method comprises the steps of receiving infusion information pertaining to one or more drugs provided to a patient, the one or more drugs including sedatives and pain therapy drugs, receiving ventilation information pertaining to ventilation provided to the patient and providing one or more analytics for display at a client device, the one or more analytics generated at least in part based on the infusion information and the ventilation information, where the one or more analytics provide indications of variation between actual care of the patient and a set of rules and protocols associated with care of the patient.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] The accompanying drawings, which are included to provide further understanding and are incorporated in and constitute a part of this specification, illustrate disclosed embodiments and together with the description serve to explain the principles of the disclosed embodiments. In the drawings:

[0012] FIGS. 1A and 1B depict exemplary hospital networks for collecting patient information and facilitating management of rules and protocols for ventilator patients in accordance with aspects of the present disclosure.

[0013] FIG. 2 illustrates an example process for providing information regarding compliance with ventilated patient care rules and protocols.

[0014] FIG. 3 illustrates an example process for generating example infusion analytics for a ventilated patient.

[0015] FIG. 4 illustrates an example process for generating example ventilation analytics for a ventilated patient.

[0016] FIG. 5 conceptually illustrates an electronic system with which some implementations of the subject technology are implemented.

DETAILED DESCRIPTION

[0017] The process of managing care of a ventilated patient to ensure optimal levels of sedation and pain therapy and proper ventilation to minimize side effects of over sedation or prolonged ventilation is essential to reduce duration of mechanical ventilation and length of stay. To facilitate managing of these concerns, many critical care facilities such as hospitals, intensive care unit (“ICU”), long term acute care (“LTAC”), skilled nursing facility and/or other care facilities, may have one or more rules and protocols, such as best practice rule sets, sedation protocols, ventilation and weaning protocols and other similar guidelines, to guide nursing and medical staff. In one example, one or more patient care rules and protocols are defined and/or communicated according to best practice rule sets, predefined rules and protocols, and/or physician orders for providing care to ventilated patients. As used herein, the phrase “rules and protocols” is used generally to refer to one or more orders (e.g., physician order), best practices, rules and/or protocols for providing care to ventilated patients.

[0018] Because following these rules and protocols is intended to lead to optimal results in patient care, it is helpful to facilitate regular oversight of whether these rules and protocols are followed, and provide for management and updating of such rules and protocols. Typically such rules and protocols provide for a set of steps to be followed for each patient placed on a mechanical ventilator with respect to dosage and titration of sedatives and pain therapy medication (e.g., analgesics), timing and frequency of spontaneous awakening trials or sedation vacations (“SATs”), timing and criteria for performing spontaneous breathing trials (“SBTs”) and timing and criteria for patient extubation when mechanical ventilation is terminated and the tube is removed from the patient.

[0019] These rules and protocols are usually put into place and/or communicated by physicians and/or care facility staff and supervisors to be followed by nurses and therapists. To provide for monitoring and improving compliance with such rules and protocols within a patient care facility or network, embodiments of the disclosed method and system provide for receiving information from one or more systems and machines including the infusion pump administering sedation and pain therapy to the patient, as well as the ventilator providing ventilation to the patient, hospital information system, monitors, laboratory systems and/or pharmacy and dispensing systems. In some embodiments, the information is collected directly from these devices without requiring any interaction from the nurse or therapist and used to generate analytics regarding the different steps of the rules and protocols for weaning a patient off of the ventilator. In addition to the infusion pump and ventilator information, other data may also be collected from other entities, including for example, demographic data regarding the patient as well as patient condition data, and may be used in assessing protocol and best practices compliance. In one example, in response to the information collected from the infusion pump and ventilator, and optionally other mechanisms or entities, one or more analytics may be generated. For example, compliance information may be generated that indicates whether the nurses and/or therapists are taking the right steps in optimal patient care. In one example, one or more markers and/or notifications may be provided to the nurse and/or therapist in response to the collected data.

[0020] Measuring and driving compliance may enable clinicians to measurably optimize and improve the ventilator weaning of patients. The data collected can be processed to generate various markers and/or analytics that provide insight into the clinical intervention events and how the timing/pattern of these events affects the weaning process and facilitate a complete view of the weaning process, including sedation/pain therapy, SATs, SBTs and extubation, thus, driving better cross-functional teamwork between physicians, nursing and respiratory technicians.

[0021] FIGS. 1A and 1B depict an example hospital network **100** for collecting patient information and facilitating management of rules and protocols for ventilator patients. As shown in FIG. 1A, the hospital network **100** includes an infusion pump **101**, an infusion system manager **102**, a ventilator **103**, a network module **104**, a hospital information system **105**, and a coordination engine **106**.

[0022] The infusion pump **101** provides sedation and pain therapy to a patient. In one example, the infusion pump **101** represents a collection of one or more infusion pumps for providing medication including pain and/or sedation medication to a patient. In one example, the infusion pump **101** may include one or more channels, and each channel may provide at least one of a sedative or pain medication (e.g., analgesics) to the patient. As described above, the infusion pump is typically operated by a nurse.

[0023] The infusion pump **101** is coupled to the infusion system manager **102** and provides infusion messages to the infusion system manager **102**. The infusion messages may, for example, indicate start and end times for specific doses/rates of medication administered to the patient. For example, each time the dosage and/or rate of one or more of the medication (e.g., sedatives and/or analgesics) is modified at the pump **101**, an infusion message is generated by the pump **101** and sent to the infusion system manager **102**. In one example, the pump **101** provides messages regarding the type of medication, dosing of medication and bolus dose patterns of medication administered at the pump **101**. The infusion system manager **102** may further receive information regarding the identification of the patient associated with infusion pump **101** from the pump **101** or hospital information system **105**. The pump **101** and infusion system manager **102** are depicted as separate elements for exemplary purposes. In some embodiments, the functionality of the infusion system manager **102** may be integrated within an infusion pump **101**.

[0024] The infusion system manager **102**, processes the infusion messages received from the pump **101**, and provides infusion information to the coordination engine **106**. In one example, the infusion information provided to the coordination engine **106** includes patient identification information (e.g., patient ID), drug information (e.g., drug type), infusion start and/or stop times for each drug, and dose and/or rates for each drug (e.g., continuous infusion dosage, bolus dosage patterns, etc.). The information may be provided for different drugs administered at pump **101**, including the sedation and pain therapy medication administered to the patient. The ventilator **103** also provides information to the coordination engine **106** through the network module **104**. Ventilation information provided to the coordination engine **106** may include the mode of ventilation, respiratory rate, tidal volume, amount of oxygen, amount of peak respiratory pressure, alarms that are triggered, and/or other ventilation information available at the ventilator **103**. In one example, the ventilator **103** may further provide a respiratory rate over tidal volume

calculation. The calculation may be the respiratory rate, which represents the number of breaths taken within a set amount of time (e.g., 60 seconds) over the tidal volume, which represents the normal volume of air displaced between normal respiration and expiration when extra effort is not applied. The information from the ventilator 103 is provided to the coordination engine 106 through network module 104. In some examples, the network module 104 may be integrated into the ventilator 103. In one embodiment, the ventilator 103, the network module 104 or a separate element in communication with the ventilator 103 and/or network module 104 may be present within the hospital network and configured to receive and/or process messages from the ventilator 103 before forwarding ventilation information to the coordination engine 106.

[0025] The coordination engine 106 may also receive patient “ADT information” from the hospital information system 105. The ADT (admission, discharge, transfer) information may include demographic information as well as patient state information. Patient demographic information may include, for example, patient sex, date of birth, attending, admitting and consulting doctors, location, blood type, height and weight, admit date and time, In/Out patient. Patient state information may include, for example, patient admit, discharge, transfer, registration, information update and other similar information regarding the state of the patient within the care facility.

[0026] In one embodiment, coordination engine 106 is embodied in any interface engine or application that aggregates data from one or more devices and systems and sends such data to an analytics application such as the knowledge portal 111. In one example, the coordination engine 106 facilitates processing, filtering and/or transformation of information received from one or more machines and/or system including the infusion system manager 102 and network module 104, for facilitating transferring the data to a respiratory knowledge portal 111 for processing and analysis. In one example, the coordination information receives the information, processes the information, and generates actionable data items for processing to the knowledge portal 111. In one embodiment, the coordination engine 105 is embodied in a processor. U.S. patent application Ser. No. 13/421,776, entitled “SCALABLE COMMUNICATION SYSTEM,” filed on Mar. 15, 2012, filed on Jan. 31, 2013 and incorporated herein by reference in its entirety, describes an example coordination engine for use with the present disclosure.

[0027] The coordination engine 106 is communicably coupled to a respiratory knowledge portal 111 of a data center 110. Data center 110 includes the knowledge portal 110 communicably coupled to one or more client devices 112 and 113. The data center 110 may be located remote from the hospital network 100 or may be part of the hospital network 100. In one example, the coordination engine 106 and knowledge portal 111 may be implemented within a single server or one or more servers communicably coupled to one another. In some examples, the functionalities of the coordination engine 106 and knowledge portal 111 may be performed by a single application or one or more applications collaborating to performing one or more of the functionalities described herein with respect to the coordination engine 105 and knowledge portal 111.

[0028] In one example, the knowledge portal 111 receives the infusion information and ventilation information from the coordination engine 106, and processes the information to

generate one or more markers and analytics and provide information regarding compliance with patient care rules and protocols. The knowledge portal 111, in some embodiments, is implemented as an application that receives information from one or more devices, such as pump 102 and ventilator 104, within a hospital network 100, and analyzes the data to provide analytics. In one embodiment, the respiratory knowledge portal 111 is embodied in a processor. U.S. patent application Ser. No. 13/756,421 entitled “RESPIRATORY KNOWLEDGE PORTAL”, filed on Jan. 31, 2013 and incorporated herein by reference in its entirety, describes an example respiratory knowledge portal for use with the present disclosure.

[0029] The knowledge portal 111 may, for example, have access to a set of pre-defined rules and protocols (e.g., best practices). The rules and protocols may be defined based on historical data and/or manually by the care facility or other entity. Using the infusion information and ventilation information received from the coordination engine 106, the knowledge portal 111 can determine one or more markers corresponding to preferences defined by the rules and protocols. The knowledge portal 111 may further be configured to measure variability from the pre-defined rules and protocols and may provide one or more analytics regarding the variance from rules and protocols (e.g., reports, notifications, etc.) to one or more entities (e.g., care facility supervisors, nurse, respiratory therapist, etc.).

[0030] In one example, a library (e.g., a drug library) is accessible by the knowledge portal 111. The drug library may include a master drug list that identifies drugs by name and/or an id. In one example, the knowledge portal 111 may further be configured with information regarding the drug type for drugs listed within the master list. For example, for one or more drugs of the master list, the knowledge portal 111 may have access to data identifying the drug type as a pain therapy drug (e.g., analgesics) or a sedative. In one example, the designation of drug types is performed by an entity such as the care facility or other third party entity.

[0031] As part of the rules and protocols, the knowledge portal 111 may further be provided with information indicating preferred drugs for a ventilator patient. For example, the rules and protocols may specify preferred pain therapy and sedative drugs for a ventilator patient as well as a preferred dosage and/or dosage ratios for each of the pain therapy and sedatives. In some embodiments, the rules and protocols specify a preferred combination of pain therapy and sedation drugs. The combination of drugs may be specified to ensure the correct combination of specific drugs and/or dosing of those drugs.

[0032] Drug preferences may be defined based on patient specific characteristics, and defined per patient or for a group of patients sharing similar characteristics. Patient specific characteristics may include demographic information such as those examples provided herein. The knowledge portal may further have access to information regarding limits (e.g., hard and soft limits) for one or more drugs listed in the master list. In one example, the library includes drug information for each drug including the drug name and identifier, drug type and/or drug limits.

[0033] Furthermore, the rules and protocols may include weaning rules and protocols, defining preferences regarding SATs and SBTs including timing, frequency and/or duration of SATs and SBTs, prerequisites to SBTs such as performing an SAT within a predefined period of time, and other patient

data that may indicate whether the patient is a good candidate for an SBT and/or weaning (e.g., patient vitals, successful SATs, etc.), and/or rules regarding extubation, including timing of extubation and/or prerequisites such as a successful SBT performed within a specific period of time from the extubation and other patient data that may indicate whether the patient is a good candidate for an SBT and/or weaning (e.g., patient vitals, etc.).

[0034] Based on the defined rules and protocols and the information available regarding drugs within the master list, and the infusion information and ventilation information received from the coordination engine **106**, the knowledge portal **111** may determine infusion and ventilation analytics. The infusion and ventilation analytics may provide insight regarding variance from the pre-defined rules and protocols.

[0035] FIG. 1B depicts an alternative example hospital network **100** for collecting patient information and facilitating management of rules and protocols for ventilator patients. The hospital network **100** of FIG. 1B is similar to that of FIG. 1A, but depicts additional systems and machines that may provide information used in addition to the infusion information and ventilation information, in generating the analytics at the knowledge portal **111**.

[0036] As shown, in addition to the elements shown in FIG. 1A, the coordination engine is further coupled to monitors **107** (e.g., vital signs monitors), dispensing system **108** (e.g., a pharmacy system and/or dispensing machine(s)), and laboratory system **109**. The coordination engine receives information regarding patient medications, condition and vital signs, from one or more machines and/or systems including, but not limited to, for example, monitors **107**, dispensing system **108**, and laboratory system **109** (e.g., a pharmacy system). The vital signs and other data may be used by the knowledge portal **111** in various steps of the processes described herein for determining analytics regarding variance from rules and protocols defining best practices, as well as, to provide indicators of when a patient is a good candidate for weaning (e.g., one or more of an SBT or extubation) in addition to various markers and analytics described herein.

[0037] In one example, the knowledge portal **111** is coupled to the client devices **112** and **113** and provides the determined metrics and analytics for display at the one or more client devices **112** and **113**. In one example, the metrics and analytics may be provided as notifications or warnings to nurses, respiratory technicians or other care providers (e.g., when a deviation from preferred rules and protocols is recognized, or when a preferred event should be performed). In another example, one or more of the markers and analytics may be provided to those in a supervisory role to provide an overall view of the process, identify issues in actual weaning processes and patient care, and provide insight into the pattern of events that lead to optimal results with respect to a patient. The metrics and analytics may be analyzed and provided in real time or near real time for display at the client devices **111**. In one example, the analytics may further be used to provide decision support for performing patient care within respect to ventilated patients. In some embodiments, the knowledge portal **111** may provide the metrics and analytics to the client devices **112** and **113** over a wired or wireless network or communication channel.

[0038] FIG. 1B depicts another example of hospital network **100**. As shown in FIG. 1B, in addition to the infusion information and ventilation information, the analytics generated at the knowledge portal **111** may further be generated

based on other machine data providing patient information and vital signs, from one or more machines and/or systems including, but not limited to, for example, monitors **107**, dispensing system **108** (e.g., a pharmacy system and/or dispensing machine(s)), and laboratory system **109**. The vital signs and other data may be used by the knowledge portal **111** in various steps of the processes described herein for determining analytics regarding variance from rules and protocols defining best practices, as well as, to provide indicators of when a patient is a good candidate for weaning (e.g., one or more of an SBT or extubation) in addition to various markers and analytics described herein.

[0039] FIG. 2 illustrates an example process **200** for providing information regarding compliance with ventilated patient care rules and protocols. In step **201**, infusion information regarding drugs administered to a patient is received at the knowledge portal **111**. The information may be provided from an infusion pump (e.g., infusion pump **101** and/or infusion system manager **103**). The information may include patient identification, drug types administered to a patient, drugs dosage and/or rates, as well as infusion start, stop.

[0040] In step **202**, ventilation information regarding ventilation provided to the patient is received at the knowledge portal **111**. The information may be received from a ventilator (e.g., ventilator **103**). The information may include the mode of ventilation, respiratory rate, tidal volume, respiratory rate divided by the tidal volume, percent of inspired oxygen (e.g., within a range of 21% to 100%), amount of peak inspiratory pressure, alarms that are triggered, and/or other ventilation information available at the ventilator. In other embodiments, information is provided from additional systems, as discussed above.

[0041] In step **203**, one or more rules and protocols regarding ventilated patient care are identified. In one example, the rules and protocols define best practices for weaning patients off of mechanical ventilation. The rules and protocols may be pre-defined by an entity such as the care-facility or other entity having knowledge of best practices.

[0042] The rules and protocols identified in step **203** may, for example, include rules and protocols regarding medication or drugs administered to patients. In one example, the information indicates preferred drugs for a ventilator patient. For example, the rules and protocols may specify preferred pain therapy and sedative drugs for a ventilator patient as well as a preferred dosage and/or dosage ratios (e.g., ratio of sedative or pain therapy drugs for each patient) for such drugs. The rules and protocols may further include limits (e.g., soft or hard limits) for one or more drugs administered to a patient. Furthermore, the rules and protocols may include weaning rules and protocols, including rules and protocols regarding SATs, SBTs, and extubation including timing, frequency, duration and/or preceding or following events.

[0043] In step **204**, one or more markers are calculated according to the information received in steps **201** and **202**. In some embodiments, the one or more markers may also be generated based on information received from the hospital information system **105**, monitors **107**, dispensing system **108** and laboratory system **109**. The one or more markers may correspond to desirable values and events defined by the rules and protocols identified in step **203**. The one or more markers may, for example, include identification of the drugs administered to a patient, weight-based doses of drugs administered to a patient, information regarding bolus doses, and occurrence and timing of one or more SATs, SBTs and extubation.

[0044] In step 205 infusion and ventilation analytics are generated by comparing the one or more markers to the rules and protocols to determine a variance from best practices. For example, the drugs administered to a patient as well as the dosages of the drugs are compared to the rules and protocols to determine if the preferred drugs are administered to a patient at the preferred dosages, and within predefined limits. Furthermore, it is determined whether SATs are administered according to best practice, including timing and frequency of SATs, and whether the SATs are successful based on at least the duration of each SAT. Additionally, it is determined whether SBTs are performed according to the rules and protocols, including whether a patient that is a good candidate for weaning undergoes an SBT and whether prerequisites for an SBT are met, as well as the success of the SBT. Also, it may be determined if extubation of a patient is performed according to the rules and protocols including the timing of the extubation and prerequisites of the extubation being met. An example process for generating infusion analytics is described in further detail below with respect to FIG. 3. An example process for generating ventilation analytics is described in further detail below with respect to FIG. 4.

[0045] In step 206, the one or more analytics are provided for display at a client device. In one example, the analytics are provided as notifications to one or more entities such as a nurse or respiratory therapist. In another example, the analytics may be provided in one or more reports to one or more user in a supervisory role.

[0046] FIG. 3 illustrates an example process 300 for generating example infusion analytics for a ventilated patient.

[0047] In step 301, identification and dosage information for each drug administered to the patient are identified. As described above, with respect to FIG. 2, the identification and dosage information is determined based on information provided by the infusion pump. In one example, a drug library including a master drug list is used to identify drugs by name and/or an id. The infusion pump 101 provides the drug name and/or id for each drug administered to the patient at the infusion pump 101. Dosage information of the drug may be a weight based dosage of each drug administered to the patient calculated according to the dosage information for each drug administered as provided by the infusion pump, and a weight of the patient that is provided as part of the ADT information regarding the patient.

[0048] In step 302, it is determined if the drugs administered to the patient are the preferred drugs as defined by the rules and protocols. In one example, the rules and protocols define specific preferred sedative and pain therapy drugs to be administered to the patient. For example, the rules and protocols may specify preferred pain therapy and sedative drugs for a ventilator patient. In one example, the preferences may be defined according to specific patient characteristics. The determination of which drugs are defined as preferred drugs for the patient may be performed by determining specific patient characteristics of the patient and determining the preferred drugs for the patient based on the characteristics.

[0049] In step 303, it is determined if the correct dosage of each drug is administered. The rules and protocols may specify preferred dosage and/or dosage ratios for the pain therapy and sedative drugs for a ventilator patient. In one example, the weight based dosages for each drug as identified in step 301 is used to determine if the dosage of each drug

meets the defined dosage preferences. Bolus doses may also be analyzed to determine if the patient is being over medicated.

[0050] A dosage ratio may be calculated based on the weight based dosages of the sedative and pain therapy medications. In one example, the ratio defines a relationship between the amount (dosage) of a sedative administered to a patient and the amount (dosage) of a pain therapy drug administered to the patient. The calculated dosage ratio is then compared to the preferred dosage ratio as defined by the rules and protocols to determine if there is a variance between the calculated dosage ratio and the preferred dosage ratio.

[0051] In step 304, it is determined if the dosage of drugs administered is within a pre-define limit. For example, information regarding limits (e.g., soft or hard limits) for one or more drugs may be accessed and compared to the dosages for each drug to determine if the dosages are within the limits for that drug.

[0052] In step 305, infusion analytics are generated according to the determinations in step 302, 303 and 304.

[0053] FIG. 4 illustrates an example process 400 for generating example ventilation analytics for a ventilated patient.

[0054] In step 401 it is determined whether one or more SATs were performed with respect to the patient. In order to perform SATs or sedation vacations, the dosage of sedation and pain therapy medication administered to a patient is typically reduced (e.g., to a lower dosage or stopped). In step 401, dosage information and infusion starts and stops provided by the infusion pump 101 to the coordinated engine 106 and knowledge portal 111 are analyzed to identify SATs. That is, changes in dosage and/or start/stop of dosage are analyzed and where the dosage is reduced to a level that indicates an SAT (e.g., reduced or stopped), a marker is generated indicating a start of an SAT. The dosages following the marker are then analyzed until an increase in dosage to a level indicating a termination of an SAT is observed (e.g., an increase or restart). Another marker is then generated indicating a termination of the SAT. Instead of a dosage increase, indicating a termination of an SAT, in some instances an SAT may be followed by an SBT. In such instances, a marker may be generated once an SBT is initiated, to indicate the termination of an SAT.

[0055] If, in step 401, one or more SATs are identified, in step 402, it is determined whether the SATs are performed according to the rules and protocols. For example, the rules and protocols may define preferred timing, frequency and/or duration of SATs. For example, the rules and protocols may define that SATs should be performed one or more times per day and/or preferred times for conducting SATs. The markers for the SATs are used to determine the frequency of the SATs and/or the timing for each SAT performed. The determined frequency and/or timing is then compared to the frequency and/or timing defined by the rules to determine if there is a variance between the frequency and/or timing actual of the performed SATs and the preferred frequency and/or timing of SATs.

[0056] Furthermore, the rules and protocols may define a preferred duration. The start/end markers for each SAT may be used to determine the duration of the SAT. The duration is then compared to the defined preferred duration. In one example, the preferred duration indicates that an SAT was successful. If, in step 401, no SATs are identified, the process continues to step 403.

[0057] In step 403, it is determined whether one or more SBTs were performed with respect to the patient. When performing an SBT, the ventilator 103 is put into a different mode in order to perform the SBT. The mode information provided by the ventilator 103 is analyzed to determine when a change in mode indicative of an SBT occurs. A marker is generated when such a change is detected, marking the beginning of the SBT. Next, ventilator information is analyzed to identify a termination of the SBT. A termination of an SBT may be indicated by a change in the mode of the ventilator 103 or by the termination of ventilation indicative of an extubation. A marker is generated when an SBT termination is identified.

[0058] If, in step 403, one or more SBTs are identified, in step 404, it is determined whether the SBTs are performed according to the rules and protocols. In one example, the rules and protocols may include rules regarding preferred timing, frequency and/or duration of SATs. Furthermore, the rules may indicate one or more prerequisites before the SBT is performed.

[0059] For example, the rules may define that once it is determined that a patient is a good candidate for a SBT (e.g., a candidate for weaning), an SAT should be performed and after a predefined amount of time an SBT should be initiated. The markers for the SBT are used to determine the timing and duration of the SBT. Furthermore, the marker for the preceding SAT is used to determine the amount of time before an SBT is initiated following the SAT, and whether the SBT is successfully completed.

[0060] The rules and protocols may also define a preferred duration for an SBT. The start/end markers for each SBT may be used to determine the duration of the SBT. The duration is then compared to the defined preferred duration. In one example, the preferred duration indicates that an SBT was successful.

[0061] Furthermore, a successful SBT (e.g., defined by a specific duration) in patients that are a good candidate for weaning should be followed by an extubation within a predefined amount of time of the SBT being initiated. The markers are used along with markers indicating an extubation to determine a time elapsed between a successful SBT and extubation in certain patients.

[0062] The information is then compared to the SBT rules and protocols to determine if there is a variance between the timing, duration and prerequisite of actual SBTs performed and the preferred timing, duration and prerequisite of SBTs. If, in step 403, no SATs are identified, the process continues to step 405.

[0063] In step 405, it is determined whether an extubation of the patient was performed. An extubation may be identified if a termination in ventilation information is detected (e.g., following a successful SBT). In one example, in response to detecting a termination of ventilation information, a marker is generated indicating an extubation. In one example, a threshold time may be defined before a termination of ventilation is interpreted as an extubation. The threshold time may, for example, account for switching the patient to a remote ventilator for various reasons.

[0064] If, in step 405, it is determined that an extubation was performed with respect to the patient, in step 406 it is determined if the extubation was performed according to the rules and protocols. For example, the rules and protocols may define a timing for performing an extubation following a successful SBT being performed. The markers for SBTs and the extubation may be used to determine if an SBT was

successfully completed and the time lapsed after the successful SBT (e.g., as defined by a specific duration), before extubation was performed. This information is then compared to the rules and protocols to determine if there is a variance between the timing and preceding events of the extubation and the defined rules and protocols for extubation.

[0065] In step 407, ventilation analytics are generated according to the determinations in steps 401-406.

[0066] Accordingly, the embodiments of the disclosed system and methods provide for processing information from one or more infusion pumps, ventilators, hospital information systems, monitors, dispensing systems, and/or laboratory systems providing information regarding a ventilated patient and analyzing the information to assess protocol and best practices compliance. The collected information can be processed to generate various markers and/or analytics that provide insight into the clinical intervention events and how the timing/pattern of these events affects the weaning process and facilitate a complete view of the weaning process, including sedation/pain therapy, SATs, SBTs and extubation, thus, driving better cross-functional team work between physicians, nursing and respiratory technicians. Measuring and driving compliance may enable clinicians to measurably optimize and improve the weaning of ventilated patients. Furthermore, the generated markers and analytics may help provide.

[0067] FIG. 5 conceptually illustrates an electronic system with which some implementations of the subject technology are implemented. Electronic system 500 can be a server, computer, phone, PDA, laptop, tablet computer, television with one or more processors embedded therein or coupled thereto, or any other sort of electronic device. Such an electronic system includes various types of computer readable media and interfaces for various other types of computer readable media. Electronic system 500 includes a bus 508, processing unit(s) 512, a system memory 504, a read-only memory (ROM) 510, a permanent storage device 502, an input device interface 514, an output device interface 506, and a network interface 516.

[0068] Bus 508 collectively represents all system, peripheral, and chipset buses that communicatively connect the numerous internal devices of electronic system 500. For instance, bus 508 communicatively connects processing unit(s) 512 with ROM 510, system memory 504, and permanent storage device 502.

[0069] From these various memory units, processing unit(s) 512 retrieves instructions to execute and data to process in order to execute the processes of the subject disclosure. The processing unit(s) can be a single processor or a multi-core processor in different implementations.

[0070] ROM 510 stores static data and instructions that are needed by processing unit(s) 512 and other modules of the electronic system. Permanent storage device 502, on the other hand, is a read-and-write memory device. This device is a non-volatile memory unit that stores instructions and data even when electronic system 500 is off. Some implementations of the subject disclosure use a mass-storage device (such as a magnetic or optical disk and its corresponding disk drive) as permanent storage device 502.

[0071] Other implementations use a removable storage device (such as a floppy disk, flash drive, and its corresponding disk drive) as permanent storage device 502. Like permanent storage device 502, system memory 504 is a read-and-write memory device. However, unlike storage device 502, system memory 504 is a volatile read-and-write memory,

such a random access memory. System memory **504** stores some of the instructions and data that the processor needs at runtime. In some implementations, the processes of the subject disclosure are stored in system memory **504**, permanent storage device **502**, and/or ROM **510**. For example, the various memory units include instructions for determining compliance with one or more patient care rules and protocols according to various implementations. From these various memory units, processing unit(s) **512** retrieves instructions to execute and data to process in order to execute the processes of some implementations.

[0072] Bus **508** also connects to input and output device interfaces **514** and **506**. Input device interface **514** enables the user to communicate information and select commands to the electronic system. Input devices used with input device interface **514** include, for example, alphanumeric keyboards and pointing devices (also called “cursor control devices”). Output device interfaces **506** enables, for example, the display of images generated by the electronic system **500**. Output devices used with output device interface **506** include, for example, printers and display devices, such as cathode ray tubes (CRT) or liquid crystal displays (LCD). Some implementations include devices such as a touchscreen that functions as both input and output devices.

[0073] Finally, as shown in FIG. **5**, bus **508** also couples electronic system **500** to a network (not shown) through a network interface **516**. In this manner, the computer can be a part of a network of computers (such as a local area network (“LAN”), a wide area network (“WAN”), or an Intranet, or a network of networks, such as the Internet. Any or all components of electronic system **500** can be used in conjunction with the subject disclosure.

[0074] These functions described above can be implemented in digital electronic circuitry, in computer software, firmware or hardware. The techniques can be implemented using one or more computer program products. Programmable processors and computers can be included in or packaged as mobile devices. The processes and logic flows can be performed by one or more programmable processors and by one or more programmable logic circuitry. General and special purpose computing devices and storage devices can be interconnected through communication networks.

[0075] Some implementations include electronic components, such as microprocessors, storage and memory that store computer program instructions in a machine-readable or computer-readable medium (alternatively referred to as computer-readable storage media, machine-readable media, or machine-readable storage media). Some examples of such computer-readable media include RAM, ROM, read-only compact discs (CD-ROM), recordable compact discs (CD-R), rewritable compact discs (CD-RW), read-only digital versatile discs (e.g., DVD-ROM, dual-layer DVD-ROM), a variety of recordable/rewritable DVDs (e.g., DVD-RAM, DVD-RW, DVD+RW, etc.), flash memory (e.g., SD cards, mini-SD cards, micro-SD cards, etc.), magnetic and/or solid state hard drives, read-only and recordable Blu-Ray® discs, ultra density optical discs, any other optical or magnetic media, and floppy disks. The computer-readable media can store a computer program that is executable by at least one processing unit and includes sets of instructions for performing various operations. Examples of computer programs or computer code include machine code, such as is produced by a com-

piler, and files including higher-level code that are executed by a computer, an electronic component, or a microprocessor using an interpreter.

[0076] While the above discussion primarily refers to microprocessor or multi-core processors that execute software, some implementations are performed by one or more integrated circuits, such as application specific integrated circuits (ASICs) or field programmable gate arrays (FPGAs). In some implementations, such integrated circuits execute instructions that are stored on the circuit itself.

[0077] As used in this specification and any claims of this application, the terms “computer”, “server”, “processor”, and “memory” all refer to electronic or other technological devices. These terms exclude people or groups of people. For the purposes of the specification, the terms display or displaying means displaying on an electronic device. As used in this specification and any claims of this application, the terms “computer readable medium” and “computer readable media” are entirely restricted to tangible, physical objects that store information in a form that is readable by a computer. These terms exclude any wireless signals, wired download signals, and any other ephemeral signals.

[0078] To provide for interaction with a user, implementations of the subject matter described in this specification can be implemented on a computer having a display device, e.g., a CRT (cathode ray tube) or LCD (liquid crystal display) monitor, for displaying information to the user and a keyboard and a pointing device, e.g., a mouse or a trackball, by which the user can provide input to the computer. Other kinds of devices can be used to provide for interaction with a user as well; for example, feedback provided to the user can be any form of sensory feedback, e.g., visual feedback, auditory feedback, or tactile feedback; and input from the user can be received in any form, including acoustic, speech, or tactile input. In addition, a computer can interact with a user by sending documents to and receiving documents from a device that is used by the user; for example, by sending web pages to a web browser on a user’s client device in response to requests received from the web browser.

[0079] Implementations of the subject matter described in this specification can be implemented in a computing system that includes a back end component, e.g., as a data server, or that includes a middleware component, e.g., an application server, or that includes a front end component, e.g., a client computer having a graphical user interface or a Web browser through which a user can interact with an implementation of the subject matter described in this specification, or any combination of one or more such back end, middleware, or front end components. The components of the system can be interconnected by any form or medium of digital data communication, e.g., a communication network. Examples of communication networks include a local area network (“LAN”) and a wide area network (“WAN”), an inter-network (e.g., the Internet), and peer-to-peer networks (e.g., ad hoc peer-to-peer networks).

[0080] The computing system can include clients and servers. A client and server are generally remote from each other and typically interact through a communication network. The relationship of client and server arises by virtue of computer programs running on the respective computers and having a client-server relationship to each other. In some implementations, a server transmits data (e.g., an HTML page) to a client device (e.g., for purposes of displaying data to and receiving user input from a user interacting with the client device). Data

generated at the client device (e.g., a result of the user interaction) can be received from the client device at the server.

[0081] In the previous detailed description, numerous specific details have been set forth to provide a full understanding of the present disclosure. It will be apparent, however, to one ordinarily skilled in the art that embodiments of the present disclosure may be practiced without some of the specific details. In other instances, well-known structures and techniques have not been shown in detail so as not to obscure the disclosure.

[0082] The previous description is provided to enable any person skilled in the art to practice the various aspects described herein. While the foregoing has described what are considered to be the best mode and/or other examples, it is understood that various modifications to these aspects will be readily apparent to those skilled in the art, and the generic principles defined herein may be applied to other aspects. Thus, the claims are not intended to be limited to the aspects shown herein, but is to be accorded the full scope consistent with the language claims, wherein reference to an element in the singular is not intended to mean “one and only one” unless specifically so stated, but rather “one or more.” Unless specifically stated otherwise, the terms “a set” and “some” refer to one or more. Pronouns in the masculine (e.g., his) include the feminine and neuter gender (e.g., her and its) and vice versa. Headings and subheadings, if any, are used for convenience only and do not limit the invention.

[0083] It is understood that the specific order or hierarchy of steps in the processes disclosed is an illustration of exemplary approaches. Based upon design preferences, it is understood that the specific order or hierarchy of steps in the processes may be rearranged. Some of the steps may be performed simultaneously. The accompanying method claims present elements of the various steps in a sample order, and are not meant to be limited to the specific order or hierarchy presented.

[0084] Terms such as “top,” “bottom,” “front,” “rear” and the like as used in this disclosure should be understood as referring to an arbitrary frame of reference, rather than to the ordinary gravitational frame of reference. Thus, a top surface, a bottom surface, a front surface, and a rear surface may extend upwardly, downwardly, diagonally, or horizontally in a gravitational frame of reference.

[0085] A phrase such as an “aspect” does not imply that such aspect is essential to the subject technology or that such aspect applies to all configurations of the subject technology. A disclosure relating to an aspect may apply to all configurations, or one or more configurations. A phrase such as an aspect may refer to one or more aspects and vice versa. A phrase such as an “embodiment” does not imply that such embodiment is essential to the subject technology or that such embodiment applies to all configurations of the subject technology. A disclosure relating to an embodiment may apply to all embodiments, or one or more embodiments. A phrase such as an embodiment may refer to one or more embodiments and vice versa.

[0086] The word “exemplary” is used herein to mean “serving as an example or illustration.” Any aspect or design described herein as “exemplary” is not necessarily to be construed as preferred or advantageous over other aspects or designs.

[0087] All structural and functional equivalents to the elements of the various aspects described throughout this disclosure that are known or later come to be known to those of

ordinary skill in the art are expressly incorporated herein by reference and are intended to be encompassed by the claims. Moreover, nothing disclosed herein is intended to be dedicated to the public regardless of whether such disclosure is explicitly recited in the claims. No claim element is to be construed under the provisions of 35 U.S.C. §112, sixth paragraph, unless the element is expressly recited using the phrase “means for” or, in the case of a method claim, the element is recited using the phrase “step for.” Furthermore, to the extent that the term “include,” “have,” or the like is used in the description or the claims, such term is intended to be inclusive in a manner similar to the term “comprise” as “comprise” is interpreted when employed as a transitional word in a claim.

What is claimed is:

1. A method of determining compliance with one or more patient care rules and protocols, the method including the steps of:

sending infusion information from a pump to a processor pertaining to one or more drugs provided to a patient; sending ventilation information from a ventilator to the processor pertaining to ventilation provided to the patient; and

determining, with the processor, a variation between actual care of the patient and a set of rules and protocols associated with care of the patient at least in part based on the infusion information and the ventilation information.

2. The method of claim 1, further comprising the steps of: determining whether one or more spontaneous awakening trials (“SATs”) have occurred based on at least in part one or more of the infusion information and ventilation information; and

when it is determined if one or more SATs have occurred, for each of one or more SATs determining a start time and a stop time of the SAT based at least in part on one or more of the infusion information and ventilation information.

3. The method of claim 2, further comprising:

comparing a frequency of the one or more SATs to a preferred frequency of SATs defined by the set of rules and protocols, when it is determined that one or more SATs have occurred.

4. The method of claim 2, further comprising:

determining if each of the one or more SATs were successful based on a duration of the SAT, wherein the duration of the SAT is determined based on the start time and stop time of the SAT, when it is determined that one or more SATs have occurred.

5. The method of claim 1, further comprising the steps of: determining whether one or more spontaneous breathing trials (“SBTs”) have occurred based at least in part on one or more of the infusion information and ventilation information; and

when it is determined that one or more SBTs have occurred, for each of one or more SBTs determining a start time and a stop time of the SBT based at least in part on one or more of the infusion information and ventilation information.

6. The method of claim 5, further comprising the steps of: determining if each of the one or more SBTs was successful based on a duration of the SBT, wherein the duration of the SBT is determined based on the start time and stop time of the SBT, when it is determined that one or more SBTs have occurred.

7. The method of claim 5, further comprising the steps of: identifying one or more preceding events that occurred previous to the SBT and comparing the one or more preceding events to one or more preferred preceding events defined by the set of rules and protocols, when it is determined that one or more SBTs have occurred.

8. The method of claim 1, further comprising the step of: determining if an extubation has occurred based at least in part on one or more of the infusion information and the ventilation information; and

identifying one or more preceding events that occurred previous to the extubation and comparing the one or more preceding events to one or more preferred preceding events defined by the set of rules and protocols, when it is determined that the extubation has occurred.

9. The method of claim 1, further comprising the steps of: sending patient vital signs indicating vital conditions of the patient from one or more of a laboratory system, a monitor, or dispensing system to the processor; and wherein the determining step is further based on the patient vital signs.

10. The method of claim 1, further comprising the steps of: sending ADT information including one or more of demographic information and state information for the patient from a hospital information system to the processor; and wherein the determining step is further based on the ADT information.

11. The method of claim 1, further comprising the steps of: sending information from at least one of a laboratory system, dispensing system or a monitor to the processor, and wherein the determination of the variation is further based, at least in part, on the information from the at least one of the laboratory system, dispensing system or the monitor.

12. The method of claim 1, wherein the infusion information includes one or more of a drug type for each drug administered to the patient, a dosage of each drug administered to the patient, a rate of each drug administered to the patient, or an indication of infusion started or stopped.

13. The method of claim 1, wherein the ventilation information includes one or more of a mode of ventilation, respiratory rate, tidal volume, amount of oxygen, amount of peak respiratory pressure, or alarms triggered at the ventilator.

14. The method of claim 1, further comprising the steps of: calculating a weight based dosage of each drug administered to the patient based at least in part on the infusion information and a weight of the patient, wherein the set of rules and protocols includes a preferred dosage for each drug administered to the patient; and comparing the weight based dosage of each drug to the preferred dosage for the drug.

15. The method of claim 1, wherein the drugs administered to the patient includes at least a sedative and an analgesic.

16. The method of claim 15, further comprising the steps of:

calculating a weight based dosage of each of the sedative and analgesic administered to the patient based at least in part on the infusion information and a weight of the patient;

calculating a ratio of sedative to analgesic based on the dosage of weight based dosage of each of the sedative

and analgesic, wherein the set of rules and protocols includes a preferred ratio of sedative to analgesic; and comparing the calculated ratio to the preferred ratio.

17. The method of claim 1, further comprising the steps of: identifying the set of rules and protocols, wherein the set of rules and protocols include preferences regarding the drugs administered to the patient and a weaning process followed with regards to the patient.

18. A system for determining compliance with one or more patient care protocols, comprising:

an infusion pump providing infusion information pertaining to one or more drugs provided to a patient;

a ventilator providing ventilation information pertaining to ventilation provided to the patient; and

a processor communicably coupled to the infusion pump and the ventilator and configured to determine a variation between actual care of the patient and a set of rules and protocols associated with care of the patient at least in part based on the infusion information and the ventilation information.

19. The system of claim 18, further comprising:

a coordination engine coupled to the infusion pump, the ventilator and the processor, and configured to collect the infusion information and ventilation information and provide the information to the processor.

20. The system of claim 18, wherein:

the infusion pump is coupled to an infusion system manager configured to receive infusion messages from the infusion pump and generate the infusion information provided to the processor.

21. The system of claim 18, further comprising:

one or more of a laboratory system, a vital signs monitor, or a dispensing system; and

wherein the processor is configured to determine the variation further based at least in part on information provided by at least one of the laboratory system, vital signs monitor or the dispensing system.

22. A non-transitory computer-readable medium having computer-executable instructions stored thereon for execution by a processor to perform a method of determining compliance with one or more patient care protocols, the method comprising the steps of:

receiving infusion information pertaining to one or more drugs provided to a patient, the one or more drugs including sedatives and pain therapy drugs;

receiving ventilation information pertaining to ventilation provided to the patient; and

providing one or more analytics for display at a client device, the one or more analytics generated at least in part based on the infusion information and the ventilation information, where the one or more analytics provide indications of variation between actual care of the patient and a set of rules and protocols associated with care of the patient.

* * * * *

专利名称(译)	关于通气患者的分析		
公开(公告)号	US20140371618A1	公开(公告)日	2014-12-18
申请号	US13/917614	申请日	2013-06-13
申请(专利权)人(译)	CAREFUSION 303 , INC.		
当前申请(专利权)人(译)	CAREFUSION 303 , INC.		
[标]发明人	STEINHAUER TOM BLANSFIELD TERRY LEE MULKOWSKY LEONARD CALDERON III ANDRES JESUS		
发明人	STEINHAUER, TOM BLANSFIELD, TERRY LEE MULKOWSKY, LEONARD CALDERON, III, ANDRES JESUS		
IPC分类号	A61M16/00 A61B5/087 A61B5/08 A61B5/091 A61B5/00 A61M5/172		
CPC分类号	A61M16/0051 A61B5/4833 A61M5/172 A61B5/4848 A61B5/082 A61B5/091 A61B5/0871 A61B5/0816 A61M16/021 G06F19/325 G06F19/3468 G06F19/3481 G16H20/17 G16H20/40 G16H40/20 G16H70/20 G16H20/00 G16H20/10		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于确定对一个或多个患者护理规则和协议的依从性的方法，系统和计算机可读介质，该方法包括将输注信息从泵发送到与提供给患者的一种或多种药物有关的处理器的步骤，将来自呼吸机的通气信息发送到与提供给患者的通气有关的处理器，并且利用处理器确定患者的实际护理与一组与患者护理相关的规则和协议之间的变化，至少部分地基于输液信息和通气信息。

