



US010342470B2

(12) **United States Patent**  
**Al-Ali et al.**

(10) **Patent No.:** **US 10,342,470 B2**  
(45) **Date of Patent:** **\*Jul. 9, 2019**

(54) **SYSTEM AND METHOD FOR MONITORING  
THE LIFE OF A PHYSIOLOGICAL SENSOR**

(71) Applicant: **Masimo Corporation**, Irvine, CA (US)

(72) Inventors: **Ammar Al-Ali**, San Juan Capistrano,  
CA (US); **Walter M. Weber**, Laguna  
Hills, CA (US); **Ryan Timothy  
McHale**, Tustin, CA (US)

(73) Assignee: **Masimo Corporation**, Irvine, CA (US)

(\*) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 0 days.  
  
This patent is subject to a terminal dis-  
claimer.

(21) Appl. No.: **16/047,364**

(22) Filed: **Jul. 27, 2018**

(65) **Prior Publication Data**

US 2019/0021638 A1 Jan. 24, 2019

**Related U.S. Application Data**

(63) Continuation of application No. 15/388,075, filed on  
Dec. 22, 2016, now Pat. No. 10,039,482, which is a  
(Continued)

(51) **Int. Cl.**  
**A61B 5/1495** (2006.01)  
**A61B 5/1455** (2006.01)  
**A61B 5/00** (2006.01)

(52) **U.S. Cl.**  
CPC ..... **A61B 5/1495** (2013.01); **A61B 5/0002**  
(2013.01); **A61B 5/14551** (2013.01);  
(Continued)

(58) **Field of Classification Search**

CPC . A61B 5/1495; A61B 5/14551; A61B 5/6838;  
A61B 5/0002; A61B 5/6826;  
(Continued)

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,103,214 A 9/1963 Smith  
3,313,290 A 4/1967 Chance et al.  
(Continued)

**FOREIGN PATENT DOCUMENTS**

AU 85938/91 4/1992  
CA 2052650 4/1992  
(Continued)

**OTHER PUBLICATIONS**

De Kock, J.P. et al., "The Effect of Varying LED Intensity on Pulse  
Oximeter Accuracy", Journal of Medical Engineering & Technol-  
ogy, Vo. 15, No. 3.

(Continued)


*Primary Examiner* — Adnan Azizi

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson  
& Bear, LLP

(57) **ABSTRACT**

Aspects of the present disclosure include a sensor configured  
to store in memory indications of sensor use information and  
formulas or indications of formulas for determining the  
useful life of a sensor from the indications of sensor use  
information. A monitor connected to the sensor monitors  
sensor use and stores indications of the use on sensor  
memory. The monitor and/or sensor compute the useful life  
of the sensor from the indications of use and the formulas.  
When the useful life of the sensor is reached, an indication  
is given to replace the sensor.

**20 Claims, 9 Drawing Sheets**

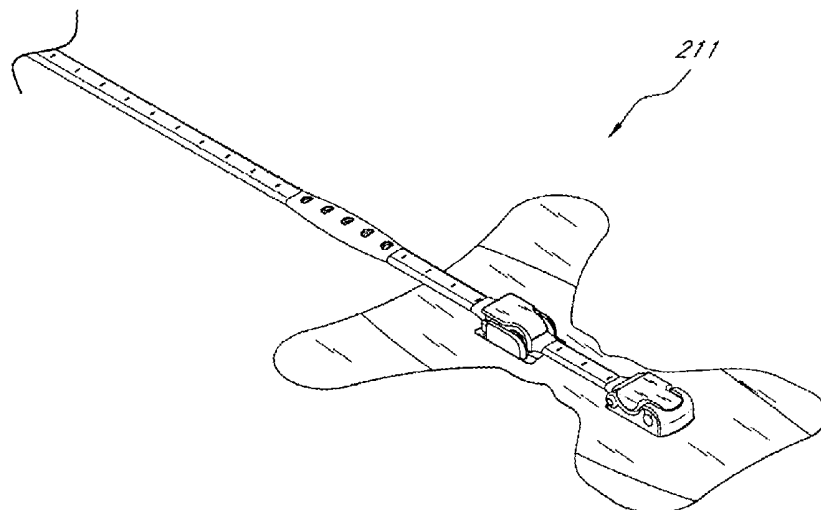

**Related U.S. Application Data**

continuation of application No. 14/821,590, filed on Aug. 7, 2015, now Pat. No. 9,560,998, which is a continuation of application No. 14/573,332, filed on Dec. 17, 2014, now Pat. No. 9,107,626, which is a continuation of application No. 13/015,207, filed on Jan. 27, 2011, now Pat. No. 8,922,382, which is a continuation of application No. 11/580,214, filed on Oct. 12, 2006, now Pat. No. 7,880,626.

**(52) U.S. Cl.**

CPC ..... *A61B 5/14552* (2013.01); *A61B 5/6826* (2013.01); *A61B 5/6838* (2013.01); *A61B 2560/028* (2013.01); *A61B 2560/0238* (2013.01); *A61B 2560/0266* (2013.01); *A61B 2560/0276* (2013.01); *A61B 2560/045* (2013.01); *A61B 2560/0475* (2013.01); *A61B 2562/0238* (2013.01); *A61B 2562/043* (2013.01); *A61B 2562/085* (2013.01)

**(58) Field of Classification Search**

CPC ..... A61B 5/14552; A61B 2560/0276; A61B 2560/0475; A61B 2560/045; A61B 2560/028; A61B 2560/0266; A61B 2560/0238; A61B 2562/0238; A61B 2562/043; A61B 2562/085

See application file for complete search history.

**(56)****References Cited**

## U.S. PATENT DOCUMENTS

3,319,216 A	5/1967	McCullough	4,684,246 A	8/1987	Downing et al.
3,463,142 A	8/1969	Harte et al.	4,685,464 A	8/1987	Goldberger et al.
3,482,565 A	12/1969	Gowen	4,690,492 A	9/1987	Beard
3,543,310 A	10/1970	Pelissier	4,695,258 A	9/1987	Hanson et al.
3,647,299 A	3/1972	Lavallee	4,700,708 A	10/1987	New, Jr. et al.
3,704,706 A	12/1972	Herczfeld et al.	4,770,179 A	9/1988	New, Jr. et al.
3,710,303 A	1/1973	Gallagher, Jr.	4,797,125 A	1/1989	Malana
3,711,272 A	1/1973	Randall et al.	4,815,469 A	3/1989	Cohen et al.
3,740,570 A	6/1973	Kaelin et al.	4,824,242 A	4/1989	Frick et al.
3,799,672 A	3/1974	Vurek	4,825,872 A	5/1989	Tan et al.
3,970,353 A	7/1976	Kaufman	4,825,879 A	5/1989	Tan et al.
3,995,209 A	11/1976	Weston	4,830,014 A	5/1989	Goodman et al.
4,086,915 A	5/1978	Kofsky et al.	4,838,808 A	6/1989	Fujiura
4,129,124 A	12/1978	Thalmann	4,844,784 A	7/1989	Suzuki et al.
4,169,976 A	10/1979	Cirri	4,848,901 A	7/1989	Hood, Jr.
4,182,977 A	1/1980	Stricklin, Jr.	4,858,615 A	8/1989	Meinema
4,305,401 A	12/1981	Reissmueller et al.	4,859,057 A	8/1989	Taylor et al.
4,308,456 A	12/1981	Van Der Gaag et al.	4,865,038 A	9/1989	Rich et al.
4,321,930 A	3/1982	Jobsis et al.	4,867,165 A	9/1989	Noller et al.
4,334,544 A	6/1982	Hill et al.	4,877,322 A	10/1989	Hill
4,346,590 A	8/1982	Brown	4,880,304 A	11/1989	Jacob et al.
4,350,165 A	9/1982	Striese	4,907,594 A	3/1990	Muz
4,380,240 A	4/1983	Jöbsis et al.	4,913,150 A	4/1990	Cheung et al.
4,406,289 A	9/1983	Wesseling et al.	4,927,264 A	5/1990	Shiga et al.
4,407,290 A	10/1983	Wilber	4,938,218 A	7/1990	Goodman et al.
4,414,980 A	11/1983	Mott	4,942,877 A	7/1990	Sakai et al.
4,449,821 A	5/1984	Lee	4,952,177 A	8/1990	Drake et al.
4,451,694 A	5/1984	Harper et al.	4,960,128 A	10/1990	Gordon et al.
4,480,886 A	11/1984	Bergamin	4,961,711 A	10/1990	Fujiura et al.
4,481,804 A	11/1984	Eberhard et al.	4,964,408 A	10/1990	Hink et al.
4,490,003 A	12/1984	Robinson	4,974,591 A	12/1990	Awazu et al.
4,498,722 A	2/1985	Fedder et al.	4,996,975 A	3/1991	Nakamura
4,505,848 A	3/1985	Kobayashi	5,007,704 A	4/1991	McCartney
4,528,986 A	7/1985	Arundel et al.	RE33,643 E	7/1991	Isaacson et al.
4,531,795 A	7/1985	Sinclair	5,031,608 A	7/1991	Weinstein
4,580,867 A	4/1986	Wright et al.	5,041,187 A	8/1991	Hink et al.
4,621,643 A	11/1986	New, Jr. et al.	5,058,098 A	10/1991	Sakaue et al.
4,636,786 A	1/1987	Haertling	5,058,588 A	10/1991	Kaestle
4,642,627 A	2/1987	Hodsdon	5,066,859 A	11/1991	Karkar et al.
4,653,498 A	3/1987	New, Jr. et al.	5,069,213 A	12/1991	Polczynski
4,684,245 A	8/1987	Goldring	5,080,098 A	1/1992	Willett et al.
			5,086,229 A	2/1992	Rosenthal et al.
			5,087,242 A	2/1992	Petelenz et al.
			5,090,410 A	2/1992	Saper et al.
			5,099,842 A	3/1992	Mannheimer et al.
			5,108,298 A	4/1992	Simmel
			5,109,848 A	5/1992	Thomas et al.
			5,109,849 A	5/1992	Goodman et al.
			5,113,862 A	5/1992	Mortazavi
			5,125,403 A	6/1992	Culp
			5,140,228 A	8/1992	Biegel
			5,163,438 A	11/1992	Gordon et al.
			5,170,786 A	12/1992	Thomas et al.
			5,188,098 A	2/1993	Hoffman et al.
			5,209,230 A	5/1993	Swedlow et al.
			5,217,013 A	6/1993	Lewis et al.
			5,224,478 A	7/1993	Sakai et al.
			5,224,882 A	7/1993	Olms
			5,246,003 A	9/1993	DeLonzor
			5,247,931 A	9/1993	Norwood
			5,249,576 A	10/1993	Goldberger et al.
			5,266,792 A	11/1993	Crowne et al.
			5,267,562 A	12/1993	Ukawa et al.
			5,287,853 A	2/1994	Vester et al.
			5,295,852 A	3/1994	Renn et al.
			5,295,872 A	3/1994	Christensson
			5,302,133 A	4/1994	Tondreault
			5,308,919 A	5/1994	Minnich
			5,309,908 A	5/1994	Friedman et al.
			5,313,940 A	5/1994	Fuse et al.
			5,317,269 A	5/1994	Mills et al.
			5,319,355 A	6/1994	Russek
			5,337,744 A	8/1994	Branigan
			5,339,810 A	8/1994	Ivers et al.
			5,341,805 A	8/1994	Stavridi et al.
			5,365,937 A	11/1994	Reeves et al.
			D353,195 S	12/1994	Savage et al.
			D353,196 S	12/1994	Savage et al.
			5,377,676 A	1/1995	Vari et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

5,380,213 A	1/1995	Piorunneck et al.	5,934,925 A	8/1999	Tobler et al.
5,387,122 A	2/1995	Goldberger et al.	5,939,609 A	8/1999	Knapp et al.
5,390,670 A	2/1995	Centa et al.	5,940,182 A	8/1999	Lepper, Jr. et al.
5,397,247 A	3/1995	Aoki et al.	5,957,885 A	9/1999	Bollish et al.
5,400,267 A	3/1995	Denen et al.	5,970,353 A	10/1999	Sultan
5,407,368 A	4/1995	Strand et al.	5,987,343 A	11/1999	Kinast
5,415,629 A	5/1995	Henley	5,991,355 A	11/1999	Dahlke
D359,546 S	6/1995	Savage et al.	5,995,855 A	11/1999	Kiani et al.
5,422,632 A	6/1995	Bucholtz et al.	5,997,343 A	12/1999	Mills et al.
5,425,375 A	6/1995	Chin et al.	6,002,952 A	12/1999	Diab et al.
5,431,170 A	7/1995	Mathews	6,011,986 A	1/2000	Diab et al.
D361,840 S	8/1995	Savage et al.	6,027,452 A	2/2000	Flaherty et al.
5,438,986 A	8/1995	Disch et al.	6,036,642 A	3/2000	Diab et al.
D362,063 S	9/1995	Savage et al.	6,045,509 A	4/2000	Caro et al.
5,452,717 A	9/1995	Branigan et al.	6,067,462 A	5/2000	Diab et al.
D363,120 S	10/1995	Savage et al.	6,081,735 A	6/2000	Diab et al.
5,456,252 A	10/1995	Vari et al.	6,088,607 A	7/2000	Diab et al.
5,469,845 A	11/1995	DeLonzor et al.	6,110,522 A	8/2000	Lepper, Jr. et al.
5,479,934 A	1/1996	Imran	6,124,597 A	9/2000	Shehada
5,482,036 A	1/1996	Diab et al.	6,128,521 A	10/2000	Marro et al.
5,490,505 A	2/1996	Diab et al.	6,129,675 A	10/2000	Jay
5,490,523 A	2/1996	Isaacson et al.	6,144,868 A	11/2000	Parker
5,494,043 A	2/1996	O'Sullivan et al.	6,151,516 A	11/2000	Kiani-Azarbayjany et al.
5,498,235 A	3/1996	Flower	6,152,754 A	11/2000	Gerhardt et al.
5,509,823 A	4/1996	Harting et al.	6,157,850 A	12/2000	Diab et al.
5,515,169 A	5/1996	Cargill et al.	6,165,005 A	12/2000	Mills et al.
5,520,177 A	5/1996	Ogawa et al.	6,174,283 B1	1/2001	Nevo
5,521,997 A	5/1996	Rovenolt et al.	6,184,521 B1	2/2001	Coffin, IV et al.
5,533,509 A	7/1996	Koashi et al.	6,206,830 B1	3/2001	Diab et al.
5,533,511 A	7/1996	Kaspari et al.	6,223,064 B1	4/2001	Lynn et al.
5,534,851 A	7/1996	Russek	6,229,856 B1	5/2001	Diab et al.
5,561,275 A	10/1996	Savage et al.	6,232,609 B1	5/2001	Snyder et al.
5,562,002 A	10/1996	Lalin	6,236,872 B1	5/2001	Diab et al.
5,564,417 A	10/1996	Chance	6,241,683 B1	6/2001	Macklem et al.
5,569,823 A	10/1996	Schreier et al.	6,253,097 B1	6/2001	Aronow et al.
5,570,002 A	10/1996	Castleman	6,256,523 B1	7/2001	Diab et al.
5,584,296 A	12/1996	Cui et al.	6,263,222 B1	7/2001	Diab et al.
5,588,427 A	12/1996	Tien	6,278,522 B1	8/2001	Lepper, Jr. et al.
5,590,649 A	1/1997	Caro et al.	6,280,213 B1	8/2001	Tobler et al.
5,602,924 A	2/1997	Durand et al.	6,285,896 B1	9/2001	Tobler et al.
5,617,857 A	4/1997	Chader et al.	6,301,493 B1	10/2001	Marro et al.
5,632,272 A	5/1997	Diab et al.	6,308,089 B1	10/2001	von der Ruhr et al.
5,638,816 A	6/1997	Kiani-Azarbayjany et al.	6,317,627 B1	11/2001	Ennen et al.
5,638,818 A	6/1997	Diab et al.	6,321,100 B1	11/2001	Parker
5,645,440 A	7/1997	Tobler et al.	6,325,761 B1	12/2001	Jay
5,660,567 A	8/1997	Nierlich et al.	6,330,468 B1	12/2001	Scharf
5,685,299 A	11/1997	Diab et al.	6,334,065 B1	12/2001	Al-Ali et al.
5,692,503 A	12/1997	Kuenstner	6,343,224 B1	1/2002	Parker
5,720,293 A	2/1998	Quinn et al.	6,349,228 B1	2/2002	Kiani et al.
D393,830 S	4/1998	Tobler et al.	6,360,114 B1	3/2002	Diab et al.
5,743,262 A	4/1998	Lepper, Jr. et al.	6,368,283 B1	4/2002	Xu et al.
5,758,644 A	6/1998	Diab et al.	6,371,921 B1	4/2002	Caro et al.
5,760,910 A	6/1998	Lepper, Jr. et al.	6,377,829 B1	4/2002	Al-Ali
5,769,785 A	6/1998	Diab et al.	6,388,240 B2	5/2002	Schulz et al.
5,779,630 A	7/1998	Fein et al.	6,397,091 B2	5/2002	Diab et al.
5,782,757 A	7/1998	Diab et al.	6,430,437 B1	8/2002	Marro
5,785,659 A	7/1998	Caro et al.	6,430,525 B1	8/2002	Weber et al.
5,791,347 A	8/1998	Flaherty et al.	6,433,696 B1	8/2002	Deiterman et al.
5,803,909 A	9/1998	Maki et al.	6,463,142 B1	10/2002	Kilp
5,807,247 A	9/1998	Mechant et al.	6,463,311 B1	10/2002	Diab
5,807,248 A	9/1998	Mills	6,470,199 B1	10/2002	Kopotic et al.
5,810,724 A	9/1998	Gronvall	6,473,632 B1	10/2002	Myers
5,810,734 A	9/1998	Caro et al.	6,501,975 B2	12/2002	Diab et al.
5,817,010 A	10/1998	Hibl	6,505,059 B1	1/2003	Kollias et al.
5,818,985 A	10/1998	Merchant et al.	6,515,273 B2	2/2003	Al-Ali
5,823,950 A	10/1998	Diab et al.	6,519,487 B1	2/2003	Parker
5,830,129 A	11/1998	Baer et al.	6,525,386 B1	2/2003	Mills et al.
5,830,131 A	11/1998	Caro et al.	6,526,300 B1	2/2003	Kiani et al.
5,833,618 A	11/1998	Caro et al.	6,541,756 B2	4/2003	Schulz et al.
5,860,919 A	1/1999	Kiani-Azarbayjany et al.	6,542,764 B1	4/2003	Al-Ali et al.
5,890,929 A	4/1999	Mills et al.	6,553,241 B2	4/2003	Mannheimer et al.
5,895,369 A	4/1999	Flower	6,580,086 B1	6/2003	Schulz et al.
5,904,654 A	5/1999	Wohlmann et al.	6,584,336 B1	6/2003	Ali et al.
5,919,133 A	7/1999	Taylor et al.	6,595,316 B2	7/2003	Cybulski et al.
5,919,134 A	7/1999	Diab	6,597,932 B2	7/2003	Tian et al.
			6,597,933 B2	7/2003	Kiani et al.
			6,606,511 B1	8/2003	Ali et al.
			6,611,320 B1	8/2003	Lindberg et al.
			6,632,181 B2	10/2003	Flaherty et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

6,639,668	B1	10/2003	Trepagnier	RE39,672	E	6/2007	Shehada et al.
6,640,116	B2	10/2003	Diab	7,239,905	B2	7/2007	Kiani-Azarbayjany et al.
6,643,530	B2	11/2003	Diab et al.	7,241,270	B2	7/2007	Horzewski et al.
6,650,917	B2	11/2003	Diab et al.	7,245,953	B1	7/2007	Parker
6,654,624	B2	11/2003	Diab et al.	7,248,910	B2	7/2007	Li et al.
6,658,276	B2	12/2003	Kiani et al.	7,254,429	B2	8/2007	Schurman et al.
6,661,161	B1	12/2003	Lanzo et al.	7,254,431	B2	8/2007	Al-Ali
6,671,531	B2	12/2003	Al-Ali et al.	7,254,433	B2	8/2007	Diab et al.
6,678,543	B2	1/2004	Diab et al.	7,254,434	B2	8/2007	Schulz et al.
6,684,090	B2	1/2004	Ali et al.	7,272,425	B2	9/2007	Al-Ali
6,684,091	B2	1/2004	Parker	7,274,955	B2	9/2007	Kiani et al.
6,697,656	B1	2/2004	Al-Ali	D554,263	S	10/2007	Al-Ali
6,697,657	B1	2/2004	Shehada et al.	7,280,858	B2	10/2007	Al-Ali et al.
6,697,658	B2	2/2004	Al-Ali	7,289,835	B2	10/2007	Mansfield et al.
RE38,476	E	3/2004	Diab et al.	7,292,883	B2	11/2007	De Felice et al.
6,699,194	B1	3/2004	Diab et al.	7,295,866	B2	11/2007	Al-Ali
6,714,804	B2	3/2004	Al-Ali et al.	7,319,894	B2	1/2008	Higgins
RE38,492	E	4/2004	Diab et al.	7,328,053	B1	2/2008	Diab et al.
6,721,582	B2	4/2004	Trepagnier et al.	7,332,784	B2	2/2008	Mills et al.
6,721,585	B1	4/2004	Parker	7,340,287	B2	3/2008	Mason et al.
6,725,075	B2	4/2004	Al-Ali	7,341,559	B2	3/2008	Schulz et al.
6,728,560	B2	4/2004	Kollias et al.	7,343,186	B2	3/2008	Lamego et al.
6,735,459	B2	5/2004	Parker	D566,282	S	4/2008	Al-Ali et al.
6,745,060	B2	6/2004	Diab et al.	7,355,512	B1	4/2008	Al-Ali
6,760,607	B2	7/2004	Al-Ali	7,356,365	B2	4/2008	Schurman
6,770,028	B1	8/2004	Ali et al.	7,371,981	B2	5/2008	Abdul-Hafiz
6,771,994	B2	8/2004	Kiani et al.	7,373,193	B2	5/2008	Al-Ali et al.
6,792,300	B1	9/2004	Diab et al.	7,373,194	B2	5/2008	Weber et al.
6,813,511	B2	11/2004	Diab et al.	7,376,453	B1	5/2008	Diab et al.
6,816,741	B2	11/2004	Diab	7,377,794	B2	5/2008	Al Ali et al.
6,822,564	B2	11/2004	Al-Ali	7,377,899	B2	5/2008	Weber et al.
6,826,419	B2	11/2004	Diab et al.	7,383,070	B2	6/2008	Diab et al.
6,830,711	B2	12/2004	Mills et al.	7,415,297	B2	8/2008	Al-Ali et al.
6,850,787	B2	2/2005	Weber et al.	7,428,432	B2	9/2008	Ali et al.
6,850,788	B2	2/2005	Al-Ali	7,438,683	B2	10/2008	Al-Ali et al.
6,852,083	B2	2/2005	Caro et al.	7,440,787	B2	10/2008	Diab
6,861,639	B2	3/2005	Al-Ali	7,454,240	B2	11/2008	Diab et al.
6,898,452	B2	5/2005	Al-Ali et al.	7,467,002	B2	12/2008	Weber et al.
6,920,345	B2	7/2005	Al-Ali et al.	7,469,157	B2	12/2008	Diab et al.
6,931,268	B1	8/2005	Kiani-Azarbayjany et al.	7,471,969	B2	12/2008	Diab et al.
6,934,570	B2	8/2005	Kiani et al.	7,471,971	B2	12/2008	Diab et al.
6,939,305	B2	9/2005	Flaherty et al.	7,483,729	B2	1/2009	Al-Ali et al.
6,943,348	B1	9/2005	Coffin, IV	7,483,730	B2	1/2009	Diab et al.
6,950,687	B2	9/2005	Al-Ali	7,483,731	B2	1/2009	Hoarau et al.
6,961,598	B2	11/2005	Diab	7,489,958	B2	2/2009	Diab et al.
6,970,792	B1	11/2005	Diab	7,496,391	B2	2/2009	Diab et al.
6,979,812	B2	12/2005	Al-Ali	7,496,393	B2	2/2009	Diab et al.
6,985,764	B2	1/2006	Mason et al.	D587,657	S	3/2009	Al-Ali et al.
6,993,371	B2	1/2006	Kiani et al.	7,499,741	B2	3/2009	Diab et al.
6,996,427	B2	2/2006	Ali et al.	7,499,835	B2	3/2009	Weber et al.
6,997,879	B1	2/2006	Turcott	7,500,950	B2	3/2009	Al-Ali et al.
6,999,904	B2	2/2006	Weber et al.	7,509,154	B2	3/2009	Diab et al.
7,003,338	B2	2/2006	Weber et al.	7,509,494	B2	3/2009	Al-Ali
7,003,339	B2	2/2006	Diab et al.	7,510,849	B2	3/2009	Schurman et al.
7,015,451	B2	3/2006	Dalke et al.	7,526,328	B2	4/2009	Diab et al.
7,024,233	B2	4/2006	Ali et al.	7,530,942	B1	5/2009	Diab
7,027,849	B2	4/2006	Al-Ali	7,530,949	B2	5/2009	Al Ali et al.
7,030,749	B2	4/2006	Al-Ali	7,530,955	B2	5/2009	Diab et al.
7,039,449	B2	5/2006	Al-Ali	7,563,110	B2	7/2009	Al-Ali et al.
7,041,060	B2	5/2006	Flaherty et al.	7,596,398	B2	9/2009	Al-Ali et al.
7,044,918	B2	5/2006	Diab	7,618,375	B2	11/2009	Flaherty
7,048,687	B1	5/2006	Reuss et al.	D606,659	S	12/2009	Kiani et al.
7,067,893	B2	6/2006	Mills et al.	7,647,083	B2	1/2010	Al-Ali et al.
7,096,052	B2	8/2006	Mason et al.	D609,193	S	2/2010	Al-Ali et al.
7,096,054	B2	8/2006	Abdul-Hafiz et al.	7,660,616	B1	2/2010	Poore
7,132,641	B2	11/2006	Schulz et al.	D614,305	S	4/2010	Al-Ali et al.
7,142,901	B2	11/2006	Kiani et al.	RE41,317	E	5/2010	Parker
7,149,561	B2	12/2006	Diab	7,729,733	B2	6/2010	Al-Ali et al.
7,186,966	B2	3/2007	Al-Ali	7,734,320	B2	6/2010	Al-Ali
7,190,261	B2	3/2007	Al-Ali	7,761,127	B2	7/2010	Al-Ali et al.
7,215,984	B2	5/2007	Diab	7,761,128	B2	7/2010	Al-Ali et al.
7,215,986	B2	5/2007	Diab	7,764,982	B2	7/2010	Dalke et al.
7,221,971	B2	5/2007	Diab	D621,516	S	8/2010	Kiani et al.
7,225,006	B2	5/2007	Al-Ali et al.	7,791,155	B2	9/2010	Diab
7,225,007	B2	5/2007	Al-Ali	7,801,581	B2	9/2010	Diab
				7,822,452	B2	10/2010	Schurman et al.
				RE41,912	E	11/2010	Parker
				7,844,313	B2	11/2010	Kiani et al.
				7,844,314	B2	11/2010	Al-Ali

(56)

## References Cited

## U.S. PATENT DOCUMENTS

7,844,315 B2	11/2010	Al-Ali		8,346,330 B2	1/2013	Lamego
7,848,798 B2 *	12/2010	Martinsen	..... A61B 5/0531	8,353,842 B2	1/2013	Al-Ali et al.
			600/547	8,355,766 B2	1/2013	MacNeish, III et al.
7,865,222 B2	1/2011	Weber et al.		8,359,080 B2	1/2013	Diab et al.
7,873,497 B2	1/2011	Weber et al.		8,364,223 B2	1/2013	Al-Ali et al.
7,880,606 B2	2/2011	Al-Ali		8,364,226 B2	1/2013	Diab et al.
7,880,626 B2	2/2011	Al-Ali et al.		8,374,665 B2	2/2013	Lamego
7,891,355 B2	2/2011	Al-Ali et al.		8,385,995 B2	2/2013	Al-Ali et al.
7,894,868 B2	2/2011	Al-Ali et al.		8,385,996 B2	2/2013	Smith et al.
7,899,507 B2	3/2011	Al-Ali et al.		8,388,353 B2	3/2013	Kiani et al.
7,899,518 B2	3/2011	Trepagnier et al.		8,399,822 B2	3/2013	Al-Ali
7,904,132 B2	3/2011	Weber et al.		8,401,602 B2	3/2013	Kiani
7,909,772 B2	3/2011	Popov et al.		8,405,608 B2	3/2013	Al-Ali et al.
7,910,875 B2	3/2011	Al-Ali		8,414,499 B2	4/2013	Al-Ali et al.
7,919,713 B2	4/2011	Al-Ali et al.		8,418,524 B2	4/2013	Al-Ali
7,937,128 B2	5/2011	Al-Ali		8,423,106 B2	4/2013	Lamego et al.
7,937,129 B2	5/2011	Mason et al.		8,428,967 B2	4/2013	Olsen et al.
7,937,130 B2	5/2011	Diab et al.		8,430,817 B1	4/2013	Al-Ali et al.
7,941,199 B2	5/2011	Kiani		8,437,825 B2	5/2013	Dalvi et al.
7,951,086 B2	5/2011	Flaherty et al.		8,455,290 B2	6/2013	Siskavich
7,957,780 B2	6/2011	Lamego et al.		8,457,703 B2	6/2013	Al-Ali
7,962,188 B2	6/2011	Kiani et al.		8,457,707 B2	6/2013	Kiani
7,962,190 B1	6/2011	Diab et al.		8,463,349 B2	6/2013	Diab et al.
7,976,472 B2	7/2011	Kiani		8,466,286 B2	6/2013	Bellot et al.
7,988,637 B2	8/2011	Diab		8,471,713 B2	6/2013	Poeze et al.
7,990,382 B2	8/2011	Kiani		8,473,020 B2	6/2013	Kiani et al.
7,991,446 B2	8/2011	Al-Ali et al.		8,483,787 B2	7/2013	Al-Ali et al.
8,000,761 B2	8/2011	Al-Ali		8,489,364 B2	7/2013	Weber et al.
8,008,088 B2	8/2011	Bellott et al.		8,498,684 B2	7/2013	Weber et al.
RE42,753 E	9/2011	Kiani-Azarbayjany et al.		8,504,128 B2	8/2013	Blank et al.
8,019,400 B2	9/2011	Diab et al.		8,509,867 B2	8/2013	Workman et al.
8,028,701 B2	10/2011	Al-Ali et al.		8,515,509 B2	8/2013	Bruinsma et al.
8,029,765 B2	10/2011	Bellott et al.		8,523,781 B2	9/2013	Al-Ali
8,036,727 B2	10/2011	Schurman et al.		8,529,301 B2	9/2013	Al-Ali et al.
8,036,728 B2	10/2011	Diab et al.		8,532,727 B2	9/2013	Ali et al.
8,046,040 B2	10/2011	Ali et al.		8,532,728 B2	9/2013	Diab et al.
8,046,041 B2	10/2011	Diab et al.		D692,145 S	10/2013	Al-Ali et al.
8,046,042 B2	10/2011	Diab et al.		8,547,209 B2	10/2013	Kiani et al.
8,048,040 B2	11/2011	Kiani		8,548,548 B2	10/2013	Al-Ali
8,050,728 B2	11/2011	Al-Ali et al.		8,548,549 B2	10/2013	Schurman et al.
RE43,169 E	2/2012	Parker		8,548,550 B2	10/2013	Al-Ali et al.
8,118,620 B2	2/2012	Al-Ali et al.		8,560,032 B2	10/2013	Al-Ali et al.
8,126,528 B2	2/2012	Diab et al.		8,560,034 B1	10/2013	Diab et al.
8,128,572 B2	3/2012	Diab et al.		8,570,167 B2	10/2013	Al-Ali
8,130,105 B2	3/2012	Al-Ali et al.		8,570,503 B2	10/2013	Vo et al.
8,145,287 B2	3/2012	Diab et al.		8,571,617 B2	10/2013	Reichgott et al.
8,150,487 B2	4/2012	Diab et al.		8,571,618 B1	10/2013	Lamego et al.
8,175,672 B2	5/2012	Parker		8,571,619 B2	10/2013	Al-Ali et al.
8,180,420 B2	5/2012	Diab et al.		8,577,431 B2	11/2013	Lamego et al.
8,182,443 B1	5/2012	Kiani		8,581,732 B2	11/2013	Al-Ali et al.
8,185,180 B2	5/2012	Diab et al.		8,584,345 B2	11/2013	Al-Ali et al.
8,190,223 B2	5/2012	Al-Ali et al.		8,588,880 B2	11/2013	Abdul-Hafiz et al.
8,190,227 B2	5/2012	Diab et al.		8,600,467 B2	12/2013	Al-Ali et al.
8,203,438 B2	6/2012	Kiani et al.		8,606,342 B2	12/2013	Diab
8,203,704 B2	6/2012	Merritt et al.		8,626,255 B2	1/2014	Al-Ali et al.
8,204,566 B2	6/2012	Schurman et al.		8,630,691 B2	1/2014	Lamego et al.
8,219,172 B2	7/2012	Schurman et al.		8,634,889 B2	1/2014	Al-Ali et al.
8,224,411 B2	7/2012	Al-Ali et al.		8,641,631 B2	2/2014	Sierra et al.
8,228,181 B2	7/2012	Al-Ali		8,652,060 B2	2/2014	Al-Ali
8,229,533 B2	7/2012	Diab et al.		8,663,107 B2	3/2014	Kiani
8,233,955 B2	7/2012	Al-Ali et al.		8,666,468 B1	3/2014	Al-Ali
8,244,325 B2	8/2012	Al-Ali et al.		8,667,967 B2	3/2014	Al-Ali et al.
8,255,026 B1	8/2012	Al-Ali		8,670,811 B2	3/2014	O'Reilly
8,255,027 B2	8/2012	Al-Ali et al.		8,670,814 B2	3/2014	Diab et al.
8,255,028 B2	8/2012	Al-Ali et al.		8,676,286 B2	3/2014	Weber et al.
8,260,577 B2	9/2012	Weber et al.		8,682,407 B2	3/2014	Al-Ali
8,265,723 B1	9/2012	McHale et al.		RE44,823 E	4/2014	Parker
8,274,360 B2	9/2012	Sampath et al.		RE44,875 E	4/2014	Kiani et al.
8,280,473 B2	10/2012	Al-Ali		8,690,799 B2	4/2014	Telfort et al.
8,301,217 B2	10/2012	Al-Ali et al.		8,700,112 B2	4/2014	Kiani
8,306,596 B2	11/2012	Schurman et al.		8,702,627 B2	4/2014	Telfort et al.
8,310,336 B2	11/2012	Muhsin et al.		8,706,179 B2	4/2014	Parker
8,315,683 B2	11/2012	Al-Ali et al.		8,712,494 B1	4/2014	MacNeish, III et al.
RE43,860 E	12/2012	Parker		8,715,206 B2	5/2014	Telfort et al.
8,337,403 B2	12/2012	Al-Ali et al.		8,718,735 B2	5/2014	Lamego et al.
				8,718,737 B2	5/2014	Diab et al.
				8,718,738 B2	5/2014	Blank et al.
				8,720,249 B2	5/2014	Al-Ali
				8,721,541 B2	5/2014	Al-Ali et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

8,721,542	B2	5/2014	Al-Ali et al.	9,161,696	B2	10/2015	Al-Ali et al.
8,723,677	B1	5/2014	Kiani	9,161,713	B2	10/2015	Al-Ali et al.
8,740,792	B1	6/2014	Kiani et al.	9,167,995	B2	10/2015	Lamego et al.
8,754,776	B2	6/2014	Poeze et al.	9,176,141	B2	11/2015	Al-Ali et al.
8,755,535	B2	6/2014	Telfort et al.	9,186,102	B2	11/2015	Bruinsma et al.
8,755,856	B2	6/2014	Diab et al.	9,192,312	B2	11/2015	Al-Ali
8,755,872	B1	6/2014	Marinow	9,192,329	B2	11/2015	Al-Ali
8,761,850	B2	6/2014	Lamego	9,192,351	B1	11/2015	Telfort et al.
8,764,671	B2	7/2014	Kiani	9,195,385	B2	11/2015	Al-Ali et al.
8,768,423	B2	7/2014	Shakespeare et al.	9,211,072	B2	12/2015	Kiani
8,771,204	B2	7/2014	Telfort et al.	9,211,095	B1	12/2015	Al-Ali
8,777,634	B2	7/2014	Kiani et al.	9,218,454	B2	12/2015	Kiani et al.
8,781,543	B2	7/2014	Diab et al.	9,226,696	B2	1/2016	Kiani
8,781,544	B2	7/2014	Al-Ali et al.	9,241,662	B2	1/2016	Al-Ali et al.
8,781,549	B2	7/2014	Al-Ali et al.	9,245,668	B1	1/2016	Vo et al.
8,788,003	B2	7/2014	Schurman et al.	9,259,185	B2	2/2016	Abdul-Hafiz et al.
8,790,268	B2	7/2014	Al-Ali	9,267,572	B2	2/2016	Barker et al.
8,801,613	B2	8/2014	Al-Ali et al.	9,277,880	B2	3/2016	Poeze et al.
8,821,397	B2	9/2014	Al-Ali et al.	9,289,167	B2	3/2016	Diab et al.
8,821,415	B2	9/2014	Al-Ali et al.	9,295,421	B2	3/2016	Kiani et al.
8,830,449	B1	9/2014	Lamego et al.	9,307,928	B1	4/2016	Al-Ali et al.
8,831,700	B2	9/2014	Schurman et al.	9,323,894	B2	4/2016	Kiani
8,840,549	B2	9/2014	Al-Ali et al.	D755,392	S	5/2016	Hwang et al.
8,847,740	B2	9/2014	Kiani et al.	9,326,712	B1	5/2016	Kiani
8,849,365	B2	9/2014	Smith et al.	9,333,316	B2	5/2016	Kiani
8,852,094	B2	10/2014	Al-Ali et al.	9,339,220	B2	5/2016	Lamego et al.
8,852,994	B2	10/2014	Wojtczuk et al.	9,341,565	B2	5/2016	Lamego et al.
8,868,147	B2	10/2014	Stippick et al.	9,351,673	B2	5/2016	Diab et al.
8,868,150	B2	10/2014	Al-Ali et al.	9,351,675	B2	5/2016	Al-Ali et al.
8,870,792	B2	10/2014	Al-Ali et al.	9,364,181	B2	6/2016	Kiani et al.
8,886,271	B2	11/2014	Kiani et al.	9,368,671	B2	6/2016	Wojtczuk et al.
8,888,539	B2	11/2014	Al-Ali et al.	9,370,325	B2	6/2016	Al-Ali et al.
8,888,708	B2	11/2014	Diab et al.	9,370,326	B2	6/2016	McHale et al.
8,892,180	B2	11/2014	Weber et al.	9,370,335	B2	6/2016	Al-Ali et al.
8,897,847	B2	11/2014	Al-Ali	9,375,185	B2	6/2016	Ali et al.
8,909,310	B2	12/2014	Lamego et al.	9,386,953	B2	7/2016	Al-Ali
8,911,377	B2	12/2014	Al-Ali	9,386,961	B2	7/2016	Al-Ali et al.
8,912,909	B2	12/2014	Al-Ali et al.	9,392,945	B2	7/2016	Al-Ali et al.
8,920,317	B2	12/2014	Al-Ali et al.	9,397,448	B2	7/2016	Al-Ali et al.
8,921,699	B2	12/2014	Al-Ali et al.	9,408,542	B1	8/2016	Kinast et al.
8,922,382	B2	12/2014	Al-Ali et al.	9,436,645	B2	9/2016	Al-Ali et al.
8,929,964	B2	1/2015	Al-Ali et al.	9,445,759	B1	9/2016	Lamego et al.
8,942,777	B2	1/2015	Diab et al.	9,466,919	B2	10/2016	Kiani et al.
8,948,834	B2	2/2015	Diab et al.	9,474,474	B2	10/2016	Lamego et al.
8,948,835	B2	2/2015	Diab	9,480,422	B2	11/2016	Al-Ali
8,965,471	B2	2/2015	Lamego	9,480,435	B2	11/2016	Olsen
8,983,564	B2	3/2015	Al-Ali	9,492,110	B2	11/2016	Al-Ali et al.
8,989,831	B2	3/2015	Al-Ali et al.	9,510,779	B2	12/2016	Poeze et al.
8,996,085	B2	3/2015	Kiani et al.	9,517,024	B2	12/2016	Kiani et al.
8,998,809	B2	4/2015	Kiani	9,532,722	B2	1/2017	Lamego et al.
9,028,429	B2	5/2015	Telfort et al.	9,538,949	B2	1/2017	Al-Ali et al.
9,037,207	B2	5/2015	Al-Ali et al.	9,538,980	B2	1/2017	Telfort et al.
9,060,721	B2	6/2015	Reichgott et al.	9,549,696	B2	1/2017	Lamego et al.
9,066,666	B2	6/2015	Kiani	9,554,737	B2	1/2017	Schurman et al.
9,066,680	B1	6/2015	Al-Ali et al.	9,560,996	B2	2/2017	Kiani
9,072,474	B2	7/2015	Al-Ali et al.	9,560,998	B2	2/2017	Al-Ali et al.
9,078,560	B2	7/2015	Schurman et al.	9,566,019	B2	2/2017	Al-Ali et al.
9,084,569	B2	7/2015	Weber et al.	9,579,039	B2	2/2017	Jansen et al.
9,095,316	B2	8/2015	Welch et al.	9,591,975	B2	3/2017	Dalvi et al.
9,106,038	B2	8/2015	Telfort et al.	9,622,692	B2	4/2017	Lamego et al.
9,107,625	B2	8/2015	Telfort et al.	9,622,693	B2	4/2017	Diab
9,107,626	B2	8/2015	Al-Ali et al.	D788,312	S	5/2017	Al-Ali et al.
9,113,831	B2	8/2015	Al-Ali	9,636,055	B2	5/2017	Al-Ali et al.
9,113,832	B2	8/2015	Al-Ali	9,636,056	B2	5/2017	Al-Ali
9,119,595	B2	9/2015	Lamego	9,649,054	B2	5/2017	Lamego et al.
9,131,881	B2	9/2015	Diab et al.	9,662,052	B2	5/2017	Al-Ali et al.
9,131,882	B2	9/2015	Al-Ali et al.	9,668,679	B2	6/2017	Schurman et al.
9,131,883	B2	9/2015	Al-Ali	9,668,680	B2	6/2017	Bruinsma et al.
9,131,917	B2	9/2015	Telfort et al.	9,668,703	B2	6/2017	Al-Ali
9,138,180	B1	9/2015	Coverston et al.	9,675,286	B2	6/2017	Diab
9,138,182	B2	9/2015	Al-Ali et al.	9,687,160	B2	6/2017	Kiani
9,138,192	B2	9/2015	Weber et al.	9,693,719	B2	7/2017	Al-Ali et al.
9,142,117	B2	9/2015	Muhsin et al.	9,693,737	B2	7/2017	Al-Ali
9,153,112	B1	10/2015	Kiani et al.	9,697,928	B2	7/2017	Al-Ali et al.
9,153,121	B2	10/2015	Kiani et al.	9,717,425	B2	8/2017	Kiani et al.
				9,717,458	B2	8/2017	Lamego et al.
				9,724,016	B1	8/2017	Al-Ali et al.
				9,724,024	B2	8/2017	Al-Ali
				9,724,025	B1	8/2017	Kiani et al.

(56)

## References Cited

## U.S. PATENT DOCUMENTS

9,730,640 B2	8/2017	Diab et al.	2012/0209082 A1	8/2012	Al-Ali
9,743,887 B2	8/2017	Al-Ali et al.	2012/0209084 A1	8/2012	Olsen et al.
9,749,232 B2	8/2017	Sampath et al.	2012/0283524 A1	11/2012	Kiani et al.
9,750,442 B2	9/2017	Olsen	2012/0319816 A1	12/2012	Al-Ali
9,750,443 B2	9/2017	Smith et al.	2013/0023775 A1	1/2013	Lamego et al.
9,750,461 B1	9/2017	Telfort	2013/0041591 A1	2/2013	Lamego
9,775,545 B2	10/2017	Al-Ali et al.	2013/0060147 A1	3/2013	Welch et al.
9,775,546 B2	10/2017	Diab et al.	2013/0096405 A1	4/2013	Garfio
9,775,570 B2	10/2017	Al-Ali	2013/0096936 A1	4/2013	Sampath et al.
9,778,079 B1	10/2017	Al-Ali et al.	2013/0243021 A1	9/2013	Siskavich
9,782,077 B2	10/2017	Lamego et al.	2013/0253334 A1	9/2013	Al-Ali et al.
9,782,110 B2	10/2017	Kiani	2013/0296672 A1	11/2013	O'Neil et al.
9,787,568 B2	10/2017	Lamego et al.	2013/0296713 A1	11/2013	Al-Ali et al.
9,788,735 B2	10/2017	Al-Ali	2013/0324808 A1	12/2013	Al-Ali et al.
9,788,768 B2	10/2017	Al-Ali et al.	2013/0331660 A1	12/2013	Al-Ali et al.
9,795,300 B2	10/2017	Al-Ali	2014/0012100 A1	1/2014	Al-Ali et al.
9,795,310 B2	10/2017	Al-Ali	2014/0051953 A1	2/2014	Lamego et al.
9,795,358 B2	10/2017	Telfort et al.	2014/0081175 A1	3/2014	Telfort
9,795,739 B2	10/2017	Al-Ali et al.	2014/0120564 A1	5/2014	Workman et al.
9,801,556 B2	10/2017	Kiani	2014/0121482 A1	5/2014	Merritt et al.
9,801,588 B2	10/2017	Weber et al.	2014/0127137 A1	5/2014	Bellott et al.
9,808,188 B1	11/2017	Perea et al.	2014/0135588 A1	5/2014	Al-Ali et al.
9,814,418 B2	11/2017	Weber et al.	2014/0163344 A1	6/2014	Al-Ali
9,820,691 B2	11/2017	Kiani	2014/0163402 A1	6/2014	Lamego et al.
9,833,152 B2	12/2017	Kiani et al.	2014/0166076 A1	6/2014	Kiani et al.
9,833,180 B2	12/2017	Shakespeare et al.	2014/0171763 A1	6/2014	Diab
9,839,379 B2	12/2017	Al-Ali et al.	2014/0180038 A1	6/2014	Kiani
9,839,381 B1	12/2017	Weber et al.	2014/0180154 A1	6/2014	Sierra et al.
9,847,002 B2	12/2017	Kiani et al.	2014/0180160 A1	6/2014	Brown et al.
9,847,749 B2	12/2017	Kiani et al.	2014/0187973 A1	7/2014	Brown et al.
9,848,800 B1	12/2017	Lee et al.	2014/0213864 A1	7/2014	Abdul-Hafiz et al.
9,848,806 B2	12/2017	Al-Ali et al.	2014/0266790 A1	9/2014	Al-Ali et al.
9,848,807 B2	12/2017	Lamego	2014/0275808 A1	9/2014	Poeze et al.
9,861,298 B2	1/2018	Eckerbom et al.	2014/0275835 A1	9/2014	Lamego et al.
9,861,304 B2	1/2018	Al-Ali et al.	2014/0275871 A1	9/2014	Lamego et al.
9,861,305 B1	1/2018	Weber et al.	2014/0275872 A1	9/2014	Merritt et al.
9,867,578 B2	1/2018	Al-Ali et al.	2014/0276115 A1	9/2014	Dalvi et al.
9,872,623 B2	1/2018	Al-Ali	2014/0288400 A1	9/2014	Diab et al.
9,876,320 B2	1/2018	Coverston et al.	2014/0316217 A1	10/2014	Purdon et al.
9,877,650 B2	1/2018	Muhsin et al.	2014/0316218 A1	10/2014	Purdon et al.
9,877,686 B2	1/2018	Al-Ali et al.	2014/0316228 A1	10/2014	Blank et al.
9,891,079 B2	2/2018	Dalvi	2014/0323825 A1	10/2014	Al-Ali et al.
9,895,107 B2	2/2018	Al-Ali et al.	2014/0323897 A1	10/2014	Brown et al.
9,924,893 B2	3/2018	Schurman et al.	2014/0323898 A1	10/2014	Purdon et al.
9,924,897 B1	3/2018	Abdul-Hafiz	2014/0330092 A1	11/2014	Al-Ali et al.
2001/0045532 A1	11/2001	Schulz et al.	2014/0330098 A1	11/2014	Merritt et al.
2002/0013538 A1	1/2002	Teller	2014/0357966 A1	12/2014	Al-Ali et al.
2002/0095077 A1 *	7/2002	Swedlow ..... A61B 5/14551 600/323	2015/0005600 A1	1/2015	Blank et al.
2003/0111592 A1	6/2003	Al-Ali	2015/0011907 A1	1/2015	Purdon et al.
2004/0111013 A1 *	6/2004	Shen ..... A61B 5/0002 600/300	2015/0012231 A1	1/2015	Poeze et al.
2004/0267103 A1	12/2004	Li et al.	2015/0032029 A1	1/2015	Al-Ali et al.
2005/0221276 A1	10/2005	Rozakis et al.	2015/0038859 A1	2/2015	Dalvi et al.
2005/0234317 A1	10/2005	Kiani	2015/0080754 A1	3/2015	Purdon et al.
2006/0161054 A1	7/2006	Reuss et al.	2015/0087936 A1	3/2015	Al-Ali et al.
2006/0167351 A1	7/2006	Isaacson et al.	2015/0094546 A1	4/2015	Al-Ali
2006/0220897 A1	10/2006	Chan	2015/0097701 A1	4/2015	Al-Ali et al.
2007/0100222 A1 *	5/2007	Mastrototaro ..... A61B 5/01 600/365	2015/0099950 A1	4/2015	Al-Ali et al.
2007/0129622 A1 *	6/2007	Bourget ..... A61B 5/0002 600/382	2015/0099955 A1	4/2015	Al-Ali et al.
2007/0170073 A1	7/2007	Wang et al.	2015/0101844 A1	4/2015	Al-Ali et al.
2007/0282478 A1	12/2007	Al-Ali et al.	2015/0106121 A1	4/2015	Muhsin et al.
2009/0247984 A1	10/2009	Lamego et al.	2015/0112151 A1	4/2015	Muhsin et al.
2009/0275813 A1	11/2009	Davis	2015/0116076 A1	4/2015	Al-Ali et al.
2009/0275844 A1	11/2009	Al-Ali	2015/0157245 A1	6/2015	Al-Ali et al.
2010/0004518 A1	1/2010	Vo et al.	2015/0165312 A1	6/2015	Kiani
2010/0030040 A1	2/2010	Poeze et al.	2015/0196249 A1	7/2015	Brown et al.
2011/0082711 A1	4/2011	Poeze et al.	2015/0216459 A1	8/2015	Al-Ali et al.
2011/0105854 A1	5/2011	Kiani et al.	2015/0238722 A1	8/2015	Al-Ali
2011/0125060 A1	5/2011	Telfort et al.	2015/0245773 A1	9/2015	Lamego et al.
2011/0208015 A1	8/2011	Welch et al.	2015/0245794 A1	9/2015	Al-Ali
2011/0230733 A1	9/2011	Al-Ali	2015/0257689 A1	9/2015	Al-Ali et al.
2012/0165629 A1	6/2012	Merritt et al.	2015/0272514 A1	10/2015	Kiani et al.
			2015/0351697 A1	12/2015	Weber et al.
			2015/0359429 A1	12/2015	Al-Ali et al.
			2015/0366507 A1	12/2015	Blank
			2016/0029932 A1	2/2016	Al-Ali
			2016/0029933 A1	2/2016	Al-Ali et al.
			2016/0058347 A1	3/2016	Reichgott et al.
			2016/0066824 A1	3/2016	Al-Ali et al.
			2016/0081552 A1	3/2016	Wojtczuk et al.

(56)

## References Cited

## FOREIGN PATENT DOCUMENTS

## U.S. PATENT DOCUMENTS

2016/0095543 A1 4/2016 Telfort et al.  
 2016/0095548 A1 4/2016 Al-Ali et al.  
 2016/0103598 A1 4/2016 Al-Ali et al.  
 2016/0143548 A1 5/2016 Al-Ali  
 2016/0166182 A1 6/2016 Al-Ali et al.  
 2016/0166183 A1 6/2016 Poeze et al.  
 2016/0192869 A1 7/2016 Kiani et al.  
 2016/0196388 A1 7/2016 Lamego  
 2016/0197436 A1 7/2016 Barker et al.  
 2016/0213281 A1 7/2016 Eckerbom et al.  
 2016/0228043 A1 8/2016 O'Neil et al.  
 2016/0233632 A1 8/2016 Scruggs et al.  
 2016/0234944 A1 8/2016 Schmidt et al.  
 2016/0270735 A1 9/2016 Diab et al.  
 2016/0283665 A1 9/2016 Sampath et al.  
 2016/0287090 A1 10/2016 Al-Ali et al.  
 2016/0287786 A1 10/2016 Kiani  
 2016/0296169 A1 10/2016 McHale et al.  
 2016/0310052 A1 10/2016 Al-Ali et al.  
 2016/0314260 A1 10/2016 Kiani  
 2016/0324486 A1 11/2016 Al-Ali et al.  
 2016/0324488 A1 11/2016 Olsen  
 2016/0327984 A1 11/2016 Al-Ali et al.  
 2016/0328528 A1 11/2016 Al-Ali et al.  
 2016/0331332 A1 11/2016 Al-Ali  
 2016/0367173 A1 12/2016 Dalvi et al.  
 2017/0000394 A1 1/2017 Al-Ali et al.  
 2017/0007134 A1 1/2017 Al-Ali et al.  
 2017/0007198 A1 1/2017 Al-Ali et al.  
 2017/0014083 A1 1/2017 Diab et al.  
 2017/0014084 A1 1/2017 Al-Ali et al.  
 2017/0027456 A1 2/2017 Kinast et al.  
 2017/0042488 A1 2/2017 Muhsin  
 2017/0055851 A1 3/2017 Al-Ali  
 2017/0055882 A1 3/2017 Al-Ali et al.  
 2017/0055887 A1 3/2017 Al-Ali  
 2017/0055896 A1 3/2017 Al-Ali et al.  
 2017/0079594 A1 3/2017 Telfort et al.  
 2017/0086723 A1 3/2017 Al-Ali et al.  
 2017/0143281 A1 5/2017 Olsen  
 2017/0147774 A1 5/2017 Kiani  
 2017/0156620 A1 6/2017 Al-Ali et al.  
 2017/0173632 A1 6/2017 Al-Ali  
 2017/0187146 A1 6/2017 Kiani et al.  
 2017/0188919 A1 7/2017 Al-Ali et al.  
 2017/0196464 A1 7/2017 Jansen et al.  
 2017/0196470 A1 7/2017 Lamego et al.  
 2017/0202490 A1 7/2017 Al-Ali et al.  
 2017/0224262 A1 8/2017 Al-Ali  
 2017/0228516 A1 8/2017 Sampath et al.  
 2017/0245790 A1 8/2017 Al-Ali et al.  
 2017/0251974 A1 9/2017 Shreim et al.  
 2017/0251975 A1 9/2017 Shreim et al.  
 2017/0258403 A1 9/2017 Abdul-Hafiz et al.  
 2017/0311891 A1 11/2017 Kiani et al.  
 2017/0325728 A1 11/2017 Al-Ali et al.  
 2017/0332976 A1 11/2017 Al-Ali et al.  
 2017/0340293 A1 11/2017 Al-Ali et al.  
 2017/0360310 A1 12/2017 Kiani et al.  
 2017/0367632 A1 12/2017 Al-Ali et al.  
 2018/0008146 A1 1/2018 Al-Ali et al.  
 2018/0014752 A1 1/2018 Al-Ali et al.  
 2018/0028124 A1 2/2018 Al-Ali et al.  
 2018/0055385 A1 3/2018 Al-Ali  
 2018/0055390 A1 3/2018 Kiani et al.  
 2018/0055430 A1 3/2018 Diab et al.  
 2018/0064381 A1 3/2018 Shakespeare et al.  
 2018/0069776 A1 3/2018 Lamego et al.  
 2018/0103874 A1 4/2018 Lee et al.  
 2018/0116575 A1 5/2018 Perea et al.  
 2018/0125368 A1 5/2018 Lamego et al.  
 2018/0125430 A1 5/2018 Al-Ali et al.  
 2018/0130325 A1 5/2018 Kiani et al.  
 2018/0132769 A1 5/2018 Weber et al.  
 2018/0132770 A1 5/2018 Lamego

DE 3619442 12/1987  
 DE 3711272 5/1989  
 EP 0 013 278 7/1980  
 EP 0 019 278 B1 11/1980  
 EP 0 019 478 A2 11/1980  
 EP 0 074 428 3/1983  
 EP 0 262 779 4/1988  
 EP 0 329 196 8/1989  
 EP 0 104 772 B1 3/1990  
 EP 0 404 562 12/1990  
 EP 0 481 612 4/1992  
 EP 0 538 631 B1 4/1993  
 EP 0 745 348 12/1996  
 EP 0 832 598 4/1998  
 EP 0 576 560 B1 5/2000  
 EP 0 790 800 B1 8/2000  
 EP 1 424 036 6/2004  
 JP 52-031736 10/1977  
 JP S62-217938 9/1987  
 JP S 63-65844 3/1988  
 JP 02-17462 1/1990  
 JP 02-191434 7/1990  
 JP 03-245042 10/1991  
 JP 04-138342 5/1992  
 JP 04-250140 9/1992  
 JP H 04-312447 11/1992  
 JP 05-207993 8/1993  
 JP 05-275746 10/1993  
 JP 06-003890 1/1994  
 JP 06-237013 8/1994  
 JP 08-015023 1/1996  
 JP 08-315919 11/1996  
 JP 09-187442 7/1997  
 JP 11-156657 11/1997  
 JP 10-165420 6/1998  
 JP 63-50694 7/1998  
 JP 10-314149 12/1998  
 JP 11-053662 2/1999  
 JP 11-170568 6/1999  
 JP 11-185193 7/1999  
 JP 3135765 B2 2/2001  
 JP 2003-521985 7/2003  
 RU 2096985 11/1997  
 WO WO 92/01894 2/1992  
 WO WO 92/16142 10/1992  
 WO WO 96/13208 5/1996  
 WO WO 97/23159 7/1997  
 WO WO 97/29678 8/1997  
 WO WO 2001/13790 A1 3/2001  
 WO WO 2001/58347 A1 8/2001  
 WO WO 2002/17779 A1 3/2002  
 WO WO 2008/054976 A2 5/2008

## OTHER PUBLICATIONS

<http://www.masimo.com/systemo.htm>, "System Overview & Performance," 2 pages reviewed on Sep. 17, 1999.  
<http://www.masimo.com/pandt.htm>, "Products & Technology," 1 page reviewed on Sep. 17, 1999.  
<http://www.masimo.com/cables.htm>, "Patient Cables," 1 page reviewed on Sep. 17, 1999.  
<http://www.masimo.com/adf.htm>, "Inop-adf-Adult Disposable Digit Sensor," 1 page reviewed on Sep. 17, 1999.  
 International Search Report dated May 21, 2008 for International Application No. PCT/US2007/081146, filed Oct. 11, 2007, 6 pages.  
 International Preliminary Report on Patentability dated Nov. 26, 2008 for International Application No. PCT/US2007/081146, filed Oct. 11, 2007, 12 pages.  
 Reynolds, K.J., et al., Temperature Dependence of LED and its Theoretical Effect on Pulse Oximetry, British Journal & Anesthesia, 1991, vol. 67, pp. 638-643.  
 Schmitt, Joseph M., "Simple Photon Diffusion Analysis of the Effects of Multiple Scattering on Pulse Oximetry", IEEE Transactions on Biomedical Engineering, vol. 38, No. 12, Dec. 1991, pp. 1194-1203.



(56)

**References Cited**

OTHER PUBLICATIONS

Office Action dated May 21, 2010 issued in European Application No. 07868424.8, 4 pages.

Office Action dated Mar. 25, 2014 issued in European Application No. 07868424.8, 4 pages.

Oral Summons dated Mar. 23, 2016 issued in European Application No. 07868424.8, 4 pages.

Office Action dated Jan. 31, 2013 issued in Japanese Application No. 2009-532585, along with its English Translation, 6 pages.


Office Action dated Oct. 25, 2013 issued in Japanese Application No. 2009-532585, along with its English Translation, 10 pages.

Final Office Action dated Apr. 1, 2014 issued in Japanese Application No. 2009-532585, along with its English Translation, 6 pages.


Office Action dated Feb. 15, 2018 in corresponding Indian Application No. 2355/DELNP/2009 in 7 pages.


Office Action dated Feb. 15, 2018 in corresponding India Application No. 2355/DELNP/2009 in 7 pages.

\* cited by examiner

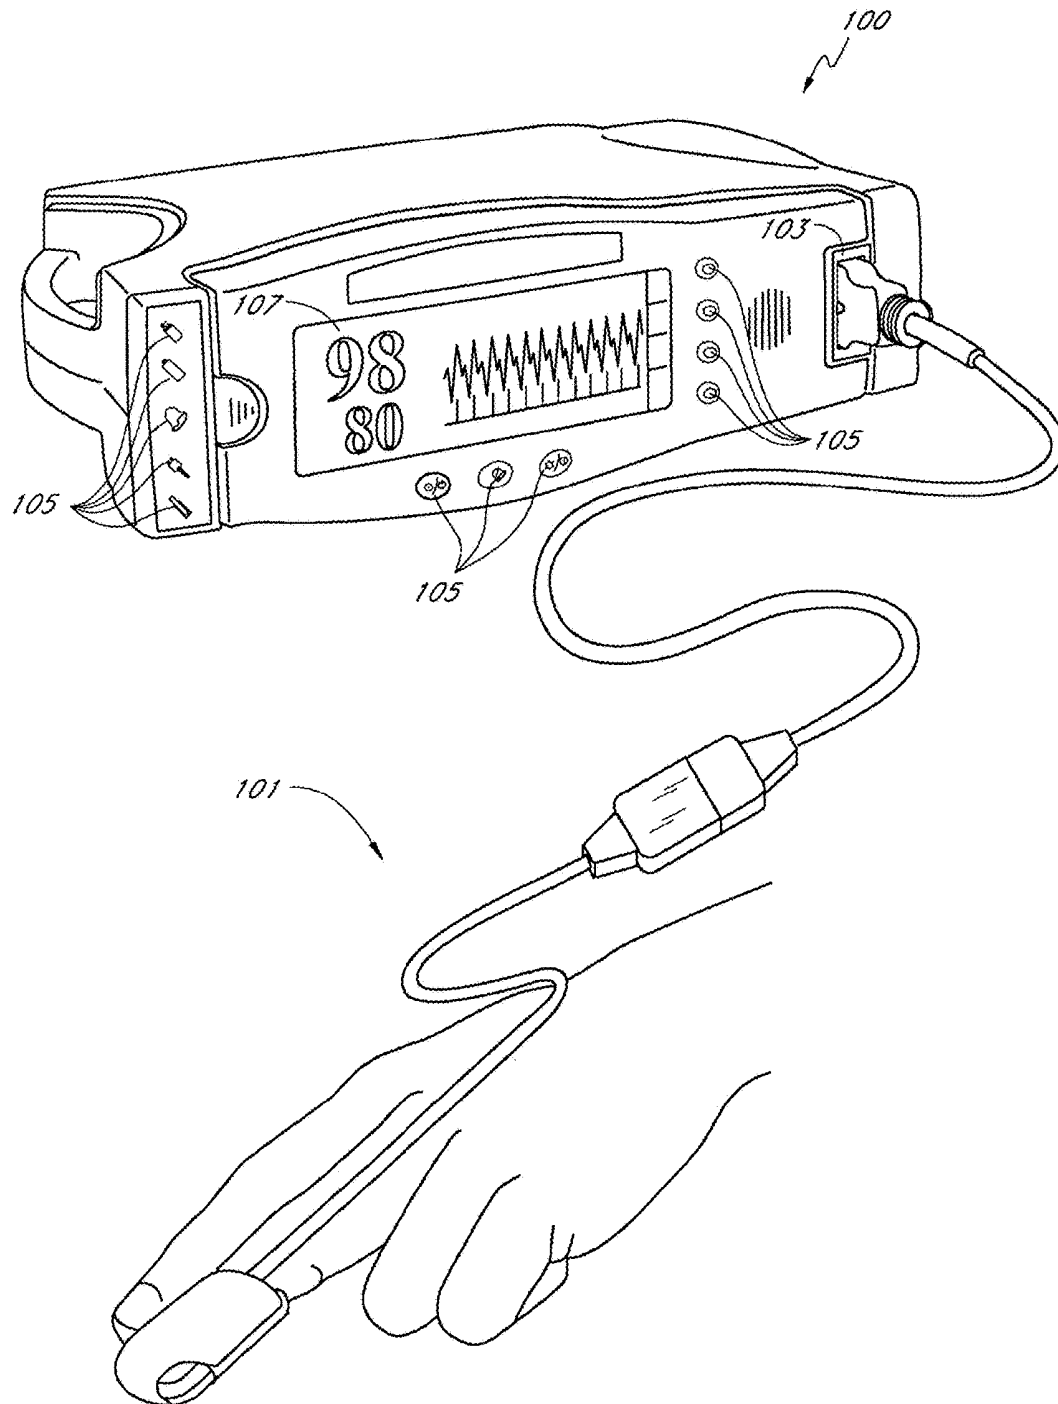


**FIG.1**  
(PRIOR ART)

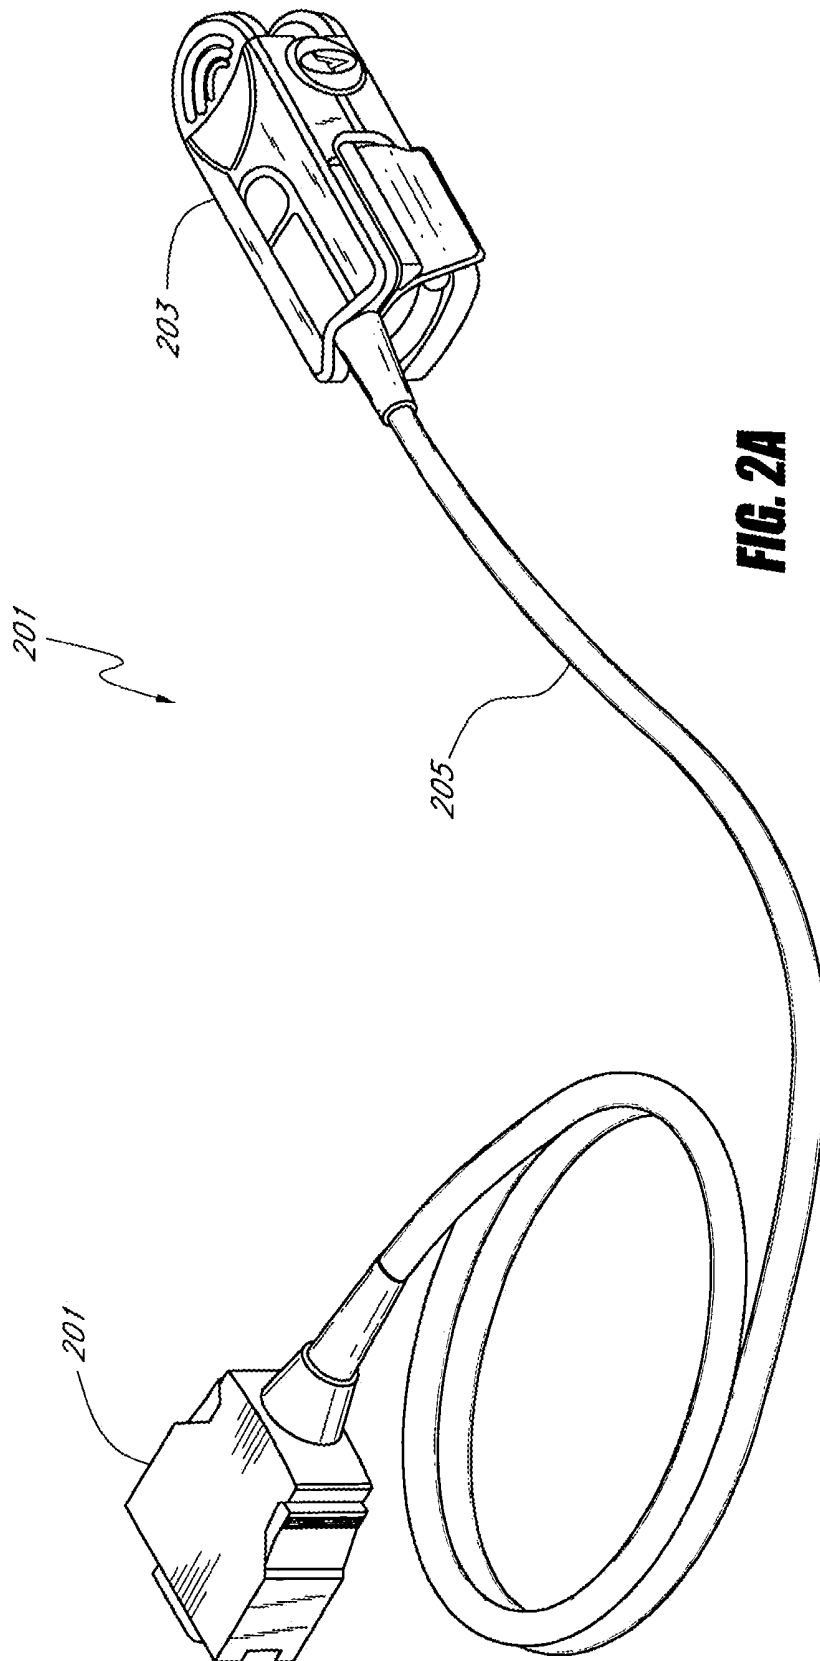


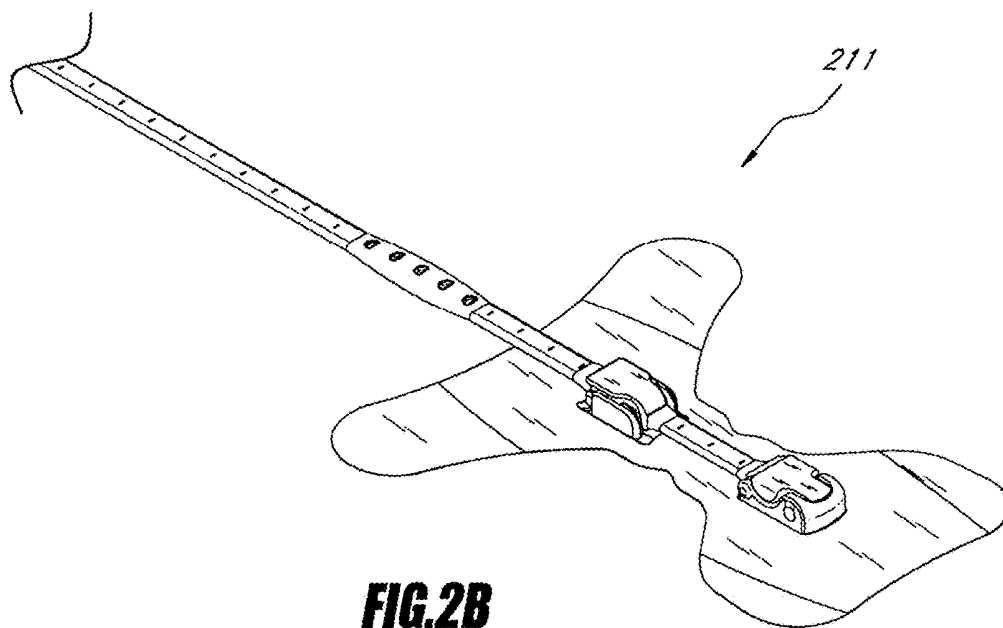



**FIG. 2B**

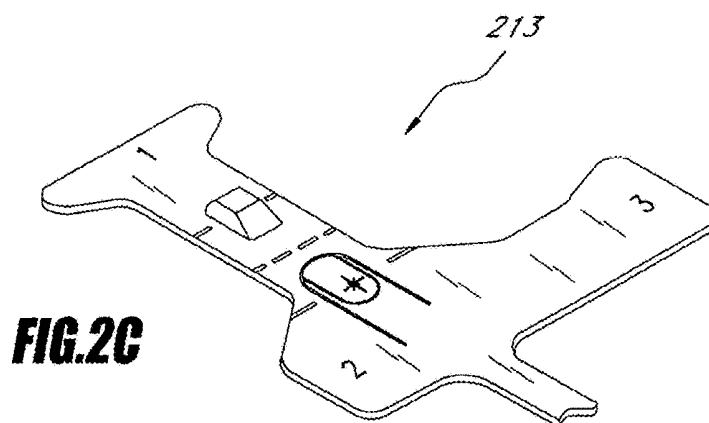


**FIG. 2C**

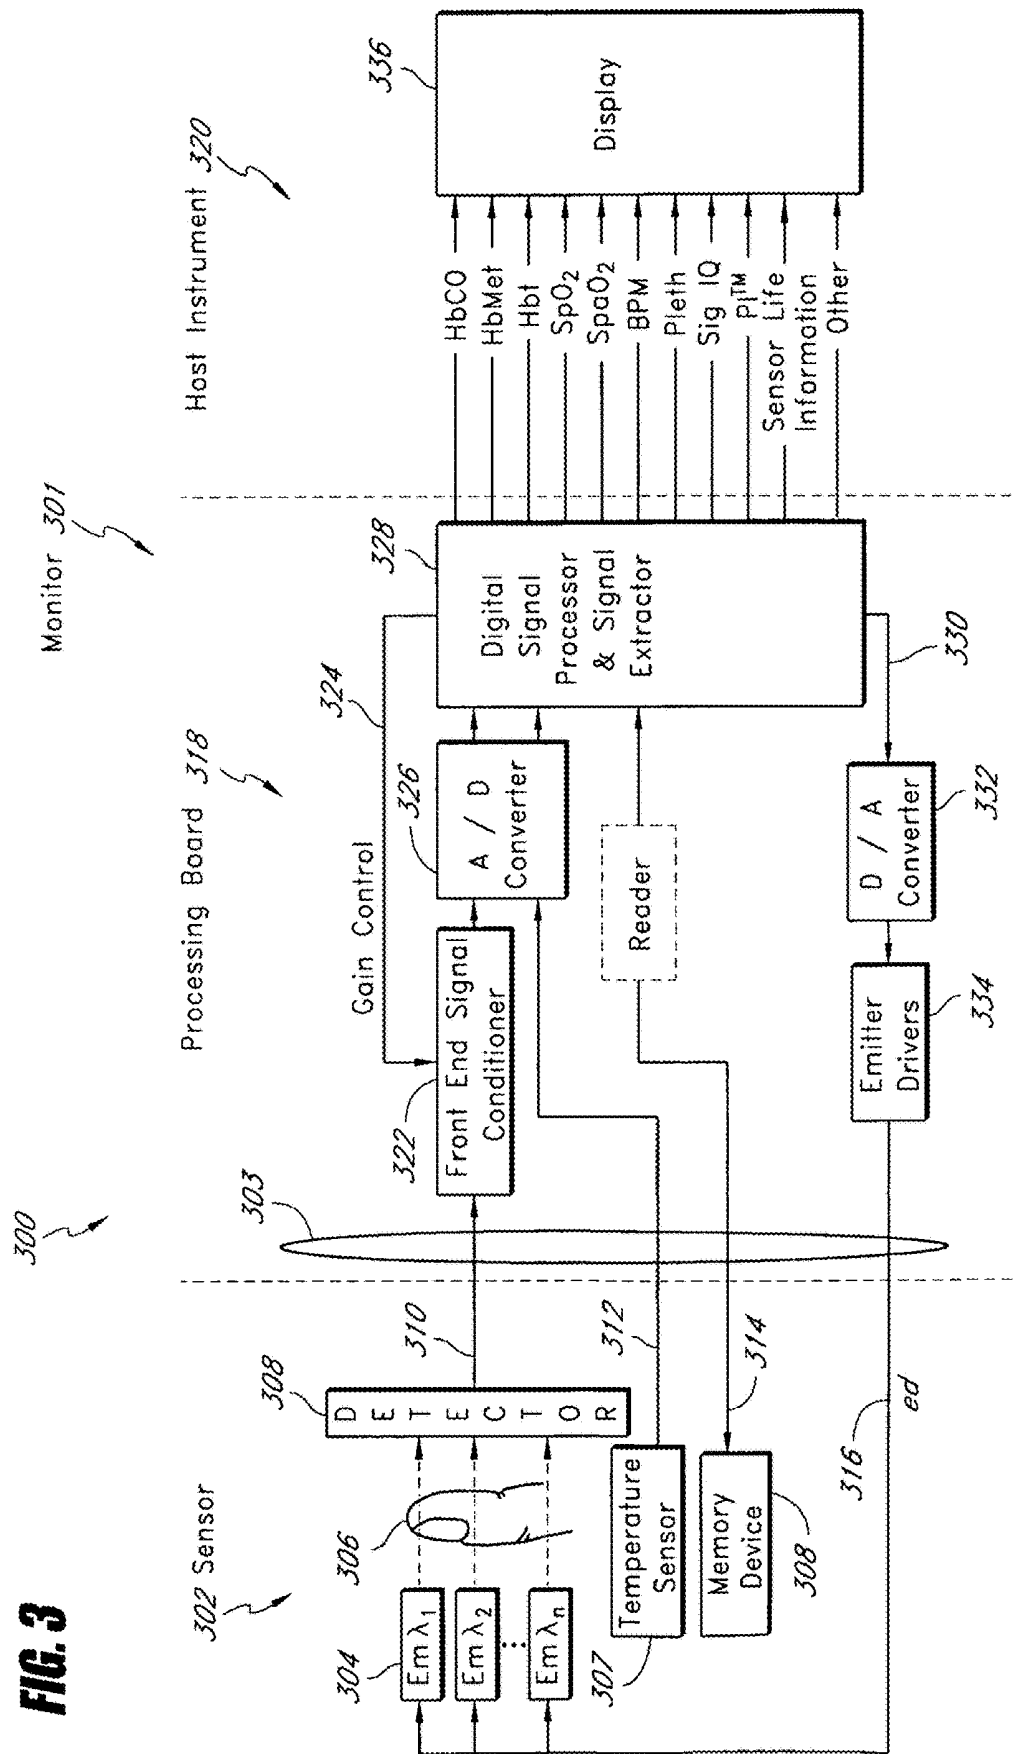
**FIG. 3**

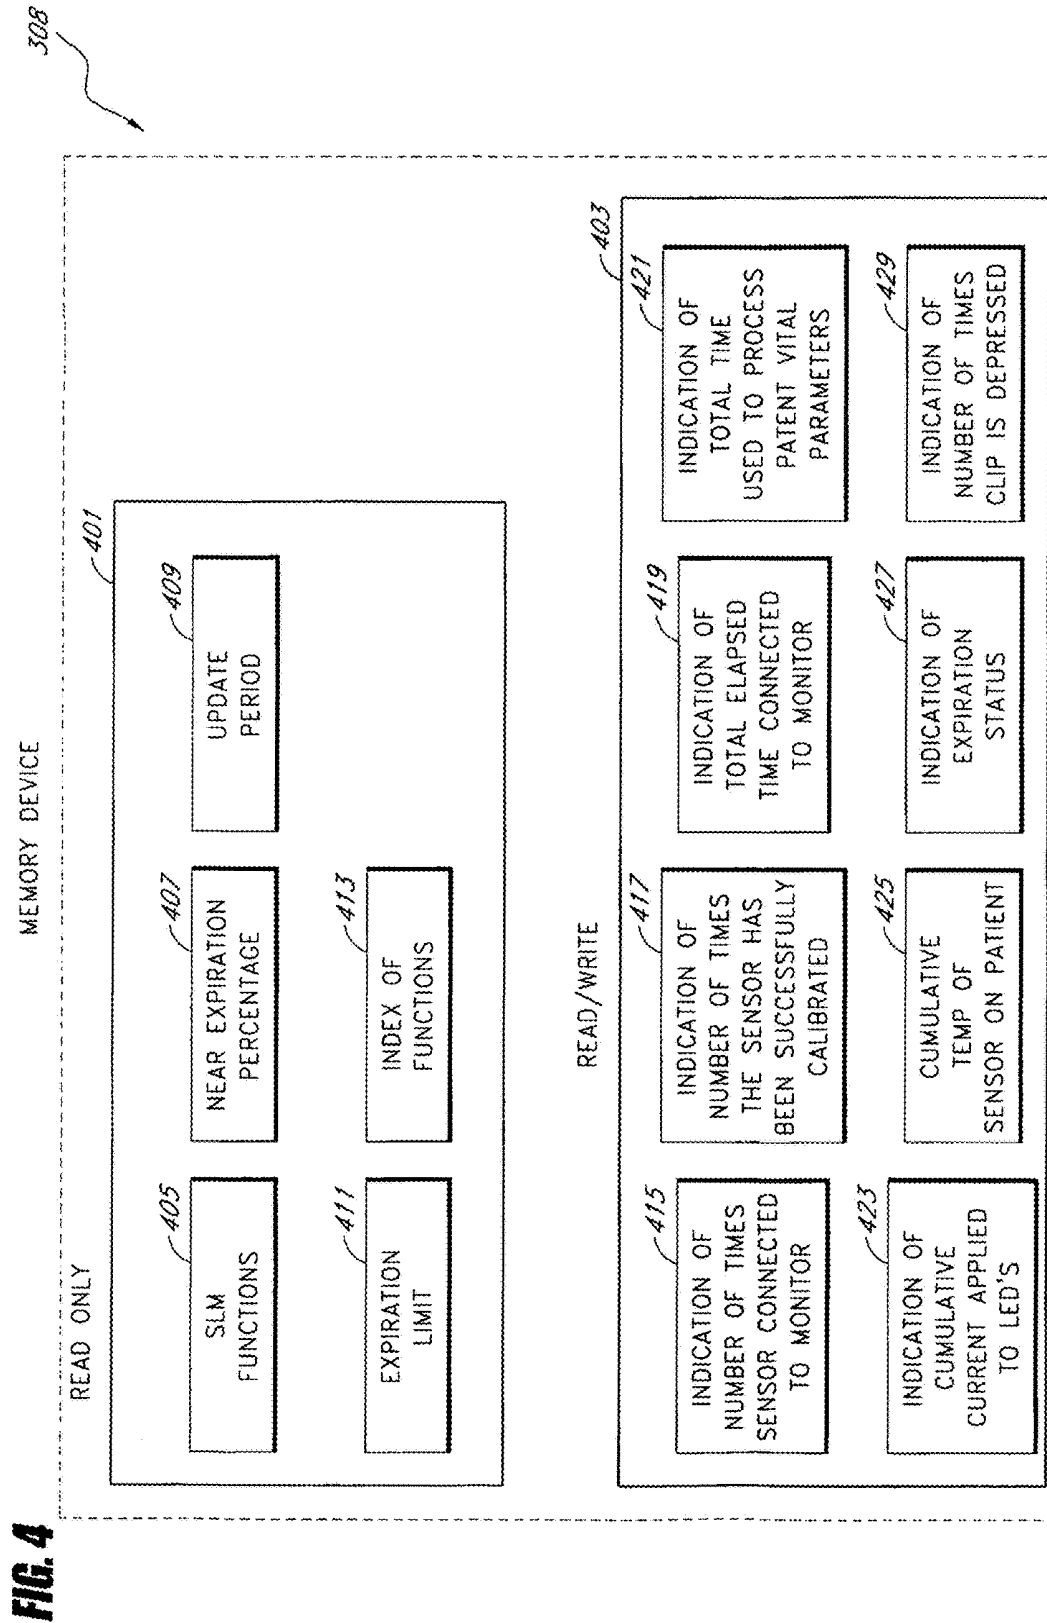


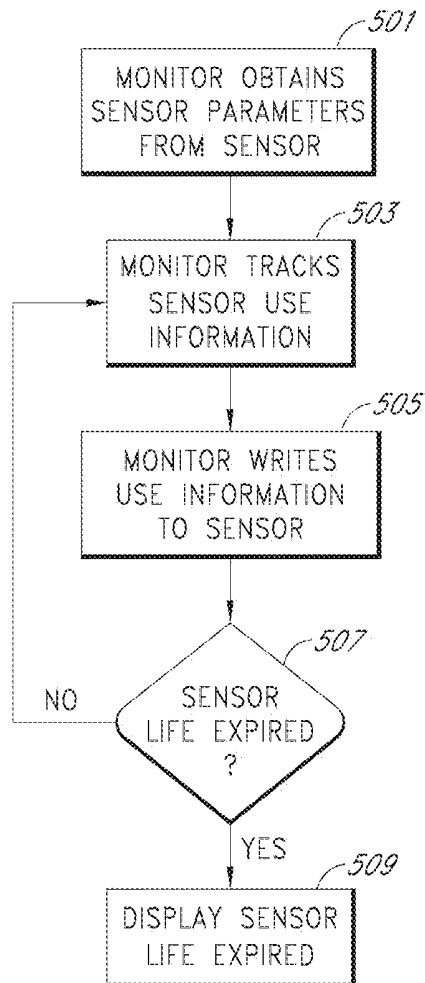**FIG. 5**

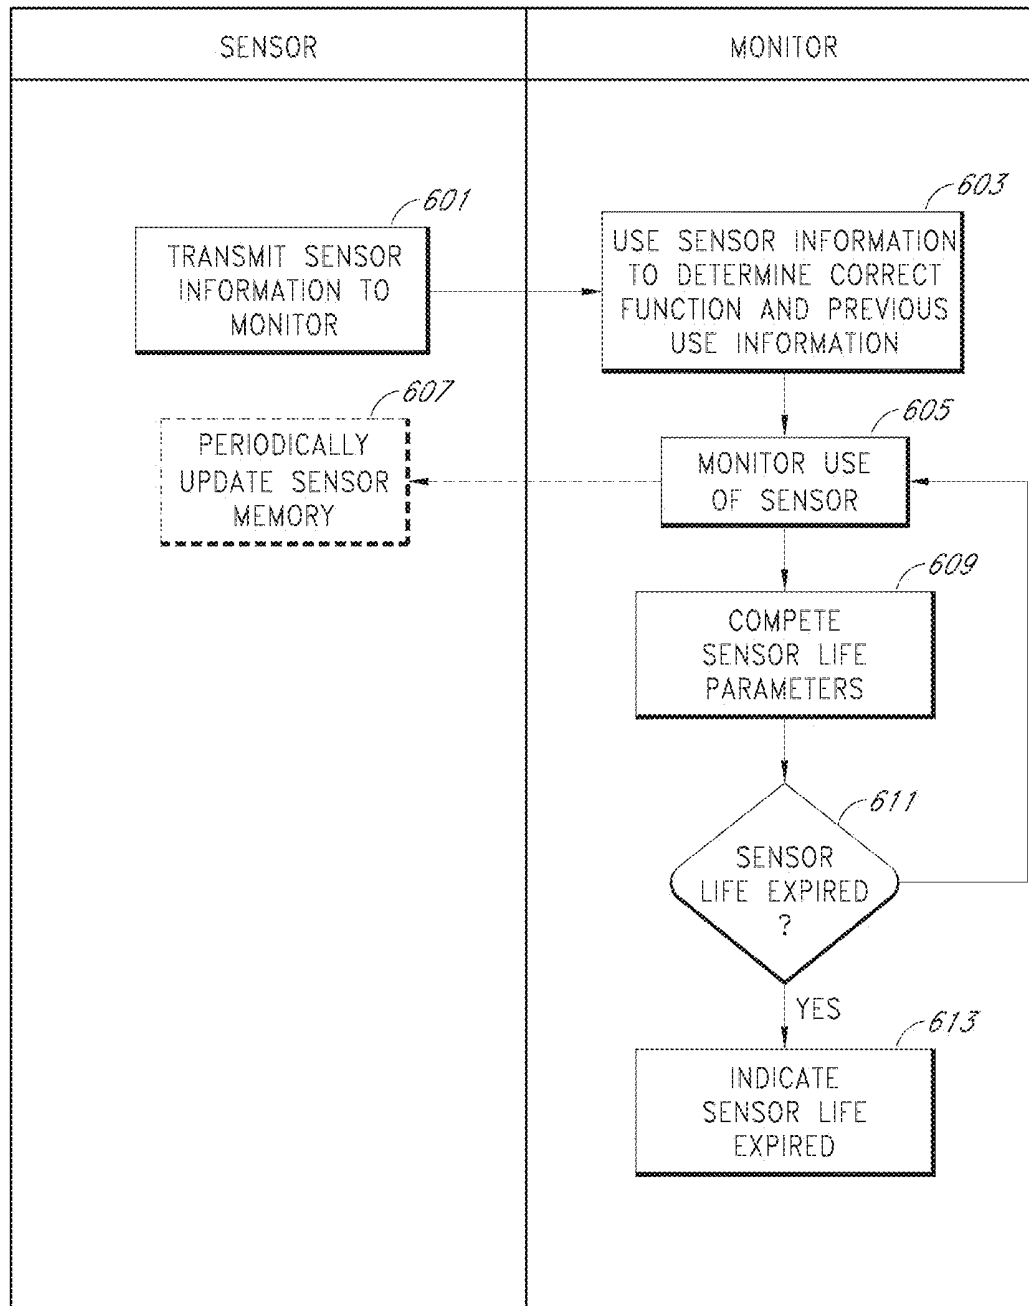**FIG. 6A**

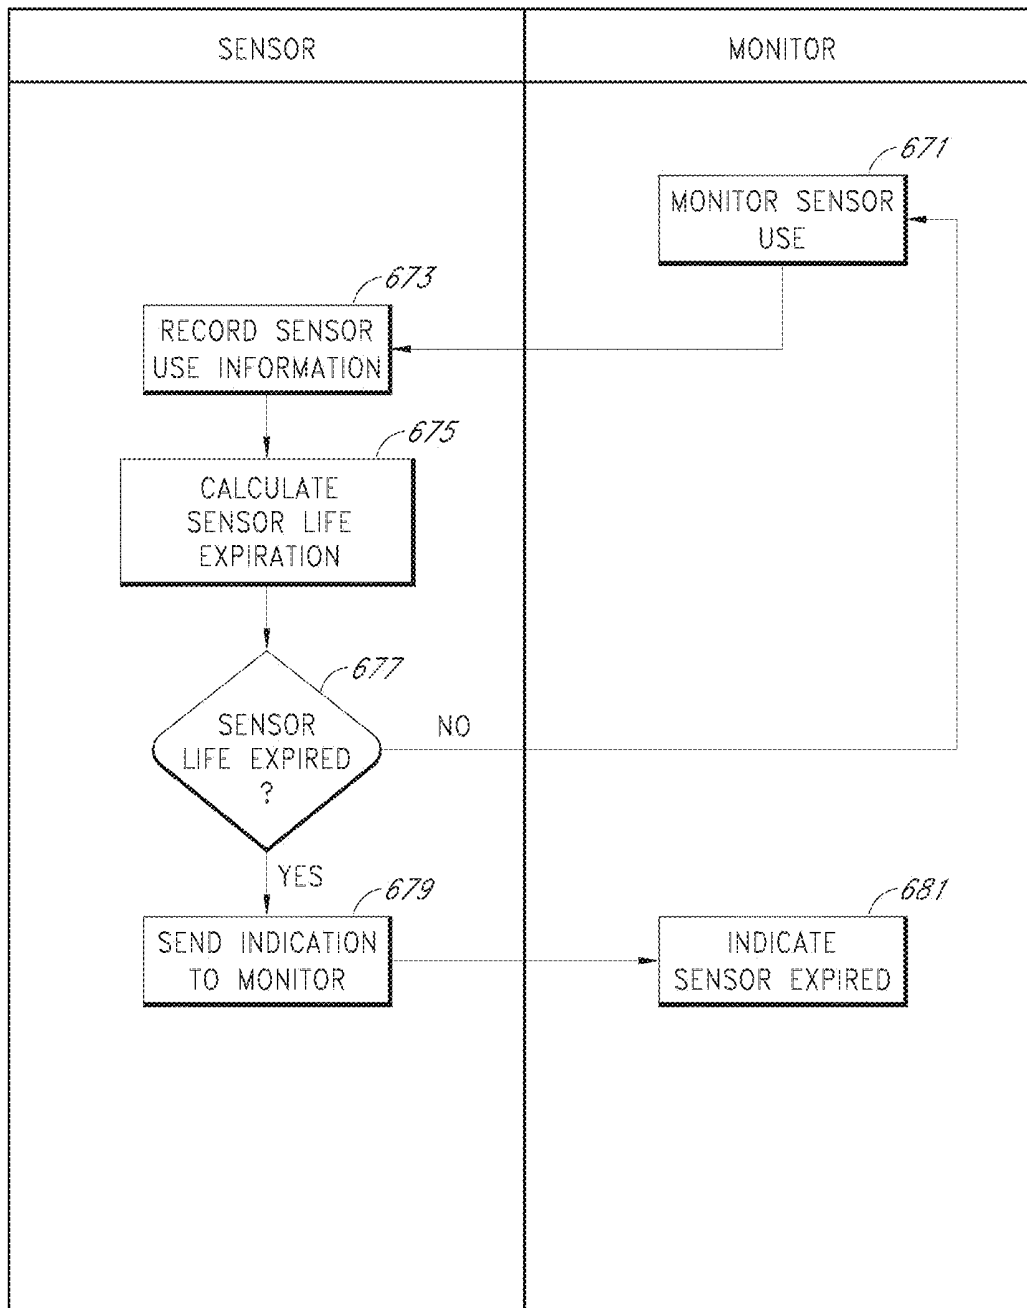

**FIG. 6B**

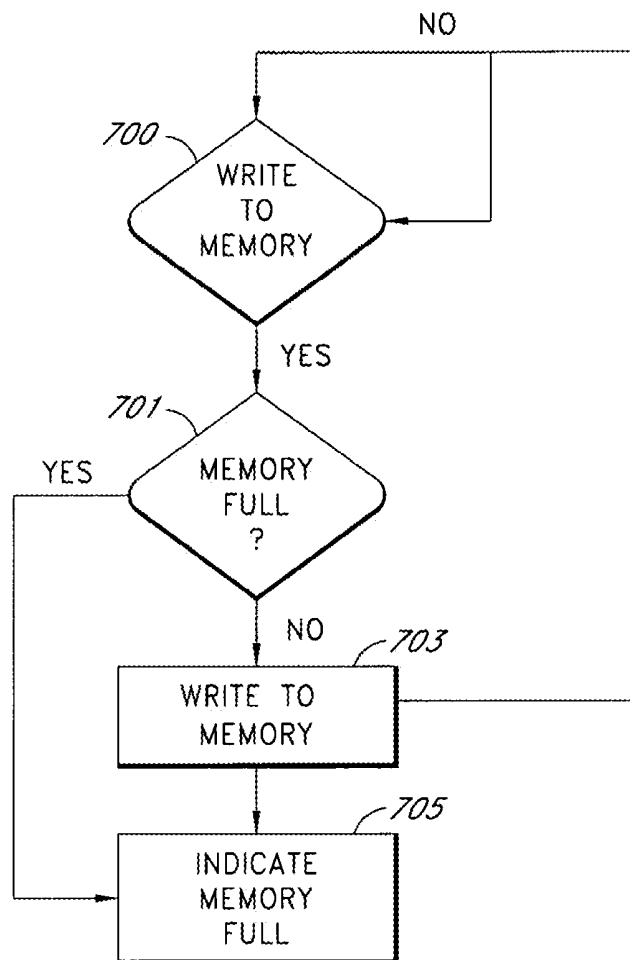**FIG. 7**

# SYSTEM AND METHOD FOR MONITORING THE LIFE OF A PHYSIOLOGICAL SENSOR

## CROSS REFERENCE TO RELATED APPLICATIONS

The present application is a continuation of U.S. application Ser. No. 15/388,075, filed Dec. 22, 2016, entitled "System and Method for Monitoring the Life of a Physiological Sensor", which is a continuation of U.S. application Ser. No. 14/821,590, filed Aug. 7, 2015, entitled "System and Method for Monitoring the Life of a Physiological Sensor," which is a continuation of U.S. application Ser. No. 14/573,332, filed Dec. 17, 2014, entitled "System and Method for Monitoring the Life of a Physiological Sensor", which is a continuation of U.S. application Ser. No. 13/015,207, filed Jan. 27, 2011, entitled "System and Method for Monitoring the Life of a Physiological Sensor," which is a continuation of U.S. application Ser. No. 11/580,214, filed Oct. 12, 2006, entitled "System and Method for Monitoring the Life of a Physiological Sensor," each of which is incorporated herein by reference in its entirety.

The present application also relates to U.S. Pat. No. 6,388,240, filed Mar. 2, 2001, entitled "Shielded Optical Probe and Method Having a Longevity Indication," and U.S. Pat. No. 6,515,273, filed Feb. 10, 2000, entitled "A system for Indicating the Expiration of the Useful Operating Life of a Pulse Oximetry Sensor," their continuations, divisionals, continuation-in-parts and the like, and incorporates each of the foregoing disclosures herein by reference in their entirety.

## FIELD

The present invention relates to a sensor for measuring oxygen content in the blood, and, in particular, relates to an apparatus and method for monitoring the life of a pulse oximetry sensor.

## BACKGROUND

Early detection of low blood oxygen is critical in a wide variety of medical applications. For example, when a patient receives an insufficient supply of oxygen in critical care and surgical applications, brain damage and death can result in just a matter of minutes. Because of this danger, the medical industry developed pulse oximetry, a noninvasive procedure for measuring the oxygen saturation of the blood. A pulse oximeter interprets signals from a sensor attached to a patient in order to determine that patient's blood oxygen saturation.

A conventional pulse oximetry sensor has a red emitter, an infrared emitter, and a photodiode detector. The sensor is typically attached to a patient's finger, earlobe, or foot. For a finger, the sensor is configured so that the emitters project light from one side of the finger, through the outer tissue of the finger, and into the blood vessels and capillaries contained inside. The photodiode is positioned at the opposite side of the finger to detect the emitted light as it emerges from the outer tissues of the finger. The photodiode generates a signal based on the emitted light and relays that signal to the pulse oximeter. The pulse oximeter determines blood oxygen saturation by computing the differential absorption by the arterial blood of the two wavelengths (red and infrared) emitted by the sensor.

The foregoing conventional sensor is typically detachable from the oximeter to allow for periodic replacement. Peri-

odic replacement is advantageous for a wide variety of reasons. For example, the sensor can become soiled, thereby possibly inhibiting sensor sensitivity or causing cross-patient contamination. Furthermore, the electronic circuitry in the sensor can become damaged, thereby causing sensor failure or inaccurate results. Moreover, the securing mechanism for the sensor, such as an adhesive substrate, can begin to fail, thereby improperly positioning the sensor in proximity to a measurement site and providing inaccurate data. Accordingly, periodic replacement of the sensor is an important aspect of maintaining a sterile, highly sensitive, accurate pulse oximetry system.

However, a conventional pulse oximetry sensor is generally reliant on an operator for timely replacement of soiled, damaged, or otherwise overused sensors. This approach is problematic not only from the standpoint of operator mistake or negligence, but also from the perspective of deliberate misuse for cost saving or other purposes.

## SUMMARY

Accordingly, one aspect of the present invention is to provide an inexpensive, accurate sensor life monitoring system for monitoring the useful and safe life of a pulse oximetry sensor. In an embodiment, a sensor is provided with a memory device, such as, for example, an EPROM or EEPROM. At predetermined intervals and/or in response to predetermined events, information is written onto the memory device. When the sensor reaches a predetermined level of use, a sensor replacement signal is indicated to a user.

In an embodiment, depending on the characteristics of the sensor, the sensor stores information related to the life expectancy of the sensor. In an embodiment, the life expectancy information is a function or set of functions that is used to calculate the useful life of the sensor. In an embodiment, the information is an indication of the use of the sensor. In an embodiment, the function or set of functions is stored on the sensor with an indication of the use of the sensor. In an embodiment, the function or set of functions is used in conjunction with the indication of the use of the sensor in order to determine the useful life of the sensor.

In an embodiment, the function or set of functions is a predetermined function or set of functions based on empirical data obtained from observing sensor use and/or inspecting used sensors. In an embodiment the empirical data is obtained experimentally in the normal course of using a sensor on a patient. In an embodiment, the empirical data is obtained experimentally without using patients. In an embodiment, the function or set of functions is based on theoretical data. In an embodiment, the function or set of functions is based on the individual life of each component of the sensor.

In an embodiment, a patient monitor works in conjunction with the sensor to determine the useful life of the sensor. In an embodiment, the monitor tracks information related to the use of the sensor and stores an indication of the information related to the use on the sensor. In an embodiment, the monitor uses the information stored on the sensor, including the functions and/or the previously stored indications of use and calculates the useful sensor life. In an embodiment, the monitor updates the already stored indications of use on the sensor. In an embodiment, the monitor indicates a sensor life expired status to a user.

In an embodiment, the sensor uses the function(s) and/or the indications of use and calculates the useful sensor life. In an embodiment, the sensor calculates the useful life of the

sensor based on information provided by the monitor. In an embodiment, the monitor stores the functions and or the sensor use information relevant to a particular sensor. In an embodiment, a range or set of functions is stored on the monitor and the sensor stores an indication of which function or set of functions are to be used to calculate the useful life of the sensor. In an embodiment, indications of use information are stored on the sensor, so as to conserve memory space. In an embodiment, the sensor memory includes both read only and read/write memory. In an embodiment, the read only memory stores the functions and other read only information such as the update period, expiration limit, index of functions, near expiration percentage, or the like. In an embodiment, the read/write memory stores use information which changes periodically based on the use of the sensor.

In an embodiment, the use information includes one or more of the following: the number of times a sensor has been connected and/or disconnected from a monitor, the number of times the sensor has been successfully calibrated, the total elapsed time the sensor has been connected to the monitor, the total time the sensor has been used to process the patient vital parameters, the age of the sensor, the cumulative or average current applied to the LED's, the cumulative or average current provided to the sensor, the cumulative or average temperature of the sensor during use, an indication of the expiration status or existing life of the sensor, the number of times the clip has been depressed, the number of times the clip has been placed on a patient, the number of patients the sensor has been used on, the number of times and time between cleanings and/or sterilization of the sensor, the number of monitors a particular sensor has been connected to, the number of times a sensor has been refurbished, the number of times the sensor has been sterilized, the time period between uses, as well as any other information useful in determining the life of a sensor as would be understood by a person of ordinary skill in the art from the disclosure herein.

In an embodiment, a reusable noninvasive physiological sensor is disclosed. The sensor has a first and second emitter which emit light of at least two wavelengths through tissue, a detector which senses the light after it has passed through the tissue and generates a signal indicative of the sensed light, a memory device which stores an indication of sensor use information and an indication of a function to be used in determining the useful life of the sensor, and a communication port which communicates at least the signal and information stored on the memory with a patient monitor. In an embodiment, the memory device has a read only portion and a read/write portion. In an embodiment, the indication of the function is stored in the read only portion and the indication of sensor use information is stored in the read/write portion of the memory. In an embodiment, the memory device is made up of a plurality of memory devices. In an embodiment, the indication of the sensor use information is an indication of one or more of an age of the sensor, a use time of the sensor, a current supplied to the sensor, a temperature of the sensor, a number of times the sensor is depressed, a number of times the sensor is calibrated, or a number of times the sensor is powered up. In an embodiment, the monitor tracks the use information and sends an indication of the use information to the sensor for storage in the memory.

In an embodiment, a method of determining the useful life of a physiological sensor is disclosed, the method includes the steps of using a physiological sensor having a memory device to obtain physiological information, monitoring the

use of the sensor, storing an indication of the use of the sensor on the memory device, and determining when the useful life of the sensor has been exceeded by using a mathematical function and the indications of use. In an embodiment, the indication of the use of the sensor includes an indication of one or more of an age of the sensor, a use time of the sensor, a current supplied to the sensor, a temperature of the sensor, a number of times the sensor is depressed, a number of times the sensor is calibrated, or a number of times the sensor is powered up. In an embodiment, the step of monitoring the use of the sensor is performed by a patient monitor. In an embodiment, the step of monitoring the use of the sensor is performed by the sensor. In an embodiment, the mathematical function is stored in the sensor memory. In an embodiment, the mathematical function is stored in the memory of a patient monitor. In an embodiment, an indication of the mathematical function is stored in the sensor memory. In an embodiment, the mathematical function is derived from use data. In an embodiment, the use data is obtained from used sensors. In an embodiment, the used sensors have been used on patients. In an embodiment, the physiological sensor is one or more of a blood oxygen sensor, a blood pressure sensor, or an ECG sensor.

In an embodiment, a method of reusing at least portion of a sensor is disclosed. The method includes the steps of accessing a memory device of a physiological sensor, retrieving sensor use information on the memory device, and using the retrieved sensor use information determine if at least one portion of the sensor can be reused. In an embodiment, the method also includes the step of reusing at least one portion of the sensor. In an embodiment, the step of reusing includes producing a refurbished sensor including at least one part of the sensor. In an embodiment, the method also includes the step of analyzing the use information to determine an extent of use of the sensor. In an embodiment, the method includes the step of storing reuse information on the refurbished sensor.

In an embodiment, a method of indicating when a physiological sensor needs to be replaced is disclosed. The method includes the steps of emitting light from a light emitting element, detecting light from the light emitting element after it has been attenuated by tissue, storing information on a sensor memory module, determining when the sensor memory module is full, and indicating that the sensor needs be replaced when it is determined that the sensor memory module is full. In an embodiment, the method includes the step of storing information at predetermined time intervals. In an embodiment, the information includes usage information.

#### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 illustrates an embodiment of a physiological measurement system.

FIG. 2A illustrates an embodiment of a sensor assembly. FIGS. 2B-C illustrate alternative sensor embodiments.

FIG. 3 illustrates a block diagram of an exemplary embodiment of a monitoring system.

FIG. 4 illustrates a block diagram of the contents of one embodiment of a sensor memory.

FIG. 5 illustrates a flowchart of one embodiment of a sensor life monitoring system.

FIGS. 6A-6B illustrate flowcharts of embodiments of sensor life monitoring systems.

FIG. 7 illustrates a flowchart of one embodiment of a sensor life monitoring system.

#### DETAILED DESCRIPTION

FIG. 1 illustrates an embodiment of a physiological measurement system **100** having a monitor **101** and a sensor assembly **101**. The physiological measurement system **100** allows the monitoring of a person, including a patient. In particular, the multiple wavelength sensor assembly **101** allows the measurement of blood constituents and related parameters, including oxygen saturation, HbCO, HbMet and pulse rate.

In an embodiment, the sensor assembly **101** is configured to plug into a monitor sensor port **103**. Monitor keys **105** provide control over operating modes and alarms, to name a few. A display **107** provides readouts of measured parameters, such as oxygen saturation, pulse rate, HbCO and HbMet to name a few.

FIG. 2A illustrates a multiple wavelength sensor assembly **201** having a sensor **203** adapted to attach to a tissue site, a sensor cable **205** and a monitor connector **201**. In an embodiment, the sensor **203** is incorporated into a reusable finger clip adapted to removably attach to, and transmit light through, a fingertip. The sensor cable **205** and monitor connector **201** are integral to the sensor **203**, as shown. In alternative embodiments, the sensor **203** can be configured separately from the cable **205** and connector **201**, although such communication can advantageously be wireless, over public or private networks or computing systems or devices, through intermediate medical or other devices, combinations of the same, or the like.

FIGS. 2B-C illustrate alternative sensor embodiments, including a sensor **211** (FIG. 2B) partially disposable and partially reusable (resposable) and utilizing an adhesive attachment mechanism. Also shown is a sensor **213** being disposable and utilizing an adhesive attachment mechanism. In other embodiments, a sensor can be configured to attach to various tissue sites other than a finger, such as a foot or an ear. Also a sensor can be configured as a reflectance or transreflectance device that attaches to a forehead or other tissue surface. The artisan will recognize from the disclosure herein that the sensor can include mechanical structures, adhesive or other tape structures, Velcro wraps or combination structures specialized for the type of patient, type of monitoring, type of monitor, or the like.

FIG. 3 illustrates a block diagram of an exemplary embodiment of a monitoring system **300**. As shown in FIG. 3, the monitoring system **300** includes a monitor **301**, a noninvasive sensor **302**, communicating through a cable **303**. In an embodiment, the sensor **302** includes a plurality of emitters **304** irradiating the body tissue **306** with light, and one or more detectors **308** capable of detecting the light after attenuation by tissue **306**. As shown in FIG. 3, the sensor **302** also includes a temperature sensor **307**, such as, for example, a thermistor or the like. The sensor **302** also includes a memory device **308** such as, for example, an EEPROM, EPROM or the like. The sensor **302** also includes a plurality of conductors communicating signals to and from its components, including detector composite signal conductors **310**, temperature sensor conductors **312**, memory device conductors **314**, and emitter drive signal conductors **316**.

According to an embodiment, the sensor conductors **310**, **312**, **314**, **316** communicate their signals to the monitor **301** through the cable **303**. Although disclosed with reference to the cable **303**, a skilled artisan will recognize from the

disclosure herein that the communication to and from the sensor **306** can advantageously include a wide variety of cables, cable designs, public or private communication networks or computing systems, wired or wireless communications (such as Bluetooth or WiFi, including IEEE 801.11a, b, or g), mobile communications, combinations of the same, or the like. In addition, communication can occur over a single wire or channel or multiple wires or channels.

In an embodiment, the temperature sensor **307** monitors the temperature of the sensor **302** and its components, such as, for, example, the emitters **304**. For example, in an embodiment, the temperature sensor **307** includes or communicates with a thermal bulk mass having sufficient thermal conduction to generally approximate a real-time temperature of a substrate of the light emission devices **304**. The foregoing approximation can advantageously account for the changes in surface temperature of components of the sensor **302**, which can change as much or more than ten degrees Celsius (10° C.) when the sensor **302** is applied to the body tissue **306**. In an embodiment, the monitor **101** can advantageously use the temperature sensor **307** output to, among other things, ensure patient safety, especially in applications with sensitive tissue. In an embodiment, the monitor **301** can advantageously use the temperature sensor **307** output and monitored operating current or voltages to correct for operating conditions of the sensor **302** as described in U.S. patent application Ser. No. 11/366,209, filed Mar. 1, 2006, entitled "Multiple Wavelength Sensor Substrate," and which is hereby incorporated by reference in its entirety.

The memory **308** can include any one or more of a wide variety of memory devices known to an artisan from the disclosure herein, including an EPROM, an EEPROM, a flash memory, a combination of the same or the like. The memory **308** can include a read-only device such as a ROM, a read and write device such as a RAM, combinations of the same, or the like. The remainder of the present disclosure will refer to such combination as simply EPROM for ease of disclosure; however, an artisan will recognize from the disclosure herein that the memory **308** can include the ROM, the RAM, single wire memories, combinations, or the like.

The memory device **308** can advantageously store some or all of a wide variety data and information, including, for example, information on the type or operation of the sensor **302**, type of patient or body tissue **306**, buyer or manufacturer information, sensor characteristics including the number of wavelengths capable of being emitted, emitter specifications, emitter drive requirements, demodulation data, calculation mode data, calibration data, software such as scripts, executable code, or the like, sensor electronic elements, sensor life data indicating whether some or all sensor components have expired and should be replaced, encryption information, monitor or algorithm upgrade instructions or data, or the like. In an embodiment, the memory device **308** can also include emitter wavelength correction data.

In an advantageous embodiment, the monitor reads the memory device on the sensor to determine one, some or all of a wide variety of data and information, including, for example, information on the type or operation of the sensor, a type of patient, type or identification of sensor buyer, sensor manufacturer information, sensor characteristics including the number of emitting devices, the number of emission wavelengths, data relating to emission centroids, data relating to a change in emission characteristics based on varying temperature, history of the sensor temperature, current, or voltage, emitter specifications, emitter drive requirements, demodulation data, calculation mode data, the

parameters it is intended to measure (e.g., HbCO, HbMet, etc.) calibration data, software such as scripts, executable code, or the like, sensor electronic elements, whether it is a disposable, reusable, or multi-site partially reusable, partially disposable sensor, whether it is an adhesive or non-adhesive sensor, whether it is reflectance or transmittance sensor, whether it is a finger, hand, foot, forehead, or ear sensor, whether it is a stereo sensor or a two-headed sensor, sensor life data indicating whether some or all sensor components have expired and should be replaced, encryption information, keys, indexes to keys or has functions, or the like monitor or algorithm upgrade instructions or data, some or all of parameter equations, information about the patient, age, sex, medications, and other information that can be useful for the accuracy or alarm settings and sensitivities, trend history, alarm history, sensor life, or the like.

FIG. 3 also shows the monitor **301** comprising one or more processing boards **318** communicating with one or more host instruments **320**. According to an embodiment, the board **318** includes processing circuitry arranged on one or more printed circuit boards capable of installation into the handheld or other monitor **301**, or capable of being distributed as an OEM component for a wide variety of host instruments **320** monitoring a wide variety of patient information, or on a separate unit wirelessly communicating to it. As shown in FIG. 3, the board **318** includes a front end signal conditioner **322** including an input receiving the analog detector composite signal from the detector **308**, and an input from a gain control signal **324**. The signal conditioner **322** includes one or more outputs communicating with an analog-to-digital converter **326** ("A/D converter **326**").

The A/D converter **326** includes inputs communicating with the output of the front end signal conditioner **322** and the output of the temperature sensor **307**. The converter **326** also includes outputs communicating with a digital signal processor and signal extractor **328**. The processor **328** generally communicates with the A/D converter **326** and outputs the gain control signal **324** and an emitter driver current control signal **330**. The processor **328** also communicates with the memory device **308**. As shown in phantom, the processor **328** can use a memory reader, memory writer, or the like to communicate with the memory device **308**. Moreover, FIG. 3 also shows that the processor **328** communicates with the host instrument **320** to for example, display the measured and calculated parameters or other data.

FIG. 3 also shows the board **318** including a digital-to-analog converter **332** ("D/A converter **332**") receiving the current control signal **330** from the processor **328** and supplying control information to emitter driving circuitry **334**, which in turn drives the plurality of emitters **304** on the sensor **302** over conductors **316**. In an embodiment, the emitter driving circuitry **334** drives sixteen (16) emitters capable of emitting light at sixteen (16) predefined wavelengths, although the circuitry **334** can drive any number of emitters. For example, the circuitry **334** can drive two (2) or more emitters capable of emitting light at two (2) or more wavelengths, or it can drive a matrix of eight (8) or more emitters capable of emitting light at eight (8) or more wavelengths. In addition, one or more emitters could emit light at the same or substantially the same wavelength to provide redundancy.

In an embodiment, the host instrument **320** communicates with the processor **328** to receive signals indicative of the physiological parameter information calculated by the processor **328**. The host instrument **320** preferably includes one

or more display devices **336** capable of providing indicia representative of the calculated physiological parameters of the tissue **306** at the measurement site. In an embodiment, the host instrument **320** can advantageously include virtually any housing, including a handheld or otherwise portable monitor capable of displaying one or more of the foregoing measured or calculated parameters. In still additional embodiments, the host instrument **320** is capable of displaying trending data for one or more of the measured or determined parameters. Moreover, an artisan will recognize from the disclosure herein many display options for the data available from the processor **328**.

In an embodiment, the host instrument **320** includes audio or visual alarms that alert caregivers that one or more physiological parameters are falling below or above predetermined safe thresholds, which are trending in a predetermined direction (good or bad), and can include indications of the confidence a caregiver should have in the displayed data. In further embodiment, the host instrument **320** can advantageously include circuitry capable of determining the expiration or overuse of components of the sensor **302**, including, for example, reusable elements, disposable elements, or combinations of the same. Moreover, a detector could advantageously determine a degree of clarity, cloudiness, transparency, or translucence over an optical component, such as the detector **308**, to provide an indication of an amount of use of the sensor components and/or an indication of the quality of the photo diode.

An artisan will recognize from the disclosure herein that the emitters **304** and/or the detector **308** can advantageously be located inside of the monitor, or inside a sensor housing. In such embodiments, fiber optics can transmit emitted light to and from the tissue site. An interface of the fiber optic, as opposed to the detector can be positioned proximate the tissue. In an embodiment, the physiological monitor accurately monitors HbCO in clinically useful ranges. This monitoring can be achieved with non-fiber optic sensors. In another embodiment, the physiological monitor utilizes a plurality, or at least four, non-coherent light sources to measure one or more of the foregoing physiological parameters. Similarly, non-fiber optic sensors can be used. In some cases the monitor receives optical signals from a fiber optic detector. Fiber optic detectors are useful when, for example, monitoring patients receiving MRI or cobalt radiation treatments, or the like. Similarly, light emitters can provide light from the monitor to a tissue site with a fiber optic conduit. Fiber optics are particularly useful when monitoring HbCO and HbMet. In another embodiment, the emitter is a laser diode placed proximate tissue. In such cases, fiber optics are not used. Such laser diodes can be utilized with or without temperature compensation to affect wavelength.

FIG. 4 shows one embodiment of a memory device on the sensor **308**. Memory device **308** has a read only section **401** and a read write section **403**. One of ordinary skill in the art will understand that the read only and read write sections can be on the same memory or on a separate physical memory. One of ordinary skill in the art will also understand that the read only block **401** and the read write block **403** can consist of multiple separate physical memory devices or a single memory device. The read only section **401** contains read only information, such as, for example, sensor life monitoring functions (SLM) **405**, near expiration percentage **407**, update period **409**, expiration limit **411**, index of functions **413**, sensor type or the like.

The read write section **403** contains numerous read write parameters, such as the number of times sensor is connected to a monitoring system **415**, the number of times the sensor

Sensor use information can be determined in any number of ways. For example, in an embodiment, in order to determine the life of the emitters, the number of emitter pulses can be counted and an indication stored in memory. In an embodiment, the time period in which power is provided to the sensor is determined and an indication stored in memory. In an embodiment, the amount of current supplied to the sensor and/or LEDs is monitored and an indication is stored in memory. In an embodiment, the number of times the sensor is powered up or powered down is monitored and an indication is stored in memory. In an embodiment, the number of times the sensor is connected to a monitor is tracked and an indication is stored in memory. In an embodiment, the number of times the sensor is placed on or removed from a patient is monitored and an indication is stored in the memory. The number of times the sensor is placed on or removed from a patient can be monitored by monitoring the number of probe off conditions sensed, or it can be monitored by placing a separate monitoring device on the sensor to determine when the clip is depressed, opened, removed, replaced, attached, etc. In an embodiment, the average operating temperature of the sensor is monitored

In an embodiment, a weighted function or average of functions is determined based on the sensor/monitor configuration. For example, in an embodiment, the sensor life function is the sum of a weighted indication of use, for example, in an embodiment, the following sensor life function is used:

where  $f_{ij}$  refers to a function determined based on operating conditions and  $c_j$  refers to an indication of sensor use. For example, the correct  $f_{ij}$  can be determined from a table such as:

[illegible]

Where  $F_i$  refers the type of sensor and/or the type and number of parameters being monitored. For each different sensor and for each different parameter, a separate function is used in determining the useful life of a sensor. In an embodiment, the correct  $F_i$  for a given sensor can be stored on the sensor memory. In an embodiment, all of the functions  $f_{ij}$  for a sensor are stored in the sensor memory. In an embodiment, the entire table is stored in the sensor memory.  $c_j$  can be determined from the monitored sensor parameters. For example, a  $c_j$  for can be determined by counting the total time in use, averaging use time during certain parameters, squaring use time, etc. Thus a  $c_j$  can be an indication of use. In an embodiment, the correct  $c_j$  for the number of times the sensor has been turned on or off can be determined by the following formula:

$$e^{\frac{c}{100}} \quad (2)$$

where  $c$  is the number of times turned on or off.

In an embodiment, when the useful life of a sensor has been reached, the monitor or sensor sounds an alarm or gives a visual indication that the sensor is at the end of its life. In an embodiment, the monitor will give an indication that the sensor is bad. In an embodiment, the monitor will not output data. In an embodiment, an indication of the end of the sensor life is not given while the sensor is actively measuring vital signs. In an embodiment, the percent of life left in a sensor is indicated. In an embodiment, an estimated remaining use time is indicated. In an embodiment, an indication that the end of the sensor life is approaching is indicated without giving a specific percentage or time period.

FIGS. 6A and 6B illustrate flowcharts of embodiments of sensor life monitoring systems. Referring to FIG. 6A, in an embodiment of a sensor life monitoring system, a sensor including a memory device is connected to a monitor. The sensor transmits sensor information to the monitor at block 601. The information can include one or more of a function, use parameters, expiration parameters, or any other sensor specific information useful in determining the life expiration of a sensor. At block 603, the sensor information is used to determine the correct function to use in determining the sensor expiration date. Any previous use information transmitted is also used during the monitoring process. At block 605, the patient monitor monitors the sensor use. Optionally, the monitor periodically writes updated use information to the sensor at block 607 or in an embodiment, the use information is written once at the end of a monitoring cycle. At block 609, the monitor computes sensor life parameters and sensor life expiration. The system then moves onto decision block 611 where it is determined whether the sensor life has expired. If the sensor life has expired, then the system moves to block 613 where an indication of the sensor life expiration is given. If the sensor life has not expired at decision block 611, then the system returns to block 605, where sensor use is monitored.

FIG. 6B illustrates a flowchart where the sensor life is calculated on the sensor instead of the monitor. At block 671, the patient monitor monitors sensor use. The use information is supplied to the sensor at block 673, the use information is recorded. At block 675, the sensor calculates the sensor life expiration. The system then moves onto decision block 677. At decision block 677, if the sensor has expired, the system moves onto block 679, where the sensor sends an expiration

indication to the monitor and the monitor indicates the sensor expiration at block 681. If, however, at block 671 the sensor has not expired, the system returns to block 671 where the sensor use is monitored.

FIG. 7 illustrates a flowchart of an embodiment of a system for measuring the life of a sensor. In the course of monitoring a patient, information is written on the EPROM. Because the EPROM is finite in the amount of information it can hold, at some point, the EPROM becomes full. When the EPROM becomes full, the sensor will need to be replaced. Thus, an EPROM full signal indicates that the life span of the sensor has expired. The EPROM's memory capacity can be chosen to so as to estimate the life of the sensor. In addition, the monitor can be programmed to write to the sensor at set intervals so that after a predictable period of time, the EPROM's memory will be full. Once the EPROM is full, the monitor gives an audio and/or visual indication that the sensor needs to be replaced.

Referring to FIG. 7, the patient monitoring system determines whether to write to the sensor EPROM at block 700. If information is not to be written to the EPROM at block 700, then the system continues at block 700. If information is to be written to the EPROM at block 700, then the system continues to block 701, where the system determines if the EPROM is full. If the EPROM is full, then the system moves to block 703, where the system writes information to the EPROM. Once the information has been written, the system returns to block 700 where it waits until information is to be written to the EPROM. If at block 701, the system determines that the EPROM is full, then the system moves to block 703, where an indication is given to the user that the sensor needs to be replaced.

In an embodiment, the sensor can be refurbished and used again. For example, if the memory used is an erasable memory module, then the sensor's memory can be erased during the refurbishment process and the entire sensor can be used again. In an embodiment, each time part or all of the memory is erased, an indicator of the number of times the memory has been erased is stored on the memory device. In this way, an indication of the number of refurbishments of a particular sensor can be kept. If a write only memory is used, then parts of the sensor can be salvaged for reuse, but a new memory module will replace the used memory module. In an embodiment, once the sensor memory is full, the sensor is discarded.

In an embodiment, various parts of used sensors can be salvaged and reused. In an embodiment, the sensor keeps track of various use information as described above. The sensor memory can then be reviewed to see which parts of the used sensor can be salvaged based on the use information stored in the memory. For example, in an embodiment, an indication of the number of times the clip is depressed is stored in memory. A refurbisher can look at that use information and determine whether the mechanical clip can be salvaged and used on a refurbished sensor. Of course, the same principals apply to other aspects of the sensor, such as, for example, the LEDs, the cables, the detector, the memory, or any other part of the sensor.

Although the foregoing invention has been described in terms of certain preferred embodiments, other embodiments will be apparent to those of ordinary skill in the art from the disclosure herein. For example, although disclosed with respect to a pulse oximetry sensor, the ideas disclosed herein can be applied to other sensors such as ECG/EKG sensor, blood pressure sensors, or any other physiological sensors. Additionally, the disclosure is equally applicable to physiological monitor attachments other than a sensor, such as,



13

for example, a cable connecting the sensor to the physiological monitor. Additionally, other combinations, omissions, substitutions and modifications will be apparent to the skilled artisan in view of the disclosure herein. It is contemplated that various aspects and features of the invention described can be practiced separately, combined together, or substituted for one another, and that a variety of combination and subcombinations of the features and aspects can be made and still fall within the scope of the invention. Furthermore, the systems described above need not include all of the modules and functions described in the preferred embodiments. Accordingly, the present invention is not intended to be limited by the recitation of the preferred embodiments, but is to be defined by reference to the appended claims.

What is claimed is:

1. A physiological sensor configured to store a sensor life function, the physiological sensor comprising:

one or more emitters configured to transmit light of at least a first wavelength and a second wavelength into tissue of a patient;

one or more detectors configured to detect the light after it has interacted with the tissue and to generate a signal responsive to the detected light;

a memory device storing at least one sensor life function for use by a separately housed patient monitor in determining a useful life of the physiological sensor; and

a communication port configured to communicate the at least one sensor life function to the separately housed patient monitor, wherein the separately housed patient monitor calculates the useful life of the physiological sensor using the at least one sensor life function.

2. The physiological sensor of claim 1, wherein the memory device comprises a read only portion and a read/write portion and the at least one sensor life function is stored in the read only portion of the memory device.

3. The physiological sensor of claim 1, wherein the memory device comprises a read only portion and a read/write portion and the at least one sensor life function is stored in the read/write portion of the memory device.

4. The physiological sensor of claim 1, wherein the memory device is configured to store sensor use information, wherein the communication port is further configured to communicate the sensor use information to the separately housed patient monitor, wherein to calculate the useful life of the physiological sensor, the separately housed patient monitor uses the sensor use information.

5. The physiological sensor of claim 4, wherein the sensor use information comprises one or more of an amount of time the physiological sensor has been used, an amount of time power has been provided to the physiological sensor, a number of times the physiological sensor has been powered up, a number of times the physiological sensor has been powered down, a number of times the physiological sensor has been connected to a monitor, a number of different monitors that have been connected to the physiological sensor, a number of patients that have used the physiological sensor, a number of times the physiological sensor has been calibrated, an amount of time the physiological sensor has been connected to a finger, a number of times the physiological sensor has been opened or closed, an average temperature of the physiological sensor, or an average current provided to the physiological sensor.

6. The physiological sensor of claim 1, wherein the memory device is configured to store at least two indications of sensor use information, wherein the at least one sensor

14

life function assigns weighting values to each of the at least two indications of sensor use information.

7. A method of determining a useful life of a physiological sensor, the method comprising:

storing at least one sensor life function in a memory device of the physiological sensor, wherein the at least one sensor life function indicates to a separately housed patient monitor how to calculate a useful life of the physiological sensor; and

communicating the at least one sensor life function to the separately housed patient monitor, wherein the separately housed patient monitor calculates the useful life of the physiological sensor using the at least one sensor life function.

8. The method of claim 7, wherein the memory device comprises a read only portion and a read/write portion, wherein the at least one sensor life function is stored in the read only portion of the memory device.

9. The method of claim 7, wherein the memory device comprises a read only portion and a read/write portion, wherein the at least one sensor life function is stored in the read/write portion of the memory device.

10. The method of claim 7, wherein the memory device is configured to store at least two indications of sensor use information, wherein the at least one sensor life function assigns weighting values to each of the at least two indications of sensor use information.

11. The method of claim 10, further comprising:

storing the at least two indications of sensor use information in the memory device of the physiological sensor; and

communicating the at least two indications of sensor use information to the separately housed patient monitor, wherein to calculate the useful life of the physiological sensor, the separately housed patient monitor uses the at least two indications of sensor use information.

12. The method of claim 10, wherein at least one indication of sensor use information of the at least two indications of sensor use information comprises one or more of an amount of time the physiological sensor has been used, an amount of time power has been provided to the physiological sensor, a number of times the physiological sensor has been powered up, a number of times the physiological sensor has been powered down, a number of times the physiological sensor has been connected to a monitor, a number of different monitors that have been connected to the physiological sensor, a number of patients that have used the physiological sensor, a number of times the physiological sensor has been calibrated, an amount of time the physiological sensor has been connected to a finger, a number of times the physiological sensor has been opened or closed, an average temperature of the physiological sensor, or an average current provided to the physiological sensor.

13. The method of claim 7, further comprising selecting the at least one sensor life function from a plurality of sensor life functions stored in the memory device of the physiological sensor.

14. The method of claim 13, wherein said selecting is based at least in part on a sensor type of the physiological sensor.

15. A method of determining a useful life of a reusable noninvasive physiological sensor, the method comprising:

receiving at least one sensor life function from a reusable noninvasive physiological sensor, wherein the at least one sensor life function indicates how to calculate a useful life of the reusable noninvasive physiological sensor, the at least one sensor life function assigning a

15

first weighting value to a first indication of sensor use information and assigning a second weighting value to a second indication of sensor use information; updating the at least one sensor life function to assign a third weighting value to the first indication of sensor use information and to assign a fourth weighting value to the second indication of sensor use information, wherein the third weighting value is different from the first weighting value, wherein the fourth weighting value is different from the second weighting value; and calculating the useful life of the reusable noninvasive physiological sensor using at least the first indication of sensor use information, the second indication of sensor use information, the third weighting value, the fourth weighting value, and the updated at least one sensor life function.

16. The method of claim 15, further comprising receiving the first and second indications of sensor use information from the reusable noninvasive physiological sensor.

17. The method of claim 15, further comprising storing the updated at least one sensor life function in a memory device of the reusable noninvasive physiological sensor.

18. The method of claim 15, wherein the sensor life function is stored in a memory device of the reusable noninvasive physiological sensor, wherein the method fur-

16

ther comprises replacing, in the memory device, the stored sensor life function with the updated sensor life function.

19. The method of claim 15, wherein at least one indication of the first indication of sensor use information or the second indication of sensor use information comprises one or more of an amount of time the physiological sensor has been used, an amount of time power has been provided to the physiological sensor, a number of times the physiological sensor has been powered up, a number of times the physiological sensor has been powered down, a number of times the physiological sensor has been connected to a monitor, a number of different monitors that have been connected to the physiological sensor, a number of patients that have used the physiological sensor, a number of times the physiological sensor has been calibrated, an amount of time the physiological sensor has been connected to a finger, a number of times the physiological sensor has been opened or closed, an average temperature of the physiological sensor, or an average current provided to the physiological sensor.

20. The method of claim 15, further comprising: determining that the useful life of the reusable noninvasive physiological sensor has been exceeded; and causing a display device to display an indication that the useful life of the reusable noninvasive physiological sensor has been exceeded.

\* \* \* \* \*

专利名称(译)	用于监测生理传感器寿命的系统和方法		
公开(公告)号	<a href="#">US10342470</a>	公开(公告)日	2019-07-09
申请号	US16/047364	申请日	2018-07-27
[标]申请(专利权)人(译)	梅西莫股份有限公司		
申请(专利权)人(译)	Masimo公司		
当前申请(专利权)人(译)	Masimo公司		
[标]发明人	AL ALI AMMAR WEBER WALTER M MCHALE RYAN TIMOTHY		
发明人	AL-ALI, AMMAR WEBER, WALTER M. MCHALE, RYAN TIMOTHY		
IPC分类号	A61B5/1495 A61B5/00 A61B5/1455		
CPC分类号	A61B5/1495 A61B5/14551 A61B5/14552 A61B5/6826 A61B5/6838 A61B5/0002 A61B2562/085 A61B2560/028 A61B2560/0238 A61B2560/0266 A61B2560/0276 A61B2560/045 A61B2560/0475 A61B2562/0238 A61B2562/043		
优先权	14/573332 2015-08-18 US		
其他公开文献	US20190021638A1		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

本公开的各方面包括传感器，该传感器被配置为在存储器中存储传感器使用信息的指示和用于根据传感器使用信息的指示确定传感器的使用寿命的公式或公式的指示。连接到传感器的监视器监视传感器的使用并在传感器存储器上存储使用的指示。监视器和/或传感器根据使用指示和公式计算传感器的使用寿命。当达到传感器的使用寿命时，给出指示以更换传感器。

