



US 20170231571A1

(19) **United States**

(12) **Patent Application Publication**
ROGERS et al.

(10) **Pub. No.: US 2017/0231571 A1**

(43) **Pub. Date: Aug. 17, 2017**

(54) **DEVICES AND RELATED METHODS FOR EPIDERMAL CHARACTERIZATION OF BIOFLUIDS**

Publication Classification

(51) **Int. Cl.**
A61B 5/00 (2006.01)
A61B 5/01 (2006.01)
A61B 5/053 (2006.01)
A61B 5/145 (2006.01)

(52) **U.S. Cl.**
 CPC *A61B 5/6833* (2013.01); *A61B 5/14514* (2013.01); *A61B 5/14532* (2013.01); *A61B 5/14539* (2013.01); *A61B 5/14517* (2013.01); *A61B 5/002* (2013.01); *A61B 5/01* (2013.01); *A61B 5/053* (2013.01); *A61B 5/14546* (2013.01)

(71) Applicant: **The Board of Trustees of the University of Illinois, Urbana, IL (US)**

(72) Inventors: **John A. ROGERS, Champaign, IL (US); Ahyeon KOH, Champaign, IL (US); Daeshik KANG, Urbana, IL (US); YuHao LIU, Urbana, IL (US); Xian HUANG, Rolla, MO (US)**

(21) Appl. No.: **15/501,373**

(22) PCT Filed: **Aug. 11, 2015**

(86) PCT No.: **PCT/US15/44638**

§ 371 (c)(1),


(2) Date: **Feb. 2, 2017**

Related U.S. Application Data

(60) Provisional application No. 62/035,823, filed on Aug. 11, 2014, provisional application No. 62/142,877, filed on Apr. 3, 2015.

(57) **ABSTRACT**

Skin-mounted or epidermal devices and methods for monitoring biofluids are disclosed. The devices comprise a functional substrate that is mechanically and/or thermally matched to skin to provide durable adhesion for long-term wear. The functional substrates allow for the microfluidic transport of biofluids from the skin to one or more sensors that measure and/or detect biological parameters, such as rate of biofluid production, biofluid volume, and biomarker concentration. Sensors within the devices may be mechanical, electrical or chemical, with colorimetric indicators being observable by the naked eye or with a portable electronic device (e.g., a smartphone). By monitoring changes in an individual's health state over time, the disclosed devices may provide early indications of abnormal conditions.

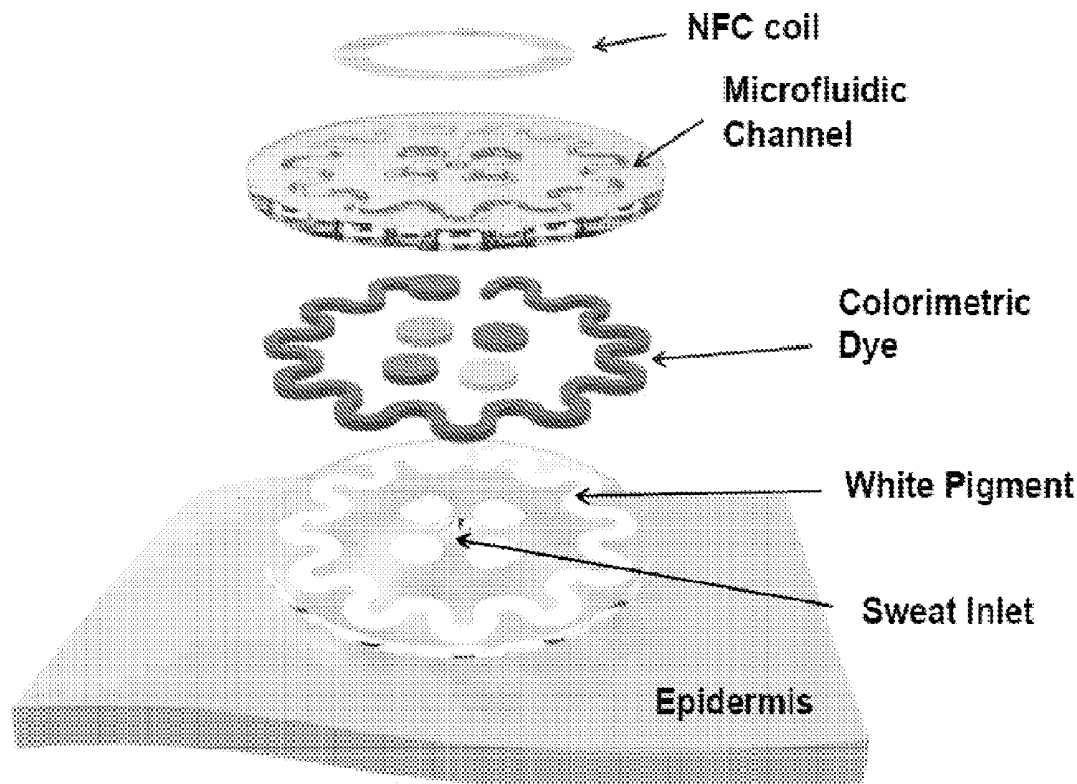

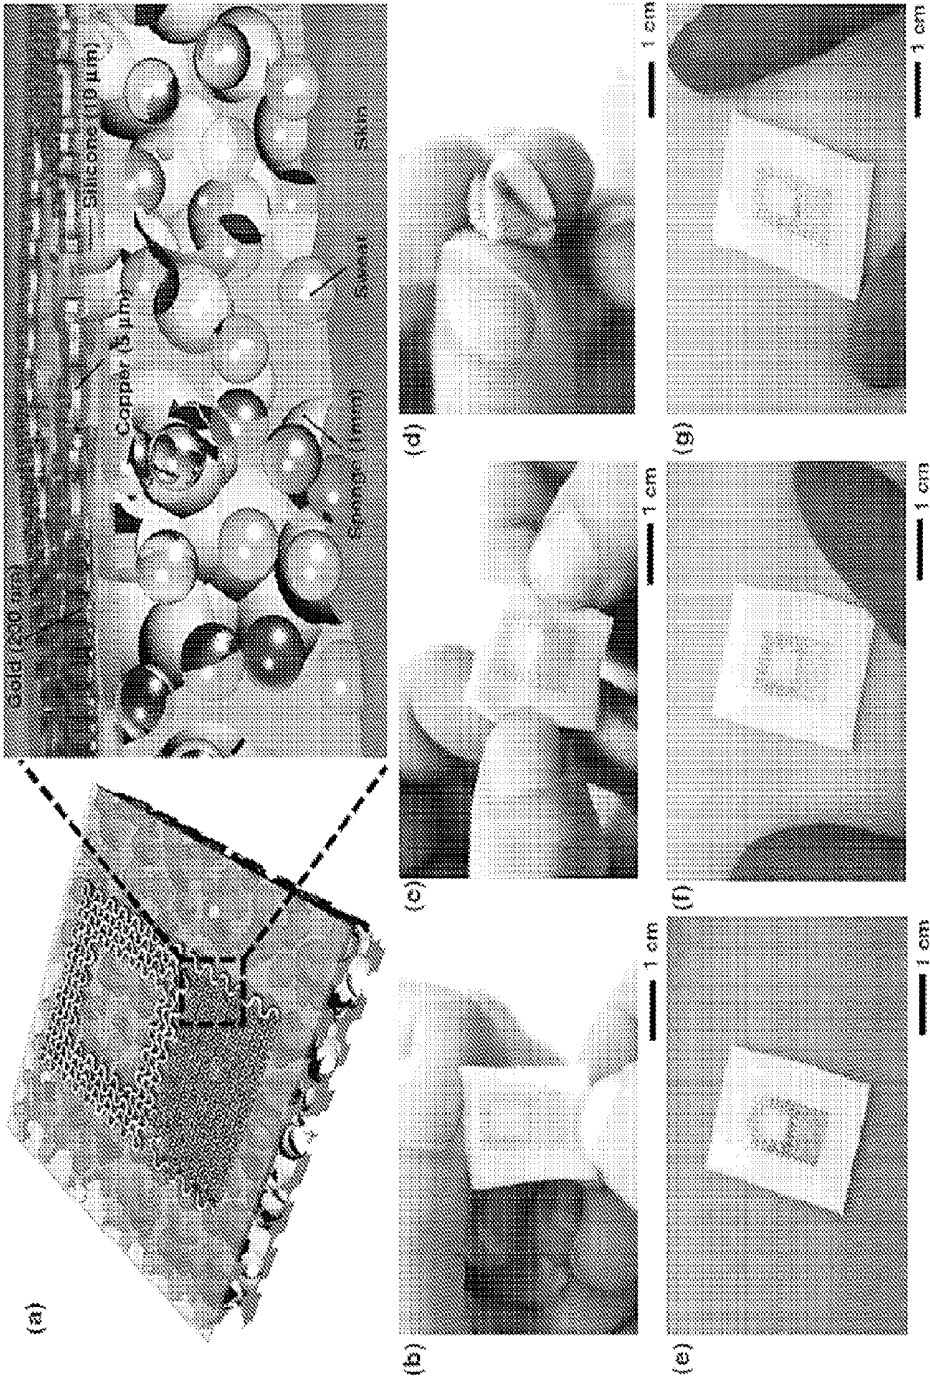


FIG. 1

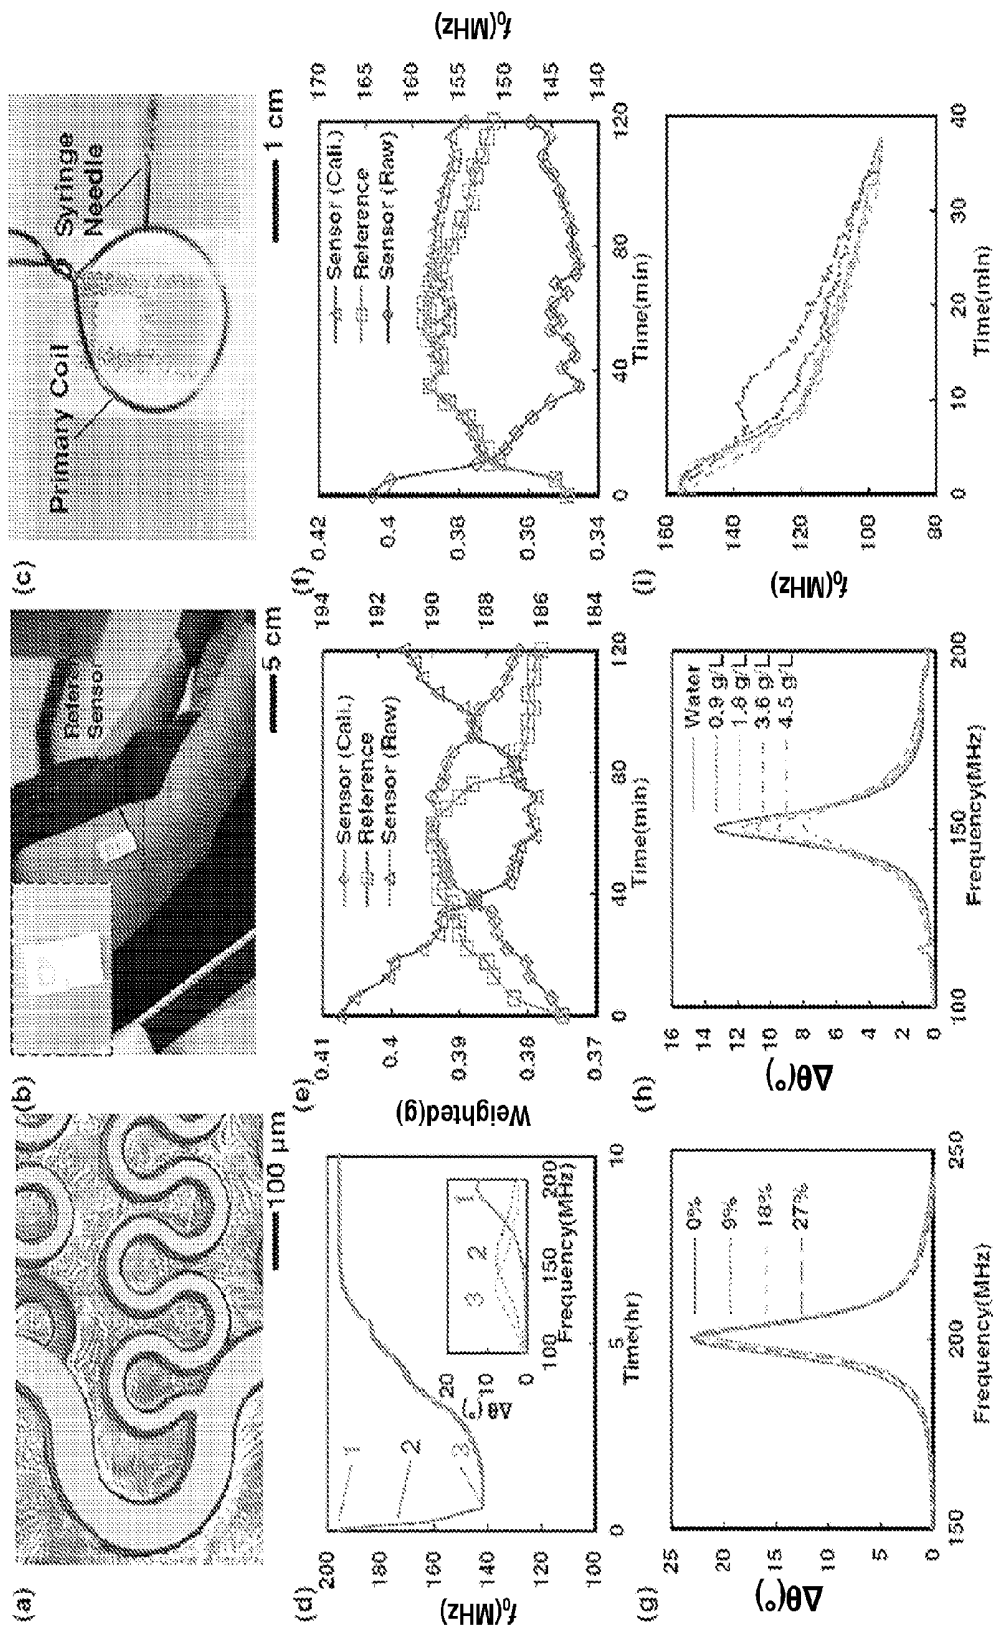


FIG. 2

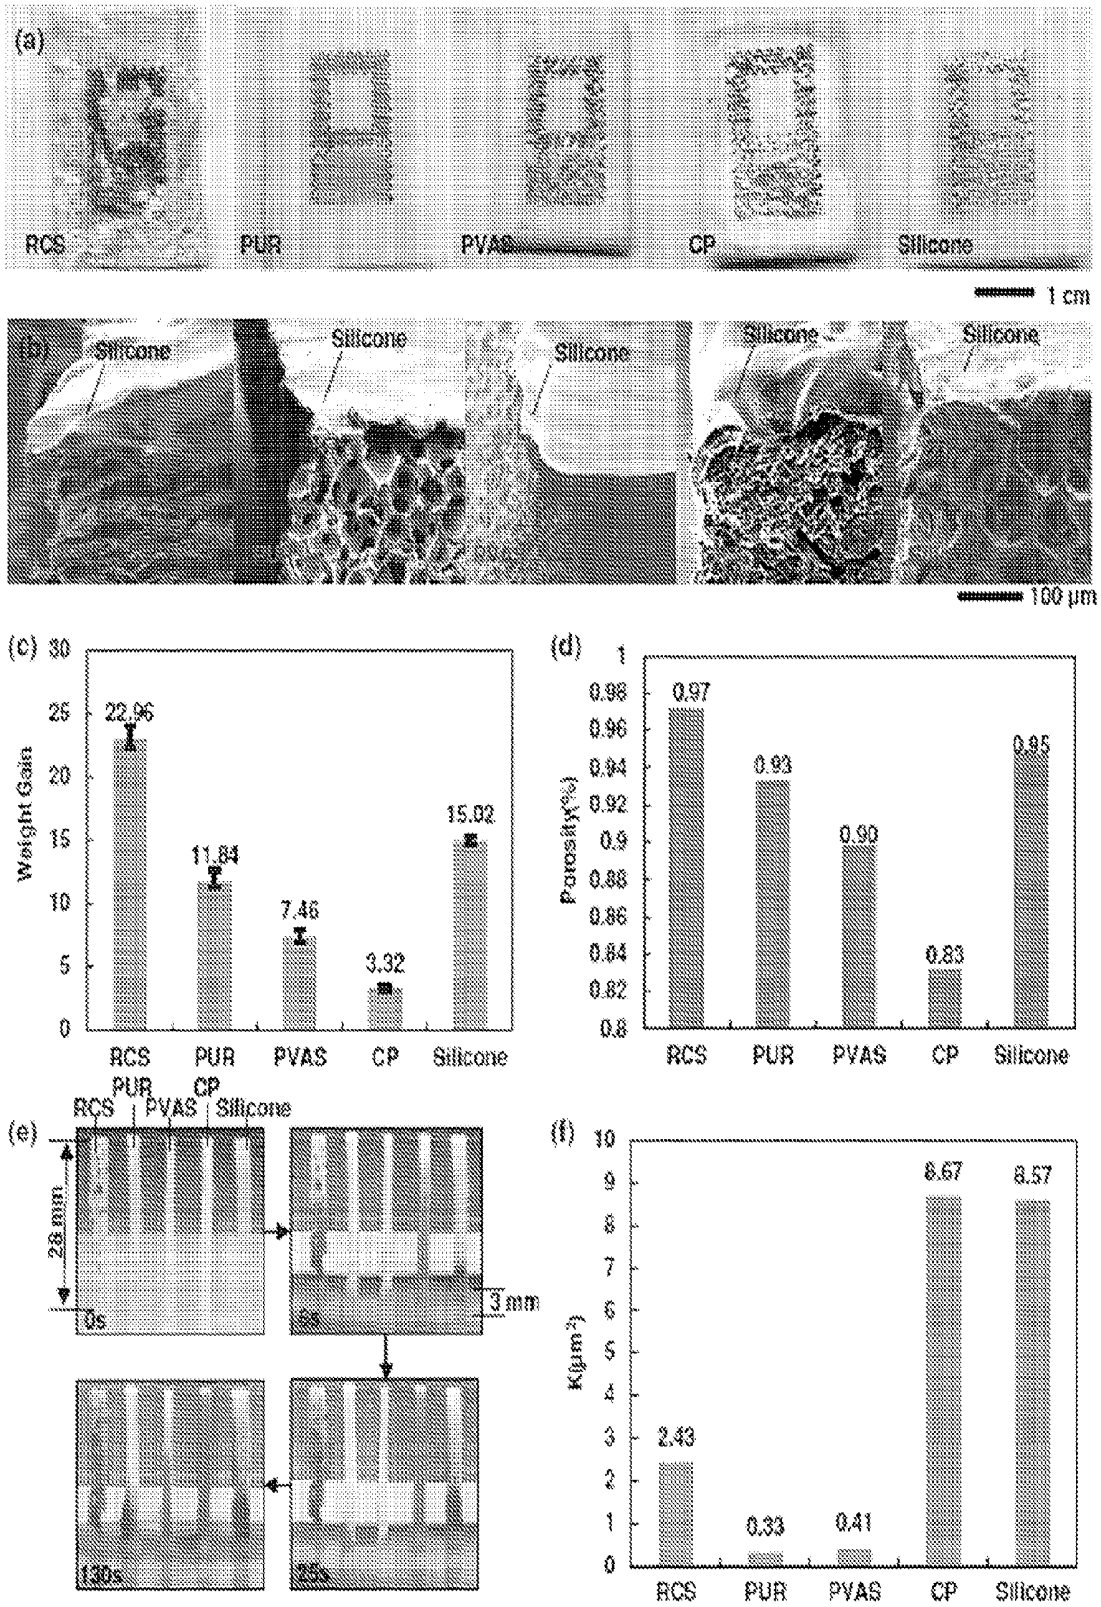


FIG. 3

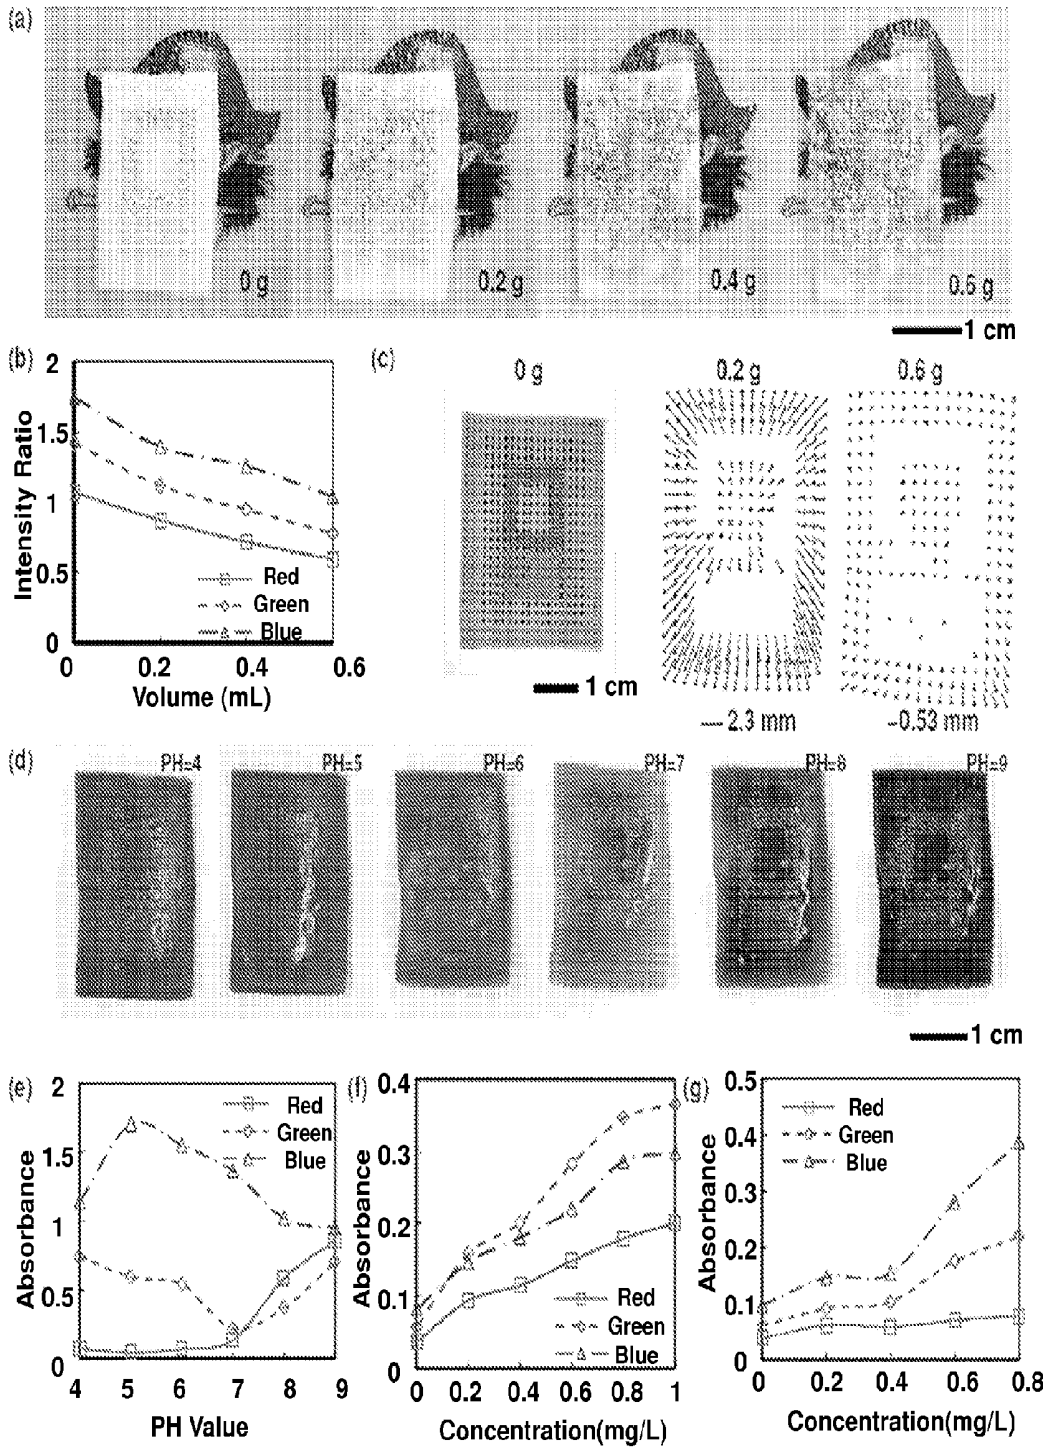


FIG. 4

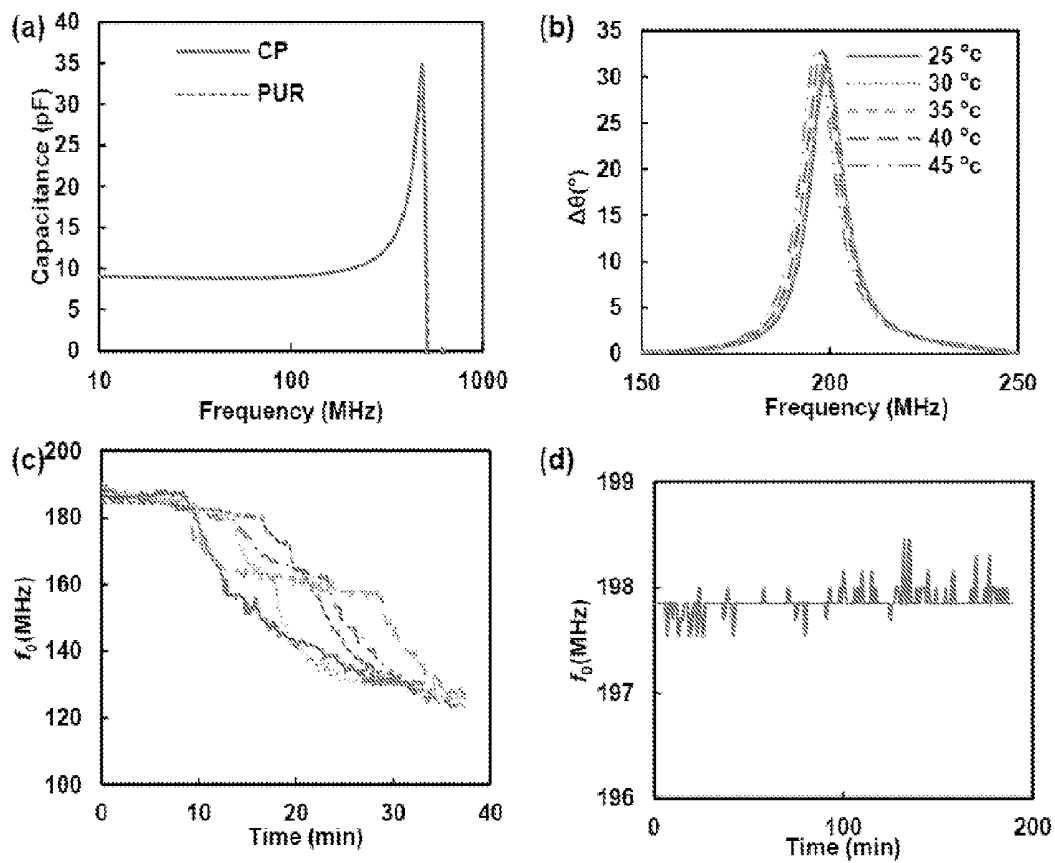


FIG. 5

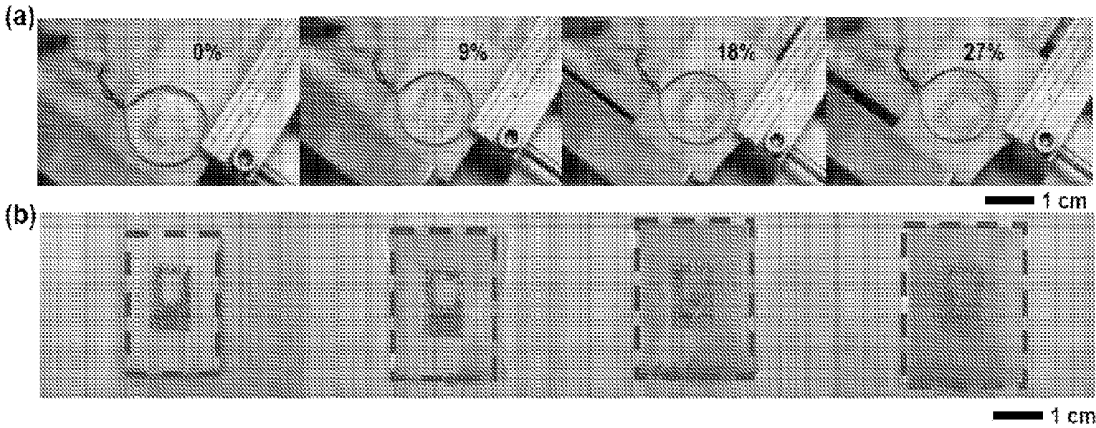


FIG. 6

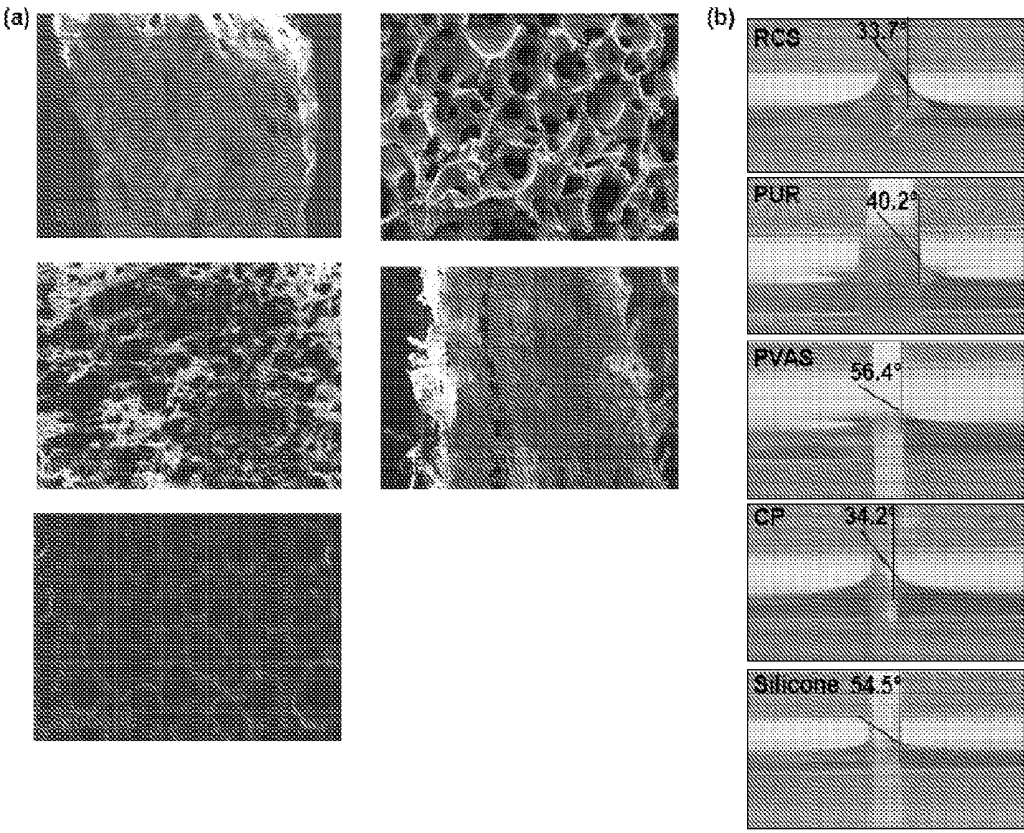


FIG. 7

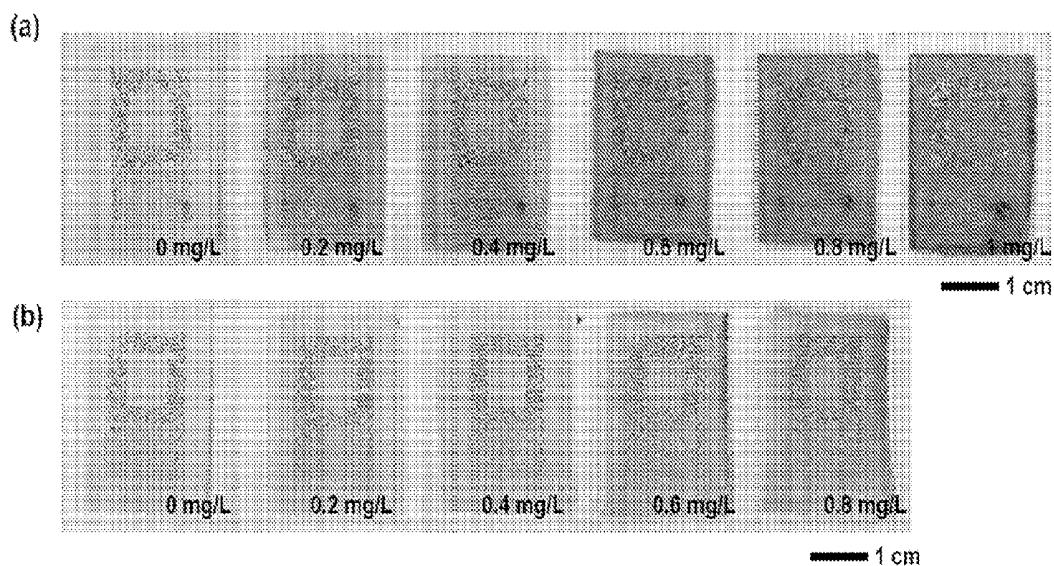


FIG. 8

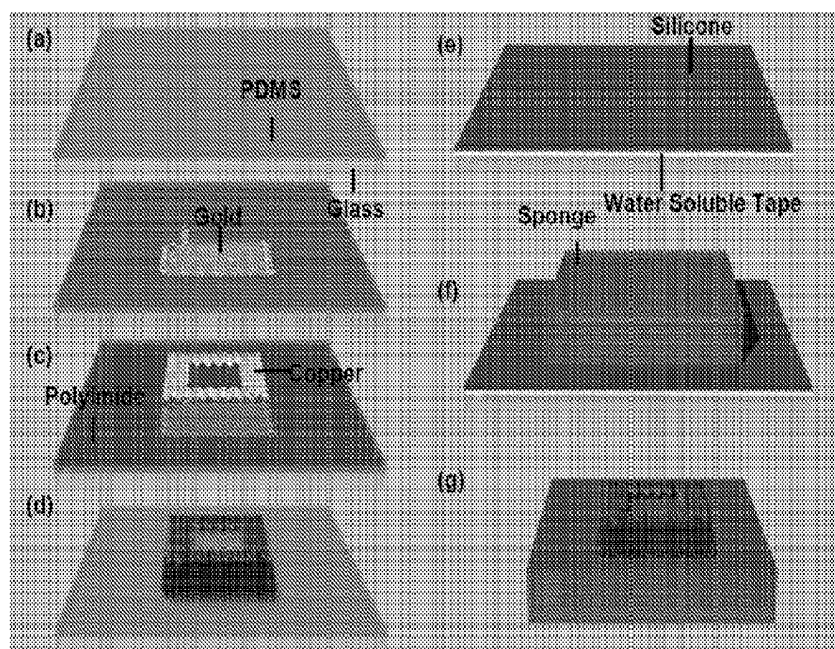


FIG. 9

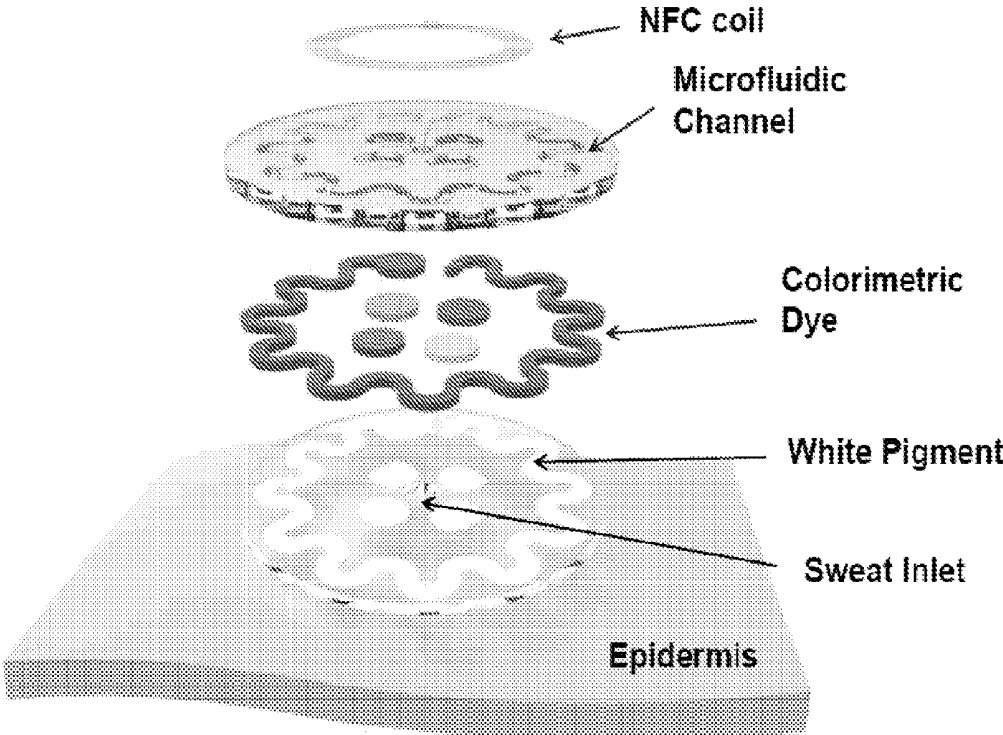


FIG. 10

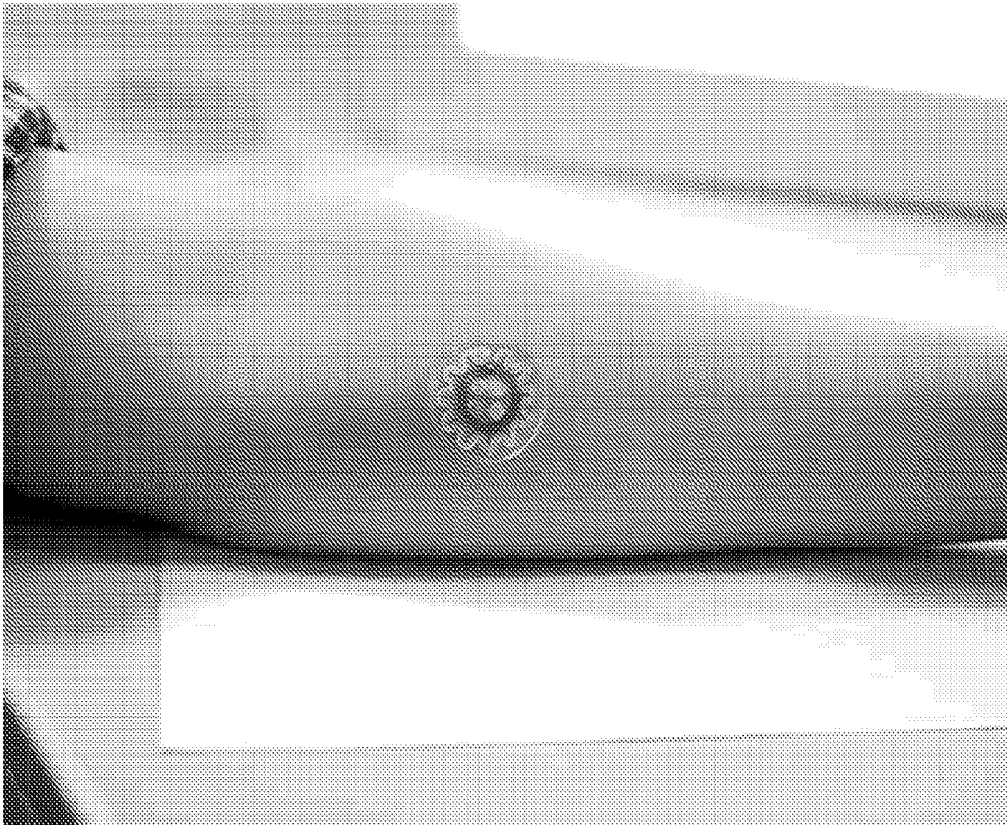


FIG. 11

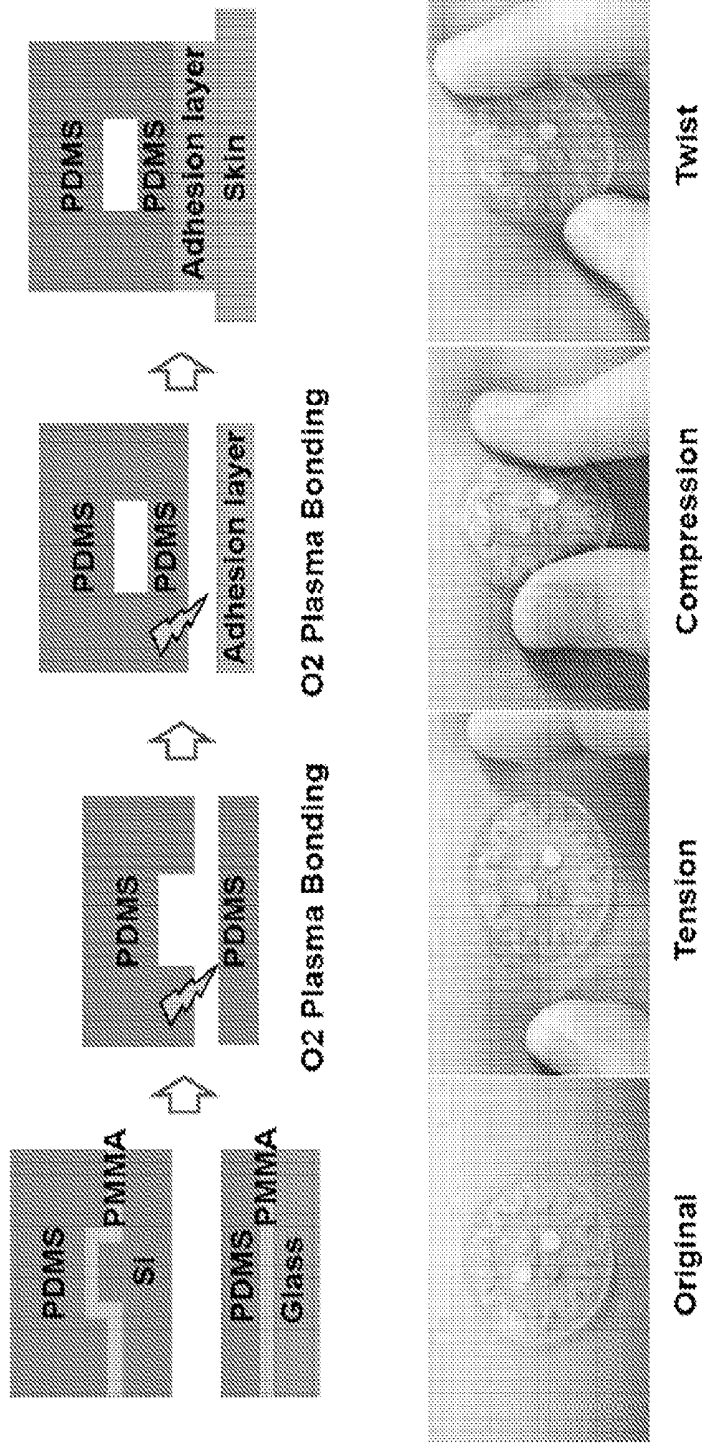


FIG. 12

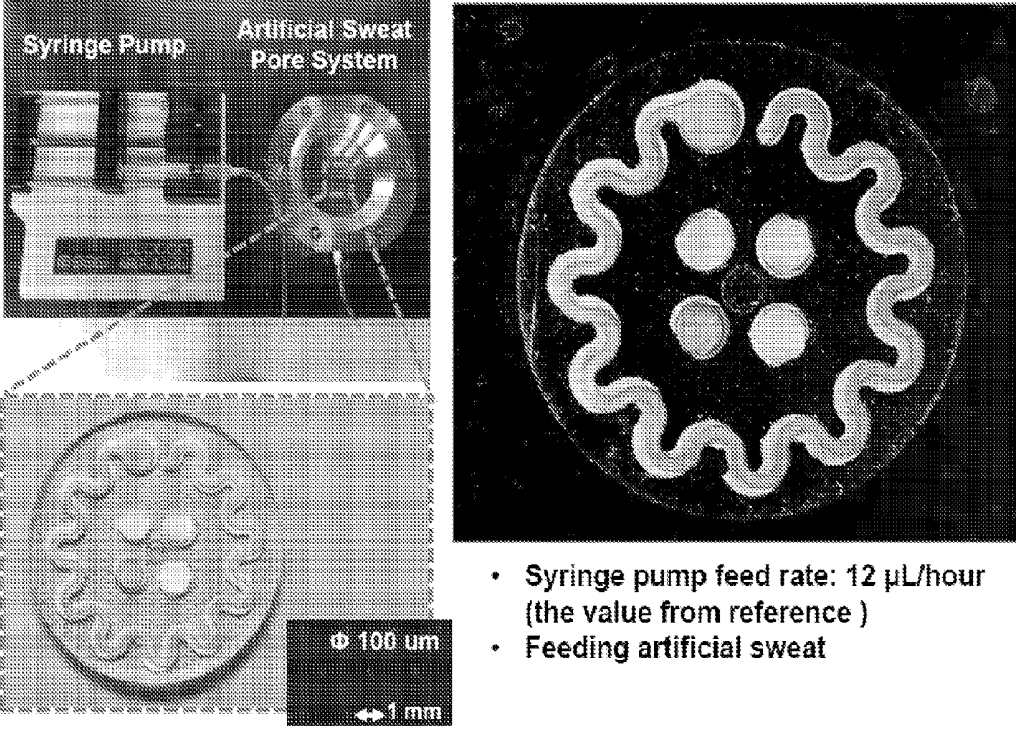


FIG. 13

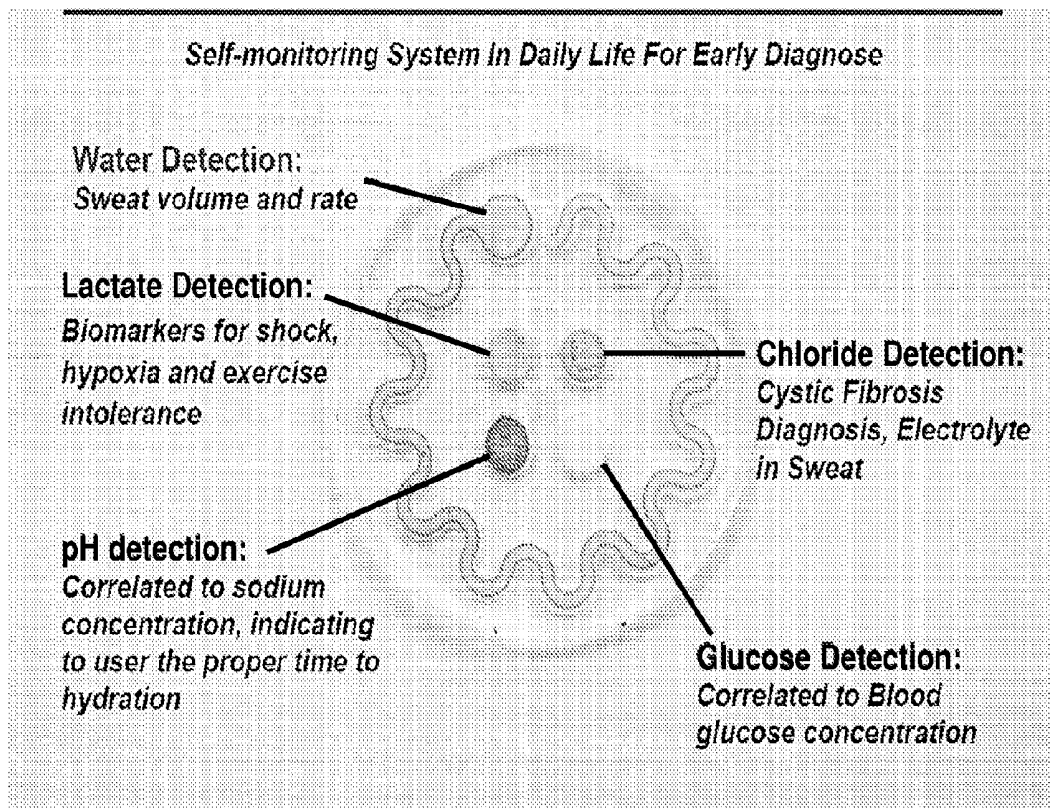


FIG. 14

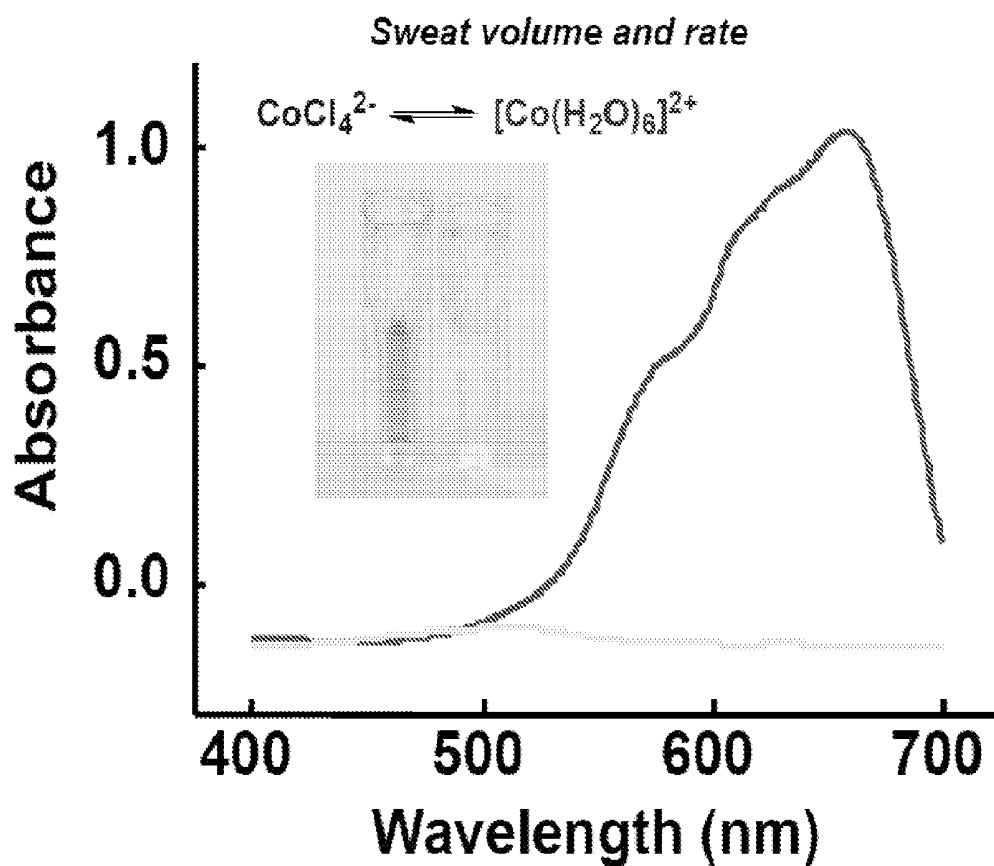


FIG. 15

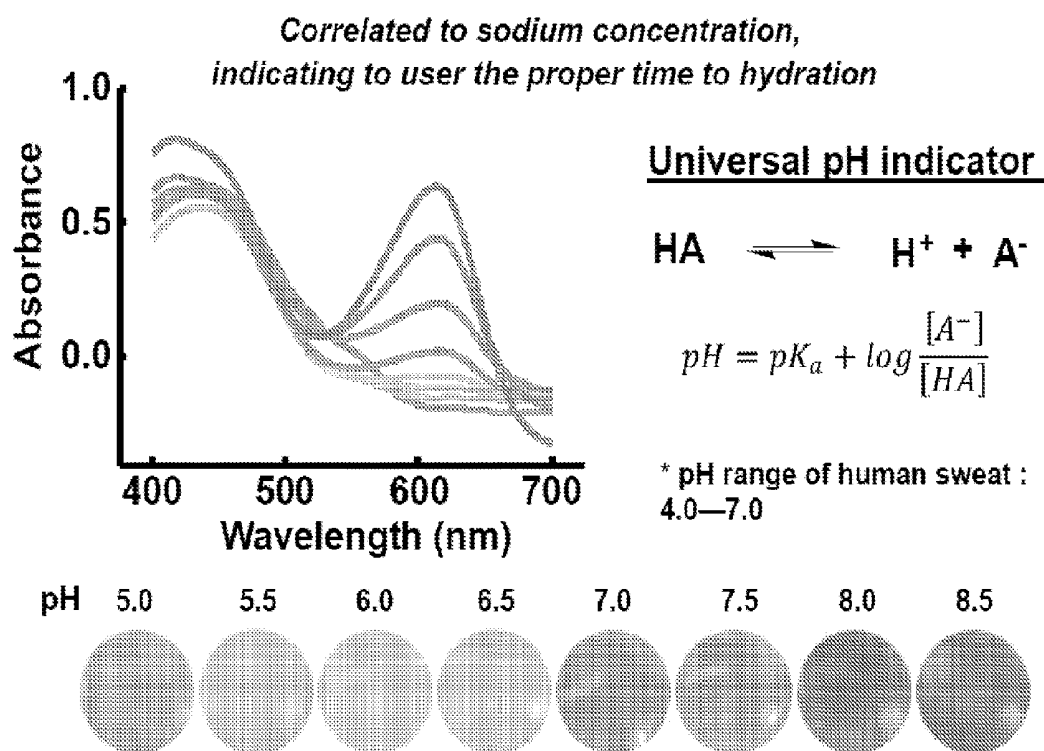


FIG. 16

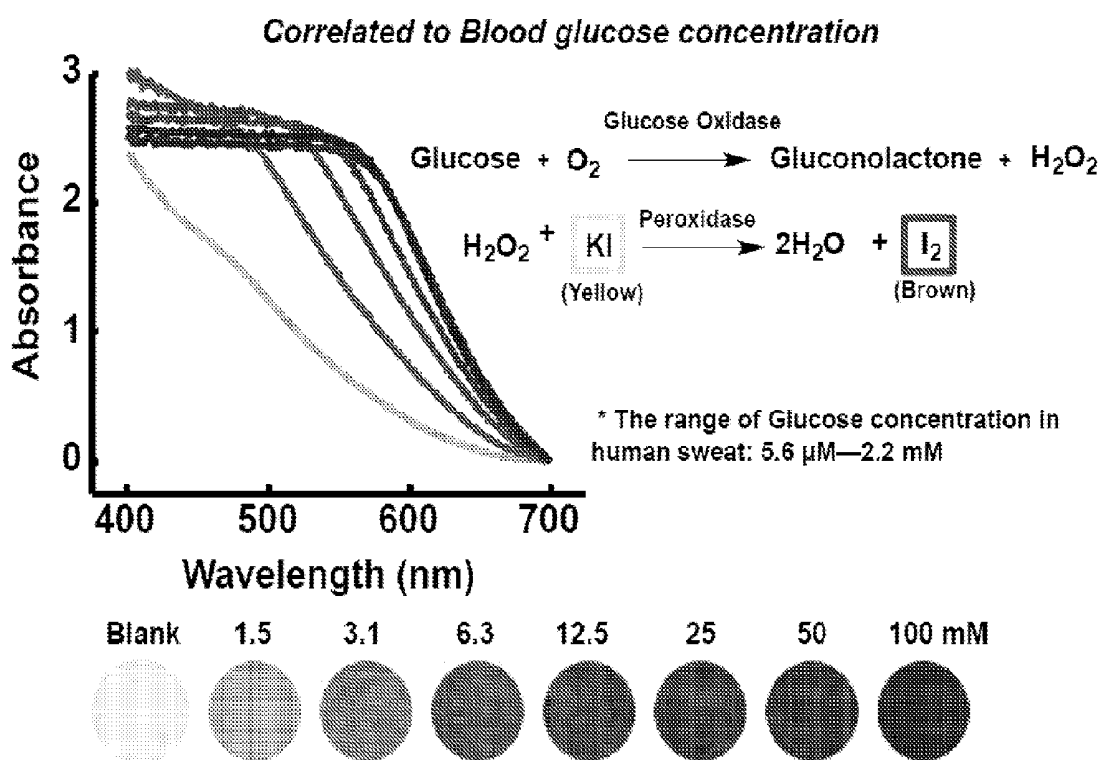


FIG. 17

Biomarkers for shock, hypoxia and exercise intolerance

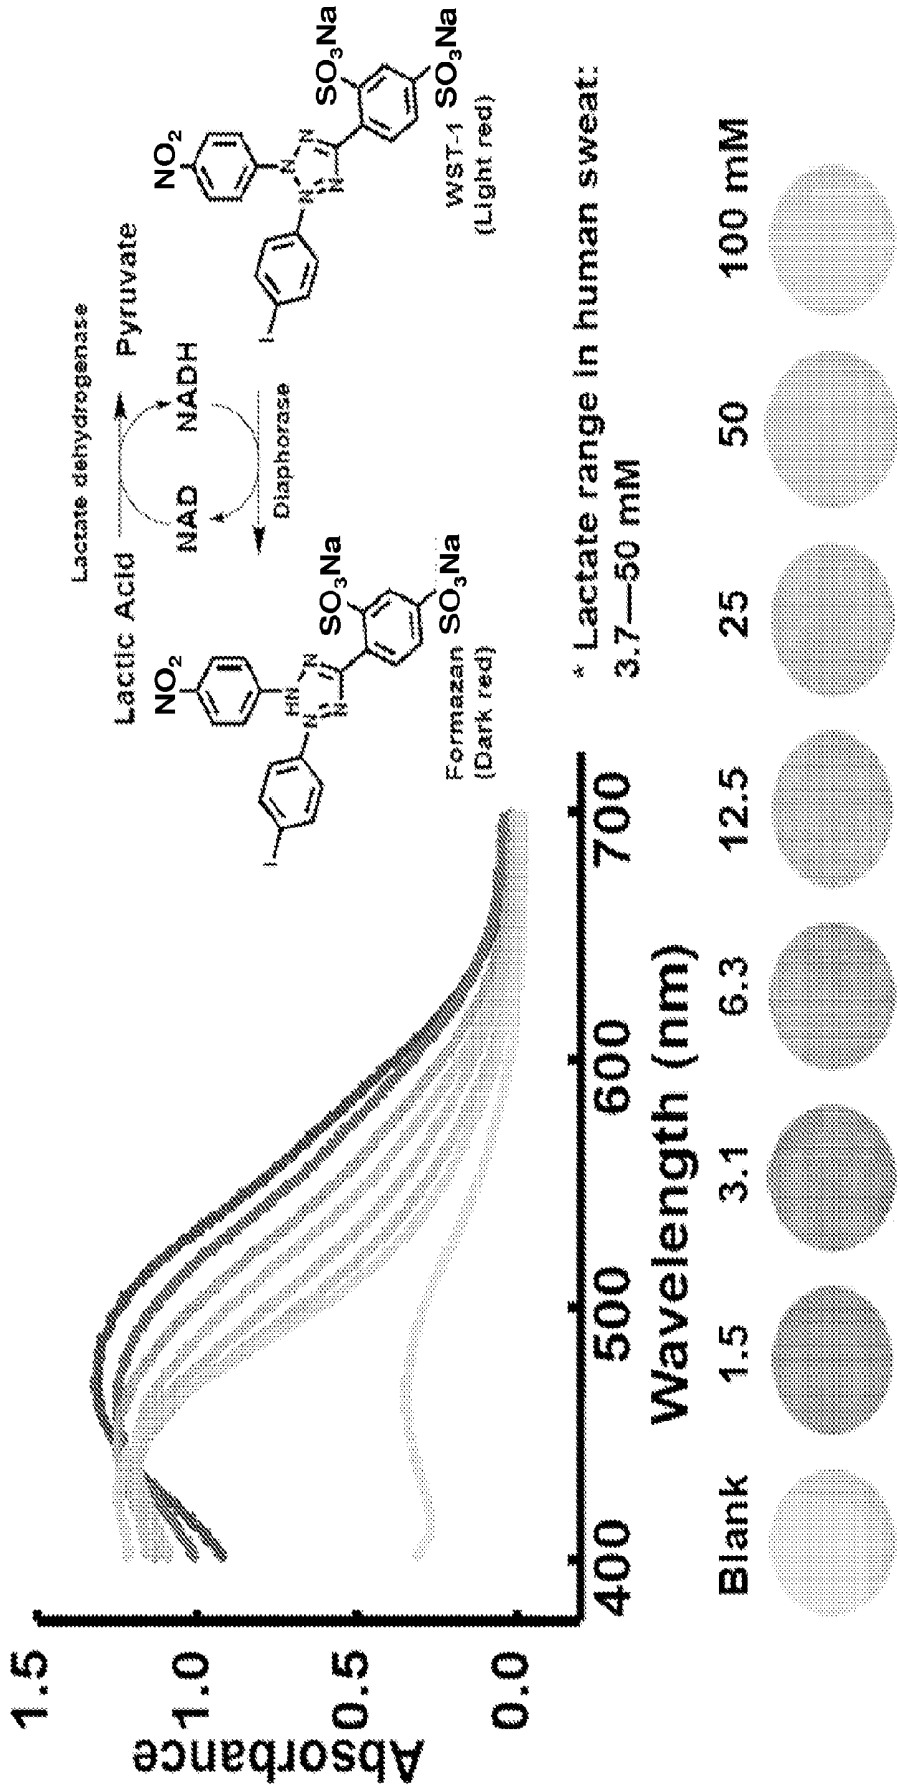


FIG. 18

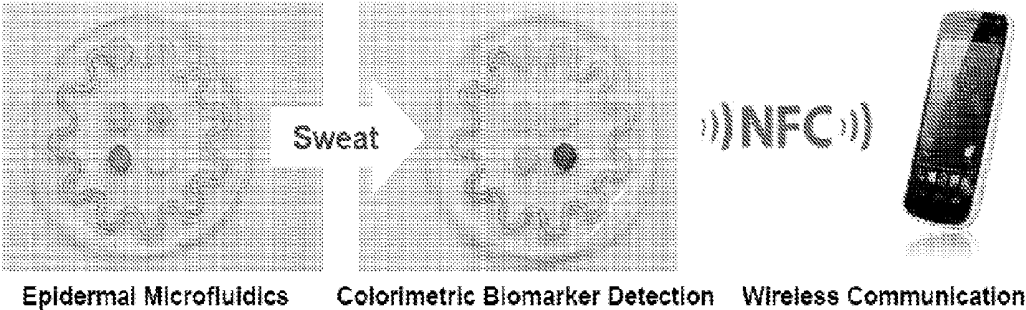


FIG. 19

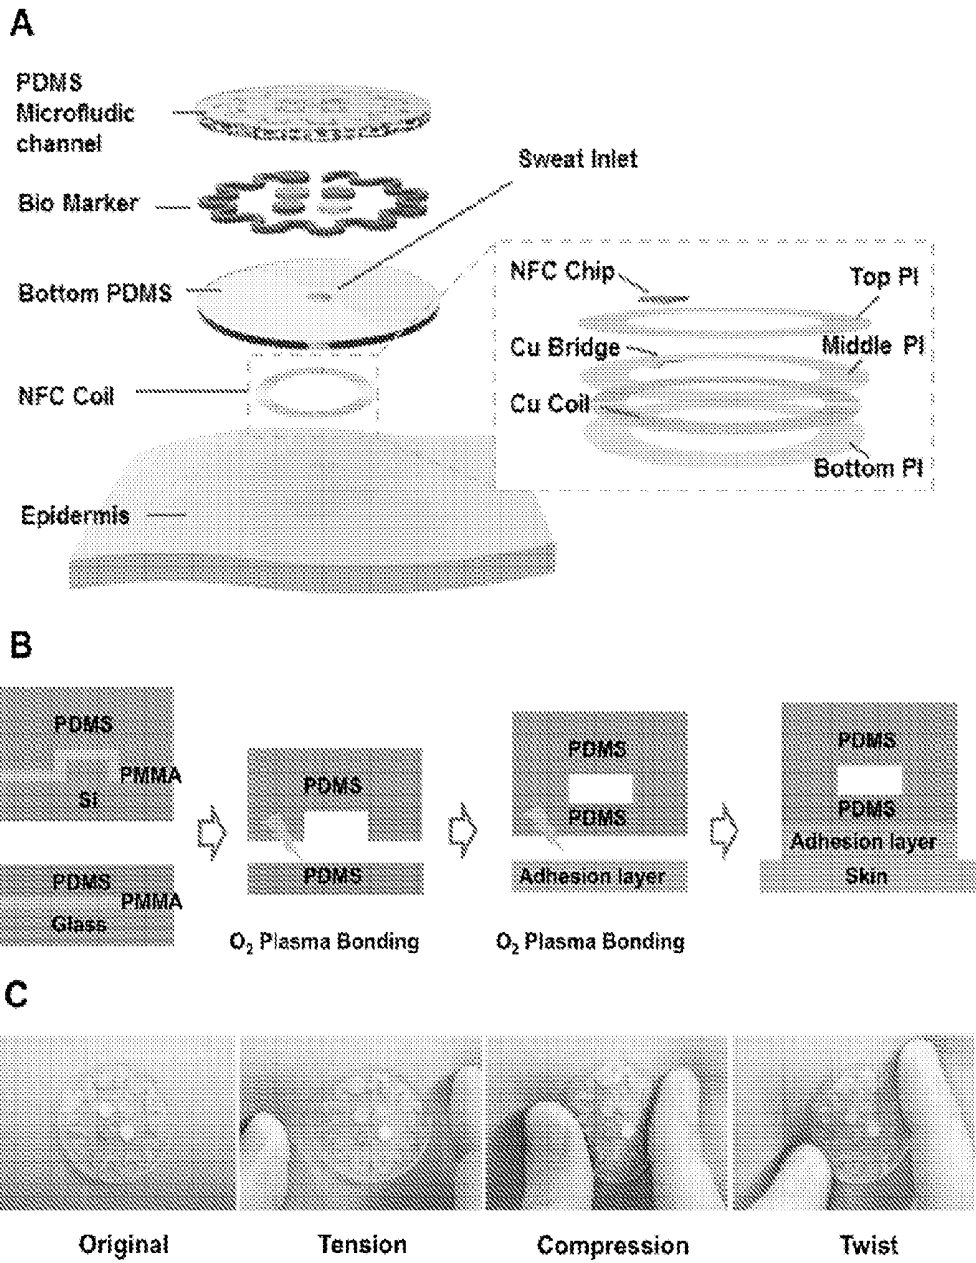


FIG. 20

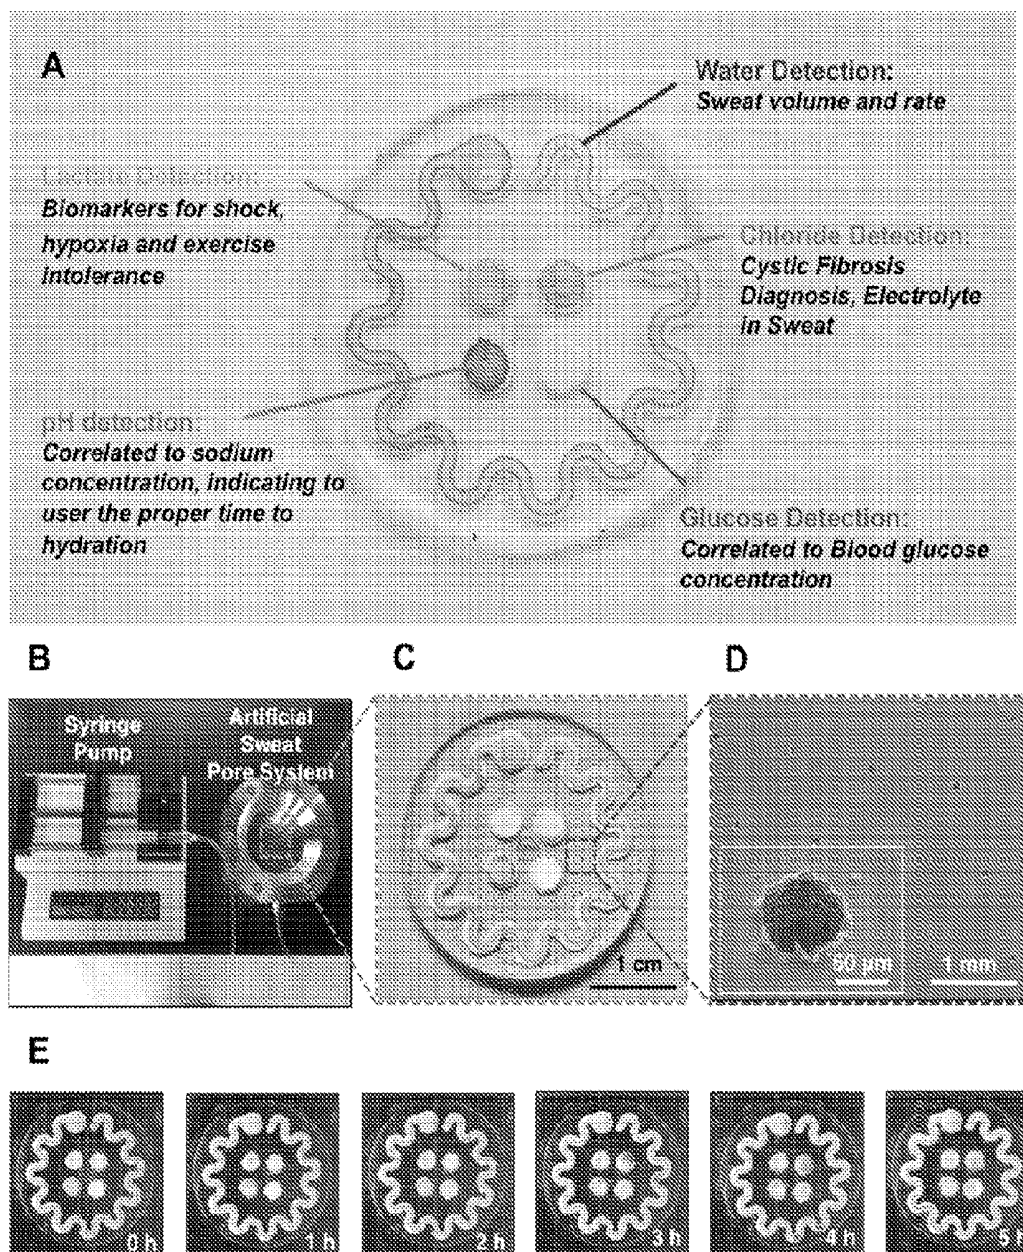


FIG. 21

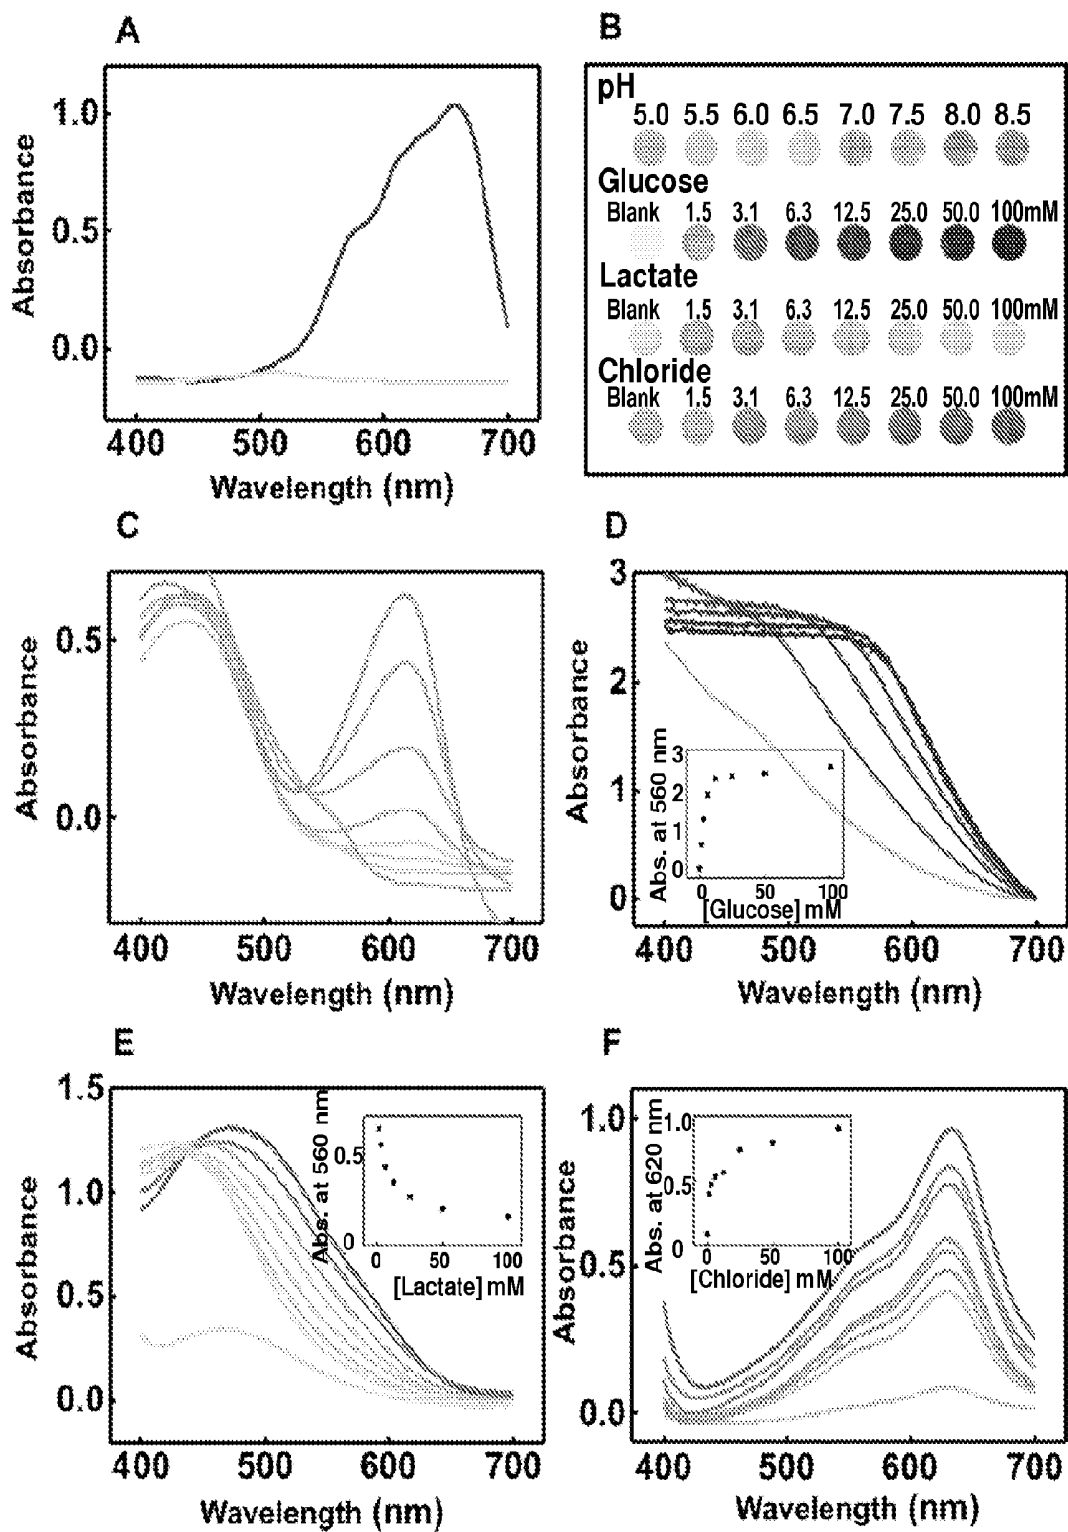


FIG. 22

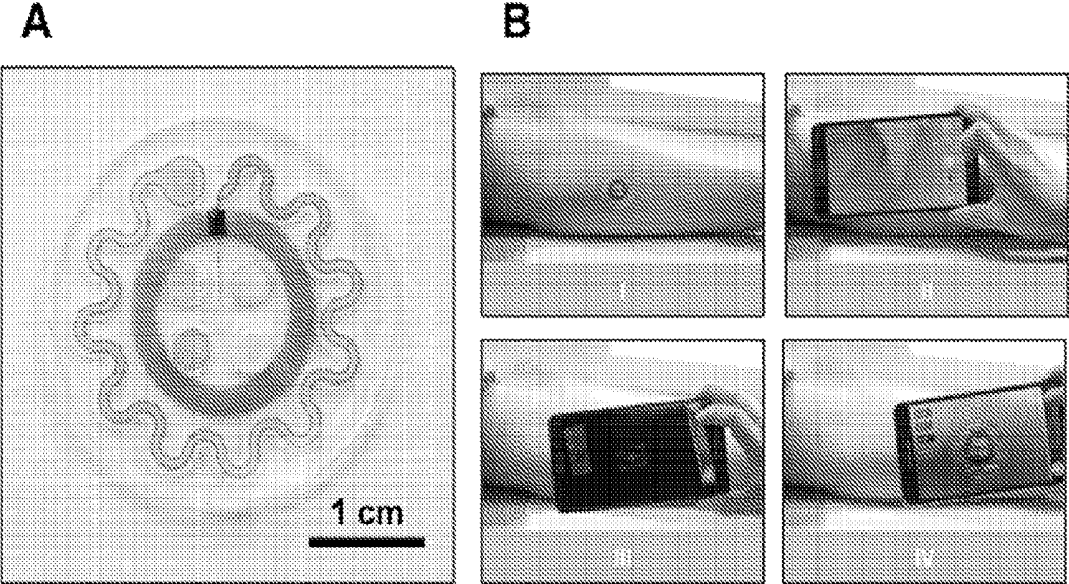


FIG. 23




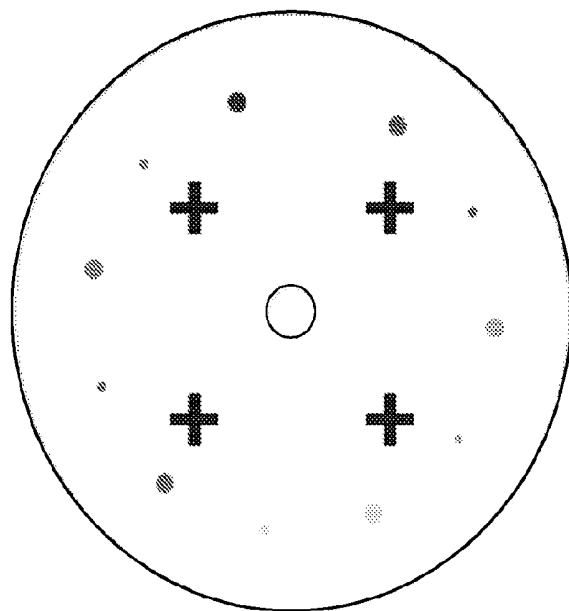


FIG. 24

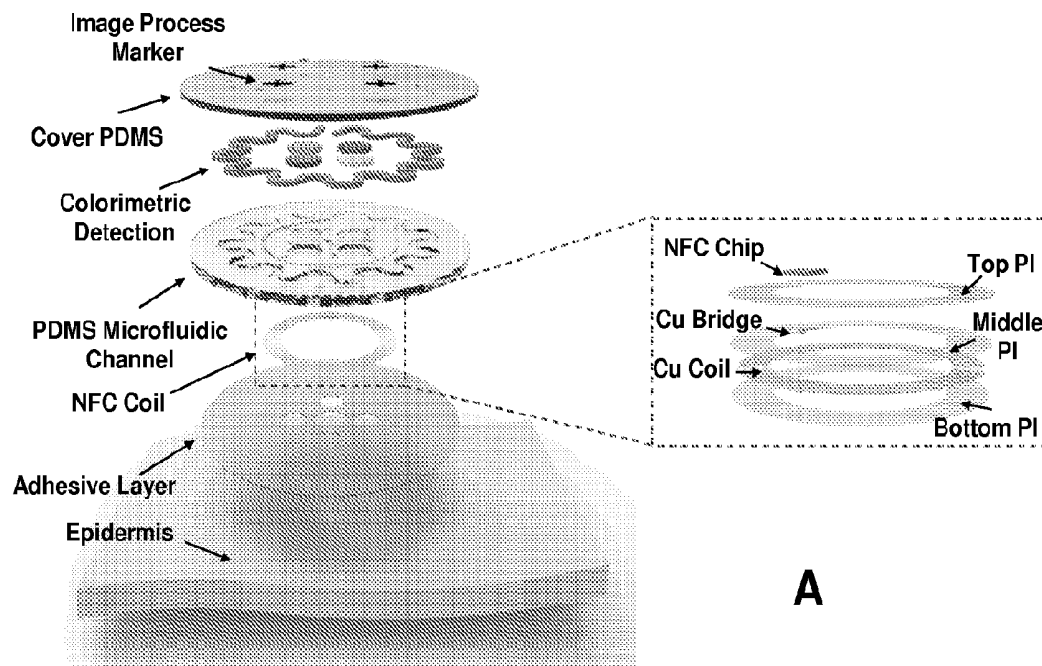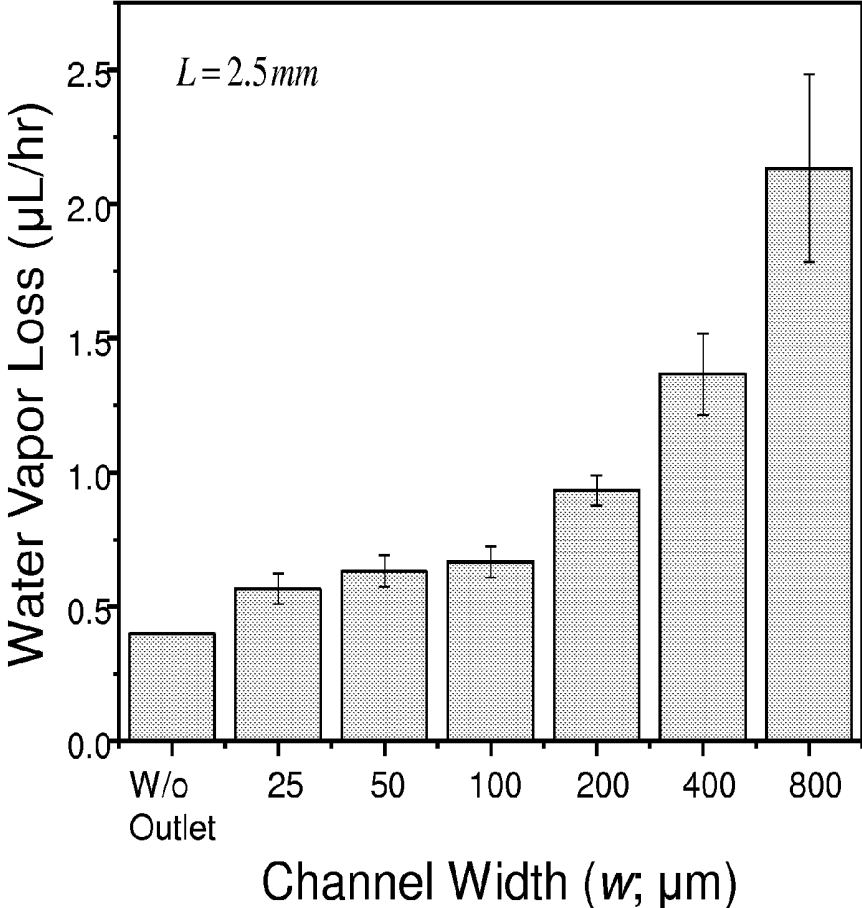

A

FIG. 25

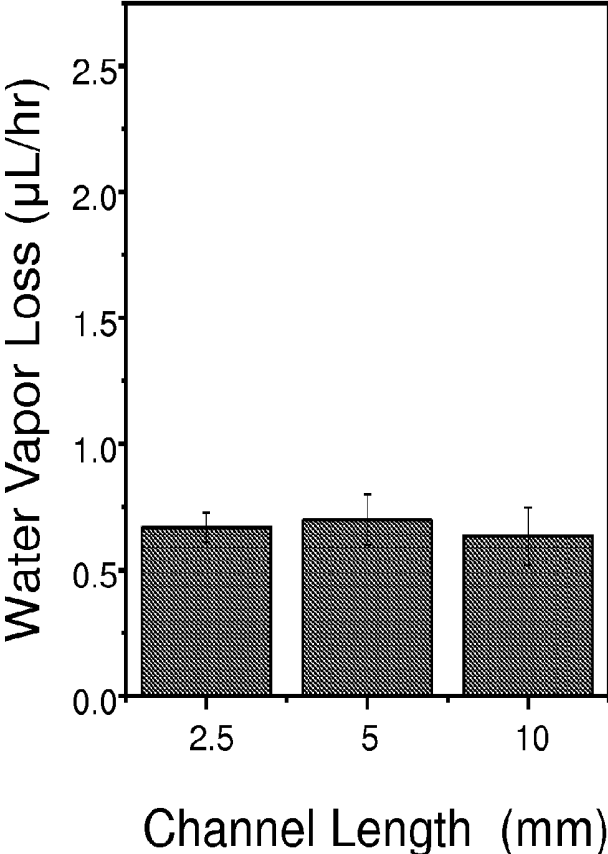

B

FIG. 25

Back pressure in side of channel



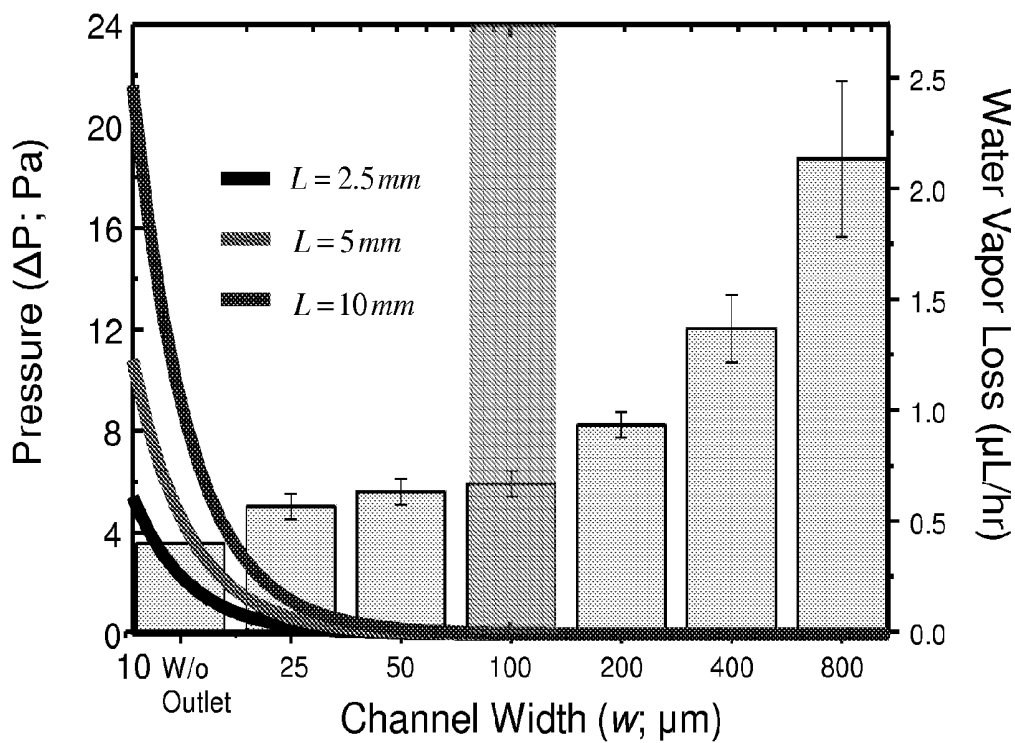


FIG. 26

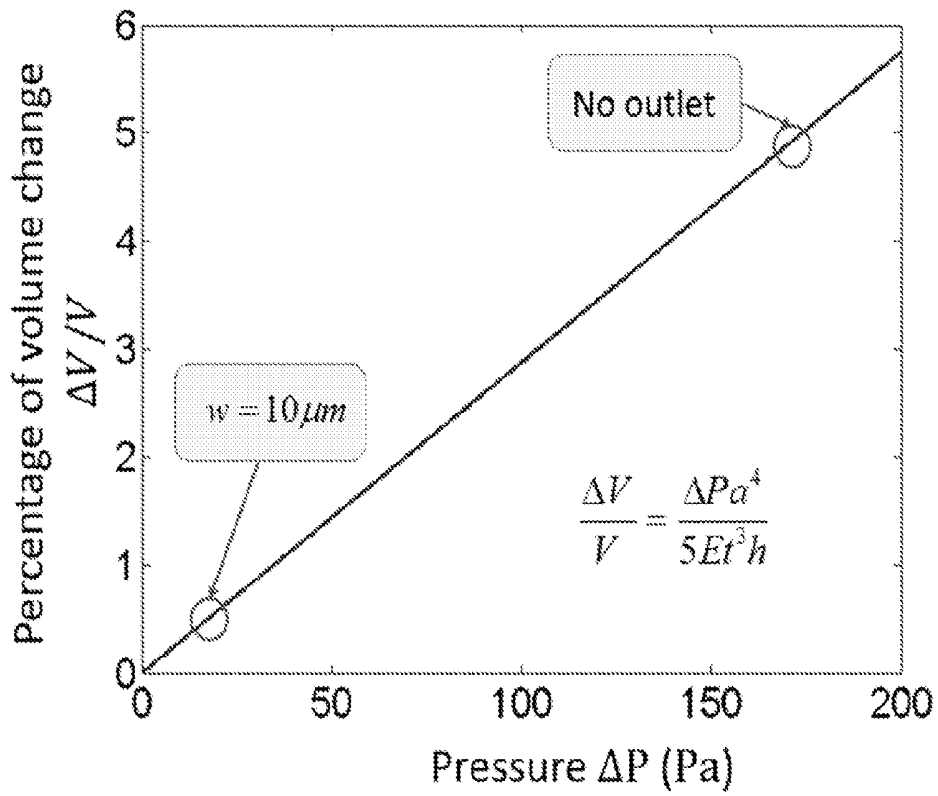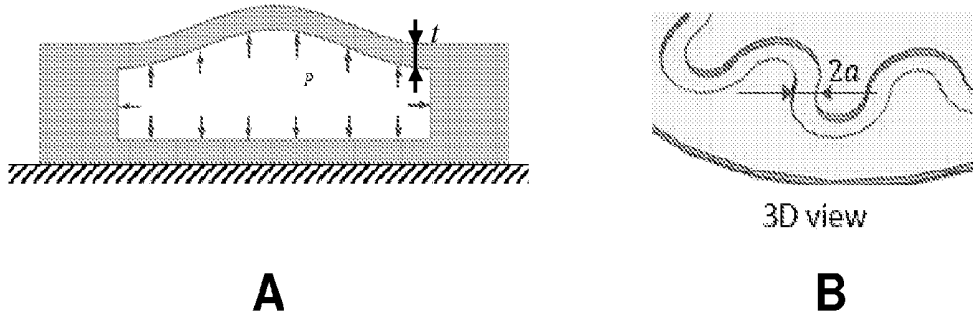

C

FIG. 27

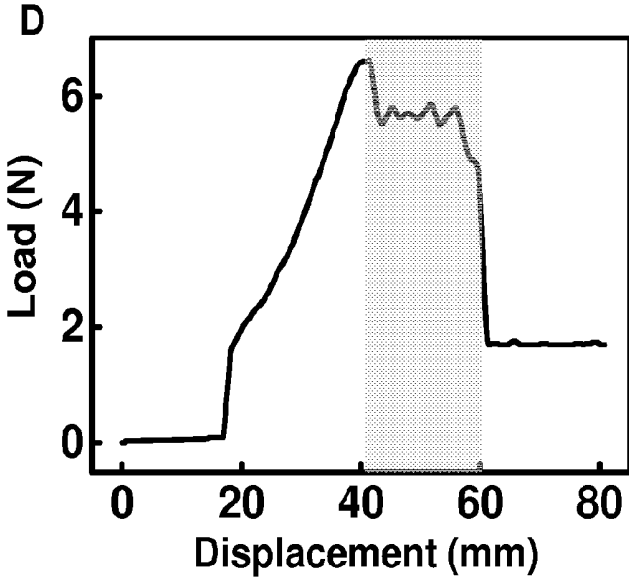
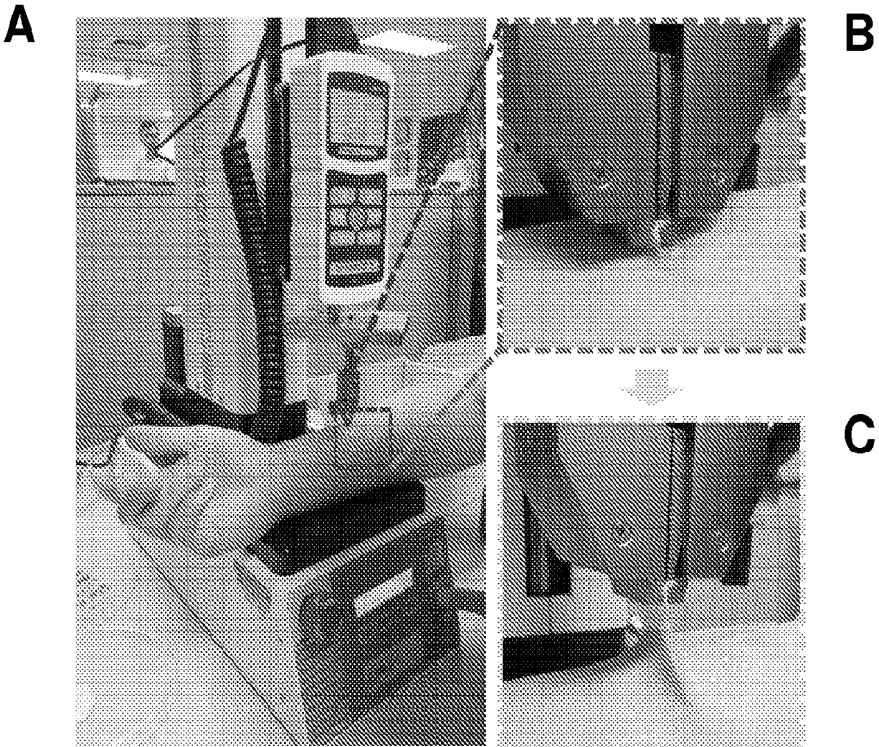


FIG. 28

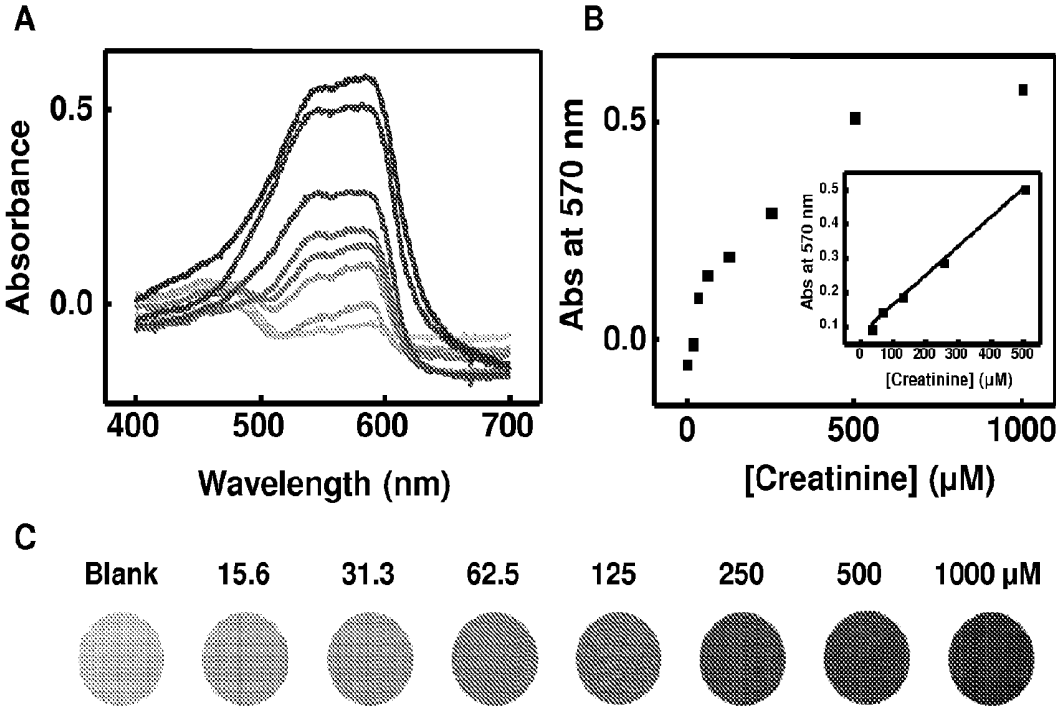


FIG. 29



FIG. 30


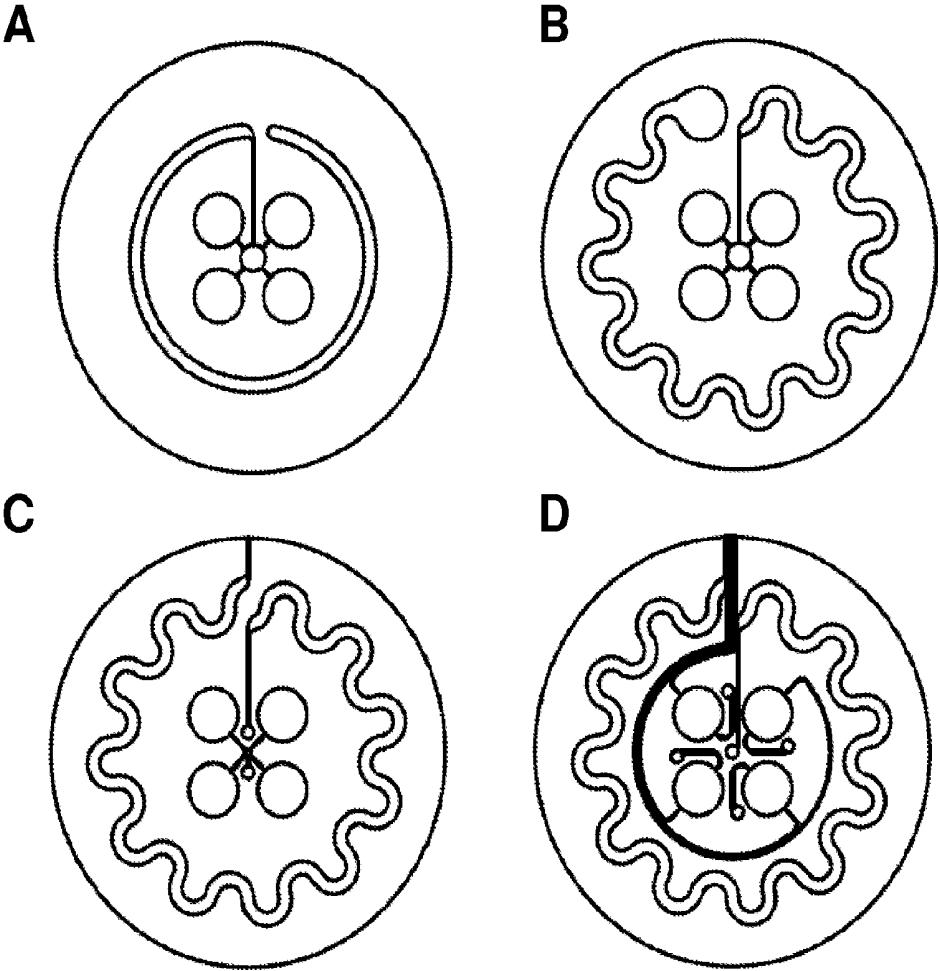


FIG. 31

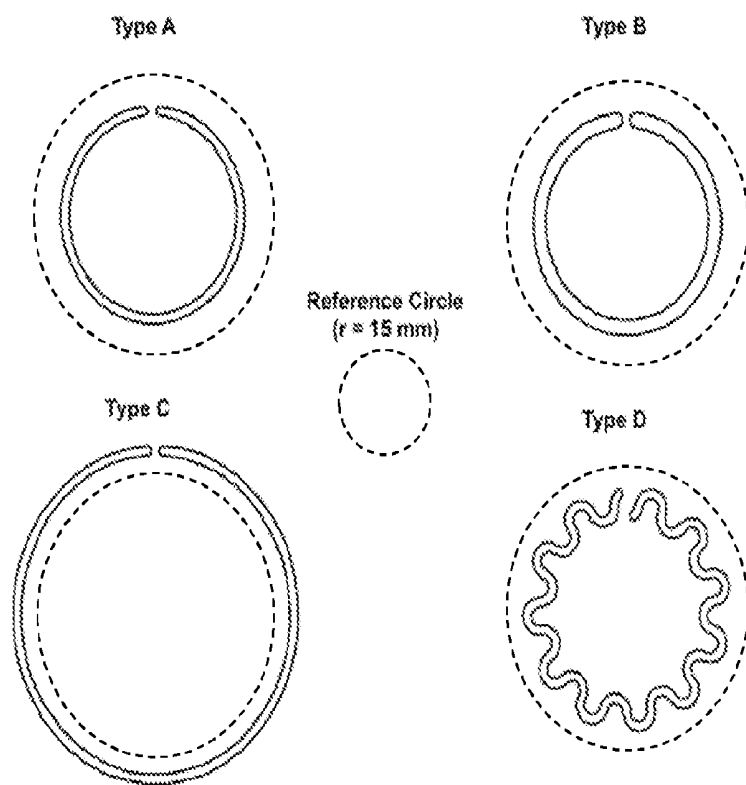

Type	Channel Width (mm)	Radius of Neutral Circle (mm)	Area (mm ²)
A	1.00	10.93	67.70
B	1.58	10.93	106.96
C	1.00	17.31	107.63
D	1.00	10.93	107.17

FIG. 32

DEVICES AND RELATED METHODS FOR EPIDERMAL CHARACTERIZATION OF BIOFLUIDS

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit and priority of U.S. Provisional Patent Application No. 62/035,823, filed Aug. 11, 2014, and U.S. Provisional Patent Application No. 62/142,877, filed Apr. 3, 2015, each of which is hereby incorporated by reference in its entirety.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

[0002] Not Applicable.

BACKGROUND

[0003] Emerging wearable sensor technologies offer attractive solutions for continuous, personal health/wellness assessment, forensic examination, patient monitoring and motion recognition. Recent advances in epidermal electronics provide classes of skin-mounted sensors and associated electronics in physical formats that enable intimate contact with the skin for long-term, reliable health monitoring.

[0004] An important measurement mode in such devices may involve the analysis of body fluids (e.g., blood, interstitial fluid, sweat, saliva, and tear), to gain insights into various aspects of physiological health. Such function in wearable sensors, generally, and epidermal electronics in particular, is relatively unexplored. Existing devices either use complex microfluidic systems for sample handling or involve purely concentration-based measurement without sample collection and storage, or access to parameters related to quantity and rate. In addition, mechanical fixtures, straps and/or tapes that are typically required to maintain contact of these devices with the skin do not lend themselves well to continuous, long term monitoring without discomfort.

SUMMARY OF THE INVENTION

[0005] Skin-mounted or epidermal devices and methods for monitoring biofluids are disclosed. The devices comprise a functional substrate that is mechanically and/or thermally matched to skin to provide durable adhesion for long-term wear. The functional substrates allow for the microfluidic transport of biofluids from the skin to one or more sensors that measure and/or detect biological parameters, such as rate of biofluid production, biofluid volume, and biomarker concentration. Sensors within the devices may be mechanical, electrical or chemical, with colorimetric indicators being observable by the naked eye or with a portable electronic device (e.g., a smartphone). By monitoring changes in an individual's health state over time, the disclosed devices may provide early indications of abnormal conditions.

[0006] Epidermal devices disclosed herein may be used to monitor parameters such as temperature, pressure, electric potential, impedance and biomarker concentration.

[0007] Analytes that may be detected by the disclosed devices include but are not limited to iron ion, copper ion, chromium ion, mercury ion, sodium ion, potassium ion, calcium ion, chloride ion, hydronium, hydroxide, ammonium, bicarbonate, urea, lactate, glucose, creatinine, ethanol, ketone, nitrite, nitrate, uric acid, glutathione, blood urea

nitrogen (BUN), human serum albumin (HSA), high-sensitivity C-reactive protein (hs-CRP), interleukin 6 (IL-6), cholesterol, brain natriuretic peptide (BNP) and glycoprotein.

TABLE 1

Examples of biofluids and their respective sampling methods	
Biological Fluid	Sampling Method
Saliva	Non-invasive
Sweat	
Gingival crevicular fluid	
Tears	
Interstitial fluid	Micro-needle
Blood	
	Reverse iontophoresis
	Thermal ablation

TABLE 2

Potential biomarkers for quantitative colorimetric detection	
Colorimetric detection reagent/scheme	Analyte biomarkers
Chromogen	Iron ion, copper ion, chloride ion, pH (H ⁺ and OH ⁻), bicarbonate
Enzymatic reaction	Urea, lactate, glucose, creatinine, ethanol, ketone, nitrite/nitrate, uric acid, glutathione, blood urea nitrogen (BUN)
Immunoassay	Human serum albumin (HSA), high-sensitivity C-reactive protein (hs-CRP), interleukin 6 (IL-6), cholesterol, brain natriuretic peptide (BNP), glycoprotein

[0008] The disclosed devices may mobilize and access biofluids by mechanical, electrical and/or thermal mechanisms including but not limited to surface wicking, microneedle extraction, reverse iontophoresis and/or thermal microablation.

[0009] In an embodiment, a device comprises at least one microneedle or an array of microneedles for accessing interstitial fluid or blood. Microneedles may, for example, be fabricated from polymeric materials, silicon or glass using known micromachining techniques. Some methods for making and using microneedles and microneedle arrays are disclosed, for example, in E. V. Mukerjee, "Microneedle array for transdermal biological fluid extraction and in situ analysis," *Sensors and Actuators A*, 114 (2004) 267-275. In an embodiment, a microneedle or microneedle array may be disposed at a surface of an epidermal device, for example, at a microchannel opening.

[0010] In an aspect, a device for monitoring a biofluid comprises a functional substrate that is mechanically matched to skin; wherein the functional substrate provides for microfluidic transport of the biofluid; and at least one sensor supported by the functional substrate.

[0011] In an aspect, a device for monitoring a biofluid comprises a functional substrate that is thermally matched to skin; wherein the functional substrate provides for microfluidic transport of the biofluid; and at least one sensor supported by the functional substrate.

[0012] In an aspect, a device for monitoring a biofluid comprises a functional substrate providing for microfluidic transport of the biofluid through one or more microfluidic

channels each having a substantially uniform lateral dimension; and at least one sensor supported by the functional substrate.

[0013] In an embodiment, a device for monitoring a biofluid further comprises a component for extracting interstitial fluid or blood from a subject. For example, the component for extracting interstitial fluid or blood may be selected from a microneedle component, a reverse iontophoresis component and a thermal microabrasion component.

[0014] In an embodiment, a functional substrate is an elastomeric substrate. In an embodiment, the functional substrate is substantially colorless and substantially transparent. In an embodiment, the functional substrate has a modulus less than or equal to 100 MPa and optionally in some embodiments less than or equal to 10 MPa. In an embodiment, the functional substrate has a modulus selected from a range of 10 kPa to 10 MPa and in some embodiments selected from a range of 100 kPa to 1 MPa. In an embodiment, the functional substrate has a thickness selected from a range of 500 μm to 2 mm and in some embodiments selected from a range of 500 μm to 1 mm. In some embodiments, the functional substrate is selected from the group consisting of polydimethylsiloxane (PDMS), polyurethane, cellulose paper, cellulose sponge, polyurethane sponge, polyvinyl alcohol sponge, silicone sponge, polystyrene, polyimide, SU-8, wax, olefin copolymer, polymethyl methacrylate (PMMA) and polycarbonate. In some embodiments, the functional substrate has a dielectric constant greater than or equal to 2.0. In some embodiments, the functional substrate has a dielectric constant selected from a range of 2.20 to 2.75. In some embodiments, the functional substrate has lateral dimensions or a diameter less than or equal to 700 mm². In some embodiments, the functional substrate has a permeability for the biofluid greater than or equal to 0.2 g/h m². In some embodiments, the functional substrate has a coefficient of thermal expansion selected from a range of 1^o C. ($\times 10^{-6}$) to 3^o C. ($\times 10^{-4}$). In some embodiments, the functional substrate has a porosity greater than or equal to 0.5.

[0015] In some embodiments, microfluidic transport is spontaneous microfluidic transport via capillary force.

[0016] In some embodiments, a device for monitoring a biofluid comprises at least one microfluidic channel having a substantially uniform lateral dimension. For example, the microfluidic channel may have a length selected from a range of 1 mm to 7 cm and optionally in some embodiments selected from a range of 1 cm to 5 cm. In some embodiments, a microfluidic channel has a width selected from a range of 100 μm to 1 mm and optionally in some embodiments selected from a range of 200 μm to 700 μm .

[0017] In some embodiments, the biofluid is selected from the group consisting of sweat, tears, saliva, gingival crevicular fluid, interstitial fluid, blood and combinations thereof.

[0018] In some embodiments, a sensor of the device is a non-pH colorimetric indicator. In some embodiments, the sensor of the device may comprise an electrical sensor, a chemical sensor, a biological sensor, a temperature sensor, an impedance sensor, an optical sensor, a mechanical sensor or a magnetic sensor. In some embodiments, the sensor of the device is an LC resonator.

[0019] In some embodiments, the device further comprises an actuator. For example, the actuator may generate electromagnetic radiation, acoustic energy, an electric field,

a magnetic field, heat, a RF signal, a voltage, a chemical change or a biological change. In some embodiments, the actuator comprises a heater, a reservoir containing a chemical agent capable of causing a chemical change or a biological change, a source of electromagnetic radiation, a source of an electric field, a source of RF energy or a source of acoustic energy.

[0020] In some embodiment, the device further comprises a transmitter, receiver or transceiver. In some embodiments, the device further comprises at least one coil. For example, the at least one coil may be a near-field communication coil or an inductive coil. In some embodiments, the at least one coil comprises a serpentine trace.

[0021] In some embodiments, the sensor is a colorimetric indicator. For example, the colorimetric indicator may be disposed within a cavity of the functional substrate. The cavity may be connected to an opening at a surface of the functional substrate by a microfluidic channel.

[0022] In some embodiments, the colorimetric indicator changes color in response to an analyte in the biofluid. In some embodiments, the colorimetric indicator is embedded in a matrix material selected from the group consisting of filter paper, polyhydroxyethylmethacrylate hydrogel (pHEMA), agarose gel, sol-gel and combinations thereof. In some embodiments, the colorimetric indicator comprises a cobalt dichloride salt. In some embodiments, the colorimetric indicator comprises a chemical selected from the group consisting of glucose oxidase, peroxidase, potassium iodide and combinations thereof. In some embodiments, the colorimetric indicator comprises a chemical selected from lactate dehydrogenase, diaphorase, formazan dyes and combinations thereof. In some embodiments, the colorimetric indicator comprises a 2,4,6-tris(2-pyridyl)-s-triazine (TPTZ) complexed with mercury ion or iron ion. In some embodiments, the colorimetric indicator comprises a 2,2'-bicinchoninic acid. In some embodiments, the colorimetric indicator comprises a 1,10-phenanthroline. In some embodiments, the colorimetric indicator comprises a universal pH indicator.

[0023] In some embodiments, the device is a skin-mounted sensor. In some embodiments, the skin-mounted sensor quantitatively and/or qualitatively monitors the biofluid of a subject.

[0024] In some embodiments, the device has a modulus and a thickness within a factor of 1000 of a modulus and a thickness of an epidermal layer of the skin of a subject, optionally for some embodiments a factor of 10 of a modulus and a thickness of an epidermal layer of the skin of a subject, and optionally for some embodiments a factor of 2 of a modulus and a thickness of an epidermal layer of the skin of a subject. In an embodiment, for example, the device has an average modulus equal to or less than 100 times, optionally equal to or less than 10 times, the average modulus of the skin at the interface.

[0025] In an embodiment, for example, the device has an average thickness less than or equal to 3000 microns, optionally for some embodiments less than or equal to 1000 microns. In an embodiment, for example, the device has an average thickness selected over the range of 1 to 3000 microns, optionally for some applications selected over the range of 1 to 1000 microns.

[0026] In some embodiments, the device has an average modulus less than or equal to 100 MPa, optionally for some embodiments less than or equal to 500 kPa, optionally for

some embodiments less than or equal to 200 KPa, and optionally for some embodiments less than or equal to 100 KPa. In some embodiments, the device has an average modulus selected from a range of 0.5 kPa to 100 MPa, optionally for some embodiments 0.5 kPa to 500 kPa, and optionally for some embodiments 1 kPa to 100 kPa.

[0027] In some embodiments, the device has a net bending stiffness less than or equal to 1 mN m, optionally for some embodiments less than or equal to 1 nN m. In some embodiments, the device has a net bending stiffness selected from a range of 0.1 nN m to 1 N m, optionally for some embodiments selected from a range of 0.1 nN m to 1 mN m, and optionally for some embodiments selected from a range of 0.1 nN m to 1 nN m.

[0028] In some embodiments, the device has a footprint selected from a range of 10 mm² to 2000 cm², and optionally selected from a range of 300 mm² to 2000 cm².

[0029] In an aspect, a method of making a device for monitoring a biofluid comprises: providing a functional substrate that is mechanically matched to skin; wherein the functional substrate provides for microfluidic transport of the biofluid; and providing at least one sensor supported by the functional substrate.

[0030] In an aspect, a method of making a device for monitoring a biofluid comprises: providing a functional substrate that is thermally matched to skin; wherein the functional substrate provides for microfluidic transport of the biofluid; and providing at least one sensor supported by the functional substrate.

[0031] In an aspect, a method of making a device for monitoring a biofluid comprises: providing a functional substrate that provides for microfluidic transport of the biofluid through one or more microfluidic channels each having a substantially uniform lateral dimension; and providing at least one sensor supported by the functional substrate.

[0032] In an aspect, a method for monitoring a biofluid comprises: providing a device comprising a functional substrate that is mechanically matched to skin; wherein the functional substrate provides for microfluidic transport of the biofluid; and at least one sensor supported by the functional substrate; applying the device to the skin of a subject; and obtaining data from the at least one sensor; wherein the data provide quantitative and/or qualitative information about the biofluid of the subject.

[0033] In an aspect, a method for monitoring a biofluid comprises: providing a device comprising a functional substrate that is thermally matched to skin; wherein the functional substrate provides for microfluidic transport of the biofluid; and at least one sensor supported by the functional substrate; applying the device to the skin of a subject; and obtaining data from the at least one sensor; wherein the data provide quantitative and/or qualitative information about the biofluid of the subject.

[0034] In an aspect, a method for monitoring a biofluid comprises: providing a functional substrate that provides for microfluidic transport of the biofluid through one or more microfluidic channels each having a substantially uniform lateral dimension; and at least one sensor supported by the functional substrate; applying the device to the skin of a subject; and obtaining data from the at least one sensor; wherein the data provide quantitative and/or qualitative information about the biofluid of the subject.

BRIEF DESCRIPTION OF THE DRAWINGS

[0035] FIG. 1. (a) Schematic illustration of a passive wireless capacitive sensor designed for sensing of sweat from the surface of the skin. Pictures of a device in (b) longitudinal and (c) latitudinal states of deformation, and crumpled between the fingers (d). Pictures of a device mounted on the skin in (e) undeformed, (f) uniaxially stretched and (g) biaxially stretched configurations.

[0036] FIG. 2. (a) Scanning electron micrograph of a sensor on a PUR substrate coated with a thin silicone film; the regions colorized in yellow represent the interdigitated gold electrodes. (b) Picture of a sweat sensor and a reference sensor on the arm of a volunteer for in-vivo testing. (c) Picture of a sweat sensor underneath a primary coil. A syringe needle inserted into the sensor delivers controlled amounts of a buffer solution through a syringe pump. (d) Representative data showing the response of the sensor (resonant frequency, f_0) as a function of time after introduction of 0.6 mL buffer solution (labeled 1). The initial response (labeled 2) corresponds to wicking of the solution into the porous substrate, to yield a stable overall shift in f_0 (labeled 3). As the solution evaporates over the next several hours, f_0 recovers to approximately the initial value. The inset shows the phase difference measured by the primary coil at the three time points indicated in the main frame. (e, f) Results of testing on two volunteers, with comparisons to changes in weight evaluated using similar porous substrates (without detection coils) placed next to the sensors. Both f_0 and the weight of the sensors calibrated from f_0 are shown, along with comparison to the weight of the reference substrates. (g) Phase response of a sensor under biaxial strain from 0 to 27%. (h) Phase response as a function of concentration of sodium chloride, from 0 to 4.5 g/L. (i) Change in f_0 of a sweat sensor on a CP substrate as a function of time during controlled injection of 0.6 mL buffer solution.

[0037] FIG. 3. (a) Wireless sweat sensors based on different porous substrates. (b) SEM images of the substrates coated with thin layer of silicone to facilitate chemical bonding between the sensors and the substrates. (c) Weight gain of different substrate materials associated with immersion in water. (d) Porosity of the substrate materials. (e) Images of strips of the substrate materials when partially immersed into water with red dye. (f) Water permeability of the substrate materials.

[0038] FIG. 4. (a) Images that illustrate a simple colorimetric detection scheme, based on systematic increases in transparency with water absorption. (b) The ratio of RGB intensity for a sensor like the one illustrated in (a), as a function of water absorption. (c) An image and vector diagrams corresponding to a sensor and its expansion due to water absorption. (d) Series of pictures of a sensor doped with a pH indicator, each collected with absorbed water at a different pH value. (e) Absorbance of RGB channels at different pH values. (f) Absorbance of RGB channels at different copper concentrations. (g) Absorbance of RGB channels at different iron concentrations.

[0039] FIG. 5. (a) Capacitance values of a coaxial cable probe when in contact with sensors on CP and PUR substrates injected with 0.6 mL buffer solution. (b) Stability of a sweat sensor at temperatures from 25 to 45° C. (c) Time variation of f_0 for a sweat sensor on a silicone substrate in response to the injection of 0.6 mL buffer solution. (d) Drift and stability of a sensor output at dry state over an extended period of 3 hours.

[0040] FIG. 6. (a) A sensor is biaxially stretched by two perpendicular stretchers at a strain from 0 to 27%. (b) Expansion of the surface area of the sensor in response to water absorption.

[0041] FIG. 7. (a) SEM images of porous materials, showing that the pores of PUR and Silicone dressing are uniform and that the pores of RCS, PVAS, and CP are amorphous. (b) Contact angle measurements performed by partially immersing strips of the porous materials into water dyed with red color, and recording the angle at the interface of two materials.

[0042] FIG. 8. (a) Color changes in the sensor when the free copper concentration changes from 0 to 1 mg/L, (b) Color changes in the sensor when the iron concentration changes from 0 to 0.8 mg/L.

[0043] FIG. 9. (a)-(g) Fabrication processes for a wireless sweat sensor.

[0044] FIG. 10. Exploded view of a colorimetric sensor comprising a near-field communication coil.

[0045] FIG. 11. Photograph of the device of FIG. 10 adhered to the skin of a subject.

[0046] FIG. 12. Fabrication method and adhesion test on skin.

[0047] FIG. 13. Artificial sweat pore test using a syringe to feed artificial sweat at a rate of 12 $\mu\text{L/hr}$.

[0048] FIG. 14. Colorimetric detection of various biomarkers using a sweat sensor for self-monitoring and early diagnosis.

[0049] FIG. 15. Absorbance spectrum illustrating the color change of a reactant that may be used to determine sweat volume and rate.

[0050] FIG. 16. Absorbance spectrum and legend illustrating the color change of a reactant(s) that may be used to determine sweat pH, which may be correlated with sodium concentration, indicating to a user the proper time to hydrate.

[0051] FIG. 17. Absorbance spectrum and legend illustrating the color change of a reactant(s) that may be used to determine glucose concentration in sweat, which may be correlated with blood glucose concentration.

[0052] FIG. 18. Absorbance spectrum and legend illustrating the color change of a reactant(s) that may be used to determine lactate concentration in sweat, which may provide an indication of shock, hypoxia and/or exercise intolerance.

[0053] FIG. 19. A sweat sensor incorporating colorimetric biomarker indicators provides qualitative and quantitative data that may be observed by the naked eye and/or wirelessly observed by a detection device, such as a smartphone.

[0054] FIG. 20. (A) Schematic illustration of an epidermal microfluidic sweat sensor providing information of sweat volume and rate as well as concentration of biomarkers in sweat incorporated with wireless communication electronics. (B) Fabrication process for flexible and stretchable epidermal microfluidics. (C) Pictures of fabricated sweat sensors mounted on the skin under various mechanical stresses.

[0055] FIG. 21. (A) Picture of fabricated epidermal sweat sensor indicating informative detection schemes for sweat analysis. (B) In vitro artificial sweat pore system set up. (C) Optical image of sweat sensor applied on artificial pore membrane. (D) Scanning electron microscopy (SEM) image of the artificial pore membrane. Inset shows magnified image of single pore. (E) Representative images of sweat patch on the artificial sweat pore system while mimicking

sweating events for 5 h. Sweat flowed continuously in the microfluidic systems along with color change accordingly.

[0056] FIG. 22. Analytical colorimetric detections and respective UV-Vis spectrums of critical biomarkers in sweat. (A) Spectrum of anhydrous (blue) and hexahydrate (pale pink) cobalt (II) chloride. The presented color in the spectrum corresponds to the observed color with naked eye. (B) Optical images of resulted color change of the filter papers as a function of various pH values and analyte concentrations. (C) Spectrum of universal pH assay with various buffer solutions in the range of pH 5.0-8.5. (D-F) Spectrum of biomarkers in sweat as a function of concentration of analytes: glucose (D), lactate (E) and chloride (F). The presented color for each spectrum corresponds to exhibited color on paper-based colorimetric results, which is presented in image (B). Insets indicate calibration curves of respective analytes corresponding with concentration in the optical images (B). All spectra were determined at room temperature.

[0057] FIG. 23. (A) An image of fabricated sweat sensor incorporated with near-field communication electronics. (B) Demonstration pictures of wireless communication via smartphone. The RGB information was determined using an android image analysis app.

[0058] FIG. 24. (A) Schematic illustration of an epidermal microfluidic sweat sensor providing information on sweat volume and rate as well as concentration of biomarkers in sweat incorporated with wireless communication electronics and an adhesive layer. (B) Schematic illustration of image process markers applied to an epidermal microfluidic sweat sensor.

[0059] FIG. 25. Graphical representation of water loss as a function of outlet channel (A) width and (B) length.

[0060] FIG. 26. Graphical representation of back pressure inside a channel showing that shorter outlet channels and larger channel widths produce lower back pressures.

[0061] FIG. 27. (A) Schematic illustration of a cross section of a microfluidic channel deformed due to pressure. (B) Schematic illustration of a top perspective view of a section of an epidermal microfluidic sweat sensor showing a width of the microfluidic channel. (C) Graphical representation of deformation shown as volume change due to pressure.

[0062] FIG. 28. (A) Experimental set-up for 90° peel adhesion property testing (standard ISO 29862:2007) using a force gauge (Mark-10, Copiague, N.Y.). Images of (B) holding devices adhered on the skin with a force gauge and (C) peeling devices at an angle of 90°. (D) Force measurement while displacing the device at a rate of 300 mm/min indicated by the gray region where peeling occurs. Determined average peeling force is 5.7 N.

[0063] FIG. 29. Colorimetric determination of creatinine. (A) UV-VIS spectrum with various creatinine concentrations (i.e., 15-1000 μM) and (B) constructed calibration based on this spectrum. The presented color for each spectrum corresponds to exhibited color on paper-based colorimetric detection reservoirs as a function of creatinine concentration, which is presented in optical image (C).

[0064] FIG. 30. Colorimetric determination of ethanol. (A) UV-VIS spectrum with various ethanol concentrations (i.e., 0.04-7.89% (w/v)) and (B) constructed calibration based on this spectrum. The presented color for each spectrum corresponds to exhibited color on paper-based colorimetric detection reservoirs as a function of ethanol concentration, which is presented in optical image (C).

metric detection reservoirs as a function of ethanol concentration, which is presented in optical image (C).

[0065] FIG. 31. (A)-(D) Various microfluidic sweat sensor designs.

[0066] FIG. 32. Various types of orbicular channel designs and respectively calculated channel properties.

DETAILED DESCRIPTION OF THE INVENTION

[0067] In general, the terms and phrases used herein have their art-recognized meaning, which can be found by reference to standard texts, journal references and contexts known to those skilled in the art. The following definitions are provided to clarify their specific use in the context of the invention.

[0068] “Functional substrate” refers to a substrate component for a device having at least one function or purpose other than providing mechanical support for a component(s) disposed on or within the substrate. In an embodiment, a functional substrate has at least one skin-related function or purpose. In an embodiment, a functional substrate of the present devices and methods exhibits a microfluidic functionality, such as providing transport of a bodily fluid through or within the substrate, for example via spontaneous capillary action or via an active actuation modality (e.g. pump, etc.). In an embodiment, a functional substrate has a mechanical functionality, for example, providing physical and mechanical properties for establishing conformal contact at the interface with a tissue, such as skin. In an embodiment, a functional substrate has a thermal functionality, for example, providing a thermal loading or mass small enough so as to avoid interference with measurement and/or characterization of a physiological parameter, such as the composition and amount of a biological fluid. In an embodiment, a functional substrate of the present devices and method is biocompatible and/or bioinert. In an embodiment, a functional substrate may facilitate mechanical, thermal, chemical and/or electrical matching of the functional substrate and the skin of a subject such that the mechanical, thermal, chemical and/or electrical properties of the functional substrate and the skin are within 20%, or 15%, or 10%, or 5% of one another.

[0069] In some embodiments, a functional substrate that is mechanically matched to a tissue, such as skin, provides a conformable interface, for example, useful for establishing conformal contact with the surface of the tissue. Devices and methods of certain embodiments incorporate mechanically functional substrates comprising soft materials, for example exhibiting flexibility and/or stretchability, such as polymeric and/or elastomeric materials. In an embodiment, a mechanically matched substrate has a modulus less than or equal to 100 MPa, and optionally for some embodiments less than or equal to 10 MPa, and optionally for some embodiments, less than or equal to 1 MPa. In an embodiment, a mechanically matched substrate has a thickness less than or equal to 0.5 mm, and optionally for some embodiments, less than or equal to 1 cm, and optionally for some embodiments, less than or equal to 3 mm. In an embodiment, a mechanically matched substrate has a bending stiffness less than or equal to 1 nN m, optionally less than or equal to 0.5 nN m.

[0070] In some embodiments, a mechanically matched functional substrate is characterized by one or more mechanical properties and/or physical properties that are within a specified factor of the same parameter for an

epidermal layer of the skin, such as a factor of 10 or a factor of 2. In an embodiment, for example, a functional substrate has a Young’s Modulus or thickness that is within a factor of 20, or optionally for some applications within a factor of 10, or optionally for some applications within a factor of 2, of a tissue, such as an epidermal layer of the skin, at the interface with a device of the present invention. In an embodiment, a mechanically matched functional substrate may have a mass or modulus that is equal to or lower than that of skin.

[0071] In some embodiments, a functional substrate that is thermally matched to skin has a thermal mass small enough that deployment of the device does not result in a thermal load on the tissue, such as skin, or small enough so as not to impact measurement and/or characterization of a physiological parameter, such as a characteristic of a biological fluid (e.g. composition, rate of release, etc.). In some embodiments, for example, a functional substrate that is thermally matched to skin has a thermal mass low enough such that deployment on skin results in an increase in temperature of less than or equal to 2 degrees Celsius, and optionally for some applications less than or equal to 1 degree Celsius, and optionally for some applications less than or equal to 0.5 degree Celsius, and optionally for some applications less than or equal to 0.1 degree Celsius. In some embodiments, for example, a functional substrate that is thermally matched to skin has a thermal mass low enough that it does not significantly disrupt water loss from the skin, such as avoiding a change in water loss by a factor of 1.2 or greater. Therefore, the device does not substantially induce sweating or significantly disrupt transdermal water loss from the skin.

[0072] In an embodiment, the functional substrate may be at least partially hydrophilic and/or at least partially hydrophobic.

[0073] In an embodiment, the functional substrate may have a modulus less than or equal to 100 MPa, or less than or equal to 50 MPa, or less than or equal to 10 MPa, or less than or equal to 100 kPa, or less than or equal to 80 kPa, or less than or equal to 50 kPa. Further, in some embodiments, the device may have a thickness less than or equal to 5 mm, or less than or equal to 2 mm, or less than or equal to 100 μ m, or less than or equal to 50 μ m, and a net bending stiffness less than or equal to 1 nN m, or less than or equal to 0.5 nN m, or less than or equal to 0.2 nN m. For example, the device may have a net bending stiffness selected from a range of 0.1 to 1 nN m, or 0.2 to 0.8 nN m, or 0.3 to 0.7 nN m, or 0.4 to 0.6 nN m.

[0074] A “component” is used broadly to refer to an individual part of a device.

[0075] “Sensing” refers to detecting the presence, absence, amount, magnitude or intensity of a physical and/or chemical property. Useful device components for sensing include, but are not limited to electrode elements, chemical or biological sensor elements, pH sensors, temperature sensors, strain sensors, mechanical sensors, position sensors, optical sensors and capacitive sensors.

[0076] “Actuating” refers to stimulating, controlling, or otherwise affecting a structure, material or device component. Useful device components for actuating include, but are not limited to, electrode elements, electromagnetic radiation emitting elements, light emitting diodes, lasers, mag-

netic elements, acoustic elements, piezoelectric elements, chemical elements, biological elements, and heating elements.

[0077] The terms “directly and indirectly” describe the actions or physical positions of one component relative to another component. For example, a component that “directly” acts upon or touches another component does so without intervention from an intermediary. Contrarily, a component that “indirectly” acts upon or touches another component does so through an intermediary (e.g., a third component).

[0078] “Encapsulate” refers to the orientation of one structure such that it is at least partially, and in some cases completely, surrounded by one or more other structures, such as a substrate, adhesive layer or encapsulating layer. “Partially encapsulated” refers to the orientation of one structure such that it is partially surrounded by one or more other structures, for example, wherein 30%, or optionally 50%, or optionally 90% of the external surface of the structure is surrounded by one or more structures. “Completely encapsulated” refers to the orientation of one structure such that it is completely surrounded by one or more other structures.

[0079] “Dielectric” refers to a non-conducting or insulating material.

[0080] “Polymer” refers to a macromolecule composed of repeating structural units connected by covalent chemical bonds or the polymerization product of one or more monomers, often characterized by a high molecular weight. The term polymer includes homopolymers, or polymers consisting essentially of a single repeating monomer subunit. The term polymer also includes copolymers, or polymers consisting essentially of two or more monomer subunits, such as random, block, alternating, segmented, grafted, tapered and other copolymers. Useful polymers include organic polymers or inorganic polymers that may be in amorphous, semi-amorphous, crystalline or partially crystalline states. Crosslinked polymers having linked monomer chains are particularly useful for some applications. Polymers useable in the methods, devices and components disclosed include, but are not limited to, plastics, elastomers, thermoplastic elastomers, elastoplastics, thermoplastics and acrylates. Exemplary polymers include, but are not limited to, acetal polymers, biodegradable polymers, cellulosic polymers, fluoropolymers, nylons, polyacrylonitrile polymers, polyamide-imide polymers, polyimides, polyarylates, polybenzimidazole, polybutylene, polycarbonate, polyesters, polyetherimide, polyethylene, polyethylene copolymers and modified polyethylenes, polyketones, poly(methyl methacrylate), polymethylpentene, polyphenylene oxides and polyphenylene sulfides, polyphthalamide, polypropylene, polyurethanes, styrenic resins, sulfone-based resins, vinyl-based resins, rubber (including natural rubber, styrene-butadiene, polybutadiene, neoprene, ethylene-propylene, butyl, nitrile, silicones), acrylic, nylon, polycarbonate, polyester, polyethylene, polypropylene, polystyrene, polyvinyl chloride, polyolefin or any combinations of these.

[0081] “Elastomer” refers to a polymeric material which can be stretched or deformed and returned to its original shape without substantial permanent deformation. Elastomers commonly undergo substantially elastic deformations. Useful elastomers include those comprising polymers, copolymers, composite materials or mixtures of polymers and copolymers. Elastomeric layer refers to a layer comprising

at least one elastomer. Elastomeric layers may also include dopants and other non-elastomeric materials. Useful elastomers include, but are not limited to, thermoplastic elastomers, styrenic materials, olefinic materials, polyolefin, polyurethane thermoplastic elastomers, polyamides, synthetic rubbers, PDMS, polybutadiene, polyisobutylene, poly(styrene-butadiene-styrene), polyurethanes, polychloroprene and silicones. Exemplary elastomers include, but are not limited to silicon containing polymers such as polysiloxanes including poly(dimethyl siloxane) (i.e. PDMS and h-PDMS), poly(methyl siloxane), partially alkylated poly(methyl siloxane), poly(alkyl methyl siloxane) and poly(phenyl methyl siloxane), silicon modified elastomers, thermoplastic elastomers, styrenic materials, olefinic materials, polyolefin, polyurethane thermoplastic elastomers, polyamides, synthetic rubbers, polyisobutylene, poly(styrene-butadiene-styrene), polyurethanes, polychloroprene and silicones. In an embodiment, a polymer is an elastomer.

[0082] “Conformable” refers to a device, material or substrate which has a bending stiffness that is sufficiently low to allow the device, material or substrate to adopt any desired contour profile, for example a contour profile allowing for conformal contact with a surface having a pattern of relief features. In certain embodiments, a desired contour profile is that of skin.

[0083] “Conformal contact” refers to contact established between a device and a receiving surface. In one aspect, conformal contact involves a macroscopic adaptation of one or more surfaces (e.g., contact surfaces) of a device to the overall shape of a surface. In another aspect, conformal contact involves a microscopic adaptation of one or more surfaces (e.g., contact surfaces) of a device to a surface resulting in an intimate contact substantially free of voids. In an embodiment, conformal contact involves adaptation of a contact surface(s) of the device to a receiving surface(s) such that intimate contact is achieved, for example, wherein less than 20% of the surface area of a contact surface of the device does not physically contact the receiving surface, or optionally less than 10% of a contact surface of the device does not physically contact the receiving surface, or optionally less than 5% of a contact surface of the device does not physically contact the receiving surface.

[0084] “Young’s modulus” is a mechanical property of a material, device or layer which refers to the ratio of stress to strain for a given substance. Young’s modulus may be provided by the expression:

$$E = \frac{(\text{stress})}{(\text{strain})} = \left(\frac{L_0}{\Delta L} \right) \left(\frac{F}{A} \right), \quad (\text{I})$$

where E is Young’s modulus, L_0 is the equilibrium length, ΔL is the length change under the applied stress, F is the force applied, and A is the area over which the force is applied. Young’s modulus may also be expressed in terms of Lamé constants via the equation:

$$E = \frac{\mu(3\lambda + 2\mu)}{\lambda + \mu}, \quad (\text{II})$$

where Δ and μ are Lamé constants. High Young’s modulus (or “high modulus”) and low Young’s modulus (or “low

modulus”) are relative descriptors of the magnitude of Young’s modulus in a given material, layer or device. In some embodiments, a high Young’s modulus is larger than a low Young’s modulus, preferably about 10 times larger for some applications, more preferably about 100 times larger for other applications, and even more preferably about 1000 times larger for yet other applications. In an embodiment, a low modulus layer has a Young’s modulus less than 100 MPa, optionally less than 10 MPa, and optionally a Young’s modulus selected from the range of 0.1 MPa to 50 MPa. In an embodiment, a high modulus layer has a Young’s modulus greater than 100 MPa, optionally greater than 10 GPa, and optionally a Young’s modulus selected from the range of 1 GPa to 100 GPa. In an embodiment, a device of the invention has one or more components having a low Young’s modulus. In an embodiment, a device of the invention has an overall low Young’s modulus.

[0085] “Low modulus” refers to materials having a Young’s modulus less than or equal to 10 MPa, less than or equal to 5 MPa or less than or equal to 1 MPa.

[0086] “Bending stiffness” is a mechanical property of a material, device or layer describing the resistance of the material, device or layer to an applied bending moment. Generally, bending stiffness is defined as the product of the modulus and area moment of inertia of the material, device or layer. A material having an inhomogeneous bending stiffness may optionally be described in terms of a “bulk” or “average” bending stiffness for the entire layer of material.

[0087] The invention can be further understood by the following non-limiting examples.

Example 1: Stretchable, Wireless Sensors and Functional Substrates for Epidermal Characterization of Sweat

[0088] This Example introduces materials and architectures for ultrathin, stretchable wireless sensors that mount on functional elastomeric substrates for epidermal analysis of biofluids. Measurement of the volume and chemical properties of sweat via dielectric detection and colorimetry demonstrates some capabilities. Here, inductively coupled sensors comprising LC resonators with capacitive electrodes show systematic responses to sweat collected in microporous substrates. Interrogation occurs through external coils placed in physical proximity to the devices. The substrates allow spontaneous sweat collection through capillary forces, without the need for complex microfluidic handling systems. Furthermore, colorimetric measurement modes are possible in the same system by introducing indicator compounds into the depths of the substrates, for sensing specific components (OH^- , H^+ , Cu^+ , and Fe^{2+}) in the sweat. The complete devices offer Young’s moduli that are similar to skin, thus allowing highly effective and reliable skin integration without external fixtures. Experimental results demonstrate volumetric measurement of sweat with an accuracy of $0.06 \mu\text{L}/\text{mm}^2$ with good stability and low drift. Colorimetric responses to pH and concentrations of various ions provide capabilities relevant to analysis of sweat. Similar materials and device designs can be used in monitoring other body fluids.

1. Introduction

[0089] Emerging wearable sensor technologies offer attractive solutions for continuous, personal health/wellness

assessment,^[1,2] forensic examination^[3] patient monitoring^[4,5] and motion recognition.^[6,7] Recent advances in epidermal electronics^[8] provide classes of skin-mounted sensors and associated electronics in physical formats that enable intimate, conformal contact with the skin. The soft, non-irritating nature of this contact yields an interface that simultaneously provides high precision, accurate measurement of biophysiological parameters, such as temperature,^[9] hydration,^[10] strain,^[11] and biopotential.^[12] Such epidermal sensors are ultrathin, breathable and stretchable, with mechanical and thermal properties that closely match to the skin itself, to enable effective skin integration with minimum constraints on natural processes. The results provide unique capabilities in long-term, reliable health monitoring.

[0090] An important measurement mode in such devices may involve the analysis of body fluids (blood, interstitial fluid, sweat, saliva, and tear), to gain insights into various aspects of physiological health.^[13-16] Such function in wearable sensors, generally, and epidermal electronics in particular, is relatively unexplored. Existing devices either use complex microfluidic systems for sample handling^[17-20] or involve purely concentration-based measurement without sample collection and storage, or access to parameters related to quantity and rate.^[21-23] In addition, mechanical fixtures, straps and/or tapes that are typically required to maintain contact of these devices with the skin do not lend themselves well to continuous, long term monitoring without discomfort.^[24] In the following, a set of materials and device architectures that provide advanced capabilities in this area is reported. The key concept involves the use of functional soft substrates to serve as a means for microfluidic collection, analysis and presentation to co-integrated electronic sensors and/or external camera systems. The pores of these substrates spontaneously fill with body fluids that emerge from the skin, where they induce colorimetric changes in the substrate and alter the radio frequency characteristics of integrated electrical antenna structures. The results offer valuable insights into the properties and volume of sweat, and their relationships to fluctuations in body temperature,^[25] fluid and electrolyte balance,^[26] and disease state.^[27] The devices also eliminate the need for direct skin-electrode contacts, thereby minimizing irritation that can be caused by contact between the skin and certain metals,^[28] while at the same time enabling repeated use of a single device with minimal noise induced by motion artifacts. The sensors exploit inductive coupling schemes, without on-chip detection circuits but with some potential for compatibility using near-field communication systems that are found increasingly in portable consumer electronic devices. The entire sensing system offers flexible and stretchable mechanics, with form factors that approach those of epidermal electronics.

2. Results and Discussion

[0091] FIG. 1a shows images and schematic illustrations of a typical device ($22 \times 28 \text{ mm}^2$ for the surface area of the substrate, and $10 \times 15 \text{ mm}^2$ for the dimension of the sensor) that includes an inductive coil and a planar capacitor formed with interdigitated electrodes. The coil consists of four turns of thin copper traces in a filamentary serpentine design that affords both flexibility and stretchability. The width of the trace is $140 \mu\text{m}$, and the lengths of the inner and outer turns are 4.8 and 9.5 mm, respectively. The electrodes consist of serpentine wires ($50 \mu\text{m}$ in width) that have lengths between

6.5 to 8.4 mm, to form 9 digits with a digit-to-digit spacing of 600 μm . The dielectric properties of the microporous supporting substrate strongly influence the capacitance of the structure.

[0092] In this way, the sweat sensor enables capacitive detection of the change of the dielectric properties of the substrate as its pores fill with biofluids (e.g. sweat). An external primary coil generates a time varying electromagnetic field that induces a current flow within the sensor. The impedance of the sensor is then determined by the amount of sweat within the substrate; this impedance influences that of the primary coil placed in proximity to the device. The resonance frequency (f_0) of the sensor can be determined from the frequency of a phase dip (or a peak in the phase difference, $\Delta\theta$, obtained from the subtraction of the phase of the primary coil with and without the sensor underneath) in the phase-frequency spectrum of the primary coil.^[29-32] At measurement frequencies examined here (100 to 200 MHz), free water molecules are under the influence of δ relaxation.^[33] The responses of the functional polymer substrates only involve contributions from induced charges. The movement of the water molecules and dynamics of the induced charges are sufficiently fast to respond to the external electromagnetic field. As a result, the combined dielectric properties of substrate and the sweat exhibit an invariant dielectric response over a wide range of frequencies (FIG. 5(a)). For present purposes, the frequency-dependence in the dielectric properties of the substrate can be ignored.

[0093] The sensor offers mechanical properties (elastic modulus ≈ 80 kPa) similar to those of the skin.^[34] The thickness of the substrate (1 mm), along with its lateral dimensions and porosity define the amount of fluid that it can capture. The devices exhibit robust, elastic behavior under axial stretching (FIGS. 1b and 1c) and other more complex modes of deformation (FIG. 1d). Attachment of the sensor onto the skin (FIG. 1e) using a thin layer of commercial spray-on bandage as adhesive leads to reversible skin/sensor bonding that can withstand significant extension and compression of the skin with sufficient mechanical strength to prevent delamination (FIGS. 1f and 1g).

[0094] In vitro experiments involve slow introduction of 0.6 mL of buffer solution (phosphate buffered saline, Sigma-Aldrich Corporation, St. Louis, Mo., USA) onto the substrates with a syringe pump, over the course of ≈ 40 minutes (FIG. 2d). The resonance frequency of the sensor (f_0), as measured by the shift of the phase peak of a primary coil placed in proximity to the device (FIG. 2c), decreases with increasing buffer solution content in the substrate. This response reflects increases in the permittivity due to replacement of air with buffer solution in the pores of the substrate, leading to an increase in the capacitance of the interdigitated electrodes associated with their proximity to the substrate. For a typical porous polyurethane (PUR) (PUR permittivity = 7,^[35] PUR substrate permittivity = 1.42 at 0.93 porosity in air) (FIG. 2a), f_0 shifts from 195.3 to 143.3 MHz in this experiment (FIG. 2d). Drying of the sensor in air at room temperature leads to the recovery of f_0 , eventually to the original value (195.3 MHz) over a period of ≈ 6 hours, indicating a reversible response with relative insensitivity to residual salt that might remain in the substrate.

[0095] Assessment of performance with human subjects involves use of sensors on cellulose paper (CP) and silicone substrates attached to the arms of two volunteers. Reference substrates made of the same materials with similar sizes

placed in close proximity to the sensors provide means for determining the accuracy and establishing a calibrated response (FIG. 2b). The monitoring includes measuring the value of f_0 of the sensors and the weight of the reference substrates every 5 min for a period of 2 hours. The results indicate that f_0 is inversely proportional to the weight of the reference sensor, such that the response can be calibrated with any two measured weights. The calibrated results closely follow weight changes of 0.4 (FIG. 2e) and 0.2 g (FIG. 2f) in the reference substrates, corresponding to 0.4 and 0.2 mL of sweat over the sensing areas.

[0096] Dimensional changes associated with deformation of the skin or swelling of the device caused by sweat absorption could, conceivably, lead to changes in f_0 . Strain induced effects can be examined by biaxially stretching a device and measuring f_0 at various states of deformation (FIG. 6(a)). The results show changes of only ≈ 0.9 MHz for biaxial strains of 27% (FIG. 2g) that are comparable to those caused by the absorption of water (FIG. 6(b)). The modest changes in f_0 under biaxial stretching may be attributed to the symmetric design of the sensor coil as well as mutual compensation of the changes in lengths and spacings of the interdigitated electrodes. The effects of temperature are also small. In particular, data indicate (FIG. 5(b)) that f_0 shifts from 199.25 MHz to 196.63 MHz when the temperature is changed from 25 to 45° C. Finally, although the salinity and ionic content of the sweat may lead to changes in both conductivity and permittivity, experiments with buffer solutions having various concentrations of sodium chloride (0 to 4.5 g/L) reveal only small variations in f_0 (≈ 0.6 MHz; FIG. 2h).

[0097] The sensors exhibit excellent repeatability and are suitable for repeated use. Multiple (i.e. five) measurements using sensors on CP and silicone substrates serve as demonstrations. Between each measurement, immersion in water followed by drying on a hot plate regenerates the devices. The changes in f_0 are repeatable for experiments that involve injection of 0.6 mL buffer solution (FIGS. 2i and 5(c)). The average change in f_0 is 58.3 MHz with a standard deviation of 1.1 MHz for the sensor on CP; the corresponding values for silicone are 60.1 MHz and 3.6 MHz, respectively. The changes in f_0 undergo different temporal patterns, as might be expected due to the differences in chemistry, microstructure and pore geometry for these two substrates. Measurements over 3 hours show no drifts in f_0 (FIG. 5(d)). The noise levels are < 0.7 MHz; this parameter, together with an average change of f_0 of 58.3 to 60.1 MHz for 0.6 mL buffer solution over a surface area of 22×28 mm², suggests a measurement accuracy of ≈ 0.06 mL/mm².

[0098] The coil structures can be mounted onto various types of functional substrates. Demonstrated examples include recycled cellulose sponge (RCS), polyurethane sponge (PUR), polyvinyl alcohol sponge (PVAS), cellulose paper (CP), and silicone sponge (FIG. 3a). Cutting with a hot-wire device (PUR, silicone) or with a razor blade (other) yields the appropriate lateral dimensions and thicknesses. Spin-coated silicone films with accurately controlled thickness (≈ 10 μm ; FIG. 3b) enable strong bonding between each of these functional substrates and the sensors through surface chemical functionalization, while preventing direct contact between the sensors and the sweat. Relative characteristics in water absorption are also important to consider, as described in the following.

[0099] The percentage gain in weight of the various porous materials after immersion in water defines their ability to hold fluids; the results are $\approx 2300\%$ (RCS), $\approx 1200\%$ (PUR), $\approx 750\%$ (PVAS), $\approx 350\%$ (CP), and $\approx 1500\%$ (silicone) (FIG. 3*c*). These data, together with measured volume changes yield the porosity levels: 0.97 (RCS), 0.93 (PUR), 0.90 (PVAS), 0.83 (CP) and 0.95 (silicone) (FIG. 3*d*). The water permeability can be determined from the capillary water absorption rate by combining Darcy's law^[36] and the Hagen-Poiseuille equation.^[37] Strips of the substrates (3 mm in width and 28 mm in length) are partially immersed into water with red dye (3 mm under the water). A camera enables measurements of changes in height of the absorbed water as a function of time (FIG. 3*e*). The CP material exhibits the fastest absorption rate (complete filling in ≈ 6 s), followed by the RCS (≈ 25 s). The PUR shows the smallest rate, with an increase in height of 8.3 mm over 130 s. These rates depend strongly on the pore size and degree of interconnectedness and on the contact angle. The latter can be determined optically (FIG. 7*b*); the former can be obtained by scanning electron microscopy (FIG. 7*a*) or by calculation and measurement of the height of absorbed water at a long period of time (details in supporting information). The permeability of the five substrates are 2.4 (RCS), 0.3 (PUR), 0.4 (PVAS), 8.7 (CP), and 8.6 (silicone) μm^2 (FIG. 3*f*).

[0100] In addition to dielectric response, absorption of water changes both the transparency, due to index matching effects, and the overall dimensions, due to swelling (FIGS. 4*a* and 4*c*). These effects can be used as additional measurement parameters to complement the electrical data described previously. The optical behavior can be illustrated by placing a sensor on a region of the skin with a temporary tattoo pattern. Continuous introduction of a buffer solution, up to a total of 0.6 mL, leads to increasing levels of transparency. Selected regions of the images in FIG. 4*a* can be used to obtain RGB (red, green, and blue) intensities at different locations. The resulting data (FIG. 4*b*) indicate that the water content is inversely proportional to the ratio of the RGB intensity on the sensor and the skin. The water also induces changes in the lateral dimensions. These changes can be measured by optically tracking the displacements of an array of opaque dots (Cr, by electron beam evaporation through a shadow mask) on the device (FIG. 4*c*). The results indicate a large displacement response to introduction of 0.2 mL of the buffer solution (≈ 2.3 mm dot displacement), but with diminishing response for an additional 0.4 mL (≈ 0.5 mm dot displacement). Nevertheless, these motions, which may be limited by mechanical constraints associated with mounting on the skin, might have some utility in measuring sweat loss.

[0101] The substrates can be rendered more highly functional, from an optical standpoint, by introduction of chemicals or immobilized biomolecules. Resulting interactions with the sweat can be evaluated through electrical dielectric measurement or simply colorimetric detection. For example, silicone substrates doped with colorimetric indicators render sensitivity to relevant biophysical/chemical parameters, such as pH values (FIG. 4*d*), free copper concentrations (FIG. 8*a*), and iron concentrations (FIG. 8*b*). To demonstrate pH detection, standard buffer solutions with pH values from 4 to 9 are introduced into a substrate that is dyed with a mixture of several different pH indicators (bromothymol blue, methyl red, methyl yellow, thymol blue, and

phenolphthalein). These chemicals reversibly react with free —OH groups and/or protons in the buffer solutions, leading to changes in absorption spectra. Accordingly, the substrate undergoes a series of color changes that reveal the pH values (FIG. 4*d*). In addition, buffer solutions with copper (FIG. 8*a*) and iron (FIG. 8*b*) at physiological concentrations (0.8 to 1 mg/L) can also be detected using similar colorimetric schemes. The intensities of individual colors (red, green, and blue) extracted from the images determine changes in analyte concentrations (FIGS. 4*e*, 4*f* and 4*g*). This type of strategy has potential utility when used in combination with the sorts of wireless schemes introduced here. For example, near field communication^[38] enabled devices such as cellphones also offer digital image capture capabilities, for simultaneous colorimetric measurement.

3. Conclusions

[0102] The results presented here provide materials and design strategies for integrating flexible and stretchable wireless sensors on functional substrates. Demonstrated devices intimately mounted on the skin enable non-invasive, wireless quantification of sweat loss as well as colorimetric detection of sweat composition. Similar strategies can be used to develop sensors for monitoring a range of key parameters associated not only with sweat but with other body fluids.

4. Experimental Section

[0103] To fabricate the device, a layer of polydimethylsiloxane (PDMS, 20 μm thick) is first spin-coated onto a glass slide (FIG. 9*a*). Curing the PDMS at 120° C. for 10 min and treating its surface with reactive ion etching (RIE) for 5 min (20 sccm O₂, 300 mTorr pressure, 150 W power) allows conformal spin-coating of a layer of polyimide (PI; 1 μm thick) on top. A bilayer of chrome (5 nm) and gold (200 nm) deposited by electron beam (ebeam) evaporation is photolithographically patterned to form serpentine interdigitated electrodes (FIG. 9*b*). An additional spin-coated PI (1 μm) layer electrically insulates the surfaces of the electrode patterns, while selective regions on the PI layer are etched by RIE for electrical contact between the electrode and serpentine coils formed by patterning a layer of ebeam deposited copper (6 μm) (FIG. 9*c*). The entire patterns are encapsulated by another spin-coated PI layer (1 μm). Patterned RIE yields an open mesh layout, capable of release onto the surface of a target substrate by use of water-soluble tape (Aquasol ASWT-2, Aquasol Corporation, North Tonawanda, N.Y., USA). To prepare the functional substrates, a layer of uncured silicone (10 μm thick) is spin-coated onto a water soluble tape fixed on its edges to a glass slide by Scotch tape. Pre-curing the silicone at 150° C. for 1 min transforms the liquid precursor into a tacky, soft solid (FIG. 9*e*). Placing the substrates on the silicone film with gentle pressure allows the partially cured film to crosslink with porous structures on the surface. The silicone and the substrates are then fully cured at 120° C. to achieve robust bonding (FIG. 9*f*). The resulting structure is removed from the glass, and rinsed with water to remove the water soluble tape. Deposition of Ti/SiO₂ (5/60 nm) onto the exposed backside of the sensor facilitates chemical bonding to the PDMS film on the functional substrates after UV ozone activation. Dissolving the water soluble tape yields an integrated device with excellent levels of mechanical

stretchability and flexibility (FIG. 9(g) and FIG. 1b). The functional substrates can be immersed into colorimetric indicators, followed by baking at 100° C. on a hotplate to dry the devices.

[0104] Five hydrophilic porous substrates serve as the sweat absorption materials, including Whatman GB003 cellulose paper (GE Healthcare Life Sciences, Pittsburgh, Pa., USA), Scotch-Brite recycled cellulose sponge (3M Cooperation, St. Paul, Minn., USA), polyvinyl alcohol sponge (Perfect & Glory Enterprise Co., Ltd., Taipei), Kendall hydrophilic polyurethane foam dressing (Covidien Inc., Mansfield, MA, USA), and Mepilex silicone foam dressing (Mölnlycke Health Care AB, Sweden). For colorimetric detection, a universal pH indicator (pH 2-10) (Ricca Chemical, Arlington, Tex., USA) yields responses to buffer solutions with well-defined pH (Sigma-Aldrich Corporation, St. Louis, Mo., USA). Colorimetric copper and iron ion detection is enabled by a copper color disc test kit (CU-6, Hach Company, Loveland, Colo., USA) and an iron color disc test kit (IR-8, Hach Company, Loveland, Colo., USA), while standard stock solutions of copper and iron (Hach Company, Loveland, Colo., USA) are diluted to achieve different ion concentrations.

[0105] The sensors can be integrated onto the skin. Briefly, spray bandage (Nexcare No Sting Liquid Bandage Spray, 3M Cooperation, St. Paul, Minn., USA) is first applied onto the corresponding skin region. Evaporation of the solvent results in a tacky, water-permeable film that does not significantly influence the transdermal water loss from the skin and provides sufficient adhesion to fix the sweat sensors onto the skin. The sensor is then applied to the skin with continuous pressure over several seconds. The bonding is reversible, but is sufficiently strong to accommodate heavy sweating and shear forces.

[0106] The electrical responses of the sensors are evaluated using a HP 4291A impedance analyzer (Agilent Technologies, Santa Clara, Calif., USA) with a frequency range from 1 MHz to 1.8 GHz. The analyzer connects to a one-turn hand-wound copper primary coil whose resonance frequency is significantly different from the sweat sensor. The coil is placed 2 mm away from the sweat sensor during the measurement. However, small variations in the distance between the coil and the sweat sensor are tolerable, with negligible effects on the results. A xyz mechanical stage and a rotational platform allow manual adjustment of the position and orientation of the primary coil relative to the sweat sensor. The primary coil provides a time varying electromagnetic field that induces alternating voltages in the sweat sensor. Changes of sweat content within the substrate of the sensor lead to changes in the capacitance of the sweat sensor and its f_0 . A syringe pump (KD Scientific Inc., Holliston, Mass., USA) is used to deliver buffer solutions to the sensors during the in vitro experiments. The sweat sensors with a CP substrate and a silicone porous material are mounted on the arms of two volunteers for 2 hour in vivo testing, with reference substrates of the same materials and sizes placed in close proximity to the sweat sensors (FIG. 2b). For the first hour, the volunteers exercise continuously to generate sweat, and then stop to rest for the second hour. During the measurement, the sweat sensors remain on the skin, while the reference sensors are peeled off every 5 min to record their weight using a precise balance and reattached back to the same positions afterwards.

[0107] The absorbance values are estimated from the digital images by accessing the RGB (red, green, blue) values of the selected regions on the experimental images using ImageJ^[39]. The average RGB values are determined from multiple pixels enclosed within a rectangular frame drawn by ImageJ with a plugin called, “measure RGB”. The Absorbance (A) defined as the negative log of the transmittance (I_n/I_{blank}), is then calculated using the following formula:

$$A = -\log(I_n/I_{blank}) \quad (1)$$

in which I_n denotes the R, G or B values for the functional substrates and I_{blank} the R, G, or B value for the background, both obtained from the experimental images.

REFERENCES

- [0108]** [1] M. Chan, EstC, J.-Y. Fourniols, C. Escriba, E. Campo, *Artif. Intell. Med.* 2012, 56, 137.
- [0109]** [2] A. Lay-Ekuakille, S. Mukhopadhyay, A. Lymberis, in *Wearable and Autonomous Biomedical Devices and Systems for Smart Environment*, Vol. 75, Springer, Berlin Heidelberg, 237.
- [0110]** [3] A. J. Bhandodkar, A. M. O'Mahony, J. Ramirez, I. A. Samek, S. M. Anderson, J. R. Windmiller, J. Wang, *Anal.* 2013, 138, 5288.
- [0111]** [4] P. Bonato, *IEEE Eng. Med. Biol. Mag.* 2010, 29, 25.
- [0112]** [5] P. M. Deshmukh, C. M. Russell, L. E. Lucarino, S. N. Robinovitch, *Enhancing clinical measures of postural stability with wear-able sensors*, presented at Engineering in Medicine and Biology Society (EMBC), 2012 Annual International Conference of the IEEE, Aug. 28 2012-Sep. 1 2012.
- [0113]** [6] J. Varkey, D. Pompili, T. Walls, *Pers. Ubiquit. Comput.* 2011, 16,897.
- [0114]** [7] J. R. Windmiller, J. Wang, *Electroanal.* 2013, 25, 29.
- [0115]** [8] D.-H. Kim, N. Lu, R. Ma, Y.-S. Kim, R.-H. Kim, S. Wang, J. Wu, S. M. Won, H. Tao, A. Islam, K. J. Yu, T.-i. Kim, R. Chowdhury, M. Ying, L. Xu, M. Li, H.-J. Chung, H. Keum, M. McCormick, P. Liu, Y.-W. Zhang, F. G. Omenetto, Y. Huang, T. Coleman, J. A. Rogers, *Science* 2011,333, 838.
- [0116]** [9] R. C. Webb, A. P. Bonifas, A. Behnaz, Y. Zhang, K. J. Yu, H. Cheng, M. Shi, Z. Bian, Z. Liu, Y. S. Kim, W. H. Yeo, J. S. Park, J. Song, Y. Li, Y. Huang, A. M. Gorbach, J. A. Rogers, *Nat. Mater.* 2013, 12, 938.
- [0117]** [10] X. Huang, H. Cheng, K. Chen, Y. Zhang, Y. Liu, C. Zhu, S. C. Ouyang, G. W. Kong, C. Yu, Y. Huang, J. A. Rogers, *IEEE Trans. Biomed. Eng.* 2013, 60, 2848.
- [0118]** [11] N. Lu, C. Lu, S. Yang, J. Rogers, *Adv. Funct. Mater.* 2012, 22, 4044.
- [0119]** [12] W.-H. Yeo, Y.-S. Kim, J. Lee, A. Ameen, L. Shi, M. Li, S. Wang, R. Ma, S. H. Jin, Z. Kang, Y. Huang, J. A. Rogers, *Adv. Mater.* 2013, 25, 2773.
- [0120]** [13] K. Virkler, I. K. Lednev, *Forens. Sci. Int.* 2009, 188, 1.
- [0121]** [14] T. L. Guidotti, J. McNamara, M. S. Moses, *Indian J. Med. Res.* 2008, 128, 524.
- [0122]** [15] V. Sikirzhyski, K. Virkler, I. K. Lednev, *Sensors* 2010, 10, 2869.
- [0123]** [16] S. Hu, J. A. Loo, D. T. Wong, *Proteomics* 2006, 6, 6326.

[0124] [17] P. Salvo, F. Di Francesco, D. Costanzo, C. Ferrari, M. G. Trivella, D. De-Rossi, IEEE Sens. J. 2010, 10, 1557.

[0125] [18] Y. Haixia, L. Dachao, R. C. Roberts, X. Kexin, N. C. Tien, J. Micro-electromech. Syst. 2012, 21, 917.

[0126] [19] A. Lay-Ekuakille, S. Mukhopadhyay, S. Coyle, F. Benito-Lopez, R. Byrne, D. Diamond, in Wearable and Autonomous Biomedical

[0127] Supporting Information 1. Methods for Determination of Weight Gain, Porosity, and Permeability

[0128] The percentage weight gain (W %) of the substrates can be obtained by measuring the weight of the materials in dry (W_{dry}) and water-saturated (W_{sat}) states. Thus, W % can be expressed as.

$$W \% = \frac{W_{sat} - W_{dry}}{W_{dry}} \times 100\% \quad (1)$$

[0129] The porosity (ϕ) of the materials is determined by the volume of pores (V_{pores}) to the total volume of the medium (V_{bulk}), is thus defined by

$$\phi = \frac{V_{pores}}{V_{bulk}} = \frac{(W_{sat} - W_{dry})\rho_{water}}{(W_{sat} - W_{dry})\rho_{water} + W_{dry}\rho_{bulk}} \quad (2)$$

[0130] where, ρ_{water} and ρ_{bulk} are the density of the water and the substrate materials, respectively.

[0131] To obtain the water permeability of the substrates, the Darcy law^[1], which describes the water flow in porous materials, can be used. It is found that the pressure gradient (∇P) that causes the water to flow in the porous materials can be described by

$$\nabla P = \frac{\mu}{K} q \quad (3)$$

where q is the volume average velocity (or flux), which represents discharge per unit area, with units of length per time. The factor K is the permeability of the material and μ the viscosity of the water. Determination of ∇P typically involves an experimental setup containing two chambers with well-controlled pressures. An alternative method uses the Hagen-Poiseuille equation^[2] to determine ∇P by considering the porous materials as bundles of capillaries. As a result, the pressure gradient can be further expressed as:

$$\nabla P = \frac{\nabla P}{L} = \frac{8\mu Q}{\pi R^4} \quad (4)$$

where ΔP is the pressure loss, L the length of the pipe, μ the dynamic viscosity, Q the volumetric flow rate (volume of fluid passing through the surface of the pipe per unit time), R the radius of the capillaries. Combing Eq. (3) and Eq. (4) yields

$$\frac{\mu}{K} q = \frac{8\mu Q}{\pi R^4} \quad (5)$$

[0132] Here, $Q/\pi R^2$ represents the interstitial velocity of the flow, while q represents the superficial velocity of the flow. As a result, the ratio between $Q/\pi R^2$ and q is equivalent to the porosity of the materials

$$\phi = \left(\frac{Q/\pi R^2}{q} \right).$$

Thus, Eq. (5) can be further simplified as

$$R^2 = \frac{8K}{\phi} \quad (6)$$

[0133] The linear momentum balance of the flow within a capillary tube can be expressed as

$$\frac{2\sigma \cos(\theta)}{R} = \rho gh + \frac{8\mu h t}{R^2} + \frac{d(h t')}{dt} \quad (7)$$

where terms from left to right refer to the capillary pressure, the hydrostatic pressure, the viscous pressure loss, and the inertia terms, respectively. In Eq. (7), σ is the surface tension of water, h is the height of water in the capillary tube at time t , and θ is the contact angle at the interface of the capillary tube and the water. As the porous materials may not have uniform R (especially for the porous materials with amorphous pores), such as RCS, PVAS, and CP in FIG. 7(a), it is possible to replace R in Eq. (7) with a more general term R_s , which represents the static radius of the porous materials and can be obtained from the equilibrium height (h_{eq}) in the static case (height of the absorbed water in the porous materials when t reaches ∞). The static radius R_s can be calculated from

$$h_{eq} = \frac{2\sigma \cos(\theta)}{R_s \rho g} \quad (8)$$

[0134] As a result, Eq. (7) can be further expressed as

$$\frac{2\sigma \cos(\theta)}{R_s} = \rho gh + \frac{8\mu h t}{R_s^2} + \rho \frac{d(h t')}{dt} \quad (9)$$

by considering a flow regime where the influence of inertia as well as the influence of gravity can be neglected^[3,4]. Thus, Eq. (8) can be simplified to

$$\frac{2\sigma \cos(\theta)}{R_s} = \frac{8\mu h t}{R_s^2} \quad \text{or} \quad (10)$$

-continued

$$\frac{hdh}{dt} = \frac{\sigma \cos(\theta)}{4\mu} \quad (11)$$

[0135] Solving this ordinary differential equation with the initial condition $h(0)=0$ leads to the Lucas-Washburn equation [4].

$$h^2 = \frac{\sigma R_s \cos(\theta)}{2\mu} t \quad (12)$$

[0136] According to Eq. (6), Eq. (12) can be further expressed as

$$h^2 = \frac{\sigma R_s \cos(\theta)}{2\mu} t \cong \frac{4\sigma \cos(\theta)}{\mu} \frac{K}{\phi R_s} t \quad (13)$$

[0137] As a result, the permittivity (K) can then be determined using the following equation

$$K = \frac{h^2 \mu \phi R_s}{4\sigma \cos(\theta) t} \quad (14)$$

[0138] where h , t , ϕ , and R_s of individual materials can all be experimentally determined, as summarized in Table 3.

TABLE 3

Parameters of the porous materials used for functional substrates							
Materials	W %	ρ_{bulk} (g/cm ³)	ϕ	h (m)	t (s)	R_s (m)	K (μm^2)
RCS	2296	1.5	0.97	0.025	25	2.52E-5	2.43
PUR	1184	1.2	0.94	0.008	130	1.52E-4	0.33
PVAS	746	1.2	0.90	0.013	130	6.34E-5	0.41
CP	332	1.5	0.83	0.025	6	2.50E-5	8.67
Silicone	1502	1.2	0.95	0.025	70	1.78E-4	8.57

[0139] 2. Experiments for Determination of Weight Gain, Porosity, and Permeability

[0140] R_s can be determined from the h_{eq} measurement, in which 50 cm strips of the porous materials are partially immersed into the water (approximately 1 cm strip in the water), while the heights of the water in the strips after one day immersion are measured. As PUR and silicone have more uniform pore sizes (FIG. 7(a)), their R_s can also be determined by measuring the radii of 10 pores in their SEM images and taking the average numbers. The contact angle θ can be measured through the analysis of images taken by a camera on the interface of water and the porous materials (FIG. 7(b)). The relation between h and t can be obtained using video captured throughout the process of water absorption.

REFERENCES

- [0141] [1] N. Fries, Capillary Transport Processes in Porous Materials: Experiment and Model, Cuvillier.
 [0142] [2] S. P. Sutera, R. Skalak, Annu. Rev. Fluid Mech. 1993, 25, 1.

- [0143] [3] E. W. Washburn, Phys. Rev. 1921, 17, 273.
 [0144] [4] A. Hamraoui, T. Nylander, J. Colloid Interf. Sci. 2002, 250, 415.

Example 2: Epidermal Microfluidic Sweat Patch

[0145] This Example discloses an epidermal microfluidic sweat patch incorporating at least one microfluidic channel and a plurality of colorimetric indicators disposed within cavities of the patch. The patch optionally includes a near-field communication coil.

[0146] Table 4 shows concentrations of parameters and chemical species relevant to sweat monitoring.

TABLE 4

Parameters and chemical species relevant to sweat monitoring.		
Constituents	Median Concentration	Range
Sweat gland density	100 pores/cm ²	50~300 pores/cm ²
Sweat rate	50 $\mu\text{L}/\text{hour} \cdot \text{cm}^2$	12-120 $\mu\text{L}/\text{hour} \cdot \text{cm}^2$
pH		4.0-6.8
Glucose	0.17 mM	5.6 μM -2.2 mM
Lactic acid	14 mM	3.7-50 mM
Chloride	23 mM	0.02-280 mM
Sodium ion	31 mM	0.11-390 mM

[0147] FIG. 10 shows an exploded view of a colorimetric sensor comprising a near-field communication coil. FIG. 11 is a photograph of the device of FIG. 10 adhered to the skin of a subject.

[0148] FIG. 12 illustrates a fabrication method for a sweat patch and an adhesion test on skin.

[0149] FIG. 13 illustrates an artificial sweat pore test using a syringe to feed artificial sweat at a rate of 12 $\mu\text{L}/\text{hr}$.

[0150] FIG. 14 shows a sweat patch incorporating colorimetric detection of various biomarkers for self-monitoring and early diagnosis. For example, FIG. 15 shows an absorbance spectrum illustrating the color change of a reactant that may be used to determine sweat volume and rate. FIG. 16 shows an absorbance spectrum and legend illustrating the color change of a reactant(s) that may be used to determine sweat pH, which may be correlated with sodium concentration, indicating to a user the proper time to hydrate. FIG. 17 shows an absorbance spectrum and legend illustrating the color change of a reactant(s) that may be used to determine glucose concentration in sweat, which may be correlated with blood glucose concentration. FIG. 18 shows an absorbance spectrum and legend illustrating the color change of a reactant(s) that may be used to determine lactate concentration in sweat, which may provide an indication of shock, hypoxia and/or exercise intolerance.

[0151] As shown in FIG. 19, a sweat sensor incorporating colorimetric biomarker indicators provides qualitative and quantitative data that may be observed by the naked eye and/or wirelessly observed by a detection device, such as a smartphone.

Example 3: Sweat Patches

[0152] Overview

[0153] Provided herein are epidermal microfluidic sweat patches for daily wear as personal healthcare monitoring systems that are highly conformable and stretchable. The patches allow for the non-invasive determination of sweat rate, sweat volume, and biomarker concentration, thereby

providing clinically reliable information. This technology relates to self-diagnostic systems for monitoring an individual's health state by tracking color changes of indicators within the devices by the naked eye or with a portable electronic device (e.g., a smartphone). By monitoring changes over time or trends, the disclosed devices may provide early indications of abnormal conditions.

[0154] The disclosed sweat sensor enables detection of sweat volume and rate, as well as concentration of biomarkers in sweat (e.g., pH, glucose, lactate, chloride, creatinine and ethanol) via various quantitative colorimetric assays. In an embodiment, the colorimetric indicators are incorporated into a polydimethylsiloxane (PDMS) substrate because PDMS is a silicon-based organic polymer approved for a wide range of medical applications, including contact lenses and medical devices.

[0155] Epidermal Microfluidics

[0156] Microfluidic analytical devices for sweat monitoring were developed based on a 2D channel system within poly(dimethylsiloxane) (PDMS) without pumps, valves, or fluid detectors. The chemical and physical characteristics of PDMS made it suitable for epidermal applications. For example, PDMS is optically transparent, elastomeric, non-toxic, chemically inert toward most reagents, and possesses a low surface energy.¹ The fabricated epidermal sweat patch was composed of four individual quantitative colorimetric detection reservoirs and an orbicular outer-circle serpentine fluidic channel (FIG. 21A). Each of the biomarker detection reservoirs holds 4 μL while the orbicular water detection channel contains 24 μL . The sample inlet located at the bottom of the device (0.5 cm^2) may cover about 50 sweat glands, thus introducing sweat into the device, filling the detection reservoirs, and allowing sweat to flow through the outer-circle channel for approximately 6 hours calculated based on an average sweat rate of 12 $\mu\text{L}/\text{hour}\cdot\text{cm}^2$ for humans. Due to the interfacial permeability of PDMS, which is impermeable to liquid water but permeable to gases, the water loss of the sweat patch was moderate (3% of the total volume during the sensor life-time). The device was 3 cm in diameter and 500 μm in thickness constructed with PDMS consisting of 30:1 (v/v) base:curing agent resulting in a modulus of 145 kPa. The mass of the device was \sim 970 mg.

[0157] The epidermal microfluidic sweat sensors were fabricated using soft lithography. The schematic illustration and fabrication processes are shown in FIG. 20. A master device was prepared from a silicon wafer by photolithography and dip-etching to generate a reverse image having 300 μm deep channels. To produce replicas, the mixture of 30:1 (v/v) base:curing agent of PDMS was poured over the master that was coated with a thin layer of poly(methyl methacrylate) (PMMA) and cured at 70° C. for 1 h. Once the PDMS was fully cured, the replica was released from the master. The prepared replica was then sealed with a PDMS film by oxygen plasma bonding for 1 min to activate surface silanol groups to form siloxane bonds. Finally, the fabricated microfluidic devices were attached to a commercial medical dressing (i.e., Tegederm®) via oxygen plasma bonding and applied on the skin surface. This epidermal microfluidic sweat-monitoring device was able to withstand significant tension, compression, and twist of the skin while maintaining sufficient adhesion (FIG. 20C).

[0158] Quantitative Colorimetric Detection of Biomarkers

[0159] The colorimetric determination holds great advantages for diagnosis in quantitative analysis. In this sweat

sensor, four colorimetric analyses were introduced for critical biomarkers being able to self-diagnosis and monitor a variety of medical conditions. Each detection reservoir represented a different analyte for determination of (1) water (for sweat volume and rate evaluation), (2) pH, (3) glucose, (4) lactate, and (5) chloride concentrations.

[0160] Thermal regulation and dehydration are highly related to sweat rate and volume and thus continuous monitoring is a vital tool for assessing health states of individuals and providing information relating to electrolyte balance and rehydration. The orbicular channel in the sweat sensor was coated with cobalt (II) chloride (i.e., CoCl_2) contained in a polyhydroxyethylmethacrylate hydrogel (pHEMA) matrix. As the sweat is introduced into the channel the blue colored anhydrous cobalt (II) chloride reacts with water turning into hexahydrate cobalt chloride (i.e., $\text{CoCl}_2\cdot 6\text{H}_2\text{O}$) presenting a pale purple color (FIG. 22A). By determining the distance of color change within the channel during a certain period of time, the sweat rate and volume could be assessed.

[0161] Not only physical sweat analysis, but chemical detection of biomarkers in sweat is essential. In some embodiments, quantitative colorimetric assays were demonstrated with paper-based reservoirs individually located in the middle of the sweat sensor. Filter paper was chosen as a matrix material among other materials (e.g., hydrogel, sol-gel, and agarose gel) since the hydrophilic cellulose fibers wicked biofluids at a fast absorption rate, as well as provided a solid support for assay reagent and allowed clear contrast regarding color changes.² A colorimetric sweat sensor was developed that consisted of four critical biomarker detection reservoirs: pH, glucose, lactate, and chloride.

[0162] The pH value of sweat has been known to exhibit a proportional relationship with sweat rate and sodium ion concentration. As an indicator of proper hydration time for a user, sweat pH was determined using a universal pH indicator consisting of various pH dyes (e.g., bromothymol blue, methyl red, and phenolphthalein), which covers a wide range of pH values. While the sweat was introduced in the reservoir, the pH indicator changed color based on the ratio of weak acid and its conjugate base form of the indicator based on the Henderson-Hasselbalch equation. The color change was observed according to various pH values of buffer solution in a medically reliable range (i.e., pH 4.0-7.0) as shown in FIG. 22B and its respective spectrum is presented in FIG. 22C.

[0163] Glucose concentration in the sweat is one of the most critical biomarkers for monitoring health state, especially playing a crucial role for improving diabetes treatment. In this device, the glucose was detected based on an enzymatic reaction that governed the selectivity of the measurement. Physically immobilized glucose oxidase produced hydrogen peroxide associated with oxidation of glucose and reduction of oxygen, next, iodide was oxidized to iodine by peroxidase, which was also contained in the paper-based reservoir.³ Therefore, a color change was observed from yellow to brown, the respective colors of iodide and iodine, to indicate the concentration of glucose.³ The color change illustrating the glucose concentration is presented in FIG. 22B as well as the respective spectrum in FIG. 22D. Thus, this device may warn of abnormal blood glucose concentrations for not only diabetes patients but also

prediabetes and healthy persons by correlating perspiration glucose concentration in a completely noninvasive manner on a daily basis.⁴

[0164] The sweat lactate concentration is an indicator of exercise intolerance, tissue hypoxia, pressure ischemia, and even pathological conditions (e.g., cancer, diabetes, and lactate acidosis).⁵ Lactate is produced by anaerobic energy metabolism from the eccrine gland, so lactate concentration in perspiration is a good criterion for determining individuals' abilities to endure rigorous exercise, especially for athletes and military personnel, and/or severe physical activity while on life support.⁶ Enzymatic reactions between lactate and co-factor NAD⁺ by lactate dehydrogenase and diaphorase allowed a color change of a chromogenic reagent (i.e., Formazan dyes) resulting in an orange color. As shown in FIGS. 22B and 22E, the color change within the detection reservoir was observed with regard to the concentration of lactate within the medically relevant range of 1.5-100 mM.

[0165] The representative sweat tests rely on determination of chloride ion concentration in perspiration. These tests may diagnose cystic fibrosis (CF) since excreted chloride content increases when there are defective chloride channels in sweat glands.⁷ Additionally, the level of chloride is considered to be an index of hydration. Accordingly, the level of chloride in sweat was determined using colorimetric detection by competitive binding between Hg²⁺ and Fe²⁺ with 2,4,6-tris(2-pyridyl)-s-triazine (TPTZ). In the presence of chloride ion, iron ion prefers to bind with TPTZ while Hg²⁺ participates as HgCl₂, which results in a color change from transparent to blue binding with respective metal ions. The quantitative colorimetric results are shown in FIGS. 22B and 22F.

[0166] Not only the biomarkers mentioned above, but copper ion, iron ion, and ethanol concentrations in sweat may also be detected by colorimetric assay. The trace copper ion in sweat was determined using a 1,2-bicinchoninate acid (BCA). The copper complex with BCA exhibited an intense purple color demonstrating a quantitative color change from 0 to 1 mg/mL.⁸ Similarly, iron ions were detected by a colored complex formed with 1,10-phenanthroline in the range of 0-0.8 mg/L.^{8b} Additionally, colorimetric detection of ethanol was demonstrated using an enzymatic reaction consisting of alcohol dehydrogenase, peroxidase, and formazan dye.

[0167] Collectively, these quantitative colorimetric analyses provide pre-diagnostic information of multiple biomarkers in sweat. By combining the colorimetric devices with telemedicine technology, this sweat patch could provide a user-friendly self-monitoring system for daily wear.

[0168] Telemedicine Technologies

[0169] In order to provide personalized clinical health care with a smartphone, near field communication (NFC) electronics were applied to the sweat patch. The NFC communication devices were fabricated with an ultrathin construction using ultralow modulus materials, which enable wireless communication under extreme deformations in daily usage.⁹ The NFC coils were incorporated on the sweat patch as shown in FIG. 23A. The biomedical information of sweat is quantitatively analyzed by taking images of the sweat sensor showing the color changes of the reservoirs (FIG. 23B). Using wireless NFC electronics to communicate to a smartphone permits the images to be examined based on an RGB digital color specification, converted into health informatics (e.g., concentration of biomarkers) and option-

ally transmitted from an individual's smartphone to medical staff or a medical records database.

REFERENCES

- [0170]** 1. McDonald, J. C.; Whitesides, G. M., Poly(dimethylsiloxane) as a Material for Fabricating Microfluidic Devices. *Accounts of Chemical Research* 2002, 35 (7), 491-499.
- [0171]** 2. Martinez, A. W.; Phillips, S. T.; Whitesides, G. M.; Carrilho, E., Diagnostics for the Developing World: Microfluidic Paper-Based Analytical Devices. *Analytical Chemistry* 2010, 82 (1), 3-10.
- [0172]** 3. (a) Martinez, A. W.; Phillips, S. T.; Butte, M. J.; Whitesides, G. M., Patterned Paper as a Platform for Inexpensive, Low-Volume, Portable Bioassays. *Angewandte Chemie International Edition* 2007, 46 (8), 1318-1320; (b) Martinez, A. W.; Phillips, S. T.; Carrilho, E.; Thomas, S. W.; Sindi, H.; Whitesides, G. M., Simple Telemedicine for Developing Regions: Camera Phones and Paper-Based Microfluidic Devices for Real-Time, Off-Site Diagnosis. *Analytical Chemistry* 2008, 80 (10), 3699-3707.
- [0173]** 4. Moyer, J.; Wilson, D.; Finkelshtein, I.; Wong, B.; Potts, R., Correlation Between Sweat Glucose and Blood Glucose in Subjects with Diabetes. *Diabetes Technology & Therapeutics* 2012, 14 (5), 398-402.
- [0174]** 5. (a) Polliack, A.; Taylor, R.; Bader, D., Sweat analysis following pressure ischaemia in a group of debilitated subjects. *J Rehabil Res Dev* 1997, 34 (3), 303-308; (b) Biagi, S.; Ghimenti, S.; Onor, M.; Bramanti, E., Simultaneous determination of lactate and pyruvate in human sweat using reversed-phase high-performance liquid chromatography: a noninvasive approach. *Biomedical Chromatography* 2012, 26 (11), 1408-1415.
- [0175]** 6. Jia, W.; Bandodkar, A. J.; Valdes-Ramirez, G.; Windmiller, J. R.; Yang, Z.; Ramirez, J.; Chan, G.; Wang, J., Electrochemical tattoo biosensors for real-time noninvasive lactate monitoring in human perspiration. *Anal Chem* 2013, 85 (14), 6553-60.
- [0176]** 7. Mishra, A.; Greaves, R.; Massie, J., The Relevance of Sweat Testing for the Diagnosis of Cystic Fibrosis in the Genomic Era. *The Clinical biochemist. Reviews/Australian Association of Clinical Biochemists*. 2005, 26 (4), 135-153.
- [0177]** 8. (a) Brenner, A. J.; Harris, E. D., A quantitative test for copper using bicinchoninic acid. *Anal Biochem* 1995, 226 (1), 80-4; (b) Huang, X.; Liu, Y. H.; Chen, K. L.; Shin, W. J.; Lu, C. J.; Kong, G. W.; Patnaik, D.; Lee, S. H.; Cortes, J. F.; Rogers, J. A., Stretchable, Wireless Sensors and Functional Substrates for Epidermal Characterization of Sweat. *Small* 2014, 10 (15), 3083-3090.
- [0178]** 9. Kim, J.; Banks, A.; Cheng, H. Y.; Xie, Z. Q.; Xu, S.; Jang, K. I.; Lee, J. W.; Liu, Z. J.; Gutruf, P.; Huang, X.; Wei, P. H.; Liu, F.; Li, K.; Dalal, M.; Ghaffari, R.; Feng, X.; Huang, Y. G.; Gupta, S.; Paik, U.; Rogers, J. A., Epidermal Electronics with Advanced Capabilities in Near-Field Communication. *Small* 2015, 11 (8), 906-912.

Example 4: Additional Sweat Patches

[0179] FIG. 24(A) shows a schematic illustration of an epidermal microfluidic sweat sensor providing information on sweat volume and rate as well as concentration of biomarkers in sweat incorporated with wireless communi-

cation electronics and an adhesive layer for adhering the sensor to the epidermis of a subject. FIG. 24(B) shows a schematic illustration of image process markers applied to an epidermal microfluidic sweat sensor. Image process markers are laminated on or disposed in a top layer of the sensor for white balance and color calibration, which enables the sensors to function under various light conditions. The image process markers also provide a reference for device orientation and a border-line for color change within a channel.

[0180] FIG. 25 provides graphical representations of water loss as a function of outlet channel (A) width and (B) length. Smaller channel widths generally lead to a lower rate of water vapor loss than larger channel widths, but channel length does not significantly affect the rate of water vapor loss. FIG. 26 provides a graphical representation of back pressure inside a channel showing that shorter outlet channels and larger channel widths produce lower back pressures. At a channel width of 100 μm , back pressure became negligible for all channel lengths studied. The following equation was used to calculate the theoretical pressure in the channel:

$$\nabla P \approx \frac{8L(w=h)^2}{w^3h^3} \frac{\mu M}{\rho} \frac{\dot{V}_{inlet} P_0}{RT} \quad (15)$$

where $h=300 \mu\text{m}$, $M=29\text{E-}3 \text{ Kg/mol}$, $\rho=1.2 \text{ Kg/m}^3$, $\mu=1.8\text{E-}5 \text{ Pa}\cdot\text{s}$, $P_0=1\text{E}5 \text{ Pa}$, $\dot{V}_{inlet}=15 \mu\text{L/hour}$, $R=8.314 \text{ J/(mol}\cdot\text{K)}$, $T=300 \text{ K}$.

[0181] FIG. 27 shows a schematic illustration of a cross section of a microfluidic channel deformed due to pressure (A) and a top perspective view of a section of an epidermal microfluidic sweat sensor showing a width of the microfluidic channel (B), as well as a graphical representation of deformation shown as volume change due to pressure. The volume change was calculated using:

$$\frac{\Delta V}{V} = \frac{\nabla P a^4}{5E^2 h} \quad (16)$$

where $2a=1 \text{ mm}$, $t=100 \mu\text{m}$, $E=145 \text{ KPa}$ and $\nu=0.5$. At an outlet width greater than 10 μm , a pressure-induced volume change can be avoided.

[0182] To harvest biofluids using pump-less microfluidics, sufficient adhesion force is required to drive fluid into the microfluidics system. The disclosed microfluidic devices demonstrate great adhesion on the epidermis facilitated by medical-grade adhesives (e.g., Tagaderm®). FIG. 28 shows an experimental set-up for 90° peel adhesion property testing (standard ISO 29862:2007) using a force gauge (Mark-10, Copiague, N.Y.) (A). A holding device is adhered on the skin with a force gauge (B) and devices are peeled at an angle of 90° (C.). The force measurement while displacing the device at a rate of 300 mm/min is shown graphically in (D) and the area where peeling occurs is indicated by the gray region. The average peeling force was determined to be 5.7 N. Thus, the disclosed microfluidic sweat sensors may be bonded to the epidermis of a subject with an adhesion force in the range from 1 N to 10 N, or 2 N to 8 N, or 3 N to 6 N.

[0183] FIG. 29 illustrates one example of colorimetric determination of creatinine. A UV-VIS spectrum illustrating various creatinine concentrations (i.e., 15-1000 μM) is shown in (A) and a constructed calibration curve based on this spectrum is shown in (B). The presented color for each spectrum corresponds to exhibited color on paper-based colorimetric detection reservoirs as a function of creatinine concentration, which is presented in optical image (C). This colorimetric analysis is based on an enzymatic reaction using a mixture of creatinine amidohydrolase, creatine amidohydrolase and sarcosine oxidase. Reaction of creatinine with this enzyme mixture generates hydrogen peroxide proportional to the concentration of creatinine in biological fluids. The hydrogen peroxide concentration is determined colorimetrically by the chromogen 2,5-dichloro-2-hydroxy-benzenesulfonic acid and 4-amino-phenazone in a reaction catalyzed by horseradish peroxidase.

[0184] FIG. 30 illustrates one example of colorimetric determination of ethanol. Ethanol is detected via reaction with alcohol dehydrogenase in the presence of formazan dye. A UV-VIS spectrum illustrating various ethanol concentrations (i.e., 0.04-7.89% (w/v)) is shown in (A) and a constructed calibration curve based on this spectrum is shown in (B). The presented color for each spectrum corresponds to exhibited color on paper-based colorimetric detection reservoirs as a function of ethanol concentration, which is presented in optical image (C).

[0185] FIG. 31 shows various microfluidic sweat sensor designs including four individual quantitative colorimetric detection reservoirs and an orbicular outer-circle fluidic channel. In some embodiments, a single microfluidic channel is in fluidic communication with all of the colorimetric detection reservoirs and an orbicular fluidic channel. In another embodiment, one microfluidic channel transports fluids from the epidermis of a subject to the colorimetric detection reservoirs and a second microfluidic channel transports fluids from the epidermis of the subject to the orbicular fluidic channel (C). In another embodiment, each colorimetric detection reservoir and the orbicular microfluidic channel may be independently connected to a microfluidic channel that transports fluid from the epidermis of a subject. Optionally, each of the colorimetric detection reservoirs may comprise an outlet to a channel that allows vapor to escape to the surrounding environment. As shown in (D), the outlet channel may be tapered to increase in volume nearer the outlet to the surrounding environment, thereby accommodating larger quantities of vapor without increasing back pressure within the outlet channel. In any of the embodiments disclosed, the orbicular fluidic channel may be circular or serpentine and the orbicular fluidic channel may have a sealed distal end, optionally including a reservoir, or an outlet to the surrounding environment. As shown in FIG. 32, a serpentine orbicular fluidic channel provides a greater area and channel volume than a circular orbicular fluidic channel while controlling for channel width and height to avoid collapse of the channel. For example, a serpentine channel may provide an increased area of up to 58% compared to a circular channel having an identical channel width. An increased area of the orbicular channel increases the amount of time a microfluidic sweat sensor can be used for monitoring a subject without being replaced or dried.

STATEMENTS REGARDING INCORPORATION
BY REFERENCE AND VARIATIONS

[0186] All references throughout this application, for example patent documents including issued or granted patents or equivalents; patent application publications; and non-patent literature documents or other source material are hereby incorporated by reference herein in their entireties, as though individually incorporated by reference, to the extent each reference is at least partially not inconsistent with the disclosure in this application (for example, a reference that is partially inconsistent is incorporated by reference except for the partially inconsistent portion of the reference).

[0187] The terms and expressions which have been employed herein are used as terms of description and not of limitation, and there is no intention in the use of such terms and expressions of excluding any equivalents of the features shown and described or portions thereof, but it is recognized that various modifications are possible within the scope of the invention claimed. Thus, it should be understood that although the present invention has been specifically disclosed by preferred embodiments, exemplary embodiments and optional features, modification and variation of the concepts herein disclosed may be resorted to by those skilled in the art, and that such modifications and variations are considered to be within the scope of this invention as defined by the appended claims. The specific embodiments provided herein are examples of useful embodiments of the present invention and it will be apparent to one skilled in the art that the present invention may be carried out using a large number of variations of the devices, device components, methods and steps set forth in the present description. As will be obvious to one of skill in the art, methods and devices

useful for the present embodiments can include a large number of optional composition and processing elements and steps.

[0188] When a group of substituents is disclosed herein, it is understood that all individual members of that group and all subgroups, including any isomers, enantiomers, and diastereomers of the group members, are disclosed separately. When a Markush group or other grouping is used herein, all individual members of the group and all combinations and subcombinations possible of the group are intended to be individually included in the disclosure. When a compound is described herein such that a particular isomer, enantiomer or diastereomer of the compound is not specified, for example, in a formula or in a chemical name, that description is intended to include each isomer and enantiomer of the compound described individually or in any combination. Additionally, unless otherwise specified, all isotopic variants of compounds disclosed herein are intended to be encompassed by the disclosure. For example, it will be understood that any one or more hydrogens in a molecule disclosed can be replaced with deuterium or tritium. Isotopic variants of a molecule are generally useful as standards in assays for the molecule and in chemical and biological research related to the molecule or its use. Methods for making such isotopic variants are known in the art. Specific names of compounds are intended to be exemplary, as it is known that one of ordinary skill in the art can name the same compounds differently.

[0189] The following references relate generally to fabrication methods, structures and systems for making electronic devices, and are hereby incorporated by reference to the extent not inconsistent with the disclosure in this application.

Attorney Docket No.	Application No.	Filing Date	Publication No.	Publication Date	Patent No.	Issue Date
145-03 US	11/001,689	Dec. 1, 2004	2006/0286488	Dec. 21, 2006	7,704,684	Apr. 27, 2010
18-04 US	11/115,954	Apr. 27, 2005	2005/0238967	Oct. 27, 2005	7,195,733	Nov. 27, 2007
38-04A US	11/145,574	Jun. 2, 2005	2009/0294803	Dec. 3, 2009	7,622,367	Nov. 24, 2009
38-04B US	11/145,542	Jun. 2, 2005	2006/0038182	Feb. 23, 2006	7,557,367	Jul. 7, 2009
43-06 US	11/421,654	Jun. 1, 2006	2007/0032089	Feb. 8, 2007	7,799,699	Sep. 21, 2010
38-04C US	11/423,287	Jun. 9, 2006	2006/0286785	Dec. 21, 2006	7,521,292	Apr. 21, 2009
41-06 US	11/423,192	Jun. 9, 2006	2009/0199960	Aug. 13, 2009	7,943,491	May 17, 2011
25-06 US	11/465,317	Aug. 17, 2006	—	—	—	—
137-05 US	11/675,659	Feb. 16, 2007	2008/0055581	Mar. 6, 2008	—	—
90-06 US	11/782,799	Jul. 25, 2007	2008/0212102	Sep. 4, 2008	7,705,280	Apr. 27, 2010
134-06 US	11/851,182	Sep. 6, 2007	2008/0157235	Jul. 3, 2008	8,217,381	Jul. 10, 2012
151-06 US	11/585,788	Sep. 20, 2007	2008/0108171	May 8, 2008	7,932,123	Apr. 26, 2011
216-06 US	11/981,380	Oct. 31, 2007	2010/0283069	Nov. 11, 2010	7,972,875	Jul. 5, 2011
116-07 US	12/372,605	Feb. 17, 2009	—	—	—	—
213-07 US	12/398,811	Mar. 5, 2009	2010/0002402	Jan. 7, 2010	8,552,299	Oct. 8, 2013
38-040 US	12/405,475	Mar. 17, 2009	2010/0059863	Mar. 11, 2010	8,198,621	Jun. 12, 2012
170-07 US	12/418,071	Apr. 3, 2009	2010/0052112	Mar. 4, 2010	8,470,701	Jun. 25, 2013
216-06A US	12/522,582	Jul. 9, 2009	—	—	—	—
38-04A1 US	12/564,566	Sep. 22, 2009	2010/0072577	Mar. 25, 2010	7,982,296	Jul. 19, 2011
71-07 US	12/669,287	Jan. 15, 2010	2011/0187798	Aug. 4, 2011	—	—
60-09 US	12/778,588	May 12, 2010	2010/0317132	Dec. 16, 2010	—	—
43-06A US	12/844,492	Jul. 27, 2010	2010/0289124	Nov. 18, 2010	8,039,847	Oct. 18, 2011
15-10 US	12/892,001	Sep. 28, 2010	2011/0230747	Sep. 22, 2011	8,666,471	Mar. 4, 2014
19-10 US	12/916,934	Nov. 1, 2010	2012/0105528	May 3, 2012	8,562,095	Oct. 22, 2013
3-10 US	12/947,120	Nov. 16, 2010	2011/0170225	Jul. 14, 2011	—	—
118-08 US	12/996,924	Dec. 8, 2010	2011/0147715	Jun. 23, 2011	8,946,683	Feb. 3, 2015
126-09 US	12/968,637	Dec. 15, 2010	2012/0157804	Jun. 21, 2012	—	—
50-10 US	13/046,191	Mar. 11, 2011	2012/0165759	Jun. 28, 2012	—	—
151-06A US	13/071,027	Mar. 24, 2011	2011/0171813	Jul. 14, 2011	—	—
137-05A US	13/095,502	Apr. 27, 2011	—	—	—	—
216-06B US	13/100,774	May 4, 2011	2011/0266561	Nov. 3, 2011	8,722,458	May 13, 2014
38-04A2 US	13/113,504	May 23, 2011	2011/0220890	Sep. 15, 2011	8,440,546	May 14, 2013
136-08 US	13/120,486	Aug. 4, 2011	2011/0277813	Nov. 17, 2011	8,679,888	Mar. 25, 2014

-continued

Attorney Docket No.	Application No.	Filing Date	Publication No.	Publication Date	Patent No.	Issue Date
151-06B US	13/228,041	Sep. 8, 2011	2011/0316120	Dec. 29, 2011	—	—
43-06B US	13/270,954	Oct. 11, 2011	2012/0083099	Apr. 5, 2012	8,394,706	Mar. 12, 2013
3-11 US	13/349,336	Jan. 12, 2012	2012/0261551	Oct. 18, 2012	—	—
38-04E US	13/441,618	Apr. 6, 2012	2013/0100618	Apr. 25, 2013	8,754,396	Jun. 17, 2014
134-06B US	13/441,598	Apr. 6, 2012	2012/0327608	Dec. 27, 2012	8,729,524	May 20, 2014
28-11 US	13/472,165	May 15, 2012	2012/0320581	Dec. 20, 2012	—	—
7-11 US	13/486,726	Jun. 1, 2012	2013/0072775	Mar. 21, 2013	8,934,965	Jan. 13, 2015
29-11 US	13/492,636	Jun. 8, 2012	2013/0041235	Feb. 14, 2013	—	—
84-11 US	13/549,291	Jul. 13, 2012	2013/0036928	Feb. 14, 2013	—	—
25-06A US	13/596,343	Aug. 28, 2012	2012/0321785	Dec. 20, 2012	8,367,035	Feb. 5, 2013
150-11 US	13/624,096	Sep. 21, 2012	2013/0140649	Jun. 6, 2013	—	—
38-04A3 US	13/801,868	Mar. 13, 2013	2013/0320503	Dec. 5, 2013	8,664,699	Mar. 4, 2014
125-12 US	13/835,284	Mar. 15, 2013	2014/0220422	Aug. 7, 2014	—	—
30-13 US	13/853,770	Mar. 29, 2013	2013/0333094	Dec. 19, 2013	—	—
213-07A US	13/974,963	Aug. 23, 2013	2014/0140020	May 22, 2014	8,905,772	Dec. 9, 2014
19-10A US	14/033,765	Sep. 23, 2013	2014/0092158	Apr. 3, 2014	—	—
15-10A US	14/140,299	Dec. 24, 2013	2014/0163390	Jun. 12, 2014	—	—
38-04A4 US	14/155,010	Jan. 14, 2014	2014/0191236	Jul. 10, 2014	—	—
136-08A US	14/173,525	Feb. 5, 2014	2014/0216524	Aug. 7, 2014	—	—
216-06C US	14/209,481	Mar. 13, 2014	2014/0373898	Dec. 25, 2014	—	—
134-06C US	14/220,910	Mar. 20, 2014	2014/0374872	Dec. 25, 2014	—	—
38-04F US	14/220,923	Mar. 20, 2014	2015/0001462	Jan. 1, 2015	—	—
151-06C US	14/246,962	Apr. 7, 2014	2014/0361409	Dec. 11, 2014	—	—
62-13 US	14/250,671	Apr. 11, 2014	2014/0305900	Oct. 16, 2014	—	—
56-13 US	14/251,259	Apr. 11, 2014	2014/0323968	Oct. 30, 2014	—	—
60-09A US	12/778,588	Sep. 5, 2014	2015/0132873	May 14, 2015	—	—
84-13 US	14/504,736	Oct. 2, 2014	2015/0141767	May 21, 2015	—	—
213-07B US	14/521,319	Oct. 22, 2014	—	—	—	—
7-11A US	14/532,687	Nov. 4, 2014	2015/0080695	Mar. 19, 2015	—	—
2-14 US	14/599,290	Jan. 16, 2015	—	—	—	—
71-07A US	12/669,287	Apr. 14, 2015	—	—	—	—
213-07C US	12/398,811	May 7, 2015	—	—	—	—
15-13 WO	PCT/US2014/015825	Feb. 19, 2014	WO2014/126927	Aug. 21, 2014	—	—
128-13 WO	PCT/US2014/014932	Feb. 5, 2014	WO 2014/124044	Aug. 14, 2014	—	—
8-14 WO	PCT/US2014/014944	Feb. 18, 2014	WO 2014/124049	Aug. 14, 2014	—	—
35-13 WO	PCT/US2014/021371	Mar. 6, 2014	WO 2014/138465	Sep. 12, 2014	—	—
54-13 WO	PCT/US2014/032848	Apr. 3, 2014	WO 2014/165686	Oct. 9, 2014	—	—

[0190] Every formulation or combination of components described or exemplified herein can be used to practice the invention, unless otherwise stated.

[0191] Whenever a range is given in the specification, for example, a number range, a temperature range, a time range, or a composition or concentration range, all intermediate ranges and subranges, as well as all individual values included in the ranges given are intended to be included in the disclosure. It will be understood that any subranges or individual values in a range or subrange that are included in the description herein can be excluded from the claims herein.

[0192] All patents and publications mentioned in the specification are indicative of the levels of skill of those skilled in the art to which the invention pertains. References cited herein are incorporated by reference herein in their entirety to indicate the state of the art as of their publication or filing date and it is intended that this information can be employed herein, if needed, to exclude specific embodiments that are in the prior art. For example, when compositions of matter are claimed, it should be understood that compounds known and available in the art prior to Applicant's invention, including compounds for which an enabling disclosure is provided in the references cited herein, are not intended to be included in the composition of matter claims herein.

[0193] As used herein, "comprising" is synonymous with "including," "containing," or "characterized by," and is

inclusive or open-ended and does not exclude additional, unrecited elements or method steps. As used herein, "consisting of" excludes any element, step, or ingredient not specified in the claim element. As used herein, "consisting essentially of" does not exclude materials or steps that do not materially affect the basic and novel characteristics of the claim. In each instance herein any of the terms "comprising", "consisting essentially of" and "consisting of" may be replaced with either of the other two terms. The invention illustratively described herein suitably may be practiced in the absence of any element or elements and/or limitation or limitations, which are not specifically disclosed herein.

[0194] One of ordinary skill in the art will appreciate that starting materials, biological materials, reagents, synthetic methods, purification methods, analytical methods, assay methods, and biological methods other than those specifically exemplified can be employed in the practice of the invention without resort to undue experimentation. All art-known functional equivalents, of any such materials and methods are intended to be included in this invention. The terms and expressions which have been employed are used as terms of description and not of limitation, and there is no intention in the use of such terms and expressions of excluding any equivalents of the features shown and described or portions thereof, but it is recognized that various modifications are possible within the scope of the invention claimed. Thus, it should be understood that although the present invention has been specifically dis-

closed by preferred embodiments and optional features, modification and variation of the concepts herein disclosed may be resorted to by those skilled in the art, and that such modifications and variations are considered to be within the scope of this invention as defined by the appended claims.

[0195] It must be noted that as used herein and in the appended claims, the singular forms “a”, “an”, and “the” include plural reference unless the context clearly dictates otherwise. Thus, for example, reference to “a cell” includes a plurality of such cells and equivalents thereof known to those skilled in the art, and so forth. As well, the terms “a” (or “an”), “one or more” and “at least one” can be used interchangeably herein. It is also to be noted that the terms “comprising”, “including”, and “having” can be used interchangeably. The expression “of any of claims XX-YY” (wherein XX and YY refer to claim numbers) is intended to provide a multiple dependent claim in the alternative form, and in some embodiments is interchangeable with the expression “as in any one of claims XX-YY.”

[0196] Unless defined otherwise, all technical and scientific terms used herein have the same meanings as commonly understood by one of ordinary skill in the art to which this invention belongs. Although any methods and materials similar or equivalent to those described herein can be used in the practice or testing of the present invention, the preferred methods and materials are described.

We claim:

1. A device for monitoring a biofluid comprising: a functional substrate that is mechanically matched to skin; wherein said functional substrate provides for microfluidic transport of said biofluid; and at least one sensor supported by said functional substrate.
2. A device for monitoring a biofluid comprising: a functional substrate that is thermally matched to skin; wherein said functional substrate provides for microfluidic transport of said biofluid; and at least one sensor supported by said functional substrate.
3. A device for monitoring a biofluid comprising: a functional substrate providing for microfluidic transport of said biofluid through one or more microfluidic channels each having a substantially uniform lateral dimension; and at least one sensor supported by said functional substrate.
4. The device of any one of claims 1-3, wherein said functional substrate is an elastomeric substrate.
5. The device of any one of claims 1-3 further comprising a component for extracting interstitial fluid or blood from a subject.
6. The device of claim 5, wherein the component for extracting interstitial fluid or blood is selected from a microneedle component, a reverse iontophoresis component and a thermal microabrasion component.
7. The device of any one of claims 1-3, wherein said functional substrate is substantially colorless and substantially transparent.
8. The device of any one of claims 1-3, wherein said functional substrate has a modulus less than or equal to 100 MPa.
9. The device of any one of claims 1-3, wherein said functional substrate has a modulus selected from a range of 10 kPa to 10 MPa.
10. The device of any one of claims 1-3, wherein said functional substrate has a thickness selected from a range of 500 μm to 2 mm.

11. The device of any one of claims 1-3, wherein said functional substrate is selected from the group consisting of polydimethylsiloxane (PDMS), polyurethane, cellulose paper, cellulose sponge, polyurethane sponge, polyvinyl alcohol sponge, silicone sponge, polystyrene, polyimide, SU-8, wax, olefin copolymer, polymethyl methacrylate (PMMA) and polycarbonate.

12. The device of any one of claims 1-3, wherein said functional substrate has a dielectric constant greater than or equal to 2.0.

13. The device of any one of claims 1-3, wherein said functional substrate has a dielectric constant selected from a range of 2.20 to 2.75.

14. The device of any one of claims 1-3, wherein said functional substrate has lateral dimensions or a diameter less than or equal to 700 mm^2 .

15. The device of any one of claims 1-3, wherein said functional substrate has a permeability for said biofluid greater than or equal to 0.2 g/h m^2 .

16. The device of any one of claims 1-3, wherein said functional substrate has a coefficient of thermal expansion selected from a range of 1 $^\circ$ C. ($\times 10^{-6}$) to 3 $^\circ$ C. ($\times 10^4$).

17. The device of any one of claims 1-3, wherein said functional substrate has a porosity greater than or equal to 0.5.

18. The device of any one of claims 1-3, wherein said microfluidic transport is spontaneous microfluidic transport via capillary force.

19. The device of any one of claims 1-2 further comprising at least one microfluidic channel having a substantially uniform lateral dimension.

20. The device of any one of claims 3 and 19, wherein said microfluidic channel has a length selected from a range of 1 mm to 7 cm.

21. The device of any one of claims 3 and 19, wherein said microfluidic channel has a width selected from a range of 100 μm to 1 mm.

22. The device of any one of claims 1-3, wherein said biofluid is selected from the group consisting of sweat, tears, saliva, gingival crevicular fluid, interstitial fluid, blood and combinations thereof.

23. The device of any one of claims 1-3, wherein said sensor is a non-pH colorimetric indicator.

24. The device of any one of claims 1-3, wherein said sensor comprises an electrical sensor, a chemical sensor, a biological sensor, a temperature sensor, an impedance sensor, an optical sensor, a mechanical sensor or a magnetic sensor.

25. The device of any one of claims 1-3, wherein said sensor is an LC resonator.

26. The device of any one of claims 1-3 further comprising an actuator.

27. The device of claim 26, wherein said actuator generates electromagnetic radiation, acoustic energy, an electric field, a magnetic field, heat, a RF signal, a voltage, a chemical change or a biological change.

28. The device of claim 26, wherein said actuator comprises a heater, a reservoir containing a chemical agent capable of causing a chemical change or a biological change, a source of electromagnetic radiation, a source of an electric field, a source of RF energy or a source of acoustic energy.

29. The device of any one of claims 1-3 further comprising a transmitter, receiver or transceiver.

30. The device of any one of claims 1-3 further comprising at least one coil.

31. The device of claim 30, wherein said at least one coil is a near-field communication coil.

32. The device of claim 30, wherein said at least one coil is an inductive coil.

33. The device of claim 30, wherein said at least one coil comprises a serpentine trace.

34. The device of any one of claims 1-3, wherein said sensor is a colorimetric indicator.

35. The device of claim 34, wherein said colorimetric indicator is disposed within a cavity of said functional substrate.

36. The device of claim 35, wherein said cavity is connected to an opening at a surface of said functional substrate by a microfluidic channel.

37. The device of claim 34, wherein said colorimetric indicator changes color in response to an analyte in said biofluid.

38. The device of claim 34, wherein said colorimetric indicator is embedded in a matrix material selected from the group consisting of filter paper, polyhydroxyethylmethacrylate hydrogel (pHEMA), agarose gel, sol-gel and combinations thereof.

39. The device of claim 34, wherein said colorimetric indicator comprises a cobalt dichloride salt.

40. The device of claim 34, wherein said colorimetric indicator comprises a chemical selected from the group consisting of glucose oxidase, peroxidase, potassium iodide and combinations thereof.

41. The device of claim 34, wherein said colorimetric indicator comprises a chemical selected from lactate dehydrogenase, diaphorase, formazan dyes and combinations thereof.

42. The device of claim 34, wherein said colorimetric indicator comprises a 2,4,6-tris(2-pyridyl)-s-triazine (TPTZ) complexed with mercury ion or iron ion.

43. The device of claim 34, wherein said colorimetric indicator comprises a 2,2'-bichinchoninic acid.

44. The device of claim 34, wherein said colorimetric indicator comprises a 1,10-phenanthroline.

45. The device of claim 34, wherein the colorimetric indicator comprises a universal pH indicator.

46. The device of any one of claims 1-3, wherein the device is a skin-mounted sensor.

47. The device of claim 46, wherein said skin-mounted sensor quantitatively and/or qualitatively monitors said biofluid of a subject.

48. The device of any one of claims 1-3, wherein the device has a modulus and a thickness within a factor of 2 of a modulus and a thickness of an epidermal layer of the skin of a subject.

49. The device of any one of claims 1-3, wherein the device has an average modulus less than or equal to 500 kPa.

50. The device of any one of claims 1-3, wherein the device has an average modulus selected from a range of 0.5 kPa to 100 kPa.

51. The device of any one of claims 1-3, wherein the device has a net bending stiffness less than or equal to 1 nN m.

52. The device of any one of claims 1-3, wherein the device has a net bending stiffness selected from a range of 0.1 to 1 nN m.

53. The device of any one of claims 1-3, wherein the device has a footprint selected from a range of 300 mm² to 2000 cm².

54. A method of making a device for monitoring a biofluid comprising:

providing a functional substrate that is mechanically matched to skin; wherein said functional substrate provides for microfluidic transport of said biofluid; and providing at least one sensor supported by said functional substrate.

55. A method of making a device for monitoring a biofluid comprising:

providing a functional substrate that is thermally matched to skin; wherein said functional substrate provides for microfluidic transport of said biofluid; and providing at least one sensor supported by said functional substrate.

56. A method of making a device for monitoring a biofluid comprising:

providing a functional substrate that provides for microfluidic transport of said biofluid through one or more microfluidic channels each having a substantially uniform lateral dimension; and providing at least one sensor supported by said functional substrate.

57. A method for monitoring a biofluid comprising:

providing a device comprising a functional substrate that is mechanically matched to skin; wherein said functional substrate provides for microfluidic transport of said biofluid; and at least one sensor supported by said functional substrate;

applying said device to the skin of a subject; and obtaining data from said at least one sensor; wherein said data provide quantitative and/or qualitative information about said biofluid of said subject.

58. A method for monitoring a biofluid comprising:

providing a device comprising a functional substrate that is thermally matched to skin; wherein said functional substrate provides for microfluidic transport of said biofluid; and at least one sensor supported by said functional substrate;

applying said device to the skin of a subject; and obtaining data from said at least one sensor; wherein said data provide quantitative and/or qualitative information about said biofluid of said subject.

59. A method for monitoring a biofluid comprising:

providing a functional substrate that provides for microfluidic transport of said biofluid through one or more microfluidic channels each having a substantially uniform lateral dimension; and at least one sensor supported by said functional substrate;

applying said device to the skin of a subject; and obtaining data from said at least one sensor; wherein said data provide quantitative and/or qualitative information about said biofluid of said subject.

60. The method of any one of claims 54-59, wherein said functional substrate is an elastomeric substrate.

61. The method of any one of claims 54-59, wherein the device further comprises a component for extracting interstitial fluid or blood from a subject.

62. The method of claim 61, wherein the component for extracting interstitial fluid or blood is selected from a microneedle component, a reverse iontophoresis component and a thermal microabrasion component.

63. The method of any one of claims 54-59, wherein said functional substrate has a modulus less than or equal to 100 MPa.

64. The method of any one of claims 54-59, wherein said functional substrate has a dielectric constant greater than or equal to 2.0.

65. The method of any one of claims 54-59, wherein said functional substrate has a permeability for said biofluid greater than or equal to 0.2 g/h m².

66. The method of any one of claims 54-59, wherein said functional substrate has a coefficient of thermal expansion selected from a range of 1/° C. ($\times 10^{-6}$) to 3/° C. ($\times 10^4$).

67. The method of any one of claims 54-59, wherein said sensor is a colorimetric indicator.

68. The method of any one of claims 54-59, wherein said sensor is a non-pH colorimetric indicator.

69. The method of any one of claims 54-59, wherein said sensor comprises an electrical sensor, a chemical sensor, a biological sensor, a temperature sensor, an optical sensor, a mechanical sensor or a magnetic sensor.

70. The method of any one of claims 54-59, wherein said sensor is an LC resonator.

71. The method of any one of claims 54-59, wherein said device further comprises an actuator that generates electromagnetic radiation, acoustic energy, an electric field, a magnetic field, heat, a RF signal, a voltage, a chemical change or a biological change.

72. The method of any one of claims 54-59, wherein said device further comprises a transmitter or receiver.

73. The method of any one of claims 54-59, wherein said device further comprises at least one coil.

74. The method of claim 73, wherein said at least one coil is a near-field communication coil.

75. The method of claim 73, wherein said at least one coil is an inductive coil.

76. The method of any one of claims 54-59, wherein the device has a modulus and a thickness within a factor of 2 of a modulus and a thickness of an epidermal layer of the skin of a subject.

77. The method of any one of claims 54-59, wherein said device has an average modulus less than or equal to 500 kPa.

78. The method of any one of claims 54-59, wherein said device has a net bending stiffness less than or equal to 1 nN m.

* * * * *

专利名称(译)	用于生物流体的表皮表征的装置和相关方法		
公开(公告)号	US20170231571A1	公开(公告)日	2017-08-17
申请号	US15/501373	申请日	2015-08-11
申请(专利权)人(译)	洽伊利诺州大学董事会		
当前申请(专利权)人(译)	洽伊利诺州大学董事会		
[标]发明人	ROGERS JOHN A KOH AHYEON KANG DAESHIK LIU YUHAO HUANG XIAN		
发明人	ROGERS, JOHN A. KOH, AHYEON KANG, DAESHIK LIU, YUHAO HUANG, XIAN		
IPC分类号	A61B5/00 A61B5/01 A61B5/053 A61B5/145		
CPC分类号	A61B5/6833 A61B5/14514 A61B5/14532 A61B5/14539 A61B5/14546 A61B5/002 A61B5/01 A61B5/053 A61B5/14517 A61B5/0059 A61B5/0075 A61B5/1032 A61B5/1455 A61B5/1468 A61B5/1477 A61B5/4266 A61B5/6898 A61B2562/12 A61B2576/00 B01L3/502707 B01L3/505 G16H30/40		
优先权	62/035823 2014-08-11 US 62/142877 2015-04-03 US		
外部链接	Espacenet USPTO		

摘要(译)

公开了皮肤安装或表皮装置和用于监测生物流体的方法。该装置包括与皮肤机械和/或热匹配的功能性基底，以提供长期佩戴的持久粘合。功能性基底允许生物流体从皮肤到一个或多个传感器的微流体传输，所述传感器测量和/或检测生物参数，例如生物流体产生速率，生物流体体积和生物标记物浓度。装置内的传感器可以是机械的，电气的或化学的，其中比色指示器可以通过肉眼或便携式电子设备（例如智能手机）观察到。通过监测个体健康状态随时间的变化，所公开的装置可以提供异常状况的早期指示。

