



(19) **United States**  
(12) **Patent Application Publication**  
**Shaanan et al.**

(10) **Pub. No.: US 2013/0245392 A1**  
(43) **Pub. Date: Sep. 19, 2013**

- (54) **ANALYTE TESTING DEVICES**
- (71) Applicant: **YOFIMETER, LLC**, La Jolla (CA)
- (72) Inventors: **Gad Shaanan**, La Jolla, CA (US); **Marc Goldman**, La Jolla, CA (US)
- (73) Assignee: **YOFIMETER, LLC**, La Jolla, CA (US)
- (21) Appl. No.: **13/868,831**
- (22) Filed: **Apr. 23, 2013**

- A61B 5/15* (2006.01)
- A61B 5/145* (2006.01)
- A61B 5/11* (2006.01)
- (52) **U.S. Cl.**
- CPC ..... *A61B 5/15113* (2013.01); *A61B 5/145* (2013.01); *A61B 5/14532* (2013.01); *A61B 5/1118* (2013.01); *A61B 5/15148* (2013.01); *A61B 5/150175* (2013.01); *A61B 5/15194* (2013.01); *A61B 5/742* (2013.01); *A61B 5/0004* (2013.01); *A61B 5/746* (2013.01); *A61B 5/150961* (2013.01)
- USPC ..... **600/301**; 600/309; 600/365

**Related U.S. Application Data**


- (63) Continuation of application No. 13/689,618, filed on Nov. 29, 2012, which is a continuation-in-part of application No. 13/188,399, filed on Jul. 21, 2011, now abandoned, which is a continuation-in-part of application No. 13/187,360, filed on Jul. 20, 2011, which is a continuation-in-part of application No. 13/165,621, filed on Jun. 21, 2011, now abandoned, said application No. 13/188,399 is a continuation-in-part of application No. 13/187,397, filed on Jul. 20, 2011, now Pat. No. 8,333,716, which is a continuation-in-part of application No. 13/165,621, filed on Jun. 21, 2011, now abandoned.


**Publication Classification**





- (51) **Int. Cl.**
- A61B 5/151* (2006.01)
- A61B 5/00* (2006.01)

**ABSTRACT**

(57) Systems, devices, techniques and methods are disclosed for implementing an actuator mechanism of an analyte testing device. In one aspect, a method to test an analyte includes advancing an analyte sensor from a first position within a sensor cartridge of an analyte testing device to a second position that exposes at least a portion of the analyte sensor outside of the device, advancing a lancet projecting component from an initial position to a cocked position for a subsequent projection of a lancet, in which the advancing the analyte sensor and the advancing the lancet projecting component are initiated by a single operation, projecting the lancet to expose at least a portion of the lancet outside of the device, receiving a testing sample including an analyte at the exposed portion of the analyte sensor, processing the testing sample to determine a parameter of the analyte, and ejecting the analyte sensor from the device.

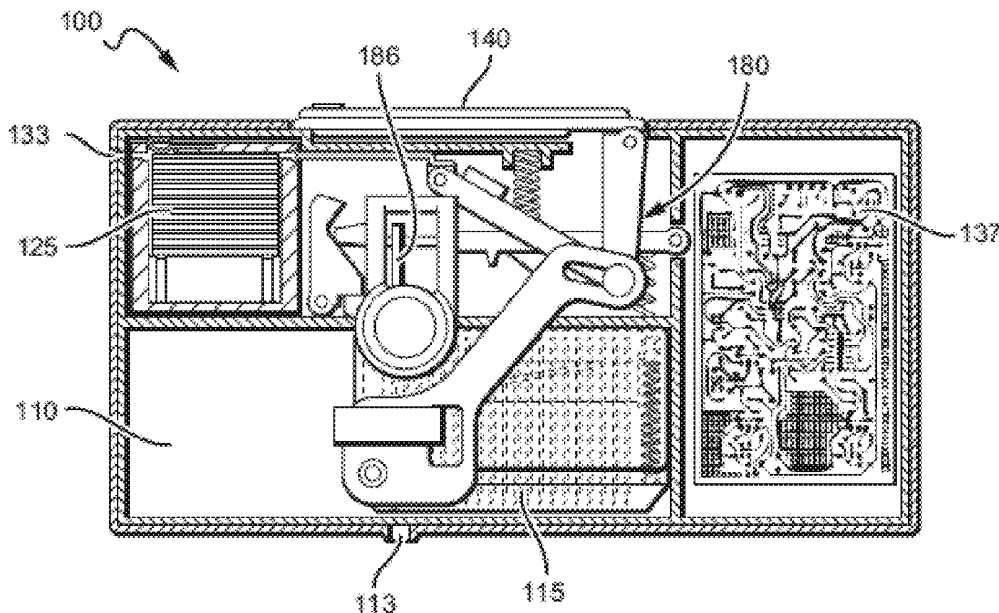

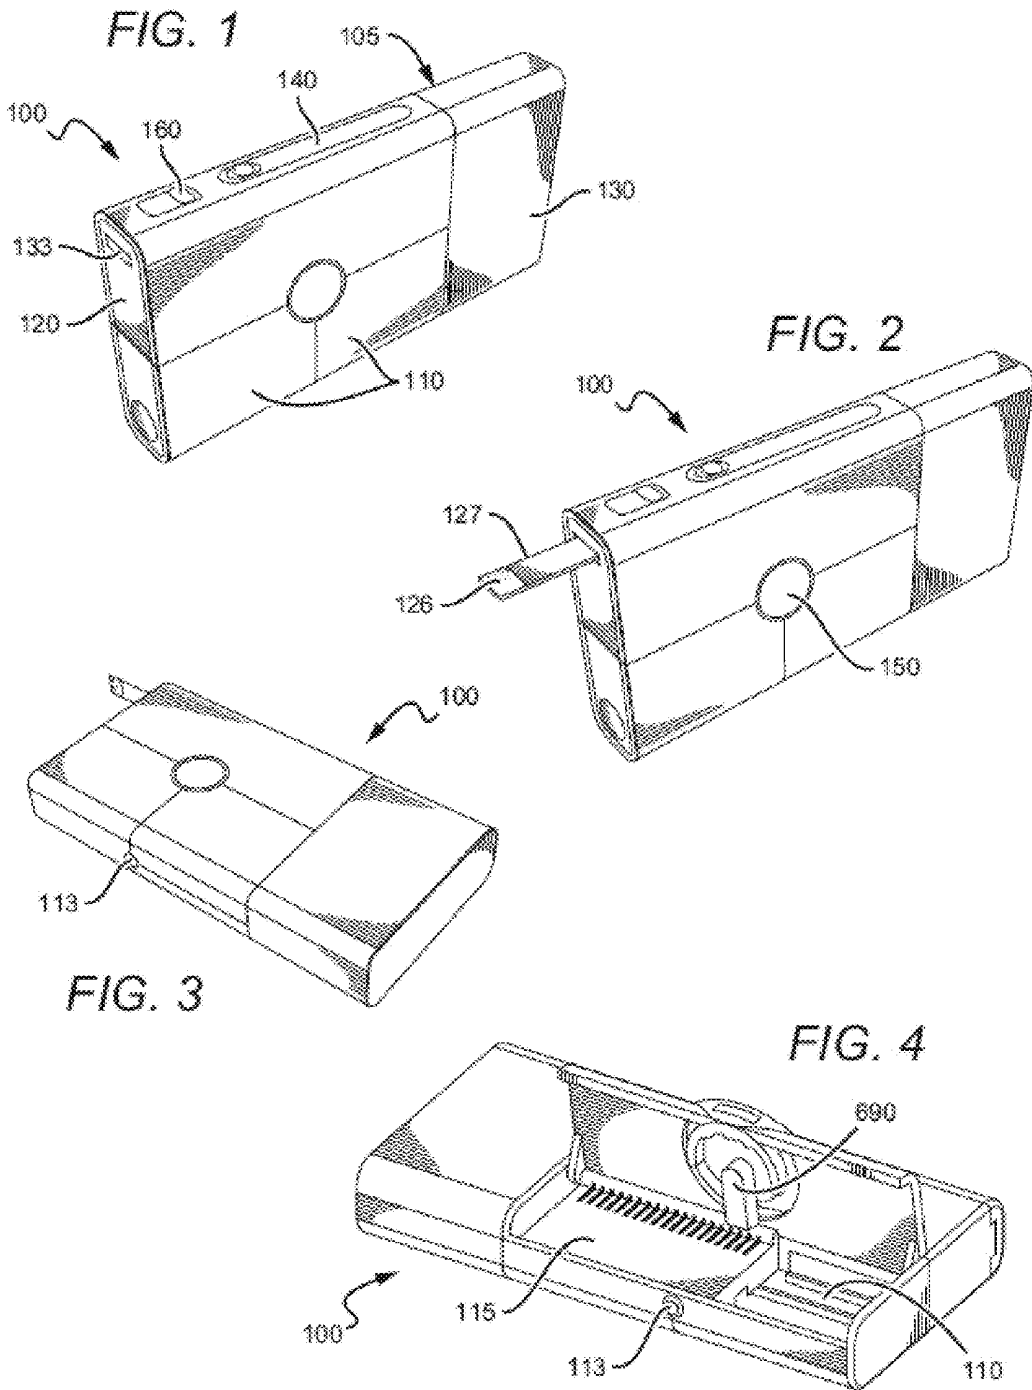

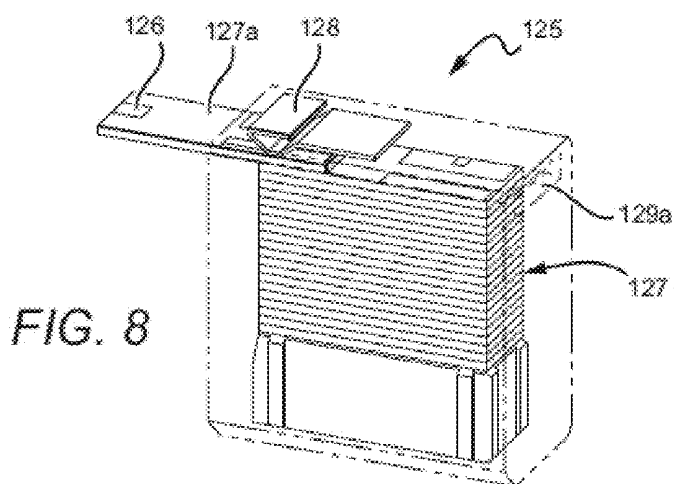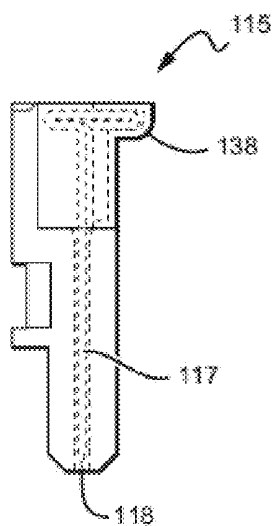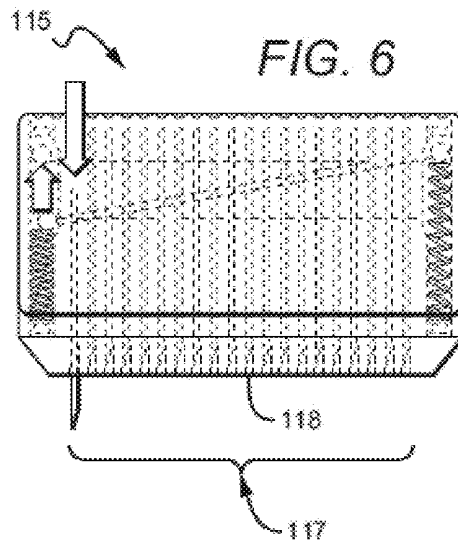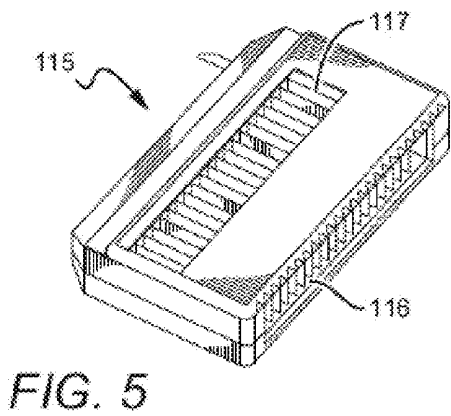





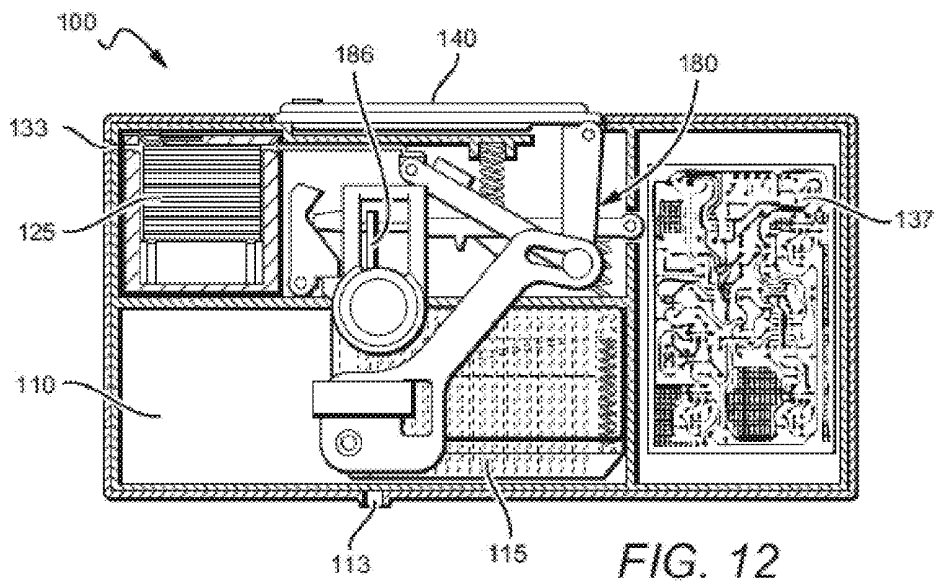



FIG. 11

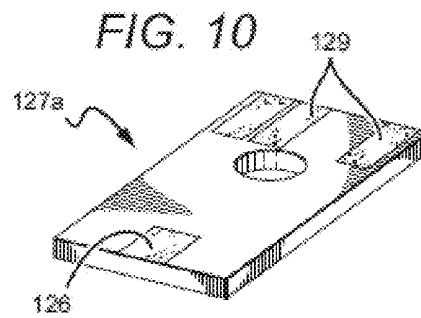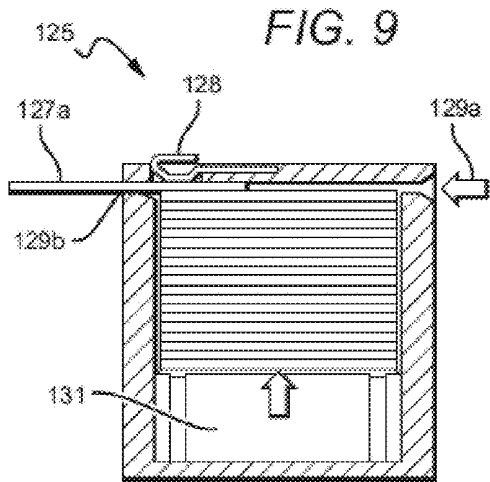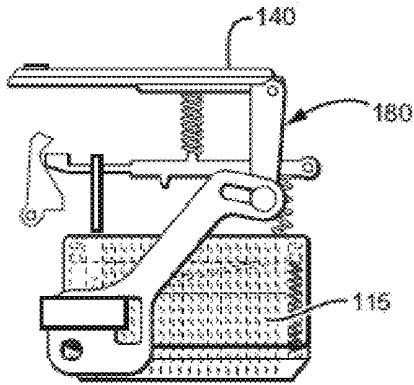


REST POSITION

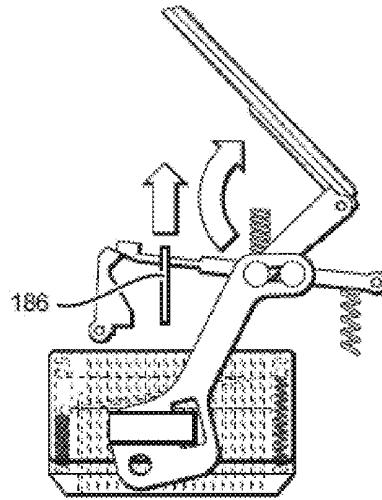

LEVER PULLED TO  
COCK HAMMER AND  
ADVANCE CASSETTE  
TO NEXT LANCET

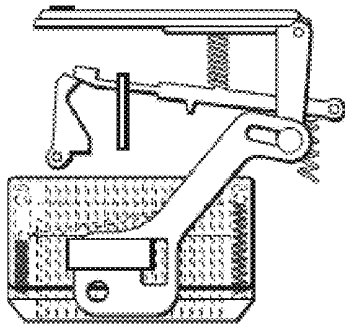

COCKED AND READY

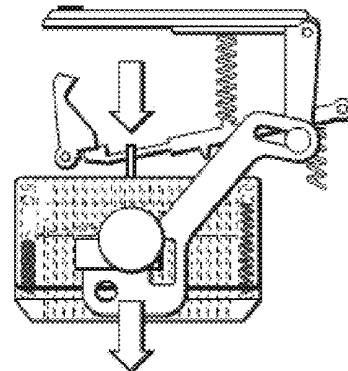

BUTTON IS PRESSED  
TO RELEASE HAMMER  
AND PROJECT LANCET



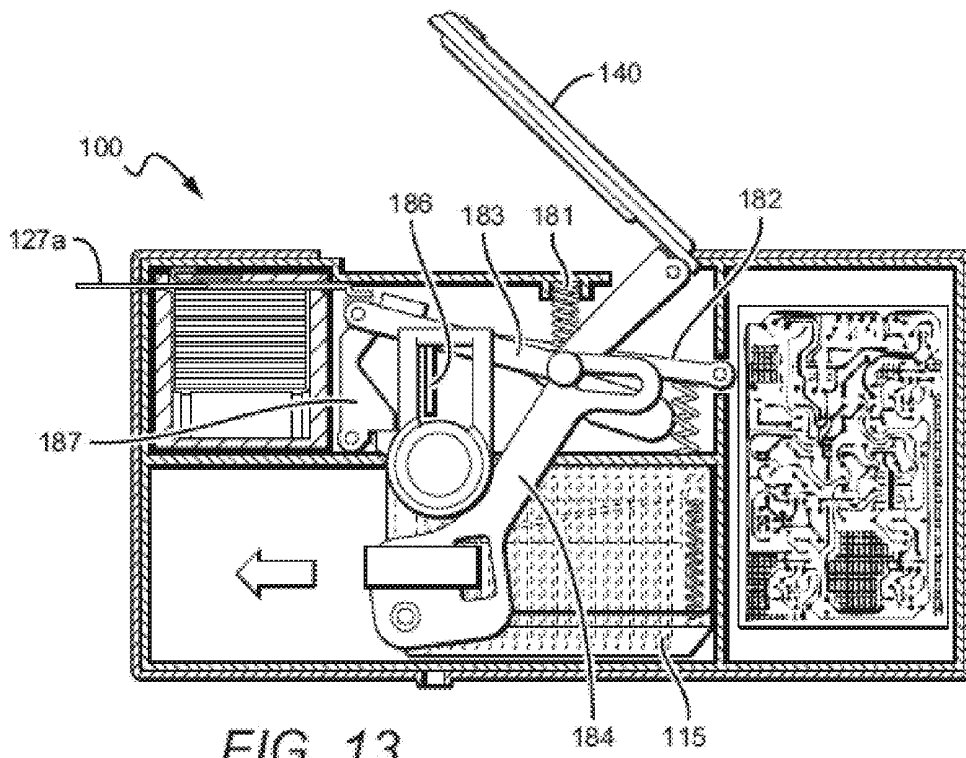


FIG. 13

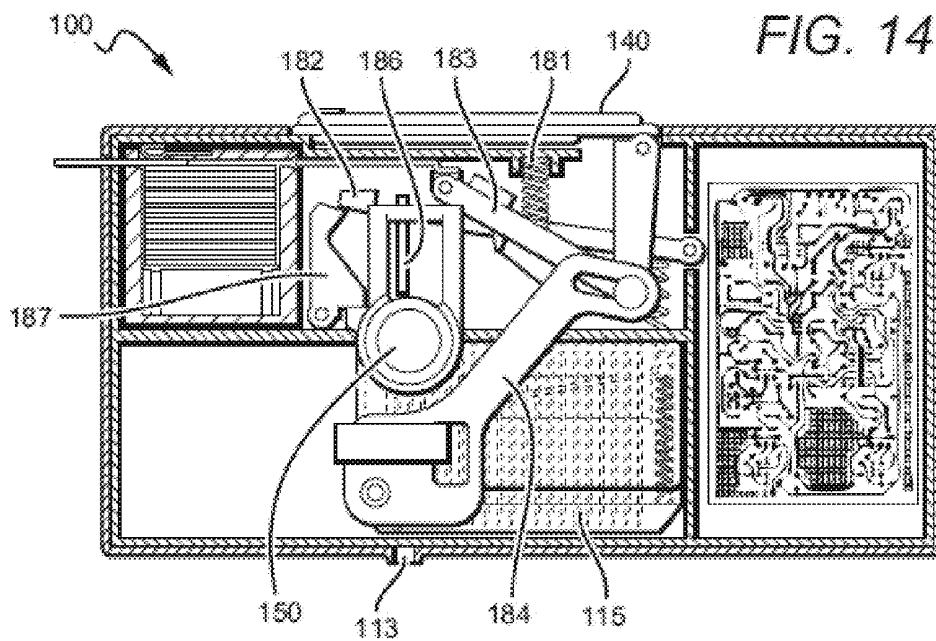


FIG. 14

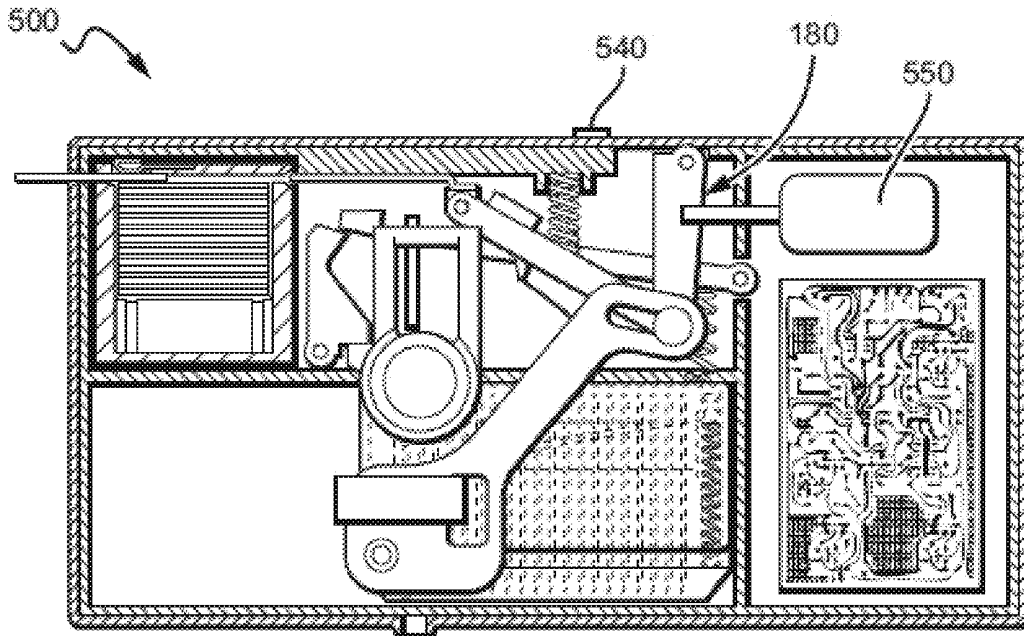


FIG. 15

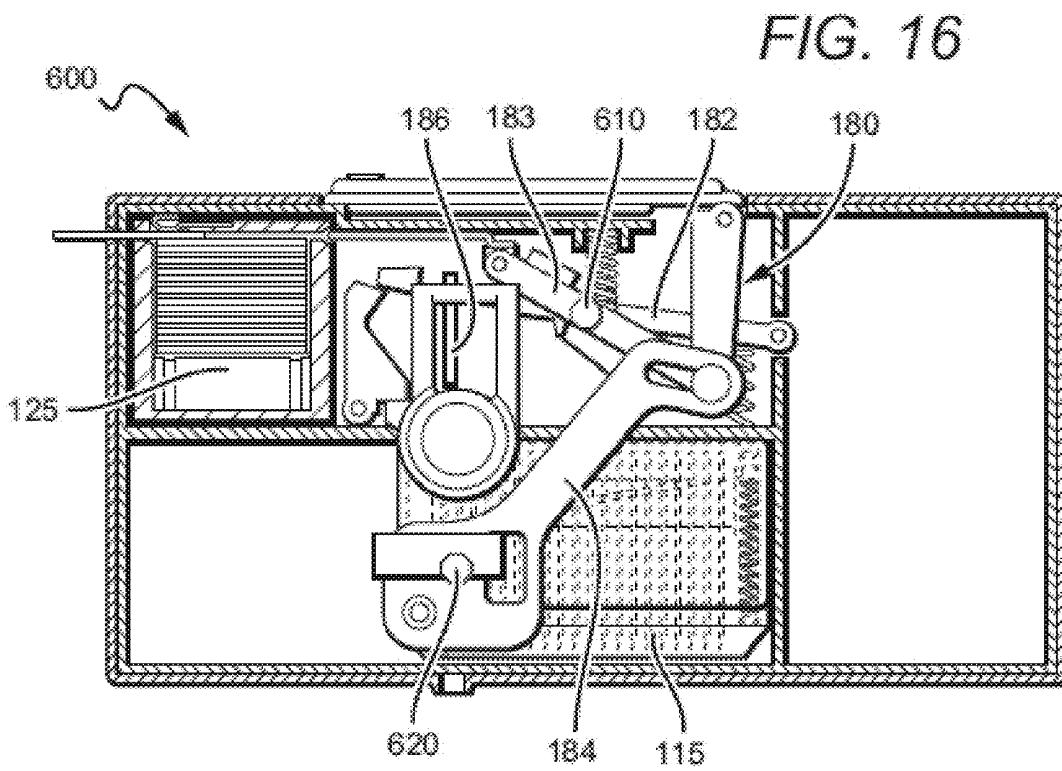


FIG. 16

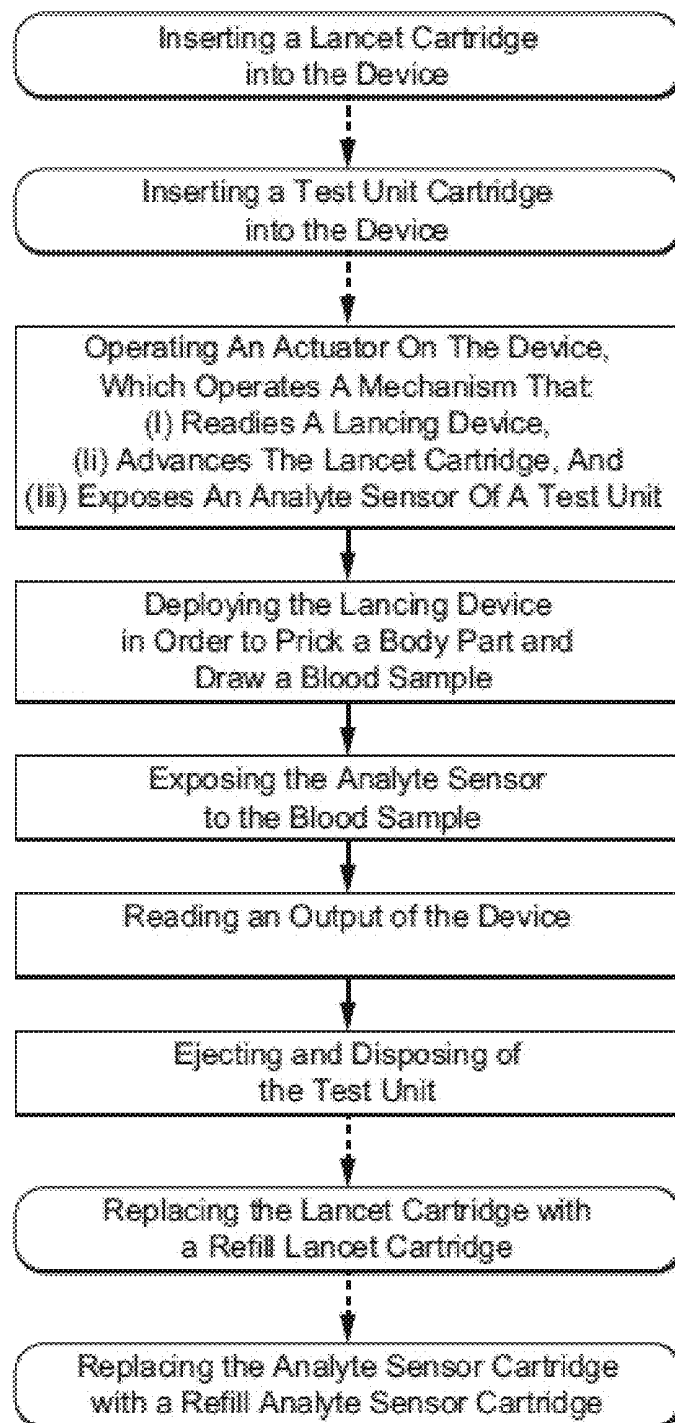


FIG. 17a

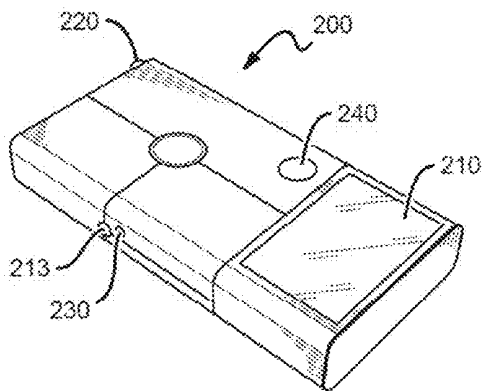


FIG. 17b

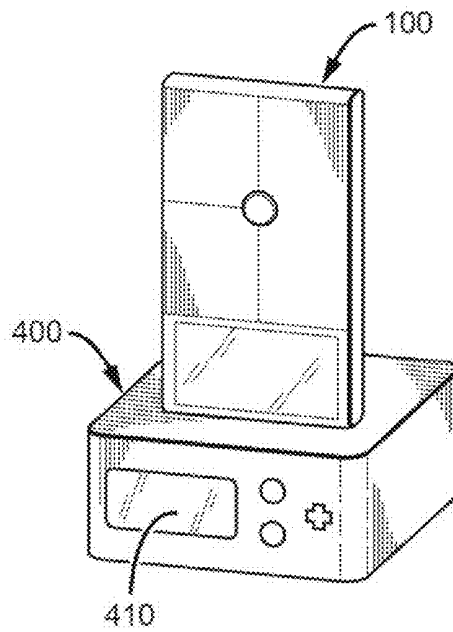


FIG. 17d

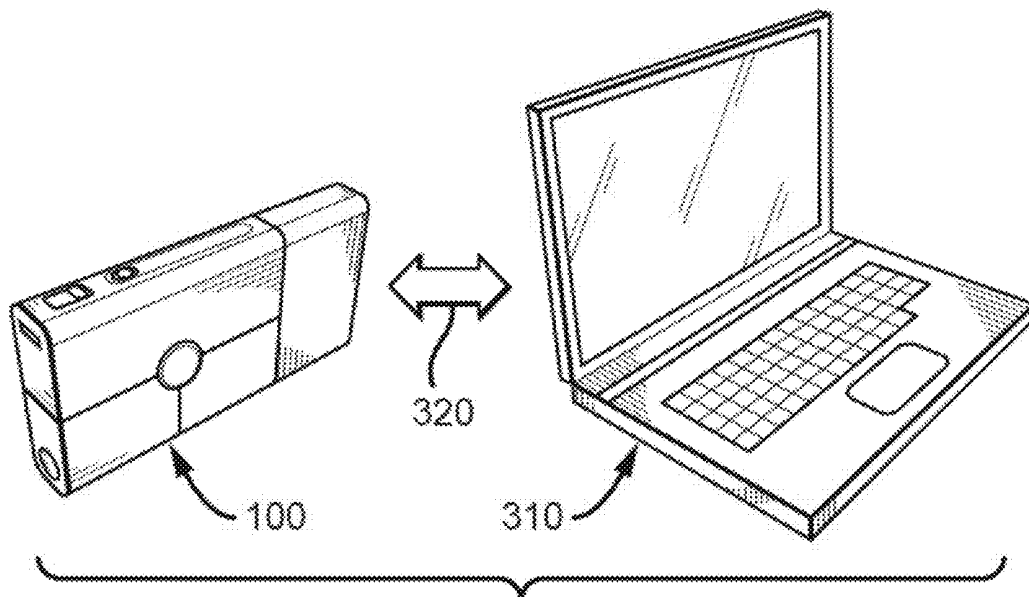


FIG. 17c

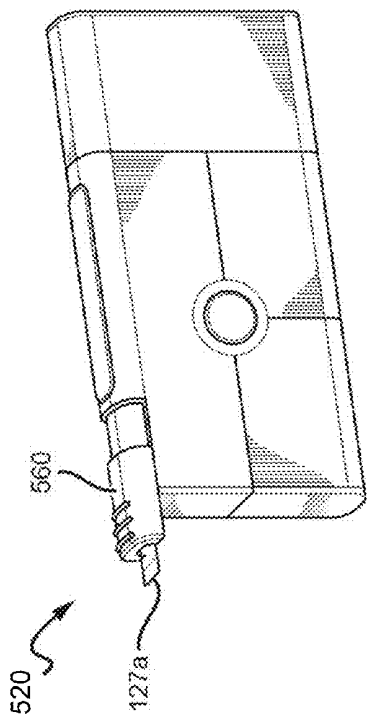


FIG. 17e

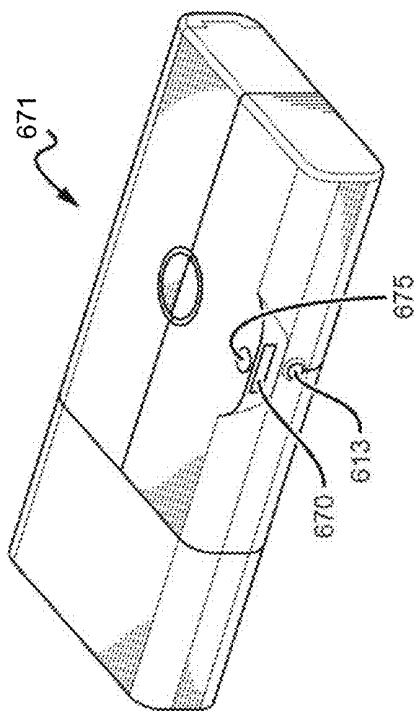


FIG. 17g

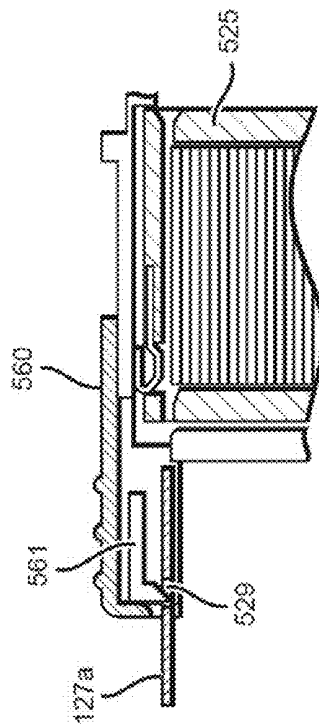


FIG. 17f

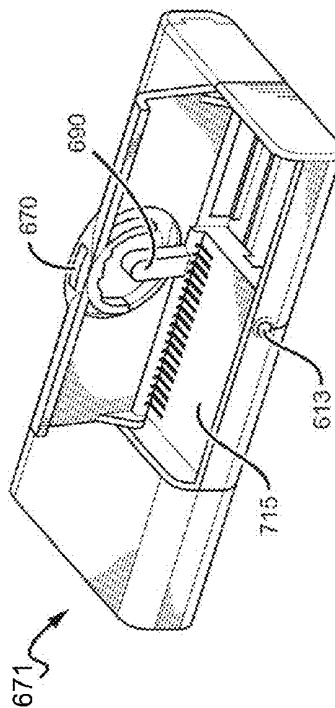


FIG. 17h

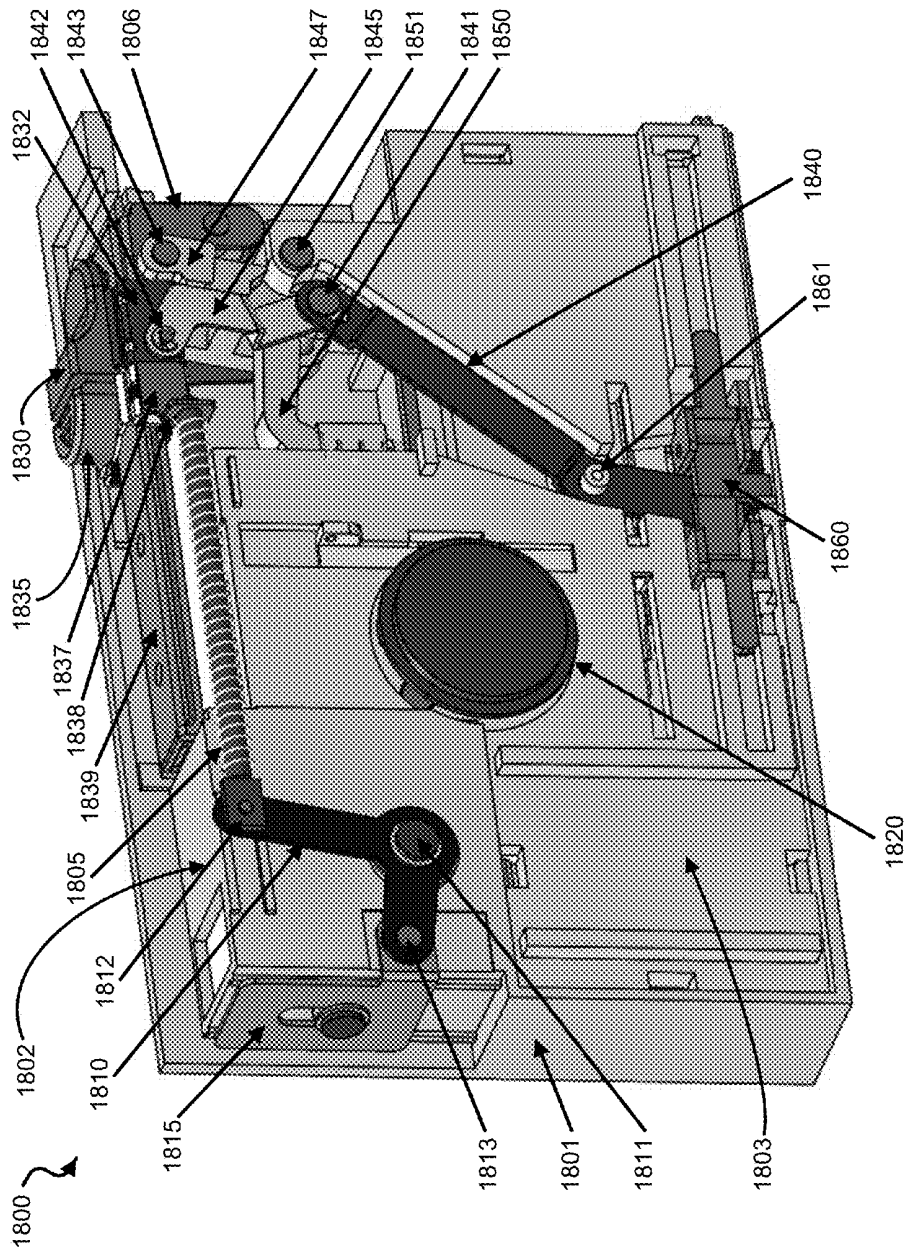


FIG. 18A

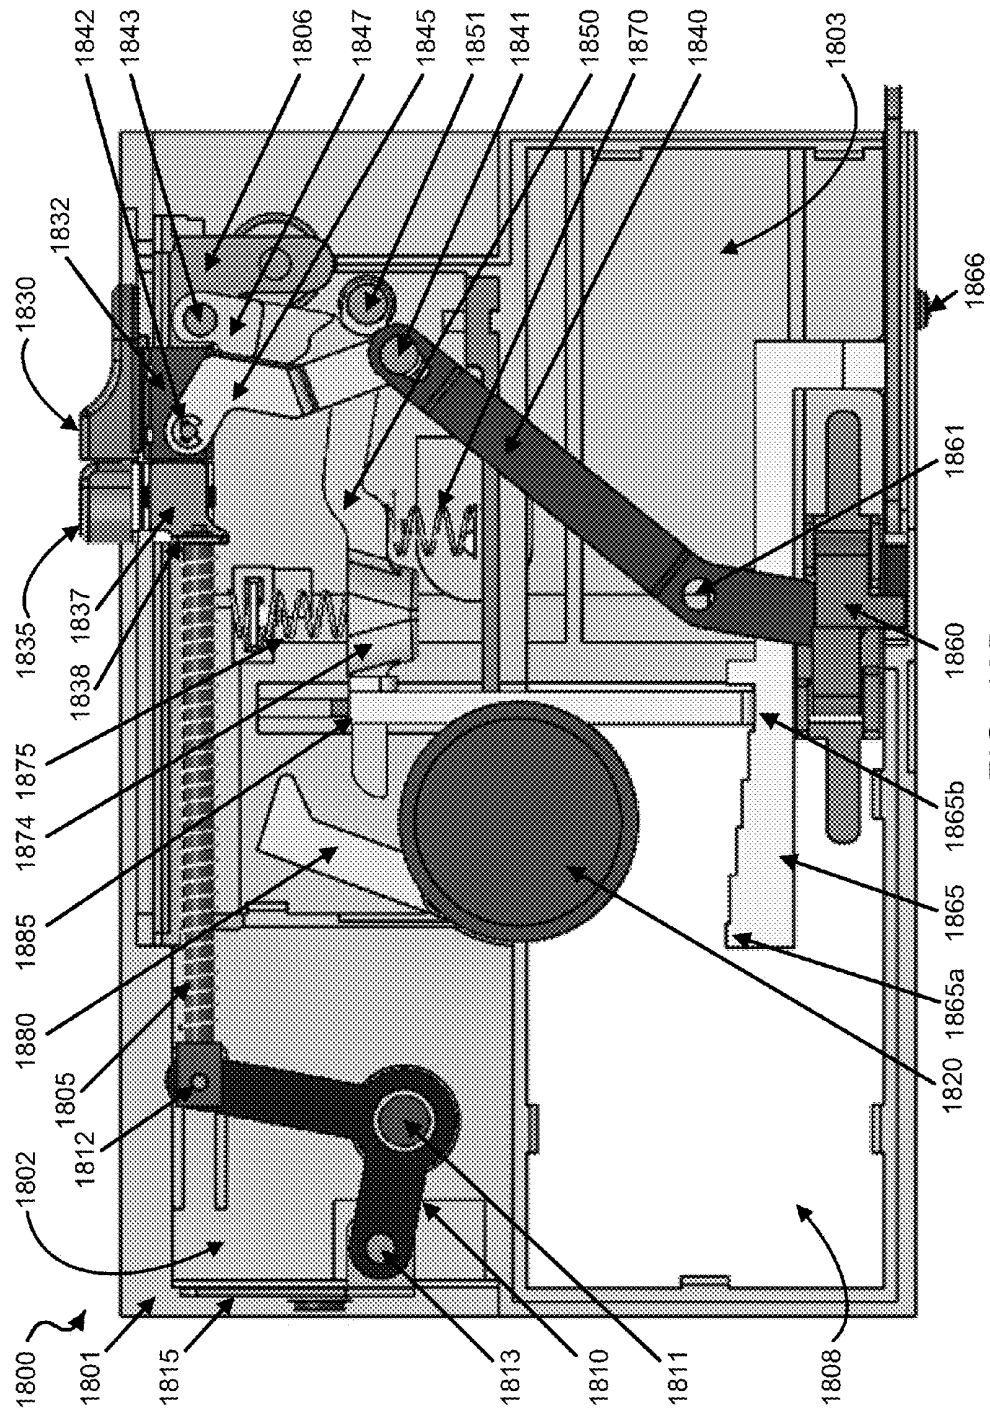


FIG. 18B

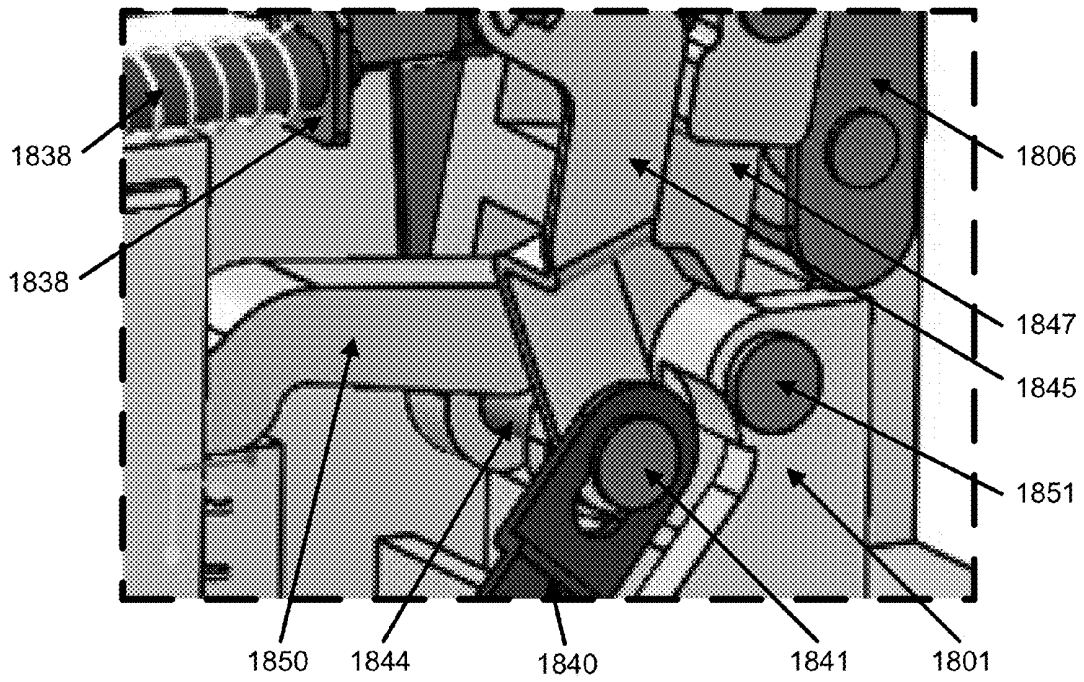


FIG. 18C



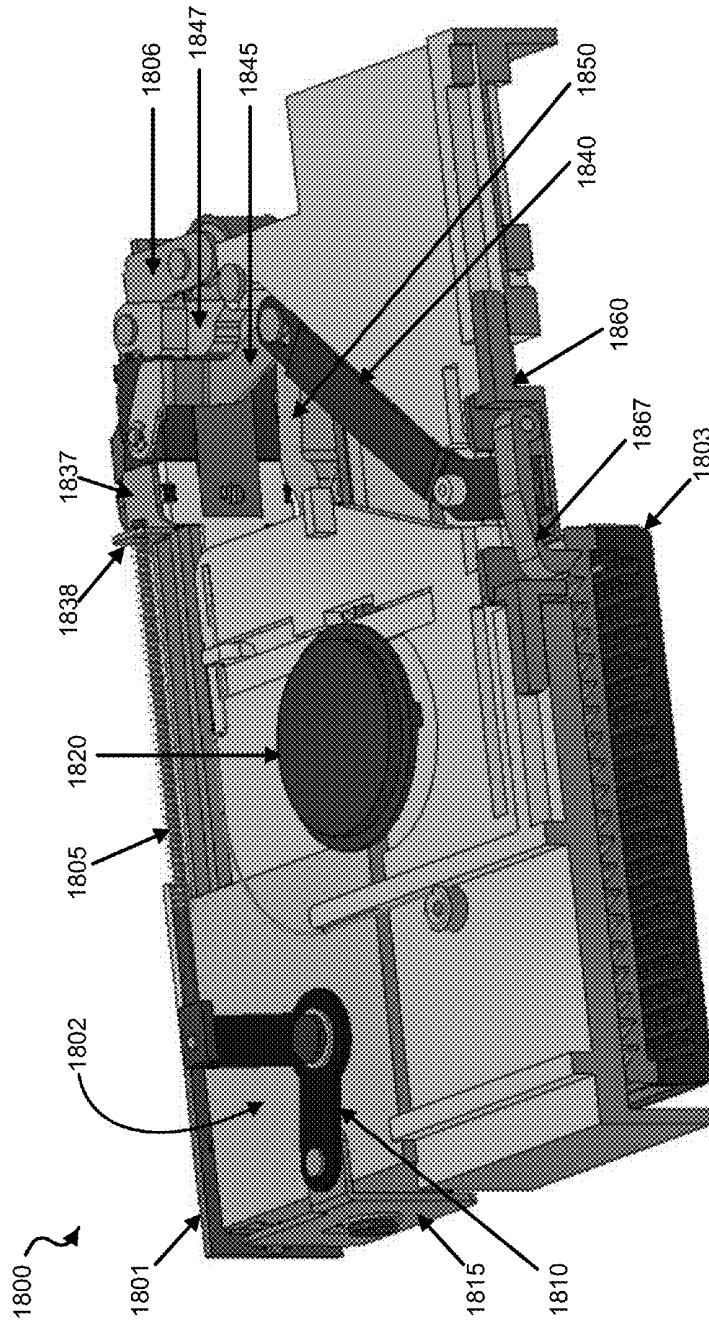


FIG. 18D

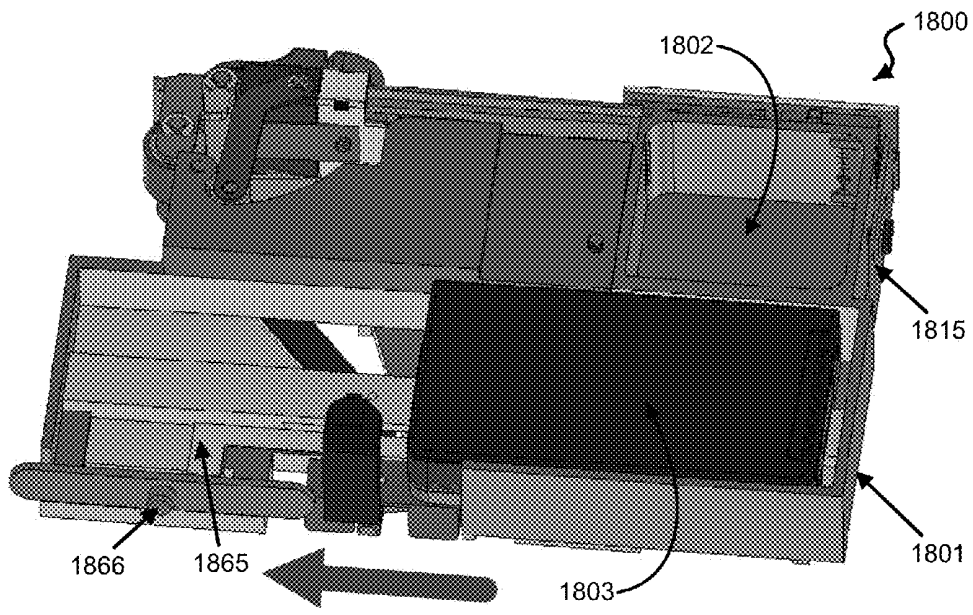

**Initial position of the lancet cartridge 1803**

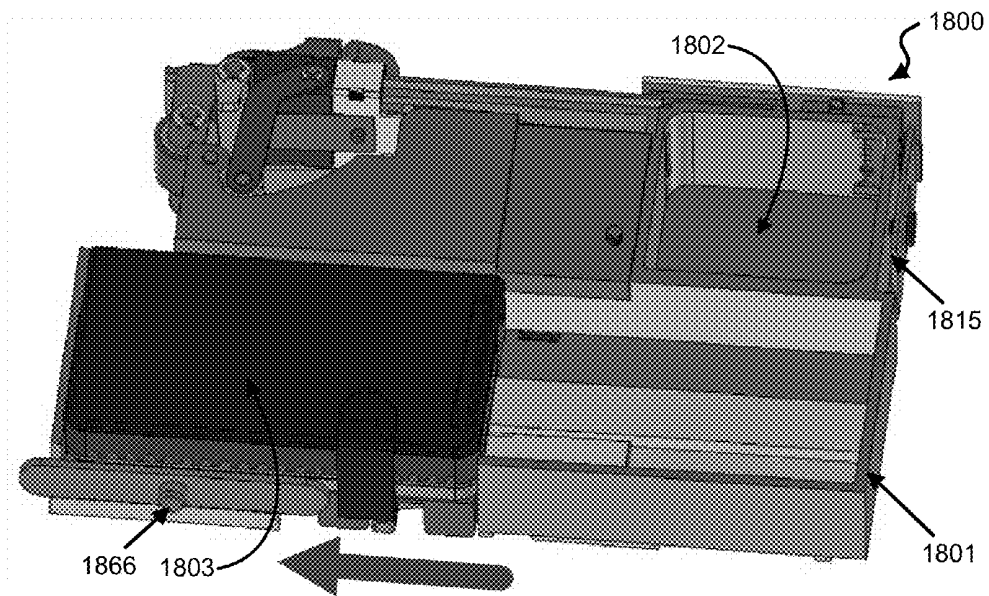

**Final position of the lancet cartridge 1803**

*FIG. 18E*



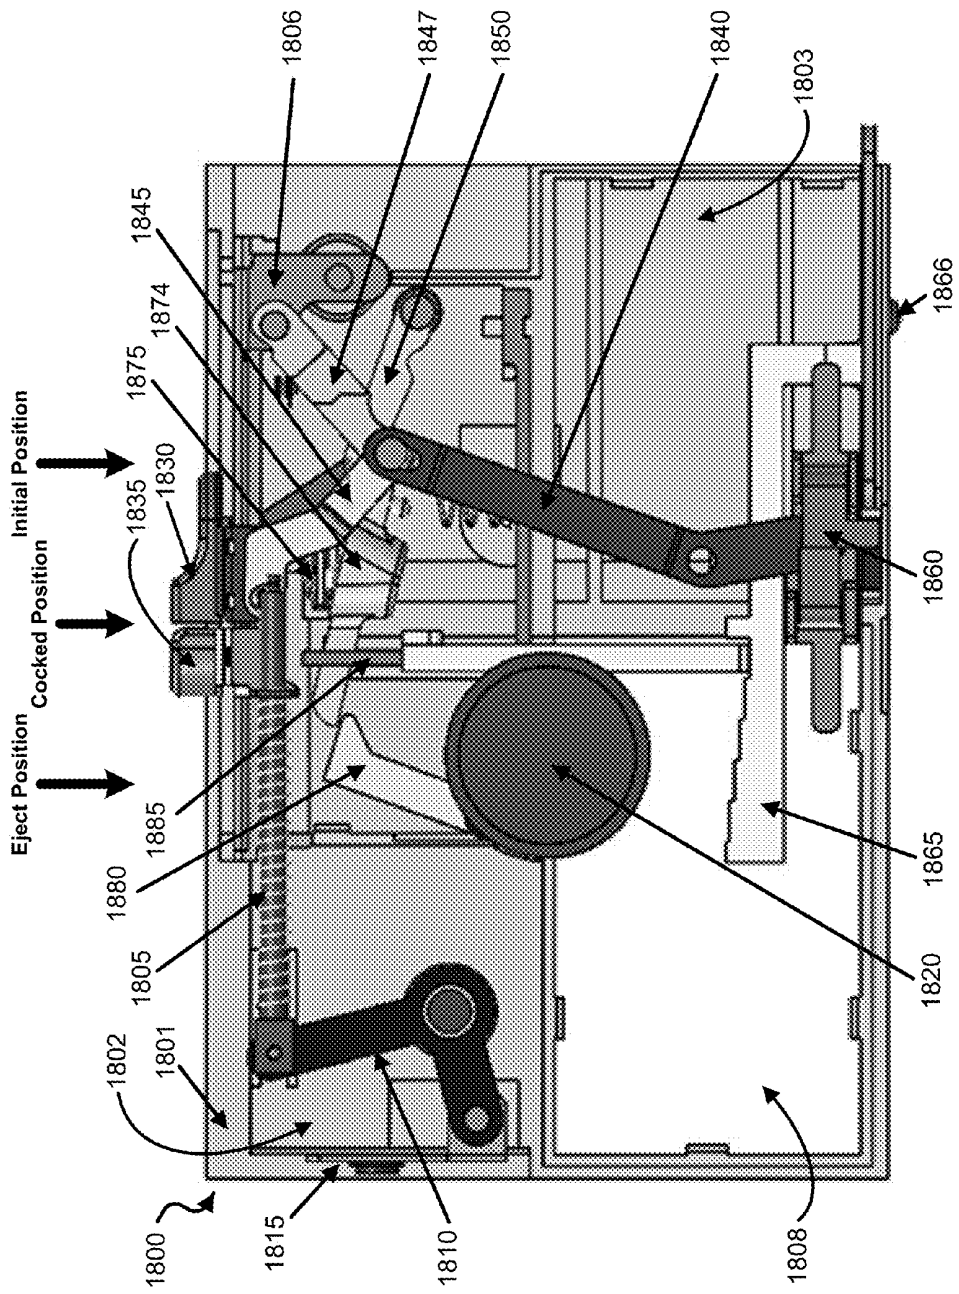
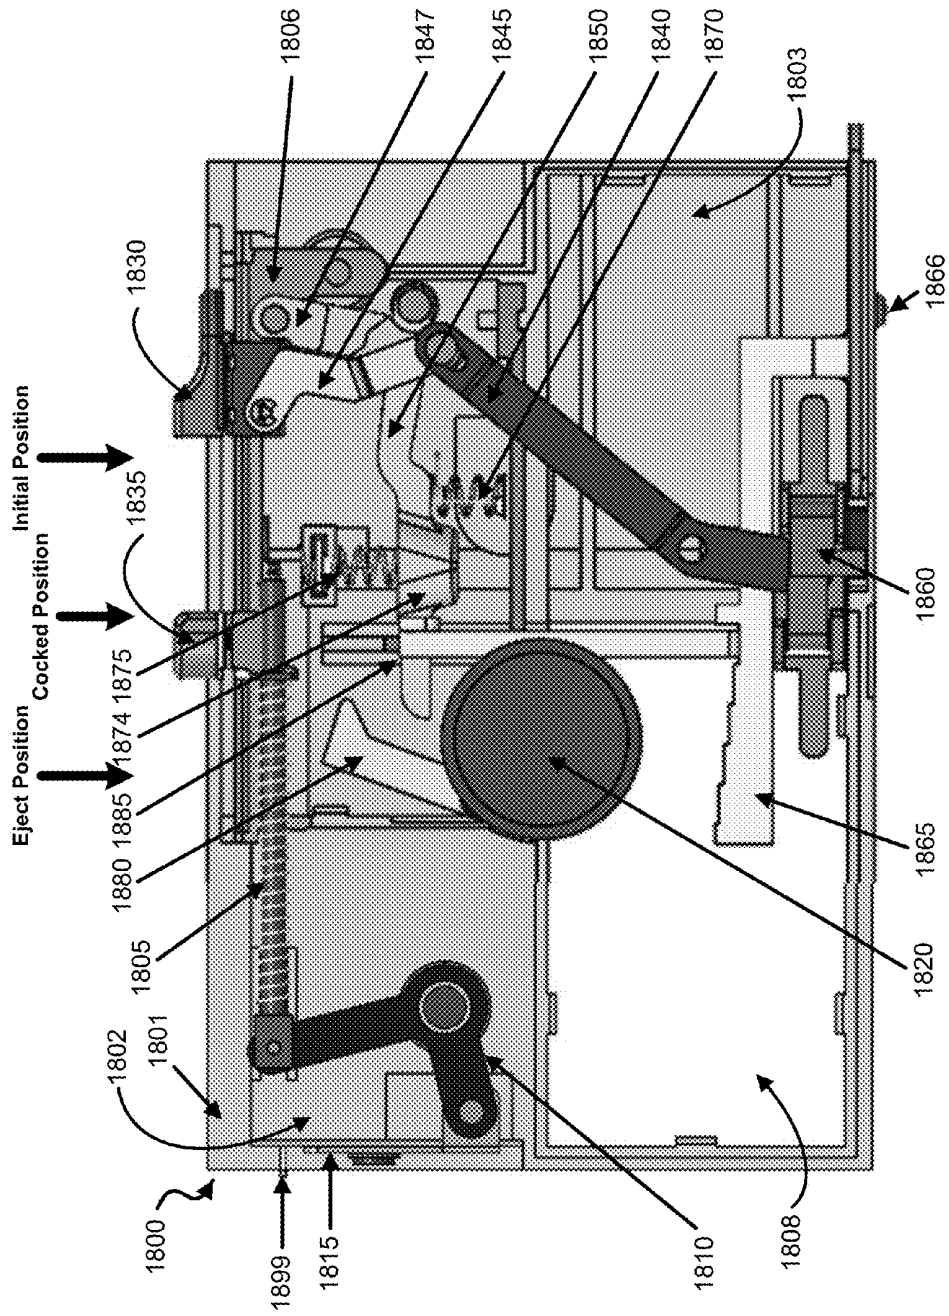


FIG. 19B



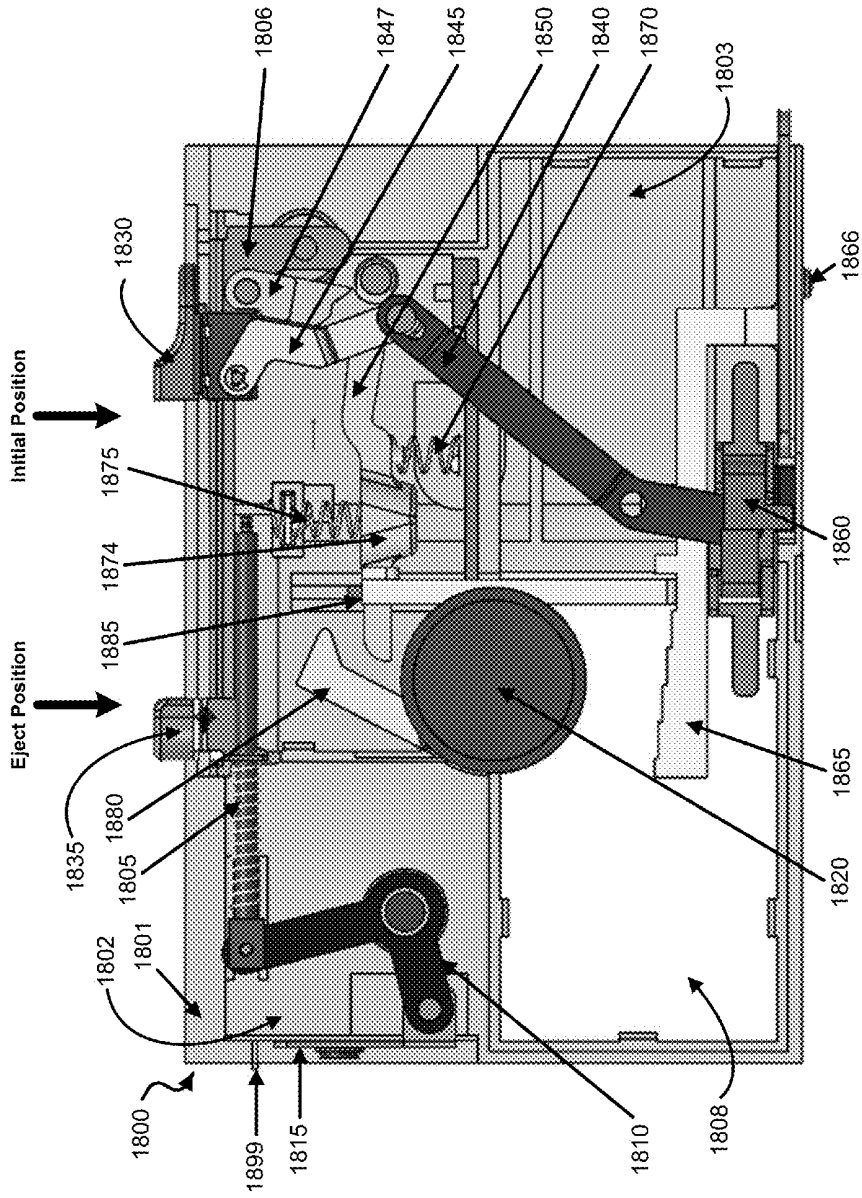


FIG. 20B

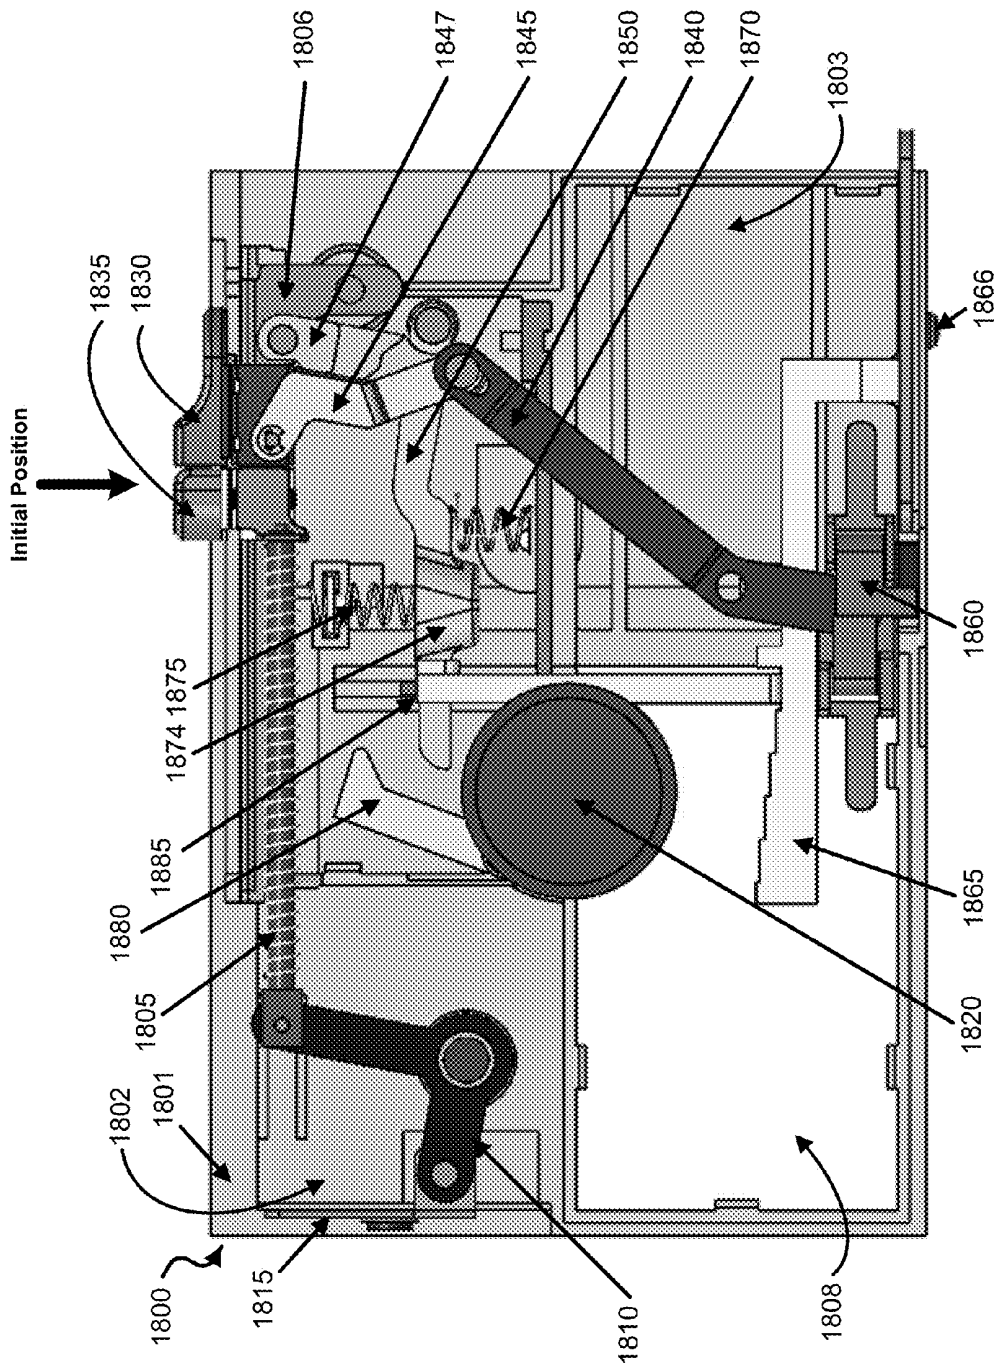


FIG. 20C

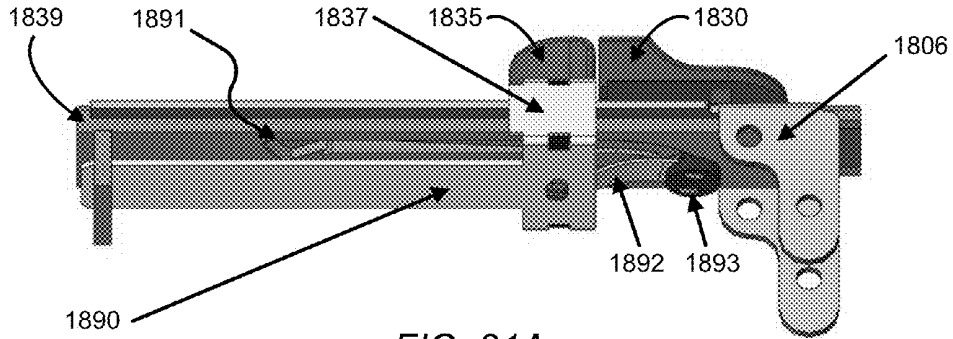


FIG. 21A

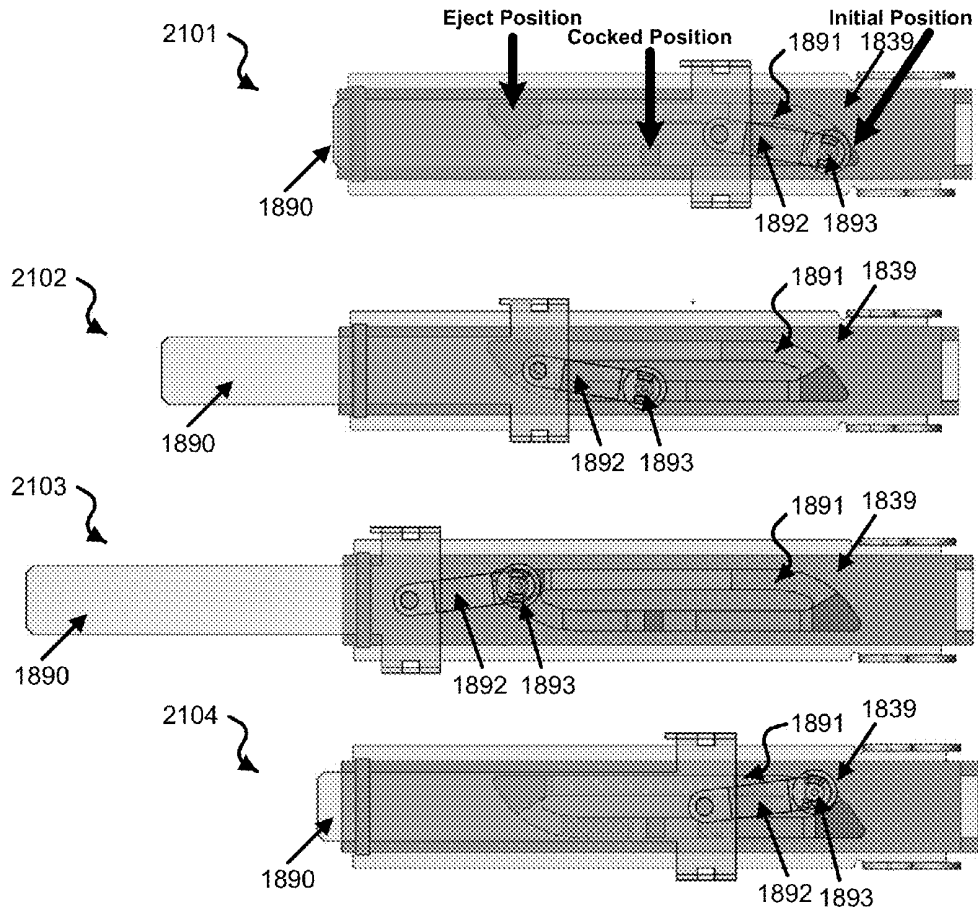
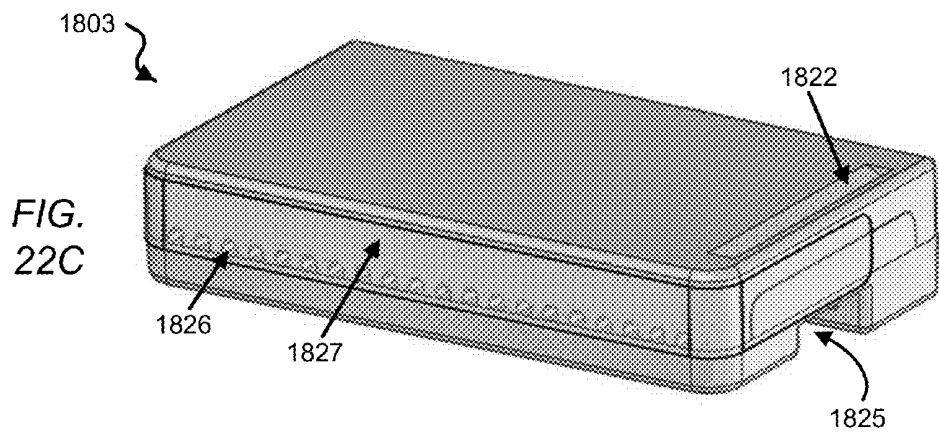
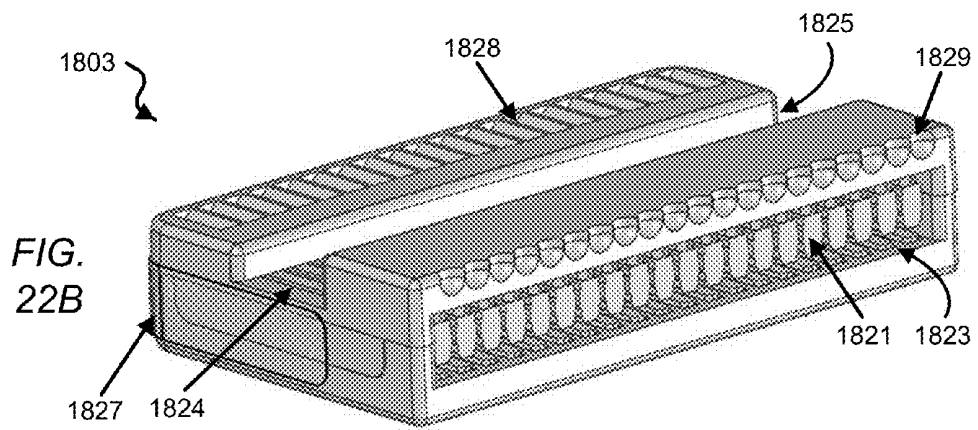
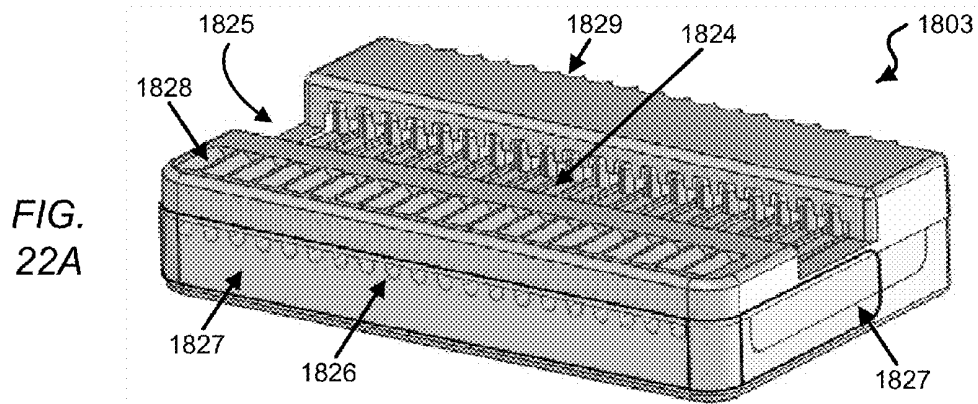


FIG. 21B



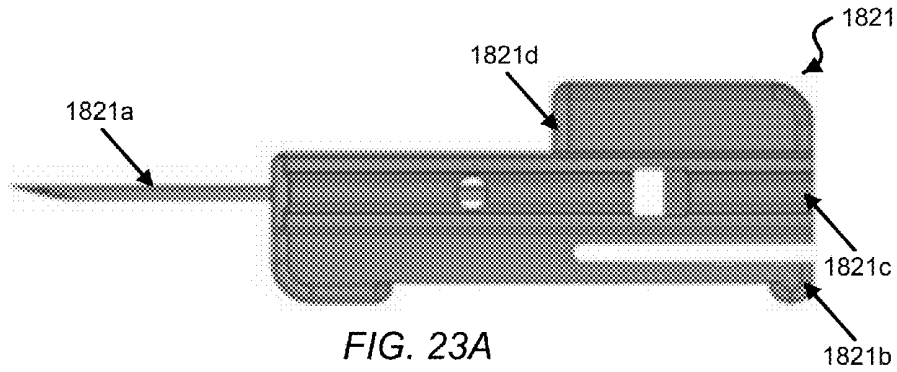


FIG. 23A

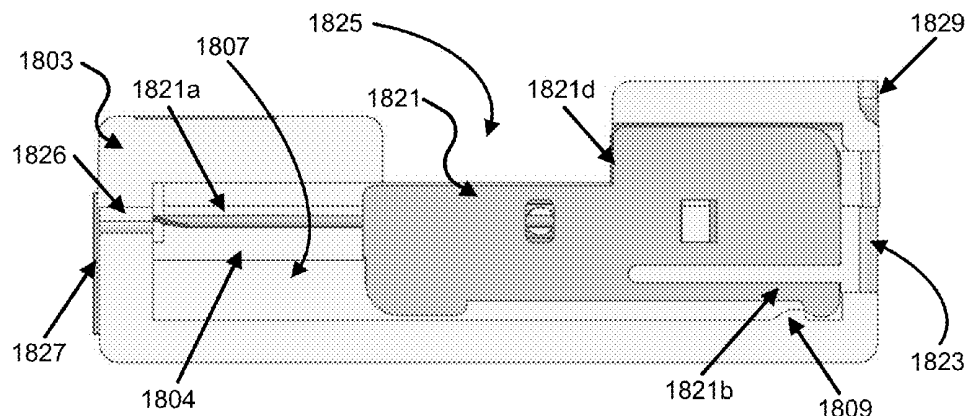


FIG. 23B

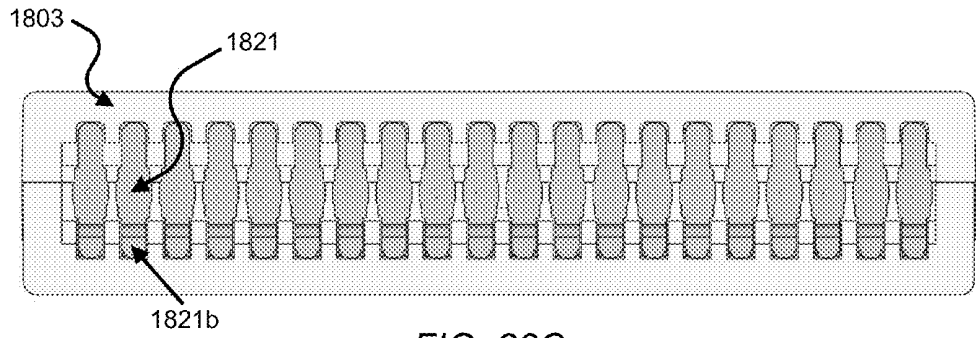


FIG. 23C

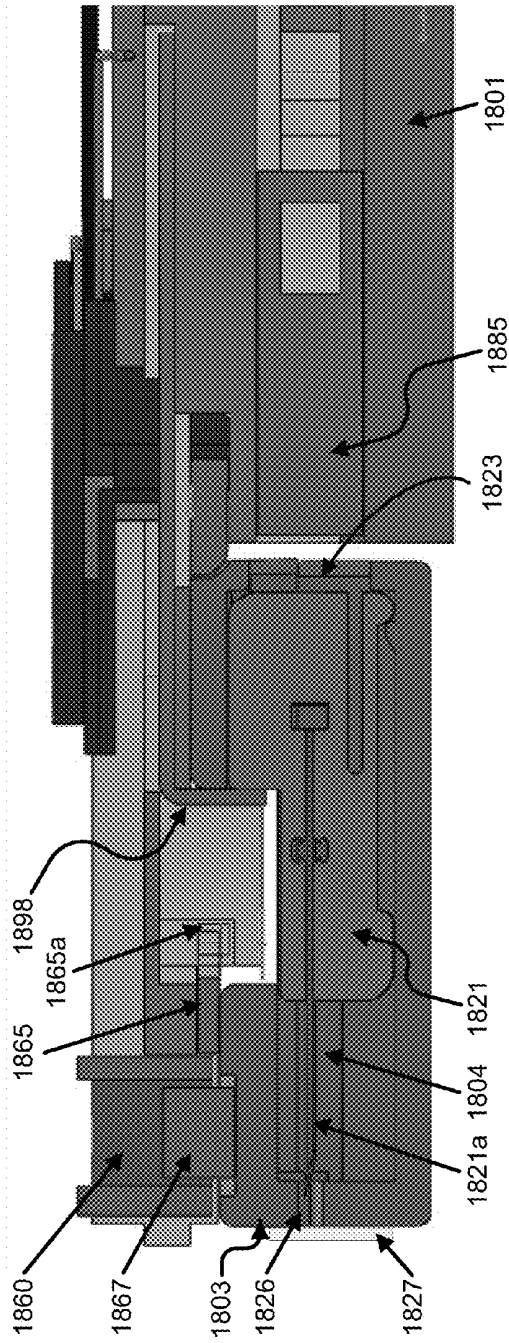


FIG. 24A

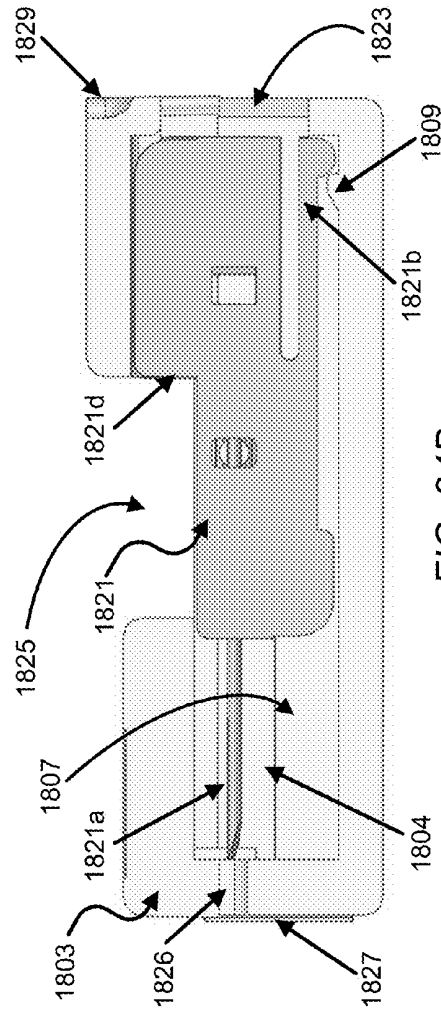


FIG. 24B

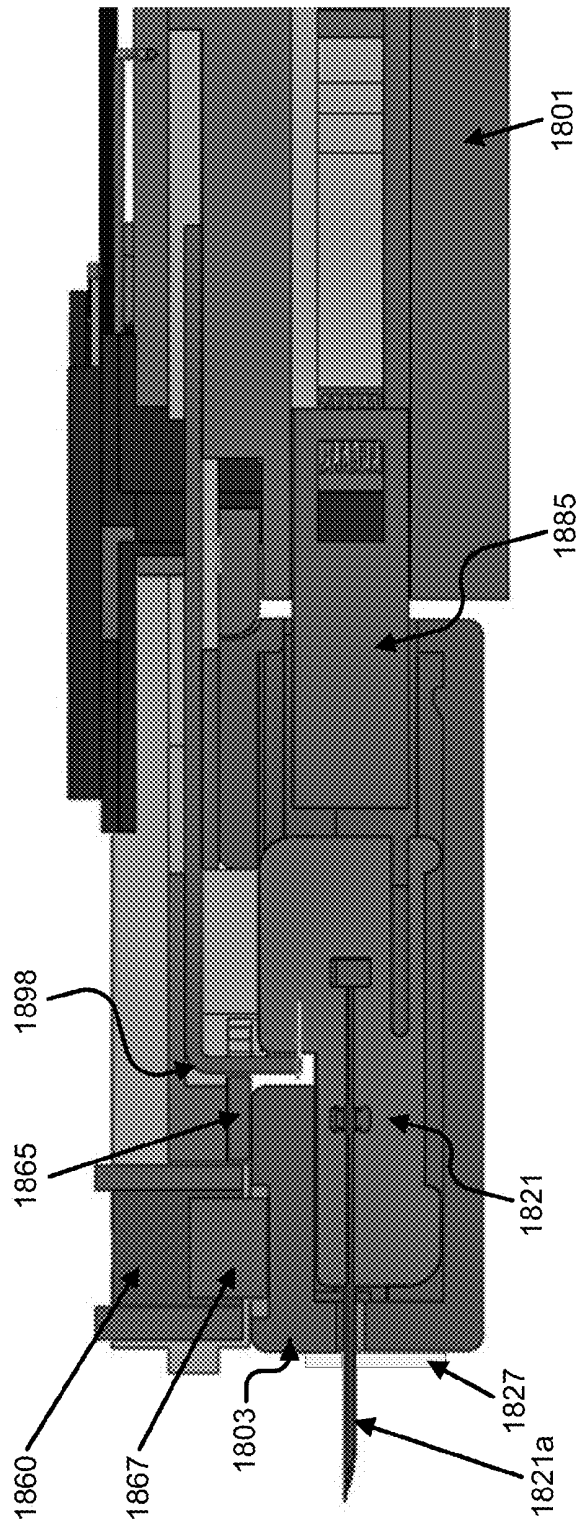
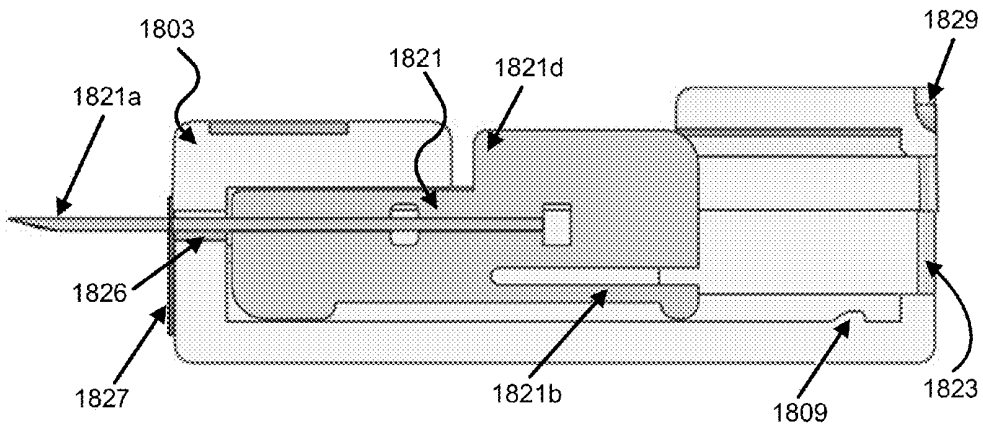
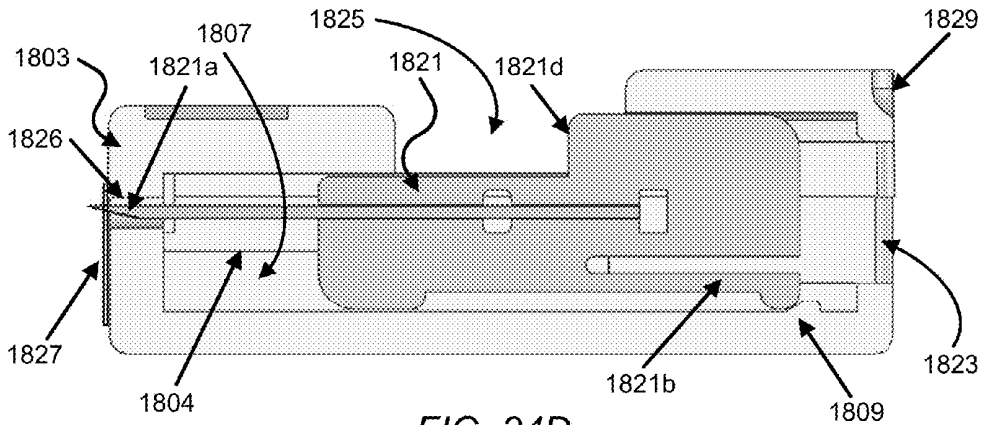


FIG. 24C



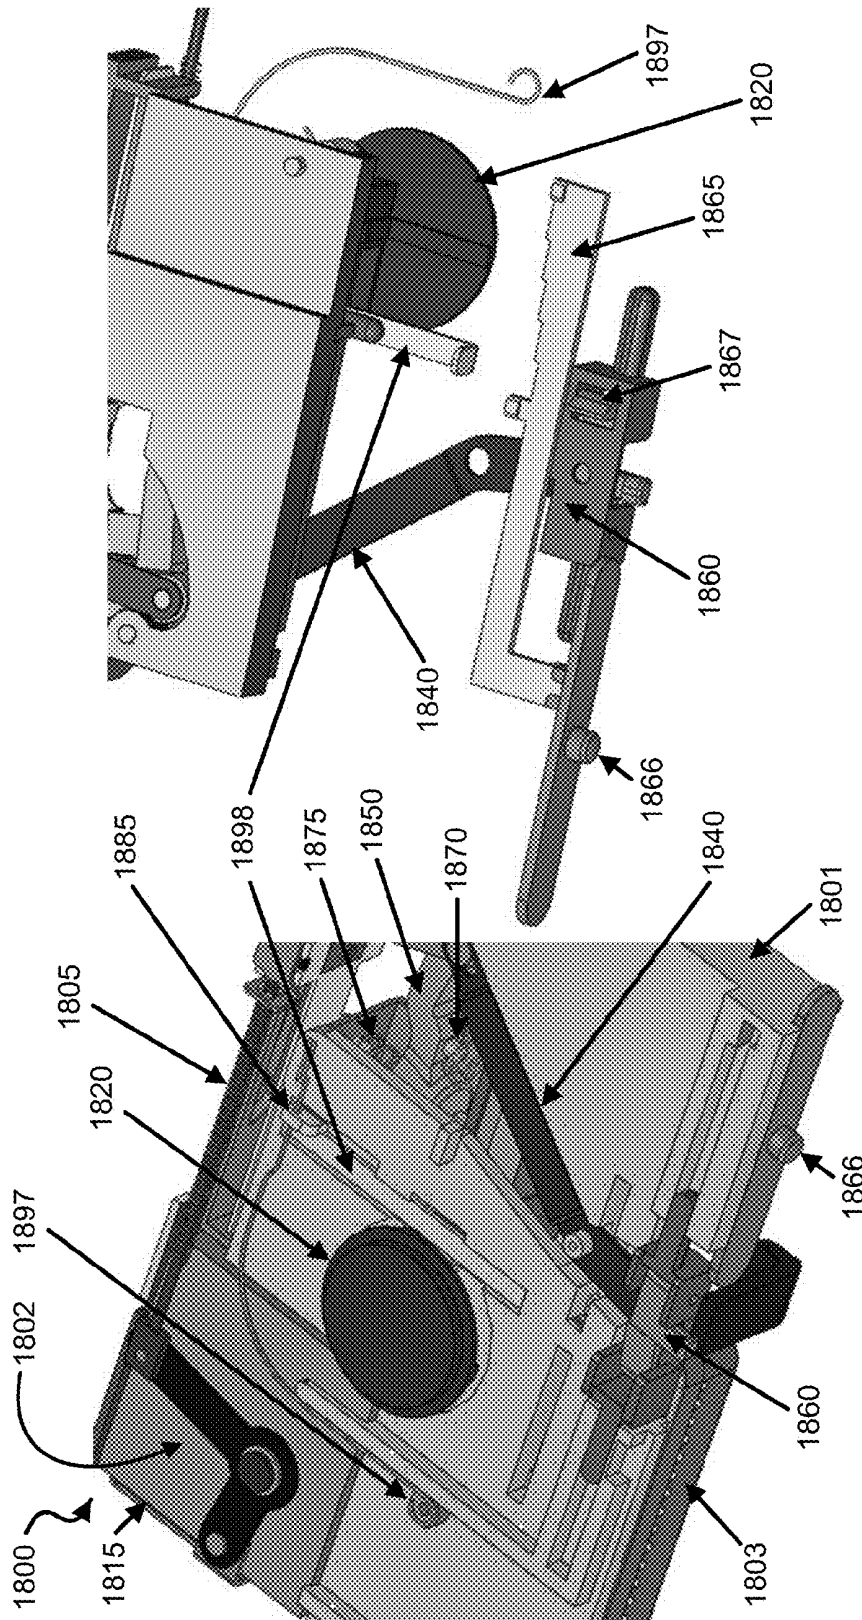


FIG. 25

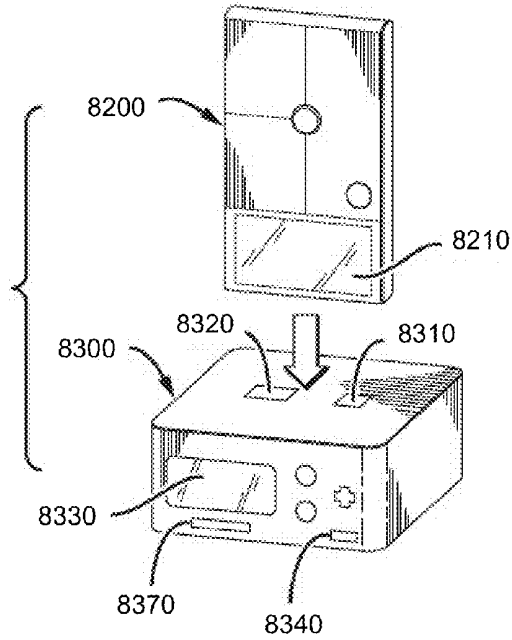


FIG. 26a

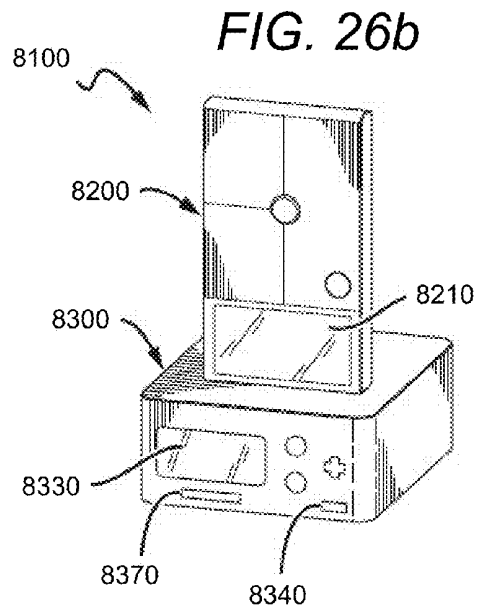


FIG. 26b

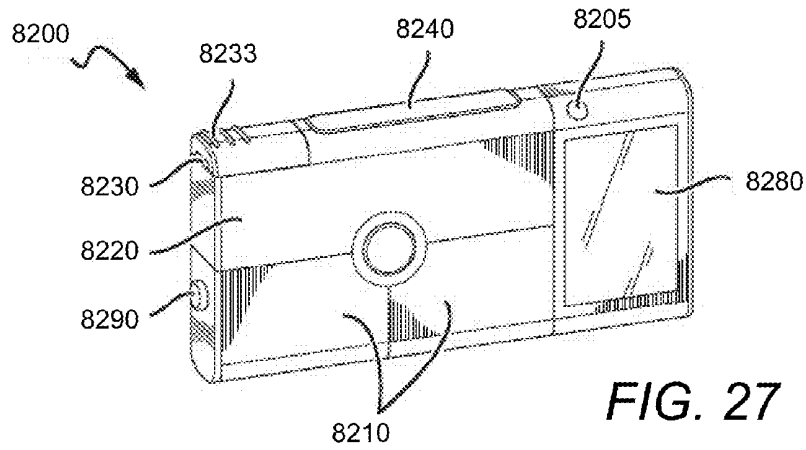


FIG. 27

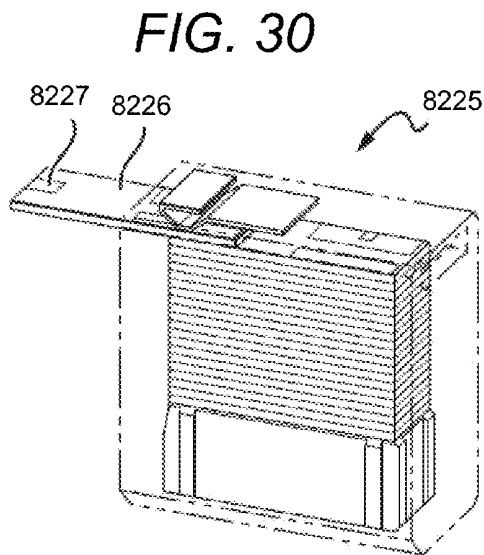
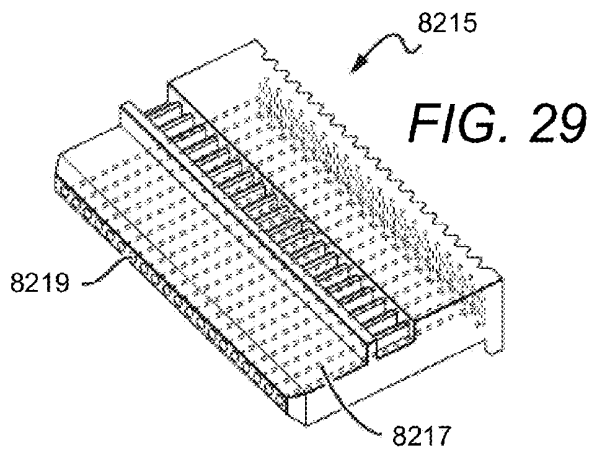
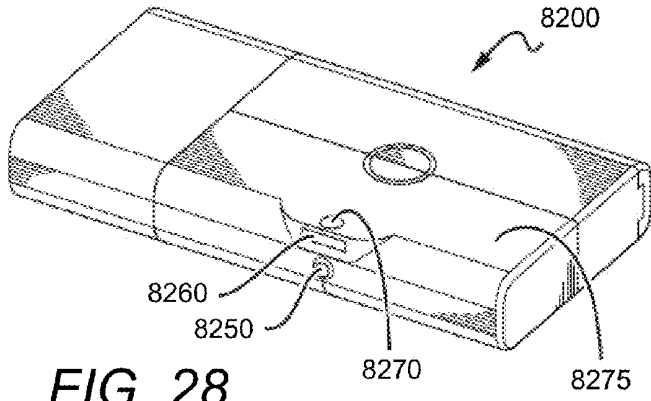


FIG. 31

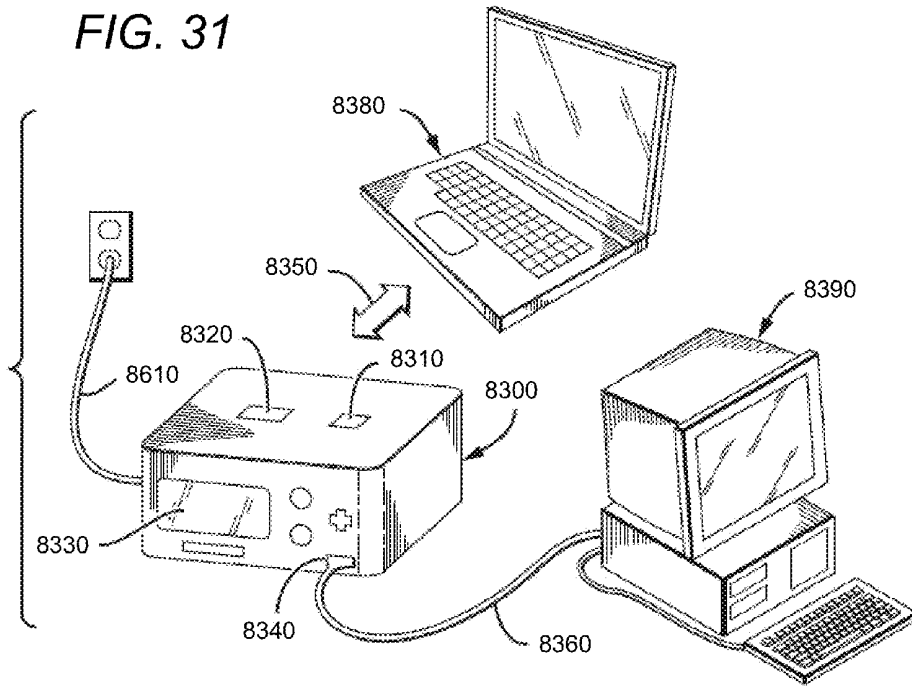
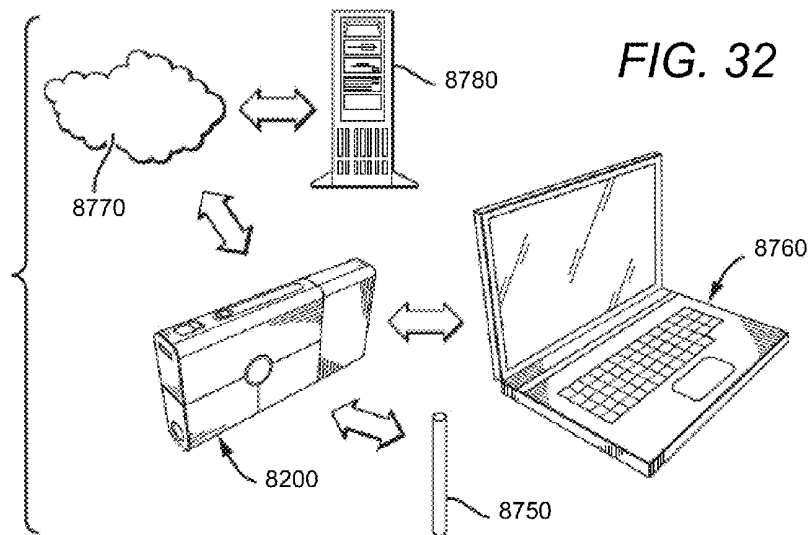


FIG. 32



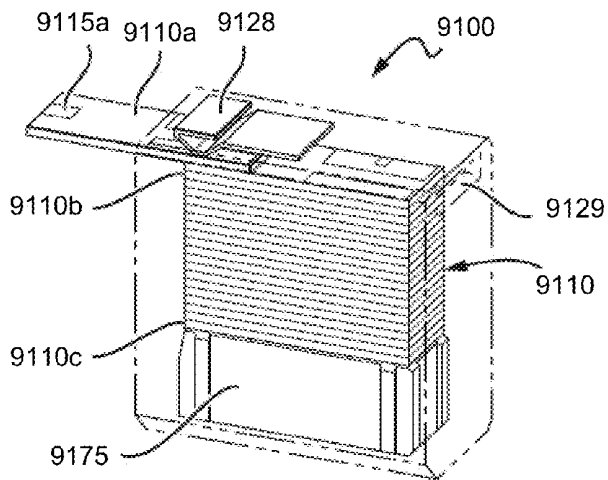


FIG. 33

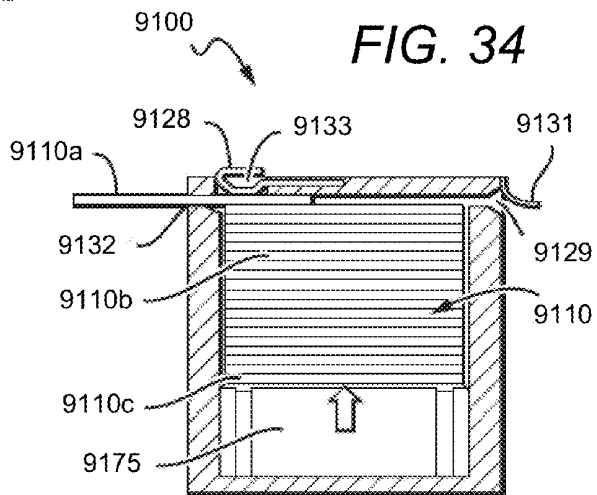


FIG. 34




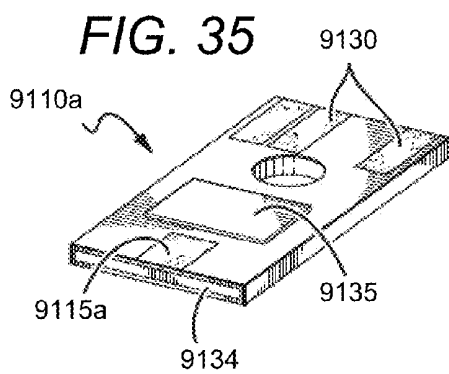


FIG. 35

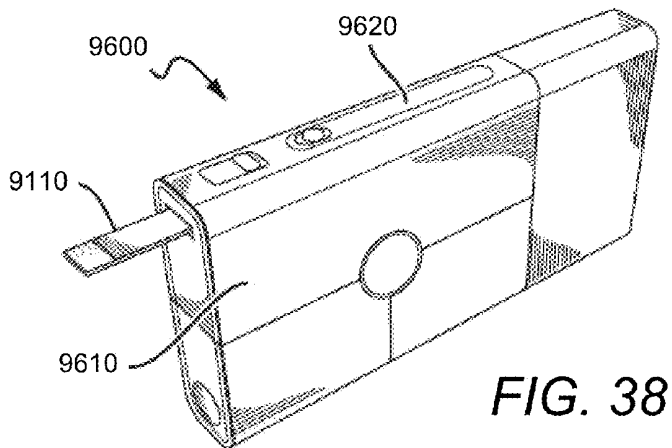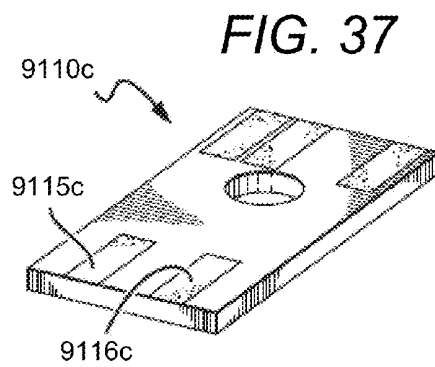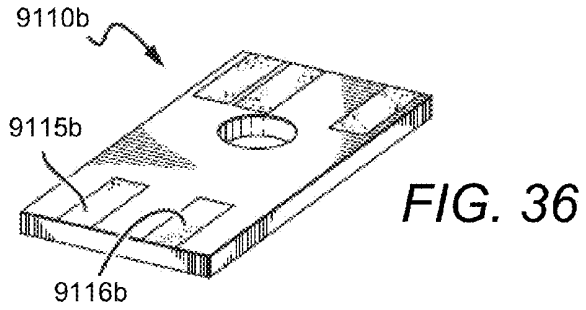

## ANALYTE TESTING DEVICES

### PRIORITY CLAIM AND RELATED PATENT APPLICATIONS

**[0001]** This application is a continuation of, under 35 U.S.C. §120, U.S. patent application Ser. No. 13/689,618 entitled “ANALYTE TESTING DEVICES” and filed on Nov. 29, 2012, which is a continuation-in-part of U.S. patent application Ser. No. 13/188,399 entitled “COCKING AND ADVANCING MECHANISM FOR ANALYTE TESTING DEVICE” and filed on Jul. 21, 2011, now abandoned, which in turn is a continuation-in-part application of U.S. patent application Ser. No. 13/187,360 filed on Jul. 20, 2011 and U.S. patent application Ser. No. 13/187,397 filed on Jul. 20, 2011, now U.S. Pat. No. 8,333,716, which in turn are continuation-in-part applications of U.S. patent application Ser. No. 13/165,621 filed on Jun. 21, 2011, now abandoned. The entire contents of the before-mentioned patent applications are incorporated by reference as part of the disclosure of this application.

### TECHNICAL FIELD

**[0002]** This patent document relates to analyte testing devices and related techniques.

### BACKGROUND

**[0003]** Analyte testing devices play a critical roll in modern diagnosis and management of health-related issues. For example, a sample of human blood, urine, and/or saliva can be tested for glucose, fructosamine, hematocrit, hemoglobin blood oxygen saturation, lactates, iron, pH, cholesterol, liver enzymes (AST, ALT, alkaline phosphatase/GGT, LDH, bilirubin, etc), hormones, and other compounds.

**[0004]** For many diabetic patients, monitoring glucose levels and administering appropriate insulin dosages is a daily activity that requires a significant amount of time and mental energy. Current glucose meters and lancing devices often involve multiple devices, components, and supplies, and require numerous steps to monitor glucose levels. For example, conventional glucose monitoring systems may require numerous steps involving reading a test strip, readying a lancet, using the lancet, putting blood on the test strip and inserting the strip into the glucose meter, reading data from a meter, recording the data in a journal and remembering to bring the journal to the next doctor visit, and then putting away the strip and lancet packages, disposing of loose components, and storing the glucose meter. Thus, there is a need to reduce steps and simplify devices and supplies for monitoring analytes. Other needs include a compact analyte testing device and hands-free disposal of test strips.

**[0005]** Several known prior art references are directed at simplifying the devices and processes for monitoring analytes. Significantly, however, the prior art systems each appear to address only a subset of the convenience issues. U.S. Pat. No. 6,472,220 to Simons, for example, discloses an integrated lancing device and glucose meter. The device holds a cassette that stores a plurality of lancets and test strips. Each lancet is paired with a test strip into a single integrated unit, thus simplifying the number of separate supply components. Unfortunately, the test strip-lancet unit contemplated in Simons prevents the user from using lancets independently of the test strips.

**[0006]** Simons, and all other extrinsic materials discussed herein, are incorporated by reference in their entirety. Where a definition or use of a term in an incorporated reference is inconsistent or contrary to the definition of that term provided herein, the definition of that term provided herein applies and the definition of that term in the reference does not apply.

**[0007]** U.S. Pat. No. 7,192,405 to DeNuzzio also provides an integrated lancet-test strip unit, similar to Simons. DeNuzzio suffers from the same drawbacks as Simons.

**[0008]** U.S. Pat. No. 7,582,063 to Wurster discloses a glucose meter that includes a plurality of analyte sensors and a plurality of lancets on the same carrier. Each time a new blood test is performed, the carrier is rotated into position, which simultaneously exposes an analyte sensor, advances a lancet for use, and cocks a spring to operate the pre-positioned lancet. Since the analyte sensors and lancets are rotated together on the same carrier, exposing of an analyte sensor is not independent of advancing a lancet. That can be a disadvantage to a user who might want to use more than one sensor for a given stick (or for example where two different readings are desired), or might need to use two or more lancets to secure an adequate sample for a single sensor.

**[0009]** Wurster is also designed such that during use, the operative sensor is immediately adjacent (indeed surrounds) the operative lancet tip. That design could be viewed as being inherently problematic because the sensor will tend to sense components in the first amount of blood that is drawn. To avoid that problem it would be more desirable to expose the analyte sensor at a position at least several millimeters away from where the lancet is projected from the housing.

**[0010]** U.S. Pat. No. 4,794,926 to Munsch discloses a lancing device that holds a cartridge with a plurality of lancets. Rotating the cartridge in the lancing device simultaneously loads the next lancet into position for ejection while “cocking” the lancet for ejection. However, Munsch fails to integrate the lancing device with a glucose meter, and also fails to partially expose a test strip when the lancet cartridge is rotated.

**[0011]** U.S. Pat. Nos. 7,922,971, 6,997,343, 7,211,096, and 6,616,616 are other examples of known references that attempt to simplify methods and devices for monitoring glucose levels.

**[0012]** The POGO™ System by Intuity Medical, Inc. (see <http://www.presspogo.com/pogo/system/>) is a commercially available glucose and lancing device that is designed to simplify glucose monitoring. While the POGO™ System reduces the steps and components required, and is an improvement over many other systems, the POGO system fails to provide a separate lancet cartridge and test strip cartridge. As such, the user cannot use lancets independently of test strips.

**[0013]** It has yet to be appreciated that an analyte testing device can house a plurality of analyte sensors and a plurality of lancets, where a single operation of an actuator can expose an analyte sensor while advancing a lancet for projection for use, where the sensors are exposed at a distance of at least several millimeters from where the lancets are projected, and/or where the sensors and lancets can be operated independently from each other.

### SUMMARY

**[0014]** The subject matter includes devices, systems, techniques and methods in which an analyte testing device can house a plurality of analyte sensors and a plurality of lancets,

where a single operation of an actuator can eject an analyte sensor while advancing a lancet for projection for use.

**[0015]** In some aspects of disclosed embodiments, the analyte sensor is included in an analyte sensor cartridge. The cartridge preferably holds a plurality of analyte sensors. In other aspects of disclosed embodiments, each analyte sensor is disposed in a test unit (e.g., a test strip).

**[0016]** In yet other aspects of some disclosed embodiments, the lancet is included in a lancet cartridge. The lancet cartridge preferably holds a plurality of lancets.

**[0017]** In other aspects of disclosed embodiments, the actuator comprises a manually operated lever. In some embodiments, the mechanism is entirely manually operated. In other embodiments, the mechanism is operated at least in part by a motor.

**[0018]** In some aspects of disclosed embodiments, the mechanism includes a hammer, and the actuator operates to cock the hammer. For example, the hammer can be spring loaded and then released to eject a lancet for drawing a blood sample.

**[0019]** In yet other aspects of disclosed embodiments, the mechanism has a linkage that exposes the analyte sensor, advances the lancet for use, and cocks the hammer, all in a single motion of the actuator. In some embodiments, the single motion comprises pulling a lever. In some embodiments the mechanism includes a first link that exposes the analyte sensor, and a second link, different from the first link, that advances the advancing the lancet. Exposing of the analyte sensor is preferably done independently relative to advancing the lancet. For example, the mechanism can include a disengagement control that is capable of disengaging the actuator from either exposing the analyze sensor or advancing the lancet.

**[0020]** In some aspects of disclosed embodiments, the sensors are ejected at a distance of at least several millimeters from where the lancets are projected. In other aspects, the sensors and lancets can be operated independently from each other. For example, the sensors and lancets are each stored in a separate cartridge and the cartridges couple with the analyte testing device independently of one another.

**[0021]** Various features, aspects, and advantages of the inventive subject matter will become more apparent from the following detailed description of various embodiments, the accompanying drawing figures and claims.

#### BRIEF DESCRIPTION OF THE DRAWING

**[0022]** FIG. 1 is a top perspective view of one embodiment of an analyte testing device.

**[0023]** FIG. 2 is the device of FIG. 1, wherein an analyte sensor of a test unit has been exposed.

**[0024]** FIG. 3 is a bottom perspective view of the device of FIG. 1.

**[0025]** FIG. 4 is a back perspective view the device of FIG. 1.

**[0026]** FIG. 5 is a perspective views of one embodiment of a lancet cartridge.

**[0027]** FIG. 6 is a side view of the lancet cartridge of FIG. 5.

**[0028]** FIG. 7 is a side view of the lancet cartridge of FIG. 5.

**[0029]** FIG. 8 is a perspective view of one embodiment of an analyte sensor cartridge.

**[0030]** FIG. 9 is a side view of the analyte sensor cartridge of FIG. 8.

**[0031]** FIG. 10 is a perspective view of one embodiment of a test unit that has an analyte sensor.

**[0032]** FIG. 11 shows one embodiment of a linkage mechanism of the device of FIG. 1 engaged with the lancet cartridge of FIG. 5. The linkage mechanism is shown at four different stages of use: (i) rest position; (ii) lever pulled; (iii) lever released (cocked and ready); and (iv) button pressed to project hammer.

**[0033]** FIG. 12 is a side view of the device of FIG. 1, showing the inner components of the device in a rest position.

**[0034]** FIG. 13 is a side view of the device of FIG. 1, showing the inner components of the device as a lever is being pulled.

**[0035]** FIG. 14 is a side view of the device of FIG. 1, showing the inner compartments of the device after a lever has been pulled and a hammer has been spring-loaded.

**[0036]** FIG. 15 is a side view of an analyte device with a motor.

**[0037]** FIG. 16 is a side of an analyte device with a first and second disengagement control.

**[0038]** FIG. 17a is a schematic of one embodiment of a method of using the device of FIG. 1.

**[0039]** FIG. 17b is a perspective view of one embodiment of an analyte testing device having an LCD touch-screen display.

**[0040]** FIG. 17c is perspective view of the device of FIG. 1 transmitting wireless communications to a laptop.

**[0041]** FIG. 17d is a perspective view of one embodiment of a docking station coupled with the device of FIG. 1.

**[0042]** FIGS. 17e and 17f show one embodiment of an analyte testing device with a no-contact test strip ejecting mechanism.

**[0043]** FIGS. 17g and 17h show perspective views of one embodiment of an analyte testing device with a wheel for adjusting lancet puncture depth and window for displaying depth setting.

**[0044]** FIGS. 18A-18E show schematics of one embodiment of an exemplary actuator mechanism of an analyte testing device.

**[0045]** FIGS. 19A and 19B show schematics illustrating an operation of the exemplary actuator mechanism of the analyte testing device.

**[0046]** FIGS. 20A-20C show schematics illustrating another operation of the exemplary actuator mechanism of the analyte testing device.

**[0047]** FIGS. 21A and 21B show schematics of exemplary sliding button components of the actuator mechanism of the analyte testing device.

**[0048]** FIGS. 22A-22C show schematics of an exemplary lancet cartridge of the analyte testing device.

**[0049]** FIG. 23A shows a schematic of an exemplary lancet.

**[0050]** FIGS. 23B and 23C show schematics of the exemplary lancet in the lancet cartridge.

**[0051]** FIGS. 24A-24E show schematics illustrating a firing operation of the exemplary lancet of the actuator mechanism.

**[0052]** FIG. 25 shows schematics of components of the exemplary actuator mechanism of the analyte testing device.

**[0053]** FIGS. 26a and 26b are perspective views of one embodiment of an analyte testing system.

**[0054]** FIG. 27 is a perspective view of one embodiment of a handheld analyte testing device.

**[0055]** FIG. 28 is a perspective view of a back side of the handheld analyte testing device of FIG. 27.

[0056] FIG. 29 is a perspective view of a lancet cartridge.

[0057] FIG. 30 is a perspective view of an analyte sensor cartridge.

[0058] FIG. 31 is a perspective view of a docking station communicatively coupled with two external devices.

[0059] FIG. 32 is a perspective view of a handheld analyte testing device communicatively coupled with two external devices.

[0060] FIG. 33 is a perspective view of one embodiment of a test unit cartridge for housing a plurality of test units.

[0061] FIG. 34 is a side view of the test unit cartridge of FIG. 33.

[0062] FIG. 35 is a perspective view of one embodiment of a test unit.

[0063] FIG. 36 is a perspective view of another embodiment of a test unit.

[0064] FIG. 37 is a perspective view of a calibration test unit.

[0065] FIG. 38 is a perspective view of one embodiment of an analyte testing device.

#### DETAILED DESCRIPTION

[0066] The following discussion provides example embodiments of the inventive subject matter. Although each embodiment represents a single combination of inventive elements, the inventive subject matter is considered to include all possible combinations of the disclosed elements. Thus if one embodiment comprises elements A, B, and C, and a second embodiment comprises elements B and D, then the inventive subject matter is also considered to include other remaining combinations of A, B, C, or D, even if not explicitly disclosed.

[0067] FIG. 1 shows an analyte testing device 100. The housing 105 of device 100 has a first compartment 110 and a second compartment 120, for storing a lancet cartridge 115 (see FIGS. 5-7) and an analyte sensor cartridge 125 (see FIGS. 8-9), respectively. The analyte sensor cartridge 125 contains test units 127 each having an analyte sensor 126 for contacting and sensing a particular analyte such as blood. Device 100 includes an exterior facet outside the second compartment 120 to have a slot 133 for receiving from, and for ejecting a test unit 127 out of, the analyte sensor cartridge 125, when device 100 is operated to perform a test. The first compartment 110 includes an exterior facet that is configured to include an opening or hole 113 for rejecting a lancet that allows a precise cut into a user for generating a small amount of bleeding for a blood test. The lancet cartridge 115 contained inside the first compartment 110 is designed to store a plurality of lancets 117 (see FIGS. 5 and 6) to allow a lancet 117 to be protruded at the hole 113 (see FIG. 3) during a test. Hole 113 and slot 133 are separated by a substantial distance (more than 5 mm), thus allowing a user to bleed out an initial amount of blood before applying a blood sample to an analyte sensor. In the illustrated example, hole 113 and slot 133 are on two different facets of device 100. Device 100 also has an electronics compartment 130 for housing conversion electronics 137 (see FIG. 12). Conversion electronics 137 are communicatively coupled to an analyte sensor 126 (see FIGS. 8 and 10) within cartridge 125. Conversion electronics 137 is configured to convert a signal from analyte sensor 126 into readable data (e.g., glucose levels).

[0068] The operation of device 100 will become more apparent from the following descriptions, including those with respect to FIGS. 11-14.

[0069] Device 100 has an actuator 140 comprising a lever. Actuator 140 can be cocked by operating the lever to be in an actuated state to (i) ready a lancing device (e.g., cock a hammer, see FIGS. 11 and 14), (ii) expose an analyte sensor or test unit 127 (see FIGS. 2 and 14), and (iii) advance a lancet cartridge 115 for actuating a lancet 117 for taking a test (see FIGS. 11 and 13). Device 100 also has a test unit ejector 160, which advantageously allows for hands-free disposal of a used test strip 127 after each test.

[0070] The housing of device 100 can be made of plastic, metal, composite, or any other material with structural and mechanical properties suitable for housing a lancet cartridge, test strip cartridge, electronics, and a linkage mechanism. Device 100 can be designed to be compact for easy storage and for convenient portability. For example, device 100 can be configured to have a height no more than 50 mm, a width no more than 17 mm, and a length no more than 100 mm in some implementations while in more compact form for other implementations with the height being no more than 40 mm, a width being no more than 12 mm, and a length being no more than 75 mm. In some disclosed embodiments, the housing of device 100 comprises an outer protective shell made of a suitable shell material to protect the device components from elements or conditions in the surroundings. For example, the outer protective shell may be made of molded plastic and may include an inner desiccant liner to minimize exposure to moisture.

[0071] Unless the context dictates the contrary, all ranges set forth herein should be interpreted as being inclusive of their endpoints, and open-ended ranges should be interpreted to include commercially practical values. Similarly, all lists of values should be considered as inclusive of intermediate values unless the context indicates the contrary.

[0072] Conversion electronics 137 preferably includes a facility for transmitting data and information out of the housing and to an external storage device (e.g., docking station, laptop, smart phone). It is contemplated that the data can be transmitted using a wireless protocol, and can even transmit data using two or more wireless protocols. Wired protocols and methods are also contemplated.

[0073] It is also contemplated that conversion electronics 137 can include a processor programmed to correlate individual instances of data and information derived from the data with time stamps. The processor can also be programmed to correlate individual instances of data with user-entered information such as voice recordings or text. In addition, the processor can be programmed to make an evaluation of the data and information, and send a notification to different recipients as a function of the evaluation. Yet still, the processor can be programmed to keep track of inventory of lancets and test strips, both within and outside the device, and re-order supplies as needed.

[0074] In other aspects of preferred embodiments, conversion electronics 137 includes a processor programmed to store voice recordings of diary information selected from the group consisting of supplies used or ordered, food eaten, exercise, medication taken, and estimated calories burned. The processor is also preferably programmed to prompt a user to use the device according to a pre-selected time and/or pre-selected time interval. Alternatively, electronics 137 can be equipped with an accelerometer or pedometer for measuring and calculating distance traveled and calories burned.

[0075] Conversion electronics 137 can also include a pedometer and/or accelerometer for calculating a distance

traveled and calories burned. In such embodiments, electronics 137 preferably includes a processor for time-stamping the distances traveled and calories burned, and correlating this data with analyte test data.

[0076] FIG. 2 shows device 100 after actuator 140 has been cocked. The cocking of actuator 140 has caused a test unit 127 to be partially ejected from slot 133, thus exposing analyte sensor 126 (see FIGS. 8 and 10). Once actuator 140 has been cocked, a lancing device within device 100 can be projected by pressing button 150, causing one of a plurality of lancets 117 (see FIGS. 5 and 6) to exit from hole 113 (see FIG. 3).

[0077] FIG. 4 shows a back perspective view of device 100. A door on the backside of device 100 has been opened to reveal compartment 110. A lancet cartridge 115 is disposed within compartment 110. Device 100 has a spring-loaded return slider 690, which is configured to retract a lancet back into cartridge 115 after the lancet has been partially ejected for drawing a blood sample.

[0078] FIGS. 5-7 show different views of a lancet cartridge 115. Cartridge 115 holds a plurality of lancets 117. A slot 116 is disposed on a side of cartridge 115, so that a hammer 186 (see FIGS. 11-14) of a lancing device within device 100 can contact one of the plurality of lancets 117, thus causing the lancet to partially exit cartridge 115 via slot 118. The lancet is retracted by return slider 690 of device 100 (see FIG. 4). Cartridge 115 also has a molded bump 138 that provides friction to the plurality of lancets 117 and helps to maintain each lancet stationary when not being fired.

[0079] Cartridge 115 can include any appropriate number of lancets, preferably between 15 and 25 lancets, more preferably between 18 and 22 lancets, and most preferably 20 lancets. The lancets are preferably sterilized and sealed prior to use.

[0080] FIGS. 8 and 9 show different views of an analyte sensor cartridge 125. Cartridge 125 holds a plurality of test units 127 (e.g., test strips). Cartridge 125 has electrical contacts 128 for communicatively coupling the analyte sensors to the conversion electronics 137. Alternatively, contacts 128 could be eliminated and electronics 137 could directly interface with contacts 129 of test unit 127 (see FIG. 10) via an open aperture in cartridge 125. Cartridge 125 also has a slot 129a that couples with a test unit lateral ejection mechanism of device 100. When actuator 140 is cocked, the advance mechanism enters slot 129a and pushes a portion of test unit 127a out of slot 129b, thus exposing analyte sensor 126 for use.

[0081] Cartridge 125 can include any appropriate number of test strips, preferably between 15 and 25 test strips, more preferably between 18 and 22 test strips, and most preferably 20 test strips.

[0082] Cartridge 125 preferably includes test strips configured to test for different analytes. For example, some test strips may test for glucose while other test strips test for fructosamine. Furthermore, cartridge 125 can have at least one test strip capable of testing for two analytes simultaneously, either by including two analyte-binding chemicals/reactants within one absorbing material or by including two different analyte sensors on one test strip. In addition, cartridge 125 preferably includes at least one calibration test strip for verifying the calibration of conversion electronics 137. In one embodiment, the calibration test strip is an analyte sensor that has a known amount of glucose.

[0083] Cartridge 125 also has a spring-load base 131 configured to push the plurality of test strips 127 upward, thus repositioning a new test strip into place after test strip 127a is removed from cartridge 125.

[0084] FIG. 10 shows a test unit 127a having an analyte sensor 126. Analyte sensors are well known and generally comprise an absorbent material with an analyte-binding reactant. While test unit 127a is configured as a test "strip", those of skill in the art will appreciate that other shapes and configurations (e.g., capsules, disks) can be used consistently with the inventive subject matter. Analyte sensor 126 is configured to generate a signal that is sent to electrical contacts 129. Electrical contacts 129 are communicatively coupled with electrical contacts 128 of cartridge 125 and allows the signal generated by analyte sensor 126 to reach the conversion electronics 137 for analysis. Alternatively, electrical contacts 129 could directly interface with conversion electronics 137 via an open aperture on cartridge 125.

[0085] FIG. 11 shows a linkage mechanism 180 of device 100 coupled with lancet cartridge 115. FIG. 11 provides a summary of the four progressive stages for using linkage 180 and lancet cartridge 115 as a lancing device: (i) initial resting position; (ii) cocking of actuator 140; (iii) cocked and ready position; and (iv) releasing and projecting a lancet. At the final stage, a finger or other body part can be placed over hole 113 in order to prick the body part and draw a blood sample. These four stages will now be explained in more detail.

[0086] FIG. 12 is a side view of device 100 showing various internal components of device 100, such as: electronics 137, linkage mechanism 180, cartridge 115, and cartridge 125. FIG. 12 shows device 100 at a resting position (i.e., before actuator 140 has been cocked). Hammer 186 is in an uncocked position.

[0087] FIG. 13 shows the internal components of device 100 as actuator 140 is being cocked. The cocking of actuator 140 has caused link 182 to raise up and compress spring 181. At the same time, hammer 186 has been raised via link 183. In addition, the left end of link 182 has been raised over the top of link 187 such that link 182 is maintained in an inclined position and spring 181 is maintained in a compressed position (i.e., hammer 186 has been "cocked" or "readied"). At the same time, link 183 is driven to the left, pushing test strip 127a out of slot 133 (see FIG. 1). In addition, link 184 has been advanced to the left, causing cartridge 115 to advance left and into position. In disclosed embodiments, link 183 couples with cartridge 115 such that when cartridge 115 has been completely advanced to the left, link 183 allows the last lancet of cartridge 115 to remain in a usable (i.e., projectable) position. For example, link 183 could release (e.g., de-couple) from cartridge 115 during subsequent cocking of actuator 140. In this manner, linkage mechanism 180 allows a lancet to be available for use, even after cartridge 115 has been advanced through each of the plurality of lancets 117.

[0088] In this manner, actuator 140 and linkage mechanism 180 are configured to (i) cock a lancing device (e.g., lift hammer 186, link 182, and spring 181) (ii) partially expose an analyte sensor on a test unit; and (iii) advance a lancet cartridge into position, all in a single motion (e.g., pulling up actuator 140). It is also contemplated that an analyte testing device could have a linkage mechanism that is configured to accomplish the three steps above using two or more motions (e.g., pulling a lever, then pushing a lever).

[0089] FIG. 14 shows the position of linkage 180 after actuator 140 has been cocked. Once actuator 140 has been

cocked, button **150** can be pressed to release link **187** from under link **182**, thus causing spring **181** to push link **182** and hammer **186** downward to project a lancet from cartridge **115**.

[0090] One of skill in the art will appreciate that configurations of linkage mechanism **180** other than that shown in the drawings can be used consistently with the inventive subject matter taught herein. In some alternative embodiments, linkage mechanism **180** is controlled and/or actuated by electrical drivers rather than pure mechanical means. For example, pulling actuator **140** could send an electrical signal to conversion electronics **137**, which then operates a motor, or multiple motors, in order to perform any combination of: (i) cocking a lancing device, (ii) partially exposing a test strip for use, and (iii) advancing a lancet cartridge into position. In yet other embodiments, the lancing system is designed such that a cocking step is not required.

[0091] FIG. **15** shows an analyte testing device **500** that has an actuator **540** and a motor **550**. Actuator **540** comprises a button that sends a signal to motor **550**. Motor **550** operates to drive linkage mechanism **180** upon receiving a signal. Motor **550** and actuator **540** is one embodiment of an analyte testing device that is not purely mechanical.

[0092] FIG. **16** shows an analyte testing device **600** that has a first disengagement control **610** and a second disengagement control **620**. Control **610** operates to disengage link **182** from link **183**, thus disengaging cartridge **125** from linkage mechanism **180**. Control **620** operates to disengage link **184** from cartridge **115**. In this manner, cartridges **115** and **125** can be disengaged from linkage mechanism **180**, and thus can be used independently of one another.

[0093] FIG. **17a** shows a method of using device **100**, comprising: inserting a lancet cartridge into the device; inserting a test strip cartridge into the device; operating an actuator on the device, which operates a mechanism that (i) readies a lancing device, (ii) advances the lancet cartridge, and (iii) exposes an analyte sensor of a test unit; deploying the lancing device in order to prick a body part and draw a blood sample; and exposing the analyte sensor to the blood sample. The method of FIG. **15** can optionally include the steps of: reading an output of the device; ejecting and disposing of the test unit; replacing the lancet cartridge with a refill lancet cartridge; and replacing the analyte sensor cartridge with a refill analyte sensor cartridge.

[0094] The first two and last two steps are displayed in round boxes and with dotted lines to indicate that these steps need not be repeated at every cycle of usage of the device. For example, in embodiments having twenty lancets and test strips per cartridge, the steps of inserting/removing cartridges need only be performed every twentieth cycle of use.

[0095] FIG. **17b** shows an analyte testing device **200** having an LCD touch screen display **210**. Display **210** can be used to display test results, supplies used/remaining, calories burned, time/date, history of drugs administered, journal entries, or any other number of data useful for monitoring analytes. Display **210** can also be used to type and input data into device **100**.

[0096] Device **200** also has a first work light **220** positioned to illuminate a test strip that has been partially pushed out from device **200**, and a second work light **230** positioned to illuminate a lancet hole **213**. First and second work lights **220** and **230** are useful for using device **200** in poor lighting conditions.

[0097] Conversion electronics within device **200** additionally includes a Personal Emergency Response System

(PERS), including a PERS button **240**. Button **240** is configured to (i) contact a third party, (ii) identify the user of device **200**, and (iii) provide a user's health data to the third-party. Examples of third parties can include spouse, relative, friend, home nurse, doctor, health care worker, ambulance operator, police operator, or any other person that can provide health care assistance. The Personal Emergency Response System is also preferably configured to automatically contact a third party as a function of the user's health data. For example, when the user is a diabetic patient, PERS can be configured to contact a third party when the user's glucose test results are below a predetermined threshold. PERS can also be configured to notify the third party of an urgency level (e.g., low, moderate, high, critical, etc), and can determine who to contact based on the urgency level.

[0098] FIG. **17c** shows device **100** communicatively coupled to a laptop **310** via a wireless connection **320**. Numerous wireless protocols can be used, for example Bluetooth, WiFi, 802.11, cellular, or any other protocol suitable for wireless communication. Connection **320** can be used to back up data, transmit data to a health care provider's server via the internet, reorder supplies, receive notifications from a doctor, or receive data analysis reports from an analytics software running on the laptop. It is also contemplated that connection **320** can be a wired connection. Furthermore, it is contemplated that device **100** can connect to devices other than laptop **310**, for example a home computer, a smart phone, a server, or any other computing device suitable for storing, analyzing, and/or exchanging data.

[0099] FIG. **17d** shows device **100** coupled with a docking station **400**. Docking station **400** is configured to provide power and data connectivity to device **100**. For example, station **400** can be configured to charge a re-chargeable battery within device **100**. Station **400** can also be configured to back up data on device **100** and transmit data to another device, such as a home computer or a medical provider server. Docking station **400** also has a visual interface **410**, through which a user can view and/or input data.

[0100] FIG. **17e** shows an analyte testing device **520**, with a test strip **127a** and a test strip ejector **560**. FIG. **17f** is a side view cut-out of device **520**, showing how ejector **560** operates to completely eject test strip **127a** for disposal after usage. Ejector **560** advantageously obviates the need for direct hand contact with a used test strip. Ejector **560** has a plunger **561** configured to engage an aperture **529** of test strip **127a**, thus preventing test strip **127a** from being accidentally re-inserted back into cartridge **525** when a user applies finger pressure to the test strip **127** for blood application.

[0101] FIGS. **17g** and **17h** show an alternate analyte testing device **671**. Unlike device **100**, device **671** has a wheel **670** for adjusting a lancet penetration depth. A lancet within lancet cartridge **715** exits device **671** via hole **613** according to an adjustable depth determined by the setting of wheel **670**. Device **671** also has a window **675** for indicating the current lancet penetration depth setting. Spring-loaded return slider **690** is configured to retract the lancet back into cartridge **715**.

[0102] In another embodiment of the disclosed technology, an analyte testing device can include a plurality of analyte sensors (e.g., housed in an analyte sensor cartridge) and a plurality of lancets (e.g., housed in a lancet cartridge), in which a one-handed operation of an actuator mechanism can be implemented to ready the device for a test, prick the user to extract blood to be analyzed in the test, and reset the device for another use. For example, the actuator mechanism can be

implemented to ready the device for a test by moving an analyte sensor (e.g., a test strip) forward to expose the sensor and advancing a firing component to a position for projection of a lancet. The actuator mechanism can subsequently be implemented to project (or fire) the lancet to prick a user to draw blood for analysis in the test. The actuator mechanism can be implemented to reset the device by ejecting the test strip and returning the components of the actuator mechanism to an initial position.

[0103] FIGS. 18A and 18B show an example of an analyte testing device 1800 that includes one exemplary implementation of the above actuator mechanism. FIG. 18A shows a three dimensional cross sectional view of the components that make up the actuator mechanism. FIG. 18B shows a two dimensional cross sectional view of the components that make up the actuator mechanism. It is noted that some components included in the analyte testing device 1800 may not necessarily be shown in the schematic of FIGS. 18A and 18B.

[0104] As shown in FIGS. 18A and 18B, the actuator mechanism is encased in a containment structure 1801, also referred to as a chassis or an internal housing structure. The containment structure 1801 can be encased within an external housing or device casing. The containment structure 1801 can be used to provide positioning and/or structural support to various modules and components contained within the chassis of the analyte testing device 1800. The device 1800 includes an analyte sensor cartridge 1802 and a lancet cartridge 1803, in which the analyte sensor cartridge 1802 and the lancet cartridge 1803 are contained within separate cavities located within the chassis 1801. The schematics of FIGS. 18A and 18B, as well as other subsequent figures, show the cavities of the chassis 1801 where the analyte sensor cartridge 1802 and the lancet cartridge 1803 are located.

[0105] The actuator mechanism includes a sliding button that includes a cocking button 1830 and an eject button 1835 that move translationally along a sliding track 1839 formed on the top facet of the device 1800. For example, implementing the sliding button results in (1) moving a new test strip from a position within the analyte sensor cartridge 1802 to a position that exposes a portion of the test strip (e.g., such as the site on the test strip to receive the testing sample) outside of the containment structure 1801 and (2) advancing a firing component to a readied position for projection of a lancet from the lancet cartridge 1803 (e.g., a firing position). Also, for example, implementing the sliding button can result in (3) advancing the lancet cartridge 1803 within the analyte testing device 1800 to a position in which the lancet is positioned in a firing path of the firing component for projection. The sliding button can be implemented by pushing the cocking button 1830 from an initial position forward to a cocked position in a sliding motion along the track 1839, as shown later in FIGS. 19A and 19B. In the described embodiment, sliding the cocking button 1830 forward includes sliding the eject button 1835 forward to the cocked position as well, e.g., as the forward motion of the cocking button 1830 pushes forward the eject button 1835. The cocking button 1830 includes a button pad where a user can make contact to engage the sliding button, e.g., to ready the device. The cocking button 1830 includes a sliding base component 1832 that facilitates the sliding of the cocking button 1830 on the sliding track 1839 and links the cocking button 1830 to other components of the actuator mechanism. The eject button 1835 includes an eject button pad where a user can make contact to engage the eject button 1835 of the sliding button,

e.g., to eject a used test strip from the device. The eject button 1835 includes an eject base component 1837 that facilitates the sliding of the eject button 1835 on the sliding track 1839 and links the eject button 1835 to other components of the actuator mechanism. After the sliding button reaches the cocked position, the cocking button 1830 can be brought back to the initial position by a linear spring coupled between the cocking button 1830 and a cocking base component 1806 of the actuator mechanism. For example, this return of the cocking button 1830 from the cocked position to the initial position can thus be implemented automatically, without a user intervention to manually return the cocking button to the initial position. In some examples, sliding the cocking button 1830 forward from the initial position to the cocked position can include producing a clicking sound when the cocking button arrives in the cocked position.

[0106] The actuator mechanism includes, underneath the sliding track 1839, a spring-loaded arm component 1805 that is utilized in the movement of the new test strip from within the analyte sensor cartridge 1802 to expose the test strip outside of the containment structure 1801 of the device 1800 via an opening slot covered by a sliding door 1815 of the actuator mechanism that conceals the slot opening of the analyte sensor cartridge 1802 when a test is not performed for blocking moisture and contaminants from getting into contact with and polluting test strips stored inside the device 1800. A door crank component 1810 is provided to open or close the sliding door 1815 under operation of the actuator mechanism.

[0107] The spring-loaded arm component 1805 is configured between the eject base component 1837 of the sliding button and a door crank component 1810 of the actuator mechanism. The door crank component 1810 is configured between the spring-loaded arm component 1805 and the door 1815 of the actuator mechanism. The spring-loaded arm component 1805 includes a rod shaft that is configured with a spring surrounding the exterior of the rod shaft. The rod shaft is connected to the eject base component 1837 via a push link component 1838. In some examples, the push link component 1838 can be configured as a portion or facet of the eject base component 1837. For example, the end of the rod shaft can rest within an opening of the push link component 1838 such that the external spring is in an initial compression state (e.g., which can be partially compressed or substantially uncompressed) when the sliding button is in the initial position. For example, when the cocking button 1830 of the sliding button (along with the eject button 1835) moves forward along the track 1839 from the initial position to the cocked position, the spring of the spring-loaded arm component 1805 compresses against the push link component 1838 from its the initial compression state to an intermediate compression state, as a portion of the rod shaft of the spring-loaded arm component 1805 passes through the opening of the push link component 1838. Also, for example, when the eject button 1835 of the sliding button moves forward along the track 1839, the spring of the spring-loaded arm component 1805 further compresses against the push link component 1838, as the rod shaft of the spring-loaded arm component 1805 passes further through the opening of the push link component 1838 while the eject button 1835 advances along the remaining travel distance of the sliding track 1839 until it reaches a final position (e.g., eject position). For example, the actuator mechanism can be configured to not set the eject button 1835 at the eject position upon its arrival, in which the spring of the spring-loaded arm component 1805 can uncompress to drive the eject button

**1835** back to the initial position. Thus, the return of the eject button **1835** from the final position to the initial position can be implemented automatically, without a user intervention to manually return the eject button to the initial position.

[0108] The door crank component **1810** is structured in a (substantially) L-shaped form having two arms at a fixed angle (e.g., which can be substantially perpendicular) and meeting at a joint **1811**. The door crank component **1810** is configured between the spring-loaded arm component **1805** and the sliding door **1815** of the actuator mechanism that conceals the slot opening of the analyte sensor cartridge **1802**. The door crank component **1810** is connected to the spring-loaded arm component **1805** at a joint **1812** and connected to the door **1815** at a joint **1813**. The movement of the sliding button from the initial position to the cocked position drives the spring-loaded arm component **1805** forward. The forward motion of the spring-loaded arm component **1805** to the cocked position results in a rotational motion of the door crank component **1810** about the joint **1811**, in which the door crank component **1810** moves the door **1815** from a closed position covering the slot opening of the analyte sensor cartridge **1802** to an opened position, e.g., such that a test strip can advance out of the slot opening to expose the sample-receiving portion of the strip. For example, one arm of the door crank component **1810** is moved forward by the translational advancement (e.g., pushing) of the spring-loaded arm component **1805**, which causes the rotation the door crank component **1810** about the joint **1811**. The rotation results in the other arm of the door crank component **1810** moving the door **1815** in a translational motion (e.g., pulling) to expose the slot opening.

[0109] In the initial position, the door **1815** completely covers the slot opening of the analyte sensor when a test strip is not in use. For example, moisture and other contaminants or particulates can contaminate the stored unused test strips if permitted to enter, e.g., and damage chemical reagents on the test strips, which can cause inaccurate analyte testing results. The door **1815** prevents sunlight, moisture and particulates in the air from entering the analyte sensor cartridge **1802**. The door **1815** also helps to maintain a constant ambient temperature within the analyte sensor cartridge **1802**, e.g., by providing a seal over the slot opening that prevents heat from diffusing in or out of the analyte sensor cartridge **1802**.

[0110] The analyte sensor cartridge **1802** can include, in some implementations, a temperature sensor that is in communication with an electronic processing unit within the device **1800**, e.g., such as the conversion electronics **137** previously described and shown in FIG. 12. The conversion electronics **137** can be configured to continuously monitor temperature data provided by the temperature sensor and provide reports and alarms to a user on a display of the device. In some implementations, the temperature sensor can be configured within the cavity encased by the chassis **1801** of the analyte sensor module configured to hold the analyte sensor cartridge **1802**. For example, the temperature sensor can be configured to continuously or continually sense the ambient temperature in the analyte sensor module, e.g., in which the ambient temperature at a given instance in time or the ambient temperature over a duration of time can be sensed and recorded as data (e.g., by the processing unit). For example, the processing unit can determine if the temperature is within or outside of a suitable range (e.g., high or low) of the analytes. The analyte testing device **1800** can be in wired or wireless communication with a mobile device or a computing

device that includes a web portal featuring a user interface that the user of the device **1800** can use for various functions, including monitoring the status of the device **1800** such as the temperature data in the analyte sensor cartridge **1802**. Some examples for wireless communications of the device **1800** include 3G wireless communication standards, 4G wireless communication standards including, LTE, WiFi, Bluetooth, and other suitable wireless communications via radio frequency waves and other electromagnetic waves.

[0111] The actuator mechanism includes a lancet advance component **1840** that is utilized to ready a lancet for projection from the lancet cartridge **1803** (e.g., advance lancet firing components to a firing position). One end of the lancet advance component **1840** is coupled to the sliding base component **1832** of the cocking button **1830** via a lancet cocking link **1845** of the actuator mechanism. The lancet advance component **1840** is connected to the lancet cocking link **1845** at a joint **1841**. The lancet cocking link **1845** is connected to the sliding base component **1832** at a joint **1842**. The lancet advance component **1840** is also coupled to the cocking base component **1806** via a lancet cocking crank **1847** of the actuator mechanism. The lancet advance component **1840** is connected to the lancet cocking crank **1847** at the joint **1841**. The lancet cocking crank **1847** is connected to the cocking base component **1806** at the joint **1843**. The other end of the lancet advance component **1840** is coupled to a lancet slider component **1860** of the actuator mechanism and can move the lancet slider component **1860** translationally, e.g., via the movement of the cocking button **1830**. The lancet advance component **1840** can be structured to have two arms (e.g., a long arm and a short arm) that meet at a point (e.g., at a fixed angle) that can rotate about a joint **1861**. The exemplary long arm of the lancet advance component **1840** is connected to the lancet cocking link **1845** at the joint **1841**, and the exemplary short arm of the lancet advance component **1840** is coupled to the lancet slider component **1860**.

[0112] The actuator mechanism includes a lancet fire arm component **1850** that is also utilized to ready a lancet for projection from the lancet cartridge **1803** (e.g., advance lancet firing components to a firing position). One end of the lancet fire arm component **1850** is coupled to the chassis **1801** at a joint **1851** to rotate about the joint **1851** at a fixed point. As shown in FIG. 18B, the other end of the lancet fire arm component **1850** is configured with a curved geometry, e.g., capable of sliding along another surface with a reduced friction. In the initial position, the lancet fire arm component **1850** can rest between two springs: a return spring **1870** that is positioned underneath the lancet fire arm component **1850** and that can be fixed to a structure of the chassis, and a firing spring **1875** that is positioned above the lancet fire arm component **1850** and that can be fixed to a structure of the chassis near the spring-loaded arm component **1805**. In the described embodiment, the lancet fire arm component **1850** can include a weight **1874** configured on the lancet fire arm component **1850** directly underneath the firing spring **1875**, e.g., such that the firing spring contacts the weight **1874**. In the initial position, the return spring **1870** and the firing spring **1875** are in an initial compression state (e.g., which can be partially compressed or substantially uncompressed). The lancet fire arm component **1850** is coupled to a firing hammer component **1885** of the actuator mechanism through an opening in the top end of the firing hammer component **1885**, e.g., in which motion of the lancet fire arm component **1850** can push the firing hammer component **1885** in a linear direction to the

firing position. For example, as the lancet fire arm component **1850** pushes the firing hammer component **1885** to the firing position, the curved end of the lancet fire arm component **1850** also contacts and moves about a trigger catch component **1880** of the actuator mechanism until the curved end has been raised above and is seated upon the top surface of the trigger catch component **1880**, as shown later in FIG. 19B. In other examples, the lancet fire arm component **1850** can be coupled to the firing hammer component **1885** by a joint that allows the lancet fire arm component **1850** to pull and push the firing hammer component **1885** in the linear direction. As described later in the patent document, a lancet can be fired from the device by depressing a firing button **1820** of the actuator mechanism located on an external side of the device **1800**, in which the firing button **1820** retracts the trigger catch component **1880** to release the lancet fire arm component **1850**, such that the firing spring **1875** (and the weight **1874**) drives the lancet fire arm component **1850** downward to drive the firing hammer component **1885** downward to push a lancet to project out of the device **1800**.

[0113] The movement of the sliding button from the initial position to the cocked position advances the lancet advance component **1840** forward, e.g., by pulling of the lancet cocking link **1845** forward, which pulls the lancet advance component **1840** forward. The forward motion of the lancet advance component **1840** to the cocked position includes a rotation of the lancet advance component **1840** with respect to the lancet cocking link **1845** about the joint **1841**. The forward motion of the lancet advance component **1840** to the cocked position also includes a rotation of the lancet advance component **1840** with respect to the lancet cocking crank **1847** about the joint **1841**. The forward motion of the lancet advance component **1840** to the cocked position results in motion of the lancet fire arm component **1850**, which can drive the firing hammer component **1885** to the firing position. For example, the movement of the lancet fire arm component **1850** is actuated by the movement of the long arm of the lancet advance component **1840** and/or the lancet cocking link **1845**. As shown in FIG. 18C, which shows an enlarged cut-out portion of the schematic of FIG. 18A, the actuator mechanism can include a roller pin structure **1844** that is connected to the lancet advance component **1840** and/or the lancet cocking link **1845**. The roller pin structure **1844** is configured directly beneath the lancet fire arm component **1850** to slide or roll on the underside of the lancet fire arm component **1850** to drive the movement of the lancet fire arm component **1850** upwards. The upwards movement of the lancet fire arm component **1850** pushes the firing hammer component **1885** to the firing position and is seated upon the top surface of the trigger catch component **1880**.

[0114] For example, referring to FIG. 18B, when the cocking button **1830** of the sliding button (along with the eject button **1835**) moves forward along the track **1839** from the initial position to the cocked position, the long arm of the lancet advance component **1840** is moved by the lancet cocking link **1845** such that the lancet advance component **1840** rotates about the joint **1861**, in which the short arm of the lancet advance component **1840** moves the sliding component **1860** in a linear direction. The movement of the sliding component **1860** in the linear direction advances the lancet cartridge **1803** by one lancet position from a previous lancet position of the lancet cartridge **1803** in a lancet loading compartment **1808**, in which the lancet loading compartment **1808** is a compartment of the chassis **1801** to initially load the

lancet cartridge **1803**. The movement of the sliding component **1860** in the linear direction advances the lancet cartridge **1803** by one lancet position such that the lancet that is to be fired is placed in a position aligned in the firing path of the firing hammer component **1885** for projection of that lancet. As shown in FIG. 18D, the sliding component **1860** includes a spring loaded pawl **1867** that engages an indented (e.g., toothed) rack of the lancet cartridge **1803** (shown later in FIG. 22A) to latch or clutch the lancet cartridge **1803** during the cocking motion (e.g., the advancement of the lancet advance component **1840** forward). The spring loaded pawl **1867** releases the rack during the return motion of the sliding component **1860**. The pawl can be driven by the short arm of the lancet advance component **1840** as it moves the sliding component **1860** in the linear direction. As shown in FIG. 18E, which shows the device **1800** flipped 180 degrees from the side shown in FIG. 18D, the advancement of the lancet cartridge **1803** moves from a position in the lancet loading compartment **1808** in the linear direction shown by the arrow. In some implementations, the lancet cartridge **1803** is not advanced while the sliding button actuator mechanism is implemented from the initial position to the cocked position. In such examples, the final lancet stored in the lancet cartridge **1803** can be reused over and over again even as the spring loaded pawl **1867** is implemented to latch the next rack as the sliding component **1860** moves in the linear direction (and return it to its initial position). In this exemplary case, the spring loaded pawl **1867** clutches a void and does not alter the position of the lancet cartridge **1803**, allowing the final lancet stored in the cartridge to remain in a position to be fired repeatedly by the firing hammer component **1885**.

[0115] Additionally, in some implementations, the actuator mechanism can include a lancet depth adjustment component **1865** that sets a particular position to control the depth at which the lancet protrudes from the device when fired. Studies have shown that more than a third of the participants in the studies stated that pain is the main reason people with diabetes refrain from regular blood glucose testing. For example, to potentially reduce pain felt by a user, the penetration depth of a lancet can be minimized by adjusting the lancet depth adjustment component **1865** to a particular position such that the selected penetration depth is as shallow as possible while still producing blood at the puncture site of the user. The exemplary lancet depth adjustment component **1865** includes a series of steps that are fitted within a channel along the exterior of the lancet cartridge **1803**, as shown later in FIGS. 22A and 22B. For example, one of the steps of the lancet depth adjustment component **1865** can be positioned at the end of the travel path of the readied lancet. For example, the particular step can be aligned by moving the exemplary lancet depth adjustment component **1865** using a knob **1866** or another type interface on the exterior of the chassis **1801**. For example, a step **1865a** at a distal end of the lancet depth adjustment component **1865** can be positioned in the travel path of the fired lancet to create a shorter distance of travel of the fired lancet, thereby minimizing the length at which the tip of the lancet can protrude outwards from the device during firing. For example, a step **1865b** of the lancet depth adjustment component **1865** can be positioned in the travel path of the fired lancet to create a longer distance of travel of the fired lancet, thereby maximizing the length at which the tip of the lancet can protrude outwards from the device during firing.

[0116] FIGS. 19A and 19B show a sequence of schematic illustrations showing the movement of the sliding button from

the initial position to the cocked position. Implementation of the analyte testing device **1800** can include a first operation of the actuator mechanism that can (1) advance a new test strip from a position within the analyte sensor cartridge **1802** to a position outside of the chassis **1801** partially exposing the sample receiving site of the test strip and (2) advance the firing hammer component **1885** to the firing position for projection of a lancet from the lancet cartridge **1803**, in which both advancements are initiated by the same operation of the actuator mechanism. Additionally or optionally, for example, implementation of the first operation of the actuator mechanism can (3) advance the lancet cartridge **1803** to a position in which the lancet is positioned in the firing path of the firing hammer component **1885** for projection of the lancet. The first operation can be performed using one hand. For example, the first operation can be implemented by a thumb or other finger sliding the sliding button (e.g., pushing the button pad of the cocking button **1830**) from the initial position (as shown in FIG. **19A**) forward to the cocked position (as shown in FIG. **19B**), e.g., such that the chassis **1801** of the device **1800** rests in the palm of the user's hand.

[0117] FIG. **19A** shows the status of the analyte testing device **1800** before operation, in which the components of the actuator mechanism are in an initial state and/or 'home' position. For example, the sliding button is set in the initial position; the spring of the spring-loaded arm component **1805** is in the initial compression state and the rod shaft of the spring-loaded arm component **1805** and the door crank component **1810** are not extended forward; the door **1815** is in the closed position covering the slot opening of the analyte sensor cartridge **1802**; the lancet advance component **1840**, as well as the lancet cocking link **1845** and the lancet cocking crank **1847**, are not extended forward; the sliding component **1860** is in a position ready to advance the lancet cartridge **1803**; and the lancet fire arm component **1850** is not raised upwards and rests between the return spring **1870** and the firing spring **1875** (in the initial compression state).

[0118] FIG. **19B** shows the status of the analyte testing device **1800** during the implementation of the first operation. For example, the sliding button is set in the cocked position; the spring of the spring-loaded arm component **1805** is in the intermediate compression state and the rod shaft of the spring-loaded arm component **1805** and the door crank component **1810** are extended forward; the door **1815** is in the opened position permitting a test strip to be exposed from the analyte sensor cartridge **1802**; the lancet advance component **1840**, as well as the lancet cocking link **1845** and the lancet cocking crank **1847**, are extended forward; the sliding component **1860** is in a position that has advanced the lancet cartridge **1803** (e.g., by one lancet position); and the lancet fire arm component **1850** is raised upwards, compressing the firing spring **1875**, and seated upon the top surface of the trigger catch component **1880**, having positioned the firing hammer component **1885** in the firing position.

[0119] Implementation of the analyte testing device **1800** can include a second operation of the actuator mechanism that can project (e.g., fire) the lancet to prick a user to draw blood for analysis in the test. This operation is described later in the patent document, as shown in FIGS. **24A-24C** and **25A** and **25B**.

[0120] FIGS. **20A**, **20B** and **20C** show a sequence of schematic illustrations of the movement of the eject button **1835** of the sliding button from the cocked position to the eject position and back to the initial position. Implementation of the

analyte testing device **1800** can include a third operation of the actuator mechanism that can eject the used test strip from its exposed position outside of the chassis **1801** and reset the analyte testing device **1800** for another test, e.g., return the any of the components of the actuator mechanism that are not in the home position back to the home position. The third operation can be performed using one hand. For example, the third operation can be implemented by a thumb or other finger sliding the sliding button (e.g., pushing the eject button pad of the eject button **1835**) from the cocked (as shown in FIG. **20A**) forward to the eject position (as shown in FIG. **20B**), which can return back to the initial position (as shown in FIG. **20C**), e.g., such that the chassis **1801** of the device **1800** rests in the palm of the user's hand.

[0121] FIG. **20A** shows the status of the analyte testing device **1800** after implementation of the second operation prior to the third operation, in which some of the components of the actuator mechanism are in a position for receiving the testing sample and other components of the actuator mechanism are in the home position. For example, the cocking button **1830** of the sliding button is set in the initial position; the eject button **1835** of the sliding button is set in the cocked position; the spring of the spring-loaded arm component **1805** is in the intermediate compression state and the rod shaft of the spring-loaded arm component **1805** and the door crank component **1810** remain extended forward; the door **1815** is in the opened position exposing a test strip **1899** from the analyte sensor cartridge **1802** (e.g., to receive a sample from a user); the lancet advance component **1840**, as well as the lancet cocking link **1845** and the lancet cocking crank **1847**, are in the home position; the sliding component **1860** is in home position; and the lancet fire arm component **1850** and the return spring **1870** and the firing spring **1875** are in the home position.

[0122] FIG. **20B** shows a schematic of the analyte testing device **1800** during the implementation of the third operation, in which the actuator mechanism ejects the test strip from the device (e.g., after receiving blood from a patient and receiving the results of the test of the blood sample, for example, which can be displayed on a display of the device **1800**). For example, the eject button **1835** of the sliding button has been advanced to the eject position; the spring of the spring-loaded arm component **1805** is further compressed beyond the intermediate compression state and the rod shaft of the spring-loaded arm component **1805** and the door crank component **1810** remain extended forward; the door **1815** remains in the opened position while the test strip **1899** is at least partially protruding from the slot opening (e.g., and the door immediately closes as the test strip **1899** is fully ejected); and the cocking button **1830** of the sliding button, the lancet advance component **1840**, the lancet cocking link **1845**, the lancet cocking crank **1847**, sliding component **1860**, the lancet fire arm component **1850** and the return spring **1870** and the firing spring **1875** are in the home position.

[0123] FIG. **20C** shows a schematic of the analyte testing device **1800** after implementation of the third operation, in which the components of the actuator mechanism are in the home position.

[0124] FIGS. **21A** and **21B** show schematics of the exemplary sliding button components of the actuator mechanism of the analyte testing device **1800**. As shown in FIG. **21A**, the sliding button includes the cocking button **1830** and the eject button **1835** that can move (e.g., slide) translationally along the sliding track **1839**. The eject button **1835** includes the

eject base component **1837**, which is coupled to a projection tongue component **1890** of the actuator mechanism to project a test strip from the analyte sensor cartridge **1802**, e.g., by pushing the test strip out of the slot opening of the device **1800**. For example, the analyte sensor cartridge **1802** can be configured to include an opening on an internal side to allow the projection tongue component **1890** to enter the cartridge **1802** and make contact with the test strip and move (e.g., push) the test strip through the slot opening. In some implementations, for example, the eject base component **1837** and the projection tongue component **1890** can be a single component. The bottom side of the sliding track **1839** includes an indented channel **1891**, e.g., which is shaped in a closed-loop path, as shown in FIG. 21B. The sliding button includes sliding pin **1893** that is configured within the indented channel **1891** of the sliding track **1839** to control the motion of the sliding pin **1893** when the sliding button is engaged and in motion. The sliding pin **1893** is coupled to a connector link **1892** that connects the sliding pin **1893** to the projection tongue component **1890**. The indented channel **1891** includes various depths along the channel to provide a ramp for the sliding pin **1893** to travel. For example, the ramping of the indented channel **1891** can control the sliding pin **1893** to travel along a single pathway of the closed-loop path (e.g., in a clockwise travel in the path of the indented channel **1891**). The indented channel **1891** includes various catch stops along the channel for the sliding pin **1893** to stop in the initial position, the cocked position, and the eject position and prevent back-travel of the sliding pin **1893** along the pathway of the indented channel **1891**. The indented channel **1891** can also include a safety catch stop located at a position between the initial position and the cocked position that can prevent back-travel of the sliding pin **1893** from returning to the initial position before the sliding button has fully traveled to the catch stop of the cocked position to implement the first operation. For example, premature back-travel of the sliding pin **1893** to the initial position can result in the projection tongue component **1890** losing contact with the analyte sensor it projects (e.g., during the first or third operations), which may result in a subsequent analyte sensor (e.g., directly under the advanced analyte sensor in the analyte sensor cartridge **1802**) raising up within the cartridge in the analyte sensor projection path, thereby potentially creating a jam of the two analyte sensors in the analyte sensor cartridge **1802**. The safety catch stop can prevent potential jamming of analyte sensors in the cartridge in the event that the sliding button is brought back prematurely by stopping the sliding button from returning to the initial position prior to arriving at the catch stop of the cocked position, thereby maintaining at least a portion of the projection tongue component **1890** in the analyte sensor projection path.

[0125] FIG. 21B shows a sequence of schematic illustrations showing the movement of the sliding button along the sliding track **1839** from the initial position to the cocked position to the eject position and back to the initial position. For example, as shown in the schematic **2101** of FIG. 21B, prior to the first operation of the actuator mechanism, the sliding pin **1893** is stationary in a catch stop of the initial position, such that the projection tongue component **1890** is in a retracted position located in a region under the sliding track **1839**. For example, as shown in the schematic **2102** of FIG. 21B, implementation of the first operation of the actuator mechanism moves the sliding pin **1893** from the catch stop of the initial position to a catch stop of the cocked position,

such that the projection tongue component **1890** is partially protruded from the region under the sliding track **1839** (e.g., which can push the test strip partially out of the device to expose a portion of the test strip). For example, as shown in the schematic **2103** of FIG. 21B, implementation of the third operation of the actuator mechanism moves the sliding pin **1893** from the catch stop of the cocked position to a catch stop of the eject position, such that the projection tongue component **1890** is fully protruded from the region under the sliding track **1839** (e.g., which can push the test strip entirely out from the device to eject the test strip). For example, as shown in the schematic **2104** of FIG. 21B, implementation of the third operation of the actuator mechanism also moves the sliding pin **1893** from the catch stop of the eject position back to the catch stop of the initial position, such that the projection tongue component **1890** is retracted back to the region under the sliding track **1839**. For example, in some implementations, the catch stop of the eject position can be configured not to catch the sliding pin **1893** and allow the sliding button to slide back to the initial position in one continuous movement.

[0126] FIGS. 22A-22C show schematics of the lancet cartridge **1803** of the analyte testing device **1800**. FIG. 22A shows a three dimensional view of an internal side and bottom side of the lancet cartridge **1803**. The lancet cartridge **1803** includes a channel **1825** along the exterior of the internal side of the cartridge. The channel **1825** provides a region in which the lancet depth adjustment component **1865** passes through such that a step of the series of steps can be aligned in the firing path of the lancet to be fired. The lancet cartridge **1803** includes a toothed rack **1828** along the exterior of the internal side of the lancet cartridge **1803**. The toothed rack **1828** provides indentations into the exterior that can engage the spring loaded pawl **1867** for the advancement of the lancet cartridge **1803** in the linear direction, e.g., which can be implemented in the first operation. The lancet cartridge **1803** includes a covering layer **1827** (e.g., such as a film) along the exterior of the bottom side of the lancet cartridge **1803** (e.g., which is shown to wrap around the side(s) of the cartridge). The covering layer **1827** provides a protective covering over openings **1826** to the lancet chambers to protect the lancet from contaminations and maintain a sterile environment within the chambers, as well as bonds the top and bottom of the lancet cartridge **1803** together. The lancet cartridge **1803** includes open troughs **1824** within the channel **1825** to allow a spring arm of a lancet (shown later in FIGS. 25A and 25B) to return to its initial position after the lancet has been fired.

[0127] FIG. 22B shows a three dimensional view of an internal side and top side of the lancet cartridge **1803**. The lancet cartridge **1803** includes lancets **1821**, in which a contact side of each lancet **1821** is exposed out of an opening **1823** of the top side lancet cartridge **1803** such that the firing hammer component **1885** can contact and move the lancet **1821**, e.g., upon firing the lancet implemented in the second operation. The lancet cartridge **1803** includes detents **1829** along an edge of the top and internal side of the cartridge to retain an indexed position of the lancet cartridge after advancement. For example, the movement of the sliding component **1860** in the linear direction advances the lancet cartridge **1803** by one lancet position that is indexed by the detent **1829** such that a lancet that is to be fired is placed in a position aligned in the firing path of the firing hammer component **1885** for projection of that lancet.

[0128] FIG. 22C shows a three dimensional view of an external side and the bottom side of the lancet cartridge **1803**

showing an indented catch **1822** for a user to remove the cartridge with the user's finger.

[0129] FIG. 23A shows a schematic of the lancet **1821**. The lancet **1821** includes a lance **1821a** (also referred to as a needle) that can be used to puncture or prick a user upon projection from the device **1800**, e.g., to draw blood from the puncture or prick. The lancet **1821** includes a leaf spring **1821b** including a notch on a split tail of the lancet **1821** that can be used to provide a positive engagement with the lancet cartridge **1803** to retain the lancet **1821** in a rest position within the cartridge, as shown in the FIG. 23B. The lancet **1821** includes a guide rail structure **1821c** that protrudes out along the side of the lancet **1821** in a straight line which can align with a guide track **1804** inside the lancet chamber **1807** to control the projection of the lancet to be substantially entirely linear or straight motion. The lancet **1821** includes a retract structure **1821d** that can engage with a lancet return spring to retract the lancet back into the lancet cartridge **1803**.

[0130] FIGS. 23B and 23C show schematics of the lancet **1821** in the lancet cartridge **1803**. FIG. 23B shows a cross sectional side view of the lancet **1821** in the rest position within the lancet cartridge **1803**. For example, in the rest position, a curved protrusion notch of the leaf spring **1821b** is aligned in a groove or indentation formed by a retention bump **1809** of the lancet chamber **1807** of the lancet cartridge **1803**. The retract structure **1821d** of the lancet **1821** is positioned outside of the channel **1825** and within the casing of the lancet cartridge **1803**. The lance **1821a** is positioned near the opening **1826** within the lancet chamber **1807** of the lancet cartridge **1803**. The covering layer **1827** is intact and not punctured by the lance **1821a**. FIG. 23C shows a top view of the lancet cartridge **1803** showing a plurality of lancets **1821** contained within the cartridge. As shown in the figure, each lancet **1821** can be enclosed within the lancet chamber with a tight tolerance to closely fit the lancet, e.g., with a tight alignment of the guide rail **1821c** with the guide track **1804**.

[0131] FIGS. 24A-24E show a sequence of schematic illustrations showing the projection of the lancet **1821** based on the operation of the actuator mechanism. Implementation of the second operation of the actuator mechanism can project (e.g., fire) the lancet to prick a user to draw blood for analysis in the test. The second operation can be performed using one hand. For example, the second operation can be implemented by a thumb or other finger pressing the firing button **1820**, e.g., such that the chassis **1801** of the device **1800** rests in the palm of the user's hand. For example, pressing the firing button **1820** retracts the trigger catch component **1880** such that the lancet fire arm component **1850** can slide off from its seated position on the top surface of the trigger catch component **1880**, thereby releasing the firing hammer component **1885** from the firing position. The firing spring **1875** (and the weight **1874**) can contribute to driving the lancet fire arm component **1850** downward to drive the firing hammer component **1885** downward and into the lancet cartridge **1803** through the opening **1823**. The firing hammer component **1885** impacts the lancet **1821** and drives the lancet **1821** along the guide track **1804** in the lancet chamber **1807** in a linear motion to project the lance **1821a** straight through the opening **1826** and out of the device **1800**.

[0132] FIG. 24A shows a cross sectional side view of some components of the actuator mechanism in the cocked position prior to implementation of the second operation to fire the lancet **1821**. For example, in the cocked position, the firing hammer component **1885** is in the firing position within the

chassis **1801**. A lancet return spring **1898** of the actuator mechanism is aligned along the top side of the channel **1825** of the lancet cartridge **1803**, which can rest against the retract structure **1821d** of the lancet **1821**. For example, the lancet return spring **1898** can be utilized to return the lancet **1821** to the rest position after the lancet has been fired. FIG. 25 shows three dimensional cross sectional schematics of the lancet return spring **1898** in the analyte testing device **1800**. In some examples, the actuator mechanism can include a wire spring **1897** that assists in the retraction of the firing hammer component **1885** to the home position after it has been fired.

[0133] FIG. 24B shows an enlarged cross sectional side view of the lancet **1821** in the rest position within the lancet cartridge **1803** prior to implementation of the second operation. For example, in the rest position, the curved protrusion notch of the leaf spring **1821b** is aligned in the groove or indentation formed by the retention bump **1809** in the lancet chamber **1807** of the lancet cartridge **1803**. The retract structure **1821d** of the lancet **1821** is positioned within the casing of the lancet cartridge **1803**, e.g., by a force applied by the lancet return spring **1898**. The lance **1821a** is positioned near the opening **1826** within the lancet chamber **1807** of the lancet cartridge **1803**. The covering layer **1827** is intact and not punctured by the lance **1821a**.

[0134] FIG. 24C shows a cross sectional side view of the some components of the actuator mechanism during the implementation of the second operation to fire the lancet **1821**. For example, during firing, the firing hammer component **1885** impacts the lancet **1821** and continues into the lancet chamber **1807** of the lancet cartridge **1803** to drive the lancet **1821** in a substantially straight motion. The lance **1821a** travels through the opening **1826** and pierces the covering layer **1827** as it exits the device. Upon reaching the maximum travel distance, the firing hammer component **1885** is returned to the home position and the force applied by the lancet return spring **1898** against the retract structure **1821d** of the lancet **1821** can drive the lancet back to the rest position.

[0135] FIGS. 24D and 24E show enlarged cross sectional side views of the lancet **1821** within the lancet cartridge **1803** during the implementation of the second operation. For example, during firing, the lancet **1821** is driven in a substantially straight line in the chamber **1807** via the alignment of the guide rail structure **1821c** of the lancet **1821** and the guide track **1804** of the lancet cartridge **1803**. The force that initiates the linear movement of the lancet **1821** (e.g., the impact by the firing hammer component **1885**) drives the curved protrusion notch of the leaf spring **1821b** out of the groove or indentation formed by the retention bump **1809** in the lancet chamber **1807** of the lancet cartridge **1803**. The retract structure **1821d** of the lancet **1821** pushes against the lancet return spring **1898** such that the linear movement of the lancet **1821** is capable of overcoming force applied by the lancet return spring **1898** against the lancet. The lancet **1821** travels the available distance provided in the channel **1825**, e.g., which can be based on the full length of the channel **1825** (e.g., 6 mm) or a smaller distance based on a particular step of the lancet depth adjustment component **1865** positioned within the firing pathway in the channel **1825**. In some examples, the travel distance of the lancet **1821** during firing can be configured to be in a range between 4.5 mm and 6 mm based on the step of the lancet depth adjustment component **1865** positioned within the firing pathway in the channel **1825**. In some examples, the travel distance of the lancet **1821** during firing can be controlled

based on the adjusting the compressive force that can be applied by the lancet return spring **1898** against the retract structure **1821d**. The lance **1821a** travels through the opening **1826** and pierces the covering layer **1827** as it exits the device. Upon reaching the maximum travel distance, the firing hammer component **1885** is returned to the home position and the force applied by the lancet return spring **1898** against the retract structure **1821d** of the lancet **1821** drives the lancet back to the rest position.

**[0136]** In another embodiment of the disclosed technology, systems, devices, and methods are described for an analyte testing system includes a hand-held analyte testing device and a docking station. The analyte testing device houses: (i) a plurality of lancets, (ii) a plurality of analyte sensors usable in conjunction with the lancets, (iii) electronics for deriving test data from the analyte sensors, (iv) a visual display that displays the test data, and (v) a data recording facility that records non-test data. The handheld device is used to prick a body member for drawing a blood sample, and test the blood sample for analytes such as glucose. The docking station has a power interface for providing power to the analyte testing device. The docking station also has a data interface and a storage facility that stores the test data and the non-test data.

**[0137]** In some implementations of this disclosed embodiment, the testing device and/or the docking station has a communication facility configured to transmit and receive with an external storage device (e.g., a medical provider server, home computer, local area network). The communication facility can be wired or wireless. In some implementations, the communication facility uses at least two wireless protocols. In other implementations, the communication facility transmits data a cell phone network. Contemplated data include test data, information derived from test data, and non-test data. In some implementations, the power interface is an inductive charging pad and the data interface is a wired connection, such as a USB port. The docking station can further include a second data interface, either wired or wireless, for exchanging data with an external device (e.g., home computer, laptop, smart phone, insulin pen, health test device). The data collected by the analyte testing device electronics can include test data (i.e., analyte testing results), information derived from the test data (e.g., reports, graphs, analytics, trends), and even non-test data, such as: diary information recorded as text and/or audio; supplies used; supplies ordered; food eaten, minutes exercised and estimated calories burned; amount of medication taken, time medication was taken, supplies available in a user's personal inventory, and supply ordering history. In some implementations, at least one of the docking station and testing device includes a panic button configured to alert a third party of a user's identity and condition. The docking station also preferably has a backup rechargeable battery that can replace a rechargeable battery of the handheld analyte testing device. In some implementations, the testing device display is an LCD touch screen that indicates (i) whether the analyte testing device is charging and (ii) whether data is being transferred between the analyte testing device and the docking station. It is also contemplated that the docking station can include a display for indicating a charge status and data exchange status. The display preferably includes a graph showing a maximum threshold line, minimum threshold line, and a test data line. The max/min threshold lines indicate help the user to determine whether analyte test results are within acceptable limits. In some implementations, the recording facility is a microphone and/

or keypad, which can be used to record diary entries. In some implementations, at least one of the testing device and the docking station has a processor programmed to test the adequacy of a communication link between the testing device and the docking station. The docking station preferably has a processor and executable code that is configured to automatically (i) back-up the test data and the non-test data, (ii) track supply usage, and (iii) re-orders supplies. In some implementations, the plurality of lancets are contained in a lancet cartridge and the plurality of analyte sensors are contained in an analyte sensor cartridge. It is also contemplated that the analyte sensor cartridge can be separate from the lancet cartridge. In some implementations, the storage facility in the docking station is removable. The storage facility can also be configured to store data in a generic file format (e.g., pdf, doc, xml, eps, html, jpeg, rtf, and txt). For example, the storage facility is password protected and stores the test data and non-test data using encryption. In some implementations, the analyte testing system also includes an insulin pen for administering medication. The pen preferably has a wireless communication facility configured to exchange data with the testing device.

**[0138]** FIGS. **26a** and **26b** show an analyte testing system **8100** comprising a handheld analyte testing device **8200** and a docking station **8300**. Device **8200** couples with station **8300** via power interface **8310** and data interface **8320**, as shown in FIG. **26b**. Docking station **8300** can optionally be configured with a cradle or recessed portion for receiving device **8200** in a secure manner. FIG. **26a** shows device **8200** disconnected from station **8300**. Power interface **8310** is an inductive pad configured to provide electrical power to a rechargeable battery within device **8200**. An inductive pad advantageously allows device **8200** to charge without physically mating with the docking station. In alternative embodiments, power interface **8310** could comprise an electrical connector configured to mate with a connector on device **8200**. Data interface **8320** is physical connector configured to mate with a connector on device **8200** and provides data connectivity between storage mediums in device **8200** and docking station **8300** (not shown). However, it is also contemplated that data interface **8320** could comprise a wireless transmitter communicatively coupled with a wireless transmitter of device **8200**.

**[0139]** Interfaces **8310** and **8320** can be two separate and distinct interfaces, or alternatively, can be integrated into one interface. Power interfaces and data interfaces are well known. In one embodiment, data interface **8320** comprises a USB port and power interface **8310** comprises an inductive current loop. Interfaces **8310** and **8320** can utilize an industry standard or proprietary technology. In some embodiments, data interface **8320** is a wireless transceiver configured to communicate with a wireless transceiver of device **8200** using any number of wireless communication protocols and technologies (e.g., Bluetooth, wifi, cellular network, 802.11). The term wifi is used here generically to refer to a wireless local area network, rather than in a trademark sense to refer to Wi-Fi™. In such embodiments, station **8300** preferably uses at least two alternative wireless communication protocols so that a secondary communication link is available in case the primary communication link fails. Including multiple protocols also advantageously increases compatibility with other devices.

**[0140]** Docking station **8300** has a removable storage medium **8370** coupled with an internal processor/electronics

(not shown), and is configured to automatically backup analyte testing results data from device **8200**. The internal electronics are also preferably configured to analyze test results and identify trends. In addition to test data, it is further contemplated that other data can be stored and analyzed on station **8300** and/or device **8200**. Such data can include time-stamped diary entries, either in text or audio format. For example, a user can record verbal comments on his or her physical health (e.g., severity and frequency of symptoms). Other data can further include: medication taken (amount, time), supplies used, supply order history, supplies remaining in the user's personal inventory, exercise (minutes, type), estimated calories burned, dietary intake information (protein, sugar, fat, sodium, etc) or any other information relevant and helpful for monitoring analytes and health issues. Contemplated supplies include, but are not limited to, lancets, test strips, and medication.

[0141] A removable storage medium **8370** advantageously allows a user to take the storage facility to a health care provider for sharing the health data. The data is preferably password protected and/or encrypted in order to maintain the user's privacy. The data is preferably stored in a common or standard format (e.g., pdf, doc, xml, eps, html, jpeg, rtf, and txt) so that a doctor can view the data without the need for custom software.

[0142] Docking station **8300** has an LCD touch screen display **8330** for displaying and inputting information. For example, display **8330** can show test results, history and trending of test results, supplies used, supplies remaining, or any other data helpful for monitoring analytes and health. In some embodiments, display **8330** shows the number of lancet and test strip cartridges remaining in the user's personal inventory (e.g., closet). Display **8330** can further be used for video conference communication with a health care professional or for displaying instructional videos on how to operate system **8100**. Display **8330** can additionally serve as an input device for recording audio diary entries, dietary or exercise information, or any other data useful for monitoring analytes. However, it is also contemplated that an input device other than display **8330** can be included in station **8300** (e.g., buttons, key pad, microphone for voice-recognition commands).

[0143] Display **8330** can further display an indication of whether device **8200** is properly connected via power interface **8310** and data interface **8320**. In addition, display **8330** can show whether power interface **8310** is rechargeable charging a battery of device **8200**, estimated time to complete a full charge, and whether data is currently being exchanged via interface **8320**. The indicators can optionally comprise several LED lights having different colors and/or different blinking patterns.

[0144] Docking station **8300** can include additional data interfaces and can be configured to function as a hub for multiple handheld health monitoring devices. In this manner, docking station **8300** can act as a central point for gather a user's health data, analyzing the data, and transmitting the data to a health care provider. Station **8300** can also include a calibration mechanism for testing accuracy of device **8200**. In addition, station **8300** can include electronics for testing the adequacy and operability of the testing device's communication facility.

[0145] FIG. 27 shows handheld analyte testing device **8200**. Device **8200** is a lancing device integrated with an analyte meter. The housing of device **8200** has a first com-

partment **8210** and a second compartment **8220**, for storing a lancet cartridge **8215** (see FIG. 29) and an analyte sensor cartridge **8225** (see FIG. 30), respectively. Device **8200** houses various electrical components (memory, processor, executable code, etc) configured to convert electrical signals from analyte test strip **8226** (see FIG. 30) into a test result reading. Device **8200** also has a data recording facility **8205** for recording data, and a display **8280** for displaying data.

[0146] Data recording facility **8205** and related electronics are used to store voice recordings of diary information as previously described. The electronics can also include a speaker for communicating data to a user and for prompting a user to use the device according to a pre-selected time and/or pre-selected time interval. In addition, the electronics can be equipped with an accelerometer or pedometer for measuring and calculating distance traveled and calories burned. In other aspects of the disclosed embodiments, the electronics of device **8200** preferably includes a processor programmed to correlate individual instances of data with time stamps. For example, test result data and diary entries can be time stamped and correlated. In addition, the processor can be programmed to make an evaluation of the data, and send a notification to different recipients as a function of the evaluation. In some embodiments, the processor is used to create static reports and saved in a generic file format onto removable storage medium **8370**. Yet still, the processor can be programmed to keep track of inventory of lancets and test strips, automatically re-order supplies, and automatically backup data to storage medium **8370**.

[0147] Device **8200** has an actuator **8240** configured to (i) cock a lancing apparatus within device **8200** (not shown), (ii) expose a test strip for use, and (iii) advance the lancet cartridge. The test strip is exposed via slot **8230**. An ejection mechanism **8233** allows for ejection and disposal of the test strip after testing, without the need for directly touching the test strip.

[0148] Device **8200** has a LCD touch screen display **8280**, which can be used in a similar fashion to display **8330** of station **8300**. For example, display **8280** can be used to input diary information using a touch screen keypad. It is also contemplated that device **8200** can include a hard keypad. In some embodiments, display **8280** is used to display a graph that shows actual test data in relation to a maximum and minimum threshold line. The electronics of device **8200** can be programmed to notify the user or a medical care provider via a cellular network when test data exceeds the max/min thresholds.

[0149] Device **8200** also has a panic button **8290** that is configured to communicate the user's identity and health status to a third party. For example, the panic button can be used to contact an emergency service, identify the patient's name, current location, and health status. It is further contemplated that panic button **8290** can be configured to contact different persons (e.g., relative, home nurse, doctor, police) and convey different levels of urgency (e.g., low, moderate, high, critical) as a function of test results.

[0150] The housing of device **8200** and station **8300** can be made of plastic, metal, composite, or any other material with structural and mechanical properties suitable for housing a lancet cartridge, test strip cartridge, electronics, and a linkage mechanism. Device **8200** is preferably compact, with a height no more than 50 mm, a width no more than 17 mm, and a length no more than 100 mm. In some embodiments, the housing of device **8200** and station **8300** comprises an outer

protective shell made of molded plastic and an inner desiccant liner to minimize exposure to moisture.

[0151] Unless the context dictates the contrary, all ranges set forth herein should be interpreted as being inclusive of their endpoints, and open-ended ranges should be interpreted to include commercially practical values. Similarly, all lists of values should be considered as inclusive of intermediate values unless the context indicates the contrary.

[0152] FIG. 28 shows the back side of device 8200. Hole 8250 is used to eject a lancet for pricking a body part in order to draw a blood sample. Wheel 8260 is used to adjust the penetration depth of the lancet, while window 8270 displays the penetration setting. Cover 8275 is hingeably coupled to device 8200 and can be opened in order to insert a lancet cartridge 8215 and an analyte sensor cartridge 8225 into device 8200.

[0153] FIG. 29 shows one embodiment of a lancet cartridge 8215. Cartridge 8215 holds a plurality of lancets 8217. Holes 8219 are included on cartridge 8215 to allow a lancet to be temporarily ejected from cartridge 8215 and out of hole 8250 of device 8200 for drawing a blood sample. The lancet is safely retracted back into cartridge 8215 by a retraction mechanism within device 8200 (not shown).

[0154] FIG. 30 shows an analyte sensor cartridge 8225. Cartridge 8225 holds a plurality of test strips such as test strip 8226. Strip 8226 has an analyte sensor 8227 for testing an analyte. Analyte sensors are well known and generally comprise an absorbent material with a reactant (e.g., analyte-binding reagent). Sensor 8227 is configured to generate an electrical signal that is sent to the electronics of device 8200 for conversion into readable test data.

[0155] Cartridge 8225 can include any appropriate number of test strips, preferably between 15 and 25, more preferably between 18 and 22, and most preferably 20. The number of test strips also preferably equals the number of lancets in cartridge 8215, although other combinations are contemplated.

[0156] Cartridge 8225 preferably includes analyte sensors configured to test for different analytes. For example, some sensors may test for glucose levels while other sensors test for fructosamine levels. Furthermore, cartridge 8225 can have at least one test strip capable of testing for two analytes simultaneously, either by including two reactants within one absorbing material or by including two different analyte sensors on one test strip.

[0157] Cartridge 8225 also preferably includes an inner desiccant liner for protecting the plurality of test strips from exposure to moisture. For example, a liner can be disposed between the test strips and the inner wall of cartridge 8225, thus surrounding all the test strips (e.g., an inner sleeve). In addition, all cartridge apertures are preferably sealed with a pull-away adhesive label. Alternatively, a "sacrificial strip" can be included at the top of the stack of test strips. The sacrificial strip can be configured such that it corks and seals all apertures in cartridge 8225. In this manner, cartridge 8225 seals and protects the analyte sensors of the plurality strips from exposure to moisture and dust. The labels and/or sacrificial strip can be removed and discarded just prior to loading the cartridge into device 8200. Cartridge 8225 also preferably includes gaskets and/or o-rings at all cartridge apertures. These gaskets can be configured to mate with components of device 8200 such that a seal is provided to protect the plurality of test strips from moisture while the cartridge is loaded in device 8200 and not in use. It is also contemplated that lancet

cartridge 8215 could also include pull-away labels, seals, gaskets, and liners to protect the lancets from germs, bacteria, viruses, dirt, and other contamination.

[0158] FIG. 31 shows docking station 8300 communicatively coupled with laptop 8380 and personal computer 8390. Station 8300 has a power cord 8610 for supplying power to station 8300 and device 8200. Docking station 8300 and laptop 8380 are communicatively connected via wireless connection 8350. Connection 8350 can comprise any wireless protocol, for example Bluetooth, wifi, 802.11, and cellular networks. Personal computer 8390 is connected to docking station 8300 via wired connection 8360 and data interface 8340. In one embodiment, connection 8360 is a USB cord and interface 8340 is a USB port.

[0159] Connections 8350 and 8360 can be used to back up data, transmit data to a health care provider's server via the internet, reorder supplies, receive notifications from a doctor, or receive data analysis reports from analytics software running on the external device. Furthermore, it is contemplated that docking station 8300 can connect to other external devices (e.g., smart phone, handheld health-monitoring device, insulin pen).

[0160] FIG. 32 shows testing device 8200 in wireless communication with an insulin pen 8750, laptop 8760, and local area network (LAN) 8770. In some embodiments, the insulin pen sends medication administration data (e.g., dosage administered, time of day, patient name) to device 8200. The electronics of device 8200 preferably correlates the medication administration data with the test data and non-test data, either time stamps or by some other correlative attribute. Device 8200 can use communication with LAN 8770 to upload data to a medical server 8780, or otherwise exchange data with a third party. Alternative, LAN 8770 could comprise a cellular network. It is also contemplated that device 8200 could communicate with an external device (e.g., insulin pen, handheld health monitoring device) via a wired connection.

[0161] In another embodiment of the disclosed technology, systems, devices, and methods are described for a test unit cartridge that houses: (i) a first test unit having a first analyte sensor that includes a first reagent used to detect a first analyte; and (ii) a second test unit having a second analyte sensor that includes a second reagent used to detect a second analyte different from the first analyte, such that the first test unit is not functionally fungible with the second test unit.

[0162] In some implementations of this disclosed embodiment, the test unit comprises a single strip. With reference to this disclosed embodiment, the term "strip" means a thin (less than 5 mm thick) elongated object having at least one analyte sensor. A test unit can also comprise a non-strip configuration, such as a capsule more than 5 mm thick, or a disk. In some implementations, the first test unit has no other analyte sensors besides the first analyte sensor. Alternatively, the first test unit can include an additional analyte sensor that detects the second analyte. In some implementations, the cartridge includes a "sacrificial" test unit disposed at a beginning of an order of use of the cartridge. The sacrificial test unit is configured to provide a moisture barrier by corking and sealing all apertures of the cartridge. The "sacrificial" test unit can optionally include at least two analyte sensors for detecting multiple analytes. It is also contemplated that each test unit can include features that cork the apertures of the cartridge such that the test units are protected from moisture and dust when not in use. In some implementations, the test unit cartridge includes a third through twentieth test unit, each of

which is functionally fungible with the first test unit. In some implementations, the first reagent and second reagent are different. For example, the first reagent is configured to bind with a first analyte and the second reagent is configured to bind with a second analyte. In some implementations, the cartridge includes pull-away labels that cover every aperture of the cartridge in order to provide a seal and barrier from moisture and dust. In some implementations, the cartridge includes an aperture that allows an electrical contact of the first test unit to directly couple with an electrical contact of an analyte testing device. In some implementations, the test unit cartridge has a plurality of test units, wherein at least one of the test units has a first and second analyte sensor configured to detect a first and second analyte, respectively. The first and second analyte sensors can be completely non-overlapping, partly overlapping, or completely overlapping. In some implementations, the first and second analyte sensors are physically separated by a distance. In some implementations, the test unit cartridge includes a calibration test unit and an operating test unit. With reference to this disclosed embodiment, the term "calibration test unit" means a test unit having a known analyte presence and configured to test the accuracy of an analyte testing device (e.g., glucose meter). With reference to this disclosed embodiment, the term "operating test unit" means a test unit having an analyte sensor that is configured to detect an analyte. In some implementations, the test unit cartridge has a plurality of test units and a spring. The spring is disposed in a manner such that each test unit is advanced into a usable position after a previous test strip has been laterally ejected from the cartridge. In some implementations, the test unit cartridge houses a plurality of test units in a stacked configuration.

[0163] FIGS. 33 and 34 show perspective and side views, respectively, of a test unit cartridge 9100. Cartridge 9100 holds a plurality of test units 9110 in a stacked configuration. The stacked configuration of test units 9110 advantageously allows cartridge 9100 to have a compact and simple design that requires minimal material. Cartridge 9100 is configured to couple with an analyte testing device. For example, cartridge 9100 has electrical contacts 9128 for communicatively coupling the test units 9110 with conversion electronics in an analyte testing device. Cartridge 9100 also has a slot 9129 that couples with a linkage mechanism of an analyte device, wherein the linkage is configured to push a portion of a test unit out of cartridge 9100 in order to expose analyte sensor 9115. Cartridge 9100 is preferably sized and dimensioned to mate with a compartment of an analyte testing device.

[0164] Cartridge 9100 can include any appropriate number of test units, preferably between 15 and 25 test units, more preferably between 18 and 22 test units, and most preferably 20 test units. Cartridge 9100 includes test units configured to test for different analytes. For example, test unit 9110a has an analyte sensor 9115a, which includes an analyte-binding reagent configured to test for glucose. Test unit 9110b has two analyte sensors (sensor 9115b and sensor 9116b) for detecting two different analytes (e.g., glucose and iron) using only one fluid sample. Cartridge 9100 also has a calibration test unit 9110c that has two analyte sensors: sensor 9115c is for detecting glucose and calibration sensor 9116c is for checking the accuracy of an analyte meter.

[0165] Unless the context dictates the contrary, all ranges set forth herein should be interpreted as being inclusive of their endpoints, and open-ended ranges should be interpreted to include commercially practical values. Similarly, all lists of

values should be considered as inclusive of intermediate values unless the context indicates the contrary.

[0166] Cartridge 9100 can include a test unit that is functionally fungible with 9110b or 9110c at every  $n^{\text{th}}$  test unit within the plurality of test units 9110 in order to ensure that certain health data is gathered at particular intervals. For example, in one embodiment cartridge 9100 holds twenty test units, wherein the first and third through twentieth test units are configured to detect glucose, and the second test unit is configured to detect glucose and fructosamine. In this manner, fructosamine levels are monitored at every second test unit of every test unit cartridge.

[0167] The housing of cartridge 9100 can be made of plastic, metal, composite, or any other material with structural and mechanical properties suitable for housing a plurality of test units. Cartridge 9100 is preferably compact, with a height no more than 25 mm, a width no more than 15 mm, and a length no more than 50 mm. In some embodiments, the height is no more than 20 mm, a width is no more than 8 mm, and a length is no more than 40 mm.

[0168] Cartridge 9100 also preferably includes an inner desiccant liner (not shown) for protecting the plurality of test units from exposure to moisture. For example, a liner can be disposed between the test units and the inner wall of cartridge 9100, thus surrounding all the test units (e.g., an inner sleeve). In some embodiments, the liner comprises a crystalline structure configured to absorb moisture and prevent moisture from reaching the analyte sensors. Liners are well known and all materials suitable for absorbing and/or blocking moisture are contemplated. In addition, all cartridge apertures are preferably sealed with a pull-away adhesive label. For example, pull-away label 9131 has been placed over slot 9129 in order to seal slot 9129, thus protecting test units 9110 from exposure to moisture and dust. Preferably, slot 9132, slot 9133 and all other orifices/apertures of cartridge 9100 are sealed with a pull-away label. The labels can be removed just prior to loading cartridge 9100 into device 9600 (see FIG. 38). Cartridge 9100 also preferably includes gaskets and/or o-rings at all cartridge apertures. These gaskets can be configured to mate with components of device 9600 such that a seal is maintained while cartridge 9100 is loaded in device 9600 and not in use.

[0169] Cartridge 9100 also includes a spring 9175, which is disposed below the plurality of test units 9110 and is configured to push the test units 9110 upward. In this manner, each test unit is pushed up into a usable position after the previous test unit is laterally ejected out of slot 9132.

[0170] Cartridge 9100 provides several advantages. First, by providing a plurality of test units in one disposable and replaceable cartridge, methods and devices for monitoring analytes is significantly simplified. Second, cartridge 9100 provides a means for ensuring that secondary health data is gathered at predetermined intervals. For example, a diabetes patient monitoring glucose levels (i.e., primary health data) will nonetheless monitor secondary health data (e.g., fructosamine levels) when test unit 9110b is used. Third, cartridge 9100 allows primary and secondary health data to be gathered simultaneously in a single blood sample. Fourth, cartridge 9100 provides an enclosure that protects a plurality of test units from exposure to moisture and dust. Finally, cartridge 9100 provides a simple mechanism for advancing each test unit into place after the previous test unit has been removed and disposed.

[0171] FIG. 35 shows a test unit 9110a, which has an analyte sensor 9115a. Analyte sensors are well known and generally comprise an absorbent material that includes a reagent (e.g., an analyte-binding reagent). In this case, sensor 9115a is configured to detect glucose. The sensor 9115a is configured to generate a signal that is sent to electrical contacts 9130. Electrical contacts 9130 are communicatively coupled with electrical contacts 9128 of cartridge 9100, thus allowing the signal to reach conversion electronics in an analyte testing device (e.g., a glucose meter). Alternatively, electrical contacts 9130 could directly interface with an analyte testing device's conversion electronics via an open aperture on cartridge 9100 (e.g., slot 9133 with contacts 9128 removed). In this manner, test unit 9110a allows a diabetic patient to monitor glucose levels. As used herein, "analyte sensor" refers to an independently interpretable signal representing an amount of an analyte present in a fluid sample. Under this definition, one piece of absorbent material having one reagent that is capable of binding to two different analytes at the same time, would be considered two separate "analyte sensors" if two independently interpretable signals are produced, regardless of whether the signal is interpreted using two different lead wires or using one lead wire (e.g., one signal having two frequency spikes that represent the amount of two different analytes present in the fluid sample).

[0172] Test unit 9110a also advantageously includes a first sealing surface 9134 and a second sealing surface 9135, configured to restrict entry of moisture into the interior of cartridge 9100 via slots 9132 and 9133, respectively. Test unit 9110a is disposed at the beginning of the order of use of the plurality of test units 9110 in cartridge 9100 (i.e., on top of the stack of test units 9110, see FIG. 33). As such, test unit 9110a serves to protect the plurality of test units 9110 from damage caused by moisture and dust. Test unit 9110a can either be a "sacrificial unit," meaning its sole purpose is to provide a cork/seal to the orifices of cartridge 9100, or can optionally include analyte sensors, such as analyte sensor 9115a. Test unit 9110a also preferably includes a sealing surface on its back side to provide a seal at slot 9129. It is also contemplated that each of the plurality of test units 9110 can include sealing surfaces to protect each subsequent test unit from moisture.

[0173] While FIG. 35 shows test unit 9110a having a "strip" configuration, those of skill in the art will appreciate that other shapes can be used consistently with the inventive subject matter disclosed herein. For example, test unit 9110a could comprise a capsule or a disk rather than a strip. However, stackable test units are preferred in order to conserve space.

[0174] FIG. 36 shows a test unit 9110b, which has two analyte sensors 9115b and 9116b. Sensor 9115b is configured to detect glucose, while sensor 9116b is configured to detect fructosamine. Test unit 9110b advantageously provides a means for testing for two analytes using one blood sample (i.e., from a single prick and a single test unit). While FIG. 36 shows sensors 9115b and 9116b in completely non-overlapping positions, it is also contemplated that sensors 9115b and 9116b could be partially overlapping, or even completely overlapping. For example, sensors 9115b and 9116b could comprise one absorbent material and one analyte-binding reagent, wherein the analyte-binding reagent is capable of simultaneously binding with two or more analytes and can produce two "distinct" signals (e.g., one signal with two different detectible frequency spikes, or two different signals representing two distinct analytes). One of skill in the art will

also appreciate that additional sensors can be included on test unit 9110b for detecting additional analytes.

[0175] Test unit 9110a and test unit 9110b are "functionally nonfungible" since unit 9110a tests for glucose while unit 9110b detects glucose and fructosamine. An example of two functionally fungible test units is a first test unit that test for glucose and iron, and a second test unit that tests for glucose and iron.

[0176] FIG. 37 shows a test unit 9110c, which has two analyte sensors 9115c and 9116c. Sensor 9115c is configured to detect glucose, while calibration sensor 9116c is configured to check the accuracy of an analyte testing device. As such, sensor 9115c is an "operational sensor" and sensor 9116c is a "calibration sensor." Sensor 9116c has a known concentration of a particular analyte and produces a signal that is expected to result in a known reading on device 9600. In this manner, the electronics of device 9600 can be checked for accuracy, precision, and consistency.

[0177] FIG. 38 shows an analyte testing device 9600. Device 9600 is a glucose meter integrated with a lancing device. Device 9600 has an actuator 9620 and an internal linkage mechanism (not shown) configured to cock a lancet for drawing blood, partially expose a test unit for contacting with a blood sample, and reading a signal of the test unit. Device 9600 also has an internal compartment 9610 for loading and storing cartridge 9100. Device 9600 also preferably has an internal compartment for storing a cartridge of lancets (not shown). In this exemplary embodiment, the actuator is mechanically advantaged and the step of operating the actuator comprises cocking a lever. Device 9600 can further include a docking station and data management software.

[0178] In one aspect of the disclosed technology, an analyte testing device includes an analyte sensor module configured to hold a sensor cartridge structured to store analyte sensors, the analyte sensor module including an opening from which an analyte sensor advances to a testing position to expose at least a portion of the analyte sensor to outside of the analyte testing device; a lancet module configured to hold a lancet cartridge structured to store lancets; and an actuator, in which the actuator includes a button, a first linking component coupled to the button and the analyte sensor module, in which the first linking component moves in response to a movement of the button including a movement between a first position and a second position or a movement between the second position and a third position, a second linking component coupled to the button and the lancet module, in which the second linking component moves in response to a movement of the button between the first position and the second position, a third linking component coupled to the second linking component and moveable in response to a movement of the second linking component, and a lancet projecting component coupled to the third linking component, in which a single operation of the button moves the analyte sensor to the testing position and moves the lancet projecting component from an initial position to a cocked position for projecting a lancet.

[0179] Implementations of the analyte testing device can optionally include one or more of the following exemplary features. For example, the device can include a door covering the opening and coupled to the first linking component, in which the door moves to uncover the opening based on a movement of the first linking component. The button of the actuator of the device can be configured as a sliding button. The single operation can include the sliding of the button from the first position to the second position. The button can

be positioned on the analyte testing device to allow the single operation to be carried out using a single hand holding the device. The lancet cartridge of the device can be structured to include a hollowed chamber for each lancet in the lancet cartridge, the hollowed chamber including an opening structured to allow the lancet projecting component to enter the chamber and impact the lancet for projection, a terminal opening structured to allow a needle component of the lancet to project out of the device, and a track to control a projection path of the lancet. The projection path of the device can be structured to be substantially straight to within a particular tolerance, thereby reducing wobble of the needle component as the lancet is projected out of the device. The actuator of the device can further include a depth adjustment component structured to include a knob located on the external side of the device connected to a plurality of steps of different lengths disposed within the device, in which one step is positioned in the projection path within the hollowed chamber to reduce the distance of projection of the lancet. The actuator of the device can further include a firing button located on the exterior of the device and coupled to the lancet projecting component when the lancet projecting component is in the cocked position. The device can include a second operation that includes the activation of the firing button to release the lancet projecting component to impact the lancet for projection. The analyte sensor of the device can be disposed in a test strip. The analyte sensor of the device can receive a testing sample from a user in the testing position. The analyte sensor of the device can be ejected from the device by a third operation that includes the movement of the button from the second position to the third position. The button of the actuator of the device can be configured as a sliding button that includes two separable buttons including a first button and a second button, in which the first button returns back to the first position after the movement of the button between the first position and the second position, and the second button is moved from the second position to the third position in the third operation. The actuator of the device can further include a button stop mechanism that prevents the button from returning to the first position when the single operation is initiated and not completed. The analyte sensor module of the device can further include a temperature sensor to monitor temperature in the analyte sensor module. The device can further include a first facility configured to transmit at least one of (a) a data obtained from the analyte sensor and (b) information derived from the data out of the analyte testing device using at least one wireless protocol. The device can further include a second facility configured to transmit at least one of the data and information derived from the data out of the analyte testing device using a wired path. The device can further include a processor configured to correlate individual instances of at least one of the data obtained from the analyte sensor and information derived from the data with (a) time stamps and optionally (b) user entered information selected from the group consisting of speech and text. The device can further include a processor configured to evaluate at least one of the data obtained from the analyte sensor and information derived from the data, and to send a notification to a recipient. The device can further include a processor configured to keep track of inventory of lancets and analyte sensors, both within and outside the device. The processor can be configured to reorder inventory of lancets and analyte sensors. The device can further include a processor configured to store voice recordings of diary information selected from the group con-

sisting of supplies used or ordered, food eaten, exercise, medication taken, and estimated calories burned. The device can further include a processor configured to produce a prompt to direct a user to use the device according to at least one of a selected time and a selected time interval. The device can further include an LCD touch screen display, a first work light positioned to illuminate a lancet exit hole, and a second work light positioned to illuminate an analyte sensor exit slot. The device can be included in a system, in which the system can include a docking station that provides power and data connectivity to the device. The device can be included in a system, in which the system can include a visual interface external to the device, through which a user can view and input data. The device can further include a pedometer communicatively coupled with a processor configured to calculate a distance traveled and an amount of calories burned associated with the distance traveled. The device can further include a personal emergency response system (PERS) that includes a button for alerting a third party. The PERS can be configured to perform one or more of the following, e.g., including contact a third party, identify the device, provide health data associated with a user of the device, automatically contact a third party in response to health data associated with a user of the device, notify a third party as an urgency level of an emergency, and determine identity of a third party to be contacted.

**[0180]** In another aspect of the disclosed technology, a method for using an analyte testing device includes in a first operation, operating a button located on the exterior of an analyte testing device to advance an analyte sensor within a sensor cartridge of the analyte testing device to expose at least a portion of the analyte sensor outside of the analyte testing device and to advance a lancet projecting component of the analyte testing device from an initial position to a cocked position for a subsequent projection of a lancet; in a second operation, operating a firing button located on the exterior of an analyte testing device to advance the lancet projecting component to contact the lancet to project the lancet from the analyte testing device; and in a third operation, operating the button to eject the analyte sensor from the device, in which the first operation, second operation, and third operation are implemented using a single hand holding the device.

**[0181]** In another aspect of the disclosed technology, a method for operating an analyte testing device in testing an analyte includes advancing an analyte sensor from a first position within a sensor cartridge of an analyte testing device to a second position to expose at least a portion of the analyte sensor outside of the device; advancing a lancet projecting component of the analyte testing device from an initial position to a cocked position for a subsequent projection of a lancet, in which the advancing the analyte sensor and the advancing the lancet projecting component are initiated by a single operation; operating the lancet projecting component to project the lancet outside of the device; operating the device to contact the analyte sensor with a testing sample containing the analyte at the exposed portion of the analyte sensor; operating the device to process the testing sample to determine a parameter of the analyte; and ejecting the analyte sensor from the device.

**[0182]** Implementations of the method can optionally include one or more of the following exemplary features. For example, the method can be implemented using a single hand holding the device. The single operation can include sliding a button located on an external side of the analyte testing

device. The method can further include advancing a lancet cartridge from a previous position within the analyte testing device to a readied position in which the lancet is aligned with the lancet projection component in the cocked position, in which the advancing the lancet cartridge is initiated by the single operation. Implementations of the method can include the lancet being automatically retracted back into the lancet cartridge. The method can further include operating a lancet depth adjustment component to position a step structure disposed within the device in a projection path of the lancet to control the distance of projection of the lancet. Implementations of the method can include the lancet being projected substantially straight to within a particular tolerance, thereby reducing wobble of the lancet during projection.

**[0183]** While the disclosed embodiments are described herein primarily based on glucose monitoring to facilitate understanding of the underlying concepts, it is understood that the disclosed embodiments can also include monitoring of other analytes that include, but are not limited to, fructosamine, hematocrit, hemoglobin blood oxygen saturation, lactates, iron, pH, cholesterol, liver enzymes (e.g., AST, ALT, ALP/GGT, LDH, bilirubin, etc.), hormones, and other compounds. For example, other biomolecular substances can also be monitored using analytical monitoring techniques of the disclosed embodiments, which include, but are not limited to, nucleic acids, lipids, carbohydrates, peptides, proteins, enzymes, hormones, antibodies, glycoproteins, glycolipids, organelles, endotoxins, and viruses, among other biological materials and biomarkers.

**[0184]** As used herein, and unless the context dictates otherwise, the term “coupled to” is intended to include both direct coupling (in which two elements that are coupled to each other contact each other) and indirect coupling (in which at least one additional element is located between the two elements). Therefore, the terms “coupled to” and “coupled with” are used synonymously.

**[0185]** It should be apparent to those skilled in the art that many more modifications besides those already described are possible without departing from the inventive concepts herein. The inventive subject matter, therefore, is not to be restricted except in the scope of the appended claims. Moreover, in interpreting both the specification and the claims, all terms should be interpreted in the broadest possible manner consistent with the context. In particular, the terms “comprises” and “comprising” should be interpreted as referring to elements, components, or steps in a non-exclusive manner, indicating that the referenced elements, components, or steps may be present, or utilized, or combined with other elements, components, or steps that are not expressly referenced. Where the specification claims refers to at least one of something selected from the group consisting of A, B, C . . . and N, the text should be interpreted as requiring only one element from the group, not A plus N, or B plus N, etc.

**[0186]** While this patent document contains many specifics, these should not be construed as limitations on the scope of any invention or of what may be claimed, but rather as descriptions of features that may be specific to particular embodiments of particular inventions. Certain features that are described in this patent document in the context of separate embodiments can also be implemented in combination in a single embodiment. Conversely, various features that are described in the context of a single embodiment can also be implemented in multiple embodiments separately or in any suitable subcombination. Moreover, although features may

be described above as acting in certain combinations and even initially claimed as such, one or more features from a claimed combination can in some cases be excised from the combination, and the claimed combination may be directed to a subcombination or variation of a subcombination.

**[0187]** Similarly, while operations are depicted in the drawings in a particular order, this should not be understood as requiring that such operations be performed in the particular order shown or in sequential order, or that all illustrated operations be performed, to achieve desirable results. Moreover, the separation of various system components in the embodiments described in this patent document should not be understood as requiring such separation in all embodiments.

**[0188]** Only a few implementations and examples are described and other implementations, enhancements and variations can be made based on what is described and illustrated in this patent document.

What is claimed is:

1. A method for operating an analyte testing device in testing an analyte, comprising:
  - advancing an analyte sensor from a first position within a sensor cartridge of an analyte testing device to a second position to expose at least a portion of the analyte sensor outside of the device;
  - advancing a lancet projecting component of the analyte testing device from an initial position to a cocked position for a subsequent projection of a lancet, wherein the advancing the analyte sensor and the advancing the lancet projecting component are initiated by a single operation;
  - operating the lancet projecting component to project the lancet outside of the device;
  - operating the device to contact the analyte sensor with a testing sample containing the analyte at the exposed portion of the analyte sensor;
  - operating the device to process the testing sample to determine a parameter of the analyte; and
  - ejecting the analyte sensor from the device.
2. The method of claim 1, wherein the single operation includes sliding a button located on an external side of the device.
3. The method of claim 1, wherein the parameter includes the concentration level of the analyte.
4. The method of claim 1, wherein the projecting the lancet outside of the device punctures flesh of a user to draw blood to test glucose concentration in the blood.
5. The method of claim 1, further comprising advancing a lancet cartridge from a previous position within the analyte testing device to a readied position in which the lancet is aligned with the lancet projection component in the cocked position, wherein the advancing the lancet cartridge is initiated by the single operation.
6. The method of claim 1, wherein the lancet is automatically retracted back into the lancet cartridge.
7. The method of claim 1, wherein the method is implemented using a single hand holding the device.
8. The method of claim 1, further comprising operating a lancet depth adjustment component to position a step structure disposed within the device in a projection path of the lancet to control the distance of projection of the lancet.
9. The method of claim 1, wherein the lancet is projected substantially straight to within a particular tolerance, thereby reducing wobble of the lancet during projection.

- 10.** An analyte testing device, comprising:  
 an analyte sensor module configured to hold a sensor cartridge structured to store analyte sensors, the analyte sensor module including an opening from which an analyte sensor advances to a testing position to expose at least a portion of the analyte sensor to outside of the analyte testing device;  
 a lancet module configured to hold a lancet cartridge structured to store lancets; and  
 an actuator including:  
 a button,  
 a first linking component coupled to the button and the analyte sensor module, wherein the first linking component moves in response to a movement of the button including a movement between a first position and a second position or a movement between the second position and a third position,  
 a second linking component coupled to the button and the lancet module, wherein the second linking component moves in response to a movement of the button between the first position and the second position,  
 a third linking component coupled to the second linking component and moveable in response to a movement of the second linking component, and  
 a lancet projecting component coupled to the third linking component,  
 wherein a single operation of the button moves the analyte sensor to the testing position and moves the lancet projecting component from an initial position to a cocked position for projecting a lancet.
- 11.** The device of claim **10**, further comprising a door covering the opening and coupled to the first linking component, wherein the door moves to uncover the opening based on a movement of the first linking component.
- 12.** The device of claim **10**, wherein the button is a sliding button, and the single operation includes the sliding of the button from the first position to the second position.
- 13.** The device of claim **10**, wherein the button is positioned on the analyte testing device to allow the single operation to be carried out using a single hand holding the device.
- 14.** The device of claim **10**, wherein the lancet cartridge is structured to include a hollowed chamber for each lancet in the lancet cartridge, the hollowed chamber including an opening structured to allow the lancet projecting component to enter the chamber and impact the lancet for projection, a terminal opening structured to allow a needle component of the lancet to project out of the device, and a track to control a projection path of the lancet.
- 15.** The device of claim **14**, wherein the projection path is structured to be substantially straight to within a particular tolerance, thereby reducing wobble of the needle component as the lancet is projected out of the device.
- 16.** The device of claim **14**, wherein the actuator further includes a depth adjustment component structured to include a knob located on the external side of the device connected to a plurality of steps of different lengths disposed within the device, wherein one step is positioned in the projection path within the hollowed chamber to reduce the distance of projection of the lancet.
- 17.** The device of claim **10**, wherein the actuator further includes a firing button located on the exterior of the device and coupled to the lancet projecting component when the lancet projecting component is in the cocked position, and a

second operation includes the activation of the firing button to release the lancet projecting component to impact the lancet for projection.

**18.** The device of claim **10**, wherein the analyte sensor is disposed in a test strip and receives a testing sample from a user in the testing position.

**19.** The device of claim **10**, wherein the analyte sensor is ejected from the device by a third operation that includes the movement of the button from the second position to the third position.

**20.** The device of claim **19**, wherein the button is a sliding button that includes two separable buttons including a first button and a second button, wherein the first button returns back to the first position after the movement of the button between the first position and the second position, and the second button is moved from the second position to the third position in the third operation, and wherein the actuator further includes a button stop mechanism that prevents the button from returning to the first position when the single operation is initiated and not completed.

**21.** The device of claim **10**, wherein the analyte sensor module further includes a temperature sensor to monitor temperature in the analyte sensor module.

**22.** The device of claim **10**, further comprising one or both of:

a first facility configured to transmit at least one of data obtained from the analyte sensor or information derived from data out of the analyte testing device using at least one wireless protocol, or

a second facility configured to transmit at least one of the data obtained from the analyte sensor or the information derived from the data out of the analyte testing device using a wired path.

**23.** The device of claim **10**, further comprising a processor, the processor configured to perform one or more of the following:

correlate individual instances of at least one of data obtained from the analyte sensor or information derived from data out of the analyte testing device with (a) time stamps and optionally (b) user entered information selected from the group consisting of speech and text, evaluate at least one of data obtained from the analyte sensor or information derived from data out of the analyte testing device, and to send a notification to a recipient,

keep track of inventory of lancets and analyte sensors, both within and outside the device, wherein the processor is configured to reorder inventory of lancets and analyte sensors,

store voice recordings of diary information selected from the group consisting of supplies used or ordered, food eaten, exercise, medication taken, and estimated calories burned, or

produce a prompt to direct a user to use the device according to at least one of a selected time or a selected time interval.

**24.** The device of claim **10**, further comprising an LCD touch screen display, a first work light positioned to illuminate a lancet exit hole, and a second work light positioned to illuminate an analyte sensor exit slot.

**25.** The device of claim **10** included in a system, the system comprising a visual interface external to the device, through which a user can view and input data.

**26.** The device of claim **10**, further comprising a pedometer communicatively coupled with a processor configured to calculate a distance traveled and an amount of calories burned associated with the distance traveled.

**27.** The device of claim **10**, further comprising a personal emergency response system (PERS) that includes a button for alerting a third party, wherein the PERS is configured to perform one or more of the following:

- contact a third party,
- identify the device,
- provide health data associated with a user of the device,
- automatically contact a third party in response to health data associated with a user of the device,
- notify a third party as an urgency level of an emergency, or
- determine identity of a third party to be contacted.

**28.** A method for using an analyte testing device, comprising:

- in a first operation, operating a button located on the exterior of an analyte testing device to advance an analyte sensor within a sensor cartridge of the analyte testing device to expose at least a portion of the analyte sensor outside of the analyte testing device and to advance a lancet projecting component of the analyte testing

device from an initial position to a cocked position for a subsequent projection of a lancet;

in a second operation, operating a firing button located on the exterior of an analyte testing device to advance the lancet projecting component to contact the lancet to project the lancet from the analyte testing device; and

in a third operation, operating the button to eject the analyte sensor from the device,

wherein the first operation, second operation, and third operation are implemented using a single hand holding the device.

**29.** The method of claim **28**, wherein the operating the button in the first operation includes moving the button from a first position to a second position on the exterior of the analyte testing device, and the operating the button in the third operation includes moving the button from the second position to a third position on the exterior of the analyte testing device.

**30.** The method of claim **28**, wherein, in the first operation, the operating further includes advancing a lancet cartridge from a previous position within the analyte testing device to a readied position in which the lancet is aligned with the lancet projection component in the cocked position.

\* \* \* \* \*

专利名称(译)	分析仪测试设备		
公开(公告)号	<a href="#">US20130245392A1</a>	公开(公告)日	2013-09-19
申请号	US13/868831	申请日	2013-04-23
[标]申请(专利权)人(译)	优菲米特有限责任公司		
申请(专利权)人(译)	YOFIMETER, LLC		
当前申请(专利权)人(译)	YOFIMETER, LLC		
[标]发明人	SHAANAN GAD GOLDMAN MARC		
发明人	SHAANAN, GAD GOLDMAN, MARC		
IPC分类号	A61B5/151 A61B5/00 A61B5/15 A61B5/145 A61B5/11		
CPC分类号	A61B5/15113 A61B5/15174 A61B5/15194 A61B5/150022 A61B5/157 A61B5/150175 A61B5/14532 A61B5/15148 A61B5/1513 A61B5/0004 A61B5/150824 A61B5/742 A61B5/1118 A61B5/746 A61B5 /150267 A61B5/150961 A61B5/150358 A61B5/150412 A61B5/15117 A61B5/15153 A61B5/145 A61B5 /15087 G01N33/48757		
其他公开文献	US8961432		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

公开了用于实现分析物测试装置的致动器机构的系统，装置，技术和方法。在一个方面，测试分析物的方法包括将分析物传感器从分析物测试装置的传感器盒内的第一位置推进到第二位置，该第二位置将分析物传感器的至少一部分暴露在装置外部，推进刺血针将组件从初始位置投射到竖起位置以用于随后的刺血针投射，其中推进分析物传感器和推进刺血针突出组件通过单次操作启动，突出刺血针以暴露至少一部分刺血针。在装置外部的刺血针，接收包括分析物传感器的暴露部分处的分析物的测试样品，处理测试样品以确定分析物的参数，以及从装置中喷射分析物传感器。

