



US 20170296126A1

(19) **United States**

(12) **Patent Application Publication**  
**OKUYA et al.**

(10) **Pub. No.: US 2017/0296126 A1**

(43) **Pub. Date: Oct. 19, 2017**

(54) **BIOLOGICAL SIGNAL MEASUREMENT SYSTEM**

*A61B 5/16* (2006.01)  
*A61B 5/00* (2006.01)  
*A61B 5/00* (2006.01)

(71) Applicant: **Panasonic Intellectual Property Management Co., Ltd., Osaka (JP)**

(52) **U.S. Cl.**  
CPC ..... *A61B 5/7203* (2013.01); *A61B 5/6822* (2013.01); *A61B 5/026* (2013.01); *A61B 5/6829* (2013.01); *A61B 5/6826* (2013.01); *A61B 5/6824* (2013.01); *A61B 5/01* (2013.01); *A61B 5/6821* (2013.01); *A61B 5/4266* (2013.01); *A61B 5/165* (2013.01); *A61B 5/0478* (2013.01); *A61B 2560/0247* (2013.01); *A61B 2562/0209* (2013.01)

(72) Inventors: **Teruhisa OKUYA, Osaka (JP); Tomomi NAKAGAWA, Osaka (JP); Keita YOSHIMURA, Osaka (JP); Mikio IWAKAWA, Osaka (JP)**

(21) Appl. No.: **15/437,666**

(22) Filed: **Feb. 21, 2017**

(30) **Foreign Application Priority Data**

Apr. 14, 2016 (JP) ..... 2016-081482

**Publication Classification**

(51) **Int. Cl.**  
*A61B 5/00* (2006.01)  
*A61B 5/026* (2006.01)  
*A61B 5/00* (2006.01)  
*A61B 5/00* (2006.01)  
*A61B 5/0478* (2006.01)  
*A61B 5/01* (2006.01)  
*A61B 5/00* (2006.01)  
*A61B 5/00* (2006.01)

(57) **ABSTRACT**

A biological signal measurement system includes: a biological signal measurer that measures a biological signal including external noise of biological noise and of environmental noise; biological noise measurer that measures a signal including the biological noise; a biological noise estimator that estimates the biological noise from the signal measured by the biological noise measurer; an environmental noise measurer that measures a signal including the environmental noise; an environmental noise estimator that estimates the environmental noise from the signal measured by the environmental noise measurer; and a calculator that calculates the biological signal in consideration of an effect of the external noise using the signal measured by the biological signal measurer, the biological noise estimated by the biological noise estimator and the environmental noise estimated by the environmental noise estimator.

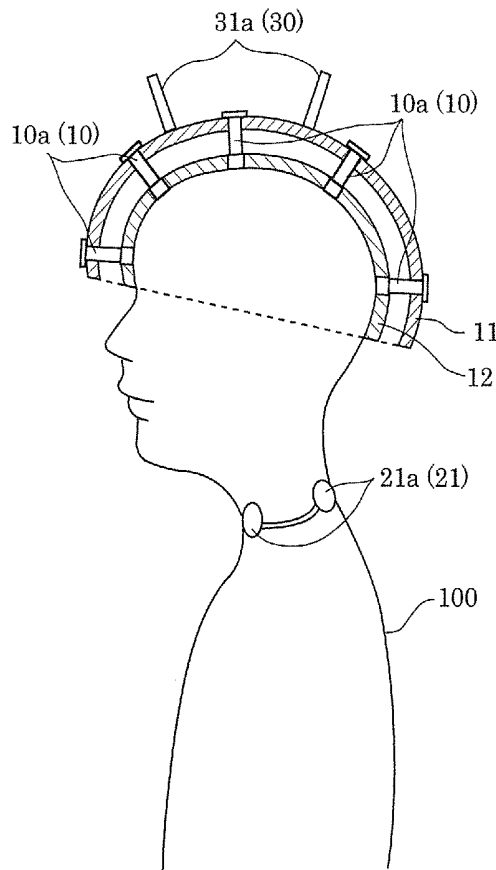


FIG. 1

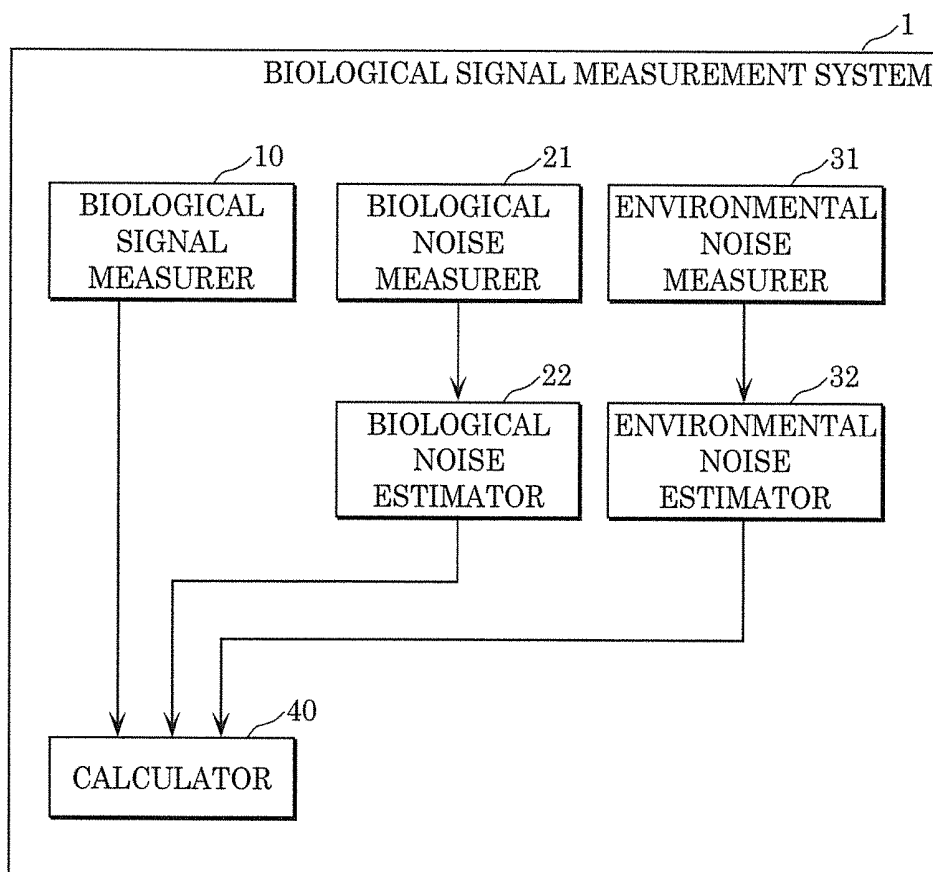


FIG. 2

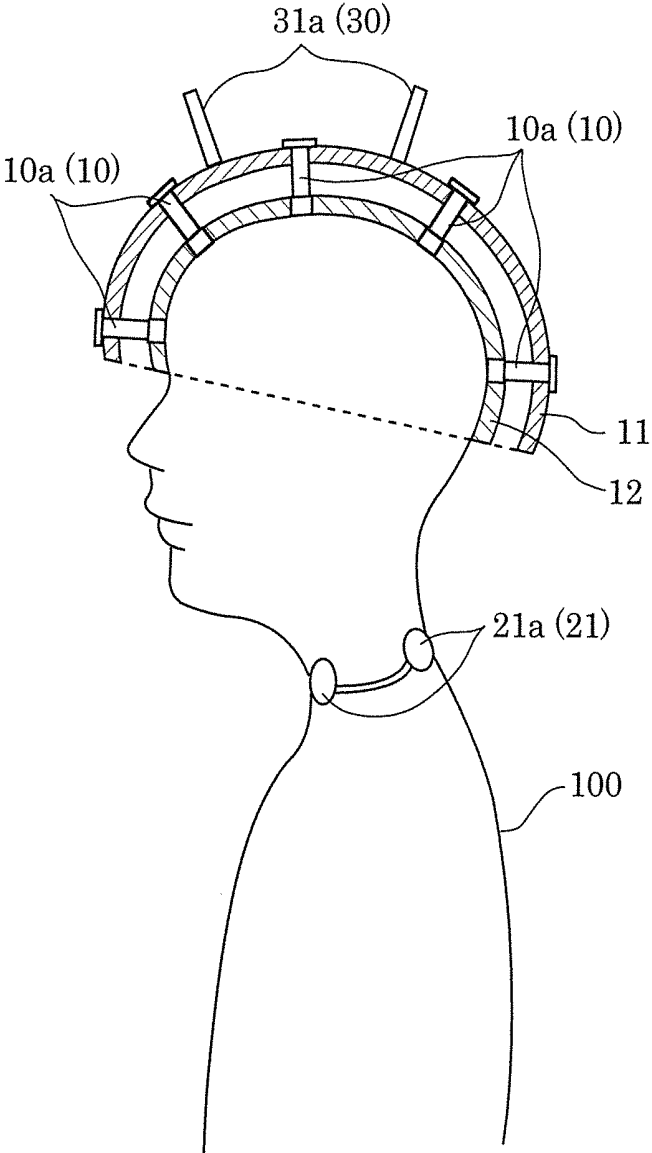


FIG. 3

BIOLOGICAL INFORMATION TO BE MEASURED	BRAIN WAVES (NO NOISE INCLUDED)
BIOLOGICAL SIGNAL MEASURER	BRAIN WAVES (NOISE INCLUDED)
BIOLOGICAL NOISE MEASURER	MYOELECTRIC POTENTIAL OF LIVING BODY (SUCH AS SWALLOWING SPIT, MOVING NECK)
ENVIRONMENTAL NOISE MEASURER	MAGNETIC OR RADIO NOISE GENERATED BY PERIPHERAL EQUIPMENT

FIG. 4

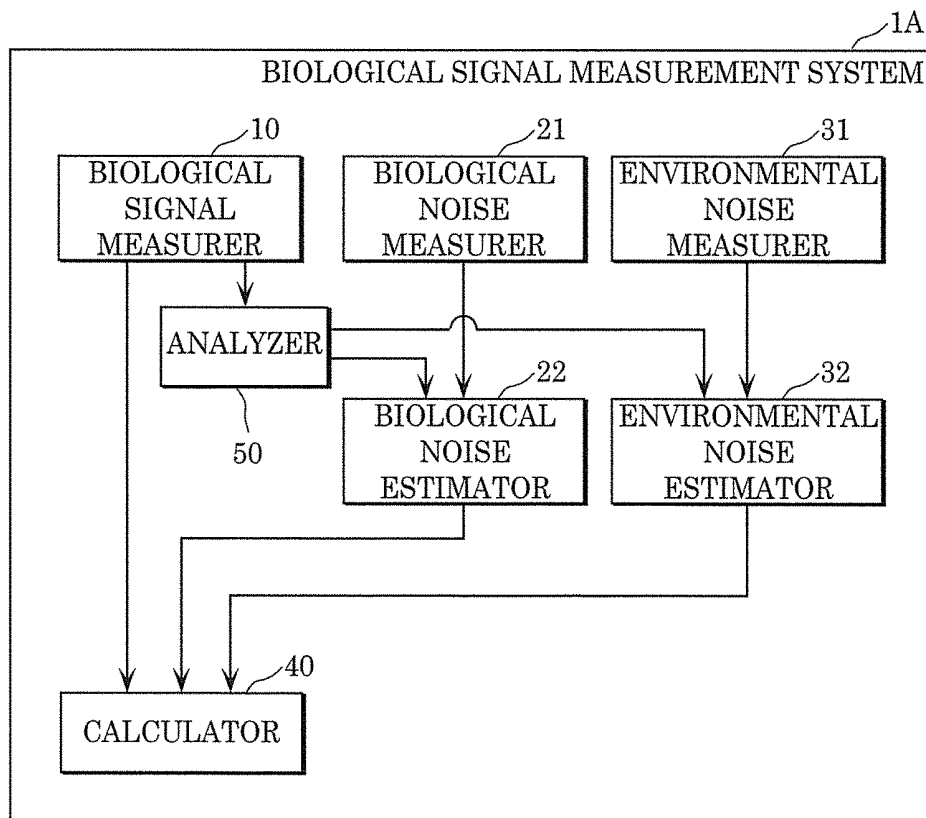


FIG. 5

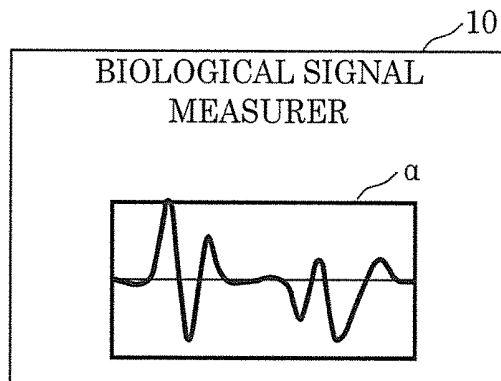


FIG. 6

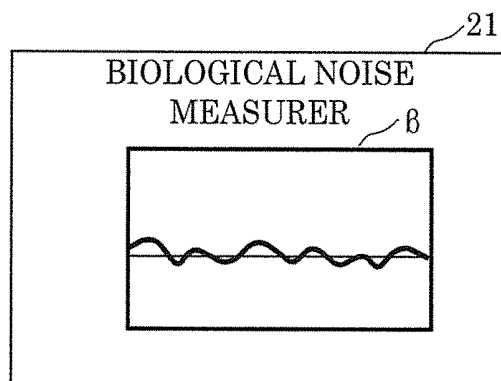


FIG. 7

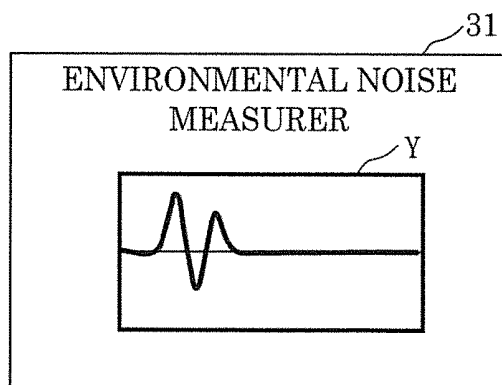


FIG. 8

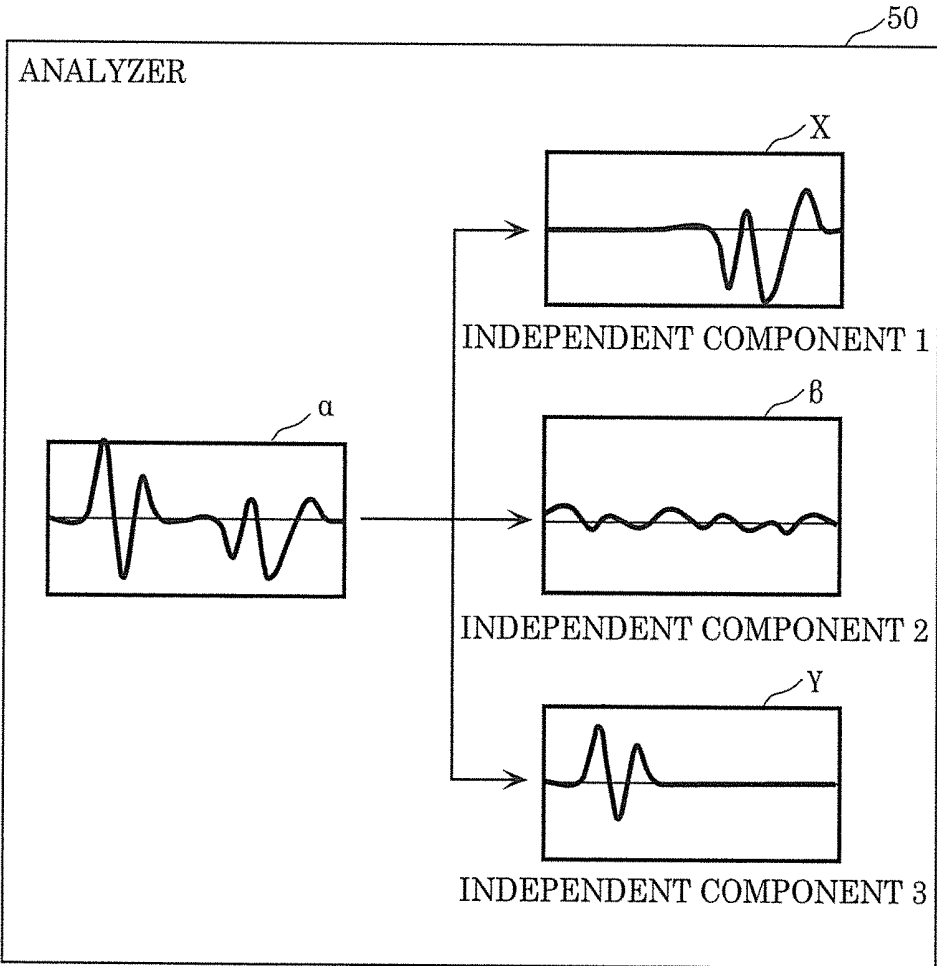


FIG. 9

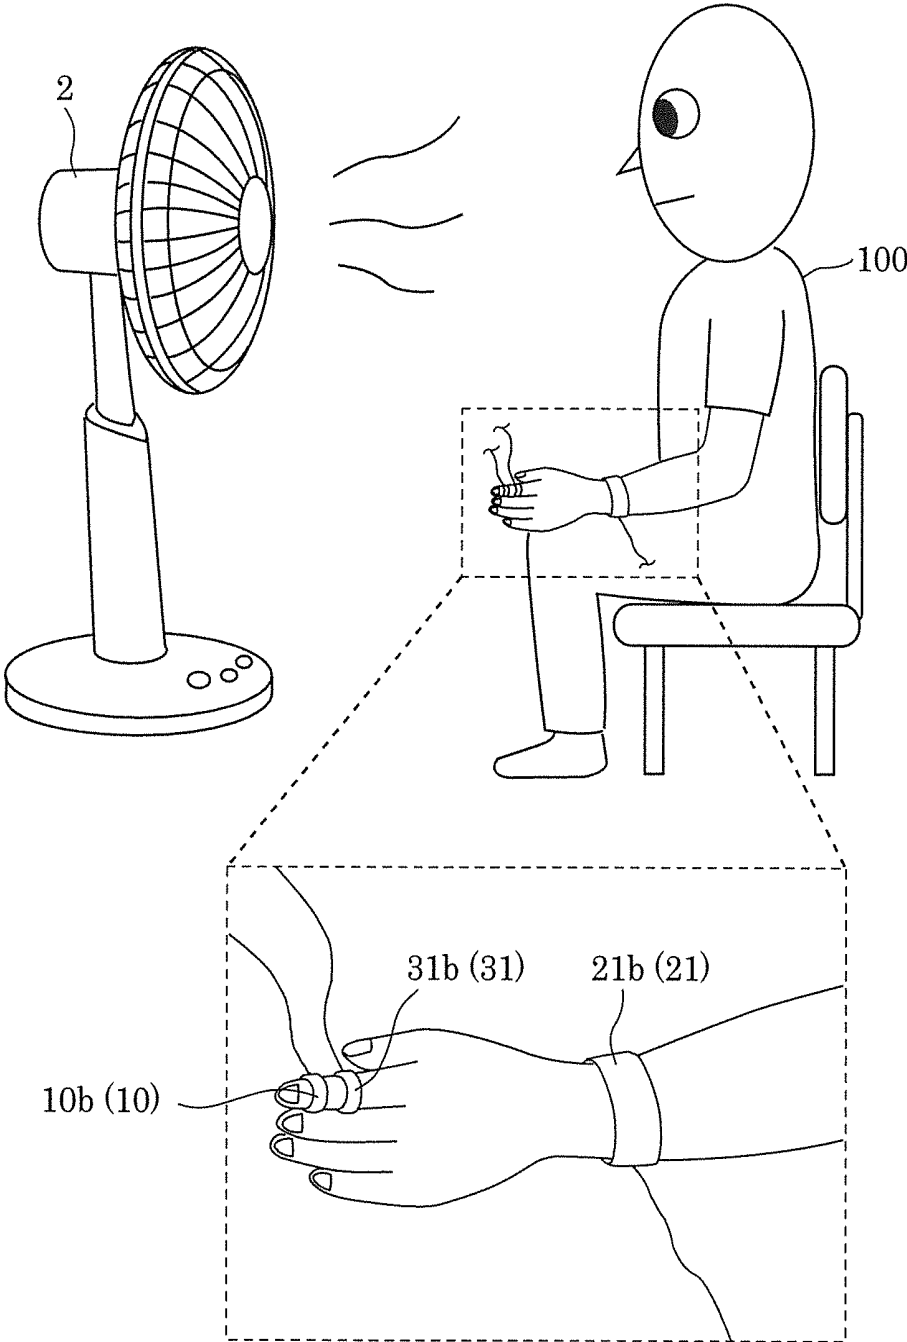


FIG. 10

	A	B	C	D
BIOLOGICAL INFORMATION TO BE MEASURED	SYMPATHETIC NERVE ACTIVITY, PARASYMPATHETIC NERVE ACTIVITY			
BIOLOGICAL SIGNAL MEASURER	FINGERTIP TEMPERATURE	NOSE TEMPERATURE	INSTEP TEMPERATURE	FOOT FINGERTIP TEMPERATURE
BIOLOGICAL NOISE MEASURER	WRIST TEMPERATURE BACK OF HAND TEMPERATURE	FOREHEAD TEMPERATURE	ANKLE TEMPERATURE	ANKLE TEMPERATURE INSTEP TEMPERATURE
ENVIRONMENTAL NOISE MEASURER	TEMPERATURE, HUMIDITY, AIR CURRENT, RADIANT HEAT			

FIG. 11

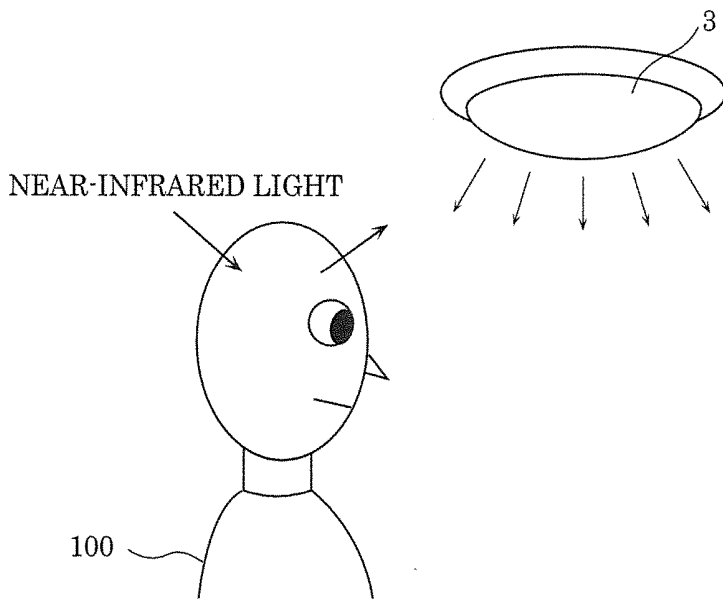


FIG. 12

BIOLOGICAL INFORMATION TO BE MEASURED	BRAIN ACTIVITY
BIOLOGICAL SIGNAL MEASURER	CHANGE IN ABSORBANCE OF PORTION OF ATTENTION (CHANGE IN BLOOD VOLUME)
BIOLOGICAL NOISE MEASURER	CHANGE IN ABSORBANCE OF WHOLE BRAIN (CHANGE IN BLOOD VOLUME)
ENVIRONMENTAL NOISE MEASURER	CHANGE IN LIGHTING IN MEASUREMENT ENVIRONMENT CHANGE IN INCIDENCE ANGLE TO MEASURING PROBE

FIG. 13

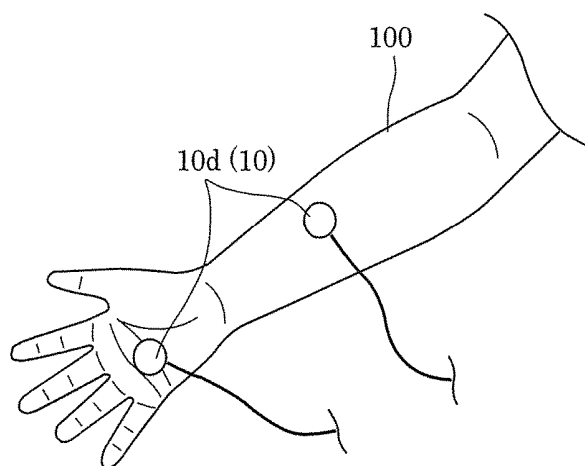


FIG. 14

BIOLOGICAL INFORMATION TO BE MEASURED	EMOTIONAL SWEATING (NO NOISE INCLUDED)
BIOLOGICAL SIGNAL MEASURER	AMOUNT OF EMOTIONAL SWEATING (SPL) (NOISE INCLUDED)
BIOLOGICAL NOISE MEASURER	AMOUNT OF EMOTIONAL SWEATING DUE TO CHANGE IN BODY TEMPERATURE
ENVIRONMENTAL NOISE MEASURER	TEMPERATURE, WIND SPEED, RADIANT HEAT

## BIOLOGICAL SIGNAL MEASUREMENT SYSTEM

### CROSS REFERENCE TO RELATED APPLICATION

[0001] This application claims the benefit of priority of Japanese Patent Application Number 2016-081482 filed on Apr. 14, 2016, the entire content of which is hereby incorporated by reference.

### BACKGROUND

#### 1. Technical Field

[0002] The present disclosure relates to a biological signal measurement system.

#### 2. Description of the Related Art

[0003] A conventional biological signal measurement system for measuring biological signals such as brain waves is known. In this type of biological signal measurement system, in order to obtain a biological signal of a user with a high S/N ratio, a technique to reduce or remove a noise component from the measured biological signal has been proposed.

[0004] For instance, in Japanese Unexamined Patent Application Publication No. 2004-154512, a noise component is reduced from the a biological signal such as a heart-rate signal, a pulse signal or a respiration signal using a signal amplification shaper including a signal amplification circuit and a bandpass filter. Specifically, a measured biological signal is amplified by a signal amplification circuit, and only signals with frequencies (for instance, approximately 7 Hz to approximately 30 Hz) necessary for measuring the intensity of a biological signal are passed by a bandpass filter, thereby reducing noise components other than the biological signal.

### SUMMARY

[0005] Using the method disclosed by Japanese Unexamined Patent Application Publication No. 2004-154512, it is possible to reduce environmental noise which is not originating from a user (subject). The environmental noise includes, for instance, a signal with approximately 1 Hz caused by wind, a signal with 50 to 60 Hz coming from a fluorescent lamp, a signal with 300 Hz or higher in sound, and low frequency noise with 20 to 300 Hz coming from a construction site or a factory.

[0006] However, external noise in various frequency bands is superimposed on a measured biological signal. Specifically, not only environmental noise which is not originating from a user, but also biological noise which is originating from a user may be superimposed on a measured biological signal. The biological noise includes, for instance, noise caused by tooth grinding of a user during measurement of a biological signal.

[0007] The present disclosure solves such a problem and it is an object to provide a biological signal measurement system capable of obtaining a biological signal with a high S/N ratio in consideration of the effect of external noise of biological noise and of environmental noise.

[0008] In order to achieve the above-mentioned object, one aspect of the present disclosure provides a biological signal measurement system including: a biological signal

measurer that measures a biological signal including external noise of biological noise and of environmental noise; a biological noise measurer that measures a signal including the biological noise; a biological noise estimator that estimates the biological noise from the signal measured by the biological noise measurer; an environmental noise measurer that measures a signal including the environmental noise; an environmental noise estimator that estimates the environmental noise from the signal measured by the environmental noise measurer; and a calculator that calculates a biological signal in consideration of an effect of the external noise, using the biological signal measured by the biological signal measurer, the biological noise estimated by the biological noise estimator and the environmental noise estimated by the environmental noise estimator.

[0009] It is possible to obtain a biological signal with a high S/N ratio in consideration of the effect of the external noise of the biological noise and of the environmental noise.

### BRIEF DESCRIPTION OF DRAWINGS

[0010] The figures depict one or more implementations in accordance with the present teaching, by way of examples only, not by way of limitations. In the figures, like reference numerals refer to the same or similar elements.

[0011] FIG. 1 is a block diagram illustrating the configuration of a biological signal measurement system according to Embodiment 1;

[0012] FIG. 2 is an illustration schematically depicting the manner in which a biological signal of a user is measured using the biological signal measurement system according to Embodiment 1;

[0013] FIG. 3 is a table illustrating examples of signals which are measured using the biological signal measurement system according to Embodiment 1;

[0014] FIG. 4 is a block diagram illustrating the configuration of a biological signal measurement system according to a modification of Embodiment 1;

[0015] FIG. 5 is a graph illustrating an example of a signal measured by a biological signal measurer in the biological signal measurement system according to the modification of Embodiment 1;

[0016] FIG. 6 is a graph illustrating an example of a signal measured by a biological noise measurer in the biological signal measurement system according to the modification of Embodiment 1;

[0017] FIG. 7 is a graph illustrating an example of a signal measured by an environmental noise measurer in the biological signal measurement system according to the modification of Embodiment 1;

[0018] FIG. 8 illustrates graphs for explaining the operation of an analyzer in the biological signal measurement system according to the modification of Embodiment 1;

[0019] FIG. 9 is an illustration schematically depicting the manner in which a biological signal of a user is measured using a biological signal measurement system according to Embodiment 2;

[0020] FIG. 10 is a table illustrating examples of signals measured by using the biological signal measurement system according to Embodiment 2;

[0021] FIG. 11 is an illustration schematically depicting the manner in which a biological signal of a user is measured using a biological signal measurement system according to Embodiment 3;

[0022] FIG. 12 is a table illustrating examples of signals measured by using the biological signal measurement system according to Embodiment 3;

[0023] FIG. 13 is an illustration schematically depicting the manner in which a biological signal of a user is measured using a biological signal measurement system according to Embodiment 4; and

[0024] FIG. 14 is a table illustrating examples of signals measured by using the biological signal measurement system according to Embodiment 4.

#### DETAILED DESCRIPTION OF THE EMBODIMENTS

[0025] Hereinafter, an embodiment of the present disclosure will be described. It is to be noted that each of the embodiments described below illustrates a specific example of the present disclosure. Therefore, the numerical values, components, arrangement positions and connection configuration of the components, steps, and order of the steps that are presented in the following embodiments are examples, which are not intended to limit the present disclosure. In the following embodiments, the components thereof, which are not recited in the independent claims that define the most generic concept of the present disclosure, are described as arbitrary structural components.

[0026] It is to be noted that the respective figures are schematic diagrams and are not necessarily precise illustrations. Furthermore, in the respective figures, the same reference sign is given to substantially identical components, and a redundant description is omitted or simplified.

#### Embodiment 1

[0027] First, biological signal measurement system 1 according to Embodiment 1 will be described using FIG. 1 to FIG. 3. FIG. 1 is a block diagram illustrating the configuration of biological signal measurement system 1 according to Embodiment 1. FIG. 2 is an illustration schematically depicting the manner in which a biological signal of user 100 is measured using biological signal measurement system 1. FIG. 3 is a table illustrating examples of signals which are measured using biological signal measurement system 1.

[0028] As illustrated in FIG. 1, biological signal measurement system 1 in this embodiment includes biological signal measurer 10, biological noise measurer 21, biological noise estimator 22, environmental noise measurer 31, environmental noise estimator 32, and calculator 40.

[0029] Biological signal measurement system 1 is a system that measures a biological signal related to a living body like a human, such as brain waves, pulsation, cardiac beat, electrocardiogram, breathing, perspiration, a temperature at a portion or a blood flow volume, and thereby analyzes biological information on the living body. As illustrated in FIG. 3, in this embodiment, the target piece of biological information to be measured is brain waves including no noise. For instance, as illustrated in FIG. 2, the brain waves of user (subject) 100 are measured as a biological signal.

[0030] Biological signal measurer 10 is a device, for instance, for measuring a target biological signal of user 100 to be measured. Biological signal measurer 10 measures a biological signal including external noise of biological noise and of environmental noise. The biological noise and the environmental noise included in the biological signal mea-

sured by biological signal measurer 10 may be zero in some cases. In other words, in the biological signal of user 100 measured by biological signal measurer 10, the external noise of the biological noise and of the environmental noise is included as zero (in short, no external noise is included) in some cases.

[0031] When brain waves are measured as a biological signal as in this embodiment, for instance, biological signal measurer 10 may have a configuration that uses electrodes 10a attachable to the head of user 100 as illustrated in FIG. 2. For instance, biological signal measurer 10 has a plurality of electrodes 10a mounted on fixing tool 11 so that electrodes 10a come into contact with a scalp, and measures a potential difference between the plurality of electrodes 10a, thereby measuring the brain waves of user 100. On the measured brain waves, the external noise of the biological noise and of the environmental noise is superimposed.

[0032] It is to be noted that fixing tool 11 is, for instance, a helmet or the like to be attached to the head of user 100. As illustrated in FIG. 2, insulator 12 composed of an insulating rubber or the like is provided in fixing tool 11 so as to cover the head and come into contact with the scalp.

[0033] The external noise included in the biological signal measured is noise component other than the target biological signal to be measured. The external noise includes biological noise which is originating from a living body, and environmental noise which is not originating from a living body.

[0034] In this embodiment, the biological noise is the noise originating from a user 100 when a biological signal is measured by the biological signal measurer 10. For instance, the biological noise is noise originating from a myoelectric potential of a living body. On the other hand, the environmental noise is noise which is not originated from user 100 when a biological signal is measured by biological signal measurer 10. For instance, the environmental noise is noise which is originated from a factor such as peripheral equipment or a temperature in measurement environment.

[0035] Biological noise measurer 21 measures a signal which includes biological noise. When brain waves are measured as biological signal, biological noise measurer 21 may have a configuration that uses electrodes 21a attachable to the vicinity of at least one of the throat, an eye, and a temple of user 100. In this embodiment, biological noise measurer 21 has a plurality of electrodes 21a which are attached so as to come into contact with the throat of user 100, and measures a potential difference between the plurality of electrodes 21a, thereby measuring biological noise which is originated from a myoelectric potential of user 100 (living body) and occurs when user 100 grinds the tooth, when user 100 swallows spit or when user 100 moves the head.

[0036] It is to be noted that for a biological signal measured by biological signal measurer 10, each electrode 21a may be disposed in the vicinity of a portion (a source of biological noise) where biological noise is more likely to occur. For this reason, in this embodiment, in order to measure biological noise originating from a myoelectric potential when user 100 grinds the tooth, electrode 21a may be disposed in the vicinity of the throat of user 100, for instance. Also, it is possible to measure biological noise originating from a myoelectric potential when user 100 grinds the tooth by disposing electrode 21a in the vicinity of a temple of user 100. In addition, it is possible to measure biological noise originating from a myoelectric potential

when user **100** blinks by disposing electrode **21a** in the vicinity of an eye of user **100**.

**[0037]** Biological noise estimator **22** estimates biological noise from the signal measured by biological noise measurer **21**. In this embodiment, biological noise estimator **22** estimates the biological noise to be a first signal ( $b \times B$ ) which is obtained by multiplying the signal ( $B$ ) measured by biological noise measurer **21** by a first constant ( $b$ ).

**[0038]** Environmental noise measurer **31** measures a signal which includes environmental noise. When brain waves are measured as a biological signal as in this embodiment, environmental noise measurer **31** measures environmental noise originating from magnetism and radio waves generated by peripheral equipment (such as a lighting device, an AC adapter) present in the environment of brain wave measurement. For instance, as illustrated in FIG. 2, environmental noise measurer **31** may have a configuration that uses electrodes **31a** attachable to the head of user **100**. In this embodiment, environmental noise measurer **31** has a plurality of electrodes **31a** mounted on fixing tool **11** so that electrodes **31a** come into no contact with the scalp, and measures a potential difference between the plurality of electrodes **31a**, thereby measuring environmental noise. Electrodes **31a** are formed so as not to come into contact with the scalp by insulator **12** provided in fixing tool **11**, and thus are electrically separated from Electrode **21a** and the living body.

**[0039]** It is to be noted that environmental noise measurer **31** may measure the environmental noise at a portion near user **100** (living body). Thus, for a biological signal measured by biological signal measurer **10**, electrodes **31a** may be disposed in the vicinity of a portion (a source of environmental noise) where environmental noise is more likely to occur. For instance, electrodes **31a** may be disposed at a portion near electrodes **10a**.

**[0040]** Environmental noise estimator **32** estimates environmental noise from the signal measured by environmental noise measurer **31**. In this embodiment, environmental noise estimator **32** estimates the environmental noise to be a second signal ( $c \times C$ ) which is obtained by multiplying the signal ( $C$ ) measured by environmental noise measurer **31** by a second constant ( $c$ ).

**[0041]** Calculator **40** calculates a biological signal in consideration of the effect of the external noise of the biological noise and of the environmental noise using the signal measured by biological signal measurer **10**, the biological noise estimated by biological noise estimator **22** and the environmental noise estimated by environmental noise estimator **32**.

**[0042]** In this embodiment, calculator **40** calculates a biological signal in consideration of the effect of the external noise by subtracting the first signal ( $b \times B$ ) which is the biological noise estimated by biological noise estimator **22** and the second signal ( $c \times C$ ) which is the environmental noise estimated by environmental noise estimator **32** from signal ( $A$ ) measured by biological signal measurer **10**.

**[0043]** In this manner, in this embodiment, the external noise of the biological noise and of the environmental noise is removed from the biological signal measured by biological signal measurer **10** by a removal method using subtraction. Specifically, the biological noise and the environmental noise are estimated to be a certain number of times a signal including the biological noise measured by biological noise measurer **21** and a signal including the environmental noise

measured by environmental noise measurer **31**, and the estimated biological noise and environmental noise are removed from the biological signal measured by biological signal measurer **10**.

**[0044]** Specifically, let  $A$  be the biological signal measured by biological signal measurer **10**,  $B$  be the signal including the biological noise measured by biological noise measurer **21**, and  $C$  be the signal including the environmental noise measured by environmental noise measurer **31**, then the biological noise is estimated to be  $b \times B$  using the first constant  $b$  and the environmental noise is estimated to be  $c \times C$  using the second constant  $c$ , and biological signal  $X$  is derived from the following (Expressions 1).

$$\text{Biological signal } X = A - b \times B - c \times C \quad (\text{Expression 1})$$

**[0045]** In this embodiment, biological signal  $X$  is calculated as needed in real time. It is to be noted that a frequency filter may be pre-applied to the value of each signal measured by biological signal measurer **10**, biological noise measurer **21** and environmental noise measurer **31**. For instance, environmental noise with 50 Hz or higher coming from a fluorescent lamp or the like may be pre-removed by a frequency filter.

**[0046]** As described above, biological signal measurement system **1** in this embodiment includes: a biological signal measurer **10** that measures a biological signal including external noise of biological noise and of environmental noise; biological noise measurer **21** that measures a signal including the biological noise; biological noise estimator **22** that estimates the biological noise from signal measured by biological noise measurer **21**; environmental noise measurer **31** that measures a signal including the environmental noise; environmental noise estimator **32** that estimates the environmental noise from the signal measured by environmental noise measurer **31**; and calculator **40** that calculates the biological signal in consideration of the effect of the external noise using the signal measured by biological signal measurer **10**, the biological noise estimated by biological noise estimator **22** and the environmental noise estimated by environmental noise estimator **32**.

**[0047]** In this manner, in this embodiment, the biological signal excluding the external noise is obtained by removing the estimated biological noise and environmental noise from the signal measured by biological signal measurer **10**. Consequently, it is possible to obtain a biological signal with a high S/N ratio in consideration of the effect of the external noise of the biological noise and of the environmental noise.

**[0048]** Also, in this embodiment, biological noise estimator **22** estimates the biological noise to be the first signal ( $b \times B$ ) which is obtained by multiplying the signal ( $B$ ) measured by biological noise measurer **21** by the first constant ( $b$ ), and environmental noise estimator **32** estimates the environmental noise to be the second signal ( $c \times C$ ) which is obtained by multiplying the signal ( $C$ ) measured by environmental noise measurer **31** by the second constant ( $c$ ). Then calculator **40** calculates a biological signal in consideration of the effect of the external noise by subtracting the first signal ( $b \times B$ ) estimated by biological noise estimator **22** and the second signal ( $c \times C$ ) estimated by environmental noise estimator **32** from signal ( $A$ ) measured by biological signal measurer **10**.

**[0049]** Thus, a biological signal excluding the external noise can be obtained by a removal method using subtraction.

tion. Therefore, it is possible to obtain a biological signal with a high S/N ratio, excluding the external noise.

#### Modification of Embodiment 1

**[0050]** Next, biological signal measurement system 1A according to a modification of Embodiment 1 will be described using FIG. 4. FIG. 4 is a block diagram illustrating the configuration of biological signal measurement system 1A according to a modification of Embodiment 1.

**[0051]** Biological signal measurement system 1A in this modification and biological signal measurement system 1 in Embodiment 1 differ in the method of removing the external noise from the biological signal measured by biological signal measurer 10.

**[0052]** Specifically, in biological signal measurement system 1 in Embodiment 1, the biological signal excluding the external noise is obtained by the removal method using subtraction, whereas in biological signal measurement system 1A in this modification, the biological signal excluding the external noise is obtained by independent component analysis. Specifically, in this modification, out of signals which are adapted to the signal measured by biological signal measurer 10 and are separated from biological signal measurer 10, a signal similar to each of the biological noise and the environmental noise is treated as external noise which is excluded from the biological signal measured by biological signal measurer 10. It is to be noted that similarly to Embodiment 1, in this modification, the target piece of biological information to be measured is brain waves.

**[0053]** As illustrated in FIG. 4, in addition to biological signal measurement system 1 of Embodiment 1 illustrated in FIG. 1, biological signal measurement system 1A in this modification includes analyzer 50 that performs the independent component analysis on the signal measured by biological signal measurer 10.

**[0054]** In this modification, biological noise estimator 22 estimates the biological noise to be an independent component similar to the signal measured by biological noise measurer 21 out of independent components as a result of signal separation by analyzer 50.

**[0055]** In addition, environmental noise estimator 32 estimates the environmental noise to be an independent component similar to the signal measured by environmental noise measurer 31 out of independent components as a result of signal separation by analyzer 50.

**[0056]** Then calculator 40 removes the biological noise estimated by biological noise estimator 22 and the environmental noise estimated by environmental noise estimator 32 from the signal measured by biological signal measurer 10, then calculates a biological signal excluding the biological noise and the environmental noise.

**[0057]** Here, a specific method of measuring a biological signal using biological signal measurement system 1A in this modification will be described using FIG. 5 to FIG. 8. FIG. 5 to FIG. 7 illustrate examples of respective signals measured by biological signal measurer 10, biological noise measurer 21 and environmental noise measurer 31 in biological signal measurement system 1A in this modification. FIG. 8 illustrates graphs for explaining the operation of analyzer 50 in biological signal measurement system 1A.

**[0058]** For instance, it is assumed that signal  $\alpha$  with a waveform illustrated in FIG. 5 is measured by biological signal measurer 10, signal  $\beta$  with a waveform illustrated in FIG. 6 is measured by biological noise measurer 21, and

signal  $\gamma$  with a waveform illustrated in FIG. 7 is measured by environmental noise measurer 31.

**[0059]** In this case, the independent component analysis is performed on signal  $\alpha$  measured by biological signal measurer 10 by analyzer 50, and for instance, as illustrated in FIG. 8, signal  $\alpha$  measured by biological signal measurer 10 is thereby separated into three signals: independent component 1, independent component 2, and independent component 3.

**[0060]** Based on the result of signal separation performed by analyzer 50, the biological noise and the environmental noise included in signal  $\alpha$  measured by biological signal measurer 10 are estimated.

**[0061]** Specifically, in biological noise estimator 22, the result of signal separation by analyzer 50 is compared with signal  $\beta$  measured by biological noise measurer 21, and an independent component most similar to signal  $\beta$  measured by biological noise measurer 21 out of three independent components resulting from the signal separation by analyzer 50 is estimated to be the biological noise. In this modification, independent component 2 is the most similar to signal  $\beta$  measured by biological noise measurer 21 out of the three independent components: independent component 1, independent component 2, and independent component 3 illustrated in FIG. 8. Thus, it is estimated that independent component 2 is the biological noise.

**[0062]** Also, in environmental noise estimator 32, the result of signal separation by analyzer 50 is compared with signal  $\gamma$  measured by environmental noise measurer 31, and an independent component most similar to signal  $\gamma$  measured by environmental noise measurer 31 out of three independent components resulting from the signal separation by analyzer 50 is estimated to be the environmental noise. In this modification, independent component 3 is the most similar to the signal measured by environmental noise measurer 31 out of the three independent components: independent component 1, independent component 2, and independent component 3 illustrated in FIG. 8. Thus, it is estimated that independent component 3 is the environmental noise.

**[0063]** Consequently, out of the three independent components, independent component 1, independent component 2, and independent component 3 illustrated in FIG. 8, independent component 1 can be determined to be the target biological signal to be acquired, that is, biological signal X excluding the external noise of the biological noise and of the environmental noise.

**[0064]** The determination is made by calculation of calculator 40. Specifically, signal  $\beta$  of the biological noise estimated by biological noise estimator 22 and signal  $\gamma$  of the environmental noise estimated by environmental noise estimator 32 are removed from signal  $\alpha$  measured by biological signal measurer 10 by calculator 40, and biological signal X is thereby derived.

**[0065]** It is to be noted that in this modification, when signal  $\alpha$ , signal  $\beta$  and signal  $\gamma$  are compared to each other, the values of the signals at a certain point are not compared, but the waveforms of the signals in a certain range are compared. Therefore, in this modification, for signal  $\alpha$ , signal  $\beta$  and signal  $\gamma$ , it is necessary to obtain signals (waveform signals) in a predetermined time range by biological signal measurer 10, biological noise measurer 21 and environmental noise measurer 31.

[0066] As described above, similarly to Embodiment 1, biological signal measurement system 1A in this modification includes biological signal measurer 10, biological noise measurer 21, biological noise estimator 22, environmental noise measurer 31, environmental noise estimator 32 and calculator 40. Calculator 40 calculates a biological signal in consideration of the effect of the external noise of the biological noise and of the environmental noise using the signal measured by biological signal measurer 10, the biological noise estimated by biological noise estimator 22, and the environmental noise estimated by environmental noise estimator 32.

[0067] In this manner, similarly to Embodiment 1, in this modification, the estimated biological noise and environmental noise are excluded from the signal measured by biological signal measurer 10, and thus the biological signal excluding the external noise is obtained. Thus, it is possible to obtain a biological signal with a high S/N ratio in consideration of the effect of the external noise of the biological noise and of the environmental noise.

[0068] Also, in this modification, analyzer 50 is provided that performs the independent component analysis of the signal measured by biological signal measurer 10. Biological noise estimator 22 then estimates the biological noise to be an independent component similar to the signal measured by biological noise measurer 21 out of independent components as a result of signal separation by analyzer 50. In addition, environmental noise estimator 32 estimates the environmental noise to be an independent component similar to the signal measured by environmental noise measurer 31 out of independent components as a result of signal separation by analyzer 50. Furthermore, calculator 40 removes estimated biological noise and environmental noise from the signal measured by biological signal measurer 10, then calculates a biological signal excluding the biological noise and the environmental noise.

[0069] Thus, a biological signal excluding the external noise can be obtained by the independent component analysis. Therefore, it is possible to obtain a biological signal with a high S/N ratio, excluding the external noise.

#### Embodiment 2

[0070] Next, a biological signal measurement system according to Embodiment 2 will be described using FIG. 9 and FIG. 10. FIG. 9 is an illustration schematically depicting the manner in which a biological signal of user 100 is measured using the biological signal measurement system according to Embodiment 2. FIG. 10 is a table illustrating examples of signals measured by using the biological signal measurement system.

[0071] The configuration of the biological signal measurement system in this embodiment is the same as the configuration of the biological signal measurement system in Embodiment 1 and modification. For instance, in this embodiment, similarly to Embodiment 1 and modification, each technique of the removal method using subtraction and the independent component analysis can be used. Therefore, the configuration of the biological signal measurement system in this embodiment is the same as the configuration of biological signal measurement systems 1 and 1A illustrated in FIG. 1 and FIG. 4, for instance.

[0072] In this embodiment and Embodiment 1, target pieces of biological information to be measured are different. Specifically, the target piece of biological information to

be measured is brain waves in Embodiment 1. However, in this embodiment, as illustrated in FIG. 10, the target piece of biological information to be measured is sympathetic nerve activity and parasympathetic nerve activity. Specifically, as illustrated in FIG. 9, the biological signal measurement system in this embodiment has a purpose of quantifying the stress (lassitude) of user 100 when receiving the wind of electric fan 2, and measures the activity of the sympathetic nerve and the parasympathetic nerve of user 100.

[0073] In this case, in general, it is believed that the temperature of a hand fingertip reflects the sympathetic nerve activity and parasympathetic nerve activity, and thus the sympathetic nerve activity and parasympathetic nerve activity can be measured by measuring the temperature of a hand fingertip.

[0074] However, the temperature of a fingertip is also affected by the biological noise and the environmental noise. These biological noise and environmental noise affect the temperature of a fingertip as external noise. For instance, the temperature of a wrist and the temperature of the back of a hand affect the temperature of a fingertip as biological noise. In addition, the temperature, humidity, air current (wind speed) and radiant heat affect the temperature of a fingertip as environmental noise.

[0075] Thus, similarly to Embodiment 1, in this embodiment, the biological signal of user 100 is measured as well as the biological noise and the environmental noise are measured, and thus only the biological signal with the external noise removed is obtained.

[0076] Specifically, when the temperature of a hand fingertip is measured as a biological signal, biological signal measurer 10 may be attachable to a hand fingertip of user 100. For instance, as illustrated in FIG. 9, biological signal measurer 10 has thermometer 10b attachable to a hand fingertip of user 100, and the temperature of a hand fingertip of user 100 is measured by thermometer 10b.

[0077] In this case, biological noise measurer 21 may be attachable to at least one of a wrist and the back of a hand of user 100. For instance, as illustrated in FIG. 9, biological noise measurer 21 has thermometer 21b attachable to a wrist of user 100, and the temperature of a wrist of user 100 is measured by thermometer 21b. It is to be noted that biological noise measurer 21 is not limited to be attachable to a wrist and the back of a hand of user 100, and may be attachable to a palm or a first joint of a finger.

[0078] As illustrated in FIG. 9, environmental noise measurer 31 has measuring instrument 31b attachable to a hand fingertip of user 100, and the temperature, humidity, air current and radiant heat are measured as environmental noise in the measurement environment by measuring instrument 31b. It is to be noted that environmental noise measurer 31 may not be attachable to a hand fingertip of user 100.

[0079] In this embodiment, biological noise estimator 22, environmental noise estimator 32 and calculator 40 are the same as those in Embodiment 1 and the modification. Specifically, biological noise estimator 22 estimates the biological noise from the signal measured by biological noise measurer 21, and environmental noise estimator 32 estimates the environmental noise from the signal measured by environmental noise measurer 31. Calculator 40 then calculates a biological signal in consideration of the effect of the external noise of the biological noise and of the environmental noise using the signal measured by biological

signal measurer **10**, the biological noise estimated by biological noise estimator **22**, and the environmental noise estimated by environmental noise estimator **32**.

**[0080]** In this embodiment, when the sympathetic nerve activity and the parasympathetic nerve activity are measured, the biological signal to be measured by biological signal measurer **10** is a signal related to the temperature of a hand fingertip. However, without being limited to this, the biological signal to be measured by biological signal measurer **10** may be, for instance, the temperature of the nose, an instep or a foot fingertip as illustrated in FIG. **10**. The sympathetic nerve activity and the parasympathetic nerve activity can be measured by the temperature of the nose, an instep or a foot fingertip. In this case, a portion at which the temperature is measured by biological noise measurer **21** can be selected as needed according to a portion at which a biological signal is measured as illustrated by the combinations of A to D of FIG. **10**. Specifically, biological noise measurer **21** may be attachable to at least one of an ankle, an instep and the forehead of user **100**.

**[0081]** As described above, similarly to Embodiment 1, in the biological-signal measurement system in this embodiment, the estimated biological noise and environmental noise are excluded from the signal measured by biological signal measurer **10**, and thus the biological signal excluding the external noise is obtained. Thus, it is possible to obtain a biological signal with a high S/N ratio in consideration of the effect of the external noise of the biological noise and of the environmental noise.

**[0082]** Particularly, in this embodiment, the sympathetic nerve activity and the parasympathetic nerve activity in relation to wind can be measured with high accuracy.

### Embodiment 3

**[0083]** Next, a biological signal measurement system according to Embodiment 3 will be described using FIG. **11** and FIG. **12**. FIG. **11** is an illustration schematically depicting the manner in which a biological signal of user **100** is measured using the biological signal measurement system according to Embodiment 3. FIG. **12** is a table illustrating examples of signals measured by using the biological signal measurement system.

**[0084]** The configuration of the biological signal measurement system in this embodiment is the same as the configuration of the biological signal measurement system in Embodiment 1 and the modification. For instance, also in this embodiment, similarly to Embodiment 1 and the modification, each technique of the removal method using subtraction and the independent component analysis can be used. Therefore, the configuration of the biological signal measurement system in this embodiment is the same as the configuration of biological signal measurement systems **1** and **1A** illustrated in FIG. **1** and FIG. **4**, for instance.

**[0085]** In this embodiment and Embodiment 1, target pieces of biological information to be measured are different. Specifically, the target piece of biological information to be measured is brain waves in Embodiment 1. However, in this embodiment, as illustrated in FIG. **12**, the target piece of biological information to be measured is brain activity. This embodiment has a purpose of quantifying the brain activity by recognizing change in the cerebral blood flow by light using Near-infrared Spectroscopy (NIRS).

**[0086]** In this embodiment, as a biological signal, biological signal measurer **10** measures change (change in blood

flow volume) in the absorbance of portion of attention by the NIRS. Specifically, as illustrated in FIG. **11**, the head of user **100** is irradiated with near-infrared light, and change in the degree (absorbance) of absorption of near-infrared light is measured. A change in the absorbance can be measured by a measuring probe.

**[0087]** Also, as a biological noise, biological noise measurer **21** measures change (change in blood flow volume) in the absorbance of the whole brain by the NIRS. For instance, biological noise measurer **21** measures change in the absorbance of the whole brain from the arteries of the neck. In this case, the arterial area of the neck of user **100** is irradiated with near-infrared light, and change in the degree (absorbance) of absorption of near-infrared light is measured by a measuring probe.

**[0088]** Also, as environmental noise, environmental noise measurer **31** measures change in lighting of lighting device **3** in the measurement environment. In this case, as environmental noise, environmental noise measurer **31** may further measure change in the incidence angle of the measuring probe when change in the absorbance is measured by biological signal measurer **10** and biological noise measurer **21**. That is, measurement of change in the incidence angle of the measuring probe allows change of the effect of the light received from lighting device **3** due to tilting of the head of user **100** to be measured.

**[0089]** In this embodiment, biological noise estimator **22**, environmental noise estimator **32** and calculator **40** are the same as those in Embodiment 1. Specifically, biological noise estimator **22** estimates the biological noise from the signal measured by biological noise measurer **21**, and environmental noise estimator **32** estimates the environmental noise from the signal measured by environmental noise measurer **31**. Calculator **40** then calculates a biological signal in consideration of the effect of the external noise of the biological noise and of the environmental noise using the signal measured by biological signal measurer **10**, the biological noise estimated by biological noise estimator **22**, and the environmental noise estimated by environmental noise estimator **32**.

**[0090]** As described above, similarly to Embodiment 1, in the biological-signal measurement system in this embodiment, the estimated biological noise and environmental noise are excluded from the signal measured by biological signal measurer **10**, and thus the biological signal excluding the external noise is obtained. Thus, it is possible to obtain a biological signal with a high S/N ratio in consideration of the effect of the external noise of the biological noise and of the environmental noise.

**[0091]** Particularly, in this embodiment, brain activity can be measured with high accuracy by the NIRS.

### Embodiment 4

**[0092]** Next, the biological signal measurement system according to Embodiment 4 will be described using FIG. **13** and FIG. **14**. FIG. **13** is an illustration schematically depicting the manner in which a biological signal of user **100** is measured using a biological signal measurement system according to Embodiment 4. FIG. **14** is a table illustrating examples of signals measured by using the biological signal measurement system according to Embodiment 4.

**[0093]** The configuration of the biological signal measurement system in this embodiment is the same as the configuration of the biological signal measurement system in

Embodiment 1 and the modification. For instance, also in this embodiment, similarly to Embodiment 1 and the modification, each technique of the removal method using subtraction and the independent component analysis can be used. Therefore, the configuration of the biological signal measurement system in this embodiment is the same as the configuration of biological signal measurement systems 1 and 1A illustrated in FIG. 1 and FIG. 4, for instance.

[0094] In this embodiment and Embodiment 1, target pieces of biological information to be measured are different. Specifically, the target piece of biological information to be measured is brain waves in Embodiment 1. However, in this embodiment, as illustrated in FIG. 14, the target piece of biological information to be measured is emotional sweating. This embodiment has a purpose of quantifying the emotional sweating by identifying an amount of emotional sweating using a specific frequency.

[0095] In this embodiment, as a biological signal, biological signal measurer 10 measures a signal related to emotional sweating. Specifically, biological signal measurer 10 measures an amount of emotional sweating of user 100 by measuring a skin potential level (SPL). For instance, as illustrated in FIG. 13, biological signal measurer 10 has a plurality of electrodes 10*d* attachable to a palm and an arm of user 100, and measures a potential difference between the plurality of electrodes 10*d*, thereby measuring a skin potential level as an amount of emotional sweating of user 100.

[0096] Also, as biological noise, biological noise measurer 21 measures an amount of emotional sweating due to change in the body temperature of user 100. For instance, biological noise measurer 21 measures an amount of emotional sweating at the chest of user 100.

[0097] Also, as environmental noise, environmental noise measurer 31 measures the temperature, wind speed, and radiant heat in the measurement environment. For instance, biological noise measurer 21 measures the temperature, wind speed, and radiant heat by the same method as in Embodiment 2.

[0098] In this embodiment, biological noise estimator 22, environmental noise estimator 32 and calculator 40 are the same as those in Embodiment 1. Specifically, biological noise estimator 22 estimates the biological noise from the signal measured by biological noise measurer 21, and environmental noise estimator 32 estimates the environmental noise from the signal measured by environmental noise measurer 31. Calculator 40 then calculates a biological signal in consideration of the effect of the external noise of the biological noise and of the environmental noise using the signal measured by biological signal measurer 10, the biological noise estimated by biological noise estimator 22, and the environmental noise estimated by environmental noise estimator 32.

[0099] As described above, similarly to Embodiment 1, in the biological-signal measurement system in this embodiment, the estimated biological noise and environmental noise are excluded from the signal measured by biological signal measurer 10, and thus the biological signal excluding the external noise is obtained. Thus, it is possible to obtain a biological signal with a high S/N ratio in consideration of the effect of the external noise of the biological noise and of the environmental noise.

[0100] Particularly, in this embodiment, emotional sweating (SPL) can be measured with high accuracy.

#### Other Modifications

[0101] Although the biological signal measurement system according to the present disclosure has been described based on the embodiments and the modification in the above, the present disclosure is not limited to the embodiments and the modification.

[0102] For instance, embodiments obtained by making various modifications, which occur to those skilled in the art, to the embodiments and the modification, and an embodiment implemented in any combination of the components and functions of the embodiments and modification in a range without departing from the scope of the present disclosure are also included in the present disclosure.

[0103] In the embodiments, the processing described as the operations of the following components can be executed by a computer: biological signal measurer 10, biological noise measurer 21, biological noise estimator 22, environmental noise measurer 31, environmental noise estimator 32, calculator 40, and analyzer 50. For instance, a computer executes a program using a processor (CPU), hardware resources such as a memory and an input/output circuit, thereby performing the aforementioned processing. Specifically, a processor obtains target data for processing from a memory or an input/output circuit to calculate the data, and outputs a calculation result to a memory or an input/output circuit, thereby performing the processing.

[0104] A program for executing the aforementioned processing may be recorded on a non-transitory recording medium such as a computer-readable CD-ROM. In this case, a computer reads a program from a non-transitory recording medium, and performs each processing by executing the program.

[0105] It is to be noted that the present disclosure can be implemented as a program for causing a computer to function as the biological signal measurement system, or as a computer-readable recording medium in which the program is stored.

[0106] While the foregoing has described one or more embodiments and/or other examples, it is understood that various modifications may be made therein and that the subject matter disclosed herein may be implemented in various forms and examples, and that they may be applied in numerous applications, only some of which have been described herein. It is intended by the following claims to claim any and all modifications and variations that fall within the true scope of the present teachings.

What is claimed is:

1. A biological signal measurement system comprising:
  - a biological signal measurer that measures a biological signal including external noise of biological noise and of environmental noise;
  - a biological noise measurer that measures a signal including the biological noise;
  - a biological noise estimator that estimates the biological noise from the signal measured by the biological noise measurer;
  - an environmental noise measurer that measures a signal including the environmental noise;
  - an environmental noise estimator that estimates the environmental noise from the signal measured by the environmental noise measurer; and
  - a calculator that calculates a biological signal in consideration of an effect of the external noise, using the biological signal measured by the biological signal

- measurer, the biological noise estimated by the biological noise estimator and the environmental noise estimated by the environmental noise estimator.
2. The biological signal measurement system according to claim 1,  
 wherein the biological noise estimator estimates the biological noise to be a first signal obtained by multiplying the biological signal measured by the biological noise measurer by a first constant,  
 the environmental noise estimator estimates the environmental noise to be a second signal obtained by multiplying the signal measured by the environmental noise measurer by a second constant, and  
 the calculator calculates the biological signal in consideration of the effect of the external noise by subtracting the first signal and the second signal from the biological signal measured by the biological signal measurer.
3. The biological signal measurement system according to claim 1, further comprising  
 an analyzer that performs independent component analysis of the biological signal measured by the biological signal measurer,  
 wherein the biological noise estimator estimates the biological noise to be an independent component most similar to the biological signal measured by the biological noise measurer out of at least one independent component as a result of signal separation by the analyzer,  
 the environmental noise estimator estimates the environmental noise to be an independent component most similar to the signal measured by the environmental noise measurer out of the at least one independent component as a result of signal separation by the analyzer, and  
 the calculator calculates a biological signal excluding the biological noise and the environmental noise by removing the estimated biological noise and the estimated environmental noise from the biological signal measured by the biological signal measurer.
4. The biological signal measurement system according to claim 1,  
 wherein the biological signal is brain waves,  
 the biological signal measurer has an electrode attachable to a head of a user, and  
 the biological noise measurer has an electrode attachable to a vicinity of at least one of a throat, an eye, and a temple of the user.
5. The biological signal measurement system according to claim 1,  
 wherein the biological signal is related to a temperature of at least one of a hand fingertip, the nose, an instep and a foot fingertip of a user,  
 the biological signal measurer is attachable to at least one of a hand fingertip, the nose, an instep and a foot fingertip of the user, and  
 the biological noise measurer is attachable to at least one of a wrist, a back of a hand, a palm, a first joint of a finger, a forehead, an ankle and an instep of the user.
6. The biological signal measurement system according to claim 1,  
 wherein the biological signal is related to a cerebral blood flow,  
 the biological signal measurer measures an absorbance at a point of attention of a head of a user, and  
 the biological noise measurer measures an absorbance of the whole brain of the user.
7. The biological signal measurement system according to claim 1,  
 wherein the biological signal is related to emotional sweating,  
 the biological signal measurer measures an amount of sweat produced by a user due to emotional sweating, and  
 the biological noise measurer measures an amount of sweat produced due to a change in body temperature of the user.

\* \* \* \* \*

专利名称(译)	生物信号测量系统		
公开(公告)号	<a href="#">US20170296126A1</a>	公开(公告)日	2017-10-19
申请号	US15/437666	申请日	2017-02-21
申请(专利权)人(译)	PANASONIC知识产权管理有限公司.		
当前申请(专利权)人(译)	PANASONIC知识产权管理有限公司.		
[标]发明人	OKUYA TERUHISA NAKAGAWA TOMOMI YOSHIMURA KEITA IWAKAWA MIKIO		
发明人	OKUYA, TERUHISA NAKAGAWA, TOMOMI YOSHIMURA, KEITA IWAKAWA, MIKIO		
IPC分类号	A61B5/00 A61B5/026 A61B5/0478 A61B5/01 A61B5/16		
CPC分类号	A61B5/7203 A61B5/0478 A61B5/6821 A61B5/6822 A61B5/01 A61B5/6824 A61B2562/0209 A61B5/6829 A61B5/026 A61B5/4266 A61B5/165 A61B2560/0247 A61B5/6826 A61B5/0205 A61B5/0476 A61B5/6814		
优先权	2016081482 2016-04-14 JP		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

一种生物信号测量系统，包括：生物信号测量器，测量包括生物噪声和环境噪声的外部噪声的生物信号；生物噪声测量器，测量包括生物噪声的信号；生物噪声估计器，用于估计生物噪声测量器测量的信号的生物噪声；环境噪声测量仪，测量包括环境噪声的信号；环境噪声估计器，用于估算环境噪声测量仪测量的信号的环境噪声；计算器，其使用由生物信号测量器测量的信号，由生物噪声估计器估计的生物噪声和由环境噪声估计器估计的环境噪声，考虑外部噪声的影响来计算生物信号。

