



US009254087B2

(12) **United States Patent**
Isaacson et al.

(10) **Patent No.:** **US 9,254,087 B2**
(45) **Date of Patent:** ***Feb. 9, 2016**

(54) **TISSUE CLAMP FOR NONINVASIVE
PHYSIOLOGICAL MEASUREMENT**

(71) Applicant: **Nonin Medical, Inc.**, Plymouth, MN
(US)

(72) Inventors: **Philip O. Isaacson**, Chanhassen, MN
(US); **Bryant Austin Jones**,
Minneapolis, MN (US); **Timothy L.
Johnson**, Plymouth, MN (US);
Christopher Holland, Mayer, MN (US);
Matthew Prior, Plymouth, MN (US)

(73) Assignee: **Nonin Medical, Inc.**, Plymouth, MN
(US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 130 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **14/223,033**

(22) Filed: **Mar. 24, 2014**

(65) **Prior Publication Data**
US 2014/0288388 A1 Sep. 25, 2014

Related U.S. Application Data

(63) Continuation of application No. 13/457,036, filed on
Apr. 26, 2012, now Pat. No. 8,695,206.

(60) Provisional application No. 61/479,544, filed on Apr.
27, 2011.

(51) **Int. Cl.**
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/0008** (2013.01); **A61B 5/01**
(2013.01); **A61B 5/02055** (2013.01);
(Continued)

(58) **Field of Classification Search**
CPC A61B 5/1455; A61B 5/14551; A61B
5/14552; A61B 5/6825; A61B 5/6826; A61B
5/6838; A61B 5/02427
See application file for complete search history.

(56) **References Cited**
U.S. PATENT DOCUMENTS

3,810,460 A 5/1974 Van Nie
5,957,840 A 9/1999 Terasawa et al.
(Continued)

FOREIGN PATENT DOCUMENTS


DE 102008007337 B3 10/2009
JP 2007-135718 A 6/2007
(Continued)

OTHER PUBLICATIONS
"U.S. Appl. No. 13/457,036, Response filed Oct. 23, 2013 to Non
Final Office Action mailed May 24, 2013", 7 pgs.
(Continued)

Primary Examiner — Eric Winakur
(74) *Attorney, Agent, or Firm* — Schwegman Lundberg &
Woessner, P.A.

(57) **ABSTRACT**
A device includes a clamp and a sensor. The sensor can be
permanently attached to the clamp and tissue by the force
exerted by the clamp. The clamp includes a first jaw member
and a second jaw member. The first jaw member has a jaw
face and the second jaw member has a complementary face.
The second jaw member is held in alignment with the first jaw
member by a joint. The joint has an elastic member config-
ured to exert a compressive force between the jaw face and the
complementary face. The joint is configured to allow move-
ment of the jaw face relative to the complementary face in
directions corresponding to pitch, roll, yaw, and heave. The
compressive force is distributed over a surface of the jaw face.
The sensor is coupled to the jaw face or held in place by the
compressive force of the jaw face. The sensor is configured to
generate a sensor signal corresponding to a physiological
parameter of tissue proximate the jaw face.

23 Claims, 14 Drawing Sheets

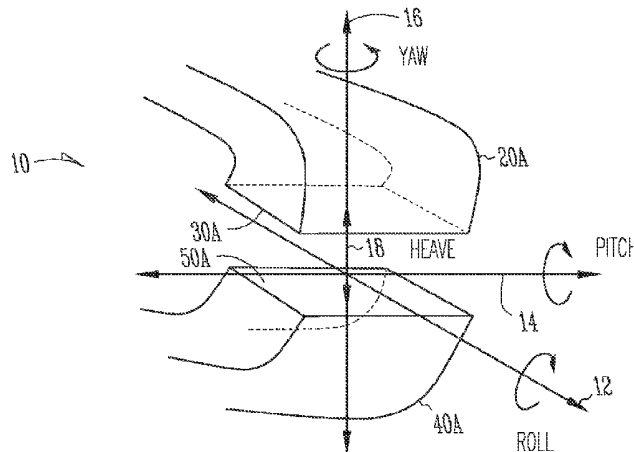

- (51) **Int. Cl.**
A61B 5/01 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/024 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61B 5/1455* (2013.01); *A61B 5/14552*
 (2013.01); *A61B 5/6825* (2013.01); *A61B*
5/6838 (2013.01); *A61B 5/742* (2013.01); *A61B*
5/02427 (2013.01); *Y10T 29/49002* (2015.01);
Y10T 29/49826 (2015.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,154,667	A	11/2000	Miura et al.
8,695,206	B2	4/2014	Isaacson et al.
2007/0260131	A1	11/2007	Chin
2010/0210924	A1	8/2010	Parthasarathy et al.
2012/0289800	A1	11/2012	Isaacson et al.

FOREIGN PATENT DOCUMENTS

JP	5632562	B2	11/2014
NO	WO-2012-149168	A1	11/2012
WO	WO-2006-009906	A2	1/2006
WO	WO-2008-154020	A1	12/2008

OTHER PUBLICATIONS

“U.S. Appl. No. 13/457,036, Non Final Office Action mailed May 24, 2013”, 6 pgs.

“U.S. Appl. No. 13/457,036, Notice of Allowance mailed Nov. 22, 2013”, 10 pgs.
 “U.S. Appl. No. 13/457,036, Preliminary Amendment filed Sep. 25, 2012”, 6 pgs
 “European Application Serial No. 12722959.9, Office Action mailed May 28, 2015”, 4 pgs.
 “European Application Serial No. 12722959.9, Office Action mailed Jan. 9, 2014”, 2 pgs.
 “European Application Serial No. 12722959.9, Office Action mailed Sep. 15, 2014”, 4 pgs.
 “European Application Serial No. 12722959.9, Response filed Jul. 16, 2014 to Office Action mailed Jan. 9, 2014”, 7 pgs.
 “International Application Serial No. PCT/US2012/035224, International Preliminary Report on Patentability mailed Nov. 7, 2013”, 7 pgs.
 “International Application Serial No, PCT/US2012/035224, International Search Report mailed Jul. 9, 2012”, 5 pgs.
 “International Application Serial No. PCT/US2012/035224, Written Opinion mailed Jul. 9, 2012”, 6 pgs.
 “Japanese Application Serial No. 2014-508552, Argument and Amendment filed Jul. 7, 2014 in response to Office Action mailed Apr. 8, 2014”, (w/English Translation of Pending Claims), 6 pgs.
 “Japanese Application Serial No. 2014-508552, Argument and Amendment filed Aug. 19, 2014 in response to Office Action mailed Aug. 5, 2014”, (w/ English Translation of Amended Claims), 6 pgs.
 “Japanese Application Serial No. 2014-508552, Decision to Grant mailed Sep. 9, 2014”, (w/English Translation), 10 pgs.
 “Japanese Application Serial No. 2014-508552, Office Action mailed Apr. 8, 2014”, (w/ English Translation), 4 pgs.
 “Japanese Application Serial No. 2014-508552, Office Action mailed Aug. 5, 2014”, 2 pgs.

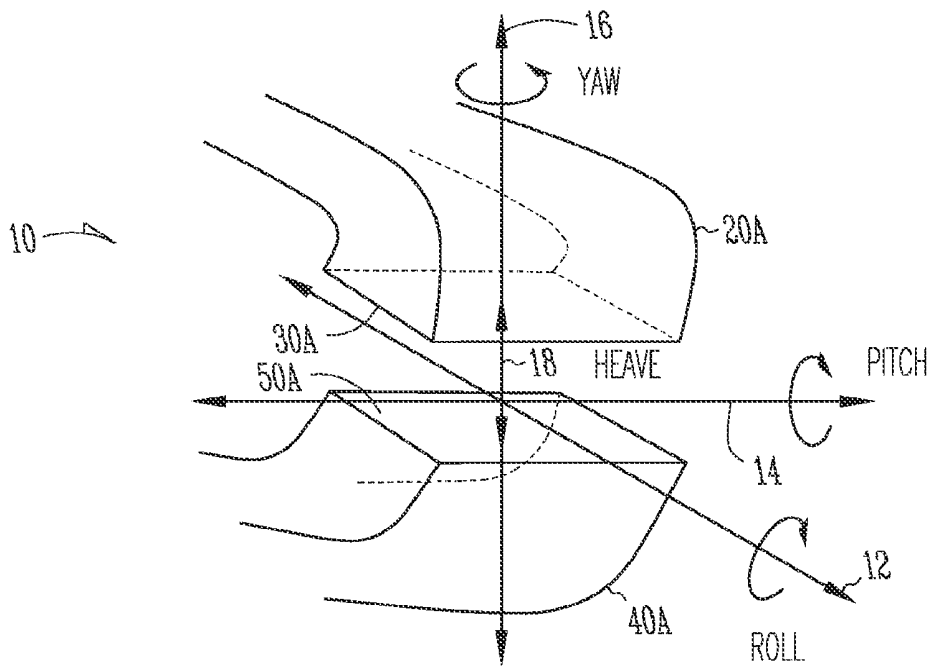


Fig. 1

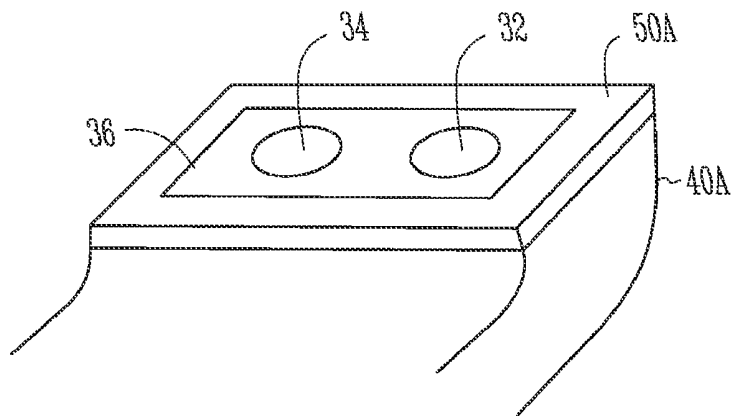


Fig. 2A

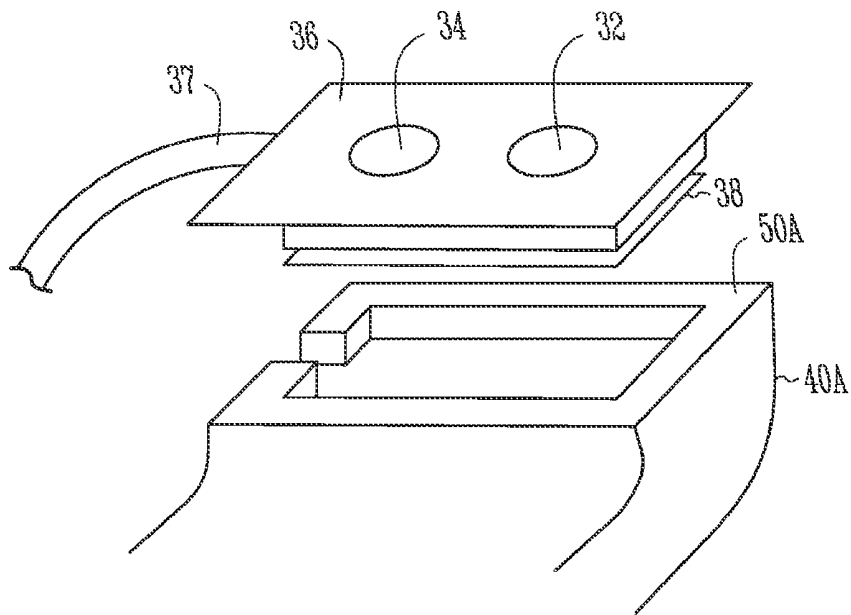


Fig. 2B

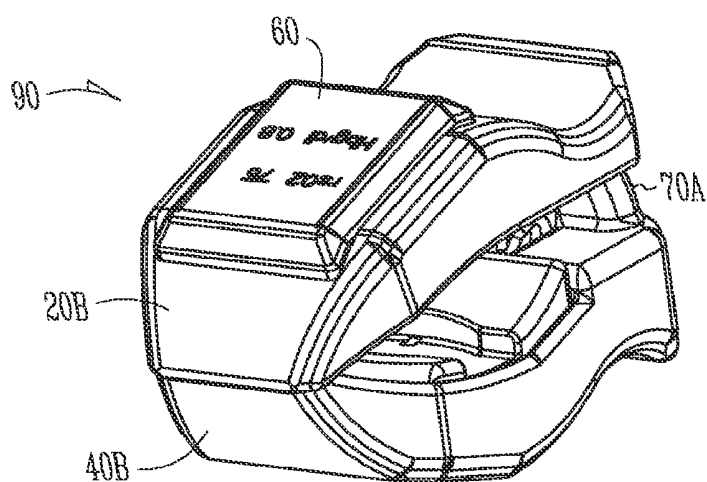


Fig. 3A

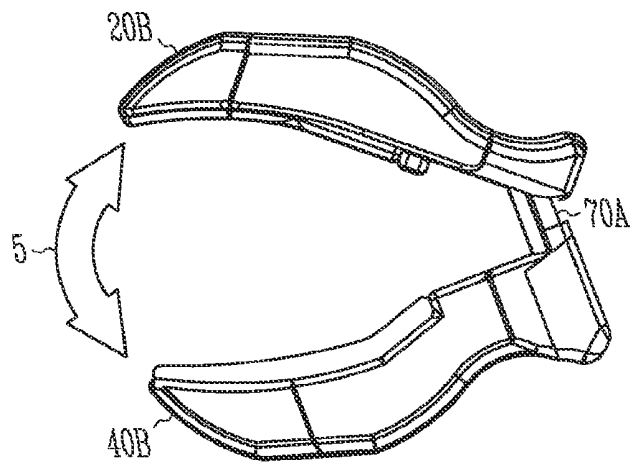


Fig. 3B

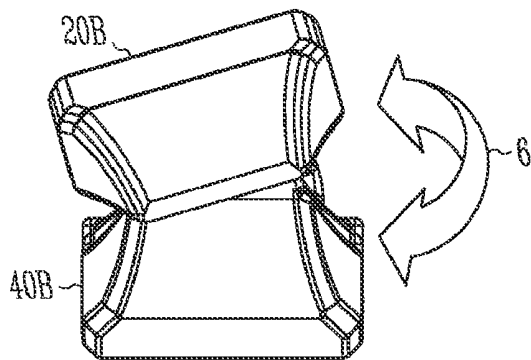


Fig. 3C

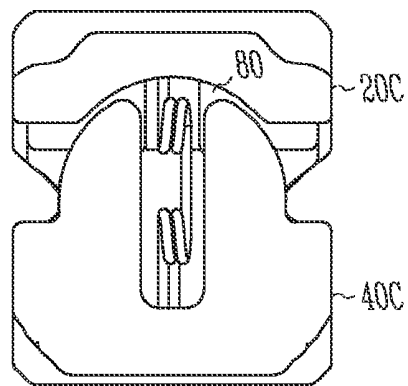


Fig. 3D

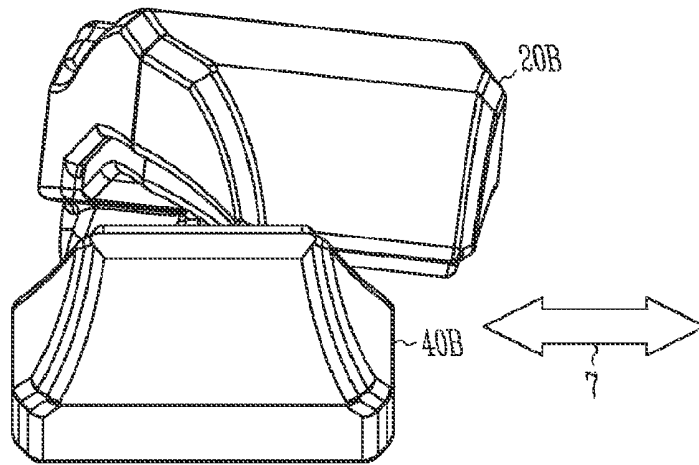


Fig. 3E

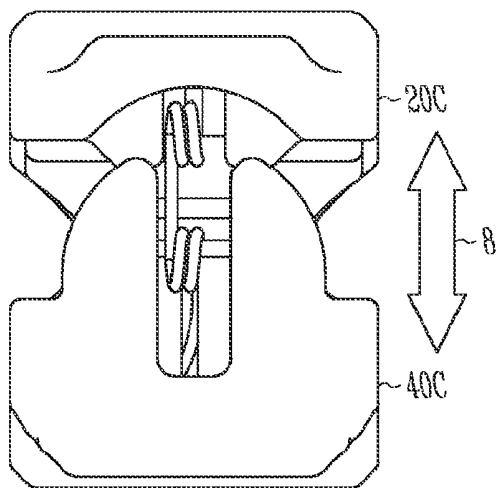


Fig. 3F

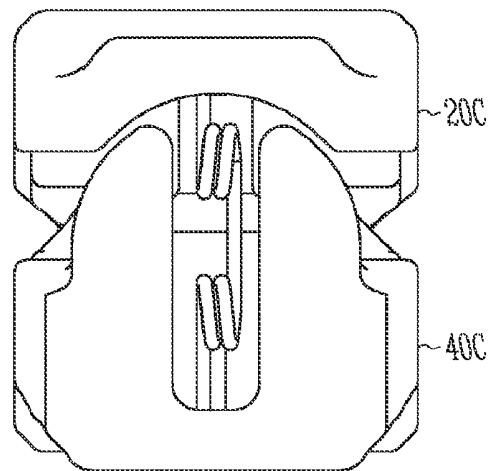


Fig. 3G

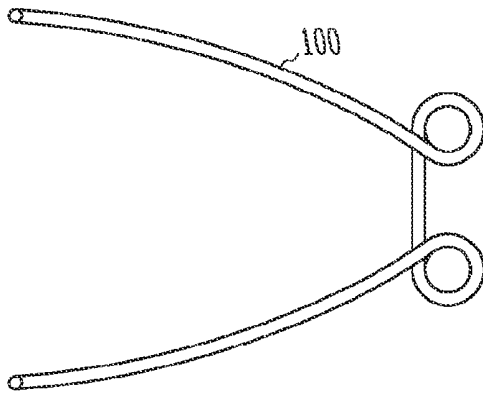


Fig. 4A

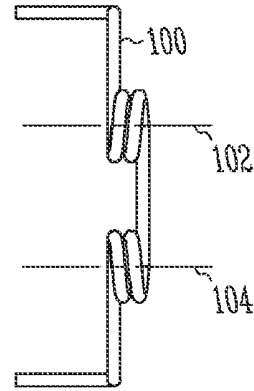


Fig. 4B

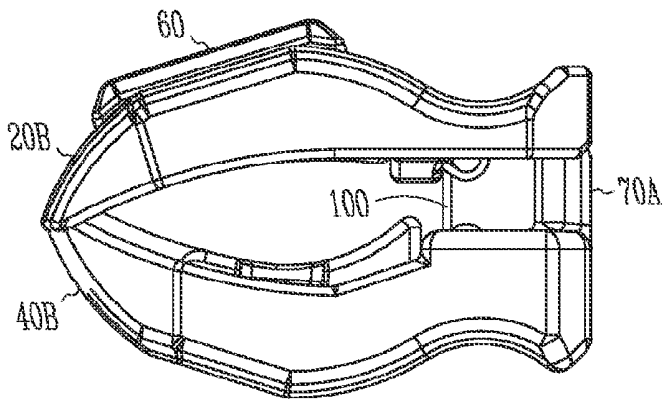


Fig. 5A

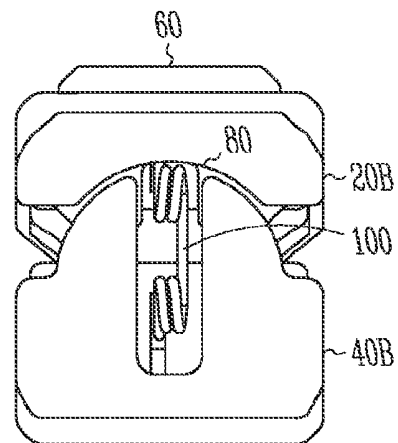


Fig. 5B

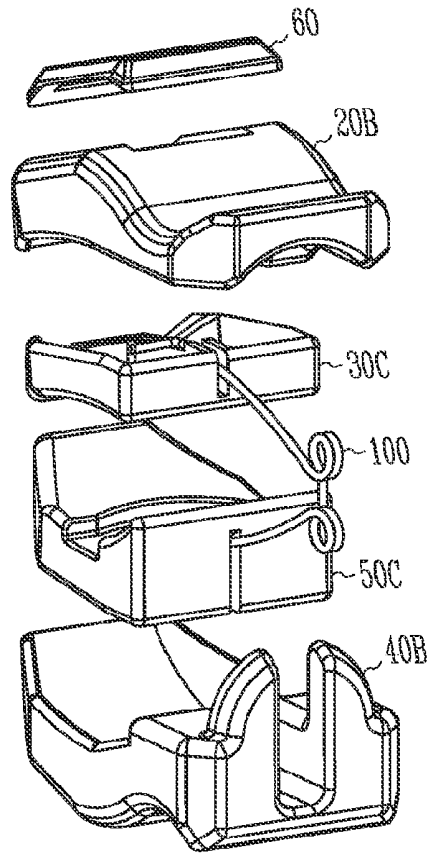


Fig. 5C

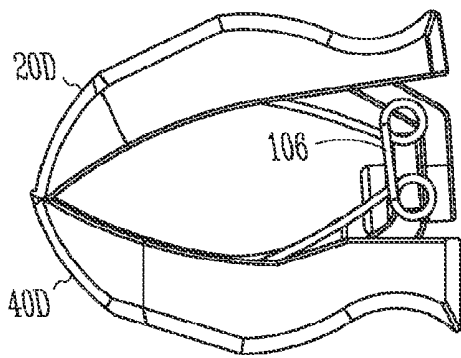


Fig. 6A

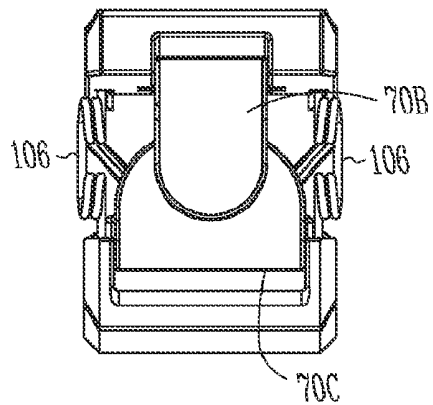


Fig. 6B

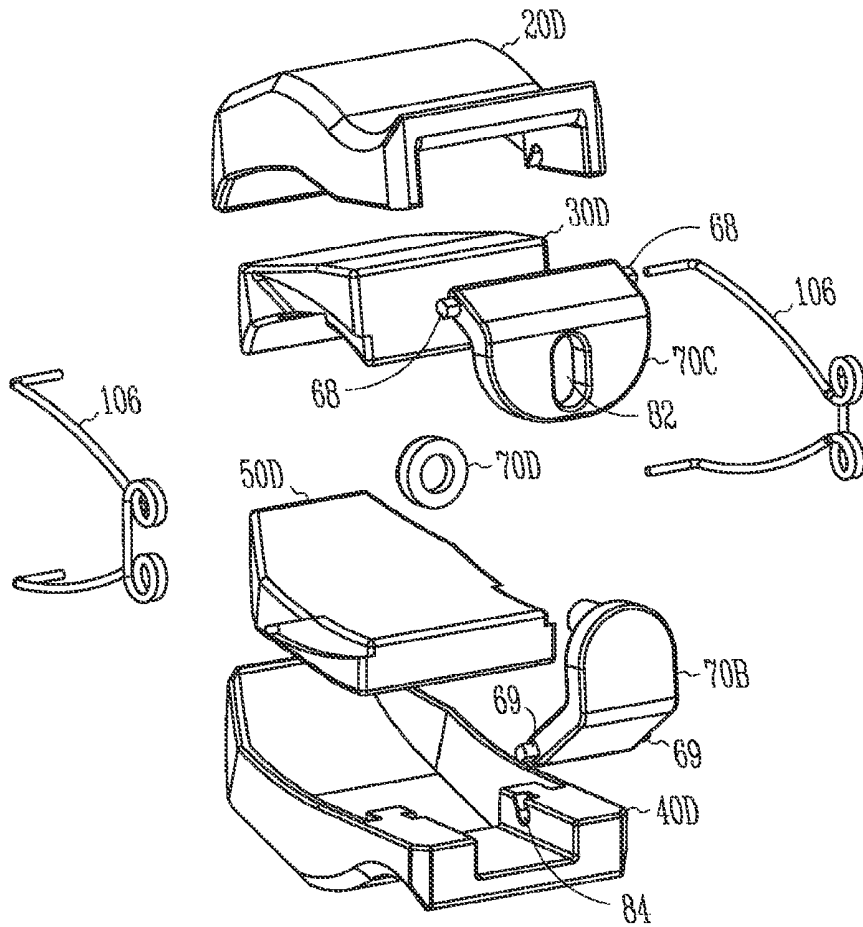


Fig. 6C

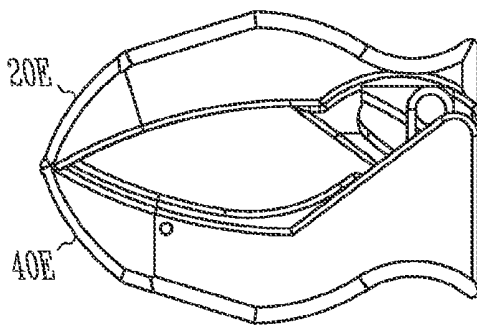


Fig. 7A

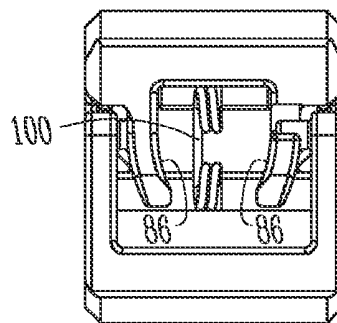


Fig. 7B

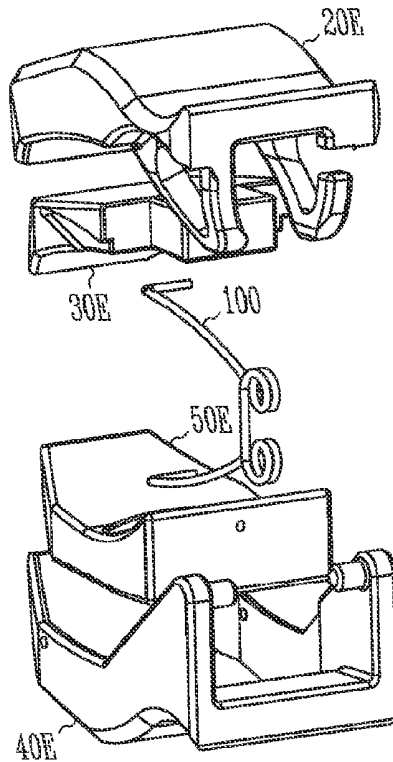


Fig. 7C

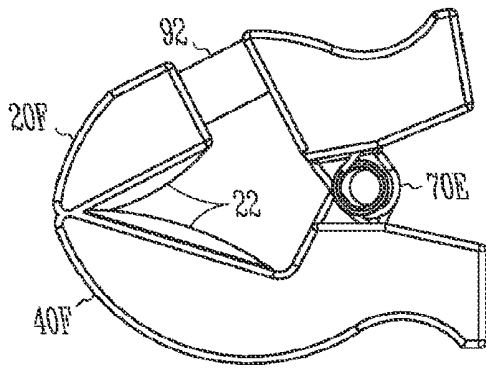


Fig. 8A

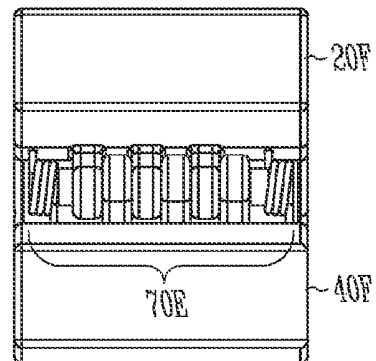


Fig. 8B

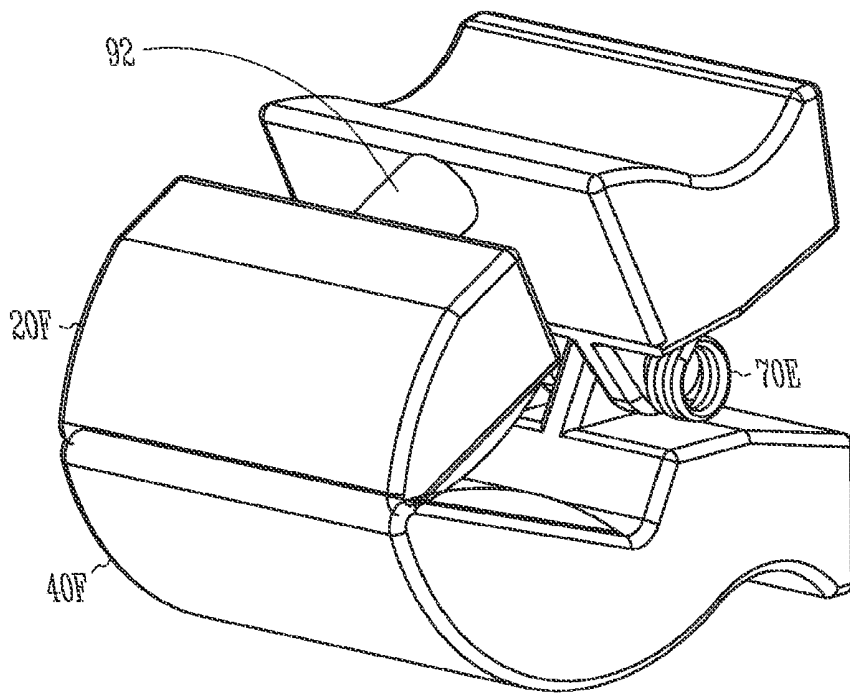


Fig. 8C

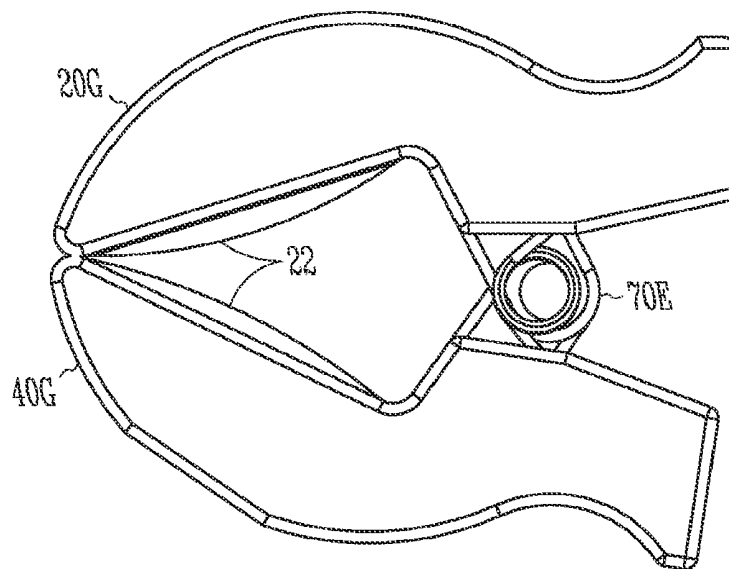


Fig. 9A

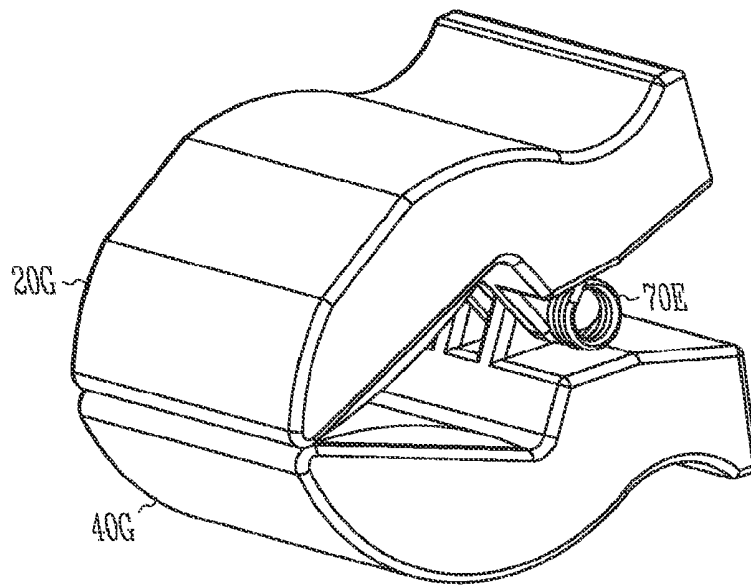


Fig. 9B

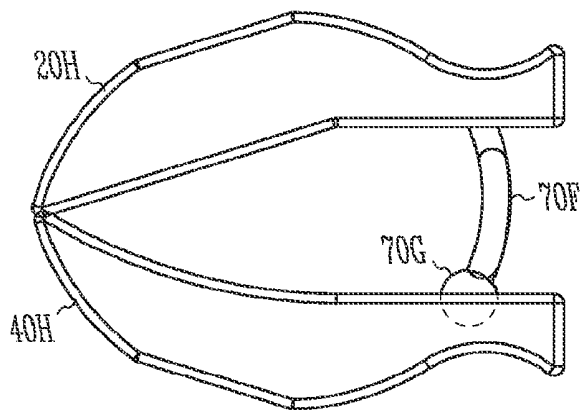


Fig. 10A

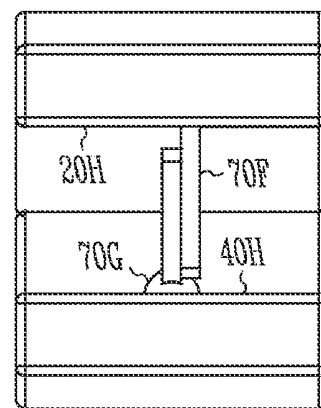


Fig. 10B

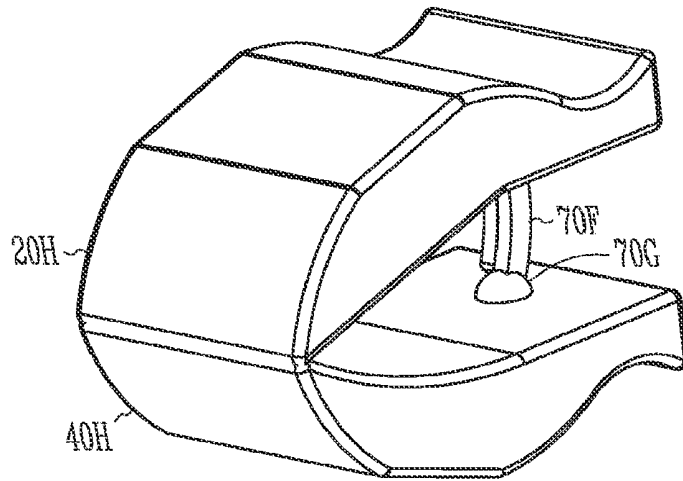


Fig. 10C

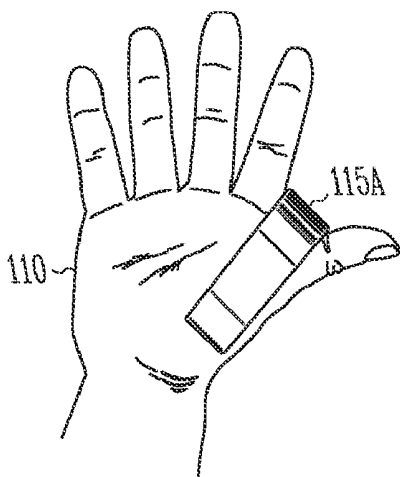


Fig. 11A

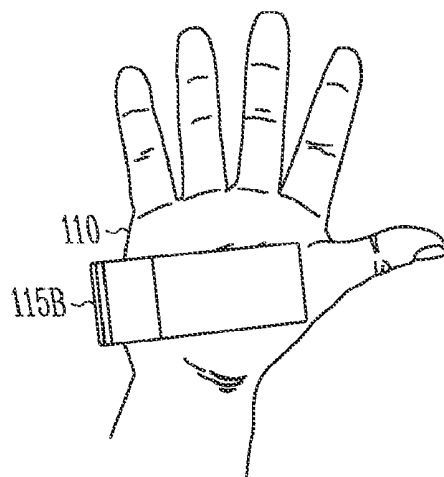


Fig. 11B

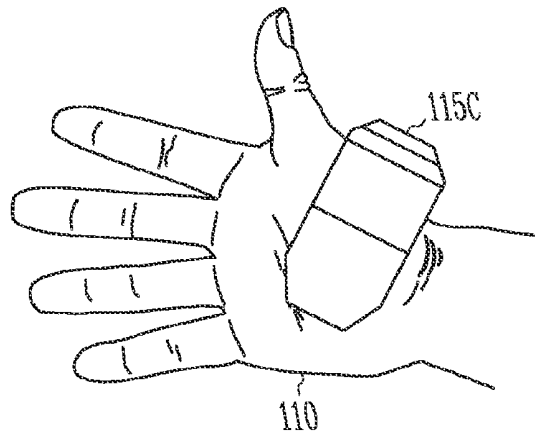


Fig. 11C

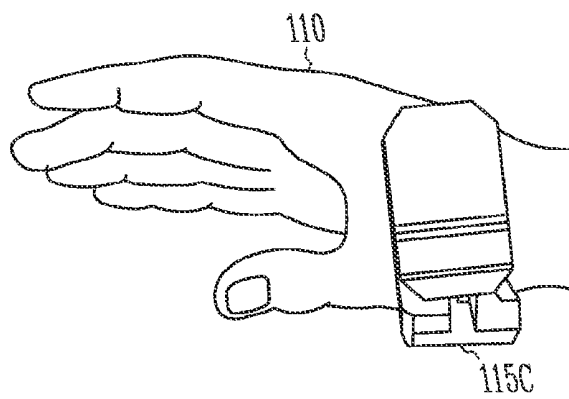


Fig. 11D

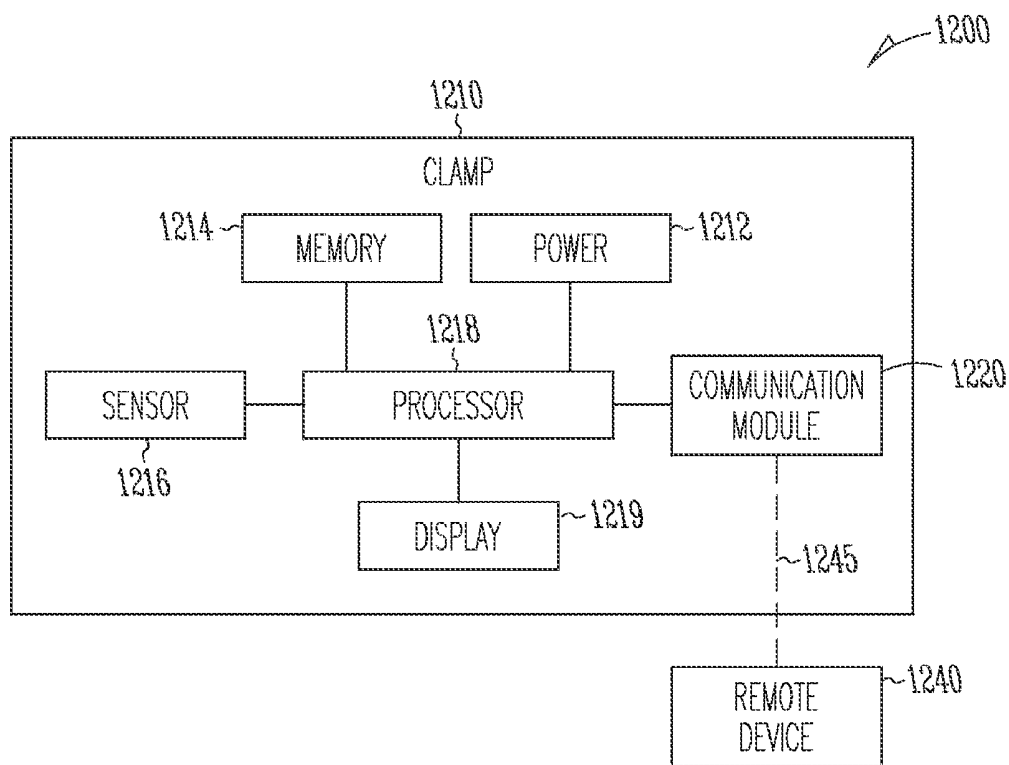


Fig. 12

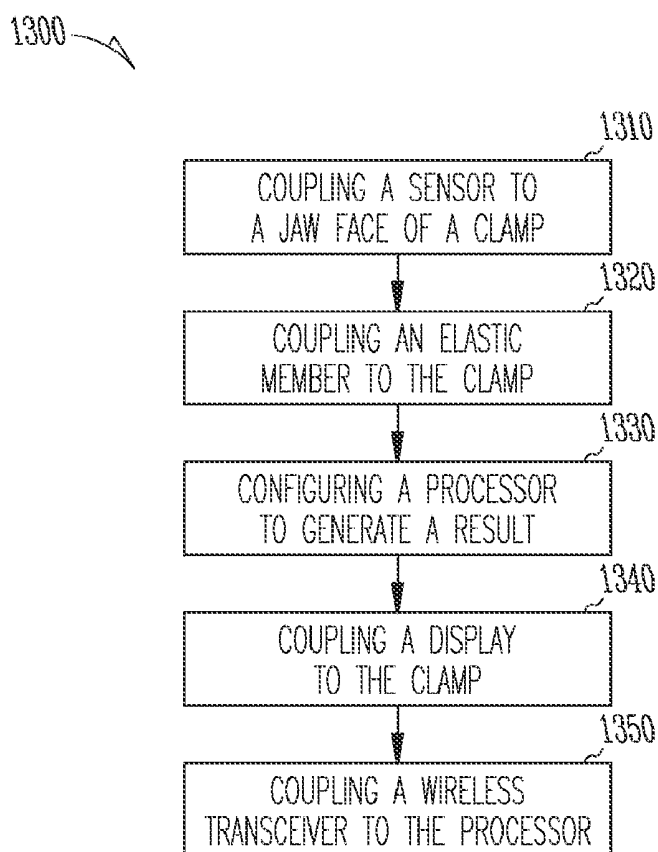


Fig. 13

TISSUE CLAMP FOR NONINVASIVE PHYSIOLOGICAL MEASUREMENT

CLAIM OF PRIORITY

This patent application is a continuation of and claims the benefit of priority under 35 U.S.C. § 120 to U.S. patent application Ser. No. 13/457,036, filed on Apr. 26, 2012, which claims the benefit of priority, under 35 U.S.C. Section 119(e), to Philip O. Isaacson, U.S. Provisional Patent Application Ser. No. 61/479,544, entitled "TISSUE CLAMP FOR NON-INVASIVE PHYSIOLOGICAL MEASUREMENT," filed on Apr. 27, 2011, each of which are hereby incorporated by reference herein in their entireties.

BACKGROUND

The shape of many areas of the human body is complex and can vary considerably from one individual to another. As such, for some non-invasive physiological measurements, the industry has turned to adhesively-applied sensors. Adhesively-applied sensors have various problems and limitations. An adhesively-applied sensor cannot be easily repositioned and may have an adhesive bond that is compromised. In addition, adhesively-applied sensors do not adhere well to some subjects or measurement sites due to moisture (perspiration), oil, hair, or fur. An adhesively-applied sensor can lift away from the tissue when the subject moves or flexes, thus resulting in erroneous data. An adhesively-applied sensor requires a cable leading away from the sensor which impairs patient mobility and measurement reliability.

OVERVIEW

An example of the present subject matter includes a non-adhesive tissue oximetry sensor. A device includes a non-invasive in vivo sensor system for optical measurement or monitoring of selected blood constituents/metabolites in living tissue. In one example, the device is configured to measure light absorption at multiple wavelengths.

A device includes an oximeter having upper and lower jaws joined by a linkage having an elastic element, such as a spring. The linkage, or joint, can be configured for a particular application and in various examples, is configured to enable two degrees of freedom (such as pitch and heave or any other two such degrees), three degrees of freedom (such as pitch, heave, yaw or roll), four degrees of freedom (pitch, heave, roll, and yaw), or more than four degrees of freedom. Various examples are configured to conform to a variety of anatomical shapes and sizes, and are, in particular, configured to measure a physiological parameter associated with the thenar eminence.

In one example, upper and lower jaws form a clamp device. The elastic element exerts a force to securely hold the device in contact with the thenar eminence or other tissue site. A user can overcome the force and disengage the device from the tissue site.

An example of the device can adapt to the shape of the body part and apply a uniform pressure to the tissue at the measurement site. A uniform pressure can enable accurate measurement using the optical sensor. The device can be sized or otherwise configured to enable measurement of various sites, including, for example, a calf, a forearm, a foot, an animal limb, or other structure.

In various examples, one or both of the jaws provide a structure for coupling to or for affixing various components or other elements, including an optical sensor, circuitry (or pro-

gramming) for determining a physiological measurement (including arterial oximetry or tissue oximetry), a power supply, a communication module (wired or wireless), a display, and power control circuitry (to detect the presence of tissue and automatically transition between a sleep mode and a powered mode).

Other configurations are also contemplated, including an example that provides pulse oximetry or regional oximetry, an example that includes a temperature sensor, and an example having a silicone gripping surface proximate the sensor element.

A device includes a clamp and a sensor. The sensor can be permanently attached to the clamp, temporarily attached to the clamp, or held in place between a jaw of the clamp and a tissue by the force exerted by the clamp. The clamp includes a first jaw member and a second jaw member. The first jaw member has a jaw face and the second jaw member has a complementary face. The second jaw member is held in alignment with the first jaw member by a joint. The joint has an elastic member configured to exert a compressive force between the jaw face and the complementary face. In various examples, the joint is configured to allow movement of the jaw face relative to the complementary face in directions corresponding to pitch, roll, yaw, heave, or any combination or permutation thereof. In one example, the compressive force is substantially uniform over a surface of the jaw face. In one example, the joint, the jaw face, and the complementary face are configured to permit the jaw faces to conform to a variety of anatomically shapes and sizes and to distribute the compressive force over the jaw faces. The contact surface of the sensor can conform, or adapt, to an irregular surface of the tissue. In one example, mechanical forces exerted on the sensor are uniformly distributed based on conformance of the sensor with the tissue. The force is distributed in the sense that it is dispersed through a space or over an area (the surface area). The sensor is coupled to the jaw face or held in place by a compressive force of the jaw face. The sensor is configured to generate a sensor signal corresponding to a physiological parameter of tissue proximate the jaw face.

The device can be coupled to the thenar eminence and configured to generate a measure of a physiological parameter. In one example, the device can be repositioned and provides good tissue contact and good measurement reliability.

In one example, the device is portable and includes an integrated processor module (such as analog or digital circuitry), a display, a power source, and a wireless communications module.

These examples can be combined in any permutation or combination. This overview is intended to provide an overview of subject matter of the present patent application. It is not intended to provide an exclusive or exhaustive explanation of the invention. The detailed description is included to provide further information about the present patent application.

BRIEF DESCRIPTION OF THE DRAWINGS

In the drawings, which are not necessarily drawn to scale, like numerals may describe similar components in different views. Like numerals having different letter suffixes may represent different instances of similar components. The drawings illustrate generally, by way of example, but not by way of limitation, various embodiments discussed in the present document.

FIG. 1 illustrates a coordinate system.

FIGS. 2A and 2B illustrate a jaw face with a sensor according to two examples.

FIG. 3A illustrates a perspective view of a device according to one example.

FIG. 3B illustrates an elevation view of a device with an indication of movement about a pitch axis according to one example.

FIG. 3C illustrates a view of a device with an indication of movement about a roll axis according to one example.

FIG. 3D illustrates a view of a device according to one example.

FIG. 3E illustrates a view of a device with an indication of movement about a yaw axis according to one example.

FIGS. 3F and 3G illustrate views of devices with and FIG. 3F includes an indication of translational movement (sometimes referred to as heave) according to one example.

FIGS. 4A and 4B illustrate views of an elastic element according to one example.

FIGS. 5A, 5B, and 5C illustrate views of a device according to one example.

FIGS. 6A, 6B, and 6C illustrate views of a device according to one example.

FIGS. 7A, 7B, and 7C illustrate views of a device according to one example.

FIGS. 8A, 8B, and 8C illustrate views of a device according to one example.

FIGS. 9A and 9B illustrate views of a device according to one example.

FIGS. 10A, 10B, and 10C illustrate views of a device according to one Example.

FIGS. 11A, 11B, 11C, and 11D illustrate devices relative to a human hand according to various examples.

FIG. 12 illustrates a block diagram of a system according to one example.

FIG. 13 illustrates a flow chart of a method according to one example.

DETAILED DESCRIPTION

FIG. 1 illustrates coordinate system **10** suitable for use in describing selected examples of the present subject matter. System **10** includes orthogonal axes **12**, **14**, and **16**, for which rotation about each is deemed roll, pitch, and yaw, respectively. In addition, a translational heave motion is along axis **16**, as denoted by reference **18**.

Pitch refers to motion that can be viewed as tilting forward or backward. Roll refers to motion that can be viewed as tilting side to side. Yaw refers to motion that can be viewed as turning left or right. Heave refers to motion that can be viewed as moving up and down along a linear path.

The figure also depicts a portion of a device according to one example. A first jaw piece is shown at **20A** and includes jaw face **30A**. Second jaw piece **40A** and includes jaw face **50A**. The axes illustrated have an origin located between the jaw faces **30A** and **50A**, however, this is merely for example and it is understood that any particular axis can pass through space without regard to whether or not it intersects with the device.

FIG. 2A illustrates a view of sensor **36** affixed to jaw face **50A** according to one example. In this example, jaw face **50A** includes sensor elements **32** and **34**. Sensor elements **32** and **34** can include an optical emitter, an optical detector, a temperature sensor, or other component configured for measurement of a physiological parameter. In this example, sensor **36** can be considered as permanently coupled to jaw face **50A**.

FIG. 2B illustrates an exploded view of sensor **36**, adhesive layer **38**, jaw face **50A**, and jaw piece **40A**. In one example, adhesive layer **38** couples sensor **36** to jaw face **50A**. In one example, adhesive layer **38** is omitted and the sensor is retained by pressure exerted by jaw face **50A** on the tissue. In these examples, sensor cable **37** is coupled to the sensor at one end and coupled to a secondary device (such as an external monitor) at a second end. In this example, sensor **36** can be considered as temporarily coupled to jaw face **50A**.

FIG. 3A illustrates a perspective view of device **90** according to one example. Device **90** is configured for four degrees of freedom (DOF) to accommodate a variety of tissue contours or sizes. In particular, device **90** is suitable for use at a thenar eminence area.

Device **90** includes display **60** coupled to jaw piece **20B**. Jaw piece **20B** is coupled to jaw piece **40B** by joint **70A**. Joint **70A** allows relative movement corresponding to pitch, roll, yaw, and heave.

FIG. 3B illustrates an elevation view of a device with an indication of movement about a pitch axis according to one example. Joint **70A** allows movement of jaw piece **20B** and jaw piece **40B** in a direction indicated by arrow **5**. Jaw piece **20B** and jaw piece **40B** can open and close. In one example, joint **70A** includes an elastic element, such as a spring, that urges jaw piece **20B** and jaw piece **40B** towards a closed (or contracted) position. A user can manipulate jaw pieces **20B** and **40B** to overcome the force exerted by the elastic element and open the jaw pieces to allow the device to be attached or released from the tissue site.

As shown in FIG. 3B, jaw piece **20B** and jaw piece **40B** each has a tail portion that extends to the right of the pivot provided by joint **70A**. The tail portions can be manipulated by a user in a manner in which they are drawn together and thereby open the jaw to allow repositioning or release of device **90** from engagement on a tissue site. In various examples, jaw piece **20B** and jaw piece **40B** can be manipulated to move in directions described as heave, roll, pitch and yaw.

FIG. 3C illustrates a view of a device with an indication of movement about a roll axis according to one example. Roll refers to rotation (or tilting) of the mechanism. In the figure, jaw piece **20B** and jaw piece **40B** are shifted about a roll axis as denoted by arrow **6**. Detail **80**, illustrated in FIG. 3D, denotes the gap or clearance formed by a curved feature on jaw piece **20C** and a corresponding curved feature on jaw piece **40C**. Detail **80** can also be referred to as a slot and enables relative movement of jaw piece **20C** and jaw piece **40C** about a roll axis.

FIG. 3E illustrates a view of a device with an indication of movement about a yaw axis according to one example. Yaw denotes side to side movement of the mechanism, and as indicated by arrow **7**, jaw piece **20B** and jaw piece **40B** are shifted on a yaw axis. In this example, the axis of rotation for yaw passes through a point offset from a jaw face.

FIGS. 3F and 3G illustrate views of devices with an indication of heave according to one example. Heave refers to up and down movement along an axis. A structural feature, such as slots in the spring inserts, allows vertical movement of jaw piece **20C** relative to jaw piece **40C**. FIG. 3F illustrates jaw piece **20C** drawn apart from jaw piece **40C** and FIG. 3G illustrates the jaw pieces drawn together.

FIGS. 4A and 4B illustrate views of elastic element **100** according to one example. Elastic element **100**, in the example shown, includes a spring. The spring includes double coils, a first coil which is formed on axis **102** and a second coil formed on axis **104** which differs from axis **102**. Other forms of springs or elastic elements are also contemplated.

plated, including a formed clip (of metal or plastic), and an elastomeric polymer band. In various examples, the elastic element is a single component located proximate a center of the device or can be distributed among multiple locations such as at the side portions of the device. Elastic element **100**, in the example shown, allows multiple degrees of freedom and is configured to provide sufficient clamping force to enable accurate measurement of a physiological parameter.

FIGS. **5A**, **5B**, and **5C** illustrate views of a device according to one example. In this example, jaw piece **20B** and jaw piece **40B** are coupled by joint **70A**. Joint **70A** is urged towards a closed position by elastic member **100**. In the example shown, jaw piece **20B** carries display **60**. Display **60**, in various examples also includes circuitry to process the data provided by the sensor elements. For example, a sensor can be provided in jaw face **30C** or jaw face **50C**. Elastic element **100** is coupled to jaw faces **30C** and **50C** each of which is coupled to a respective one of the jaw pieces **20B** and **40B**. Detail **80**, shown in FIG. **5B**, enables motion about the roll axis. In this example, a single elastic element **100** is located proximate the center of the device and provides a force to securely clamp on the tissue. The example shown allows for four degrees of freedom, namely pitch, roll, yaw, and heave.

FIGS. **6A**, **6B**, and **6C** illustrate views of a device having two hinges, according to one example. Jaw piece **20D** and jaw piece **40D** are urged together by elastic elements **106** located on the sides of the device. Pitch is provided by pins **68** and pins **69** of joint **70C** and joint **70B**, respectively. Yaw is enabled by pin **69** engagement with slot **84** shown on one side of jaw piece **40D**. Roll and heave motions are enabled by joint **70B** engagement with slot **82** and secured by fastener **70D**. A sensor is provided in one or both of jaw face **30D** and **50D**. The dual hinge configuration of this example allows motion in four degrees. In particular, the dual hinges enable motion about a pitch axis and the slots, some of which are visible in FIG. **6C**, allows roll movement to accommodate variations in tissue contours.

Elastic elements **106** can be replaced by other configurations, including a single elastic element near the device centerline.

FIGS. **7A**, **7B**, and **7C** illustrate views of a device having a joint including a flared slot, according to one example. This example enables four degrees of freedom (pitch, roll, yaw, and heave). The example shown includes jaw pieces **20E** and **40E** which are urged to a closed positions by elastic element **100** (FIG. **7B**). Jaw faces **30E** and **50E** are coupled to jaw pieces **20E** and **40E**, respectively. Curvature associated with flared members **86** is visible in FIG. **78**. In one example, members **86** are angular or straight and include sufficient clearance with mating components to enable movement having one, two, three, or four degrees of freedom.

FIGS. **8A**, **8B**, and **8C** illustrate views of a device having a rotary joint according to one example. Jaw pieces **20F** and **40F** are urged to a closed position by elastic elements at joint **70E**. In addition, jaw piece **40F** has a fixed configuration whereas jaw piece **20F** includes rotary joint **92**. Rotary joint **92** has an axis that enables rotation of a first end of jaw piece **20F** independent of a second end of jaw piece **20F**. Resilient elements **22** are provide in the example shown and enable the device to accommodate various contours of tissue. Resilient elements **22** can include a cushion of foam or silicone.

This example enables motion along two degrees of freedom. The hinge structure enables a pitch motion and jaw piece **20F** enables a roll motion. An axis of rotation of joint **92** lies concentric with the cylindrical structure shown in FIG. **8A**. FIG. **8B** illustrates a perspective view of joint **92** about which jaw piece **20F** is free to rotate.

FIGS. **9A** and **9B** illustrate views of a device according to one example. The example shown provides a single degree of freedom of movement about the pitch axis. In the example shown, both jaw piece **20G** and jaw piece **40G** are fixed and each include resilient member **22**. Joint **70E** allows rotation about a single axis and an elastic member urges closure of the jaw pieces.

FIGS. **10A**, **10B**, and **10C** illustrate views of a device according to one example. In this example, the joint includes ratchet **70F** as well as a spherical ball joint **70G**. Ratchet **70F** includes a mechanism that prevents motion in one direction and allows motion in another direction. Here, ratchet **70F** can be manually operated to enable closure of the jaw pieces **20H** and **40H** and prevent separation of the jaw pieces unless a pawl or other motion limiting component is drawn away from teeth of the ratchet. Ball joint **70G** allows circular motion akin to roll, pitch, and yaw.

In this example, ratchet **70F** allows adjustment of the clamping pressure. The ball joint **70G** allows the assembly to conform to tissue (such as the thenar eminence) by allowing, among other things, roll and yaw.

FIGS. **11A**, **11B**, **11C**, and **11D** illustrate various devices relative to a user's hand according to various examples. In each figure, the device is configured to position a sensor proximate the thenar eminence. The devices can be configured for use on either a left or a right hand. In FIG. **11A**, device **115A** is positioned with a joint portion of the device between a thumb and the index finger of hand **110**. Device **115A** is configured for motion described as having 1, 2, 3, or 4 degrees of freedom. In FIG. **11B**, device **115B** is positioned with a joint portion proximate the hypo-thenar eminence of hand **110**. In FIG. **11C**, device **115C** is positioned with a joint between the thumb and the wrist. FIG. **11D** illustrates another view of device **115C**.

FIG. **12** illustrates a block diagram of system **1200** according to one example. In this example, system **1200** includes device **1210** and remote device **1240**. Device **1210** includes processor **1218** coupled to sensor **1216**. Sensor **1216** can include one or more of an optical detector (such as a photo detector), an optical emitter (such as a light emitting diode), a temperature sensor (such as a thermistor), or other sensor configured to measure (or monitor) a physiological parameter. An output signal from sensor **1216** is coupled to processor **1218**. Processor **1218**, in this example, executes instructions stored in memory **1214** and uses data stored in memory **1214** to determine a result. The result can be stored in memory **1214**, conveyed to communication module **1220**, displayed in a human-perceivable manner on display **1219**, or any combination of stored, conveyed, and displayed. Power unit **1212** provides power to any one or all of the components of device **1210**. In one example, power unit **1212** includes a battery or other energy storage device. In one example, power unit **1212** includes a rechargeable battery and a recharging circuit. The recharging circuit includes a power connector configured to allow the device to be connected or docked with a recharging base unit.

Communication module **1220** can include a radio frequency (RF) transceiver (such as a Bluetooth device) or an optical coupler configured to communicate using infrared energy. Link **1245** can include an RF channel, an optical channel, or other communication channel. In one example, communication module **1220** includes a connector to enable a wired connection between processor **1218** and remote device **1240**.

Remote device **1240** can include a complementary device and in various examples, includes a wirelessly-coupled processor such as a laptop computer. Remote device **1240** can be

configured to store the result or can be configured to provide instructions or provide data to device 1210 via link 1245.

Processor 1218 can include a digital processor or an analog processor including an amplifier, a filter, or other circuitry.

FIG. 13 illustrates a flow chart of method 300 according to one example. Method 1300 includes, at 1310, coupling a sensor to a jaw face of a clamp. The clamp can include any of the devices described herein or variations thereof. At 1320, method 1300 includes coupling an elastic member to the clamp. The elastic member, such as a spring, can be coupled to a joint of the device and configured to urge the closure of the clamp jaws. At 1330, method 1300 includes configuring a processor to generate a result. The result can include pulse oximetry (arterial oximetry), tissue oximetry (mixed venous), temperature, or any other measure of a physiological parameter.

At 1340, method 1300 includes coupling a display to the clamp. The display can include a display screen or one or more LED lights. At 1350, method 1300 includes coupling a wireless transceiver to the processor. The wireless transceiver can include an RE transceiver or other type of wireless communication device.

The examples illustrated and described include a variety of joints, some of which can be referred to as articulating, translating, or a prismatic.

In various examples, the device is configured to provide a distance between the joint and the sensor at the jaw face sufficient to position the sensor proximate the thenar eminence region of the hand.

The elastic element can exert a tension force or an extension force to draw the jaw pieces together. In some examples, the jaw face includes a rubber, silicone, or other surface to increase frictional resistance and retain the device in a selected position.

The present subject matter can be tailored for various configurations and thus suited for a variety of applications. For example, the sensor can be coupled to the jaw face by a combination of structural features that might be considered temporary or permanent.

A temporary coupling can allow user attachment and detachment of a sensor and a jaw face. An example of a temporary coupling is illustrated in FIG. 2B, and as noted elsewhere in this document, one example includes an adhesive. Other temporary couplings are also contemplated. For example, a temporary coupling can include a variety of combinations of structural features such as a pin, a recess, a clip, a shoulder, an interference fit, or other such elements. In one example, a temporary coupling is configured to retain the sensor in alignment relative to a jaw face or configured to constrain independent movement of the sensor relative to the jaw face. In one example, a sensor is temporarily coupled to, or retained by, the jaw face by means of a compressive force exerted by the clamp. In one example, complementary features of the sensor and of the jaw face allow the sensor to float on the jaw face. A temporary coupling can be easily assembled or disassembled by a user.

A temporary coupling may allow a user to replace a sensor or select from a variety of different sensors suited for different purposes. For example, a single clamp can be reconfigured to carry a sensor suitable for measuring temperature, electrical conductivity, or other physiological parameter. In various examples, the sensor includes one or more optical elements including an emitter and a detector. The sensor can be tailored for use at a particular optical frequency, sensitivity, range, or other characteristic. A clamp can be re-used with different patients and carry different sensors or sensor configurations

depending on user requirements as to a particular measurement or monitoring application.

In one example, a sensor is replaceable and therefore, disposable. A disposable sensor is inexpensive relative to the cost associated with the complete device.

A permanent coupling does not allow user attachment and detachment of a sensor and a jaw face. An example of a permanent coupling is illustrated in FIG. 2A in which the sensor is securely affixed to the jaw face. The sensor can be coupled by a variety of structural features such as a pin, a recess, a clip, a shoulder, an interference fit, or other such element. In one example, a permanent coupling includes an adhesive configured to retain the sensor in a fixed position relative to a jaw face.

A sensor permanently coupled to a jaw face is well suited for an application corresponding to the particular sensor. A clamp can be configured to carry a sensor suited for measuring temperature, electrical conductivity, or other physiological parameter. In various examples, the sensor includes one or more optical elements including an emitter and a detector. The sensor can be tailored for use at a particular optical frequency, sensitivity, range, or other characteristic.

A jaw face can be configured to carry multiple sensors. In addition, a first sensor can be coupled to a first jaw face and a second sensor can be coupled to a complementary face. The faces and sensors can be configured for permanent or temporary coupling and the first sensor and the second sensor can be different or matching.

The jaws can be configured with a joint that allows for various combinations of freedom of movement. Using representations in which Roll=R, Pitch=P, Heave=H, and Yaw=Y, the following combinations of jaw movement are contemplated: RP, RH, RY, PH, PY, HY, RPH, RPY, RHY, PHY, and RPHY. As such, RP denotes a joint in which the combination of roll and pitch are enabled and RHY denotes a joint in which the combination of roll, heave, and yaw are enabled. Depending on the configuration of movements enabled, a joint can include structural movement limiting elements that preclude or allow movement in a particular manner.

Additional Notes

The above detailed description includes references to the accompanying drawings, which form a part of the detailed description. The drawings show, by way of illustration, specific embodiments in which the invention can be practiced. These embodiments are also referred to herein as "examples." Such examples can include elements in addition to those shown or described. However, the present inventors also contemplate examples in which only those elements shown or described are provided. Moreover, the present inventors also contemplate examples using any combination or permutation of those elements shown or described (or one or more aspects thereof), either with respect to a particular example (or one or more aspects thereof), or with respect to other examples (or one or more aspects thereof) shown or described herein.

All publications, patents, and patent documents referred to in this document are incorporated by reference herein in their entirety, as though individually incorporated by reference. In the event of inconsistent usages between this document and those documents so incorporated by reference, the usage in the incorporated reference(s) should be considered supplementary to that of this document; for irreconcilable inconsistencies, the usage in this document controls.

In this document, the terms "a" or "an" are used, as is common in patent documents, to include one or more than one, independent of any other instances or usages of "at least one" or "one or more." In this document, the term "or" is used

to refer to a nonexclusive or, such that “A or B” includes “A but not B,” “B but not A,” and “A and B,” unless otherwise indicated. In the appended claims, the terms “including” and “in which” are used as the plain-English equivalents of the respective terms “comprising” and “wherein.” Also, in the following claims, the terms “including” and “comprising” are open-ended, that is, a system, device, article, or process that includes elements in addition to those listed after such a term in a claim are still deemed to fall within the scope of that claim. Moreover, in the following claims, the terms “first,” “second,” and “third,” etc. are used merely as labels, and are not intended to impose numerical requirements on their objects.

Method examples described herein can be machine or computer-implemented at least in part. Some examples can include a computer-readable medium or machine-readable medium encoded with instructions operable to configure an electronic device to perform methods as described in the above examples. An implementation of such methods can include code, such as microcode, assembly language code, a higher-level language code, or the like. Such code can include computer readable instructions for performing various methods. The code may form portions of computer program products. Further, the code can be tangibly stored on one or more volatile or non-volatile tangible computer-readable media, such as during execution or at other times. Examples of these tangible computer-readable media can include, but are not limited to, hard disks, removable magnetic disks, removable optical disks (e.g., compact disks and digital video disks), magnetic cassettes, memory cards or sticks, random access memories (RAMs), read only memories (ROMs), and the like.

The above description is intended to be illustrative, and not restrictive. For example, the above-described examples (or one or more aspects thereof) may be used in combination with each other. Other embodiments can be used, such as by one of ordinary skill in the art upon reviewing the above description. The Abstract is provided to comply with 37 C.F.R. §1.72(b), to allow the reader to quickly ascertain the nature of the technical disclosure. It is submitted with the understanding that it will not be used to interpret or limit the scope or meaning of the claims. Also, in the above Detailed Description, various features may be grouped together to streamline the disclosure. This should not be interpreted as intending that an unclaimed disclosed feature is essential to any claim. Rather, inventive subject matter may lie in less than all features of a particular disclosed embodiment. Thus, the following claims are hereby incorporated into the Detailed Description, with each claim standing on its own as a separate embodiment, and it is contemplated that such embodiments can be combined with each other in various combinations or permutations. The scope of the invention should be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled.

The claimed invention is:

1. A device comprising:

a clamp having a first jaw member and a second jaw member, the first jaw member having a jaw face and the second jaw member having a complementary face, the second jaw member held in alignment with the first jaw member by a joint, the joint having an elastic member configured to exert a compressive force between the jaw face and the complementary face, the joint configured to allow movement of the jaw face relative to the complementary face in directions corresponding to pitch, roll, yaw, and heave, and the compressive force distributed over a surface of the jaw face;

a sensor coupled to the jaw face, the sensor configured to generate a sensor signal corresponding to a physiological parameter of a tissue proximate the jaw face.

2. The device of claim 1 wherein the sensor is permanently coupled to the jaw face.

3. The device of claim 1 wherein the sensor is temporarily coupled to the jaw face.

4. The device of claim 1 wherein the sensor is retained on the jaw face by the compressive force.

5. The device of claim 1 further including a processor coupled to the clamp, the processor configured to generate a result based on the sensor signal.

6. The device of claim 5 further including a display coupled to the processor and coupled to the clamp, the display configured to render the result in a human perceivable manner.

7. The device of claim 1 further including a wireless transceiver configured to wirelessly communicate with a remote device.

8. The device of claim 1 further including a connector configured to couple with a remote device.

9. The device of claim 1 further including a wired output, the wired output configured to communicate with a remote device.

10. The device of claim 1 wherein the clamp is configured to position the jaw face proximate a thenar eminence.

11. The device of claim 1 wherein the elastic member includes a spring.

12. The device of claim 11 wherein the spring includes a first coil having a first axis and a second coil having a second axis, the first axis different than the second axis.

13. The device of claim 1 wherein the joint includes a spherical joint.

14. The device of claim 1 wherein the sensor includes at least one of an optical emitter or at least one of an optical detector.

15. The device of claim 1 wherein the sensor includes a temperature sensor.

16. The device of claim 1 wherein the jaw face is coupled to the first jaw member by an articulating link.

17. A system comprising:

a clamp including a pair of arms configured to articulate about a joint, each arm having a jaw portion and having a sensor coupled to the jaw portion of at least one arm, the sensor configured to provide a sensor output corresponding to a physiological parameter of tissue proximate the sensor, the joint configured to allow movement of the jaw portions in directions corresponding to pitch, roll, yaw, and heave;

an elastic member coupled to the clamp and configured to exert a compressive force between the jaw portions, the compressive force distributed over a surface of the sensor;

a processor coupled to the clamp and configured to generate a result based on the sensor output; and
a display coupled to the processor and configured to generate visible data based on the result.

18. The device of claim 17 further including a communication module coupled to the processor and configured to communicate with a remote device.

19. The device of claim 17 wherein the sensor includes at least one of an optical emitter or at least one of an optical detector.

20. The device of claim 17 wherein the sensor is disposable.

21. The device of claim 17 wherein the sensor is configured for placement between the jaw face and the tissue.

22. The system of claim 17 further including a wireless transceiver coupled to the processor and configured to wirelessly communicate the result with a remote device.

23. The system of claim 17 wherein the clamp is configured for positioning the jaw face on a thenar eminence.

5

* * * * *

专利名称(译)	组织夹具用于无创生理测量		
公开(公告)号	US9254087	公开(公告)日	2016-02-09
申请号	US14/223033	申请日	2014-03-24
[标]申请(专利权)人(译)	NONIN医疗		
申请(专利权)人(译)	NONIN MEDICAL , INC.		
当前申请(专利权)人(译)	NONIN MEDICAL , INC.		
[标]发明人	ISAACSON PHILIP O JONES BRYANT AUSTIN JOHNSON TIMOTHY L HOLLAND CHRISTOPHER PRIOR MATTHEW		
发明人	ISAACSON, PHILIP O. JONES, BRYANT AUSTIN JOHNSON, TIMOTHY L. HOLLAND, CHRISTOPHER PRIOR, MATTHEW		
IPC分类号	A61B5/1455 A61B5/00 A61B5/01 A61B5/0205 A61B5/024		
CPC分类号	A61B5/0008 A61B5/01 A61B5/02055 A61B5/1455 A61B5/14552 A61B5/6825 A61B5/6838 A61B5/742 A61B5/02427 Y10T29/49002 Y10T29/49826		
代理机构(译)	SCHWEGMAN和Lundberg & 沃斯纳 , P.A.		
优先权	61/479544 2011-04-27 US		
其他公开文献	US20140288388A1		
外部链接	Espacenet USPTO		

摘要(译)

一种装置包括夹具和传感器。传感器可以通过夹具施加的力永久地连接到夹具和组织上。夹具包括第一钳口构件和第二钳口构件。第一钳口构件具有钳口面，第二钳口构件具有互补面。第二钳口构件通过接头保持与第一钳口构件对齐。该接头具有弹性构件，该弹性构件构造成在钳口面和互补面之间施加压缩力。该接头构造成允许钳口面相对于互补面在与俯仰，滚动，偏航和起伏相对应的方向上移动。压缩力分布在钳口面的表面上。传感器连接到钳口面或通过钳口面的压缩力保持在适当位置。传感器配置成产生对应于靠近颌面的组织的生理参数的传感器信号。

A device includes a clamp and a sensor. The sensor can be permanently attached to the clamp and tissue by the force exerted by the clamp. The clamp includes a first jaw member