



US 20150101608A1

(19) **United States**
(12) **Patent Application Publication**
SIRIWARDENA et al.

(10) **Pub. No.: US 2015/0101608 A1**
(43) **Pub. Date: Apr. 16, 2015**

(54) **TOROIDAL RING VENTILATOR**

(71) Applicants: **MAPATUNAGE A. SIRIWARDENA**,
New Hartford, NY (US);
CHAMKURKISHTIAH P. RAO,
Mohawk, NY (US)

(72) Inventors: **MAPATUNAGE A. SIRIWARDENA**,
New Hartford, NY (US);
CHAMKURKISHTIAH P. RAO,
Mohawk, NY (US)

(21) Appl. No.: **14/055,705**

(22) Filed: **Oct. 16, 2013**


Publication Classification

(51) **Int. Cl.**
A61M 16/00 (2006.01)
A61B 5/0205 (2006.01)
A61B 5/1455 (2006.01)
A61B 5/00 (2006.01)
A61M 16/10 (2006.01)
A61M 16/12 (2006.01)

(52) **U.S. Cl.**
CPC *A61M 16/0069* (2014.02); *A61M 16/1005*
(2014.02); *A61M 16/125* (2014.02); *A61B*
5/14552 (2013.01); *A61B 5/4836* (2013.01);
A61M 16/0003 (2014.02); *A61B 5/6801*
(2013.01); *A61M 16/0051* (2013.01); *A61B*
5/0205 (2013.01); *A61B 5/742* (2013.01);
A61M 2016/0039 (2013.01); *A61M 2016/0027*
(2013.01); *A61B 5/087* (2013.01)

(57) **ABSTRACT**

The toroidal ring ventilator system is a compact and portable artificial respiration system. A vortex ring generator delivers a FiO₂ mix from an air-oxygen blender to the patient during the patient's inhalations, but remains idle during the patient's exhalations. Exhaust gases generated by the patient are released through an exhaust gas valve. During operation, the patient's oxygen saturation level is measured by an infrared pulse-oxygen probe, and a FiO₂ autoregulator is in communication with the probe to receive oxygen saturation level signals. The FiO₂ autoregulator is coupled with the air-oxygen blender to control the oxygen proportion of the FiO₂ mix. An automatic pressure flow sensor is fluidly coupled with the patient's airway to control actuation of the vortex ring generator. The automatic flow sensor is coupled with a controller, which actuates a vortex ring generator trigger circuit in communication with the vortex ring generator.

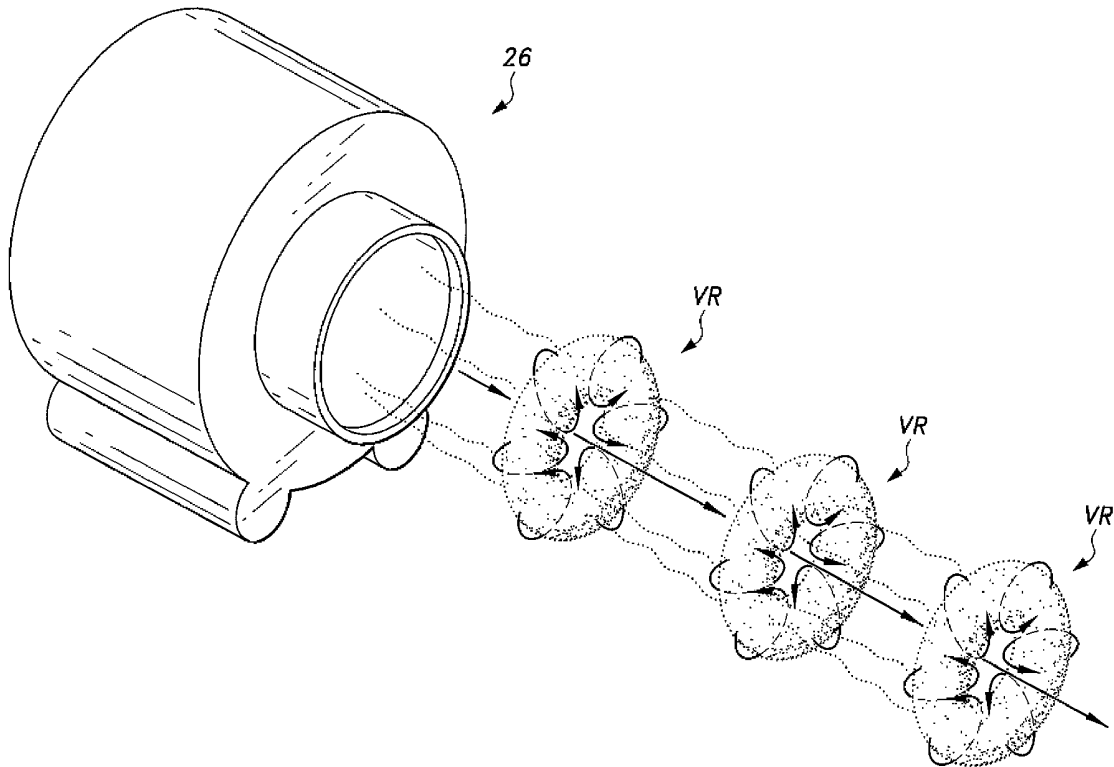

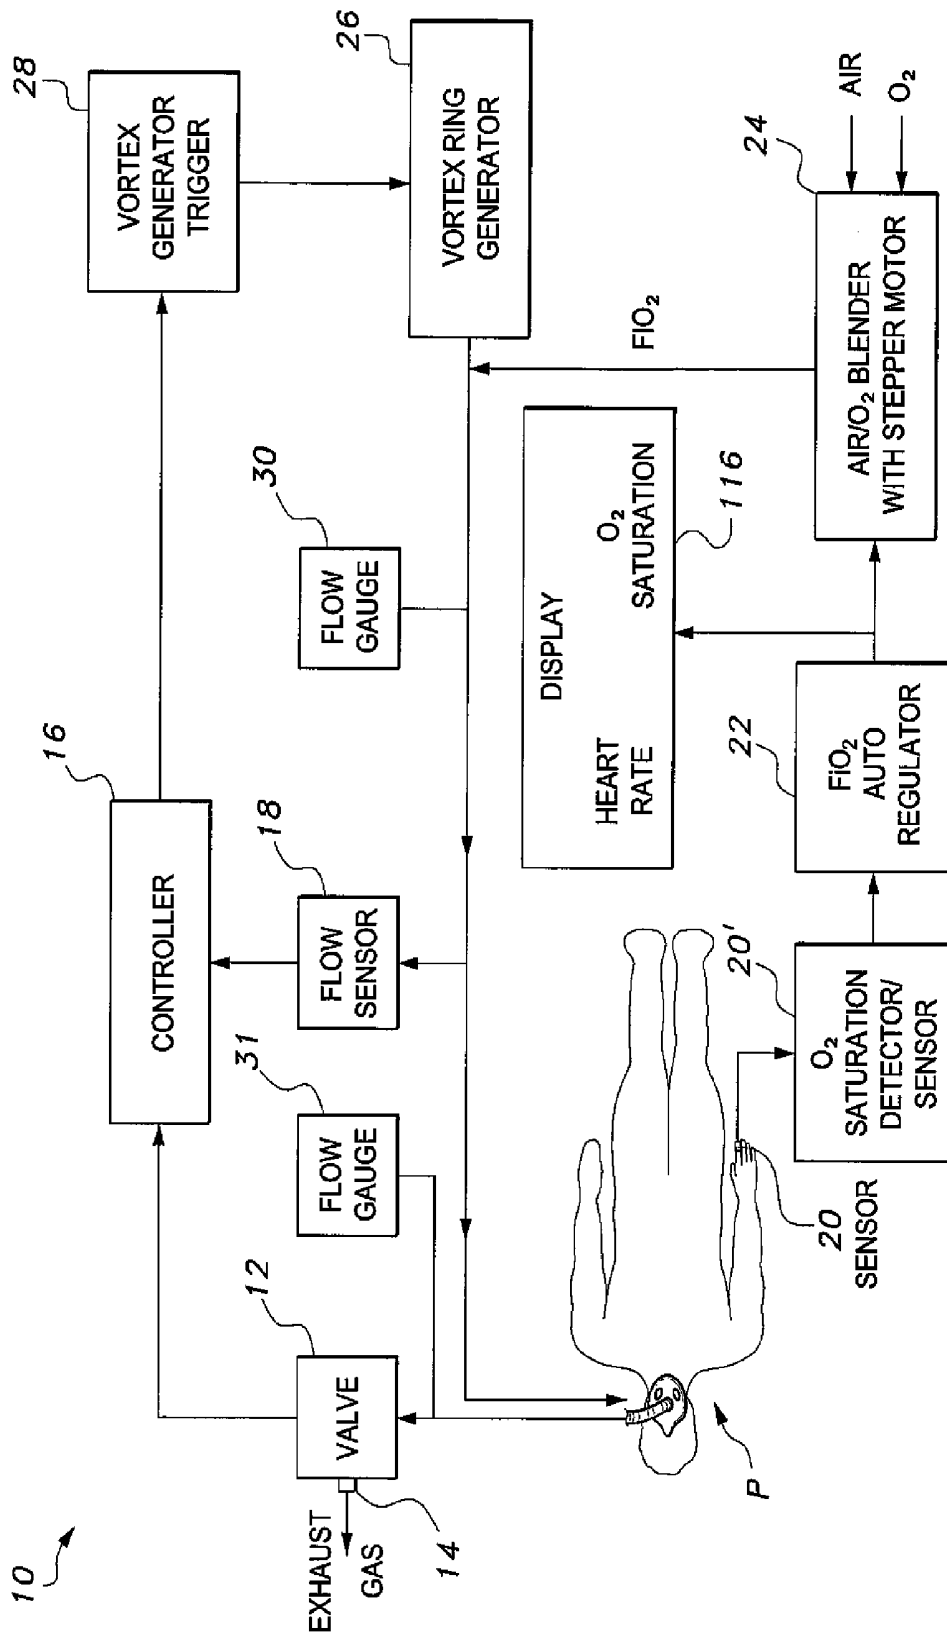


Fig. 1

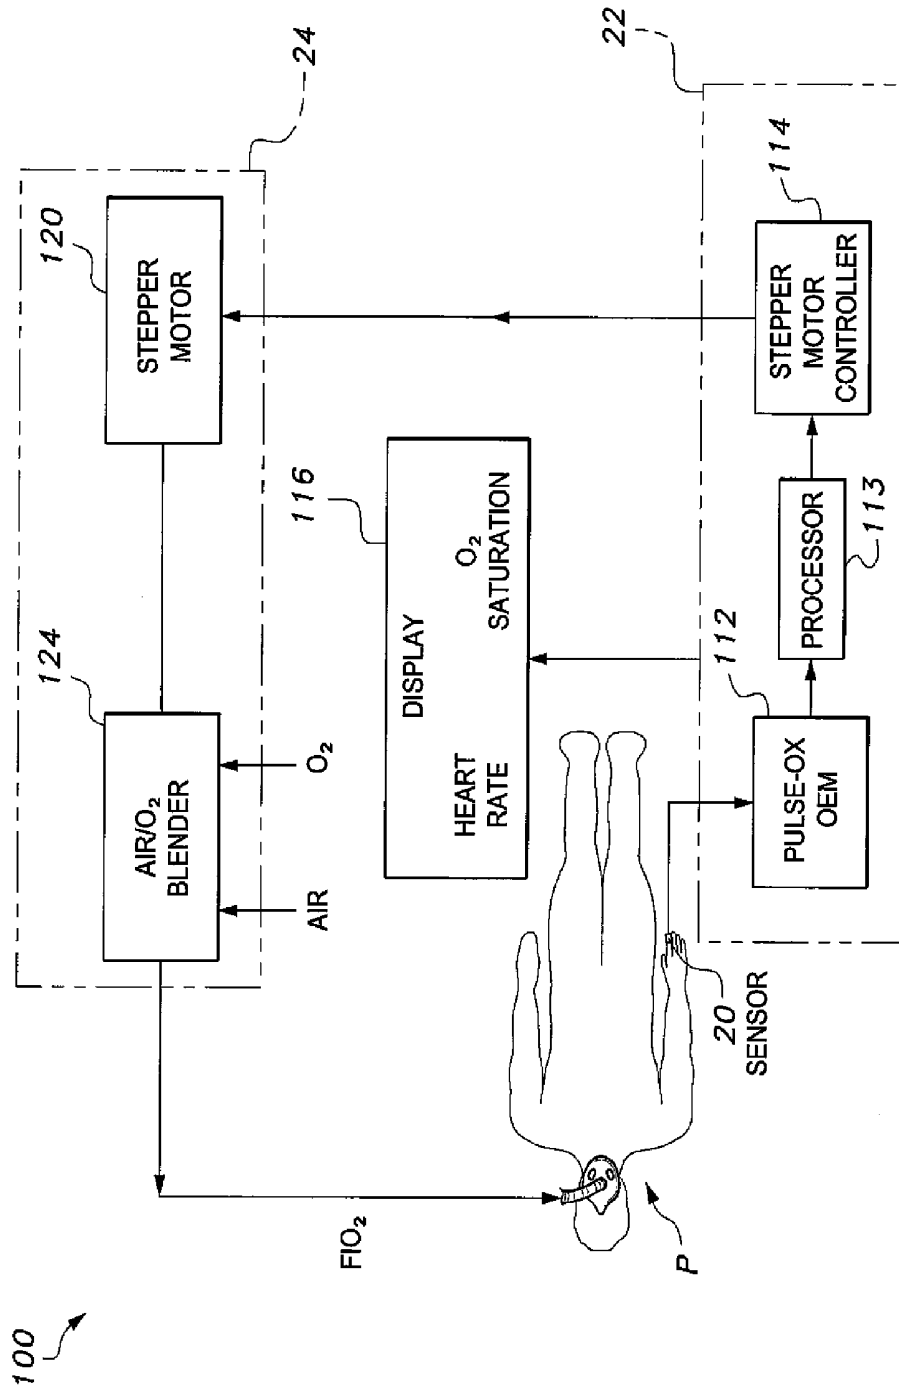


Fig. 2


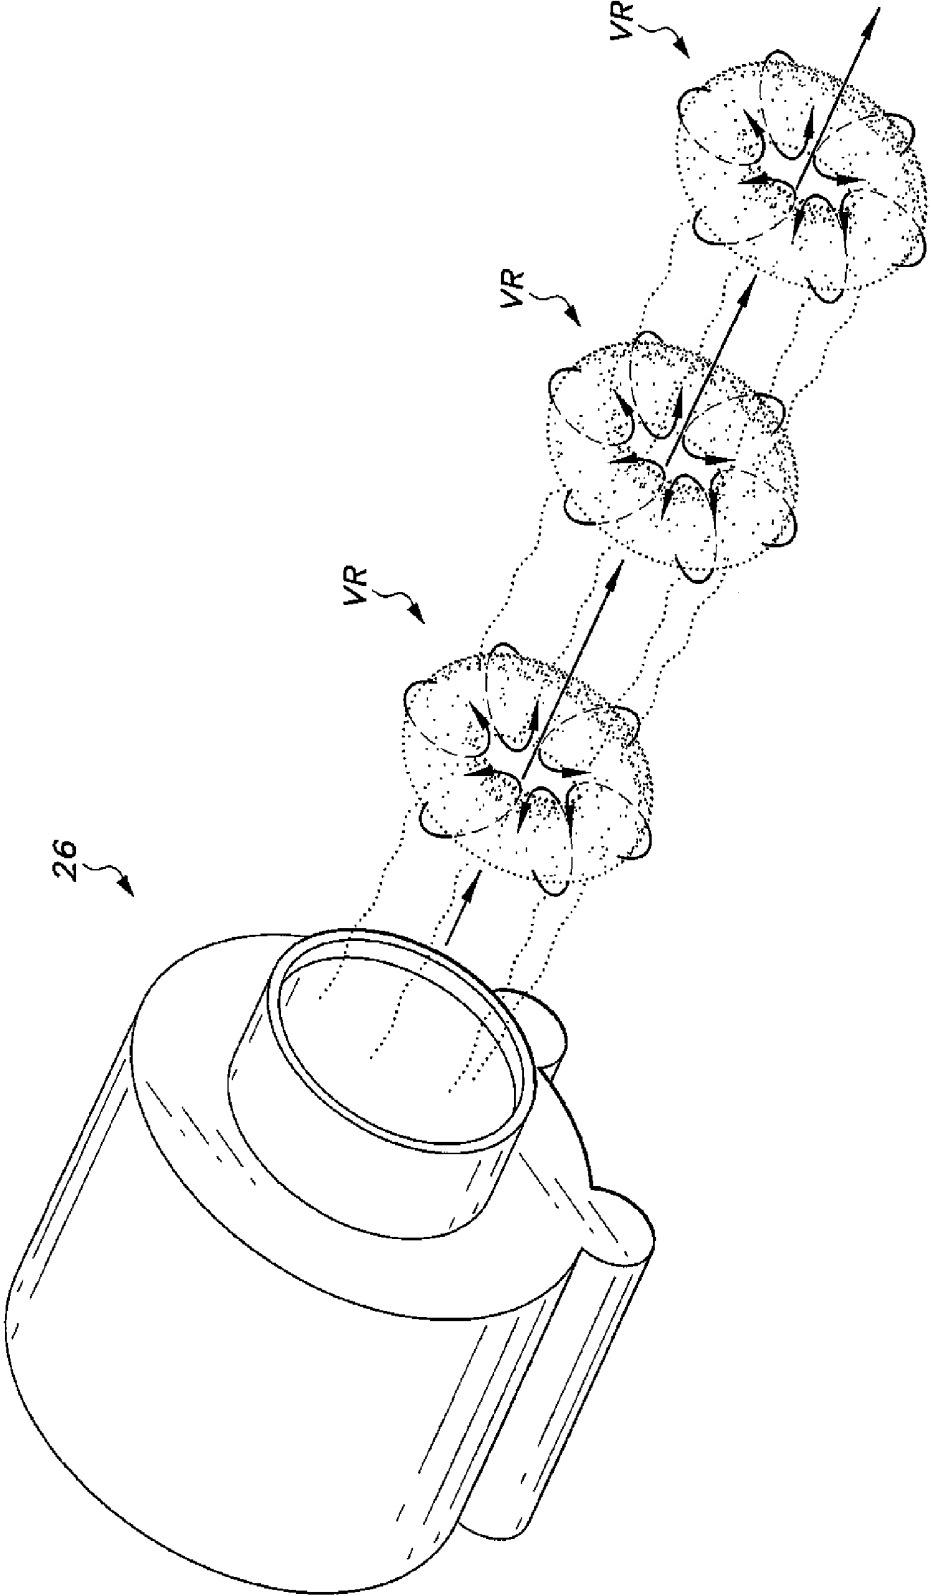


Fig. 3

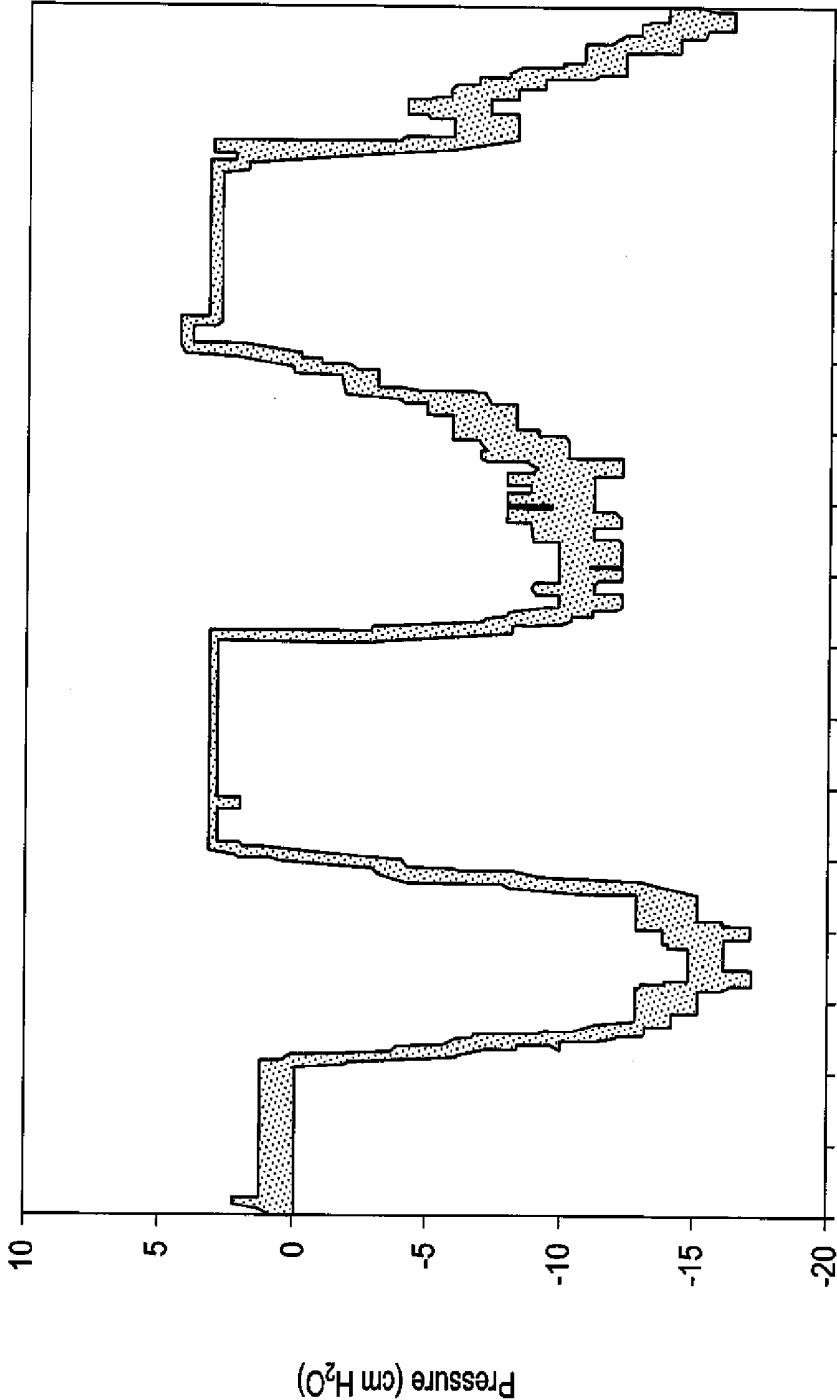

Time (T₁)
Fig. 4

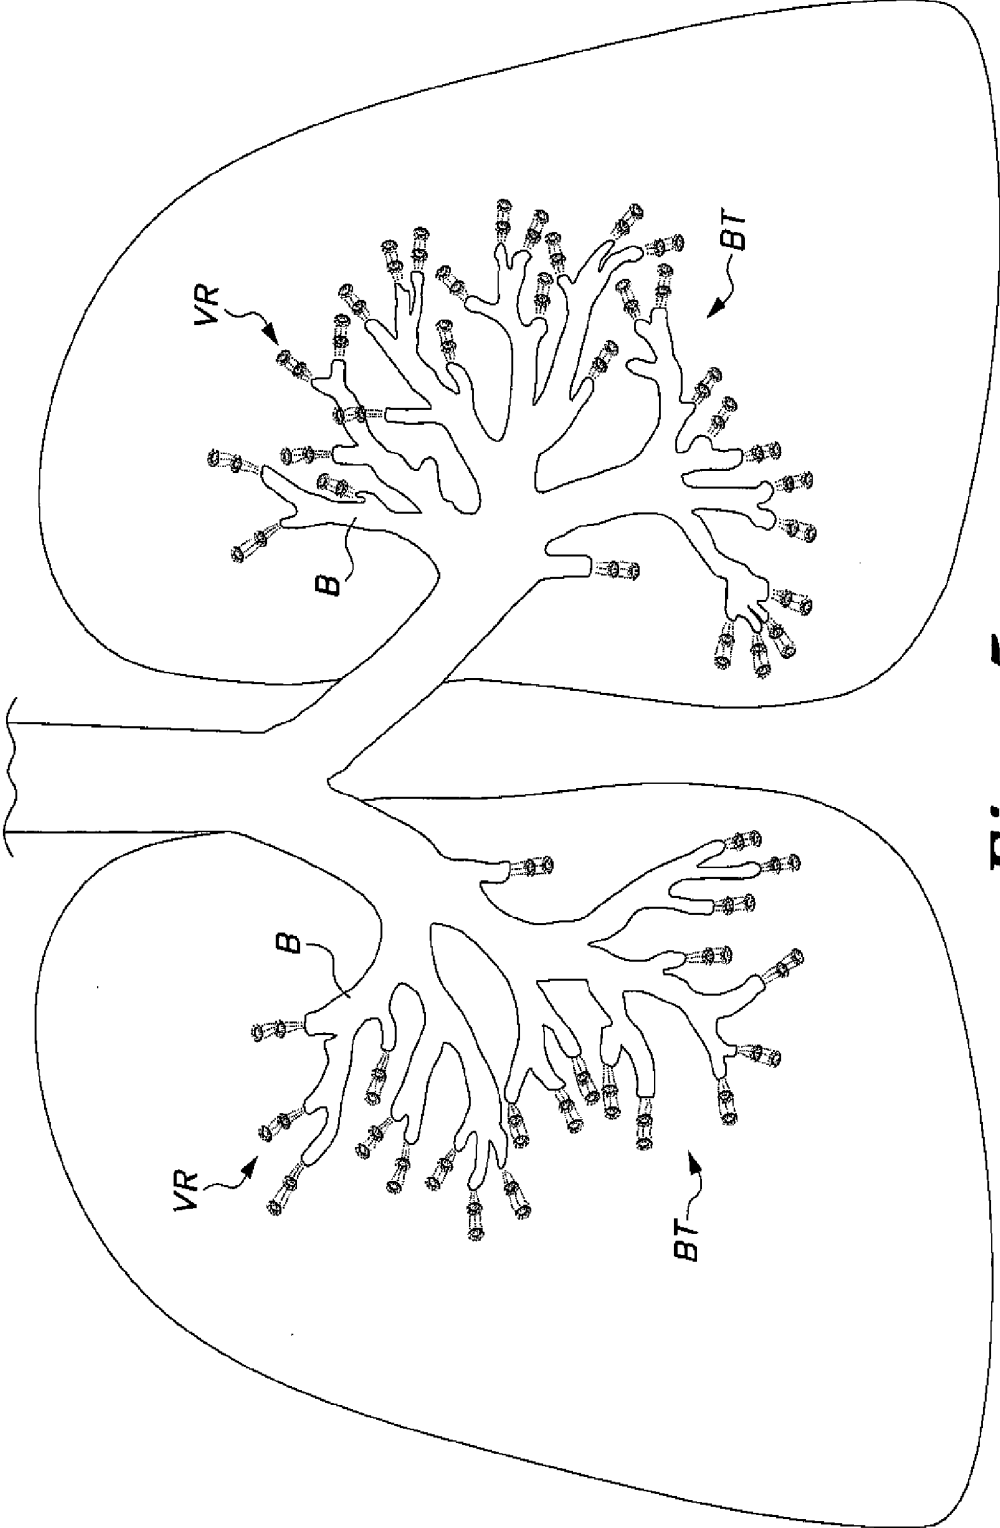


Fig. 5

TOROIDAL RING VENTILATOR

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is related to application Ser. No. 12/076,751, filed Mar. 21, 2008, now abandoned, which claims the benefit of U.S. Provisional Patent Application Ser. No. 60/996,615, filed Nov. 27, 2007.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] The present invention relates to medical devices for respiratory therapy and treatment, and particularly to a mechanical ventilator system that propels mini ring or toroidal vortices into the intrapulmonary space during the inspiratory phase of breathing, while maintaining the intrapulmonary pressure below the atmospheric pressure. These devices are intended to ease the respiratory effort of the patient by augmenting the negative intrapulmonary pressure generated by the patient during the inspiratory phase of breathing.

[0004] 2. Description of the Related Art

[0005] In medicine, mechanical ventilation is a method of mechanically assisting or replacing autonomic breathing when patients cannot do so by themselves adequately. Mechanical ventilation typically follows invasive intubation with an endotracheal or tracheostomy tube, through which air is directly delivered to the patient's lungs. Typically, mechanical ventilation is used in acute settings such as in the Intensive Care Unit (ICU) for a short period of time during a serious illness. Conventional mechanical ventilation systems typically deliver gases into the patient's lungs with a pressure greater than the ambient atmospheric pressure. This is in contrast to older negative pressure ventilators, such as an "iron lung", which generate a negative pressure environment around the patient's thorax to entrain gases into the patient's lungs. Iron lung ventilators are no longer used for typical mechanical ventilation.

[0006] A normal respiratory cycle is divided into an active inspiratory phase and a passive expiratory phase. The atmospheric pressure is approximately 760 mm Hg. Prior to inspiration both the intrapulmonary and the atmospheric pressures are equal, and the intrapleural pressure is 756 mm Hg. During inspiration, active contraction of the diaphragm and the external intercostal muscles cause the downward movement of the diaphragm and the vertical and horizontal movement of the thoracic cage. These movements cause the intrapleural pressure to decrease from 756 mm Hg to 754 mm Hg. The drop in the intrapleural pressure decreases the intrapulmonary pressure from 760 mm Hg to 758 mm Hg. The decrease in the intrapulmonary pressure relative to the atmospheric pressure causes flow of air into the intrapulmonary space until both the pressures are equal. During normal expiratory phase, both the diaphragm and the external intercostal muscles relax, causing them to return to a resting state. This passive movement causes the lungs and the thorax to return to a resting size and position. During deep or forced expiration both the internal intercostal muscles and the abdominal muscles contract causing decrease in the lung and thoracic volumes. This makes the intrapulmonary pressures to exceed the atmospheric pressure causing forced exhalation.

[0007] Modern mechanical ventilators may be classified as pressure cycled, volume cycled, and high frequency oscillator types. These systems all develop some form of positive pres-

sure to deliver the gases into the patient's lungs. The drawbacks of all of the above ventilators are: the use of positive pressures, which may lead to barotrauma to the lung tissue which leads to chronic lung disease (CLD); and inadequate regulation of inspired air/oxygen mixture (FiO_2). Low FiO_2 may cause hypoxemia, and high FiO_2 may cause direct oxygen toxicity to the lungs and remote toxicity to the eyes of the premature infants, which leads to Retinopathy of Prematurity (ROP), which may cause blindness and other eye lesions. These complications of present day ventilators are well known and demonstrated in the medical literature, particularly in the management and care of premature infants.

[0008] Further, although often a lifesaving technique, mechanical ventilation carries many potential complications including pneumothorax, airway injury, alveolar damage, and ventilator-associated pneumonia, among others. Thus, patients are typically weaned off mechanical ventilation as soon as possible.

[0009] Many different types of mechanical ventilators are presently in use. Examples of such ventilators include transport ventilators, intensive care unit (ICU) ventilators, neonatal intensive care unit (NICU) ventilators (which are designed with the preterm neonate in mind; these are a specialized subset of ICU ventilators that are designed to deliver the smaller, more precise volumes and pressures required to ventilate these patients), and positive airway pressure (PAP) ventilators, which are specifically designed for non-invasive ventilation.

[0010] Because a mechanical ventilator is responsible for assisting in a patient's breathing, it must be able to deliver an adequate amount of oxygen in each breath. The "fraction of inspired oxygen" (FiO_2) represents the percent of oxygen in each breath that is inspired. Normal room air has approximately 21% oxygen content by volume. In adult patients who can tolerate higher levels of oxygen for a period of time, the initial FiO_2 may be set at 100% until arterial blood gases can document adequate oxygenation. A FiO_2 of 100% for an extended period of time can be dangerous, but it can protect against hypoxemia from unexpected intubation problems. For infants, and especially in premature infants, avoiding high levels of FiO_2 (>60%) is important.

[0011] Positive end-expiratory pressure (PEEP) is an adjunct to the mode of ventilation used in cases where the functional residual capacity (FRC) is reduced. At the end of expiration, the PEEP exerts pressure to oppose passive emptying of the lung and to keep the airway pressure above the atmospheric pressure. The presence of PEEP opens up collapsed or unstable alveoli and increases the FRC and surface area for gas exchange, thus reducing the size of the shunt. Thus, if a large shunt is found to exist based on the estimation from 100% FiO_2 , then PEEP can be considered and the FiO_2 can be lowered (<60%) to still maintain an adequate PaO_2 , thus reducing the risk of oxygen toxicity.

[0012] In addition to treating a shunt, PEEP is also therapeutic in decreasing the work of breathing. In pulmonary physiology, compliance is a measure of the "stiffness" of the lung and chest wall. The mathematical formula for compliance (C)=change in volume/change in pressure. Therefore, a higher compliance means that only small increases in pressure can lead to large increases in volume, which means the work of breathing is reduced. As the FRC increases with PEEP, the compliance also increases, since the partially inflated lung takes less energy to inflate further.

[0013] In neonatal patients, CLD and ROP are of great concern. As noted above, NICU mechanical ventilators are typically positive pressure mechanical ventilators, converted for use with neonatal infants. CLD and ROP may be caused by barotrauma (which may be caused by positive pressure ventilators) and hyperoxia. A negative pressure ventilator, activated by the inspiratory action of the patient, with auto-regulation of FiO_2 , would aid in avoiding barotrauma, hypoxemia and hyperoxemia. Further, conventional mechanical ventilators, as described above, are typically bulky, often consisting of various pieces of equipment which take up an entire room's worth of space. Such a system is not easily transportable, particularly in emergency situations. Thus, a mechanical ventilator system solving the aforementioned problems is desired.

SUMMARY OF THE INVENTION

[0014] The mechanical ventilator system includes a vortex ring generator in fluid communication with an air oxygen blender for delivering oxygen to a patient. The system is preferably portable and provides a controllable oxygen flow to a patient, ranging from neonatal patients to adults. The system is actuated by the inspiratory effort of the patient. The inspiratory effort of the patient generates a negative air pressure in the range of approximately -4 mm to -6 mm Hg or greater relative to the ambient atmospheric pressure. During the expiratory phase, the mechanical ventilator remains idle, allowing the patient to passively exhale exhalation gases via an exhalation valve (as will be described in greater detail below) with minimal resistance.

[0015] A suitable sensor or measuring device, such as an infrared pulse-oxygen probe, is used for measuring oxygen saturation in a patient's blood. The sensor is in communication with a controller that regulates the fraction of inspired oxygen (FiO_2) of the output oxygen from the air-oxygen blender. The controller is preferably a pre-set processor or other control in communication with the sensor through wires, cables, a wireless electromagnetic interface or the like. The controller is preferably a real-time FiO_2 autoregulator. The real-time FiO_2 autoregulator communicates directly with the air-oxygen blender through wires, cables, a wireless electromagnetic interface or the like.

[0016] The air-oxygen blender receives air from the environment or compressed air, and oxygen from a pure oxygen source and outputs the FiO_2 mix. The FiO_2 mix is delivered to the patient by the vortex generator. A pressure flow gauge may be positioned along the flow path, allowing the user to manually control the pressure of the FiO_2 mix being delivered to the patient.

[0017] An automatic flow sensor, which may be pre-set to detect flow pressure or carbon dioxide or oxygen levels in the FiO_2 mix being delivered to the patient, is preferably positioned further along the flow path, or the like. The automatic flow sensor is in communication with a vortex generator control (which may be a programmable logic controller or the like), which drives a vortex generator trigger circuit to operate the vortex ring generator. Further, the inspiratory effort of the patient also triggers the automatic flow sensor, which, in turn, generates a triggering signal for the actuation of the vortex ring generator (through the vortex generator control and the vortex generator trigger circuit). The inspiratory effort of the patient allows propulsion of mini ring vortices into the intra-

pulmonary space during the inspiratory phase, thereby augmenting the negative intrapulmonary pressure generated by the patient's effort.

[0018] As noted above, exhalations from the patient pass through an expiratory valve, allowing for the release of exhaust gasses from the patient. Further, a mechanism for controlling positive end-expiratory pressure of expired air from the patient is provided, and is preferably coupled to the expiratory valve. The PEEP control mechanism may be a control knob or the like, which is attached to a valve coupled with the expiratory valve.

[0019] In an alternative embodiment, the conventional air-oxygen blender is coupled with a stepper motor (either through an external mechanical coupling, or with the air-oxygen blender and the stepper motor being an integral unit, or servo motor, or electronic air-oxygen blender, or the like). In this embodiment, the real-time FiO_2 autoregulator includes two separate controllers, namely, a pulse-oxygen controller and a separate stepper motor controller, with each being in communication with the other. The two separate controllers may be formed as an integral control unit, which is further in communication with a display (such as a liquid crystal display or the like), allowing the patient's heart rate, oxygen saturation or any other desired information to be displayed to the user. The display is coupled to the integral control unit through wires, cables, a wireless interface or the like.

[0020] The stepper motor controller is in communication with the stepper motor (through wires, cables, a wireless interface or the like), and the controlled FiO_2 mix is delivered to the patient from the air-oxygen blender by any suitable delivery mechanism, such as the vortex ring generator, as described above.

[0021] These and other features of the present invention will become readily apparent upon further review of the following specification and drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0022] FIG. 1 is a block diagram of a toroidal ring ventilator system according to the present invention.

[0023] FIG. 2 is a block diagram of an alternative embodiment of the toroidal ring ventilator system according to the present invention.

[0024] FIG. 3 is a depiction of the vortex rings generated by the vortex ring generator.

[0025] FIG. 4 is a pressure/time graph depicting approximately two and half cycles of respiration.

[0026] FIG. 5 is a view of the air-bronchial tree with ring vortices exiting from the bronchi.

[0027] Similar reference characters denote corresponding features consistently throughout the attached drawings.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0028] The present invention is directed towards a toroidal ring ventilator system 10. As best shown in FIGS. 1 and 2, the toroidal ring ventilator system 10 includes a vortex generator 26 in fluid communication with an air oxygen blender 24 for delivering oxygen to a patient. It is noted that the terms "vortex ring", or "toroidal rings", or "toroidal vortex" define the same characteristic and are used interchangeably throughout the application. The system is preferably portable and provides a controllable oxygen flow to a patient, ranging from neonatal patients to adults. The system is actuated by the

inspiratory effort of the patient. The inspiratory effort of the patient generates a negative air pressure in the range of approximately -4 mm to -6 mm Hg or greater. During the expiratory phase, the mechanical ventilator **10** remains idle, allowing the patient to exhale exhalation gases via an exhalation valve **14** (as will be described in greater detail below) with minimal resistance. Preferably, vortex ring generator **26**, auto-regulated air/oxygen blender **24**, the timing control mechanism (controller) **16**, and the digital display **116** are all encased within a portable housing for compactness and portability of the ventilator system **10**. This system may be adapted for use for patient age ranges from premature infants to adults.

[0029] Air-oxygen blenders are well known in the art, and air-oxygen blender **24** may be any conventional air-oxygen blender. Examples of conventional air-oxygen blenders are shown in U.S. Pat. Nos. 3,727,827; 3,895,642; and 5,014,694, the disclosures of which are hereby incorporated by reference.

[0030] A suitable sensor or measuring device, such as an infrared pulse-oxygen probe **20** is used for measuring oxygen saturation in a patient's blood. The sensor **20'** is in communication with a controller that regulates the fraction of inspired oxygen (FiO_2) of the output oxygen from the air-oxygen blender. The controller is preferably a pre-set processor or other control in communication with the sensor through wires, cables, a wireless electromagnetic interface or the like. The controller is preferably a real-time FiO_2 autoregulator **22**. The real-time FiO_2 autoregulator **22** communicates directly with the air-oxygen blender **24** through wires, cables, a wireless electromagnetic interface or the like. Depending upon the measured oxygen-saturation level in patient P, measured by sensor **20'**, the FiO_2 autoregulator **22** generates control signals, which are received by air-oxygen blender **24** to produce an FiO_2 mix having the desired and necessary proportion of oxygen, depending upon pre-set parameters.

[0031] The real-time autoregulation of blended oxygen is achieved through the use of an oxygen saturation measuring device, such as a pulse-oxygen sensor, which is well-known in the art. Preferably, a miniaturized pulse-oxygen sensor is incorporated in the microprocessor controlled stepper motor driver unit **24**, to be described below. The data received from the oxygen saturation sensor is processed by the microcontroller and sends instructions to the stepper motor driver which, in turn, drives the stepper motor in the desired direction to obtain desired mixture of oxygen/air in the inspired gases to keep the patient's oxygen saturation in the normal range.

[0032] The air-oxygen blender **24** receives air from the environment and oxygen from a pure oxygen source (such as bottled, pressurized oxygen, for example) and outputs the FiO_2 mix, as indicated by the directional arrow in FIG. 1. The FiO_2 mix is delivered to the patient P via mini vortices generated by vortex ring generator **26**, along a flow path which feeds directly to the patient P. A pressure flow gauge **30** may be positioned along the flow path, allowing the user to manually measure and control the pressure of the FiO_2 mix being delivered to the patient. Pressure flow gauge **30** may be any conventional gas pressure flow gauge.

[0033] An automatic flow sensor **18**, which may be pre-set to detect pressure or carbon dioxide levels in the FiO_2 mix being delivered to patient P, is preferably positioned further along the flow path, as shown. Automatic flow sensor **18** may be any suitable, conventional pressure or carbon dioxide sen-

sor. The automatic flow sensor is in communication with a vortex generator control **16** (which may be a programmable logic controller or the like), which drives a vortex generator trigger circuit **28** to operate the vortex ring generator **26**. Further, the inspiratory effort of the patient P also triggers the automatic flow sensor **18**, which, in turn, generates a triggering signal for the actuation of the vortex generator **26** (through the vortex generator control **16** and the vortex generator trigger circuit **28**). Automatic flow sensor **18** can measure changes in pressure generated by the inhalations of the patient, thus triggering delivery of the FiO_2 mix.

[0034] As noted above, the vortex generator system consists of a vortex ring generator **26**, controller **16** and at least one sensor **18**, along with pressure relief valves **14** and exhalation valves **12**, positioned within the gas delivery circuit. The sensor or sensors **18** are placed at the proximal end of the gas delivery circuit, preferably near the ET tube, nose or face mask. These sensors **18** may be used to measure the pressure, flow or carbon dioxide in the expired gases, and this data is then fed into the controller **16**. The data may be used to display the pressure in the gas delivery circuit, and also as trigger input data for the controller **16** to trigger the vortex generator trigger **28**, which controls the vortex ring generator **26**. The vortex ring generator **26** is only triggered during the inspiratory phase, during which the patient generates the required negative pressure, and the vortex ring generator **26** augments the delivery of the gases to the patient's alveoli, as depicted in FIG. 5. As shown in FIG. 5, the air-bronchial tree BT with the ring vortices VR exiting from the bronchi B. This delivery facilitates better gas exchange in the alveoli. As depicted in FIG. 3, vortex ring generators are well known in the art and the explanation of the generation of the vortex ring VR or toroidal vortex is shown in, for example, U.S. Pat. No. 6,689,225, the disclosure of which is hereby incorporated by reference.

[0035] As noted above, exhalations from the patient P pass through an expiratory valve **14**, allowing for the release of exhaust gasses from the patient. Expiratory valve **14** may be any suitable, conventional exhaust valve. Further, a mechanism for controlling positive end-expiratory pressure (PEEP) of expired air from the patient **12** is provided, and is preferably coupled to the expiratory valve **14**, as shown. The PEEP control mechanism **12** may be a control knob or the like, which is attached to a valve coupled with the expiratory valve **14**.

[0036] The vortex ring generator **26** maintains the net intrapulmonary negative pressure relative to the ambient atmospheric pressure throughout the inspiratory phase, which simulates normal breathing, thereby avoiding barotrauma to the lung tissue. The respiratory cycle is essentially under the patient's control, and the vortex ventilator system augments the patient's efforts in the inspiratory phase. The vortex ring generator **26** can be powered by AC or DC electricity, additional electromechanical means, such as solenoids, pneumatic drivers, oscillators, piston pumps, electric or pneumatic reciprocating device, or linear actuators acoustic speakers with square wave generators. As will be described in greater detail below, an LCD display **116** is used to show heart rate and oxygen saturation. Similar LCD displays may be used to show FiO_2 levels, the inspiratory and expiratory pressures and respiratory rate, and other relevant data. FIG. 4 graphically depicts a pressure/time representation of approximately two and half cycles of respiration. The stepwise depiction of inspiratory negative pressure is the augmentation of negative

pressure provided by the vortex ring generator. The positive pressure during the expiratory phase (called “PEEP” or Peak End Expiratory Pressure) is approximately 5 cm H₂O. As shown in FIG. 1, a mechanism for controlling positive end-expiratory pressure (PEEP) of expired air from the patient 12 is provided, and is preferably coupled to the expiratory valve 14, as shown.

[0037] In an alternative embodiment 100, illustrated in FIG. 2, the conventional air-oxygen blender 24 is coupled with a stepper motor 120, either through an external mechanical coupling, or with the air-oxygen blender 24 and the stepper motor 120 being formed as an integral unit 118. In the embodiment of FIG. 2, the real-time FiO₂ autoregulator (which replaces regulator 22 of FIG. 1) includes two separate controllers, namely, a pulse-oxygen OEM (a standard component, which is a conventional system in mechanical ventilators) 112 and a separate stepper motor controller 114, with each being in communication with the other. The two separate controllers 112, 114 may be formed as an integral control unit (as shown by the dashed-line box in FIG. 2), which is further in communication with a display 116 (such as a liquid crystal display or the like), allowing the patient’s heart rate, oxygen saturation or any other desired information to be displayed to the user. The display 116 is coupled to the integral control unit 110 through wires, cables, a wireless interface or the like.

[0038] The stepper motor controller 114 is in communication with the stepper motor 120 (through wires, cables, a wireless interface or the like), and the controlled FiO₂ mix is delivered to the patient from the air-oxygen blender 24 by any suitable delivery means, such as the vortex generator, described above. The control means 112, 114 may be programmable logic controllers or any other suitable processors or control device.

[0039] In system 100, the stepper motor 120 controls the oxygen proportionality module of the air-oxygen blender 24. In use, the infrared pulse-oxygen sensor 20, positioned on the patient P, and communicates this measured level to the pulse-oxygen OEM 112. This, in turn, drives the stepper motor controller 114 to drive stepper motor 120. Preferably, the system 100 is formed as a compact, portable unit.

[0040] In use, and with particular regard to the embodiment of FIG. 2, the ventilator system ventilates the patient’s lungs during the inspiratory phase (i.e., the negative pressure phase of the respiratory cycle). The ventilator then idles during expiratory phase. If the negative pressure ventilation is inadequate to maintain proper gas exchange, the system can be used as a positive pressure ventilator by controlling the exhalation valves 14. When the patient’s lung function improves, the patient may be weaned to negative pressure ventilation in order to minimize the possibility of barotrauma to the lungs. During both the positive and the negative pressure ventilation, the inspired oxygen (FiO₂) is regulated via a closed loop to maintain adequate oxygenation, thereby minimizing the oxygen toxicity and hypoxemia.

[0041] The infrared pulse-oxygen sensor 20 is typically applied to patient’s digit or ear lobe in order to detect the patient’s pulse rate and the level of oxygen saturation. The signal from pulse-oxygen sensor 20 is conveyed to the FiO₂ regulator 22.

[0042] The FiO₂ regulator 22 preferably includes a built-in pulse-oxygen saturation software controller system 112 coupled with a pulse-oxygen data processor 113. The pulse-oxygen OEM 112 and the pulse-oxygen data processor 113 form

an integral pulse-ox controller system, coupled with controller 114. The digital data of the oxygen saturation level and heart rate generated by system 112 is processed by the pulse-oxygen processor 113. The output from the pulse-oxygen processor 113 is used to drive the stepper motor controller 114, which commands the stepper motor 120. The stepper motor regulates the Air/O₂ blender 124 output to deliver the required inspired oxygen (FiO₂) to the patient in order to maintain the desired oxygenation in the patient’s blood. This is accomplished in real time with minimal lag time. Preferably, the system regulates the FiO₂ with each heart beat. It should be understood that additional safety features may be added to the FiO₂ regulator 100 in order to safeguard against any possible malfunctions or failure.

[0043] A flow/pressure or carbon dioxide sensor 18 is located proximally to the patient in the inspiratory path of the gas delivery/exhaust circuit. The signal from the sensor 18 is communicated to the controller 16. The controller 16 then triggers the vortex ring generator 26, via the vortex generator trigger 28, during the inspiratory phase of the respiratory cycle. The vortex ring generator 26 remains idle during the expiratory phase. Thus, the vortex ring generator cycling is governed by the patient’s respiratory effort and assists in the delivery of FiO₂ during the inspiratory phase.

[0044] The FiO₂ output from the air/O₂ blender with stepper motor 24 is fed into the inspiratory path of the gas delivery/exhaust circuit. There is a minimal continuous flow of FiO₂ during the idle phase of the negative ring generator 26. One or more pressure gauges are located close to the patient in the inspiratory part 30 and the expiratory part 31 of the gas delivery/exhaust circuit. This allows medical personnel to monitor the pressures generated during the inspiratory phase of ventilator operation.

[0045] Safety valves 14 are placed in the gas delivery circuit in order to relieve any unexpected rise in pressure, and there are further valves included in the circuit that are used if positive pressure modality is preferred.

[0046] It is to be understood that the present invention is not limited to the embodiments described above, but encompasses any and all embodiments within the scope of the following claims.

We claim:

1. A toroidal ring ventilator system adapted to augment the inspiratory phase of breathing, comprising:

a vortex ring generator;

means for measuring oxygen saturation in a patient’s blood;

an air-oxygen blender for outputting air-oxygen to the patient;

means for delivering the output from the air-oxygen blender to the patient, the means for delivering the output being in fluid communication with the vortex ring generator and the air-oxygen blender, the means for delivering the output from the air-oxygen blender to the patient being actuated during the patient’s inhalations, wherein negative pressure breathing is initiated by the patient during the inspiratory phase of breathing and is augmented by the ring vortices generated by the vortex ring generator, and being idle during the patient’s expiratory phase;

means for controlling a fraction of inspired oxygen in the output from the air-oxygen blender, the means for controlling being in communication with the means for measuring oxygen saturation in a patient’s blood; and

- means for controlling positive end-expiratory pressure of expired air from the patient, the means for controlling positive end-expiratory pressure being in communication with the vortex ring generator.
2. The toroidal ring ventilator system as recited in claim 1, wherein the means for controlling the fraction of inspired oxygen in the output from the air-oxygen blender comprises a stepper motor.
3. The toroidal ring ventilator system as recited in claim 1, wherein the means for measuring oxygen saturation in the patient's blood comprises a sensor adapted to be worn by the patient.
4. The toroidal ring ventilator system as recited in claim 3, wherein the sensor comprises an infrared pulse oxygen probe.
5. The toroidal ring ventilator system as recited in claim 1, further comprising means for selectively actuating said vortex ring generator.
6. The toroidal ring ventilator system as recited in claim 5, further comprising an automatic flow sensor in communication with the means for selectively actuating said vortex ring generator.
7. The toroidal ring ventilator system as recited in claim 6, wherein the automatic flow sensor is a pressure sensor.
8. The toroidal ring ventilator system as recited in claim 6, wherein the automatic flow sensor is a carbon dioxide sensor.
9. The toroidal ring ventilator system as recited in claim 1, further comprising means for measuring and controlling the output from the air-oxygen blender being delivered to the patient.
10. The toroidal ring ventilator system as recited in claim 9, wherein the means for measuring and controlling the output comprises at least one pressure gauge.
11. The toroidal ring ventilator system as recited in claim 1, further comprising a display in communication with the air-oxygen blender and the means for measuring oxygen saturation in a patient's blood.
12. A toroidal ring ventilator system, comprising:
means for measuring oxygen saturation in a patient's blood;
an air-oxygen blender for outputting oxygen to the patient;
means for delivering the output from the air-oxygen blender to the patient, the means for delivering the output being in fluid communication with the air-oxygen blender, the means for delivering the output being actuated during the patient's inhalations and being idle during the patient's exhalations;
a stepper motor coupled with the air-oxygen blender for controlling a fraction of inspired oxygen in the output from the air-oxygen blender, the stepper motor being in communication with the means for measuring oxygen saturation in a patient's blood;
means for displaying the oxygen saturation of the patient's blood; and
a vortex ring generator, the vortex ring generator being in fluid communication with the means for delivering the output from the air-oxygen blender to the patient.
13. The toroidal ring ventilator system as recited in claim 12, wherein the means for measuring oxygen saturation in a patient's blood comprises a sensor adapted to be worn by the patient.
14. The toroidal ring ventilator system as recited in claim 13, wherein the sensor is an infrared pulse oxygen probe.
15. The toroidal ring ventilator system as recited in claim 14, further comprising a pulse oxygen controller in communication with the infrared pulse oxygen probe and the stepper motor.
16. The toroidal ring ventilator system as recited in claim 15, further comprising a stepper motor controller in communication with the pulse oxygen controller and the stepper motor.
17. The toroidal ring ventilator system as recited in claim 16, further comprising means for processing pulse-oxygen data in communication with the pulse oxygen controller and the stepper motor controller, the means for processing pulse-oxygen data transmitting control signals to the stepper motor controller responsive to measured levels of the oxygen saturation of the patient's blood.
18. The toroidal ring ventilator system as recited in claim 12, further comprising means for measuring the patient's heart rate.
19. The toroidal ring ventilator system as recited in claim 18, further comprising means for displaying the patient's heart rate.

* * * * *

专利名称(译)	环形呼吸机		
公开(公告)号	US20150101608A1	公开(公告)日	2015-04-16
申请号	US14/055705	申请日	2013-10-16
[标]申请(专利权)人(译)	SIRIWARDENA MAPATUNAGE一个 饶CHAMKURKISHTIAH P		
申请(专利权)人(译)	SIRIWARDENA, MAPATUNAGE A. 饶, CHAMKURKISHTIAH P.		
当前申请(专利权)人(译)	SIRIWARDENA, MAPATUNAGE A. 饶, CHAMKURKISHTIAH P.		
[标]发明人	SIRIWARDENA MAPATUNAGE A RAO CHAMKURKISHTIAH P		
发明人	SIRIWARDENA, MAPATUNAGE A. RAO, CHAMKURKISHTIAH P.		
IPC分类号	A61M16/00 A61B5/0205 A61B5/1455 A61B5/00 A61M16/10 A61M16/12		
CPC分类号	A61M16/0069 A61M16/1005 A61M16/125 A61B5/14552 A61B5/4836 A61M16/0003 A61B5/6801 A61M16/0051 A61B5/0205 A61B5/742 A61M2016/0039 A61M2016/0027 A61B5/087 A61B5/0836 A61B5/02416 A61M16/024 A61M16/12 A61M2016/1025 A61M2230/06 A61M2230/205		
优先权	60/996615 2007-11-27 US 12/076751 2008-03-21 US		
外部链接	Espacenet USPTO		

摘要(译)

环形呼吸机系统是紧凑且便携的人工呼吸系统。在患者吸气期间，涡流环发生器从空气 - 氧气混合器向患者输送FiO₂ 混合物，但在患者呼气期间保持空转。患者产生的废气通过排气阀释放。在操作期间，通过红外脉冲氧探头测量患者的氧饱和度水平，并且FiO₂ 自动调节器与探头连通以接收氧饱和度水平信号。FiO₂ 自动调节器与空气 - 氧气混合器耦合以控制FiO₂ 混合物的氧气比例。自动压力流量传感器与患者的气道流体连接，以控制涡流环发生器的致动。自动流量传感器与控制器耦合，该控制器致动与涡流发生器通信的涡流环发生器触发电路。

