



US 20150238146A1

(19) **United States**(12) **Patent Application Publication**
Renevey et al.(10) **Pub. No.: US 2015/0238146 A1**(43) **Pub. Date: Aug. 27, 2015**(54) **METHOD FOR DETERMINING AN INSTANT
VELOCITY OF A USER AND FOR
IMPROVING ESTIMATION OF HEART RATE**(71) Applicant: **CSEM Centre Suisse d'Electronique et
de Microtechnique SA - Recherche et
Developpement, Neuchatel (CH)**(72) Inventors: **Philippe Renevey, Lausanne (CH);
Olivier Grossenbacher, Neuchatel (CH)**(21) Appl. No.: **14/627,327**(22) Filed: **Feb. 20, 2015**(30) **Foreign Application Priority Data**


Feb. 21, 2014 (EP) 14156093.8


Publication Classification(51) **Int. Cl.****A61B 5/00** (2006.01)**A61B 5/0205** (2006.01)**A61B 5/11** (2006.01)(52) **U.S. Cl.**CPC **A61B 5/721** (2013.01); **A61B 5/1123**
(2013.01); **A61B 5/1118** (2013.01); **A61B**
5/112 (2013.01); **A61B 5/0205** (2013.01);
A61B 5/6824 (2013.01); **A61B 5/4866**
(2013.01); **A61B 2560/0223** (2013.01); **A61B**
5/02438 (2013.01)

(57)

ABSTRACT

The present disclosure concerns a method for determining an instant velocity of a user using a sensing device destined to be worn on an arm of the user and comprising a motion sensor for measuring a motion signal; the method comprising: measuring the motion signal and identifying when the user is performing a rhythmical activity; identifying when the user is walking or running; providing a relationship between the measured motion signal and corresponding motion features relating to a propulsive impulsion of a user's step; estimating a frequency of the user's step and a user-relative step length of the user using the motion features; and determining a user-relative instant velocity by combining the estimated step frequency and the estimated step length; the instant velocity being determined from the user-relative instant velocity using a calibration factor from the user-relative instant velocity using a calibration factor.

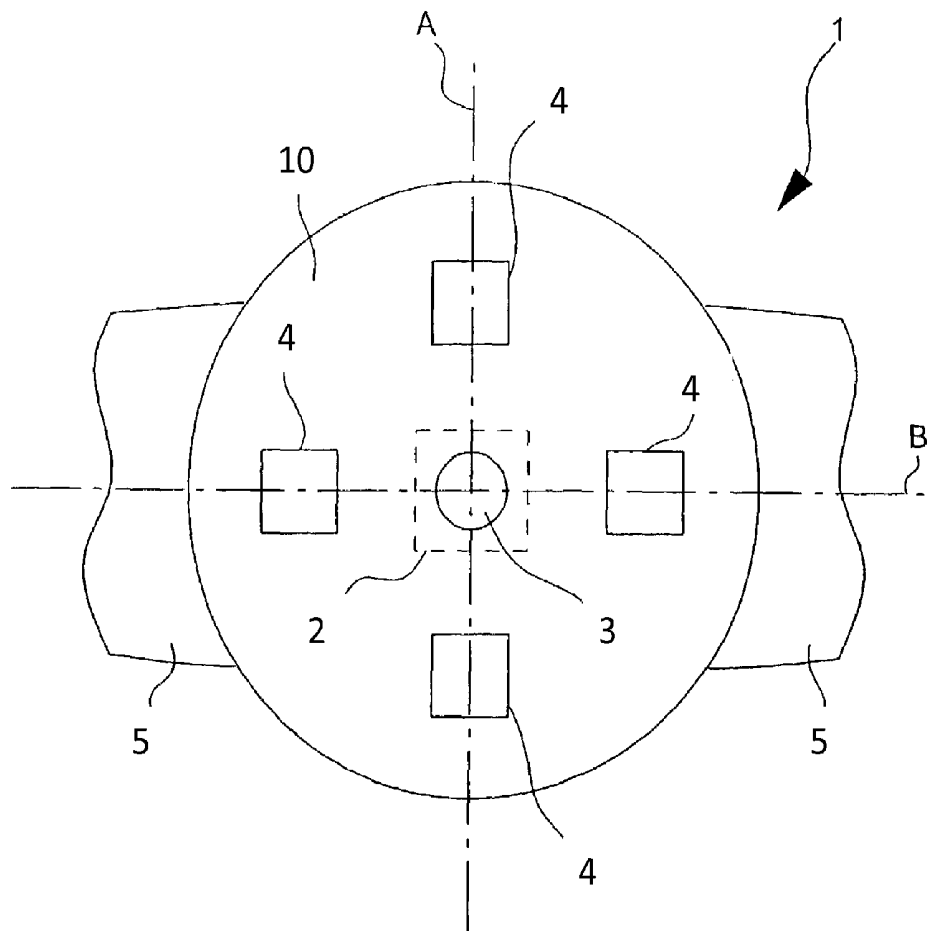

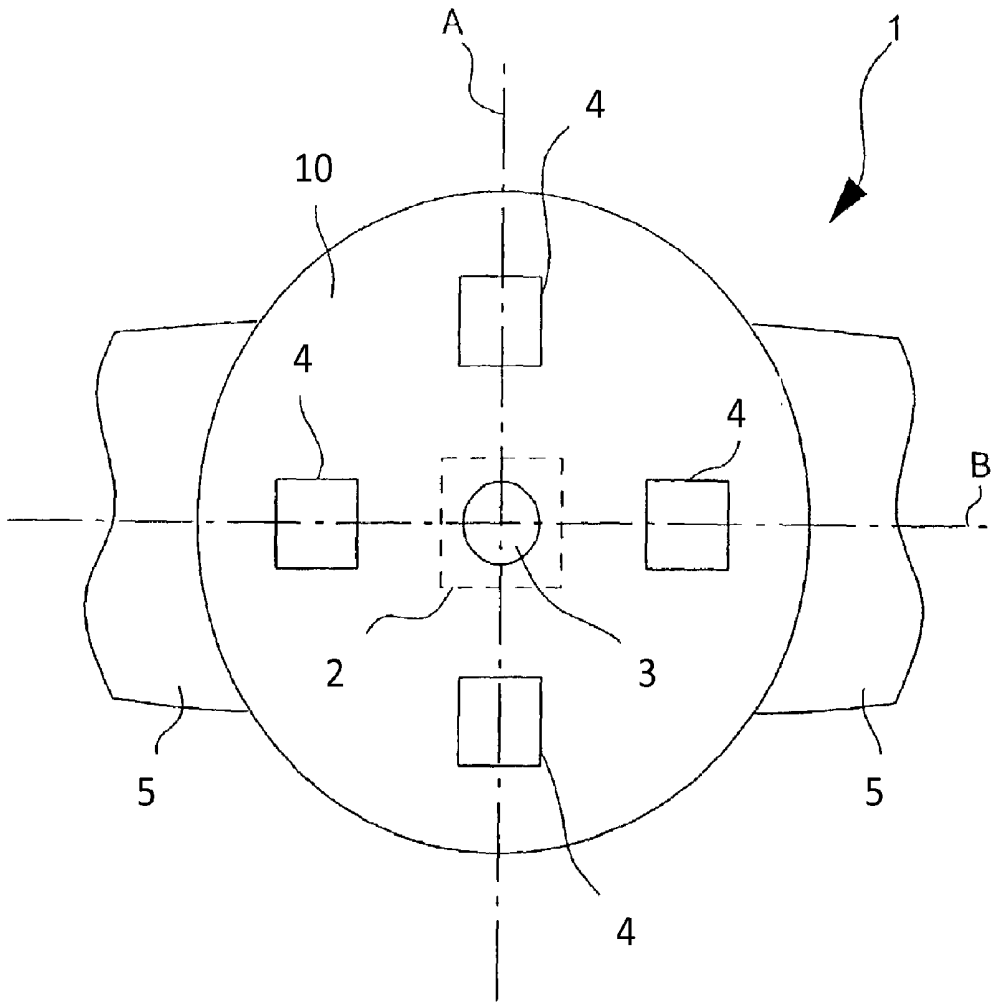

METHOD FOR DETERMINING AN INSTANT VELOCITY OF A USER AND FOR IMPROVING ESTIMATION OF HEART RATE

FIELD

[0001] The present invention concerns a method for determining an instant velocity of a user when walking or running using a sensing device destined to be worn on an arm of the user. The invention also related to using the instant velocity to improve a heart rate estimation measured with a heart rate sensor.

DESCRIPTION OF RELATED ART

[0002] Following the increasing market demand, different systems to estimate the speed of a runner (jogger, walker, etc.) have recently been developed. Such systems make use of different measurement principles, such as accelerometer measurement, the use of GPS, measuring Doppler radar or the principle of the pedometer.

[0003] Portable devices for estimating a speed of a runner usually comprise an accelerometer that is arranged such as to measure a vertical component of the acceleration. To that end, the accelerometer is placed on the shoe of the user or fastened to an ankle or knee of the user.

[0004] Other known methods for determining the speed of a runner use a measuring device that is located close to the runner's center of gravity. For example, an accelerometer can be fastened by means of a belt or clip close to the runner's center of gravity, such as the user's torso or head. Pedometers attachable to the pelvis or footwear and based on mechanical pendulums or accelerometers are also reported.

[0005] In EP1862765, an inertial sensor is placed in a wrist-watch device at the wrists of a runner. However, the device is used solely for measuring the step frequency associated with the user's stepping. Indeed, the arms follow a very different trajectory from that of the user's center of mass and even briefly return backwards at each step. Such devices are possibly useful for approximately evaluating the distance travelled or the number of calories expended during a running session, but are however incapable of analyzing a step length accurately and, consequently the user's speed.

[0006] US2012083705 discloses an activity monitoring system comprising a fixture having size/shape adapted to couple to a location on the user's body and a particular signature; and a portable monitoring device adapted to detect the fixture's particular signature. The monitoring device includes a housing that is adapted to engage the fixture; activity sensors, disposed in the housing, to detect activity of the user and to generate data which is representative of the activity of the user; and processing circuitry, disposed in the housing, to calculate an activity-related quantity of the user using the data which is representative of the activity of the user, wherein the processing circuitry determines the monitoring device is engaging the fixture by detecting the fixture's particular signature, and, in response thereto, calculates the activity-related quantity using data from a set of the activity sensors.

[0007] US2012006112 discloses a method and apparatus of a portable terminal estimate a step length of a pedestrian. An accelerometer detects acceleration caused by a movement of the portable terminal as a pedestrian carrying the portable terminal walks. A gyroscope detects angular velocity caused by the movement of the portable terminal as the pedestrian walks. A controller determines a magnitude of a swinging

motion of the portable terminal by using at least one of the detected acceleration and angular velocity, determines that the portable terminal makes the swinging motion when the magnitude of the swinging motion is equal to or greater than a predetermined value, determines a carrying position of the portable terminal in the pedestrian's body by using at least one of the detected acceleration and angular velocity, and estimates a step length of the pedestrian according to the determined carrying position of the portable terminal.

[0008] US2013080255 discloses step detection and step length estimation techniques include detecting salient points in sensor data of one or more sensors. A step frequency is estimated based on a time interval between the detected salient points. A step length of the step may then be computed based on a nonlinear combination of the estimated step frequency and a function of the sensor data, and/or a step model. Alternatively, the step length of the step may be computed based on a combination of a nonlinear function of the estimated step frequency and a (linear or nonlinear) function of the sensor data, and/or a step model.

[0009] The publication Tracking Fitness With the "Heart Rate-Running Speed Index" by Alex Hutchinson discloses an index which represents the difference between the average speed of a run of a user to a theoretical speed calculated based on average heart rate of the user during the run. If the actual speed is faster than the predicted speed, it suggests an improvement in fitness since the baseline value of the index was calculated.

SUMMARY

[0010] One aim of the present invention is to propose a method free from the limitations of the known methods, in particular a method that makes it possible to determine in a simple manner a velocity of a runner (or walker) using a motion signal measured at the wrist of the user.

[0011] According to the invention, these aims are achieved notably by a method for determining an instant velocity of a user using a sensing device destined to be worn on an arm of the user and comprising a motion sensor for measuring and delivering a motion signal representative of the user's movements when the sensing device is worn; the method comprising:

[0012] measuring the motion signal;

[0013] identifying when the user is performing a rhythmical activity and estimating a fundamental movement frequency of the user from the measured motion signal;

[0014] identifying when the user is walking or running by calculating an activity level of the user using the measured motion signal and the fundamental movement frequency;

[0015] when the user is walking or running, providing a relationship between the measured motion signal and corresponding features of the user's motion which are indicative of a propulsive impulsion of a user's step, by using a bio-mechanical model of human locomotion;

[0016] estimating a frequency of the user's step and estimating a user-relative step length of the user's step using the motion feature;

[0017] determining a user-relative instant velocity by combining the estimated user's step frequency and the estimated user-relative step length; and

[0018] determining the instant velocity from the user-relative instant velocity using a calibration factor.

[0019] In an embodiment, the instant velocity is used for estimating an a priori heart rate of the user, a distance travelled by the user, or an energy expenditure of the user.

[0020] In another embodiment, the proposed system is used in conjunction with an optical measurement system. An a priori estimation of the current heart rate is obtained by the combination of the estimated velocity and a model that relates heart rate and velocity. This a priori heart rate is then used to improve the robustness of the estimation of the heart rate using the optical signals when their quality is poor. Conversely, when the quality of the optical signals is good the model relating the velocity to the a priori heart rate is adapted to the specificities of the user.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021] The invention will be better understood with the aid of the description of an embodiment given by way of example and illustrated by the FIGURES, in which:

[0022] FIG. 1 illustrates schematically a sensor device for measuring a motion signal representative of the user's movements and a photoplethysmographic signal.

DETAILED DESCRIPTION OF POSSIBLE EMBODIMENTS

[0023] FIG. 1 illustrates schematically a sensor device 1 suitable for wearing on a wrist of user comprises a motion sensor 2 for measuring a motion signal representative of the user's movements. In the example of FIG. 1, the sensor device 1 is shown comprising a housing 10 and a strap 5 for attaching the sensor device 1 on the user's wrist. The motion sensor 2 is preferably adapted for measuring motion in three dimensions. For example, the motion sensor 2 can be a three dimensional accelerometer such as a MEMS-based accelerometer adapted to deliver an acceleration (or motion) signal along three axes. It will however be appreciated that other types of accelerometers or motion detecting devices can be used provided they deliver a reliable measure of motion. For example, the motion sensor 2 could be a gyro-sensor of any suitable technology incorporating a one or multi-dimensional accelerometer, or a rotating or vibrating. The motion sensor 2 can further comprise an ADC module (not shown) outputting acquired motion signal.

[0024] Although the sensor device 1 is shown as being worn on a wrist of the user, it is understood that the sensor device 1 is adapted to be worn on an arm of the user, for example at the wrist, somewhere around the arm or at any other location on the arm of the user. A different calibration factor for the sensor device 1 could however be needed depending on the possible different locations of the sensor device 1 on the arm.

[0025] In an embodiment, a method for determining an instant velocity of the user using the sensing device 1 comprises:

[0026] providing the sensing device 1 on the arm of the user;

[0027] measuring the motion signal with the motion sensor 2;

[0028] identifying when the user is performing a rhythmical activity and estimating a fundamental movement frequency of the user from the measured motion signal;

[0029] identifying when the user is walking or running by calculating an activity level of the user using the measured motion signal and the fundamental movement frequency;

[0030] when the user is walking or running, providing a relationship between the measured motion signal and corresponding motion features related to a propulsive impulsion of a user's step by using a bio-mechanical model of human locomotion;

[0031] estimating a frequency of the user's step and estimating user-relative step length of the user's step using the motion features;

[0032] determining a user-relative instant velocity by combining the estimated user's step frequency and the estimated user-relative step length; and

[0033] determining the instant velocity from the user-relative instant velocity using a calibration factor, e.g., by multiplying the user-relative instant velocity by the calibration factor.

[0034] Calculating an activity level of the user using the measured motion signal is carried out by calculating an energy value from the motion signal, for example using the norm of the motion signal. The calculated energy value can be compared with a threshold energy such that when the calculated energy value is equal or below the threshold energy the user can be considered at rest. Conversely, when the calculated energy value is above the threshold energy the user can be considered as performing an activity.

[0035] In the case the calculated energy value is above the threshold energy, calculating an activity level can further comprise detecting segments of the measured motion signal having rhythmical characteristics, for example, by frequency spectral analysis of the motion signal. The fundamental movement frequency can then be extracted from the motion signal through one of the following technique: zero-crossing, parametric or non-parametric spectral estimation, autocorrelation, recurrence plots, and adaptive filters.

[0036] The fundamental movement frequency can then be combined with the calculated energy in order to differentiate between an activity level of the user corresponding to walking, running or another type of rhythmical activity. For example, the ratio of the fundamental movement frequency over the calculated energy can be used for identifying when the user is walking or running. The classification of the activity when a rhythmical motion is detected is based on two features: the amplitude of the motion and the motion frequency. The orientation of the device in the gravity field can be used as an additional feature (generally the fore-arm is close to vertical during walking and close to horizontal during running). Classical classification methods such as Bayesian classifiers, artificial neural network (ANN) or hidden Markov models (HMM) can be used. If not explicitly included in the model (such as in HMM) constraints have to be applied to the output of the classification system in order to discard short duration events (such as checking the display of the device) that would result in misclassification errors and lead to erroneous estimation of the estimated velocity.

[0037] During walking or running, the position of the user's legs relatively to the floor can be divided into two phases: on-floor (impact of the user's foot on the ground) and off-floor (propulsive impulsion of the user's step or propulsive phase). This alternate of impact and propulsive phases produce a rotation moment on the trunk that has to be compensated in order to provide an efficient locomotion. This compensation is provided by a counter-moment provided by the arms moving in anti-phase with the legs. The estimation of the counter-moment produced by the arms is related to the moment produced by the impact and the propulsion phases of

the legs. The compensation further depends on the mass and the length of the user's arms as well as on the angle of the elbow. The inertia moment is related to the mass distribution relatively to the center of rotation. The arm has two degrees of freedom: the shoulder and the elbow. The shoulder is the center of rotation for the damping system (arm). Depending on the velocity and on the walking/running preferences of the user the elbow's angle can vary between approximately 180° (generally during walking activity) and approximately 90° (generally during running activity). The changes of the elbow's angle modify the mass distribution relatively to the shoulder rotation center and therefore modify the inertia moment of the arm. In the present invention the orientation of the motion sensor **2** relatively to the gravity field is used to estimate the angle of the elbow and to compensate the value of the inertia moment of the arm accordingly.

[0038] In an embodiment, the bio-mechanical model comprises an active damper model wherein the arms act as an active damper of the torque produced by the propulsive phase of the legs. In other words, the model comprises a damper model provided by the motion of the arm, wherein the damper model is active to damp the torque produced by the propulsive phase of the legs of the user. The angle of the elbow can be used in the active damper model to compensate the inertia moment of the arm accordingly to the different position of the arm. For example, the arm positions are different between walking and running.

[0039] In another embodiment, the step frequency is estimated by using the motion features. The step frequency can be estimated either by the estimation of time intervals between repetitive events in the acceleration signal (e.g. maxima, minima or zero-crossings), by applying an adaptive filter to track the dominant frequency or by applying a spectral transformation such as Fourier transform and by determining the dominant frequency.

[0040] The step length is dependent on the user, i.e., user's leg length, user's weight, user's running style, etc. Therefore, a user-relative step length is first estimated by using the motion features. A step length can then be determined by using a user-specific calibration. For example, the user-relative step length can be multiplied by a user-specific calibration factor.

[0041] The user-specific calibration factor can be obtained by performing a calibration session where an average velocity is measured. The user-specific calibration factor is then calculated as the ratio of the measured average velocity over the user-relative instant. Alternatively, the calibration factor is obtained by performing a calibration session where a distance travelled by the user is measured. The calibration factor is then calculated as the ratio of the measured distance over a user-relative distance.

[0042] In another variant, the calibration factor is estimated by using morphological parameters of the user in combination with an empirically determined model. The model has to be determined by using measurements from a sufficiently large population of users that spans over the selected set of morphological parameters. The morphological parameters can comprise any one of: gender, age, weight, height, legs' length of the user, or a combination of two or more of the parameters.

[0043] The user-relative instant velocity can be determined by multiplying the estimated step frequency with the estimated step length. The instant velocity can then be obtained by multiplying the relative velocity by the calibration factor.

[0044] In an embodiment, the distance travelled by the user is estimated by using the instant velocity. The estimated distance can then be used for estimating the step length.

[0045] In another embodiment, an energy expenditure of the user is calculated using the instant velocity. For example, the user's energy expenditure can correspond to the instant velocity multiplied by the weight of the user.

[0046] In yet another embodiment, the method further comprises a step of estimating an a priori heart rate of the user using the determined instant velocity and a model relating the heart rate value with the instant velocity. The a priori heart rate can be determined using a linear or non-linear relationship between the determined instant velocity and the heart rate value. The relationship between velocity and heart rate can be identified using recordings of a representative population of users for different running speeds. Since such regressions are user dependent, the method can further comprise the step of using a physiological model including one of age, gender, weight or height of the user.

[0047] In yet another embodiment, the sensing device **1** further comprises a heart rate sensor for measuring a heart rate signal when the sensing device **1** is worn on the arm of the user. The heart rate sensor can be any suitable device for measuring a heart rate signal such as a photoplethysmographic sensor, an electrocardiogram (ECG) or any heart rate estimation system. The a priori heart rate can then be used as additional information about heart rate to improve the measured heart rate estimated from the heart rate signal when the quality of the heart rate signal degrades. In the example of FIG. 1, the heart rate sensor is a photoplethysmographic (PPG) sensor **3, 4** adapted to measure a PPG signal when the sensing device **1** is worn on the user's arm. The motion sensor **2** and the heart rate sensor can be placed in the sensor device **1** such as to form an integrated sensor device. In this latter configuration, the motion signal is better correlated with the measured PPG signal than if the motion sensor **2** is placed further from the multichannel PPG sensor.

[0048] A reliability of the measured heart rate can be determined such as to determine when the measured heart rate reliable or unreliable (for example due to motion artifacts). In the case where the measured heart rate is unreliable, the a priori heart rate can be used in combination with the measured heart rate such as to obtain a more robust value for the measured heart rate.

[0049] The a priori heart rate supplies additional information for the estimation of the measured heart rate. For example, when the heart rate sensor fails to estimate the measured heart rate with sufficient reliability, the a priori heart rate can be used to improve the performance of the heart rate sensor. On the other hand, when the heart rate sensor estimates a measured heart rate with sufficient reliability, the measured heart rate obtained from the heart rate sensor can be used alone. Such a reliable measured heart rate obtained during walking or running can be used to adapt the model relating the velocity to the motion heart rate to the user's specificities.

[0050] In an embodiment, the a priori heart rate is used to filter the measured heart rate around the value of the a priori heart rate.

[0051] In an embodiment not represented, the sensor device **1** further comprises a display arranged for displaying the measured heart rate and/or a priori heart rate. The display can be arranged on the arm of the user, for example by being integrated to the sensor device **1** itself, or in any other location

of the user. The display can be further arranged for displaying any other information including the calculated activity level, the determined instantaneous velocity, the energy expenditure, or the estimated travelled distance.

REFERENCE NUMBERS

- [0052] 1 sensor device
- [0053] 2 motion sensor
- [0054] 3 light source
- [0055] 4 optical receiver
- [0056] 5 strap
- [0057] 10 housing
- [0058] A first axe
- [0059] B second axe

1. Method for determining an instant velocity of a user using a sensing device destined to be worn on an arm of the user and comprising a motion sensor for measuring and delivering a motion signal representative of the user's movements when the sensing device is worn; the method comprising:

measuring the motion signal;

identifying when the user is performing a rhythmical activity and estimating a fundamental movement frequency of the user from the measured motion signal;

identifying when the user is walking or running by calculating an activity level of the user using the measured motion signal and the fundamental movement frequency;

when the user is walking or running, providing a relationship between the measured motion signal and corresponding features of the user's motion which are indicative of a propulsive impulsion of a user's step, by using a bio-mechanical model of human locomotion;

estimating a frequency of the user's step and estimating a user-relative step length of the user's step using the motion features;

determining a user-relative instant velocity by combining the estimated user's step frequency and the estimated user-relative step length; and

determining the instant velocity from the user-relative instant velocity using a calibration factor.

2. Method according to claim 1,

wherein the calibration factor is determined using one of: cumulated distance when the user is walking or running, average velocity of the user when walking or running, or a morphological parameter of the user.

3. Method according to claim 1,

wherein said model comprises a damper model provided by the motion of the arm, wherein the damper model is active to damp the torque produced by the propulsive phase of the legs of the user.

4. Method according to claim 1,

wherein said estimating a step frequency comprises identifying a time of impact of the user's foot using the motion features.

5. Method according to claim 1,

wherein said estimating a step length further comprises using a calibration measurement taken at the determined instantaneous velocity or at an estimated travelled distance by the user.

6. Method according to claim 1,

wherein combining the estimated step frequency and the estimated step length comprised multiplying the estimated step frequency with the estimated step length.

7. Method according to claim 1,

further comprising multiplying the estimated user-relative step length by a user-specific calibration factor.

8. Method according to claim 6,

wherein the calibration factor is obtained by measuring an average velocity or a distance travelled by the user when the user is walking or running.

9. Method according to claim 6,

wherein the calibration factor is estimated by using morphological parameters of the user in combination with an empirically determined model.

10. Method according to claim 1,

further comprising estimating an a priori heart rate of the user by using the determined instant velocity and a model relating a heart rate value with the instant velocity.

11. Method according to claim 10,

wherein the model comprises a linear or a non-linear relationship between the determined instant velocity and said heart rate value.

12. Method according to claim 10,

wherein the model comprises a physiological model including one of age, gender, weight or height of the user.

13. Method according to claim 10,

wherein the sensing device further comprises a heart rate sensor adapted to measure a heart rate signal when the sensing device is worn; and

wherein the method further comprises measuring the heart rate signal and estimating a measured heart rate from the measured heart rate signal.

14. Method according to claim 13,

wherein said estimating a measured heart rate comprises determining a reliability of the measured heart rate; and wherein the a priori heart rate is used in combination with the measured heart rate when the measured heart rate is unreliable.

15. Method according to claim 14,

further comprising user-specifically adapting the model by using the measured heart rate when the measured heart rate is reliable.

16. Method according to claim 1,

further comprising estimating a distance travelled by the user by using the integration of the determined instant velocity.

17. Method according to claim 1,

further comprising calculating an energy expenditure of the user by using the determined instant velocity.

* * * * *

专利名称(译)	用于确定用户的即时速度和用于改善心率估计的方法		
公开(公告)号	US20150238146A1	公开(公告)日	2015-08-27
申请号	US14/627327	申请日	2015-02-20
申请(专利权)人(译)	CSEM中心SUISSE D'电子与DE显微技术SA - RECHERCHE ET DEVELOPPEMENT		
当前申请(专利权)人(译)	CSEM中心SUISSE D'电子与DE显微技术SA - RECHERCHE ET DEVELOPPEMENT		
[标]发明人	RENEVEY PHILIPPE GROSSENBACHER OLIVIER		
发明人	RENEVEY, PHILIPPE GROSSENBACHER, OLIVIER		
IPC分类号	A61B5/00 A61B5/0205 A61B5/11		
CPC分类号	A61B5/721 A61B5/1123 A61B5/1118 A61B5/112 A61B5/02438 A61B5/6824 A61B5/4866 A61B2560 /0223 A61B5/0205 A61B5/02416 A61B5/681 A61B5/7221 A61B2562/0219 G01C22/006 G06K9/00342		
优先权	2014156093 2014-02-21 EP		
其他公开文献	US9592013		
外部链接	Espacenet USPTO		

摘要(译)

本公开涉及一种用于使用预定佩戴在用户的手臂上的感测装置来确定用户的瞬时速度的方法，并且该方法包括用于测量运动信号的运动传感器；该方法包括：测量运动信号并识别用户何时进行节奏活动；识别用户何时行走或跑步；提供测量的运动信号与与用户步骤的推进冲击相关的相应运动特征之间的关系；使用运动特征估计用户步数的频率和用户的用户相对步长；通过组合估计的步进频率和估计的步长来确定用户相对时刻速度；使用校准因子，使用来自用户相对瞬时速度的校准因子，根据用户相对瞬时速度确定瞬时速度。

