



US010130310B2

(12) **United States Patent**
Alpert et al.

(10) **Patent No.:** **US 10,130,310 B2**
(45) **Date of Patent:** **Nov. 20, 2018**

(54) **BEDSIDE CONTROLLER FOR ASSESSMENT OF VESSELS AND ASSOCIATED DEVICES, SYSTEMS, AND METHODS**

(71) Applicant: **Volcano Corporation**, San Diego, CA (US)

(72) Inventors: **Howard David Alpert**, El Dorado Hills, CA (US); **David Anderson**, Temecula, CA (US); **Asher Cohen**, Sacramento, CA (US); **Fergus Merritt**, Escondido, CA (US); **Meng Lim**, San Diego, CA (US)

(73) Assignee: **VOLCANO CORPORATION**, San Diego, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 532 days.

(21) Appl. No.: **14/850,720**

(22) Filed: **Sep. 10, 2015**

(65) **Prior Publication Data**

US 2016/0073972 A1 Mar. 17, 2016

Related U.S. Application Data

(60) Provisional application No. 62/049,265, filed on Sep. 11, 2014.

(51) **Int. Cl.**
A61B 5/026 (2006.01)
A61B 5/0215 (2006.01)

(Continued)

(52) **U.S. Cl.**
CPC **A61B 5/7445** (2013.01); **A61B 5/026** (2013.01); **A61B 5/02007** (2013.01);
(Continued)

(58) **Field of Classification Search**

CPC A61B 5/7445; A61B 5/02007; A61B 5/02158; A61B 5/026; A61B 5/7425; A61B 5/743; A61B 5/7475

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

7,134,994 B2 * 11/2006 Alpert A61B 5/0215 600/300

8,754,865 B2 6/2014 Merritt et al.
(Continued)

FOREIGN PATENT DOCUMENTS

WO WO2012/093260 1/2012
WO WO2012/093266 1/2012


(Continued)

Primary Examiner — Navin Natnithithadha

(57) **ABSTRACT**

Devices, systems, and methods for evaluating a vessel of a patient are provided. The method includes outputting, to a touch-sensitive display of a bedside controller, a screen display including: a visual representation of a first pressure ratio of pressure measurements obtained by first and second instruments positioned within a vessel while the second instrument is moved from a distal position to a proximal position relative a stenosis and the first instrument remains stationary; and a first proximal pressure waveform and a first distal pressure waveform; receiving, through the touch-sensitive display of the bedside controller, a user touch input on the first proximal pressure waveform and/or the first distal pressure waveform identifying a time at which pressure measurements were obtained; and modifying the screen display, in response to the user touch input, to further include a visual representation of the obtained pressure measurements corresponding to the identified time.

20 Claims, 18 Drawing Sheets

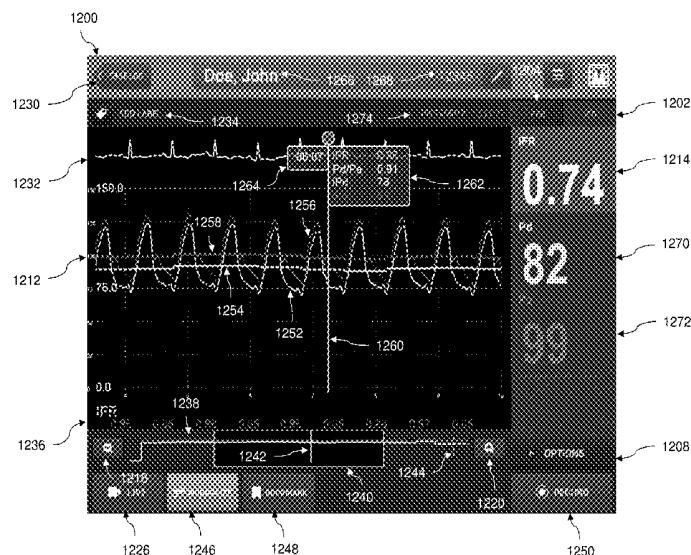

Page 2

(51)	Int. Cl. A61B 5/00 (2006.01) A61B 5/02 (2006.01)	2007/0060822 A1 *	3/2007	Alpert	A61B 5/0215 600/481
(52)	U.S. Cl. CPC A61B 5/02158 (2013.01); A61B 5/743 (2013.01); A61B 5/7425 (2013.01); A61B 5/7475 (2013.01)	2010/0234698 A1 *	9/2010	Manstrom	A61M 5/007 600/301
(58)	Field of Classification Search USPC 600/481, 483–486, 488, 490–499 See application file for complete search history.	2013/0046190 A1 2013/0345574 A1 *	2/2013 12/2013	Davies Davies	A61B 5/02007 600/486
(56)	References Cited U.S. PATENT DOCUMENTS	2014/0135633 A1 2014/0258743 A1 2015/0025330 A1 2015/0025398 A1 2015/0080749 A1 *	5/2014 9/2014 1/2015 1/2015 3/2015	Anderson et al. Nool Davies Davies Anderson	A61B 5/0215 600/483
	9,026,384 B2 *	5/2015	Davies	A61B 5/02007 702/182	FOREIGN PATENT DOCUMENTS
	9,339,348 B2 *	5/2016	Davies	A61B 5/742	WO WO2013/028612 8/2012
	9,364,153 B2 *	6/2016	Merritt	A61B 5/7278	WO WO2012/154335 11/2012
	9,775,524 B2 *	10/2017	Davies	A61B 5/02007	
	2003/0216621 A1 *	11/2003	Alpert	A61B 5/0215 600/300	
					* cited by examiner

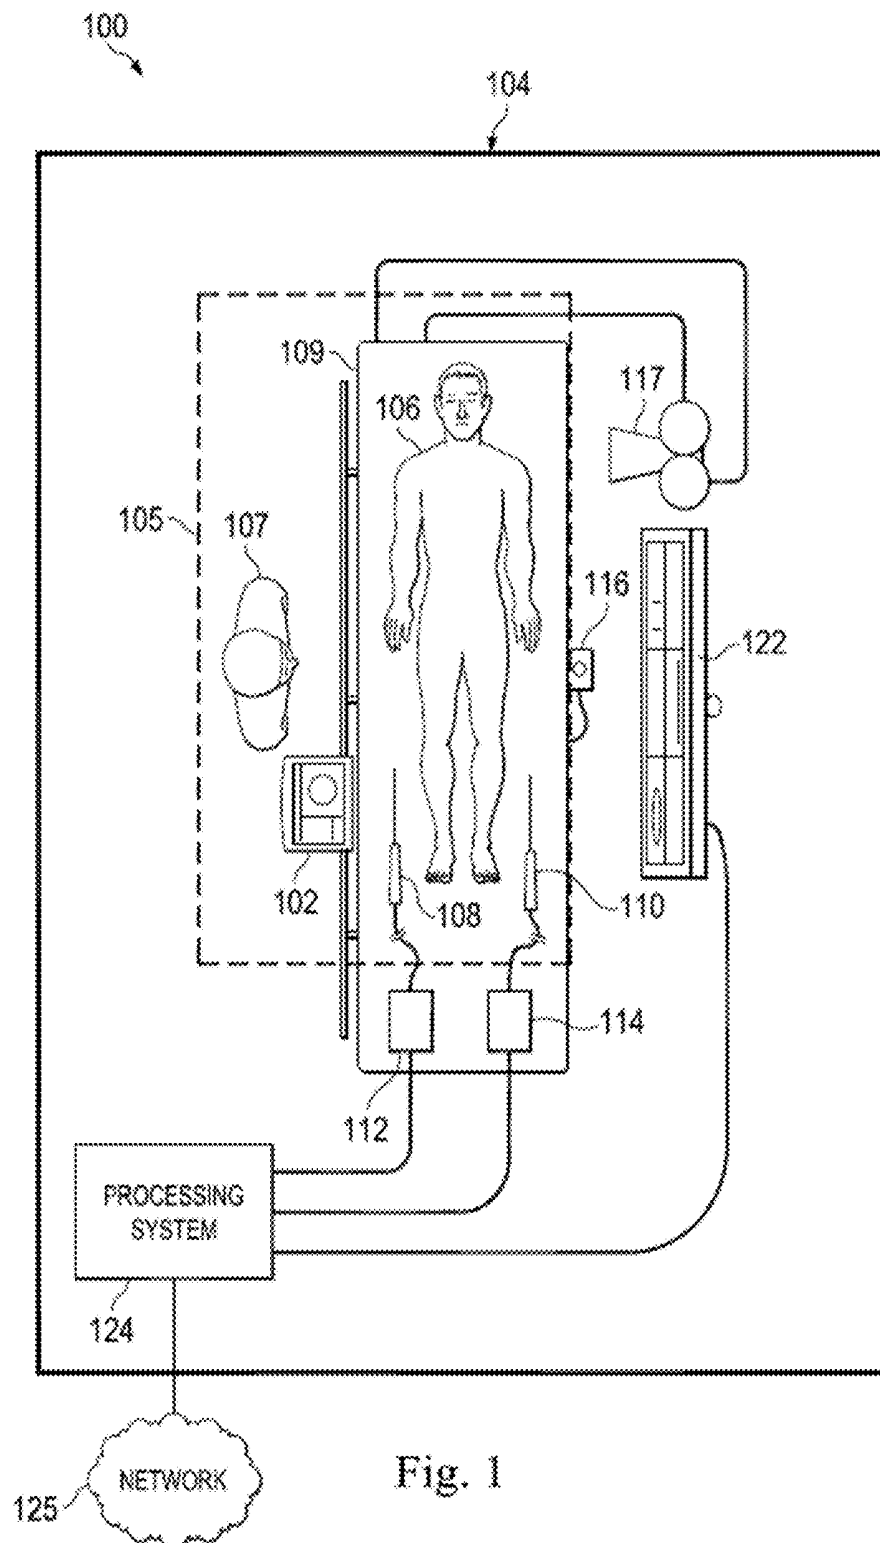


Fig. 1

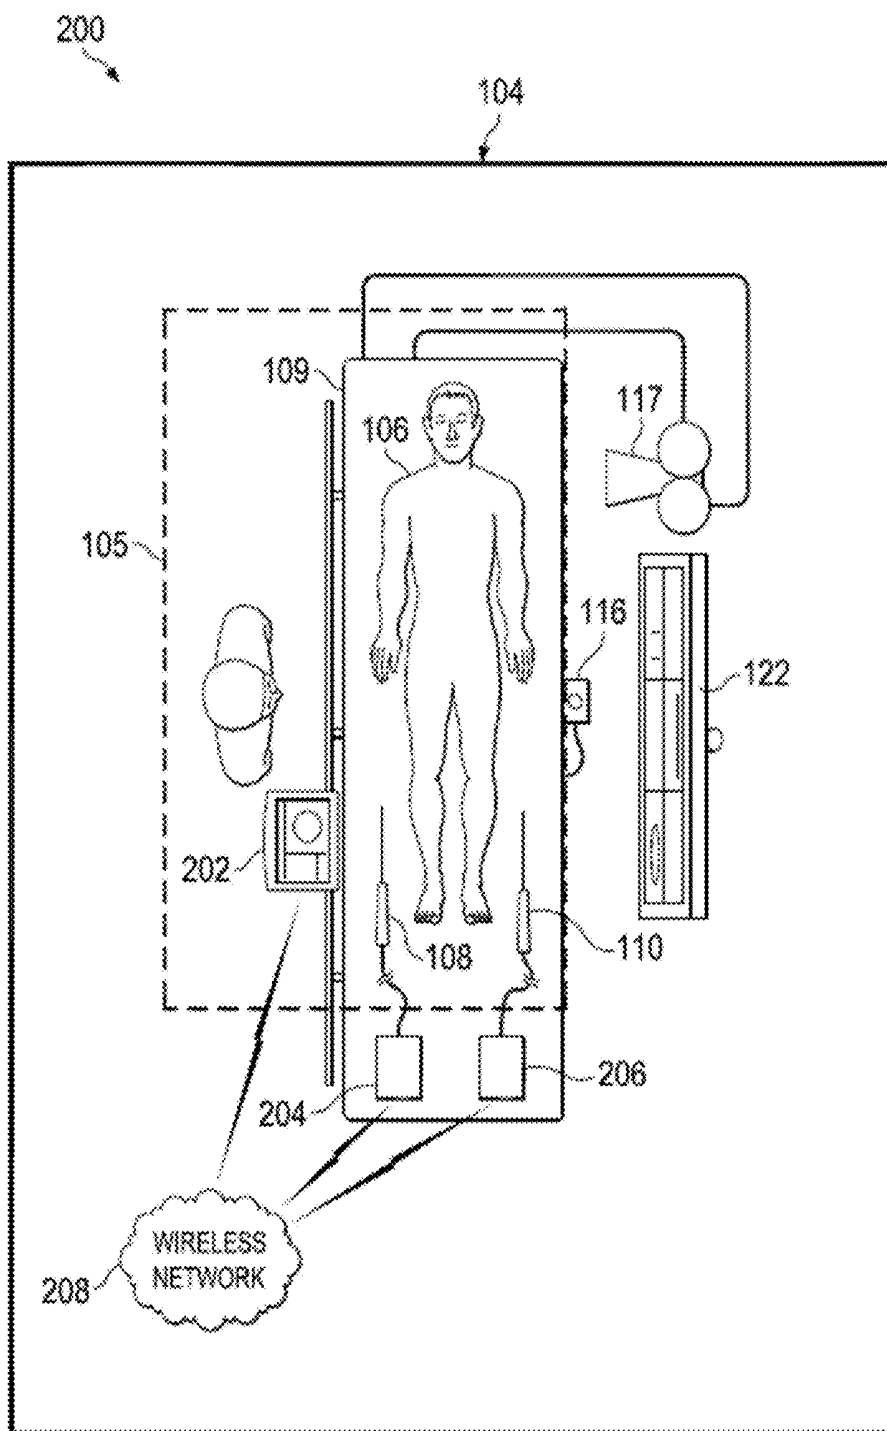
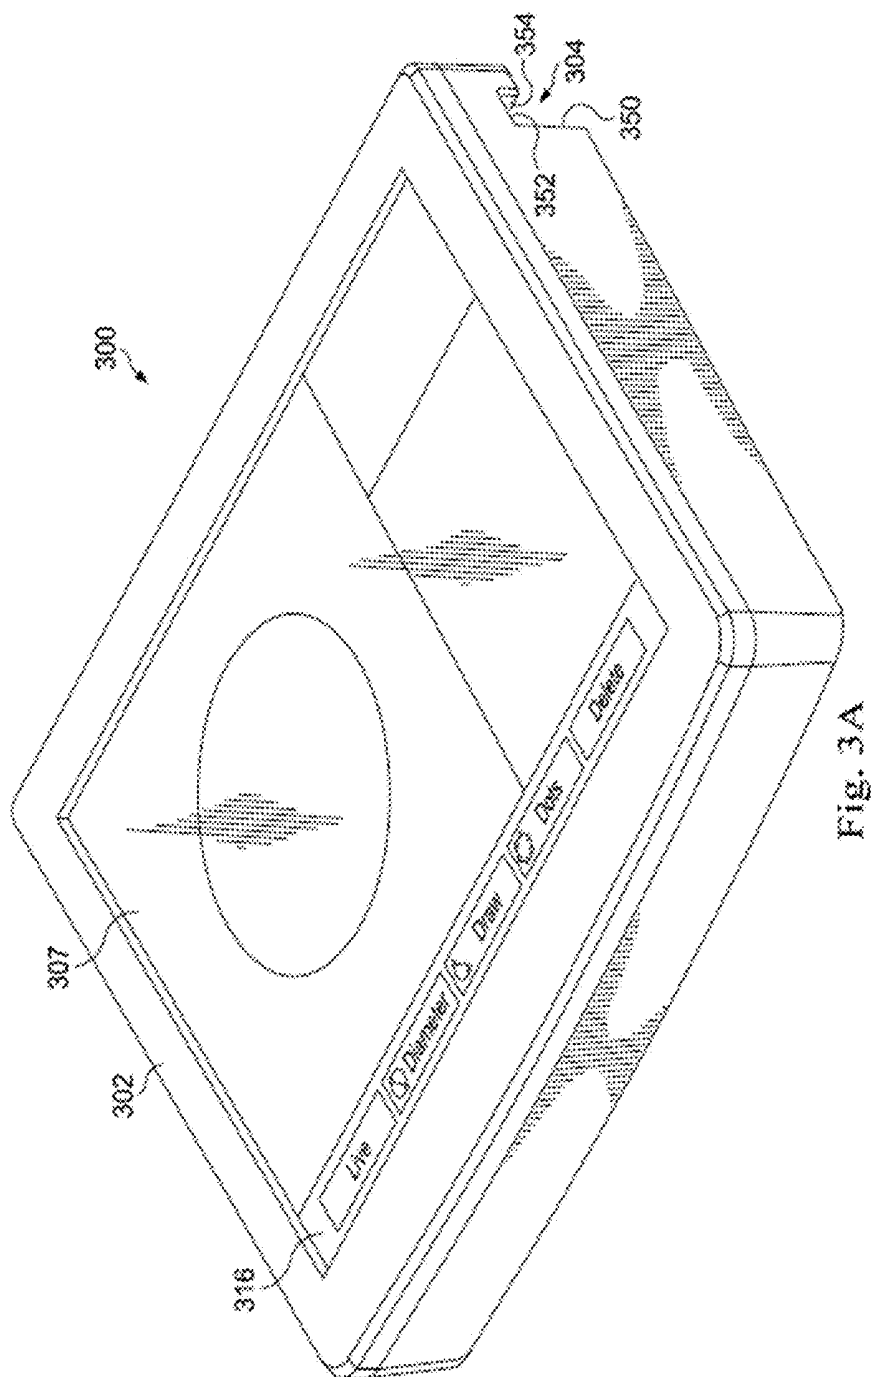


Fig. 2



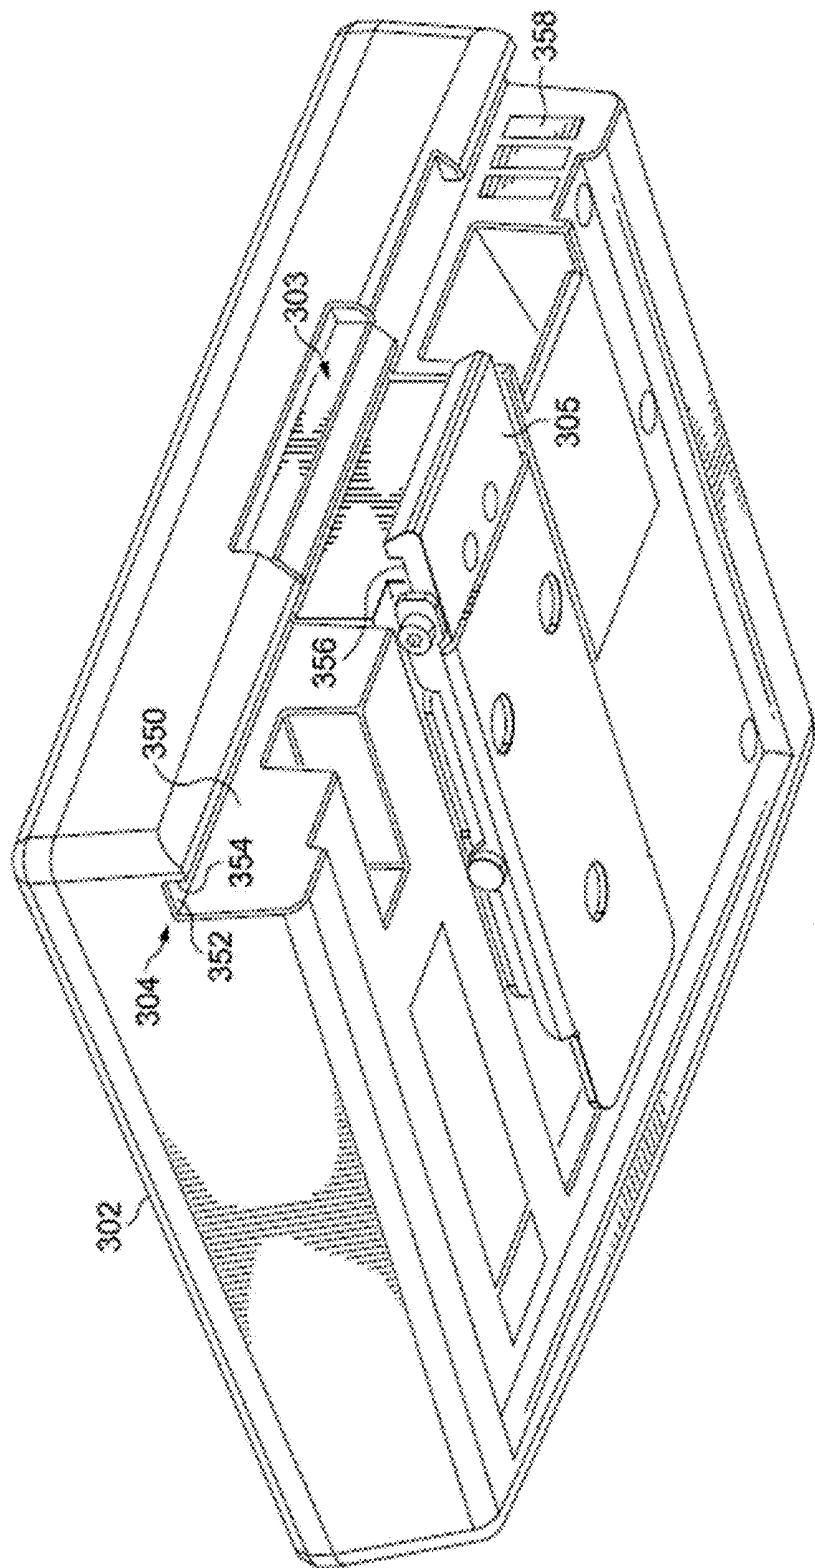
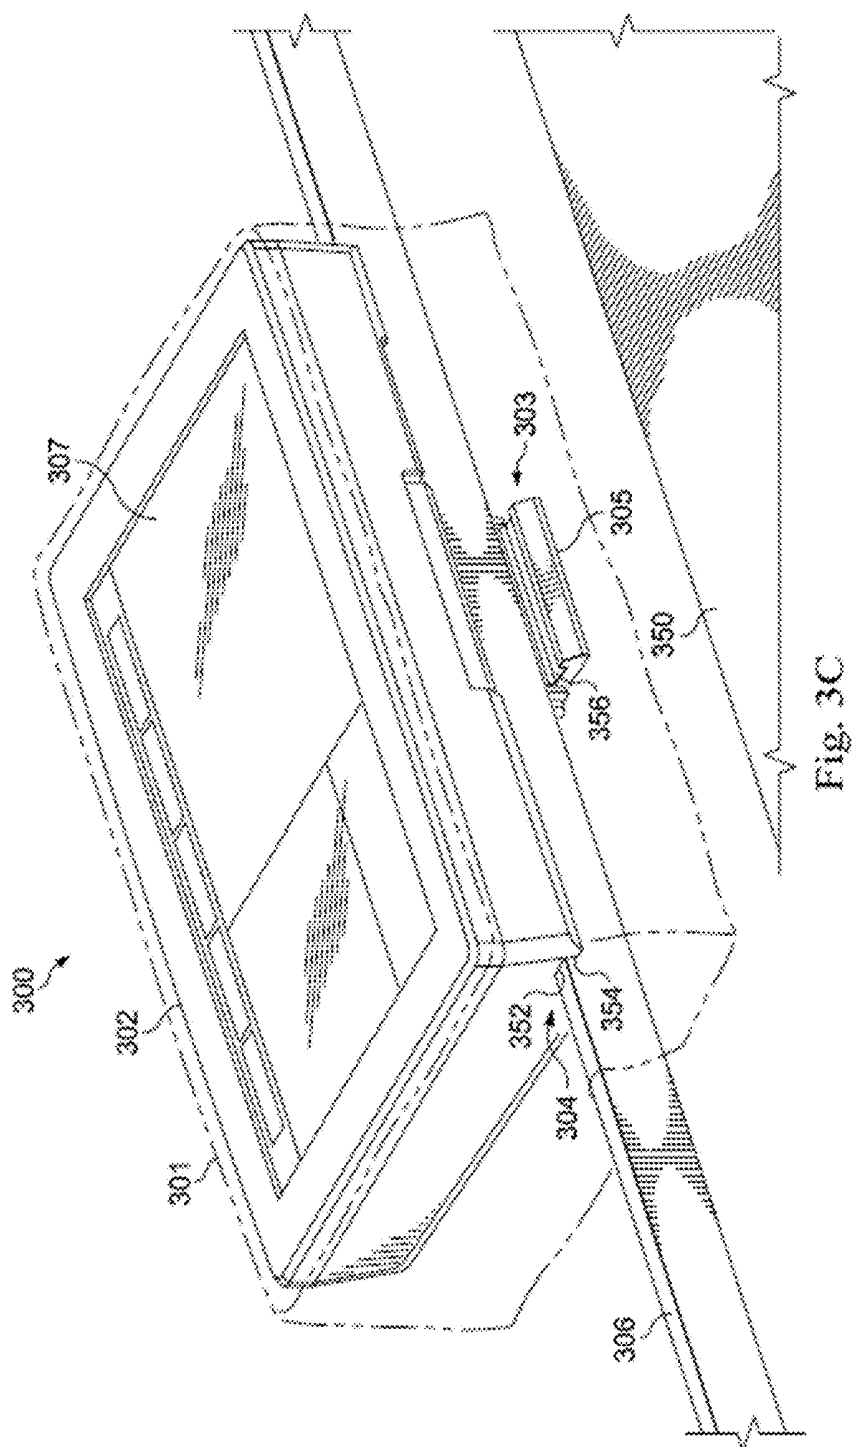


Fig. 3B



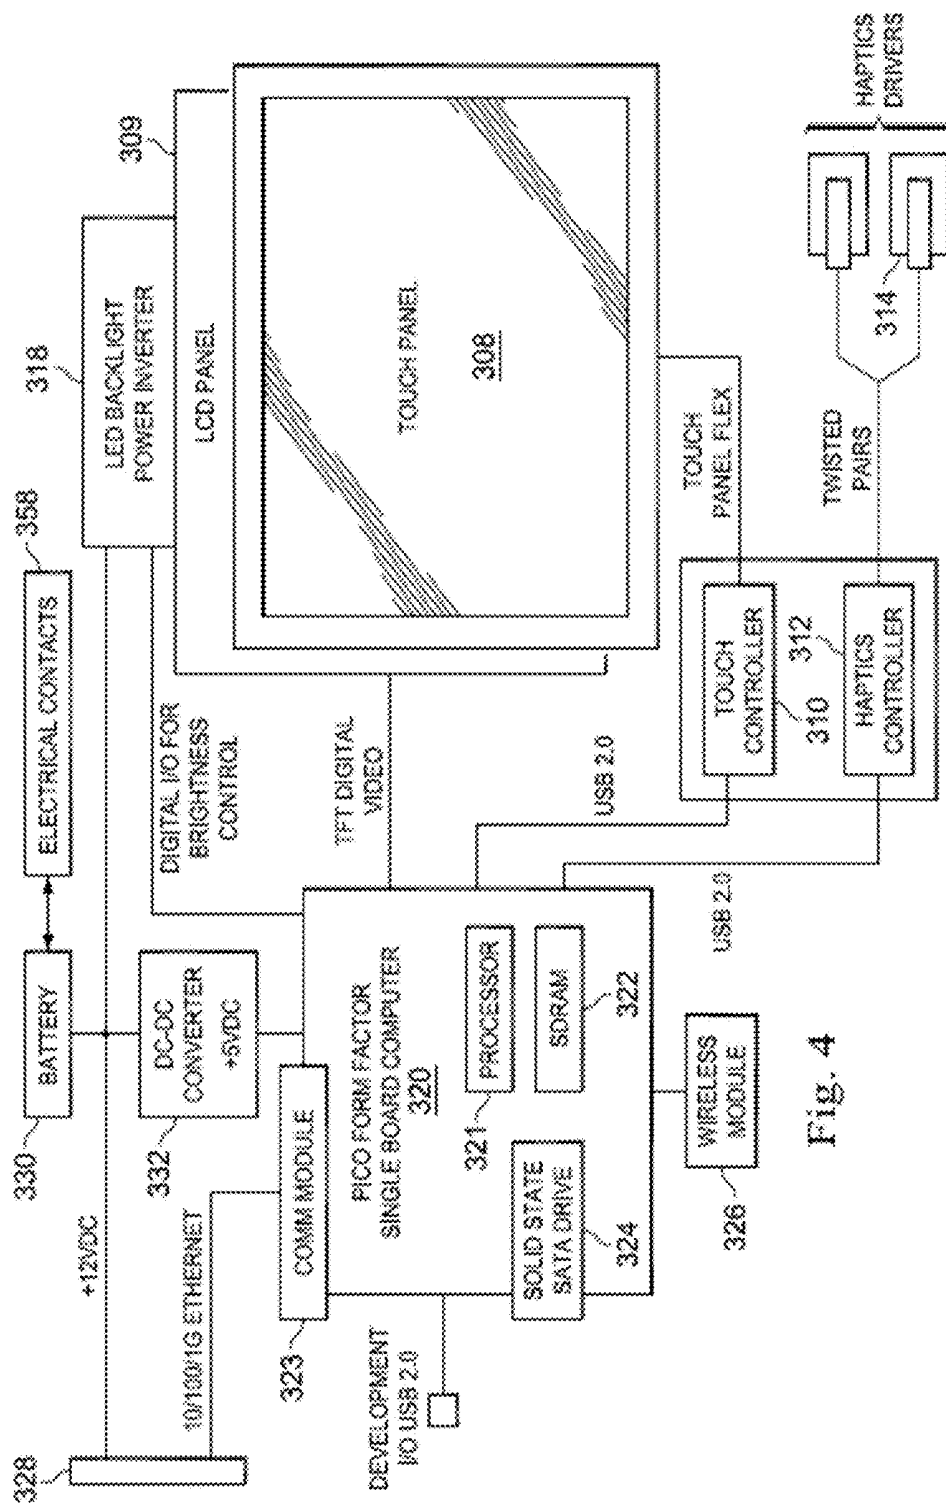


Fig. 4

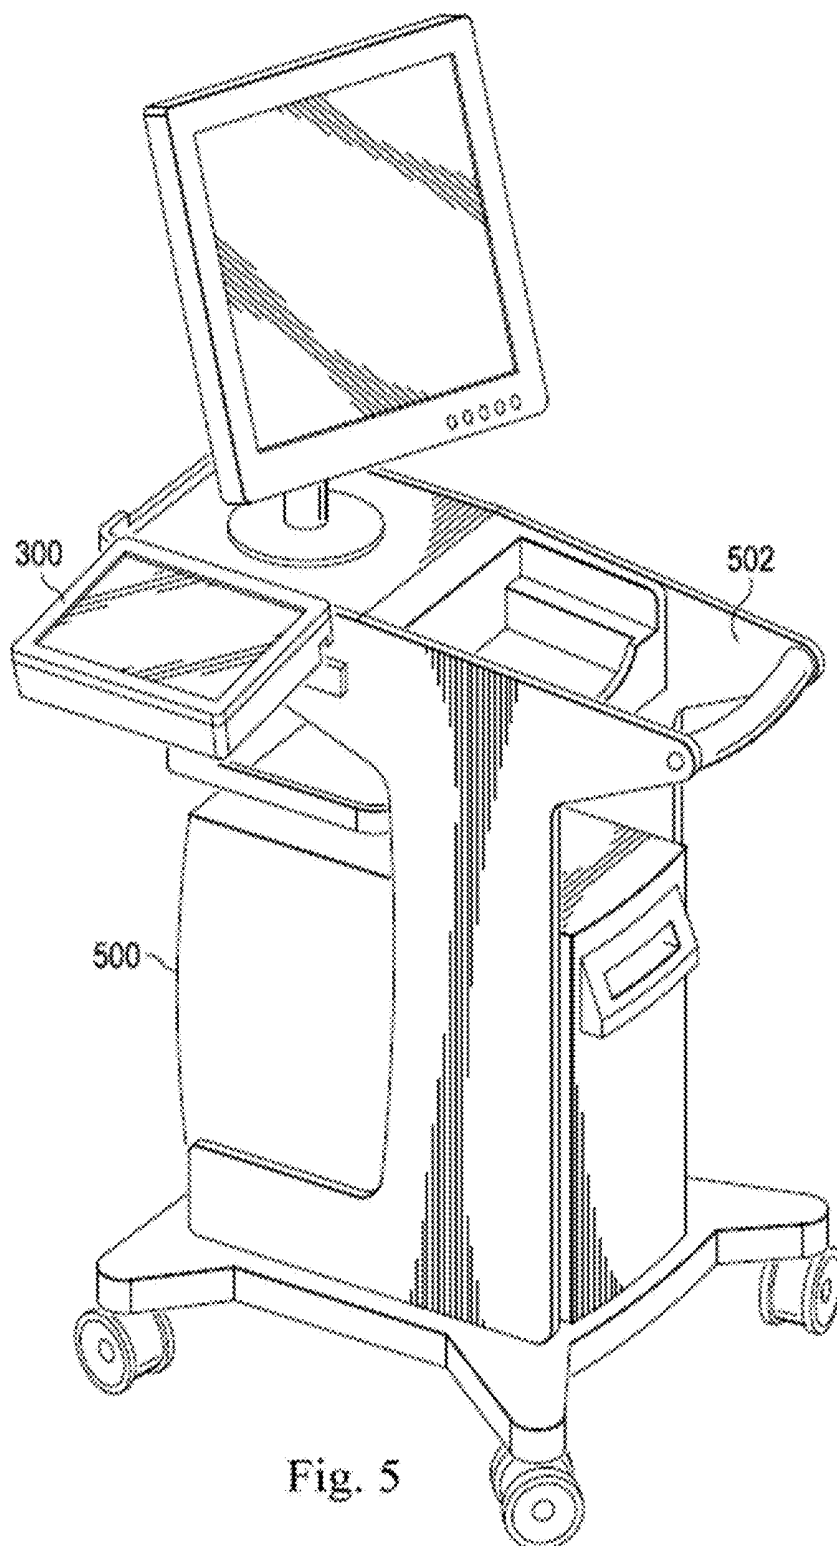


Fig. 5

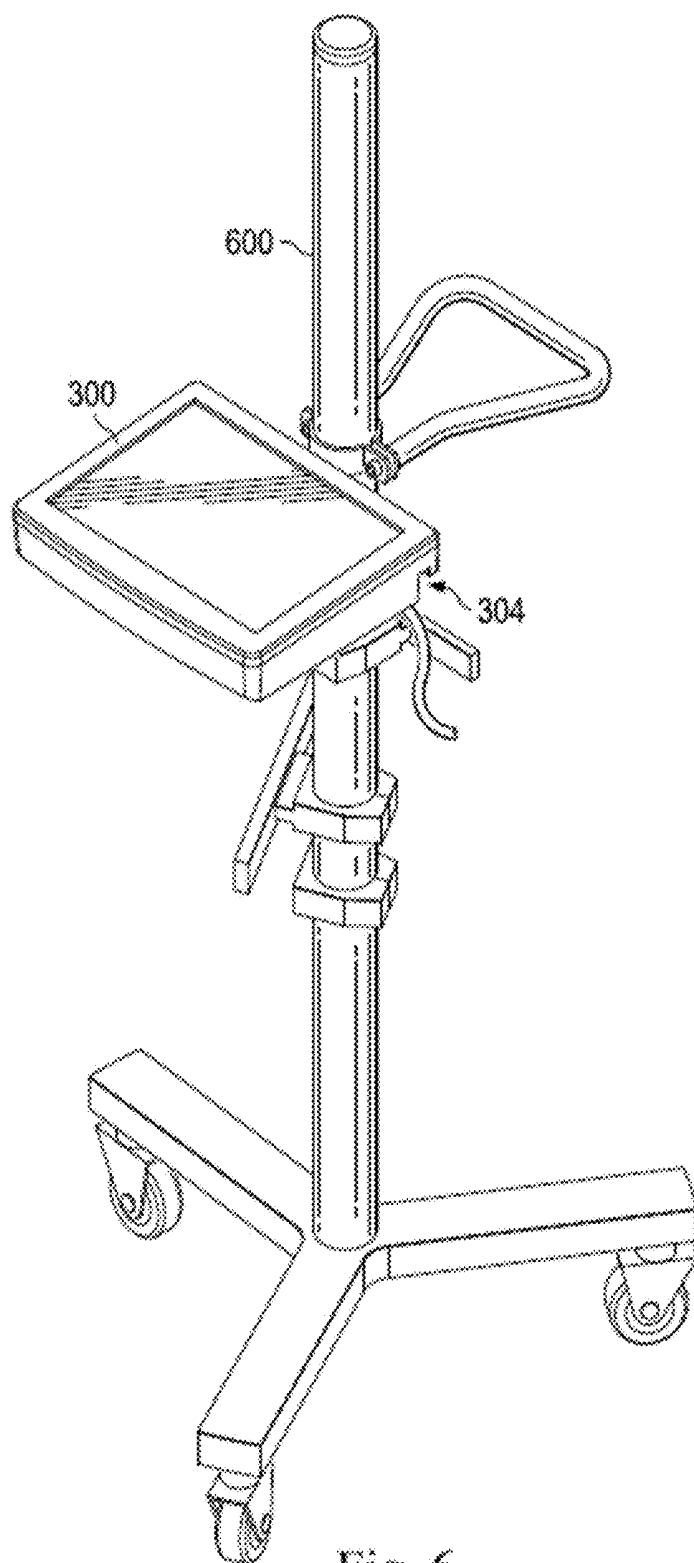


Fig. 6

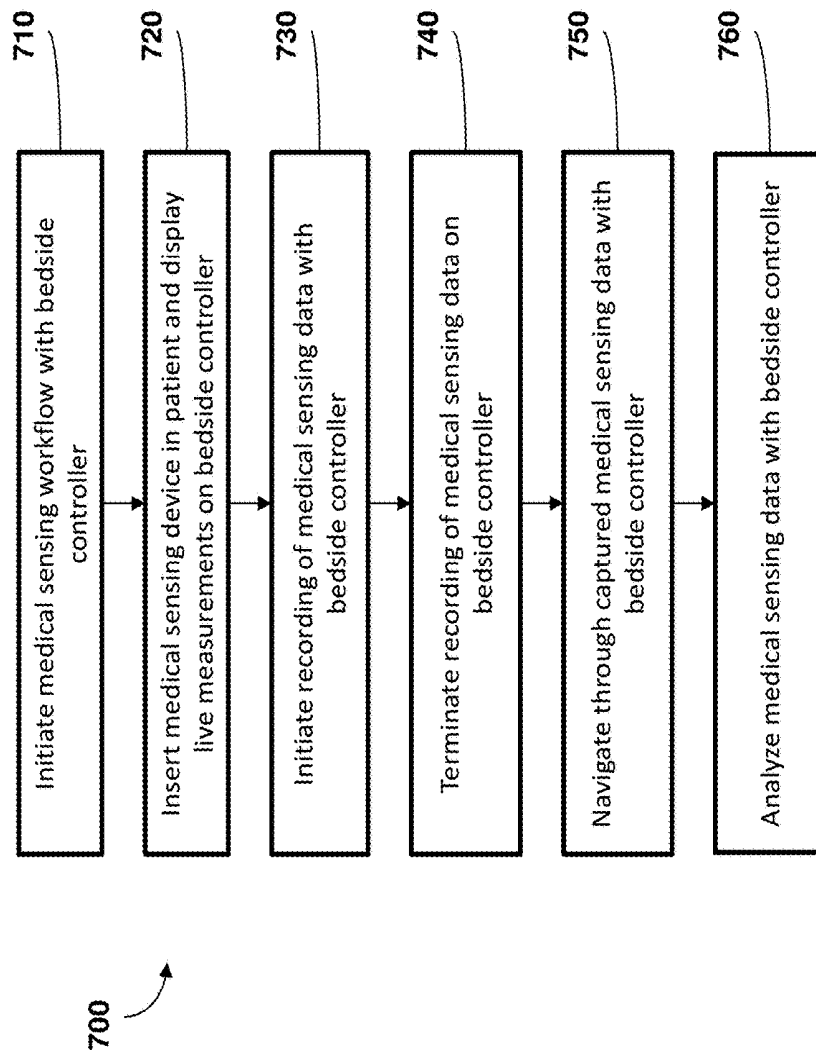


Fig. 7

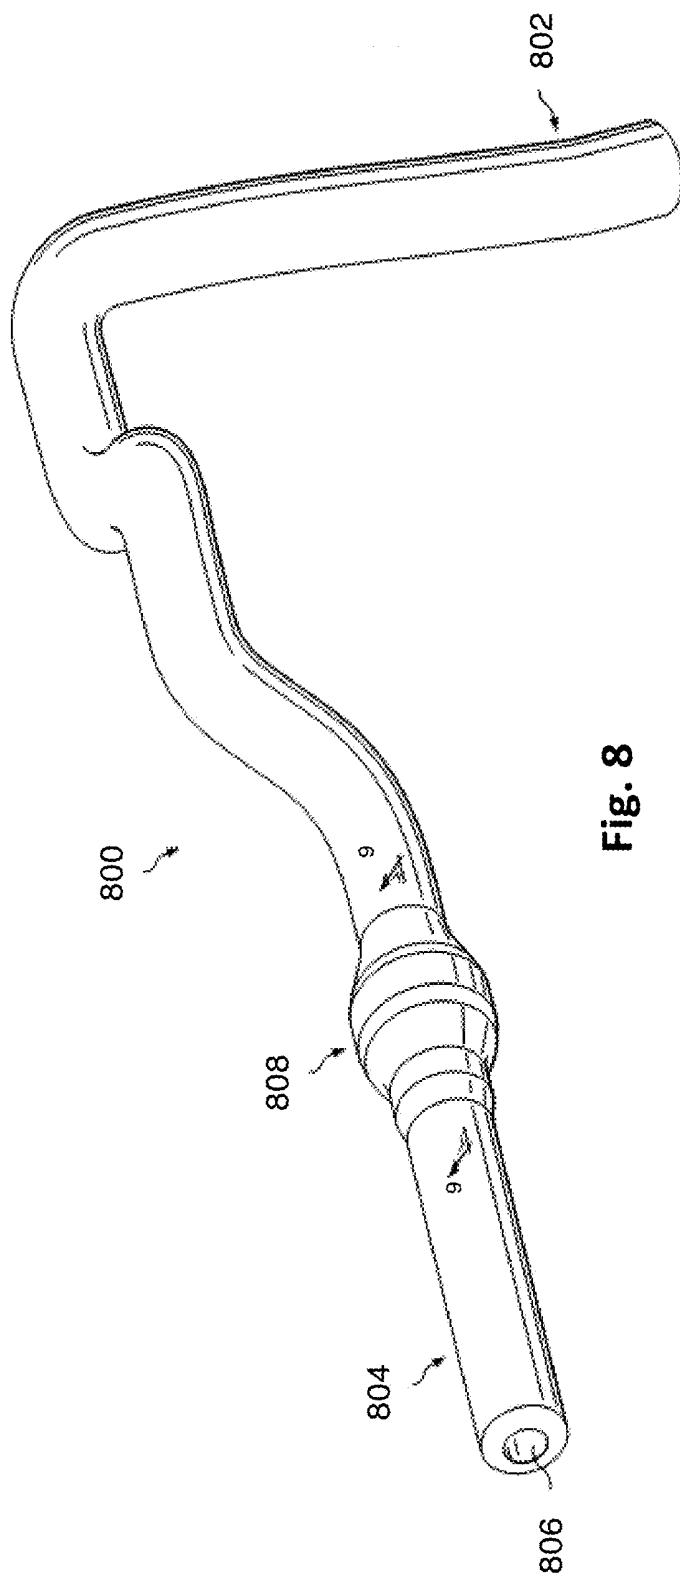


Fig. 8

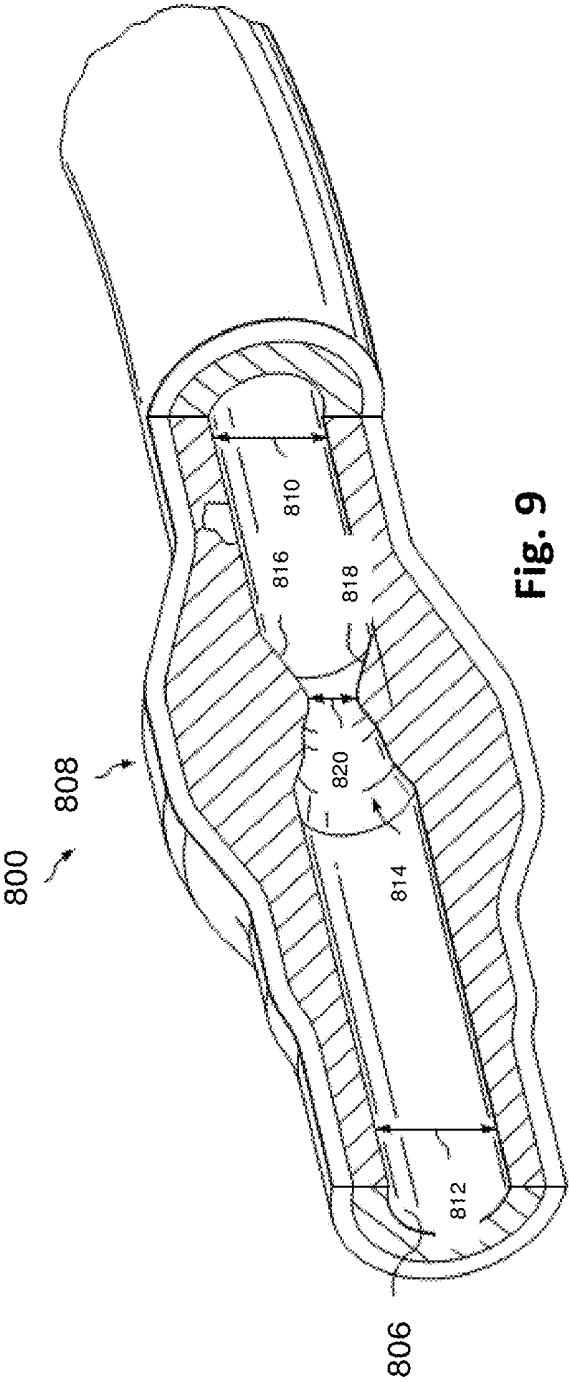


Fig. 9

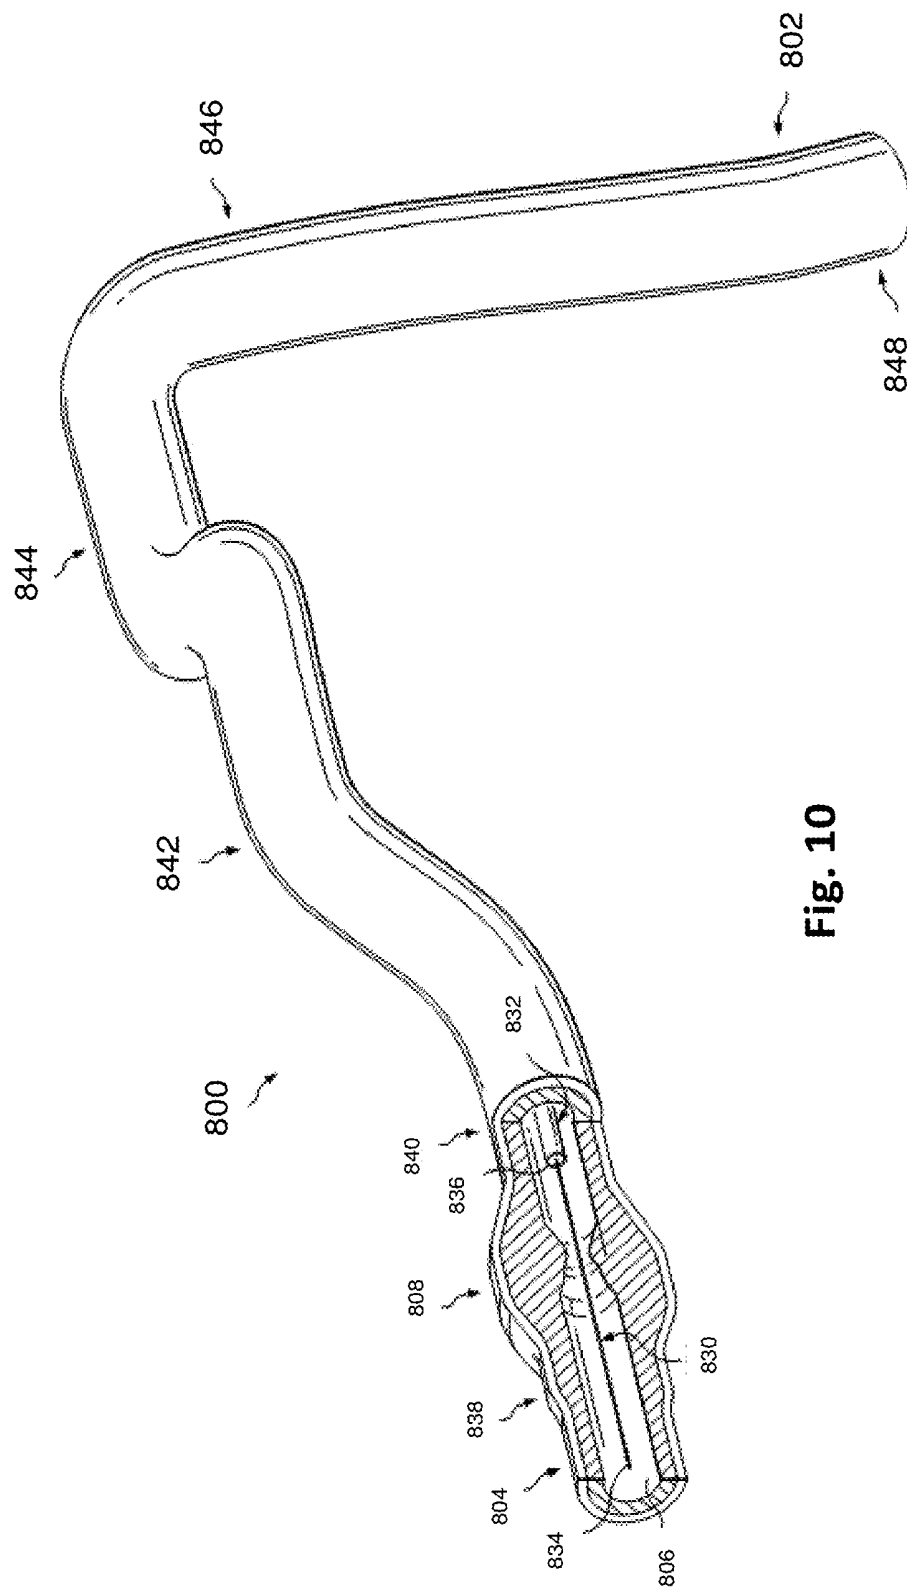


Fig. 10

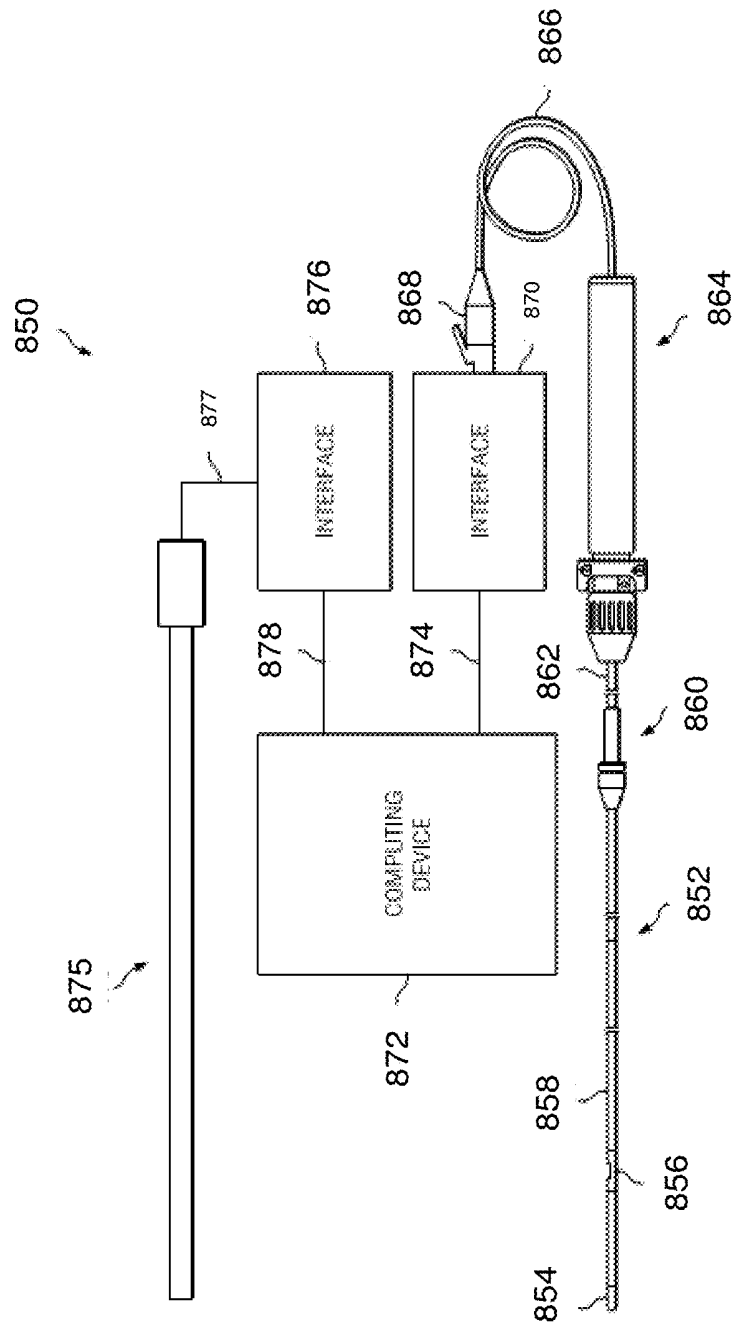


Fig. 11

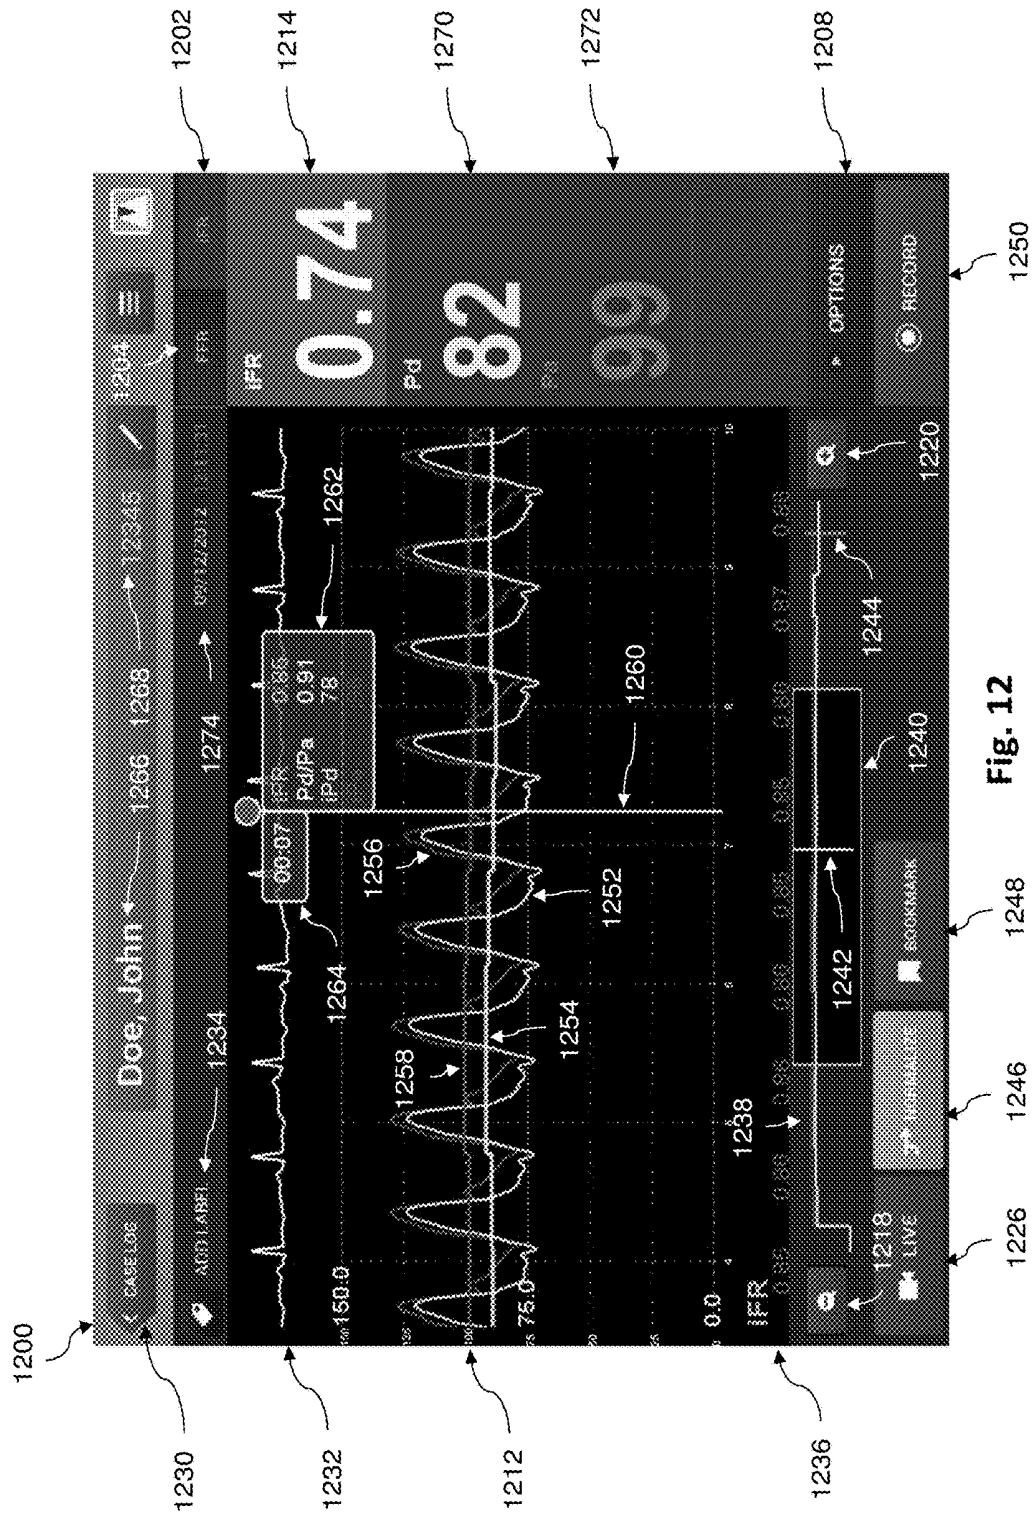
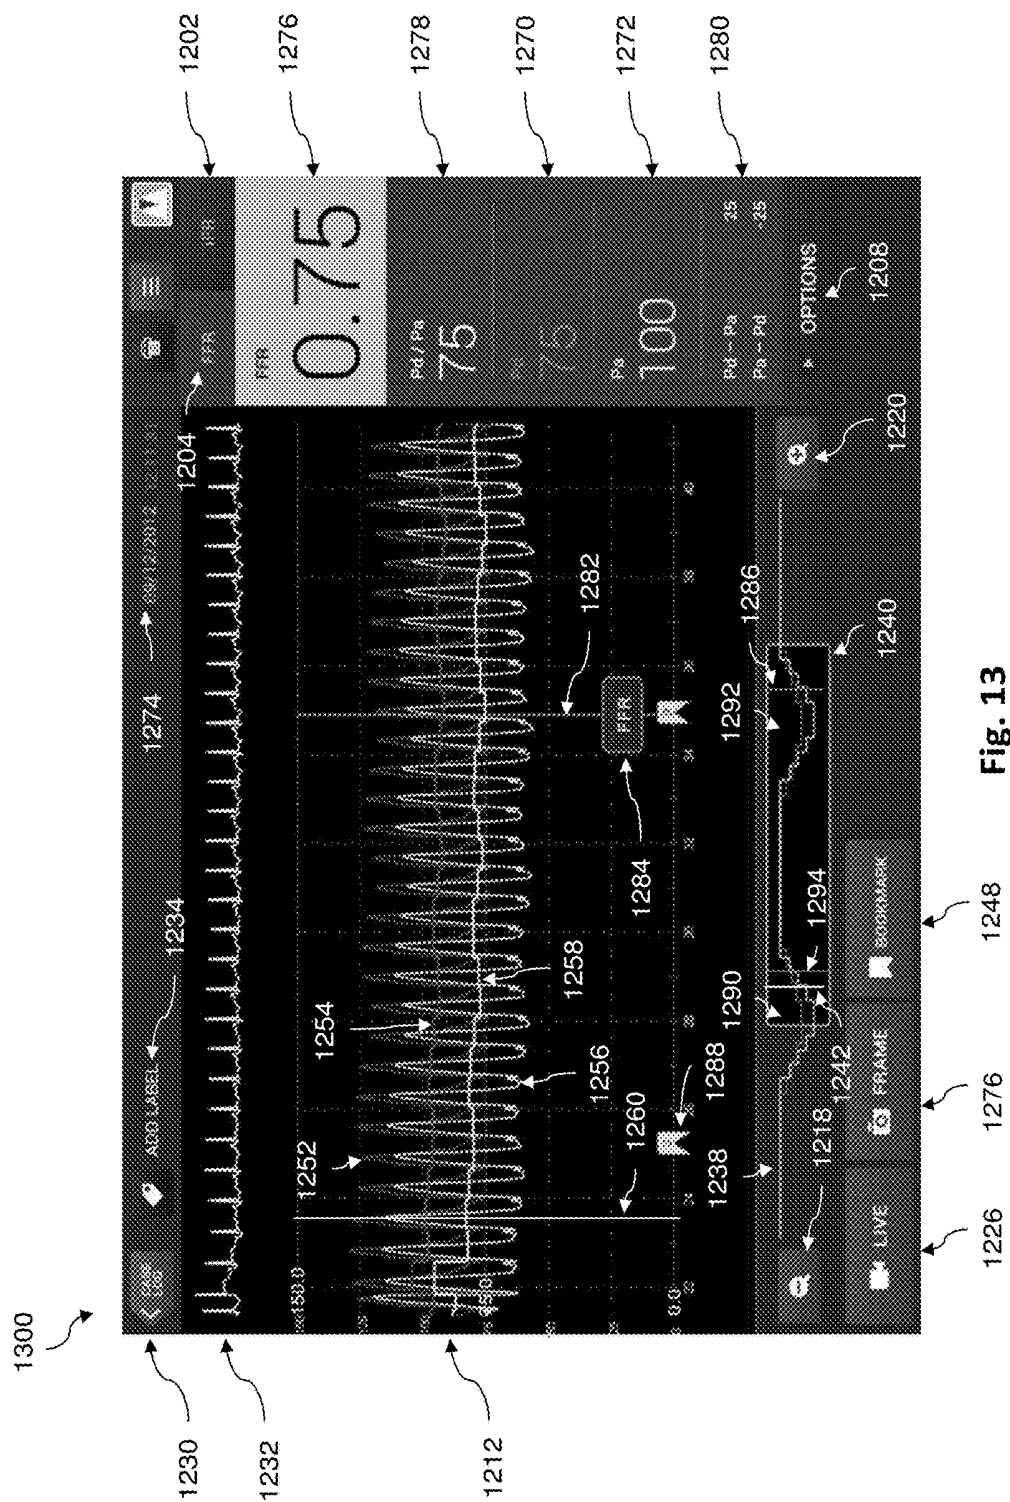


Fig. 12



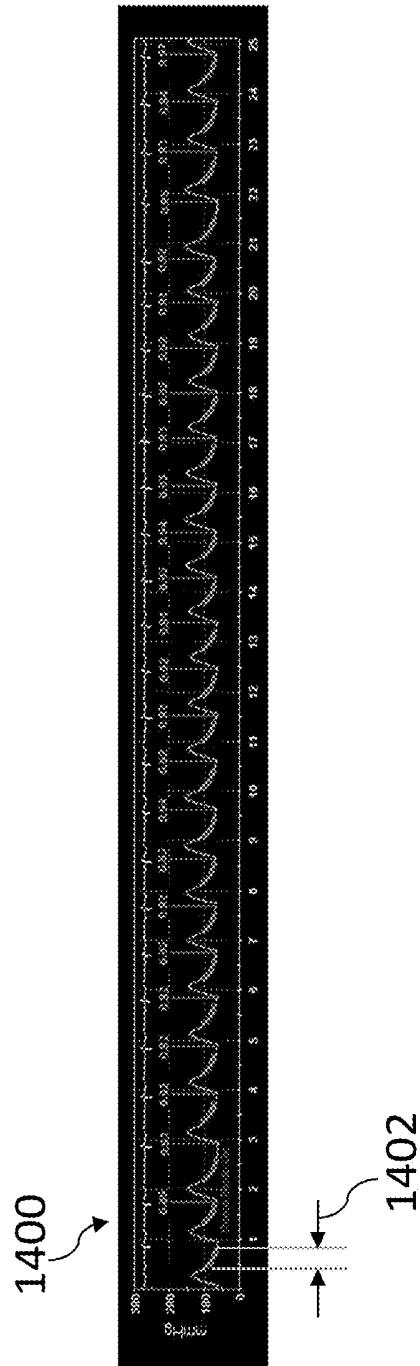


Fig. 14

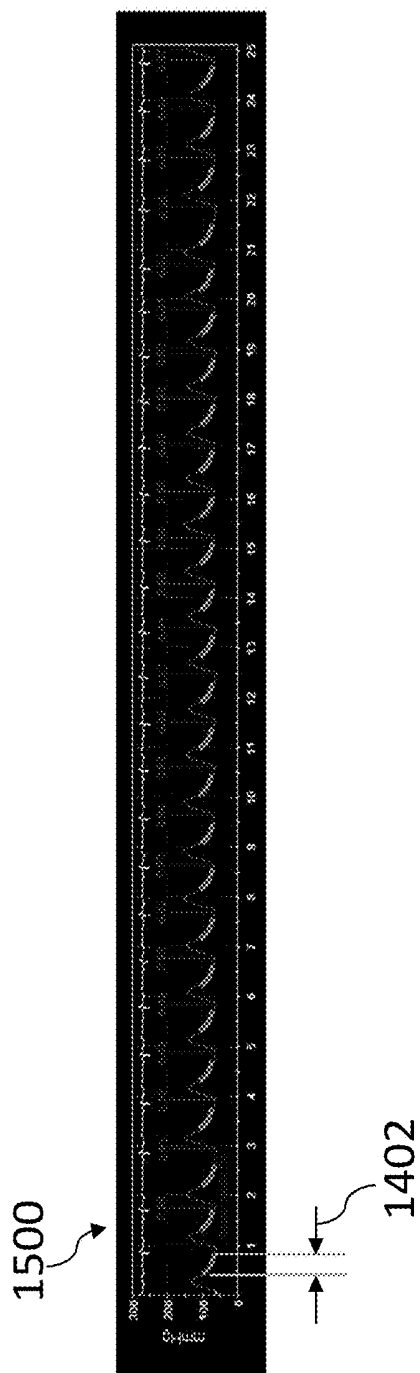


Fig. 15

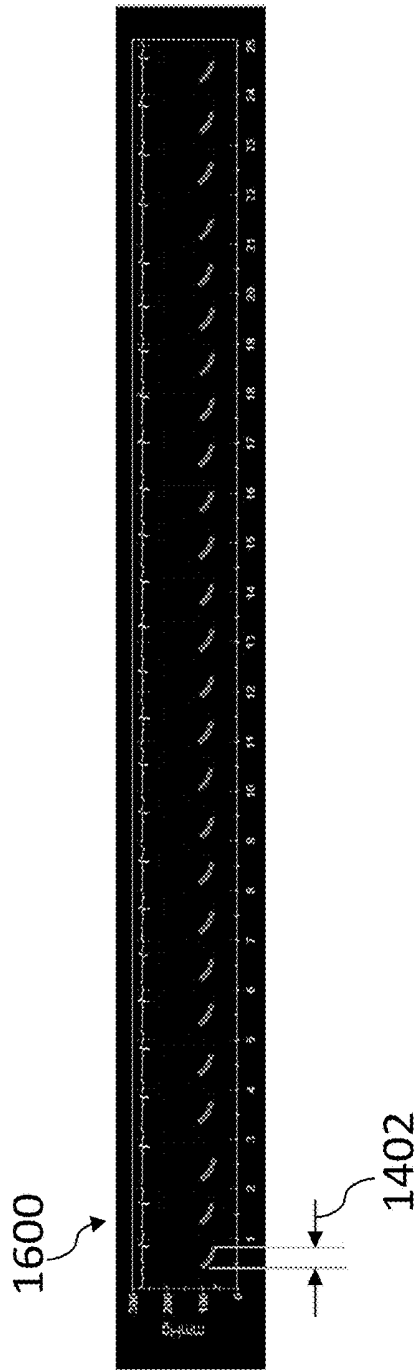


Fig. 16

1

BEDSIDE CONTROLLER FOR ASSESSMENT OF VESSELS AND ASSOCIATED DEVICES, SYSTEMS, AND METHODS

CROSS REFERENCE TO RELATED APPLICATIONS

The present application claims priority to and the benefit of the U.S. Provisional Patent Application No. 62/049,265, filed Sep. 11, 2014, which is hereby incorporated by reference in its entirety.

TECHNICAL FIELD

The present disclosure relates generally to the assessment of vessels using a bedside controller. For example, some embodiments of the present disclosure are suited for assessing the severity of a blockage or other restriction to the flow of fluid through a vessel, such as a stenosis of a human blood vessel, by analyzing medical sensing data collected from the vessel using a touch-sensitive display of the bedside controller.

BACKGROUND

Innovations in diagnosing and verifying the level of success of treatment of disease have progressed from solely external imaging processes to include internal diagnostic processes. In addition to traditional external image techniques such as X-ray, MRI, CT scans, fluoroscopy, and angiography, small sensors may now be placed directly in the body. For example, diagnostic equipment and processes have been developed for diagnosing vasculature blockages and other vasculature disease by means of ultra-miniature sensors placed upon the distal end of a flexible elongate member such as a catheter, or a guide wire used for catheterization procedures. For example, known medical sensing techniques include intravascular ultrasound (IVUS), forward looking IVUS (FL-IVUS), fractional flow reserve (FFR) determination, a coronary flow reserve (CFR) determination, optical coherence tomography (OCT), transesophageal echocardiography, and image-guided therapy. Traditionally, many of these procedures are carried out by a multitude of physicians and clinicians, where each performs an assigned task. For example, a physician may stand next to a patient in the sterile field and guide the insertion and pull back of a medical sensing catheter. A clinician near the physician may control the procedure workflow with a controller, for example by starting and stopping the acquisition of medical data. Further, once medical data has been acquired, a second clinician in an adjacent control room working at a desktop computer may analyze the data, such as by reviewing quantities calculated from the acquired data. Typically, the physician in the catheter lab and the clinician in the control room must communicate in order to acquire and analyze the relevant medical data. This may lengthen the time of the procedure, increase the cost of the procedure, and may lead to errors due to miscommunication or clinician inexperience.

One exemplary type of procedure involves pressure measurements within a blood vessel. A currently accepted technique for assessing the severity of a stenosis in the blood vessel, including ischemia causing lesions, is fractional flow reserve (FFR). FFR is a calculation of the ratio of a distal pressure measurement (taken on the distal side of the stenosis) relative to a proximal pressure measurement (taken on the proximal side of the stenosis). FFR provides an index

2

of stenosis severity that allows determination as to whether the blockage limits blood flow within the vessel to an extent that treatment is required. The normal value of FFR in a healthy vessel is 1.00, while values less than about 0.80 are generally deemed significant and require treatment. Common treatment options include angioplasty and stenting.

Coronary blood flow is unique in that it is affected not only by fluctuations in the pressure arising proximally (as in the aorta) but is also simultaneously affected by fluctuations arising distally in the microcirculation. Accordingly, it is not possible to accurately assess the severity of a coronary stenosis by simply measuring the fall in mean or peak pressure across the stenosis because the distal coronary pressure is not purely a residual of the pressure transmitted from the aortic end of the vessel. As a result, for an effective calculation of FFR within the coronary arteries, it is necessary to reduce the vascular resistance within the vessel. Currently, pharmacological hyperemic agents, such as adenosine, are administered to reduce and stabilize the resistance within the coronary arteries. These potent vasodilator agents reduce the dramatic fluctuation in resistance predominantly by reducing the microcirculation resistance associated with the systolic portion of the heart cycle to obtain a relatively stable and minimal resistance value.

However, the administration of hyperemic agents is not always possible or advisable. First, the clinical effort of administering hyperemic agents can be significant. In some countries (particularly the United States), hyperemic agents such as adenosine are expensive, and time consuming to obtain when delivered intravenously (IV). In that regard, IV-delivered adenosine is generally mixed on a case-by-case basis in the hospital pharmacy. It can take a significant amount of time and effort to get the adenosine prepared and delivered to the operating area. These logistic hurdles can impact a physician's decision to use FFR. Second, some patients have contraindications to the use of hyperemic agents such as asthma, severe COPD, hypotension, bradycardia, low cardiac ejection fraction, recent myocardial infarction, and/or other factors that prevent the administration of hyperemic agents. Third, many patients find the administration of hyperemic agents to be uncomfortable, which is only compounded by the fact that the hyperemic agent may need to be applied multiple times during the course of a procedure to obtain FFR measurements. Fourth, the administration of a hyperemic agent may also require central venous access (e.g., a central venous sheath) that might otherwise be avoided. Finally, not all patients respond as expected to hyperemic agents and, in some instances, it is difficult to identify these patients before administration of the hyperemic agent.

Accordingly, there remains a need for improved devices, systems, and methods for assessing the severity of a blockage in a vessel and, in particular, a stenosis in a blood vessel. In that regard, there remains a need for improved devices, systems, and methods for assessing the severity of a stenosis in the coronary arteries that do not require the administration of hyperemic agents. There also remains a need for improved devices, systems, and methods for providing visual depictions of vessel that allow assessment of the vessel and, in particular, any stenosis or lesion of the vessel. Further, there remains a need for assessing the severity of a stenosis and for providing visual depictions of the vessel in an efficient manner.

SUMMARY

Embodiments of the present disclosure are configured to efficiently assess the severity of a blockage in a vessel and,

in particular, a stenosis in a blood vessel using a bedside controller. In some particular embodiments, the devices, systems, and methods of the present disclosure are configured to provide screen displays that allow assessment of the vessel and, in particular, any stenosis or lesion of the vessel on a touch-sensitive display of the bedside controller. Vessel data can be efficiently assessed using touch inputs received on the bedside controller.

In an exemplary aspect, the present disclosure is directed to a method of evaluating a vessel of a patient. The method includes outputting, to a touch-sensitive display of a bedside controller, a screen display including: a visual representation of a first pressure ratio of pressure measurements obtained by first and second instruments positioned within a vessel while the second instrument is moved longitudinally through the vessel from a first position distal of a stenosis of the vessel to a second position proximal of the stenosis and the first instrument remains stationary within the vessel; and a first proximal pressure waveform and a first distal pressure waveform of the obtained pressure measurements; receiving, through the touch-sensitive display of the bedside controller, a user touch input on at least one of the first proximal pressure waveform and the first distal pressure waveform identifying a time at which pressure measurements were obtained; and modifying the screen display, in response to the user touch input, to further include a visual representation of the obtained pressure measurements corresponding to the identified time.

In some aspects, the visual representation of the obtained pressure measurements corresponding to the identified time is displayed at a location proximate the at least a portion of the first pressure waveform defined by a point of initial contact with the touch-sensitive display. In some aspects, the visual representation of the obtained pressure measurements corresponding to the identified time includes a numerical value of the obtained pressure measurements at the identified time. In some aspects, the visual representation of the obtained pressure measurements corresponding to the identified time includes a first pressure ratio of the obtained pressure measurements at the identified time. In some aspects, the visual representation of the obtained pressure measurements corresponding to the identified time includes a second pressure ratio of the obtained pressure measurements at the identified time, wherein the second pressure ratio is calculated differently than the first pressure ratio. In some aspects, the visual representation of the obtained pressure measurements corresponding to the identified time includes a numerical value of the obtained pressure measurements at the identified time, a first pressure ratio of the obtained pressure measurements at the identified time, and a second pressure ratio of the obtained pressure measurements at the identified time, wherein the second pressure ratio is calculated differently than the first pressure ratio. In some aspects, the screen display includes a second proximal pressure waveform and a second distal pressure waveform of the obtained pressure measurements, wherein the second proximal and distal pressure waveforms illustrates the obtained pressure measurements over a greater amount of time compared to the first proximal and distal pressure waveforms. In some aspects, the screen display includes an overlay positioned over a portion of the second proximal and distal pressure waveforms, the overlay illustrating a portion of the obtained pressure measurement represented in the first proximal and distal pressure waveforms. In some aspects, the method further includes receiving, through the touch-sensitive display of the bedside controller, a user touch input on the overlay to move the overlay to be positioned over a

different portion of the second proximal and distal pressure waveforms; and modifying the screen display, in response to the user touch input, such that the at least a portion of the first proximal and distal pressure waveforms include the obtained pressure measurements corresponding to the position of the overlay over the different portion of the second proximal and distal pressure waveforms. In some aspects, the screen display includes a plurality of pressure ratios of the obtained pressure measurements, each of the plurality of pressure ratios separated by a fixed interval. In some aspects, the screen display includes numerical values of the obtained pressure measurements. In some aspects, the visual representation of a first pressure ratio of the obtained pressure measurements includes a numerical value. In some aspects, the screen display includes a second pressure ratio of the obtained pressure measurements, wherein the second pressure ratio is calculated differently than the first pressure ratio. In some aspects, the screen display includes visual representation of a difference in the pressure measurements.

In an exemplary aspect, the present disclosure is directed to a system for evaluating a vessel of a patient, comprising: a first instrument sized and shaped for introduction into the vessel of the patient; a second instrument sized and shaped for introduction into the vessel of the patient; a bedside controller comprising a touch-sensitive display, the bedside controller being configured to display a screen display and to receive user touch inputs on the touch-sensitive display; and a processing system communicatively coupled to the first and second instruments and the bedside controller, the processing system configured to: receive pressure measurements from the first and second instruments positioned within a vessel while the second instrument is moved longitudinally through the vessel from a first position distal of a stenosis of the vessel to a second position proximal of the stenosis and the first instrument remains stationary within the vessel; output, to the touch-sensitive display of the bedside controller, the screen display including: a visual representation of a pressure ratio of the obtained pressure measurements; and a first proximal pressure waveform and a first distal pressure waveform of the obtained pressure measurements; receive a signal from the bedside controller in response to a user touch input received at the touch-sensitive display, the user touch input identifying a time at which pressure measurements were obtained on at least one of the first proximal pressure waveform and the first distal proximal pressure waveform; and modify the screen display, in response to the received signal, to further include a visual representation of the obtained pressure measurements corresponding to the identified time.

In some aspects, wherein the visual representation of the obtained pressure measurements corresponding to the identified time includes a numerical value of the obtained pressure measurements at the identified time and a numerical value of a first pressure ratio of the obtained pressure measurements at the identified time. In some aspects, the visual representation of the obtained pressure measurements corresponding to the identified time further includes a numerical value of a second pressure ratio of the obtained pressure measurements at the identified time, wherein the second pressure ratio is calculated differently than the first pressure ratio. In some aspects, the processing system is configured to output the screen display further including: a second proximal pressure waveform and a second distal pressure waveform of the obtained pressure measurements, the second proximal and distal pressure waveforms illustrating the obtained pressure measurements over a greater amount of time compared to the first proximal and distal

5

pressure waveforms; and an overlay positioned over a portion of the second proximal and distal pressure waveforms, the overlay illustrating a portion of the obtained pressure measurements represented in the first proximal and distal pressure waveforms. In some aspects, the processing system is further configured to: receive a signal from the bedside controller in response to a user touch input received at the touch-sensitive display, the user touch input moving the overlay to be positioned over a different portion of the second pressure waveform; and modify the screen display, in response to the received signal, such that the at least a portion of the first waveform includes the obtained pressure measurements corresponding to the position of the overlay over the different portion of the second pressure waveform. In some aspects, the processing system is configured to output the screen display further including: a plurality of pressure ratios of the obtained pressure measurements, each of the plurality of pressure ratios separated by a fixed interval.

Additional aspects, features, and advantages of the present disclosure will become apparent from the following detailed description.

BRIEF DESCRIPTION OF THE DRAWINGS

Illustrative embodiments of the present disclosure will be described with reference to the accompanying drawings, of which:

FIG. 1 is a schematic drawing depicting a medical sensing system including a bedside controller according to one embodiment of the present disclosure.

FIG. 2 is a schematic drawing depicting a medical sensing system including a wireless bedside controller according to another embodiment of the present disclosure.

FIG. 3A is a diagrammatic perspective view of a bedside controller.

FIG. 3B is a diagrammatic rear perspective view of the bedside controller of FIG. 3A.

FIG. 3C is a diagrammatic perspective view of the bedside controller of FIGS. 3A and 3B mounted to a bed rail.

FIG. 4 is a functional block diagram of the bedside controller of FIGS. 3A-3C according to aspects of the present disclosure.

FIG. 5 is a diagrammatic perspective view of a mobile processing system with the bedside controller of FIGS. 3A-3C attached thereto.

FIG. 6 is a diagrammatic perspective view of the bedside controller of FIGS. 3A-3C releasably mounted on an IV pole.

FIG. 7 is a flowchart illustrating a method of conducting a medical sensing workflow with a bedside controller according to various aspects of the present disclosure.

FIG. 8 shows a diagrammatic perspective view of a vessel having a stenosis according to an embodiment of the present disclosure.

FIG. 9 shows a diagrammatic, partial cross-sectional perspective view of a portion of the vessel of FIG. 8 taken along section line 9-9 of FIG. 8.

FIG. 10 shows a diagrammatic, partial cross-sectional perspective view of the vessel of FIGS. 8 and 9 with instruments positioned therein according to an embodiment of the present disclosure.

FIG. 11 shows a diagrammatic, schematic view of a system according to an embodiment of the present disclosure.

FIG. 12 shows a screen display according to an embodiment of the present disclosure.

6

FIG. 13 shows a screen display according to an embodiment of the present disclosure.

FIG. 14 shows a portion of a screen display according to another embodiment of the present disclosure.

FIG. 15 shows a portion of a screen display according to another embodiment of the present disclosure.

FIG. 16 shows a portion of a screen display according to another embodiment of the present disclosure.

DETAILED DESCRIPTION

For the purposes of promoting an understanding of the principles of the present disclosure, reference will now be made to the embodiments illustrated in the drawings, and specific language will be used to describe the same. It is nevertheless understood that no limitation to the scope of the disclosure is intended. Any alterations and further modifications to the described devices, systems, and methods, and any further application of the principles of the present disclosure are fully contemplated and included within the present disclosure as would normally occur to one skilled in the art to which the disclosure relates. In particular, it is fully contemplated that the features, components, and/or steps described with respect to one embodiment may be combined with the features, components, and/or steps described with respect to other embodiments of the present disclosure. For the sake of brevity, however, the numerous iterations of these combinations will not be described separately.

FIG. 1 is a schematic drawing depicting a medical sensing system **100** including a bedside controller **102** according to one embodiment of the present disclosure. In general, the medical sensing system **100** provides for coherent integration and consolidation of multiple forms of acquisition and processing elements designed to be sensitive to a variety of methods used to acquire and interpret human biological physiology and morphological information. More specifically, in system **100**, the bedside controller **102** is a touch-enabled, integrated computing device for the acquisition, control, interpretation, measurement, and display of medical sensing data. In the illustrated embodiment, the bedside controller **102** is a tablet-style touch-sensitive computer that provides user controls and diagnostic images on a single surface. In the medical sensing system **100**, the bedside controller **102** is operable to present workflow control options and patient image data via graphical user interfaces (GUIs) corresponding to a plurality of medical sensing modalities. The bedside controller **102** will be described in greater detail in association with FIGS. 3A, 3B, and 4.

In the illustrated embodiment, the medical sensing system **100** is deployed in a catheter lab **104**. The catheter lab **104** may be used to perform on a patient **106** any number of medical sensing procedures alone or in combination such as, by way of example and not limitation, angiography, intravascular ultrasound (IVUS), virtual histology (VH), forward looking IVUS (FL-IVUS), intravascular photoacoustic (IVPA) imaging, pressure, fractional flow reserve (FFR) determination, flow velocity, flow volume, coronary flow reserve (CFR) determination, optical coherence tomography (OCT), computed tomography, intracardiac echocardiography (ICE), forward-looking ICE (FLICE), intravascular palpography, transesophageal ultrasound, or any other medical sensing modalities known in the art. Catheter lab **104** can also conduct medical sensing procedures associated with Instant Wave-Free Ratio™ Functionality (iFR® Functionality) (both trademarks of Volcano Corp.) and those disclosed in U.S. patent application Ser. No. 13/460,296 filed Apr. 30, 2012, now published as U.S. Patent Application

Publication No. US 2013-0046190 A1 on Feb. 21, 2013 and entitled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSING A VESSEL," hereby incorporated by reference in its entirety, which discloses the use of pressure ratios that are available without application of a hyperemic agent. Further, medical sensing procedures associated with compensated Pd/Pa ratios suitable for estimating iFR®, FFR, and/or other accepted diagnostic pressure ratios as disclosed in U.S. Provisional Patent Application No. 62/024,005, filed Jul. 14, 2014 and entitled "DEVICES, SYSTEMS, AND METHODS FOR TREATMENT OF VESSELS," which is hereby incorporated by reference in its entirety, can be conducted in the catheter lab **104**. In addition to controlling medical sensing systems, the bedside controller may be used to cooperate with and control medical treatment systems such as, for example but without limitation, those used for stent placement, coil embolism, ablation therapy, kidney stone treatments, basket placement in a cystoscopy, tumor removal, and chemical therapies. The catheter lab **104** further includes a sterile field **105** that encompasses the portions of the catheter lab surrounding the patient **106** on a procedure table **109** and a clinician **107**, who may perform any number of medical sensing procedures or treatments. As shown in FIG. 1, the bedside controller **102** may be positioned within the sterile field **105** and may be utilized by the clinician **107** to control a workflow of a medical sensing procedure or treatment being performed on the patient **106**. For example, the clinician **107** may initiate the procedure workflow, watch real-time medical sensing data, such as pressure measurements (e.g., visual representations of pressure data, such as pressure waveforms), obtained during the procedure, and interact with the obtained medical sensing data using the bedside controller **102** inside of the sterile field **105**. In alternative embodiments, the bedside controller **102** may be utilized outside of the sterile field **105**, for instance, in other locations within the catheter lab **104** or in a control room adjacent to the catheter lab. A method of utilizing the bedside controller **102** to control a medical sensing workflow or treatment workflow will be discussed in greater detail below. In some embodiments, the medical sensing system **100** can be implemented as the system **850** (FIG. 8), described below. In some embodiments, one or more components of the system **850** can be implemented in the medical sensing system **100**.

In the embodiment illustrated in FIG. 1, the medical sensing system **100** additionally includes a number of interconnected medical sensing-related tools in the catheter lab **104** to facilitate a pressure-sensing workflow procedure, such as a medical sensing device **108** and a medical sensing device **110**, and a processing system **124**. The medical sensing devices **108** and **110** can include pressure monitoring elements. Some embodiments of the medical sensing system **100** can include an patient interface module (PIM) **112** communicatively coupled to the medical sensing device **108**, PIM **114** communicatively coupled to the medical sensing device **110**, an electrocardiogram (ECG) device **116**, an angiogram system **117**, and a boom display **122**. The bedside controller **102**, PIMs **112** and **114**, ECG device **116**, angiography system **117**, and boom display **122** are communicatively coupled to the processing system **124**. In some embodiments, the medical sensing devices **108** and **110** can include imaging elements to facilitate an imaging workflow. In one embodiment, the processing system **124** is a computer workstation with the hardware and software to acquire, process, and display medical sensing data, but in other

data. For example, during a pressure-sensing workflow, the processing system **124** is operable to accept raw pressure data from the medical sensing devices **108** and **110** and/or the PIMs **112** and **114**, transform the pressure data into screen displays including, e.g., visual representations such as pressure waveforms, numerical values, computed values, etc., and make the screen display available to the bedside controller **124**, so that they may be displayed to the clinician **107** for analysis. In the embodiments in which the processing system **124** is a computer workstation, the system includes at least a processor such as a microcontroller or a dedicated central processing unit (CPU), a non-transitory computer-readable storage medium such as a hard drive, random access memory (RAM), and/or compact disk read only memory (CD-ROM), a video controller such as a graphics processing unit (GPU), and a network communication device such as an Ethernet controller. Further, the processing system **124** is communicatively coupled to a data network **125**. In the illustrated embodiment, the data network **125** is a TCP/IP-based local area network (LAN), however in other embodiments, it may utilize a different protocol such as Synchronous Optical Networking (SONET), or may be a wide area network (WAN). The processing system **124** may connect to various resources via the network **125**, such as a Digital Imaging and Communications in Medicine (DICOM) system, a Picture Archiving and Communication System (PACS), and a Hospital Information System. The processing system **124** can be similar to a multi-modality processing system that processes medical sensing data disclosed in U.S. Pat. No. 8,754,865, entitled "MEDICAL MEASURING SYSTEM AND METHOD" and issued on Jun. 17, 2014, and U.S. Patent Application No. 61/473,570, filed on Apr. 8, 2011 entitled "MULTI-MODALITY MEDICAL SENSING SYSTEM AND METHOD" and published as PCT Patent Application Publication No. WO/2012/154335 on Nov. 15, 2012, both of which are hereby incorporated by reference herein in their entireties.

In the medical sensing system **100**, the PIM **112** and PIM **114** are operable to respectively receive medical sensing data collected from the patient **106** by the medical sensing device **108** and medical sensing device **110** and are operable to transmit the received data to the processing system **124**. In one embodiment, the PIM **112** and PIM **114** transmit the medical sensing data over a Peripheral Component Interconnect Express (PCIe) data bus connection, but, in other embodiments, they may transmit data over a USB connection, a Thunderbolt connection, a FireWire connection, or some other high-speed data bus connection. Additionally, the ECG device **116** is operable to transmit electrocardiogram signals or other hemodynamic data from patient **106** to the processing system **124**. To aid the clinician in data capture, the bedside controller **102** is operable to display the ECG data alongside medical sensing data. Further, in some embodiments, the processing system **124** may be operable to synchronize data collection with the catheters **108** and **110** using ECG signals from the ECG **116**. Further, the angiogram system **117** is operable to collect x-ray, computed tomography (CT), or magnetic resonance images (MRI) of the patient **106** and transmit them to the processing system **124**. After the x-ray, CT, or MRI data has been processed into human-readable images by the processing system **124**, the clinician **107** may navigate the GUI on the bedside controller **124** to retrieve the images from the processing system **124** and display them on the controller. In some embodiments, the processing system **124** may co-register image data from angiogram system **117** (e.g. x-ray data,

MRI data, CT data, etc.) with sensing data from the and catheters **108** and **110**. As one aspect of this disclosure, the co-registration may be performed to generate three-dimensional images with the sensing data. Such co-registered 3-D images data may be viewable on the bedside controller **124**. In one embodiment, a clinician may rotate, zoom, and otherwise manipulate such 3-D images on the bedside controller **102** using simultaneous touch inputs (i.e. multi-touch) and gestures.

Additionally, in the illustrated embodiment of FIG. **1**, medical sensing tools in system **100**, are communicatively coupled to the processing system **124** via a wired connection such as a standard copper link or a fiber optic link. Specifically, the bedside controller **124** may be communicatively and/or electrically coupled to the processing system **124** via a Universal Serial Bus (USB) connection, a Power-over-Ethernet connection, a Thunderbolt connection, a FireWire connection, or some other high-speed data bus connection.

However, in an alternative embodiment, such as that shown in FIG. **2**, the medical sensing tools may communicate wirelessly. In that regard, FIG. **2** is a schematic drawing depicting a medical sensing system **200** including a wireless bedside controller **202** according to another embodiment of the present disclosure. The medical sensing system **200** is similar to the system **100** of FIG. **1** but the medical sensing tools including the wireless bedside controller **202**, a wireless PIM **204**, and a wireless PIM **206** communicate with a wireless network **208** via wireless networking protocols. For example, the bedside controller **202** may send and receive workflow control parameters, medical sensing images, and measurement data to and from a remote processing system via IEEE 802.11 Wi-Fi standards, Ultra Wide-Band (UWB) standards, wireless FireWire, wireless USB, Bluetooth, or another high-speed wireless networking standard. Such wireless capability allows the clinician **107** to more freely position the bedside controller **202** inside or outside of the sterile field **105** for better workflow management.

With reference now to FIGS. **3A**, **3B**, **3C** and **4**, FIG. **3A** is a diagrammatic perspective view of a bedside controller **300**, FIG. **3B** is a diagrammatic rear perspective view of the bedside controller, FIG. **3C** is a diagrammatic perspective view of the bedside controller mounted to a bed rail, and FIG. **4** is a functional block diagram of the bedside controller **300** according to aspects of the present disclosure. The bedside controller **300** is similar to the bedside controllers **102** and **202** in medical sensing systems **100** and **200**, and is operable to, among other things, initiate a medical sensing or treatment procedure workflow, display real-time data (e.g., visual representations of pressure data) obtained during the procedure, and accept user touches on the visual representations of pressure data from a clinician. The bedside controller **300** generally improves system control available to a clinician working at a patient table. For instance, giving a clinician both workflow control and analysis capability within the sterile field reduces errors and improves workflow efficiency.

As show in FIG. **3A**, the bedside controller **300** includes an integrally formed housing **302** that is easy to grasp and move around a catheter lab or other medical setting. In one embodiment, the integrally formed housing **302** may be seamlessly molded from materials such as thermoplastic or thermosetting plastic or moldable metal. In other embodiments, the integrally formed housing **302** may comprise a plurality of housing portions fixedly bonded in a substantially permanent manner to form an integral housing. The housing **302** is resistant to fluids, and, in one embodiment, may have a rating of IPX4 against fluid ingress as defined by

the International Electrotechnical Commission (IEC) standard 60529. In other embodiments in which the housing **302** may be used in different environments, the hub may have a different fluid ingress rating. In the illustrated embodiment, the housing **302** is about 10.5 inches in width, about 8.25 inches in height, and has as thickness of about 2.75 inches. In alternative embodiments, the housing may have a different width, height, or thickness that is similarly conducive to portability.

As shown in FIG. **3B**, the housing **302** further includes self-contained mounting structure **303** disposed on the housing. In the illustrated embodiment, the mounting structure is disposed near an outer edge of the housing. The mounting structure **303** allows the bedside controller **300** to be releasably mounted in a variety of places in and out of a catheter lab in a self-contained manner. That is, the bedside controller **300** may be directly secured to another object without the use of a separate external mount. In the illustrated embodiment, the mounting structure **303** includes a mounting channel **304** and a retaining clamp **305** that pivots over the mounting channel to secure a mounting platform there-within. The mounting channel **304** is defined by a longer front wall **350**, a top wall **352**, and a shorter back wall **354**, and the retaining clamp includes a slot **356** that extends through the clamp in a manner generally parallel to the mounting channel. The front wall **350** and the back wall **354** are generally perpendicular to a touch-sensitive display **307** in the housing **302**, and the top wall **352** is generally parallel to the display **307**. In the illustrated embodiment, the retaining clamp is spring-loaded and releasably exerts pressure on objects situated in the mounting channel. In alternative embodiments, the retaining clamp may be configured differently and exert force via mechanisms other than springs.

As shown in FIG. **3C**, in operation, the bedside controller **300** may be releasably secured to a mounting platform, for example a bed rail **306**, by pivoting the mounting clamp **305** to an open position, positioning the controller such that the rail extends through the length of the channel **304**, and releasing the clamp such that it secures the rail within the channel. When the rail **306** is positioned in the mounting channel **304** and the clamp **305** is holding it therein, three surfaces of the rail are respectively engaged by the front wall **350**, the top wall **352**, and the back wall **354**, and a fourth surface of the rail extends through the slot **356** in the clamp **305**. In this manner, the mounting structure **303** may maintain the bedside controller **300** in a position generally parallel to a procedure table **350** associated with the bed rail **306**, as shown in FIG. **3B**. Described differently, the mounting structure **303** is a cantilevered mounting structure in that it secures one end of the controller to an object while the majority of the controller extends away from the object in an unsupported manner. Such a cantilevered position allows for a display of the controller to be both readable and at a comfortable input angle for an operator. Further, the self-contained mounting structure **303** allows the bedside controller **300** to be quickly released from the bed rail **306** and reattached to an IV pole, a cart on which a processing system is deployed, or other location in or out of the sterile field to allow for convenient workflow control and image analysis. In alternative embodiments the mounting structure **303** of the bedside controller may vary from the design illustrated in FIGS. **3A** and **3B** and include additional and/or different components to allow for self-contained mounting.

Embedded into the front of the housing **302** is the touch-sensitive display **307** that comprises both a touch panel **308** and a flat panel display **309**. The touch panel **308** overlays the flat panel display **308** and accepts user input via human

touch, stylus touch, or some other analogous input method. In other words, the touch-sensitive display 307 displays images and accepts user input on the same surface. In the current embodiment, the touch panel 308 is a resistive-type panel, but in alternative embodiments it may be a capacitive-type panel, projective-type panel, or some other suitable type of touch enabled input panel. Further, the touch panel 308 is operable to accept multiple inputs simultaneously (multitouch), for instance, to enable rotation of a three-dimensional rendering of a vessel along multiple axes. Additionally, the touch panel 308 is capable of receiving input when a sterile drape 301 is covering the bedside controller 300 and also when a user is gloved. The touch panel 308 is controlled by a touch controller 310 disposed within the housing 302. Further, when a clinician makes contact with the touch panel 308, the touch panel is operable to provide haptic feedback via a haptics controller 312 and haptics drivers 314. This haptic technology is operable to simulate a plurality of sensations on the touch panel 308 by varying the intensity and frequency of vibrations generated when a user contacts the touch panel. In some embodiments, the housing 302 may include a sheath configured to store a stylus therein. Thus, a clinician may remove the stylus from the sheath in the housing to make measurements on the bedside controller and store it when the measurements have been completed.

Beneath the touch panel 308 is the flat panel display 309 that presents a graphical user interface (GUI) 316 to a user. In the illustrated embodiment, the flat panel display 309 is a LCD display but in alternative embodiments, it may be a different type of display such an LED display or an AMOLED display. In the illustrated embodiment, the flat panel display 309 is illuminated by a LED backlight power inverter 318. As mentioned above, the GUI 316 not only allows a clinician to control a medical sensing workflow, but also view and interact with pressure data obtained from a patient in the sterile field. A method of interacting with the GUI 316 to view and interact with the data will be discussed in greater detail in association with FIGS. 7-12.

The bedside controller 300 includes a single board processing platform 320 within the housing 302 that is operable to render the GUI 316 and process user touch input. In the illustrated embodiment, the processing platform has a pico form factor and includes integrated processing components such as a processor 321, system memory 322, graphics processing unit (GPU), communications module 323, and I/O bus controller. In some embodiments, the processor 321 may be a low power processor such as an Intel Atom® processor or an ARM-based processor, and the communications module 323 may be a 10/100/1 Gb Ethernet module. And, the I/O bus controller may be a Universal Serial Bus (USB) controller. The bedside controller 300 further includes a storage module 324 that is a non-transitory computer readable storage medium operable to store an operating system (i.e. software to render and control the GUI), data and/or visual representation manipulation software, medical sensing data and visual representations received from a processing system, and other medical sensing-related software. The processor 321 is configured to execute software and instructions stored on the storage module 324. In the illustrated embodiment, the storage module 324 is a solid state drive (SSD) hard drive communicatively coupled to the processing platform 320 via a SATA connection, but, in alternative embodiments, it may be any other type of non-volatile or temporary storage module. The bedside controller 300 further includes a wireless communications module 326 communicatively coupled to the

processing platform 320. In some embodiments, the wireless communications module is a IEEE 802.11 Wi-Fi module, but in other may be a Ultra Wide-Band (UWB) wireless module, a wireless FireWire module, a wireless USB module, a Bluetooth module, or another high-speed wireless networking module.

In the illustrated embodiment, the bedside controller 300 is powered via both a wired 12VDC power-over-Ethernet (PoE) connection 328 and a battery 330 disposed within the housing 302. In one embodiment, the battery 330 may be sealed within the integrally formed housing 302 and may be recharged through electrical contacts disposed on the exterior of the housing and electrically coupled to the battery. As shown in the embodiment of FIG. 3B, the front wall 350 may include one or more electrical contacts 358 through which the battery 330 may be charged when the controller is mounted to objects with compatible charging structure. In other embodiments, the housing 302 may include a battery compartment with a removable cover to permit battery replacement. Such a battery compartment cover may be resistant to fluid ingress (e.g., with an IPX4 rating). The bedside controller 300 may be coupled to a processing system in the catheter lab via the PoE connection 328, over which it receives medical sensing images that have been captured from the patient and rendered on the processing system. In operation, when the bedside controller is coupled to the PoE connection 328, it receives power and communications over the same physical wire. When the bedside controller 300 is disconnected from the PoE connection 328, it runs on battery power and receives data wirelessly via the wireless communications module 326. When used wirelessly in a catheter lab, the bedside controller may directly communicate with a processing system (i.e. in an ad-hoc wireless mode), or, alternatively, it may communicate with a wireless network that serves a plurality of wireless devices. In alternative embodiments, the bedside controller 300 may receive power and data through different wired connections, or receive data communications through a wired data connection and power from the battery 330, or receive data communications through the wireless module 326 and power from a wired electrical connection. In some embodiments, the bedside controller 300 may be used in a semi-wireless configuration, in which the battery 330 provides backup power to the controller when the controller is temporarily disconnected from a wired power source. For example, if at the beginning of a procedure, the bedside controller 300 is connected to a PoE connection (or other type of wired connection) and during the procedure the controller must be disconnected from the PoE connection to allow for a cabling adjustment, the battery 330 may keep the controller alive until a PoE connection can be re-established. In this manner, a full power-off and reboot of the controller 300 is avoided during a procedure. As shown in FIG. 4, a DC-DC power converter 332 converts input voltage to a voltage usable by the processing platform 320.

It is understood that although the bedside controller 300 in the illustrated embodiments of FIGS. 3 and 4 includes specific components described herein, the bedside controller may include any number of additional components, for example a charge regulator interposed between the electrical contacts and the battery, and may be configured in any number of alternative arrangements in alternative embodiments.

With reference now to FIGS. 5 and 6, illustrated are examples of locations in which the bedside controller 300 may be mounted. FIG. 5 is a diagrammatic perspective view of a mobile processing system 500. The processing system

500 is disposed on a cart 502 that enables the processing system to be easily moved between different locations such as different catheter labs. As shown in FIG. 5, the bedside controller 300 is mounted to the cart 502 so that it may be transported to catheter labs with the processing system. The bedside controller 300 is releasably secured to the cart via the self-contained mounting structure 303 that is built into the housing 302. Further, in some embodiments, the cart 502 may include a dock for the bedside controller 300 such that when the controller is docked on the cart its battery is recharged through the electrical contacts 358 disposed on the housing 302. As shown in FIG. 6, the bedside controller 300 may also releasably attach to an IV pole 600 via the self-contained mounting structure 303. When so attached, the bedside controller 300 may be rolled next to a patient in the sterile field and thus within reach of a clinician who may operate the controller with a single hand.

FIG. 7 is a flowchart illustrating a method 700 of conducting a medical sensing workflow with the bedside controller 300 of FIGS. 3A-4 according to various aspects of the present disclosure. The method 700 will be described in the context of a pressure-sensing procedure, such as an iFR procedure, but may equally apply to any number of medical sensing or treatment procedures, such as an FFR procedure, an IVUS procedure, OCT procedure, a FLIVUS procedure, an ICE procedure, etc. The method 700 can be better understood with reference to the FIGS. 8-16. The method 700 begins at block 710 where a medical sensing workflow is initiated with the bedside controller 300. Using an iFR procedure as an example, a clinician in the sterile field and adjacent a patient may select the "iFR" option out of a plurality of modes (e.g., FFR, iFR, CFR, etc.) on the bedside controller's GUI to begin the iFR workflow. Next, in block 720, after a pressure-sensing intravascular device, such as a catheter or guidewire, has been inserted into the patient, the clinician may select a 'Live' option on the bedside controller's GUI to receive live pressure measurements from the intravascular device. In some embodiments, the clinician may guide the intravascular device within the patient to a desired position using the real-time pressure measurements. In typical embodiments, a processing system may collect raw pressure data from the intravascular device and process the data to render visual representations of the obtained pressure data. The bedside controller retrieves the visual representations from the processing system and displays them to a user in real-time. Then, in block 730, after the pressure sensing intravascular device has been appropriately positioned in the patient, the clinician selects a 'Record' option on the bedside controller GUI. Pressure measurements can be collected during one or more of the following procedures: an FFR "spot" measurement where the pressure sensor stays in one place while hyperemia is induced; an FFR pullback in which an elongated period of hyperemia is induced and the sensor is pulled back to the ostium; an iFR "spot" measurement that is similar to the FFR spot measurement but without hyperemia; and an iFR pullback which is that the FFR pullback but without hyperemia. The processing system responds to the record command and begins rendering and storing the pressure measurements and visual representations generated from the pressure measurements. The visual representations can include numerical, graphical, textual, and/or other suitable visualizations. The method 700 proceeds to block 740 where, after the pressure measurement collection procedure has been completed, the clinician terminates the recording of pressure measurements via the bedside controller's GUI. Then, in block 750, the clinician at the bedside recalls and navigates through the pressure

measurements or corresponding visual representations on the bedside controller. Specifically, the bedside controller may present pressure measurements or visual representations of the obtained pressure data on the bedside controller and the clinician may navigate through them using gestures on the bedside controller's touch panel. Finally, in block 760, the clinician analyzes the obtained pressure data or visual representations of the obtained pressure data, directly on the bedside controller. For example, the user of the bedside controller interacts with the obtained pressure data or visual representations through a series of presses, moves and releases using a finger or stylus on the controller's touch-sensitive display. These actions are interpreted by the bedside controller's internal processor. In some embodiments, the obtained pressure data and/or visual representations can be modified in response to the user touch inputs. For example, a user touch input on the bedside controller can select a specific point a pressure waveform that corresponds to a specific time at which pressure measurements were obtained. In response to the user touch input, pressure data obtained at the specific time can be displayed proximate the specific point on the pressure waveform on the bedside controller.

Referring to FIGS. 8 and 9, shown therein is a vessel 800 having a stenosis according to an embodiment of the present disclosure. In that regard, FIG. 8 is a diagrammatic perspective view of the vessel 800, while FIG. 9 is a partial cross-sectional perspective view of a portion of the vessel 800 taken along section line 9-9 of FIG. 1. Referring more specifically to FIG. 8, the vessel 800 includes a proximal portion 802 and a distal portion 804. A lumen 806 extends along the length of the vessel 800 between the proximal portion 802 and the distal portion 804. In that regard, the lumen 806 is configured to allow the flow of fluid through the vessel. In some instances, the vessel 800 is a blood vessel. In some particular instances, the vessel 800 is a coronary artery. In such instances, the lumen 806 is configured to facilitate the flow of blood through the vessel 800.

As shown, the vessel 800 includes a stenosis 808 between the proximal portion 802 and the distal portion 804. Stenosis 808 is generally representative of any blockage or other structural arrangement that results in a restriction to the flow of fluid through the lumen 806 of the vessel 800. Embodiments of the present disclosure are suitable for use in a wide variety of vascular applications, including without limitation coronary, peripheral (including but not limited to lower limb, carotid, and neurovascular), renal, and/or venous. Where the vessel 800 is a blood vessel, the stenosis 808 may be a result of plaque buildup, including without limitation plaque components such as fibrous, fibro-lipidic (fibro fatty), necrotic core, calcified (dense calcium), blood, fresh thrombus, and mature thrombus. Generally, the composition of the stenosis will depend on the type of vessel being evaluated. In that regard, it is understood that the concepts of the present disclosure are applicable to virtually any type of blockage or other narrowing of a vessel that results in decreased fluid flow.

Referring more particularly to FIG. 9, the lumen 806 of the vessel 800 has a diameter 810 proximal of the stenosis 808 and a diameter 812 distal of the stenosis. In some instances, the diameters 810 and 812 are substantially equal to one another. In that regard, the diameters 810 and 812 are intended to represent healthy portions, or at least healthier portions, of the lumen 806 in comparison to stenosis 808. Accordingly, these healthier portions of the lumen 806 are illustrated as having a substantially constant cylindrical profile and, as a result, the height or width of the lumen has

been referred to as a diameter. However, it is understood that in many instances these portions of the lumen **806** will also have plaque buildup, a non-symmetric profile, and/or other irregularities, but to a lesser extent than stenosis **808** and, therefore, will not have a cylindrical profile. In such instances, the diameters **810** and **812** are understood to be representative of a relative size or cross-sectional area of the lumen and do not imply a circular cross-sectional profile.

As shown in FIG. 9, stenosis **808** includes plaque buildup **814** that narrows the lumen **806** of the vessel **800**. In some instances, the plaque buildup **814** does not have a uniform or symmetrical profile, making angiographic evaluation of such a stenosis unreliable. In the illustrated embodiment, the plaque buildup **814** includes an upper portion **816** and an opposing lower portion **818**. In that regard, the lower portion **818** has an increased thickness relative to the upper portion **816** that results in a non-symmetrical and non-uniform profile relative to the portions of the lumen proximal and distal of the stenosis **808**. As shown, the plaque buildup **814** decreases the available space for fluid to flow through the lumen **806**. In particular, the cross-sectional area of the lumen **806** is decreased by the plaque buildup **814**. At the narrowest point between the upper and lower portions **816**, **818** the lumen **806** has a height **820**, which is representative of a reduced size or cross-sectional area relative to the diameters **810** and **812** proximal and distal of the stenosis **808**. Note that the stenosis **808**, including plaque buildup **814** is exemplary in nature and should be considered limiting in any way. In that regard, it is understood that the stenosis **808** has other shapes and/or compositions that limit the flow of fluid through the lumen **806** in other instances. While the vessel **800** is illustrated in FIGS. 8 and 9 as having a single stenosis **808** and the description of the embodiments below is primarily made in the context of a single stenosis, it is nevertheless understood that the devices, systems, and methods described herein have similar application for a vessel having multiple stenosis regions.

Referring now to FIG. 10, the vessel **800** is shown with instruments **830** and **832** positioned therein according to an embodiment of the present disclosure. In general, instruments **830** and **832** may be any form of device, instrument, or probe sized and shaped to be positioned within a vessel. The instruments **830** and **832** can be implemented in the medical sensing system **100** (FIG. 1) as medical sensing devices **108** and **110**. In the illustrated embodiment, instrument **830** is generally representative of a guide wire, while instrument **832** is generally representative of a catheter. In that regard, instrument **830** extends through a central lumen of instrument **832**. However, in other embodiments, the instruments **830** and **832** take other forms. In that regard, the instruments **830** and **832** are of similar form in some embodiments. For example, in some instances, both instruments **830** and **832** are guide wires. In other instances, both instruments **830** and **832** are catheters. On the other hand, the instruments **830** and **832** are of different form in some embodiments, such as the illustrated embodiment, where one of the instruments is a catheter and the other is a guide wire. Further, in some instances, the instruments **830** and **832** are disposed coaxial with one another, as shown in the illustrated embodiment of FIG. 10. In other instances, one of the instruments extends through an off-center lumen of the other instrument. In yet other instances, the instruments **830** and **832** extend side-by-side. In some particular embodiments, at least one of the instruments is as a rapid-exchange device, such as a rapid-exchange catheter. In such embodiments, the other instrument is a buddy wire or other device configured to facilitate the introduction and removal of the

rapid-exchange device. Further still, in other instances, instead of two separate instruments **830** and **832** a single instrument is utilized. In some embodiments, the single instrument incorporates aspects of the functionalities (e.g., data acquisition) of both instruments **830** and **832**.

Instrument **830** is configured to obtain diagnostic information about the vessel **800**. In that regard, the instrument **830** includes one or more sensors, transducers, and/or other monitoring elements configured to obtain the diagnostic information about the vessel. The diagnostic information includes one or more of pressure, flow (velocity and/or volume), images (including images obtained using ultrasound (e.g., IVUS), OCT, thermal, and/or other imaging techniques), temperature, and/or combinations thereof. The one or more sensors, transducers, and/or other monitoring elements are positioned adjacent a distal portion of the instrument **830** in some instances. In that regard, the one or more sensors, transducers, and/or other monitoring elements are positioned less than 30 cm, less than 10 cm, less than 5 cm, less than 3 cm, less than 2 cm, and/or less than 1 cm from a distal tip **834** of the instrument **830** in some instances. In some instances, at least one of the one or more sensors, transducers, and/or other monitoring elements is positioned at the distal tip of the instrument **830**.

The instrument **830** includes at least one element configured to monitor pressure within the vessel **800**. The pressure monitoring element can take the form a piezo-resistive pressure sensor, a piezo-electric pressure sensor, a capacitive pressure sensor, an electromagnetic pressure sensor, a fluid column (the fluid column being in communication with a fluid column sensor that is separate from the instrument and/or positioned at a portion of the instrument proximal of the fluid column), an optical pressure sensor, and/or combinations thereof. In some instances, one or more features of the pressure monitoring element are implemented as a solid-state component manufactured using semiconductor and/or other suitable manufacturing techniques. Examples of commercially available guide wire products that include suitable pressure monitoring elements include, without limitation, the PrimeWire PRESTIGE® pressure guide wire, the PrimeWire® pressure guide wire, and the ComboWire® XT pressure and flow guide wire, each available from Volcano Corporation, as well as the PressureWire™ Certus guide wire and the PressureWire™ Aeris guide wire, each available from St. Jude Medical, Inc. Generally, the instrument **830** is sized such that it can be positioned through the stenosis **808** without significantly impacting fluid flow across the stenosis, which would impact the distal pressure reading. Accordingly, in some instances the instrument **830** has an outer diameter of 0.018" or less. In some embodiments, the instrument **830** has an outer diameter of 0.014" or less.

Instrument **832** is also configured to obtain diagnostic information about the vessel **100**. In some instances, instrument **832** is configured to obtain the same diagnostic information as instrument **830**. In other instances, instrument **832** is configured to obtain different diagnostic information than instrument **830**, which may include additional diagnostic information, less diagnostic information, and/or alternative diagnostic information. The diagnostic information obtained by instrument **832** includes one or more of pressure, flow (velocity and/or volume), images (including images obtained using ultrasound (e.g., IVUS), OCT, thermal, and/or other imaging techniques), temperature, and/or combinations thereof. Instrument **832** includes one or more sensors, transducers, and/or other monitoring elements configured to obtain this diagnostic information. In that regard, the one or

more sensors, transducers, and/or other monitoring elements are positioned adjacent a distal portion of the instrument **832** in some instances. In that regard, the one or more sensors, transducers, and/or other monitoring elements are positioned less than 30 cm, less than 10 cm, less than 5 cm, less than 3 cm, less than 2 cm, and/or less than 1 cm from a distal tip **836** of the instrument **832** in some instances. In some instances, at least one of the one or more sensors, transducers, and/or other monitoring elements is positioned at the distal tip of the instrument **832**.

Similar to instrument **830**, instrument **832** also includes at least one element configured to monitor pressure within the vessel **800**. The pressure monitoring element can take the form a piezo-resistive pressure sensor, a piezo-electric pressure sensor, a capacitive pressure sensor, an electromagnetic pressure sensor, a fluid column (the fluid column being in communication with a fluid column sensor that is separate from the instrument and/or positioned at a portion of the instrument proximal of the fluid column), an optical pressure sensor, and/or combinations thereof. In some instances, one or more features of the pressure monitoring element are implemented as a solid-state component manufactured using semiconductor and/or other suitable manufacturing techniques. Currently available catheter products suitable for use with one or more of Siemens AXIOM Sensis, Mennen Horizon XVu, and Philips Xper IM Physiomonitring 5 and include pressure monitoring elements can be utilized for instrument **832** in some instances.

In accordance with aspects of the present disclosure, at least one of the instruments **830** and **832** is configured to monitor a pressure within the vessel **800** distal of the stenosis **808** and at least one of the instruments **830** and **832** is configured to monitor a pressure within the vessel proximal of the stenosis. In that regard, the instruments **830**, **832** are sized and shaped to allow positioning of the at least one element configured to monitor pressure within the vessel **800** to be positioned proximal and/or distal of the stenosis **808** as necessary based on the configuration of the devices. In that regard, FIG. **10** illustrates a position **838** suitable for measuring pressure distal of the stenosis **808**. In that regard, the position **838** is less than 5 cm, less than 3 cm, less than 2 cm, less than 1 cm, less than 5 mm, and/or less than 2.5 mm from the distal end of the stenosis **808** (as shown in FIG. **9**) in some instances. FIG. **10** also illustrates a plurality of suitable positions for measuring pressure proximal of the stenosis **808**. In that regard, positions **840**, **842**, **844**, **846**, and **848** each represent a position that is suitable for monitoring the pressure proximal of the stenosis in some instances. In that regard, the positions **840**, **842**, **844**, **846**, and **848** are positioned at varying distances from the proximal end of the stenosis **808** ranging from more than 20 cm down to about 5 mm or less. Generally, the proximal pressure measurement will be spaced from the proximal end of the stenosis. Accordingly, in some instances, the proximal pressure measurement is taken at a distance equal to or greater than an inner diameter of the lumen of the vessel from the proximal end of the stenosis. In the context of coronary artery pressure measurements, the proximal pressure measurement is generally taken at a position proximal of the stenosis and distal of the aorta, within a proximal portion of the vessel. However, in some particular instances of coronary artery pressure measurements, the proximal pressure measurement is taken from a location inside the aorta. In other instances, the proximal pressure measurement is taken at the root or ostium of the coronary artery.

In some embodiments, at least one of the instruments **830** and **832** is configured to monitor pressure within the vessel

800 while being moved through the lumen **806**. In some instances, instrument **830** is configured to be moved through the lumen **806** and across the stenosis **808**. In that regard, the instrument **830** is positioned distal of the stenosis **808** and moved proximally (i.e., pulled back) across the stenosis to a position proximal of the stenosis in some instances. In other instances, the instrument **830** is positioned proximal of the stenosis **808** and moved distally across the stenosis to a position distal of the stenosis. Movement of the instrument **830**, either proximally or distally, is controlled manually by medical personnel (e.g., hand of a surgeon) in some embodiments. In other embodiments, movement of the instrument **830**, either proximally or distally, is controlled automatically by a movement control device (e.g., a pullback device, such as the Trak Back® II Device available from Volcano Corporation). In that regard, the movement control device controls the movement of the instrument **830** at a selectable and known speed (e.g., 2.0 mm/s, 1.0 mm/s, 0.5 mm/s, 0.2 mm/s, etc.) in some instances. Movement of the instrument **830** through the vessel is continuous for each pullback or push through, in some instances. In other instances, the instrument **830** is moved step-wise through the vessel (i.e., repeatedly moved a fixed amount of distance and/or a fixed amount of time). Some aspects of the visual depictions discussed below are particularly suited for embodiments where at least one of the instruments **830** and **832** is moved through the lumen **806**. Further, in some particular instances, aspects of the visual depictions discussed below are particularly suited for embodiments where a single instrument is moved through the lumen **806**, with or without the presence of a second instrument.

In some instances, use of a single instrument has a benefit in that it avoids issues associated with variations in pressure measurements of one instrument relative to another over time, which is commonly referred to as drift. In that regard, a major source of drift in traditional Fractional Flow Reserve (FFR) measurements is divergence in the pressure reading of a guide wire relative to the pressure reading of a guide catheter. In that regard, because FFR is calculated as the ratio of the pressure measurement obtained by the guide wire to the pressure measurement obtained by the catheter, this divergence has an impact on the resulting FFR value. In contrast, where a single instrument is utilized to obtain pressure measurements as it is moved through the vessel, drift is negligible or non-existent. For example, in some instances, the single instrument is utilized to obtain relative changes in pressures as it is moved through the vessel such that the time period between pressure measurements is short enough to prevent any impact from any changes in pressure sensitivity of the instrument (e.g., less than 500 ms, less than 100 ms, less than 50 ms, less than 10 ms, less than 5 ms, less than 1 ms, or otherwise).

Referring now to FIG. **11**, shown therein is a system **850** according to an embodiment of the present disclosure. In that regard, FIG. **11** is a diagrammatic, schematic view of the system **850**. In some embodiments, the system **850** can be implemented as the medical sensing system **100** (FIG. **1**). In some embodiments, one or more components of the medical sensing system **100** can be additionally implemented in the system **850**, such as a bedside controller having a touch-sensitive display. As shown, the system **850** includes an instrument **852**. In that regard, in some instances instrument **852** is suitable for use as at least one of instruments **830** and **832** (FIGS. **8-10**) and/or medical sensing devices **108** and **110** (FIG. **1**), discussed above. Accordingly, in some instances the instrument **852** includes features similar to those discussed above with respect to instruments **830** and

832 in some instances. In the illustrated embodiment, the instrument **852** is a guide wire having a distal portion **854** and a housing **856** positioned adjacent the distal portion. In that regard, the housing **856** is spaced approximately 3 cm from a distal tip of the instrument **852**. The housing **856** is configured to house one or more sensors, transducers, and/or other monitoring elements configured to obtain the diagnostic information about the vessel. In the illustrated embodiment, the housing **856** contains at least a pressure sensor configured to monitor a pressure within a lumen in which the instrument **852** is positioned. A shaft **858** extends proximally from the housing **856**. A torque device **860** is positioned over and coupled to a proximal portion of the shaft **858**. A proximal end portion **862** of the instrument **852** is coupled to a connector **864**. A cable **866** extends from connector **864** to a connector **868**. In some instances, connector **868** is configured to be plugged into an interface **870**. In that regard, interface **870** is a patient interface module (PIM) in some instances. The interface **870** can be implemented as the PIM **112** (FIG. 1). In some instances, the cable **866** is replaced with a wireless connection. In that regard, it is understood that various communication pathways between the instrument **852** and the interface **870** may be utilized, including physical connections (including electrical, optical, and/or fluid connections), wireless connections, and/or combinations thereof.

The interface **870** is communicatively coupled to a computing device **872** via a connection **874**. Computing device **872** is generally representative of any device suitable for performing the processing and analysis techniques discussed within the present disclosure. In some embodiments, the computing device **872** includes a processor, random access memory, and a storage medium. In that regard, in some particular instances the computing device **872** is programmed to execute steps associated with the data acquisition and analysis described herein. Accordingly, it is understood that any steps related to data acquisition, data processing, instrument control, and/or other processing or control aspects of the present disclosure may be implemented by the computing device using corresponding instructions stored on or in a non-transitory computer readable medium accessible by the computing device. In some instances, the computing device **872** is the bedside controller. For example, the processing steps described herein can be performed by one or more processing components of the bedside controller, such as the processing platform **320** (FIG. 4). In some instances, the computing device **872** is a console device. In some particular instances, the computing device **872** is similar to the s5™ Imaging System or the s5i™ Imaging System, each available from Volcano Corporation. In some instances, the computing device **872** is portable (e.g., handheld, on a rolling cart, etc.). Further, it is understood that in some instances the computing device **872** comprises a plurality of computing devices. In that regard, it is particularly understood that the different processing and/or control aspects of the present disclosure may be implemented separately or within predefined groupings using a plurality of computing devices. Any divisions and/or combinations of the processing and/or control aspects described below across multiple computing devices are within the scope of the present disclosure.

Together, connector **864**, cable **866**, connector **868**, interface **870**, and connection **874** facilitate communication between the one or more sensors, transducers, and/or other monitoring elements of the instrument **852** and the computing device **872**. However, this communication pathway is exemplary in nature and should not be considered limiting in

any way. In that regard, it is understood that any communication pathway between the instrument **852** and the computing device **872** may be utilized, including physical connections (including electrical, optical, and/or fluid connections), wireless connections, and/or combinations thereof. In that regard, it is understood that the connection **874** is wireless in some instances. In some instances, the connection **874** includes a communication link over a network (e.g., intranet, internet, telecommunications network, and/or other network). In that regard, it is understood that the computing device **872** is positioned remote from an operating area where the instrument **152** is being used in some instances. Having the connection **874** include a connection over a network can facilitate communication between the instrument **852** and the remote computing device **872** regardless of whether the computing device is in an adjacent room, an adjacent building, or in a different state/country. Further, it is understood that the communication pathway between the instrument **852** and the computing device **872** is a secure connection in some instances. Further still, it is understood that, in some instances, the data communicated over one or more portions of the communication pathway between the instrument **852** and the computing device **872** is encrypted.

The system **850** also includes an instrument **875**. In that regard, in some instances instrument **875** is suitable for use as at least one of instruments **130** and **132** (FIGS. 8-10) and/or medical sensing devices **108** and **110** (FIG. 1), discussed above. Accordingly, in some instances the instrument **875** includes features similar to those discussed above with respect to instruments **130** and **132** in some instances. In the illustrated embodiment, the instrument **875** is a catheter-type device. In that regard, the instrument **875** includes one or more sensors, transducers, and/or other monitoring elements adjacent a distal portion of the instrument configured to obtain the diagnostic information about the vessel. In the illustrated embodiment, the instrument **875** includes a pressure sensor configured to monitor a pressure within a lumen in which the instrument **875** is positioned. The instrument **875** is in communication with an interface **876** via connection **877**. In some instances, interface **876** is a hemodynamic monitoring system or other control device, such as Siemens AXIOM Sensis, Mennen Horizon XVu, and Philips Xper IM Physiomonitring 5. In one particular embodiment, instrument **875** is a pressure-sensing catheter that includes fluid column extending along its length. In such an embodiment, interface **876** includes a hemostasis valve fluidly coupled to the fluid column of the catheter, a manifold fluidly coupled to the hemostasis valve, and tubing extending between the components as necessary to fluidly couple the components. In that regard, the fluid column of the catheter is in fluid communication with a pressure sensor via the valve, manifold, and tubing. In some instances, the pressure sensor is part of interface **876**. In other instances, the pressure sensor is a separate component positioned between the instrument **875** and the interface **876**. The interface **876** is communicatively coupled to the computing device **872** via a connection **878**.

Similar to the connections between instrument **852** and the computing device **872**, interface **876** and connections **877** and **878** facilitate communication between the one or more sensors, transducers, and/or other monitoring elements of the instrument **875** and the computing device **872**. However, this communication pathway is exemplary in nature and should not be considered limiting in any way. In that regard, it is understood that any communication pathway between the instrument **875** and the computing device **872**

may be utilized, including physical connections (including electrical, optical, and/or fluid connections), wireless connections, and/or combinations thereof. In that regard, it is understood that the connection **878** is wireless in some instances. In some instances, the connection **878** includes a communication link over a network (e.g., intranet, internet, telecommunications network, and/or other network). In that regard, it is understood that the computing device **872** is positioned remote from an operating area where the instrument **875** is being used in some instances. Having the connection **878** include a connection over a network can facilitate communication between the instrument **875** and the remote computing device **872** regardless of whether the computing device is in an adjacent room, an adjacent building, or in a different state/country. Further, it is understood that the communication pathway between the instrument **875** and the computing device **872** is a secure connection in some instances. Further still, it is understood that, in some instances, the data communicated over one or more portions of the communication pathway between the instrument **875** and the computing device **872** is encrypted.

It is understood that one or more components of the system **850** are not included, are implemented in a different arrangement/order, and/or are replaced with an alternative device/mechanism in other embodiments of the present disclosure. For example, in some instances, the system **850** does not include interface **870** and/or interface **876**. In such instances, the connector **868** (or other similar connector in communication with instrument **852** or instrument **875**) may plug into a port associated with computing device **872**. Alternatively, the instruments **852**, **875** may communicate wirelessly with the computing device **872**. Generally speaking, the communication pathway between either or both of the instruments **852**, **875** and the computing device **872** may have no intermediate nodes (i.e., a direct connection), one intermediate node between the instrument and the computing device, or a plurality of intermediate nodes between the instrument and the computing device. The system **850** can additionally include a bedside controller, such as the bedside controller of medical sensing system **100** (FIG. 1). The bedside controller may be utilized by a clinician to control a instruments **852** and **875** to acquire pressure data during a procedure, watch real-time medical pressure measurements (e.g., visual representations of pressure data, such as pressure waveforms, numerical values, etc.), and interact with the obtained medical sensing data using the bedside controller. In that regard, the bedside controller can be communicatively coupled to the computing device **872**, the interfaces **870** and **876**, and/or the instruments **864** and **875**.

Referring now to FIGS. 12-16, shown therein are various visual depictions of screen displays for evaluating a vessel based on obtained pressure measurements according to embodiments of the present disclosure. The screen displays are displayed on a touch-sensitive display of a bedside controller. A clinician can view, analyze, and interact with the pressure data and/or visual representations of the pressure data. Referring more specifically to FIG. 12, shown therein is a screen display **1200** according to an embodiment of the present disclosure. As illustrated, the screen display **1200** is associated with an iFR workflow. The screen display **1200** includes an FFR tab **1204** and an iFR tab **1202**. The iFR tab **1202** can include the obtained pressure measurements, and visual representations of the pressure measurements. As shown, the iFR tab **1202** includes pressure waveform plots **1212** and **1238**, both of which illustrate acquired pressure data over the same time period. The screen display

1200 also includes a window **1214** that shows a calculated pressure ratio (e.g., FFR, iFR, or otherwise).

In that regard, the pressure waveform plots **1212** and **1238** and the calculated pressure ratio of screen display **1200** illustrate aspects of pressure measurements obtained as one instrument is moved through the vessel and another instrument is maintained at a fixed location. In that regard, in some instances the pressure measurements are representative of a pressure ratio between a fixed location within the vessel and the moving position of the instrument as the instrument is moved through the vessel. For example, in some instances a proximal pressure measurement is obtained at a fixed location within the vessel while the instrument is pulled back through the vessel from a first position distal of the position where the proximal pressure measurement is obtained to a second position more proximal than the first position (i.e., closer to the fixed position of the proximal pressure measurement). For clarity in understanding the concepts of the present disclosure, this arrangement will be utilized to describe many of the embodiments of the present disclosure. However, it is understood that the concepts are equally applicable to other arrangements. For example, in some instances, the instrument is pushed through the vessel from a first position distal of the proximal pressure measurement location to a second position further distal (i.e., further away from the fixed position of the proximal pressure measurement). In other instances, a distal pressure measurement is obtained at a fixed location within the vessel and the instrument is pulled back through the vessel from a first position proximal of the fixed location of the distal pressure measurement to a second position more proximal than the first position (i.e., further away from the fixed position of the distal pressure measurement). In still other instances, a distal pressure measurement is obtained at a fixed location within the vessel and the instrument is pushed through the vessel from a first position proximal of the fixed location of the distal pressure measurement to a second position less proximal than the first position (i.e., closer the fixed position of the distal pressure measurement).

The pressure differential between the two pressure measurements within the vessel (e.g., a fixed location pressure measurement and a moving pressure measurement) is calculated as a ratio of the two pressure measurements (e.g., the moving pressure measurement divided by the fixed location pressure measurement), in some instances. In some instances, the pressure differential is calculated for each heartbeat cycle of the patient. In that regard, the calculated pressure differential is the average pressure differential across a heartbeat cycle in some embodiments. For example, in some instances where a hyperemic agent is applied to the patient, the average pressure differential across the heartbeat cycle is utilized to calculate the pressure differential. In other embodiments, only a portion of the heartbeat cycle is utilized to calculate the pressure differential. The pressure differential is an average over the portion or diagnostic window of the heartbeat cycle, in some instances.

In some embodiments a diagnostic window is selected using one or more of the techniques described in U.S. patent application Ser. No. 13/460,296, filed Apr. 30, 2012, now published as U.S. Patent Application Publication No. 2013-0046190 A1 on Feb. 21, 2013 and titled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSING A VESSEL," which is hereby incorporated by reference in its entirety. As discussed therein, the diagnostic windows and associated techniques are particularly suitable for use without application of a hyperemic agent to the patient. In general, the diagnostic window for evaluating differential pressure

across a stenosis without the use of a hyperemic agent is identified based on characteristics and/or components of one or more of proximal pressure measurements, distal pressure measurements, proximal velocity measurements, distal velocity measurements, ECG waveforms, and/or other identifiable and/or measurable aspects of vessel performance. In that regard, various signal processing and/or computational techniques can be applied to the characteristics and/or components of one or more of proximal pressure measurements, distal pressure measurements, proximal velocity measurements, distal velocity measurements, ECG waveforms, and/or other identifiable and/or measurable aspects of vessel performance to identify a suitable diagnostic window.

The visual representations in the screen display **1200** illustrate the pressure ratio and/or the underlying pressure measurements in any suitable way. Generally speaking, the representation of the data can be utilized to identify gradients/changes in the pressure ratio and/or the underlying pressure measurements that can be indicative of a significant lesion in the vessel. In that regard, the visual representation of the data can include the pressure measurement(s); a ratio of the pressure measurements; a difference in the pressure measurements; a gradient of the pressure measurement(s), the ratio of the pressure measurements, and/or the difference in the pressure measurements; first or second derivatives of the pressure measurement(s), the ratio of the pressure measurements, and/or the difference in the pressure measurements; and/or combinations thereof.

For example, the pressure waveform plots **1212** and **1238** show corresponding pressure data. In that regard, the pressure waveform plots **1212** and **1238** can include the pressure waveform for the pressure sensing device moved through the vessel during the pullback, the pressure waveform for the stationary pressure sensing device, or both. In the illustrated embodiment, the pressure waveform plots **1212** and **1238** include the pressure waveforms for both. As will be discussed below with respect to FIGS. **14-16**, in some instances the pressure waveform plot **1212** is augmented to highlight or otherwise accentuate the pressure data corresponding to the diagnostic window utilized for the pressure ratio calculations.

The pressure waveform plots **1212** and **1238** include time on the x-axis and magnitude of pressure on the y-axis. The pressure waveform plot **1238** illustrates the obtained pressure measurements over a greater amount of time compared to the waveform plot **1212**. For example, the pressure waveform plot **1238** illustrates the entire acquisition, pullback, or "run" while the pressure waveform **1212** illustrates at least a portion thereof. The pressure waveform plot **1212** includes a curve **1256** that is representative of the pressure measured by the instrument maintained at a fixed location (for sake of brevity, this will be referred to as Pa below) and a curve **1252** that is representative of the pressure measured by the instrument moved through the vessel for the pullback over time (for sake of brevity, this will be referred to as Pd below). The pressure waveform plot **1212** also includes the averages of the acquired Pa and Pd values. The curve **1254** is representative of the average Pd values, while the curve **1258** is representative of the average Pa values. In that regard, the average Pa and Pd values can be a mean, median, mode, and/or other suitable value (e.g., filtering to remove outliers, then using mean, median, and/or mode, etc.) for each heartbeat cycle. In some embodiments, the pressure waveform plot **1212** includes all four curves **1252**, **1254**, **1256**, and **1258**. In some embodiments, the pressure waveform plot **1212** includes a subset (e.g., one or more, but not all) of the curves **1252**, **1254**, **1256**, and **1258**. For example,

the pressure waveform plot **1212** can illustrate only the acquired Pa and Pd values by including the curves **1242** and **1256**, or only the average Pa and Pd values by including the curves **1254** and **1258**. The pressure waveform plot **1238** can similarly illustrate one or more of the curves **1252**, **1254**, **1256**, and **1258** over the entire acquisition. In FIG. **12**, the pressure waveform plot **1212** includes all four curves **1252**, **1254**, **1256**, and **1258**, while the pressure waveform plot **1238** includes the average Pa and Pd values. The pressure waveform plots **1212** and **1238** can include raw pressure data and/or data that smoothed, filtered, conditioned, and/or otherwise treated to remove abnormalities in the data as described in U.S. Provisional Patent Application No. 61/856,518, filed Jul. 19, 2013, now published as U.S. Patent Application Publication No. 2015/0025398 A1 on Jan. 22, 2015 and titled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSING A VESSEL WITH AUTOMATED DRIFT CORRECTION," which is hereby incorporated by reference in its entirety. A normalize option **1246** can be provided to perform a normalization procedure described in U.S. application Ser. No. 14/157,404, filed Jan. 16, 2014, now published as U.S. Patent Application Publication No. 2014/0135633 A1 on May 15, 2014 and titled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSING A VESSEL," which is hereby incorporated by reference herein, in its entirety.

A graphical overlay **1240** overlay can be positioned over a portion of the pressure waveform plot **1238**. The overlay **1240** illustrates a portion of the obtained pressure measurements represented in the pressure waveform plot **1212**. Thus, for example, the pressure waveform plot **1212** is a "zoomed in" version of the pressure waveform plot **1238** in that the pressure waveform plot **1212** covers a shorter acquisition period but includes more detail about the pressure measurements during that selected time period. A user can interact with the pressure data by, e.g., touch and dragging the overlay **1240** and or the pressure waveform plot **1212** to the left or right, on the touch-sensitive display of the bedside controller, to view other portions of the acquisition. The screen display **1200** can automatically update, in real time, as the user clicks and drags the overlay **1240**. For example, the screen display **1200** can be automatically modified as the overlay **1240** shifts position over the pressure waveform plot **1238** and as the pressure waveform plot **1212** updates to include pressure data collected over the selected time period. The screen display **1200** also includes zoom buttons **1218**, **1220** that allow a user to zoom out or in, respectively, on the pressure waveform plot **1212**. The screen display **1200** can automatically update the pressure waveform plot **1212** to include the appropriate portions of pressure data, and the width and/or the position of the overlay **1240** over the pressure waveform plot **1238** in response to the user touch inputs on the zoom buttons **1218**, **1220**.

The screen display **1200** can include a visual representation of the acquired pressure measurements at a particular time. For example, a user can touch and release at a point on the pressure waveform plot **1212**, on touch-sensitive display of the bedside controller. The selected point or location in the plot **1212** corresponds to a particular time during the acquisition. As shown in FIG. **12**, a user provides a touch input near seven seconds on the pressure waveform plot **1212**. In response to the user touch input, the screen display **1200** can be modified to include one or more information overlays **1260**, **1262**, and/or **1264**. The overlay **1260** is a vertical line highlighting the time selected by the user by the touch input. The overlay **1260** can be variously colored to

visually distinguish the selected time. The overlay **1264** provides the numerical value of the time that is selected by the user touch input. The overlay **1262** provides pressure data at the selected time. In that regard, the overlay **1262** can include a numerical value of a calculated pressure ratio (iFR, FFR, etc.) at the selected time, a numerical value of a compensated Pd/Pa at the selected time, a numerical value of the average Pd value at the selected time, a numerical value of the average Pa value at the selected time, a numerical value of the actual Pd value at the selected time, and/or a numerical value of the actual Pa value at the selected time. The numerical values in the overlay **1262** can be raw or modified values. When a particular time is highlighted in response to a user touch input in the pressure waveform plot **1212**, the screen display **1200** can be automatically modified to include a corresponding overlay **1242** in the pressure waveform plot **1238** to contextualize the highlighted time within the entire acquisition. As described with respect to FIG. **13**, some embodiments of the screen display can include a fixed indicator **1244** in one or both of the pressure waveform plots **1212** and **1238**, which highlights a particular fixed time in the acquisition (e.g., a time associated with maximal hyperemia, at which point FFR is calculated). In some embodiments, the overlay(s) highlighting the selected time can be removed in response to a user touch input on the bedside controller.

The screen display **1200** also provides pressure ratios **1236** (e.g., iFR, compensated Pa/Pd values, etc.) at fixed intervals. For example, in FIG. **12**, the iFR values **1236** for each heartbeat cycle are displayed below the pressure waveform plot **1212**. In other embodiments, the pressure ratios are displayed at various locations relative to the pressure waveform plot **1212**, such as proximate the curve **1252**, **1254**, **1256**, and/or **1258**.

The screen display **1200** also includes a window **1214** that shows a calculated pressure ratio (e.g., FFR, iFR, or otherwise). In the illustrated embodiment of FIG. **12**, the window **1214** shows an iFR pressure ratio value during a pullback. In that regard, the iFR pressure ratio and/or associated data may be calculated and/or displayed as described in one or more of PCT Patent Application Publication No. WO 2012/093260, filed Jan. 6, 2012 and titled "APPARATUS AND METHOD OF CHARACTERISING A NARROWING IN A FLUID FILLED TUBE," PCT Patent Application Publication No. WO 2012/093266, filed Jan. 6, 2012 and titled "APPARATUS AND METHOD OF ASSESSING A NARROWING IN A FLUID FILLED TUBE," U.S. patent application Ser. No. 13/460,296, filed Apr. 30, 2012, now published as U.S. Patent Application Publication No. 2013-0046190-A1 on Feb. 21, 2013, and titled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSING A VESSEL," PCT Patent Application Publication No. WO 2013/028612, filed Aug. 20, 2012 and titled "DEVICES, SYSTEMS, AND METHODS FOR VISUALLY DEPICTING A VESSEL AND EVALUATING TREATMENT OPTIONS," U.S. Provisional Patent Application No. 61/856,509, filed Jul. 19, 2013, now published as U.S. Patent Application Publication No. 2015-0025330 A1 on Jan. 22, 2015, and titled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSMENT OF VESSELS," and U.S. Provisional Patent Application No. 61/856,518, filed Jul. 19, 2013, now published as U.S. Patent Application Publication No. 2015/0025398 A1 on Jan. 22, 2015 and titled "DEVICES, SYSTEMS, AND METHODS FOR ASSESSING A VESSEL WITH AUTOMATED DRIFT CORRECTION," each of which is hereby incorporated by reference in its entirety. In some instances, the numerical value of the pressure ratio

displayed in window **1214** is updated based on portion of pressure data displayed the pressure waveform plot **1212** and/or the position of the overlay **1240** over the pressure waveform plot **1238**. In that regard, in some instances the numerical value of the pressure ratio displayed in window **214** is based solely on the pressure data being displayed in the pressure waveform plot **1212**. However, in other instances the numerical value of the pressure ratio displayed in window **214** is based one of or a combination of the pressure data being displayed in the plot **1212** and pressure data not displayed in the pressure waveform plot **1212**. For example, the pressure ratio displayed in the window **214** can be based on the entire acquisition (as illustrated by the pressure waveform plot **1240**, in some embodiments). The screen display **1200** also includes windows **1270** and **1272** that show the Pd and Pa values, respectively, used to calculate the pressure ratio shown in window **1214**.

As shown in FIG. **12**, the screen display **1200** provided on the touch-sensitive display of the bedside controller includes a button **1226** indicating that the data is being displayed in a "Live" mode, which indicates that the screen display **1200**, including pressure waveform plots **1212** and **1238**, calculated pressure ratios **1236**, and/or the windows **1214**, **1270**, **1272** are being updated in real time as a procedure is being performed. The record button **1250** can be selected by a user touch input on the bedside controller to begin storing the acquired pressure data. In other instances, the button **1226** of the screen display **1200** will indicated that it is in "Playback" or "Review" mode, which indicates that the screen display **1200** is showing data obtained previously. With respect to the "Live" mode, it should be noted that the determination of the diagnostic window and/or the calculation of the pressure differential are performed in approximately real time or live to identify the diagnostic window of the heartbeat cycle and calculate the pressure differential. In that regard, calculating the pressure differential in "real time" or "live" within the context of the present disclosure is understood to encompass calculations that occur within 10 seconds of data acquisition. It is recognized, however, that often "real time" or "live" calculations are performed within 1 second of data acquisition. In some instances, the "real time" or "live" calculations are performed concurrent with data acquisition. In some instances the calculations are performed by a processor in the delays between data acquisitions. For example, if data is acquired from the pressure sensing devices for 1 ms every 5 ms, then in the 4 ms between data acquisitions the processor can perform the calculations. It is understood that these timings are for example only and that data acquisition rates, processing times, and/or other parameters surrounding the calculations will vary. In other embodiments, the pressure differential calculation is performed 10 or more seconds after data acquisition. For example, in some embodiments, the data utilized to identify the diagnostic window and/or calculate the pressure differential are stored for later analysis.

By comparing the calculated pressure differential to a threshold or predetermined value, a physician or other treating medical personnel can determine what, if any, treatment should be administered. In that regard, in some instances, a calculated pressure differential above a threshold value (e.g., 0.80 on a scale of 0.00 to 1.00) is indicative of a first treatment mode (e.g., no treatment, drug therapy, etc.), while a calculated pressure differential below the threshold value is indicative of a second, more invasive treatment mode (e.g., angioplasty, stent, etc.). In some instances, the threshold value is a fixed, preset value. In other instances, the threshold value is selected for a particu-

lar patient and/or a particular stenosis of a patient. In that regard, the threshold value for a particular patient may be based on one or more of empirical data, patient characteristics, patient history, physician preference, available treatment options, and/or other parameters.

In that regard, the coloring and/or other visually distinguishing aspect of the pressure differential measurements depicted in pressure ratios **1236** and/or window **1214** of the screen display **1200** of FIG. **12** are configured based on the threshold value in some instances. For example, a first color (e.g., green, white, or otherwise) can be utilized to represent values well above the threshold value (e.g., where the threshold value is 0.80 on a scale of 0.00 to 1.00, values above 0.90), a second color (e.g., yellow, gray, or otherwise) can be utilized to represent values near but above the threshold value (e.g., where the threshold value is 0.80 on a scale of 0.00 to 1.00, values between 0.81 and 0.90), and a third color (e.g., red, black, or otherwise) can be utilized to represent values equal to or below the threshold value (e.g., where the threshold value is 0.80 on a scale of 0.00 to 1.00, values of 0.80 and below). It is appreciated that any number of color combinations, scalings, categories, and/or other characteristics can be utilized to visually represent the relative value of the pressure differential to the threshold value. However, for the sake of brevity Applicants will not explicitly describe the numerous variations herein.

The screen display **1200** includes an ECG waveform **1232**. The ECG waveform can be temporally synced with the pressure waveform plots **1212** and/or **1238**. In that regards, the ECG waveform **1232** can be modified in response to modifications of the pressure waveform plots **1212** and/or **1238**. For example, the ECG waveform **1232** can be “zoomed in” or “zoomed in” when a user views different portions of the pressure waveform plots **1212** and/or **1238** such that the times in the ECG waveform **1232** and the pressure waveform plots **1212** and **1238** are synced. The screen display **1200** additionally includes a patient name **1266**, patient identifier **1268**, and a date/time **1274**. The case log button **1200** can be selected access additional information about the patient (e.g., other pressure acquisitions) and/or retrieve the current pressure acquisition data at a later time. A label field **1234** allows the user to input additional notes regarding the patient or the procedure. Selecting the label field **1266** by a touch input on the bedside controller can cause an on-screen keyboard to be displayed. The user can input characters into the label field **1266** by touch inputs on the on-screen keyboard. The screen display also includes an options tab **1208** and a bookmark option **1248**, which described in greater detail with respect to FIG. **13**.

Referring now to FIG. **13**, shown therein a screen display **1300** according to an embodiment of the present disclosure. The screen display **1300** is similar in many respects to screen display **1200** described above. In that regard, one or more features of screen display **1200** can be included in the screen display **1300** (e.g., the overlays **1262** and/or **1264**). However, the screen display **1300** is associated with an FFR workflow. In that regard, a hyperemic agent can be administered to the patient at two intervals **1290** and **1292**, as illustrated in the pressure waveform plot **1238**. The FFR tab **1204** can include the obtained pressure measurements and visual representations of the pressure measurements. In that regard, the FFR tab **1204** includes a window **1276** that shows a numerical value of the calculated pressure ratio (e.g., FFR, iFR, or otherwise) as well as windows **1270** and **1272** that show the numerical values of the average Pd and Pa at maximum hyperemia, which are used to calculate FFR.

The screen display **1300** can also include a window **1278** that shows the numerical compensated Pd/Pa value and/or a window **1280** that includes one or both of the numerical differences between Pd and Pa (e.g., Pd—Pa and/or Pa—Pd).

The pressure waveform plot **1212** can include one or both of overlays **1282** and **1284** that highlight the time during the acquisition corresponding to maximum hyperemia. The time at which maximum hyperemia can be automatically determined by the processing system. A time at which maximum hyperemia occurs can be determined for each hyperemia interval **1290** and **1292**. The overlay **1282** is vertical line highlighting the time at which hyperemia occurred during the hyperemia interval **1292**. The overlay **1282** can be variously colored to visually distinguish the selected time. For example, the overlay **1282** can be differently colored than the overlay **1260**, which is a user highlighted time during the acquisition, as described above with respect to FIG. **12**. The average Pa and Pd values at the determined time of maximum hyperemia are used to calculate the FFR for the interval **1292**. The overlay **1284** is a textual indicator that that specifies that the FFR is calculated based on average Pa and Pd values at the highlighted time. The pressure waveform plot **1238** includes an overlay **1286** contextualizing the time(s) during the acquisition when maximum hyperemia occurs for the interval **1292** and an overlay **1294** indicating when maximum hyperemia occurs for the interval **1290**. The pressure waveform plot **1238** also includes the overlay **1242** that highlights the user-selected time. As with the overlays **1260** and **1282** in the pressure waveform plot **1212**, the overlay **1242** is colored differently than the overlays **1286** and **1292** in pressure waveform **1238**. The overlays **1282**, **1286**, and/or **1294** can be positioned at fixed locations in the waveforms **1212** and/or **1238**, which correspond to the determined times at which maximum hyperemia occur in the intervals **1290** and **1292**. The overlays **1242** and/or **1260** can be selectively added or removed in response to a user's touch input at any location in the waveforms **1212** and/or **1238**, which corresponding to any time during the acquisition.

The pressure waveform plot **1212** in screen display **1300** includes a bookmark **1288**. The bookmark **1288** can be added during “Live” or “Review” mode when a user touches and releases the bookmark option **1248** on the touch-sensitive display of the bedside controller. The bookmark can highlight a time during the acquisition that a clinician is interested in later reviewing in more detail. For example, a clinician can touch and release the pressure waveform **1212** at the point corresponding to the bookmark **1288** such that, e.g., the overlay **1262** providing pressure data at the selected time is displayed on the bedside controller. In some embodiments, touching and release the bookmark **1288** can cause the overlay **1262** to be displayed. In some embodiments the screen display **1300** includes a screenshot option **1276** for the user to take a picture of the screen display in its current form. The screenshot can be saved in a memory of the bedside controller and later accessed by the user by selecting, e.g., the case log **1230**.

Referring generally to FIGS. **14-16**, shown therein are additional visual representations of pressure measurements that can be provided in addition to and/or in lieu of the elements of screen displays **1200** and **1300**. In that regard, the screen displays **1200** and **1300** can include one or more features described in U.S. Provisional Application No. 61/942,338, filed Feb. 20, 2014, now published as U.S. Patent Application Publication Nos. 2015-0230713 A1 on Aug. 20, 2015, and 2015-0238096 A1 on Aug. 27, 2015

titled “Devices, Systems, and Methods and Associated Display Screens for Assessment of Vessels” and U.S. Provisional Application No. 62/024,901, titled “Devices, Systems, and Methods and Associated Display Screens for Assessment of Vessels with Multiple Sensing Components” and filed Jul. 15, 2014, both of which are hereby incorporated by reference herein in their entireties. For example, the screen displays **1200** and **1300** can include numerical, visual, and/or graphical representations of an pressure ratio (iFR, FFR, compensated Pa/Pd, etc.) over time, a pressure difference during a pullback, a cumulative change in a pressure ratio value over time during a pullback, a localized change in pressure ratio value over time, Pa and Pd pressures over time during a pullback, pressure measurements obtained from multiple distal pressure sensing components over time as part of a virtual pullback, an enhanced angiographic image of a vessel based on overlaid intravascular measurements, etc. The screen displays can be provided to the bedside controller where a user can view and interact with the data with touch inputs on the touch-sensitive display.

Referring now to FIGS. **14-16**, shown therein are various displays of pressure waveform plots according to the present disclosure. In particular, the embodiments of FIGS. **14-16** may be used in place of the pressure waveform plot **1212** and/or **1238** in any of the screen displays of the present disclosure. To that end, the pressure waveform plots of FIGS. **14-16** highlight, emphasis, and/or otherwise accentuate the portion(s) of the pressure data utilized in making the pressure ratio calculations depicted in the other graphs and/or windows of the screen displays. In particular, in some implementations the pressure waveform plots of FIGS. **14-16** identify the diagnostic window utilized in making iFR calculations.

Referring more specifically to FIG. **14**, shown therein is a pressure waveform plot **100** that corresponds to similar data as shown in pressure waveform plot **1212** of FIG. **12**, but where the pressure data for each heartbeat that is within the diagnostic window utilized for making the iFR calculations shown in window **1214** has been highlighted. For example, for the first heartbeat cycle on the left side of the pressure waveform plot **1400**, the pressure data within a diagnostic window **1402** has been highlighted. By highlighting the portions of the pressure waveform plot **1400** within the diagnostic window for each heartbeat cycle, a user can quickly visualize the pressure data being relied upon for the resulting pressure ratio calculations.

FIGS. **15** and **16** illustrate other ways of identifying the portions of the pressure waveform plot within the diagnostic window for each heartbeat cycle. For example, FIG. **15** shows a pressure waveform plot **1500** that corresponds to the similar data as shown in pressure waveform plots **1212** and **1400** above, but where the pressure data for each heartbeat that is within the diagnostic window utilized for making the iFR calculations shown window **1214** has been highlighted and the pressure data for each heartbeat that is outside of the diagnostic window has been faded. In particular, for the first heartbeat cycle on the left side of the pressure waveform plot **1500**, the pressure data within the diagnostic window **1402** has been highlighted and the remaining pressure data for the first heartbeat cycle is shown in faded or other low contrast setting. Similarly, FIG. **16** shows a pressure waveform plot **1600** that corresponds to the same data as shown in pressure waveform plots **1212**, **1400**, and **1500** above, but where the pressure data for each heartbeat that is within the diagnostic window utilized for making the iFR calculations shown in window **1214** has

been highlighted and the pressure data for each heartbeat that is outside of the diagnostic window has been removed entirely. In particular, for the first heartbeat cycle on the left side of the pressure waveform plot **1600**, the pressure data within the diagnostic window **1402** has been highlighted and the remaining pressure data for the first heartbeat cycle has been removed. Accordingly, the pressure waveform plot **1600** only shows the pressure data within the diagnostic window **1402**. It is understood that the pressure data within the diagnostic window can be identified and/or accentuated in any suitable manner.

Persons skilled in the art will also recognize that the apparatus, systems, and methods described above can be modified in various ways. Accordingly, persons of ordinary skill in the art will appreciate that the embodiments encompassed by the present disclosure are not limited to the particular exemplary embodiments described above. In that regard, although illustrative embodiments have been shown and described, a wide range of modification, change, and substitution is contemplated in the foregoing disclosure. It is understood that such variations may be made to the foregoing without departing from the scope of the present disclosure. Accordingly, it is appropriate that the appended claims be construed broadly and in a manner consistent with the present disclosure.

What is claimed is:

1. A method of evaluating a vessel of a patient, comprising:
 - obtaining pressure measurements from a first instrument and a second instrument positioned within the vessel of the patient while the second instrument is moved longitudinally through the vessel from a distal position in the vessel to a proximal position in the vessel and the first instrument remains stationary within the vessel;
 - outputting, to a touch-sensitive display of a bedside controller, a screen display including:
 - a visual representation of a first pressure ratio of the pressure measurements;
 - a first proximal pressure waveform, a first distal pressure waveform, a second proximal pressure waveform, and a second distal pressure waveform, wherein the first proximal pressure waveform, the first distal pressure waveform, the second proximal pressure waveform, and the second distal pressure waveform are representative of the obtained pressure measurements, and wherein the second proximal and distal pressure waveforms illustrate the pressure measurements obtained over a greater amount of time compared to the first proximal and distal pressure waveforms; and
 - an overlay positioned over a portion of the second proximal and distal pressure waveforms, the overlay identifying a first portion of the obtained pressure measurements represented in the first proximal and distal pressure waveforms;
 - receiving, through the touch-sensitive display of the bedside controller, a user touch input modifying the overlay to identify a second portion of the pressure measurements; and
 - modifying the screen display, in response to the user touch input, to illustrate the second portion of the pressure measurements in the first proximal and distal pressure waveforms.
2. The method of claim 1,
 - wherein modifying the overlay comprises moving the overlay to be positioned over a different portion of the second proximal and distal pressure waveforms, and

wherein modifying the screen display comprises modifying the screen display, in response to the user touch input, such that the first proximal and distal pressure waveforms include the obtained pressure measurements corresponding to the position of the overlay over the different portion of the second proximal and distal pressure waveforms.

3. The method of claim 1, wherein the screen display includes numerical values of the obtained pressure measurements.

4. The method of claim 1, wherein the visual representation of a first pressure ratio of the obtained pressure measurements includes a numerical value.

5. The method of claim 4, wherein the screen display includes a second pressure ratio of the obtained pressure measurements, wherein the second pressure ratio is calculated differently than the first pressure ratio.

6. The method of claim 1, wherein the screen display includes a visual representation of a difference in the pressure measurements.

7. A method of evaluating a vessel of a patient, comprising:

obtaining pressure measurements from a first instrument and a second instrument positioned within the vessel of the patient while the second instrument is moved longitudinally through the vessel from a distal position in the vessel to a proximal position in the vessel and the first instrument remains stationary within the vessel;

outputting, to a touch-sensitive display of a bedside controller, a screen display including:

a first proximal pressure waveform and a first distal pressure waveform, wherein the first proximal pressure waveform and the first distal pressure waveform are representative of the obtained pressure measurements; and

a plurality of pressure ratios of the obtained pressure measurements, each of the plurality of pressure ratios separated by a fixed interval;

receiving, through the touch-sensitive display of the bedside controller, a user touch input; and

modifying the screen display in response to the user touch input.

8. The method of claim 7, further comprising:

receiving, through the touch-sensitive display of the bedside controller, a further user touch input identifying a time at which pressure measurements were obtained; and

modifying, in response to the further user touch input, the screen display to include a visual representation of the obtained pressure measurements corresponding to the identified time.

9. The method of claim 8, wherein the visual representation of the obtained pressure measurements corresponding to the identified time is displayed at a location proximate the at least a portion of the first pressure waveform defined by a point of initial contact with the touch-sensitive display.

10. The method of claim 9, wherein the visual representation of the obtained pressure measurements corresponding to the identified time includes a numerical value of the obtained pressure measurements at the identified time.

11. The method of claim 9, wherein visual representation of the obtained pressure measurements corresponding to the identified time includes a first pressure ratio of the obtained pressure measurements at the identified time.

12. The method of claim 11, wherein the visual representation of the obtained pressure measurements corresponding to the identified time includes a second pressure ratio of the

obtained pressure measurements at the identified time, wherein the second pressure ratio is calculated differently than the first pressure ratio.

13. The method of claim 9, wherein the visual representation of the obtained pressure measurements corresponding to the identified time includes a numerical value of the obtained pressure measurements at the identified time, a first pressure ratio of the obtained pressure measurements at the identified time, and a second pressure ratio of the obtained pressure measurements at the identified time, wherein the second pressure ratio is calculated differently than the first pressure ratio.

14. A system for evaluating a vessel of a patient, comprising:

a first instrument sized and shaped for introduction into the vessel of the patient;

a second instrument sized and shaped for introduction into the vessel of the patient, wherein the second instrument is configured to move longitudinally through the vessel from a distal position in the vessel to a proximal position in the vessel while the first instrument remains stationary within the vessel;

a bedside controller comprising a touch-sensitive display, the bedside controller being configured to display a screen display and to receive user touch inputs on the touch-sensitive display; and

a processing system communicatively coupled to the first and second instruments and the bedside controller, the processing system configured to:

receive pressure measurements from the first and second instruments;

output, to the touch-sensitive display of the bedside controller, the screen display including:

a first proximal pressure waveform and a first distal pressure waveform, wherein the first proximal pressure waveform and the first distal pressure waveform are representative of the obtained pressure measurements; and

a plurality of pressure ratios of the obtained pressure measurements, each of the plurality of pressure ratios separated by a fixed interval;

receive a signal from the bedside controller in response to a user touch input received at the touch-sensitive display; and

modify the screen display in response to the received signal.

15. The system of claim 14, wherein the processing system is configured to:

receive a further signal in response to a further user touch input identifying a time at which the pressure measurements were obtained; and

modify the screen display, in response to the received further signal, to include a visual representation of the obtained pressure measurements corresponding to the identified time.

16. The system of claim 15, wherein the visual representation of the obtained pressure measurements corresponding to the identified time includes a numerical value of the obtained pressure measurements at the identified time and a numerical value of a first pressure ratio of the obtained pressure measurements at the identified time.

17. The system of claim 16, wherein the visual representation of the obtained pressure measurements corresponding to the identified time further includes a numerical value of a second pressure ratio of the obtained pressure measurements at the identified time, wherein the second pressure ratio is calculated differently than the first pressure ratio.

33

18. A system for evaluating a vessel of a patient, comprising:

- a first instrument sized and shaped for introduction into the vessel of the patient;
- a second instrument sized and shaped for introduction into the vessel of the patient, wherein the second instrument is configured to move longitudinally through the vessel from a distal position in the vessel to a proximal position in the vessel while the first instrument remains stationary within the vessel;
- a bedside controller comprising a touch-sensitive display, the bedside controller being configured to display a screen display and to receive user touch inputs on the touch-sensitive display; and
- a processing system communicatively coupled to the first and second instruments and the bedside controller, the processing system configured to:
 - receive pressure measurements from the first and second instruments;
 - output, to the touch-sensitive display of the bedside controller, the screen display including:
 - a visual representation of a pressure ratio of the pressure measurements;
 - a first proximal pressure waveform, a first distal pressure waveform, a second proximal pressure waveform, and a second distal pressure waveform, wherein the first proximal pressure waveform, first distal pressure waveform, the second proximal pressure waveform, and the second distal pressure waveform are representative of the obtained pressure measurements, and wherein the second proximal and distal pressure waveforms illustrate the pressure measurements obtained over a greater amount of time compared to the first proximal and distal pressure waveforms; and

34

an overlay positioned over a portion of the second proximal and distal pressure waveforms, the overlay identifying a first portion of the pressure measurements represented in the first proximal and distal pressure waveforms;

receive a signal from the bedside controller in response to a user touch input received at the touch-sensitive display, the user touch input modifying the overlay to identify a second portion of the pressure measurements; and

modify the screen display, in response to the received signal, to illustrate the second portion of the pressure measurements in the first proximal and distal pressure waveforms.

19. The system of claim 18, wherein modifying the overlay comprises moving the overlay to be positioned over a different portion of the second proximal and distal pressure waveforms; and

wherein modifying the screen display comprising modifying the screen display, in response to the received signal, such that the first proximal and distal pressure waveforms include the obtained pressure measurements corresponding to the position of the overlay over the different portion of the second proximal and distal pressure waveforms.

20. The system of claim 18,

wherein the first proximal and distal pressure waveforms comprise a plot of measured pressure values and/or average pressure values, and

wherein the second proximal and distal pressure waveforms comprise a plot of measured pressure values and/or average pressure values.

* * * * *

专利名称(译)	用于评估船舶及相关设备，系统和方法的床旁控制器		
公开(公告)号	US10130310	公开(公告)日	2018-11-20
申请号	US14/850720	申请日	2015-09-10
[标]申请(专利权)人(译)	火山公司		
申请(专利权)人(译)	火山CORPORATION		
当前申请(专利权)人(译)	火山CORPORATION		
[标]发明人	ALPERT HOWARD DAVID ANDERSON DAVID COHEN ASHER MERRITT FERGUS LIM MENG		
发明人	ALPERT, HOWARD DAVID ANDERSON, DAVID COHEN, ASHER MERRITT, FERGUS LIM, MENG		
IPC分类号	A61B5/026 A61B5/02 A61B5/00 A61B5/0215		
CPC分类号	A61B5/7445 A61B5/026 A61B5/02007 A61B5/7475 A61B5/743 A61B5/7425 A61B5/02158		
优先权	62/049265 2014-09-11 US		
其他公开文献	US20160073972A1		
外部链接	Espacenet		

摘要(译)

提供了用于评估患者血管的装置，系统和方法。该方法包括向床边控制器的触敏显示器输出屏幕显示，该屏幕显示包括：通过位于容器内的第一和第二仪器获得的压力测量的第一压力比的视觉表示，同时第二仪器从a移动远端位置相对于狭窄的近端位置，第一个器械保持静止；第一近端压力波形和第一远端压力波形；通过床边控制器的触敏显示器接收第一近端压力波形上的用户触摸输入和/或识别获得压力测量值的时间的第一远端压力波形；响应于用户触摸输入，修改屏幕显示，以进一步包括对应于所识别的时间的所获得的压力测量的视觉表示。

