



US 20150157238A1

(19) **United States**
(12) **Patent Application Publication**
Edelman

(10) **Pub. No.: US 2015/0157238 A1**
(43) **Pub. Date: Jun. 11, 2015**

(54) **METHOD FOR NON-CONTRAST ENHANCED MAGNETIC RESONANCE ANGIOGRAPHY**

A61B 5/02 (2006.01)
A61B 5/0402 (2006.01)

(71) Applicant: **Robert Edelman**, Highland Park, IL (US)

(52) **U.S. Cl.**
CPC *A61B 5/055* (2013.01); *A61B 5/0402* (2013.01); *A61B 5/7292* (2013.01); *A61B 5/02007* (2013.01)

(72) Inventor: **Robert Edelman**, Highland Park, IL (US)

(21) Appl. No.: **14/621,347**

(57) **ABSTRACT**

(22) Filed: **Feb. 12, 2015**

Related U.S. Application Data


(63) Continuation of application No. 12/574,856, filed on Oct. 7, 2009.

(60) Provisional application No. 61/169,925, filed on Apr. 16, 2009.

Publication Classification

(51) **Int. Cl.**
A61B 5/055 (2006.01)
A61B 5/00 (2006.01)

A method for non-contrast enhanced magnetic resonance angiography (“MRA”) that has a short scan time and is insensitive to patient motion is provided. More particularly, the method provides significant arterial conspicuity and substantial venous signal suppression. A two-dimensional single shot acquisition is employed and timed to occur a specific time period after the occurrence of an R-wave in a contemporaneously recorded electrocardiogram. In this manner, k-space data is acquired that is substantially insensitive to variations in arterial flow velocity, or heart rate, and that further substantially suppresses unwanted venous signal in a prescribed imaging slice.

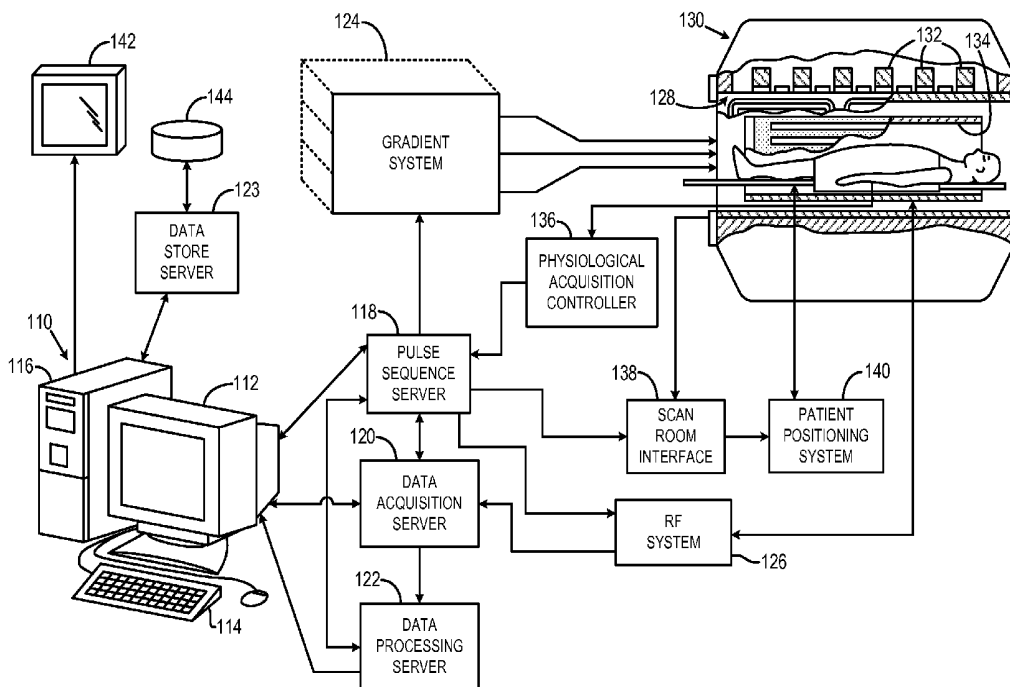

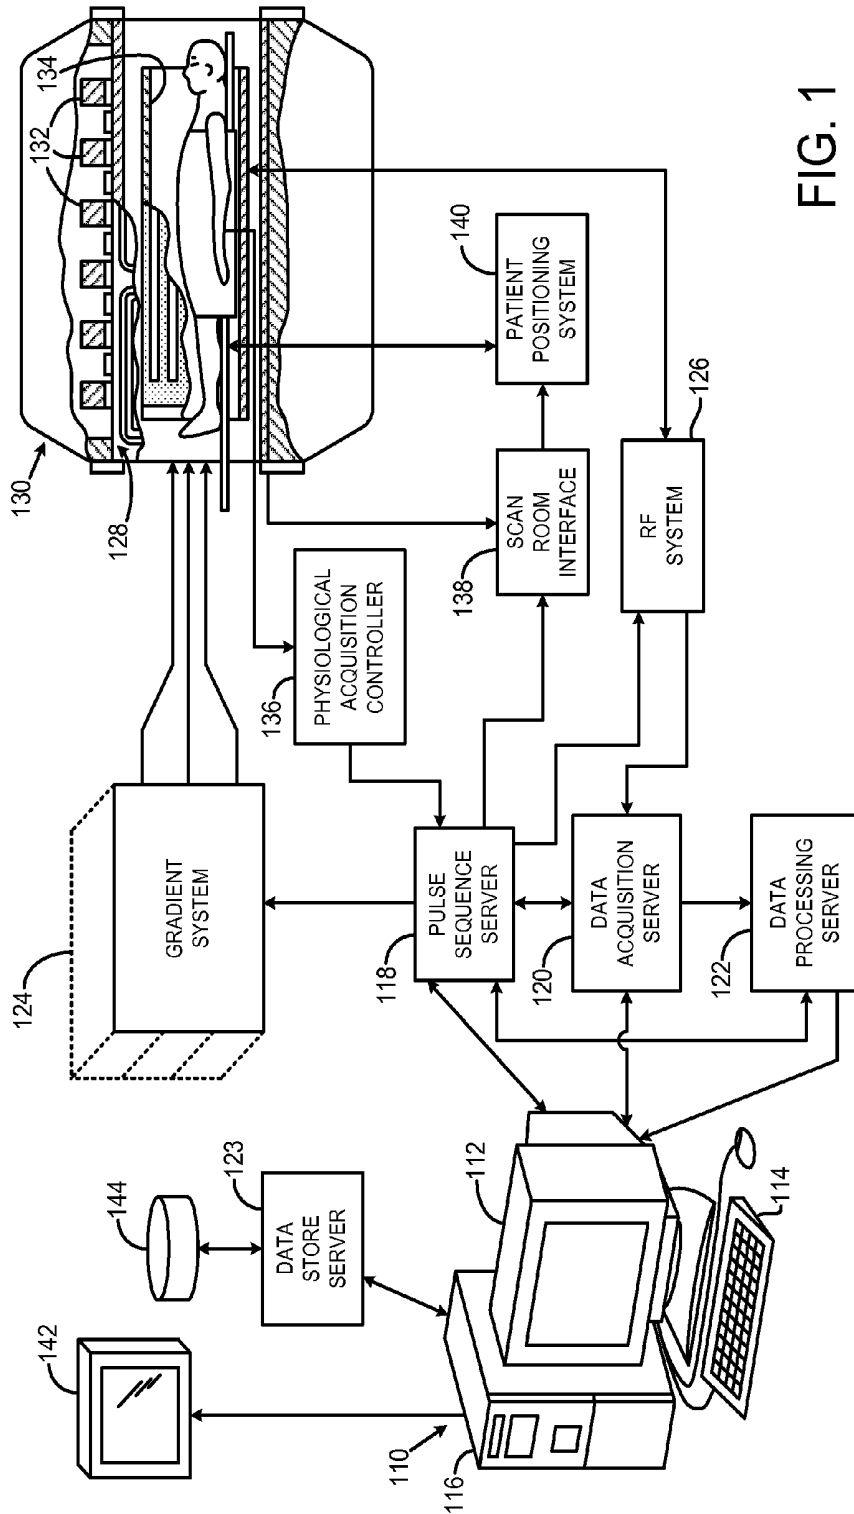


FIG. 1

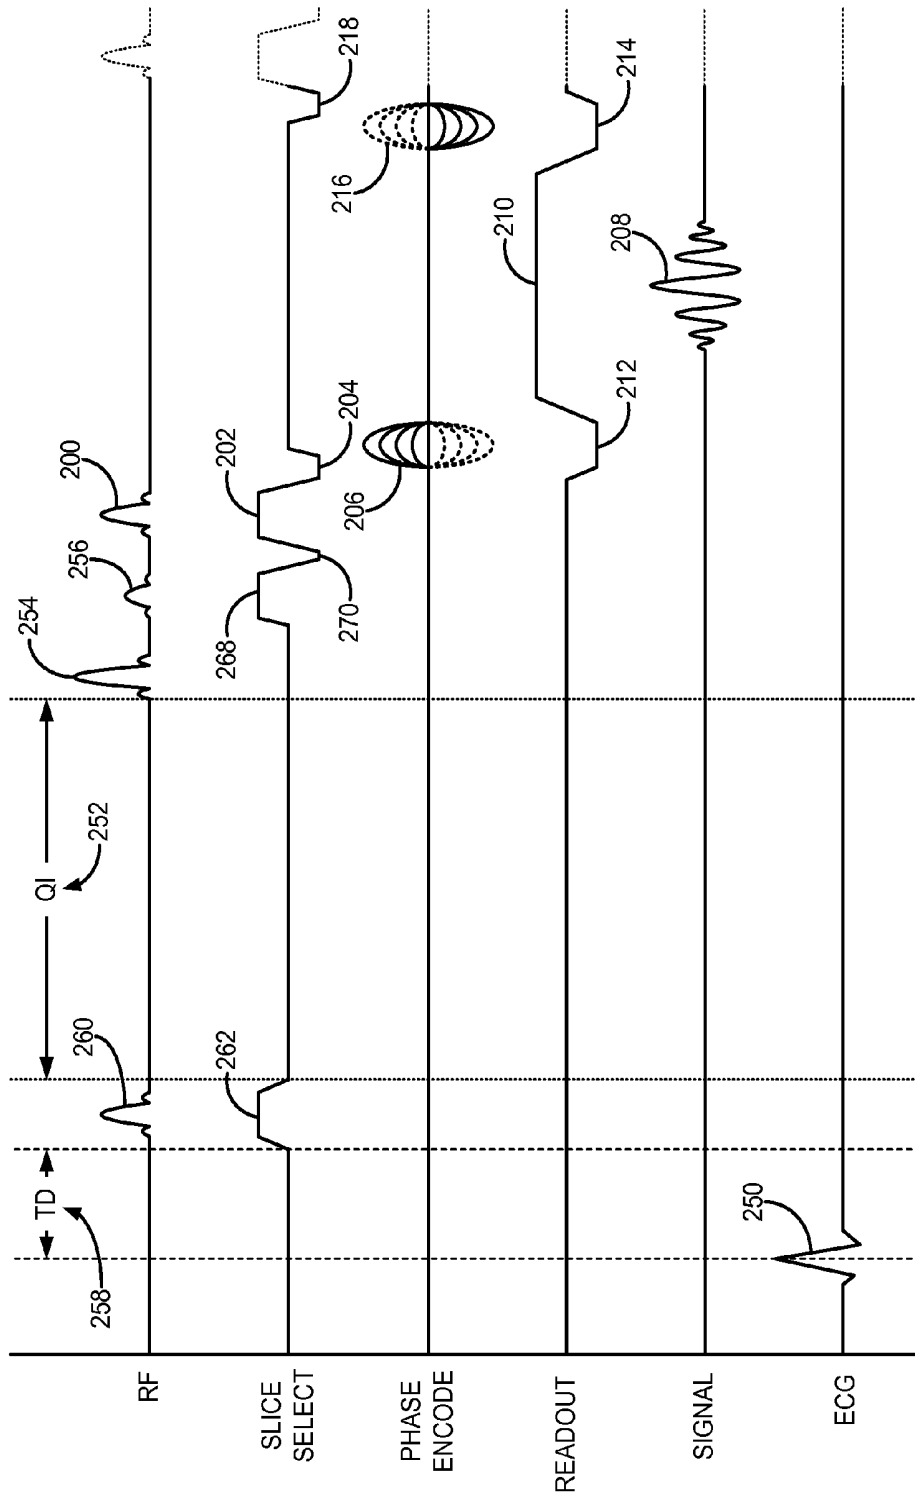


FIG. 2

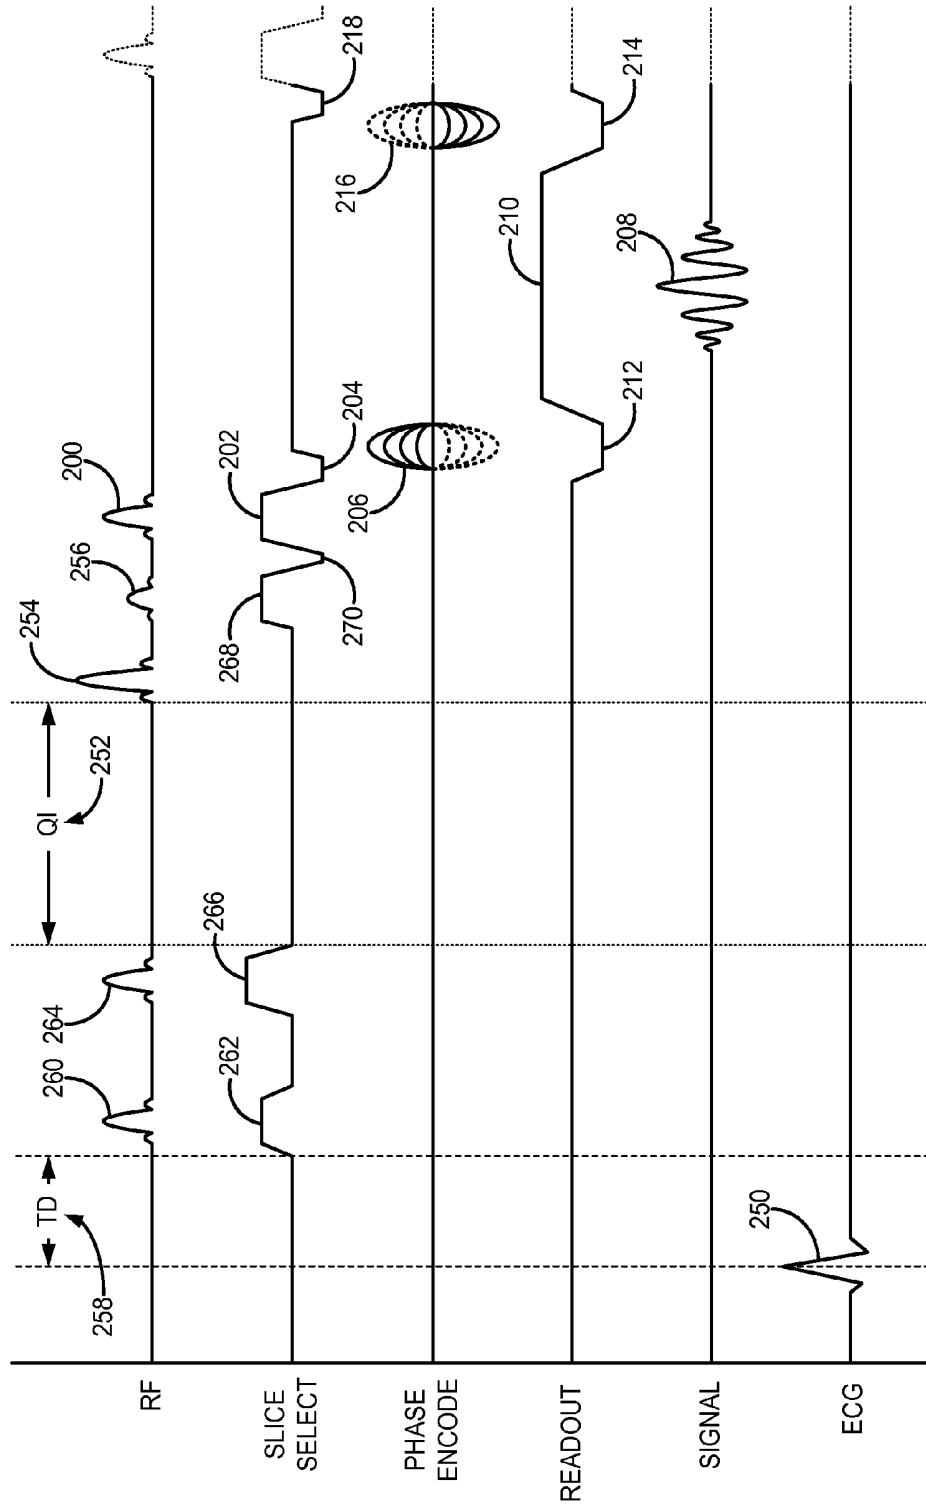


FIG. 3

METHOD FOR NON-CONTRAST ENHANCED MAGNETIC RESONANCE ANGIOGRAPHY

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. application Ser. No. 12/574,856, filed Oct. 10, 2009, and entitled “Method for Non-Contrast Enhanced Magnetic Resonance Angiography,” and claims the benefit of U.S. Provisional patent application Ser. No. 61/169,925 filed on Apr. 16, 2009, and entitled “Method for Non-Contrast Enhanced Magnetic Resonance Angiography.”

BACKGROUND OF THE INVENTION

[0002] The field of the invention is magnetic resonance imaging (“MRI”) and systems. More particularly, the invention relates to methods for non-contrast enhanced magnetic resonance angiography (“MRA”).

[0003] When a substance such as human tissue is subjected to a uniform magnetic field (polarizing field B_0), the individual magnetic moments of the nuclei in the tissue attempt to align with this polarizing field, but precess about it in random order at their characteristic Larmor frequency. If the substance, or tissue, is subjected to a magnetic field (excitation field B_1) that is in the x-y plane and that is near the Larmor frequency, the net aligned moment, M_z , may be rotated, or “tipped”, into the x-y plane to produce a net transverse magnetic moment M_{xy} . A signal is emitted by the excited nuclei or “spins”, after the excitation signal B_1 is terminated, and this signal may be received and processed to form an image.

[0004] When utilizing these “MR” signals to produce images, magnetic field gradients (G_x , G_y , and G_z) are employed. Typically, the region to be imaged is scanned by a sequence of measurement cycles in which these gradients vary according to the particular localization method being used. The resulting set of received MR signals are digitized and processed to reconstruct the image using one of many well known reconstruction techniques.

[0005] The measurement cycle used to acquire each MR signal is performed under the direction of a pulse sequence produced by a pulse sequencer. Clinically available MRI systems store a library of such pulse sequences that can be prescribed to meet the needs of many different clinical applications. Research MRI systems include a library of clinically proven pulse sequences and they also enable the development of new pulse sequences.

[0006] Magnetic resonance angiography (“MRA”) uses the magnetic resonance phenomenon to produce images of the human vasculature. To enhance the diagnostic capability of MRA, a contrast agent such as gadolinium can be injected into the patient prior to the MRA scan. The trick with this contrast enhanced (“CE”) MRA method is to acquire the central k-space views at the moment the bolus of contrast agent is flowing through the vasculature of interest. Collection of the central lines of k-space during peak arterial enhancement, therefore, is key to the success of a CE-MRA exam. If the central lines of k-space are acquired prior to the arrival of contrast, severe image artifacts can limit the diagnostic information in the image. Alternatively, arterial images acquired after the passage of the peak arterial contrast are sometimes obscured by the enhancement of veins. In many

anatomic regions, such as the carotid or renal arteries, the separation between arterial and venous enhancement can be as short as 6 seconds.

[0007] The short separation time between arterial and venous enhancement dictates the use of acquisition sequences of either low spatial resolution or very short repetition times (“TR”). Short TR acquisition sequences severely limit the signal-to-noise ratio (“SNR”) of the acquired images relative to those exams in which a longer TR is employed. The rapid acquisitions required by first pass CE-MRA methods thus impose an upper limit on either spatial or temporal resolution.

[0008] Recently, a rare and serious pathology involving fibrosis of skin, joints, eyes, and internal organs referred to as nephrogenic systemic fibrosis (“NSF”) has been correlated to the administration of gadolinium-based contrast agents to patients undergoing contrast-enhanced MRA studies. The link between gadolinium-based contrast agents and NSF is described, for example, by P. Marckmann, et al., in “Nephrogenic Systemic Fibrosis: Suspected Causative Role of Gadodiamide Used for Contrast-Enhanced Magnetic Resonance Imaging,” *J. Am. Soc. Nephrol.*, 2006; 17 (9):2359-2362. As a result of the increased incidence of NSF, methods for MRA that do not rely on the administration of a contrast agent to the patient have become an important field of research. However, current methods for non-contrast angiography are limited in their utility because they are sensitive to patient motion, do not consistently or accurately portray vessel anatomy in patients with severe vascular disease, and require excessively long scan times.

[0009] While single shot acquisition methods such as two-dimensional (“2D”) balanced steady-state free precession (“bSSFP”) have the potential to reduce motion artifacts and shorten exam times, arterial conspicuity is inadequate due to high background signal. Moreover, bSSFP methods do not lend themselves to the creation of maximum intensity projection (“MIP”) angiograms. In one example, a saturation-recovery bSSFP pulse sequence employed for cardiac perfusion imaging following the administration of a paramagnetic contrast agent is described by W. G. Schreiber, et al., in “Dynamic Contrast-Enhanced Myocardial Perfusion Imaging Using Saturation-Prepared TrueFISP,” *JMRI*, 2002; 16:641-652. However, this pulse sequence applies a spatially non-selective saturation pulse that suppresses the signal from blood and, thus, cannot be employed for MRA. Additionally, Schreiber’s method does not provide a means for distinguishing arteries from veins.

[0010] It is, in fact, particularly challenging to suppress venous signal with a single shot acquisition since, unlike arterial blood, venous blood typically flows slowly or even, for periods of time, not at all. In addition, the venous flow pattern is largely unpredictable, sometimes varying with a patient’s respiration cycle, cardiac cycle, or both. Consequently, it is problematic to eliminate the signals from veins with single shot acquisitions, since venous blood flows only a short distance or not at all during the short scan time. Unfortunately, venous signals tend to overlap with arterial signals on projection images, thereby making it difficult or impossible to diagnose arterial disease using such methods for MRA. In addition, a robust single shot non-contrast MRA technique must provide an accurate depiction of arterial anatomy over a wide range of flow velocities, ranging from a few centimeters per second (“cm/sec”) to more than 100

cm/sec. Moreover, the arterial anatomy must be depicted with sufficient arterial conspicuity to allow creation of a projection angiogram.

[0011] Several approaches have been previously described to suppress venous signal on non-contrast MR angiograms as follows. One method for venous suppression has been accomplished using image subtraction. Techniques like fresh blood imaging ("FBI") involve the subtraction of two images with different arterial signals, but identical venous signals. In this manner, the venous, but not arterial, signals cancel with subtraction. Unlike the saturation-based methods, subtraction techniques eliminate the signals from both stationary and moving venous spins. However, image subtraction doubles scan time and greatly increases the sensitivity of the technique to patient motion. In addition, these methods require prior knowledge of flow velocities in order to maximize arterial conspicuity.

[0012] Another method for suppressing venous signals is to employ a T_2 -weighted magnetization preparation pulse, which diminishes signal in veins since venous blood has a reduced oxygen tension. However, this method is inconsistently effective since the level of venous oxygenation varies widely and unpredictably.

[0013] Yet another method is to repeatedly apply a saturation radio frequency ("RF") pulse just prior to the pulse sequence used for data acquisition, and to repeat this process multiple times at typical intervals of 20-200 milliseconds ("ms"). However, the use of a single shot acquisition with subsecond data acquisition time does not afford the time to repeatedly apply a saturation RF pulse. As a result, this approach is only applicable to multi-shot acquisition techniques where the data is acquired over tens of seconds to several minutes. Moreover, the repeated application of RF pulses causes marked suppression of arterial signal in tortuous vessels, thereby limiting the diagnostic accuracy of these methods.

[0014] A single shot acquisition method for MRA is described by R. Edelman, et al., in "Fast Time-of-Flight MR Angiography with Improved Background Suppression," *Radiology*, 1991; 179:867-870. This method requires the use of an inversion recovery preparation pulse and relies on arterial inflow during the data acquisition period to produce arterial contrast. In this respect, the inversion time ("TI") is selected solely to match the center lines of k-space to the "null" point for the longitudinal magnetization of background tissue, and is not selected in order to allow for the inflow of arterial blood into the imaging slice. In other words, the purpose of the TI is to reduce the signal intensity of background tissues.

[0015] This method suffers from several drawbacks. For example, the method acquires data over a lengthy time period on the order of one second, thereby encompassing both systole and diastole. With this lengthy time period required for data acquisition, it is not possible to synchronize TI to the period of rapid, systolic arterial flow, nor to the period of slow diastolic flow. Moreover, the TI employed by Edelman is too short (on the order of 75 ms) to allow for substantial arterial inflow. As a result, most of the arterial inflow occurs during the application of repeated RF pulses. As described above, the repeated application of RF pulses in this manner causes marked suppression of arterial signal in tortuous vessels, thereby limiting the diagnostic accuracy of such methods for

MRA. The method also does not allow for the effective suppression of venous or fat signals, which are both essential to accurately depict the arteries.

[0016] Other methods of non-contrast enhanced MRA are described, for example, by M. Katoh, et al., in "Free-Breathing Renal MR Angiography With Steady-State Free-Precession (SSFP) and Slab-Selective Spin Inversion: Initial Results," *Kidney International*, 2004; 66:1272-1278, and by Y. Yamashita, et al., in "Selective Visualization of Renal Artery Using SSFP with Time-Spatial Labeling Inversion Pulse: Non-Contrast Enhanced MRA for Patients with Renal Failure," *Proc. Intl. Soc. Mag. Reson. Med.* 13 (2005) p. 1715. The method described by Katoh utilizes a three-dimensional ("3D") acquisition with a pre-inversion of the 3D region, while Yamashita employs two inversion pulses (one spatially selective and the other spatially non-selective). Each of these methods uses inversion preparation pulses rather than saturation pulses and further requires the use of a 3D, rather than 2D, acquisition for MRA. Given the substantial thickness of the 3D imaging slab, inflowing unsaturated spins must travel a large distance (for example, up to several centimeters) to replace in-plane saturated ones. Consequently, there is poor depiction of slowly flowing arterial spins. In fact, the inversion time, TI, must be very long (on the order of 1 second) to provide adequate inflow of even moderately fast flowing arterial spins. The long TI spans both the systolic and diastolic phases of the cardiac cycle. Given the long TI, it is problematic to synchronize data acquisition to diastole. In addition, 3D acquisitions are too time-consuming to permit data acquisition within a single breath-holding period.

[0017] A 2D adaptation of Yamashita's "time-SLIP" acquisition is described by S. Yamada, et al., in "Visualization of Cerebrospinal Fluid Movement with Spin Labeling at MR Imaging: Preliminary Results in Normal and Pathophysiologic Conditions," *Radiology*, 2008; 249; 644-652. This method, however, is employed to image the flow of cerebrospinal fluid flow rather than for MRA applications. Additionally, it uses two inversion pulses, rather than saturation pulses, and has a very long TI (on the order of 2500 ms) that is incompatible with MRA studies.

[0018] It would therefore be desirable to provide a method for non-contrast enhanced MRA that produced images of a patient's vasculature in a relatively short duration of time while maintaining significant discrimination of the arteries and substantially suppressing venous signals. Moreover, it would be desirable to provide a method for non-contrast enhanced MRA that was insensitive to flow velocities and was relatively insensitive to patient motion and other imaging artifacts.

SUMMARY OF THE INVENTION

[0019] The present invention overcomes the aforementioned drawbacks by providing a method for non-contrast enhanced magnetic resonance angiography ("MRA") that has a short scan time and is insensitive to patient motion, while maintaining significant arterial conspicuity and substantial venous signal suppression. This is achieved by employing a two-dimensional ("2D") single shot acquisition.

[0020] It is an aspect of the invention to provide a method for non-contrast enhanced MRA that is substantially insensitive to variations in arterial flow velocity or heart rate and that further substantially suppresses unwanted venous signal in a prescribed 2D imaging slice. A method for accurately depicting normal and diseased arteries despite a wide range of flow

velocities is provided by synchronizing a quiescent interval (“QI”) to the period of rapid, systolic arterial blood flow so as to maximize flow-related enhancement into the imaging slice. Additionally, this method is provided by synchronizing data acquisition to occur during diastole when arterial blood is stationary or flowing relatively slowly into a prescribed imaging slice. If venous blood flow is flowing in a cranial direction and arterial blood flow in a caudal direction, as is the case for the peripheral arteries, this venous suppression can be further augmented by the application of saturation pulses prior to the QI. The saturation pulses are applied not only in the imaging slice, but also in a slab contiguous with and caudal to the imaging slice. Likewise, when venous blood is flowing in a caudal direction and arterial blood in the cranial direction, as is the case in the internal jugular vein and common carotid artery, respectively, the slab is selected to be contiguous with and cranial to the imaging slice. In this manner, saturated venous spins and unsaturated arterial spins will flow into the imaging slice over the duration of the QI. Such a method differs fundamentally from previously described methods for suppressing venous signal since, in prior methods, saturation pulses were applied directly before the radio frequency (“RF”) excitation, allowing negligible time for inflow of saturated venous spins into the imaging slice.

[0021] It is another aspect of the invention to provide a method for non-contrast enhanced MRA that can produce images in a relatively short duration of time. For example, the entire length of the peripheral arteries can be imaged in 8 minutes with high arterial conspicuity and marked suppression of venous signal. Since the method uses a single shot acquisition, no ghost artifacts occur and the method is highly resistant to motion artifact. Previously described MRA techniques, including fresh blood imaging and 2D time of flight, do not use a single shot acquisition and thus are prone to motion artifacts and longer scan times. Additionally, the shortened scan time required with the method of the present invention allows for a series of 2D images to be obtained within a single breath-hold.

[0022] The foregoing and other aspects and advantages of the invention will appear from the following description. In the description, reference is made to the accompanying drawings which form a part hereof, and in which there is shown by way of illustration a preferred embodiment of the invention. Such embodiment does not necessarily represent the full scope of the invention, however, and reference is made therefore to the claims and herein for interpreting the scope of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

[0023] FIG. 1 is a block diagram of an MRI system that employs the present invention;

[0024] FIG. 2 is a pictorial representation of a pulse sequence performed by the MRI system of FIG. 1 when practicing an embodiment the present invention; and

[0025] FIG. 3 is a pictorial representation of a pulse sequence performed by the MRI system of FIG. 1 when practicing another embodiment the present invention.

DETAILED DESCRIPTION OF THE INVENTION

[0026] Referring particularly to FIG. 1, the preferred embodiment of the invention is employed in an MRI system. The MRI system includes a workstation 110 having a display 112 and a keyboard 114. The workstation 110 includes a

processor 116 that is a commercially available programmable machine running a commercially available operating system. The workstation 110 provides the operator interface that enables scan prescriptions to be entered into the MRI system. The workstation 110 is coupled to four servers: a pulse sequence server 118; a data acquisition server 120; a data processing server 122, and a data store server 123. The workstation 110 and each server 118, 120, 122 and 123 are connected to communicate with each other.

[0027] The pulse sequence server 118 functions in response to instructions downloaded from the workstation 110 to operate a gradient system 124 and a radio frequency (“RF”) system 126. Gradient waveforms necessary to perform the prescribed scan are produced and applied to the gradient system 124 that excites gradient coils in an assembly 128 to produce the magnetic field gradients G_x , G_y , and G_z used for position encoding MR signals. The gradient coil assembly 128 forms part of a magnet assembly 130 that includes a polarizing magnet 132 and a whole-body RF coil 134.

[0028] RF excitation waveforms are applied to the RF coil 134 by the RF system 126 to perform the prescribed magnetic resonance pulse sequence. Responsive MR signals detected by the RF coil 134 or a separate local coil (not shown in FIG. 1) are received by the RF system 126, amplified, demodulated, filtered and digitized under direction of commands produced by the pulse sequence server 118. The RF system 126 includes an RF transmitter for producing a wide variety of RF pulses used in MR pulse sequences. The RF transmitter is responsive to the scan prescription and direction from the pulse sequence server 118 to produce RF pulses of the desired frequency, phase and pulse amplitude waveform. The generated RF pulses may be applied to the whole body RF coil 134 or to one or more local coils or coil arrays (not shown in FIG. 1).

[0029] The RF system 126 also includes one or more RF receiver channels. Each RF receiver channel includes an RF amplifier that amplifies the MR signal received by the coil to which it is connected and a detector that detects and digitizes the I and Q quadrature components of the received MR signal. The magnitude of the received MR signal may thus be determined at any sampled point by the square root of the sum of the squares of the I and Q components:

$$M = \sqrt{I^2 + Q^2},$$

[0030] and the phase of the received MR signal may also be determined:

$$\phi = \tan^{-1}\left(\frac{Q}{I}\right).$$

[0031] The pulse sequence server 118 also optionally receives patient data from a physiological acquisition controller 136. The controller 136 receives signals from a number of different sensors connected to the patient, such as ECG signals from electrodes or respiratory signals from a bellows. Such signals are typically used by the pulse sequence server 118 to synchronize, or “gate”, the performance of the scan with the subject’s respiration or heart beat.

[0032] The pulse sequence server 118 also connects to a scan room interface circuit 138 that receives signals from various sensors associated with the condition of the patient and the magnet system. It is also through the scan room

interface circuit **138** that a patient positioning system **140** receives commands to move the patient to desired positions during the scan.

[0033] The digitized MR signal samples produced by the RF system **126** are received by the data acquisition server **120**. The data acquisition server **120** operates in response to instructions downloaded from the workstation **110** to receive the real-time MR data and provide buffer storage such that no data is lost by data overrun. In some scans the data acquisition server **120** does little more than pass the acquired MR data to the data processor server **122**. However, in scans that require information derived from acquired MR data to control the further performance of the scan, the data acquisition server **120** is programmed to produce such information and convey it to the pulse sequence server **118**. For example, during prescans MR data is acquired and used to calibrate the pulse sequence performed by the pulse sequence server **118**. Also, navigator signals may be acquired during a scan and used to adjust RF or gradient system operating parameters or to control the view order in which k-space is sampled. And, the data acquisition server **120** may be employed to process MR signals used to detect the arrival of contrast agent in a magnetic resonance angiography (MRA) scan. In all these examples the data acquisition server **120** acquires MR data and processes it in real-time to produce information that is used to control the scan.

[0034] The data processing server **122** receives MR data from the data acquisition server **120** and processes it in accordance with instructions downloaded from the workstation **110**. Such processing may include, for example: Fourier transformation of raw k-space MR data to produce two or three-dimensional images; the application of filters to a reconstructed image; the performance of a backprojection image reconstruction of acquired MR data; the calculation of functional MR images; the calculation of motion or flow images, etc.

[0035] Images reconstructed by the data processing server **122** are conveyed back to the workstation **110** where they are stored. Real-time images are stored in a data base memory cache (not shown) from which they may be output to operator display **112** or a display **142** that is located near the magnet assembly **130** for use by attending physicians. Batch mode images or selected real time images are stored in a host database on disc storage **144**. When such images have been reconstructed and transferred to storage, the data processing server **122** notifies the data store server **123** on the workstation **110**. The workstation **110** may be used by an operator to archive the images, produce films, or send the images via a network to other facilities.

[0036] Referring now particularly to FIG. 2, a pulse sequence employed when practicing an embodiment of the present invention is pictorially shown. The pulse sequence is cardiac gated, such that the acquisition of k-space data is timed with respect to the flow of arterial blood. Specifically, the pulse sequence is timed to be played out with respect to the peak of the R-wave **250** in a concurrently acquired echocardiogram ("ECG"). It should be appreciated by those skilled in the art, however, that other methods for cardiac synchronization of the following pulse than relying on an ECG signal are possible. For example, cardiac synchronization can be achieved using self-gating techniques that rely on measurement of flow signal or phase. Turning now to the pulse sequence, a slice-selective RF saturation pulse **260** is first played out in the presence of a slice-selective gradient

262 The application of this slice-selective RF saturation pulse **260** has the effect of suppressing the signals from background tissues as well as those venous spins that are present in the prescribed slice. The flip angle for this slice-selective RF saturation pulse **260** is typically about 90 degrees; however, larger or smaller flip angles may be desirable in some circumstances. The slice-selective RF saturation pulse **260** is timed to occur at a preset time delay ("TD") after the occurrence of the R-wave **250**. For example, TD is set to 100 ms.

[0037] The duration of time that is allowed to pass after the application of the slice-selective RF saturation pulse **260** is herein referred to as the "quiescent interval" ("QI"). This duration of time is specifically tailored to coincide with the rapid inflow of arterial blood into a prescribed imaging slice, and so that the zero line of k-space is acquired during the slow, diastolic inflow of arterial blood into the imaging slice. More particularly, a central portion of k-space is sampled during the slow, diastolic inflow of arterial blood into the imaging slice before the peripheral regions of k-space are sampled. The result of this is a substantial suppression of flow-based image artifacts. Put another way, this provides a method that is substantially insensitive to flow velocities in the prescribed image slice. Moreover, the QI allows for a maximal inflow of unsaturated arterial spins into the imaging slice, such that an improved discrimination of arterial spins is provided in the resultant images. This is even so when the patient's vasculature is significantly impacted by vascular diseases such as peripheral vascular disease ("PVD"). Exemplary values of QI in this configuration of the pulse sequence are on the order of 260 ms.

[0038] After the QI has passed, the pulse sequence proceeds with data acquisition, which is accomplished, for example, with a single shot balanced steady-state free precession (SSFP) gradient echo pulse sequence. First, a spectrally selective fat saturation RF pulse **254** is applied to further suppress unwanted MR signals originating from fat tissue. This is subsequently followed by a slice-selective $\alpha/2$ magnetization RF pulse **256** that is played out in the presence of a slice-selective gradient **268**, where α is a user selected flip angle. The slice-selective gradient includes a rephasing lobe **270** that acts to mitigate unwanted phase accruals that occur during the application of the slice-selective gradient **268**. This portion of the pulse sequence includes a slice-selective RF excitation pulse **200** that is played out in the presence of a slice-selective gradient pulse **202** to produce transverse magnetization in a prescribed slice. The slice-selective gradient includes a rephasing lobe **204** that acts to mitigate unwanted phase accruals that occur during the application of the slice-selective gradient **202**. After excitation of the spins in the slice, a phase encoding gradient pulse **206** is applied to position encode the MR signal **208** along one direction in the slice. A readout gradient pulse **210** is also applied after a dephasing gradient lobe **212** to position encode the MR signal **206** along a second, orthogonal direction in the slice. Like the slice-selective gradient **202**, the readout gradient **210** also includes a rephasing lobe **214** that acts to mitigate unwanted phase accruals.

[0039] To maintain the steady state condition, the integrals along the three gradients each sum to zero during the repetition time ("TR") period. To accomplish this, a rewinder gradient lobe **216** that is equal in amplitude, but opposite in polarity of the phase encoding gradient **206**, is played out along the phase encoding gradient axis. Likewise, a dephasing lobe **218** is added to the slice select gradient axis, such that

the dephasing lobe **218** precedes the repetition of the slice-selective gradient **202** in the next TR period. As is well known in the art, the reading out of MR signals following the single shot of the RF excitation pulse **200** is repeated and the amplitude of the phase encoding gradient **206** and its equal, but opposite rewinder **216** are stepped through a set of values to sample 2D k-space in a prescribed manner. It should be appreciated by those skilled in the art that any number of data acquisition schemes can be employed to acquire k-space data instead of balanced SSFP. For example, spoiled gradient echo, spiral acquisition, or echo planar imaging (“EPI”) pulse sequences can alternatively be utilized.

[0040] Referring now particularly to FIG. 3, another configuration of the pulse sequence employed when practicing the present invention is pictorially shown. This pulse sequence is also cardiac gated, such that the acquisition of k-space data is timed with respect to the flow of arterial blood. Specifically, the pulse sequence is timed to be played out with respect to the peak of the R-wave **250** in a concurrently acquired echocardiogram (“ECG”). However, the data acquisition portion of the pulse sequence is preceded by the application of two RF saturation pulses. By employing RF saturation pulses instead of inversion recovery pulses, the longitudinal magnetization is always reset to zero prior to the beginning of the QI. This is not necessarily the case when employing inversion recovery-based methods, as residual longitudinal magnetization resulting from inadequate inversion may confound the subsequently detected MR signals. Moreover, by always resetting the longitudinal magnetization of the slice to zero, the use of a slice-selective RF saturation pulse ensures that the tissue signal remains substantially uniform across different slices despite variations in the R-R interval due to cardiac arrhythmias. This is not the case with inversion-recovery based methods.

[0041] First, a slice-selective RF saturation pulse **260** is played out in the presence of a slice-selective gradient **262**. The application of this slice-selective RF saturation pulse **260** has the effect of suppressing the signals from background tissues as well as those venous spins that are present in the prescribed slice. The slice-selective RF saturation pulse **260** is timed to occur at a preset time delay (“TD”) after the occurrence of the R-wave **250**. For example, TD is set to 100 ms.

[0042] To suppress signals from venous spins that will flow into the prescribed slice, a second, slab-selective RF saturation pulse **264** is played out in the presence of a slab-selective gradient **266**. The slab-selective RF saturation pulse **264** has the effect of suppressing venous signals in a slab that is contiguous with the prescribed imaging slice. Specifically, when imaging the peripheral arteries, the prescribed slab is chosen to be caudal to, and contiguous with, the prescribed imaging slice such that saturated venous blood flows into the imaging slice in the caudal-cranial direction while unsaturated arterial spins flow into the imaging slice in the cranial-caudal direction. Similarly, when imaging, for example, the carotid artery, the prescribed slab is chosen to be cranial to, and contiguous with, the prescribed imaging slice such that saturated venous blood flows into the imaging slice in the cranial-caudal direction while unsaturated arterial spins flow into the imaging slice in the caudal-cranial direction. Exemplary RF excitation slab thicknesses are on the order of 150 mm; however, it will be appreciated by those skilled in the art that other thicknesses can be selected depending on the intended application and subject at hand. It will also be appre-

ciated that in some circumstances it may be desirable to shift the RF excitation slab so that it is not contiguous with the imaging slice.

[0043] In this alternate configuration of the pulse sequence, the QI is defined as the duration of time occurring after the application of the slab-selective RF saturation pulse **264** and before the fat saturation pulse **254**. Like the previously described QI, however, this duration of time is specifically tailored so that the zero line of k-space is acquired during the slow, diastolic inflow of arterial blood into the prescribed imaging slice. As described above, the result of allowing the QI to pass before data acquisition is a substantial suppression of flow-based image artifacts. Put another way, this provides a method that is substantially insensitive to flow velocities in the prescribed image slice. Exemplary values of QI in this configuration of the pulse sequence are on the order of 250 ms. The proceeding data acquisition is played out similar to the above-described pulse sequence, which is so described with respect to FIG. 2.

[0044] Unlike previous methods that rely on multi-shot acquisitions, the repetition time of the pulse sequences employed when practicing the present invention are significantly shorter than, say, the 30 ms typically required of such multi-shot sequences. In this manner, the overall scan time is less than the several seconds required of previous methods. This allows the method of the present invention to acquire the desired image data without becoming significantly sensitive to subject motion. Additionally, the shortened data acquisition period provided by the present invention allows image data to be acquired during only a portion of arterial flow, such that variations in flow velocity during the cardiac cycle do not confound the acquired MR signals.

[0045] The present invention has been described in terms of one or more preferred embodiments, and it should be appreciated that many equivalents, alternatives, variations, and modifications, aside from those expressly stated, are possible and within the scope of the invention. For example, it should be appreciated by those skilled in the art that a plurality of different saturation pulses may be employed prior to the beginning of the QI, with an appropriate change in QI. For example, as more saturation pulses are added, QI may decrease down to about 100 ms. Additionally, the specific order of the RF saturation pulses can be altered, such that a slab-selective saturation pulse is applied prior to a slice-selective saturation pulse, without significantly changing the resultant image contrast.

1. A method for non-contrast-enhanced magnetic resonance angiography for imaging vasculature of a subject with the steps comprising:

- a) directing a magnetic resonance imaging (MRI) system to perform a pulse sequence timed using an acquired cardiac signal, the pulse sequence comprising:
 - i) a first radio frequency (RF) saturation pulse applied at a time point determined based on the acquired cardiac signal to an imaging slice, such that MR signals in the imaging slice are substantially suppressed;
 - ii) a second RF saturation pulse applied to a prescribed slab that is outside of the imaging slice, such that MR signals indicative of venous blood flowing into the imaging slice are substantially suppressed;
 - iii) a quiescent interval following application of the second RF saturation pulse sufficient to allow spins asso-

ciated with unsaturated arterial blood and spins associated with saturated venous blood to flow into the imaging slice;

- iv) a data acquisition, performed following an RF excitation after the quiescent interval, to acquire k-space data from the subject;
 - b) reconstructing, using the acquired k-space data, an image of the subject that is representative of the vasculature of a subject.
2. The method as recited in claim 1, wherein the acquired cardiac signal is an electrocardiogram.
3. The method as recited in claim 1 in which step a)iv) includes acquiring k-space data as a single shot in coordination with the application of a series of RF excitation pulses.
4. The method as recited in claim 3 in which step a)iv) includes acquiring k-space data from a central portion of k-space before acquiring k-space data from a peripheral portion of k-space.
5. The method as recited in claim 3 in which step a)iv) includes acquiring k-space data from a zero-line in k-space using zero phase-encoding before acquiring k-space data from the remainder of k-space.
6. The method as recited in claim 1, the method further comprising repeating step a) to acquire another k-space data.
7. The method as recited in claim 6 in which the another k-space data is acquired for a different imaging slice during the quiescent interval.
8. The method as recited in claim 6 in which step b) includes using the another k-space data to reconstruct the image.
9. The method as recited in claim 1 in which the quiescent interval substantially occurs during rapid systolic inflow of arterial blood into the imaging slice.
10. The method as recited in claim 1 in which the pulse sequence further comprises waiting for a period of time before performing step a)i).

11. The method as recited in claim 10 in which the period of time and the quiescent interval are selected such that step a)iv) substantially occurs during slow diastolic inflow of arterial blood into the imaging slice.

12. The method as recited in claim 10 in which the period of time is between around 0 and 150 milliseconds.

13. The method as recited in claim 1 in which the quiescent interval is between around 100 and 400 milliseconds.

14. The method as recited in claim 1 in which the quiescent interval is selected such that step a)iv) substantially occurs during slow diastolic inflow of arterial blood into the imaging slice.

15. A method for non-contrast-enhanced magnetic resonance angiography for imaging vasculature of a subject with the steps comprising:

- a) directing a magnetic resonance imaging (MRI) system to perform a pulse sequence timed using an acquired cardiac signal, the pulse sequence comprising:
 - i) a radio frequency (RF) saturation pulse applied at a time point determined based on the acquired cardiac signal to an imaging slice, such that MR signals in the imaging slice are substantially suppressed;
 - ii) a quiescent interval following application of the RF saturation pulse sufficient to allow spins associated with unsaturated arterial blood to flow into the imaging slice;
 - iii) a data acquisition, performed following an RF excitation after the quiescent interval, to acquire k-space data from the subject;
- b) reconstructing, using the acquired k-space data, an image of the subject that is representative of the vasculature of a subject.

* * * * *

专利名称(译)	非对比增强磁共振血管造影的方法		
公开(公告)号	US20150157238A1	公开(公告)日	2015-06-11
申请号	US14/621347	申请日	2015-02-12
[标]申请(专利权)人(译)	爱德曼ROBERT		
申请(专利权)人(译)	埃德尔曼ROBERT		
当前申请(专利权)人(译)	GHOST医疗技术有限公司		
[标]发明人	EDELMAN ROBERT		
发明人	EDELMAN, ROBERT		
IPC分类号	A61B5/055 A61B5/00 A61B5/02 A61B5/0402		
CPC分类号	A61B5/055 A61B5/02007 A61B5/7292 A61B5/0402 A61B5/004 A61B5/7285 G01R33/5607 G01R33/5613 G01R33/5635 G01R33/56509 G01R33/5673		
优先权	61/169925 2009-04-16 US		
其他公开文献	US9380960		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于非对比增强磁共振血管造影 (“MRA”) 的方法，其具有短扫描时间并且对患者运动不敏感。更具体地，该方法提供显著的动脉显著性和显著的静脉信号抑制。采用二维单次发射采集并定时在同时记录的心电图中发生R波之后的特定时间段内发生。以这种方式，获取k空间数据，其对动脉血流速度或心率的变化基本上不敏感，并且进一步基本上抑制规定的成像切片中的不需要的静脉信号。

