



US 20160135701A1

(19) **United States**

(12) **Patent Application Publication**
DRAKE

(10) **Pub. No.: US 2016/0135701 A1**

(43) **Pub. Date: May 19, 2016**

(54) **SYSTEMS AND METHODS FOR
PERFORMING ELECTROCARDIOGRAMS**

A61B 5/00 (2006.01)

A61B 5/04 (2006.01)

(71) Applicant: **Stefan DRAKE**, Los Angeles, CA (US)

(52) **U.S. Cl.**

CPC *A61B 5/0404* (2013.01); *A61B 5/0006*
(2013.01); *A61B 5/0408* (2013.01); *A61B*
5/04012 (2013.01); *A61B 5/0432* (2013.01);
A61B 5/0428 (2013.01); *A61B 5/6824*
(2013.01); *A61B 5/6828* (2013.01); *A61B*
5/044 (2013.01); *A61B 5/7475* (2013.01)

(72) Inventor: **Stefan DRAKE**, Los Angeles, CA (US)

(21) Appl. No.: **14/941,556**

(22) Filed: **Nov. 14, 2015**

Related U.S. Application Data

(60) Provisional application No. 62/080,203, filed on Nov. 14, 2014.

Publication Classification

(51) **Int. Cl.**

A61B 5/0404 (2006.01)

A61B 5/0408 (2006.01)


A61B 5/044 (2006.01)

A61B 5/0432 (2006.01)

A61B 5/0428 (2006.01)

(57) **ABSTRACT**

A system for performing an electrocardiogram (ECG) can include a handheld electrocardiograph device having a right arm electrode, a left arm electrode, and a left leg electrode, and can be configured to receive signals from the electrodes and to send data based on the electrode signals to a mobile electronic device. The mobile electronic device can be configured to process and analyze the receive information to provide ECG data, such as 6-lead ECG data. The mobile electronic device can analyze the ECG data to provide diagnostic information. The mobile electronic device can transfer the ECG data to a remote computing system, which can analyze the ECG data to provide diagnostic information.

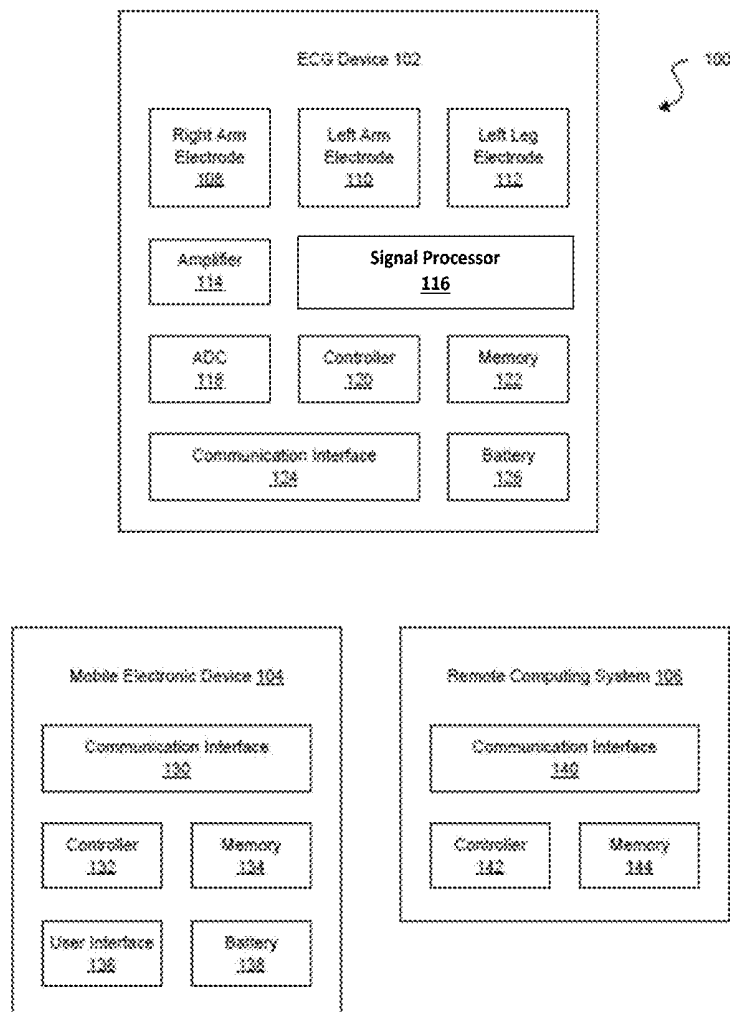

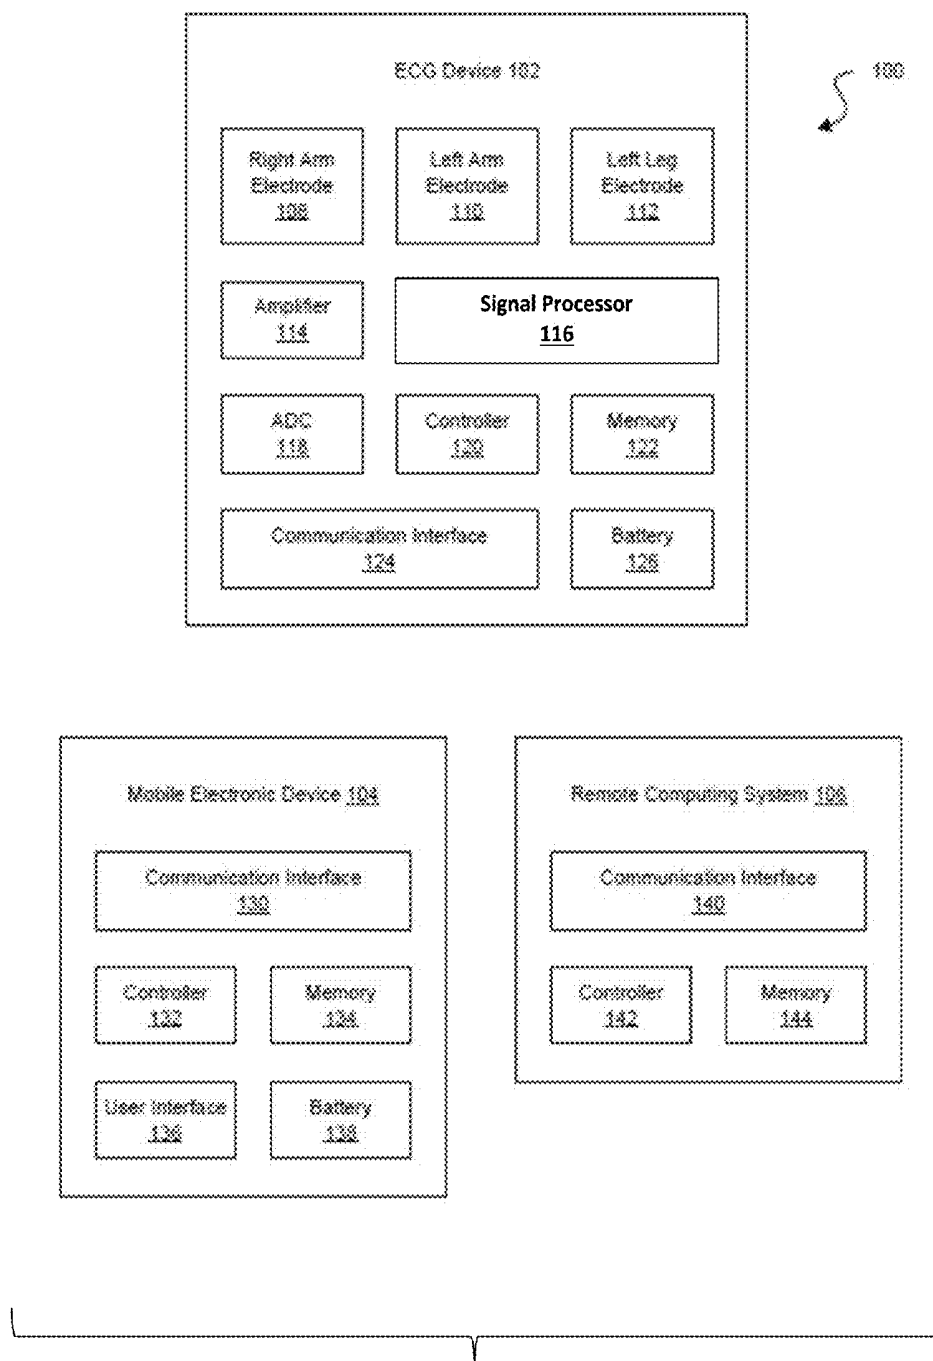


FIG. 1

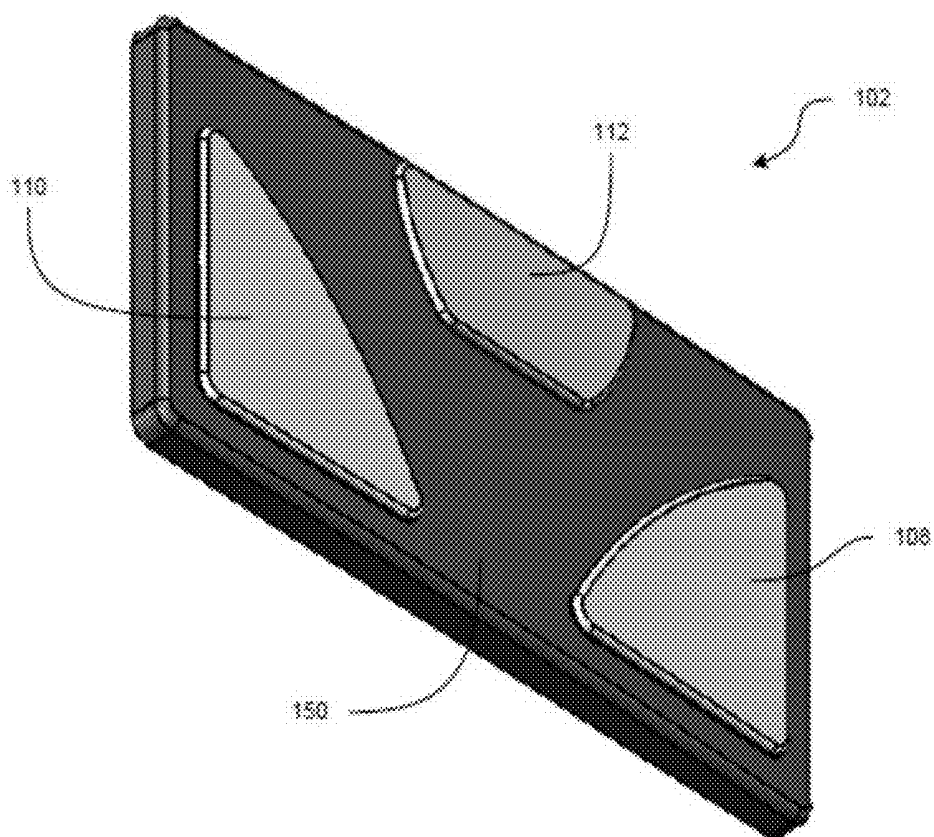


FIG. 2

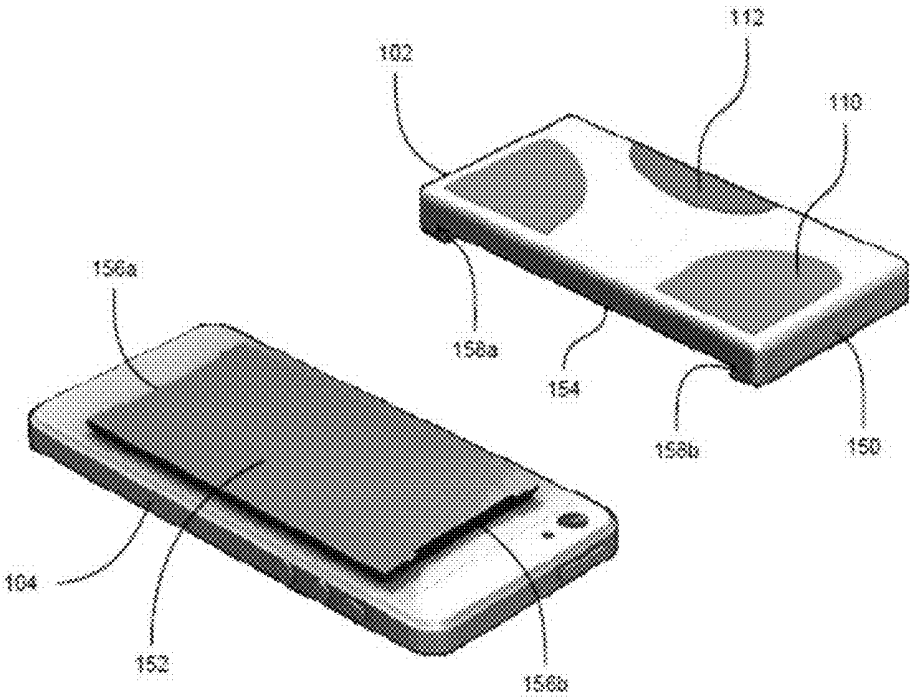


FIG. 3

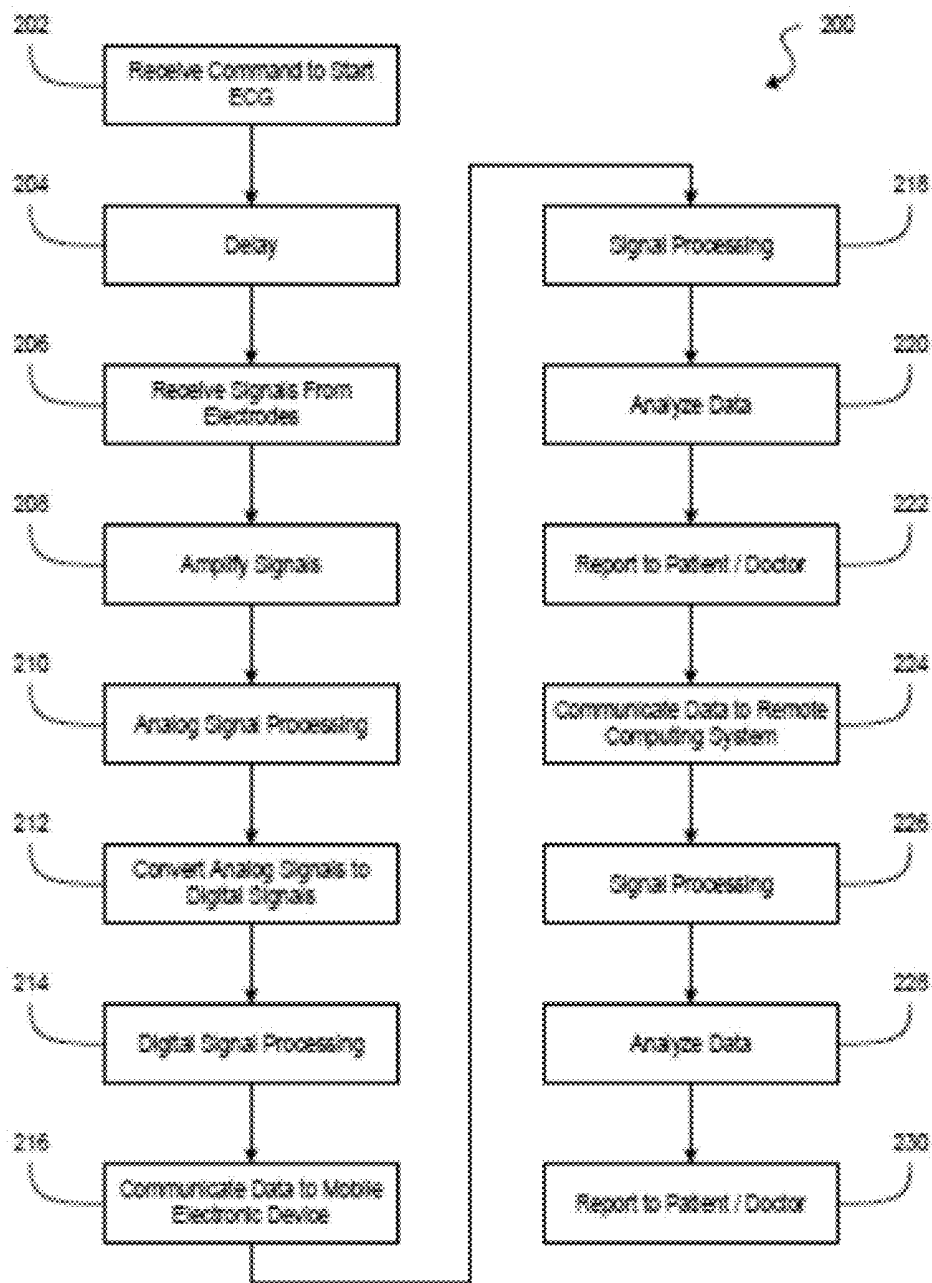


FIG. 4

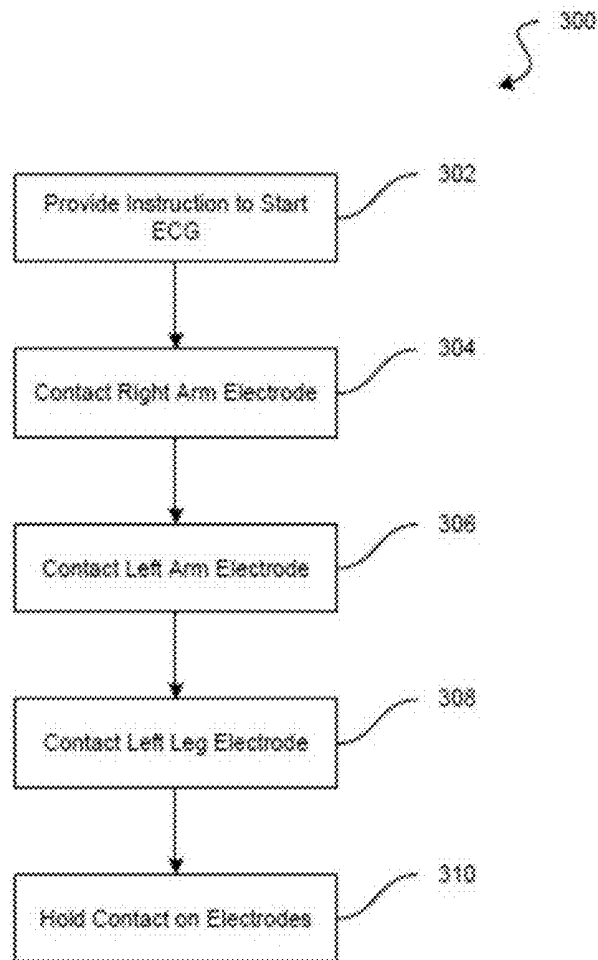


FIG. 5

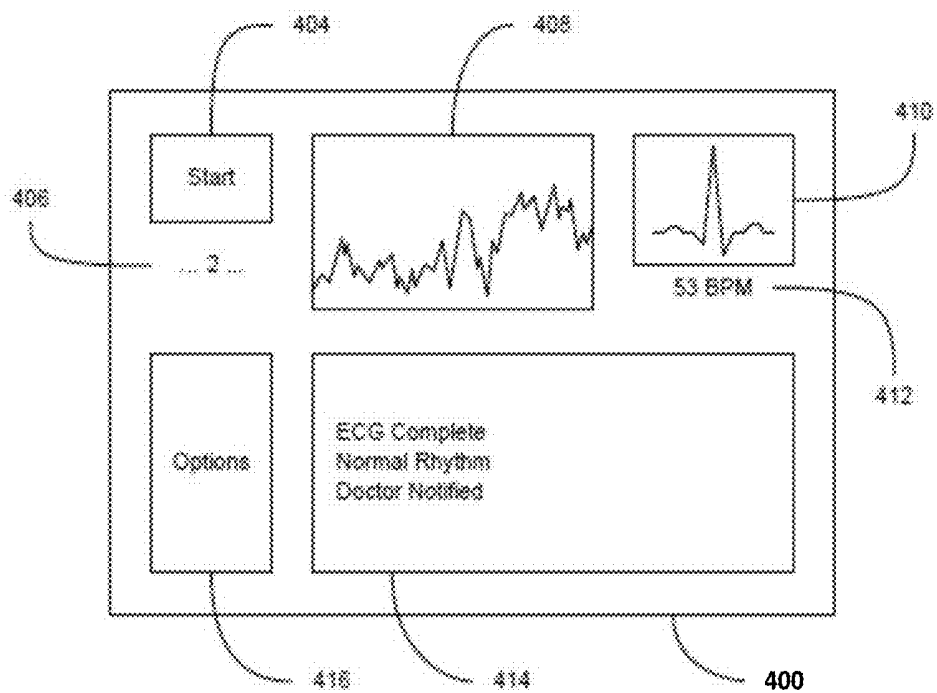


FIG. 6

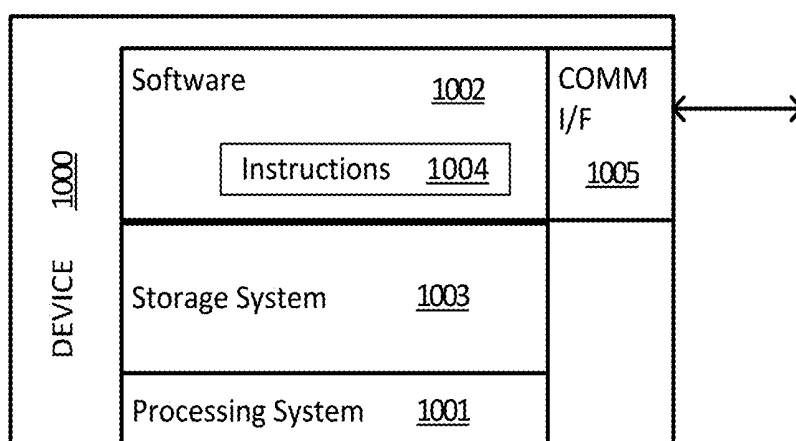


FIG. 7

SYSTEMS AND METHODS FOR PERFORMING ELECTROCARDIOGRAMS

CROSS-REFERENCE TO A RELATED APPLICATION

[0001] This application claims the priority benefit of U.S. Provisional Application Ser. No. 62/080,203, filed Nov. 14, 2014, which is incorporated herein by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] The electrocardiogram (ECG or EKG) is recognized as one of the most successful and important tools for rapid, noninvasive assessments of cardiac conditions. The resting 12-lead ECG (standard 12-lead ECG) recordings have been used to determine cardiac conditions in the presence of conflicting or ambiguous clinical symptoms. A 12-lead ECG can be obtained by attaching 10 electrodes to a patient: 4 limb lead electrodes are attached to limbs (left and right wrist, left and right ankle) and 6 precordial lead electrodes are attached to the torso. This configuration allows for recording leads I, II, Vi leads (where i=1 to 6), and calculating leads III, aVR, aVL and aVF. Electrocardiographs can be used to display/print ECG waveforms and for generating clinical statements based on diagnostic criteria derived from ECG measurements. Interpretation of an ECG is performed by electrocardiogram waveform analysis and can sometimes be performed by a serial comparison of a current ECG to a previously recorded ECG.

[0003] However, the resting 12-lead ECG obtained in the hospital or doctor's office can have limitations imposed by the recording environment. Everyday life, exercise, stress and a number of physiological conditions can elicit cardiac problems that can be masked or are not present during recordings on the human body at rest. Therefore, a stress test and ambulatory recordings can be used as additional sources of information on cardiac status. During a stress test, limb electrodes can be moved to the torso to reduce noise and artifacts caused by movement of long wires, muscle activity, and unstable electrode-skin interface.

[0004] Moreover, the acquisition of cardiac signals from a patient while in a non-hospital setting can be hampered by a variety of circumstances. To obtain high-quality ECG recordings, the electrode-skin interface needs to be stable, otherwise noise and artifacts can distort the recording of signals. Furthermore, in some situations, it is impractical to attach electrodes and wires to the body of a patient in motion. In ambulatory settings, it can be impractical to record with a large number of wires, so a small recorder can be used to record only a few ECG channels.

BRIEF SUMMARY OF THE INVENTION

[0005] Systems and techniques are disclosed for obtaining electrocardiogram recordings with a portable handheld device that enables obtaining 6-lead electrocardiogram data. Obtaining 6-lead electrocardiogram data requires a device capable of recording leads I and II simultaneously in standard ECG mode. Such recordings require connection of the device with a patient's left arm, right arm, and left leg, therefore various embodiments disclosed herein relate to electrocardiograph devices that can have three electrodes (e.g., three dry electrodes). To obtain recordings, left and right hand device electrodes can be held by left and right hands and the third electrode can be pressed against the left leg. The device's

third electrode can be pressed against the skin, for example, just above the knee or above the ankle.

[0006] In some embodiments, 3-electrode electrocardiograph devices can be coupled with mobile electronic devices that can provide 6-lead electrocardiogram data. In some cases, a mobile electronic device can display user interface elements configured to output information based on the 6-lead electrocardiogram data. In certain embodiments, a remote computing system may receive the 6-lead electrocardiogram data and provide diagnostic information.

[0007] This Summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This Summary is not intended to identify key features or essential features of the claimed subject matter, nor is it intended to be used to limit the scope of the claimed subject matter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008] FIG. 1 shows an example embodiment of a system for performing electrocardiogram (ECG or EKG) recordings.

[0009] FIG. 2 shows an example embodiment of a handheld electrocardiograph device.

[0010] FIG. 3 shows an example embodiment of a handheld electrocardiograph device that is removably attached to a mobile electronic device.

[0011] FIG. 4 shows a flow chart of an example method for performing electrocardiogram recordings.

[0012] FIG. 5 shows a flow chart of an example method of operating an electrocardiogram system.

[0013] FIG. 6 shows an example embodiment of a user interface for an electrocardiogram system.

[0014] FIG. 7 shows a block diagram illustrating components of a computing device or system used in some implementations of systems and techniques for performing an electrocardiogram.

DETAILED DESCRIPTION OF THE INVENTION

[0015] Various embodiments disclosed herein relate to a portable handheld electrocardiograph device with three dry electrodes allowing for recordings of left arm (LA), right arm (RA) and left leg (LL) signals, which can be used to obtain 6 ECG leads (I, II, III, aVR, aVF, and aVL), as discussed herein. Various embodiments relate to medical instrumentation and information systems. A handheld electrocardiographic device, as disclosed herein, can provide the ability to record limb leads and auxiliary limb leads (e.g., 6 leads total) from subjects in ambulatory settings, which can be comparable the 12 leads recorded using a standard 12-lead electrocardiograph in hospital settings.

[0016] Use of a presently available single-lead handheld ECG device in ambulatory settings has limited diagnostic value compared to 12-lead ECG recorders. It can provide basic heart monitoring and it can be useful for characterizing various arrhythmias. When a recording is made between the left and right hand, it represents lead I (I=LA-RA) and it is equivalent to only lead I of a standard 12-lead ECG.

[0017] A device capable of recording leads I and II simultaneously in standard ECG mode would increase diagnostic yield compared to using a single-lead device. As recordings of lead II (II=LL-RA) requires connection of the device to the left leg, various embodiments disclosed herein relate to ECG devices that can have three electrodes (e.g., three dry electrodes). To obtain recordings, device left and right hand elec-

trodes can be held by the subject's left and right hands and the third electrode can be pressed against the left leg. The device's third electrode can be pressed against the skin, for example, just above the knee or above the ankle.

[0018] ECG signals I and II obtained from electrodes can be amplified and digitized (e.g., by a microcontroller with an internal analog-to-digital converter. Data can then be transferred (e.g., via serial interface and Bluetooth module) to a mobile electronic device (e.g., a cellular phone) for initial display and storage. The mobile electronic device (e.g., a cellular phone) can perform initial processing and transmit data to a remote computing system (e.g., an ECG server or ECG cloud service) for interpretation, serial comparison, and analysis.

[0019] Various embodiments disclosed herein can relate to a handheld electrocardiographic device for simultaneous acquisition of six leads (limb leads and auxiliary limb leads). The device can include three dry electrodes for obtaining ECG signals I and II from a subject. Signals I and II can be obtained in the same manner as on a traditional 12-lead electrocardiograph. Leads III and auxiliary leads aVR, aVL, and aVF can be calculated (e.g., based on Leads I and II). To emphasize ambulatory use, the conventional wet electrodes (usually silver-silver chloride Ag/AgCl) and skin preparation that hospitals use are replaced with dry electrodes requiring no skin preparation.

[0020] Lead I is defined as LA-RA, and can be obtained by holding the device's left and right electrodes with both the left and right hands while the device is faced down. Lead II is defined as LL-RA. Lead II can be obtained by holding the device with both the left and right hands while simultaneously pressing the third electrode against the skin just above the subject's knee or ankle.

[0021] The electrodes can be connected to amplifiers. The input of the amplifiers can be designed to accept signals from the dry electrodes. The output of the amplifiers can be connected to an analog-to-digital converter (ADC). Digital data from the ADC can be connected to a microcontroller. Data from the microcontroller can be sent to a communication interface (e.g., a Bluetooth interface) for transmission to a mobile electronic device (e.g., a cellular phone). The mobile electronic device can be used for initial data evaluation and/or to transfer data to a remote computing system (e.g., an ECG server). The data on the remote computing system (e.g., ECG server) can be evaluated (e.g., by automatic algorithms) and the diagnosis/results can be sent to the end user or to a doctor or other medical professional.

[0022] FIG. 1 shows an example of a system 100 for performing electrocardiogram (ECG or EKG) recordings according to some embodiments. The system 100 can be configured to perform a 6-lead ECG. The system 100 can include an electrocardiograph (ECG) device 102 and a mobile electronic device 104, and in some embodiments the system 100 can include a remote computing system 106. The ECG device 102 can include three electrodes, such as a right arm electrode 108, a left arm electrode 110, and a left leg electrode 112. In some embodiments, the system 100 can use fewer electrodes than a traditional 12-lead ECG, which would use ten electrodes, which can facilitate performance of the ECG procedure, especially for ECG procedures performed by a patient himself or herself. The system 100 can be configured to perform an ECG procedure (e.g., a 6-lead ECG) without using a right leg electrode, a V1 electrode, a V2 electrode, a V3 electrode, a V4 electrode, a V5 electrode, or a V6 elec-

trode, which would ordinarily be used for a traditional 12-lead ECG. The system 100 can be configured to perform the ECG procedure using only the three electrodes 108, 110, and 112.

[0023] In some embodiments, the electrodes 108, 110, and 112 can be dry electrodes, which can be configured to be used by a patient without applying a gel between the electrodes and the skin and/or with little or no skin preparation (e.g., shaving, cleaning, sanding, etc.). In some embodiments, the use of dry electrodes can result in higher impedance, and the system 100 (e.g., with amplifier 114) can be configured to compensate for the higher impedance that can result from the use of dry electrodes instead of wet electrodes, which would generally be used for a traditional 12-lead ECG. In some embodiments, the electrodes 108, 110, and 112 can be made of stainless steel (e.g., low-carbon stainless steel such as 316L grade stainless steel). Various other conductive materials can be used for the electrodes 108, 110, and 112, such as gold, silver, copper, aluminum, metal alloys, and various other suitably conductive materials.

[0024] In some embodiments, one or more wet electrodes can be used, but the use of dry electrodes can facilitate the performance of quick ECG recording procedures, especially those performed by the patient using a mobile device without direct involvement of a medical professional.

[0025] The ECG device 102 can include one or more amplifiers 114 configured to amplify signals (e.g., analog signals) from the electrodes 108, 110, and 112. In some embodiments, each electrode 108, 110, and 112 has a corresponding amplifier 114 that is configured to amplify the signals from that electrode. In some embodiments, a single amplifier 114 can amplify the signals from two or all three of the electrodes 108, 110, and 112. The one or more amplifiers 114 can be configured to amplify the signals to compensate for impedance, which may be produced, e.g., by the use of dry electrodes.

[0026] The ECG device 102 can include a signal processor 116, which can be configured to perform one or more signal processing operations on the signals received from the right arm electrode 108, from the left arm electrode 110, and from the left leg electrode 112 (e.g., on the amplified analog signals output by the one or more amplifiers 114). In some cases, the signal processor 116 can be configured to perform analog signal processing operations. In some embodiments, the signal processor 116 can be configured to compare and calculate signals from the different electrodes 108, 110, and 112. For example, a first lead (Lead I) can be based at least in part on a voltage difference measured (e.g., by the signal processor 116) between the left arm electrode 110 and the right arm electrode 108, and a second lead (Lead II) can be based at least in part on a voltage difference measured (e.g., by the signal processor 116) between the left leg electrode 112 and the right arm electrode 108.

[0027] In some embodiments, the signal processor 116 can be configured to perform one or more signal processing operations to improve the signal-to-noise ratio for the signals. In some embodiments, the signal processor 116 can be configured to perform one or more signal processing operations to remove or reduce baseline wander. In some embodiments, the signal processor 116 can be configured to perform one or more signal processing operations to compensate for impedance (e.g., produced by the use of dry electrodes).

[0028] The ECG device 102 can include an analog-to-digital converter (ADC) 118, which can be configured to convert analog signals (e.g., received from the signal processor 116,

from the one or more amplifiers 114, or directly from the electrodes 108, 110, and 112) to digital signals.

[0029] The ECG device 102 can include a controller 120. The controller 120 can be a processor or processing system as described herein. In some embodiments, the ECG device 102 can include memory 122, which can store executable program instructions that can be executed by the controller 120 to implement various methods, operations, and features described herein. Memory 122 can be a type of computer readable storage media as described herein. In some embodiments, the controller 120 can store data to the memory 122. For example, data corresponding to the digital signals received over time can be stored on the memory 122 for use in signal processing operations that depend on previous signals. Results of signal processing and/or data analysis can be stored in the memory 122, and can be accessed by the controller 120 to be used for later calculations. In some embodiments, data received and/or generated (e.g., by the controller 120) can be stored on the memory 122 so that it can be periodically transmitted by the communication interface 124 (e.g., as packets of data).

[0030] In some embodiments, the controller 120 can be a digital controller and can be configured to receive digital signals (e.g., digital signals output by the ADC). The controller 120 can receive, for example, digital representations of the signals from the right arm electrode 108, the left arm electrode 110, and the left leg electrode 112, or of the amplified (from 114) and/or signal-processed (from 116) versions of the original analog signals from the electrodes 108, 110, and 112.

[0031] The controller 120 can receive separate signals corresponding to the three electrodes 108, 110, and 112, or the controller 120 can receive signals that represent information from different combinations of the electrodes 108, 110, and 112 (e.g., signals associated with the voltage differences between electrodes). For example, in some embodiments, the controller 120 can receive a digital signal representing a voltage difference between the left arm electrode 110 and the right arm electrode 108 and a digital signal representing a voltage difference between the left leg electrode 112 and the right arm electrode 108.

[0032] The controller 120 can perform one or more signal processing operations (e.g., digital signal processing on the digital signals received). The controller 120 can perform one or more digital signal processing operations to remove or reduce baseline wander, to improve the signal-to-noise ratio, to compensate for impedance (e.g., produced by the use of dry electrodes), etc. In some embodiments, the controller 120 can perform one or more linear phase filtering operations (e.g., recursive or non-recursive linear phase filtering).

[0033] The controller 120 can analyze the signals received by the controller 120. For example, the controller 120 can compare and analyze signals corresponding to the different electrodes 108, 110, and 112, for example, to determine a voltage difference between the left arm electrode 110 and the right arm electrode 108 (Lead I) and/or to determine a voltage difference between the left leg electrode 112 and the right arm electrode 108 (Lead II). In some embodiments, the controller 120 can determine the 6 leads for a 6-lead ECG, as discussed herein.

[0034] The ECG device 102 can include a communication interface 124, which can be configured to enable the ECG device 102 to communicate with other communication interfaces to coupled interpretive devices, e.g., the communication

interface 130 on the mobile electronic device 104, the communication interface 140 on the remote computing system 106, and/or other external systems for reporting results (e.g., a hospital information system, and a doctor email system). The controller 120 can send data to the communication interface 124 for transmission to coupled interpretive devices and/or external devices and systems. The communication interfaces 124, 130, and 140 described herein can be wireless communication interfaces as described with respect to device 1000 (FIG. 7). Communication interfaces 124, 130, and 140 can include, for example, Wi-Fi, Bluetooth, Bluetooth Low Energy (BLE), near field communication (NFC), 3G, and 4G. In some embodiments, the communication interface 124, 130, 140 can use a wire or cable or physical communication port to communicate data. For example, the ECG device 102 can include an electrical connector (e.g., a micro-USB connector or lightning connector) that is configured to engage a corresponding port on the mobile electronic device 104 (e.g., a micro-USB port or lightning port), or on another external device or system, to communicate information between the devices and/or systems. Other communication methods can be used as well. For example, the communication interfaces 124, 130, and 140 can be configured to transfer data via an audio input port or microphone.

[0035] The ECG device 102 can be a portable device, such as an accessory for use with the mobile electronic device 104. The ECG device 102 can include a battery 126, which can facilitate the portable nature of the ECG device 102. Other power sources can be used. For example, the ECG device 102 can receive electrical power from an external power source (e.g., a wall outlet), or a battery 138 of the mobile electronic device 104 can supply electrical power to the ECG device 102, for instance, when the ECG device 102 and the mobile electronic device 104 are coupled via a wire or cable (e.g., via a micro-USB or lightning connection) or passive charging system.

[0036] The mobile electronic device 104 can be a mobile phone (e.g., a smart phone), a tablet computer, a laptop computer, or other computing device. The mobile electronic device 104 can include a communication interface 130 as discussed. The communication interface 130 can be configured to send and/or receive information to and/or from the ECG device 102 (e.g., via a first communication protocol, which can have a relatively short range, such as Bluetooth, BLE, or NFC). The communication interface 130 can be configured to send and/or receive information to and/or from a remote computing system 106 (e.g., using a second communication protocol, which can have a relatively long range, such as Wi-Fi, 3G, 4G, TCP/IP over Ethernet, the Internet, etc.). In some embodiments, the mobile electronic device 104 can operate as a middleman to relay information between the ECG device 102 and the remote computing system 106 (or another external device or system).

[0037] The mobile electronic device 104 can include a controller 132. The controller 132 can be a processor or processing system as described herein. In some embodiments, the mobile electronic device 104 can include memory 134, which can store executable instructions that can be executed by the controller 132 to implement various methods, operations, and features described herein. In some embodiments, the controller 132 can store data to the memory 134. For example, data corresponding to the digital signals received over time can be stored on the memory 134 for use in signal processing operations that depend on previous signals. Results of signal pro-

cessing and/or data analysis can be stored in the memory 134, and can be accessed by the controller 132 to be used for later calculations. In some embodiments, data received and/or generated (e.g., by the controller 132) can be stored on the memory 134, such as for archiving, for later reference, or to be periodically transmitted by the communication interface 130 (e.g., as packets of data). Memory 134 can be a type of computer readable storage media as described herein.

[0038] In some embodiments, the controller 132 can run an application or program (which can be stored on memory 134), which can perform the ECG processing, as described herein. In some embodiments, an application or program can run remotely (e.g., on the remote computing system 106, using cloud computing, or as Software as a Service (SaaS)) to perform the ECG procedure.

[0039] The controller 132 can be configured to perform one or more signal processing operations (e.g., digital signal processing) on the data received from the ECG device 102. The controller 132 can perform one or more digital signal processing operations to remove or reduce baseline wander, to improve the signal-to-noise ratio, to compensate for impedance (e.g., produced by the use of dry electrodes), etc. In some embodiments, the controller 132 can perform one or more linear phase filtering operations (e.g., recursive or non-recursive linear phase filtering).

[0040] The controller 132 can analyze data (e.g., received from the ECG device 102). For example, the controller 132 can compare signals corresponding to the different electrodes 108, 110, and 112, for example, to determine a voltage difference between the left arm electrode 110 and the right arm electrode 108 (Lead I) and/or to determine a voltage difference between the left leg electrode 112 and the right arm electrode 108 (Lead II).

[0041] In some embodiments, the controller 132 can determine the 6 leads for a 6-lead ECG, as discussed herein. The controller 132 can provide a 6-lead ECG having three limb leads: Lead I, Lead II, and Lead III, and three augmented limb leads: augmented vector right (aVR), augmented vector left (aVL), and augmented vector foot (aVF). The 6 leads can be represented by the following equations:

$$\text{Lead I} = \text{LA} - \text{RA};$$

$$\text{Lead II} = \text{LL} - \text{RA};$$

$$\text{Lead III} = \text{LL} - \text{LA};$$

$$\text{Augmented vector right (aVR)} = \text{RA} - \frac{1}{2}(\text{LA} + \text{LL});$$

$$\text{Augmented vector left (aVL)} = \text{LA} - \frac{1}{2}(\text{RA} + \text{LL}); \text{ and}$$

$$\text{Augmented vector foot (aVF)} = \text{LL} - \frac{1}{2}(\text{RA} + \text{LA}).$$

[0042] In the equations above, LA can correspond to a voltage of the left arm electrode 110, RA can correspond to a voltage of the right arm electrode 108, and LL can correspond to a voltage of the left leg electrode 112. In some embodiments, the system 100 does not produce the precordial leads, which would normally be produced by a 12-lead ECG.

[0043] In some embodiments, Lead III, a VR, a VL, and a VF can be calculated based on Lead I and Lead II, as set forth in the following equations (wherein "I" corresponds to Lead I and "II" corresponds to Lead II):

$$\text{Lead III} = \text{II} - \text{I};$$

$$\text{aVR} = -(\text{I} + \text{II})/2;$$

$$\text{aVL} = \text{I} - \text{II}/2; \text{ and}$$

$$\text{aVF} = \text{II} - \text{I}/2.$$

[0044] In some embodiments, the controller 132 can perform analysis on the ECG data (e.g., the 6-lead ECG data) to determine a heart rate, to make a determination of normal heart rhythm, and/or to diagnose one or more disorders. In some embodiments, data, algorithms, and methods that are established for analysis of 12-lead ECG data can be used to analyze the 6-lead ECG data (which can include 6 of the same leads as a traditional 12-lead ECG).

[0045] The mobile electronic device 104 can include a user interface 136, which can be configured to receive input from a user and/or to output information to a user. In some embodiments, the user interface 136 can include one or more user input elements (e.g., buttons, switches, etc.), a microphone (e.g., for receiving dictated instructions), a display, a touch-screen display, a speaker, etc. The user interface 136 can receive an instruction (e.g., via input from a user) to initiate an ECG recording procedure. The communication interface 130 of the mobile electronic device 104 can send an instruction to the ECG device 102 to initiate the ECG procedure. The user interface 136 can provide instructions to a user for performing the ECG or related activities (e.g., to hold or touch the electrodes 108, 110, and 112, to wait during a delay period or while signals are collected, to contact a doctor or emergency services, etc.). The user interface 136 can report information to a user (e.g., a heart rate, an ECG tracing, an indication of normal rhythm, a diagnosis, etc.).

[0046] The mobile electronic device can include a battery 138, which can facilitate the portable nature of the mobile electronic device 104. Other power sources can be used. For example, the mobile electronic device 104 can receive electrical power from an external power source (e.g., a wall outlet).

[0047] The communication interface 130 of the mobile electronic device 104 can be configured to send ECG data (e.g., 6-lead ECG data) to the remote computing system 106 (using the communication interface 140), as discussed herein. The remote computing system 106 can be a server, a computer, or other computing system.

[0048] The remote computing system 106 can include a controller 142. The controller 142 can be a processor or processing system as described herein. In some embodiments, the remote computing system 106 can include memory 144, which can store executable program instructions that can be executed by the controller 142 to implement various methods, operations, and features described herein. Memory 144 can be a type of computer readable storage media as described herein. In some embodiments, the controller 142 can store data to the memory 144. For example, data corresponding to the digital signals received over time can be stored on the memory 144 for use in signal processing operations that depend on previous signals. Results of signal processing and/or data analysis can be stored in the memory 144, and can be accessed by the controller 142 to be used for later calculations. In some embodiments, data received and/or generated (e.g., by the controller 142) can be stored on the memory 144, such as for archiving, for later reference, etc. In some embodiments, the controller 142 can run an application or program (which can be stored on memory 144), which can perform the ECG procedure (e.g., using cloud computing, or as Software as a Service (SaaS)).

[0049] The controller **142** of the remote computing system **106** can execute program instructions for performing an analysis on the ECG data (e.g., the 6-lead ECG data), which can be received from the mobile electronic device **104**, for example, to determine a heart rate, to make a determination of normal heart rhythm, and/or to diagnose one or more disorders.

[0050] In some embodiments, data, algorithms, and methods that are established for analysis of 12-lead ECG data can be used to analyze the 6-lead ECG data (which can include 6 of the same leads as a traditional 12-lead ECG). In some embodiments, the remote computing system **106** may have access to data and program instructions (e.g., stored in memory **144**) that are not directly accessible to the mobile electronic device **104** and/or more resources such as more powerful processor(s), so that the remote computing system **106** can perform more thorough analysis on the ECG data than would be performed on the mobile electronic device **104**. In some embodiments, the mobile electronic device **104** can perform an initial analysis (which can be performed relatively quickly on the local device) on the ECG data to make one or more initial determinations (e.g., regarding diagnosis and rhythm analysis), and the remote computing system **106** can perform a more detailed analysis (which may take longer time due to transmission of data, backlog of analysis requests, complexity of algorithms for data analysis, and/or the volume of calculations needed for the detailed analysis).

[0051] In some implementations, the controller **142** of the remote computing system **106** can be used to perform various signal processing and data analysis tasks described herein (e.g., digital signal processing, improvement of signal-to-noise ratio, removal or reduction of baseline wander, compensation for impedance, linear phase filtering, providing a 6-lead ECG), especially for embodiments where an application or program that performs the ECG procedure runs on the remote computing system **106** (e.g., using cloud computing or SaaS).

[0052] In some embodiments, the ECG device **102** can have a relatively low power processor (e.g., controller **120**) as compared to the processor(s) of the mobile electronic device **104** and/or the remote computing system **106** (e.g., controllers **132** and **142**), and the ECG device **102** can have more limited resources (e.g., less battery power, less memory storage, etc.) than the mobile electronic device **104** and/or the remote computing system **106**. Accordingly, in some implementations, the system **100** is configured to minimize or reduce the operations performed by the ECG device **102** and may preferentially perform operations on the mobile electronic device **104** and/or the remote computing system **106**.

[0053] In some embodiments, the ECG device **102** can be configured to perform the digital signal processing and analysis, as discussed herein, because the signals are converted to digital data before being transmitted from the ECG device **102**. In some embodiments, the ECG device **102** is configured to perform operations to reduce the amount of data to be transferred by the communication interface **124**, which can save power and time during the transfer of data from the ECG device **102**. For example, in some embodiments, the ECG device **102** is configured to send data corresponding to two voltage differences (leads I and II) instead of sending data corresponding to three signals from the three electrodes **108**, **110**, and **112**. Any or all of these variations of raw, transformed, or interpreted signal data may be referred to as "signal-related data."

[0054] The system **100** shown and described in connection with FIG. 1 can be modified in various ways. For example, in some embodiments, the ECG device **102** and the mobile electronic device **104** can be combined into a single device (which can be a dedicated ECG and mobile device). In some embodiments, an ECG system can include a single device that performs the functions of the ECG device **102**, the mobile electronic device **104**, and the remote computing system **106** (e.g., a 6-lead ECG machine such as for use in a hospital or doctor's office). Embodiments of a combined ECG system may include fewer components than three separate devices to eliminate redundancy (e.g., controller **120**, **132**, and **142** may be combined into a single controller, communication interface **124**, **130**, and **140** into a single communication interface, etc.).

[0055] FIG. 2 shows an example embodiment of an ECG device **102**. The ECG device **102** can include a housing **150**, which can house or enclose various components of the ECG device **102** (e.g., the one or more amplifiers **114**, the signal processor **116**, the analog-to-digital converter **118**, the controller **120**, the memory **122**, the communication interface **124**, and the battery **126**). The ECG device **102** can include the right arm electrode **108**, the left arm electrode **110**, and the left leg electrode **112**, which can be exposed to facilitate contact to the patient's skin. The electrodes **108**, **110** and **112** can be positioned on the bottom of the housing **150**. The right arm electrode **108** can be positioned on a right side to facilitate contact to the patient's right arm or hand. The left arm electrode **110** can be positioned on a left side to facilitate contact to the patient's left arm or hand. The left leg electrode **112** can be positioned in a central portion, to facilitate contact to the patient's left leg (e.g., to the left knee, left ankle, or left foot). The left leg electrode **112** can be positioned closer to the patient than the right arm electrode **108** and/or the left arm electrode **110**, when the electrodes face downward with the right arm electrode **108** on the right and the left arm electrode **110** on the left, which can reduce undesired contact between the electrodes **108**, **110**, and **112** with undesired parts of the patient's body and/or can reduce undesired contact between the parts of the patient's body being monitored, which could interfere with the readings for the ECG procedure.

[0056] In some embodiments, the right arm electrode **108** and the left arm electrode **110** may be positioned differently, e.g., in reverse of the configuration shown in FIG. 2. This positioning may vary in accordance with the chosen placement of the left leg electrode **112** of the device on the left leg, for example, on the dorsal or ventral sides of the left leg. In some embodiments, the designation of the pads as right arm electrode **108** and left arm electrode **110** may be selectable or configurable by the user, for instance via a user interface provided on the ECG device **102** or the mobile electronic device **104**.

[0057] In some embodiments, mobile electronic device **104** can include a user interface that can receive input from the user to assign or reassign one of the three electrodes to a particular limb. The designation can then be transmitted, in some cases, to the ECG device **102** via a communication interface (e.g., **124**, **130**) to associate a particular electrode to a limb reading. Advantageously, a user may be able to reassign the function of a physical electrode to a limb designation that is more comfortable to the user for gathering a particular signal. For example, if the user is more comfortable reading the left leg signal from the dorsal (rear) side of the leg, then the right and left arm electrodes may be assigned to the right and

left electrodes, respectively, when the ECG device **102** is facing up. On the other hand, if the user is more comfortable reading the left leg signal from the ventral (front) side of the leg, then the right and left arm electrodes may be assigned to the left and right electrodes (i.e., opposite), respectively, when the ECG device **102** is facing up.

[0058] In some embodiments, the electrodes **108**, **110**, and **112** can be positioned immovably on the housing and immovably with respect to each other. In some embodiments, the ECG device **102** does not include wires or cables outside of the housing **150** that couple to the electrodes **108**, **110**, and **112**. The electrodes **108**, **110**, and **112** can be positioned close to each other to facilitate the portable and compact nature of the ECG device **102**, and the electrodes **108**, **110**, and **112** can be spaced apart sufficiently to reduce the likelihood of unintended contact between the electrodes **108**, **110**, and **112** (e.g., such as a body part contacting two or more of the electrodes simultaneously). The electrodes **108**, **110**, and **112** can be spaced apart by a distance that is at least about 3 mm, at least about 5 mm, at least about 10 mm, at least about 25 mm, at least about 50 mm or more, less than or equal to about 100 mm, less than or equal to about 75 mm, less than or equal to about 50 mm, less than or equal to about 25 mm, less than or equal to about 10 mm or less, although values outside these ranges can be used in some instances.

[0059] FIG. 3 shows an example embodiment of an ECG device **102** that is removably attachable to a mobile electronic device **104** (e.g., a smart phone). The mobile electronic device **104** can include an attachment mechanism **152**, which can be configured to interface with an attachment mechanism **154** on the ECG device **102** to removably attach the ECG device **102** to the mobile electronic device **104** (e.g., onto the back side of the mobile electronic device **104** such as on a side opposite the display on a smart phone). The attachment mechanisms **152** and **154** can use sliding engagement, a snap fit, a clamp, etc. to removably couple the ECG device **102** to the mobile electronic device **104**. In some embodiments, only one or the other of the ECG device **102** and the mobile electronic device **104** may include an attachment mechanism. In the embodiment illustrated in FIG. 3, the attachment mechanism **152** can include rails or guides **156a** and **156b** (e.g., formed at the sides of a raised platform) that are configured to slidably engage rails or guides **158a** and **158b** (e.g., formed at the sides of a recessed slot in the housing **150**). Various alternatives are possible for the attachment mechanisms. For example, in some embodiments, the ECG device **102** can be incorporated into a protective case that is configured to enclose at least a portion of the mobile electronic device **104**.

[0060] FIG. 4 is a flowchart of an example method **200** of operation for performing an ECG procedure in accordance with some embodiments herein. At block **202**, the system can receive a command (e.g., from a user, which can be the patient) to start an ECG procedure. The command from the user can be received by the user interface **136** on the mobile electronic device, although in some embodiments, the ECG device can include a user input element configured to receive a user command to start an ECG procedure. In some embodiments, the ECG device **102** can receive an instruction to start an ECG procedure from the mobile electronic device **104** (e.g., via the communication interfaces **124** and **130**). At block **204**, the method **200** can include a delay, which can give the user time to position the electrodes **108**, **110**, and **112** into contact with the proper body portions (e.g., since the patient can be the user that issued the start command such as by

pressing a button on the mobile electronic device **104**). The delay can be between about 1 and about 10, between about 2 seconds and about 5 second, or about 3 seconds, although other amounts of delay outside these ranges can be used in some instances. In some cases the delay may terminate when the user issues a continue command, e.g., by interacting with an element of the user interface on the touchscreen of the mobile electronic device **104** or by pressing a button on the housing of **104** or ECG device **102**.

[0061] At block **206**, signals from the electrodes **108**, **110**, and **112** can be received, as discussed herein. At block **208**, the signals from the electrodes **108**, **110**, and **112** can be amplified, as discussed herein. The amplification can compensate for impedance (such as produced by the use of dry electrodes). The amplification can be performed on analog signals received from the electrodes **108**, **110**, and **112**.

[0062] At block **210**, analog signal processing can be performed, such as described in connection with the signal processing module **116**. At block **212**, the analog signals can be converted to digital signals, such as by the analog-to-digital converter **118**, as discussed herein. At block **214**, digital signal processing can be performed, such as by the controller **120**, as discussed herein.

[0063] At block **216**, the ECG device **102** can communicate data (e.g., raw or interpreted data, depending on embodiment) to the mobile electronic device **104** (e.g., via the communication interfaces **124** and **130**). At block **218**, the mobile electronic device **104** can perform signal processing on the received data, as discussed herein. At block **220**, the mobile electronic device **104** can perform data analysis, such as to produce ECG data (e.g., 6-lead ECG data), to analyze the data to provide a heart rate, to provide a determination of normal or abnormal heart rhythm, and/or to provide a diagnosis of a heart disorder. At block **222**, information can be reported (e.g., to the user/patient, to a doctor, or other entity such as a hospital information system). The memory **134** can include information to facilitate reporting to external devices and systems, such as a doctor email address, hospital information system access information, etc.) In some information, information can be reported to a user via the user interface **136** on the mobile electronic device **104**.

[0064] At block **224**, data can be communicated to a remote computing system **106** (e.g., via the communication interfaces **130** and **140**). In some embodiments, the ECG data (e.g., 6-lead ECG data) can be transmitted to the remote computing system **106**, for example, for further processing and/or analysis (blocks **226** and **228**). In some embodiments, the mobile electronic device **104** can send information to the remote computing system **106** regarding initial determinations made by the analysis performed by the mobile electronic device **104**, and the remote computing system **106** can perform additional analysis to confirm or refute the initial determinations made by the mobile electronic device **104**. At block **230**, information, including concerning an additional analysis, can be reported (e.g., to the user/patient, to a doctor, or to another entity such as a hospital information system). The memory **144** at the remote computing system **106** can include information to facilitate reporting to external devices and systems, such as a doctor email address, hospital information system access information, etc. Reporting information can be transferred from the remote computing system **106** to the mobile electronic device **104** (via the communication interfaces **130** and **140**) for reporting to the user (e.g., via the user interface **136**). Many variations are possible. For

example, various operations shown and described in connection with FIG. 4 can be omitted, combined with other operations, or separated into sub-operations, and additional operations can be added.

[0065] FIG. 5 is a flowchart showing an example embodiment of a method of use 300 for an ECG system. At block 302, the user can provide an instruction to start an ECG procedure (e.g., via the user interface 136 on the mobile electronic device 104). At block 304, the user can contact the right arm electrode 108 to a portion of the user's right arm, such as by holding the ECG device 102 with a right thumb or finger on the right arm electrode 108. At block 306, the user can contact the left arm electrode 110 to a portion of the user's left arm, such as by holding the ECG device 102 with a left thumb or finger on the left arm electrode 110. At block 308, the user can contact the left leg electrode 112 to a portion of the user's left leg, such as by holding the ECG device 102 such that the left leg electrode 112 contacts the user's left leg (e.g., at the left knee or left ankle). At block 310, the user can hold the contact with the electrodes 108, 110, and 112 for the duration of the ECG procedure, for example, until instructed via the user interface 136 that the procedure is completed such as with a visual, auditory, or tactile signal from the mobile electronic device 104 or ECG device 102.

[0066] FIG. 6 shows an example embodiment of a user interface 400 for an ECG system, which can be used, for example, for the user interface 136, described herein. The user interface can be implemented on a display, such as a touch screen display, of a mobile electronic device 104. The user interface 400 can include a user input element (e.g., a digital button on a touch screen display) for initiating an ECG procedure, such as a start button 404. The user interface 400 can include a notification element 406 to notify the user of a delay period after receipt of a command to start an ECG procedure, such as a displayed count down from 3 to 2 to 1. The user interface 400 can include an ECG tracing portion 408, which can be configured to show ECG tracing information during the ECG procedure, which can alert the user that the ECG procedure is being performed. In some embodiments, the ECG tracing portion 408 can display information that is unprocessed or only partially processed, which can result in the ECG tracing portion displaying a graphical representation that does not necessarily look like a normal ECG waveform, but which can inform the user that the system is successfully gathering information from the electrodes 108, 110, 112. The user interface 400 can include an ECG waveform portion 410, which can display a processed ECG tracing (e.g., for a single beat). The processed ECG tracing shown by portion 410 can be an average or weighted average based on some or all of the ECG data that was collected and processed. The user interface 400 can display heart rate information 412. The user interface 400 can include a reporting portion for displaying commands or reports for the user. For example, as shown in element 414, the reporting portion can report to the user that the ECG process was completed, that a determination of normal heart rhythm was determined, and that the user's doctor was notified. The user interface 410 can have an options section 416, which can enable the user to change various options and parameters of the system. For example, the user can set an email address or other contact information for a doctor to be notified of ECG results, the user can change the delay time, etc.

[0067] FIG. 7 shows a block diagram illustrating components of a computing device or system used in some imple-

mentations of techniques and systems for performing an electrocardiogram as described herein. For example, components of the system, including an electrocardiograph device, mobile electronic device, and/or remote computing system may be implemented as described with respect to device 1000. Device 1000 can itself include one or more computing devices. The hardware can be configured according to any suitable computer architectures such as Symmetric Multi-Processing (SMP) architecture or Non-Uniform Memory Access (NUMA) architecture.

[0068] The device 1000 can include a processing system 1001, which may include a processing device such as a central processing unit (CPU) or microprocessor and other circuitry that retrieves and executes software 1002 from storage system 1003. Processing system 1001 may be implemented within a single processing device but may also be distributed across multiple processing devices or sub-systems that cooperate in executing program instructions. A controller, such as might be found on one or more system devices, can be a processing system or processor as described herein.

[0069] Examples of processing system 1001 include general purpose central processing units, application specific processors, and logic devices, as well as any other type of processing device, combinations, or variations thereof. The one or more processing devices may include multiprocessors or multi-core processors and may operate according to one or more suitable instruction sets including, but not limited to, a Reduced Instruction Set Computing (RISC) instruction set, a Complex Instruction Set Computing (CISC) instruction set, or a combination thereof. In certain embodiments, one or more digital signal processors (DSPs) may be included as part of the computer hardware of the system in place of or in addition to a general purpose CPU.

[0070] Storage system 1003 may comprise any computer readable storage media readable by processing system 1001 and capable of storing software 1002 including, e.g., processing instructions performing an electrocardiogram as described herein. Storage system 1003 may include volatile and nonvolatile, removable and non-removable media implemented in any method or technology for storage of information, such as computer readable instructions, data structures, program modules, or other data.

[0071] Examples of storage media include random access memory (RAM), read only memory (ROM), magnetic disks, optical disks, CDs, DVDs, flash memory, solid state memory, phase change memory, 3D-XPoint memory, or any other suitable storage media. Certain implementations may involve either or both virtual memory and non-virtual memory. In no case do storage media consist of a propagated signal. In addition to storage media, in some implementations, storage system 1003 may also include communication media over which software 1002 may be communicated internally or externally.

[0072] Storage system 1003 may be implemented as a single storage device but may also be implemented across multiple storage devices or sub-systems co-located or distributed relative to each other. Storage system 1003 may include additional elements capable of communicating with processing system 1001.

[0073] Software 1002 may be implemented in program instructions and, among other functions, may, when executed by device 1000 in general or processing system 1001 in particular, direct device 1000 or processing system 1001 to operate as described herein for performing an electrocardio-

gram. Software **1002** may provide program instructions **1004** that implement components for performing an electrocardiogram. Software **1002** may implement on device **1000** components, programs, agents, or layers that implement in machine-readable processing instructions **1004** the methods and techniques described herein.

[**0074**] In general, software **1002** may, when loaded into processing system **1001** and executed, transform device **1000** overall from a general-purpose computing system into a special-purpose computing system customized to perform an electrocardiogram in accordance with the techniques herein. Indeed, encoding software **1002** on storage system **1003** may transform the physical structure of storage system **1003**. The specific transformation of the physical structure may depend on various factors in different implementations of this description. Examples of such factors may include, but are not limited to, the technology used to implement the storage media of storage system **1003** and whether the computer-storage media are characterized as primary or secondary storage. Software **1002** may also include firmware or some other form of machine-readable processing instructions executable by processing system **1001**. Software **1002** may also include additional processes, programs, or components, such as operating system software and other application software.

[**0075**] Device **1000** may represent any computing system on which software **1002** may be staged and from where software **1002** may be distributed, transported, downloaded, or otherwise provided to yet another computing system for deployment and execution, or yet additional distribution. Device **1000** may also represent other computing systems that may form a necessary or optional part of an operating environment for the disclosed techniques and systems, e.g., remote computing system or mobile electronic device.

[**0076**] A communication interface **1005** may be included, providing communication connections and devices that allow for communication between device **1000** and other computing systems (not shown) over a communication network or collection of networks (not shown) or the air. Examples of connections and devices that together allow for inter-system communication may include network interface cards, antennas, power amplifiers, RF circuitry, transceivers, and other communication circuitry. The connections and devices may communicate over communication media to exchange communications with other computing systems or networks of systems, such as metal, glass, air, or any other suitable communication media. The aforementioned communication media, network, connections, and devices are well known and need not be discussed at length here.

[**0077**] It should be noted that many elements of device **1000** may be included in a system-on-a-chip (SoC) device. These elements may include, but are not limited to, the processing system **1001**, a communications interface **1005**, and even elements of the storage system **1003** and software **1002**.

[**0078**] Alternatively, or in addition, the functionality, methods and processes described herein can be implemented, at least in part, by one or more hardware modules (or logic components). For example, the hardware modules can include, but are not limited to, application-specific integrated circuit (ASIC) chips, field programmable gate arrays (FPGAs), system-on-a-chip (SoC) systems, complex programmable logic devices (CPLDs) and other programmable logic devices now known or later developed. When the hardware modules are activated, the hardware modules perform the functionality, methods and processes included within the

hardware modules. In some cases, one or more capabilities, e.g., the processing system, storage system, and communication interface may be included on a single device such as a microcontroller.

[**0079**] Furthermore, while certain types of user interfaces and controls are described herein for illustrative purposes, other types of user interfaces and controls may be used. A user interface may be generated on a local computer or on a mobile device, or it may be generated from a service or cloud server and sent to a client for rendering, e.g., in a browser or “app.”

[**0080**] Certain aspects of the invention provide the following non-limiting embodiments:

Example 1

[**0081**] A system for performing an electrocardiogram comprising: an electrocardiograph device, comprising: a housing comprising three electrodes, wherein the three electrodes are not coupled to the device with wires exterior to the housing; a communication interface; one or more computer readable storage media; program instructions stored on the one or more computer readable storage media that, when executed by a controller, direct the controller to: receive signals from the three electrodes; analyze the signals to determine signal-related data; transmit the signal-related data, via the communication interface, to a coupled interpretive device.

Example 2

[**0082**] The system of example 1, wherein the electrocardiograph device is a portable handheld device.

Example 3

[**0083**] The system of any of examples 1-2, wherein the electrocardiograph device further comprises: one or more amplifiers configured to amplify analog signals received from the three electrodes; and program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to receive and analyze amplified analog signals from the one or more amplifiers.

Example 4

[**0084**] The system of any of examples 1-3, wherein the electrocardiograph device further comprises: an analog signal processor configured to perform analog signal processing on analog signals received from the three electrodes; and program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to receive and analyze processed analog signals from the analog signal processor.

Example 5

[**0085**] The system of any of examples 1-4, wherein the electrocardiograph device further comprises: an analog-to-digital converter configured to convert analog signals from the three electrodes to digital signals; and program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to receive and analyze the digital signals from the analog-to-digital converter.

Example 6

[0086] The system of any of examples 1-5, wherein the electrocardiograph device further comprises program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to perform digital signal processing on the signals received from the three electrodes.

Example 7

[0087] The system of any of examples 1-6, further comprising: a mobile electronic device comprising: a second communication interface; second program instructions stored on second computer readable storage media that, when executed by second controller, direct the second controller to: receive the signal-related data transmitted by the communication interface of the electrocardiograph device; and provide 6-lead electrocardiogram data based at least in part on the data received by the second communication interface.

Example 8

[0088] The system of example 7, wherein the 6-lead electrocardiogram data includes Lead I, Lead II, Lead III, aVR, aVL, and aVF.

Example 9

[0089] The system of any of examples 7-8, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to: display user interface elements configured to receive input from a user to initiate an electrocardiogram procedure; and in response to receiving the input from the user, sending an instruction to the electrocardiograph device to initiate the electrocardiogram procedure.

Example 10

[0090] The system of example 9, wherein the system delays sending the instruction to initiate the electrocardiogram procedure by a delay time after receiving the input from the user.

Example 11

[0091] The system of any of examples 7-10, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to: display user interface elements configured to output information based on the 6-lead electrocardiogram data.

Example 12

[0092] The system of any of examples 7-11, further comprising a remote computing system comprising: third program instructions stored on third computer readable storage media that, when executed by third controller, direct the third controller to: receive the 6-lead electrocardiogram data provided from the mobile electronic device; and analyze the 6-lead electrocardiogram data; and provide diagnostic information.

Example 13

[0093] The system of example 12, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to: receive the diagnostic information provided from the remote computing system; and display user interface elements configured to output the diagnostic information provided from the remote computing system.

Example 14

[0094] The system of any of examples 7-13, wherein the electrocardiograph device is removably attached to the mobile electronic device.

Example 15

[0095] The system of any of examples 1-14, wherein the signal-related data includes 6-lead electrocardiogram data comprising Lead I, Lead II, Lead III, aVR, aVL, and aVF.

Example 16

[0096] The system of any of examples 1-15, wherein the three electrodes are fixed immovably to the outside of the housing of the electrocardiograph device.

Example 17

[0097] The system of any of examples 1-16, wherein the three electrodes comprise dry electrodes.

Example 18

[0098] The system of any of examples 17, wherein the electrocardiograph device further comprises program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to compensate for higher impedance of the dry electrodes.

Example 19

[0099] The system of any of examples claim 1-18, wherein the three electrodes comprise a right arm electrode, a left arm electrode, and a left leg electrode.

Example 20

[0100] The system of any of examples 7-18, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to: display user interface elements configured to receive input from a user to assign each of the three electrodes to a particular limb; and in response to receiving the input from the user, sending an instruction to the electrocardiograph device to associate readings from each of the three electrodes to the particular limb.

[0101] The embodiments discussed herein are provided by way of example, and various modifications can be made to the embodiments described herein. Certain features that are described in this disclosure in the context of separate embodiments can also be implemented in combination in a single embodiment. Conversely, various features that are described in the context of a single embodiment can be implemented in multiple embodiments separately or in various suitable sub-

combinations. Also, features described in connection with one combination can be excised from that combination and can be combined with other features in various combinations and subcombinations. Various features can be added to the example embodiments disclosed herein. Also, various features can be omitted from the example embodiments disclosed herein.

[0102] Similarly, while operations are depicted in the drawings or described in a particular order, the operations can be performed in a different order than shown or described. Other operations not depicted can be incorporated before, after, or simultaneously with the operations shown or described. In certain circumstances, parallel processing or multitasking can be used. Also, in some cases, the operations shown or discussed can be omitted or recombined to form various combinations and subcombinations.

1. A system for performing an electrocardiogram comprising:

- an electrocardiograph device, comprising:
 - a housing comprising three electrodes, wherein the three electrodes are not coupled to the device with wires exterior to the housing;
 - a communication interface;
 - one or more computer readable storage media;
 - program instructions stored on the one or more computer readable storage media that, when executed by a controller, direct the controller to:
 - receive signals from the three electrodes;
 - analyze the signals to determine signal-related data;
 - and
 - transmit the signal-related data, via the communication interface, to a coupled interpretive device.

2. The system of claim 1, wherein the electrocardiograph device is a portable handheld device.

3. The system of claim 1, wherein the three electrodes comprise a right arm electrode, a left arm electrode, and a left leg electrode.

4. The system of claim 1, wherein the electrocardiograph device further comprises:

- one or more amplifiers configured to amplify analog signals received from the three electrodes; and
- program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to receive and analyze amplified analog signals from the one or more amplifiers.

5. The system of claim 1, wherein the electrocardiograph device further comprises:

- an analog signal processor configured to perform analog signal processing on analog signals received from the three electrodes; and
- program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to receive and analyze processed analog signals from the analog signal processor.

6. The system of claim 1, wherein the electrocardiograph device further comprises:

- an analog-to-digital converter configured to convert analog signals from the three electrodes to digital signals; and
- program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to receive and analyze the digital signals from the analog-to-digital converter.

7. The system of claim 1, wherein the electrocardiograph device further comprises program instructions stored on the

one or more computer readable storage media that, when executed by the controller, direct the controller to perform digital signal processing on the signals received from the three electrodes.

8. The system of claim 1, further comprising:

- a mobile electronic device comprising:
 - a second communication interface;
 - second program instructions stored on second computer readable storage media that, when executed by second controller, direct the second controller to:
 - receive the signal-related data transmitted by the communication interface of the electrocardiograph device; and
 - provide 6-lead electrocardiogram data based at least in part on the data received by the second communication interface.

9. The system of claim 8, wherein the 6-lead electrocardiogram data includes Lead I, Lead II, Lead III, aVR, aVL, and aVF.

10. The system of claim 8, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to:

- display user interface elements configured to receive input from a user to initiate an electrocardiogram procedure;
- and
- in response to receiving the input from the user, sending an instruction to the electrocardiograph device to initiate the electrocardiogram procedure.

11. The system of claim 10, wherein the system delays sending the instruction to initiate the electrocardiogram procedure by a delay time after receiving the input from the user.

12. The system of claim 8, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to:

- display user interface elements configured to output information based on the 6-lead electrocardiogram data.

13. The system of claim 8, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to:

- display user interface elements configured to receive input from a user to assign each of the three electrodes to a particular limb; and
- in response to receiving the input from the user, sending an instruction to the electrocardiograph device to associate readings from each of the three electrodes to the particular limb.

14. The system of claim 8, further comprising a remote computing system comprising:

- third program instructions stored on third computer readable storage media that, when executed by third controller, direct the third controller to:
 - receive the 6-lead electrocardiogram data provided from the mobile electronic device; and
 - analyze the 6-lead electrocardiogram data; and
 - provide diagnostic information.

15. The system of claim 14, wherein the mobile electronic device further comprises program instructions stored on the second computer readable storage media that, when executed by the second controller, direct the second controller to:

- receive the diagnostic information provided from the remote computing system; and

display user interface elements configured to output the diagnostic information provided from the remote computing system.

16. The system of claim **8**, wherein the electrocardiograph device is removably attached to the mobile electronic device.

17. The system of claim **1**, wherein the signal-related data includes 6-lead electrocardiogram data comprising Lead I, Lead II, Lead III, aVR, aVL, and aVF.

18. The system of claim **1**, wherein the three electrodes are fixed immovably to the outside of the housing of the electrocardiograph device.

19. The system of claim **1**, wherein the three electrodes comprise dry electrodes.

20. The system of claim **19**, wherein the electrocardiograph device further comprises program instructions stored on the one or more computer readable storage media that, when executed by the controller, direct the controller to compensate for higher impedance of the dry electrodes.

* * * * *

专利名称(译)	用于执行心电图的系统和方法		
公开(公告)号	US20160135701A1	公开(公告)日	2016-05-19
申请号	US14/941556	申请日	2015-11-14
[标]申请(专利权)人(译)	德拉克STEFAN		
申请(专利权)人(译)	德雷克STEFAN		
当前申请(专利权)人(译)	德雷克STEFAN		
[标]发明人	DRAKE STEFAN		
发明人	DRAKE, STEFAN		
IPC分类号	A61B5/0404 A61B5/0408 A61B5/044 A61B5/0432 A61B5/0428 A61B5/00 A61B5/04		
CPC分类号	A61B5/0404 A61B5/0006 A61B5/0408 A61B5/04012 A61B5/7475 A61B5/0428 A61B5/6824 A61B5/6828 A61B5/044 A61B5/0432 A61B5/6898 A61B2560/0468 A61B5/04028 A61B5/743		
优先权	62/080203 2014-11-14 US		
其他公开文献	US9730598		
外部链接	Espacenet USPTO		

摘要(译)

用于执行心电图 (ECG) 的系统可以包括具有右臂电极, 左臂电极和左腿电极的手持式心电图装置, 并且可以被配置为从电极接收信号并且基于电极发送数据信号到移动电子设备。移动电子设备可以被配置为处理和分析接收信息以提供ECG数据, 例如6导联ECG数据。移动电子设备可以分析ECG数据以提供诊断信息。移动电子设备可以将ECG数据传送到远程计算系统, 远程计算系统可以分析ECG数据以提供诊断信息。

