



(11) **EP 1 180 974 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
16.01.2008 Bulletin 2008/03

(21) Application number: **01912972.5**

(22) Date of filing: **23.02.2001**

(51) Int Cl.:
A61B 8/00 (2006.01)

(86) International application number:
PCT/US2001/005792

(87) International publication number:
WO 2001/066015 (13.09.2001 Gazette 2001/37)

(54) **METHOD OF ULTRASONIC IMAGING AND ULTRASONIC DIAGNOSTIC APPARATUS**

VERFAHREN FÜR ULTRASCHALLBILDDARSTELLUNG UND ULTRASCHALLDIAGNOSTISCHES GERÄT

PROCEDE D'IMAGERIE ULTRASONORE ET APPAREIL DE DIAGNOSTIC ULTRASONORE

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU MC NL PT SE TR

(30) Priority: **08.03.2000 JP 2000063853**

(43) Date of publication of application:
27.02.2002 Bulletin 2002/09

(73) Proprietor: **GE Medical Systems Global Technology Company LLC**
Waukesha, WI 53188 (US)

(72) Inventor: **HASHIMOTO, Hiroshi**
Hino-shi, Tokyo 191-8503 (JP)

(74) Representative: **Bedford, Grant Richard**
GE
London Patent Operation
15 John Adam Street
London WC2N 6LU (GB)

(56) References cited:
WO-A-99/08599 **DE-A- 19 723 053**
US-A- 5 694 937

EP 1 180 974 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND OF THE INVENTION

[0001] The present invention relates to a method of ultrasonic imaging and an ultrasonic diagnostic apparatus, and more particularly to a method of ultrasonic imaging and an ultrasonic diagnostic apparatus capable of producing ultrasonic images by which it is possible to visually recognize at a glance the time-wise change of a blood flow.

[0002] In obtaining an ultrasonic image of a blood flow, there has been a convention to use small bubbles in blood as the contrast agent. These small bubbles disperse by being hit by a strong ultrasonic wave. In particular, in document WO-A-99/08599, images are formed of frames in which some beams have higher ultrasound power for dispersing the contrast agent and some beams have lower ultrasound power for not dispersing the contrast agent. Alternatively, in this document, image frames are formed in which all the beams of a frame have higher ultrasound power interposed with frames in which all the beams have lower ultrasound power.

[0003] On this account, after the imaging for a high-transmission frame (a frame taken by use of an ultrasonic wave which is strong enough to disperse the contrast agent), imaging for low-transmission frames (frames taken by use of an ultrasonic wave which is not so strong as to disperse the contrast agent) is carried out continuously, and imaging for another high-transmission frame is carried out on expiration of the time at which the view field is filled with a blood flow including the contrast agent, with these operations being implemented cyclically, as shown in FIG. 1.

[0004] In FIG. 1, vertical line segments aligning along the time axis represent transmission time points and transmission strengths of sonic beams which form the frames.

[0005] Fig. 2(a) shows sonic beams which form a high-transmission frame, and the bold lines signify an ultrasonic wave which is strong enough to disperse the contrast agent. Indicated by V is a blood vessel, and the arrow indicates the direction of blood flow.

[0006] In contrast, Fig. 2(b) shows sonic beams which form a low-transmission frame, and the thin lines signify an ultrasonic wave which is not so strong as to disperse the contrast agent.

[0007] It has been possible to view the state of a blood flow at one moment in the image of a high-transmission frame which is taken based on the above-mentioned conventional scheme.

[0008] However, this scheme has been problematic in that it cannot provide a view of the time-wise change of a blood flow. Specifically, if it is intended to view the time-wise change of a blood flow, it is necessary to compare images of high-transmission frames taken at different time points, and it necessitates skill.

SUMMARY OF THE INVENTION

[0009] It is an object of the present invention to provide a method of ultrasonic imaging and an ultrasonic diagnostic apparatus capable of producing ultrasonic images by which it is possible to visually recognize at a glance the time-wise change of a blood flow.

[0010] The present invention is defined in the independent claims 1 and 5. Preferred aspects of the invention are defined in the dependent claims.

[0011] According to the ultrasonic imaging method and ultrasonic diagnostic apparatus of this invention, which actively utilize the dispersion of contrast agent in the presence of a strong ultrasonic wave, it is possible to produce ultrasonic images which enable to visually recognize at a glance the time-wise change of a blood flow.

[0012] Further objects and advantages of the present invention will be apparent from the following description of the preferred embodiments of the invention as illustrated in the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0013]

Fig. 1 is an explanatory diagram showing the transmission order for forming high-transmission frames and low-transmission frames based on the conventional scheme.

Fig. 2 is an explanatory diagram of the high-transmission frame and low-transmission frame based on the conventional scheme.

Fig. 3 is a block diagram of an ultrasonic diagnostic apparatus based on an embodiment of the invention.

Fig. 4 is an explanatory diagram of a marking frame and no-marking frame based on said embodiment.

Fig. 5 is an explanatory diagram showing the transmission order for forming frames based on said embodiment.

Fig. 6 is a set of diagrams showing examples of ultrasonic images produced by the ultrasonic diagnostic apparatus based on said embodiment.

Fig. 7 is a different explanatory diagram of a marking frame and no-marking frame.

Fig. 8 is an explanatory diagram of the transmission strength for the marking frame based on Fig. 7.

Fig. 9 is a set of diagrams showing examples of ultrasonic images produced by the ultrasonic diagnostic apparatus based on Fig. 7.

Fig. 10 is yet a different explanatory diagram of a marking frame and no-marking frame.

Fig. 11 is a diagram of an ultrasonic image produced by the ultrasonic diagnostic apparatus based on Fig. 10.

DETAILED DESCRIPTION OF THE INVENTION

[0014] The present invention will be explained in more detail by dealing with the illustrated embodiments.

[0015] Fig. 3 is a block diagram of an ultrasonic diagnostic apparatus 100 based on an embodiment of this invention.

[0016] This ultrasonic diagnostic apparatus 100 is made up of an ultrasonic probe 1, a transmitter/receiver 2 which transmits an ultrasonic wave at a specified transmission strength, receives the echo of ultrasonic transmission, and produces a reception signal, a transmission strength controller 3 which specifies the transmission strength, an operation console 4 which is used by the operator to instruct the transmission strength controller 3, a data processor 5 which produces an ultrasonic image such as a B-mode image from the reception signal, a DSC (digital scan converter) 6 which converts the ultrasonic image into a display image, and a CRT 7 which displays the display image.

[0017] Fig. 4(a) is an explanatory diagram of a marking frame produced by the ultrasonic diagnostic apparatus 100.

[0018] The marking frame is defined to be an image of a frame which is produced by the transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for part (shown by the bold lines) of a number of sonic beams which form one frame and the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for other sonic beams (shown by the thin lines), and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0019] Fig. 4(b) is an explanatory diagram of a no-marking frame produced by the ultrasonic diagnostic apparatus 100.

[0020] The no-marking frame is defined to be an image of a frame which is produced by the transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for all of a number of sonic beams which form one frame, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0021] Fig. 5 is an explanatory diagram showing the transmission time points and transmission strengths of sonic beams of the ultrasonic diagnostic apparatus 100.

[0022] Vertical line segments aligning along the time axis represent transmission time points and transmission strengths of sonic beams which form the frames.

[0023] Following the imaging for a marking frame, imaging for no-marking frames is carried out continuously,

and imaging for another marking frame is carried out after such a time length that the flow range is present within the view field, with these operations being repeated.

[0024] Providing a time difference, which is based on the heart beat, between the timing of ultrasonic transmission for a marking frame at the strength for the dispersion of contrast agent and the timing of ultrasonic transmission for the next marking frame at the strength for the dispersion of contrast agent enables the proper observation of a pulsing flow. The time difference based on the heart beat may be a multiple of the period of heart beat measured with an electrocardiograph, or may be a multiple of an approximate heart beat period (e.g., 1 second).

[0025] Fig. 6 is a set of explanatory diagrams of images produced by the ultrasonic diagnostic apparatus 100.

[0026] Shown by (a) is a first marking frame, in which case the contrast agent on the sonic beam (bold dashed line) at the transmission strength for the dispersion of contrast agent disperses, whereas the contrast agent on the sonic beams (thin dashed line) at the transmission strength for no dispersion of contrast agent does not disperse.

[0027] Shown by (b) is a no-marking frame which follows the first marking frame, in which case the portion (bold line) where the contrast agent has dispersed in the first marking frame has a weaker echo than other portion and seems to be the black void. Thin dashed lines represent sonic beams at the transmission strength for no dispersion of contrast agent.

[0028] Shown by (c) is a second marking frame, in which case only the contrast agent on the sonic beam (bold dashed line) at the transmission strength for the dispersion of contrast agent disperses, as in the case of (a). The portion (bold line) where the contrast agent has dispersed in the first marking frame seems to be the black void.

[0029] Shown by (d) is an image after the fifth or later marking frame, in which the portions (bold line) where the contrast agent has dispersed in the preceding marking frames seem to be stripes of the black void.

[0030] The ultrasonic diagnostic apparatus 100 of the foregoing embodiment presents a stripe pattern appended to a flow which intersects the direction of sonic beams as shown by (d) in Fig. 6, whereby it becomes possible to visually recognize the time-wise change at a glance.

[0031] Fig. 7(a) is an explanatory diagram of a marking frame produced by the ultrasonic diagnostic apparatus.

[0032] The marking frame is defined to be a frame produced by the concentrated transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for a certain depth (indicated by black dots) of a number of sonic beams (thin lines) which form one frame and the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for other depths, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission. A certain depth on sonic beams may be replaced with a

certain depth seen from the ultrasonic probe.

[0033] Fig. 7(b) is an explanatory diagram of a no-marking frame.

[0034] The no-marking frame is defined to be a frame which is produced by the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for all of a number of sonic beams which form one frame, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0035] Fig. 8 is an explanatory diagram showing the depths and transmission strengths of sonic beams used for the marking frame.

[0036] Lateral line segments aligning on the depth axis represent transmission strengths.

[0037] Also, following the imaging of a marking frame, imaging for no-marking frames is carried out continuously, and imaging for another marking frame is carried out after such a time length that the flow range is present within the view field, with these operations being repeated.

[0038] Providing a time difference, which is based on the heart beat, between the timing of ultrasonic transmission for a marking frame at the strength for the dispersion of contrast agent and the timing of ultrasonic transmission for the next marking frame at the strength for the dispersion of contrast agent enables the proper observation of a pulsing flow. The time difference based on the heart beat may be a multiple of the period of heart beat measured with an electrocardiograph, or may be a multiple of an approximate heart beat period (e.g., 1 second).

[0039] Fig. 9 is a set of explanatory diagrams of images produced by the ultrasonic diagnostic apparatus.

[0040] Shown by (a) is a first marking frame, in which case the contrast agent in a portion of the depth (white dots) where the contrast agent is to be dispersed disperses, whereas the contrast agent in other portion does not disperse. Thin dashed lines represent sonic beams at the transmission strength for no dispersion of contrast agent.

[0041] Shown by (b) is a no-marking frame which follows the first marking frame, in which case the portion (black dots) where the contrast agent has dispersed in the first marking frame has weaker echoes than other portion and seems to be the black void.

[0042] Shown by (c) is a second marking frame, in which case only the contrast agent at the depth (white dots) for the dispersion of contrast agent disperses, as in the case of (a). The portion (black dots) where the contrast agent has dispersed in the first marking frame seems to be the black void.

[0043] Shown by (d) is an image after the fourth or later marking frame, in which the portions (black dots) where the contrast agent has dispersed in the preceding marking frames seem to be stripes of the black void.

[0044] The ultrasonic diagnostic apparatus of the foregoing presents a stripe pattern appended to a flow which

is virtually parallel to the direction of sonic beams as shown by (d) in Fig. 9, whereby it becomes possible to visually recognize the time-wise change at a glance.

[0045] Fig. 10(a) is an explanatory diagram of a marking frame produced by the ultrasonic diagnostic apparatus.

[0046] The marking frame is defined to be a frame produced by the transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for two or more spaced-out sonic beams (bold lines) among a number of sonic beams which form one frame and the transmission of an ultrasonic wave for other sonic beams at the strength for the dispersion of contrast agent for two or more spaced-out positions of a certain depth (black dots) and at the strength for no dispersion of contrast agent for other depths, and the formation of an image for one frame from received signals which correspond to the ultrasonic transmission. A certain depth on sonic beams may be replaced with a certain depth seen from the ultrasonic probe.

[0047] Fig. 10 (b) is an explanatory diagram of a no-marking frame.

[0048] The no-marking frame is defined to be a frame which is produced by the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for all of a number of sonic beams which form one frame, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0049] Also, following the imaging of a marking frame, imaging for no-marking frames is carried out continuously, and imaging for another marking frame is carried out after such a time length that the flow range is present within the view field, with these operations being repeated.

[0050] Providing a time difference, which is based on the heart beat, between the timing of ultrasonic transmission for a marking frame at the strength for the dispersion of contrast agent and the timing of ultrasonic transmission for the next marking frame at the strength for the dispersion of contrast agent enables the proper observation of a pulsing flow. The time difference based on the heart beat may be a multiple of the period of heart beat measured with an electrocardiograph, or may be a multiple of an approximate heart beat period (e.g., 1 second).

[0051] Fig. 11 is an explanatory diagram of an image produced by the ultrasonic diagnostic apparatus.

[0052] The portions of marking frames where the contrast agent has dispersed (bold lines and black dots) seem to be a lattice of the black void.

[0053] The ultrasonic diagnostic apparatus presents stripe patterns in both the direction orthogonal to the direction of sonic beams and the direction of flow which is virtually parallel to the direction of sonic beams (i.e., in a shape of lattice) as shown in Fig. 11, whereby it becomes possible to visually recognize at a glance the time-wise change of particularly a two-dimensional flow in the car-

diac ventricle and atrium.

[0054] Many widely different embodiments of the invention may be configured without departing from the scope of the present invention. It should be understood that the present invention is not limited to the specific embodiments described in the specification, except as defined in the appended claims.

Claims

1. A method of ultrasonic imaging comprising the steps of:

transmitting an ultrasonic wave at such a strength as to disperse the contrast agent for a number of sonic beams which form a first frame and transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for the other sonic beams which form the first frame;

transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for all the sonic beams which form a second frame;

producing an image from received signals which correspond to the ultrasonic wave transmissions;

repeating the steps of transmitting the ultrasonic waves for forming the first and second frames; and

interposing the second frames between the first frames.

2. The method of ultrasonic imaging of claim 1, wherein one timing of ultrasonic wave transmission for the first frame, and another timing of ultrasonic wave transmission for a later one of said first frames, have a time difference which is based on the heart beat.

3. The method of ultrasonic imaging of claim 1, wherein the first frames comprise at least two spaced sonic beams for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

4. The method of ultrasonic imaging of any one of claims 1 to 3 wherein the step of transmitting an ultrasonic wave at such a strength as to disperse the contrast agent for a first frame is at such a strength as to disperse the contrast agent for a certain depth, and wherein the method includes transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for other depths.

5. An ultrasonic diagnostic apparatus comprising:

an ultrasonic probe (1);
transmission/reception means (2) for transmit-

ting an ultrasonic wave from said ultrasonic probe and for receiving a signal which corresponds to the ultrasonic wave transmission;

transmission strength control means (3) for controlling the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for a number of sonic beams which form a first frame and have such a strength as not to disperse the contrast agent for the other sonic beams which form the first frame;

wherein said transmission strength control means (3) controls the ultrasonic wave transmission such that a second frame, which is formed by the ultrasonic wave transmission at such a strength as not to disperse the contrast agent for all the sonic beams which form the second frame;

image producing means (5, 6, 7) for producing an image from the received signals;

wherein the transmission strength control means (3) is operable to repeatedly generate the first and second frames and interpose the second frames between the first frames.

6. The ultrasonic diagnostic apparatus of claim 5, wherein said transmission strength control means (3) controls the ultrasonic wave transmission such that one timing of ultrasonic wave transmission for the first frame, and another timing of ultrasonic wave transmission for a later one of said first frames, have a time difference which is based on the heart beat.

7. The ultrasonic diagnostic apparatus of claim 6, wherein said transmission strength control means (3) controls the ultrasonic wave transmission such that there are in said first frames at least two spaced sonic beams for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

8. The ultrasonic diagnostic apparatus of any one of claims 5 to 7 wherein the transmission strength control means (3) is arranged for controlling the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for a certain depth and have such a strength as not to disperse the contrast agent for other depths.

Patentansprüche

1. Ultraschallbildgebungsverfahren, welches die folgenden Schritte umfasst:

Übertragung einer Ultraschallwelle bei einer Stärke, bei der das Kontrastmittel für eine Anzahl von Schallstrahlen, die einen ersten Frame bilden, dispergiert wird, sowie Übertragung ei-

- ner Ultraschallwelle bei einer Stärke, bei der das Kontrastmittel für die anderen Schallstrahlen, die den ersten Frame bilden, nicht dispergiert wird;
- Übertragung einer Ultraschallwelle bei einer Stärke, bei der das Kontrastmittel nicht für alle der Schallstrahlen dispergiert wird, die einen zweiten Frame bilden;
- Erzeugung eines Bildes aus den empfangenen Signalen, welche den Ultraschallwellenübertragungen entsprechen;
- Wiederholung der Schritte der Ultraschallwellenübertragung zur Bildung des ersten und zweiten Frames; und
- Einschieben der zweiten Frames zwischen die ersten Frames.
2. Ultraschallbildgebung gemäß Anspruch 1, **dadurch gekennzeichnet, dass** eine Zeitfestlegung der Ultraschallwellenübertragung für den ersten Frame und eine andere Zeitfestlegung der Ultraschallwellenübertragung für einen späteren der ersten Frames eine Zeitdifferenz aufweisen, die auf dem Herzschlag beruht.
3. Ultraschallbildgebungsverfahren gemäß Anspruch 1, **dadurch gekennzeichnet, dass** die ersten Frames mindestens zwei im Abstand angeordnete Schallstrahlen umfassen, für die eine Ultraschallwelle bei einer Stärke übertragen wird, bei der das Kontrastmittel dispergiert wird.
4. Ultraschallbildgebungsverfahren gemäß einem der Ansprüche 1 bis 3, **dadurch gekennzeichnet, dass** der Schritt der Ultraschallwellenübertragung bei einer Stärke, bei der das Kontrastmittel für einen ersten Frame dispergiert wird, bei einer Stärke vor sich geht, bei der das Kontrastmittel für eine bestimmte Tiefe dispergiert wird, und **dadurch gekennzeichnet, dass** das Verfahren der Ultraschallwellenübertragung bei einer Stärke vor sich geht, bei der das Kontrastmittel für andere Tiefen nicht dispergiert wird.
5. Ultraschall-Diagnostikgerät, umfassend:
- eine Ultraschallsonde (1);
- eine Sende/Empfangsvorrichtung (2) zur Aussendung einer Ultraschallwelle von der Ultraschallsonde sowie zum Empfang eines Signals, das der Ultraschallwellenübertragung entspricht;
- eine Übertragungstärkesteuervorrichtung (3) zur Steuerung der Ultraschallwellenübertragung, so dass sie eine Stärke hat, bei der das Kontrastmittel für eine Anzahl von Schallstrahlen, die einen ersten Frame bilden, dispergiert wird, und dass sie eine Stärke hat, bei der das Kontrastmittel für die anderen Schallstrahlen, die den ersten Frame bilden, nicht dispergiert wird;
- wobei die Übertragungstärkesteuervorrichtung (3) die Ultraschallwellenübertragung so steuert, dass ein zweiter Frame durch die Ultraschallwellenübertragung bei einer Stärke gebildet wird, bei der das Kontrastmittel für alle Schallstrahlen, die den zweiten Frame bilden, nicht dispergiert wird,
- eine Bilderzeugungsvorrichtung (5, 6, 7) zur Erzeugung eines Bildes aus den empfangenen Signalen,
- wobei die Übertragungstärkesteuervorrichtung (3) so bedient werden kann, dass sie wiederholt die ersten und zweiten Frame generiert und die zweiten Frame zwischen die ersten Frame einschiebt.
6. Ultraschall-Diagnostikgerät gemäß Anspruch 5, **dadurch gekennzeichnet, dass** die Übertragungstärkesteuervorrichtung (3) die Übertragung der Ultraschallwellen so steuert, dass eine Zeitfestlegung der Ultraschallwellenübertragung für den ersten Frame und eine andere Zeitfestlegung der Ultraschallwellenübertragung für einen späteren der ersten Frames eine Zeitdifferenz aufweisen, die auf dem Herzschlag beruht.
7. Ultraschall-Diagnostikgerät gemäß Anspruch 6, **dadurch gekennzeichnet, dass** die Übertragungstärkesteuervorrichtung (3) die Übertragung der Ultraschallwellen so steuert, dass in dem ersten Frame mindestens zwei im Abstand zueinander liegende Schallstrahlen vorhanden sind, für die eine Ultraschallwelle bei einer Stärke übertragen wird, bei der das Kontrastmittel dispergiert wird.
8. Ultraschall-Diagnostikgerät gemäß einem der Ansprüche 5 bis 7, **dadurch gekennzeichnet, dass** die Übertragungstärkesteuervorrichtung (3) so angeordnet ist, dass sie die Ultraschallwellenübertragung so steuert, dass sie eine Stärke hat, bei der das Kontrastmittel für eine bestimmte Tiefe dispergiert wird, und eine Stärke hat, bei der das Kontrastmittel für andere Tiefen nicht dispergiert wird.

Revendications

1. Procédé d'imagerie par ultrasons comprenant les étapes consistant à :
- transmettre une onde ultrasonore avec une puissance destinée à disperser l'agent de contraste pour un certain nombre de faisceaux soniques qui forment une première trame et transmettre une onde ultrasonore avec une puissance

- ce destinée à ne pas disperser l'agent de contraste pour les autres faisceaux sonores qui forment la première trame ;
transmettre une onde ultrasonore avec une puissance destinée à ne pas disperser l'agent de contraste pour tous les faisceaux soniques qui forment une deuxième trame ;
produire une image à partir des signaux reçus qui correspondent aux transmissions d'ondes ultrasonores ;
répéter les étapes de transmission des ondes ultrasonores pour former les première et deuxième trames ; et
intercaler les deuxièmes trames entre les premières trames.
2. Procédé d'imagerie par ultrasons selon la revendication 1, dans lequel un minutage de transmission d'onde ultrasonore pour la première trame, et un autre minutage de transmission d'onde ultrasonore pour une première trame ultérieure ont une différence temporelle qui est basée sur le battement cardiaque.
3. Procédé d'imagerie par ultrasons selon la revendication 1, dans lequel les premières trames comprennent au moins deux faisceaux soniques espacés pour lesquels une onde ultrasonore est transmise avec une puissance destinée à disperser l'agent de contraste.
4. Procédé d'imagerie par ultrasons selon l'une quelconque des revendications 1 à 3, dans lequel l'étape de transmission d'une onde ultrasonore avec une puissance destinée à disperser l'agent de contraste pour une première trame se fait à une puissance prévue pour disperser l'agent de contraste sur une certaine profondeur, et dans lequel le procédé comprend le fait de transmettre une onde ultrasonore avec une puissance destinée à ne pas disperser l'agent de contraste pour les autres profondeurs.
5. Appareil de diagnostic par ultrasons comprenant :
- une sonde à ultrasons (1) ;
 - un moyen de transmission/réception (2) pour transmettre une onde ultrasonore à partir de ladite sonde à ultrasons et pour recevoir un signal qui correspond à la transmission d'onde ultrasonore ;
 - un moyen de contrôle de puissance d'émission (3) pour commander la transmission d'onde ultrasonore de façon qu'elle ait une puissance destinée à disperser l'agent de contraste pour un certain nombre de faisceaux soniques qui forment une première trame et de façon qu'elle ait une puissance destinée à ne pas disperser l'agent de contraste pour les autres faisceaux soniques qui forment la première trame ;
dans lequel ledit moyen de contrôle de puissance d'émission (3) commande la transmission d'onde ultrasonore de façon qu'une deuxième trame, qui est formée par la transmission d'onde ultrasonore avec une puissance destinée à ne pas disperser l'agent de contraste pour tous les faisceaux soniques qui forment la deuxième trame ;
un moyen de production d'image (5, 6, 7) pour produire une image à partir des signaux reçus ;
dans lequel le moyen de contrôle de puissance d'émission (3) est utilisable pour générer de façon répétée les première et deuxième trames et intercaler les deuxièmes trames entre les premières trames.
6. Appareil de diagnostic par ultrasons selon la revendication 5, dans lequel ledit moyen de contrôle de puissance d'émission (3) commande la transmission d'onde ultrasonore de façon qu'un minutage de transmission d'onde ultrasonore pour la première trame, et un autre minutage de transmission d'onde ultrasonore pour une première trame ultérieure ont une différence temporelle qui est basée sur le battement cardiaque.
7. Appareil de diagnostic par ultrasons selon la revendication 6, dans lequel ledit moyen de contrôle de puissance d'émission (3) commande la transmission d'onde ultrasonore de telle manière qu'il y a dans lesdites premières trames au moins deux faisceaux soniques espacés pour lesquels une onde ultrasonore est transmise avec une puissance destinée à disperser l'agent de contraste.
8. Appareil de diagnostic par ultrasons selon l'une quelconque des revendications 5 à 7, dans lequel le moyen de contrôle de puissance d'émission (3) est adapté pour commander la transmission d'onde ultrasonore de façon qu'elle ait une puissance destinée à disperser l'agent de contraste sur une certaine profondeur et qu'elle ait une puissance destinée à ne pas disperser l'agent de contraste pour les autres profondeurs.

FIG. 1
PRIOR ART

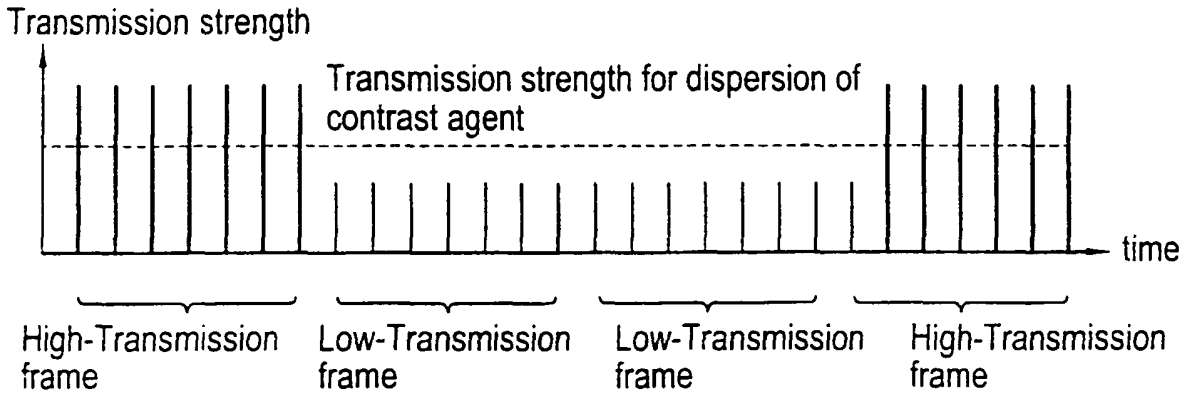


FIG. 2A
PRIOR ART

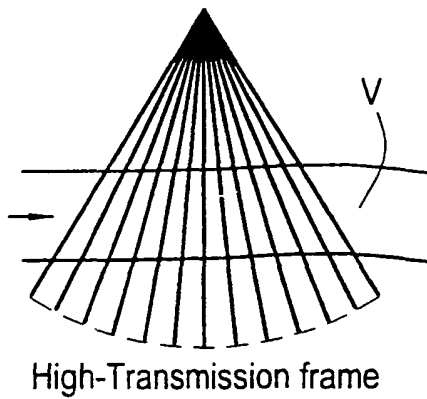


FIG. 2B
PRIOR ART

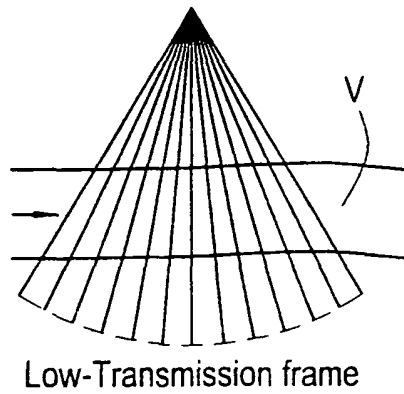


FIG. 3

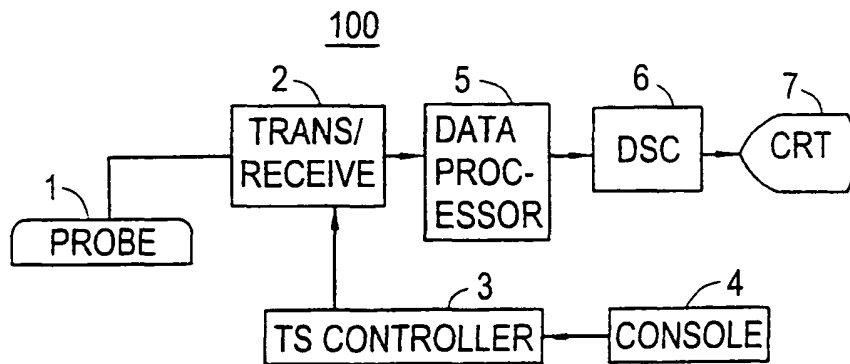


FIG.4A

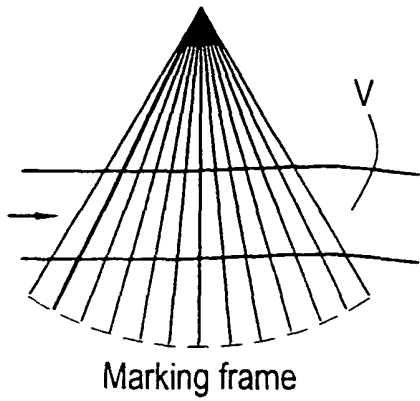


FIG.4B

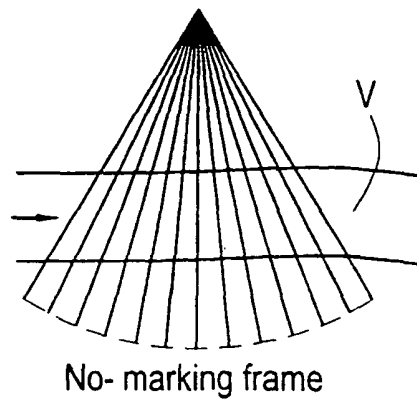


FIG. 5



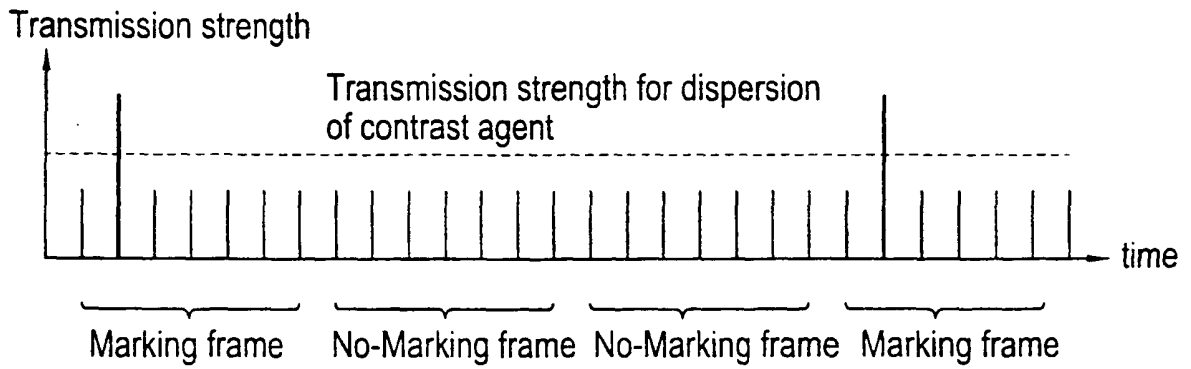


FIG. 6A

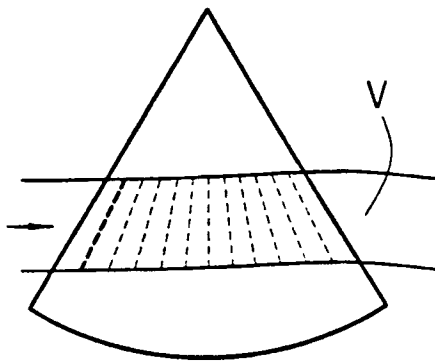


First marking frame

FIG. 6B

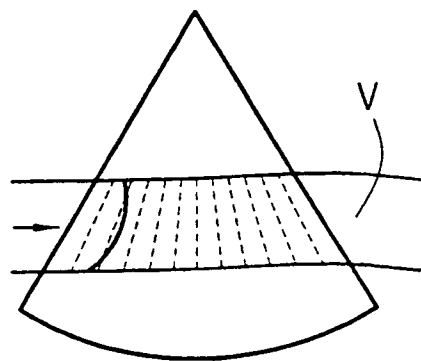

No-marking frame

FIG. 6C

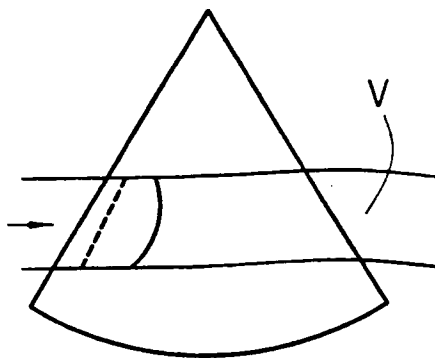

Second marking frame

FIG. 6D

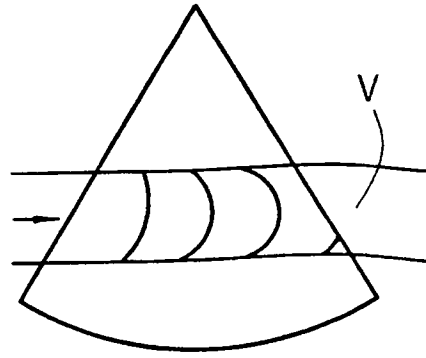


FIG. 7A

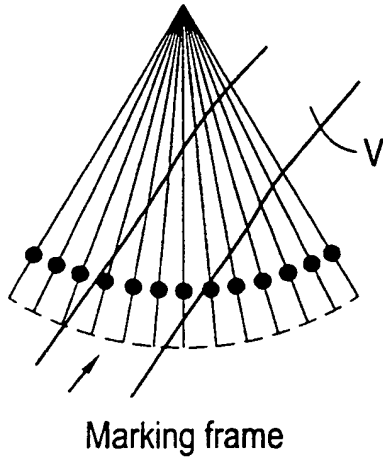


FIG. 7B

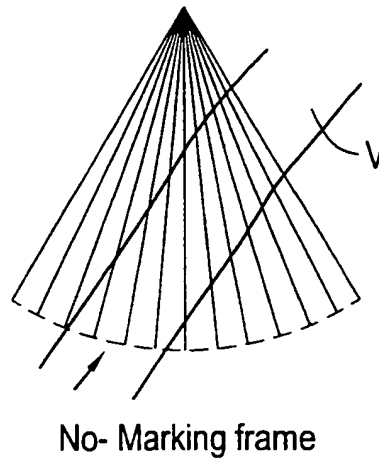


FIG. 8

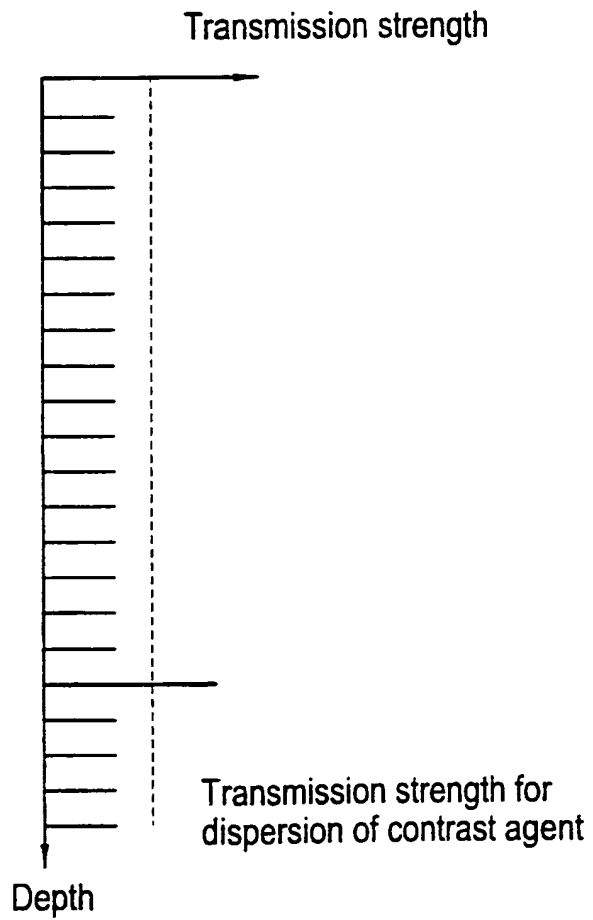


FIG. 9A

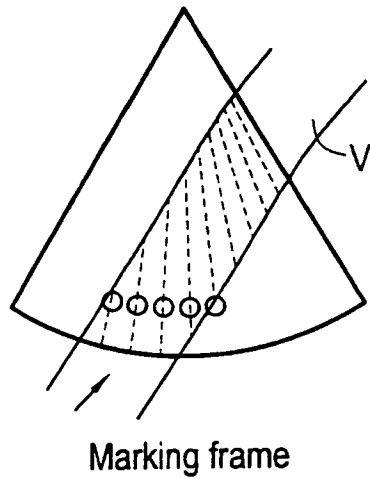


FIG. 9B

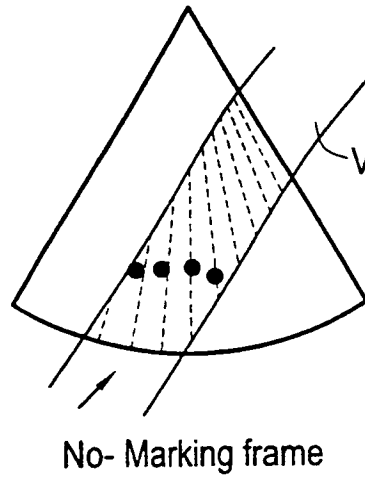


FIG. 9C

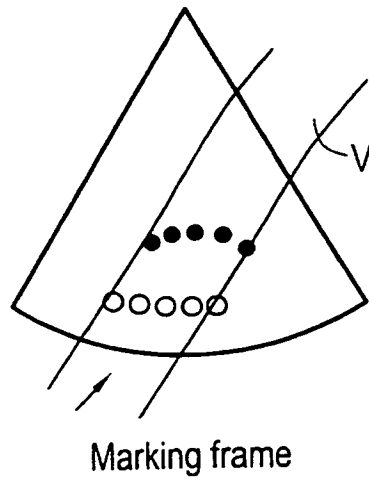


FIG. 9D



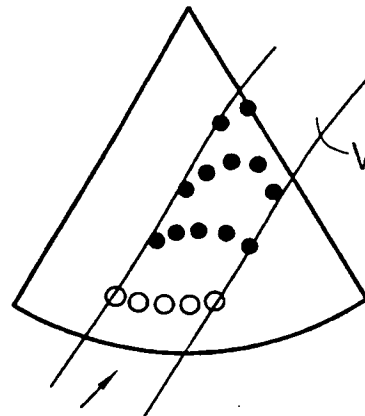


FIG. 10A

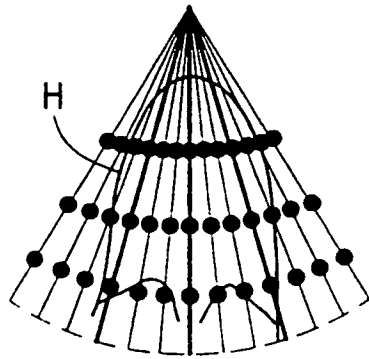


Marking frame

FIG. 10B

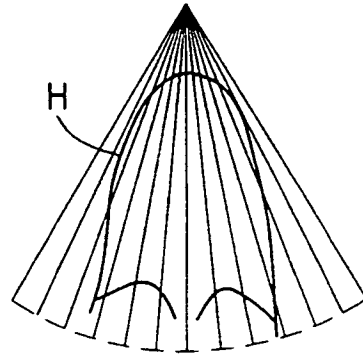

No-Marking frame

FIG. 11

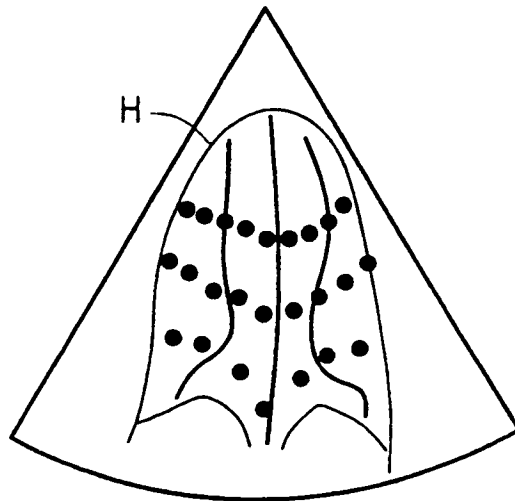

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 9908599 A [0002]

专利名称(译)	超声成像方法和超声诊断设备		
公开(公告)号	EP1180974B1	公开(公告)日	2008-01-16
申请号	EP2001912972	申请日	2001-02-23
申请(专利权)人(译)	GE医疗系统的全球技术公司LLC		
当前申请(专利权)人(译)	GE医疗系统的全球技术公司LLC		
[标]发明人	HASHIMOTO HIROSHI		
发明人	HASHIMOTO, HIROSHI		
IPC分类号	A61B8/00 A61B8/06 A61B8/14 G01S7/52 G01S15/89		
CPC分类号	A61B8/06 A61B8/481 G01S7/52038 G01S7/52041 G01S7/52066 G01S7/52073 G01S15/8979		
优先权	2000063853 2000-03-08 JP		
其他公开文献	EP1180974A1		
外部链接	Espacenet		

摘要(译)

超声波诊断装置以这样的强度发射超声波，以便将造影剂分散成多个声束的一部分，所述声束形成一个帧并且其强度使得不会将造影剂分散到其他声束中从而产生图像。对于来自超声波传输的接收回波信号的标记帧，随后连续发射超声波，其强度使得不会使所有声波束的造影剂分散，从而连续产生无标记帧的图像，并且在这样的时间之后视野中存在流量范围的长度，为另一个标记帧生成图像。重复这些操作以显示超声图像，通过该超声图像可以一目了然地识别血流的时间变化。

