

(19)



(11)

EP 1 253 855 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
10.03.2010 Bulletin 2010/10

(21) Application number: **01902000.7**

(22) Date of filing: **10.01.2001**

(51) Int Cl.:
A61B 8/08 ^(2006.01) **A61B 19/00** ^(2006.01)

(86) International application number:
PCT/US2001/000957

(87) International publication number:
WO 2001/058359 (16.08.2001 Gazette 2001/33)

(54) **ULTRASONIC IMAGER**

ULTRASCHALLBILDGERÄT

IMAGEUR A ULTRASONS

(84) Designated Contracting States:
DE ES FR GB

(30) Priority: **11.02.2000 US 502722**

(43) Date of publication of application:
06.11.2002 Bulletin 2002/45

(73) Proprietor: **Zanelli, Claudio I.**
Menlo Park, CA 94025 (US)

(72) Inventor: **Zanelli, Claudio I.**
Menlo Park, CA 94025 (US)

(74) Representative: **Bayliss, Geoffrey Cyril et al**
Boult Wade Tennant
Verulam Gardens
70 Gray's Inn Road
London WC1X 8BT (GB)

(56) References cited:
WO-A-96/25881 US-A- 5 515 853

EP 1 253 855 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionField of the Invention

[0001] The present invention relates to ultrasonic imaging. More particularly, the present invention relates to creating sectional views from volumetric ultrasound data and superimposing positional data for an interventional device, such as a catheter.

Background of the Invention

[0002] Many medical procedures involve inserting a catheter, or other interventional device, into a patient for a variety of purposes. One such procedure is cardiac catheterization for an angiogram.

[0003] To observe the condition of blood vessels within the heart, radio-opaque dye is injected into the bloodstream through the catheter and an x-ray image is taken. Typically, this procedure involves inserting a catheter into an artery in the patient's groin area and guiding the catheter through the arterial system and the aorta to the heart. In order to position the catheter and monitor its location within the patient, one or more x-ray images may be taken prior to injecting dye for the angiogram.

[0004] A catheter may be directly visible in an x-ray image, however, a heart typically is not. In order to determine the location of the catheter relative to the heart, dye may be injected through the catheter into the bloodstream. The dye acts as a contrasting agent allowing the heart to be located, by imagine the dye flowing through it. The image of the heart is then "frozen" at a point in time when the dye location (and concentration), provides the best image. Often, this snapshot image of the heart is traced on a transparent overlay which is then superimposed on a display monitor. After the dye concentration decreases, the overlay may be used to track the catheter location and movements relative to heart, as indicated by the overlay. There are two disadvantages to this process. First, the image of the heart, made visible with the dye, is only temporary, requiring the overlay to track the catheter movement. Second, if the patient's position changes, the heart imaging must be repeated.

[0005] In addition to locating a catheter relative to a heart for an angiogram, there are many other medical procedures where an interventional device is inserted into a patient. In most, if not all, such procedures, locating and positioning the interventional device within a patient is extremely important

[0006] Multiple views, or x-ray orientations, of a patient are often desirable to visualize objects and locations in three dimensions. Although there are many possible combinations of such views, some are favored by medical personnel for particular procedures. For cardiac imagine, the right anterior oblique (RAO) and the left anterior oblique (LAO) views are common. Figure 1 shows a schematic sectional depiction of a prone patient 10 and x-ray sources 12 and 14. The RAO and LAO views are taken from the patient's right and left, respectively, of the anterior (front) of the heart. The oblique angle, shown as angles 16 and 18, is the measure of how far off the vertical an x-ray source is oriented. The multiple views are often taken with a single x-ray source that is repositioned between positions 12 and 14. An imaging system that readily presents RAO and LAO views allows medical personnel to view images in a familiar format, as this is what is presently standard in the art. Multiple preferred views for other procedures might similarly be pre-defined.

[0007] There are problems with present practices. First, x-rays and fluoroscopy produce radiation, and the affect of this radiation over the long term may be harmful. This is especially true for the medical personnel subjected to repeated radiation exposures over the course of an entire career.

[0008] In addition, the radio-opaque dye may harm the patient. For example, an angiogram is often performed on patients with serious heart problems. Injecting chemicals that may cause sensitivity, or an allergic reaction, directly into the heart of such a patient may cause a serious problem, and there is the possibility of kidney damage from the dye.

[0009] Finally, x-ray techniques require complex x-ray equipment and the costly overhead associated with such equipment. While this may not be a primary concern in a well equipped modern hospital, is of concern in less developed or remote locations.

[0010] Ultrasound based imaging methods offer some potential advantages over x-ray based imaging methods. Ultrasound methods do not expose the patient or medical personnel to radiation and may reduce or eliminate the need for costly x-ray equipment. Also, the ability of ultrasound methods to directly image soft tissue and blood vessels, without the need for radio-opaque dye as a contrasting agent, eliminates the potential dye-related harms to a patient.

[0011] It would be desirable to have an imaging system that could eliminate, or serve as a partial substitution for, x-ray and fluoroscopy methods of imagine in procedures such as angiography and tissue biopsies. Preferably, such a system would present medical personnel with multiple views that are displayed simultaneously.

[0012] U.S. Patent No. 4,173,228, issued to Steenwyk and Childress on November 6, 1979, describes a catheter locating device ("the '228 patent"). The '228 patent uses an induction coil adjacent to the catheter tip, and a remote sensing device to monitor the amplitude and phase of signals induced in the coil, as a means of detecting the catheter location. However, an electrical signal from an induction coil is not well suited for detection by ultrasound imaging

equipment. The '228 patent does teach one technique for locating a catheter, but it lacks the ability to directly map that location to a 3-D ultrasonic image of tissues within the body. Instead, such a device determines a catheter location relative to a position on the skin surface and a depth estimate, based on the magnitude of the signal received at the skin surface. It would be desirable to locate the catheter relative to internal body tissues, not the skin.

[0013] U.S. Patent No. 5,515,853, issued to Smith, et al. on May 14, 1996, describes a 3-D ultrasound tracking system based on triangulation ("the '853 patent"). Using a network of at least four piezoelectric transducers exchanging signals, and an integrated personal computer (PC) as a digital controller, the 853 patent accurately measures the relative distances between the transducers. However, like the '228 patent discussed above, an apparatus based on the '853 patent lacks the ability to map the location of a catheter to a 3-D ultrasonic image of tissue within the body. Instead, the reference frame for catheter location information is the location of other piezoelectric transducers. For example, a series of transducers contained in a chest harness around a patient may be used to triangulate the position and orientation of a catheter relative to the chest harness, by measuring the distances to transducers mounted in the catheter. The '853 patent does briefly mention the possibility of "overlaying" transducer location information on a video loop, created from x-rays or ultrasound, to facilitate visualization of the catheter location. However, there is no teaching of how this overlay process might be performed. In contrast, an embodiment of the present invention is directed to describing the catheter location relative to tissue within the body in one or more 2-D views.

[0014] U.S. Patent No.'s 5,817,022 and 5,868,673, ("the '022 and '673 patents") issued to Vesely on October 6, 1998, and on February 9, 1999, respectively, are both continuations-in-part from the application that became the '853 patent. Both also claim 3-D ultrasound tracking of interventional medical instruments by triangulating between a transducer attached to the medical instrument and a network of transducers either inside a patient's body or on the body surface. It would be desirable to simplify the apparatus so that a network of transducers is not required.

[0015] The '022 patent locates a medical instrument relative to the network of transducers in 3-D, and then displays a 2-D ultrasound image within the 3-D coordinate system. The '022 patent describes a "imaging modality system", that may acquire 2-D, 3-D or 4-D image data, an "image registration system" to register the position the [medical] instrument within the image data and a "user interface" to perform a desired function, such as selecting a particular view for display. However, there are no detailed descriptions of these elements, or teachings which would permit one of ordinary skill in the art to create a system combining such elements.

[0016] The '673 patent describes a system for performing surgery while tracking the location of a medical device relative to a network of transducers, on or within the body. The medical device location is then mapped to the network of transceivers, but not directly to any portion of the body tissue.

[0017] Ultrasound image data for an object, such as a heart, consists of the "echodensity" sampled at multiple locations within an object. This echodensity can be thought of as somewhat equivalent to the color or intensity of a visual image. The echodensity is a function of the sound velocity within the tissue, as well as the tissue density. Although a 3-D image of echodensity, with continuous gradations along three dimensions, may lack the clarity of the sharp edges in a solid model, the gradations contain a significant amount of information about the tissue. A solid modeling approach to presenting a 3-D ultrasound image typically uses a threshold value. That is, all echodensity values are divided into two bins, those above and those below the threshold. Values above the threshold are opaque and those below are transparent. This threshold technique adds clarity to the wide variations of the "murky" echodensity data, by distinguishing solid features within the data, at the expense of the detail stored in those many values.

[0018] TomTec Imaging Systems, formerly of Boulder, CO, now TomTec Imaging Systems GmbH of Munich, Germany, produced a video tape describing a 3-D ultrasound imaging system ("the TomTec system"). TomTec Imaging systems, Clinical Three-Dimensional Echocardiography, VHS/NTSC, 19:20, 040-012. 0, 07-96 (video tape). The TomTec system creates a 3-D cardiac image, with the use of a ultrasound transducer in the form of an endoscope, and produces an image of the surfaces of the heart, essentially a solid model. That is, the surface of the heart is displayed without any information about the internal muscle tissue. The TomTec system does not appear to have been commercially successful.

[0019] US 5,515,853 discloses a method and apparatus for simultaneous measurement of multiple distances by means of networked piezoelectric transducers. The use of high frequency digital counters enables the propagation delay between the activation of an ultrasonic transducer and the reception by similar transducers to be defined. By alternating the duty cycle between transmit and receive modes, the system can track and triangulate the three-dimensional positions for each transducer.

[0020] WO 96/25881 discloses a method for generating quasi real-time feedback for the purpose of guiding surgical, therapeutical or diagnostical procedures by means of ultrasound imaging. The location of a surgical tool, a therapeutic radiation field or a diagnostic energy field is related to the coordinate system of an intraoperative 2-D and/or 3-D ultrasound imaging system, a 2-D plane of the volumetric information being extracted and displayed.

SUMMARY OF THE INVENTION

[0021] According the present invention there is disclosed an apparatus which displays ultrasound 3-D volumetric

object data and 3-D interventional device data by projection onto a 2-D plane as claimed in the appended claims

[0022] The ultrasound imaging system of the present invention superimposes sectional views created from volumetric ultrasound data and the location data for an intervention device, such as, but not limited to, a catheter. The position of catheter may be shown, in one or more views, relative to organs and tissues within a body as the catheter is moved, The catheter positional data is updated continuously and is superimposed on tissue images that may be updated less frequently, resulting in real-time or near real-time images of the catheter relative to the tissues.

[0023] The superimposed images allow medical personnel to perform procedures such as angiograms with minimal exposure of patients to x-rays and contrasting dye. However, the look and feel of the familiar fluoroscopy-like imaging may be maintained.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024]

Figure 1 is a schematic sectional depiction of a patient and x-ray-equipment.

Figure 2 is a diagram of a 3-D image space

Figure 3 is a schematic diagram of point location among regularly spaced image data samples.

Figure 4 is a schematic diagram of irregularly spaced image data samples.

Figure 5 is a schematic diagram of a control panel.

Figure 6 is a flow chart of the imaging process.

DETAILED DESCRIPTION

[0025] The present invention is directed at an apparatus for superimposing an image of an interventional medical device, such as a catheter, and a three-dimensional (3-D) ultrasound image of an organ or tissues, such as a heart, and creating one or more projections from the superimposed image data. The two sets of image data may be updated at the same or different frequencies. The image of the medical device may be updated more frequently to show its current location, as the device is guided or repositioned within a patient by medical personnel. The projections made from the superimposed images preferably reflect the current location of the medical device, and depending on the frequency of updating the image of the organ or tissues, may also show a real-time image of such organ or tissues.

[0026] The present invention may be used with a wide variety of interventional medical devices, such as, but not limited to, catheters, probes, cannulas, stylets, and needles, and is not intended to be limited to use with any particular interventional medical device. For convenience, this disclosure will use the term catheter, instead of the more generic term intervention medical device, since the example, described is related to the use of the apparatus in cardiac procedure; however, this is not meant to imply any limitation on the scope of the invention.

[0027] The present invention may be used in connection with ultrasound images of any organ, portion of an organ, or group of organs, and the present invention is not intended to be limited, to any particular image subject matter. There are situations in which it may be desirable to use the present invention in conjunction with x-ray methods. For example, if an ultrasound transducer is positioned so that only locations in the vicinity of the heart can be imaged, x-ray methods might be used to track a catheter from its insertion point near the groin until it comes into view with the transducer.

[0028] In an alternative arrangement an apparatus may be used with "4-D ultrasound images". That is, repetitive sequences of 3-D images in time, such as, but not limited to, images of a heart beating as it goes through one or more cycles. The 4-D ultrasound images may be depicted and displayed as repetitive sequences of images, or cine loops. Alternatively, a single point in the time sequence may be selected, effectively transforming the 4-D image into a 3-D image. Preferably, updates of the catheter location are allowed at a frequency independent of the repetitive sequence frequency and the frequency of individual image frames within the sequence. This disclosure will use the term "dynamic display" when 4-D image data is distinguished from 3-D image data. Otherwise, the term "image data" may apply to either 3-D or 4-D image data.

[0029] The output of the present invention is one or more projections created from the superimposed image data. Although the projections are typically displayed on one or more cathode ray tube (CRT) monitors, the present invention may output the projections to any type of graphic display device(s), such as a thin film transistor flat screen display, or to a graphic output file for storage or further image processing. The present invention is not intended to be limited to use with any particular type of graphic display device or output file format. Multiple projections, typically taken from

differing orientations with respect to the image data, are often beneficial in visualizing locations in a 3-D space. An embodiment of the present invention uses two standard views, right anterior oblique (RAO) and left anterior oblique (LAO) as "default" projection orientations.

[0030] As the trend towards faster computer processors continues, eventually the present invention will allow for real-time or near real-time updates of projections created from 3-D image data. At present, the acquisition of image data, and the projection processing discussed below, takes too long for such real-time updates. Given the current constraint on computing power, the present invention is preferably used in an environment where the patient is immobilized. This permits use of a single set of image data that may be used continuously while a catheter is moved relative to the patient and the image data.

[0031] For purposes of the examples described below, references to a dynamic display embodiment of the present invention, presumes that the position of the organs and tissue return to the same position and orientation within a patient at the end of each repetitive sequence, or cycle. That is, the cycle may consist of "local" movement but no "global" movement relative to the immobilized patient is anticipated. In contrast, movement of the catheter is anticipated, so the location of the catheter is updated frequently, preferably in real-time. The updated catheter location is then superimposed on the relatively static organ or tissue image data before the projections are created.

[0032] Collecting 3-D ultrasound image data, while certainly not a trivial procedure, is known to those of skill in the art, and is not intended to be an element of the present invention. Rather, the present invention uses such data, however collected, as input. U.S. Patent No. 5,181,514, issued to Salomon, et al. on January 26, 1993, describes a transesophageal echo cardiography transducer device which may be used to collect 3-D ultrasonic image data ("the '514 patent"). This device, with a rotatable ultrasound transducer array, may be inserted into a patient's esophagus and positioned adjacent to the heart. A motor and drive mechanism, which remains external to the patient, is used to control the probe with the transducer array and obtain 3-D image data. A transesophageal transducer, such as described in the '514 patent, might be used to collect cardiac image data. As the present invention is not limited to any particular apparatus for collecting image data, it is intended that as advances are made in ultrasound data collection, the present invention may utilize such improved image data as input.

[0033] Image data will preferably take the form of the 3-D array:

$$I(x, y, z)$$

Or, in the case of image data for a dynamic display, in the form of the 4-D array.

$$I(x, y, z, t)$$

Where I represents the echodensity, or "intensity," of the ultrasound image at a point defined by the 3-D Cartesian coordinates x , y and z . The particular choice of orientation for the x , y and z axes does not affect the present invention. Preferably, the axis orientation is used consistently. For a dynamic display, t refers to the instant in time representing when the echodensity data was sampled within the repetitive sequence. Image data may be collected in different formats, or coordinate systems, and then converted to the preferred format using transformation formulae known to those of ordinary skill in the art.

[0034] In one embodiment of the present invention the I values at each sampled point in space will be binary representations of the echodensity values. The values may be in either integer or floating point format. Although integer values are typically better suited to efficient mathematical algorithms, this efficiency may be effectively lost if numerical interpolation methods using floating point values are selected for integration. The need for numerical interpolation and integration will be further explained below. The I values, for monochromatic embodiments of the present invention, will preferably map to a specific gray scale value that will be used to display the image. For example, eight bit integer I values may represent 256 gray scale values, from 0 to 255. Floating point I values may be grouped in ranges, each of which corresponds to a gray scale resolution of the display. The range of gray scale resolution values chosen will depend on both the characteristics of the display (where higher resolution produces better images) and the processing speed of the image processing device (where higher resolutions require more calculations per pixel). Gray scales for displaying images are known to those of ordinary skill in the art. The present invention is not intended to be limited to any particular gray scale resolution.

[0035] In addition to the number of gray scale values, or gray scale resolution, the spatial resolution of the input image data also effects both the quality of the display and the number of calculations required. That is, image data sampled at many points in 3-D space will generally produce a better image than the same object sampled at fewer points. The trade off being that the additional image sample points may require more calculations, which typically requires a more

complex and rapid handling system or slows the image processing.

[0036] Although techniques for collecting the ultrasound image data are not within the scope of the present invention, and image data is treated as input to the present invention, an embodiment of the present invention does allow a user to call for an update of image data as needed. For example, if the medical personnel detect that a patient has shifted, changing the relative position of the object being image and the catheter, new $I(x, y, z)$ values may be collected. In another embodiment of the present invention, a patient movement that is more than a pre-defined threshold amount may trigger a call for updating the image data. As long as there is little or no relative movement between the object being image and the catheter, there is no need to update the image data. Preferably, the catheter is located using the same apparatus used to collect the 3-D ultrasound image data, $I(x, y, z)$. The format of the catheter location data will depend somewhat on the type of catheter used, as well as the associated means of locating the catheter.

[0037] The catheter location may correspond to the direct echodensity data depicting the image of the catheter, including any image enhancement from active catheter devices such as a vibration mechanism. U.S. Patent No. 5,343,865, issued to Gardineer and Vilkomerson on September 6, 1994, describes a catheter vibrating mechanism ("the '865 patent"). A vibrating mechanism, such as described in the '865 patent, may enhance the visibility of a catheter, or other interventional medical device, that is attached to it in an ultrasound imaging system. The present invention is preferably used with such an active catheter. Potential benefits include faster imaging of the location, a clearer image, and such an active catheter reduces the required sensitivity for the imaging system. The present invention is not, however, intended to be limited to use with an active catheter, or any particular type of active catheter system. The image of the catheter location may also be enhanced, for better visibility, through techniques such as brightening, increasing the contrast, or enlarging the catheter image before superimposing the catheter location data and the 3-D image data. With some embodiments of the present invention, a false image, or icon, may be used in place of the catheter image data. Such techniques will be further described below. It is very important, however, that the catheter location be matched closely to the coordinate system of the image data.

[0038] In-order to create projections of the 3-D image data, one or more projection planes must be defined. **Figure 2** depicts a 3-D space or volume 22. Volume 22 is the portion of space containing the imaged objects, such as organs within a patient's body cavity, and could take virtually any 3-D shape. Volume 22 uses (global) axes 24 to define a Cartesian coordinate system for orientation and measurement. A 2-D plane 26 is selected relative to volume 22, with (local) axes denoted as (u, v) . Typically, plane 26 is defined by a unit vector $\hat{n}$, normal to (u, v) . Unit vector $\hat{n}$ can be defined as:

$$\begin{aligned}\hat{n} &= (n_1 \hat{x} + n_2 \hat{y} + n_3 \hat{z}) \\ &= (n_1, n_2, n_3)\end{aligned}$$

and, because $\hat{n}$ is a unit vector:

$$1 = \sqrt{n_1^2 + n_2^2 + n_3^2}$$

Where $\hat{x}$, $\hat{y}$ and $\hat{z}$ are unit vectors along the x , y and z axes, respectively, and (n_1, n_2, n_3) are the direction cosines of $\hat{n}$. Those of ordinary skill in the art will recognize that there are many mathematically equivalent ways of defining plane 26 and its normal vector $\hat{n}$.

[0039] Imposing the condition:

$$\hat{u} \perp \hat{z}$$

the directions of unit sectors $\hat{u}$ and $\hat{v}$ can be defined, using the constant R , as;

$$\hat{u} = R(-n_2, n_1, 0)$$

where;

$$R = \frac{I}{\sqrt{n_1^2 + n_2^2}}$$

and;

$$\hat{n} = R (-n_1 n_3, -n_2 n_3, n_1^2 + n_2^2)$$

[0040] The construction of the projection on plane 26, can be calculated by performing the integration:

$$P(u, v) = \int_{\bar{x}} I(x, y, z) dS$$

[0041] That is, the image data, $I(x, y, z)$, is summed along the line $\bar{x}$ onto $P(u, v)$, where the vector $\bar{x}$ is an integrating line parallel to $\hat{n}$ and is defined by the equation:

$$\bar{x} = \bar{x}_0 + S \hat{n}$$

[0042] The starting point, $\bar{x}_0$, is given by:

$$\bar{x}_0 = u \hat{u} + v \hat{v}$$

$$= R u (-n_1, n_1, 0) + R v (-n_2, n_2, -n_1 n_2, n_1^2 + n_2^2)$$

$$= R (-u n_1 - v n_2, u n_1 - v n_2, v(n_1^2 + n_2^2))$$

and,

$$S = k \sigma$$

where k is an integer and σ is the integration interval used for the numerical implementation.

[0043] S can be thought of as the thickness, or depth, of the image data used to create $P(u, v)$. In some embodiments of the present invention S , and the starting point $\bar{x}_0$, are set such that the projection is created from only a relatively thin slice of the image data $I(x, y, z)$. Preferably, the depth of the image data used in projection plane 26 is defined by the user along an axis parallel to $\hat{n}$.

[0044] The numerical implementation of the integration used to calculate $P(u, v)$ may require interpolation. That is, the vector $\bar{x}$ and integration interval σ may result in locations that do not directly coincide with any data sample locations in $I(x, y, z)$. Referring now to **Figure 3**, which depicts a set of image data values 28, corresponding to image sample locations within $I(x, y, z)$. Values 28 are shown, for clarity, as regularly spaced in three dimensions, although the same principles apply for irregularly spaced image values. Location 30 is a point along $\bar{x}$ used in the calculation of $P(u, v)$, that does not correspond to the location of any value 28. Those of ordinary skill in the art will recognize that there are many techniques available for assigning a data value to location 30. A few of these techniques are, in increasing order of complexity, matching the value of the "nearest neighbour", averaging nearby values and computing weighted averages. The present invention, however, is not intended to be limited to any particular interpolation technique.

[0045] U.S. Patent No. 5,226,113, issued to Cline, et al. on July 6, 1993, describes using reverse ray casting to project volumetric images onto an image plane rotated at any arbitrary angle ("the '113 patent"). The present invention takes

3-D volumetric image data, as one input, and projects 3-D image data onto one or more image planes, which may be rotated relative to the axes of the 3-D image data. The present invention may use the projection techniques of the '113 patent, or any another technique, and is not intended to be limited to any particular method of projecting 3-D image data to create a 2-D view in an image plane. U.S. Patent No. 5,865,750, issued to Hatfield, et al. on February 2, 1999, also described using reverse ray casting to project volumetric images ("the '750 patent"). Like the '113 patent, the technique described by the '750 patent may be used by an embodiment of the present invention to project 3-D image data.

[0046] The above projection creation procedure may be repeated for each desired projection display. An embodiment of the present invention allows the user to select a first projection, corresponding to either an RAO or a LAO orientation, at a user selected number of degrees off the vertical, with a second projection (default) orientation corresponding to the other. Preferably, defining the direction of the second projection orientation would require very little input from the user, and instead would use translations from the first projection orientation to orient the second.

[0047] Presenting projections to medical personnel in a familiar format, such as RAO and LAO orientations, is merely one capability of the present invention. Unlike x-ray images taken from only one or two orientations, the 3-D image data $I(x, y, z)$ used with the present invention may create virtually any view(s) a user might select. For example, a projection could be created of the tissue in front of a catheter, as viewed along the axis of the catheter.

[0048] The simplest form for the image data, is equally spaced image samples in each of the x , y and z directions. Unequally spaced, or irregularly spaced, samples may also be used with the present invention although the calculations may become more complex, and time consuming. Irregularly spaced samples may also be pre-processed and converted to equally spaced image samples, by any one of a variety of techniques, for use by an embodiment of the present invention. An embodiment of the present invention may pre-process irregularly spaced $I(x, y, z)$ data values. Referring now to **Figure 4**, which depicts an irregularly spaced set of image data values 28, relative to a regular spacing location template 32. Data values 28 may be used to interpolate, or create, data samples on template 32. Similar to the interpolation discussed above, the present invention is not intended to be limited to any particular apparatus interpolating or translating data values 28. Some projection algorithms may benefit from such a pre-processing of irregular image data into regularly spaced locations.

[0049] A control panel for an embodiment of the present invention is shown in Figure 5. Joysticks 34 are used to choose the orientation of one or more projections, and pairs of slide bars 36 choose the upper in lower limits of the depth of the projections. S. Brightness 38 and contrast 40 controls allow the user to adjust the display on one or more CRTs or other display devices. The present invention is not intended to be limited to any particular apparatus allowing a user to choose a projection orientation or control the displays. Although direction cosines are used in this disclosure to describe projection planes, it is not intended for a user to be restricted to inputting orientation information in that format.

[0050] In one embodiment of the present invention the location of the catheter is superimposed on the image data after the projection(s) have been created. Generally, the creation of projections. $P(u, v)$, from the image data file $I(x, y, z)$ is a relatively slow process. Although it is understood that the trend towards faster and less expansive computer processing will ease this constraint, at the present time the projections are created less frequently than in real-time. This means that as the catheter moves, first superimposing the catheter location and $I(x, y, z)$ and then creating one or more projections, $P(u, v)$, may introduce a time-lag in displaying actual catheter location. Unlike the image data file $I(x, y, z)$, which typically contains non-zero data samples at many thousands of locations corresponding to the entire volume of the imaged organs or tissues, the catheter location data will typically be relatively "sparse". That is, it will contain much fewer non-zero entries than $I(x, y, z)$. An embodiment of the present invention exploits the fact that the catheter location data is relatively sparse compared to $I(x, y, z)$, and superimposes the catheter location directly on the projection(s). In this way, the changing position of the catheter can be mapped onto the projection, without the need to re-create the projection from each data point within $I(x, y, z)$. In most cases, the relatively sparse catheter location data can be directly superimposed on projections in much less time than is required to create the projection from $I(x, y, z)$.

[0051] Figure 6 shows a flow chart of the imaging process where the intervention medical device location is superimposed 42 after the projection(s) are created 44, and then the projection with the device location is displayed 46. The process of locating the device position 48 is repeated frequently, preferably at a frequency close to the display monitor video refresh rate.

[0052] Re-starting the process, by obtaining updated images data 50, may be initiated by the user in situations such as where there is patient movement. With sufficient computer processing power, obtaining updated image data 50 may be repeated at predetermined frequency without user action.

[0053] The location of the catheter is preferably detected by the same ultrasonic image equipment that is used to create the image data, $I(x, y, z)$, using the same global Cartesian coordinate system. By using an active catheter system, such as the vibrating mechanism of the '865 patent, the "catheter image may be more easily detected, and distinguished from, the relatively passive surrounding environment. An embodiment of the present invention may also use one or more filters to further distinguish the active catheter image from background. Such filtering techniques are generally known to those of ordinary skill in the art.

[0054] The catheter image may take one of two preferred formats. First, it may match the format of the input file $I(x,$

y, z) with only a relatively limited number of non-zero entries. For the catheter image this file will be called $I_C(x, y, z)$. In this format, $I_C(x, y, z)$ will contain the echodensity values of the catheter, corresponding to the actual 3-D image of the catheter, as seen by the ultrasound transducer. As discussed above, the $I_C(x, y, z)$ values may be the post-filter echodensity data.

[0055] Alternatively, the catheter image may correspond to one or more sets of Cartesian coordinates, representing the coordinates of one or more locations on the catheter in 3-D space. That is, the actual ultrasound image of the catheter is not used, only the coordinates of one or more points that may be used to determine the catheter location, and perhaps its orientation.

[0056] Using two points on a catheter to locate and orient the catheter in space is known in the art, as illustrated by **Figure 9** in the '853 patent. An embodiment of the present invention includes assignable attribute data field for each coordinate, along with the coordinates of the one or more locations on the catheter. Such a data field may store an intensity value corresponding to an amount of ultrasonic energy detected, for use in creating false color displays of the catheter image.

[0057] Regardless of the format of the catheter location data, the present invention performs a transformation of that location data into the coordinates of the projection(s). For catheter image files in the $I_C(x, y, z)$ format, this process may resemble (mathematically) the creation of $P(u, v)$ from $I(x, y, z)$, only with a much sparser input file. The projected catheter image(s) $P_C(u, v)$ can then be directly superimposed on the image data $P(u, v)$. This procedure is repeated, or performed as multiple parallel tasks, for each projection orientation.

[0058] For catheter location data stored as coordinate(s), or coordinate(s) and attribute data, only the individual coordinates need to be transformed into the coordinate systems of the projections. That is, there is no need to perform numerical integration on the larger number of data locations making up the catheter image. Such a transformation of one or more points to the coordinate system of the projections may be performed relatively quickly, in either software or hardware. The output of the transformation system may be two (planar) coordinates for each point location in a given projection, and the values of the associated attribute data. Mapping a location symbol to a CRT display at the location of these two coordinates is straight forward, and known to those of ordinary skill in the art. The attribute data may also be used in conjunction with the location symbol. For example, "cross-hairs", or an arrow symbol, could be mapped onto the CRT display of each projection at the current location of the catheter in that projection, with the color of the symbol correlated to the magnitude of vibration detected in a vibrating catheter.

[0059] An embodiment of the present invention converts catheter image data in the form of a $-I(x, y, z)$ into one or more coordinates representing the catheter location in order to speed the data processing. The full ultrasound image of the catheter is sacrificed in such an embodiment, for the ease in processing data for only a few point locations. However, with one or two point locations, and the prior knowledge of the catheter geometry, there is no need to directly map the full catheter image to the display; all of the information can be carried by, or conveyed by, the symbols mapped directly to the monitors.

[0060] Unlike the projection data created from the image data $I(x, y, z)$, the superimposed catheter image does not require that the image intensities (gray scales) be accurately transformed unto the displays, only that the catheter locations be accurately transformed. It may be advantageous to modify the intensity of the catheter image, relative to the other image data, for display clarity. One embodiment of the present invention uses the catheter location as the center of projection depth when for creating the image for display.

[0061] Another embodiment of the present invention may use color image data files, where $I(x, y, z)$ is replaced by separate color space image files, such as $I_R(x, y, z)$, $I_G(x, y, z)$ and $I_B(x, y, z)$ corresponding to an image in RGB color space. Other color space formats may also be used, and the present invention, is not intended to be limited to any particular color space representation. Given this disclosure, those of ordinary skill in the art will recognize how the present invention may be adapted to work with such color images.

[0062] Although various embodiments are specifically illustrated and described herein, it will be appreciated that modifications and variations of the present invention are covered by the above teachings and are with the purview of the appended claims, without departing from the scope of the present invention. Moreover, the present invention may be implemented in software, firmware as well as in hardware, and in a broad range of computer architectures and is intended to be a general approach that includes a broad range of specific implementations.

Claims

1. An apparatus for displaying ultrasound three-dimensional volumetric object data and three-dimensional volumetric interventional device data onto a two-dimensional plane (26), comprising:

apparatus for storing a first volumetric data file, wherein said first volumetric data file includes a plurality of object intensity values ($I(x, y, z)$) obtained by direct measurement during an interventional procedure and a

second volumetric data file which includes a plurality of interventional device intensity values ($I_c(x, y, z)$) obtained by direct measurement at least once during the same interventional procedure;

means for defining a first projection plane (26) for displaying a first projection of object intensity values ($I(x, y, z)$) and interventional device intensity values ($I_c(x, y, z)$);

a first image projector adapted for creating a first two-dimensional projection image of said object on said first projection plane (26), each value ($P(u, v)$) of the first projection image of the object being obtained by summing the object intensity values ($I(x, y, z)$) along a line perpendicular to the first projection plane (26), and a two-dimensional projection image of said interventional device on said first projection plane (26), each value ($P_c(u, v)$) of the projection image of the interventional device being obtained by summing the interventional device intensity values ($I_c(x, y, z)$) along said line perpendicular to the first projection plane (26);

an interventional device locator for locating (48) said interventional device at a device location; and
a first superimposer for superimposing (42) said two-dimensional projection image of the interventional device and said two-dimensional projection image of the object on said first projection plane (26) to provide a first two-dimensional display image.

2. An apparatus in accordance with claim 1, further comprising:

means for defining a second projection plane adapted to display a second projection of said object intensity values ($I(x, y, z)$);

a second image projector adapted to provide a second projection image of the object on said second projection plane from said object intensity values ($I(x, y, z)$), each value of the second projection image of the object being obtained by summing the object intensity values ($I(x, y, z)$) along a line perpendicular to the second projection plane; and

a second superimposer for superimposing said two-dimensional projection image of the interventional device and said second projection image of the object to create a second two-dimensional display image.

3. An apparatus in accordance with claim 2, wherein said second two-dimensional display image is a view useful to medical personnel performing a procedure.

4. An apparatus in accordance with claim 1, wherein said first display image is a right anterior oblique (RAO) view of the object.

5. An apparatus in accordance with claim 2, wherein said second display image is a left anterior oblique (LAO) view of the object.

6. An apparatus in accordance with claim 1, wherein said first display image is a LAO view of the object.

7. An apparatus in accordance with claim 2, wherein said second display image is a RAO view of the object.

8. An apparatus in accordance with claim 1, further comprising:

means for specifying a range of said object intensity values ($I(x, y, z)$) in said first display image.

9. An apparatus in accordance with claim 2, further comprising:

means for specifying a range of said object intensity values ($I(x, y, z)$) in said second display image.

10. An apparatus in accordance with claim 8, wherein said first image range is centered on said interventional device location as measured along a vector perpendicular to said object projection plane.

11. An apparatus in accordance with claim 9, wherein said second image range is centered on said interventional device location as measured along a vector perpendicular to said object projection plane.

12. An apparatus in accordance with claim 1 or 2, further comprising a display image orientation control for defining a line perpendicular to a projection plane from a user input or, a display image orientation control for defining two lines from a user input, where one line is perpendicular to a first projection plane and the other line is perpendicular to a second projection plane.

13. An apparatus in accordance with claim 1, wherein said first superimposer is capable of updating said device location continuously.

14. An apparatus in accordance with claim 13, wherein said first superimposer is capable of updating said object intensity values ($I(x, y, z)$) in response to user signal.

15. An apparatus in accordance with claim 13, wherein said first image projector is capable of updating said object intensity values ($I(x, y, z)$) in real-time.

16. An apparatus in accordance with claim 1, wherein said interventional device locator is capable of responding to a transmitted signal from said interventional device.

17. An apparatus in accordance with claim 1, further comprising an output file generator for storing said first two-dimensional display image.

18. An apparatus in accordance with claim 2, further comprising:

means for defining a third projection plane for displaying a third projection of said object intensity values ($I(x, y, z)$) and interventional device intensity values ($I_c(x, y, z)$);

a third image projector adapted to create a third projection image of the object on said third projection plane, each value of the third projection image of the object being obtained by summing the object intensity values ($I(x, y, z)$) along a line perpendicular to the third projection plane; and

a third superimposer for superimposing said two-dimensional projection-image of the interventional device and said third projection image of the object to create a third two-dimensional display image.

Patentansprüche

1. Vorrichtung zum Anzeigen dreidimensionaler volumetrischer Ultraschall-Objektdaten und dreidimensionaler volumetrischer Eingriffsvorrichtungsdaten auf einer zweidimensionalen Ebene (26), umfassend:

eine Vorrichtung zum Speichern einer ersten volumetrischen Datendatei, wobei die erste volumetrische Datendatei eine Mehrzahl von Objektintensitätswerten ($I(x, y, z)$) enthält, die durch direkte Messung während eines Eingriffs erhalten werden, und einer zweiten volumetrischen Datendatei, die eine Mehrzahl von Eingriffsvorrichtungs-Intensitätswerten ($I_c(x, y, z)$) enthält, die durch direkte Messung wenigstens einmal während desselben Eingriffs erhalten werden;

Mittel zum Definieren einer ersten Projektionsebene (26) zum Anzeigen einer ersten Projektion der Objektintensitätswerte ($I(x, y, z)$) und der Eingriffsvorrichtungs-Intensitätswerte ($I_c(x, y, z)$);

einen ersten Bildprojektor, der so ausgeführt ist, dass er ein erstes zweidimensionales Projektionsbild des Objekts auf der ersten Projektionsebene (26) erzeugt, wobei jeder Wert ($P(u, v)$) des ersten Projektionsbildes des Objekts erhalten wird durch Summieren der Objektintensitätswerte ($I(x, y, z)$) längs einer Linie senkrecht zur ersten Projektionsebene (26), und ein zweidimensionales Projektionsbild der Eingriffsvorrichtung auf der ersten Projektionsebene (26) erzeugt, wobei jeder Wert ($P_c(u, v)$) des Projektionsbildes der Eingriffsvorrichtung erhalten wird durch Summieren der Eingriffsvorrichtungs-Intensitätswerte ($I_c(x, y, z)$) längs der Linie senkrecht zur ersten Projektionsebene (26);

einen Eingriffsvorrichtungs-Lokalisierer zum Lokalisieren (48) der Eingriffsvorrichtung an einem Vorrichtungsort; und

eine erste Überlagerungsvorrichtung zum Überlagern (42) des zweidimensionalen Projektionsbildes der Eingriffsvorrichtung und des zweidimensionalen Projektionsbildes des Objekts auf der ersten Projektionsebene (26), um ein erstes zweidimensionales Anzeigebild bereitzustellen.

2. Vorrichtung nach Anspruch 1, ferner umfassend:

Mittel zum Definieren einer zweiten Projektionsebene, das so ausgeführt ist, dass es eine zweite Projektion der Objektintensitätswerte ($I(x, y, z)$) anzeigt;

einen zweiten Bildprojektor, der so ausgeführt ist, dass er ein zweites Projektionsbild des Objekts auf der zweiten Projektionsebene anhand der Objektintensitätswerte ($I(x, y, z)$) bereitstellt, wobei jeder Wert des zweiten Projektionsbildes des Objekts erhalten wird durch Summieren der Objektintensitätswerte ($I(x, y, z)$) längs einer

Linie senkrecht zur zweiten Projektionsebene; und
eine zweite Überlagerungsvorrichtung zum Überlagern des zweidimensionalen Projektionsbildes der Eingriffsvorrichtung und des zweiten Projektionsbildes des Objekts, um ein zweites zweidimensionales Anzeigebild zu erzeugen.

3. Vorrichtung nach Anspruch 2, wobei das zweite zweidimensionale Anzeigebild eine Ansicht ist, die für medizinisches Personal, das eine Behandlung durchführt, nützlich ist.

4. Vorrichtung nach Anspruch 1, wobei das erste Anzeigebild eine rechtsschräge Ansicht (RAO-Ansicht) des Objekts ist.

5. Vorrichtung nach Anspruch 2, wobei das zweite Anzeigebild eine linksschräge Ansicht (LAO-Ansicht) des Objekts ist.

6. Vorrichtung nach Anspruch 1, wobei das erste Anzeigebild eine LAO-Ansicht des Objekts ist.

7. Vorrichtung nach Anspruch 2, wobei das zweite Anzeigebild eine RAO-Ansicht des Objekts ist.

8. Vorrichtung nach Anspruch 1, ferner umfassend:

Mittel zum Spezifizieren eines Bereichs der Objektintensitätswerte ($I(x, y, z)$) im ersten Anzeigebild.

9. Vorrichtung nach Anspruch 2, ferner umfassend:

Mittel zum Spezifizieren eines Bereichs der Objektintensitätswerte ($I(x, y, z)$) im zweiten Anzeigebild.

10. Vorrichtung nach Anspruch 8, wobei der erste Bildbereich auf dem Eingriffsvorrichtungsort, längs eines Vektors senkrecht zur Objektprojektionsebene gemessen, zentriert ist.

11. Vorrichtung nach Anspruch 9, wobei der zweite Bildbereich auf dem Eingriffsvorrichtungsort, wie längs eines Vektors senkrecht zur Objektprojektionsebene gemessen, zentriert ist.

12. Vorrichtung nach Anspruch 1 oder 2, die ferner eine Anzegebildorientierungskontrolle umfasst, um eine Linie senkrecht zu einer Projektionsebene aus einer Benutzereingabe zu definieren, oder eine Anzegebildorientierungskontrolle, um zwei Linien aus einer Benutzereingabe zu definieren, wobei eine Linie senkrecht zu einer ersten Projektionsebene verläuft und die andere Linie senkrecht zu einer zweiten Projektionsebene verläuft.

13. Vorrichtung nach Anspruch 1, wobei die erste Überlagerungsvorrichtung fähig ist, den Vorrichtungsort kontinuierlich zu aktualisieren.

14. Vorrichtung nach Anspruch 13, wobei die erste Überlagerungsvorrichtung fähig ist, die Objektintensitätswerte ($I(x, y, z)$) in Reaktion auf ein Benutzersignal zu aktualisieren.

15. Vorrichtung nach Anspruch 13, wobei der erste Bildprojektor fähig ist, die Objektintensitätswerte ($I(x, y, z)$) in Echtzeit zu aktualisieren.

16. Vorrichtung nach Anspruch 1, wobei der Eingriffsvorrichtung-Lokalisierer fähig ist, auf ein von der Eingriffsvorrichtung gesendetes Signal zu antworten.

17. Vorrichtung nach Anspruch 1, die ferner einen Ausgabedateigenerator umfasst zum Speichern des ersten zweidimensionalen Anzeigebildes.

18. Vorrichtung nach Anspruch 2, ferner umfassend:

Mittel zum Definieren einer dritten Projektionsebene zum Anzeigen einer dritten Projektion der Objektintensitätswerte ($I(x, y, z)$) und der Eingriffsvorrichtungs-Intensitätswerte ($I_c(x, y, z)$);

einen dritten Bildprojektor, der so ausgeführt ist, dass er ein drittes Projektionsbild des Objekts auf der dritten Projektionsebene erzeugt, wobei jeder Wert des dritten Projektionsbildes des Objekts erhalten wird durch Summieren der Objektintensitätswerte ($I(x, y, z)$) längs einer Linie senkrecht zur dritten Projektionsebene; und eine dritte Überlagerungsvorrichtung zum Überlagern des zweidimensionalen Projektionsbildes der Eingriffsvorrichtung und des dritten Projektionsbildes des Objekts, um ein drittes zweidimensionales Anzeigebild zu erzeugen.

vorrichtung und des dritten Projektionsbildes des Objekts, um ein drittes zweidimensionales Anzeigebild zu erzeugen.

5 Revendications

1. Appareil pour afficher des données volumétriques tridimensionnelles ultrasonores d'un objet et des données volumétriques tridimensionnelles d'un dispositif d'intervention sur un plan (26) à deux dimensions, comprenant:

un appareil destiné à stocker un premier fichier de données volumétriques, dans lequel ledit premier fichier de données volumétriques comporte plusieurs valeurs d'intensité ($I(x, y, z)$) d'un objet obtenues par le biais d'une mesure directe pendant une procédure d'intervention et un second fichier de données volumétriques qui comporte plusieurs valeurs d'intensité ($I_c(x, y, z)$) d'un dispositif d'intervention obtenues par le biais d'une mesure directe au moins une fois pendant la même procédure d'intervention;

des moyens destinés à définir un premier plan de projection (26) pour afficher une première projection de valeurs d'intensité ($I(x, y, z)$) d'un objet et des valeurs d'intensité ($I_c(x, y, z)$) d'un dispositif d'intervention;

un premier projecteur d'image adapté pour créer une première image en projection à deux dimensions dudit objet sur ledit premier plan de projection (26), chaque valeur ($P(u, v)$) de la première image en projection de l'objet étant obtenue en faisant la somme des valeurs d'intensité ($I(x, y, z)$) de l'objet le long d'une ligne perpendiculaire au premier plan de projection (26), et une image en projection à deux dimensions dudit dispositif d'intervention sur ledit premier plan de projection (26), chaque valeur ($P_c(u, v)$) de l'image en projection du dispositif d'intervention étant obtenue en faisant la somme des valeurs d'intensité ($I_c(x, y, z)$) du dispositif d'intervention le long de ladite ligne perpendiculaire au premier plan de projection (26);

un localisateur de dispositif d'intervention destiné à localiser (48) ledit dispositif d'intervention à un emplacement du dispositif; et

un premier dispositif de superposition destiné à superposer (42) ladite image en projection à deux dimensions du dispositif d'intervention et ladite image en projection à deux dimensions de l'objet sur ledit premier plan de projection (26) afin de procurer une première image d'affichage bidimensionnelle.

2. Appareil selon la revendication 1, comprenant en outre:

des moyens destinés à définir un second plan de projection adapté pour afficher une seconde projection desdites valeurs d'intensité ($I(x, y, z)$) de l'objet;

un second projecteur d'image adapté pour procurer une seconde image en projection de l'objet sur ledit second plan de projection d'après lesdites valeurs d'intensité ($I(x, y, z)$) de l'objet, chaque valeur de la seconde image en projection de l'objet étant obtenue en faisant la somme des valeurs d'intensité ($I(x, y, z)$) de l'objet le long d'une ligne perpendiculaire au second plan de projection; et

un second dispositif de superposition destiné à superposer ladite image en projection à deux dimensions du dispositif d'intervention et ladite seconde image en projection de l'objet afin de créer une seconde image d'affichage bidimensionnelle.

3. Appareil selon la revendication 2, dans lequel ladite seconde image d'affichage bidimensionnelle est une vue utile à un personnel médical réalisant une procédure.

4. Appareil selon la revendication 1, dans lequel ladite première image d'affichage est une vue oblique antérieure droite (OAD) de l'objet.

5. Appareil selon la revendication 2, dans lequel ladite seconde image d'affichage est une vue oblique antérieure gauche (OAG) de l'objet.

6. Appareil selon la revendication 1, dans lequel ladite première image d'affichage est une vue OAG de l'objet.

7. Appareil selon la revendication 2, dans lequel ladite seconde image d'affichage est une vue OAD de l'objet.

8. Appareil selon la revendication 1, comprenant en outre:

des moyens destinés à spécifier une plage desdites valeurs d'intensité ($I(x, y, z)$) de l'objet dans ladite première image d'affichage.

9. Appareil selon la revendication 2, comprenant en outre:

des moyens destinés à spécifier une plage desdites valeurs d'intensité ($I(x, y, z)$) de l'objet dans ladite seconde image d'affichage.

10. Appareil selon la revendication 8, dans lequel ladite plage dans la première image est centrée sur ledit emplacement du dispositif d'intervention tel qu'on la mesure le long d'un vecteur perpendiculaire audit plan de projection de l'objet.

11. Appareil selon la revendication 9, dans lequel ladite plage dans la seconde image est centrée sur ledit emplacement du dispositif d'intervention tel qu'on la mesure le long d'un vecteur perpendiculaire audit plan de projection de l'objet.

12. Appareil selon la revendication 1 ou 2, comprenant en outre une commande d'orientation d'image d'affichage pour définir une ligne perpendiculaire à un plan de projection d'après une entrée d'un utilisateur ou, une commande d'orientation d'image d'affichage pour définir deux lignes d'après une entrée d'un utilisateur, où une ligne est perpendiculaire à un premier plan de projection et l'autre ligne est perpendiculaire à un second plan de projection.

13. Appareil selon la revendication 1, dans lequel ledit premier dispositif de superposition est apte à mettre à jour de manière continue ledit emplacement du dispositif.

14. Appareil selon la revendication 13, dans lequel ledit premier dispositif de superposition est apte à mettre à jour lesdites valeurs d'intensité ($I(x, y, z)$) de l'objet en réponse à un signal d'utilisateur.

15. Appareil selon la revendication 13 dans lequel ledit premier projecteur d'image est apte à mettre à jour en temps réel lesdites valeurs d'intensité ($I(x, y, z)$) de l'objet.

16. Appareil selon la revendication 1, dans lequel ledit localisateur du dispositif d'intervention est apte à répondre à un signal transmis depuis ledit dispositif d'intervention.

17. Appareil selon la revendication 1, comprenant en outre un générateur de fichiers de sortie destiné à stocker ladite première image d'affichage bidimensionnelle.

18. Appareil selon la revendication 2, comprenant en outre:

des moyens destinés à définir un troisième plan de projection pour afficher une troisième projection desdites valeurs d'intensité ($I(x, y, z)$) de l'objet et valeurs d'intensités ($I_c(x, y, z)$) du dispositif d'intervention;

un troisième projecteur d'image adapté pour créer une troisième image en projection de l'objet sur ledit troisième plan de projection, chaque valeur de la troisième image en projection de l'objet étant obtenue en faisant la somme des valeurs d'intensité ($I(x, y, z)$) de l'objet le long d'une ligne perpendiculaire au troisième plan de projection; et

un troisième dispositif de superposition destiné à superposer ladite image en projection à deux dimensions du dispositif d'intervention et ladite troisième image en projection de l'objet afin de créer une troisième image d'affichage bidimensionnelle.

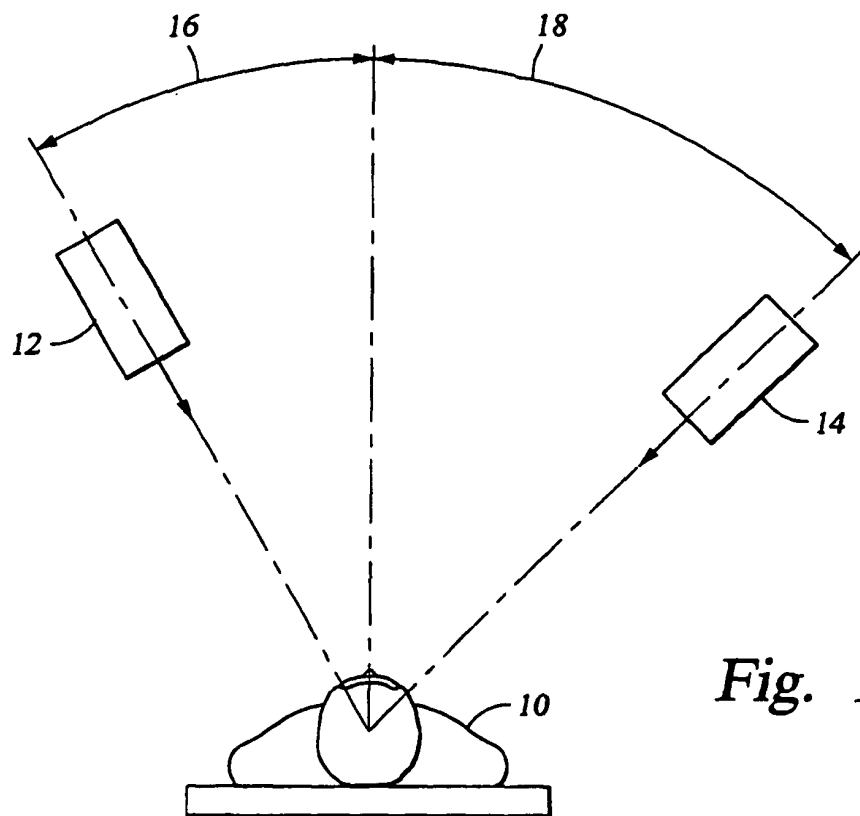


Fig. 1

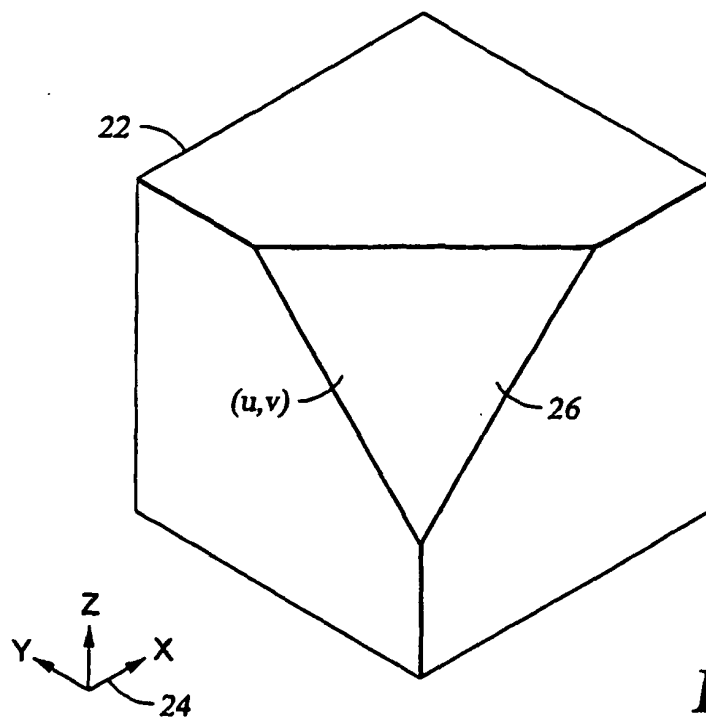
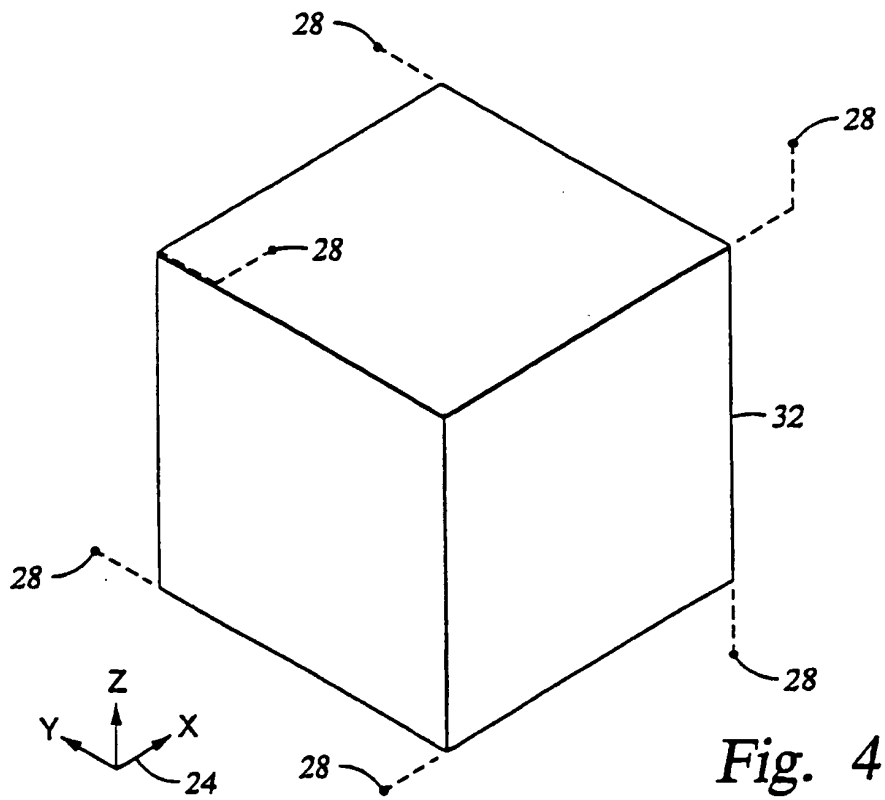
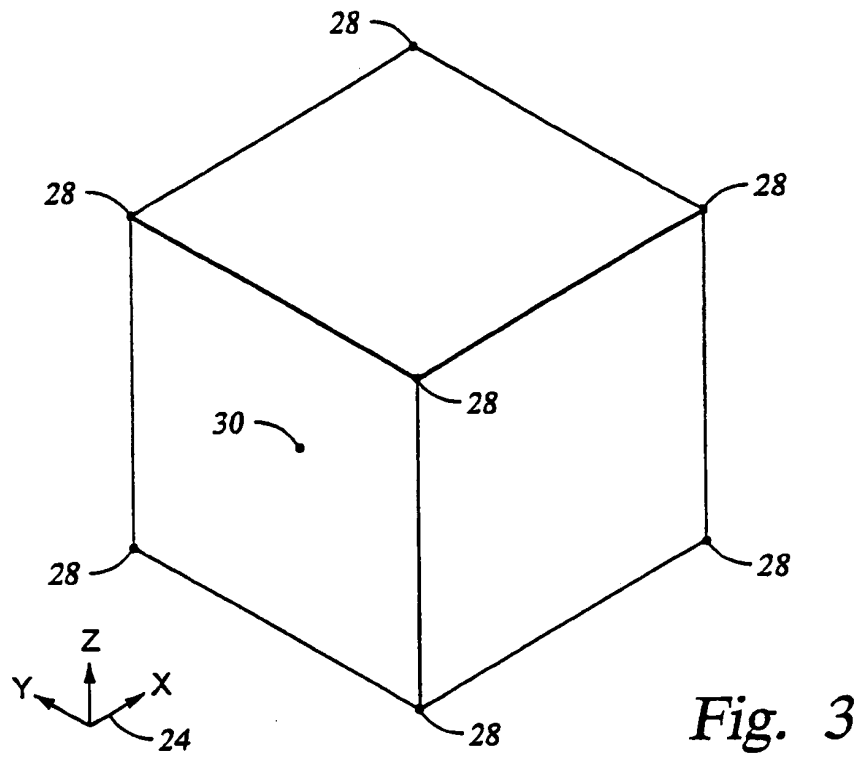


Fig. 2



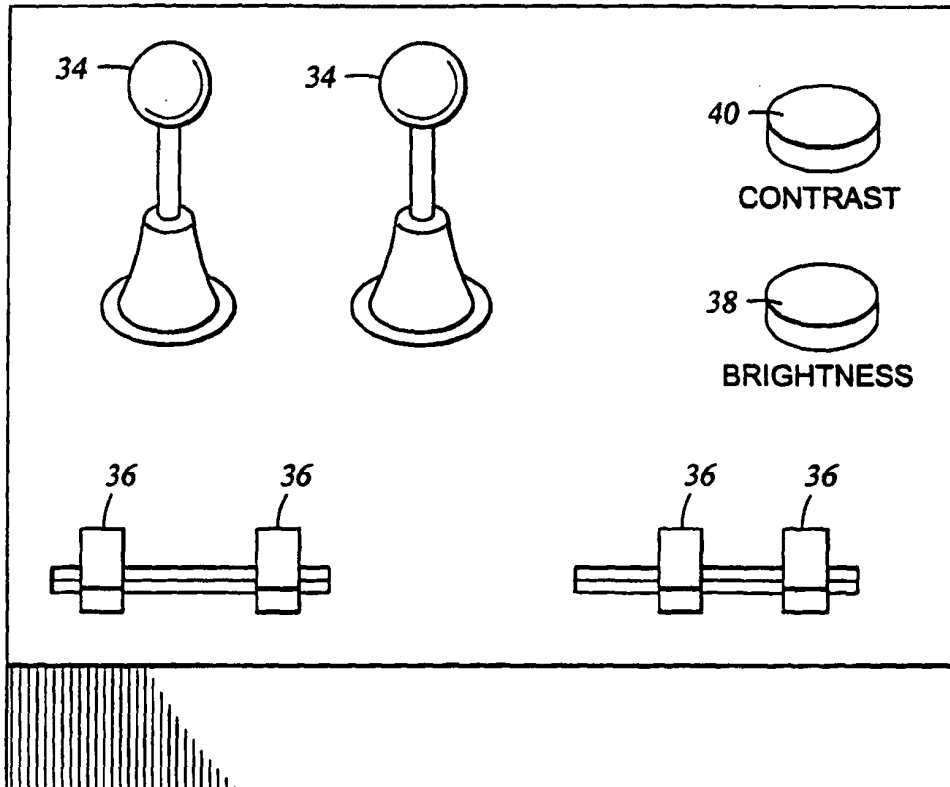


Fig. 5

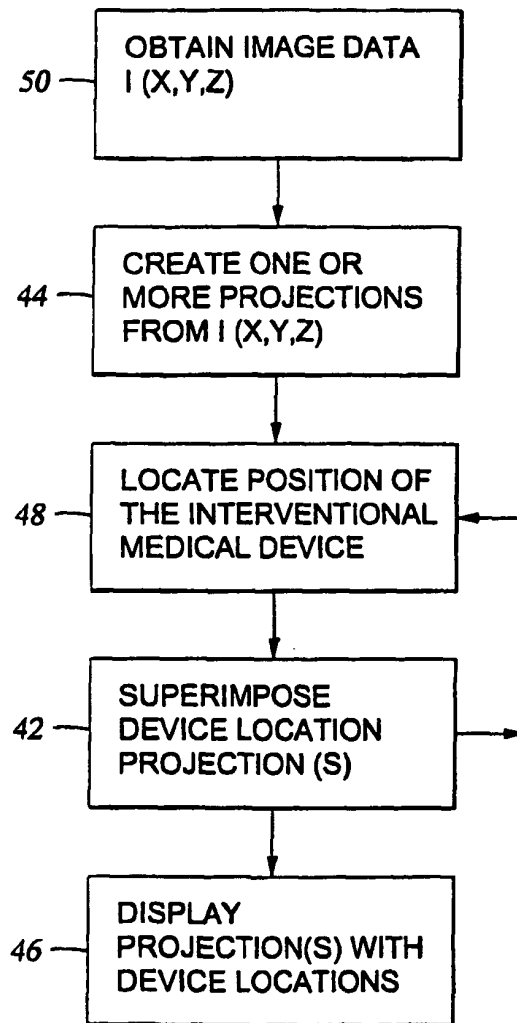


Fig. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 4173228 A, Steenwyk and Childress [0012]
- US 5515853 A, Smith [0013] [0019]
- US 5817022 A [0014]
- US 5868673 A [0014]
- WO 9625881 A [0020]
- US 5181514 A, Salomon [0032]
- US 5343865 A [0037]
- US 5226113 A, Cline [0045]
- US 5865750 A, Hatfield [0045]

专利名称(译)	超声波成像仪		
公开(公告)号	EP1253855B1	公开(公告)日	2010-03-10
申请号	EP2001902000	申请日	2001-01-10
[标]申请(专利权)人(译)	扎内利CLAUDIO我		
申请(专利权)人(译)	扎内利，CLAUDIO I.		
当前申请(专利权)人(译)	扎内利，CLAUDIO I.		
[标]发明人	ZANELLI CLAUDIO I		
发明人	ZANELLI, CLAUDIO I.		
IPC分类号	A61B8/08 A61B19/00		
CPC分类号	A61B8/0841 A61B8/0833 A61B8/461 A61B8/467 A61B90/36 A61B2090/378		
优先权	09/502722 2000-02-11 US		
其他公开文献	EP1253855A1		
外部链接	Espacenet		

摘要(译)

超声成像系统叠加由体积超声数据产生的截面图和用于干预装置（例如导管）的位置数据。在一个或多个视图中，当介入装置移动时，可以相对于身体内的器官和组织示出介入医疗装置的位置。介入装置位置数据被连续更新并且叠加在可以较不频繁地更新的组织图像上，导致介入装置相对于组织的实时或接近实时的图像。叠加的图像允许医务人员执行诸如血管造影的程序，患者对X射线和对比染料的暴露最小或没有。可以保持熟悉的类似荧光透视的成像的外观和感觉，或者可以提供介入医疗装置相对于器官或组织的三维实时或近时投影图像。

