



(11)

EP 2 309 931 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
11.12.2013 Bulletin 2013/50

(51) Int Cl.:
A61B 8/08 (2006.01) **G01S 7/52 (2006.01)**
G06T 7/00 (2006.01) **A61B 8/00 (2006.01)**
G01S 15/89 (2006.01) **G06T 7/20 (2006.01)**
A61B 5/0456 (2006.01)

(21) Application number: **09786490.4**(22) Date of filing: **30.06.2009**

(86) International application number:
PCT/IB2009/052841

(87) International publication number:
WO 2010/004479 (14.01.2010 Gazette 2010/02)

(54) ULTRASONIC ASSESSMENT OF CARDIAC SYNCHRONICITY AND VIABILITY

ULTRASCHALLUNTERSUCHUNG VON KARDIALER SYNCHRONIZITÄT UND LEBENSFÄHIGKEIT
EVALUATION PAR ULTRASONS DE SYNCHRONISME ET VIABILITE CARDIAQUE

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL
PT RO SE SI SK TR

(30) Priority: **10.07.2008 US 79663**

(43) Date of publication of application:
20.04.2011 Bulletin 2011/16

(73) Proprietor: **Koninklijke Philips N.V.**
5656 AE Eindhoven (NL)

(72) Inventors:

- **SALGO, Ivan**
Andover, MA 01810 (US)

- **SETTELMIER, Scott**
Andover, MA 01810 (US)
- **CHANG, Peter**
Briarcliff Manor
New York 10510-8001 (US)

(74) Representative: **van Velzen, Maaike Mathilde Philips**
Intellectual Property & Standards
P.O. Box 220
5600 AE Eindhoven (NL)

(56) References cited:
EP-A1- 1 804 078 **WO-A1-2007/138522**
WO-A2-2007/054861 **US-A1- 2004 254 486**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] This invention relates to medical diagnostic ultrasound systems and, in particular, to ultrasound systems which perform assessment of synchronicity and viability of cardiac performance.

[0002] There exist many ultrasonic methods to assess and quantify cardiac chamber function. Ventricular wall motion indicative of myocardial infarction and ejection fraction are basic diagnostic tools for echocardiographers. These diagnostic tools require that the heart chamber be defined and tracked over a series of images over the cardiac cycle so that measurements of the delineated myocardium and heart chamber can be made. Techniques for delineating the heart wall in an ultrasound image include for example automated border tracking of blood tissue interfaces and tissue Doppler imaging of cardiac wall motion to quantify velocity of contraction, among others. The ability to delineate and track myocardial motion is important for diagnosing the synchronicity of the electrical stimulation of the heart, and also to assess akynetic areas of the heart which can be caused by conditions such as ischemia, hibernation, or stunning. The heart is commanded to contract by electrochemical signals passed by sodium and potassium channels in the muscle cells of the myocardium. These signals, dispersed as they are over the entire heart muscle, should command the heart muscle cells to contract at the same instant in time. When this happens the heart contracts from a relaxed, full volume to a contracted minimal volume, thereby pumping a maximal volume of blood with each heartbeat. This is a characteristic of a healthy heart. However, when the signals that stimulate this contraction cause different regions of the heart to contract at different times, the erratic contraction will pump less than the maximal volume of blood, producing reduced efficiency and taxing the heart over time. It is desirable to be able to diagnose this condition so that the necessary treatment regime, generally the implantation of a pacemaker with leads placed to force synchronous contractions, can be performed if needed. This diagnosis and its treatment are referred to as cardiac resynchronization therapy, or CRT.

[0003] Documents EP-A1-1804078 and US-A1-2004/254 486 disclose ultrasonic diagnostic imaging systems displaying indicators of the relative times at which different myocardial segments participate in heart motion based on peak displacement values.

[0004] A disease condition which can affect electromechanical transduction of the heart is left bundle branch block. Left bundle branch block occurs when transmission of the cardiac electrical impulse is delayed or fails to conduct along the rapidly conducting fibers of the main left bundle branch or in both left anterior and posterior fascicles. This can cause the left ventricle to depolarize slowly via cell-to-cell conduction spreading from the right ventricle to the left ventricle. This condition results in a loss of synchronicity of chamber contraction and a con-

sequent inefficient ejection of blood volume from the chamber. Accordingly, it is desirable to be able to effectively and accurately identify and quantify indications and effects of this loss of synchronicity.

[0005] The invention is set out in independent claim 1.

[0006] In accordance with the principles of the present invention, the motion or displacement of the myocardium is tracked and measured over some or all of the systolic and/or diastolic phases of the heart cycle. A preferred measure is the distance measurement known as strain. The measurement is made at different regions of the myocardium and a family of curves is produced for the displacement measures of the different regions. The progressive contributions of the different regions to heart contraction during the heart cycle is quantified graphically, numerically, or both in a cardiac assessment referred to by the inventors as "recruitment." The degree of recruitment assessed has been found to correlate with conditions of left bundle branch block and dilated cardiomyopathy.

[0007] In the drawings:

FIGURE 1 illustrates in block diagram form an ultrasound system constructed in accordance with the principles of the present invention.

FIGURE 2 illustrates the QLab processor portion of the ultrasound system of FIGURE 1 in greater detail.

FIGURES 3a-3c illustrate three techniques for measuring displacement or strain in an ultrasound image of the myocardium.

FIGURE 4 is a schematic drawing of the segmented myocardial wall of the left ventricle.

FIGURES 5a and 5b illustrate the production of a recruitment curve in accordance with the principles of the present invention.

FIGURE 6 illustrates a numerical data entry display for the parameters of a recruitment analysis.

FIGURE 7 illustrates a parametric image of recruitment.

FIGURES 8a-8d illustrate a sequence of parametric images showing the dynamic achievement of a recruitment criterion in accordance with the principles of the present invention.

[0008] Referring first to FIGURE 1 an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention is shown in block diagram form. An ultrasonic probe 112 includes an array 114 of ultrasonic transducers that transmit and receive ultrasonic pulses. The array may be a one dimensional linear or curved array for two dimensional imaging, or may be a two dimensional matrix of transducer elements for electronic beam steering in three dimensions. The three dimensional data sets and images described below are preferably acquired using a two dimensional array probe. They may also be acquired with a mechanically swept one dimensional array probe. The ultrasonic transducers in the array 114 transmit ultrasonic energy and

receive echoes returned in response to this transmission. A transmit frequency control circuit 20 controls the transmission of ultrasonic energy at a desired frequency or band of frequencies through a transmit/receive ("T/R") switch 22 coupled to the ultrasonic transducers in the array 114. The times at which the transducer array is activated to transmit signals may be synchronized to an internal system clock (not shown), or may be synchronized to a bodily function such as the heart cycle, for which a heart cycle waveform is provided by an ECG device 26. When the heartbeat is at the desired phase of its cycle as determined by the waveform provided by ECG device 26, the probe is commanded to acquire an ultrasonic image. The frequency and bandwidth of the ultrasonic energy generated by the transmit frequency control circuit 20 is controlled by a control signal f_{tr} generated by a central controller 28.

[0009] Echoes from the transmitted ultrasonic energy are received by the transducers in the array 114, which generate echo signals that are coupled through the T/R switch 22 and digitized by analog to digital ("A/D") converters 30 when the system uses a digital beamformer. Analog beamformers may also be used. The A/D converters 30 sample the received echo signals at a sampling frequency controlled by a signal f_s generated by the central controller 28. The desired sampling rate dictated by sampling theory is at least twice the highest frequency of the received passband, and might be on the order of at least 30-40 MHz. Sampling rates higher than the minimum requirement are also desirable.

[0010] The echo signal samples from the individual transducers in the array 114 are delayed and summed by a beamformer 32 to form coherent echo signals. For 3D imaging with a two dimensional array, it is preferable to partition the beamformer between a microbeamformer located in the probe and the main beamformer in the system mainframe as described in US Pat. 6,013,032 (Savord) and US Pat. 6,375,617 (Fraser). The digital coherent echo signals are then filtered by a digital filter 34. In this embodiment, the transmit frequency and the receiver frequency are individually controller so that the beamformer 32 is free to receive a band of frequencies which is different from that of the transmitted band such as a harmonic frequency band. The digital filter 34 band-pass filters the signals, and can also shift the frequency band to a lower or baseband frequency range. The digital filter could be a filter of the type disclosed in U.S. Patent No. 5,833,613, for example. Filtered echo signals from tissue are coupled from the digital filter 34 to a B mode processor 36 for conventional B mode processing.

[0011] Filtered echo signals of a contrast agent, such as microbubbles, are coupled to a contrast signal processor 38. Contrast agents are often used to more clearly delineate the endocardial wall in relation to contrast agent in the blood pool of the heart chamber, or to perform perfusion studies of the microvasculature of the myocardium as described in US Pat. 6,692,438 for example. The contrast signal processor 38 preferably separates ech-

oes returned from harmonic contrast agents by the pulse inversion technique, in which echoes resulting from the transmission of multiple pulses to an image location are combined to cancel fundamental signal components and enhance harmonic components. A preferred pulse inversion technique is described in U.S. patent 6, 186, 950, for instance.

[0012] The filtered echo signals from the digital filter 34 are also coupled to a Doppler processor 40 for conventional Doppler processing to produce velocity and power Doppler signals. The output signals from these processors may be displayed as planar images, and are also coupled to a 3D image processor 42 for the rendering of three dimensional images, which are stored in a 3D image memory 44. Three dimensional rendering may be performed as described in U.S. patent 5,720,291, and in U.S. patents 5,474,073 and 5,485,842.

[0013] The signals from the contrast signal processor 38, the B mode processor 36 and the Doppler processor 40, and the three dimensional image signals from the 3D image memory 44 are coupled to a Cineloop® memory 48, which stores image data for each of a large number of ultrasonic images. The image data are preferably stored in the Cineloop memory 48 in sets, with each set of image data corresponding to an image obtained at a respective time. The image data in a data set can be used to display a parametric image showing tissue perfusion at a respective time during the heartbeat. The sets of image data stored in the Cineloop memory 48 may also be stored in a permanent memory device such as a disk drive or digital video recorder for later analysis.

In this embodiment the images are also coupled to a QLab processor 50, where the images are analyzed for recruitment characteristics as described below. The QLab processor also makes quantified measurements of various aspects of the anatomy in the image and delineates tissue boundaries and borders by automated border tracing as described in US patent publication no. US20050075567 and PCT publication no. 2005/054898.

[0014] FIGURE 2 is a detailed block diagram of the portion of the QLab processor 50 of FIGURE 1 when operating in accordance with the present invention. The QLab processor receives images from an image processor 440 such as those preceding the Cineloop memory 48 in FIGURE 1. The image processor 440 produces scanline data of an image which is stored in image data memory 140. A first, starting point image of a sequence of heart images is analyzed by border detection of a heart chamber in the image by an ABD processor 144 as described in PCT publication no. 2007/138522. When the border is defined in this first image its location is tracked through subsequent images by a speckle tracker 142,

which follows the recurring speckle pattern on or near a delineated tissue border. The initially defined border and the borders in subsequent images are drawn or traced by a graphics processor 148. The ultrasound images of the sequence are converted to the desired display format (e.g., sector, linear, 3D, etc.) by a scan converter 450 which displays the graphically produced borders over the defined border locations in the ultrasound images. The image with its graphic border overlay are stored in a Cineloop memory 460, along with recruitment characteristics produced by a recruitment metric processor 120 which operates on heart images as discussed in detail below. The images and recruitment information are then coupled to the display 52.

[0015] Specific points on the identified borders of the successive images are tracked by the speckle tracker 142, which tracks the starting anatomical positions of the points by the speckle pattern produced by the local tissue at the image locations of the points. The speckle tracker 142 identifies regions of pixels around the reference points in the adjacent myocardium. The speckle patterns of these pixels are saved and compared with speckle patterns in the same regions of the successive images and the speckle patterns matched by block matching, as described in US patent 6,442,289 (Olsson et al.) The difficulty and precision of the matching is determined by establishing a maximum correlation for the matching. The reference point locations in the images are thus tracked from image to image by following the speckle patterns around the points. When the speckle tracker 142 locates the reference points in a new image the reference point locations are coupled to the graphics processor 148, the border redrawn using the newly identified point locations, and a graphic overlay produced for the new image. The new image and its graphic overlay are scan converted and displayed on display 52. The ABD processor 144 may employ the same technique to identify or trace the epicardial border of the myocardium in an image. Further details of the identification of endo- and epicardial borders may be found in the aforementioned PCT publication no. 2007/138522.

[0016] Instead of tracking the speckle pattern of the myocardial tissue surrounding, underling, or adjacent to the reference points, it may be appreciated that the reference point locations may be tracked by means other than speckle tracking, that is, by tracking image characteristics which are greater than a wavelength in size. For instance, the movement of specific anatomical features such as the mitral valve plane corners may be tracked. As another example, tissue texture may be tracked. It will also be appreciated that the targeted characteristics may be tracked in either pre-scan converted or post-scan converted image data.

[0017] As a final step, the user may want to manually adjust the identified border points or traces so that they precisely outline the border of the underlying myocardium. Located on each identified myocardial border in the example of FIGURE 3a are a number of small control

points 14,16 as shown in that drawing. The number and spacing of these small control points is a system design choice or may be a variable that the user can set. Using a control on the user interface or control panel 150, the user can point at or near these control points and click and drag the points to more precisely delineate what appears to the user as the myocardial boundary in the image. This process of stretching or dragging the border is known as "rubberbanding", and is described more fully in the aforementioned 6,491,636 patent, with particular reference to Fig. 9 of that patent. As an alternative to rubberband adjustment, in a more complex embodiment the approximated borders may automatically adjust to the image borders by image processing which uses the intensity information of the pixels at and around the approximated tissue borders. When this process is finished, the control points or border tracing can precisely delineate the boundary of the myocardium in the image.

[0018] FIGURE 3a illustrates a short axis view cardiac image produced by an ultrasound system constructed in accordance with the principles of the present invention. The heart chamber 10 is shown in the center of the short axis image, surrounded by the myocardium 12. The endocardial and epicardial borders are defined using the techniques described above or those described in US Pat. 5,797,396 (Geiser et al.), for instance. A number of control points are defined on both the endo- and epi-cardinal borders. Each pair of endo- and epi-cardial control points 14,16 in this example comprises two points positioned at a separate radius of the short axis view. Each pair of control points is joined by a graphically drawn chord line 18 produced by the graphics processor 148 which connects the points. It can be seen that the radial chord lines are all directed at approximately the center of the heart chamber 10. As the myocardium contracts with each heartbeat during systole, the myocardium will move in the direction of the chord lines toward the center of the heart chamber. Correspondingly, when the myocardium relaxes during diastole, the myocardium will move back in the reverse direction. With the control points 14,16 continuing to move with the myocardial borders, the distances between the control points 14,16, that is, the lengths of the chord lines 18, will shorten and lengthen with the contractions of the heart.

[0019] In this example the border tracing graphics are not displayed; only the endo- and epi-cardial control points 14,16 and their connecting chords 18 are displayed. In this example the control points for seven lines are positioned around the myocardium and seven chord lines are drawn, although in a given implementation a greater or lesser number of chords can be used or user-defined by means of the user interface 150.

[0020] As the sequence of images moves from frame to frame through the cardiac cycle, the endo- and epicardial borders will change in relation to each other from image to image as the heart muscle contracts during systole, then relaxes during diastole. One way to quantify this motion or displacement of tissue ultrasonically is the

measure known as Lagrangian strain (fractional change in length relative to initial length) or strain rate as described in US Pat. 6,537,221 (Criton et al.) Strain is a measure of deformation in tissue and is an indicator of the mechanical effects of muscle tissue. Strain is usually depicted as a dimensionless parameter or percentage, with a change in length as the numerator and the initial length as the denominator of the parameter. Thus the changes in the chord lengths 18 in FIGURE 3a from their starting lengths as the heart contract or relaxes can be used to compute a strain measure for each chord line 18 and associated pair of border control points 14,16. Since the chord lines 18 in FIGURE 3a are approximately on radii from the center of the heart chamber, these measurements of FIGURE 3a are referred to as radial strain. [0021] FIGURE 3b illustrates a measure of longitudinal strain made along the wall of the heart chamber. In this ultrasound image, a longitudinal cross-sectional view of the left ventricle with an endocardial border tracing 15, control points 14,14' are located around the endocardial border of the heart chamber. Chord lines 18 connect control points 14,14' located along the heart chamber. As the myocardium contracts, the control points 14,14' approach each other and the chord lines 18 between them shorten. Correspondingly, when the myocardium relaxes the adjacent control points draw further apart and the chord lines 18 lengthen. These lengths and length changes can thus be used to make a strain measurement for each chord line.

[0022] FIGURE 3c illustrates another way to make a strain measurement known as circumferential strain. It is seen that the ABD processor 144 has drawn an endocardial tracing 15 which is drawn along the circumference of the heart wall in this short axis view of the heart chamber. A number of control points 14,14' are located along the border tracing 15. As the heart muscle contracts, the circumferential distance between these control points such as adjacent points 14,14' will decrease. When the heart muscle relaxes, the distance between these points will lengthen again. These displacements can be used to make a measurement of circumferential strain at locations around the endocardial border.

[0023] In accordance with the principles of the present invention, the strain measurements of myocardial motion or displacement are used to compute a characteristic which the present inventions call "recruitment." The characteristic is so named because it indicates the recruitment or participation in heart displacement or motion by different regions of the heart. Recruitment may be understood with reference to FIGURES 4, 5a and 5b. FIGURE 4 is a schematic drawing of the left ventricle (LV) with the apex of the chamber at the top and the mitral valve plane at the bottom. In this example the myocardium of the LV is segmented into four regions identified as 1, 2, 3, and 4. Strain measurements are made over a full heart cycle for each of these myocardial segments and are plotted in FIGURE 5a as strain curves 101, 102, 103 and 104, respectively. Each curve reaches its lowest

extension when its corresponding segment has moved its maximum distance during myocardial contraction; the curve returns to the top of the plot when the heart relaxes again. It can be seen that the four curves are not moving in unison in this example. That is, the four segments are not synchronized in their movement. Also, it can be seen that various segments have different strain maxima. That is, the displacements of the four segments during a contraction are different. Both of these characteristics are indicated by a recruitment measurement of the present invention.

[0024] FIGURE 5b illustrates a recruitment curve produced in accordance with the present invention. In this example the user first defines a recruitment criterion, which is a threshold strain that a segment must achieve to effectively participate in, or be recruited for, the heart contraction. In this case the user has defined a 10% recruitment criterion indicated by the horizontal dashed line in FIGURE 5a. It is seen that curve 102 of myocardial segment 2 does not achieve this threshold criterion. The segment's displacement is insufficient for segment 2 to be recruited for this criterion. The other three curves all cross this criterion and all three are recruited for effective heart contraction in this example.

[0025] The user also sets a recruitment milestone level, which is a percentage of the maximum strain of a heart wall segment. The milestone can be set at 100% of a segment's full displacement, or a fraction of the maximum strain measurement. In this example the milestone level is set to 85% of maximum strain. With these parameters defined, the QLab processor 50 can plot a recruitment curve 110 as shown in FIGURE 5b. The Curve 110 is seen to have a zero starting level prior to heart contraction, and a final plateau level 118 when all recruited segments have achieved the milestone. The steps in the curve 110 show when the segments 1, 3, and 4, represented by curves 101, 103, and 104, have achieved their milestone levels. The milestone level are indicated by 116 and vertical dashed lines are dropped down from these milestones in FIGURE 5a. The horizontal dashed lines in FIGURE 5b indicate recruitment step levels of 25%, 50%, and 75%, the three steps of the three heart wall segments which are recruited above the 10% criterion. The time taken for the curve 110 to rise from its starting level 116 to its final plateau level 118 is a time duration indicated by arrow 130. The vertical dashed lines between FIGURES 5a and 5b mark the respective times that the strain curves 101-104 reach their 85% milestone levels, which the dashed lines translate down to the recruitment curve. Thus, the rise time duration 130 of the recruitment curve is a measure of the synchronicity of the heart's electrical timing.

[0026] If all of the segment curves 101-104 reached their milestone level at the same time, the case for an ideally healthy heart, the recruitment curve 110 would not have multiple steps but would be a single step from the baseline starting level to final level 118, since the segments would be moving in complete synchronism.

The duration characteristic indicated by arrow 130 would in that case be zero. Thus, a greater duration indicates poorer synchronicity. The recruitment curve 110 of a healthy heart would also have a number of steps equal to the number of segment curves. That is, all segments of the heart would be recruited for contraction. When a segment is not recruited and is below the recruitment criterion, 10% in this example, the possibility of an infarcted heart wall segment is indicated. Thus, the recruitment curve is sensitive to the extent of the tissue which will eventually be recruited, an ischemia indicator, and is sensitive to how fast tissue will eventually be recruited, which is a synchronicity indicator. Recruitment, therefore, can simultaneously indicate viability and synchronicity. This is important because pacing non-viable tissue is one of the reasons why the CRT procedure fails.

[0027] While the preceding example segmented the myocardium into only four segments, it will be appreciated that greater or lesser numbers of segments may alternatively be used, including calculating strain for each pixel. A large number of segments would produce a multitude of steps in the recruitment curve, showing the progressive recruitment of each point of the myocardium to overall heart motion and effectiveness. By color-coding the points in the myocardium, the strain curves, and the steps of the recruitment curve, the times of maximal participation of each point of the myocardium to heart motion may be appreciated.

[0028] FIGURE 6 illustrates a data entry display box by which a user may set the recruitment curve parameters, criterion and milestone level. In this example the user has set the recruitment strain criterion to 10% and the recruitment strain milestone to 85% of maximum. The circles below these entry points can be set to indicate the use of radial, longitudinal, or circumferential strain measurements for the recruitment analysis.

[0029] As an alternative or adjunct to graphical presentation of the recruitment analysis as shown in FIGURE 5b, an anatomical parametric display can be used to indicate recruitment as shown in FIGURE 7. In this example a circular parametric display band 200 is overlaid over the myocardium shown in an ultrasound image. The cursor on the ECG waveform 210 at the bottom of the display shows the point in the cardiac cycle at which the cardiac image was acquired. The points in the parametric display band 200 are colored to indicate the recruitment of the underlying points of the heart muscle. While progressive recruitment along the strain curve can be indicated by a continuing spectrum of colors or shadings as shown by the color bar 212 to the right of the cardiac image, in this example only a dark and a light color are used to indicate whether the underlying myocardial point has exceeded or not exceeded either the recruitment criterion or the recruitment milestone. A dark shading indicates that the underlying myocardium has been recruited by this phase of the heart cycle, and a light shading indicates that the underlying myocardium has not yet been recruited. The dark region 202 in the lower half of the parametric display

band in this example indicates that the myocardial region in the inferior wall has been initially recruited, whereas the region of the myocardium in the anterior wall of the heart, underlying light display band region 204, has yet to be recruited by the time of this phase of the heart cycle.

[0030] FIGURES 8a-8d show a series of cardiac images acquired during a heart cycle which indicate the progressive recruitment of regions of the myocardium during the cycle. The dark areas of the parametric display band 200 in FIGURE 8a show that initial movement of the heart contract occurs at the upper left (antero-septal) region of the heart in this example. FIGURE 8b shows that the left side (septal portion) of the myocardium is now virtually entirely recruited by this phase of the heart cycle, with some movement beginning on the right (lateral) side of the heart. At the time of the heart cycle of FIGURE 8c, the entire endocardium and almost the entire right side of the heart are now participating in the contraction, and at the time of the FIGURE 8d image recruitment is strongly evident around the full circumference of the heart chamber. A series of images such as those of FIGURES 8a-8d give a clinician a good sense of the synchronicity of the heart contraction and of the times of participation of the different regions of the heart in a contraction.

Claims

1. An ultrasonic diagnostic imaging system for diagnosing myocardial motion comprising: to receive a probe (112) which is adapted to transmit ultrasonic waves into a heart and to receive echoes in response; an image processor responsive to the echoes which is operable to produce a sequence of images of the myocardium (12) over at least a portion of a heart cycle; a myocardial motion analyzer, responsive to the sequence of images, which is adapted to determine the motion of a plurality of segments (1, 2, 3, 4) of the myocardium; a recruitment processor (50), responsive to the motion of the segments, which is adapted to produce an indicator of the cumulative percent participation of the plurality of segments toward a percentage of the full displacement of the myocardium during the heart cycle and of the relative times of participation of the segments in myocardial motion relative to the percentage of full displacement during the heart cycle; and a display (52) coupled to the recruitment processor which is adapted to display the indicator.
2. The ultrasonic diagnostic imaging system of Claim 1, wherein the percentage of full displacement is a recruitment milestone level.

3. The ultrasonic diagnostic imaging system of Claim 2, wherein the indicator is a graphical recruitment indicator indicating the relative times of recruitment of segments of the myocardium in cardiac contraction.

4. The ultrasonic diagnostic imaging system of Claim 2, wherein the indicator is a parametric display (200) indicating the relative times of recruitment of segments of the myocardium on an anatomical basis.

5. The ultrasonic diagnostic imaging system of Claim 4, wherein the segments correspond to pixels of an ultrasonic image of the myocardium.

6. The ultrasonic diagnostic imaging system of Claim 1, wherein the motion analyzer is adapted to produce strain values.

7. The ultrasonic diagnostic imaging system of Claim 1, wherein the motion analyzer is adapted to produce values of tissue displacement.

8. The ultrasonic diagnostic imaging system of Claim 6, wherein the strain values are computed as change in length relative to an initial length.

9. The ultrasonic diagnostic imaging system of Claim 6, wherein the strain values comprise radial strain values.

10. The ultrasonic diagnostic imaging system of Claim 6, wherein the strain values comprise circumferential strain values.

11. The ultrasonic diagnostic imaging system of Claim 6, wherein the strain values comprise longitudinal strain values.

12. The ultrasonic diagnostic imaging system of Claim 1, wherein the motion analyzer is further operable to track the motion of the myocardium by speckle tracking.

13. The ultrasonic diagnostic imaging system of Claim 1, wherein the motion analyzer is further operable to track the motion of the myocardium by border detection.

14. The ultrasonic diagnostic imaging system of Claim 6, wherein the recruitment processor is further operable to produce plots of strain values during cardiac contraction for different segments of the myocardium.

15. The ultrasonic diagnostic imaging system of Claim 13, wherein the recruitment processor is further responsive to the strain value plots to produce a re-

cruitment curve (110) for the cardiac contraction.

Patentansprüche

5 1. Diagnostisches Ultraschall-Bildgebungssystem zur Diagnose von Bewegungen des Myokards, das Folgendes umfasst:

10 einen Schallkopf (112), der für das Aussenden von Ultraschallwellen in ein Herz und in Reaktion darauf das Empfangen von Echos ausgelegt ist,

15 einen Bildprozessor, der als Reaktion auf die Echos so funktioniert, dass er eine Bildersequenz des Myokards (12) über zumindest einen Teil eines Herzzyklus erzeugt,

20 einen Analysator der Bewegungen des Myokards, der auf die Bildersequenz reagiert und für die Ermittlung der Bewegungen einer Vielzahl von Segmenten (1, 2, 3, 4) des Myokards ausgelegt ist,

25 einen Rekrutierungsprozessor (50), der auf die Bewegungen der Segmente reagiert und für die Erzeugung eines Indikators für die kumulative prozentuale Beteiligung der Vielzahl von Segmenten hin zu einem prozentualen Anteil der vollen Verschiebung des Myokards während des Herzzyklus und für die relativen Zeiten der Beteiligung der Segmente an den Bewegungen des Myokards im Verhältnis zu dem prozentualen Anteil der vollen Verschiebung während des Herzzyklus ausgelegt ist, und

30 eine Anzeige (52), die mit dem Rekrutierungsprozessor gekoppelt und für die Anzeige des Indikators ausgelegt ist.

35 2. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei der prozentuale Anteil an der vollen Verschiebung ein Rekrutierungsmeilenstein ist.

40 3. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 2, wobei der Indikator ein graphischer Rekrutierungsindikator ist, der die relativen Rekrutierungszeiten von Segmenten des Myokards bei der Kontraktion des Herzens angibt.

45 4. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 2, wobei der Indikator eine Parameteranzeige (200) ist, die die relativen Rekrutierungszeiten von Segmenten des Myokards auf anatomischer Basis wiedergibt.

50 5. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 4, wobei die Segmente Pixel eines Ultraschallbildes des Myokards entsprechen.

6. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei der Bewegungsanalysator für die Erzeugung von Verformungswerten ausgelegt ist. 5

7. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei der Bewegungsanalysator für die Erzeugung von Werten der Gewebeverschiebung ausgelegt ist. 10

8. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 6, wobei die Verformungswerte als Änderung der Länge im Verhältnis zu einer ursprünglichen Länge berechnet werden. 15

9. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 6, wobei die Verformungswerte Werte der radialen Verformung umfassen. 20

10. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 6, wobei die Verformungswerte Werte der umlaufenden Verformung umfassen. 25

11. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 6, wobei die Verformungswerte Werte der longitudinalen Verformung umfassen. 30

12. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei der Bewegungsanalysator für die Verfolgung der Bewegungen des Myokards durch Speckle-Tracking ausgelegt ist. 35

13. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei der Bewegungsanalysator für die Verfolgung der Bewegungen des Myokards durch Randerkennung ausgelegt ist. 40

14. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 6, wobei der Rekrutierungsprozessor ferner so funktioniert, dass er grafische Darstellungen der Verformungswerte während der Kontraktion des Herzens für verschiedene Segmente des Myokards erzeugt. 45

15. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 13, wobei der Rekrutierungsprozessor ferner auf die grafischen Darstellungen der Verformungswerte reagiert, indem er eine Rekrutierungskurve (110) für die Kontraktion des Herzens erzeugt. 50

une sonde (112) qui est conçue pour émettre des ondes ultrasonores dans un cœur et recevoir des échos en réponse ; un processeur d'image sensible aux échos, servant à produire une séquence d'images du myocarde (12) pendant au moins une partie d'une révolution cardiaque ; un dispositif d'analyse de mouvement du myocarde, sensible à la séquence d'images, qui est conçu pour déterminer le mouvement d'une pluralité de segments (1, 2, 3, 4) du myocarde ; un processeur de recrutement (50), sensible au mouvement des segments, qui est conçu pour produire un indicateur du pourcentage de participation cumulée de la pluralité de segments dans le but d'obtenir un pourcentage du déplacement intégral du myocarde pendant la révolution cardiaque et des temps relatifs de participation des segments lors du mouvement du myocarde par rapport au pourcentage de déplacement intégral pendant la révolution cardiaque ; et un écran d'affichage (52) couplé au processeur de recrutement, qui est conçu pour afficher l'indicateur.

2. Système imageur de diagnostic à ultrasons selon la revendication 1, dans lequel le pourcentage de déplacement intégral est un niveau jalon de recrutement.

3. Système imageur de diagnostic à ultrasons selon la revendication 2, dans lequel l'indicateur est un indicateur de recrutement graphique indiquant les temps relatifs de recrutement des segments du myocarde lors d'une contraction cardiaque.

4. Système imageur de diagnostic à ultrasons selon la revendication 2, dans lequel l'indicateur est un affichage paramétrique (200) indiquant les temps relatifs de recrutement des segments du myocarde sur une base anatomique.

5. Système imageur de diagnostic à ultrasons selon la revendication 4, dans lequel les segments correspondent aux pixels d'une image ultrasonore du myocarde.

6. Système imageur de diagnostic à ultrasons selon la revendication 1, dans lequel le dispositif d'analyse de mouvement est conçu pour produire des valeurs de déformation.

7. Système imageur de diagnostic à ultrasons selon la revendication 1, dans lequel le dispositif d'analyse de mouvement est conçu pour produire des valeurs de déplacement de tissu.

Revendications

1. Système imageur de diagnostic à ultrasons permettant de diagnostiquer le mouvement du myocarde, comprenant :

8. Système imageur de diagnostic à ultrasons selon la revendication 6, dans lequel les valeurs de déformation sont calculées sous la forme d'un changement de longueur par rapport à une longueur initiale. 5

9. Système imageur de diagnostic à ultrasons selon la revendication 6, dans lequel les valeurs de déformation comprennent des valeurs de déformation radiale. 10

10. Système imageur de diagnostic à ultrasons selon la revendication 6, dans lequel les valeurs de déformation comprennent des valeurs de déformation circonférentielle. 15

11. Système imageur de diagnostic à ultrasons selon la revendication 6, dans lequel les valeurs de déformation comprennent des valeurs de déformation longitudinale. 20

12. Système imageur de diagnostic à ultrasons selon la revendication 1, dans lequel le dispositif d'analyse de mouvement sert en outre à suivre le mouvement du myocarde par suivi de granularité. 25

13. Système imageur de diagnostic à ultrasons selon la revendication 1, dans lequel le dispositif d'analyse de mouvement sert en outre à suivre le mouvement du myocarde par détection de bord. 30

14. Système imageur de diagnostic à ultrasons selon la revendication 6, dans lequel le processeur de recrutement sert en outre à produire des tracés de valeurs de déformation pendant une contraction cardiaque pour différents segments du myocarde. 35

15. Système imageur de diagnostic à ultrasons selon la revendication 13, dans lequel le processeur de recrutement est en outre sensible aux tracés de valeurs de déformation pour produire une courbe de recrutement (110) pour la contraction cardiaque. 40

45

50

55

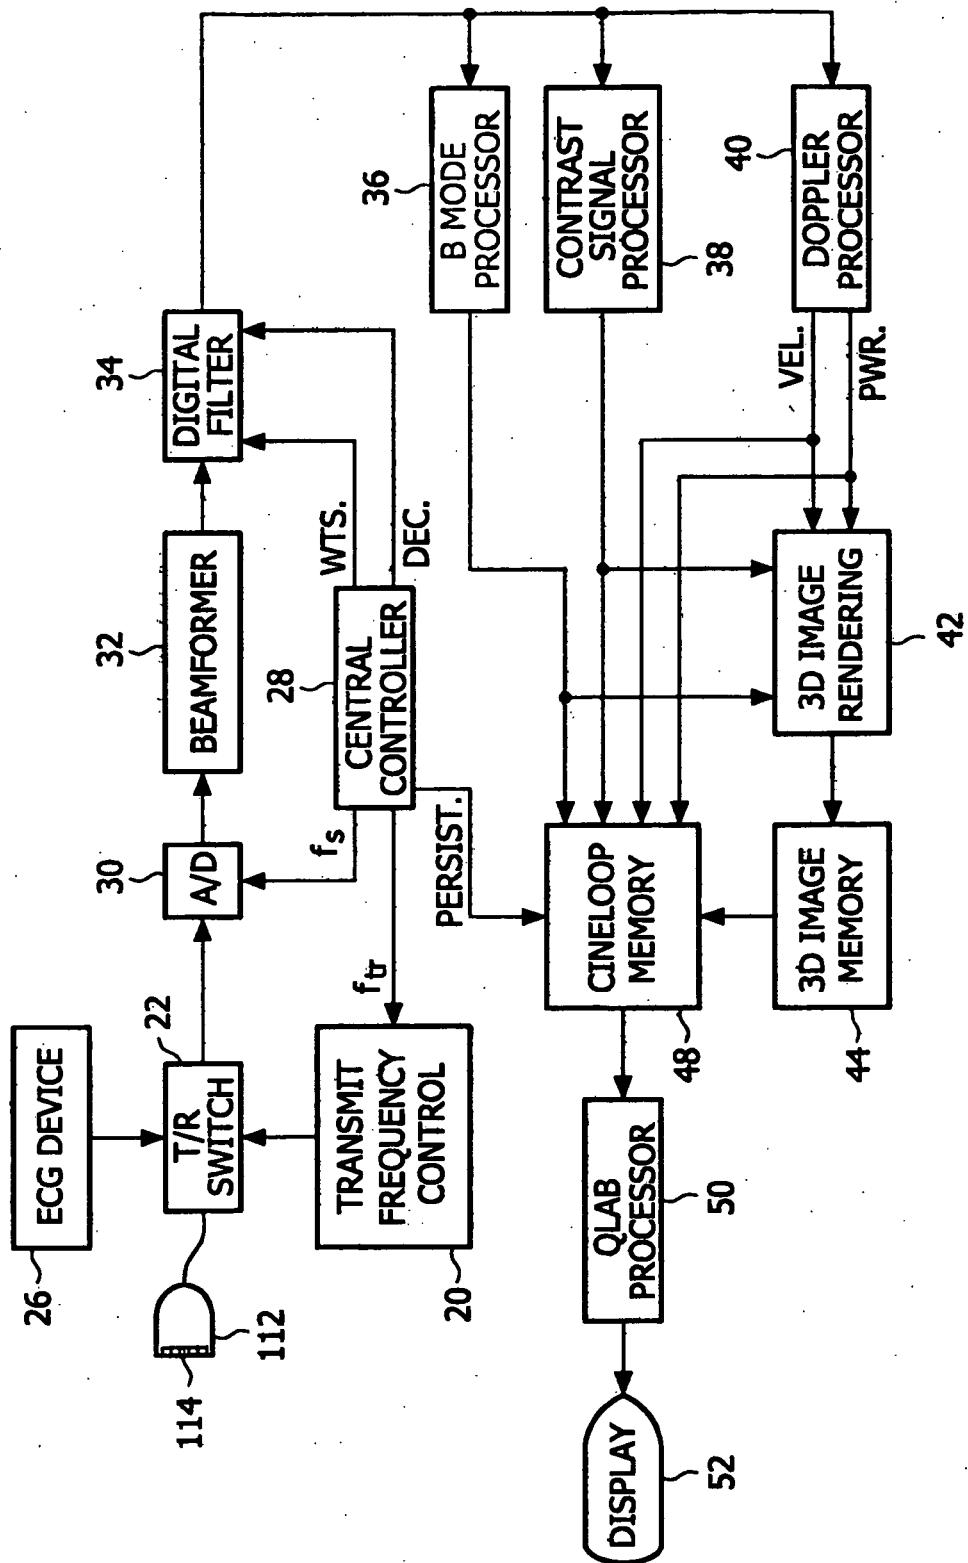


FIG. 1

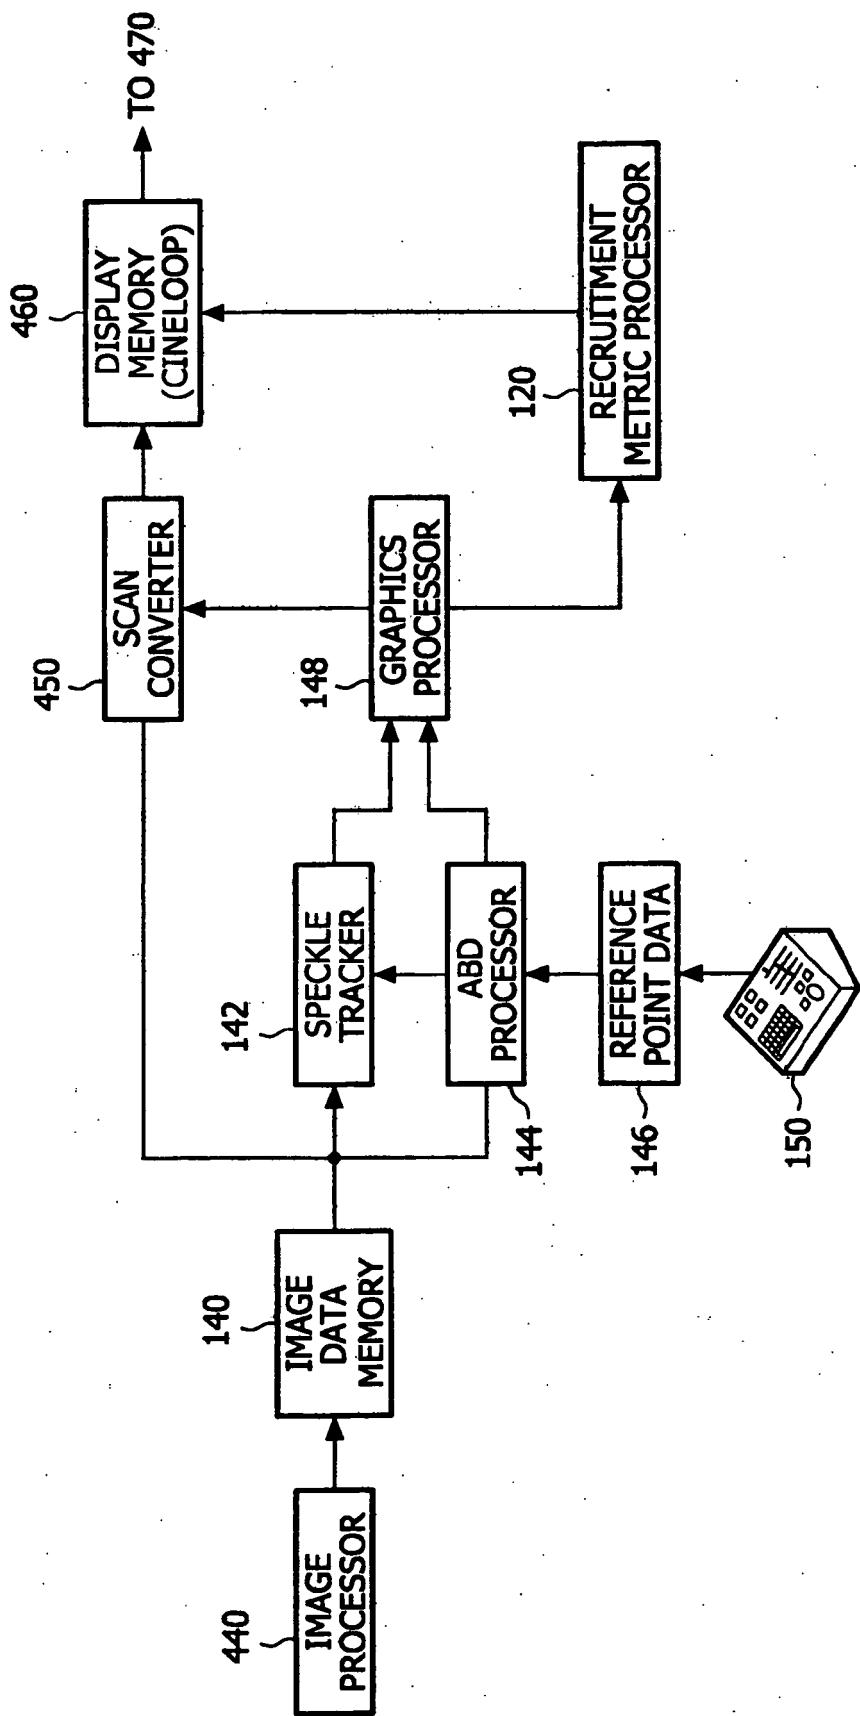


FIG. 2

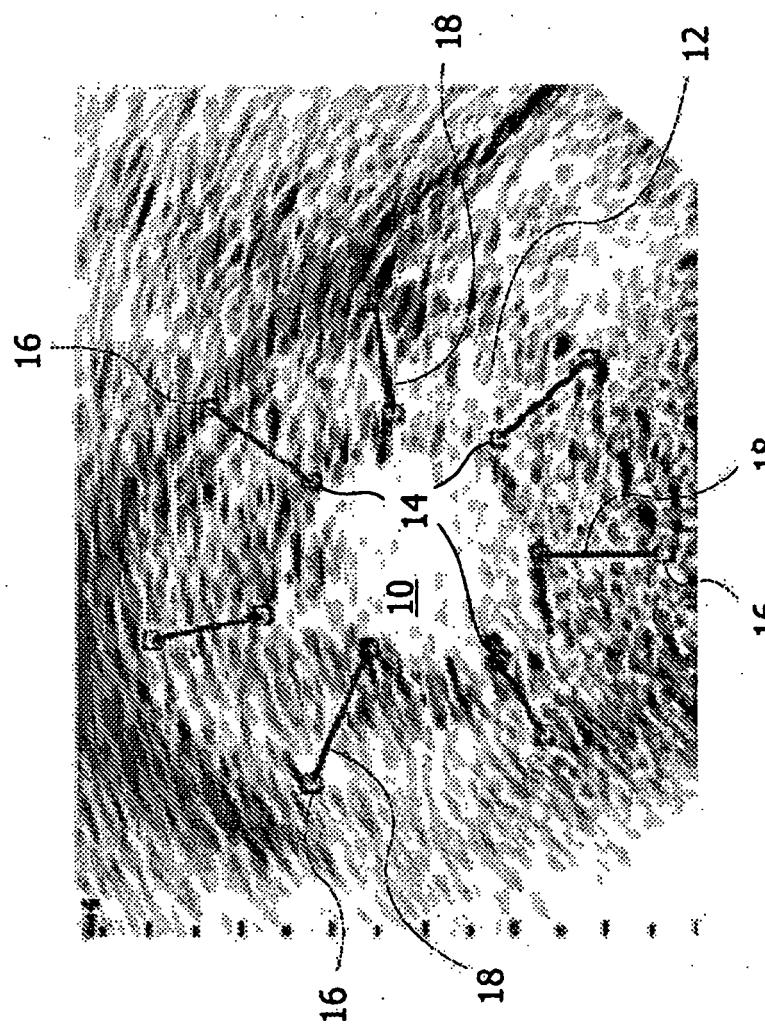


FIG. 3a

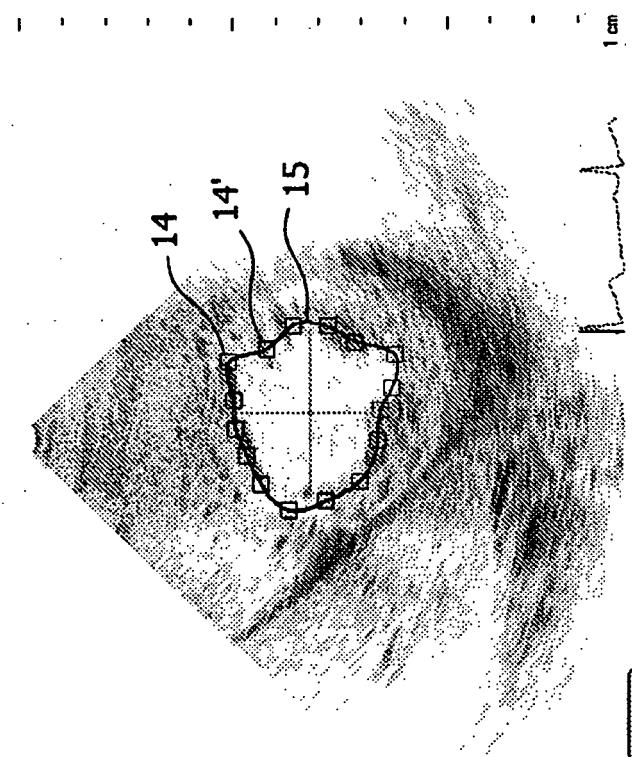


FIG. 3c

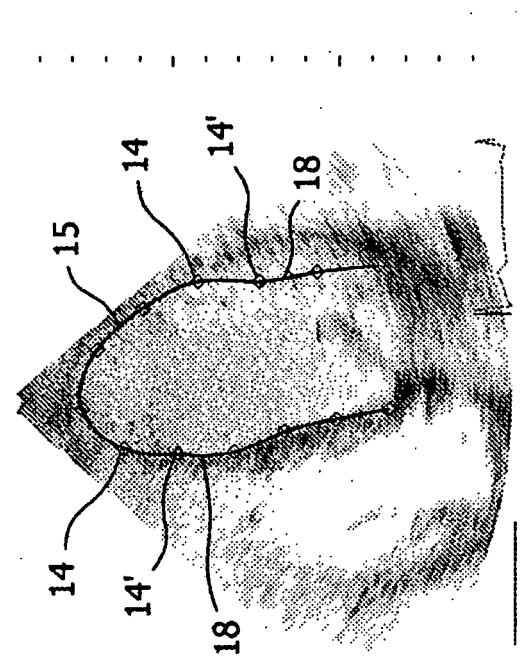


FIG. 3b

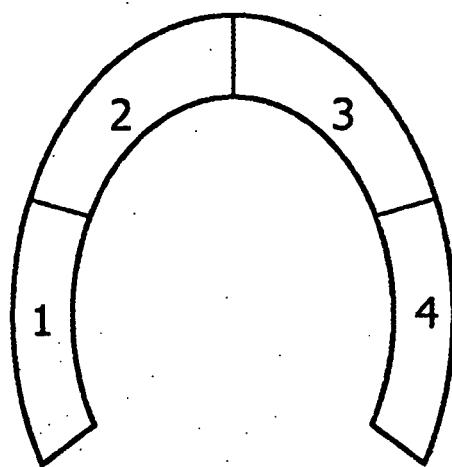


FIG. 4

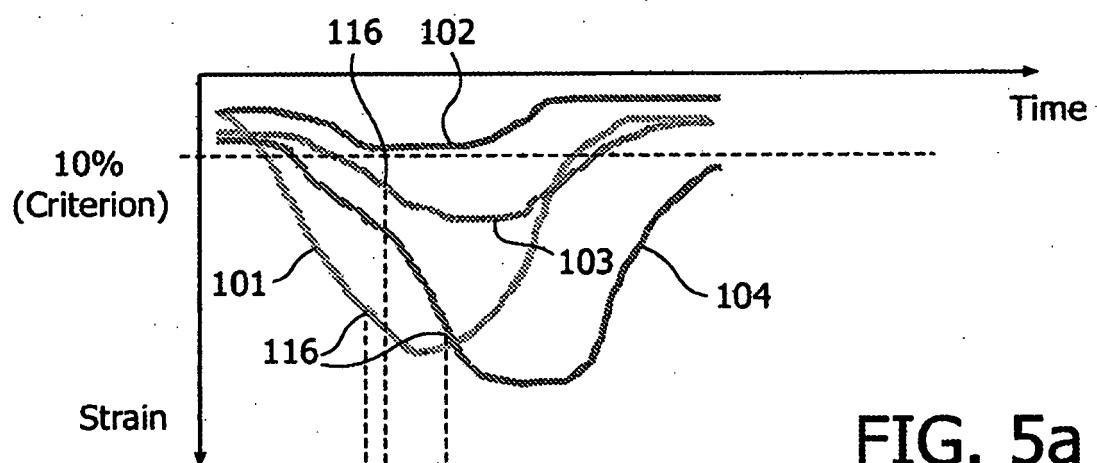


FIG. 5a

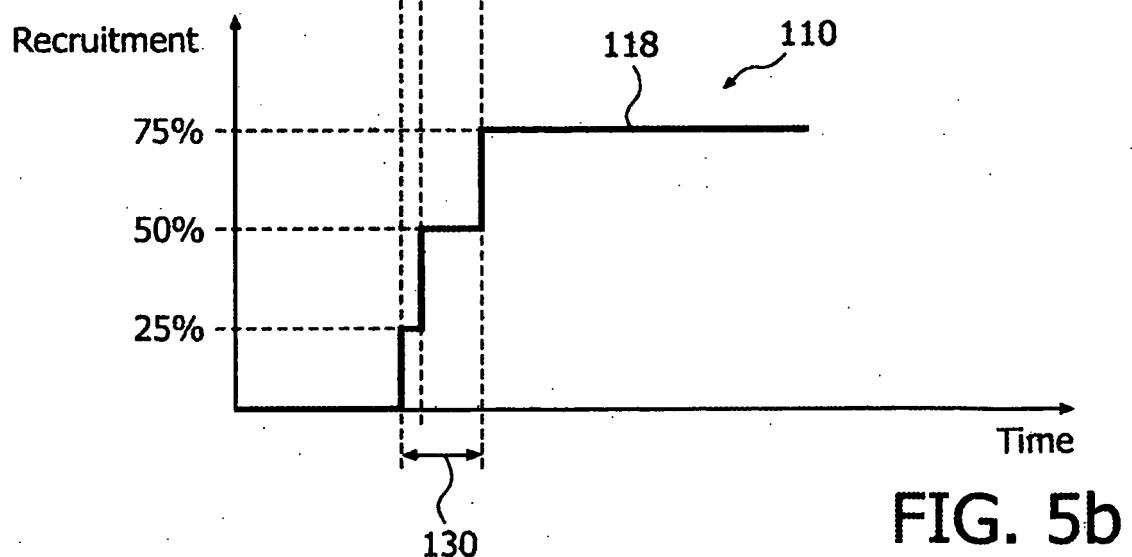


FIG. 5b

Recruitment Strain Criterion (%): 20

Recruitment Strain Milestone (% max): 85

● Radial Strain Recruitment

○ Circ. Strain Recruitment

FIG. 6

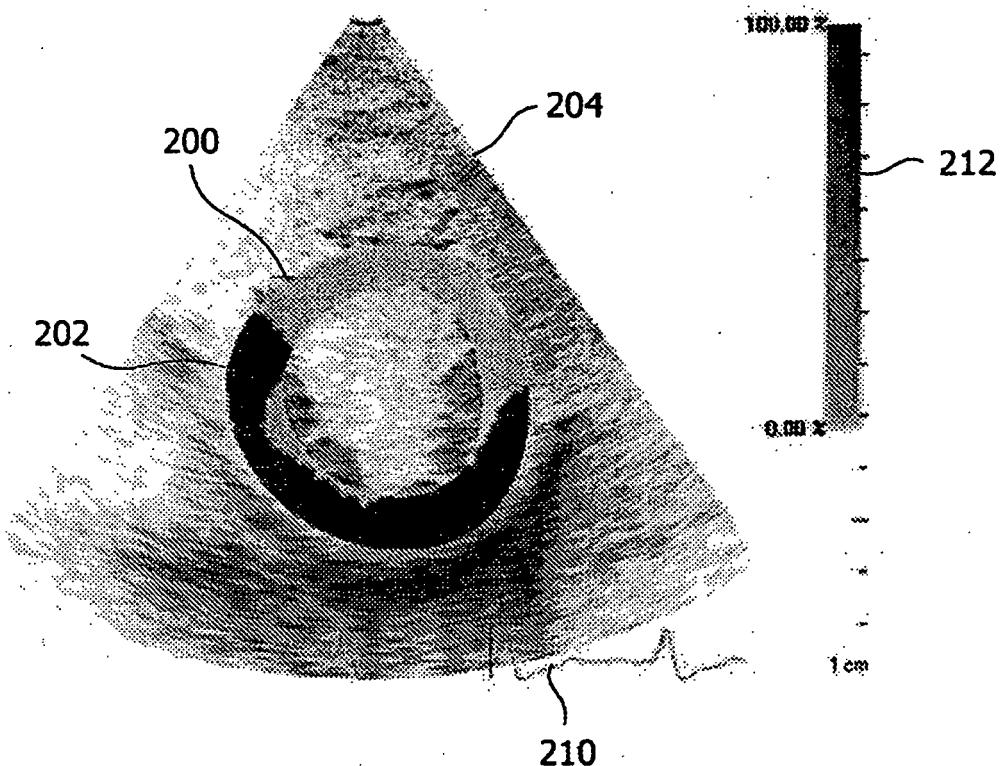


FIG. 7

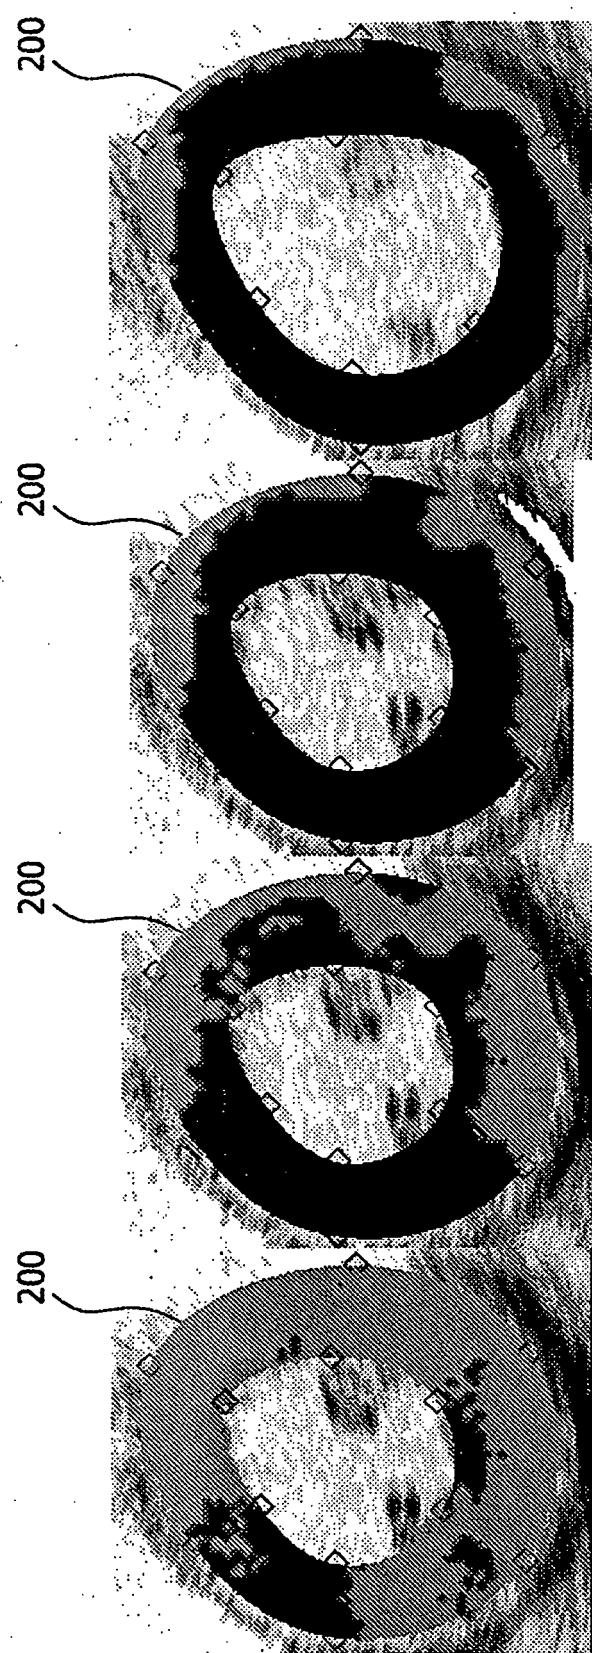


FIG. 8a FIG. 8b

FIG. 8c

FIG. 8d

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- EP 1804078 A1 [0003]
- US 2004254486 A1 [0003]
- US 6013032 A, Savord [0010]
- US 6375617 B, Fraser [0010]
- US 5833613 A [0010]
- US 6692438 B [0011]
- US 6186950 B [0011]
- US 5720291 A [0012]
- US 5474073 A [0012]
- US 5485842 A [0012]
- US 20050075567 A [0013]
- US 2005054898 W [0013]
- US 6491636 B [0013]
- US 6442289 B, Olsson [0015]
- WO 2007138522 W [0015]
- US 5797396 A, Geiser [0018]
- US 6537221 B, Criton [0020]

专利名称(译)	超声评估心脏同步性和活力		
公开(公告)号	EP2309931B1	公开(公告)日	2013-12-11
申请号	EP2009786490	申请日	2009-06-30
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	SALGO IVAN SETTLEMIER SCOTT CHANG PETER		
发明人	SALGO, IVAN SETTLEMIER, SCOTT CHANG, PETER		
IPC分类号	A61B8/08 G01S7/52 G06T7/00 A61B8/00 G01S15/89 G06T7/20 A61B5/0456		
CPC分类号	A61B8/08 A61B5/0456 A61B8/0883 A61B8/483 A61B8/485 A61B8/543 G01S7/52042 G01S7/52071 G01S15/8993 G06T7/248 G06T2207/10132 G06T2207/30048		
优先权	61/079663 2008-07-10 US		
其他公开文献	EP2309931A1		
外部链接	Espacenet		

摘要(译)

超声成像系统在心动周期期间产生心脏的图像序列。分析图像以确定心肌的节段的运动，位移或大小的变化。在优选实施例中，所确定的值是径向，纵向或周向心肌应变值。可以通过斑点跟踪或边界检测在心动周期期间跟踪心肌节段的位移。分析段的尺寸值的运动，位移或变化，以产生收集曲线和解剖显示，其显示在心脏的收缩和松弛运动中不同段的收集的相对时间。参与和实现充分招募可以通过与初始招聘阈值标准和预定最大招聘里程碑水平的比较来确定。

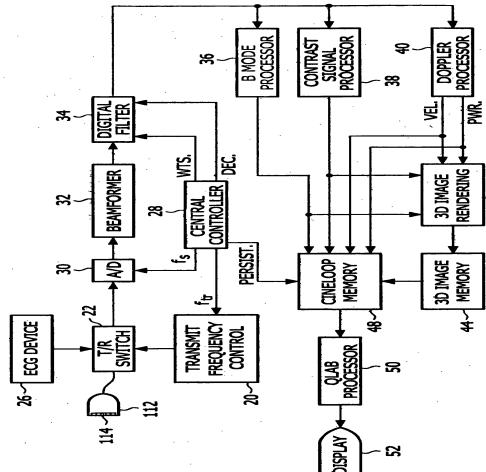


FIG. 1