



(11)

EP 2 582 302 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
14.05.2014 Bulletin 2014/20

(21) Application number: **11722913.8**

(22) Date of filing: **27.04.2011**

(51) Int Cl.:
A61B 8/02 (2006.01) A61B 8/08 (2006.01)

(86) International application number:
PCT/IB2011/051853

(87) International publication number:
WO 2011/158136 (22.12.2011 Gazette 2011/51)

(54) **AUTOMATED HEART RATE DETECTION FOR 3D ULTRASONIC FETAL IMAGING**

AUTOMATISCHE HERZFREQUENZERFASSUNG FÜR FETALE 3D-ULTASCHALLBILDGEBUNG
DETECTION AUTOMATIQUE DE LA FREQUENCE CARDIAQUE POUR IMAGERIE FOETALE 3D
A ULTRASONS

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **17.06.2010 US 355885 P**

(43) Date of publication of application:
24.04.2013 Bulletin 2013/17

(73) Proprietor: **Koninklijke Philips N.V.
5656 AE Eindhoven (NL)**

(72) Inventor: **SCHAUF, Michael
NY 10510-8001 (US)**

(74) Representative: **van Velzen, Maaïke Mathilde
Philips
Intellectual Property & Standards
P.O. Box 220
5600 AE Eindhoven (NL)**

(56) References cited:
WO-A1-2011/001309

- BREKKE S ET AL: "2H-6 Tissue Doppler Gated (TDG) Real-Time Stitching in Three-Dimensional Fetal Echocardiography", ULTRASONICS SYMPOSIUM, 2006. IEEE, IEEE, PI, 1 October 2006 (2006-10-01), pages 764-767, XP031076369, DOI: 10.1109/ULTSYM.2006.165 ISBN: 978-1-4244-0201-4

- CHAOUI R ET AL: "Three and four dimensional fetal echocardiography", DER GYNÄKOLOGE, SPRINGER, BERLIN, DE, vol. 39, no. 1, 1 January 2006 (2006-01-01), pages 15-24, XP019323083, ISSN: 1433-0393, DOI: 10.1007/S00129-005-1782-1
- KARADAYI K ET AL: "Automatic Image-based Gating for 4D Ultrasound", CONFERENCE PROCEEDINGS. ANNUAL INTERNATIONAL CONFERENCE OF THE IEEE ENGINEERING IN MEDICINE AND BIOLOGY SOCIETY (IEEE CAT. NO. 06CH37748); 30 AUG.-3 SEPT. 2006; NEW YORK, NY, USA, IEEE, PISCATAWAY, NJ, USA, 30 August 2006 (2006-08-30), pages 2388-2391, XP031339478, ISBN: 978-1-4244-0032-4
- DENG J ET AL: "Online motion-gated dynamic three-dimensional echocardiography in the fetus-preliminary results", ULTRASOUND IN MEDICINE AND BIOLOGY, NEW YORK, NY, US, vol. 27, no. 1, 1 January 2001 (2001-01-01), pages 43-50, XP004295663, ISSN: 0301-5629, DOI: 10.1016/S0301-5629(00)00313-6
- DENG J ET AL: "Conversion of umbilical arterial doppler waveforms to cardiac cycle triggering signals: a preparatory study for online motion-gated three-dimensional fetal echocardiography", ULTRASOUND IN MEDICINE AND BIOLOGY, NEW YORK, NY, US, vol. 27, no. 1, 1 January 2001 (2001-01-01), pages 51-59, XP004295664, ISSN: 0301-5629, DOI: 10.1016/S0301-5629(00)00315-X

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 582 302 B1

- DENG J ET AL: "Simultaneous use of two ultrasound scanners for motion-gated three-dimensional fetal echocardiography", **ULTRASOUND IN MEDICINE AND BIOLOGY**, NEW YORK, NY, US, vol. 26, no. 6, 1 July 2000 (2000-07-01), pages 1021-1032, XP004295636, ISSN: 0301-5629, DOI: 10.1016/S0301-5629(00)00220-9

Description

[0001] This invention relates to medical diagnostic systems and, in particular, to ultrasonic diagnostic imaging systems for diagnosing the fetal heart by three dimensional (3D) imaging.

[0002] Ultrasound is well suited for fetal imaging because it performs noninvasive imaging without exposing either the mother or the fetus to ionizing radiation. An objective of many fetal examinations is to assess the development of the fetal anatomy to determine whether the fetus is developing normally. As ultrasound image quality has improved over the years, more areas of the anatomy can be visualized for development assessment and in greater detail. Consequently fetal ultrasound exams have become more thorough with increased requirements for anatomy which is to be inspected. One area of the anatomy which is greatly scrutinized is the developing fetal heart. In recent years the outflow tracts of the heart have become a focus of greater attention. The cardiac outflow tracts of the fetal heart can be difficult to image, however. One reason for this is the small size of this fetal anatomy. Another reason is that it is desirable to not simply view the anatomy, but also the dynamics of the flow characteristics through the outflow tracts over the full fetal heart cycle. A further reason is that the outflow tracts undergo considerable development as the fetus grows, and consequently can have varying appearances and complexity depending on fetal age. The outflow tracts can thus be difficult to identify on the ultrasound display, and it can be even more difficult to acquire an image frame of the proper orientation for an adequate diagnosis.

[0003] Some of these demands have been eased by the recent use of 3D ultrasound to image the fetal heart. With 3D imaging, the full fetal heart can be imaged and a sequence of 3D image data sets can be acquired for later replay and diagnosis. When data of the full fetal heart is acquired in the data sets, the image data can be examined during post-acquisition diagnosis to locate the outflow tracts of the heart. Different varying 2D image planes can be extracted from the 3D data in multiplanar reconstruction (MPR), so that an image plane of a desired orientation can be examined. Three dimensional imaging thus addresses many of the static imaging challenges which are problematic with 2D fetal imaging. Recently the problem of analyzing the temporal dynamics of fetal blood flow have been addressed by a technique called "spatial-temporal image correlation," or STIC. With STIC, a sweep is made through the fetal heart with ultrasound and many image frames are acquired over a sequence of heart cycles. When done by manually scanning with a 2D ultrasound probe, this image acquisition can take ten seconds or longer. The same acquisition can be performed with a mechanical 3D probe which mechanically sweeps the image plane through the fetal heart region, but 3D mechanical probes often have poorer elevation focus which leads to inaccuracies when constructing

MPR images in the elevation dimension. After the acquisition is complete and the image frames are stored, image frames of the desired anatomy, created by MPR reconstruction if necessary, are reassembled into a loop of images according to their phase sequence in the fetal heart cycle. This task is made difficult by the fact that no ECG signal of the fetal heart is available for this reordering. A fetal ECG cannot be acquired during imaging since ECG electrodes cannot be attached to the fetus and the fetal electrical impulses are overwhelmed by the mother's own ECG signals. Consequently it is necessary to extract a synthetic timing signal of the fetal heart cycle from the fetal heart images. This is done by determining event triggers based on fetal tissue movement at or near the heart as described in US Pat. 7,261,695 (Brekke et al.) The synthetic heart cycle trigger signals are then used to reorder the images from multiple heart cycles into one loop of a heart cycle in which the frames are in heart beat phase order.

[0004] The STIC technique is not without its difficulties however. One is the robustness of the reassembly algorithm. Since the typical acquisition creates far too many images to reorder manually, algorithms have been developed to do the reordering of the frames automatically. These algorithms are dependent upon image data quality, which can be less than adequate. Efforts have been made to improve this situation by using recommended manipulation of the probe to acquire optimal data sets, but this is technique-dependent and its use of anatomical statistics can cause it to be individual patient-dependent. But a greater problem is that the fetus frequently moves and may not remain stationary during the full ten or more seconds needed for data acquisition. When the fetus moves the orientation of the desired image data relative to the probe will change, and may leave the field of view entirely, resulting in an absence of the desired anatomy from the acquired data set. Also, fetal movement during the acquisition limits the accuracy of the derived synthetic fetal heart cycle, which introduces artifacts into the reconstructed 3D data.

[0005] An alternative to STIC which addresses these problems is described in Brekker S. et al, "Tissue Doppler Gated (TDOG) Real-Time Stitching in Three-Dimensional Fetal Echocardiography", 2006 IEEE ULTRASONICS SYMPOSIUM, pages 764-767. That article, representing the closest prior art document for the invention, suggests a real-time gating signal for fetal echocardiography. An ultrasound system discussed in the article was set up to acquire 3D gray-scale data and 3D tissue Doppler data simultaneously, with only the gray-scale data visible to the sonographer. Derived from the Doppler data, a gating signal was calculated in real-time. The gating signal trigger events were used to induce changes in the geometry setup of the 3D gray-scale scan, ensuring that data from consecutive cardiac cycles were captured from separate parts of the total volumetric scan.

[0006] Similar problems were addressed in U.S. patent application publication US 2012/0123267A1 by Jago et

al. and entitled THREE DIMENSIONAL FETAL HEART IMAGING BY NON-ECG PHYSIOLOGICAL GATED ACQUISITION. In that application, a diagnostic ultrasound system is described which acquires 3D fetal heart data sets gated to the fetal heart cycle by a physiologically derived gating signal. The fetal heart is imaged by either 1D, 2D or 3D imaging and echo signals from a target exhibiting suitable motion are acquired. For fetal heart imaging the target could be the heart muscle of the fetus or motion of blood in the fetal carotid artery, for example. The motion signals are processed to produce a gating signal synchronized to the fetal heart cycle, which is used to gate 3D image data acquisition. Three dimensional data sets are then acquired in timed relation to the phase of the fetal heartbeat using this physiologically derived gating signal. Gating of acquisition in 3D is much easier to achieve with a 2-dimensional matrix transducer incorporating a micro-beamformer, since in this case imaging planes can be generated electronically in any sequence or orientation. Using such a matrix transducer, a loop of a heart cycle can generally be acquired in less than one second and several loops can be acquired in only a few seconds. Since the acquired image data is already in phase with the fetal heart cycle there is no need to reorder the image data, and since the acquisition takes only a few seconds, fetal movement is less of a concern. One other advantage of this approach, compared to STIC, is that the user can be presented with reconstructed images that show the quality of the acquisition, so that the user can decide if any motion artifacts are present before completing the data acquisition. If the fetus does move during the short acquisition interval the probe can be repositioned and another 3D data acquisition performed. The successfully acquired 3D data can thereafter be carefully analyzed during post-acquisition diagnosis. It is desirable to provide a workflow for the clinician which makes such a system easy to use. In particular it is desirable for the system workflow to easily and reliably acquire the physiologically derived gating signal, to know when a stable gating signal is being produced, and to enable the clinician to promptly acquire the desired loops of the fetal heart with the gating signal.

[0007] In accordance with the principles of the present invention, a diagnostic ultrasound has a workflow and controls which facilitate acquisition of a loop of 3D fetal heart images with a synthetically derived heart gating signal. The heart rate is derived during 3D imaging without the need to exit to another imaging mode. The workflow enables the clinician to set a 3D region of interest (ROI) about the fetal heart, then automatically acquire the fetal heart rate. When the clinician presses the "triggered" control, the system begins to acquire the fetal heart rate, and provides feedback to the clinician when a suitable heart rate signal is being acquired. The clinician then presses a "start" control to initiate triggered 3D acquisition. Within a second or two the triggered 3D image acquisition is complete and the image loops are ready for post-acquisition analysis.

[0008] In the drawings:

FIGURE 1 illustrates in block diagram form an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention. FIGURE 2 illustrates a typical ultrasound system on which a 3D fetal heart imaging system of the present invention has been implemented.

FIGURE 3 is a flowchart of a workflow of the present invention for acquiring a trigger signal for fetal heart imaging, then using the trigger signal for 3D image acquisition.

FIGURE 4 illustrates a control panel in accordance with the present invention for setting an ROI of the fetal heart.

FIGURE 5 illustrates a 3D display which is suitable for use in carrying out the fetal heart acquisition workflow of the present invention.

FIGURES 6a and 6b illustrate a control panel for optionally acquiring a trigger signal either manually or automatically.

FIGURE 7 illustrates one technique for automatically acquiring a fetal heart trigger signal.

FIGURE 8 illustrates a 3D display which additionally displays an M mode image which supports and provides user confidence in the synthetically derived fetal heart rate signal.

[0009] Referring first to FIGURE 1, an ultrasound system 10 constructed in accordance with the principles of the present invention is shown in block diagram form. The ultrasound system is configured by two subsystems, a front end acquisition subsystem 10A and a display subsystem 10B. An ultrasound probe is coupled to the acquisition subsystem which includes a two-dimensional matrix array transducer 70 and a micro-beamformer 72. The micro-beamformer contains circuitry which control the signals applied to groups of elements ("patches") of the array transducer 70 and does some processing of the echo signals received by elements of each group. Micro-beamforming in the probe advantageously reduces the number of conductors in the cable between the probe and the ultrasound system and is described in US Pat. 5,997,479 (Savord et al.) and in US Pat. 6,436,048 (Pesque).

[0010] The probe is coupled to the acquisition subsystem 10A of the ultrasound system. The acquisition subsystem includes a beamform controller 74 which is responsive to a user control 36 and provides control signals to the microbeamformer 72, instructing the probe as to the timing, frequency, direction and focusing of transmit beams. The beamform controller also control the beamforming of echo signals received by the acquisition subsystem by its control of analog-to-digital (A/D) converters 18 and a beamformer 20. Echo signals received by the probe are amplified by preamplifier and TGC (time gain control) circuitry 16 in the acquisition subsystem, then digitized by the A/D converters 18. The digitized echo

signals are then formed into fully steered and focused beams by a beamformer 20. The echo signals are then processed by an image processor 22 which performs digital filtering, B mode and M mode detection, and Doppler processing, and can also perform other signal processing such as harmonic separation, speckle reduction, and other desired image signal processing.

[0011] The echo signals produced by the acquisition subsystem 10A are coupled to the display subsystem 10B, which processes the echo signals for display in the desired image format. The echo signals are processed by an image line processor 24, which is capable of sampling the echo signals, splicing segments of beams into complete line signals, and averaging line signals for signal-to-noise improvement or flow persistence. The image lines for a 2D image are scan converted into the desired image format by a scan converter 26 which performs R-theta conversion as is known in the art. The image is then stored in an image memory 28 from which it can be displayed on a display 38. The image in memory is also overlaid with graphics to be displayed with the image, which are generated by a graphics generator 34 which is responsive to the user control 36. Individual images or image sequences can be stored in a cine memory 30 during capture of image loops or sequences.

[0012] For real-time volumetric imaging the display subsystem 10B also includes a 3D image rendering processor 32 which receives image lines from the image line processor 24 for the rendering of real-time three dimensional images. The 3D images can be displayed as live (real time) 3D images on the display 38 or coupled to the image memory 28 for storage of the 3D data sets for later review and diagnosis.

[0013] In accordance with the principles of the present invention a fetal heart rate synthesizer produces a heart rate trigger signal for gated 3D acquisition of fetal heart images. In the implementation of FIGURE 1, the fetal heart rate synthesizer comprises a motion estimator 40 which receives temporally discrete echo signals from a designated location of the imaged anatomy, an ROI, and processes the echoes to produce a signal representative of motion at the designated location. The location in the anatomy from which the temporally discrete echo signals are acquired can be a default image location such as the center of the image, or it can be a location designated by the user by manipulation of a control of the user controls 36. For instance, the user can manipulate a joystick, trackball, or other control of the user controls to locate a sample volume in the carotid artery of the fetus. Motion estimation can then be performed from samples of the moving fetal tissue or blood. Some of this processing may be performed by the image processor, such as Doppler processing of echo signals from the sample volume location. Flow or tissue motion velocity estimates produced by the image processor can then be forwarded directly to the motion estimator, for example. If the sample volume is placed on tissue such as the fetal heart muscle, the echo signals from the fetal heart can be processed

for motion discrimination by tissue Doppler processing. Another way to detect motion is by tracking the movement of speckle at a given tissue location in the image. Yet another way to detect motion is by comparing changes in tissue location over consecutive images by MSAD block matching as described in US Pat. 6,299,579 (Peterson et al.) Still another technique for detecting motion is to use M mode with the M line positioned through the fetal heart. This is illustrated in FIGURE 7, which shows an M mode image 60 produced by an M line located by positioning the M line cursor on the ultrasound image so that it extends through the left ventricle (LV) of the fetal heart. When positioned in this manner the M line will pass through the myocardial wall 12 on one side of the fetal heart, through the chamber of the LV, and through the myocardial tissue 14 on the other side of the heart. An ultrasound beam is transmitted along this M line direction through the LV periodically, and the received A-line from each transmission is shown on the display in a scrolling manner along the previously received A-lines. The result is an M mode image as shown in FIGURE 7 where the opposite sides of the heart are most greatly separated when the fetal heart is relaxed at the end diastole point in the heart cycle as indicated by arrow 52'. The opposite walls of the heart are in closest proximity at the peak systole phase of the heart cycle as indicated by arrow 54'. FIGURE 7 illustrates this cyclical pattern of the movement of the heart wall as the fetal heart contracts and expands with each heart beat. By tracking the changing position (motion) of the heart wall 12 or 14, a waveform in phase with the heart cycle can be produced by a heart cycle synthesizer 42 coupled to receive the fetal heart motion signals.

[0014] Other techniques of fetal heart rate detection such as frequency estimation of the fetal heart motion with peak frequency detection can also be used to develop a heart rate trigger signal. Once a trigger signal has been produced by these or any other technique, the heart rate trigger signal is applied to the beamformer controller 74 where it is used to gate the acquisition of fetal heart images. The heart rate signal is also coupled to the graphics generator 34 where it may be displayed as feedback to the user as discussed more fully below.

[0015] FIGURE 2 illustrates an ultrasound system 50 on which an embodiment of the present invention has been implemented. The system 50 includes a display 56 on which the acquired ultrasound images are displayed. Control of the ultrasound system is provided in two ways. One is the control panel 36 at the front of the system, which includes the trackball, buttons, and controls used for basic system operation. A touch screen display 58 is at the top of the control panel and displays softkeys for advanced features which can be changed periodically or for each step of a procedure. The softkeys of the touch screen display 58 are used extensively in the implementation of the present invention as described below.

[0016] FIGURE 3 is a flow chart showing the sequence of workflow of an implementation of the present invention.

This workflow sequence begins with a step 70 when the sonographer touches a softkey button on the touch screen display to enter the 3D biplane mode from the normal 3D imaging mode. FIGURE 4 illustrates the touch screen buttons displayed when the sonographer has entered the biplane mode. The 3D biplane mode is described in US Pat. 6,709,994 (Frisa et al.), and is a mode in which two planes of a volumetric region of the body are alternately imaged in rapid succession, thereby producing live images of each plane of the body. When the imaging system first enters the biplane mode, two images aligned with the center of the 2D array transducer and of orthogonal planes are scanned and displayed. With the biplane images shown on the image display 56, the sonographer in step 72 touches the "3D ROI" button shown on the touch screen display of FIGURE 4 at the bottom of the screen. This button turns on a dashed ROI outline on each biplane image which is produced by the graphics generator 34. FIGURE 5 illustrates two biplane images 102 and 104, each with a dashed trapezoidal ROI outline 106, 108 in the center of the image. When the fetal heart is positioned in the center of the initial 3D image, the two ROI outlines 106 and 108 will each define a region of interest which includes the fetal heart in the center of each biplane image 102 and 104.

[0017] With the fetal heart thus indicated by the ROIs, the sonographer enables auto-acquisition of a trigger signal in step 74 for gated acquisition of 3D images of the fetal heart. The sonographer first determines whether a manually set heart rate or an automatically determined heart rate is to be used for gated acquisition. This is done by setting an auto-acquisition mode button to the desired mode as shown by the "Acq Mode" button in FIGURES 6a and 6b. This button has two modes of operation, one in which the sonographer sets the heart rate manually (FIGURE 6a), and another where the trigger signal is automatically acquired (FIGURE 6b). When the manual mode has been selected, the notation "Estim HR" appears on the "Acq Mode" button as seen in FIGURE 6a. The sonographer then sets the heart rate manually by tapping on incrementing and decrementing arrows on either side of the heart rate number of the "Heart Rate" button just below the "Acq Mode" button. In the example of FIGURE 6a the heart rate value has been set to 60 bpm. The sonographer may elect to set the heart rate to the value previously indicated by the M mode display of heart motion, for instance.

[0018] If the "Acq Mode" button is in the manual mode, the sonographer can touch the button to toggle to the automatic mode, in which case "Auto" appears on the "Acq Mode" button as shown in FIGURE 6b. The sonographer then touches the "Triggered" button above the "Acq Mode" button to acquire the fetal heart rate automatically as indicated by step 76 in FIGURE 3. The system then begins to estimate the fetal heart rate automatically by use of, for instance, one of the measurement techniques described above. As the system does this, the current automatically estimated heart rate value ap-

pears on the "Heart Rate" button and changes as the system updates its estimate of the fetal heart rate. When the estimate becomes stable, the system is ready for triggered acquisition of 3D fetal heart images. This stability is indicated by audible or visual feedback as indicated in step 78. For example, the dashed ROI outline can be one color initially (e.g., white or yellow) and can change to a second color (e.g., green) when the automatically detected heart rate has become stable. Another alternative is for the number of beats per minute on the "Heart Rate" button to turn green when the estimated heart rate has become stable. When the detected heart rate has become stable, the sonographer touches the "Start" button (step 80 of FIGURE 3) at the upper left of the touch screen display 58 as seen in FIGURE 6b. The ultrasound system will then use the automatically determined trigger signal to acquire gated 3D fetal images over a number of heartbeats, such as four heartbeats. The acquired images are stored and are ready for subsequent replay and diagnosis.

[0019] At the end of 3D image acquisition, the constructed system displays the biplane images 102, 104 as shown in FIGURE 8 with an M mode display 110 below the biplane images. A M line such as M line 112 or M line 114 indicates the location in the anatomy where the M mode display was acquired. The sonographer can have confidence in the automatically acquired gated 3D images by viewing the M mode display 110, which was acquired at the same time as the gated 3D images. When the M mode display shows a steady cyclical pattern of heart motion, the sonographer can be confident that the trigger signal estimated from the M mode display was stable and suitable for use as a fetal gating signal.

Claims

1. An ultrasonic diagnostic imaging system (10) for gated acquisition of 3D fetal heart images comprising:
 - an ultrasound probe including a two dimensional array transducer (70) adapted for 3D fetal imaging;
 - an image processor (22) adapted to process image signals from the probe for display;
 - an image display (38) coupled to the image processor (22);
 - a user control (36) having a plurality of user-operable controls;
 - a graphics generator (34) responsive to a user control (36) which identifies a region of interest (ROI) in an ultrasound image;
 - a user control adapted to initiate processing of ultrasound data identified by the ROI to determine a fetal heart rate;
 - an indicator responsive to the processing of ultrasound data to determine a fetal heart rate which indicates that a fetal heart rate has been

- determined; and
 an acquisition control adapted to be actuated by
 a user to acquire gated 3D fetal heart images
 when the indicator indicates that a fetal heart
 rate has been determined. 5
2. The ultrasonic diagnostic imaging system of Claim
 1, wherein the user control adapted to initiate
 processing of ultrasound data identified by the ROI
 is further adapted to actuate a heart cycle synthe- 10
 sizer (42) responsive to echo signals received from
 the ROI to produce a synthetic fetal heart rate signal.
3. The ultrasonic diagnostic imaging system of Claim
 2, wherein the heart cycle synthesizer is responsive 15
 to estimates of motion produced by a motion estima-
 tor (40) in response to echo signals received from
 the ROI.
4. The ultrasonic diagnostic imaging system of Claim 20
 2, wherein the heart cycle synthesizer is responsive
 to estimates of frequency produced in response to
 echo signals received from the ROI.
5. The ultrasonic diagnostic imaging system of Claim 25
 1, wherein the indicator produces a visual or audible
 indication when a fetal heart rate has been deter-
 mined.
6. The ultrasonic diagnostic imaging system of Claim 30
 5, wherein the indicator produces a visual indication
 in conjunction with the display of an ultrasound im-
 age.
7. The ultrasonic diagnostic imaging system of Claim 35
 5, wherein the visual indication is produced in con-
 junction with a user control.
8. The ultrasonic diagnostic imaging system of Claim 40
 1, wherein the acquisition control is further adapted
 to acquire gated 3D fetal heart images for a plurality
 of heart cycles in synchronism with the determined
 fetal heart rate.
9. The ultrasonic diagnostic imaging system of Claim 45
 1, further comprising a user control by which a user
 can manually set a fetal heart rate.
10. A method for acquiring 3D fetal heart images gated 50
 by a synthetic fetal heart rate signal comprising:
- acquiring ultrasound images of a fetal heart;
 defining a region of interest (ROI) in an ultra-
 sound image which delineates the fetal heart in
 the image; 55
 using echo signals returned from the ROI to au-
 tomatically estimate the fetal heart rate;
 producing an indication that the fetal heart rate

has been estimated; and
 following the indication that the fetal heart rate
 has been estimated, acquiring gated 3D fetal
 heart images in synchronism with the estimated
 fetal heart rate.

11. The method of Claim 10, wherein producing an in-
 dication further comprises producing an audible or
 visual indication that a stable fetal heart rate has
 been estimated.
12. The method of Claim 10, wherein using echo signals
 to automatically estimate the fetal heart rate further
 comprises estimating the fetal heart rate by one of
 motion estimation or frequency estimation.
13. The method of Claim 10, wherein acquiring further
 comprises acquiring biplane images of the fetal
 heart;
 wherein defining an ROI further comprises defining
 an ROI (106,108) in each biplane image (102, 104).
14. The method of Claim 10, wherein acquiring gated
 3D fetal heart images further comprises acquiring
 gated 3D fetal heart images for a plurality of fetal
 heart cycles.
15. The method of Claim 10, further comprising display-
 ing an ultrasound image with an ROI defined therein,
 together with an M mode image (110) produced from
 ultrasound echo signals received from the ROI.

Patentansprüche

1. Diagnostisches Ultraschall-Bildgebungssystem (10)
 zur getriggerten Erfassung von 3D-Bildern des fetalen
 Herzens, das Folgendes umfasst:
- einen Schallkopf mit einem zweidimensionalen
 Array (70), das für die fetale 3D-Bildgebung aus-
 gelegt ist,
 - einen Bildprozessor (22), der für die Verarbei-
 tung von vom Schallkopf kommenden Bildsig-
 nalen für die Darstellung ausgelegt ist,
 - einen Monitor (38), der mit dem Bildprozessor
 (22) verbunden ist,
 - eine Benutzersteuerung (36) mit einer Vielzahl
 von vom Benutzer bedienbaren Bedienelemen-
 ten,
 - einen Grafikgenerator (34), der auf eine Be-
 nutzersteuerung (36) reagiert, die eine interes-
 sierende Region (ROI) in einem Ultraschallbild
 identifiziert,
 - eine Benutzersteuerung, die für die Initiierung
 der Verarbeitung von Ultraschalldaten ausge-
 legt ist, die von dem ROI identifiziert wurden,
 um eine fetale Herzfrequenz zu ermitteln,

- eine Anzeige, die auf die Verarbeitung von Ultraschalldaten zur Ermittlung einer fetalen Herzfrequenz reagiert und anzeigt, dass eine fetale Herzfrequenz ermittelt wurde, und
 - ein Aufnahme-Bedienelement, das für die Betätigung durch einen Benutzer ausgelegt ist, um getriggerte 3D-Bilder des fetalen Herzens zu erfassen, wenn die Anzeige anzeigt, dass eine fetale Herzfrequenz ermittelt wurde.
2. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei die Benutzersteuerung, die für die Initiierung der Verarbeitung von Ultraschalldaten ausgelegt ist, die von dem ROI identifiziert wurden, ferner dafür ausgelegt ist, einen Herzzyklus-Synthesizer (42) zu aktivieren, der auf von dem ROI empfangene Echosignale reagiert, indem er ein synthetisches fetales Herzfrequenzsignal erzeugt.
3. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 2, wobei der Herzzyklus-Synthesizer auf Schätzungen der Bewegungen reagiert, die von einer Bewegungsermittlungseinheit (40) als Reaktion auf die von dem ROI empfangenen Echosignale erzeugt werden.
4. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 2, wobei der Herzzyklus-Synthesizer auf Schätzungen der Frequenz reagiert, die als Reaktion auf die von dem ROI empfangenen Echosignale erzeugt werden.
5. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei die Anzeige eine optische oder akustische Anzeige erzeugt, wenn eine fetale Herzfrequenz ermittelt wurde.
6. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 5, wobei die Anzeige eine optische Anzeige zusammen mit der Darstellung eines Ultraschallbildes erzeugt.
7. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 5, wobei die optische Anzeige zusammen mit einer Benutzersteuerung erzeugt wird.
8. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, wobei das Aufnahme-Bedienelement ferner für die Erfassung von getriggerten 3D-Bildern des fetalen Herzens während einer Vielzahl von Herzzyklen synchron mit der bestimmten fetalen Herzfrequenz ausgelegt ist.
9. Diagnostisches Ultraschall-Bildgebungssystem nach Anspruch 1, das ferner ein Bedienelement umfasst, mit dem der Benutzer manuell eine fetale Herzfrequenz einstellen kann.
10. Verfahren zur Erfassung von 3D-Bildern des fetalen Herzens, die durch ein synthetisches fetales Herzfrequenzsignal getriggert wird, wobei das Verfahren Folgendes umfasst:
- Erfassen von Ultraschallbildern eines fetalen Herzens,
 - Festlegen einer interessierenden Region (ROI) in einem Ultraschallbild, die das fetale Herz in dem Bild abgrenzt,
 - Verwenden von Echosignalen, die von dem ROI zurückkehren, um automatisch die fetale Herzfrequenz zu ermitteln,
 - Erzeugen einer Anzeige, dass die fetale Herzfrequenz ermittelt wurde und
 - im Anschluss an die Anzeige, dass die fetale Herzfrequenz ermittelt wurde, Erfassen von getriggerten 3D-Bildern des fetalen Herzens synchron mit der ermittelten fetalen Herzfrequenz.
11. Verfahren nach Anspruch 10, wobei die Erzeugung einer Anzeige ferner die Erzeugung einer akustischen oder optischen Anzeige, dass eine stabile fetale Herzfrequenz ermittelt wurde.
12. Verfahren nach Anspruch 10, wobei die Verwendung von Echosignalen zur automatischen Ermittlung der fetalen Herzfrequenz ferner die Ermittlung der fetalen Herzfrequenz entweder durch die Ermittlung von Bewegungen oder durch die Ermittlung von Frequenzen umfasst.
13. Verfahren nach Anspruch 10, wobei die Erfassung ferner die Erfassung von Zweiebenen-Bildern des fetalen Herzens umfasst, wobei die Festlegung eines ROI ferner die Festlegung eines ROI (106, 108) in jedem Zweiebenen-Bild (102, 104) umfasst.
14. Verfahren nach Anspruch 10, wobei die Erfassung von getriggerten 3D-Bildern des fetalen Herzens ferner die Erfassung von getriggerten 3D-Bildern des fetalen Herzens während einer Vielzahl von fetalen Herzzyklen umfasst.
15. Verfahren nach Anspruch 10, das ferner die Darstellung eines Ultraschallbildes mit einem darin festgelegten ROI zusammen mit einem M-Mode-Bild (110) umfasst, das ausgehend von den von dem ROI empfangenen Ultraschall-Echosignalen erzeugt wurde.

Revendications

1. Système d'imagerie diagnostique ultrasonique (10) pour l'acquisition synchronisée d'images cardiaques fœtales 3D, comprenant :

- une sonde ultrasonore comprenant un transducteur en réseau bidimensionnel (70) adapté pour l'imagerie foetale 3D ;
 - un processeur d'image (22) adapté pour traiter des signaux d'image à partir de la sonde pour l'affichage ;
 - un affichage d'image (38) couplé au processeur d'image (22) ;
 - une commande utilisateur (36) comportant une pluralité de commandes utilisables par utilisateur ;
 - un générateur graphique (34) répondant à une commande utilisateur (36) qui identifie une région d'intérêt (ROI) dans une image ultrasonore ;
 - une commande utilisateur adaptée pour commencer le traitement de données ultrasonores identifiées par la ROI pour déterminer une fréquence cardiaque foetale ;
 - un indicateur répondant au traitement de données ultrasonores pour déterminer une fréquence cardiaque foetale qui indique qu'une fréquence cardiaque foetale a été déterminée ; et
 - une commande d'acquisition adaptée pour être actionnée par un utilisateur pour acquérir des images cardiaques foetales 3D synthétisées lorsque l'indicateur indique qu'une fréquence cardiaque foetale a été déterminée.
2. Système d'imagerie diagnostique ultrasonique selon la revendication 1, dans lequel la commande utilisateur adaptée pour commencer un traitement de données ultrasonores identifiées par la ROI est en outre adaptée pour actionner un synthétiseur de révolution cardiaque (42) répondant à des signaux d'écho reçus à partir de la ROI pour produire un signal de fréquence cardiaque foetale synthétique.
3. Système d'imagerie diagnostique ultrasonique selon la revendication 2, dans lequel le synthétiseur de révolution cardiaque répond à des estimations de mouvement produites par un estimateur de mouvement (40) en réponse à des signaux d'écho reçus à partir de la ROI.
4. Système d'imagerie diagnostique ultrasonique selon la revendication 2, dans lequel le synthétiseur de révolution cardiaque répond à des estimations de fréquence produites en réponse à des signaux d'écho reçus à partir de la ROI.
5. Système d'imagerie diagnostique ultrasonique selon la revendication 1, dans lequel l'indicateur produit une indication visuelle ou audible lorsqu'une fréquence cardiaque foetale a été déterminée.
6. Système d'imagerie diagnostique ultrasonique selon la revendication 5, dans lequel l'indicateur produit une indication visuelle conjointement avec l'affichage d'une image ultrasonore.
7. Système d'imagerie diagnostique ultrasonique selon la revendication 5, dans lequel l'indication visuelle est produite conjointement avec une commande utilisateur.
8. Système d'imagerie diagnostique ultrasonique selon la revendication 1, dans lequel la commande d'acquisition est en outre adaptée pour acquérir des images cardiaques foetales 3D synchronisées pour une pluralité de cycles cardiaques en synchronisme avec la fréquence cardiaque foetale déterminée.
9. Système d'imagerie diagnostique ultrasonique selon la revendication 1, comprenant en outre une commande utilisateur par laquelle un utilisateur peut régler manuellement une fréquence cardiaque foetale.
10. Procédé pour acquérir des images cardiaques foetales 3D synchronisées par un signal de fréquence cardiaque foetale synthétique comprenant :
- l'acquisition d'images ultrasonores d'un coeur foetal ;
 - la définition d'une région d'intérêt (ROI) dans une image ultrasonore qui délimite le coeur foetal dans l'image ;
 - l'utilisation de signaux d'écho renvoyés à partir de la ROI pour estimer automatiquement la fréquence cardiaque foetale ;
 - la production d'une indication que la fréquence cardiaque foetale a été estimée ; et
 - suivant l'indication que la fréquence cardiaque foetale a été estimée, l'acquisition d'images cardiaques foetales 3D synchronisées en synchronisme avec la fréquence cardiaque foetale estimée.
11. Procédé selon la revendication 10, dans lequel la production d'une indication comprend en outre la production d'une indication audible ou visuelle qu'une fréquence cardiaque foetale stable a été estimée.
12. Procédé selon la revendication 10, dans lequel l'utilisation de signaux d'écho pour estimer automatiquement la fréquence cardiaque foetale comprend en outre l'estimation de la fréquence cardiaque foetale par une parmi l'estimation de mouvement ou l'estimation de fréquence.
13. Procédé selon la revendication 10, dans lequel l'acquisition comprend en outre l'acquisition d'images en deux plans du coeur foetal ; dans lequel la définition d'une ROI comprend en

autre la définition d'une ROI (106,108) dans chaque image en deux plans (102, 104).

14. Procédé selon la revendication 10, dans lequel l'acquisition d'images cardiaques fœtales 3D synchronisées comprend en outre l'acquisition d'images cardiaques fœtales 3D synchronisées pour une pluralité de cycles cardiaques fœtaux. 5
15. Procédé selon la revendication 10, comprenant en outre l'affichage d'une image ultrasonore avec une ROI définie dans celle-ci, conjointement avec une image en mode M (110) produite à partir de signaux d'écho ultrasonore reçus à partir de la ROI. 10

15

20

25

30

35

40

45

50

55

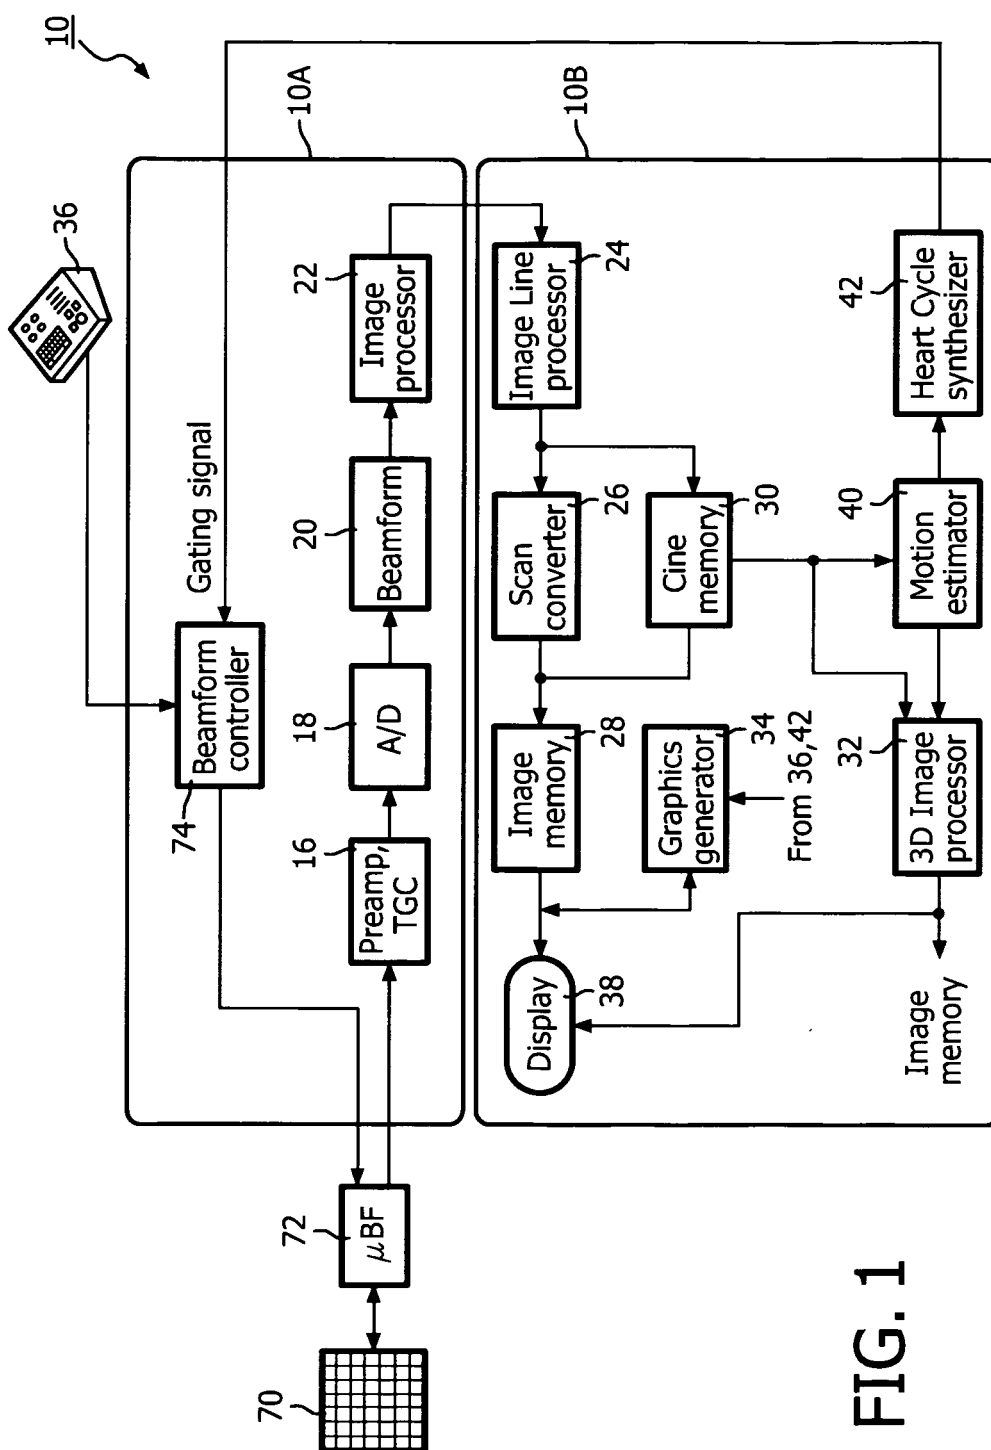


FIG. 1

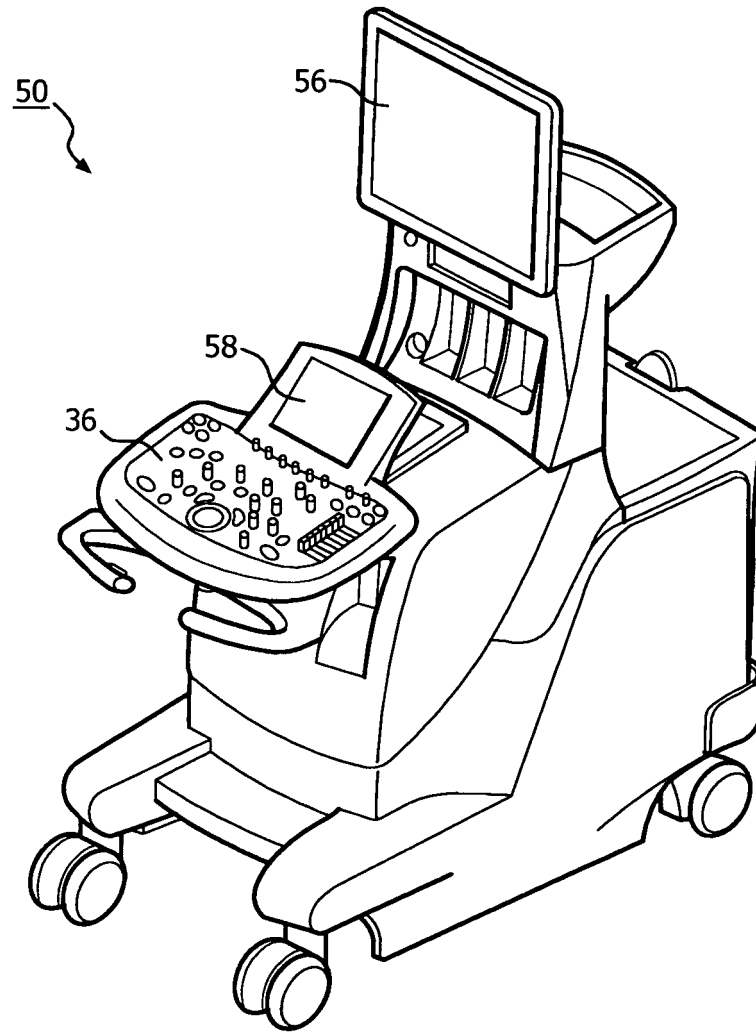
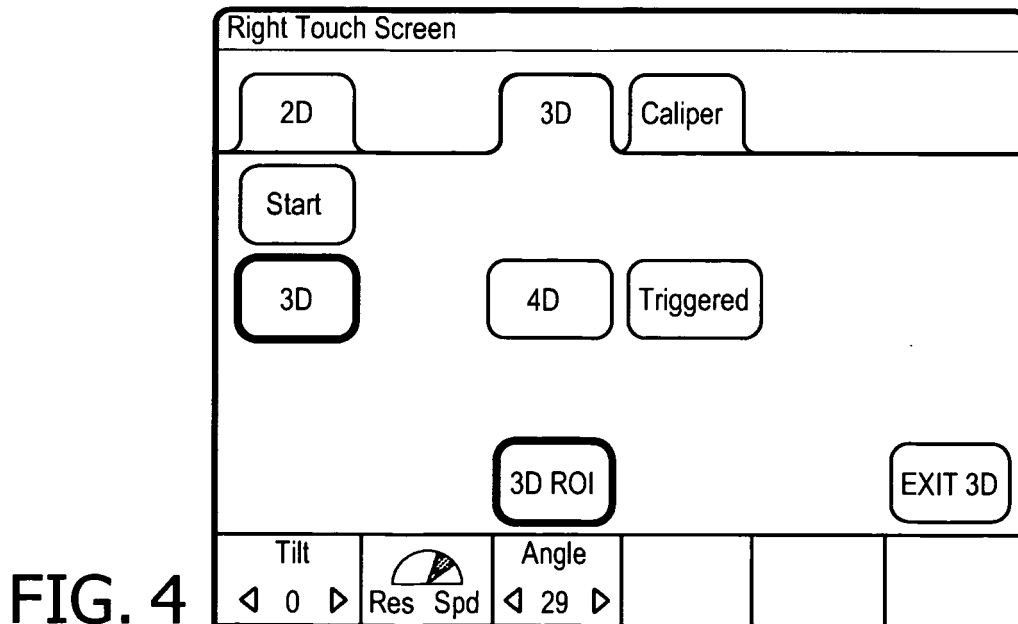
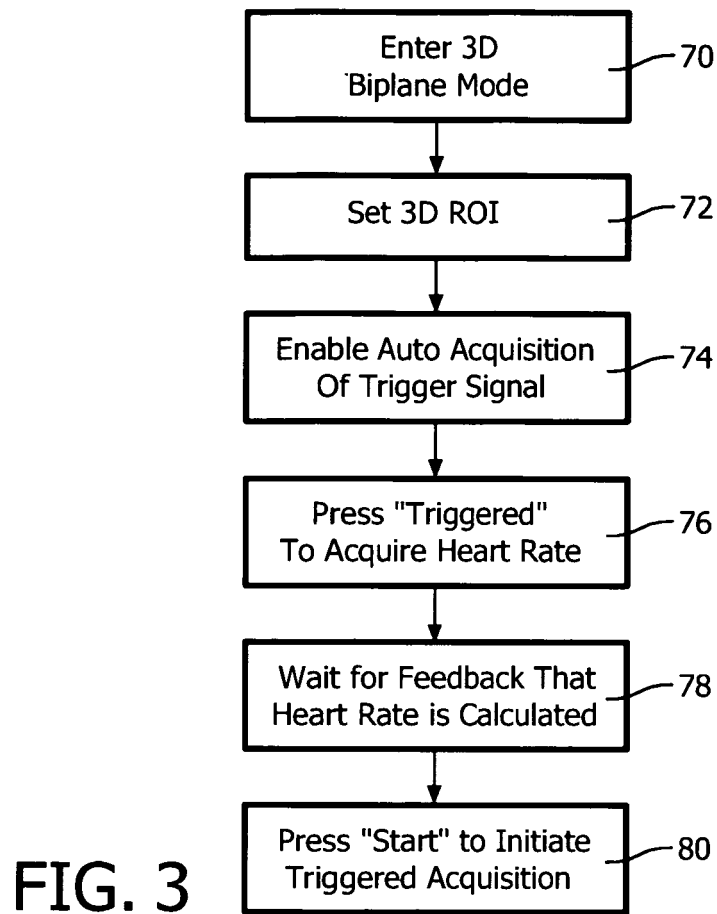


FIG. 2



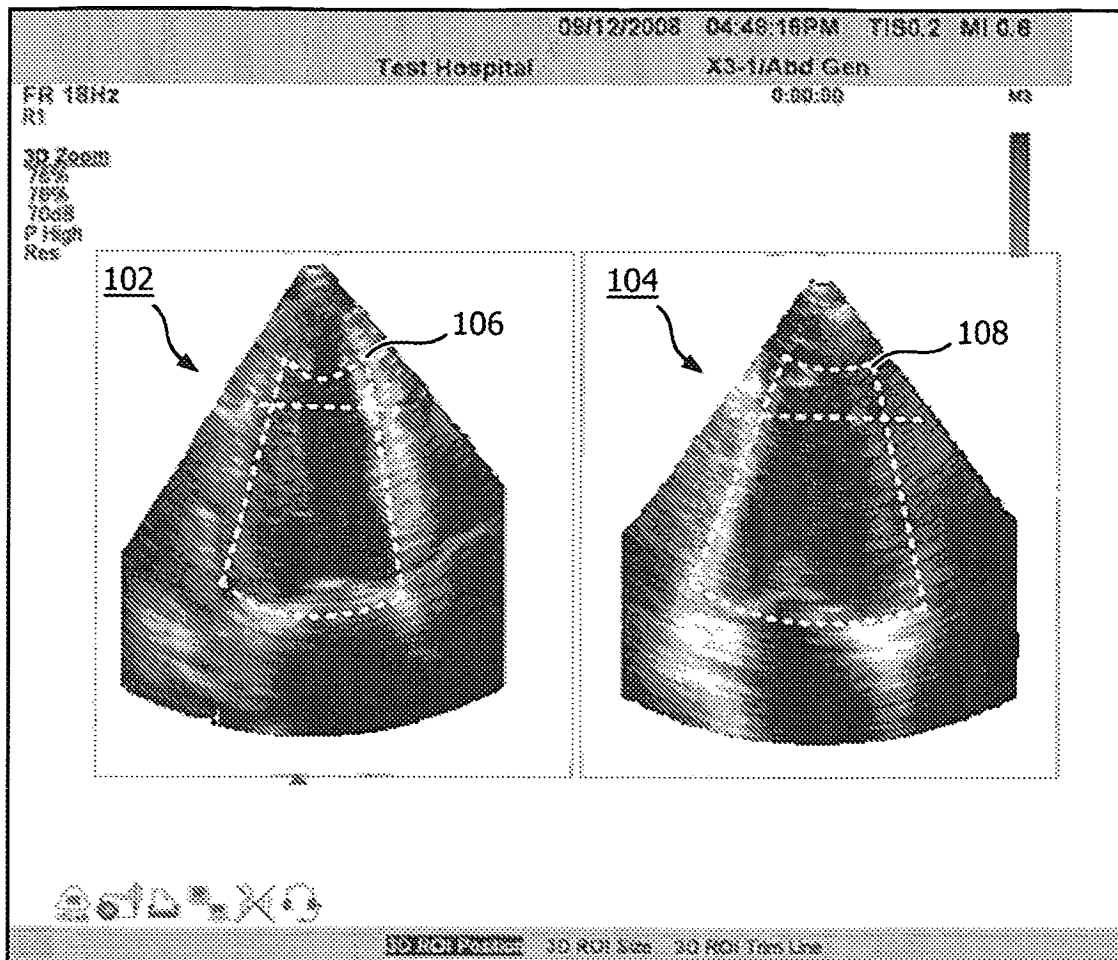


FIG. 5

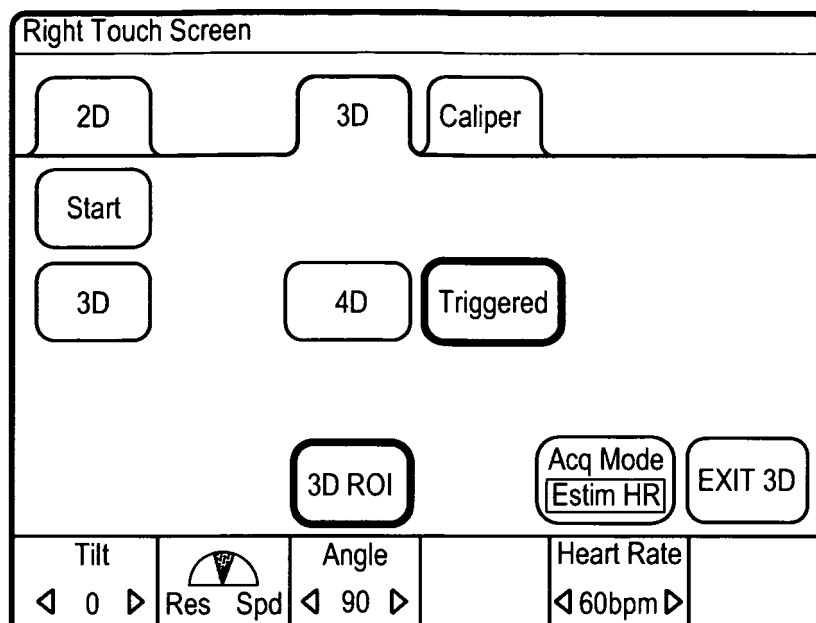


FIG. 6a

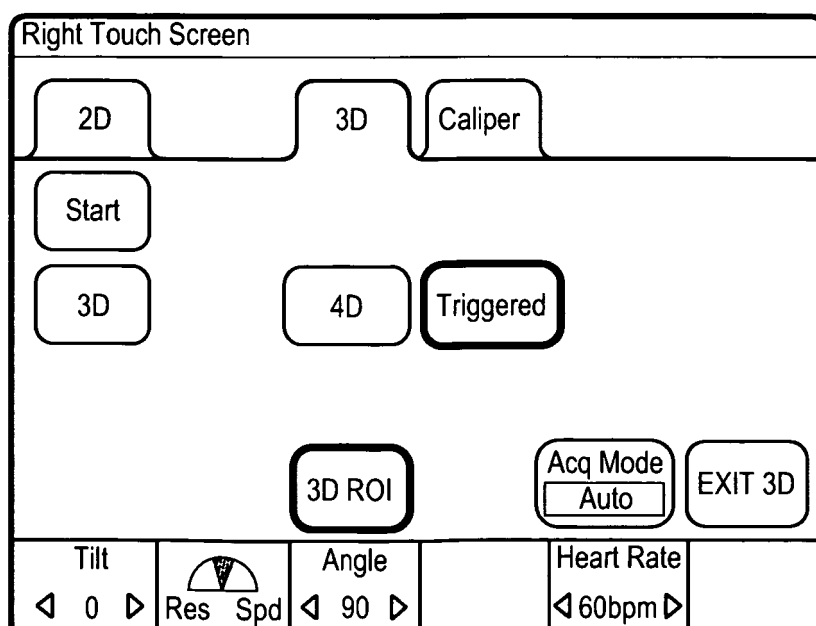


FIG. 6b

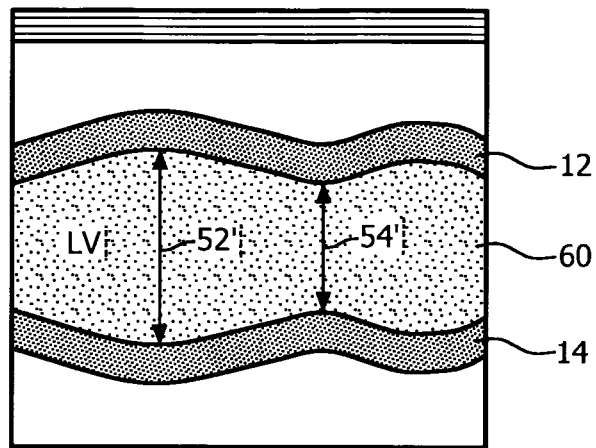


FIG. 7

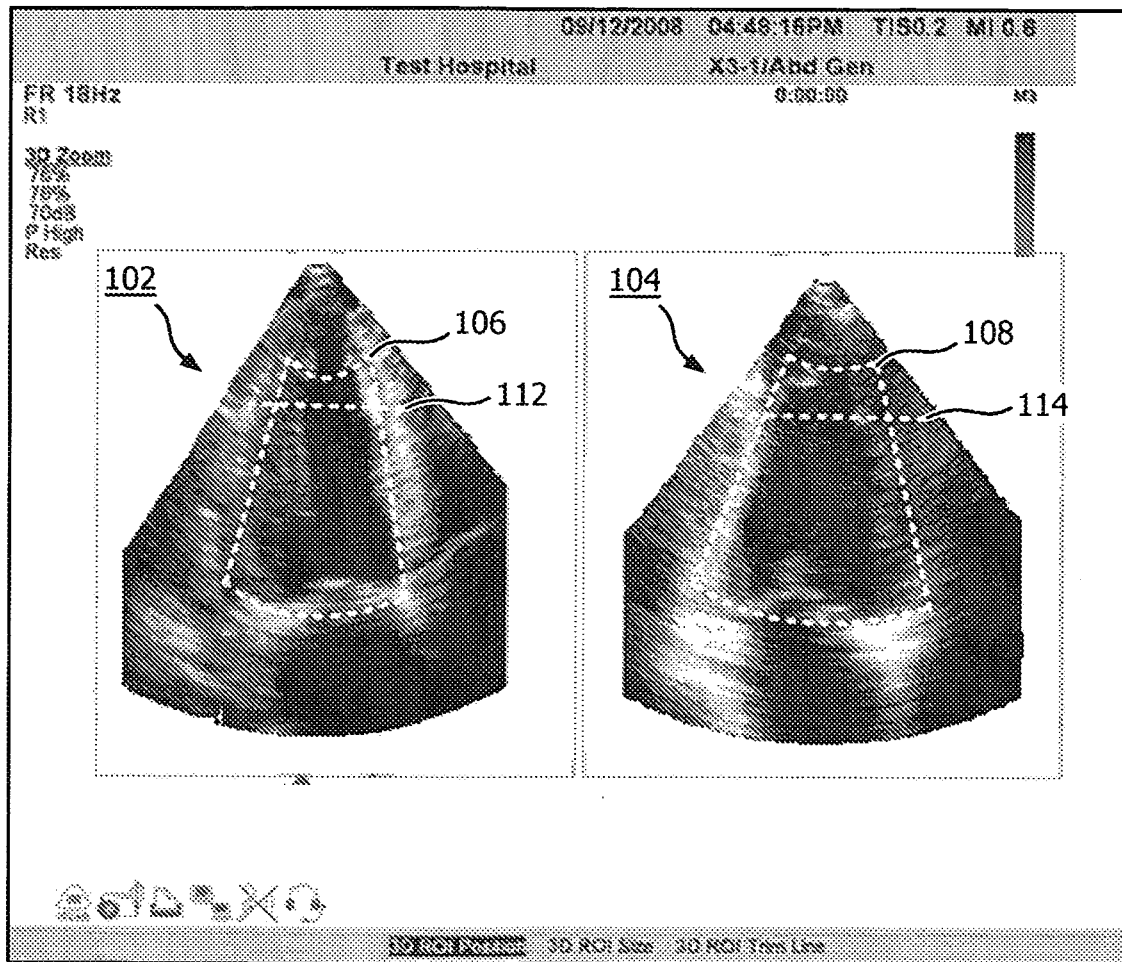


FIG. 8

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 7261695 B, Brekke [0003]
- US 20120123267 A1, Jago [0006]
- US 5997479 A, Savord [0009]
- US 6436048 B, Pesque [0009]
- US 6299579 B, Peterson [0013]
- US 6709994 B, Frisa [0016]

Non-patent literature cited in the description

- **BREKKER S. et al.** Tissue Doppler Gated (TDOG) Real-Time Stitching in Three-Dimensional Fetal Echocardiography. *IEEE ULTRASONICS SYMPOSIUM*, 2006, 764-767 [0005]

专利名称(译)	用于3D超声胎儿成像的自动心率检测		
公开(公告)号	EP2582302B1	公开(公告)日	2014-05-14
申请号	EP2011722913	申请日	2011-04-27
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	SCHAUF MICHAEL		
发明人	SCHAUF, MICHAEL		
IPC分类号	A61B8/02 A61B8/08		
CPC分类号	A61B8/02 A61B8/0866 A61B8/0883 A61B8/4405 A61B8/483 A61B8/5223 A61B8/543 G01S7/52073 G01S7/52074 G01S15/8993 G16H50/30 A61B8/14 A61B8/145 A61B8/4488 A61B8/466 A61B8/469		
优先权	61/355885 2010-06-17 US		
其他公开文献	EP2582302A1		
外部链接	Espacenet		

摘要(译)

超声系统和方法提供了获取由合成心脏门控信号门控的胎儿心脏的3D图像的工作流程。在超声图像中定义ROI，其描绘胎儿心脏。控制超声系统以根据从ROI接收的回波信号自动估计胎儿心率。当系统已经获得稳定的合成心率信号时，向用户给出其指示，然后用户命令系统获取用于使用合成心率信号门控的多个胎儿心脏周期的3D胎儿心脏图像。

