

(19)



(11)

EP 3 184 050 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
27.05.2020 Bulletin 2020/22

(51) Int Cl.:
A61B 8/00 (2006.01) **G01S 15/89** (2006.01)
G06T 7/30 (2017.01) **G06T 7/11** (2017.01)
G01S 7/52 (2006.01)

(21) Application number: **16184051.7**

(22) Date of filing: **12.08.2016**

(54) METHOD AND APPARATUS FOR DISPLAYING ULTRASOUND IMAGES

VERFAHREN UND VORRICHTUNG ZUR ANZEIGE VON ULTRASCHALBILDERN

PROCÉDÉ ET APPAREIL D’AFFICHAGE D’IMAGE ULTRASONORE

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **22.12.2015 KR 20150184080**

(43) Date of publication of application:
28.06.2017 Bulletin 2017/26

(73) Proprietor: **Samsung Medison Co., Ltd.
Hongcheon-gun, Gangwon-do, 25108 (KR)**

(72) Inventors:
• **Lee, Bong-heon
Gangwon-do 25108 (KR)**

• **Shin, Dong-kuk
Gangwon-do 25108 (KR)**

(74) Representative: **D’Halleweyn, Nele Veerle Trees
Gertrudis
Arnold & Siedsma
Bezuidenhoutseweg 57
2594 AC The Hague (NL)**

(56) References cited:
**US-A1- 2014 378 836 US-A1- 2015 011 872
US-A1- 2015 305 718**

EP 3 184 050 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present disclosure relates to methods and apparatuses for displaying ultrasound images.

[0002] Ultrasound diagnosis apparatuses transmit ultrasound signals generated by transducers of a probe to an object and receive echo signals reflected from the object, thereby obtaining at least one image of an object or an internal part of the object (e.g., soft tissues or blood flow). In particular, ultrasound diagnosis apparatuses are used for medical purposes including observation of the interior of an object, detection of foreign substances, and diagnosis of damage to the object. Such ultrasound diagnosis apparatuses provide high stability, display images in real time, and are safe due to the lack of radioactive exposure, compared to X-ray apparatuses. Therefore, ultrasound diagnosis apparatuses are widely used together with other image diagnosis apparatuses including a computed tomography (CT) apparatus, a magnetic resonance imaging (MRI) apparatus, and the like.

[0003] Methods for displaying a medical image are known from document US 2015/0305718 A1, US 2015/0011872 A1, and US 2014/0378836 A1.

[0004] Provided are methods and apparatuses for displaying ultrasound images.

[0005] Provided are non-transitory computer-readable recording media having recorded thereon programs for executing the methods of displaying ultrasound images on a computer.

[0006] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0007] According to an aspect of an embodiment, a method of displaying a medical image includes: generating a first image showing a region of interest (ROI) by using echo signals corresponding to ultrasound signals transmitted toward the ROI; selecting second images showing the ROI from among prestored images; and displaying the first image and the second images on a screen.

[0008] The displaying of the first image and the second images on the screen may include: displaying thumbnail images corresponding to the second images in a region of the screen; and displaying images that are most similar to the first image from among the second images in a region of the screen other than the region where the thumbnail images are displayed.

[0009] The displaying of the first image and the second images on the screen may include: displaying thumbnail images corresponding to the second images in a region of the screen; and displaying an image selected based on a user input from among the second images in a region of the screen other than the region where the thumbnail images are displayed.

[0010] The displaying of the first image and the second images on the screen may include displaying the second images in different regions into which the screen is par-

tioned, based on at least one time point when the second images are generated.

[0011] The at least one time point may include at least one time point selected based on a user input from among time points when the prestored images are generated.

[0012] The displaying of the first image and the second images on the screen may include aligning the second images based on time points when the second images are generated to thereby display the aligned second images.

[0013] The displaying of the first image and the second images on the screen may include displaying an image that is most similar to the first image from among the second images in such a manner that the most similar image is distinguished from the other ones among the second images.

[0014] The selecting of the second images may include selecting, from among the prestored images, images on which the same parameter as a parameter measured based on the first image is measured, as the second images.

[0015] The selecting of the second images may include selecting, from among the prestored images, images generated under the same conditions as those used to generate the first image.

[0016] According to an aspect of another embodiment, a non-transitory computer-readable recording medium has recorded thereon a program for executing the method on a computer.

[0017] According to an aspect of another embodiment, an apparatus for displaying a medical image includes: an image processor configured to generate a first image showing an ROI by using echo signals corresponding to ultrasound signals transmitted toward the ROI; a controller configured to select second images showing the ROI from among prestored images; and a display configured to display the first image and the second images on a screen in response to a control signal generated by the controller.

[0018] The controller may generate the control signal so that thumbnail images corresponding to the second images are displayed in a region of the screen while images that are most similar to the first image among the second images are displayed in a region of the screen other than the region where the thumbnail images are displayed.

[0019] The controller may generate the control signal so that thumbnail images corresponding to the second images are displayed in a region of the screen while an image selected based on a user input from among the second images is displayed in a region of the screen other than the region where the thumbnail images are displayed.

[0020] The controller may generate the control signal so that the second images are displayed in different regions into which the screen is partitioned, based on at least one time point when the second images are generated.

[0021] The at least one time point may include at least one time point selected based on a user input from among time points when the prestored images are generated.

[0022] The controller may generate the control signal so that the second images are aligned based on time points when the second images are generated and displayed.

[0023] The controller may generate the control signal so that an image that is most similar to the first image from among the second images is displayed in such a manner that the most similar image is distinguished from the other ones among the second images.

[0024] The controller may select, from among the prestored images, images on which the same parameter as a parameter measured based on the first image is measured, as the second images.

[0025] The controller may select, from among the prestored images, images generated under the same conditions as those used to generate the first image.

BRIEF DESCRIPTION OF THE DRAWINGS

[0026] These and/or other aspects will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings in which:

FIGS. 1A and 1B illustrate examples of ultrasound diagnosis systems according to embodiments;

FIG. 2 is a diagram of a configuration of an ultrasound diagnosis system according to an embodiment;

FIG. 3 is a diagram of a configuration of a wireless probe according to an embodiment;

FIGS. 4A and 4B illustrate examples in which a probe transmits ultrasound signals to an object, according to an embodiment;

FIG. 5 is a diagram of a configuration of a display apparatus for displaying a medical image according to an embodiment;

FIG. 6 is a flowchart of an example of a method of displaying a medical image according to an embodiment;

FIG. 7 illustrates an example in which a controller selects second images from among prestored images, according to an embodiment;

FIG. 8 illustrates another example in which a controller selects second images from among prestored images, according to an embodiment;

FIG. 9 illustrates another example in which a controller selects second images from among prestored images according to an embodiment;

FIG. 10 illustrates an example in which first and second images are displayed on a screen, according to an embodiment;

FIG. 11 illustrates another example in which first and second images are displayed on a screen, according to an embodiment;

FIG. 12 illustrates an example in which a controller

matches first thumbnail images to second thumbnail images according to an embodiment;

FIG. 13 illustrates another example in which first and second images are displayed on a screen, according to an embodiment;

FIG. 14 illustrates another example in which first and second images are displayed on a screen, according to an embodiment;

FIG. 15 illustrates another example in which first and second images are displayed on a screen, according to an embodiment;

FIG. 16 illustrates another example in which first and second images are displayed on a screen, according to an embodiment;

FIG. 17 illustrates another example in which first and second images are displayed on a screen, according to an embodiment; and

FIGS. 18A through 18D illustrate examples in which measured values of a parameter are output on a screen, according to an embodiment.

DETAILED DESCRIPTION

[0027] The terms used in this specification are those general terms currently widely used in the art in consideration of functions regarding the inventive concept, but the terms may vary according to the intention of those of ordinary skill in the art, precedents, or new technology in the art. Also, some terms may be arbitrarily selected by the applicant, and in this case, the meaning of the selected terms will be described in detail in the detailed description of the present specification. Thus, the terms used in the specification should be understood not as simple names but based on the meaning of the terms and the overall description of the invention. Expressions such as "at least one of," when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

[0028] Throughout the specification, it will also be understood that when a component "includes" an element, unless there is another opposite description thereto, it should be understood that the component does not exclude another element and may further include another element. In addition, terms such as "... unit", "... module", or the like refer to units that perform at least one function or operation, and the units may be implemented as hardware or software or as a combination of hardware and software.

[0029] Throughout the specification, an "ultrasound image" refers to an image of an object, which is obtained using ultrasound waves or an image showing a region of interest (ROI) included in the object. An ROI refers to a region of an object that a user desires to observe with more focused attention, and, for example, may be a region including a lesion. Furthermore, an "object" may be a human, an animal, or a part of a human or animal. For example, the object may be an organ (e.g., the liver, heart, womb, brain, breast, or abdomen), a blood vessel,

or a combination thereof. Also, the object may be a phantom. The phantom means a material having a density, an effective atomic number, and a volume that are approximately the same as those of an organism. For example, the phantom may be a spherical phantom having properties similar to a human body.

[0030] Throughout the specification, a "user" may be, but is not limited to, a medical expert, for example, a medical doctor, a nurse, a medical laboratory technologist, or a medical imaging expert, or a technician who repairs medical apparatuses.

[0031] Hereinafter, exemplary embodiments will be described in detail with reference to the accompanying drawings.

[0032] FIGS. 1A and 1B are diagrams showing examples of ultrasound diagnosis systems 1000 and 1001 according to embodiments.

[0033] FIGS. 1A and 1B are diagrams showing examples of ultrasound diagnosis systems 1000 and 1001 according to embodiments.

[0034] Referring to FIG. 1A, in the ultrasound diagnosis system 1000, a probe 20 may be connected by wire to an ultrasound imaging apparatus 100. In other words, the probe 20 for transmitting and receiving ultrasound waves may be connected to a main body of the ultrasound diagnosis system 1000, i.e., the ultrasound imaging apparatus 100 via a cable 110.

[0035] Referring to FIG. 1B, in the ultrasound diagnosis system 1001, a probe 20 may be connected wirelessly to an ultrasound imaging apparatus 210. In other words, the probe 20 may be connected to the ultrasound imaging apparatus 210 via the same wireless network. For example, the probe 20 and the ultrasound imaging apparatus 210 may be combined with a Millimeter Wave (mmWave) based wireless network, and the probe 20 may transmit echo signals received through transducers to the ultrasound imaging apparatus 210 in the 60 GHz frequency band. The ultrasound imaging apparatus 210 may generate ultrasound images via various imaging modalities by using echo signals received in the 60 GHz frequency band and display the generated ultrasound images. In this case, the mmWave based wireless network may use a wireless communication method compliant with the Wi-Gig standard developed by Wireless Gigabit Alliance (WGA), but is not limited thereto.

[0036] FIG. 2 is a block diagram of a configuration of an ultrasound diagnosis system 1002 according to an embodiment.

[0037] Referring to FIG. 2, the ultrasound diagnosis system 1002 may include a probe 20 and an ultrasound imaging apparatus 100. Here, the ultrasound imaging apparatus 100 may include an ultrasound transceiver 1100, an image processor 1200, a communication module 1300, a display 1400, a memory 1500, an input unit 1600, and a controller 1700, which may be connected to one another via buses 1800.

[0038] The ultrasound diagnosis system 1002 may be a cart type apparatus or a portable type apparatus. Ex-

amples of portable ultrasound diagnosis apparatuses may include, but are not limited to, a picture archiving and communication system (PACS) viewer, a smartphone, a laptop computer, a personal digital assistant (PDA), and a tablet PC.

[0039] The probe 20 transmits ultrasound signals to an object 10 (or to an ROI in the object 10) in response to a driving signal applied by the ultrasound transceiver 1100 and receives echo signals reflected by the object 10 (or by the ROI in the object 10). The probe 20 includes a plurality of transducers, and the plurality of transducers oscillate in response to electric signals and generate acoustic energy, that is, ultrasound waves. Furthermore, the probe 20 may be connected to the main body of the ultrasound diagnosis system 1002 by wire or wirelessly, and according to embodiments, the ultrasound diagnosis system 1002 may include a plurality of probes 20.

[0040] A transmitter 1110 supplies a driving signal to the probe 20. The transmitter 1110 includes a pulse generator 1112, a transmission delaying unit 1114, and a pulser 1116. The pulse generator 1112 generates pulses for forming transmission ultrasound waves based on a predetermined pulse repetition frequency (PRF), and the transmission delaying unit 1114 delays the pulses by delay times necessary for determining transmission directionality. The pulses which have been delayed correspond to a plurality of piezoelectric vibrators included in the probe 20, respectively. The pulser 1116 applies a driving signal (or a driving pulse) to the probe 20 based on timing corresponding to each of the pulses which have been delayed.

[0041] A receiver 1120 generates ultrasound data by processing echo signals received from the probe 20. The receiver 1120 may include an amplifier 1122, an analog-to-digital converter (ADC) 1124, a reception delaying unit 1126, and a summing unit 1128. The amplifier 1122 amplifies echo signals in each channel, and the ADC 1124 performs analog-to-digital conversion with respect to the amplified echo signals. The reception delaying unit 1126 delays digital echo signals output by the ADC 1124 by delay times necessary for determining reception directionality, and the summing unit 1128 generates ultrasound data by summing the echo signals processed by the reception delaying unit 1126. In some embodiments, the receiver 1120 may not include the amplifier 1122. In other words, if the sensitivity of the probe 20 or the capability of the ADC 1124 to process bits is enhanced, the amplifier 1122 may be omitted.

[0042] The image processor 1200 generates an ultrasound image by scan-converting ultrasound data generated by the ultrasound transceiver 1100. The ultrasound image may be not only a grayscale ultrasound image obtained by scanning an object in an amplitude (A) mode, a brightness (B) mode, and a motion (M) mode, but also a Doppler image showing a movement of an object via a Doppler effect. The Doppler image may be a blood flow Doppler image showing flow of blood (also referred to as a color Doppler image), a tissue Doppler image showing

a movement of tissue, or a spectral Doppler image showing a moving speed of an object as a waveform.

[0043] A B mode processor 1212 extracts B mode components from ultrasound data and processes the B mode components. An image generator 1220 may generate an ultrasound image indicating signal intensities as brightness based on the extracted B mode components 1212.

[0044] Similarly, a Doppler processor 1214 may extract Doppler components from ultrasound data, and the image generator 1220 may generate a Doppler image indicating a movement of an object as colors or waveforms based on the extracted Doppler components.

[0045] According to an embodiment, the image generator 1220 may generate a three-dimensional (3D) ultrasound image via volume-rendering with respect to volume data and may also generate an elasticity image by imaging deformation of the object 10 due to pressure. Furthermore, the image generator 1220 may display various pieces of additional information in an ultrasound image by using text and graphics. In addition, the generated ultrasound image may be stored in the memory 1500.

[0046] A display 1400 displays the generated ultrasound image. The display 1400 may display not only an ultrasound image, but also various pieces of information processed by the ultrasound imaging apparatus 1002 on a screen image via a graphical user interface (GUI). In addition, the ultrasound diagnosis apparatus 1000 may include two or more displays 1400 according to embodiments.

[0047] The communication module 1300 is connected to a network 30 by wire or wirelessly to communicate with an external device or a server. Furthermore, when the probe 20 is connected to the ultrasound imaging apparatus 1002 via a wireless network, the communication module 1300 may communicate with the probe 20.

[0048] The communication module 1300 may exchange data with a hospital server or another medical apparatus in a hospital, which is connected thereto via a PACS. Furthermore, the communication module 1300 may perform data communication according to the digital imaging and communications in medicine (DICOM) standard.

[0049] The communication module 1300 may transmit or receive data related to diagnosis of an object, e.g., an ultrasound image, ultrasound data, and Doppler data of the object, via the network 30 and may also transmit or receive medical images captured by another medical apparatus, e.g., a computed tomography (CT) apparatus, a magnetic resonance imaging (MRI) apparatus, or an X-ray apparatus. Furthermore, the communication module 1300 may receive information about a diagnosis history or medical treatment schedule of a patient from a server and utilizes the received information to diagnose the patient. Furthermore, the communication module 1300 may perform data communication not only with a server or a medical apparatus in a hospital, but also with a portable terminal of a medical doctor or patient.

[0050] The communication module 1300 is connected to the network 30 by wire or wirelessly to exchange data with a server 32, a medical apparatus 34, or a portable terminal 36. The communication module 1300 may include one or more components for communication with external devices. For example, the communication module 1300 may include a local area communication module 1310, a wired communication module 1320, and a mobile communication module 1330.

[0051] The local area communication module 1310 refers to a module for local area communication within a predetermined distance. Examples of local area communication techniques according to an embodiment may include, but are not limited to, wireless LAN, Wi-Fi, Bluetooth, ZigBee, Wi-Fi Direct (WFD), ultra wideband (UWB), infrared data association (IrDA), Bluetooth low energy (BLE), and near field communication (NFC).

[0052] The wired communication module 1320 refers to a module for communication using electric signals or optical signals. Examples of wired communication techniques according to an embodiment may include communication via a twisted pair cable, a coaxial cable, an optical fiber cable, and an Ethernet cable.

[0053] The mobile communication module 1330 transmits or receives wireless signals to or from at least one selected from a base station, an external terminal, and a server on a mobile communication network. The wireless signals may be voice call signals, video call signals, or various types of data for transmission and reception of text/multimedia messages.

[0054] The memory 1500 stores various data processed by the ultrasound diagnosis apparatus 1000. For example, the memory 1500 may store medical data related to diagnosis of an object 10, such as ultrasound data and an ultrasound image that are input or output, and may also store algorithms or programs which are to be executed in the ultrasound imaging apparatus 1002.

[0055] The memory 1500 may be any of various storage media, e.g., a flash memory, a hard disk drive, EEPROM, etc. Furthermore, the ultrasound imaging apparatus 1002 may utilize web storage or a cloud server that performs the storage function of the memory 1500 online.

[0056] The input unit 1600 refers to a unit via which a user inputs data for controlling the ultrasound imaging system 1002. The input unit 1600 may include hardware components, such as a keyboard, a mouse, a touch pad, a touch screen, a trackball, and a jog switch, and software modules for operating the hardware components. However, embodiments are not limited thereto, and the input device 1600 may further include any of various other input units including an electrocardiogram (ECG) measuring module, a respiration measuring module, a voice recognition sensor, a gesture recognition sensor, a fingerprint recognition sensor, an iris recognition sensor, a depth sensor, a distance sensor, etc.

[0057] The controller 1700 may control all operations of the ultrasound diagnosis apparatus 1000. In other words, the controller 1700 may control operations among

the probe 20, the ultrasound transceiver 1100, the image processor 1200, the communication module 1300, the display 1400, the memory 1500, and the input device 1600 shown in FIG. 1.

[0058] All or some of the probe 20, the ultrasound transceiver 1100, the image processor 1200, the communication module 1300, the display 1400, the memory 1500, the input device 1600, and the controller 1700 may be implemented as software modules. Furthermore, at least one selected from the ultrasound transceiver 1100, the image processor 1200, and the communication module 1300 may be included in the controller 1600. However, embodiments of the present invention are not limited thereto.

[0059] FIG. 3 is a diagram showing a wireless probe 2000 according to an embodiment.

[0060] Referring to FIG. 3, as described above with reference to FIG. 2, the wireless probe 2000 may include a plurality of transducers, and, according to embodiments, may include some or all of the components of the ultrasound transceiver 1100 shown in FIG. 2.

[0061] The wireless probe 2000 according to the embodiment shown in FIG. 2 includes a transmitter 2100, a transducer 2200, and a receiver 2300. Since descriptions thereof are given above with reference to FIG. 2, detailed descriptions thereof will be omitted here. In addition, according to embodiments, the wireless probe 2000 may selectively include a reception delaying unit 2330 and a summing unit 2340.

[0062] The wireless probe 2000 may transmit ultrasound signals to the object 10, receive echo signals from the object 10, generate ultrasound data, and wirelessly transmit the ultrasound data to the ultrasound imaging apparatus 1002 shown in FIG. 2.

[0063] FIGS. 4A and 4B illustrate examples in which a probe transmits ultrasound signals to an object, according to an embodiment.

[0064] Probes 410 and 430 respectively shown in FIGS. 4A and 4B may correspond to the probe 20 shown in FIG. 1A, or the probe 20 and the wireless probe 2000 respectively shown in FIGS. 1B and 3.

[0065] Referring to FIG. 4A, the probe 410 may be formed by a one-dimensional (1D) array of a plurality of transducers. In this case, the transducers are elements constituting the probe 410 and transmit ultrasound signals to an object 420 and receive echo signals reflected from the object 420. The plurality of transducers oscillate in response to reflected echo signals, generate electrical pulses corresponding to the oscillations, and output the electrical pulses to the ultrasound transceiver 1100.

[0066] Furthermore, transducers in the probe 410 may constitute an aperture or sub-array. In this case, the aperture is a set of some of the plurality of transducers in the probe 410. The number of transducers that constitute an aperture is not limited to a specific number, and one aperture may be composed of a single transducer.

[0067] Furthermore, referring to FIG. 4B, the probe 430 may be formed by a 2D array of a plurality of transducers.

The probe 430 may transmit ultrasound signals to a 3D object 440 and receive echo signals reflected from the object 440. In this case, the probe 430 may transmit ultrasound signals to the object 440 and receive echo signals in the same manner as described with reference to FIG. 4A.

[0068] FIG. 5 is a diagram of a configuration of a display apparatus 101 for displaying a medical image according to an embodiment.

[0069] Referring to FIG. 5, the display apparatus 101 includes an image processor 1201, a display 1401, and a memory 1501, and a controller 1701, all of which are connected to one another via a bus 1801. In this case, all or some of the image processor 1201, the display 1401, the memory 1501, and the controller 1701 may be implemented using software modules, but are not limited thereto. Some of the components may also be implemented as hardware modules. Furthermore, each of the image processor 1201, the display 1401, and the input unit 1601 may include an independent control module.

[0070] The display apparatus 101 displays a first image generated by the image processor 1201 and at least one second image read from the memory 1501 on a screen. For example, the display 1401 may display second images showing the same ROI (e.g., the same application, etc.) as an ROI shown in the first image, together with the first image. Furthermore, the display 1401 may display, together with the first image, second images on which a same parameter (e.g., a size, a volume, a length, etc.) as a parameter measured by a user based on the first image is measured. Furthermore, the display 1401 may display, together with the first image, second images generated under the same conditions as those used to generate the first image (e.g., probe type, time gain compensation (TGC)/lateral gain compensation (LGC) values, depth, etc.).

[0071] Thus, the user may determine how an ROI changes over time based on images displayed by the display apparatus 101. Furthermore, the display apparatus 101 may automatically select an image similar to a currently captured image from among prestored images and display the automatically selected image, thus reducing the amount of time that it takes for a user to diagnose an object based on the image.

[0072] Examples in which the display apparatus 1001 displays a first image and second images on a single screen will be described in more detail below with reference to FIGS. 6 through 18.

[0073] FIG. 6 is a flowchart of an example of a method of displaying a medical image according to an embodiment.

[0074] Referring to FIG. 6, the method of displaying a medical image includes operations sequentially performed by the ultrasound diagnosis systems 1000, 1001, and 1002 of FIGS. 1A, 1B, and 2 or the display apparatus 101 of FIG. 5. Thus, although omitted hereinafter, the descriptions with respect to the ultrasound diagnosis systems 1000, 1001, and 1002 of FIGS. 1A, 1B, and 2 or

the display apparatus 101 of FIG. 5 apply to the method of FIG. 6.

[0075] The image processor 1201 generates at least one first image showing an ROI by using echo signals corresponding to ultrasound signals transmitted toward the ROI (operation 610). In this case, the ROI refers to a target inside an object that a user desires to observe, and, for example, may include a lesion or an internal tissue of the object. The image processor 1201 generates at least one first image in the same manner as described above with reference to FIG. 2.

[0076] The controller 1701 selects second images showing an ROI from among images prestored in the memory 1501 (operation 620). In this case, the second images mean images that are read by the controller 1701 from the memory 1501 from among images stored in the memory 1501. A plurality of medical images generated by the image processor 1201 may be stored in the memory 1501. In other words, captured medical images of various objects may be stored in the memory 1501. The controller 1701 may read captured medical images of an object that is a target contained in the first image from among the medical images stored in the memory 1501. For example, the controller 1701 may select and read captured images of the same ROI as an ROI shown in the first image from among captured images of the object stored in the memory 1501. As another example, the controller 1701 may select and read, from among captured images of the object stored in the memory 1501, images on which the same parameter as a parameter measured by the user based on the first image is measured. As another example, the controller 1701 may select and read, from among captured images of the object stored in the memory 1501, images generated under the same conditions as those used to generate the first image.

[0077] Examples in which the controller 1701 selects second images from among images stored in the memory 1501 will now be described with reference to FIGS. 7 through 9.

[0078] FIG. 7 illustrates an example in which the controller 1701 selects second images from among prestored images, according to an embodiment.

[0079] In detail, FIG. 7 shows an example of first images 710 generated by the image processor 1201 and images stored in the memory 1501. It is assumed herein that the first images 710 have been captured at a time point T_n and the images stored in the memory 1501 have been captured at time points T_{n-1} , T_{n-2} , and T_{n-3} that are earlier than the time point T_n .

[0080] The image processor 1201 may generate at least one first image at current time point T_n . In other words, the user may capture one or more first images showing an ROI 711 by using the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 101.

[0081] The controller 1701 may identify the ROI 711 shown in the first images 710 and select and read captured images 720 and 720 of the same region as the ROI

711 from among images stored in the memory 1501. In this case, the images 720 and 730 may be captured respectively at different earlier time points T_{n-1} and T_{n-3} . In other words, to observe a change in the ROI 711, the user may continue capturing images showing the ROI 711 from a specific time point in the past. For example, the user may use the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 101 to capture the images 730 at the earlier time point T_{n-3} , the images 720 at the earlier time point T_{n-1} , and the images 710 at the current time point T_n . Furthermore, the user may capture images of a region other than the ROI 711 at the earlier time point T_{n-2} .

[0082] Images captured at the earlier time points T_{n-1} , T_{n-2} , and T_{n-3} are stored in the memory 1501, and the controller 1701 may select and read images showing the ROI 711 from among the images stored in the memory 1501. For example, the controller 1701 may extract a shape of the ROI 711 from the first images 710 and select and read the images 720 and 730 respectively including a shape corresponding to the extracted shape.

[0083] FIG. 8 illustrates another example in which the controller 1701 selects second images from among prestored images, according to an embodiment.

[0084] In detail, FIG. 8 shows an example of first images 810 generated by the image processor 1201 and images stored in the memory 1501. It is assumed herein that the first images 810 have been captured at a time point T_n and the images stored in the memory 1501 have been captured at time points T_{n-1} , T_{n-2} , and T_{n-3} that are earlier than the time point T_n . As described above with reference to FIG. 7, the images captured at the earlier time points T_{n-1} , T_{n-2} , and T_{n-3} may be stored in the memory 1501.

[0085] The controller 1701 may select and read images 820 on which the same parameter as a parameter measured based on at least one of the first images 810 from among the images stored in the memory 1501. In this case, a parameter means a numerical value that can be measured by the user based on an image. For example, a parameter may be a size, a volume, and a length of an object (e. g., a lesion, tissue, etc.) shown in an image.

[0086] For example, if the user measures a diameter of an ROI 811 based on one of the first images 810, the controller 1701 may select and read the images 820 on which a diameter of the ROI 811 has been measured and recorded from among the images stored in the memory 1501.

[0087] FIG. 9 illustrates another example in which the controller 1701 selects second images from among prestored images according to an embodiment.

[0088] FIG. 9 shows an example of first images 910 generated by the image processor 1201 and images stored in the memory 1501. It is assumed herein that the first images 910 have been captured at a time point T_n and the images stored in the memory 1501 have been captured at time points T_{n-1} , T_{n-2} , and T_{n-3} that are earlier than the time point T_n . As described above with reference

to FIG. 7, the images captured at the earlier time points T_{n-1} , T_{n-2} , and T_{n-3} may be stored in the memory 1501.

[0089] The controller 1701 may select and read images 920 generated under the same conditions as those used to generate the first images 910 from among the images stored in the memory 1501. In this case, the conditions may be a type of the probe 20 and setting values stored in the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 101. For example, the conditions may be a type of the probe 20 (a linear probe or convex probe), a TGC or LGC value of an image, a depth of the image, etc., which are used to generate the image.

[0090] For example, if the first images 910 are generated based on signals transmitted or received via a linear probe, the controller 1701 may select and read, from among the images stored in the memory 1501, the images 920 generated based on signals transmitted or received via a linear probe.

[0091] While it has been described with reference to FIGS. 7 through 9 that the controller 1701 automatically reads the second images 720, 730, 820, and 920 from the memory 1501 based on the first images 710, 810, and 910, respectively, embodiments are not limited thereto. In other words, the controller 1701 may read second images from the memory 1501 based on a user input for instructing reading of images captured at a specific time point in the past (e.g., time point T_{n-2}).

[0092] Referring back to FIG. 6, the display 1401 displays the first image and the second images on a screen (operation 630). In detail, the display 1401 may display the first image and the second images on a single screen in response to a control signal received from the controller 1701.

[0093] For example, the display 1401 may display thumbnail images corresponding to the second images in a region of the screen while displaying images that are most similar to the first image among the second images in a region of the screen other than the region where the thumbnail images are displayed. As another example, the display 1401 may display thumbnail images corresponding to the second images in a region of the screen while displaying an image selected based on a user input from among the second images in a region of the screen other than the region where the thumbnail images are displayed.

[0094] As another example, the display 1401 may display the second images in different regions of the screen based on time points when the second images are generated. As another example, the display 1401 may align the second images based on time points when they are generated to thereby display the aligned second images. As another example, the display 1401 may display an image that is most similar to the first image among the second images in such a manner that the most similar image is distinguished from the other ones among the second images.

[0095] Examples in which the display 1401 displays a first image and second images on a screen will be de-

scribed below with reference to FIGS. 10 through 17.

[0096] FIG. 10 illustrates an example in which first and second images are displayed on a screen 3100, according to an embodiment

[0097] FIG. 10 shows an example of the screen 3100 on which first and second images are displayed. Thumbnail images 3110 corresponding to the first images (hereinafter, referred to as 'first thumbnail images') may be displayed in a region of the screen 3100. Furthermore, thumbnail images 3130 corresponding to the second images (hereinafter, referred to as 'second thumbnail images') may be displayed in another region of the screen 3100. In this case, examples in which the controller 1701 reads the second images among images stored in the memory 1501 are as described above with reference to FIGS. 7 through 9.

[0098] A thumbnail image is a smaller version of a graphic file corresponding to an original image. Thus, thumbnail images (e.g., the first thumbnail images) hereinafter mean the same images as original images (e.g., the first images).

[0099] The controller 1701 may generate a control signal so that an image 3140 that is most similar to an image selected by the user among the second thumbnail images 3130 may be displayed in a region other than the region where the second thumbnail images 3130 are displayed.

[0100] In detail, the user may select one image from among the first thumbnail images 3110. For example, the user may select one of the first thumbnail images 3110 via the input unit 1600. If the screen 3100 is a touch screen, the user may select one image from among the first thumbnail images 3110 by performing a gesture over the screen 3100. The image selected by the user from among the first thumbnail images 3110 may be displayed as its enlarged version 3120 in a region of the screen 3100.

[0101] When the image 3120 is selected by the user, the controller 1701 may select an image that is most similar to the image 3120 from among the second thumbnail images 3130. The image selected by the controller 1701 may be displayed as its enlarged version 3140 in a region of the screen 3100.

[0102] FIG. 11 illustrates another example in which first and second images are displayed on a screen 3200, according to an embodiment.

[0103] FIG. 11 shows an example of the screen 3200 where the first and second images are displayed. In detail, first thumbnail images 3210 are displayed in a region of the screen 3200 while second thumbnail images 3230 are displayed in another region thereof. Furthermore, information 3250 about a time point when the first images are generated and information 3260 about a time point when the second images are generated may be output on the screen 3200.

[0104] In addition, results of matching the first thumbnail images 3210 to the second thumbnail images 3230 may be output on the screen 3200. In other words, infor-

mation about which of the second thumbnail images 3230 is most similar to each of the first thumbnail images 3210 may be output onto the screen 3200.

[0105] The first thumbnail images 3210 (or the first images) of the same ROI may all be captured, but ROIs respectively shown in the first thumbnail images 3210 may have different shapes. For example, shapes of the ROIs respectively shown in the first thumbnail images 3210 may vary depending on a position of the probe 20 over an object or motion of the object.

[0106] The controller 1701 may compare the first thumbnail images 3210 with the second thumbnail images 3210 (or the second images), respectively, and match each of the first thumbnail images to its most similar one among the second thumbnail images 3210 based on a result of the comparison. The controller 1701 may then output matching results on the screen 3200. FIG. 11 shows an example in which the results of matching the first thumbnail images 3210 to the second thumbnail images 3230 are indicated by the same numbers.

[0107] An example in which the controller 1701 respectively matches the first thumbnail images 3210 to the second thumbnail images 3230 will now be described in detail with reference to FIG. 12.

[0108] FIG. 12 illustrates an example in which the controller 1701 matches first thumbnail images 3310 to second thumbnail images 3320 according to an embodiment.

[0109] Referring to FIG. 12, the controller 1701 selects one image 3311 from among the first thumbnail images 3310. The controller 1701 also compares the image 3311 with each of the second thumbnail images 3320.

[0110] In detail, the controller 1701 may adjust a scale of the image 3311 or the second thumbnail images 3320 so that the image 3311 and the second thumbnail images 3320 have the same scale (operation 3331). For example, the controller 1701 may adjust a scale of the image 3311 or the second thumbnail images 3320 by enlarging or reducing the image 3311 or the second thumbnail images 3320 or using a depth of the image 3311 or the second thumbnail images 3320.

[0111] The controller 1701 extracts feature points from the image 3311 and the second thumbnail images 3320 according to a feature-based algorithm (operation 3332). The controller 1701 then uses the extracted feature points to calculate a similarity between the image 3311 and each of the second thumbnail images 3320 (operation 3333). In operations 3332 and 3333, the controller 1701 may extract feature points from the image 3311 and the second thumbnail images 3320 and calculate a similarity therebetween by using various algorithms. For example, the controller 1701 may perform operations 3332 and 3333 by using an algorithm such as Histogram of Oriented Gradient (HOG), Scale Invariant Feature Transform (SIFT), Haar-like features, Ferns, Local Binary Pattern (LBP), or Modified Census Transform (MCT).

[0112] The controller 1701 selects an image 3321 that is most similar to the image 3311 from among the second

thumbnail images 3320 (operation 3334). Then, the display 1401 outputs information indicating that the selected image 3321 is most similar to the image 3311 on a screen. For example, the display 1401 may output the same marker (e.g., the same number) on the images 3311 and 3321 in order to indicate that the images 3311 and 3321 are most similar ones.

[0113] The controller 1701 may perform operations 3331 through 3334 on each of the other ones among the first thumbnail images 3310 in order to respectively match the first thumbnail images 3310 to the second thumbnail images 3320.

[0114] As described above with reference to FIGS. 10 through 12, second images (or second thumbnail images) include images generated at a time point in the past. However, the second images may include images generated at each of a plurality of time points in the past. Examples in which second images generated at a plurality of earlier time points are displayed on a screen will now be described with reference to FIGS. 13 and 14.

[0115] FIG. 13 illustrates another example in which first and second images are displayed on a screen 3400, according to an embodiment

[0116] FIG. 13 shows an example in which a plurality of thumbnail images 3410, 3420, 3430, and 3440 are displayed on the screen 3400. For example, first thumbnail images 3410 may be generated at a current time point, and second thumbnail images 3420, 3430, and 3440 may respectively be generated at a plurality of earlier time points.

[0117] As described above with reference to FIGS. 7 through 9, the controller 1701 may read images (e.g., the second thumbnail images 3420, 3430, and 3440) related to the first thumbnail images 3410 among a plurality of images stored in the memory 1501. In this case, when the related images are generated at different time points, the display 1401 may display the related images respectively in different regions of the screen 3400 based on the time points when they are generated.

[0118] Furthermore, as described with reference to FIGS. 7 through 9, the controller 1701 may select images selected based on a user input from among images stored in the memory 1501. In this case, referring to FIG. 13, the display 1401 may display images (e.g., the second thumbnail images 3420, 3430, and 3440) generated at time points selected by the user.

[0119] In addition, as described above with reference to FIGS. 11 and 12, the controller 1701 may compare the first thumbnail images 3410 with the second thumbnail images 3420, 3430, and 3440, respectively, and match each of the first thumbnail images 410 to its most similar ones among the second thumbnail images 3420, 3430, and 3440 based on results of the comparison. The controller 1701 may then output matching results on the screen 3400. However, if the second thumbnail images 3420, 3430, or 3440 include an image that is not similar to any one of the first thumbnail images 3410, a matching result may not be output on the screen 3400.

[0120] For example, if an image similar to image ㉓ among the first thumbnail images 3410 is not included in the second thumbnail images 3430 and 3440 respectively captured on August 31, 2012 and August 31, 2014, a matching result may not be output on the screen 3400. For example, as described above with reference to FIG. 12, if the second thumbnail images 3430 and 3440 do not include any image whose similarity with image ㉓ among the first thumbnail images 3410 is greater than a predetermined value, a matching result may not be output on the screen 3400.

[0121] FIG. 14 illustrates another example in which first and second images are displayed on a screen 3500, according to an embodiment.

[0122] FIG. 14 shows an example in which a plurality of thumbnail images 3510 are displayed on the screen 3500. For example, the plurality of thumbnail images 3510 may include first and second thumbnail images, and may be aligned based on time points when the plurality of thumbnails 3510 are generated and displayed in a region of the screen 3500.

[0123] For example, if the first thumbnail images are captured on August 31, 2015 and the second thumbnail images are captured on August 31, 2014, the plurality of thumbnails 3510 may be displayed on the screen 3500 in an order from the first thumbnail images to the second thumbnail images or from the second thumbnail images to the first thumbnail images.

[0124] Although not shown in FIG. 14, the second thumbnail images may include images captured at a plurality of time points. In this case, thumbnail images may be aligned according to an order of time points when the first thumbnail images are captured and when the second thumbnail images are captured and displayed on the screen 3500.

[0125] As described with reference to FIGS. 11 through 14, results of matching first images (or first thumbnail images) to second images (or second thumbnail images) may be output on a screen. In addition, when the user selects one image from among the images (e.g., the first and second images), output on the screen, the display 1401 may display an image that is most similar to the selected image in such a manner that the most similar image is distinguished from the other ones. Examples in which the display 1401 displays an image that is most similar to an image selected by the user in such a manner that the most similar image is distinguished from the other ones will now be described in detail with reference to FIGS. 15 through 17.

[0126] FIG. 15 illustrates another example in which first and second images are displayed on a screen 3600, according to an embodiment;

[0127] FIG. 15 shows an example of the screen 3600 on which a plurality of thumbnail images 3610, 3620, 3630, and 3640 are displayed. It is assumed herein that thumbnail images 3610 among the plurality of thumbnail images 3610, 3620, 3630, and 3640 are first thumbnail images.

[0128] The user may select one thumbnail image 3621 from among the plurality of thumbnail images 3610, 3620, 3630, and 3640. In this case, the thumbnail image 3621 selected by the user may be a first or second thumbnail image. For example, the user may select the thumbnail image 3621 from among the plurality of thumbnail images 3610, 3620, 3630, and 3640 via the input unit 1600. If the screen 3600 is a touch screen, the user may select the thumbnail image 3621 from among the plurality of thumbnail images 3610, 3620, 3630, and 3640 by performing a gesture over the screen 3600. The thumbnail image 3621 selected by the user may be displayed as its enlarged version 3662 in a region of the screen 3600.

[0129] When the user selects the thumbnail image 3621, the controller 1701 selects images 3611, 3631, and 3641 that are most similar to the thumbnail image 3621 respectively from among the thumbnail images 3610, 3630, and 3640. Then, the display 1401 displays the selected images 3611, 3631, and 3641 on the screen 3600 so that they are distinguished from the other images. Furthermore, the display 1401 may display the selected images 3611, 3631, and 3641 respectively as their enlarged versions 3661, 3663, and 3664 in a region of the screen 3600.

[0130] If there is a history of measurement of a parameter based on the thumbnail image 3621 selected by the user, the display 1401 may output information 3650 about the type of the measured parameter on a region of the screen 3600.

[0131] FIG. 16 illustrates another example in which first and second images are displayed on a screen 3700, according to an embodiment;

[0132] FIG. 16 shows an example of the screen 3700 on which a plurality of thumbnail images 3710, 3720, 3730, and 3740 are displayed. It is assumed herein that thumbnail images 3710 among the plurality of thumbnail images 3710, 3720, 3730, and 3740 are first thumbnail images.

[0133] The user may select one thumbnail image 3721 from among the plurality of thumbnail images 3710, 3720, 3730, and 3740. In this case, the thumbnail image 3721 selected by the user may be a first or second thumbnail image.

[0134] When the user selects the thumbnail image 3721, the controller 1701 selects images 3711, 3731, and 3741, on which the same parameter as a parameter measured based on the thumbnail image 3721 is measured, from among the thumbnail images 3710, 3730, and 3740. Then, the display 1401 displays the selected images 3711, 3731, and 3741 on the screen 3700 so that they are distinguished from the other images. Furthermore, the display 1401 may display the selected images 3711, 3731, and 3741 respectively as their enlarged versions 3761, 3763, and 3764 in a region of the screen 3700. Furthermore, the display 1401 may output information 3750 about the type of a measured parameter on a region of the screen 3700.

[0135] Although not shown in FIG. 16, when the user

selects the thumbnail image 3721, the controller 1701 may select the images 3711, 3731, and 3741 that are generated under the same conditions as those used to generate the thumbnail image 3721 respectively from among the thumbnail images 3710, 3730, and 3740. Then, the display 1401 may display the selected images 3711, 3731, and 3741 on the screen 3700 so that they are distinguished from the other images.

[0136] FIG. 17 illustrates another example in which first and second images are displayed on a screen 3800, according to an embodiment.

[0137] FIG. 17 shows an example of the screen 3800 on which a plurality of thumbnail images 3810, 3820, 3830, and 3840 are displayed. It is assumed herein that thumbnail images 3810 among the plurality of thumbnail images 3810, 3820, 3830, and 3840 are first thumbnail images.

[0138] In addition, an object 3850 representing an ROI as well as the thumbnail images 3810, 3820, 3830, and 3840 are displayed on the screen 3800. In this case, the object 3850 may be a body marker representing the ROI.

[0139] When the user selects a portion 3851 of the object 3850, the controller 1701 selects images 3811, 3821, 3831, and 3841 showing the selected portion 3851 from among the thumbnail images 3810, 3820, 3830, and 3840. The display 1401 displays the selected images 3811, 3821, 3831, and 3841 on the screen 3800 so that they are distinguished from the other images. Furthermore, the display 1401 may display the selected images 3811, 3821, 3831, and 3841 respectively as enlarged versions 3851, 3852, 3853, and 3854 in a region of the screen 3800.

[0140] As described above with reference to FIGS. 6 through 17, the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 1001 may display second images that are most similar to a first image on a screen. Furthermore, the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 101 may display on the screen second images used to measure the same parameter as a parameter measured based on the first image. Furthermore, the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 101 may display on the screen the second images generated under the same conditions as those used to generate the first image

[0141] In addition, the ultrasound diagnosis systems 1000, 1001, and 1002 may output on a screen parameter values measured based on images (i.e., first and second images). In other words, if there is a history of measurement of a specific parameter on the same ROI from a time point in the past, the ultrasound diagnosis systems 1000, 1001, and 1002 or the display apparatus 101 may output measured values of the parameter on the screen. Examples in which measured values of a parameter are output onto a screen will now be described with reference to FIGS. 18A through 18D.

[0142] FIGS. 18A through 18D illustrate examples in which measured values of a parameter are output on a

screen, according to an embodiment.

[0143] FIGS. 18A through 18D show examples in which values of a parameter are aligned based on an order of time points of measurement and output on a screen. Referring to FIGS. 18A and 18B, a graph showing a time point when a parameter is measured on an x-axis and a value of the parameter on a y-axis may be output on the screen. Furthermore, referring to FIG. 18C, images on which the parameter is measured may be aligned in order of time and output onto the screen. Furthermore, referring to FIG. 18D, measured values of the parameter may be output on the screen in a table form.

[0144] A mode in which measured values of a parameter are output is not limited to the examples shown in FIGS. 18A through 18D and may be changed in various ways depending on user settings.

[0145] As described above, the user may identify how an ROI changes over time based on images displayed by the display apparatus 101. Furthermore, the display apparatus 101 may automatically select an image similar to a currently captured image from among prestored images and display the automatically selected image, so the amount of time that it takes for the user to diagnose an object based on the image may be shortened.

[0146] The above methods according to the embodiments can be recorded in programs that can be executed on a computer and be implemented through general purpose digital computers which can run the programs using a non-transitory computer-readable recording medium. Data structures described in the above methods can also be recorded on a non-transitory computer-readable medium in a variety of ways, with examples of the medium including recording media, such as magnetic storage media (e.g., ROM, RAM, USB, floppy disks, hard disks, etc.) and optical recording media (e.g., CD-ROMs or DVDs).

[0147] While one or more embodiments have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope of the inventive concept as defined by the following claims. Thus, it should be understood that the embodiments described therein should be considered in a descriptive sense only and not for purposes of limitation. The scope of the present inventive concept is defined not by the detailed description thereof but by the appended claims, and all differences within the scope of the appended claims and their equivalents will be construed as being included in the present inventive concept.

Claims

1. A method of displaying a medical image, the method comprising:

generating, by an image processor, first images showing a region of interest (ROI) by using echo

signals corresponding to ultrasound signals transmitted toward the ROI;
 selecting, by a controller, second images showing the ROI from among prestored images, the second images being generated at a time point in the past; and
 displaying, by a display, the first images and the second images on a screen;
 wherein the displaying the first images and the second images on the screen comprises:

displaying first thumbnail images corresponding to the first images in a region of the screen and second thumbnail images corresponding to the second images in another region of the screen;
 receiving a user selection of a thumbnail image among the first thumbnail images, and selecting, by the controller, an image that is most similar to the selected first thumbnail image from among the second thumbnail images; or receiving a user selection of a thumbnail image among the second thumbnail images, and selecting, by the controller, an image that is most similar to the selected second thumbnail image from among the first thumbnail images; and
 displaying the selected first and second thumbnail images as their enlarged version in regions of the screen other than the regions where the first and second thumbnail images are displayed.

2. The method of claim 1, wherein the displaying of the first thumbnail images and the second thumbnail images in the regions of the screen comprises displaying the second thumbnail images in different regions into which the screen is partitioned, based on at least one time point when the second thumbnail images are generated.

3. The method of claim 1, wherein the displaying of the first thumbnail images and the second thumbnail images in the regions of the screen comprises aligning the second thumbnail images based on time points when the second thumbnail images are generated to thereby display the aligned second thumbnail images.

4. A non-transitory computer-readable recording medium having recorded thereon a program for executing the method of claim 1.

5. An apparatus for displaying a medical image, the apparatus comprising:

an image processor (1200, 1201) configured to generate first images showing a region of inter-

est (ROI) by using echo signals corresponding to ultrasound signals transmitted toward the ROI;

a controller (1700, 1701) configured to select second images showing the ROI from among prestored images, the second images being generated at a time point in the past; and
 a display (1400, 1401) configured to display the first images and the second images on a screen in response to a control signal generated by the controller;

wherein the display (1400, 1401) is further configured to display first thumbnail images corresponding to the first images in a region of the screen, and display second thumbnail images corresponding to the second images in another region of the screen;

wherein the controller (1700, 1701) is further configured to receive a user selection of a thumbnail image among the first thumbnail images, and select an image that is most similar to the selected first thumbnail image from among the second thumbnail images; or to receive a user selection of a thumbnail image among the second thumbnail images, and select an image that is most similar to the selected second thumbnail image from among the first thumbnail images; and

wherein the display (1400, 1401) is further configured to display the selected first and second thumbnail images as their enlarged version in regions of the screen other than the regions where the first and second thumbnail images are displayed.

6. The apparatus of claim 5, wherein the controller is further configured to generate the control signal so that the second thumbnail images are displayed in different regions into which the screen is partitioned, based on at least one time point when the second thumbnail images are generated.

7. The apparatus of claim 5, wherein the controller is further configured to generate the control signal so that the second thumbnail images are aligned based on time points when the second thumbnail images are generated and displayed.

Patentansprüche

1. Verfahren zum Anzeigen eines medizinischen Bildes, wobei das Verfahren Folgendes umfasst:

mittels eines Bildprozessors Erzeugen von ersten Bildern, die eine Region von Interesse (ROI, Region Of Interest) zeigen, durch Echosignale, die Ultraschallsignalen entsprechen, welche in

Richtung der ROI gesendet wurden;
mittels einer Steuerung Auswählen zweiter Bilder, die die ROI zeigen, unter vorgeschicherten Bildern, wobei die zweiten Bilder zu einem Zeitpunkt in der Vergangenheit erzeugt wurden; und
mittels einer Anzeige Anzeigen der ersten Bilder und der zweiten Bilder auf einem Bildschirm;
wobei das Anzeigen der ersten Bilder und der zweiten Bilder auf dem Bildschirm Folgendes umfasst:

Anzeigen erster Miniaturansichtsbilder, die den ersten Bildern entsprechen, in einem Bereich des Bildschirms, und zweiter Miniaturansichtsbilder, die den zweiten Bildern entsprechen, in einem anderen Bereich des Bildschirms;

Empfangen einer Benutzerauswahl eines Miniaturansichtsbildes unter den ersten Miniaturansichtsbildern, und mittels der Steuerung Auswählen eines Bildes unter den zweiten Miniaturansichtsbildern, das dem ausgewählten ersten Miniaturansichtsbild am ähnlichsten ist;

oder Empfangen einer Benutzerauswahl eines Miniaturansichtsbildes unter den zweiten Miniaturansichtsbildern, und mittels der Steuerung Auswählen eines Bildes unter den ersten Miniaturansichtsbildern, das dem ausgewählten zweiten Miniaturansichtsbild am ähnlichsten ist; und

Anzeigen des ausgewählten ersten und zweiten Miniaturansichtsbildes als vergrößerte Version in anderen Bereichen des Bildschirms als den Bereichen, in denen das erste und das zweite Miniaturansichtsbild angezeigt werden.

2. Verfahren nach Anspruch 1, wobei das Anzeigen der ersten Miniaturansichtsbilder und der zweiten Miniaturansichtsbilder in den Bereichen des Bildschirms Folgendes umfasst: Anzeigen der zweiten Miniaturansichtsbilder in verschiedenen Bereichen, in die der Bildschirm unterteilt ist, basierend auf wenigstens einem Zeitpunkt, an dem die zweiten Miniaturansichtsbilder erzeugt wurden.

3. Verfahren nach Anspruch 1, wobei das Anzeigen der ersten Miniaturansichtsbilder und der zweiten Miniaturansichtsbilder in den Bereichen des Bildschirms Folgendes umfasst: Ausrichten der zweiten Miniaturansichtsbilder basierend auf den Zeitpunkten, zu denen die zweiten Miniaturansichtsbilder erzeugt wurden, um so die ausgerichteten zweiten Miniaturansichtsbilder anzuzeigen.

4. Nicht-flüchtiges computerlesbares Aufzeichnungsmedium, auf dem ein Programm zur Ausführung des

Verfahrens nach Anspruch 1 aufgezeichnet ist.

5. Vorrichtung zum Anzeigen eines medizinischen Bildes, wobei die Vorrichtung Folgendes umfasst:

einen Bildprozessor (1200, 1201), der konfiguriert ist zum Erzeugen von ersten Bildern, die eine Region von Interesse (ROI, Region Of Interest) zeigen, durch Echosignale, die Ultraschallsignalen entsprechen, welche in Richtung der ROI gesendet wurden;

eine Steuerung (1700, 1701), die konfiguriert ist zum Auswählen zweiter Bilder, die die ROI zeigen, unter vorgeschicherten Bildern, wobei die zweiten Bilder zu einem Zeitpunkt in der Vergangenheit erzeugt wurden; und

eine Anzeige (1400, 1401), die konfiguriert ist zum Anzeigen der ersten Bilder und der zweiten Bilder auf einem Bildschirm als Reaktion auf ein durch die Steuerung erzeugtes Steuersignal; wobei die Anzeige (1400, 1401) weiterhin konfiguriert ist zum Anzeigen erster Miniaturansichtsbilder, die den ersten Bildern entsprechen, in einem Bereich des Bildschirms, und zum Anzeigen zweiter Miniaturansichtsbilder, die den zweiten Bildern entsprechen, in einem anderen Bereich des Bildschirms;

wobei die Steuerung (1700, 1701) weiterhin konfiguriert ist zum Empfangen einer Benutzerauswahl eines Miniaturansichtsbildes unter den ersten Miniaturansichtsbildern, und zum Auswählen eines Bildes unter den zweiten Miniaturansichtsbildern, das dem ausgewählten ersten Miniaturansichtsbild am ähnlichsten ist; oder zum Empfangen einer Benutzerauswahl eines Miniaturansichtsbildes unter den zweiten Miniaturansichtsbildern, und zum Auswählen eines Bildes unter den ersten Miniaturansichtsbildern, das dem ausgewählten zweiten Miniaturansichtsbild am ähnlichsten ist; und

wobei die Anzeige (1400, 1401) weiterhin konfiguriert ist zum Anzeigen des ausgewählten ersten und zweiten Miniaturansichtsbildes als vergrößerte Version in anderen Bereichen des Bildschirms als den Bereichen, in denen das erste und das zweite Miniaturansichtsbild angezeigt werden.

6. Vorrichtung nach Anspruch 5, wobei die Steuerung weiterhin konfiguriert ist zum Erzeugen des Steuersignals, so dass die zweiten Miniaturansichtsbilder in verschiedenen Bereichen angezeigt werden, in die der Bildschirm unterteilt ist, basierend auf wenigstens einem Zeitpunkt, an dem die zweiten Miniaturansichtsbilder erzeugt wurden.

7. Vorrichtung nach Anspruch 5, wobei die Steuerung weiterhin konfiguriert ist zum Erzeugen des Steuer-

signals, so dass die zweiten Miniaturansichtsbilder ausgerichtet werden basierend auf Zeitpunkten, an denen die zweiten Miniaturansichtsbilder erzeugt wurden, und so angezeigt werden.

Revendications

1. Procédé d'affichage d'une image médicale, le procédé comprenant :

la production, par un processeur d'image, de premières images montrant une région d'intérêt (ROI) au moyen de signaux d'écho correspondant à des signaux ultrasonores émis vers la ROI,

la sélection, par un organe de commande, de deuxièmes images montrant la ROI parmi des images préenregistrées, lesdites deuxièmes images ayant été produites à un instant passé, et l'affichage, par un dispositif d'affichage, des premières images et des deuxièmes images sur un écran ;

ledit affichage des premières images et des deuxièmes images sur l'écran comprenant :

l'affichage de premières images miniatures correspondant aux premières images dans une zone de l'écran et de deuxièmes images miniatures correspondant aux deuxièmes images dans une autre zone de l'écran, la réception d'une sélection, effectuée par l'utilisateur, d'une image miniature parmi les premières images miniatures, et la sélection, par l'organe de commande, parmi les deuxièmes images miniatures, d'une image qui est le plus similaire à la première image miniature sélectionnée ; ou la réception d'une sélection, effectuée par l'utilisateur, d'une image miniature parmi les deuxièmes images miniatures, et la sélection, par l'organe de commande, parmi les premières images miniatures, d'une image qui est le plus similaire à la deuxième image miniature sélectionnée, et

l'affichage des premières et deuxièmes images miniatures sélectionnées sous leur version agrandie, dans des zones de l'écran autres que les zones dans lesquelles sont affichées les premières et deuxièmes images miniatures.

2. Procédé selon la revendication 1, dans lequel l'affichage des premières images miniatures et des deuxièmes images miniatures dans les zones de l'écran comprend l'affichage des deuxièmes images miniatures dans différentes zones de division de l'écran, compte tenu d'au moins un instant auquel

les deuxièmes images miniatures ont été produites.

3. Procédé selon la revendication 1, dans lequel l'affichage des premières images miniatures et des deuxièmes images miniatures dans les zones de l'écran comprend l'alignement des deuxièmes images miniatures compte tenu d'instantanés auxquels les deuxièmes images miniatures ont été produites pour ainsi afficher les deuxièmes images miniatures alignées.

4. Support d'enregistrement non transitoire lisible par ordinateur sur lequel est enregistré un programme permettant d'exécuter le procédé selon la revendication 1.

5. Dispositif d'affichage d'une image médicale, le dispositif comprenant :

un processeur d'image (1200, 1201) conçu pour produire des premières images montrant une région d'intérêt (ROI) au moyen de signaux d'écho correspondant à des signaux ultrasonores émis vers la ROI,

un organe de commande (1700, 1701) conçu pour sélectionner, parmi des images préenregistrées, des deuxièmes images montrant la ROI, lesdites deuxièmes images ayant été produites à un instant passé, et

un dispositif d'affichage (1400, 1401) conçu pour afficher les premières images et les deuxièmes images sur un écran en réaction à un signal de commande produit par l'organe de commande ;

ledit dispositif d'affichage (1400, 1401) étant conçu en outre pour afficher des premières images miniatures correspondant aux premières images dans une zone de l'écran, et pour afficher des deuxièmes images miniatures correspondant aux deuxièmes images dans une autre zone de l'écran,

ledit organe de commande (1700, 1701) étant conçu en outre pour recevoir une sélection, effectuée par l'utilisateur, d'une image miniature parmi les premières images miniatures, et pour sélectionner, parmi les deuxièmes images miniatures, une image qui est le plus similaire à la première image miniature sélectionnée ; ou pour recevoir une sélection, effectuée par l'utilisateur, d'une image miniature parmi les deuxièmes images miniatures, et pour sélectionner, parmi les premières images miniatures, une image qui est le plus similaire à la deuxième image miniature sélectionnée, et

ledit dispositif d'affichage (1400, 1401) étant conçu en outre pour afficher les premières et deuxièmes images miniatures sélectionnées, sous leur version agrandie, dans des zones de

l'écran autres que les zones dans lesquelles sont affichées les premières et deuxièmes images miniatures.

6. Dispositif selon la revendication 5, dans lequel l'organe de commande est conçu en outre pour produire le signal de commande de manière que les deuxièmes images miniatures soient affichées dans différentes zones de division de l'écran, compte tenu d'au moins un instant auquel les deuxièmes images miniatures ont été produites. 5 10
7. Dispositif selon la revendication 5, dans lequel l'organe de commande est conçu en outre pour produire le signal de commande de manière que les deuxièmes images miniatures soient alignées compte tenu d'instantaux auxquels les deuxièmes images miniatures ont été produites et soient ainsi affichées. 15

20

25

30

35

40

45

50

55

FIG. 1B

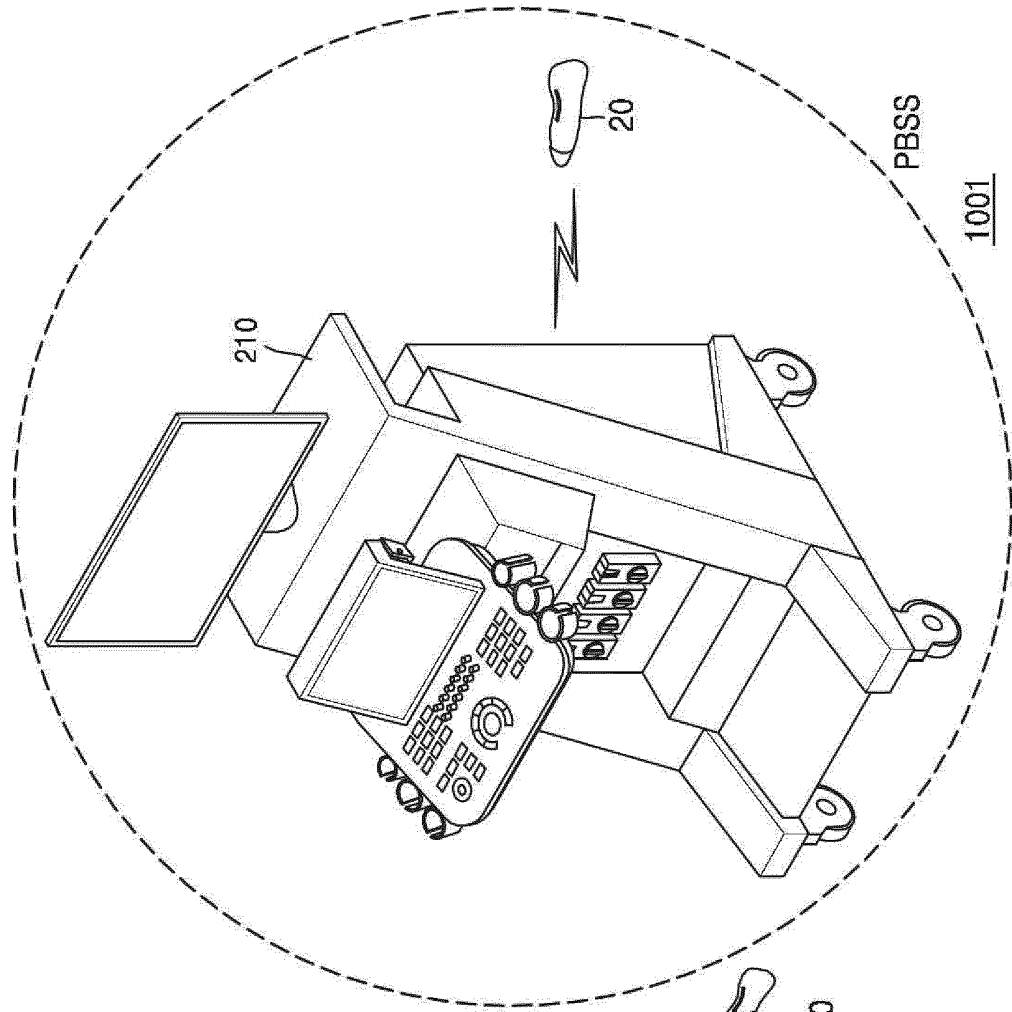


FIG. 1A

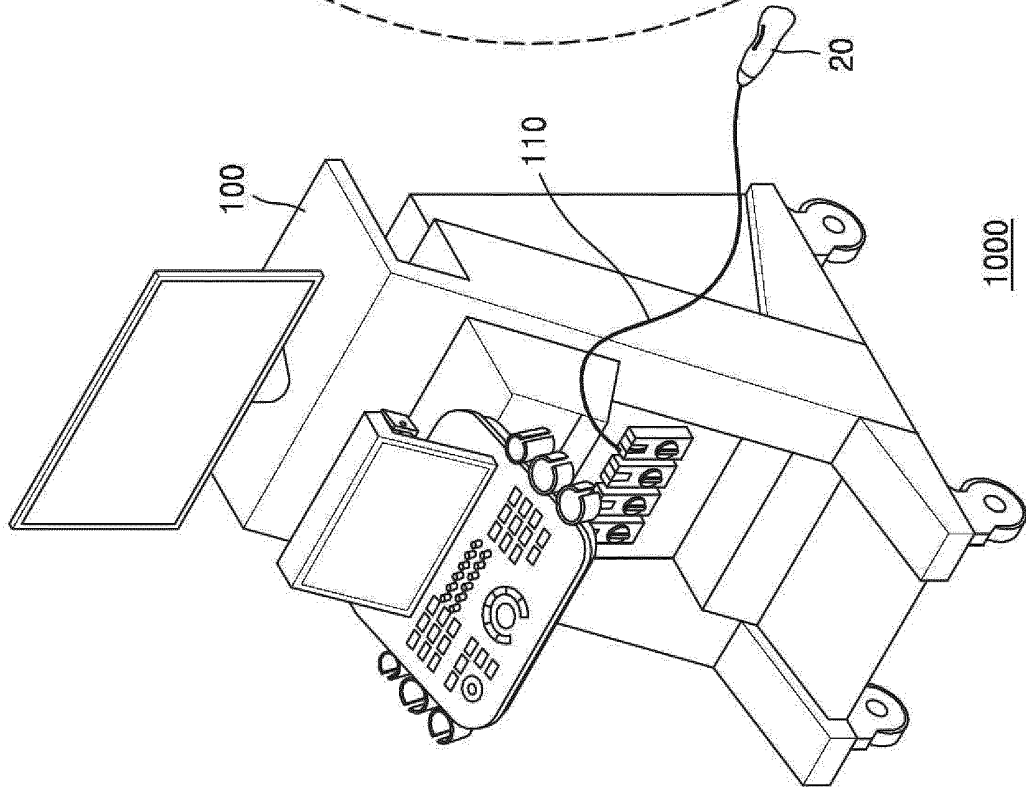


FIG. 2

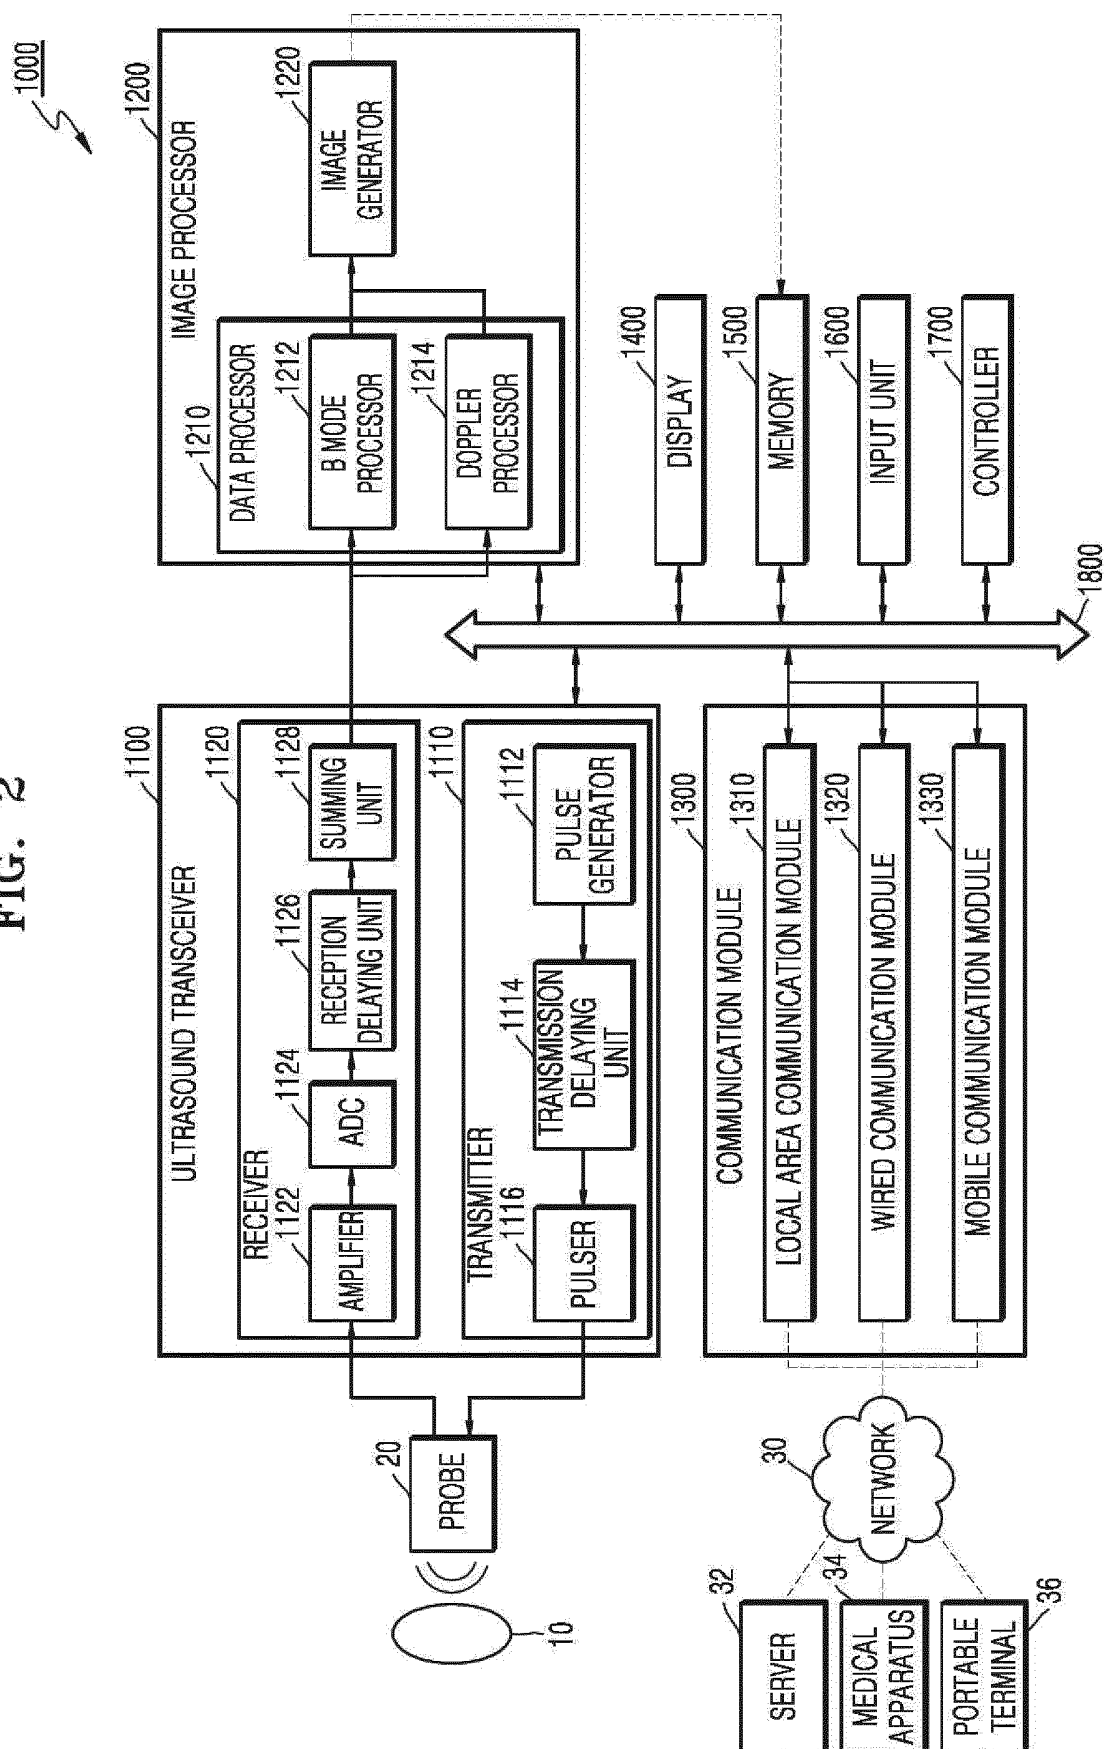


FIG. 3

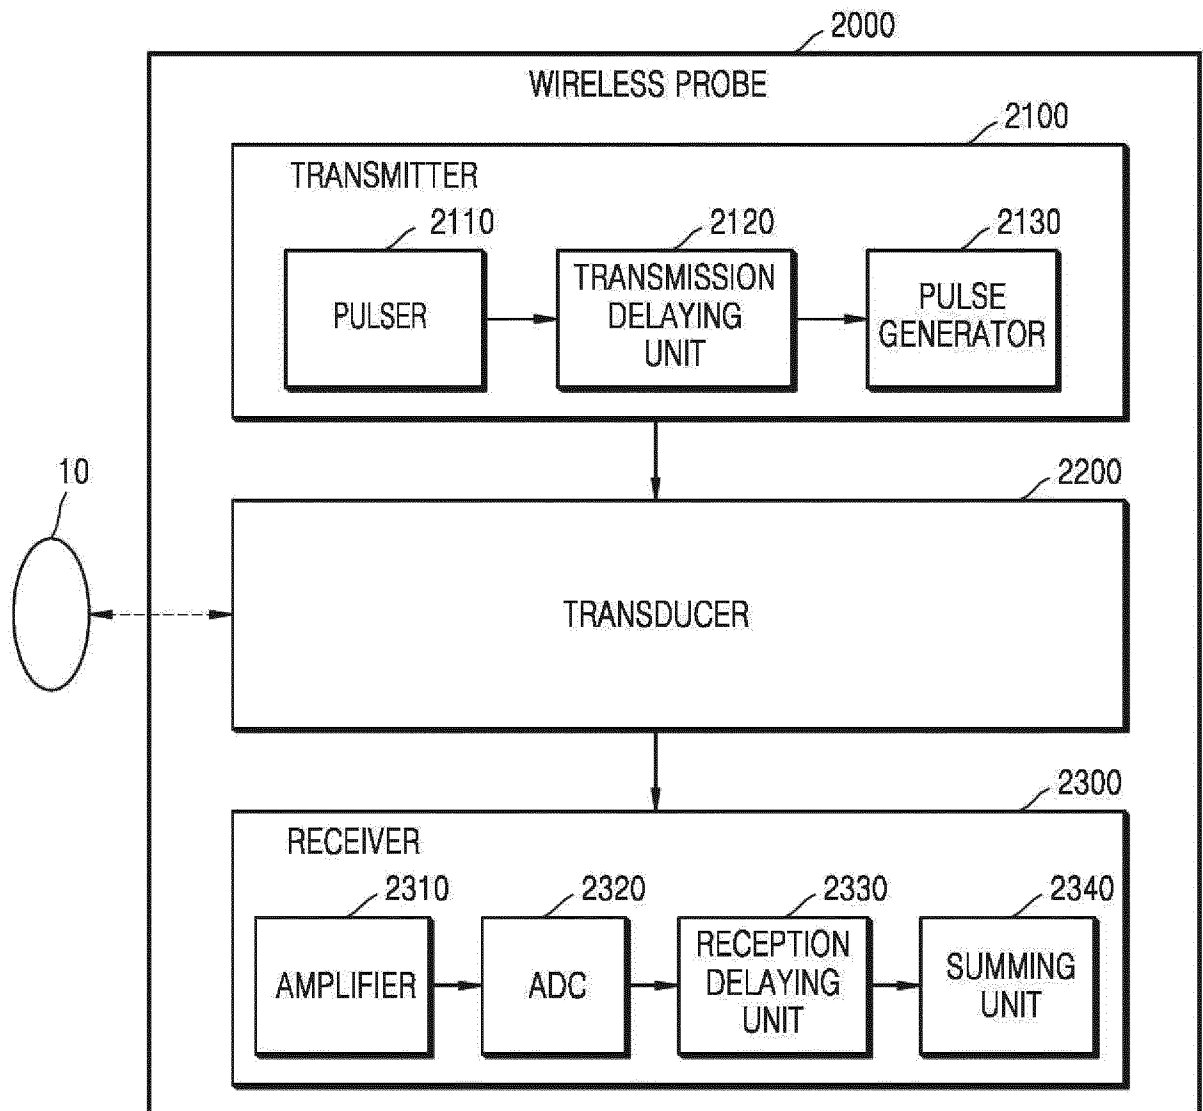


FIG. 4A

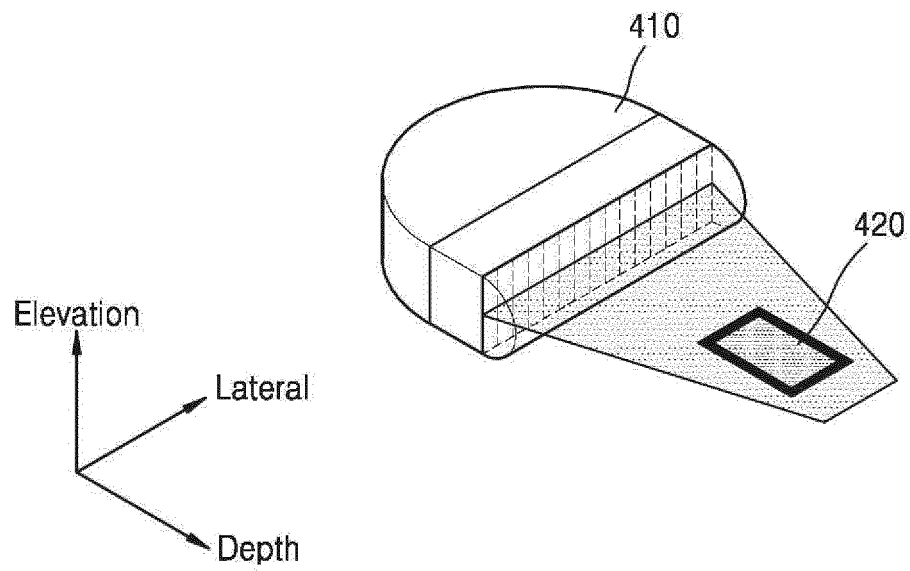


FIG. 4B

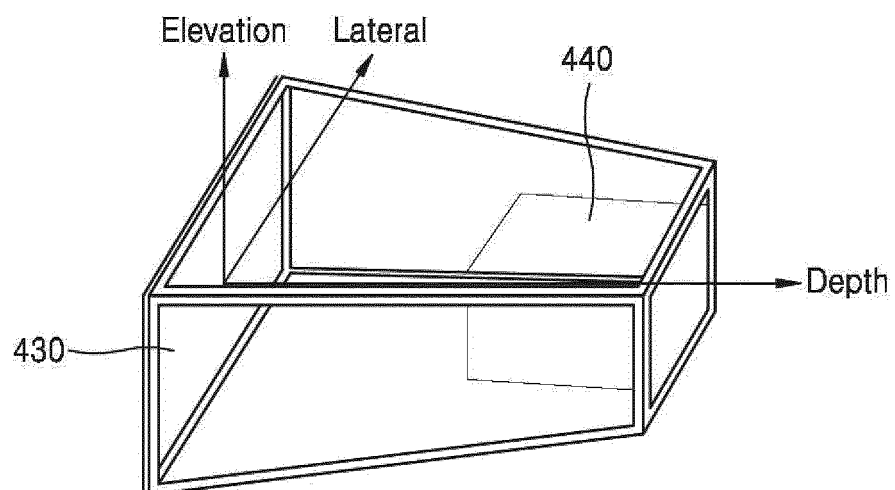


FIG. 5

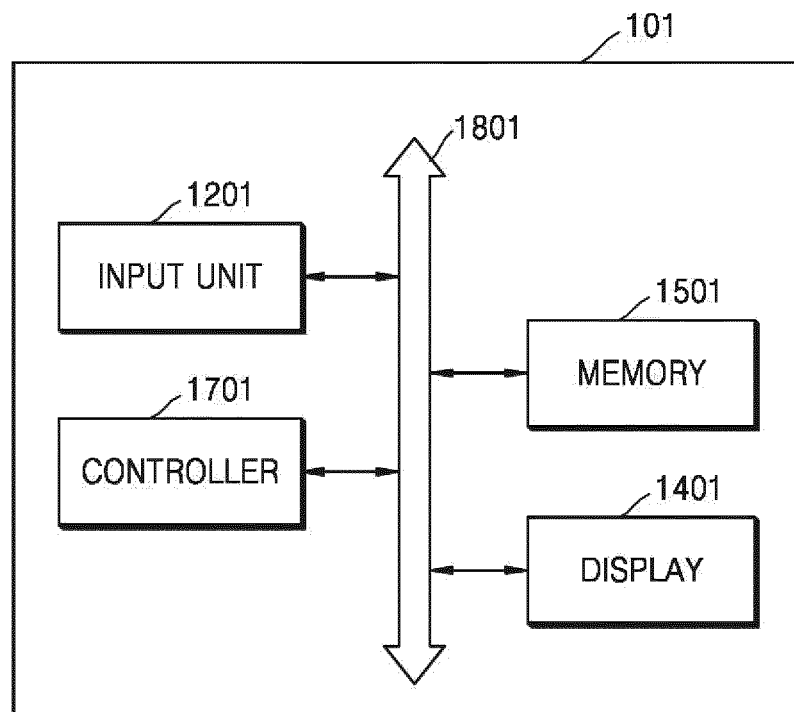


FIG. 6

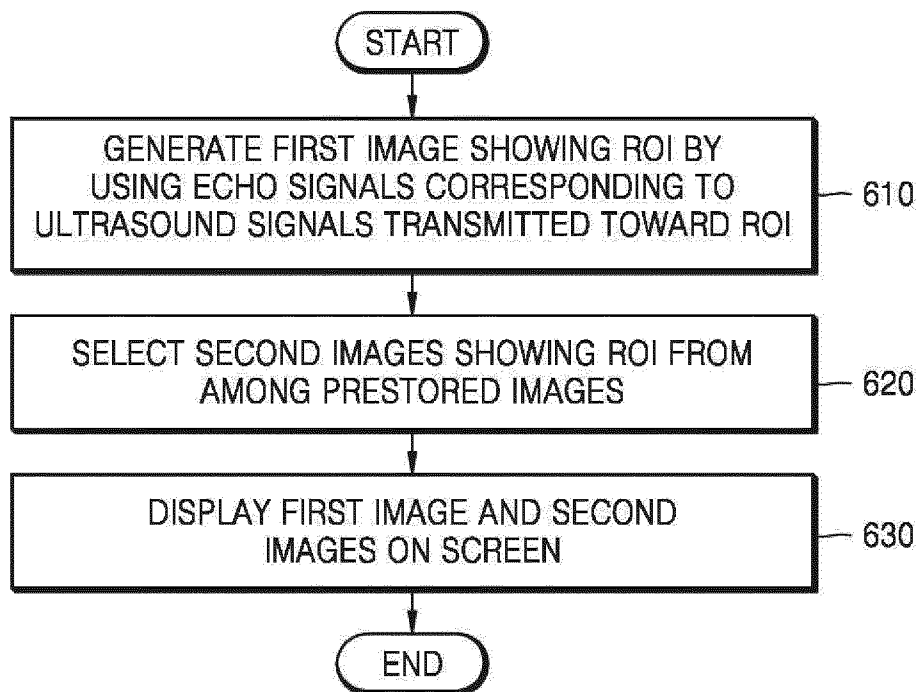


FIG. 7

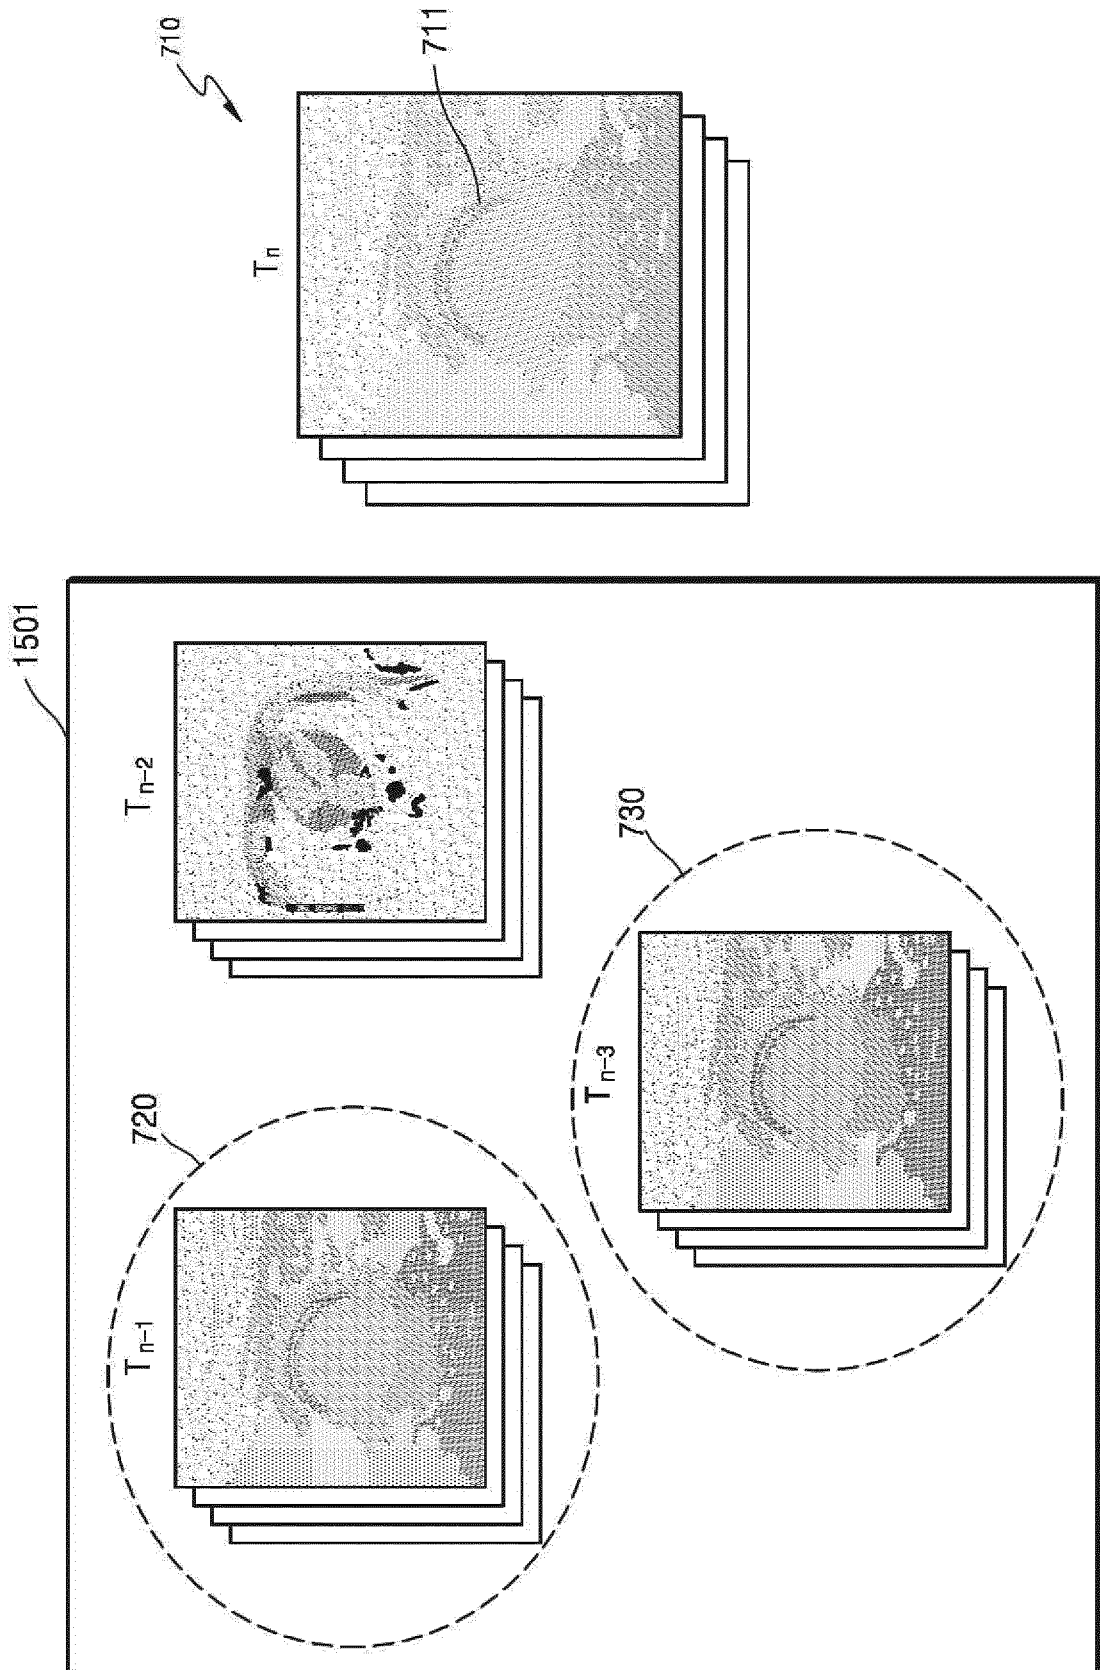


FIG. 8

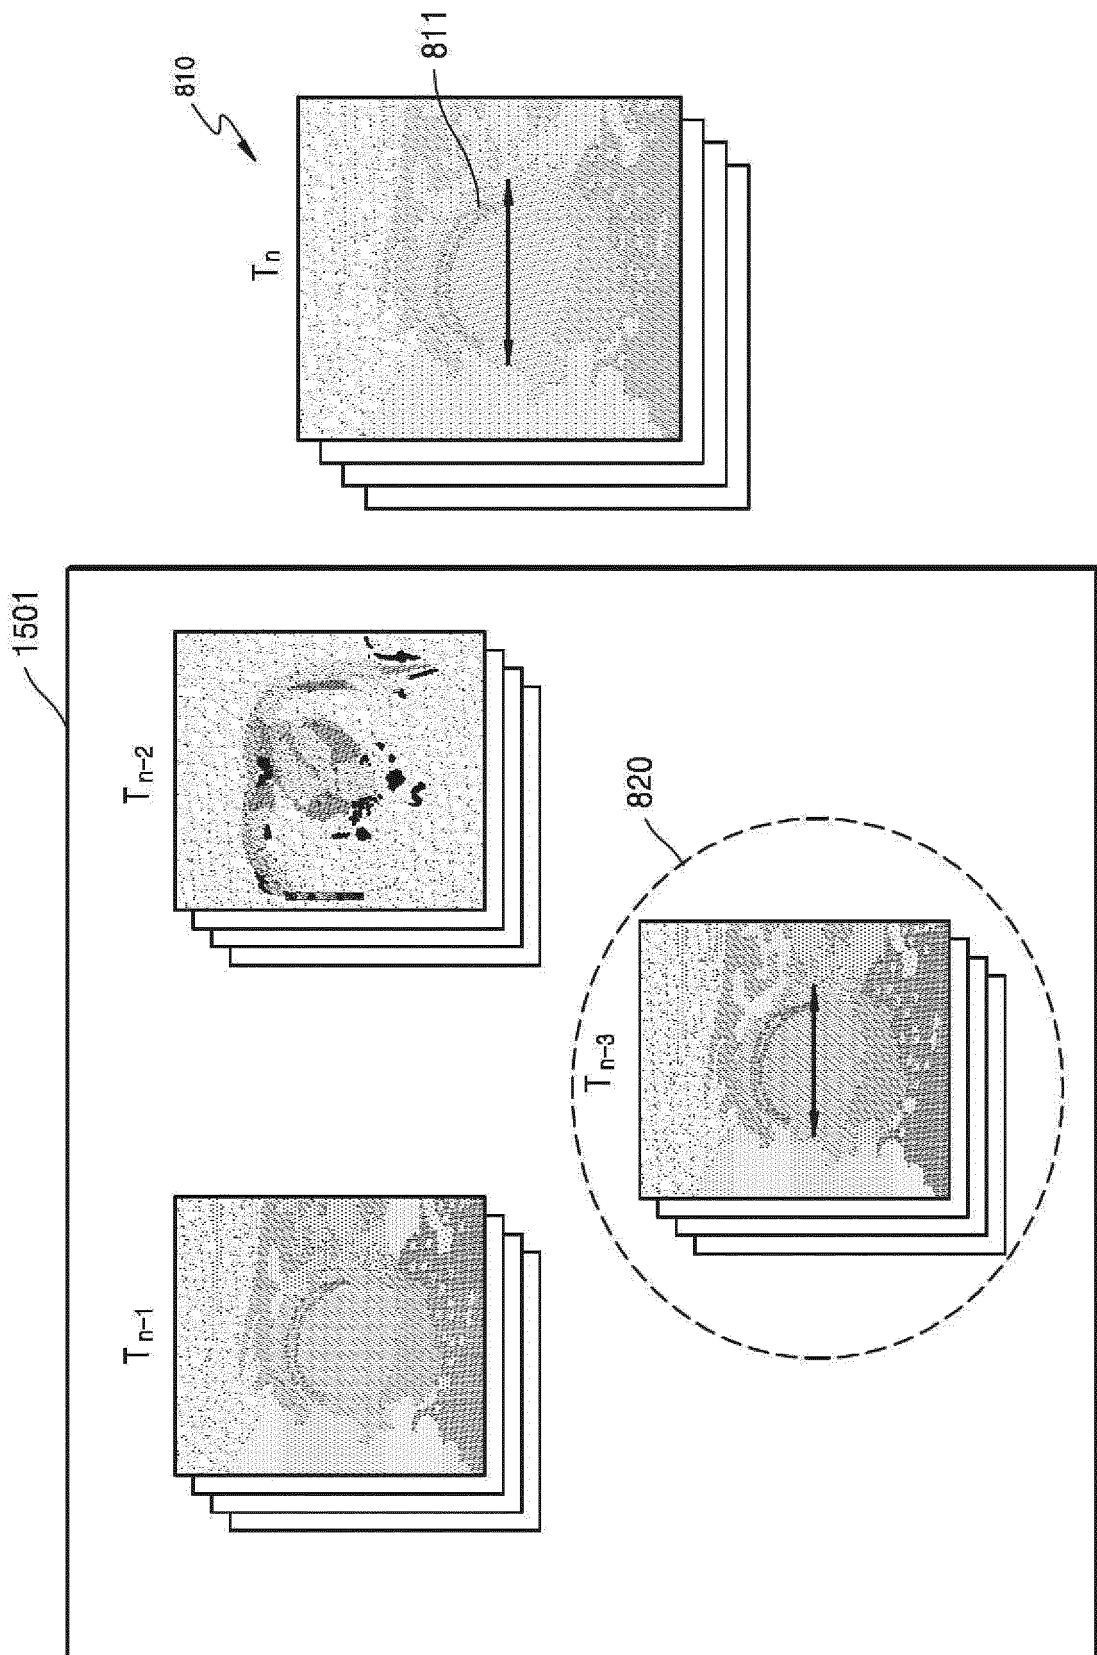


FIG. 9

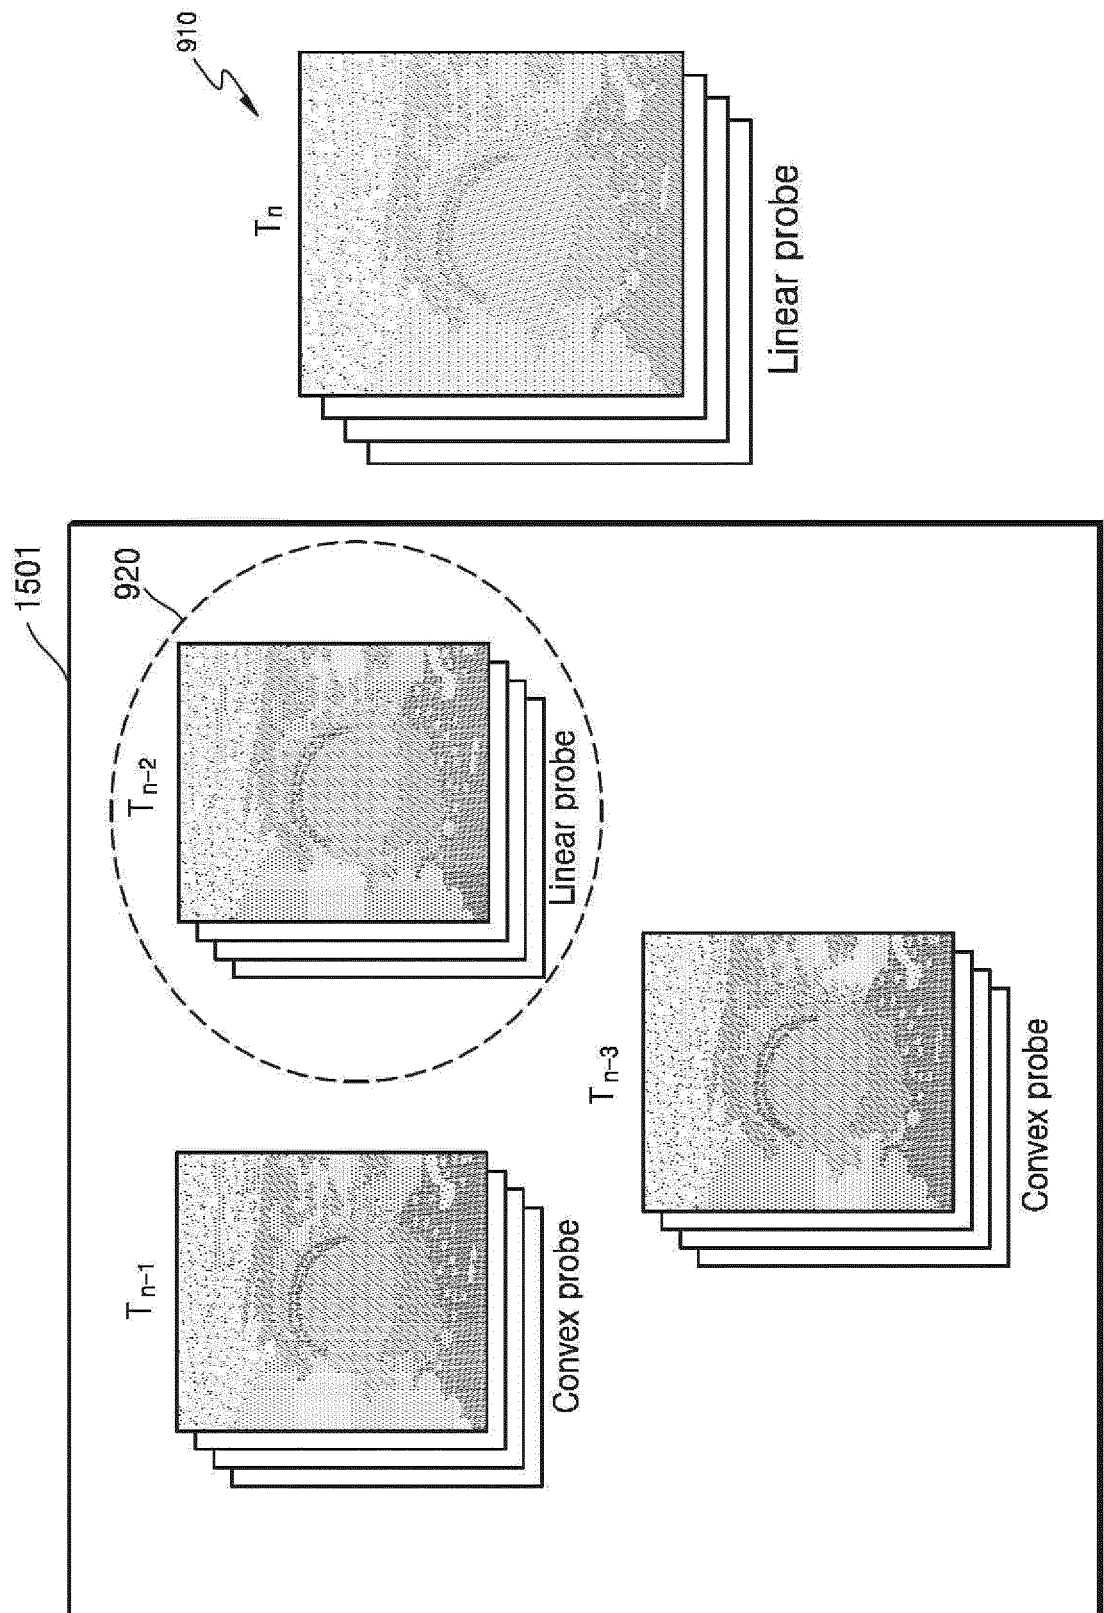


FIG. 10

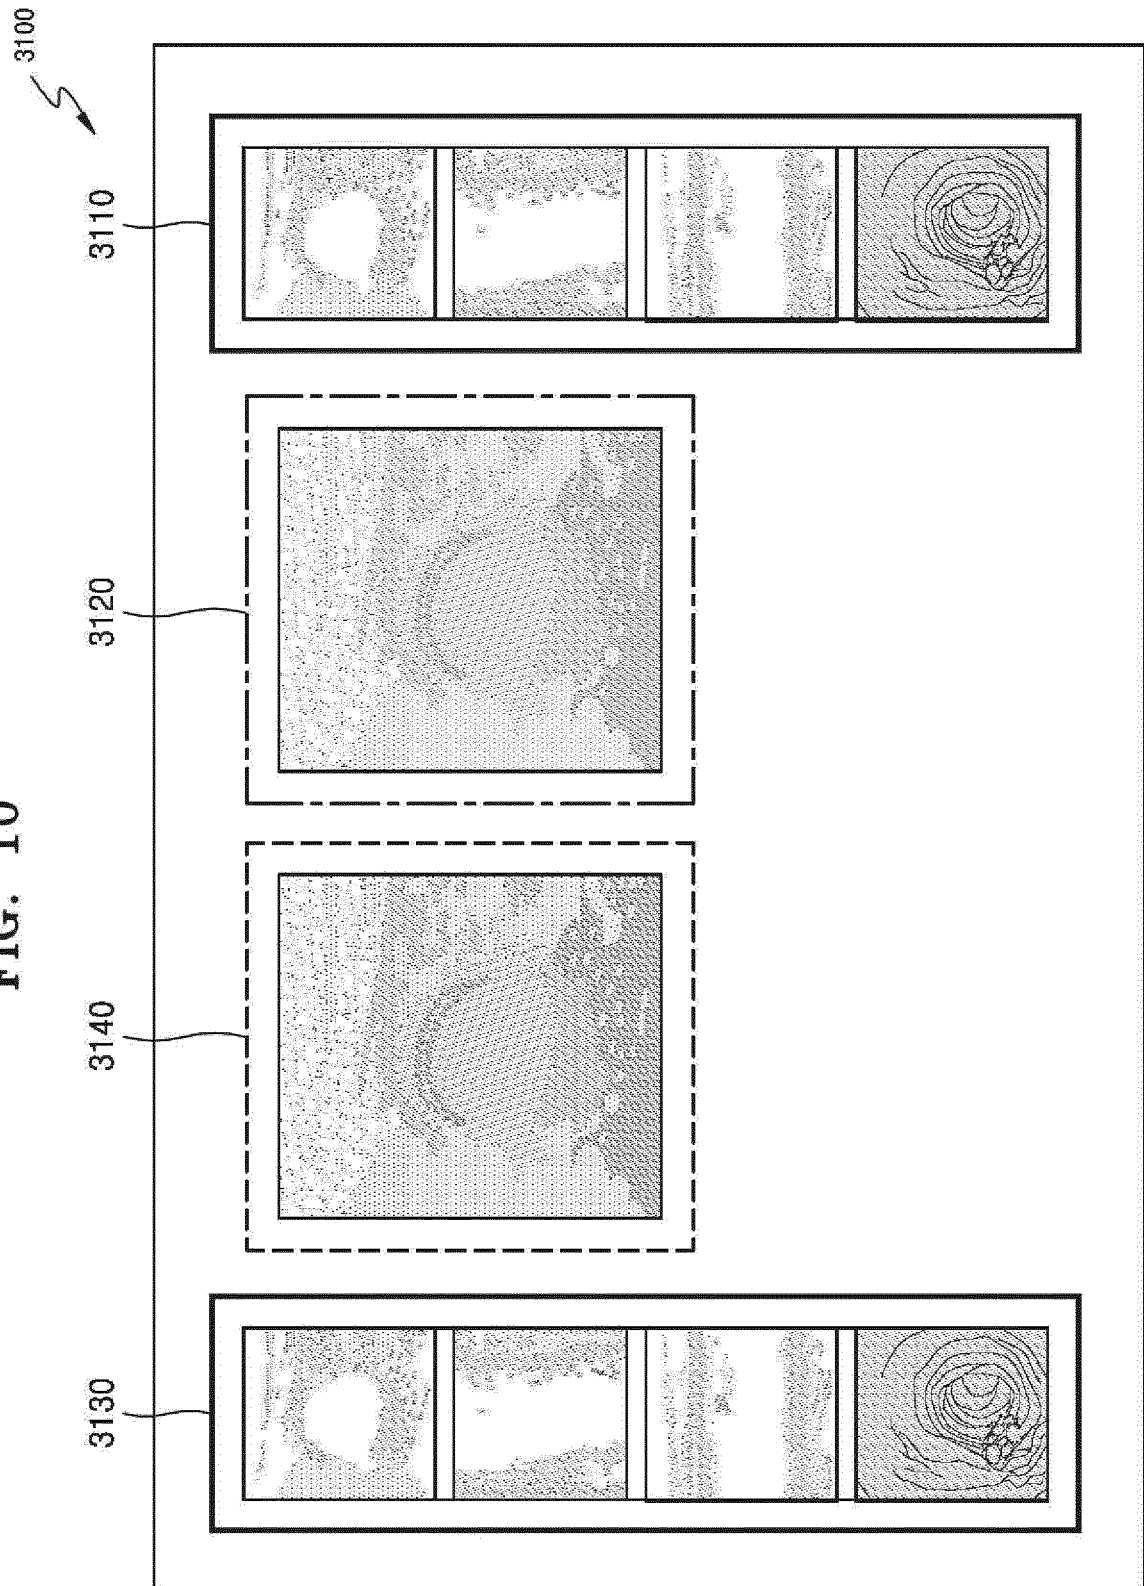


FIG. 11

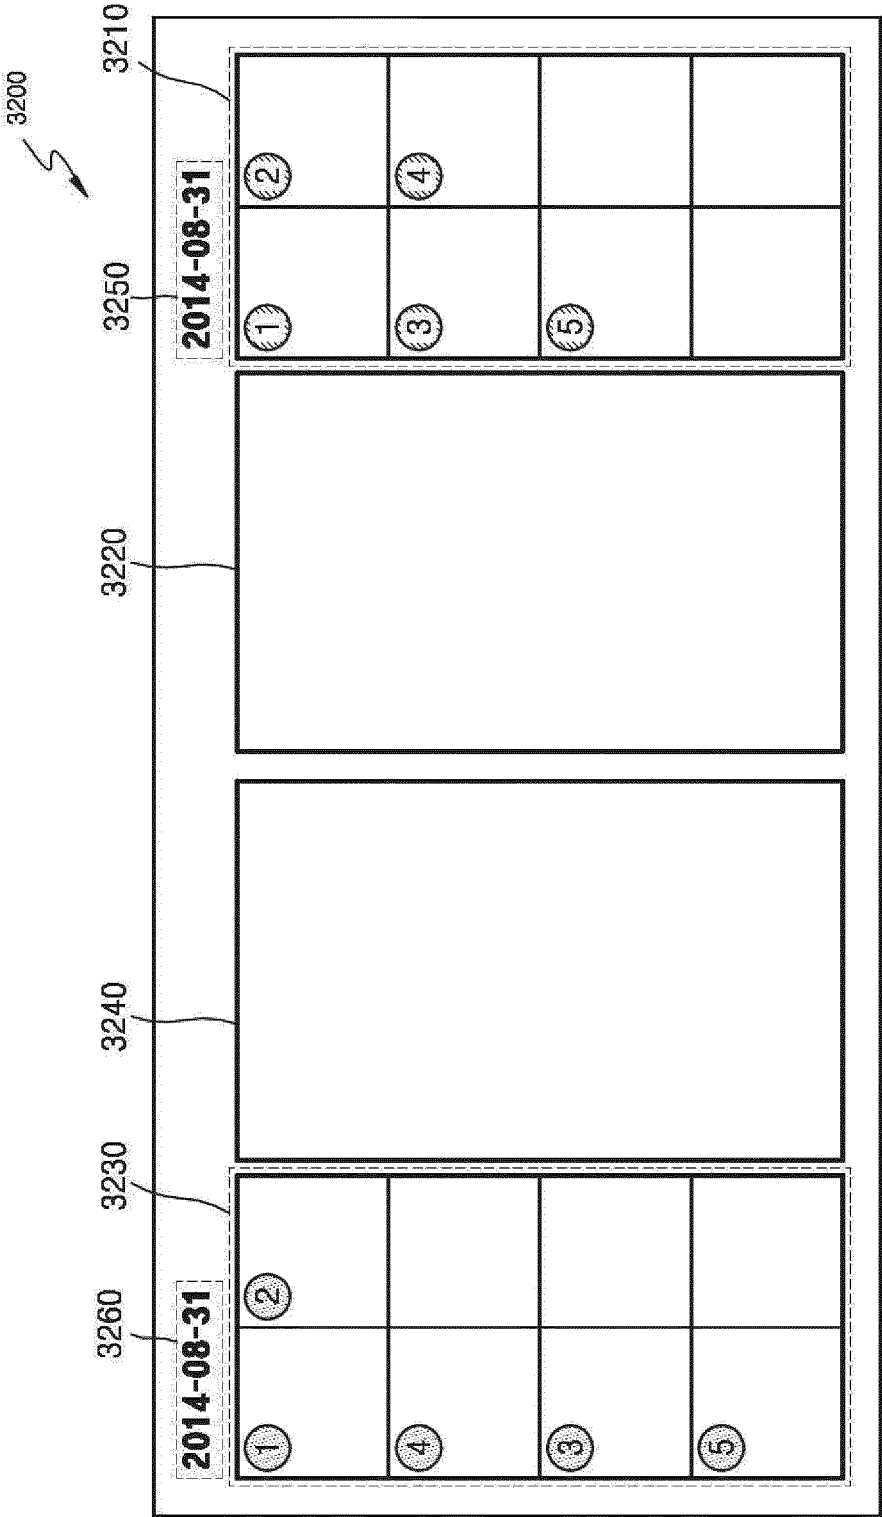


FIG. 12

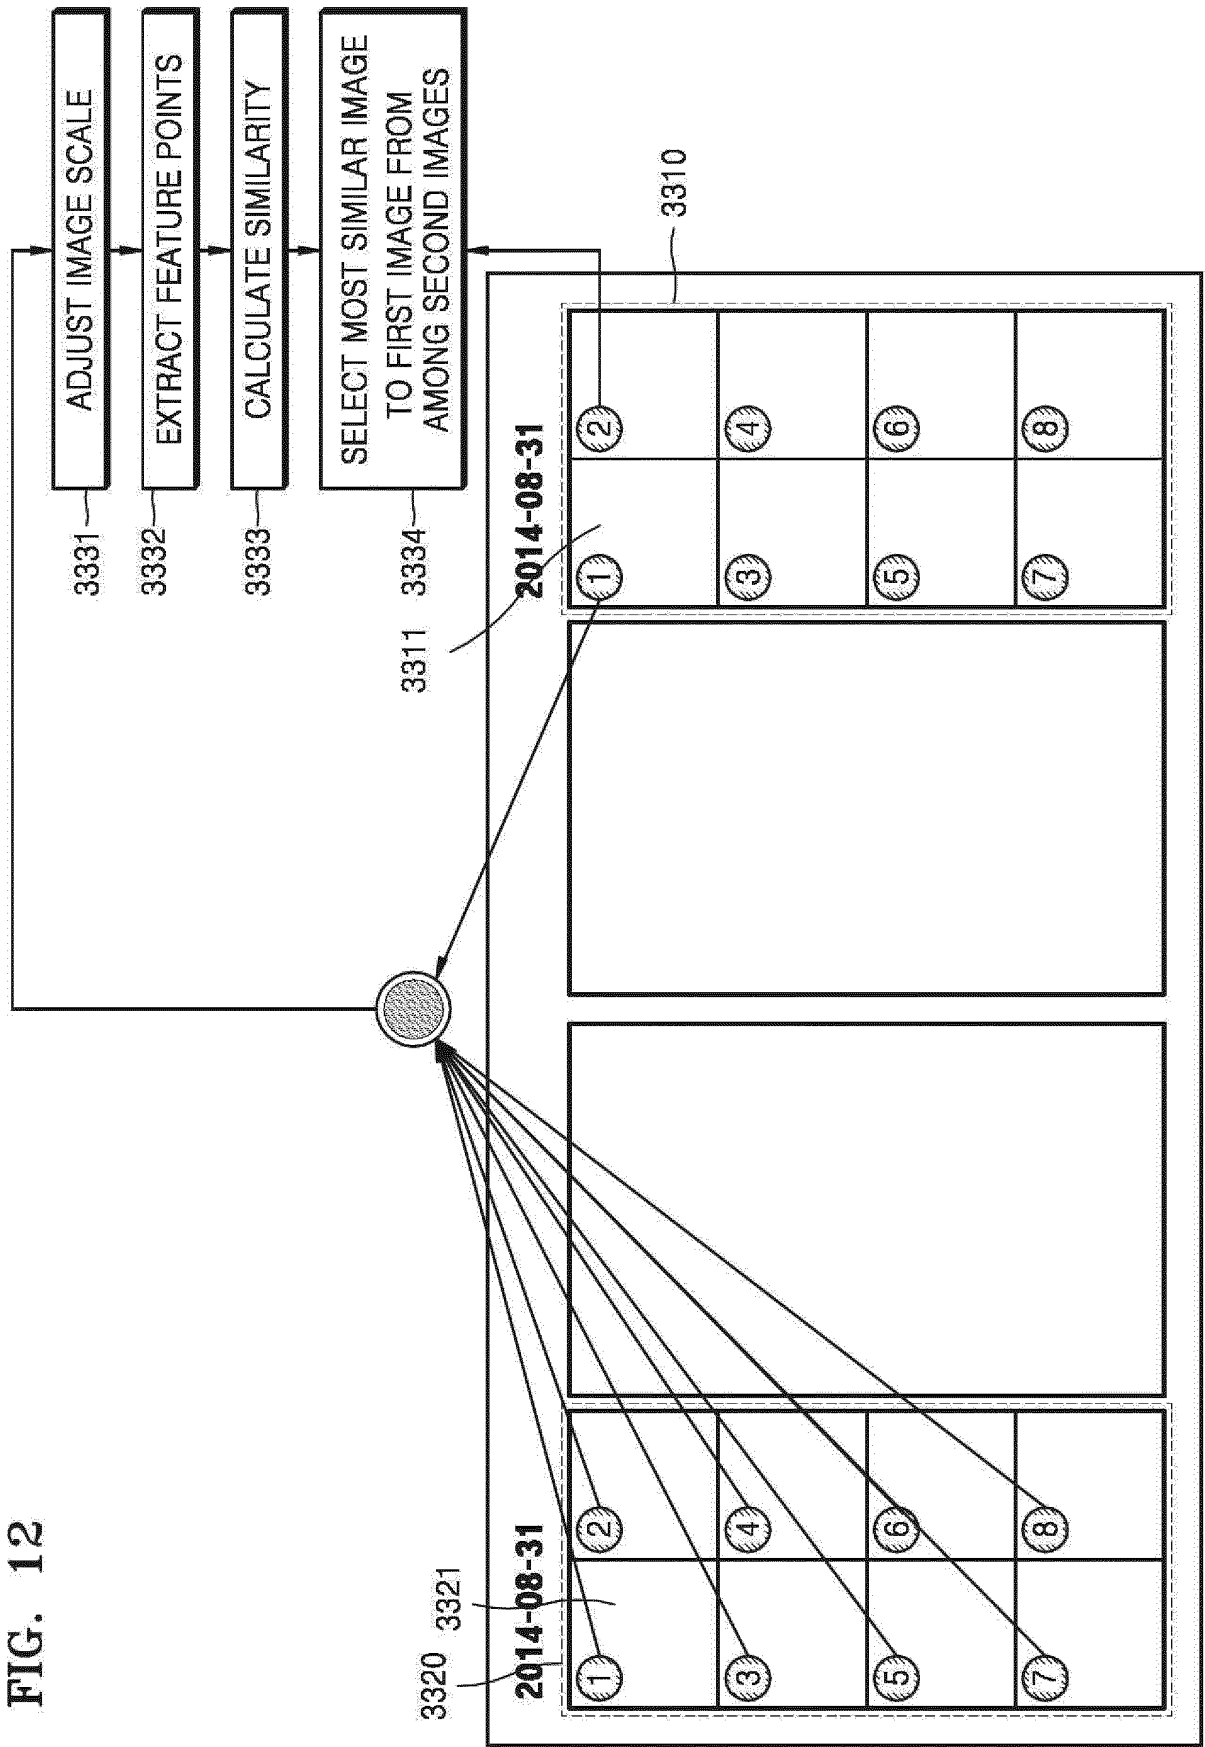


FIG. 13

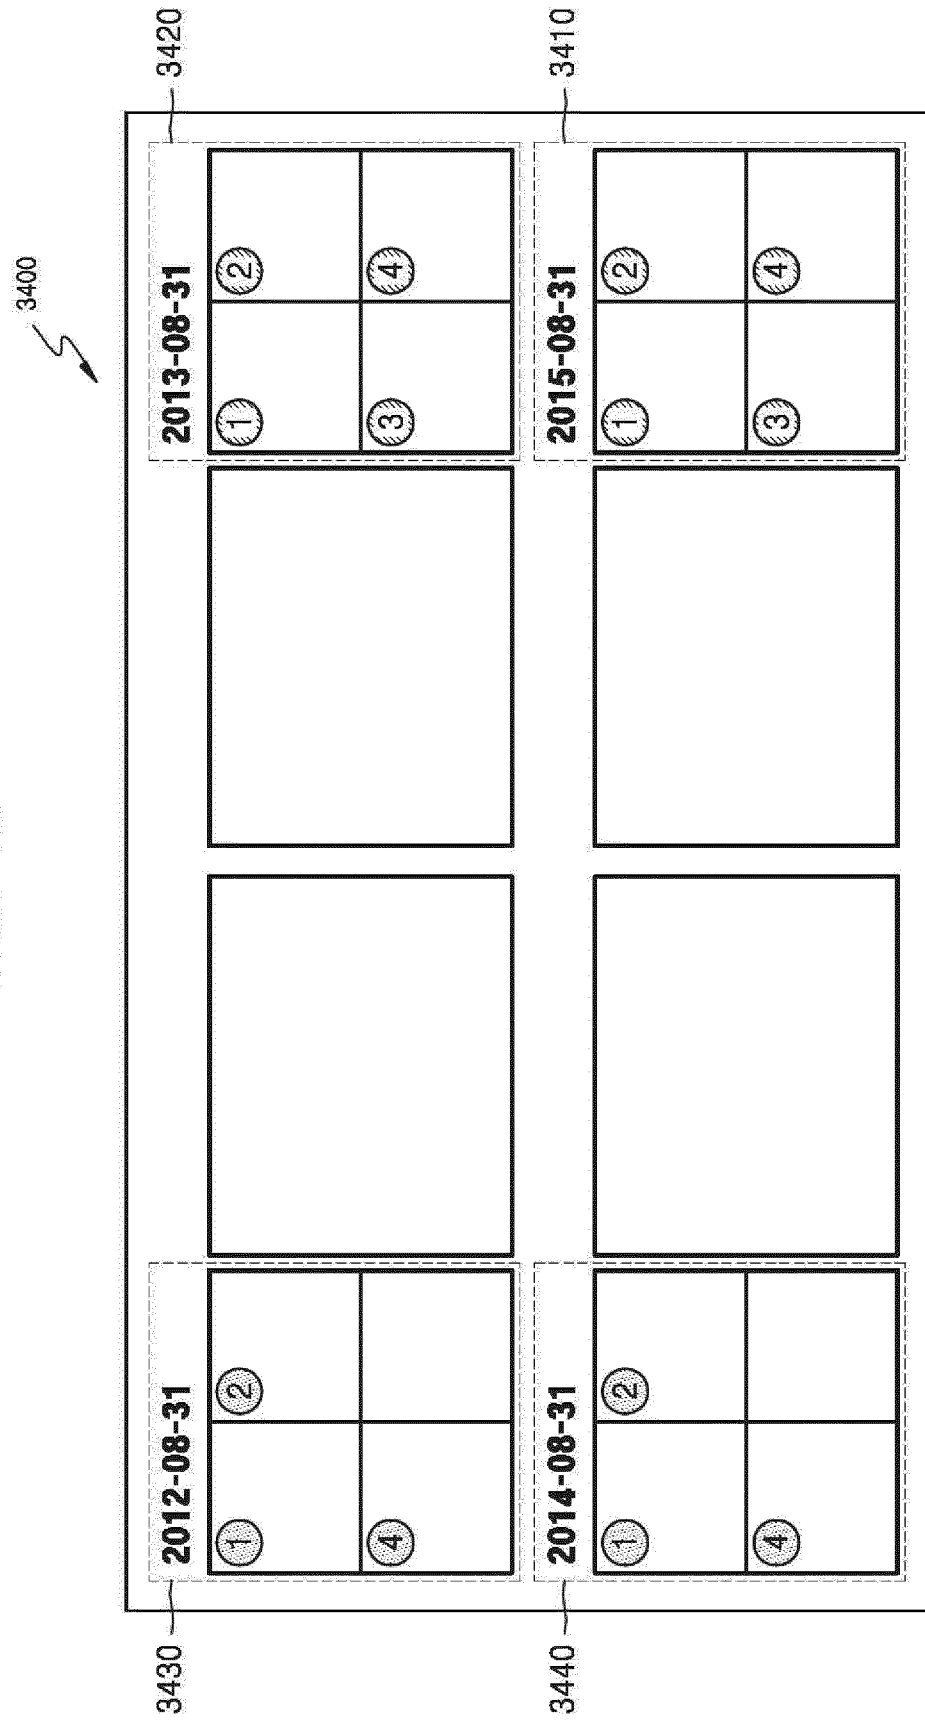


FIG. 14

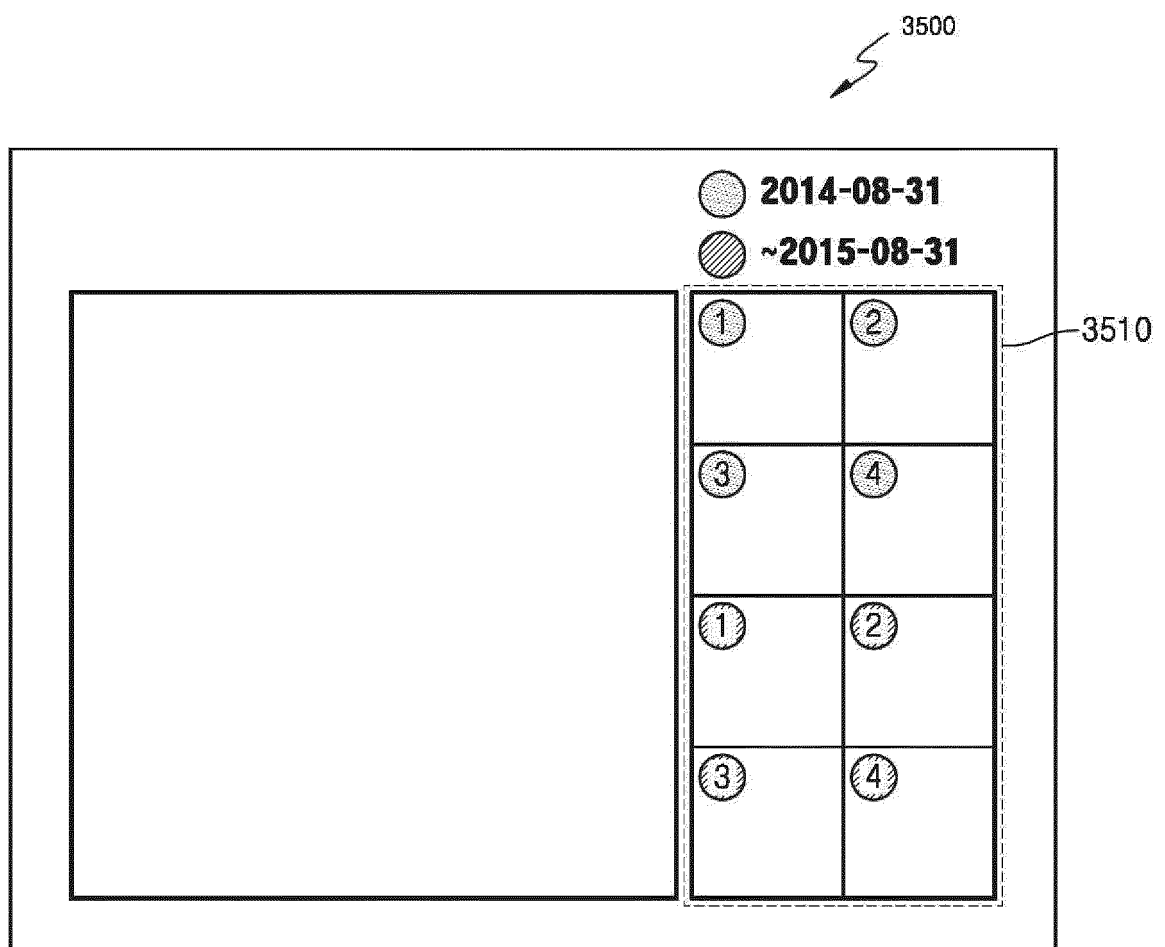


FIG. 15

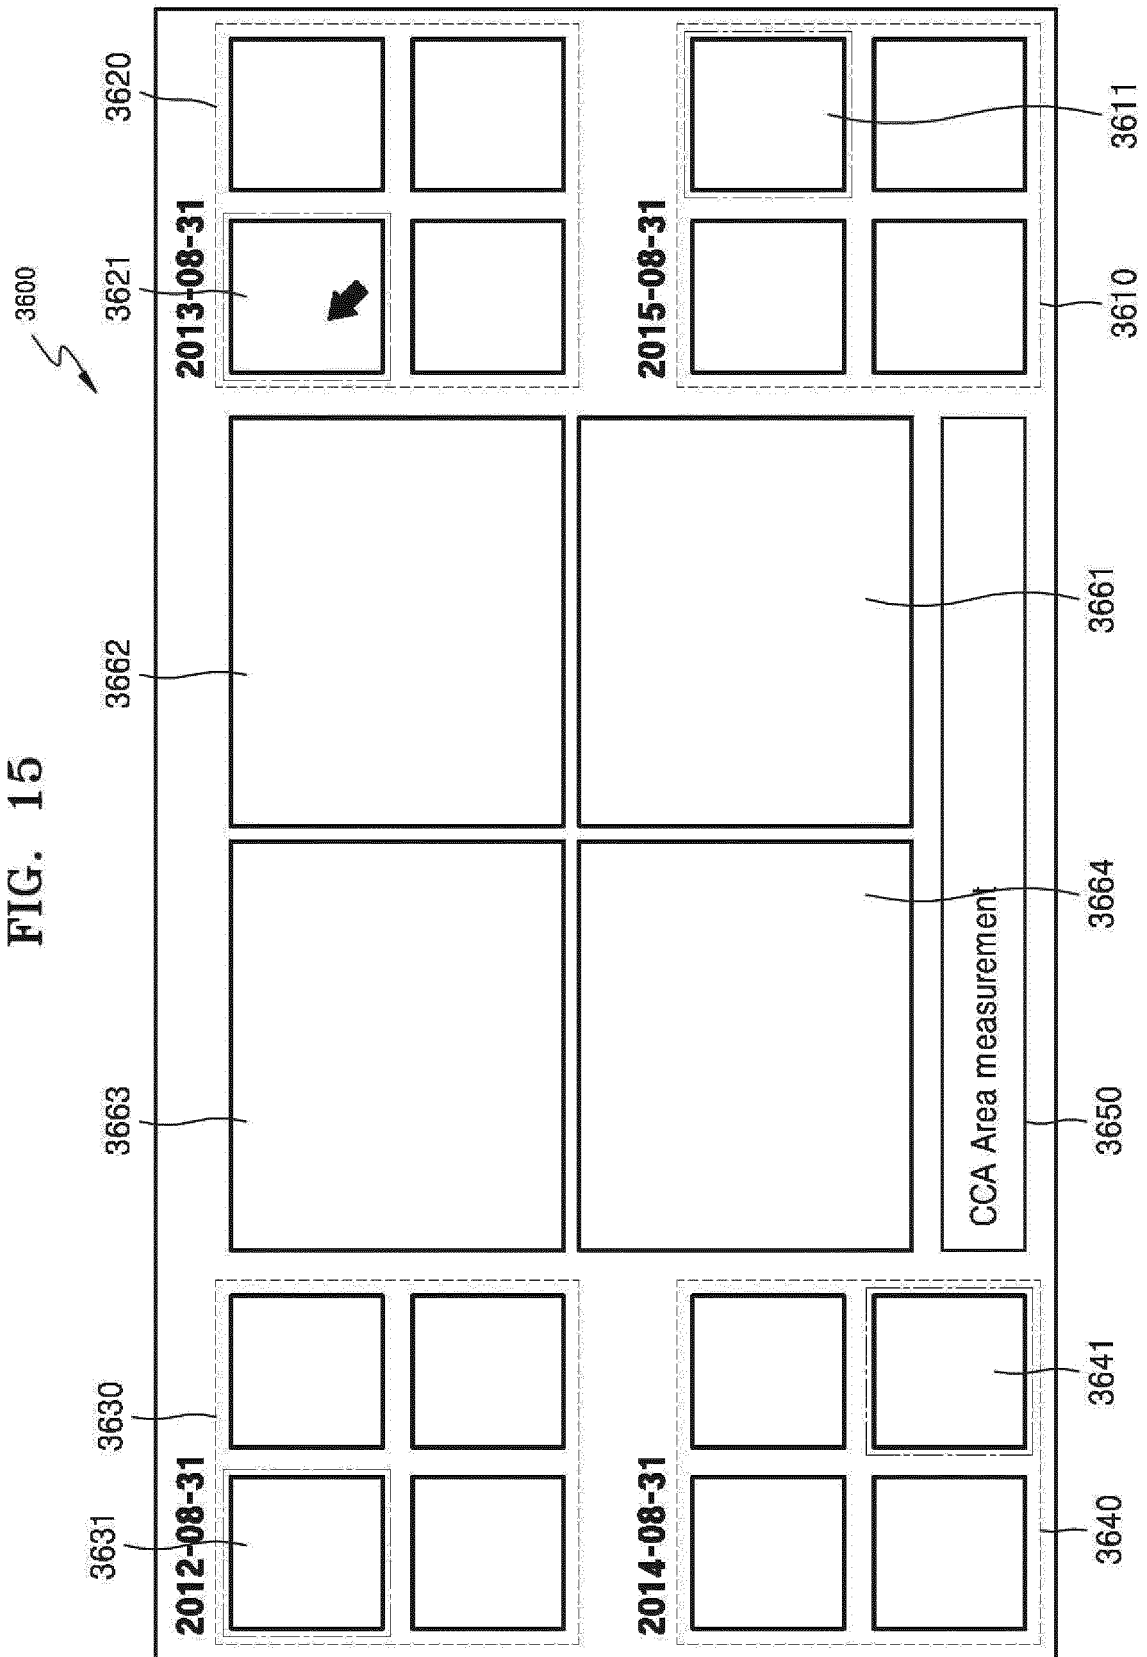


FIG. 16

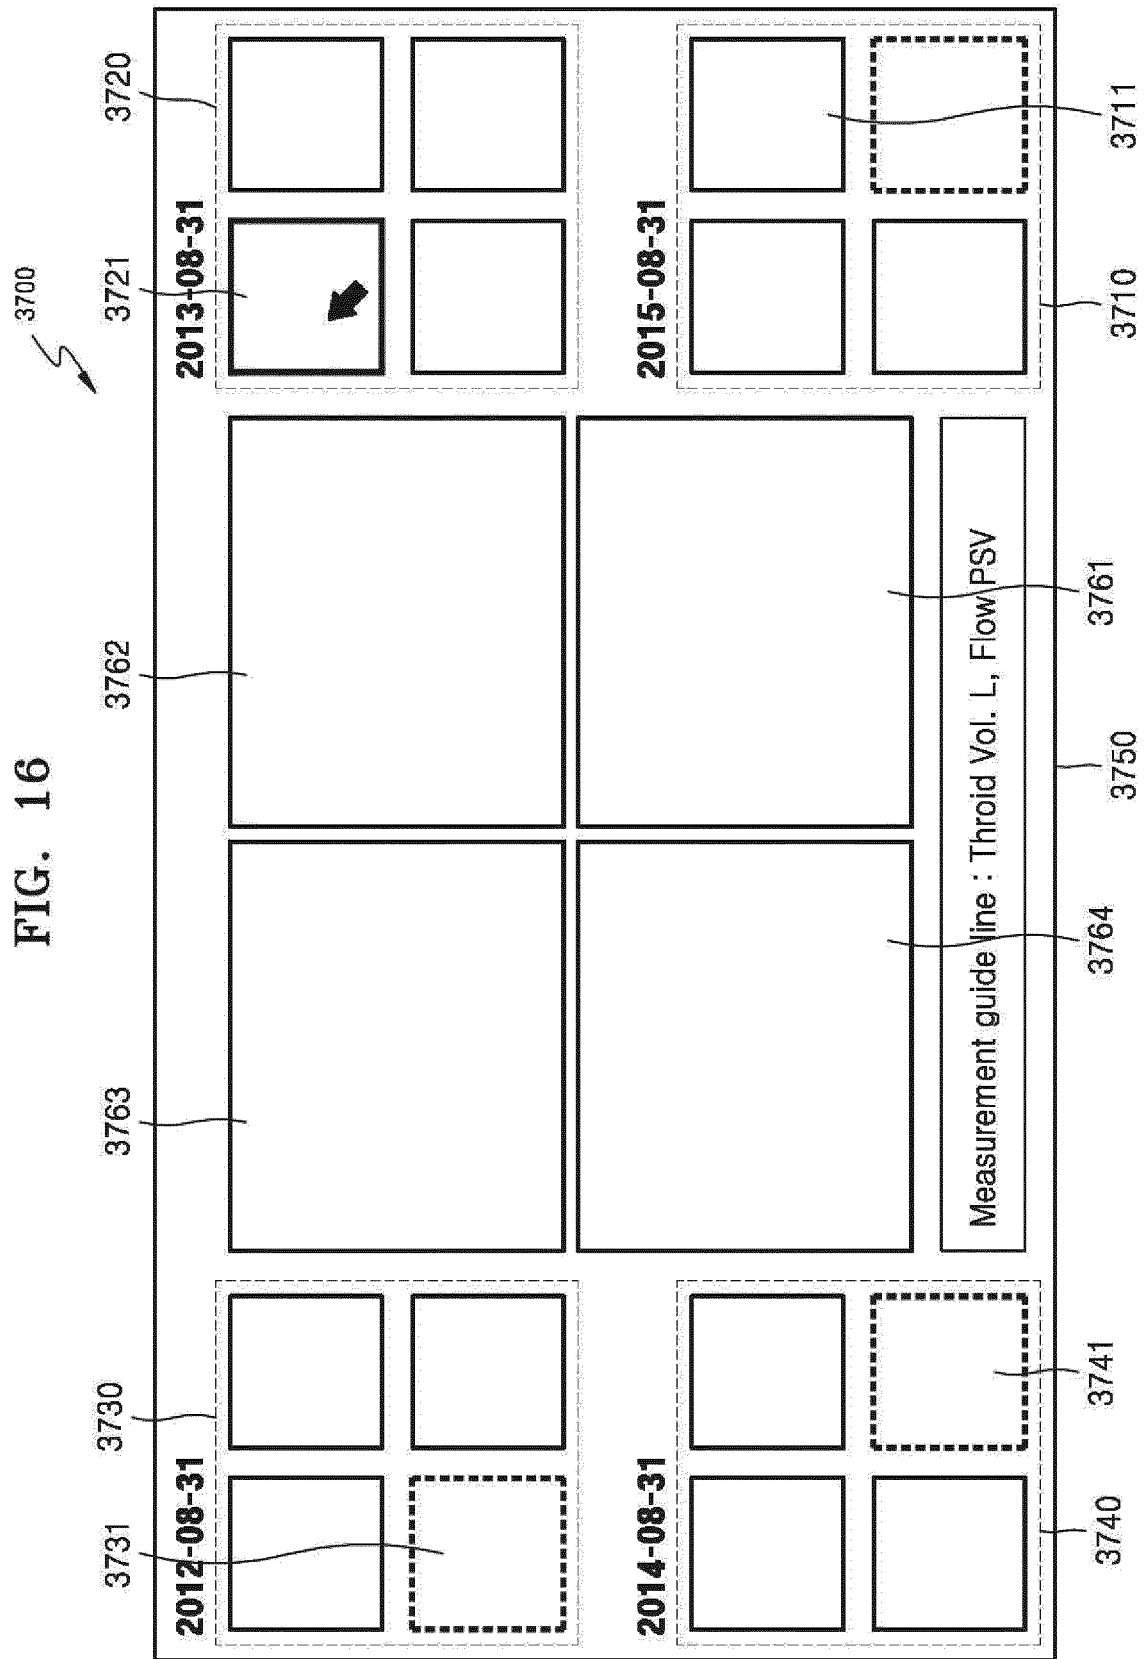


FIG. 17

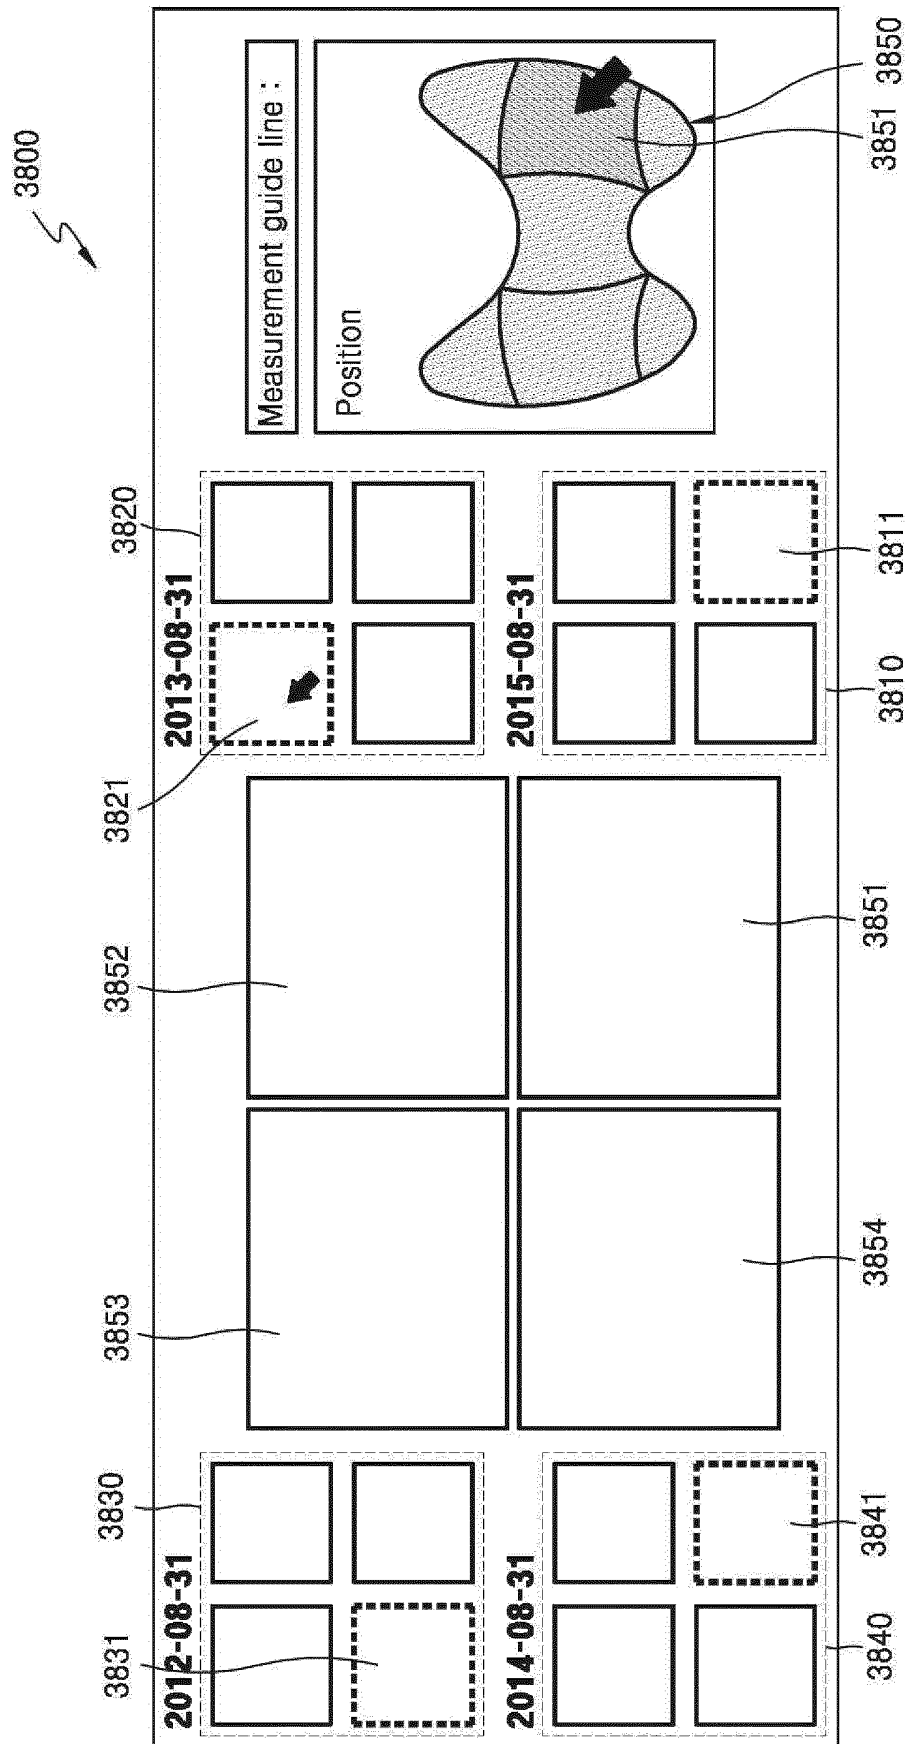


FIG. 18A

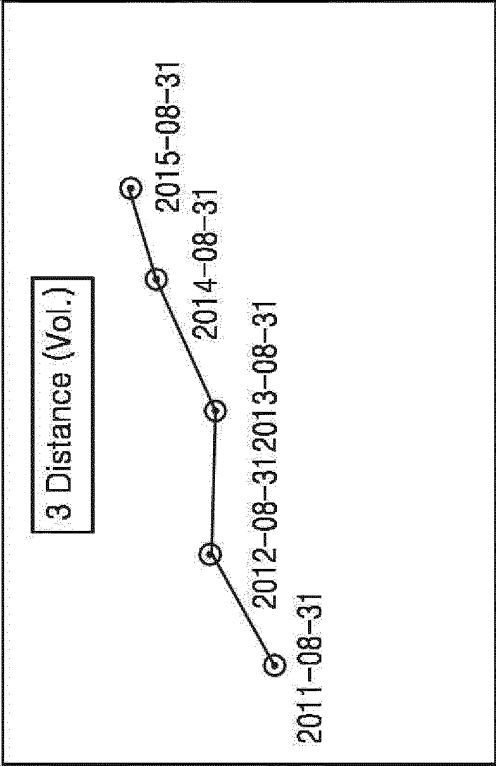


FIG. 18B

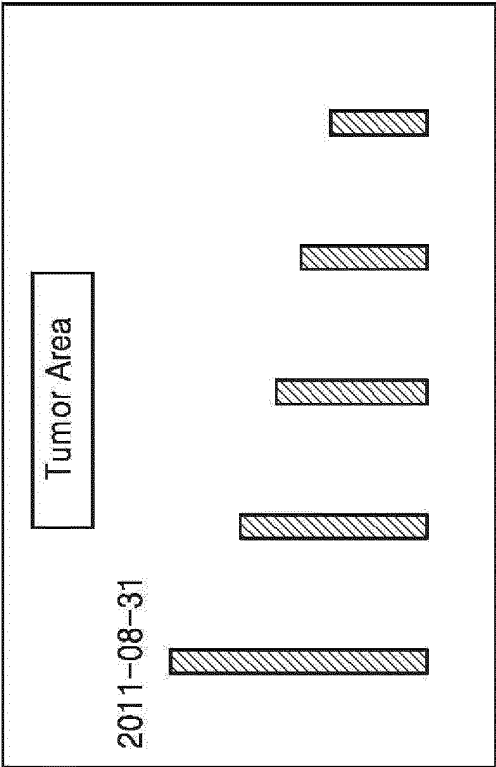


FIG. 18C

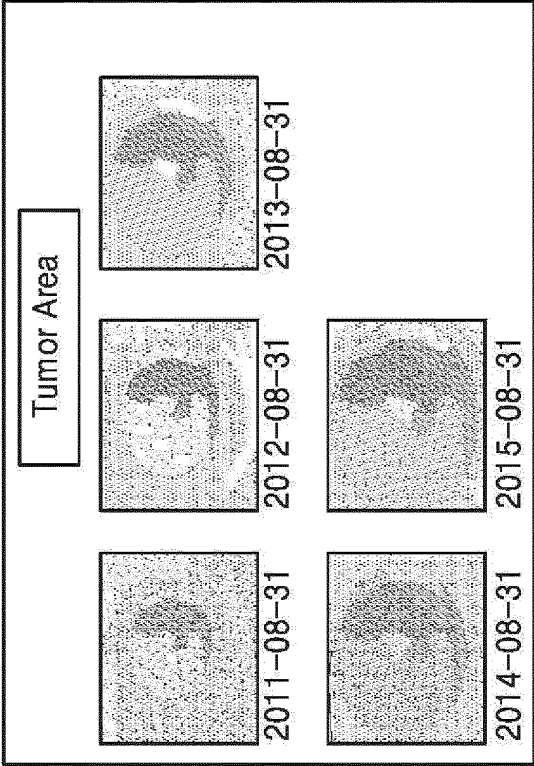


FIG. 18D

	2011-08	2012-08	2013-08	2014-08	2015-08
measurement 1	88.235	40.4517	57.06005	5.151227	69.21944
measurement 2	92.95219	46.2977	47.94677	33.1239	48.10357
measurement 3	95.16844	44.07981	40.74034	56.28862	36.55781
measurement 4	74.20378	8.382523	48.01769	10.76682	65.15684

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20150305718 A1 [0003]
- US 20150011872 A1 [0003]
- US 20140378836 A1 [0003]

专利名称(译)	显示超声图像的方法和装置		
公开(公告)号	EP3184050B1	公开(公告)日	2020-05-27
申请号	EP2016184051	申请日	2016-08-12
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	LEE BONG HEON SHIN DONG KUK		
发明人	LEE, BONG-HEON SHIN, DONG-KUK		
IPC分类号	A61B8/00 G01S15/89 G06T7/30 G06T7/11 G01S7/52		
CPC分类号	A61B8/4405 A61B8/463 G01S7/52063 G01S7/52073 G01S7/52074 G01S15/8915 G06T7/11 G06T7/30 A61B6/463 A61B8/00 A61B8/485 A61B8/488 A61B8/5223 G01S7/52036 G06F3/04842 G06F40/106 G06F40/166 G06T7/0012 G06T2207/10132 G06T2207/30004 G16H10/60 G16H15/00 G16H30/40 G16H50/70		
优先权	1020150184080 2015-12-22 KR		
其他公开文献	EP3184050A1		
外部链接	Espacenet		

摘要(译)

提供了一种显示医学图像的方法，该方法包括：通过使用与朝着ROI发射的超声信号相对应的回波信号来生成示出感兴趣区域 (ROI) 的第一图像；以及 从预存图像中选择显示ROI的第二图像； 在屏幕上显示第一图像和第二图像。

