



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
14.08.2019 Bulletin 2019/33

(51) Int Cl.:
A61B 8/08 (2006.01) A61B 8/00 (2006.01)

(21) Application number: **18200566.0**

(22) Date of filing: **16.10.2018**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
 Designated Extension States:
BA ME
 Designated Validation States:
KH MA MD TN

(72) Inventors:
 • **KIM, Jung-ho Gyeonggi-do (KR)**
 • **LEE, Yoon-chang Gyeonggi-do (KR)**

(74) Representative: **Grootscholten, Johannes A.M. et al**
Arnold & Siedsma
Bezuidenhoutseweg 57
2594 AC The Hague (NL)

(30) Priority: **13.02.2018 KR 20180018062**


(71) Applicant: **Samsung Medison Co., Ltd.**
Hongcheon-gun, Gangwon-do, 25108 (KR)

(54) **ULTRASOUND IMAGING APPARATUS AND METHOD OF CONTROLLING SAME**

(57) An ultrasound imaging apparatus and a controlling method thereof are provided. The ultrasound imaging apparatus acquires a plurality of ultrasound contrast agent images of a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted to the region of interest of the object, into which the contrast agent is injected, at time intervals of t_k ($k = 1,$

$2, \dots, n,$ and n is an integer of 2 or more), generates a k^{th} cumulative ultrasound contrast agent image by accumulating the acquired ultrasound contrast agent images at every time intervals of t_k to generate n cumulative ultrasound contrast agent images, and displays the generated n cumulative ultrasound contrast agent images, wherein t_k satisfies $t_k > t_{k-1}$.

FIG. 4

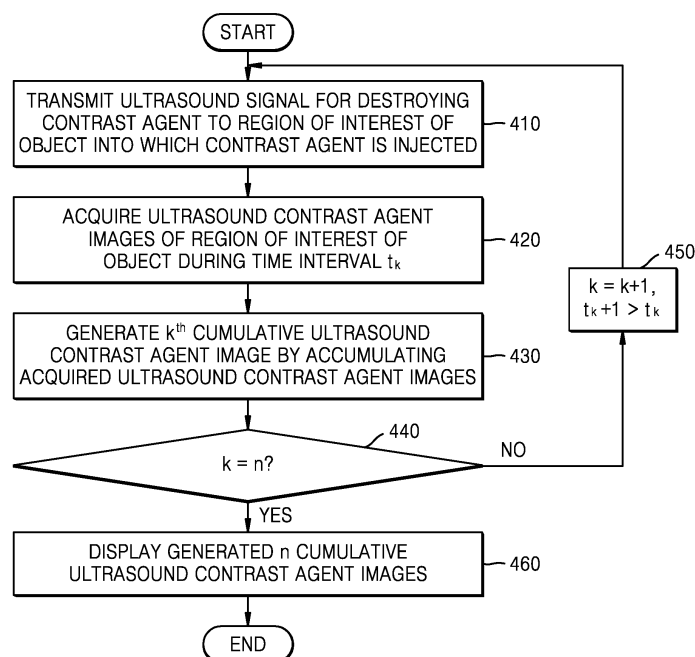

Description

CROSS-REFERENCE TO RELATED APPLICATION(S)

[0001] This application is based on and claims priority under 35 U.S.C. §119 to Korean Patent Application No. 10-2018-0018062, filed on February 13, 2018, in the Korean Intellectual Property Office, the disclosure of which is incorporated by reference herein in its entirety.

BACKGROUND

1. Field

[0002] The disclosure relates to an ultrasound imaging apparatus and a method of controlling the ultrasound imaging apparatus.

2. Description of Related Art

[0003] Ultrasound diagnostic apparatuses transmit, to an object, ultrasound signals generated by transducers of a probe and detect information about signals reflected from the object, thereby obtaining at least one image of an internal part, for example, soft tissue or blood flow, of the object.

[0004] In addition, ultrasound diagnosis apparatuses utilize ultrasound contrast agents made of micro-bubbles to obtain ultrasound contrast agent images for diagnosis of various lesions. The ultrasound contrast agents made of micro-bubbles act as reflectors that are robust against ultrasound signals. Therefore, since echo signals reflected from the ultrasound contrast agents are stronger than other general echo signals, information about blood vessels into which the contrast agents are injected may be obtained in more detail through the ultrasound contrast agent images.

SUMMARY

[0005] Provided are ultrasound imaging apparatuses for providing a user with ultrasound contrast agent images of an object and methods of controlling the ultrasound imaging apparatuses.

[0006] Provided are ultrasound imaging apparatuses for providing an image obtained by accumulating a plurality of ultrasound contrast agent images for a region of interest of an object and methods of controlling the ultrasound imaging apparatuses.

[0007] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0008] In accordance with an aspect of the disclosure, an ultrasound imaging apparatus includes: a probe configured to transmit an ultrasound signal to an object and detect an echo signal; one or more processors configured to acquire a plurality of ultrasound contrast agent images

for a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted through the probe to the region of interest of the object, into which the contrast agent is injected, at time intervals of t_k ($k = 1, 2, \dots, n$, and n is an integer of 2 or more), generate a k^{th} cumulative ultrasound contrast agent image by accumulating the plurality of acquired ultrasound contrast agent images at every time intervals of t_k to generate n cumulative ultrasound contrast agent images; and a display configured to display the generated n cumulative ultrasound contrast agent images, wherein t_k satisfies $t_k > t_{k-1}$.

[0009] A sound pressure of the ultrasound signal may be determined based on an energy level for destroying the contrast agent.

[0010] The ultrasound imaging apparatus may further include an input interface configured to receive a user input of setting t_k and n , wherein the one or more processors are further configured to set t_k and n based on the user input.

[0011] The ultrasound imaging apparatus may further include a storage storing the plurality of acquired ultrasound contrast agent images and the k^{th} cumulative ultrasound contrast agent image.

[0012] The one or more processors may be further configured to correct shaking of the plurality of ultrasound contrast agent images according to movement of the object.

[0013] The one or more processors may be further configured to generate one video edited so that the n cumulative ultrasound contrast agent images are sequentially reproduced, and the display may be further configured to display the video.

[0014] The one or more processors may be further configured to generate first to n^{th} total cumulative ultrasound contrast agent images by performing, n times from $k=1$ to $k=n$, a process of generating a k^{th} total cumulative ultrasound contrast agent image obtained by accumulating first to k^{th} cumulative ultrasound contrast agent images, and the display may be further configured to display the first to n^{th} total cumulative ultrasound contrast agent images.

[0015] The one or more processors may be further configured to generate one video edited so that the first to n^{th} total cumulative ultrasound contrast agent images are sequentially reproduced, and the display may be further configured to display the video.

[0016] In accordance with another aspect of the disclosure, an ultrasound imaging apparatus includes: a probe configured to transmit an ultrasound signal to an object and detect an echo signal; one or more processors configured to acquire f_k ultrasound contrast agent images for a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted through the probe to the region of interest of the object into which the contrast agent is injected ($k = 1, 2, \dots, n$, and n is an integer of 2 or more), and generate n cumulative ultrasound contrast agent images by performing, n times

from $k=1$ to $k=n$, a process of generating a k^{th} cumulative ultrasound contrast agent image by accumulating the acquired f_k ultrasound contrast agent images; and a display configured to display the generated n cumulative ultrasound contrast agent images, wherein f_k satisfies $f_k > f_{k-1}$.

[0017] In accordance with another aspect of the disclosure, a method of controlling an ultrasound imaging apparatus includes: acquiring a plurality of ultrasound contrast agent images for a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted to the region of interest of the object, into which the contrast agent is injected, at time intervals of t_k ($k=1, 2, \dots, n$, and n is an integer of 2 or more), generating a k^{th} cumulative ultrasound contrast agent image by accumulating the plurality of acquired ultrasound contrast agent images at every time intervals of t_k to generate n cumulative ultrasound contrast agent images; and displaying the generated n cumulative ultrasound contrast agent images, wherein t_k satisfies $t_k > t_{k-1}$.

BRIEF DESCRIPTION OF THE DRAWINGS

[0018] The above and other aspects, features, and advantages of certain embodiments of the present disclosure will be more apparent from the following description taken in conjunction with the accompanying drawings, in which:

FIG. 1 is a block diagram illustrating an ultrasound diagnosis apparatus according to an exemplary embodiment;

FIGS. 2A, 2B, and 2C are diagrams respectively illustrating an ultrasound diagnosis apparatus according to an exemplary embodiment;

FIG. 3 is a block diagram illustrating an ultrasound imaging apparatus according to an embodiment;

FIG. 4 is a flowchart of a method by which an ultrasound imaging apparatus displays a cumulative ultrasound contrast agent image of a region of interest of an object, according to an embodiment;

FIG. 5 is a flowchart of a method by which an ultrasound imaging apparatus generates and displays a cumulative ultrasound contrast agent image of a region of interest of an object, according to an embodiment;

FIG. 6 is a diagram illustrating an example of an ultrasound signal transmitted to an object by an ultrasound imaging apparatus, according to an embodiment;

FIG. 7 is a diagram illustrating an example in which the number of ultrasound contrast agent bubbles of an object is changed as an ultrasound imaging apparatus transmits an ultrasound signal to an object; FIG. 8 is a diagram illustrating an example in which an ultrasound imaging apparatus displays a cumulative ultrasound contrast agent image of a region of interest of an object, according to an embodiment; and

FIG. 9 is a diagram illustrating an example of a video edited so that an ultrasound imaging apparatus sequentially reproduces a plurality of cumulative ultrasound contrast agent images of a region of interest of an object, according to an embodiment.

DETAILED DESCRIPTION

[0019] Reference will now be made in detail to embodiments, examples of which are illustrated in the accompanying drawings, wherein like reference numerals refer to like elements throughout. In this regard, the present embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein. Accordingly, the embodiments are merely described below, by referring to the figures, to explain aspects. As used herein, the term "and/or" includes any and all combinations of one or more of the associated listed items.

[0020] Certain exemplary embodiments are described in greater detail below with reference to the accompanying drawings.

[0021] In the following description, the same drawing reference numerals are used for the same elements even in different drawings. The matters defined in the description, such as detailed construction and elements, are provided to assist in a comprehensive understanding of exemplary embodiments. However, it is to be understood that exemplary embodiments can be carried out without such specifically defined matters. Also, well-known functions or constructions are not described in detail since they may obscure exemplary embodiments with unnecessary detail.

[0022] Terms such as "part" and "portion" used herein denote entities that may be embodied by software or hardware. According to exemplary embodiments, a plurality of parts or portions may be embodied by a single unit or element, or a single part or portion may include a plurality of elements.

[0023] In exemplary embodiments, an image may include any medical image acquired by various medical imaging apparatuses such as a magnetic resonance imaging (MRI) apparatus, a computed tomography (CT) apparatus, an ultrasound imaging apparatus, or an X-ray apparatus.

[0024] Also, in the present specification, an "object", which is a thing to be imaged, may include a human, an animal, or a part thereof. For example, an object may include a part of a human, that is, an organ or a tissue, or a phantom.

[0025] Throughout the specification, an ultrasound image refers to an image of an object processed based on ultrasound signals transmitted to the object and reflected therefrom.

[0026] FIG. 1 is a block diagram illustrating a configuration of an ultrasound diagnosis apparatus 100, i.e., a diagnostic apparatus, according to an exemplary embodiment.

[0027] Referring to FIG. 1, the ultrasound diagnosis apparatus 100 may include a probe 20, an ultrasound transceiver 110, a controller 120, an image processor 130, one or more displays 140, a storage 150, e.g., a memory, a communicator 160, i.e., a communication device or an interface, and an input interface 170.

[0028] The ultrasound diagnosis apparatus 100 may be of a cart-type or a portable-type ultrasound diagnosis apparatus, that is portable, moveable, mobile, or handheld. Examples of the portable-type ultrasound diagnosis apparatus 100 may include a smart phone, a laptop computer, a personal digital assistant (PDA), and a tablet personal computer (PC), each of which may include a probe and a software application, but embodiments are not limited thereto.

[0029] The probe 20 may include a plurality of transducers. The plurality of transducers may transmit ultrasound signals to an object 10 in response to transmitting signals received by the probe 20, from a transmitter 113. The plurality of transducers may receive ultrasound signals reflected from the object 10 to generate reception signals. In addition, the probe 20 and the ultrasound diagnosis apparatus 100 may be formed in one body (e.g., arranged in a single housing), or the probe 20 and the ultrasound diagnosis apparatus 100 may be formed separately (e.g., arranged separately in separate housings) but linked by wire or wirelessly. In addition, the ultrasound diagnosis apparatus 100 may include one or more probes 20 according to embodiments.

[0030] The controller 120 may control the transmitter 113 for the transmitter 113 to generate transmitting signals to be applied to each of the plurality of transducers based on a position and a focal point of the plurality of transducers included in the probe 20.

[0031] The controller 120 may control the ultrasound receiver 115 to generate ultrasound data by converting reception signals received from the probe 20 from analogue to digital signals and summing the reception signals converted into digital form, based on a position and a focal point of the plurality of transducers.

[0032] The image processor 130 may generate an ultrasound image by using ultrasound data generated from the ultrasound receiver 115.

[0033] The display 140 may display a generated ultrasound image and various pieces of information processed by the ultrasound diagnosis apparatus 100. The ultrasound diagnosis apparatus 100 may include two or more displays 140 according to the present exemplary embodiment. The display 140 may include a touch screen in combination with a touch panel.

[0034] The controller 120 may control the operations of the ultrasound diagnosis apparatus 100 and flow of signals between the internal elements of the ultrasound diagnosis apparatus 100. The controller 120 may include a memory for storing a program or data to perform functions of the ultrasound diagnosis apparatus 100 and a processor and/or a microprocessor (not shown) for processing the program or data. For example, the con-

troller 120 may control the operation of the ultrasound diagnosis apparatus 100 by receiving a control signal from the input interface 170 or an external apparatus.

[0035] The ultrasound diagnosis apparatus 100 may include the communicator 160 and may be connected to external apparatuses, for example, servers, medical apparatuses, and portable devices such as smart phones, tablet personal computers (PCs), wearable devices, etc., via the communicator 160.

[0036] The communicator 160 may include at least one element capable of communicating with the external apparatuses. For example, the communicator 160 may include at least one among a short-range communication module, a wired communication module, and a wireless communication module.

[0037] The communicator 160 may receive a control signal and data from an external apparatus and transmit the received control signal to the controller 120 so that the controller 120 may control the ultrasound diagnosis apparatus 100 in response to the received control signal.

[0038] The controller 120 may transmit a control signal to the external apparatus via the communicator 160 so that the external apparatus may be controlled in response to the control signal of the controller 120.

[0039] For example, the external apparatus connected to the ultrasound diagnosis apparatus 100 may process the data of the external apparatus in response to the control signal of the controller 120 received via the communicator 160.

[0040] A program for controlling the ultrasound diagnosis apparatus 100 may be installed in the external apparatus. The program may include instructions to perform part of an operation of the controller 120 or the entire operation of the controller 120.

[0041] The program may be pre-installed in the external apparatus or may be installed by a user of the external apparatus by downloading the program from a server that provides applications. The server that provides applications may include a recording medium where the program is stored.

[0042] The storage 150 may store various data or programs for driving and controlling the ultrasound diagnosis apparatus 100, input and/or output ultrasound data, ultrasound images, applications, etc.

[0043] The input interface 170 may receive a user's input to control the ultrasound diagnosis apparatus 100 and may include a keyboard, button, keypad, mouse, trackball, jog switch, knob, a touchpad, a touch screen, a microphone, a motion input means, a biometrics input means, etc. For example, the user's input may include inputs for manipulating buttons, keypads, mice, trackballs, jog switches, or knobs, inputs for touching a touchpad or a touch screen, a voice input, a motion input, and a bioinformation input, for example, iris recognition or fingerprint recognition, but an exemplary embodiment is not limited thereto.

[0044] An example of the ultrasound diagnosis apparatus 100 according to the present exemplary embodi-

ment is described below with reference to FIGS. 2A, 2B, and 2C.

[0045] FIGS. 2A, 2B, and 2C are diagrams respectively illustrating an ultrasound diagnosis apparatus according to an exemplary embodiment.

[0046] Referring to FIGS. 2A and 2B, the ultrasound diagnosis apparatus 100 may include a main display 121 and a sub-display 122. At least one among the main display 121 and the sub-display 122 may include a touch screen. The main display 121 and the sub-display 122 may display ultrasound images and/or various information processed by the ultrasound diagnosis apparatus 100. The main display 121 and the sub-display 122 may provide graphical user interfaces (GUIs), thereby receiving a user's inputs of data to control the ultrasound diagnosis apparatus 100. For example, the main display 121 may display an ultrasound image and the sub-display 122 may display a control panel to control display of the ultrasound image as a GUI. The sub-display 122 may receive an input of data to control the display of an image through the control panel displayed as a GUI. The ultrasound diagnosis apparatus 100 may control the display of the ultrasound image on the main display 121 by using the input control data.

[0047] Referring to FIG. 2B, the ultrasound diagnosis apparatus 100 may include a control panel 165. The control panel 165 may include buttons, trackballs, jog switches, or knobs, and may receive data to control the ultrasound diagnosis apparatus 100 from the user. For example, the control panel 165 may include a time gain compensation (TGC) button 171 and a freeze button 172. The TGC button 171 is to set a TGC value for each depth of an ultrasound image. Also, when an input of the freeze button 172 is detected during scanning an ultrasound image, the ultrasound diagnosis apparatus 100 may keep displaying a frame image at that time point.

[0048] The buttons, trackballs, jog switches, and knobs included in the control panel 165 may be provided as a GUI to the main display 121 or the sub-display 122.

[0049] Referring to FIG. 2C, the ultrasound diagnosis apparatus 100 may include a portable device. An example of the portable ultrasound diagnosis apparatus 100 may include, for example, smart phones including probes and applications, laptop computers, personal digital assistants (PDAs), or tablet PCs, but an exemplary embodiment is not limited thereto.

[0050] The ultrasound diagnosis apparatus 100 may include the probe 20 and a main body 40. The probe 20 may be connected to one side of the main body 40 by wire or wirelessly. The main body 40 may include a touch screen 145. The touch screen 145 may display an ultrasound image, various pieces of information processed by the ultrasound diagnosis apparatus 100, and a GUI.

[0051] FIG. 3 is a block diagram illustrating an ultrasound imaging apparatus 300 according to an embodiment. The ultrasound imaging apparatus 300 may correspond to the ultrasound diagnosis apparatus 100 of FIG. 1. In addition, the ultrasound imaging apparatus 300

may be implemented in the form of the ultrasound diagnosis apparatuses 100a, 100b, and 100c.

[0052] As illustrated in FIG. 3, the ultrasound imaging apparatus 300 may include a probe 310, a processor 320, and a display 330. The probe 310 may correspond to the probe 20 of FIG. 1. The processor 320 may correspond to the controller 120 and the image processor 130 of FIG. 1. The display 330 may correspond to the display 140 of FIG. 1. In addition, the processor 320 may include one or more processors.

[0053] The probe 310 may transmit an ultrasound signal to an object and detect an echo signal. According to an embodiment, the probe 310 may transmit an ultrasound signal to a region of interest of an object into which a contrast agent is injected, and detect a contrast agent signal reflected from the contrast agent as an echo signal. For example, the probe 310 may transmit an ultrasound signal to a region of interest of an object while a contrast agent is injected into the region of interest of the object and the contrast agent is rising, and may detect, as an echo signal, a contrast agent signal for the rising contrast agent and a contrast agent signal for a state in which the contrast agent has risen.

[0054] According to an embodiment, the ultrasound signal transmitted to the object by the probe 310 so as to detect the echo signal may be an ultrasound signal of a sound pressure having an energy level that does not destroy the contrast agent. Therefore, the contrast agent injected into the object may not be destroyed by the ultrasound signal transmitted to the object by the probe 310 so as to detect the echo signal.

[0055] The probe 310 may transmit an ultrasound signal for destroying the contrast agent to the object. According to an embodiment, the probe 310 may destroy the contrast agent by transmitting an ultrasound signal of a sound pressure having an energy level for destroying the contrast agent to the region of interest of the object into which the contrast agent is injected. For example, the probe 310 may destroy the contrast agent by transmitting the ultrasound signal having a high sound pressure for destroying the contrast agent.

[0056] According to an embodiment, the probe 310 may transmit an ultrasound signal to a region of interest of an object while a contrast agent is rising again in the region of interest of the object after the contrast agent is destroyed, and may detect a contrast agent signal for the rising contrast agent as an echo signal. When the contrast agent is destroyed by transmitting the ultrasound signal having a high sound pressure to the region of interest of the object in which the contrast agent has risen, the contrast agent rises again in the region of interest of the object for a predetermined time. Therefore, the probe 310 may detect, as an echo signal, a plurality of contrast agent signals when the contrast agent rises in the region of interest of the object by transmitting the ultrasound signal to the object for a predetermined time after the contrast agent is destroyed.

[0057] The processor 320 may control the probe 310

to destroy the contrast agent by transmitting the ultrasound signal for destroying the contrast agent to the region of interest of the object into which the contrast agent is injected, and to detect a plurality of contrast agent signals.

[0058] According to an embodiment, the processor 320 may control the probe 310 to detect a plurality of contrast agent signals by transmitting an ultrasound signal for detecting the plurality of contrast agent signals to a region of interest of an object in which the contrast agent is rising again after an ultrasound signal for destroying the contrast agent is transmitted to the region of interest of the object, into which the contrast agent is injected, at time intervals of t_k . In other words, the processor 320 may control the probe 310 to perform the process of detecting the plurality of contrast agent signals n times from $k=1$ to $k=n$ during the time interval of t_k after the contrast agent is destroyed.

[0059] According to an embodiment, the processor 320 may control the probe 310 to detect f_k contrast agent signals by transmitting an ultrasound signal for detecting the plurality of contrast agent signals to a region of interest of an object in which the contrast agent is rising again after an ultrasound signal for destroying the contrast agent is transmitted to the region of interest of the object into which the contrast agent is injected. In other words, the processor 320 may control the probe 310 to perform the process of detecting f_k contrast agent signals n times from $k=1$ to $k=n$ after the contrast agent is destroyed.

[0060] The processor 320 may set the time interval of t_k to detect the plurality of contrast agent signals after the contrast agent is destroyed. According to an embodiment, the processor 320 may set t_k based on an input of setting t_k which is received through an input interface (not illustrated). For example, t_k may be set to a predetermined time based on an input of setting t_k to a predetermined time (for example, 5 ms), which is received through the input interface. In addition, t_k may be set to increase as k increases based on an input of setting t_k to satisfy $t_k > t_{k-1}$, which is received through the input interface.

[0061] According to an embodiment, the processor 320 may automatically set t_k by taking into account the time at which the contrast agent rises in the region of interest of the object after the contrast agent is destroyed, the property of the object, and the number of cumulative ultrasound contrast agent images necessary for lesion diagnosis.

[0062] The processor 320 may set the number f_k of contrast agent signals detected by the probe 310 after the contrast agent is destroyed. According to an embodiment, the processor 320 may set f_k based on an input of setting f_k , which is received through the input interface. For example, f_k may be set to a predetermined number based on an input of setting f_k to a predetermined number (for example, 5), which is received through the input interface. In addition, f_k may be set to increase as k increases based on an input of setting f_k to satisfy $f_k > f_{k-1}$, which is received through the input interface.

[0063] According to an embodiment, the processor 320 may automatically set f_k by taking into account the time at which the contrast agent rises to the region of interest of the object after the contrast agent is destroyed, the property of the object, and the number of cumulative ultrasound contrast agent images necessary for lesion diagnosis.

[0064] According to an embodiment, when the processor 320 differently sets t_k and f_k , the probe 310 may detect contrast agent signals having different degrees of the rising of the contrast agent in the region of interest of the object. When the processor 320 sets t_k to be longer or sets f_k to be greater, the time for the probe 310 to detect the contrast agent signal after the contrast agent is destroyed is prolonged. In addition, as the time passes by, the contrast agent moves through the bloodstream and the degree of the rising of the contrast agent is changed. Therefore, the processor 320 sets t_k to be gradually longer or sets f_k to be gradually greater, so that the probe 310 detects a plurality of contrast agent signals after the contrast agent is destroyed. Thus, the probe 310 may detect contrast agent signals having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by.

[0065] The processor 320 may generate the ultrasound contrast agent image by using the contrast agent signal detected by the probe 310. According to an embodiment, the processor 320 may generate a plurality of ultrasound contrast agent images by using a plurality of contrast agent signals detected during the time interval of t_k by the probe 310 after the contrast agent is destroyed. Since the probe 310 is capable of, under the control of the processor 320, repeating the process of detecting the contrast agent signals n times from $k=1$ to $k=n$ during the time interval of t_k after the contrast agent is destroyed, the processor 320 may generate the ultrasound contrast agent images by using the contrast agent signals detected through the probe 310 with respect to each of n -time repetitions.

[0066] According to an embodiment, the processor 320 may generate f_k ultrasound contrast agent images by using f_k contrast agent signals detected by the probe 310 after the contrast agent is destroyed. Since the probe 310 is capable of, under the control of the processor 320, repeating the process of detecting f_k contrast agent signals n times from $k=1$ to $k=n$ after the contrast agent is destroyed, the processor 320 may generate f_k ultrasound contrast agent images by using the contrast agent signals detected by the probe 310 with respect to each of n -time repetitions.

[0067] The processor 320 may generate a cumulative ultrasound contrast agent image by accumulating a plurality of ultrasound contrast agent images. According to an embodiment, the processor 320 may generate a cumulative ultrasound contrast agent image by accumulating a plurality of ultrasound contrast agent images generated by using a plurality of contrast agent signals detected during the time interval of t_k by the probe 310 after

the contrast agent is destroyed. In addition, the processor 320 may generate n cumulative ultrasound contrast agent images by performing, n times from k=1 to k=n, a process of generating a cumulative ultrasound contrast agent image by accumulating a plurality of ultrasound contrast agent images generated by using a plurality of contrast agent signals detected during the time interval of t_k by the probe 310 after the contrast agent is destroyed.

[0068] According to an embodiment, the processor 320 may generate a cumulative ultrasound contrast agent image by accumulating f_k ultrasound contrast agent images generated by using f_k contrast agent signals detected by the probe 310 after the contrast agent is destroyed. In addition, the processor 320 may generate n cumulative ultrasound contrast agent images by performing, n times from k=1 to k=n, a process of generating a cumulative ultrasound contrast agent image by accumulating f_k ultrasound contrast agent images generated by using f_k contrast agent signals detected by the probe 310 after the contrast agent is destroyed.

[0069] The n cumulative ultrasound contrast agent images generated herein may be ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object according to t_k or f_k set by the processor 320. In particular, when the processor 320 sets t_k to be gradually longer or sets f_k to be gradually greater so that the probe 310 detects a plurality of contrast agent signals after the contrast agent is destroyed, the processor 320 may use the detected contrast agent signals to generate, step by step, cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object as the times passes by.

[0070] That is, according to an embodiment, the position at which the contrast agent begins to rise in the region of interest of the object and the shape thereof may be identified through the cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by. Information necessary for lesion diagnosis may be obtained by identifying the position at which the contrast agent begins to rise and the shape thereof. For example, in the case of focal nodular hyperplasia (FNH) and adenoma, which are the lesions present in the liver, the two lesions are difficult to distinguish from each other since the two lesions show very similar characteristics. However, for the contrast agent images, the two lesions show distinctive characteristics in terms of the position at which the contrast agent rises and the shape thereof. Therefore, the two lesions may be distinguished and diagnosed by identifying the distinctive characteristics. Therefore, according to the disclosed embodiment, the lesions may be easily diagnosed by identifying the position at which the contrast agent begins to rise and the shape thereof.

[0071] According to an embodiment, the processor 320 may generate a cumulative ultrasound contrast

agent image by accumulating all or part of the generated n cumulative ultrasound contrast agent images again (indicating first to n^{th} cumulative ultrasound contrast agent images in the disclosure). For example, the processor 320 may additionally generate n cumulative ultrasound contrast agent images (indicating first to n^{th} total cumulative ultrasound contrast agent images in the disclosure) by performing, n times from k=1 to k=n, a process of generating a cumulative ultrasound contrast agent image by accumulating first to k^{th} cumulative ultrasound contrast agent images.

[0072] When the first to k^{th} cumulative ultrasound contrast agent images are cumulative ultrasound contrast agent images having stepwise different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by, the additionally generated first to n^{th} total cumulative ultrasound contrast agent images may also be cumulative ultrasound contrast agent images having stepwise different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by.

[0073] According to an embodiment, the additionally generated n cumulative ultrasound contrast agent images (the first to n^{th} total cumulative ultrasound contrast agent images) may be images obtained by accumulating contrast agent images with respect to a short time at which the contrast agent begins to rise immediately after the contrast agent is destroyed. Therefore, the additionally generated n cumulative ultrasound contrast agent images are images in which the position where the contrast agent begins to initially rise are shown more clearly than other positions within the region of interest of the object, and the position where the contrast agent begins to rise may be more clearly identified through these images.

[0074] According to an embodiment, the processor 320 may generate a cumulative ultrasound contrast agent image by selectively accumulating only part of a plurality of generated ultrasound contrast agent images. For example, the processor 320 may generate a cumulative ultrasound contrast agent image by selecting part of a plurality of ultrasound contrast agent images (for example, images having little shaking according to the movement of the object) generated by using a plurality of ultrasound contrast agent signals detected by the probe 310.

[0075] The processor 320 may set the number n of times of repetitions of a series of processes. According to an embodiment, the processor 320 may set n based on an input of setting n, which is received through the input interface. In addition, according to an embodiment, the processor 320 may automatically set n by taking into account the time at which the contrast agent rises in the region of interest of the object after the contrast agent is destroyed, the property of the object, and the number of cumulative ultrasound contrast agent images necessary for lesion diagnosis.

[0076] The processor 320 may correct the shaking of

a plurality of ultrasound contrast agent images according to the movement of the object. The probe 310 may detect a plurality of contrast agent signals during the time interval of t_k under the control of the processor 320, or the object may move during the detection of f_k contrast agent signals. Therefore, the plurality of ultrasound contrast agent images generated by the processor 320 by using the plurality of contrast agent signals detected by the probe 310 may be shaken by the influence of the movement of the object. In this case, the processor 320 may set the image serving as the reference among the plurality of generated ultrasound contrast agent images and correct the shaking of the other ultrasound contrast agent images.

[0077] According to an embodiment, before accumulating the ultrasound contrast agent images, the processor 320 may correct the shaking of the ultrasound contrast agent images according to the movement of the object, so as to generate much clearer cumulative ultrasound contrast agent images.

[0078] The processor 320 may generate one video edited so that a plurality of cumulative ultrasound contrast agent images are sequentially reproduced. According to an embodiment, the processor 320 may generate one video edited so that cumulative ultrasound contrast agent images (including total cumulative ultrasound contrast agent images in the disclosure) having different degrees of the rising of the contrast agent in the region of interest of the object are sequentially reproduced as the time passes by. The position at which the contrast agent begins to rise in the region of interest of the object and the shape of the rising of the contrast agent as the time passes by may be identified through the generated video.

[0079] The processor 320 may store the ultrasound contrast agent image in a storage (not illustrated). According to an embodiment, the processor 320 may store, in the storage, the ultrasound contrast agent images generated by using the signals detected by the probe 310, the cumulative ultrasound contrast agent images, the total cumulative ultrasound contrast agent images, and the video obtained by editing the cumulative ultrasound contrast agent images.

[0080] The display 330 may display the ultrasound contrast agent image. According to an embodiment, the display 330 may sequentially display the n cumulative ultrasound contrast agent images generated by the processor 320 on one screen at the same time. For example, under the control of the processor 320, the display 330 may sequentially display the cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object in the order of time lapse as the time passes by.

[0081] According to an embodiment, the display 330 may display one video edited so that the cumulative ultrasound contrast agent images are sequentially reproduced by the processor 320.

[0082] FIG. 4 is a flowchart of a method by which the ultrasound imaging apparatus 300 generates and dis-

plays a cumulative ultrasound contrast agent image of a region of interest of an object, according to an embodiment.

[0083] Referring to FIG. 4, a method of generating and displaying a cumulative ultrasound contrast agent image of a region of interest of an object, according to an embodiment, may include operations processed in time series by the ultrasound imaging apparatus 300 illustrated in FIG. 3. Therefore, even though omitted below, the description provided for the ultrasound imaging apparatus 300 illustrated in FIG. 3 may be applied to the method of generating and displaying the cumulative ultrasound contrast agent image of the region interest of the object as illustrated in FIG. 4.

[0084] In operation 410, the ultrasound imaging apparatus 300 transmits an ultrasound signal for destroying a contrast agent to a region of interest of an object into which the contrast agent is injected. A sound pressure of the transmitted ultrasound signal may have an energy level capable of destroying the contrast agent. The contrast agent injected into the region of interest of the object may be destroyed by the transmitted ultrasound signal.

[0085] In operation 420, the ultrasound imaging apparatus 300 acquires a plurality of ultrasound contrast agent images of the region of interest of the object during the time interval of t_k . At this time, the ultrasound imaging apparatus 300 may acquire a plurality of ultrasound contrast agent images based on a plurality of contrast agent signals for the region of interest of the object detected during the time interval of t_k .

[0086] In operation 430, the ultrasound imaging apparatus 300 generates a k^{th} cumulative ultrasound contrast agent image by accumulating the acquired ultrasound contrast agent images.

[0087] In operation 440, the ultrasound imaging apparatus 300 determines whether operations 410 to 430 are repeated n times (that is, whether $k=n$). In operation 450, when the number of times of repetitions is not n , the ultrasound imaging apparatus 300 sets t_{k+1} to satisfy $t_{k+1} > t_k$ and repeats operations 410 to 430.

[0088] In operation 460, when the ultrasound imaging apparatus 300 repeats operations 410 to 430 n times, the ultrasound imaging apparatus 300 displays the n cumulative ultrasound contrast agent images.

[0089] FIG. 5 is a flowchart of a method by which the ultrasound imaging apparatus 300 generates and displays a cumulative ultrasound contrast agent image of a region of interest of an object, according to an embodiment.

[0090] Referring to FIG. 5, a method of generating and displaying a cumulative ultrasound contrast agent image of a region of interest of an object, according to another embodiment, may include operations processed in time series by the ultrasound imaging apparatus 300 illustrated in FIG. 3. Therefore, even though omitted below, the description provided for the ultrasound imaging apparatus 300 illustrated in FIG. 3 may be applied to the method of generating and displaying the cumulative ultrasound

contrast agent image of the region interest of the object as illustrated in FIG. 5.

[0091] In operation 510, the ultrasound imaging apparatus 300 transmits an ultrasound signal for destroying a contrast agent to a region of interest of an object into which the contrast agent is injected. A sound pressure of the transmitted ultrasound signal may have an energy level capable of destroying the contrast agent. The contrast agent injected into the region of interest of the object may be destroyed by the transmitted ultrasound signal.

[0092] In operation 520, the ultrasound imaging apparatus 300 acquires f_k ultrasound contrast agent images of the region of interest of the object. At this time, the ultrasound imaging apparatus 300 may acquire f_k ultrasound contrast agent images based on f_k contrast agent signals detected for the region of interest of the object.

[0093] In operation 530, the ultrasound imaging apparatus 300 generates a k^{th} cumulative ultrasound contrast agent image by accumulating the acquired f_k ultrasound contrast agent images.

[0094] In operation 540, the ultrasound imaging apparatus 300 determines whether operations 510 to 530 are repeated n times (that is, whether $k=n$). In operation 550, when the number of times of repetitions is not n , the ultrasound imaging apparatus 300 sets f_{k+1} to satisfy $f_{k+1} > f_k$ and repeats operations 510 to 530.

[0095] In operation 560, when the ultrasound imaging apparatus 300 repeats operations 510 to 530 n times, the ultrasound imaging apparatus 300 displays n cumulative ultrasound contrast agent images.

[0096] FIG. 6 is a diagram illustrating an example of an ultrasound signal transmitted to an object by the ultrasound imaging apparatus 300, according to an embodiment.

[0097] As illustrated in FIG. 6, the ultrasound imaging apparatus 300 according to the embodiment transmits, to an object, an ultrasound signal 610 for destroying a contrast agent and an ultrasound signal 620 for detecting a contrast agent signal (that is, an echo signal). The ultrasound signal 610 for destroying the contrast agent has an energy level capable of destroying the contrast agent and is illustrated in FIG. 6 as having a high sound pressure. The ultrasound signal 620 for detecting the contrast agent signal has an energy level capable of detecting the contrast agent signal and is illustrated in FIG. 6 as having a relative low sound pressure, as compared with the ultrasound signal 610 for destroying the contrast agent.

[0098] In addition, as illustrated in FIG. 6, the ultrasound imaging apparatus 300 according to the embodiment transmits the ultrasound signal 610 for destroying the contrast agent to the region of interest of the object at time intervals of t_k , and transmits the ultrasound signal 620 for detecting the contrast agent signal to the region of interest of the object during the time interval of t_k after the ultrasound signal 620 for destroying the contrast agent is transmitted (that is, after the contrast agent is destroyed). The ultrasound imaging apparatus 300 may detect the contrast agent signal as the echo signal for

each transmitted ultrasound signal 620 for detecting the contrast agent signal.

[0099] FIG. 6 illustrates an example in which the ultrasound imaging apparatus 300 sets t_k to satisfy $t_{k+1} > t_k$, according to an embodiment. It can be seen from FIG. 6 that as k increases, the time interval t_k also increases, and as the time interval t_k increases, more ultrasound signals 620 for detecting the contrast agent signals are transmitted. Therefore, the example illustrated in FIG. 6 may be an example of an ultrasound signal transmitted to an object by the ultrasound imaging apparatus 300 when the ultrasound imaging apparatus 300 generates, step by step, cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by.

[0100] FIG. 7 is a diagram illustrating an example in which the number of ultrasound contrast agent bubbles of an object is changed as the ultrasound imaging apparatus 300 transmits an ultrasound signal to an object.

[0101] As illustrated in FIG. 7, the ultrasound imaging apparatus 300 according to the embodiment transmits an ultrasound signal for destroying a contrast agent to a region of interest of an object at time intervals of t_k , so as to destroy the contrast agent of the region of interest of the object at the time intervals of t_k .

[0102] Referring to FIG. 7, the number of ultrasound contrast agent bubbles in the region of interest of the region approaches to zero when the ultrasound signal for destroying the contrast agent is transmitted to the region of interest of the object and the contrast agent is destroyed, and the number of ultrasound contrast agent bubbles in the region of interest of the object is increased since the ultrasound contrast agent rises again during the time interval of t_k after the contrast agent is destroyed.

[0103] FIG. 7 illustrates an example in which the ultrasound imaging apparatus 300 sets t_k to satisfy $t_{k+1} > t_k$, according to an embodiment. It can be seen from FIG. 7 that as k increases, the time interval t_k also increases, and as the time interval t_k increases, a larger number of ultrasound contrast agent bubbles rise. Therefore, the example illustrated in FIG. 7 may be an example in which the number of ultrasound contrast agent bubbles is changed when the ultrasound imaging apparatus 300 generates, step by step, cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by.

[0104] However, the example illustrated in FIG. 7 is merely an example showing that the degree of the rising of the contrast agent in the region of interest of the object is changed according to t_k , and the aspect of the rising of the contrast agent after the contrast agent is destroyed may be differently shown by the region of interest of the object, the type of the contrast agent, and the like.

[0105] FIG. 8 is a diagram illustrating an example in which the ultrasound imaging apparatus 300 displays a cumulative ultrasound contrast agent image of a region

of interest of an object, according to an embodiment.

[0106] Referring to FIG. 8, the ultrasound imaging apparatus 300 according to the embodiment displays an ultrasound image 810 before a contrast agent is injected as a control group, and sequentially displays cumulative ultrasound contrast agent images 820 to 860 having different degrees of the rising of the contrast agent in the region of interest of the object in the order of time lapse as the time passes by. The position at which the contrast agent begins to rise in the region of interest of the object and the shape of the rising of the contrast agent as the time passes by may be identified through the cumulative ultrasound contrast agent images 820 to 860 illustrated in FIG. 8.

[0107] According to an embodiment, since the cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by are sequentially displayed in the order of time lapse, the position at which the contrast agent begins to initially rise in the region of interest of the object may be clearly identified, and the shape of the rising of the contrast agent may also be clearly identified.

[0108] FIG. 9 is a diagram illustrating an example of a video edited so that the ultrasound imaging apparatus 300 sequentially reproduces a plurality of cumulative ultrasound contrast agent images of a region of interest of an object, according to an embodiment.

[0109] When a video is started, the ultrasound imaging apparatus 300 according to the embodiment may reproduce an ultrasound image 910 before a contrast agent is injected as a control group. The ultrasound imaging apparatus 300 may edit the video so that cumulative ultrasound contrast agent images 920 to 960 having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by are sequentially reproduced (for example, reproduced at the corresponding elapsed time (for example, t_k)). An example of the edited video is illustrated in FIG. 9. The position at which the contrast agent begins to rise in the region of interest of the object and the shape of the rising of the contrast agent as the time passes by may be identified through the video obtained by editing the cumulative ultrasound contrast agent images 920 to 960 illustrated in FIG. 9.

[0110] According to an embodiment, the position at which the contrast agent begins to initially rise in the region of interest of the object and the shape of the rising of the contrast agent may be clearly identified through the video edited so that the cumulative ultrasound contrast agent images having different degrees of the rising of the contrast agent in the region of interest of the object as the time passes by are sequentially displayed in the order of time lapse.

[0111] The disclosed embodiments may be embodied in the form of a non-transitory computer-readable recording medium having recorded thereon instructions and data executable by a computer. The instructions may be

stored in the form of a program code, and when executed by a processor, a predetermined program module may be generated to perform a predetermined operation. In addition, the instructions, when executed by the processor, may perform certain operations of the disclosed embodiments.

[0112] It should be understood that embodiments described herein should be considered in a descriptive sense only and not for purposes of limitation. Descriptions of features or aspects within each embodiment should typically be considered as available for other similar features or aspects in other embodiments.

[0113] While one or more embodiments have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope as defined by the following claims.

Claims

1. An ultrasound imaging apparatus comprising:
 - a probe configured to transmit an ultrasound signal to an object and detect an echo signal;
 - one or more processors configured to acquire a plurality of ultrasound contrast agent images of a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted through the probe to the region of interest of the object, into which the contrast agent is injected, at time intervals of t_k ($k = 1, 2, \dots, n$, and n is an integer of 2 or more), generate a k^{th} cumulative ultrasound contrast agent image by accumulating the plurality of acquired ultrasound contrast agent images at every time intervals of t_k to generate n cumulative ultrasound contrast agent images; and
 - a display configured to display the generated n cumulative ultrasound contrast agent images, wherein t_k satisfies $t_k > t_{k-1}$.
2. The ultrasound imaging apparatus of claim 1, wherein a sound pressure of the ultrasound signal is determined based on an energy level for destroying the contrast agent.
3. The ultrasound imaging apparatus of claim 1, further comprising an input interface configured to receive a user input of setting t_k and n , wherein the one or more processors are further configured to set t_k and n based on the user input.
4. The ultrasound imaging apparatus of claim 1, further comprising a storage storing the plurality of acquired ultrasound contrast agent images and the k^{th} cumulative ultrasound contrast agent image.

5. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to correct shaking of the plurality of ultrasound contrast agent images according to movement of the object.
6. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to generate one video edited so that the n cumulative ultrasound contrast agent images are sequentially reproduced, and the display is further configured to display the video.
7. The ultrasound imaging apparatus of claim 1, wherein the one or more processors are further configured to generate first to nth total cumulative ultrasound contrast agent images by performing, n times from k=1 to k=n, a process of generating a kth total cumulative ultrasound contrast agent image obtained by accumulating first to kth cumulative ultrasound contrast agent images, and the display is further configured to display the first to nth total cumulative ultrasound contrast agent images.
8. The ultrasound imaging apparatus of claim 7, wherein the one or more processors are further configured to generate one video edited so that the first to nth total cumulative ultrasound contrast agent images are sequentially reproduced, and the display is further configured to display the video.
9. An ultrasound imaging apparatus comprising:
 a probe configured to transmit an ultrasound signal to an object and detect an echo signal;
 one or more processors configured to acquire f_k ultrasound contrast agent images of a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted through the probe to the region of interest of the object, into which the contrast agent is injected (k 1, 2, ..., n, and n is an integer of 2 or more), and generate n cumulative ultrasound contrast agent images by performing, n times from k=1 to k=n, a process of generating a kth cumulative ultrasound contrast agent image by accumulating the acquired f_k ultrasound contrast agent images; and
 a display configured to display the generated n cumulative ultrasound contrast agent images, wherein f_k satisfies $f_k > f_{k-1}$.
10. The ultrasound imaging apparatus of claim 9, wherein one or more processors are further configured to generate one video edited so that the n cumulative ultrasound contrast agent images are sequentially reproduced, and the display is further configured to display the video.
11. The ultrasound imaging apparatus of claim 9, wherein the one or more processors are further configured to generate first to nth total cumulative ultrasound contrast agent images by performing, n times from k=1 to k=n, a process of generating a kth total cumulative ultrasound contrast agent image obtained by accumulating first to kth cumulative ultrasound contrast agent images, and the display is further configured to display the first to nth total cumulative ultrasound contrast agent images.
12. A method of controlling an ultrasound imaging apparatus, the method comprising:
 acquiring a plurality of ultrasound contrast agent images of a region of interest of the object after an ultrasound signal for destroying a contrast agent is transmitted to the region of interest of the object, into which the contrast agent is injected, at time intervals of t_k (k 1, 2, ..., n, and n is an integer of 2 or more), generating a kth cumulative ultrasound contrast agent image by accumulating the plurality of acquired ultrasound contrast agent images at every time intervals of t_k to generate n cumulative ultrasound contrast agent images; and
 displaying the generated n cumulative ultrasound contrast agent images, wherein t_k satisfies $t_k > t_{k-1}$.
13. The method of claim 12, further comprising:
 generating one video edited so that the n cumulative ultrasound contrast agent images are sequentially reproduced; and
 displaying the video.
14. The method of claim 12, further comprising:
 generating first to nth total cumulative ultrasound contrast agent images by performing, n times from k=1 to k=n, a process of generating a kth total cumulative ultrasound contrast agent image obtained by accumulating first to kth cumulative ultrasound contrast agent images; and
 displaying the first to nth total cumulative ultrasound contrast agent images.
15. A computer program product comprising a computer-readable storage medium storing instructions for performing the method of claim 12.

FIG. 1

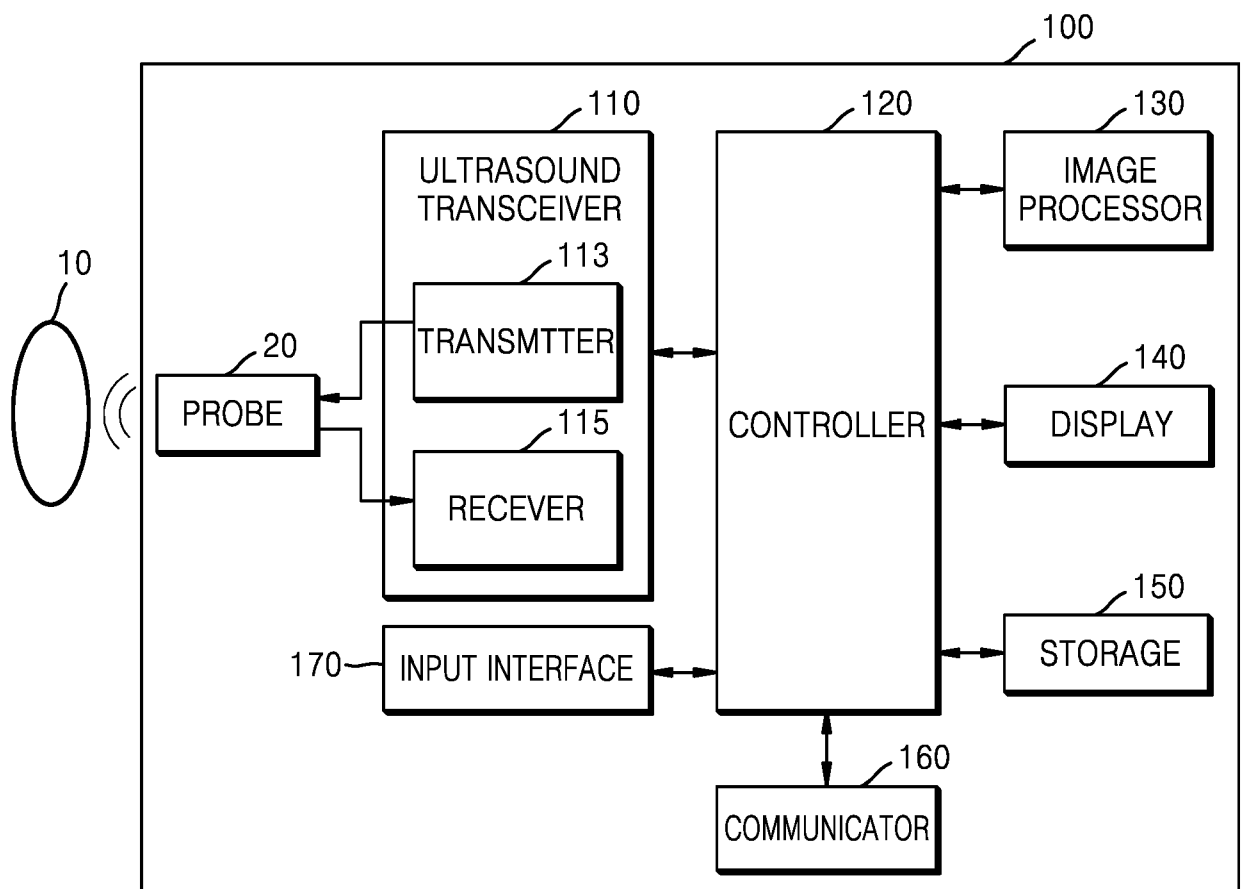


FIG. 2C

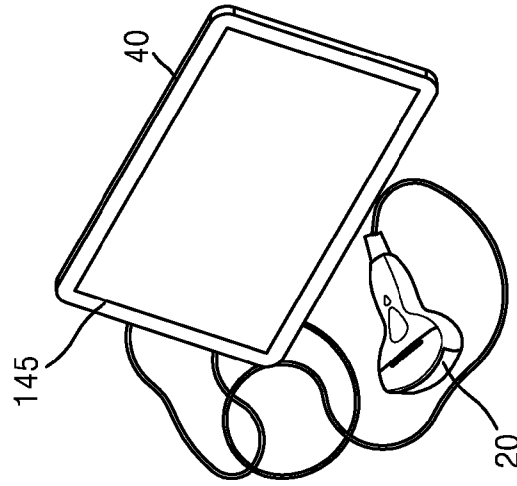


FIG. 2B

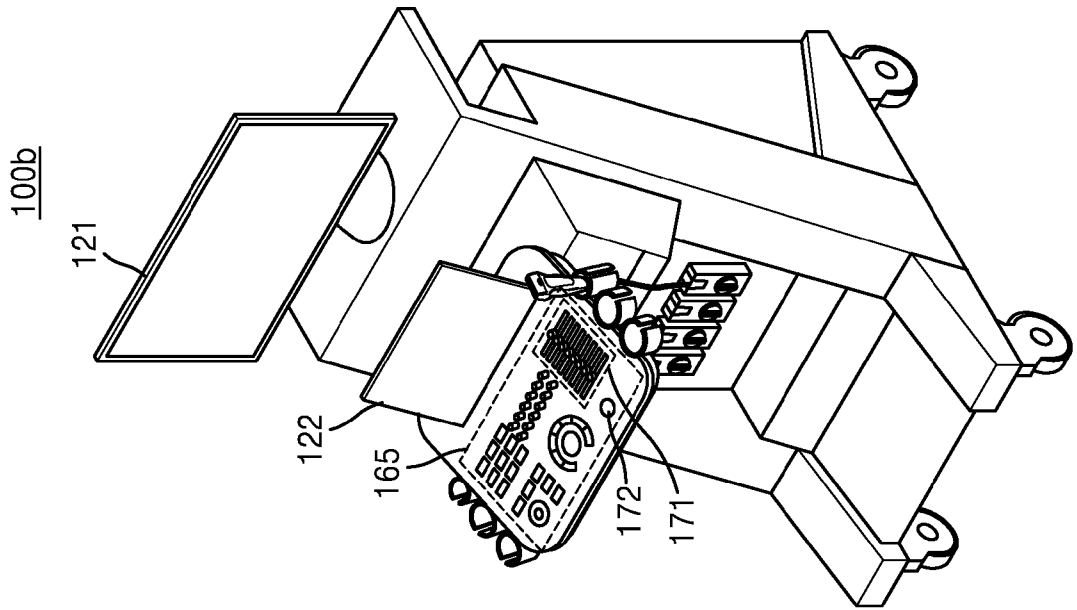


FIG. 2A

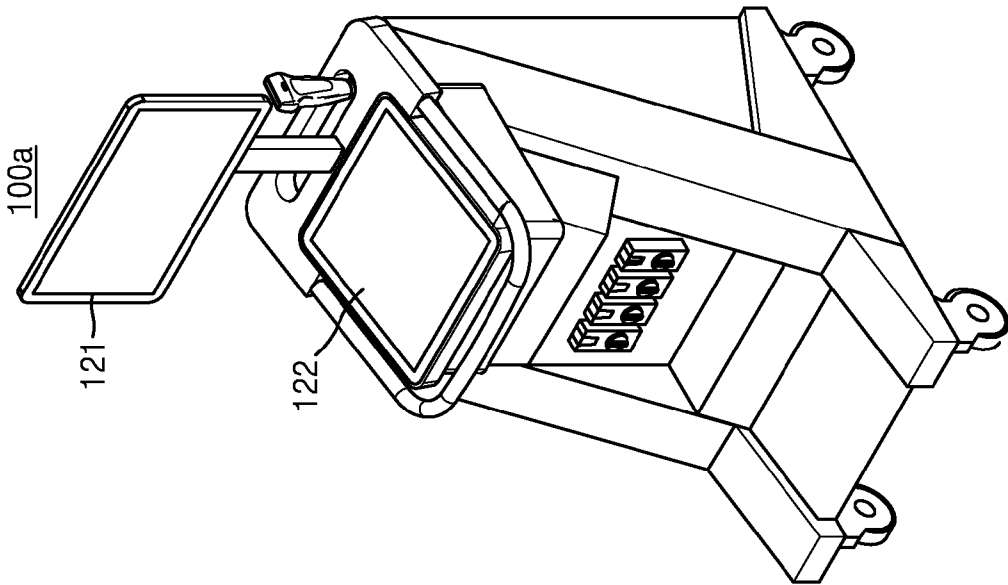


FIG. 3

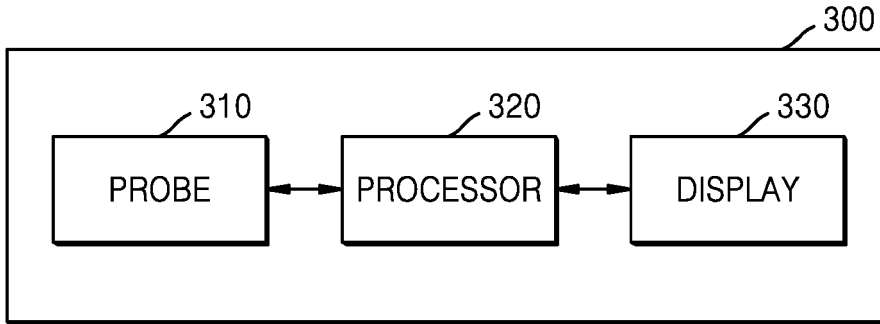


FIG. 4

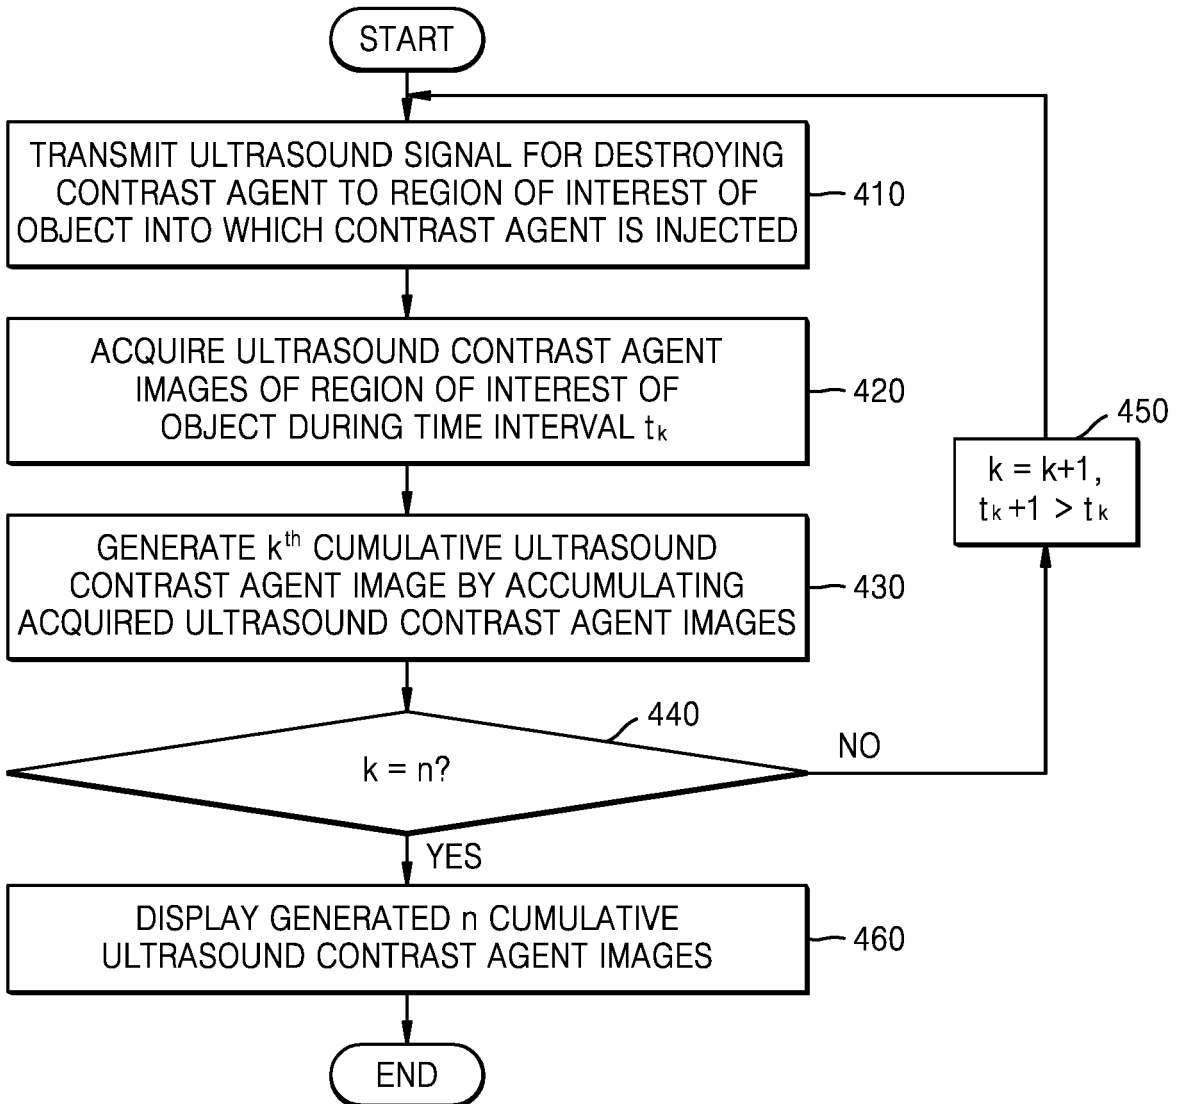


FIG. 5

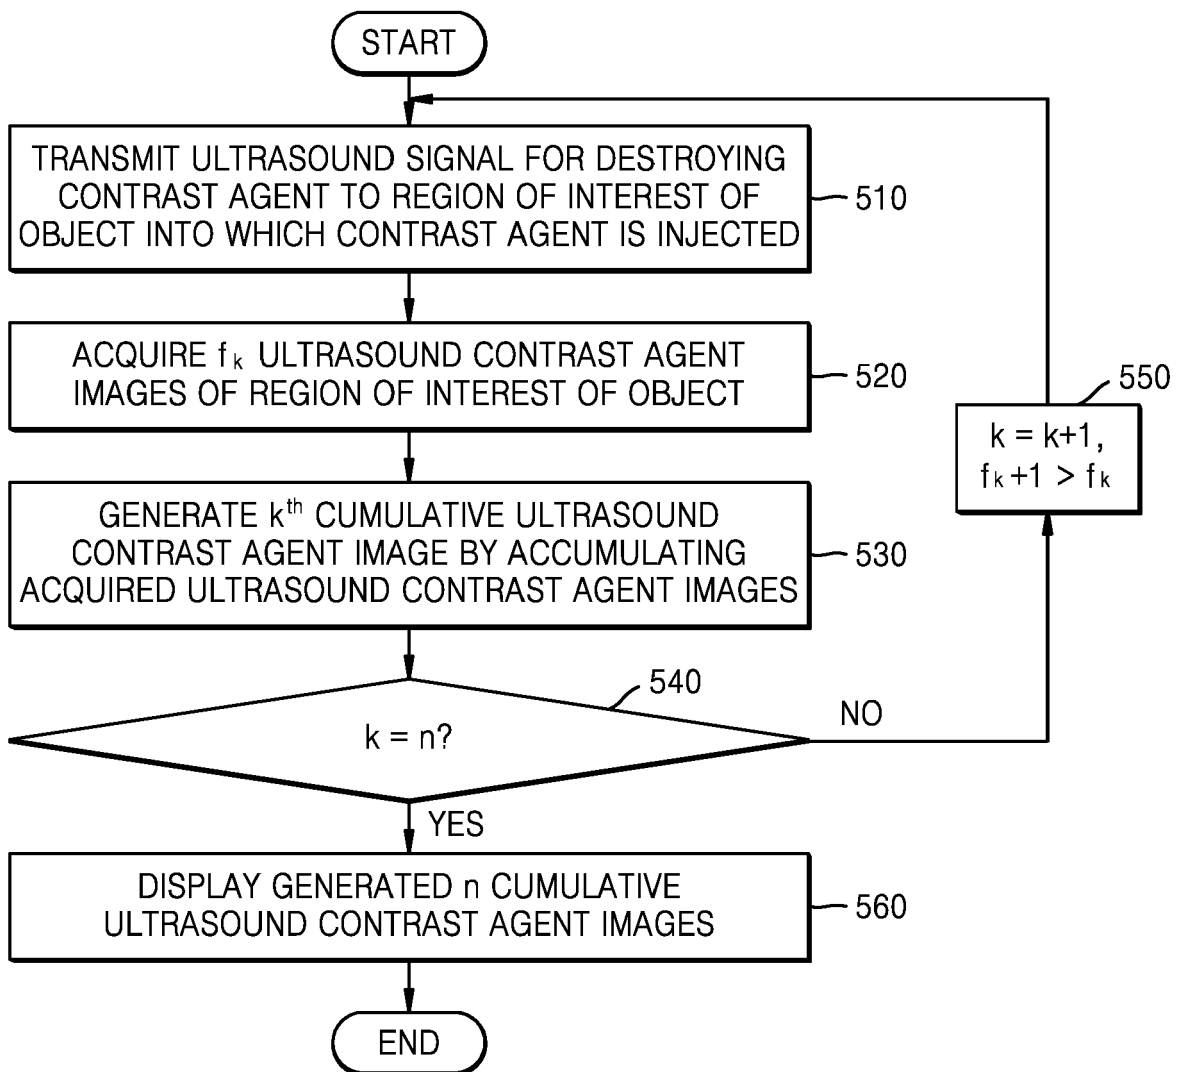


FIG. 6

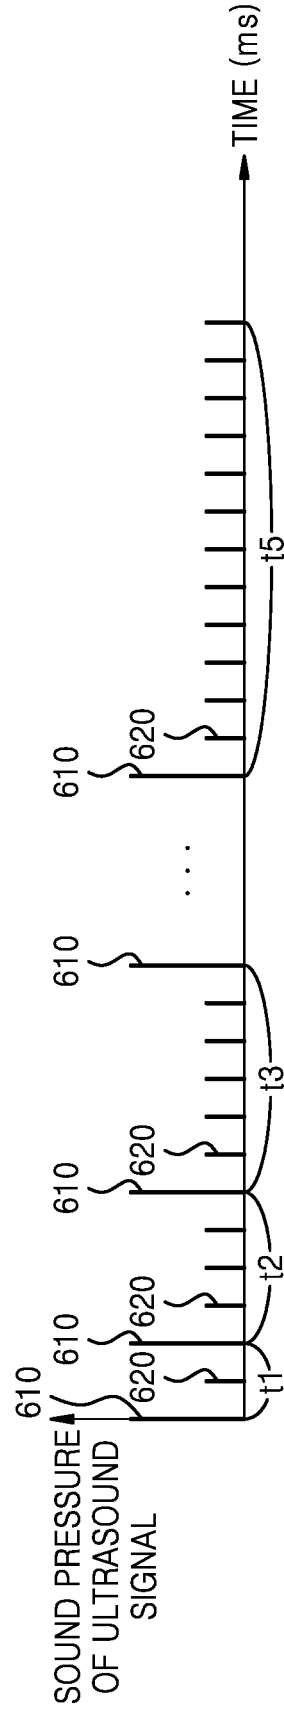


FIG. 7

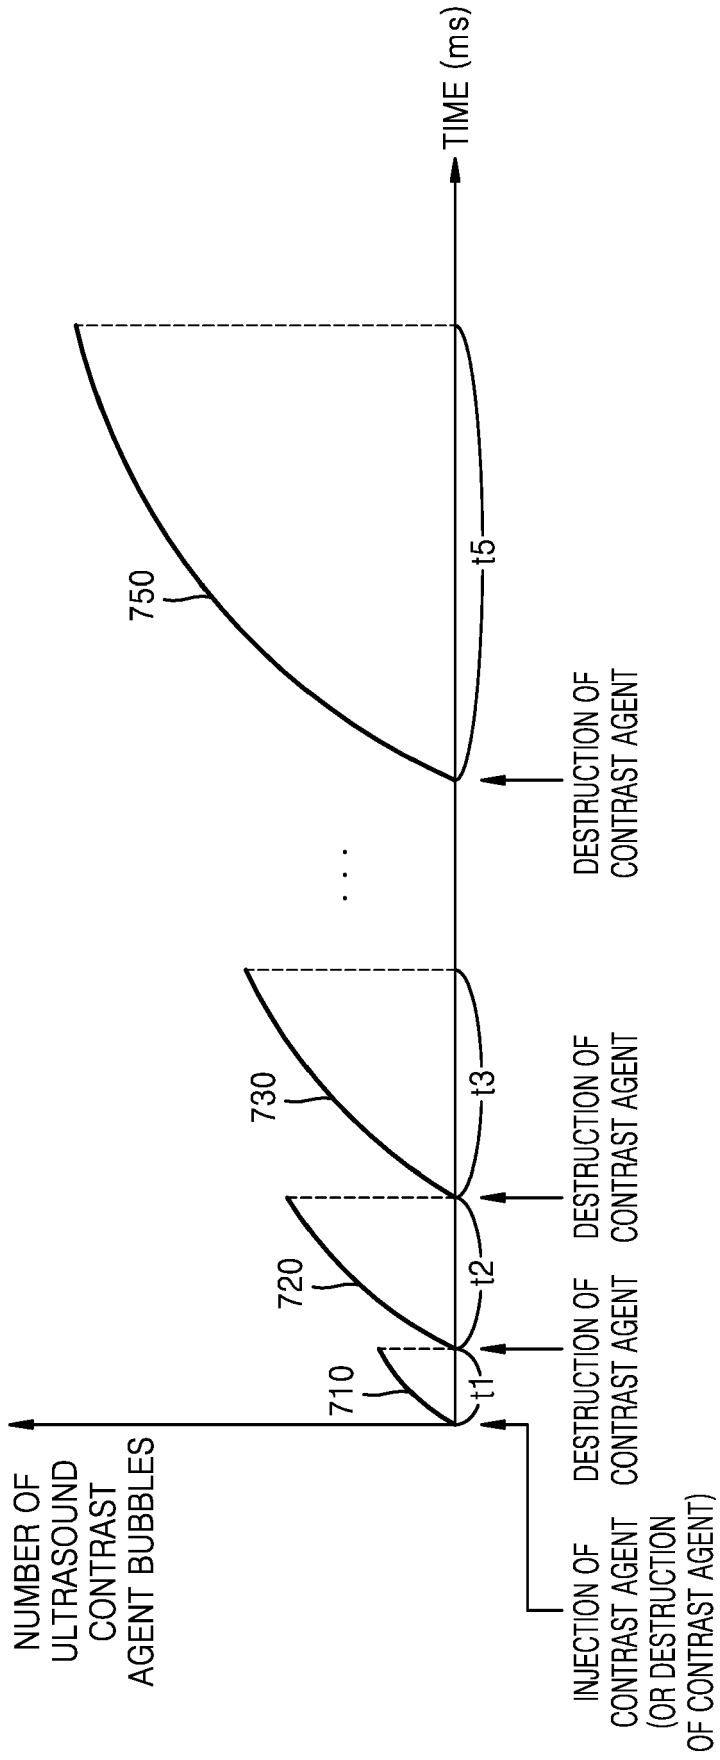


FIG. 8


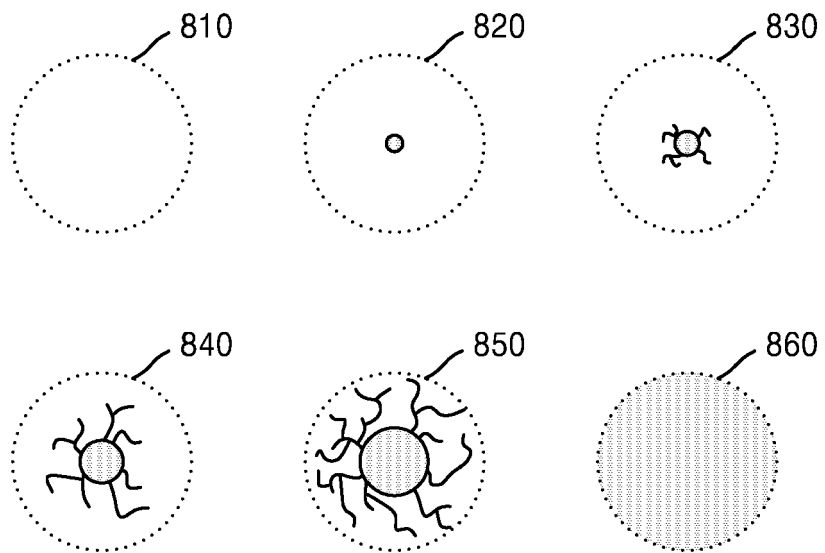


FIG. 9



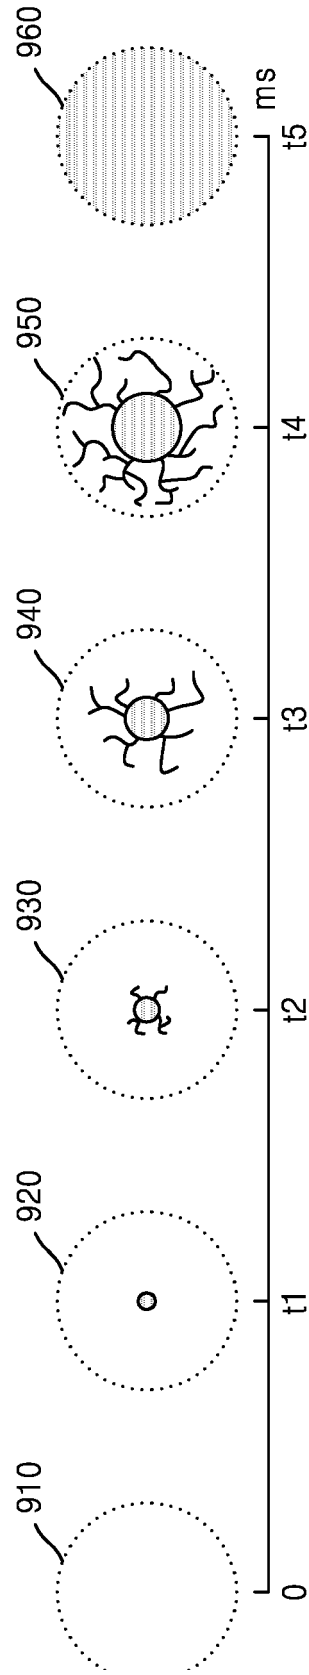

EUROPEAN SEARCH REPORT

Application Number
EP 18 20 0566

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 6 319 204 B1 (BROCK-FISHER GEORGE A [US] ET AL) 20 November 2001 (2001-11-20) * the whole document *	1-15	INV. A61B8/08 A61B8/00
A	US 2002/165454 A1 (OGASAWARA YOICHI [JP] ET AL) 7 November 2002 (2002-11-07) * the whole document *	1-15	
A	US 2009/112097 A1 (KATO SEI [JP] ET AL) 30 April 2009 (2009-04-30) * the whole document *	1-15	
A	KR 2017 0053103 A (SAMSUNG MEDISON CO LTD [KR]) 15 May 2017 (2017-05-15) * the whole document *	1-15	
The present search report has been drawn up for all claims			TECHNICAL FIELDS SEARCHED (IPC)
			A61B
Place of search		Date of completion of the search	Examiner
Munich		8 April 2019	Mundakapadam, S
CATEGORY OF CITED DOCUMENTS			
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

EPO FORM 1503 03/02 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 18 20 0566

5 This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

08-04-2019

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 6319204 B1	20-11-2001	NONE	
US 2002165454 A1	07-11-2002	JP 2002209898 A US 2002165454 A1	30-07-2002 07-11-2002
US 2009112097 A1	30-04-2009	CN 101416887 A JP 2009100971 A US 2009112097 A1	29-04-2009 14-05-2009 30-04-2009
KR 20170053103 A	15-05-2017	NONE	

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 1020180018062 [0001]

专利名称(译)	超声成像设备及其控制方法		
公开(公告)号	EP3524168A1	公开(公告)日	2019-08-14
申请号	EP2018200566	申请日	2018-10-16
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO., LTD.		
当前申请(专利权)人(译)	三星MEDISON CO., LTD.		
[标]发明人	KIM JUNG HO LEE YOON CHANG		
发明人	KIM, JUNG-HO LEE, YOON-CHANG		
IPC分类号	A61B8/08 A61B8/00		
优先权	1020180018062 2018-02-13 KR		
外部链接	Espacenet		

摘要(译)

提供了一种超声成像设备及其控制方法。在用于破坏造影剂的超声信号被发送到对象的感兴趣区域之后，超声成像设备获取对象的感兴趣区域的多个超声造影剂图像，造影剂被注入其中。 t_k 的间隔 ($k = 1, 2, \dots, n$ 和 n 是 2 或更大的整数)，通过在 t_k 的每个时间间隔累积所获取的超声造影剂图像来生成第 k 累积超声造影剂图像以生成 n 累积超声造影剂图像，并显示生成的 n 个累积超声造影剂图像，其中 t_k 满足 $t_k > t_{k-1}$ 。

FIG. 4

