



(11) **EP 1 974 672 B9**

(12) **CORRECTED EUROPEAN PATENT SPECIFICATION**

(15) Correction information:
Corrected version no 1 (W1 B1)
Corrections, see
Claims EN 2

(51) Int Cl.:
A61B 8/00 ^(2006.01) **G01S 7/52** ^(2006.01)
G10K 11/34 ^(2006.01)

(48) Corrigendum issued on:
16.04.2014 Bulletin 2014/16

(45) Date of publication and mention
of the grant of the patent:
20.11.2013 Bulletin 2013/47

(21) Application number: **08005681.5**

(22) Date of filing: **26.03.2008**

(54) **Ultrasonic imaging apparatus and ultrasonic velocity optimization method**

Ultraschallabbildungsvorrichtung und Verfahren zur Optimierung der Ultraschallgeschwindigkeit

Appareil d'imagerie par ultrasons et procédé d'optimisation de la vitesse ultrasonique

(84) Designated Contracting States:
DE NL

(30) Priority: **28.03.2007 JP 2007085918**

(43) Date of publication of application:
01.10.2008 Bulletin 2008/40

(73) Proprietors:
• **Kabushiki Kaisha Toshiba**
Minato-ku,
Tokyo 105-8001 (JP)
• **Toshiba Medical Systems Corporation**
Otawara-shi, Tochigi-ken 324-8550 (JP)

(72) Inventor: **Kakee, Akihiro**
Otawara-shi
Tochigi 324-8550 (JP)

(74) Representative: **Kramer - Barske - Schmidtchen**
Landsberger Strasse 300
80687 München (DE)

(56) References cited:
EP-A- 0 421 279 US-A- 5 415 173
US-A- 5 638 820 US-A1- 2003 092 990
US-B1- 6 305 225

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 974 672 B9

Description

[0001] The present invention relates to an ultrasonic imaging apparatus and ultrasonic velocity optimization method which can automatically optimize a sound velocity in ultrasonic imaging used for image diagnosis, non-destructive inspection, or the like.

[0002] Examples of an ultrasonic imaging apparatus which performs imaging by using ultrasonic waves include an ultrasonic inspection apparatus for nondestructively inspecting abnormality in a structure and an ultrasonic diagnosis apparatus which transmits ultrasonic waves to a subject (patient) and acquires tomograms associated with a diagnosis region on the basis of the reflected waves. For example, an ultrasonic diagnosis apparatus can display, in real time, how a heart beats or a fetus moves, with simple operation of bringing an ultrasonic probe into contact with the body surface. In addition, this apparatus offers a high level of safety, and hence can be repeatedly used for examination. Furthermore, the system size is smaller than those of other diagnosis apparatuses such as X-ray, CT, and MRI apparatuses. Therefore, this apparatus allows easy examination upon being moved to a bed side. That is, the apparatus is a convenient diagnosis technique. Ultrasonic diagnosis apparatuses used in such ultrasonic diagnosis vary depending on the types of functions which they have. Some compact apparatuses which can be carried with one hand have been developed. Ultrasonic diagnosis is free from the influence of radiation exposure such as X-ray exposure, and hence can be used in obstetric treatment, treatment at home, and the like.

[0003] An ultrasonic imaging apparatus typified by such an ultrasonic diagnosis apparatus uses a method of converging transmission and reception beams to improve the azimuth resolution of an image. Electronic scanning type array transducers, in particular, use an electronic convergence method based on delay time control for transmission/reception signals of each channel. A problem in this electronic convergence method is that a beam diverges at a place (depth) apart from a convergence point, and the azimuth resolution decreases.

[0004] For this problem, a conventional ultrasonic imaging apparatus uses a technique called a dynamic convergence method. This technique performs delay time control to continuously move a convergence point in the depth direction with a lapse of time at the time of reception. This technique allows to always acquire a reception ultrasonic beam from a converged area.

[0005] FIG. 13 is a view showing the positional relationship between each ultrasonic transducer of an ultrasonic probe and a focal point P in a subject to be examined. As shown in FIG. 13, letting X be the coordinates of the focal point P in the depth direction, and Yi be the coordinates of an ultrasonic transducer Ti in the array direction from the aperture center (origin O) of the ultrasonic probe, a delay time Δti from the time when the wavefront of a reflected sound wave reaches the aperture

center to the time when the wavefront reaches the ultrasonic transducer Ti is given by

$$\Delta ti = [(X^2 + Yi^2)^{1/2} - X] / C$$

where C is a sound velocity.

[0006] In this calculation, if the sound velocity used for the calculation is equal to the actual sound velocity of propagation in the subject, as shown in FIG. 14A, desired positions Fn-1, Fn, and Fn+1 can be made to coincide with the beam convergence point, thereby acquiring a high-resolution ultrasonic image.

[0007] A conventional ultrasonic diagnosis apparatus, however, calculates the delay time Δti by using a preset velocity (representative velocity) v representing a visualization target slice regardless of the position of the slice and the components of a propagation medium, and sets the calculated time. The actual sound velocity of propagation in the subject does not always coincide with the representative velocity v. If, for example, the representative sound velocity used for calculation is lower than the actual sound velocity of propagation in the subject, as shown in FIG. 14B, a beam convergence point is located before the desired positions Fn-1, Fn, and Fn+1, resulting in a low resolution as compared with the case shown in FIG. 14A.

[0008] It has recently been reported that C = 1560 cm/s in the muscle, and C = 1480 cm/s in the fat. In addition, the sound velocity varies in individuals. The difference between the representative sound velocity v and the actual sound velocity of propagation C causes the difference between the assumed position of a convergence point and the actual position of the convergence point, resulting in image degradation.

[0009] As techniques for solving the difference between the assumed position of a convergence point and the actual position of the convergence point in a conventional ultrasonic diagnosis apparatus, techniques such as phase correction techniques based on a reflection method and a cross-correlation method are available. These techniques, however, require the presence of a reflector such as a calculus or a boundary wall, and has limitations such as the necessity of the presence of a reflector as a point. Even if, therefore, these techniques are used, it is impossible to acquire good images as a whole.

[0010] US 6 305 225 B1 relates to an ultrasonic focusing method for focusing a received ultrasonic signal reflected from an object, and more particularly, to an ultrasonic signal focusing method for controlling a focusing delay time of a received ultrasonic signal to obtain a maximum resolution for use in an ultrasonic imaging system.

[0011] US 5 638 820 relates to a method for improving the quality of ultrasound images in an ultrasound system.

[0012] US 2003/0092990 A1 relates to an ultrasonic imaging apparatus for examining internal structure of a

living body and goods, such as an ultrasonic diagnosis apparatus used for medical diagnosis, and a non-destructive examination apparatus used for non-destructive examination of goods. More, particularly, the documents relates to an ultrasonic imaging apparatus that can obtain images of high quality even when the internal structure of a living body and goods are different in their propagation velocity of ultrasonic waves.

[0013] The present invention has been made in consideration of the above situation, and has as its object to provide an ultrasonic imaging apparatus and ultrasonic velocity optimization method which can acquire ultrasonic images higher in resolution than that in the prior art by optimizing a sound velocity used for delay time calculation in ultrasonic imaging.

[0014] This is achieved by the ultrasonic imaging apparatus according to claim 1 and the ultrasonic velocity optimization method according to claim 12.

[0015] Further advantageous embodiments are defined in the dependent claims.

[0016] The invention can be more fully understood from the following detailed description when taken in conjunction with the accompanying drawings, in which:

FIG. 1 is a block diagram showing the arrangement of an ultrasonic diagnosis apparatus 1 according to an embodiment;

FIG. 2 is a block diagram showing an example of the arrangement of a resolution optimization unit 17;

FIG. 3 is a flowchart showing the sequence of processing (resolution optimization processing) based on a resolution optimization function;

FIG. 4 is a view showing a visualization target slice segmented into $m \times n$ small areas;

FIG. 5 is a view showing an example of a contrast value distribution map indicating the distribution of contrast values in the respective areas in the visualization target slice;

FIG. 6 is a graph for explaining an example of determination processing for a sound velocity at which the contrast value is maximized in each small area;

FIG. 7 is a view showing an example of an optimal sound velocity map for each small area which is obtained by resolution optimization processing;

FIG. 8 is a view showing an example of an optimal sound velocity map for each depth which is obtained by resolution optimization processing;

FIG. 9 is a view showing an example of an optimal sound velocity map on a visualization target slice which is obtained by resolution optimization processing;

FIG. 10 is a flowchart showing each processing sequence when a real scan is performed by using a resolution optimization function;

FIG. 11 is a view showing an example of the display form of a color sound velocity map;

FIG. 12 are a view exemplarily showing an ultrasonic image (a) obtained by a conventional technique, and

a view exemplarily showing an ultrasonic image (b) acquired by correcting the difference between the set sound velocity used for the calculation of a reception delay time and the actual in vivo sound velocity;

FIG. 13 is a view for explaining a reception delay time calculation technique; and

FIG. 14 is a view for explaining convergence line shifts due to sound velocity differences.

[0017] The embodiments of the present invention will be described below with reference to the views of the accompanying drawing. Note that the same reference numerals denote constituent elements having substantially the same functions and arrangements, and a repetitive description will be made only when required. This embodiment exemplifies a case in which the technical idea of the present invention is applied to an ultrasonic diagnosis apparatus as an ultrasonic imaging apparatus. However, the technical idea of the present invention is not limited to this, and can be applied to, for example, an ultrasonic inspection apparatus used for nondestructive inspection and the like.

[0018] FIG. 1 is a block diagram showing the arrangement of an ultrasonic diagnosis apparatus 1 according to this embodiment. The ultrasonic diagnosis apparatus 1 comprises an apparatus body 2 and an ultrasonic probe 3. The apparatus body 2 comprises an ultrasonic transmission unit 11, an ultrasonic reception unit 13, a B mode processing unit 15, a resolution optimization unit 17, an image generating unit 23, an image combining unit 25, a monitor 27, a control processor (CPU) 29, an interface unit 31, an input unit 33, and a storage unit 35.

[0019] The ultrasonic probe 3 includes a plurality of piezoelectric transducers which generate ultrasonic waves on the basis of driving signals from the apparatus body 2 and convert reflected waves from a subject to be examined into electrical signals, a matching layer provided for the piezoelectric transducers, a backing member which prevents ultrasonic waves from propagating backward from the piezoelectric transducers, and the like. When an ultrasonic wave is transmitted from the ultrasonic probe 3 to a subject P to be examined, the transmitted ultrasonic wave is sequentially reflected by a discontinuity surface of acoustic impedance of internal body tissue, and is received as an echo signal by the ultrasonic probe 3. The amplitude of this echo signal depends on an acoustic impedance difference on the discontinuity surface by which the echo signal is reflected. The echo produced when an ultrasonic pulse is reflected by the surface of a moving blood flow, cardiac wall, or the like is subjected to a frequency shift depending on the velocity component of the moving body in the ultrasonic transmission direction due to a Doppler effect.

[0020] Note that the ultrasonic probe 3 can perform ultrasonic scanning on a three-dimensional area of a subject. In this case, the ultrasonic probe 3 has, for example, an arrangement designed to perform ultrasonic scanning

on a three-dimensional area by mechanically swinging transducers along a direction perpendicular to the array direction of the transducers or an arrangement designed to perform ultrasonic scanning on a three-dimensional area by electrical control using two-dimensional vibration elements arrayed two-dimensionally. When the ultrasonic probe 3 has the former arrangement, three-dimensional scanning on the subject is performed by the swinging circuit. An examiner can therefore automatically acquire a plurality of two-dimensional tomograms by only bringing the probe body into contact with the subject. It is also possible to detect the accurate distance between slices from a controlled swinging velocity. When the ultrasonic probe 3 has the latter arrangement, it is possible in theory to perform ultrasonic scanning on a three-dimensional area in the same time as that required to acquire a conventional two-dimensional tomogram.

[0021] The ultrasonic transmission unit 11 has a trigger generating circuit, delay circuit, pulser circuit, and the like (none are shown). The pulser circuit repeatedly generates rate pulses for the formation of transmission ultrasonic waves at a predetermined rate frequency f_r Hz (period: $1/f_r$ sec). The delay circuit gives each rate pulse the delay time required to focus an ultrasonic wave into a beam for each channel and determine a transmission directivity. The trigger generating circuit applies a driving pulse to the probe 3 at the timing based on this rate pulse.

[0022] The ultrasonic reception unit 13 has an amplifier circuit, A/D converter, adder, and the like (none are shown). The amplifier circuit amplifies echo signals received through the ultrasonic probe 3 on a channel basis. The A/D converter gives each amplified echo signal the delay time required to determine a reception directivity. The adder then performs addition processing. With this addition, the reflection component of the echo signal from the direction corresponding to the reception directivity is enhanced, and a synthetic beam for ultrasonic transmission/reception is formed in accordance with the reception directivity and transmission directivity.

[0023] The B mode processing unit 15 receives the echo signal from the ultrasonic reception unit 13, and performs logarithmic amplification, envelope detection processing, and the like, thereby generating data whose signal strength is represented by a brightness level. This data is transmitted to the image generating unit 23 and is displayed as a B mode image representing the strength of a reflected wave as a brightness on the monitor 27.

[0024] A Doppler processing unit 16 frequency-analyzes velocity information from the echo signal received from the ultrasonic reception unit 13 to extract a blood flow, tissue, and contrast medium echo component by the Doppler effect, and obtains blood flow information such as an average velocity, variance, and power at multiple points.

[0025] The resolution optimization unit 17 executes processing (resolution optimization processing) based on a resolution optimization function (to be described later) under the control of the control processor 29.

[0026] FIG. 2 is a block diagram showing an example of the arrangement of the resolution optimization unit 17. Referring to FIG. 2, the resolution optimization unit 17 includes a contrast evaluation unit 170, a computation memory 172, and an optimal sound velocity calculation unit 174.

[0027] The contrast evaluation unit 170 uses the amplitude value at each position in a predetermined area (or the luminance value of each pixel) to, for example, evaluate contrast information about the area and generate a contrast value distribution map.

[0028] The computation memory 172 stores the contrast value distribution map and the like acquired by the contrast evaluation unit 170 and the optimal sound velocity map and the like acquired by the optimal sound velocity calculation unit 174.

[0029] The optimal sound velocity calculation unit 174, for example, calculates an optimal velocity and generates an optimal sound velocity map for each predetermined area, each depth, each visualization target slice, or the like on the basis of the contrast value distribution acquired by the contrast evaluation unit 170.

[0030] The image generating unit 23 generates an ultrasonic diagnosis image as a display image on the basis of various data received from the B mode processing unit 15 and Doppler processing unit 16. Note that data before it is input to the image generating unit 23 is sometimes called "raw data".

[0031] The image combining unit 25 combines the image received from the image generating unit 23 with character information of various types of parameters, scale marks, and the like, and outputs the resultant signal as a video signal to the monitor 27.

[0032] The monitor 27 displays morphological information (B mode image) in the living body, blood flow information (an average velocity image, variance image, power image, or the like) in the living body, various types of map images obtained by resolution optimization processing (to be described later), and the like in predetermined forms on the basis of video signals from the image combining unit 25.

[0033] The control processor 29 has a function as an information processing apparatus (computer) and controls the overall operation of this ultrasonic diagnosis apparatus. The control processor 29 reads out a dedicated program for implementing the resolution optimization function and control programs for executing a predetermined scan sequence, image generation/display, and the like from the storage unit 35, maps them in its internal memory, and executes computation/control and the like associated with various types of processing.

[0034] The interface unit 31 is an interface associated with the input unit 33, a network, and a new external storage device (not shown). The interface unit 31 can transfer data such as ultrasonic images, analysis results, and the like obtained by this apparatus to another apparatus through a network.

[0035] The input unit 33 has various types of switches,

buttons, a trackball, a mouse, a keyboard, and the like which are used to input, to the ultrasonic diagnosis apparatus 1, various types of instructions and conditions, an instruction to set a region of interest (ROI), various types of image quality condition setting instructions, and the like from an operator. When, for example, the operator operates the end button or FREEZE button of the input unit 33, the transmission/reception of ultrasonic waves is terminated, and the ultrasonic diagnosis apparatus is set in a temporary stop state.

[0036] In addition, the input unit 33 includes switches and the like for issuing an instruction to start resolution optimization processing and setting/changing the initially set sound velocity in this processing, the optimal sound velocity calculation technique, and the like.

[0037] The storage unit 35 comprises recording media such as magnetic disks (floppy (registered trademark) disks, hard disks, and the like), optical disks (CD-ROMs, DVDs, and the like), and semiconductor memories, and a device which reads out information recorded on the media. The storage unit 35 stores transmission/reception conditions, a predetermined scan sequence, a program for executing the resolution optimization function, a control program for executing image generation/display processing, diagnosis information (a patient ID, findings by a doctor, and the like), a diagnosis protocol, a body mark generation program, various types of signal data, image data, and other data. Data in the storage unit 35 can be transferred to an external peripheral apparatus through the interface unit 31.

(Resolution Optimization Function)

[0038] The resolution optimization function which the ultrasonic diagnosis apparatus 1 has will be described next. This function determines an optimal sound velocity corresponding to a tissue component at each position within a scan slice, and calculates a reception delay time for each reception beam from each position within the scan slice by using the optimal sound velocity. The reception delay time (optimal reception delay time) calculated by using an optimal sound velocity is used to execute delay addition (phased addition) processing in a scan (real scan) for acquiring an ultrasonic image actually used for diagnosis. This corrects the difference between the sound velocity used for the calculation of a reception delay time and the actual sound velocity of propagation in the subject, thereby acquiring an ultrasonic image with optimized resolution.

[0039] For a concrete description of this embodiment, the resolution optimization function using image data after processing in the image generating unit 23 (i.e., data indicating a luminance value at each position on a slice, which is obtained through scan conversion processing) will be described. However, this resolution optimization function is not limited to this, and may be configured to use raw data before processing in the image generating unit 23 (i.e., data indicating an amplitude value at each

position on a slice, which is obtained before scan conversion processing).

[0040] FIG. 3 is a flowchart showing a processing sequence based on the resolution optimization function. Referring to FIG. 3, first of all, when the operator issues an instruction to start resolution optimization processing by operating the resolution optimization switch of the input unit 33 or the like, the control processor 29 sets a sound velocity v to an initial value (e.g., $v = 1400$ m/s) (step S21), and calculates a delay time at each position in one frame (i.e., a two-dimensional scan plane) (step S22).

[0041] The control processor 29 then two-dimensionally scans a visualization target slice, and executes delay addition by using the delay times calculated in step S22, thereby acquiring raw data or image data corresponding to one or a few frames associated with the visualization target slice (step S23). For a concrete description, assume that image data corresponding to one frame is acquired in step S23.

[0042] The contrast evaluation unit 170 segments the image data associated with the visualization target slice into $m \times n$ small areas like those shown in FIG. 4, and evaluates a contrast value for each small area (step S24). In this case, the evaluation method to be used for contrast values is not specifically limited. For example, the contrast evaluation unit 170 can calculate the variance of luminance values existing in each area (the variance of amplitudes in the case of raw data), the difference value or slope value between the maximum and minimum values of luminances in each area (the difference value between the maximum and minimum values of amplitudes in the case of raw data), and a differential value (a first-order differential value or second-order differential value), and directly or indirectly evaluate contrast values by using the calculated values. For a concrete description, assume that in this embodiment, a contrast value in each area is evaluated by the variance or differential value of luminance values existing in each area.

[0043] The resolution optimization unit 17 extracts some of the small areas constituting the visualization target slice which are excluded from this resolution optimization processing on the basis of the obtained variances (step S25). More specifically, the resolution optimization unit 17 determines whether a given variance value falls within a predetermined range having a lower limit α and an upper limit β . If the variance value falls outside the predetermined range, contrast value = 0 is set in the small area corresponding to the variance value.

[0044] The contrast evaluation unit 170 then generates a contrast value distribution map indicating the distribution of contrast values V_{mn} in the respective small areas in the visualization target slice, as shown in, for example, FIG. 5. The computation memory 172 stores the generated contrast value distribution map in correspondence with set sound velocity information (step S26).

[0045] The control processor 29 determines whether the current sound velocity v exceeds a predetermined

upper limit value (e.g., 1,600 m/s) (step S27). If the current sound velocity v exceeds the upper limit value, the process shifts to step S29.

[0046] If the current sound velocity v does not exceed the predetermined upper limit value, the value obtained by adding, for example, +20 m/s to the current sound velocity v is set as a new sound velocity v . The respective processes in steps S22 to S27 are repeated in the same manner as described above (step S26). With this operation, a contrast value distribution map is generated for each sound velocity (in this case, for each sound velocity at 20 m/s intervals in the range of 1,400 m/s to 1,600 m/s), and is stored in the computation memory 172.

[0047] The optimal sound velocity calculation unit 174 determines, for each small area, a sound velocity at which the contrast value is maximized (step S29).

[0048] FIG. 6 is a graph for explaining an example of determination processing for a sound velocity at which the contrast value is maximized. The optimal sound velocity calculation unit 174 plots the relationship between the contrast value and the sound velocity, as shown in, for example, FIG. 6. The optimal sound velocity calculation unit 174 calculates a regression curve associated with each plotted point, and determines a sound velocity $v_{\max}$ at which the contrast value is maximized, on the basis of the regression curve.

[0049] The optimal sound velocity calculation unit 174 then calculates an optimal sound velocity V by using the sound velocity $v_{\max}$ at which the contrast value in each small area is maximized (step S30). Various techniques can be used to calculate an optimal sound velocity V . Several techniques will be described according to the examples.

[Example 1]

[0050] First of all, with regard to a small area in which contrast value = 0 is not set in step S26, a sound velocity $v_{\max}$ at which the contrast value is maximized is set as the optimal sound velocity V in the small area. With regard to a small area in which contrast value = 0 is set, the optimal sound velocity V is calculated by interpolation using a preset sound velocity or the optimal sound velocities in a plurality of neighboring small areas. As a result of this calculation, an optimal sound velocity map for each small area on the slice can be obtained, as shown in, for example, FIG. 7.

[Example 2]

[0051] Example 1 has exemplified the case in which an optimal sound velocity is calculated and set for each small area. In contrast to this, Example 2 exemplifies a case in which an optimal velocity is calculated and set for each depth.

[0052] An optimal sound velocity calculation unit 174 calculates the average value of the optimal sound velocities in a plurality of small areas belonging to the same

depth from the ultrasonic wave application surface (or the body surface of the subject) on the optimal sound velocity map for each small area shown in, for example, FIG. 7, and sets the average value as a small area optimal sound velocity belonging to the depth. As a result of this calculation, an optimal sound velocity map for each depth on the slice can be obtained as shown in, for example, FIG. 8.

10 [Example 3]

[0053] Example 3 exemplifies a case in which one optimal velocity is set for the visualization target slice.

[0054] An optimal sound velocity calculation unit 174 calculates the average value of the optimal sound velocities in all the small areas or the average value of the optimal sound velocities at all the depths on the optimal sound velocity map for each small area shown in FIG. 7 or the optimal sound velocity map for each depth shown in FIG. 8, and sets the average value as an optimal sound velocity associated with the visualization target slice. As a result of this calculation, one optimal sound velocity map is obtained for the visualization target slice as shown in, for example, FIG. 9.

[0055] It is possible to arbitrarily select one of the above techniques. In addition, it suffices to analyze the distribution state of optimal sound velocities in the respective small areas and automatically select one of the techniques on the basis of the analysis result.

[0056] Note that a sound velocity has a correlation only with an azimuth resolution (a resolution in the horizontal direction), and hence evaluation including a distance resolution (a resolution in the time direction) with no correlation may degrade the accuracy. It is therefore preferable to limit the evaluation of a contrast value to the horizontal direction (the direction perpendicular to a scanning line). That is, an average value or maximum value in the time direction is obtained from contrast values in each small area which are evaluated at each depth, and is set as an optimal velocity for each small area. This can implement the optimization of resolutions with high accuracy.

(Operation)

[0057] The operation of an ultrasonic diagnosis apparatus 1 when performing a real scan using the resolution optimization function will be described next.

[0058] FIG. 10 is a flowchart showing each processing sequence when a real scan is performed by using the resolution optimization function. As shown in FIG. 10, first of all, when patient information, scan conditions, and the like are input through an input unit 33 (step S1), a control processor 29 executes the above resolution optimization processing in response to the operation of the resolution optimization switch (step S2).

[0059] An image generating unit 23 then generates a color sound velocity map by using the optimal sound ve-

locity map for each small area which is obtained by the resolution optimization processing (step S3).

[0060] In this case, a color sound velocity map indicates the distribution of optimal sound velocities in the form of a color distribution by assigning predetermined colors to the respective small areas (used in the resolution optimization processing) constituting a visualization target slice in accordance with the values of optimal sound velocities. Note that the sound velocity changes depending on the components of a propagation medium. That is, the color sound velocity map allows the operator to visually recognize the distribution of the tissue components of a visualization target slice by colors.

[0061] As shown in FIG. 11, this color sound velocity map is displayed together with a B mode image associated with the visualization target slice which is acquired in real time (or acquired in resolution optimization processing) and color bars indicating the correspondence between optimal sound velocities and colors (step S4). Assume that the operator observes the color sound velocity map and finds various colors are scattered and distributed on the map. In this case, the optimal velocities obtained by the technique according to the first embodiment can be set. If color changes almost in accordance with changes in depth on the color sound velocity map, the optimal velocities obtained by the technique according to the second embodiment can be set. In addition, if similar colors are in large amount on the color sound velocity map, the optimal velocity obtained by the technique according to the third embodiment may be set

[0062] The control processor 29 then executes a real scan by using the optimal velocity or velocities (step S5). In this case, if the optimal velocities are set in the form shown in, for example, FIG. 7, the control processor 29 executes delay addition processing by using the delay times calculated by using the set optimal velocities. If the optimal velocities are set in the form shown in, for example, FIG. 8, the control processor 29 executes delay addition processing by using the delay times calculated by using the set optimal velocities is in accordance with the respective depths. If the optimal velocity is set in the form shown in, for example, FIG. 9, the control processor 29 newly calculates a delay time by using the optimal velocity and executes delay addition processing by using the delay time.

[0063] The ultrasonic image acquired by this real scan is displayed on the monitor 27 in a predetermined form (step S6).

(Effect)

[0064] According to the above arrangements, the following effects can be obtained.

[0065] This ultrasonic diagnosis apparatus determines an optimal sound velocity corresponding to a tissue component at each position in a scan slice, and calculates a reception delay time or the like for each reception beam from each position in the scan slice by using the deter-

mined optimal sound velocity. Executing delay addition processing in a scan for acquiring an ultrasonic image actually used for diagnosis by using the reception delay time calculated by using an optimal sound velocity in this manner makes it possible to correct the difference between the set sound velocity used for the calculation of a reception delay time and the actual in vivo sound velocity and acquire an ultrasonic image with optimized resolution.

[0066] In the case in which differential values are used as contrast values, in particular, edges in the respective small areas can be actively extracted, and hence this technique is preferable for the implementation of optimization of a resolution. That is, if an average value or a variance value is used, an evaluation result may be influenced by the position of an ROI set for the calculation of a variation. If a frequency is used as a contrast value, a large amount of data are required for frequency analysis. This will degrade the real-time performance, and increase the apparatus size and cost. In contrast to these cases, using differential values as contrast values can more preferably acquire an ultrasonic image with optimized resolution easily at a low cost.

[0067] FIG. 12 is a view exemplarily showing an ultrasonic image (a) obtained by the conventional technique (i.e., an ultrasonic image acquired without any correction of the difference between the set sound velocity used for the calculation of a reception delay time and the actual in vivo sound velocity). FIG. 12 is a view exemplarily showing an ultrasonic image (b) acquired by correcting the difference between the set sound velocity used for the calculation of a reception delay time and the actual in vivo sound velocity by this resolution optimization processing. A comparison between the two ultrasonic images (a) and (b) will reveal that the targets within the circular frames in the ultrasonic images (b) are visualized with higher resolution as compared with the targets within the circular frames in the ultrasonic images (a).

[0068] In addition, this ultrasonic diagnosis apparatus can generate and display a color sound velocity map by resolution optimization processing. The operator can therefore visually recognize the structure of the visualization target slice and the distribution of components from the viewpoint of velocity by using the color sound velocity map. In addition, a calculation technique for optimal sound velocities can be selected on the basis of the observation result on the color sound velocity map.

[0069] The present invention is not limited to the above embodiment, and constituent elements can be modified and embodied in the execution stage within the spirit and scope of the invention. The following are concrete modifications.

(1) Each function according to the embodiment can also be implemented by installing programs for executing the corresponding processing in a computer such as a workstation and unarchiving them in a memory. In this case, the programs which can cause

the computer to execute the corresponding techniques can be distributed by being stored in recording media such as magnetic disks (floppy (registered trademark) disks, hard disks, and the like), optical disks (CD-ROMs, DVDs, and the like), and semiconductor memories.

(2) In the above embodiment, the size of each small area is not specifically limited. If, for example, each small area is set as an area for each depth as shown in FIG. 8, acquiring an optimal sound velocity for each small area is equivalent to acquiring an optimal sound velocity for each depth. In addition, making small areas correspond to the respective pixels can acquire optimal velocities unique to all the points on a visualization target slice.

(3) The above embodiment has exemplified the case in which a visualization target is a slice. However, the present invention is not limited to this. This resolution optimization function can also be used even when a three-dimensional area is to be visualized. In such a case, it suffices to perform the above resolution optimization processing for each of slices constituting a three-dimensional area as a visualization target or segment a three-dimensional area as a visualization target into small three-dimensional areas and perform the above resolution optimization processing for each small area.

[0070] In addition, various inventions can be formed by proper combinations of a plurality of constituent elements disclosed in the above embodiments. For example, several constituent elements may be omitted from all the constituent elements disclosed in the above embodiment. Furthermore, constituent elements in different embodiments may be properly combined.

[0071] It is explicitly stated that all features disclosed in the description and/or the claims are intended to be disclosed separately and independently from each other for the purpose of original disclosure as well as for the purpose of restricting the claimed invention independent of the composition of the features in the embodiments and/or the claims. It is explicitly stated that all value ranges or indications of groups of entities disclose every possible intermediate value or intermediate entity for the purpose of original disclosure as well as for the purpose of restricting the claimed invention, in particular as limits of value ranges.

Claims

1. An ultrasonic imaging apparatus (1) comprising:

a storage unit (35) adapted to store a plurality of ultrasonic data acquired by using reception delay addition processing, based on different sound velocities, for a visualization target slice or a subject;

a contrast value acquisition unit (170) adapted to segment said each ultrasonic data into a plurality of small areas and to acquire a contrast value for each of different sound velocities for each of the small areas;

a determination unit (174) adapted to determine an optimal sound velocity to be set in execution of an ultrasonic scan on the visualization target slice by using a contrast value for each of different sound velocities for said each small area, and by using the sound velocity at which the contrast value in each small area is maximized; **characterized in that**

the contrast value acquisition unit (170) is adapted to exclude areas from being subjected to a sound velocity optimization out of the plurality of small areas based on the contrast value falling outside a predetermined range.

2. An apparatus (1) according to claim 1, **characterized in that** the contrast value acquisition unit (170) is adapted to acquire a contrast value for each of different sound velocities for said each small area on the basis of a differential value in said each small area.

3. An apparatus (1) according to claim 1, **characterized in that** the contrast value acquisition unit (170) is adapted to acquire a contrast value for each of different sound velocities for said each small area on the basis of one of an amplitude value and a difference value between a maximum value and a minimum value of luminance values in said each small area.

4. An apparatus (1) according to any of claims 1 to 3, **characterized in that** the determination unit (174) is adapted to determine a maximum sound velocity in said each small area which maximizes a contrast values as an optimal sound velocity to be set when an ultrasonic can is performed on the visualization target slice.

5. An apparatus (1) according to any of claims 1 to 3, **characterized in that** the determination unit (174) is adapted to determine a maximum sound velocity in said each small area which maximizes a contrast value, and to determine an average velocity for each depth, which is obtained by using a maximum sound velocity in said each small area, as an optimal sound velocity when an ultrasonic scan is performed on the visualization target slice.

6. An apparatus (1) according to any of claims 1 to 3, **characterized in that** the determination unit (174) is adapted to determine a maximum sound velocity in said each small area which maximizes a contrast value, and to determine an average velocity on the

visualization target slice, which is obtained by using a maximum sound velocity in said each small area, as an optimal sound velocity when an ultrasonic scan is performed on the visualization target slice.

7. An apparatus (1) according to any of claims 1 to 6, **characterized by** further comprising:

a map generating unit (170, 172) adapted to generate a color velocity map by assigning a predetermined color to said each small area in accordance with a maximum sound velocity which maximizes a contrast value; and a display unit (27) adapted to display the color velocity map in a predetermined form.

8. An apparatus (1) according to any of claims 1 to 7, **characterized by** further comprising a reception unit (13) adapted to perform reception delay addition for an echo signal, which is received by each ultrasonic transducer by ultrasonic transmission/reception, by using the optimal velocity.

9. An apparatus (1) according to any of claims 1 to 8, **characterized in that** the contrast value acquisition unit (170) is adapted to segment said plurality of ultrasonic data into said plurality of small areas along a horizontal direction which is a direction perpendicular to an ultrasonic scanning line, and to acquire a contrast value for said each sound velocity for each depth corresponding to said each small area.

10. The apparatus according to claim 1, wherein an evaluation of the contrast value is performed in an azimuth direction normally crossing a beam.

11. The apparatus according to claim 1, wherein an evaluation of the contrast value and a calculation of the velocities to be set are performed in each of a plurality of depths in each of the small areas, and the average value of the velocities to be set, obtained for each depth, is determined as the velocity to be set for each respective small area belonging to the depth.

12. An ultrasonic velocity optimization method comprising:

segmenting a plurality of ultrasonic data acquired by using reception delay addition processing for a visualization target slice of a subject on the basis of different sound velocities into a plurality of small areas;

acquiring a contrast value for each of different sound velocities for said each small area; and determining an optimal sound velocity to be set in execution of an ultrasonic scan on the visualization target slice by using a contrast value for

each of different sound velocities for said each small area;

characterized by

excluding areas from being subjected to a sound velocity optimisation out of the plurality of small areas based on the contrast value falling outside a predetermined range.

13. A method according to claim 12, **characterized in that** in acquiring a contrast value, a contrast value for each of different sound velocities is acquired for said each small area on the basis of one of differential value in said each small area.

14. A method according to claim 12, **characterized in that** in acquiring a contrast value, a contrast value for each of different sound velocities is acquired for said each small area on the basis of one of an amplitude value and a difference value between a maximum value and a minimum value of luminance values in said each small area.

15. A method apparatus according to any of claims 10 to 14, **characterized in that** in determining, a maximum sound velocity in said each small area which maximizes a contrast value is determined as an optimal sound velocity to be set when an ultrasonic scan is performed on the visualization target slice.

16. A method according to any of claims 10 to 14, **characterized in that** in determining, a maximum sound velocity is determined in said each small area which maximizes a contrast value, and an average velocity for each depth which is obtained by using a maximum sound velocity in said each small area is determined as an optimal sound velocity to be set when an ultrasonic scan is performed on the visualization target slice.

17. A method according to any of claims 10 to 14, **characterized in that** in the determining, a maximum sound velocity in said each small area which maximizes a contrast value is determined, and an average velocity on the visualization target slice which is obtained by using a maximum sound velocity in said each small area is determined as an optimal sound velocity to be set when an ultrasonic scan is performed on the visualization target slice.

18. A method according to any of claims 10 to 17, **characterized by** further comprising:

generating a color velocity map by assigning a predetermined color to said each small area in accordance with a maximum sound velocity which maximizes a contrast value; and displaying the color velocity map in a predeter-

mined form.

19. A method according to any of claims 10 to 18, **characterized by** further comprising performing reception delay addition for an echo signal, which is received by each ultrasonic transducer by ultrasonic transmission/reception, by using the optimal velocity.
20. A method according to any of claims 10 to 19, **characterized in that** in acquiring a contrast value, said plurality of ultrasonic data are segmented into said plurality of small areas along a horizontal direction which is a direction perpendicular to an ultrasonic scanning line, and a contrast value is acquired for said each sound velocity for each depth corresponding to said each small area.

Patentansprüche

1. Ultraschallbildgebungsvorrichtung (1), enthaltend:

eine Speichereinheit (35), die angepasst ist zum Speichern einer Vielzahl von Ultraschalldaten, die erfasst werden durch Verwenden einer Empfangungsverzögerungsadditionsverarbeitung, basierend auf unterschiedlichen Schallgeschwindigkeiten für einen Visualisierungszielschnitt eines Subjekts;

eine Kontrastwerterfassungseinheit (170), die angepasst ist zum Segmentieren der jeweiligen Ultraschalldaten in eine Vielzahl von kleinen Bereichen und zum Erfassen eines Kontrastwerts für jede der unterschiedlichen Schallgeschwindigkeiten für jeden der kleinen Bereiche;

eine Bestimmungseinheit (174), die angepasst ist zum Bestimmen einer optimalen Schallgeschwindigkeit, die bei der Ausführung eines Ultraschallscans für den Visualisierungszielschnitt einzustellen ist, indem ein Kontrastwert für jede der unterschiedlichen Schallgeschwindigkeiten für den jeweiligen kleinen Bereich verwendet wird, und indem die Schallgeschwindigkeit verwendet wird, bei der der Kontrastwert in jedem kleinen Bereich ein Maximum ist;

dadurch gekennzeichnet, dass

die Kontrastwerterfassungseinheit (170) angepasst ist Bereiche davor auszuschließen einer Schallgeschwindigkeitsoptimierung unterworfen zu werden, von der Vielzahl von kleinen Bereichen, basierend auf dem Kontrastwert, der außerhalb eines vorbestimmten Bereichs liegt.

2. Vorrichtung (1) nach Anspruch 1, **dadurch gekennzeichnet, dass** die Kontrastwerterfassungseinheit (170) angepasst ist zum Erfassen eines Kontrastwerts für jede der

unterschiedlichen Schallgeschwindigkeiten für jeden jeweiligen kleinen Bereich basierend auf einem Differenzwert in dem jeweiligen kleinen Bereich.

3. Vorrichtung (1) nach Anspruch 1, **dadurch gekennzeichnet, dass**

die Kontrastwerterfassungseinheit (170) angepasst ist zum Erfassen eines Kontrastwerts für jede der unterschiedlichen Schallgeschwindigkeiten für den jeweiligen kleinen Bereich basierend auf einem von einem Amplitudenwert und einem Differenzwert zwischen einem maximalen Wert und einem minimalen Wert von Helligkeitswerten in dem jeweiligen kleinen Bereich.

4. Vorrichtung (1) nach einem der Ansprüche 1 bis 3, **dadurch gekennzeichnet, dass**

die Bestimmungseinheit (174) angepasst ist zum Bestimmen einer maximalen Schallgeschwindigkeit in dem jeweiligen kleinen Bereich, die Kontrastwerte maximiert, als eine optimale Schallgeschwindigkeit, die einzustellen ist, wenn eine Ultraschallabtastung für den Visualisierungszielschnitt durchgeführt wird.

5. Vorrichtung (1) nach einem der Ansprüche 1 bis 3, **dadurch gekennzeichnet, dass**

die Bestimmungseinheit (174) angepasst ist zum Bestimmen einer maximalen Schallgeschwindigkeit in dem jeweiligen kleinen Bereich, die einen Kontrastwert maximiert, und zum Bestimmen einer durchschnittlichen Geschwindigkeit für jede Tiefe, die erlangt wird, indem eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich als eine optimale Schallgeschwindigkeit verwendet wird, wenn eine Ultraschallabtastung für den Visualisierungszielschnitt durchgeführt wird.

6. Vorrichtung (1) nach einem der Ansprüche 1 bis 3, **dadurch gekennzeichnet, dass**

die Bestimmungseinheit (174) angepasst ist zum Bestimmen einer maximalen Schallgeschwindigkeit in dem jeweiligen kleinen Bereich, die einen Kontrastwert maximiert, und zum Bestimmen einer durchschnittlichen Geschwindigkeit für den Visualisierungszielschnitt, die erlangt wird, indem eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich als eine optimale Schallgeschwindigkeit verwendet wird, wenn eine Ultraschallabtastung für den Visualisierungszielschnitt durchgeführt wird.

7. Vorrichtung (1) nach einem der Ansprüche 1 bis 6, ferner **gekennzeichnet durch:**

eine Kartenerzeugungseinheit (170, 172), die angepasst ist zum Erzeugen einer Farbgeschwindigkeitskarte, indem eine vorbestimmte Farbe zu dem jeweiligen kleinen Bereich zugeordnet wird gemäß einer maximalen Schallge-

- schwindigkeit, die einen Kontrastwert maximiert; und
eine Anzeigeneinheit (27), die angepasst ist zum Anzeigen der Farbgeschwindigkeitskarte in einer vorbestimmten Form.
8. Vorrichtung (1) nach einem der Ansprüche 1 bis 7, ferner **gekennzeichnet durch** eine Empfangseinheit (13), die angepasst ist zum Durchführen einer Empfangsverzögerungsaddition für ein Echosignal, das **durch** Ultraschall-Sendung/Empfang **durch** jeden Ultraschalltransducer empfangen wird, indem die optimale Geschwindigkeit verwendet wird.
9. Vorrichtung (1) nach einem der Ansprüche 1 bis 8, **dadurch gekennzeichnet, dass** die Kontrastwerterfassungseinheit (170) angepasst ist zum Segmentieren der Vielzahl von Ultraschall-daten in die Vielzahl von kleinen Bereichen entlang einer horizontalen Richtung, die eine Richtung senkrecht zu einer Ultraschallabtastzeile ist, und zum Erfassen eines Kontrastwerts für die jeweilige Schallgeschwindigkeit für jede Tiefe, die dem jeweiligen kleinen Bereich entspricht.
10. Vorrichtung nach Anspruch 1, bei der eine Evaluierung des Kontrastwerts in einer Azimut-Richtung durchgeführt wird, die einen Strahl senkrecht kreuzt.
11. Vorrichtung nach Anspruch 1, bei der eine Evaluierung des Kontrastwerts und eine Berechnung der einzustellenden Geschwindigkeiten in jeder von einer Vielzahl von Tiefen in jedem der kleinen Bereiche durchgeführt wird, und der Durchschnittswert der einzustellenden Geschwindigkeiten, der für jede Tiefe erlangt wird, bestimmt wird als die für jeden entsprechenden kleinen Bereich, der zu der Tiefe gehört, einzustellende Geschwindigkeit.
12. Ultraschallgeschwindigkeitsoptimierungsverfahren, mit:
- Segmentieren einer Vielzahl von Ultraschall-daten, die durch Verwendung einer Empfangsverzögerungsadditionsverarbeitung für einen Visualisierungszielschnitt eines Subjekts basierend auf unterschiedlichen Schallgeschwindigkeiten erlangt werden, in eine Vielzahl von kleinen Bereichen;
Erfassen eines Kontrastwerts für jede der unterschiedlichen Schallgeschwindigkeiten für den jeweiligen kleinen Bereich; und
Bestimmen einer optimalen einzustellenden Schallgeschwindigkeit bei der Ausführung einer Ultraschallabtastung für den Visualisierungszielschnitt, indem ein Kontrastwert für jede der unterschiedlichen Schallgeschwindigkeiten für den jeweiligen kleinen Bereich verwendet wird; **gekennzeichnet durch**, Bereiche davor auszuschließen einer Schallgeschwindigkeitsoptimierung der Vielzahl von kleinen Bereichen basierend auf dem Kontrastwert unterzogen zu werden, der außerhalb eines vorbestimmten Bereichs liegt.
13. Verfahren nach Anspruch 12, **dadurch gekennzeichnet, dass** bei dem Erfassen eines Kontrastwerts ein Kontrastwert für den jeweiligen kleinen Bereich basierend auf einem Differenzwert in dem jeweiligen kleinen Bereich erfasst wird.
14. Verfahren nach Anspruch 12, **dadurch gekennzeichnet, dass** bei dem Erfassen eines Kontrastwerts ein Kontrastwert für jede der unterschiedlichen Schallgeschwindigkeiten erfasst wird für den jeweiligen kleinen Bereich basierend auf einem von einem Amplitudenwert und einem Differenzwert zwischen einem maximalen Wert und einem minimalen Wert von Helligkeitswerten in dem jeweiligen kleinen Bereich.
15. Verfahrensvorrichtung nach einem der Ansprüche 10 bis 14, **dadurch gekennzeichnet, dass** bei dem Bestimmen eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich, die einen Kontrastwert maximiert, bestimmt wird als eine optimale einzustellende Geschwindigkeit, wenn eine Ultraschallabtastung für den Visualisierungszielschnitt durchgeführt wird.
16. Verfahren nach einem der Ansprüche 10 bis 14, **dadurch gekennzeichnet, dass** bei dem Bestimmen eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich bestimmt wird, die einen Kontrastwert maximiert, und eine Durchschnittsgeschwindigkeit für jede Tiefe, erlangt wird, indem eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich als eine optimale Schallgeschwindigkeit bestimmt wird, die einzustellen ist, wenn eine Ultraschallabtastung für den Visualisierungszielschnitt durchgeführt wird.
17. Verfahren nach einem der Ansprüche 10 bis 14, **dadurch gekennzeichnet, dass** bei dem Bestimmen eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich bestimmt wird, die einen Kontrastwert maximiert, und eine Durchschnittsgeschwindigkeit für den Visualisierungszielschnitt erlangt wird, indem eine maximale Schallgeschwindigkeit in dem jeweiligen kleinen Bereich als eine optimale Schallgeschwindigkeit bestimmt wird, die einzustellen ist, wenn eine Ultraschallabtastung für den Visualisierungszielschnitt durchgeführt wird.
18. Verfahren nach einem der Ansprüche 10 bis 17, fer-

ner **gekennzeichnet durch**:

Erzeugen einer Farbgeschwindigkeitskarte, indem eine vorbestimmte Farbe dem jeweiligen kleinen Bereich zugeordnet wird gemäß einer maximalen Schallgeschwindigkeit, die einen Kontrastwert maximiert; und
Anzeigen der Farbgeschwindigkeitsmarke in einer vorbestimmten Form.

19. Verfahren nach einem der Ansprüche 10 bis 18, **gekennzeichnet durch** ferner enthaltend ein Durchführen einer Empfangsverzögerungsaddition für ein Echosignal, das empfangen wird **durch** jeden Ultraschalltransducer **durch** Ultraschall-Sendung/Empfang, indem die optimale Geschwindigkeit verwendet wird.
20. Verfahren nach einem der Ansprüche 10 bis 19, **dadurch gekennzeichnet, dass** bei dem Erfassen eines Kontrastwerts die Vielzahl von Ultraschalldaten in die Vielzahl von kleinen Bereichen entlang einer horizontalen Richtung segmentiert werden, die eine Richtung senkrecht zu einer Ultraschallabtastzeile ist, und ein Kontrastwert für die jeweilige Schallgeschwindigkeit für jede Tiefe, die dem jeweiligen kleinen Bereich entspricht, erfasst wird.

Revendications

1. Appareil d'imagerie par ultrasons (1), comprenant :

une unité de mémorisation (35) qui mémorise plusieurs données ultrasonores acquises en utilisant un traitement d'addition de retard de réception, sur la base de vitesses du son différentes, pour une tranche cible de visualisation d'un sujet ;

une unité d'acquisition de valeur de contraste (170) adaptée pour segmenter chacune des données ultrasonores en plusieurs petites zones et pour acquérir une valeur de contraste pour chacune des différentes vitesses du son de chacune des petites zones, et

une unité de détermination (174) adaptée pour déterminer une vitesse du son optimale à fixer dans l'exécution d'un balayage d'ultrasons sur la tranche cible de visualisation en utilisant une valeur de contraste pour chacune des différentes vitesses du son pour chaque petite zone, et en utilisant la vitesse du son à laquelle la valeur de contraste dans chaque petite zone est maximisée ;

caractérisé en ce que

l'unité d'acquisition de valeur de contraste (170) est adaptée pour empêcher de soumettre à une optimisation de la vitesse du son des zones

autres que les plusieurs petites zones sur la base de la valeur de contraste tombant à l'extérieur d'une plage prédéterminée

2. Appareil (1) selon la revendication 1, **caractérisé en ce que** l'unité d'acquisition de valeur de contraste (170) est adaptée pour acquérir pour chaque petite zone une valeur de contraste pour chacune des vitesses du son différentes sur la base d'une valeur différentielle dans chaque petite zone.
3. Appareil (1) selon la revendication 1, **caractérisé en ce que** l'unité d'acquisition de valeur de contraste (170) est adaptée pour acquérir pour chaque petite zone une valeur de contraste pour chacune des vitesses du son différentes sur la base d'une parmi une valeur d'amplitude et une valeur de différence entre une valeur maximale et une valeur minimale des valeurs de luminance dans chaque petite zone.
4. Appareil (1) selon l'une quelconque des revendications 1 à 3, **caractérisé en ce que** l'unité de détermination (174) est adaptée pour déterminer dans chaque petite zone une vitesse du son maximale qui maximalise une valeur de contraste comme vitesse du son optimale à fixer quand un balayage d'ultrasons est effectué sur la tranche cible de visualisation.
5. Appareil (1) selon l'une quelconque des revendications 1 à 3, **caractérisé en ce que** l'unité de détermination (174) est adaptée pour déterminer dans chaque petite zone une vitesse du son maximale qui maximalise une valeur de contraste, et pour déterminer une vitesse moyenne pour chaque profondeur, qui est obtenue en utilisant une vitesse maximale du son dans chaque petite zone, en tant que vitesse de son optimale quand un balayage d'ultrasons est effectué sur la tranche cible de visualisation.
6. Appareil (1) selon l'une quelconque des revendications 1 à 3, **caractérisé en ce que** l'unité de détermination (174) est adaptée pour déterminer dans chaque petite zone une vitesse du son maximale qui maximalise une valeur de contraste, et pour déterminer une vitesse moyenne sur la tranche cible de visualisation, qui est obtenue en utilisant dans chaque petite zone une vitesse maximale du son, en tant que vitesse du son optimale quand un balayage d'ultrasons est effectué sur la tranche cible de visualisation.
7. Appareil (1) selon l'une quelconque des revendications 1 à 6, **caractérisé en ce qu'il** comprend en outre :

une unité de production de carte (170, 172) qui produit une carte de vitesse de couleur en affectant une couleur prédéterminée à chaque pe-

- tite zone, conformément à une vitesse maximale du son qui maximalise une valeur de contraste, et
une unité d'affichage (27) adaptée pour afficher la carte de vitesse de couleur sous une forme prédéterminée.
8. Appareil (1) selon l'une quelconque des revendications 1 à 7, **caractérisé en ce qu'il** comprend en outre une unité de réception (13) adaptée pour effectuer une addition de retard de réception pour un signal d'écho, qui est reçu par chaque transducteur à ultrasons par émission/réception d'ultrasons, en utilisant la vitesse optimale.
9. Appareil (1) selon l'une quelconque des revendications 1 à 8, **caractérisé en ce que** l'unité d'acquisition de valeur de contraste (170) est adaptée pour segmenter les plusieurs données ultrasonores en plusieurs petites zones le long d'une direction horizontale qui est une direction perpendiculaire à une ligne de balayage d'ultrasons, et pour acquérir une valeur de contraste pour chaque vitesse du son pour chaque profondeur correspondant à chaque petite zone.
10. Appareil selon la revendication 1, dans lequel une évaluation de la valeur de contraste est effectuée dans une direction azimutale recoupant normalement un faisceau.
11. Appareil selon la revendication 1, dans lequel une évaluation de la valeur de contraste et un calcul des vitesses à fixer sont effectués dans chacune de plusieurs profondeurs dans chacune des petites zones, et la valeur moyenne des vitesses à fixer, obtenue pour chaque profondeur, est déterminée comme la vitesse à fixer pour chaque petite zone respective appartenant à la profondeur.
12. Procédé d'optimisation de la vitesse d'ultrasons, consistant à :
- segmenter plusieurs données ultrasonores acquises en utilisant un traitement d'addition de retard de réception pour une tranche cible de visualisation d'un sujet sur la base de vitesses du son différentes dans plusieurs petites zones acquérir une valeur de contraste pour chacune des différentes vitesses du son pour chaque petite zone, et
déterminer une vitesse optimale du son à fixer dans l'exécution d'un balayage d'ultrasons sur la tranche cible de visualisation en utilisant une valeur de contraste pour chacune des différentes vitesses du son pour chaque petite zone ;
caractérisé par
empêcher de soumettre à une optimisation de
- la vitesse du son des zones autres que les plusieurs petites zones sur la base de la valeur de contraste tombant à l'extérieur d'une plage prédéterminée
13. Procédé selon la revendication 12, **caractérisé en ce que** dans l'acquisition d'une valeur de contraste, une valeur de contraste pour chacune des différentes vitesses du son est acquise pour chaque petite zone sur la base d'une valeur différentielle dans chaque petite zone.
14. Procédé selon la revendication 12, **caractérisé en ce que** dans l'acquisition d'une valeur de contraste, une valeur de contraste pour chacune des différentes vitesses du son est acquise pour chaque petite zone sur la base d'une valeur parmi une valeur d'amplitude et une valeur de différence entre une valeur maximale et une valeur minimale des valeurs de luminance dans chaque petite zone.
15. Appareil et Procédé selon l'une quelconque des revendications 10 à 14, **caractérisé en ce que** dans la détermination, dans chaque petite zone une vitesse maximale du son qui maximalise une valeur de contraste est déterminée comme vitesse optimale du son à fixer lorsqu'un balayage d'ultrasons est effectué sur la tranche de la cible de visualisation.
16. Procédé selon l'une quelconque des revendications 10 à 14, **caractérisé en ce que** dans la détermination, une vitesse du son maximale est déterminée dans chaque petite zone qui maximalise une valeur de contraste et une vitesse moyenne pour chaque profondeur qui est obtenue en utilisant une vitesse maximale du son dans chaque petite zone est déterminée comme vitesse du son optimale quand un balayage d'ultrasons est effectué sur la tranche cible de visualisation.
17. Procédé selon l'une quelconque des revendications 10 à 14, **caractérisé en ce que** dans la détermination, dans chaque petite zone une vitesse maximale du son qui maximalise la valeur de contraste est déterminée, et une vitesse moyenne sur la tranche cible de visualisation qui est obtenue en utilisant une vitesse maximale du son dans chaque petite zone est déterminée comme vitesse du son optimale lorsqu'un balayage d'ultrasons est effectué sur la tranche de la cible de visualisation.
18. Procédé selon l'une quelconque des revendications 10 à 17, **caractérisé en ce qu'il** comprend en outre :
- la production d'une carte de vitesse de couleur en affectant une couleur prédéterminée à chaque petite zone, conformément à une vitesse

maximale du son qui maximalise une valeur de contraste, et
l'affichage de la carte de vitesse de couleur sous une forme prédéterminée.

5

19. Procédé selon l'une quelconque des revendications 10 à 18, **caractérisé en ce qu'**il comprend en outre la réalisation de l'addition de retard de réception pour un signal d'écho, qui est reçu par chaque transducteur à ultrasons par émission/réception d'ultrasons, en utilisant la vitesse optimale.

10

20. Procédé selon l'une quelconque des revendications 10 à 19, **caractérisé en ce que** dans l'acquisition d'une valeur de contraste, les plusieurs données ultrasonores sont segmentées en plusieurs petites zones le long d'une direction horizontale qui est une direction perpendiculaire à une ligne de balayage d'ultrasons, et une valeur de contraste est acquise pour chaque vitesse du son pour chaque profondeur correspondant à chaque petite zone.

15

20

25

30

35

40

45

50

55

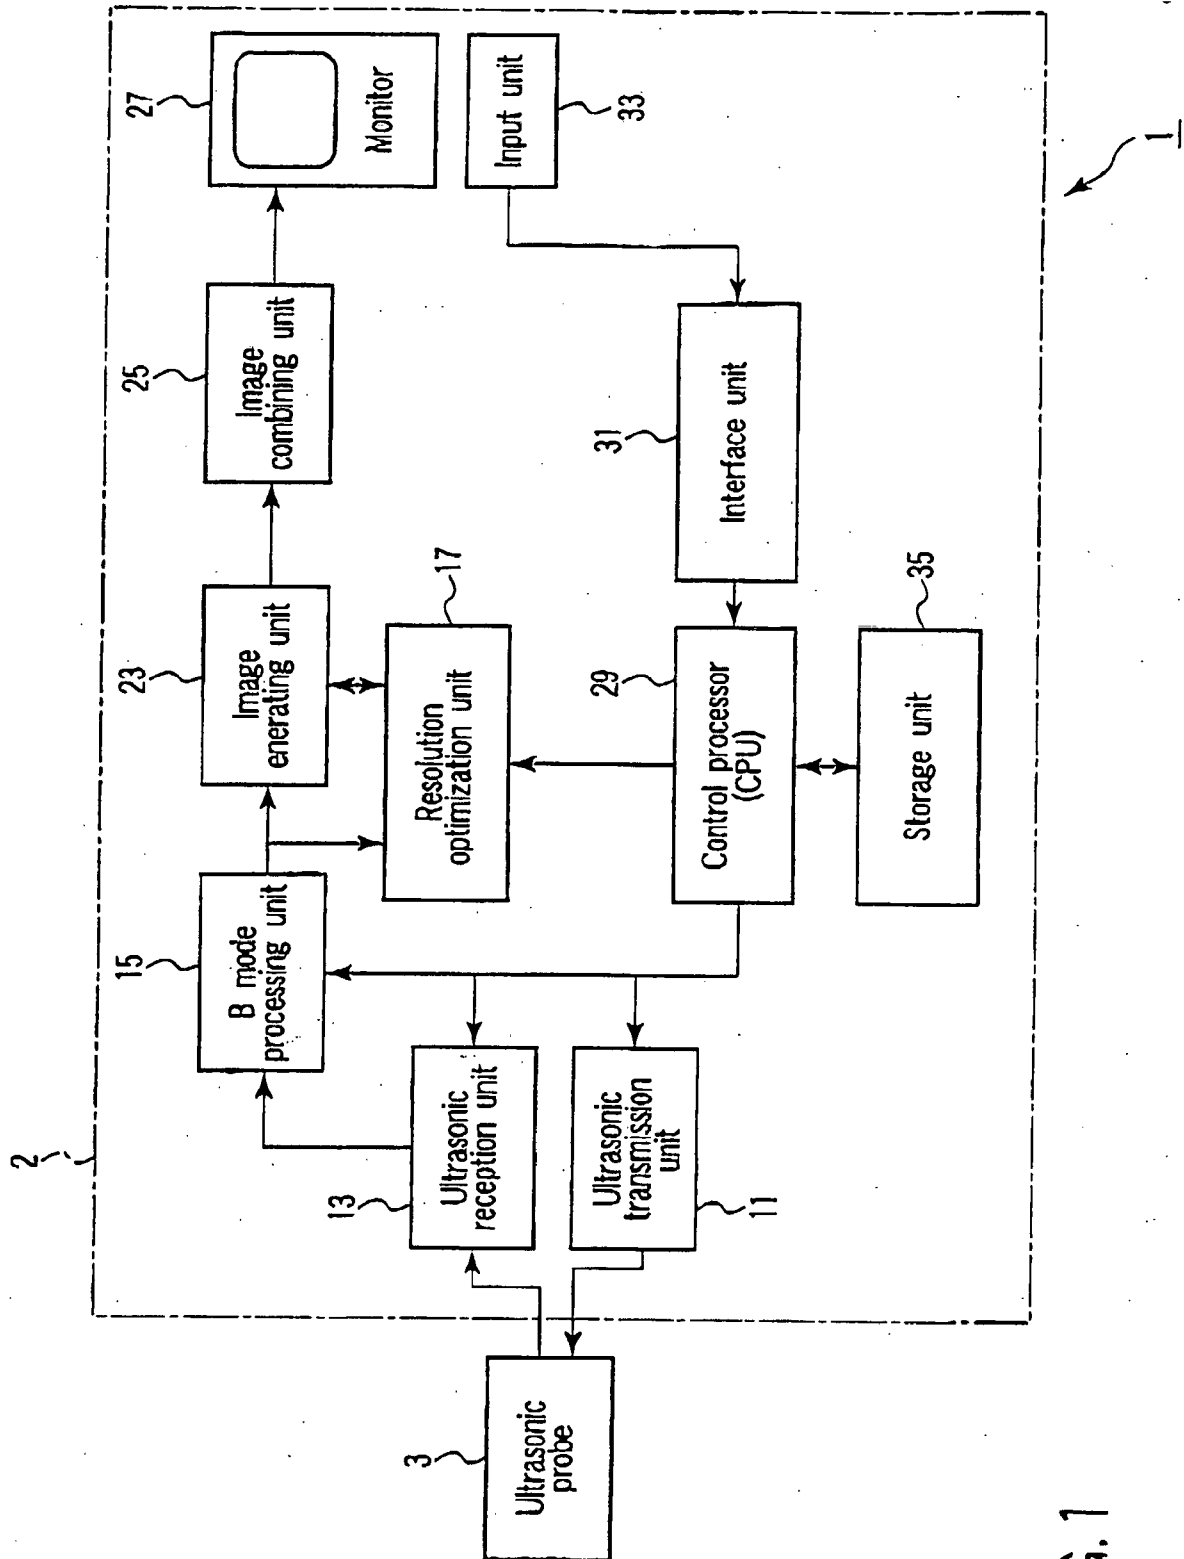


FIG. 1

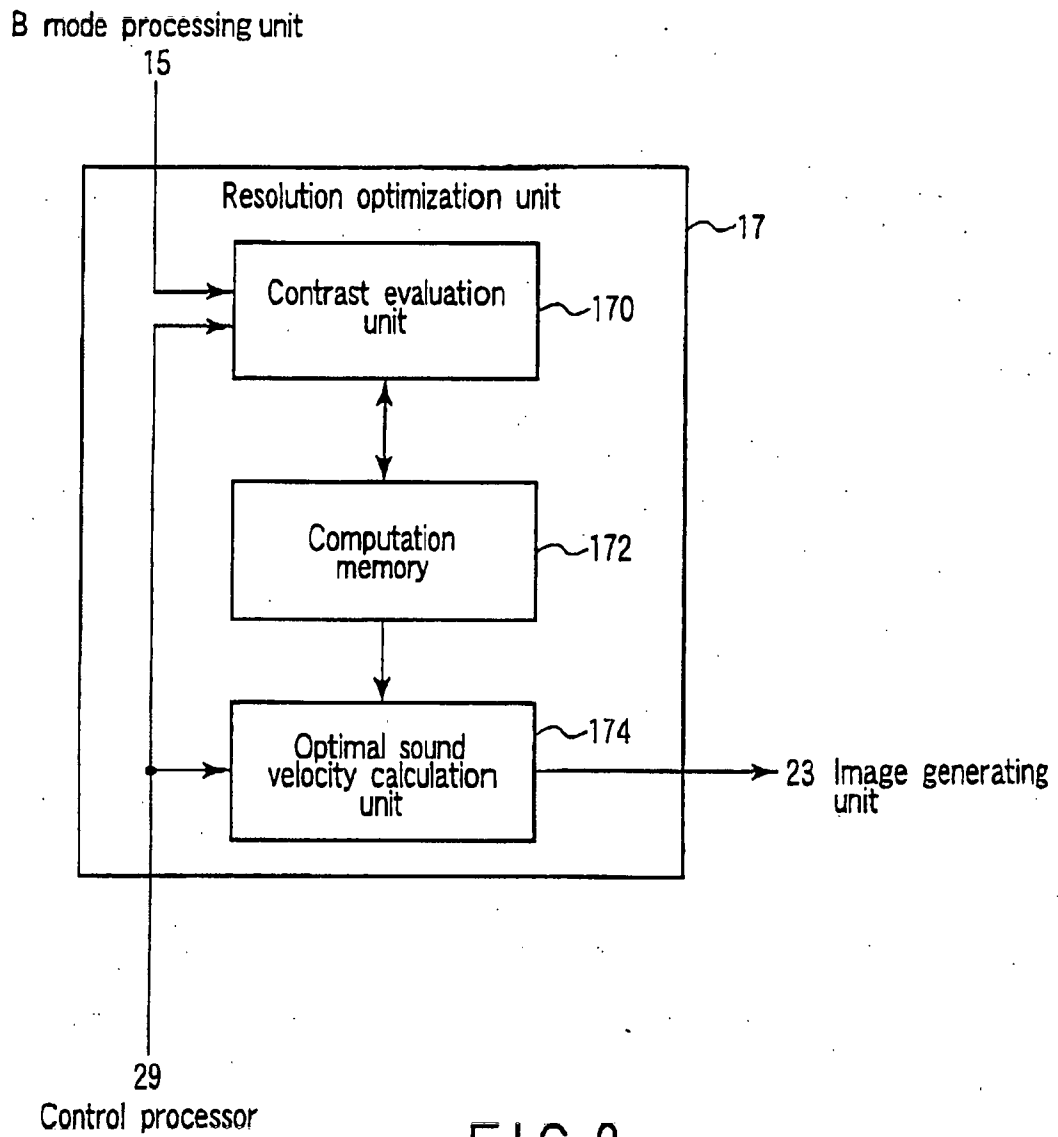


FIG. 2

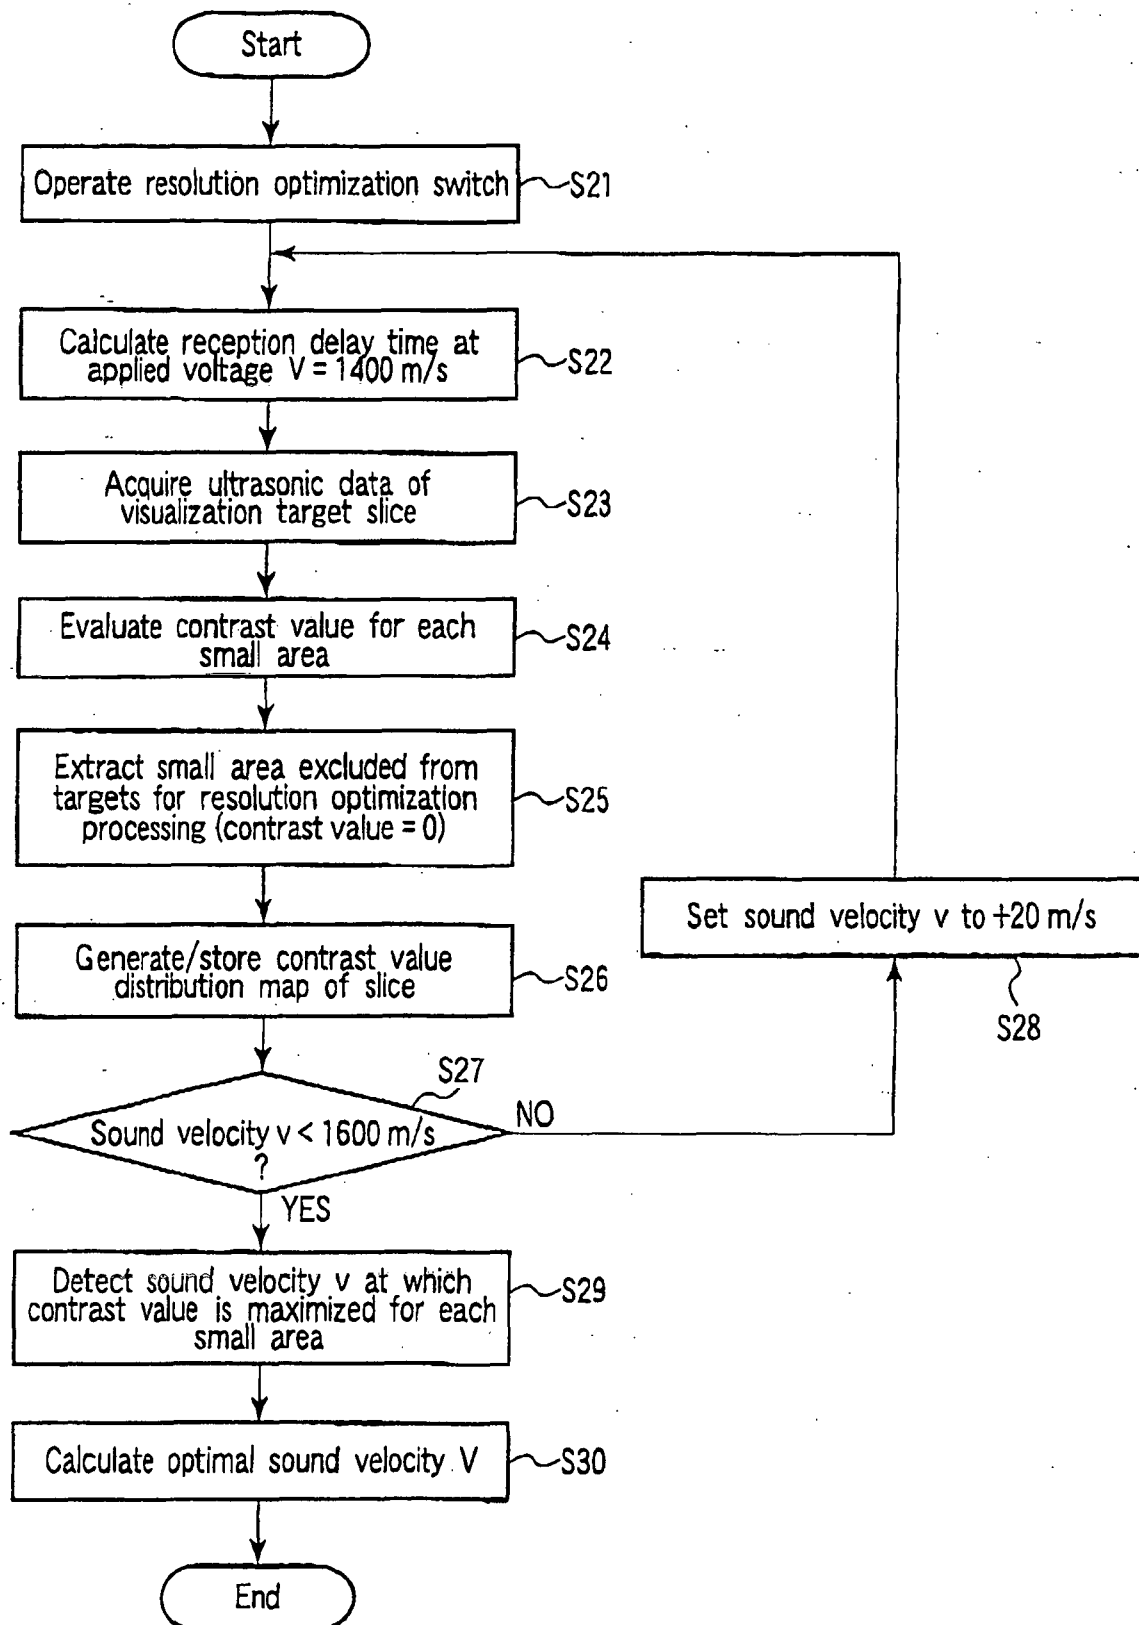


FIG. 3

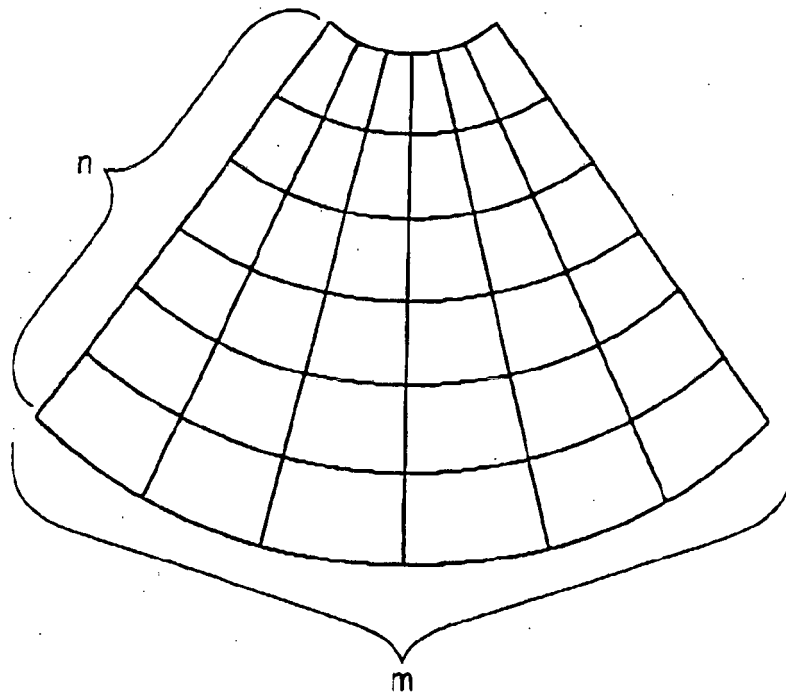


FIG. 4

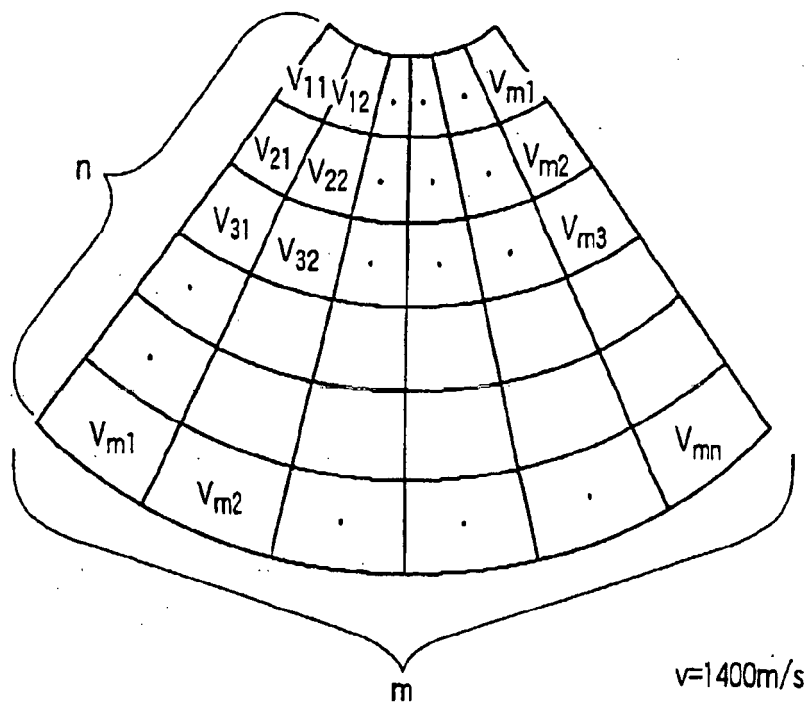


FIG. 5

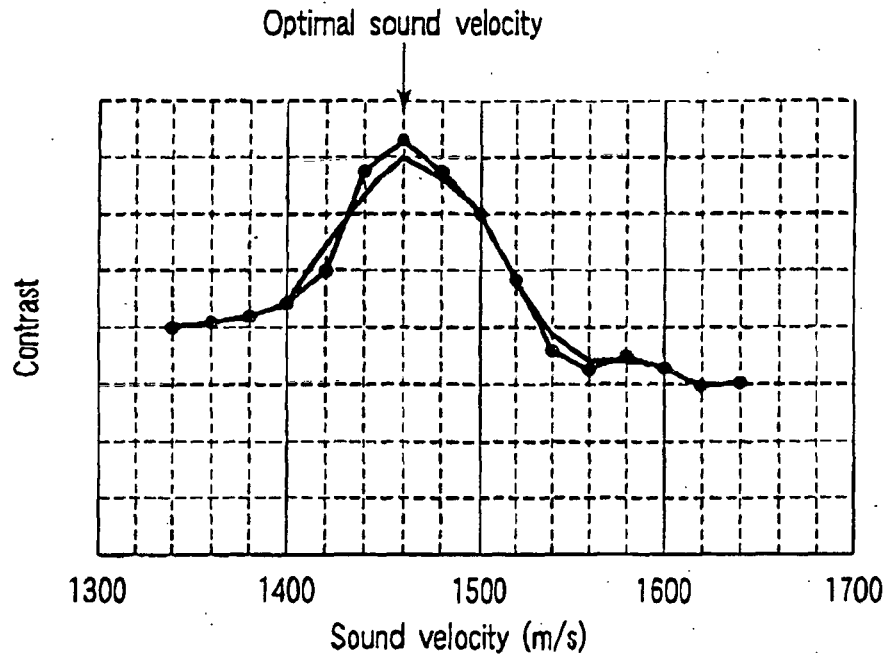


FIG. 6

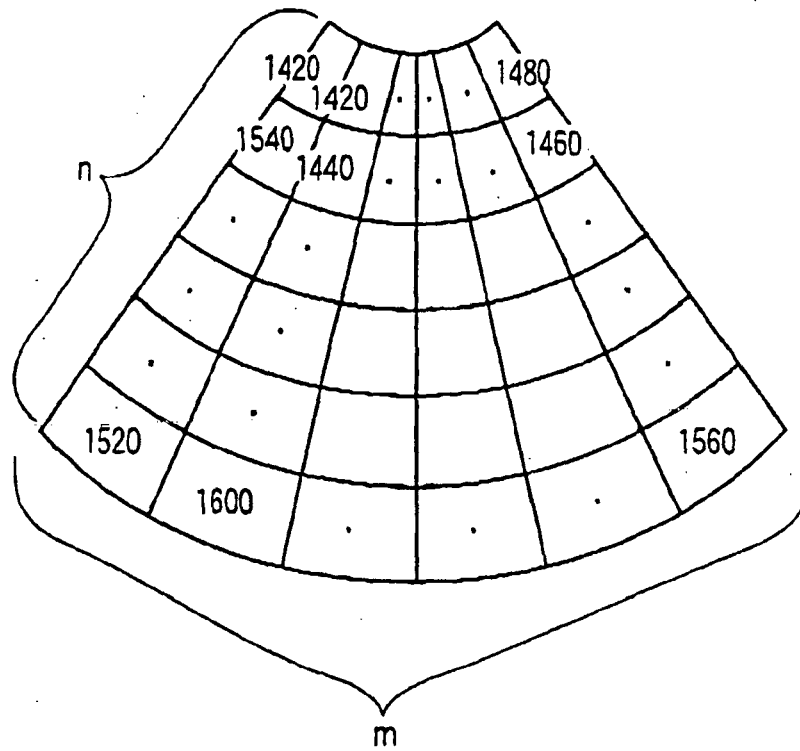


FIG. 7

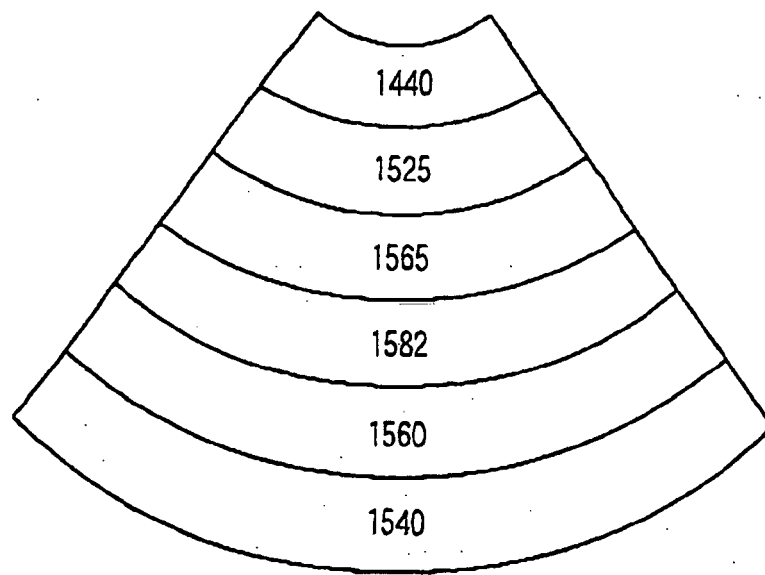


FIG. 8

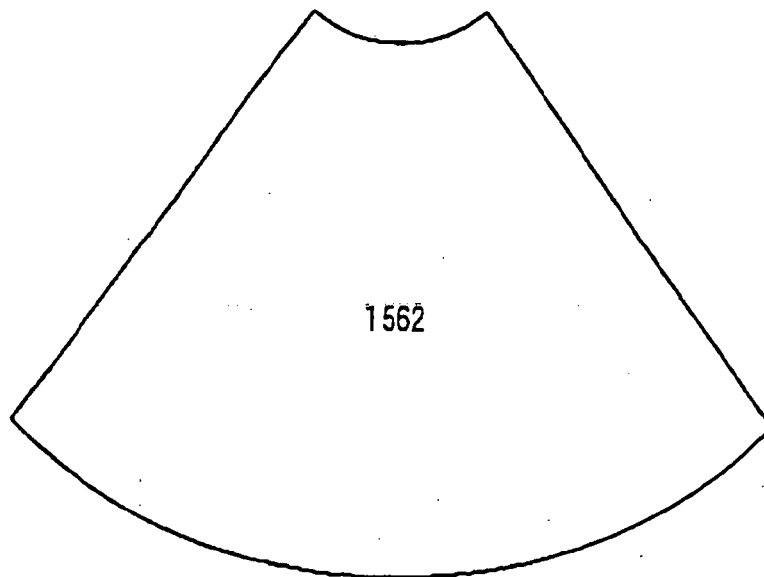


FIG. 9

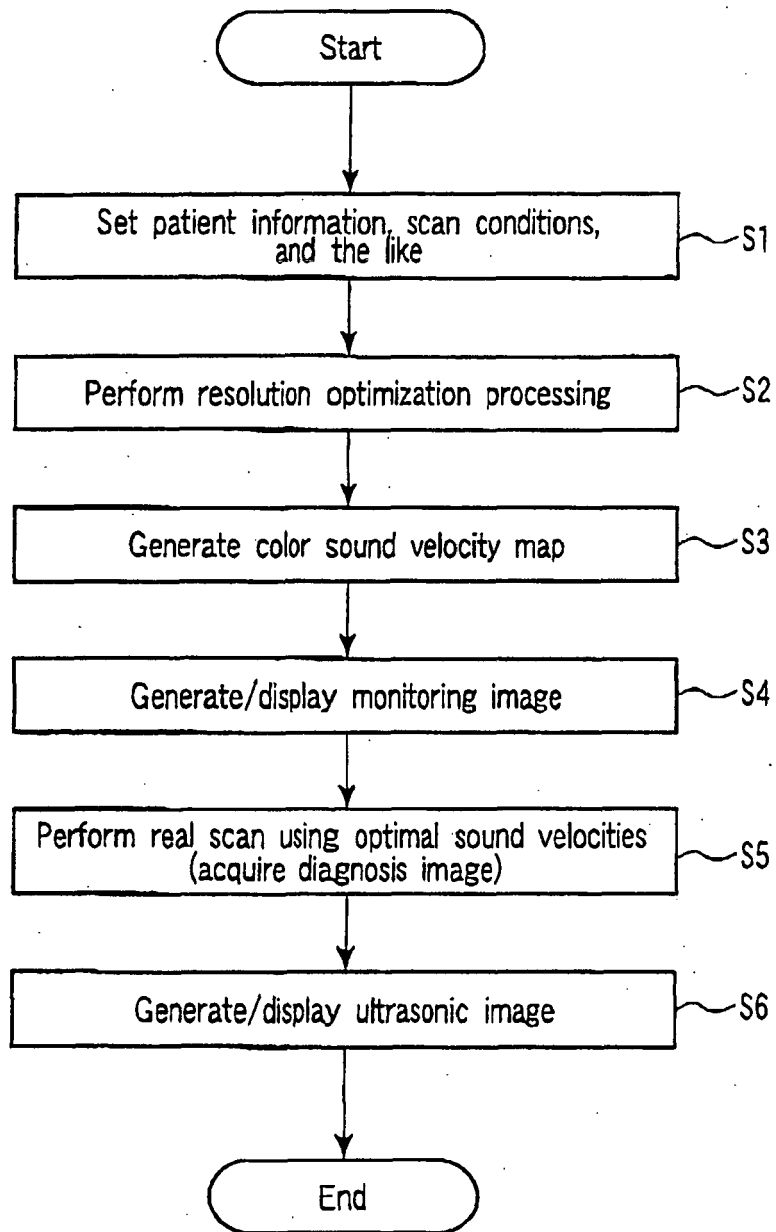


FIG. 10


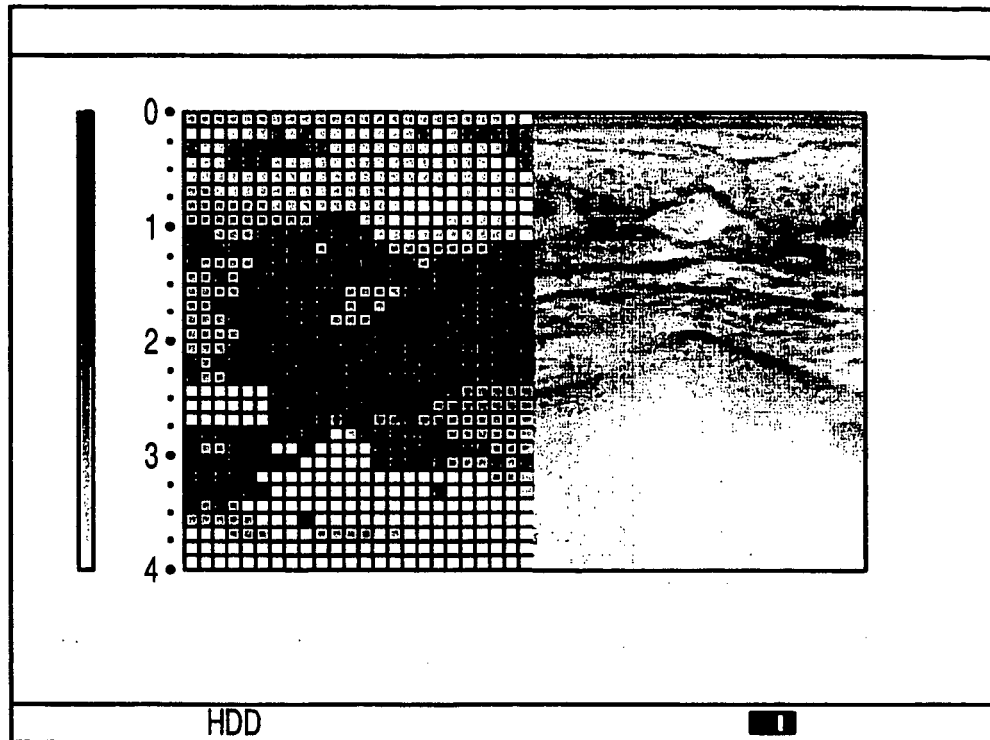


FIG. 11

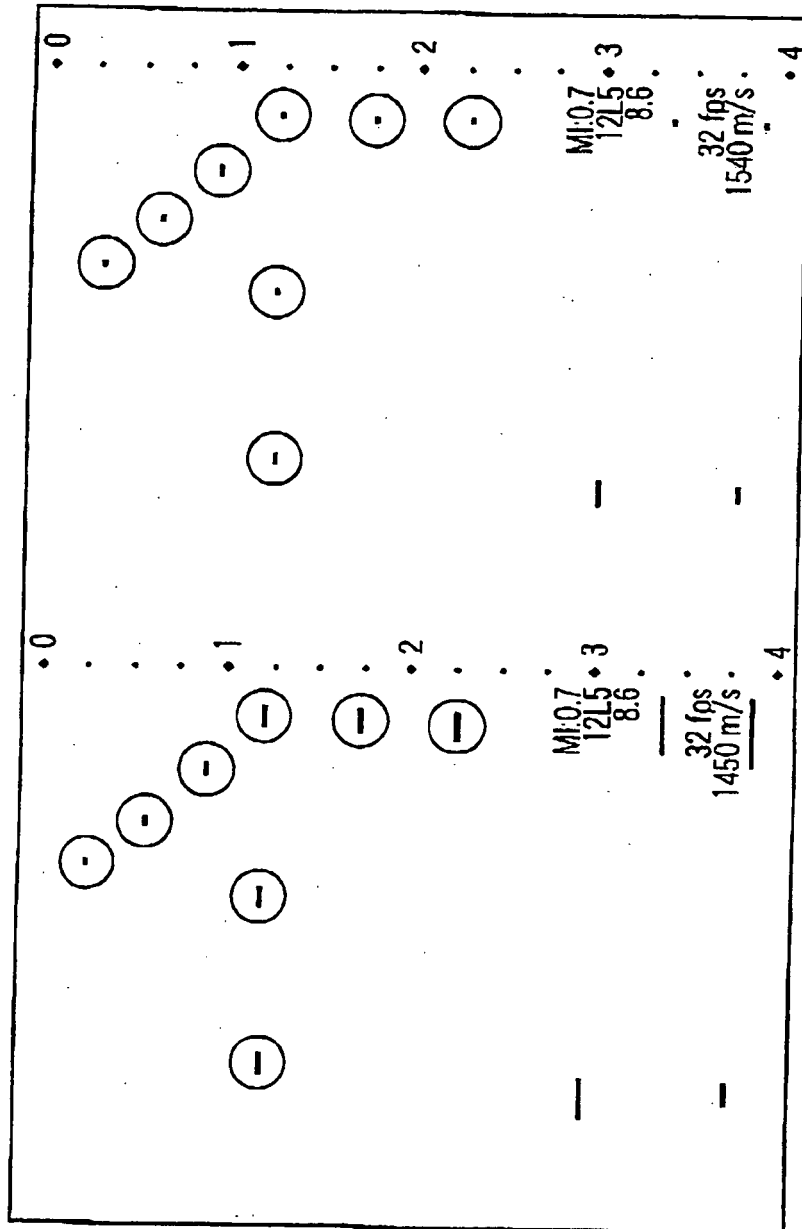

(a)

(b)

FIG.12

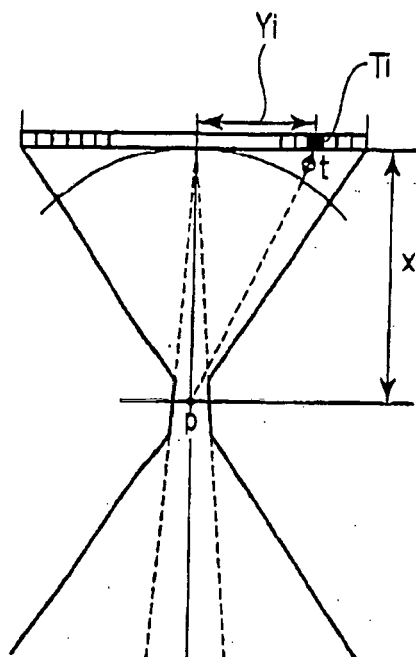


FIG. 13

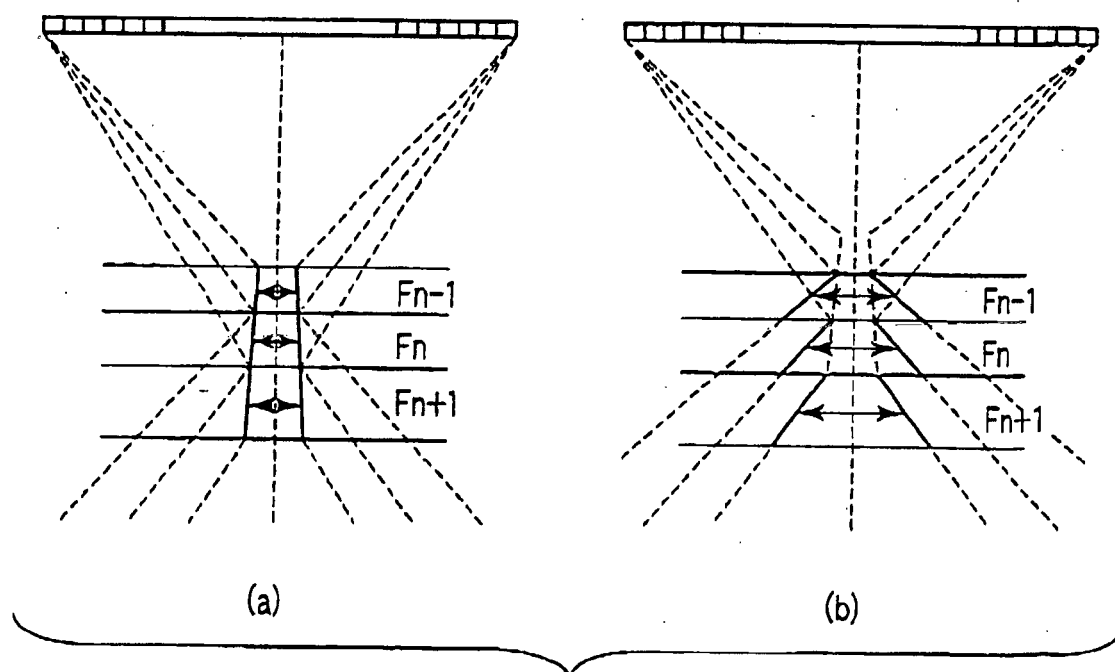


FIG. 14

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6305225 B1 [0010]
- US 5638820 A [0011]
- US 20030092990 A1 [0012]

专利名称(译)	超声成像设备和超声速度优化方法		
公开(公告)号	EP1974672B9	公开(公告)日	2014-04-16
申请号	EP2008005681	申请日	2008-03-26
[标]申请(专利权)人(译)	株式会社东芝 东芝医疗系统株式会社		
申请(专利权)人(译)	株式会社东芝 东芝医疗系统公司		
当前申请(专利权)人(译)	东芝医疗系统公司 株式会社东芝		
[标]发明人	KAKEE AKIHIRO		
发明人	KAKEE, AKIHIRO		
IPC分类号	A61B8/00 G01S7/52 G10K11/34		
CPC分类号	A61B8/00 A61B8/54 G01S7/52046 G01S7/52049 G01S15/8979		
代理机构(译)	KRAMER - HARSH - 施密特陈		
优先权	2007085918 2007-03-28 JP		
其他公开文献	EP1974672B1 EP1974672A3 EP1974672A2		
外部链接	Espacenet		

摘要(译)

分辨率优化单元 (17) 确定与扫描切片中的每个位置处的组织成分对应的最佳声速, 并且计算来自扫描切片A控制处理器中的每个位置的每个接收束的接收延迟时间等 (29) 通过使用利用最佳声速计算的接收延迟时间, 在扫描中执行延迟相加处理, 以获取实际用于诊断的超声图像。这可以校正用于计算接收延迟时间的设定声速与实际体内声速之间的差异, 并获得具有优化分辨率的超声图像。

$$\Delta t_i = [(x_i^2 + y_i^2)^{1/2} - x_i] / c$$