



(11) **EP 2 654 573 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention  
of the grant of the patent:  
**25.07.2018 Bulletin 2018/30**

(51) Int Cl.:  
**A61B 8/08 (2006.01) A61B 8/06 (2006.01)**

(21) Application number: **11811390.1**

(86) International application number:  
**PCT/IB2011/055744**

(22) Date of filing: **16.12.2011**

(87) International publication number:  
**WO 2012/085798 (28.06.2012 Gazette 2012/26)**

(54) **AUTOMATED IDENTIFICATION OF THE LOCATION OF A REGURGITANT ORIFICE OF A MITRAL VALVE IN AN ULTRASOUND IMAGE**

AUTOMATISIERTE IDENTIFIZIERUNG DER POSITION EINER REGURGITATIONSÖFFNUNG  
EINER MITRALKLAPPE AUF EINEM ULTRASCHALLBILD

IDENTIFICATION AUTOMATISÉE DE L'EMPLACEMENT D'UN ORIFICE DE RÉGURGITATION  
D'UNE VALVULE MITRALE DANS UNE IMAGE ULTRASONORE

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB  
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO  
PL PT RO RS SE SI SK SM TR**

• **YAP, Choon Hwai**  
**5656 AE Eindhoven (NL)**

(30) Priority: **23.12.2010 US 201061426669 P**  
**22.03.2011 US 201161466059 P**

(74) Representative: **Steffen, Thomas**  
**Philips Intellectual Property & Standards**  
**High Tech Campus 5**  
**5656 AE Eindhoven (NL)**

(43) Date of publication of application:  
**30.10.2013 Bulletin 2013/44**

(56) References cited:  
**DE-A1-102007 020 314 US-A- 4 913 159**  
**US-A- 5 062 427 US-A1- 2002 151 794**

(73) Proprietor: **Koninklijke Philips N.V.**  
**5656 AE Eindhoven (NL)**

• **P. M. VANDERVOORT ET AL: "Application of  
color Doppler flow mapping to calculate effective  
regurgitant orifice area. An in vitro study and  
initial clinical observations", CIRCULATION, vol.  
88, no. 3, 1 September 1993 (1993-09-01), pages  
1150-1156, XP055356056, US ISSN: 0009-7322,  
DOI: 10.1161/01.CIR.88.3.1150**

(72) Inventors:  
• **WEI, Qifeng**  
**5656 AE Eindhoven (NL)**  
• **THIELE, Karl Erhard**  
**5656 AE Eindhoven (NL)**  
• **YOGANATHAN, Ajit**  
**5656 AE Eindhoven (NL)**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

**[0001]** This application claims the benefit of U.S. provisional patent application serial number 61/426,669, filed December 23, 2010.

**[0002]** This invention relates to medical diagnostic ultrasound systems and, in particular, to the use of diagnostic ultrasonic imaging systems for the analysis of mitral regurgitation flow.

**[0003]** Regurgitant flow is a serious medical condition which required analysis and appropriate treatment. Just prior to the contraction of the left ventricle to pump blood into the body, the mitral valve must close completely so that the contraction will eject all of the blood flow into the aorta. If the valve does not close completely, some of the blood in the left ventricle will be ejected back into the left atria through the opening in the incompletely sealed valve. This backflow of blood, typically a small, momentary jet of blood flow squirting back through the incompletely closed valve leaflets, reduces the outflow of blood from the heart and hence the efficiency of each heart contraction. The heart must then pump more rapidly in order to supply the body with its necessary supply of nourishing blood flow. The heart is overworked due to its inefficiency, leading to heart failure.

**[0004]** Clinicians have used ultrasonic imaging for many years to try to detect regurgitant blood flow. Ultrasonic detection of valvular regurgitation was initially done by looking for the above-mentioned jet of blood in an ultrasound image of the left side of the heart. During the past twenty years observation of the jet has been facilitated by two dimensional (2D) colorflow Doppler imaging, in which the high speed and turbulence of the small jet of blood is detected by careful search for these abnormal local flow velocities near the leaking heart valve. But acquisition of the image plane in which the jet is most prevalent, coupled with heart and valve motion and blood flow turbulence in the vicinity of the mitral valve, as well as the momentary occurrence of the jet, pose challenges to this subjective approach. In recent years, in cases where the location of the jet can be observed ultrasonically, clinicians have used a technique called PISA, an acronym for Proximal Iso-velocity Surface Area, to try to quantify the regurgitant blood flow. In this method the suspect valve and the region inside the LV heart chamber and proximal to the valve are imaged by colorflow Doppler imaging. At the time of occurrence of the jet a flow convergence region (FCR) is formed in the proximal region as blood flow velocities in the region instantaneously accelerate toward the regurgitant orifice. This flow pattern results in aliasing in the colorflow image as the flow velocities momentarily exceed the velocity range used for the colorflow image. A colorflow image at this moment is captured and frozen on the display screen. A measurement is then made of the velocity  $v$  at the first aliasing line of the FCR, and a measurement is made of the distance  $r$  from the aliasing line to the presumed center of the valve orifice. These two measurements are then used

to compute the flow rate through the orifice using the expression  $Q_i = 2\pi r^2 v$ .

**[0005]** Several difficulties arise when conducting this procedure. One is that the greatest accuracy is obtained when the jet is captured in the colorflow image at its very peak. The duration of the jet during a heart cycle can be only 300-450 milliseconds, however, while a typical colorflow frame rate may be in the range of 10-20 frames per second. Thus it is probable that the time of acquisition of one of the colorflow image frames will not be the same as the exact moment when the jet is at its peak. The clinician can repeat the colorflow acquisition sequence for additional cardiac cycles, or can settle for the inaccuracy caused by making the measurements at other than the exact peak of the jet.

**[0006]** Another problem is that the center of the valve orifice is not easy to define in the colorflow image. The valve tissue produces large reflections of ultrasound and is moving rapidly as scanning takes place, and can appear as a bulky, blurred or indistinct mass in the image. Thus it is possible that the accuracy of the measurement  $r$  will be compromised by the inability to estimate the exact location of the orifice.

**[0007]** Yet a third problem is that the basic PISA technique is only a single, one-dimensional measurement. Only one velocity measurement is made and only a single radius  $r$  to the orifice is used in the computation. The method assumes that the rest of the blood flow in the FCR is behaving the same as that of the single measurement. Obviously, any inaccuracy in making the single measurement will yield an inaccurate result.

**[0008]** An extension of the basic PISA technique which attempts to cure these inaccuracies is to make multiple velocity measurements, as described in US 4,913,159 on the example of two Doppler images obtained along two perpendicular directions, around the arc delineating the outer boundary of the FCR in the two dimensional image. The distance  $r$  from each velocity measurement point to the orifice is measured, and the multiple measurements are used to calculate the flow rate  $Q_i$ . While the multiple measurements may prevent reliance on a single inaccurate measurement, another problem arises. The single measurement (1D) technique generally is done by aiming a center beam of the ultrasound probe through the apex of the heart and directly through the presumed regurgitant orifice, and making the velocity  $v$  and distance  $r$  measurements along this beam line. With the beam line thus aligned with this vector of the regurgitant flow, the velocity measured will be accurate and not affected by a non-zero Doppler angle. As is well known, ultrasound Doppler velocity measurements are affected by the angle between the flow direction and the ultrasound beam direction. Flow which is directly in line with the beam direction will be accurately measured, whereas flow which is at a non-zero angle to the beam direction will be reduced by the cosine of the angle. Flow which is orthogonal ( $90^\circ$ ) to the beam direction will produce no Doppler response. Hence, a Doppler velocity

measured by ultrasound must be corrected as a function of the angle between the flow vector and the beam direction in order to produce a more accurate velocity measurement. In the case of the 2D PISA technique, the additional velocity measurements along the FCR arc will be inaccurate due to variation of the angles between their flow vectors and the beam direction at each point where a velocity measurement is made. Thus, whereas multiple measurements can compensate for an error made in a single velocity measurement, the aggregate measurements will understate the flow rate due to the variation in the Doppler angles at each measurement point.

**[0009]** Yet a further problem inherent in the PISA technique is inaccuracy in knowing the precise location of the regurgitant orifice of the valve. As mentioned above, aliasing in the colorflow image is prevalent in the vicinity of the valve leak due to the sudden acceleration of the blood flow toward and through the orifice. The colorflow image is thus cluttered with the flash of aliasing colors in the Doppler image in the vicinity of the orifice. Additionally, the mitral valve plane is in motion during the heart contraction. As the accuracy of the PISA technique is reliant upon knowing the orifice location in order to measure the distance  $r$ , these impediments to precisely knowing the orifice location can result in an inaccurate  $r$  measurement and hence an inaccurate calculation of flow rate. Experiments have demonstrated that an error of as little as one millimeter in the orifice location can lead to a significant error in calculating the flow rate through the leak. Furthermore, it is known that many regurgitant valves do not have a single pinhole leak, but leak along a slit of imprecise valve closure. The assumption of a leak as being caused by a single pinhole through the valve may thus not be valid.

**[0010]** In scientific publication P. M. Vandervoort et al. "Application of Color Doppler Flow Mapping to Calculate Effective Regurgitant Orifice Area. An In Vitro Study and Initial Clinical Observations", Circulation, vol. 88, no. 3, pp. 1150-1156, American Heart Association Inc., 1993-09-01 (XP055356056), it is described a methodology to calculate regurgitant orifice area noninvasively using color Doppler echocardiography, based on the analysis of a proximal flow convergence zone.

**[0011]** Accordingly it is desirable to provide a method and apparatus for quantifying the flow rate and volume flow of mitral valve regurgitation which overcomes the above limitations of the PISA technique. It is an object of the present invention to accurately identify the precise location of the orifice of the valve regurgitation. It is a further object of the present invention to make a range of measurements which are unaffected by the Doppler angle at each measurement location. It is a further object of the present invention to be able to identify and quantify mitral valve regurgitation due not only to a single pinhole leak, but also due to a slit along the closure of the valve.

**[0012]** These objects are solved by the independent claim. Advantageous embodiments are defined in the dependent claims.

**[0013]** In accordance with the principles of the present invention, an ultrasonic diagnostic imaging system is described for quantifying regurgitant blood flow. An arcuate (two dimensional) or hemispherical (three dimensional) region of blood flow is delineated proximal to a presumed location of a mitral valve leak in an ultrasound image of the regurgitant valve. The inner boundary of the region is at or just beyond the aliasing region adjacent to the orifice of the leak, and the outer boundary of the region is outward from and concentric with the inner boundary. Initial assumptions are made as to the regurgitant flow, including the location of the regurgitant orifice. These assumptions are used to compute a model of the velocity field of the regurgitant flow. The parameters of the model are adjusted in accordance with the physics of ultrasound and/or settings of the ultrasound system to determine expected velocity vectors to be observed by the ultrasound system,  $V_{OBS}$ , in the delineated region. Velocity measurements are made by the ultrasound system within the delineated region, and the measured velocities are compared with the expected velocities. Differences between the measured and expected values are computed and, through non-linear curve-fitting, adjustments are made to one or more of the model values. The processed is iteratively repeated until the expected and measured values acceptably converge. The iteratively adjusted model parameters are used to produce a quantified measurement of the flow rate or the location of the leaking orifice in the valve.

**[0014]** In accordance with a further aspect of the present invention, an initially assumed location of the regurgitant orifice in the ultrasound image is automatically updated by the foregoing process to indicate the actual location of the orifice in the image. The clinician is thus shown a precise location of the regurgitant orifice despite the presence of image clutter in the vicinity of the mitral valve.

**[0015]** In accordance with yet another aspect of the present invention, the foregoing technique is repeated at multiple spatial locations along a mitral valve. The aggregate regurgitant flow measured at the spatial locations provides a measure of regurgitant flow due to a regurgitant leak which is a slit in the mitral valve closure rather than a single leaking pinhole orifice.

**[0016]** In accordance with a further aspect of the present invention, several wall filter characteristics are described which are preferred for an implementation of regurgitant flow measurement in accordance with the present invention, including a wall filter with a characteristic that peaks at intermediate flow velocities which are often found in a flow region proximal a regurgitant orifice.

**[0017]** In the drawings:

FIGURE 1 illustrates in block diagram form an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention. FIGURE 2 is a block diagram illustrating the functioning of the flow quantification processor of FIG-

FIGURE 1.

FIGURE 3 illustrates an ultrasound Doppler image of a regurgitant jet.

FIGURE 4 illustrates an ultrasound image with an initially assumed orifice location and an automatically indicated orifice location in accordance with the present invention.

FIGURE 5 illustrates a technique for quantifying the regurgitant flow of a slit along a valve in accordance with the present invention.

FIGURE 6 illustrates the response characteristic of a wall filter suitable for use in an ultrasound system of the present invention.

**[0018]** Referring first to FIGURE 1, an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention is shown in block diagram form. In FIGURE 1 a transducer array 10' is provided in an ultrasound probe 10 for transmitting ultrasonic waves and receiving echo information. The transducer array 10' is preferably a two dimensional array of transducer elements capable of scanning in three dimensions, for instance, in both elevation and azimuth about the location of the mitral valve, for 3D imaging. The transducer array is coupled to a microbeamformer 12 in the probe which controls transmission and reception of signals by the array elements. Microbeamformers are capable of at least partial beamforming of the signals received by groups or "patches" of transducer elements as described in US Pats. 5,997,479 (Savord et al.), 6,013,032 (Savord), and 6,623,432 (Powers et al.) The microbeamformer is coupled by the probe cable to a transmit/receive (T/R) switch 16 which switches between transmission and reception and protects the main beamformer 20 from high energy transmit signals. The transmission of ultrasonic beams from the transducer array 10 under control of the microbeamformer 12 is directed by the transmit controller 18 coupled to the T/R switch and the beamformer 20, which receives input from the user's operation of the user interface or control panel 38. One of the functions controlled by the transmit controller is the direction in which beams are steered. Beams may be steered straight ahead from (orthogonal to) the transducer array, or at different angles for a wider field of view.

**[0019]** The partially beamformed signals produced by the microbeamformer 12 are coupled to a main beamformer 20 where partially beamformed signals from the individual patches of elements are combined into a fully beamformed signal. For example, the main beamformer 20 may have 128 channels, each of which receives a partially beamformed signal from a patch of 12 transducer elements. In this way the signals received by over 1500 transducer elements of a two dimensional array can contribute efficiently to a single beamformed signal.

**[0020]** The beamformed signals are coupled to a signal processor 22. The signal processor 22 can process the received echo signals in various ways, such as bandpass filtering, decimation, I and Q component separation, and

harmonic signal separation which acts to separate linear and nonlinear signals so as to enable the identification of nonlinear echo signals returned from tissue and microbubbles. The signal processor may also perform additional signal enhancement such as speckle reduction, signal compounding, and noise elimination.

**[0021]** The processed signals are coupled to a B mode processor 26 and a Doppler processor 28. The B mode processor 26 employs amplitude detection for the imaging of structures in the body such as the tissue of the heart wall, the mitral valve, and blood cells. B mode images of structure of the body may be formed in either the harmonic mode or the fundamental mode or a combination of both as described in US Pat. 6,283,919 (Roundhill et al.) and US Pat. 6,458,083 (Jago et al.) The Doppler processor 28 processes temporally distinct signals from tissue and blood flow for the detection of the motion of substances such as the flow of blood cells in the image field. The Doppler processor typically includes a wall filter with parameters which may be set to pass and/or reject echoes returned from selected types of materials in the body. For instance, the wall filter can be set to have a passband characteristic which passes signal of relatively low amplitude from higher velocity materials while rejecting relatively strong signals from lower or zero velocity material. This passband characteristic will pass signals from flowing blood while rejecting signals from nearby stationary or slowly moving objects such as the wall of the heart. An inverse characteristic would pass signals from moving tissue of the heart while rejecting blood flow signals for what is referred to as tissue Doppler imaging, detecting and depicting the motion of tissue. The Doppler processor receives and processes a sequence of temporally discrete echo signals from different points in an image field, the sequence of echoes from a particular point referred to as an ensemble. An ensemble of echoes received in rapid succession over a relatively short interval can be used to estimate the Doppler shift frequency of flowing blood, with the correspondence of the Doppler frequency to velocity indicating the blood flow velocity. An ensemble of echoes received over a longer period of time is used to estimate the velocity of slower flowing blood or slowly moving tissue. For mitral regurgitation assessment of a rapidly occurring jet, short ensemble lengths (fewer samples) are generally employed so that a high acquisition frame rate can be realized. The Doppler shift  $\Delta f$  may be estimated by an equation of the form

$$\Delta f = \frac{2vf_0 \cos \theta}{c}$$

where  $f_0$  is the transmit frequency,  $c$  is the ultrasound propagation speed,  $v$  is velocity, and  $\theta$  is the angle between the beam direction and the direction of the blood flow.

**[0022]** The structural and motion signals produced by the B mode and Doppler processors are coupled to a scan converter 32 and a multiplanar reformatter 44. The scan converter arranges the echo signals in the spatial

relationship from which they were received in a desired image format. For instance, the scan converter may arrange the echo signal into a two dimensional (2D) sector-shaped format, or a pyramidal three dimensional (3D) image. The scan converter can overlay a B mode structural image with colors corresponding to motion at points in the image field corresponding with their Doppler-estimated velocities to produce a color Doppler image which depicts the motion of tissue and blood flow in the image field. The multiplanar reformatter will convert echoes which are received from points in a common plane in a volumetric region of the body into an ultrasonic image of that plane, as described in US Pat. 6,443,896 (Detmer). A volume renderer 42 converts the echo signals of a 3D data set into a projected 3D image as viewed from a given reference point as described in US Pat. 6,530,885 (Entrekin et al.) The 2D or 3D images are coupled from the scan converter 32, multiplanar reformatter 44, and volume renderer 42 to an image processor 30 for further enhancement, buffering and temporary storage for display on an image display 40.

**[0023]** In accordance with the principles of the present invention, blood flow velocity values produced by the Doppler processor 28 are coupled to a flow quantification processor 34. The flow quantification processor operates as described below to produce a measure of the flow rate through a regurgitant orifice, the volume flow through the orifice, and the spatial location of the orifice. The flow quantification processor may receive input from the user control panel 38, such as an initial estimate of the location of the orifice as described below. Output data from the flow quantification processor is coupled to a graphics processor 36 for the reproduction of output data from the processor with the image on the display 40. The graphics processor 36 can also generate graphic overlays for display with the ultrasound images. These graphic overlays can contain standard identifying information such as patient name, date and time of the image, imaging parameters, and the like. For these purposes the graphics processor receives input from the user interface 38, such as a typed patient name. The user interface is also coupled to the transmit controller 18 to control the generation of ultrasound signals from the transducer array 10' and hence the images produced by the transducer array and the ultrasound system. The user interface is also coupled to the multiplanar reformatter 44 for selection and control of a display of multiple multiplanar reformatted (MPR) images which may be used to quantify regurgitant flow in the MPR images in accordance with the present invention as described below.

**[0024]** FIGURE 2 describes the operation of the flow quantification processor of FIGURE 1. The processor is based upon a mathematical model of the flow velocity field at sample points within an inclusion zone as described below. In a 2D image embodiment the inclusion zone is preferably a curved strip delineated by two arcs centered on the regurgitant orifice location,  $\{x_o, y_o, z_o\}$ . In a 3D image embodiment the curved strip is of the form

of a hemispherical shell, as discussed in conjunction with FIGURE 3 below. In a preferred embodiment the model is a vector velocity model of the flow velocity field of the form

$$\vec{V}_{Model}(r) = \vec{n}_{rel} |V(r)|$$

or

$$\vec{V}_{Model}(r) = \frac{-\vec{r}}{\|\vec{r}\|} \circ |V(r)|$$

where  $|V(r)| = \vec{F}/2\pi r^2$  for the flow vector  $\vec{F}$ , and  $r$  is the distance from a point at  $(x, y, z)$  in three dimensional coordinates in the inclusion zone to the regurgitant orifice, and the orifice is located at coordinates  $\{x_o, y_o, z_o\}$  in three dimensional space. This means that the distance  $r$ , when expressed vectorially to indicate the direction to the orifice, is of the form

$$\vec{r} = \{x - x_o, y - y_o, z - z_o\}$$

In box 50 of FIGURE 2, the flow velocity of every point in the inclusion zone is modeled in this way. Initially the model can start with assumed or estimated values for the unknown parameters, including the flow  $\vec{F}$  and the  $\{x_o, y_o, z_o\}$  location of the regurgitant orifice. For instance, the model can start with parameters which are nominally characteristic of regurgitant flow. The user can enter parameters such as by indicating the presumed location of the regurgitant orifice in the ultrasound image. Or a known technique such as PISA can be used to calculate values used as the starting parameters for the flow velocity field.

**[0025]** The flow velocity field model approximates velocity vectors which would be accurate if the true physiologic velocity vectors were known. The velocity vectors approximated by the model are indicated at the output of box 50 as  $\sim V_{TRUE}$ . Box 52 then imposes some limits and adjustments to  $\sim V_{TRUE}$  due to practical factors such as the physics of ultrasound and operating parameters of the ultrasound system being used. The flow velocity field model is then adjusted or scaled to take these practical factors into account in consideration of the actual velocity values which would be observed by an ultrasound system. One of the practical factors for which adjustment can be made is the Doppler angle. As mentioned above, Doppler measurements as performed by an ultrasound system are precisely accurate only when the direction of flow is in line with the direction of the ultrasound beam, a Doppler angle of zero. For all other angles between the beam direction and the flow direction the velocity is understated. In the Doppler shift equation presented above, the Doppler angle is weighed in the result

by the  $\cos\theta$  term, where  $\theta$  is the Doppler angle. Another practical factor of an ultrasound system is wall filter bias. A Doppler wall filter will typically exhibit a nonlinear characteristic which, for blood flow detection, will have a zero response at DC (no motion) and rise to a maximum response at a selected high frequency of  $\pm f$ . Alternatively, the wall filter can exhibit a maximum response at a frequency less than that dictated by the Nyquist limit of the ensemble sampling rate, as discussed below. A sample volume in the body at which the Doppler shift is measured will not be a single point in the body but will have a finite size, resulting in the return of Doppler signals indicative of a range of velocities. The non-uniform response of the wall filter can cause a wide spread of velocities to experience greater gain at different locations of the response characteristic, e.g., higher velocities are more greatly emphasized than lower velocities. This non-uniform response can produce a shift in the perceived center of the spread of velocities referred to as wall filter bias. The wall filter bias effect can also be taken into account by an adjustment to the model. Another related factor which can be taken into account is spectral spread, the Doppler spectral broadening effect resulting from the different paths and angles from the sample volume to each receiving element of the active aperture of an array transducer. See US Pat. 5,606,972 (Routh). Yet another factor which can be taken into account is aliasing effects, the mis-reporting of Doppler frequencies and velocities when the motion of blood flow is at a velocity in excess of that which can be detected unambiguously by the Nyquist limit of the sampling rate of the echo ensemble. In box 52, factors such as these are taken into account by a dot product adjustment to the flow velocity field model which, for the models previous described, can be of the form

$$\vec{V}_{OBS}(r) = |V(r)| \left[ \frac{-\vec{r}}{\|\vec{r}\|} \circ \vec{n}_{scan} \right]$$

where  $\vec{n}_{scan}$  is a vectorial representation of the physical and ultrasound system factors for which adjustment is being made. The result as shown in FIGURE 2 is  $V_{OBS}$ , the model as adjusted by expected effects and what is to be expected in the signals measured by the ultrasound system.

**[0026]** A comparator 54 compares the expected velocity values from the flow velocity field model,  $V_{OBS}$ , with actual velocity measurements from points (sample volumes) in the field,  $V_{MEAS}$ , produced by the Doppler processor 28. In box 56 the differences between the expected and received values are squared to produce an error term for each point. The error terms are integrated over the full inclusion zone which may be a one dimensional (e.g., 1D line), two dimensional (e.g., 2D line arcuate area), or three dimensional (e.g., 3D hemispherical shell) inclusion zone to produce a mean squared error term from the full zone. The error term is then used to adjust the

parameters of the field model such as  $r$  and the flow rate to cause a reduction in a subsequently measured error term. The preferred adjustment technique is to use a non-linear curve fit to adapt the model toward error reduction. One such non-linear curve fitting technique which may be used is the Levenberg-Marquardt algorithm, which refines the coordinates of the regurgitant orifice location and the flow ( $\vec{F}$ ) or flow rate ( $Q$ ) of the field toward or through the orifice.

**[0027]** The loop of FIGURE 2 is iteratively repeated to reduce the error term. With each pass through the loop a more precisely adapted field model is adjusted and compared with ultrasound velocity measurements from the acceptance zone and the error term is iteratively reduced. When the error term has been reduced to an acceptable low value, the model exhibits the desired actual measurements of the orifice location and the blood flow through the orifice. These terms, and others as desired, are produced as outputs by the flow quantification processor 34 and are presented on the display to the user.

**[0028]** FIGURE 3 is a diagrammatic 2D ultrasound image illustrating practice of the present invention to measure mitral valve regurgitation. The line 100 represents the plane of the mitral valve on which a regurgitant leak exists through an orifice O. When the left ventricle contracts, a jet of blood 102 escapes back into the right atria. In the PISA method this jet would be interrogated by a Doppler beam 110 extending through the orifice O. US Pat. 6,719,697 (Li) presents an improvement to the PISA technique in which a color M mode display is produced over the the heart cycle from the location of Doppler beam 110. The color Doppler display processor is set for the display limits indicated by the color bar 120 on the right side of the image, extending from a zero velocity center reference (BK=black) to +V and -V maximum velocities in opposite directions. A range of colors (Y=yellow; DR=dark red; etc.) is displayed in accordance with this range of velocities. Aliasing occurs when a velocity being measured exceeds the Nyquist limits of +V and -V. Immediately adjacent the orifice is the flow convergent region (FCR) 104. Beyond the flow convergent region is the acceptance zone 112 (S) used by an implementation of the present invention.

**[0029]** Both the PISA technique and the present invention are premised on the assumption that the regurgitant flow in the left ventricle near the orifice is converging and flowing toward the orifice location O. This is indicated by the flow vectors  $\vec{V}_1$ ,  $\vec{V}_2$ , and  $\vec{V}_3$  in the acceptance zone S. But as the direction of the Doppler beam 110 illustrates, virtually all of the flow vectors will not be aligned with the beam direction, even when the varying beam angles of a phased array sector probe are used. Consequently there will be Doppler angles of different magnitudes for the different flow vectors, which is taken into account by the Doppler angle adjustments to the flow velocity field model in box 52 of FIGURE 2 as described above.

**[0030]** The color Doppler image of the FCR 104 will be chaotic and erratic. This is because the spatial orientation of blood cells and blood flow velocities are changing very rapidly in this region as blood flow changes direction and accelerates momentarily toward the orifice O during systolic contraction. The ensemble samples acquired during this interval are often uncorrelated with one another, which defeats the correlation within an ensemble upon which the usual Doppler estimation processors are reliant. As a result, even though the flow within the FCR may be generally laminar, the colorflow display can be that of highly turbulent flow and aliasing. The inner boundary 108 of the acceptance zone S is preferably set beyond the flow convergence region 104 to avoid the use of erratic velocity estimates from the FCR. One approach to setting the boundary 108 is to set it at or beyond the velocity shear boundary. This can be done visually with reference to the colorflow display, or automatically with reference to a velocity shear threshold.

**[0031]** The outer boundary 106 of the acceptance zone may be set in relation to measurable velocities. While the velocities of regurgitant flow are relatively high near the orifice, they become progressively lower at increasing distances from the orifice. The outer boundary 106 can be set at a distance from the orifice O at which low Doppler velocities can still be reliably measured. This may be determined in relation to a percentage of the Nyquist limit or in relation to a low flow velocity such as 5 mm/sec. The outer boundary 106 can thus be set at a distance at which acceptable sensitivity to low flows can still be realized by the Doppler processor.

**[0032]** The acceptance zone 112 in the example of FIGURE 3 is seen to be a two dimensional arcuate area S having a center of rotation at the orifice O. The present invention may be used in one, two or three dimensions. A one dimensional implementation and model may just consider the segment of the beam line 110 which is between arcs 108 and 106, for instance. A two dimensional implementation would be one which samples an acceptance zone which is planar such as acceptance zone 112 in FIGURE 3. A three dimensional implementation would consider an arcuate acceptance such as 112 but in a full hemisphere centered on the orifice. Greater accuracy would be anticipated with the two and three dimensional implementations. A preferred implementation would use a 3D imaging probe with a two dimensional array transducer as shown in FIGURE 1, with acquisition and modeling done in a hemispherical or semi-hemispherical volume shell about the orifice. Higher frame rates can be realized with two dimensional imaging, in which case an MPR frame through the orifice and jet can be selected from the volume scanned with the 3D probe by use of the multiplanar reformatter 44. The desired plane can be repeatedly scanned at a high acquisition frame rate and the velocity measurements and flow calculations done with a two dimensional acceptance zone shown in the 2D MPR image.

**[0033]** While acceptance zones from which flow con-

verges in a circular pattern toward the orifice can exist as shown in FIGURE 3, other non-circular patterns have been found to be present in some cases. Stated differently, the flow vectors pointing toward the orifice may be arranged in a pattern other than an arc of a pure circle. Instead of the circular shape of FIGURE 3, an acceptance zone may have a parabolic or flattened circular shape. In three dimensional implementations the acceptance zone may be a paraboloid or oblate spheroid shell. The shape of the acceptance zone, that is, the area or volume in which velocities are measured in comparison to the model, may be dynamically changed during iterative passages through the processing loop of FIGURE 2 so that the process will adapt and converge to an acceptance zone with an altered shape from that used in the initial model.

**[0034]** As previously mentioned, it is frequently difficult for a clinician to accurately pinpoint the location of a tiny regurgitant orifice on an ultrasound image. When the heart is not contracting, the orifice is not present, and when it is present, its location is marred by imaging artifacts of the resultant turbulence such as those in the vicinity of the flow convergence region. In accordance with a further aspect of the present invention, an implementation of the present invention can automatically indicate the location of a leaking orifice on an ultrasound image. FIGURE 4 illustrates an ultrasound image in which elements previously described in conjunction with FIGURE 3 bear the same reference numerals. This image also includes a small box 130 which has been placed over the image by a clinician at the start of a diagnosis to indicate the presumed location of the regurgitant orifice. A control of the control panel 38 such as the trackball is manipulated by the clinician to place the icon 130 at the location in the image where the clinician believes the orifice is located. The coordinates of the indicated orifice icon 130 are used to seed the processing of the flow quantification processor shown in FIGURE 2, whereby the coordinates are used as the initial coordinates of the orifice in the mathematical model of box 50. The processor 34 iteratively refines the modeled values of the flow velocity vectors toward an orifice location in response to the receipt of the measured velocity values  $V_{MEAS}$ . The vertical placement of the orifice location has been found to have the greatest effect on the convergence of the modeled velocity vectors with the measured velocity values. While the heart is contracting during systole, the movement of contraction causes the mitral valve to move vertically in the image toward the center of the left ventricle. Thus, the natural contractive movement of the heart can be the source of greatest error in regurgitant flow assessment. The processor 34 iteratively refines the location of the orifice to reduce the error disparity between the measured and estimated velocity values in the flow velocity field (acceptance zone S) between boundaries 106 and 108. As the flow quantification processor iterates to converge on the true coordinates of the orifice, the finally determined coordinates are used by the flow

quantification processor 34 and the graphics processor 36 to automatically move orifice icon 130 to the calculated coordinates in the image. Alternatively the graphics processor will place another (calculated) orifice icon 132 on the display at the true coordinate location determined by the iterative model adjustment. As mentioned previously, misplacement of the orifice by as little as 1mm can significantly affect the orifice flow rate and volume flow calculations, volume flow being the integral of the flow rate over the time during which the heart is contract (about 1/3 of a heart cycle). The flow volume will peak at approximately the middle of the systolic interval. In FIGURE 4 it is seen that the system has placed the calculated orifice icon 132 at its true location in the image field, which is different from the clinician's initial estimate of the orifice location. When the ultrasound study is performed with 2D imaging the orifice coordinates will generally be in (x,y,z) Cartesian coordinates. When 3D imaging is used a spherical (r,θ,φ) coordinate system will generally be employed. In addition, as the FIGURE 4 ultrasound image illustrates, the acceptance zone S is graphically delineated in the displayed ultrasound image and any modification of the shape of the acceptance zone as discussed above is incorporated in the displayed shape and graphical delineation of the acceptance zone on the display.

**[0035]** As mentioned above, regurgitant orifices do not always exist as single pinhole leaks in a closed valve. The leaks may be produced by slit openings or multiple small leaks. FIGURE 5 is an illustration of the use of an implementation of the present invention to assess the flow rate and volume flow of slits and multiple leaks in valve closure. As FIGURE 5 illustrates, the process of the present invention is performed for a series of orifice locations arrayed along the leaking mitral valve 100'. These discrete pinhole orifice locations can be used to model complex slit-like orifices or multiple orifices in the closed valve. FIGURE 5 shows an example of three such determinations, each with its own acceptance zone, indicated by outer zone boundaries 106, 106' and 106'', and flow vectors (indicated by the small arrows) directed to converge at a different orifice location along the valve 100'. The vector velocity field associated with each pinhole orifice is combined vectorially with the other orifices, such that a single combined acceptance zone is defined along with a single combined vector velocity field. For multiple orifices, the combined vector velocity field now approximates the true physiologic velocity vectors (-V<sub>true</sub>, output of box 50 in FIGURE 2). The processing of the combined vector velocity field determines the flow rate or volume flow of all the pinhole orifices corresponding to the entire slit along the mitral valve closure. While FIGURE 5 gives an example of a vector velocity field generated from three pinhole orifices, any number of orifices may be used to adequately model the slit. The acceptance zones used for each measurement may be combined as shown in FIGURE 5, as the flow that is determined for the combined orifices is vectorial flow directed toward a unique

orifice or position along a slit. In a three dimension implementation the line of measurements is not constrained to a straight line in a plane, but may follow a non-linear path of closure of the mitral valve leaflets.

**[0036]** FIGURE 6 illustrates the response characteristics of two Doppler wall filters which may be employed in an implementation of the present invention. The coordinates of the abscissa of the plot of FIGURE 6 are in units of the Nyquist limits of a sampled data wall filter, where the limits of +1 and -1 are the normalized Nyquist limits of the filter corresponding to the blood flow velocities. A zero (DC, or no-flow) condition is in the center. The ordinate coordinates indicate the relative amplitude response of the filter characteristic. The response curve 140 is a typical wall filter response curve for measuring blood flow and may be used in an implementation of the present invention. This characteristic has a response of zero at the center, resulting in no response to stationary objects such as stationary vessel walls. The response is seen to progressively increase as the curve extends out from zero, with a maximum response at the Nyquist limits for the highest velocity flows detectable without aliasing at the chosen sampling interval. As a result, this response characteristic is most sensitive to flow at the highest flow velocities.

**[0037]** The response curve 150 is one which is often preferred for the wall filter of an implementation of the present invention. The response of this curve 150 is seen to peak at a relatively high but intermediate sampling rate just above  $\pm 0.5$  Nyquist, preferably in the range of  $\frac{1}{2}$  to  $\frac{2}{3}$  of Nyquist, and drops to a response of zero at the Nyquist limits. This filter characteristic is designed to be more sensitive to lower flow velocities, which can be expected around the outer boundary 106 of the acceptance zone S. This is helpful to offset the low sensitivity to low velocity flow which results from the short ensembles typically used for colorflow imaging of regurgitant flow. This can be seen by the greater response of the curve 150 for lower velocities near the center of the plot. While the curve 150 is seen to drop to zero at the Nyquist limits, this loss of high velocity sensitivity is generally acceptable when traded off for greater sensitivity to low velocity flows.

## Claims

1. A diagnostic ultrasound system for assessing regurgitant flow comprising:

- an ultrasound probe (10) having a transducer array configured for transmitting ultrasonic energy to, and receiving ultrasonic echoes from, a location of regurgitant flow in a body;
- an image processor (30), responsive to received echoes, configured for producing an ultrasound image of the location of regurgitant flow;



- a Doppler processor (28), responsive to received echoes, configured for producing Doppler ultrasound measurements of blood flow velocity in the vicinity of the location of regurgitant flow; and

a user control (38);

**characterized in that** the ultrasound system further comprises:

- a flow quantification processor (34), responsive to blood flow velocity measurements in the vicinity of a regurgitant orifice, configured to produce calculated location coordinates of the orifice, wherein the flow quantification processor is responsive to an initial estimate of the location of the orifice and to flow velocity estimates to iteratively refine by use of a flow velocity field model the location coordinates of the orifice; and  
- an ultrasound image display (40), responsive to the image processor and the flow quantification processor, configured to display an indication of the location of the orifice in an ultrasound image at the calculated location coordinates;

wherein the user control (38) is operable by a user to indicate the initial estimate of the location of the orifice in the ultrasound image and wherein the flow quantification processor is responsive to said indicated initial estimate to produce the calculated location coordinates of the orifice.

2. The diagnostic ultrasound system of Claim 1, further comprising a graphics processor (36), responsive to the user indication of the location of the orifice (O), configured to display an orifice icon (130) at the location indicated by the user in the ultrasound image.
3. The diagnostic ultrasound system of Claim 2, wherein the graphics processor (36) is further configured to, responsive to the calculated location coordinates, relocate the displayed orifice icon to the calculated location coordinates.
4. The diagnostic ultrasound system of Claim 2, wherein the graphics processor (36) is further configured to, responsive to the calculated location coordinates, display a second orifice icon (132) in the ultrasound image at the calculated location coordinates.
5. The diagnostic ultrasound system of Claim 1, wherein the calculated location coordinates of the orifice are produced when an error term between values of the flow velocity field and the measurements of blood flow velocity is minimized.
6. The diagnostic ultrasound system of Claim 5, wherein the flow quantification processor is operative to

adjust the calculated location coordinates of the orifice in relation to the distance of the orifice from the mitral valve plane as the error term is minimized.

7. The diagnostic ultrasound system of Claim 6, wherein the flow quantification processor (34) is operative to:
  - produce an error term for each point of an inclusion zone (112, S), the inclusion zone being a two-dimensional curved strip delineated by two arcs centered on the regurgitant orifice location (O) or a three-dimensional hemispherical shell centered on the regurgitant orifice location;
  - integrate the error terms over the full inclusion zone; and
  - adjust a parameter of the flow velocity field model based on the integrated error term.
8. The diagnostic ultrasound system of Claim 7, wherein the flow quantification processor (34) is operative to adjust the parameter of the flow velocity field model by use of a non-linear curve fitting algorithm, said algorithm preferably being a Levenberg-Marquardt algorithm.
9. The diagnostic ultrasound system of Claim 5, wherein the flow quantification processor (34) is operative to adjust values of the flow velocity field based on at least one physical factor of the diagnostic ultrasound system.
10. The diagnostic ultrasound system of Claim 9, wherein the at least one physical factor of the diagnostic ultrasound system comprises a Doppler angle adjustment, Doppler wall filter bias, Doppler spectral spread and aliasing effects.
11. The diagnostic ultrasound system of Claim 1, wherein the flow quantification (34) processor is further operative to produce a measure of flow rate through the orifice.
12. The diagnostic ultrasound system of Claim 1, wherein the flow quantification processor (34) is further operative to produce a measure of the volume flow through the orifice.
13. The diagnostic ultrasound system of Claim 1, wherein the flow quantification processor (34) is configured to produce the calculated location of the orifice in Cartesian coordinates.
14. The diagnostic ultrasound system of Claim 1, wherein the flow quantification processor (34) is configured to produce the calculated location of the orifice in spherical coordinates.

15. The diagnostic ultrasound system of Claim 1, wherein the flow quantification processor (34) is configured to produce calculated location coordinates of each of multiple orifices in a mitral valve (100') and to vectorially combine a vector velocity field associated with each of the multiple orifice with the vectors of the other orifices.

## Patentansprüche

1. Ultraschallsystem zur diagnostischen Bildgebung für die Einschätzung von Regurgitationsströmung, umfassend:

- eine Ultraschallsonde (10) mit einem Wandlerarray, die konfiguriert ist, um Ultraschallenergie an einen Ort mit Regurgitationsströmung in einem Körper auszusenden und Ultraschallechos von diesem Ort zu empfangen;
- einen Bildprozessor (30), der auf die empfangenen Echos reagiert und konfiguriert ist, um ein Ultraschallbild des Orts mit Regurgitationsströmung zu erzeugen;
- einen Doppler-Prozessor (28), der auf die empfangenen Echos reagiert und konfiguriert ist, um Doppler-Ultraschallmessungen der Blutströmungsgeschwindigkeit in der Nähe des Orts mit Regurgitationsströmung zu erzeugen; und

eine Benutzersteuerung (38);

**dadurch gekennzeichnet, dass** das Ultraschallsystem ferner umfasst:

- einen Strömungsquantifizierungsprozessor (34), der auf Blutströmungsgeschwindigkeitsmessungen in der Nähe einer Regurgitationsöffnung reagiert und konfiguriert ist, um berechnete Ortskoordinaten der Öffnung zu erzeugen, wobei der Strömungsquantifizierungsprozessor auf eine anfängliche Schätzung des Orts der Öffnung und auf Strömungsgeschwindigkeitsschätzungen reagiert, um die Ortskoordinaten der Öffnung unter Verwendung eines Strömungsgeschwindigkeitsfeldmodells iterativ zu verfeinern, und
- eine Ultraschallbildanzeige (40), die auf den Bildprozessor und den Strömungsquantifizierungsprozessor reagiert und konfiguriert ist, um eine Angabe des Öffnungsorts in einem Ultraschallbild bei den berechneten Ortskoordinaten anzuzeigen;

wobei die Benutzersteuerung (38) durch einen Benutzer bedient werden kann, um die anfängliche Schätzung des Öffnungsorts in dem Ultraschallbild anzugeben, und wobei der Strömungsquantifizierungsprozessor auf die genannte angegebene an-

fängliche Schätzung reagiert, um die berechneten Ortskoordinaten der Öffnung zu erzeugen.

2. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, ferner umfassend einen Grafikprozessor (36), der auf die benutzerseitige Angabe des Öffnungsorts (O) reagiert und konfiguriert ist, um ein Öffnungssymbol (130) an dem durch den Benutzer angegebenen Ort in dem Ultraschallbild anzuzeigen.

3. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 2, wobei der Grafikprozessor (36) ferner konfiguriert ist, um das angezeigte Öffnungssymbol als Reaktion auf die berechneten Ortskoordinaten zu den berechneten Ortskoordinaten zu verschieben.

4. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 2, wobei der Grafikprozessor (36) ferner konfiguriert ist, um in Reaktion auf die berechneten Ortskoordinaten ein zweites Öffnungssymbol (132) in dem Ultraschallbild bei den berechneten Ortskoordinaten anzuzeigen.

5. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, wobei die berechneten Ortskoordinaten der Öffnung erzeugt werden, wenn ein Fehlerterm zwischen Werten des Strömungsgeschwindigkeitsfelds und den Messungen der Blutströmungsgeschwindigkeit minimiert ist.

6. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 5, wobei der Strömungsquantifizierungsprozessor betriebsfähig ist, um die berechneten Ortskoordinaten der Öffnung in Bezug auf den Abstand der Öffnung zu der Mitralklappenebene anzupassen, während der Fehlerterm minimiert wird.

7. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 6, wobei der Strömungsquantifizierungsprozessor (34) betriebsfähig ist zum

- Erzeugen eines Fehlerterms für jeden Punkt einer Inklusionszone (112, S), wobei die Inklusionszone ein zweidimensionaler gebogener Streifen ist, der durch zwei auf den Regurgitationsöffnungsort (O) zentrierte Bögen begrenzt wird, oder eine auf die Regurgitationsöffnungsortzentrierte dreidimensionale Kugelhalbschale ist;
- Integrieren der Fehlerterme über die gesamte Inklusionszone; und
- Anpassen eines Parameters des Strömungsgeschwindigkeitsfeldmodells basierend auf dem integrierten Fehlerterm.

8. Ultraschallsystem zur diagnostischen Bildgebung

nach Anspruch 7, wobei der Strömungsquantifizierungsprozessor (34) betriebsfähig ist, um den Parameter des Strömungsgeschwindigkeitsfeldmodells unter Verwendung eines nicht-linearen Kurvenanpassungsalgorithmus anzupassen, wobei der genannte Algorithmus vorzugsweise ein Levenberg-Marquardt-Algorithmus ist.

9. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 5, wobei der Strömungsquantifizierungsprozessor (34) betriebsfähig ist, um Werte des Strömungsgeschwindigkeitsfelds basierend auf mindestens einem physikalischen Faktor des Ultraschallsystems zur diagnostischen Bildgebung anzupassen. 10
10. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 9, wobei der mindestens eine physikalische Faktor des Ultraschallsystems zur diagnostischen Bildgebung eine Dopplerwinkel Anpassung, Dopplerwandfiltervoreinstellung, Dopplerspektralverbreiterung und Aliasing-Effekte umfasst. 20
11. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, wobei der Strömungsquantifizierungsprozessor (34) ferner betriebsfähig ist, um ein Maß der Strömungsrate durch die Öffnung zu erzeugen. 25
12. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, wobei der Strömungsquantifizierungsprozessor (34) ferner betriebsfähig ist, um ein Maß der Volumenströmung durch die Öffnung zu erzeugen. 30
13. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, wobei der Strömungsquantifizierungsprozessor (34) konfiguriert ist, um den berechneten Ort der Öffnung in kartesischen Koordinaten zu erzeugen. 35
14. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, wobei der Strömungsquantifizierungsprozessor (34) konfiguriert ist, um den berechneten Ort der Öffnung in Kugelkoordinaten zu erzeugen. 40
15. Ultraschallsystem zur diagnostischen Bildgebung nach Anspruch 1, wobei der Strömungsquantifizierungsprozessor (34) konfiguriert ist, um berechnete Ortskoordinaten von jeder von mehreren Öffnungen in einer Mitralklappe (100') zu erzeugen und um ein zu jeder der mehreren Öffnungen gehöriges Vektorgeschwindigkeitsfeld vektoriell mit den anderen Öffnungen zu kombinieren. 45

## Revendications

1. Système ultrasonore de diagnostic pour évaluer un écoulement de régurgitation comprenant :

- une sonde ultrasonore (10) ayant un réseau de transducteurs configuré pour transmettre de l'énergie ultrasonore à un emplacement d'écoulement de régurgitation dans un corps et en recevoir des échos ultrasonores ;
- un dispositif de traitement d'image (30) sensible aux échos reçus et configuré pour produire une image ultrasonore de l'emplacement de l'écoulement de régurgitation ;
- un dispositif de traitement Doppler (28) sensible aux échos reçus et configuré pour produire des mesures ultrasonores de Doppler de la vitesse d'écoulement du sang au voisinage de l'emplacement d'écoulement de régurgitation ; et

une commande utilisateur (38) ;

**caractérisé en ce que** le système ultrasonore comprend en outre :

- un dispositif de traitement de quantification d'écoulement (34) sensible aux mesures de vitesse d'écoulement du sang au voisinage d'un orifice de régurgitation et configuré pour produire des coordonnées de l'emplacement calculé de l'orifice, dans lequel le dispositif de traitement de quantification d'écoulement est sensible à une estimation initiale de l'emplacement de l'orifice et à des estimations de vitesse d'écoulement pour affiner de manière itérative par utilisation d'un modèle de champ de vitesses d'écoulement les coordonnées d'emplacement de l'orifice ; et
- un affichage d'image ultrasonore (40) sensible au dispositif de traitement d'image et au dispositif de traitement de quantification d'écoulement et configuré pour afficher une indication de l'emplacement de l'orifice dans une image ultrasonore aux coordonnées de l'emplacement calculé ;

dans lequel la commande utilisateur (38) peut être actionnée par un utilisateur pour indiquer l'estimation initiale de l'emplacement de l'orifice dans l'image ultrasonore et

dans lequel le dispositif de traitement de quantification d'écoulement est sensible à ladite estimation initiale indiquée pour produire les coordonnées de l'emplacement calculé de l'orifice.

2. Système ultrasonore de diagnostic selon la revendication 1, comprenant en outre un dispositif de traitement de graphique (36) sensible à l'indication par

l'utilisateur de l'emplacement de l'orifice (O) et configuré pour afficher une icône d'orifice (130) à l'emplacement indiqué par l'utilisateur dans l'image ultrasonore.

3. Système ultrasonore de diagnostic selon la revendication 2, dans lequel le dispositif de traitement de graphique (36) est en outre configuré pour relocaliser l'icône d'orifice affichée aux coordonnées de l'emplacement calculé en fonction des coordonnées de l'emplacement calculé.
4. Système ultrasonore de diagnostic selon la revendication 2, dans lequel le dispositif de traitement de graphique (36) est en outre configuré pour afficher une seconde icône d'orifice (132) dans l'image ultrasonore aux coordonnées de l'emplacement calculé en fonction des coordonnées de l'emplacement calculé.
5. Système ultrasonore de diagnostic selon la revendication 1, dans lequel les coordonnées de l'emplacement calculé de l'orifice sont produites lorsqu'un terme d'erreur entre les valeurs du champ de vitesse d'écoulement et des mesures de la vitesse d'écoulement du sang est minimisé.
6. Système ultrasonore de diagnostic selon la revendication 5, dans lequel le dispositif de traitement de quantification d'écoulement est à même d'ajuster les coordonnées de l'emplacement calculé de l'orifice en rapport avec la distance de l'orifice vis-à-vis du plan de la valvule mitrale lorsque le terme d'erreur est minimisé.
7. Système ultrasonore de diagnostic selon la revendication 6, dans lequel le dispositif de traitement de quantification d'écoulement (34) est à même :
  - de produire un terme d'erreur pour chaque point d'une zone d'inclusion (112, S), la zone d'inclusion étant une bande bidimensionnelle incurvée tracée par deux arcs centrés sur l'emplacement de l'orifice de régurgitation (O) ou sur une coque hémisphérique tridimensionnelle centrée sur l'emplacement de l'orifice de régurgitation ;
  - d'intégrer les termes d'erreurs sur toute la zone d'inclusion ; et
  - d'ajuster un paramètre du modèle de champ de vitesse d'écoulement sur la base du terme d'erreur intégré.
8. Système ultrasonore de diagnostic selon la revendication 7, dans lequel le dispositif de traitement de quantification d'écoulement (34) est à même d'ajuster le paramètre du modèle de champ de vitesse d'écoulement par utilisation d'un algorithme d'ajus-

tement à courbe non linéaire, ledit algorithme étant de préférence un algorithme de Levegerg-Marquardt.

9. Système ultrasonore de diagnostic selon la revendication 5, dans lequel le dispositif de traitement de quantification d'écoulement (34) est à même d'ajuster des valeurs du champ de vitesse d'écoulement sur la base d'au moins un facteur physique du système ultrasonore du diagnostic.
10. Système ultrasonore de diagnostic selon la revendication 9, dans lequel le au moins un facteur physique du système ultrasonore de diagnostic comprend un ajustement d'angle de Doppler, un biais de filtre de paroi de Doppler, des effets d'étalement spectral et de repliement spectral de Doppler.
11. Système ultrasonore de diagnostic selon la revendication 1, dans lequel le dispositif de traitement de quantification d'écoulement (34) est en outre à même de produire une mesure du débit à travers l'orifice.
12. Système ultrasonore de diagnostic selon la revendication 1, dans lequel le dispositif de traitement de quantification d'écoulement (34) est en outre à même de produire une mesure de l'écoulement volumique à travers l'orifice.
13. Système ultrasonore de diagnostic selon la revendication 1, dans lequel le dispositif de traitement de quantification d'écoulement (34) est configuré pour produire l'emplacement calculé de l'orifice en coordonnées cartésiennes.
14. Système ultrasonore de diagnostic selon la revendication 1, dans lequel le dispositif de traitement de quantification d'écoulement (34) est configuré pour produire l'emplacement calculé de l'orifice en coordonnées sphériques.
15. Système ultrasonore de diagnostic selon la revendication 1, dans lequel le dispositif de traitement de quantification d'écoulement (34) est configuré pour produire des coordonnées de l'emplacement calculé de chacun de multiples orifices d'une valvule mitrale (100') et combiner vectoriellement un champ de vitesse vectoriel associé à chacun des multiples orifices avec les vecteurs des autres orifices.

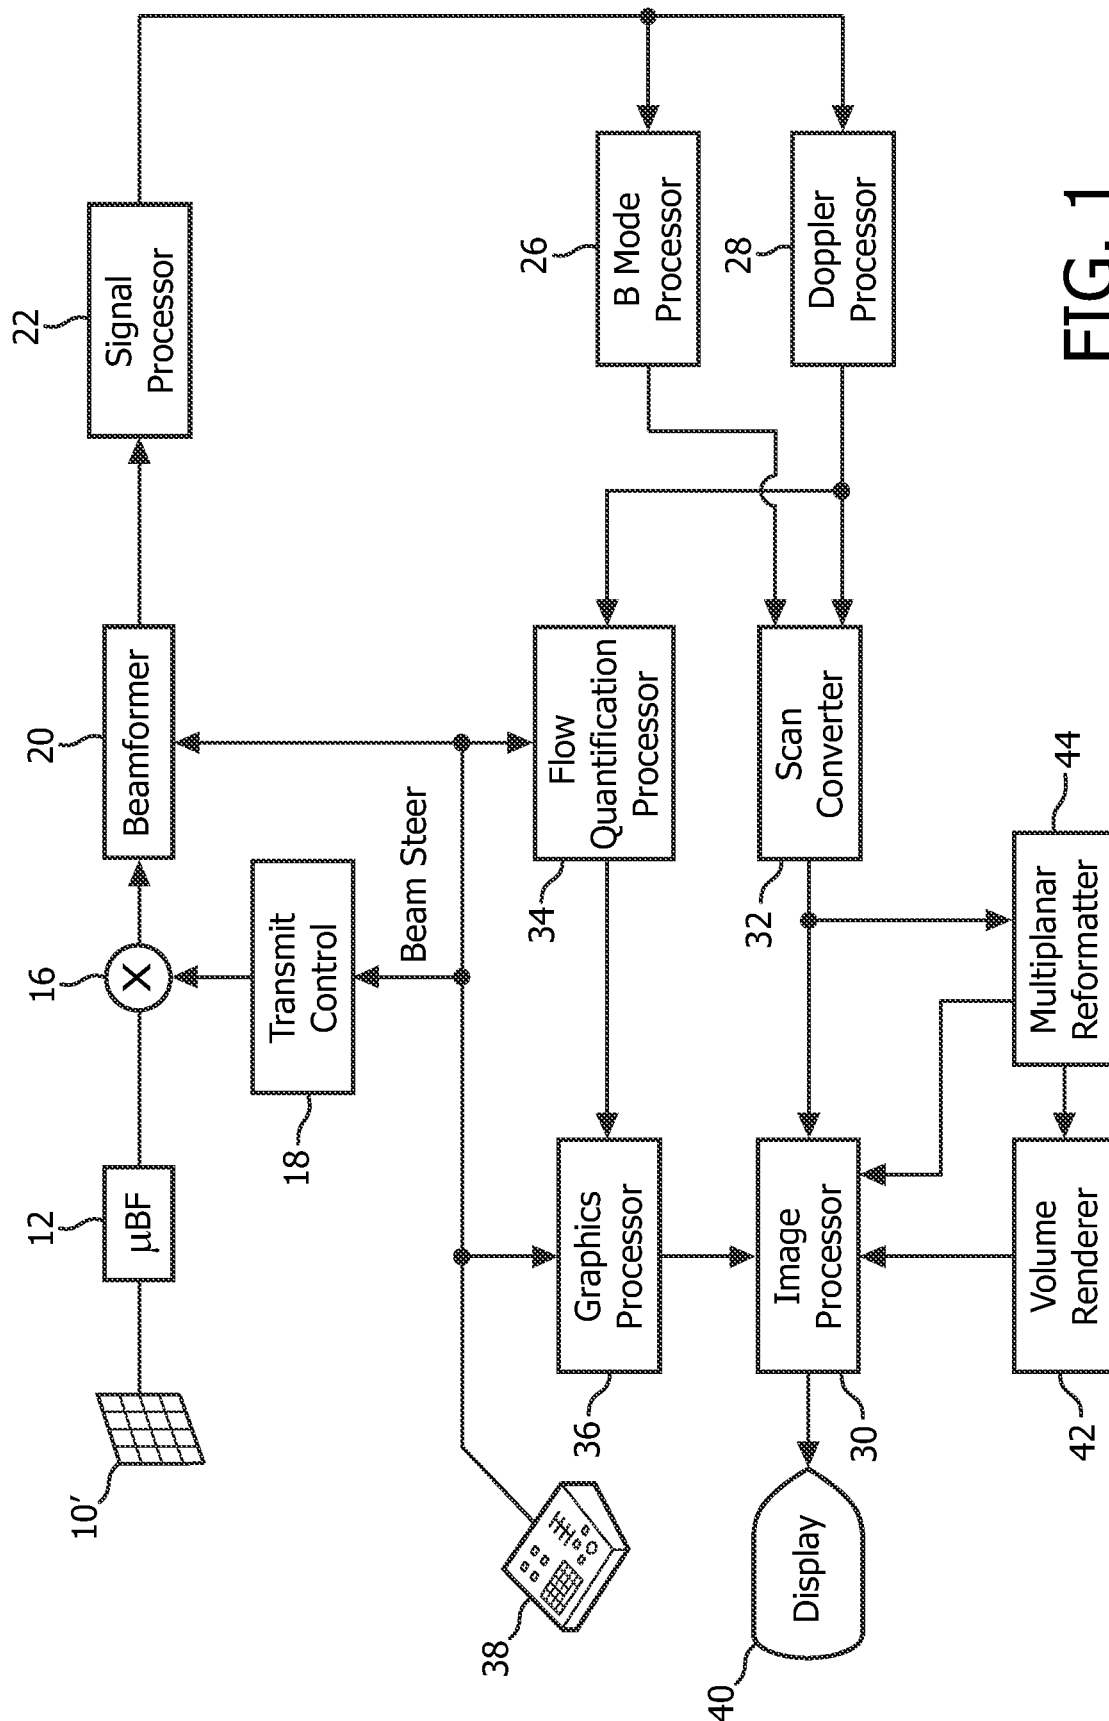


FIG. 1

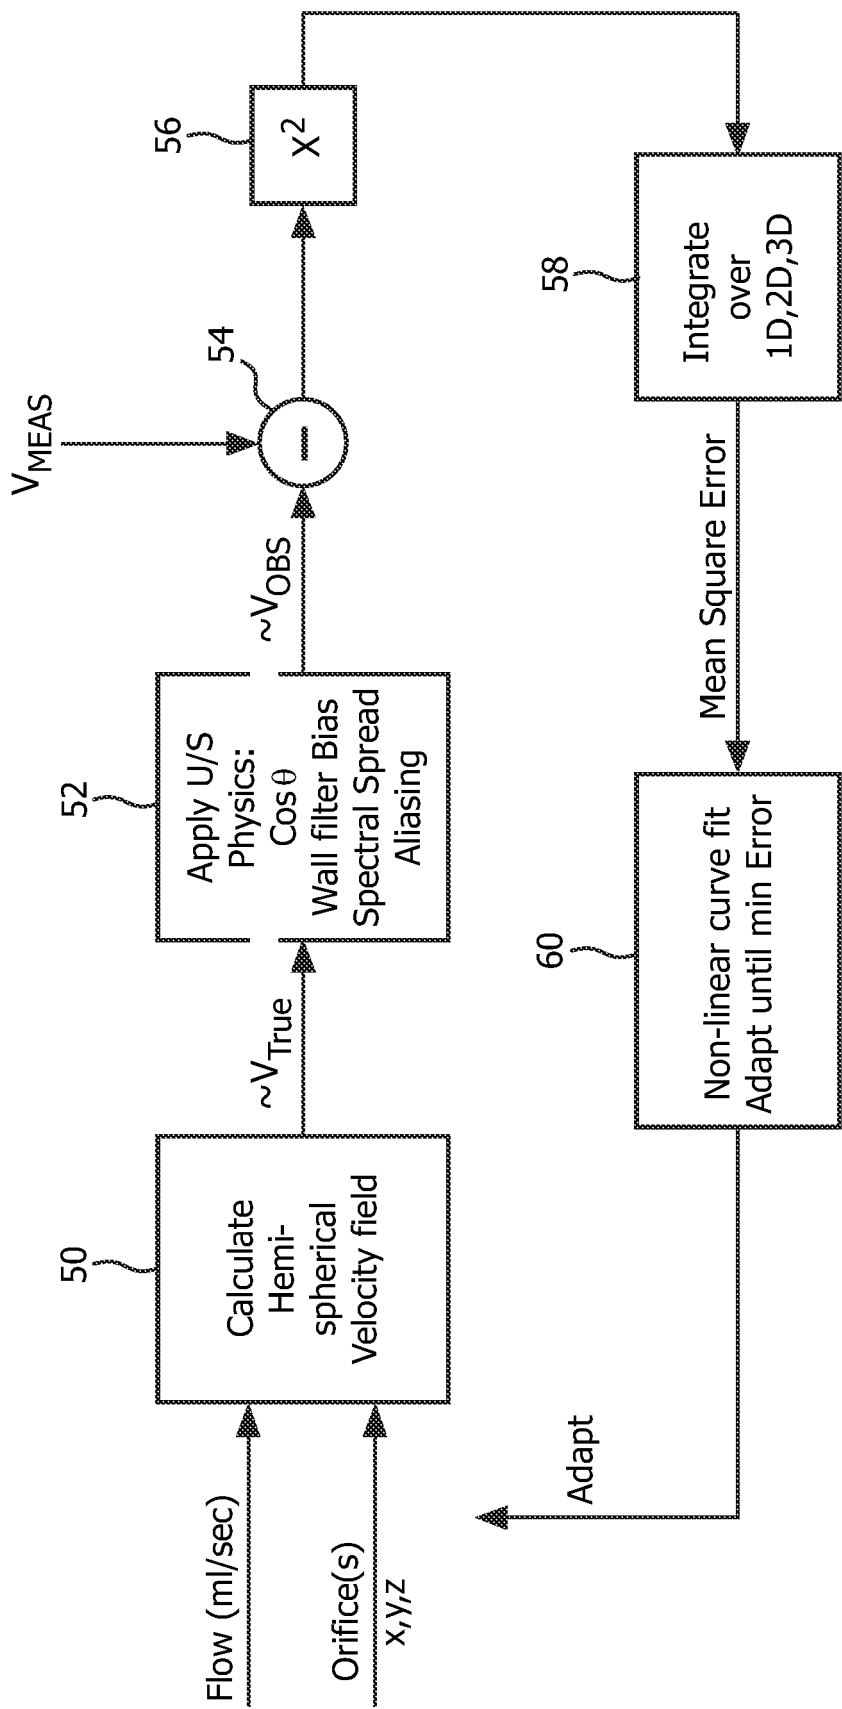
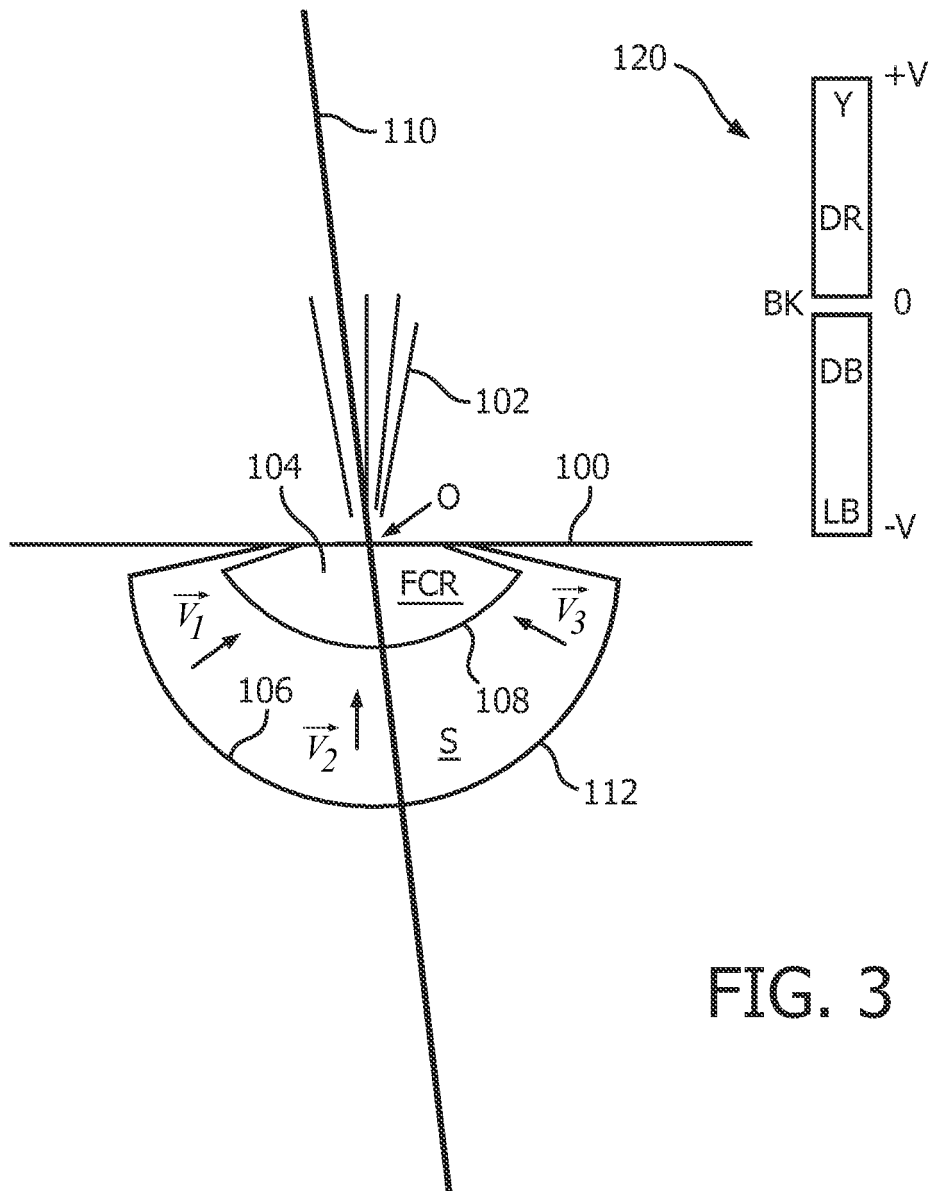


FIG. 2



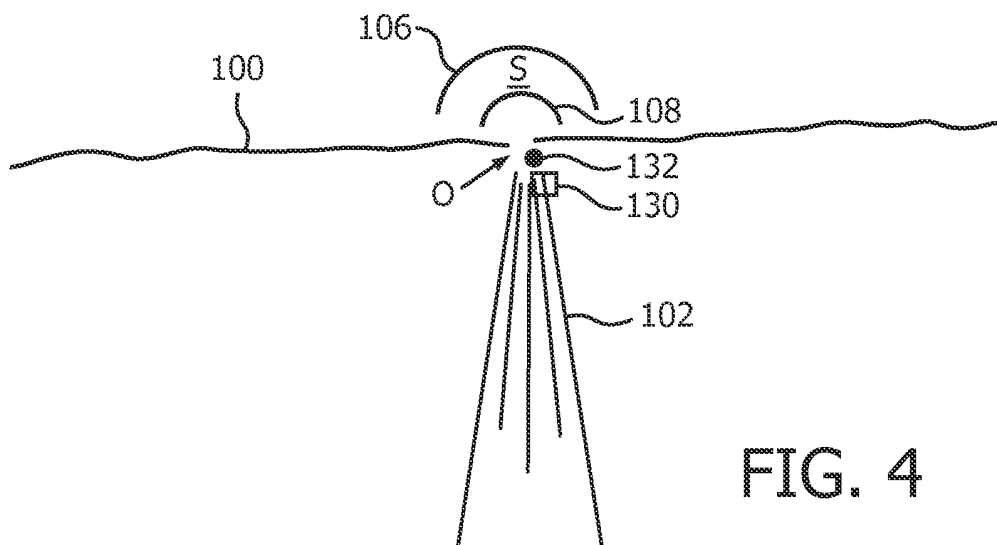


FIG. 4

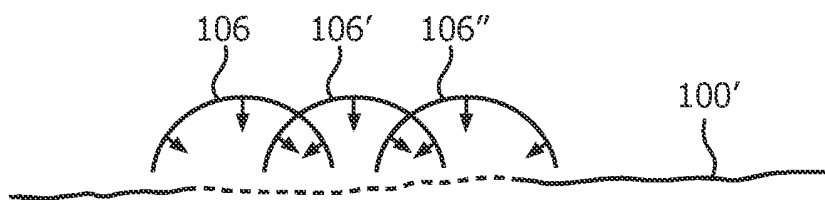


FIG. 5

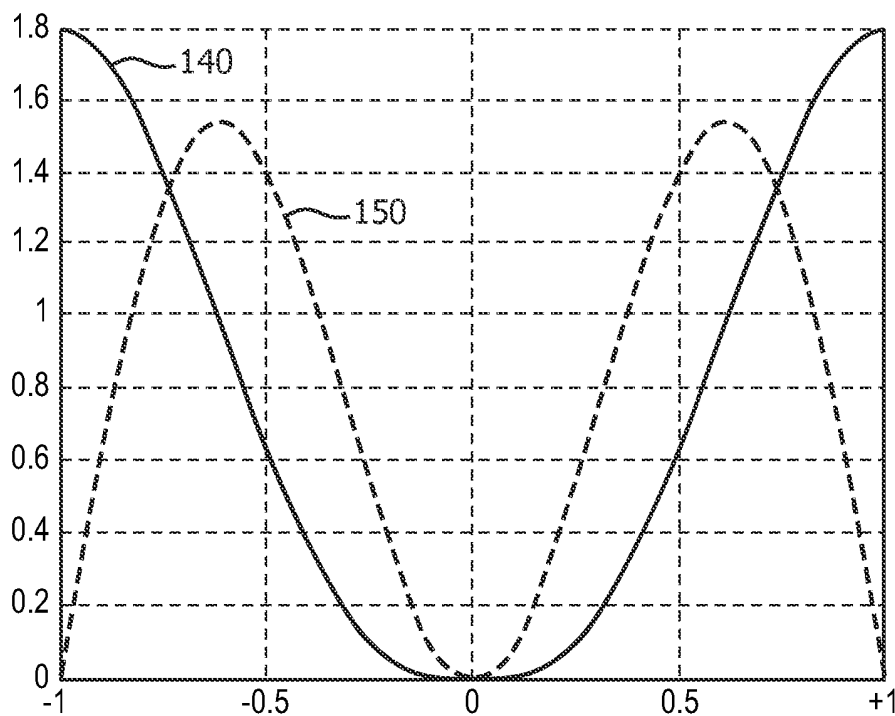


FIG. 6



## REFERENCES CITED IN THE DESCRIPTION

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

### Patent documents cited in the description

- US 61426669 A [0001]
- US 4913159 A [0008]
- US 5997479 A, Savord [0018]
- US 6013032 A, Savord [0018]
- US 6623432 B, Powers [0018]
- US 6283919 B, Roundhill [0021]
- US 6458083 B, Jago [0021]
- US 6443896 B, Detmer [0022]
- US 6530885 B, Entrekin [0022]
- US 5606972 A, Routh [0025]
- US 6719697 B, Li [0028]

### Non-patent literature cited in the description

- Application of Color Doppler Flow Mapping to Calculate Effective Regurgitant Orifice Area. An In Vitro Study and Initial Clinical Observations. **P. M. VAND-ERVOORT et al.** Circulation. American Heart Association Inc, 01 September 1993, vol. 88, 1150-1156 [0010]

|                |                                                                                                                                                                    |         |            |
|----------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 自动识别超声图像中二尖瓣回流口的位置                                                                                                                                                 |         |            |
| 公开(公告)号        | <a href="#">EP2654573A1</a>                                                                                                                                        | 公开(公告)日 | 2013-10-30 |
| 申请号            | EP2011811390                                                                                                                                                       | 申请日     | 2011-12-16 |
| [标]申请(专利权)人(译) | 皇家飞利浦电子股份有限公司                                                                                                                                                      |         |            |
| 申请(专利权)人(译)    | 皇家飞利浦N.V.                                                                                                                                                          |         |            |
| 当前申请(专利权)人(译)  | 皇家飞利浦N.V.                                                                                                                                                          |         |            |
| [标]发明人         | WEI QIFENG<br>THIELE KARL ERHARD<br>YOGANATHAN AJIT<br>YAP CHOON HWAI                                                                                              |         |            |
| 发明人            | WEI, QIFENG<br>THIELE, KARL ERHARD<br>YOGANATHAN, AJIT<br>YAP, CHOON HWAI                                                                                          |         |            |
| IPC分类号         | A61B8/08 A61B8/06                                                                                                                                                  |         |            |
| CPC分类号         | A61B8/06 A61B8/0883 A61B8/13 A61B8/145 A61B8/4444 A61B8/4488 A61B8/463 A61B8/488 A61B8/5207 A61B8/5223 G01S7/52071 G01S7/52073 G01S15/8981 G01S15/8984 G01S15/8993 |         |            |
| 代理机构(译)        | STEFFEN , THOMAS                                                                                                                                                   |         |            |
| 优先权            | 61/426669 2010-12-23 US<br>61/466059 2011-03-22 US                                                                                                                 |         |            |
| 其他公开文献         | EP2654573B1                                                                                                                                                        |         |            |
| 外部链接           | <a href="#">Espacenet</a>                                                                                                                                          |         |            |

#### 摘要(译)

描述了一种超声诊断成像系统，其量化通过二尖瓣的反流，包括自动指示超声图像中反流孔的位置。临床医生对反流阀进行成像，并在图像中指示反流孔的假定位置 ( 130 )。流量量化处理器响应临床医生的该初始位置估计来计算孔口位置的精确估计。精细位置由成像系统在超声图像上指示，或者通过重新定位由临床医生放置的图标，或者在精细位置处在图像上显示第二图标 ( 132 )。