



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
**31.12.2014 Bulletin 2015/01**

(51) Int Cl.:  
**A61B 8/00 (2006.01)**  
**A61B 6/00 (2006.01)**  
**A61B 8/08 (2006.01)**

(21) Application number: **14164309.8**

(22) Date of filing: **10.04.2014**

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**  
Designated Extension States:  
**BA ME**

(72) Inventors:  
• **Larizza, Pietro**  
**70026 Modugno (IT)**  
• **Vinci, Angelo Michele**  
**70026 Modugno (IT)**

(30) Priority: **26.06.2013 IT TO20130527**

(74) Representative: **Bongiovanni, Simone et al**  
**Studio Torta S.p.A.**  
**Via Viotti, 9**  
**10121 Torino (IT)**

(71) Applicant: **MASMEC S.p.A.**  
**Modugno (IT)**

(54) **Computer-assisted ultrasound navigation system for providing assistance during diagnostic and therapeutic operations**

(57) A computer-assisted ultrasound imaging system (100) wherein an ultrasound device (4) is provided with an ultrasound probe (3) for capturing a plurality of two-dimensional ultrasound images of a concerned region. The system processes the acquired ultrasound images in order to obtain a three-dimensional compound ultrasound graphic reconstruction (C), which is com-

pared with a three-dimensional pseudo ultrasound image (B) obtained by processing a plurality of two-dimensional images obtained by means of X-ray or magnetic resonance techniques (A). Following the adjustment procedure with a first spot-test method or, alternatively, with a second structural method, the image C is superimposed on image A.

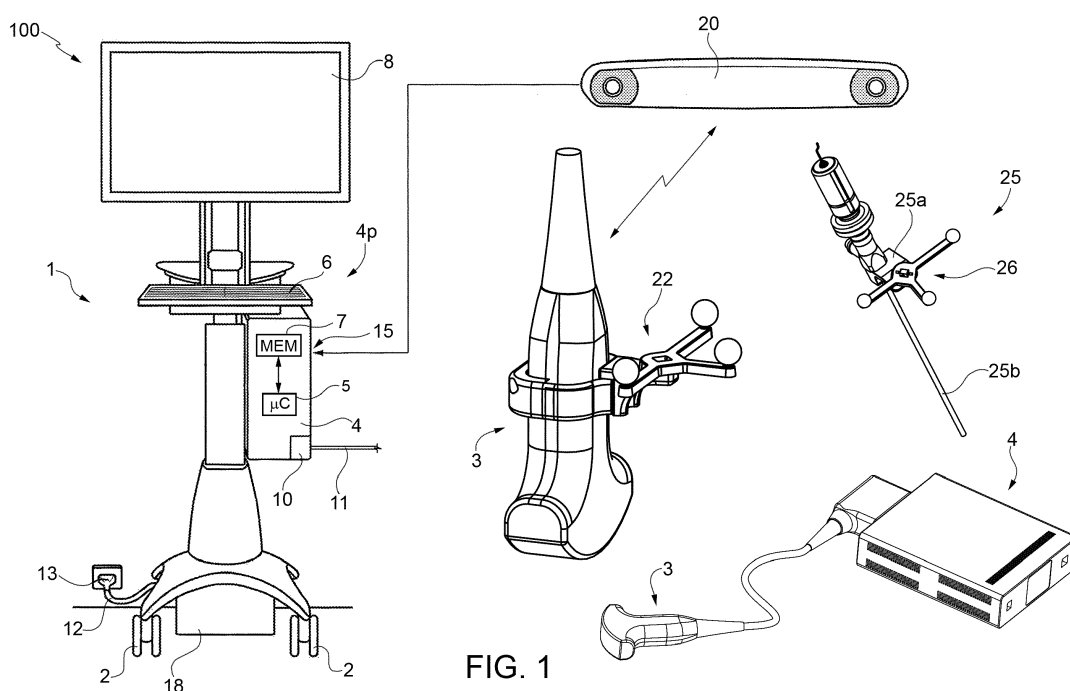


FIG. 1

**Description****TECHNICAL FIELD OF INVENTION**

**[0001]** The present invention relates to a computer-assisted ultrasound navigation system, in particular for assisting medical personnel during diagnostic and/or therapeutic operations.

**STATE OF THE ART**

**[0002]** As is known, ultrasound imaging systems enable obtaining images of a patient's internal organs without any risk (even potential) to the patient and the operator of the imaging system, as the waves striking the human body are absolutely innocuous due to their low frequency (in particular, ionizing radiation is not generated). However, ultrasound images are usually not very comprehensible and are of low resolution.

**[0003]** To obtain higher resolution, it is necessary to use a radiation of higher frequency, such as X-rays, which are used in computerized tomography or CT systems. According to some authors, the (ionizing) radiation employed could be potentially hazardous; for this reason, CT systems cannot be used for long periods on the same subject.

**[0004]** A normal CT actually releases several tens of mSv, while a full-body TAC can release up to 100mSv (according to radiation protection regulations in the workplace, an operator must not be exposed to more than 20mSv of ionizing radiation per annum).

**[0005]** Accordingly, there is a need for providing a system that integrates information arriving in real time from an ultrasound imaging system with more detailed images of the same anatomic region, previously taken by means of a computerized tomography system or a magnetic resonance MR system.

**[0006]** There are several systems on the market (for example the MyLab system produced by ESAOTE) that are capable of integrating images obtained from an ultrasound imaging system with images taken by means of a computerized tomography system.

**SUBJECT AND ABSTRACT OF THE INVENTION**

**[0007]** The object of the present invention is that of providing a system that improves the effectiveness of merging ultrasound /CT images with respect to that provided for by the known art by providing a spatial and volumetric calibration method.

**[0008]** According to the present invention, a system and a method of computer-assisted ultrasound navigation are provided, in particular for assisting medical personnel during diagnostic and/or therapeutic operations, as defined in the appended claims.

**BRIEF DESCRIPTION OF DRAWINGS****[0009]**

- 5 - Figure 1 schematically shows a computer-assisted ultrasound navigation system, in particular for providing assistance to medical personnel during diagnostic and/or therapeutic operations, according to a first embodiment;
- 10 - Figure 2 schematically shows a computer-assisted ultrasound navigation system, in particular for providing assistance to medical personnel during diagnostic and/or therapeutic operations, according to a second embodiment;
- 15 - Figure 3 illustrates a series of operations performed by the ultrasound navigation system according to the present invention; and
- Figure 4 illustrates a detail of the system in Figures 1 and 2.

**DESCRIPTION**

**[0010]** Figures 1 and 2 show a computer-assisted ultrasound navigation system, in particular for assisting medical personnel during diagnostic and/or therapeutic operations 100 embodied according to the present invention. The system 1 comprises an instrumental station 1 and an infrared (Figure 1) or electromagnet (Figure 2) tracking sensor 20, of known type, configured to cooperate with the instrumental station 1. An ultrasound probe 3 operates with an ultrasound device 4 interfaced with the instrumental station 1; the ultrasound probe 3 is of the hand-held type and is combined with a sensor 22, provided with first infrared or electromagnetic marker elements M-I-U or M-E-U to cooperate with the infrared or electromagnetic tracking sensor 20 (as better described hereinafter).

**[0011]** With special reference to Figure 4, the sensor 22 comprises an annular frame suitable for housing a central portion of the probe 3 and a mount extending radially from the annular frame. The mount carries first and second mutually aligned straight arms and a third arm perpendicular to the first two and having a shorter length than that of the first two. The end of each arm carries a spherical body that reflects infrared radiation or, in the case of the electromagnetic version, the annular frame is provided with two electromagnetic sensors (markers).

**[0012]** A surgical (or diagnostic) instrument 25 is provided with second infrared or electromagnetic instrument M-I-S or M-E-U marker elements 26 to cooperate with the infrared/electromagnetic tracking sensor 20 (as better described hereinafter).

**[0013]** In particular, the surgical instrument 25 (an operating tool in the example in Figure 1 and an endoscopic tool in the example in Figure 2) comprises a hand-held proximal portion 25a and an operative distal portion 25b; the marker instrument 26 is coupled to an intermediate

portion, leaving the distal portion 25b free. It should be noted that, for greater clarity of representation, the relative sizes of the elements shown in Figures 1 and 2 are not proportional to each other.

**[0014]** The instrumental station 1 (Figures 1 and 2) comprises a processing unit 4p, for example a computer of known type provided with a microcontroller 5 and memory 7, connected to each other; a data input user interface 6, for example including a keyboard and mouse; a display interface 8, for example a high-resolution LCD monitor; and a network interface 10, configured to support a private ad/or public network connection 11 (for example, an Ethernet network).

**[0015]** The instrumental station 1 further comprises a power connection 12, configured to provide the instrumental station 1 with electrical power by means of a wall-mounted power socket 13; a tracking input 15, configured to support a connection 17 (indifferently of the wireless or wire type) between the instrumental station 1, the infrared or electromagnetic tracking sensor 20 and the ultrasound device 4; and an energy storage unit 18, for example a battery, connected to the wall socket 13 by the power connection 12 and configured to temporarily power the instrumental station 1 in the event of an outage in the power provided by the wall socket 13.

**[0016]** According to the embodiment shown, the processing unit 4p is a personal computer (PC), comprising an external protective casing housed on a shelf of the instrumental station 1 and integral with the instrumental station 1 during any movement of the latter on the wheels 2.

**[0017]** The personal computer 4p comprises code instructions (software, described in detail hereinafter) based on algorithms for combining images that are configured to merge information arriving in real time from the ultrasound probe 3 with images previously taken (and therefore stored) by a computerized tomography (CT) or magnetic resonance (MR) diagnostic system. The result of the processing provided by this software is an image that merges the ultrasound image taken in real time with the stored images that have been adapted to the ultrasound image, instant by instant.

**[0018]** In the electromagnetic version (Figure 2) or infrared version (Figure 1), the above-indicated markers perform the role of both rotation and displacement identifiers of the related elements integral therewith (ultrasound probe 3 and surgical instrument 26).

**[0019]** The following description is therefore indifferent to whether the version considered is the one using infrared radiation or the one using electromagnetic waves.

**[0020]** The operations of the system 100 will now be described with reference to the flow chart in Figure 3.

**[0021]** Initially, this starts with a block 200 in which a plurality of two-dimensional images of a patient, obtained by X-ray or magnetic resonance techniques, are imported into the memory 7. The importing can be implemented using a network cable connected to a USB or Ethernet socket of the personal computer 4p or by using computer

media, such as a CD-ROM for example.

**[0022]** The two-dimensional images are preferably in the DICOM (Digital Imaging and COmmunications in Medicine) format that - as is known - defines the criteria for the communication, display, filing and printing of biomedical information, such as X-ray images for example. The DICOM standard is public, in the sense that its definition is accessible to everyone. Its diffusion turns out to be extremely advantageous because it enables having a solid information interchange base between apparatuses from different manufacturers, servers and PCs, specific for the biomedical environment.

**[0023]** The imported two-dimensional images regard a complete scan of a concerned anatomic region (for example, the abdomen).

**[0024]** Block 200 is followed by block 210, which starting from the imported two-dimensional images, performs (using known techniques) a very accurate three-dimensional reconstruction (image A) based on scans of the entire anatomic volume of interest.

**[0025]** Block 210 is followed by block 220, which transforms the three-dimensional reconstruction (A) processed by the block 210 into a three-dimensional pseudo ultrasound image (image B) using known methods [1], [2], [3] and [4].

[1] W. Wein et al., Automatic CT-Ultrasound Registration for Diagnostic Imaging and Image-guided Intervention, Medical Image Analysis 12(5), pp 577-585, October 2008

[2] J. L. Dillenseger et al., Fast simulation of ultrasound images from a CT volume, Computers in Biology and Medicine 2009

[3] P. Leroy et al., Rigid Registration of Freehand 3D Ultrasound and CT-Scan Kidney Images, International Journal of Computer Assisted Radiology and Surgery 2007

[4] S. Gill et al., Group-wise registration of ultrasound to CT images of human vertebrae, Medical Imaging 2009

**[0026]** The three-dimensional images A and B refer to the same reference system.

**[0027]** The three-dimensional pseudo ultrasound image is formed by a plurality of two-dimensional pseudo ultrasound images (B-2D). Subsequently, two-dimensional ultrasound images are taken directly of the patient by means of the ultrasound device 4.

**[0028]** The presence of the infrared or electromagnetic sensor 22 coupled to the ultrasound probe enables detecting the position of the sensor in the reference system of the tracking sensor 20 and therefore to orient the captured ultrasound image (image C-2D) in space.

**[0029]** The captured two-dimensional ultrasound image is selected and stored in the memory of the processing unit, together with the spatial coordinates that define it within the reference system of the viewer 20.

**[0030]** Subsequently, processing passes from block

230 to the following block 235, which performs an image comparison operation in order to find the two-dimensional pseudo ultrasound image (image B-2D) that is most similar to the previously stored ultrasound image (C-2D).

**[0031]** The comparison and the search for similarity between the B-2D and C-2D images is carried out by a medical operator in virtue of his/her experience or by means of known algorithms based on correlation methods.

**[0032]** The pseudo ultrasound image B-2D selected by the comparison operations is also stored with coordinates defined in the DICOM domain.

**[0033]** The next step of alignment, or adjustment, starts with block 250, which follows block 235.

**[0034]** In block 250, an operator manually selects at least three characteristic points on the two-dimensional ultrasound image C-2D taken of the patient by means of the ultrasound probe and previously stored and identifies the corresponding characteristic points on the two-dimensional pseudo image U-S B-2D, this also previously stored after the selection operations of block 235.

**[0035]** The identification of the characteristic points can be based on the operator's experience, in this way rendering the processing system capable of recognising shapes of known type and identifying regions of interest in the image, for example having high contrast with respect to adjacent areas or regular and differentiated shapes with respect to adjacent areas.

**[0036]** Block 250 is followed by block 260, in which a realignment operation is carried out between the reference system of the three-dimensional pseudo ultrasound image (image B) and therefore of image A and that of the operative space in which the ultrasound probe operates, in such a way that the identified characteristic points coincide in the respective reference systems of the two two-dimensional images. The realignment or adjustment operation is carried out using roto-translational algorithms known in the literature that - according to the selected characteristic points - calculate a roto-translational matrix that aligns the pseudo ultrasound image reference system (image B) with the reference system of the three-dimensional ultrasound graphic reconstruction regarding the volume associated with the two-dimensional ultrasound images (set of C-2D images) taken of the patient. After block 260, an operative step is performed (block 270 following block 260) in which the three-dimensional reconstruction (image A) processed in block 210 is displayed on the monitor 8.

**[0037]** The following are displayed on the monitor 8 at the same time:

- the two-dimensional ultrasound image acquired in real time by the ultrasound device 4 by means of the ultrasound probe 3; and
- the corresponding MR/TM two-dimensional image belonging to the three-dimensional reconstruction (image A), the respective reference systems being aligned thanks to the alignment or adjustment oper-

ation; the images - based on the operations carried out in block 260 and 270 - will thus be perfectly superimposable.

**[0038]** If the surgical instrument 26 is not equipped with sensors (as described above), according to virtual reality methods, it is possible to incorporate the image of the surgical instrument 25 in the two-dimensional image displayed on the monitor 8 based on data coming from the tracking sensor 20 according to the methods set forth in patent EP09425116.

**[0039]** The invention enables having an apparatus that is easy to use for the doctor and oriented to minimally invasive operations, capable of simultaneously displaying the image coming from computerized tomography or magnetic resonance together with the ultrasound image in real time.

**[0040]** In alternative to that described above, the operations in blocks 250 and 260 (realignment step) could comprise the following operations:

A plurality of two-dimensional ultrasound images of the concerned anatomic region (usually the abdomen, but not only) are taken by manually moving the ultrasound probe 3 with respect to the concerned anatomic region.

**[0041]** These two-dimensional images are also displayed in real time on the monitor 8.

**[0042]** The acquired two-dimensional images are processed by means of known ultrasound compound algorithms in order to obtain a very accurate three-dimensional graphic reconstruction (image C).

**[0043]** The presence of an infrared or electromagnetic sensor 22 coupled to the ultrasound probe 3 allows applying a noise reduction algorithm (NRA) in order to form two-dimensional scan planes in a three-dimensional volume with the technique of averaging algorithms.

**[0044]** The operator selects a scan plane P1 on the three-dimensional compound ultrasound image (image C) and identifies one or more characteristic points on this plane P1 (the characteristic points identify an anatomic structure that can be highlighted on the image). A first segmentation procedure is launched that selectively and automatically identifies, on a plurality of scan planes Pn different from that selected (P1), corresponding characteristic points (i.e. points that represent the same anatomic structure on different planes). In this way, a plurality of points Pi is provided that defines the anatomic structure in space on image C.

**[0045]** The operator selects a scan plane P2 on the three-dimensional pseudo ultrasound graphic reconstruction (image B) and identifies similar characteristic points on this plane (the characteristic points identify the aforesaid anatomic structure, but represented in the pseudo ultrasound domain).

**[0046]** A second segmentation procedure is launched that selectively and automatically identifies, on a plurality

of scan planes  $P_k$  different from that selected ( $P_2$ ), corresponding characteristic points (i.e. points that represent the same anatomic structure on different planes).

[0047] In this way, a plurality of points  $P_j$  is provided that defines the anatomic structure in space on image B.

[0048] The realignment operation is carried out using roto-translational algorithms known in the literature that - based on the first plurality of points  $P_i$  and the second plurality of points  $P_j$  - calculate a roto-translational matrix that aligns the pseudo ultrasound image reference system (B) with the reference system of the three-dimensional compound ultrasound graphic reconstruction (C).

## Claims

1. A computer-assisted ultrasound navigation system (100), **characterized in that** it comprises an instrumental unit (1) cooperating with:

- an ultrasound device (4) provided with an ultrasound probe (3) to capture a plurality of two-dimensional ultrasound images of a concerned region;
- an infrared or electromagnetic tracking sensor (20) adapted to detect the position of a sensor (22) coupled to the ultrasound probe and provided with infrared marker elements (M-I-U) or electromagnetic marker elements (M-E-U); said instrumental unit being configured to detect the position of the sensor in the reference system of the tracking sensor (20) and to orient the captured ultrasound images (C-2D image).

2. A system according to claim 1, wherein said computer is configured to implement:

importing means (200) which import a plurality of two-dimensional images, obtained by means of X-ray tomography CT or magnetic resonance MR techniques and related to a full scan of a concerned anatomic region, into the memory (7) of the computer; said two-dimensional images are preferably in DICOM (Digital Imaging and COmmunications in Medicine) format; first reconstruction means (210), which starting from imported two-dimensional images, form a three-dimensional reconstruction of the entire concerned anatomic region by generating a reconstructed three-dimensional image A; transformation means (220), which transform said three-dimensional image A into a three-dimensional pseudo ultrasound image B formed by a plurality of two-dimensional pseudo ultrasound images (B-2D); scanning means (230) by means of which at least one two-dimensional ultrasound image (e) of the concerned anatomic region is captured

by manually moving said ultrasound probe (3) with respect to said concerned region; said scanning means (230) being further adapted to detect the position of the sensor (22) coupled to the probe in the reference system of the tracking sensor (20) by orienting the captured two-dimensional ultrasound image in space, which is stored;

comparison means (235) configured to extract the two-dimensional pseudo ultrasound image (image B-2D) most similar to said stored ultrasound image (C-2D);

selection means (250) of characteristic points on said previously captured, detected and stored two-dimensional ultrasound image (C-2D) and on the extracted two-dimensional pseudo ultrasound image (B-2D);

alignment means (250,260) that, according to the selected characteristic points, perform a realignment operation between the reference system of the three-dimensional pseudo ultrasound image (image B) and thus of image A and that of the operative space in which the ultrasound probe operates, so that the identified characteristic points coincide in the respective reference systems of the two two-dimensional images.

3. A system according to claim 2, wherein the characteristic points are identified and selected manually by an operator.

4. A system according to claim 2, wherein the characteristic points are identified and selected by a shape recognition algorithm.

5. A system according to claim 2, wherein operative displaying means (270) are provided in which the following are contextually displayed on a monitor (8) of said computer:

- the two-dimensional ultrasound image acquired in real time by the ultrasound device (4) by means of the ultrasound probe (3); and
- the corresponding MR/TM two-dimensional image belonging to the reconstructed three-dimensional image A; said images - according to said realignment operation - being superimposable.

6. A system according to any of the preceding claims wherein, a surgical instrument is provided with infrared or electromagnetic instrument marker elements to cooperate with the tracking sensor (20); said computer (100) being configured to display - using virtual reality - the image of the surgical instrument (26) in the two-dimensional image displayed on the monitor (8) according to the data coming from the tracking sensor (20).


7. A system according to claim 2, wherein said realignment means are configured for:

- capturing a plurality of two-dimensional ultrasound images of the concerned anatomic region; 5
- processing said captured images by means of known ultrasound compound algorithms in order to obtain a three-dimensional graphic reconstruction, known as an ultrasound compound image C; 10
- selecting a scan plane P1 on the three-dimensional compound ultrasound image and identifying one or more characteristic points on such a plane P1; 15
- activating a first segmentation procedure that selectively and automatically identifies corresponding characteristic points on a plurality of scan planes Pn different from the selected scan plane (P1), providing a plurality of points Pi that define the anatomic structure in space on the ultrasound compound image; 20
- selecting a scan plane P2 on the three-dimensional pseudo ultrasound graphic reconstruction (image B) and identifying analogous characteristic points on such a plane P2; 25
- activating a second segmentation procedure that selectively and automatically identifies corresponding characteristic points on a plurality of scan planes Pk different from the selected scan plane (P2), providing a plurality of points Pj that define the anatomic structure in space on the three-dimensional pseudo ultrasound image (B); 30
- using roto-translation algorithms that - according to the first plurality of points Pi and the second plurality of points Pj - calculate a roto-translation matrix that aligns the pseudo ultrasound image reference system (B) with the reference system of the three-dimensional compound ultrasound graphic reconstruction (C). 35 40

45

50

55

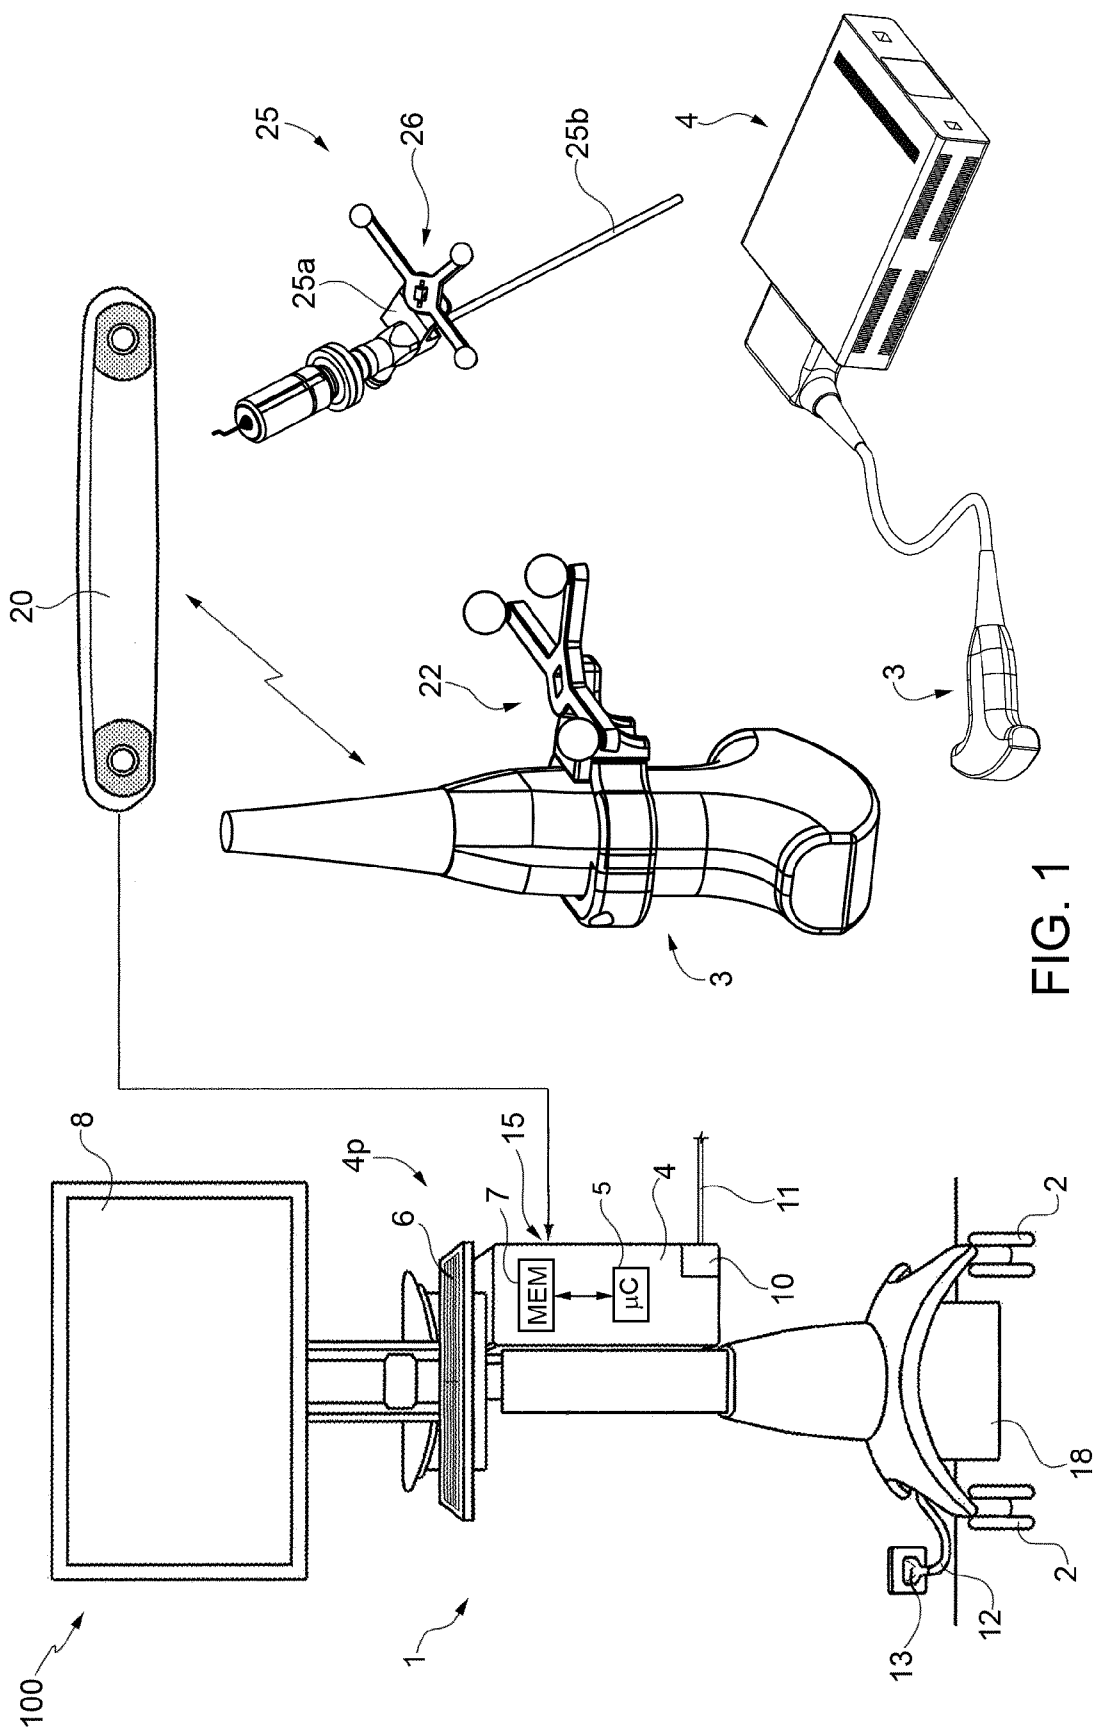

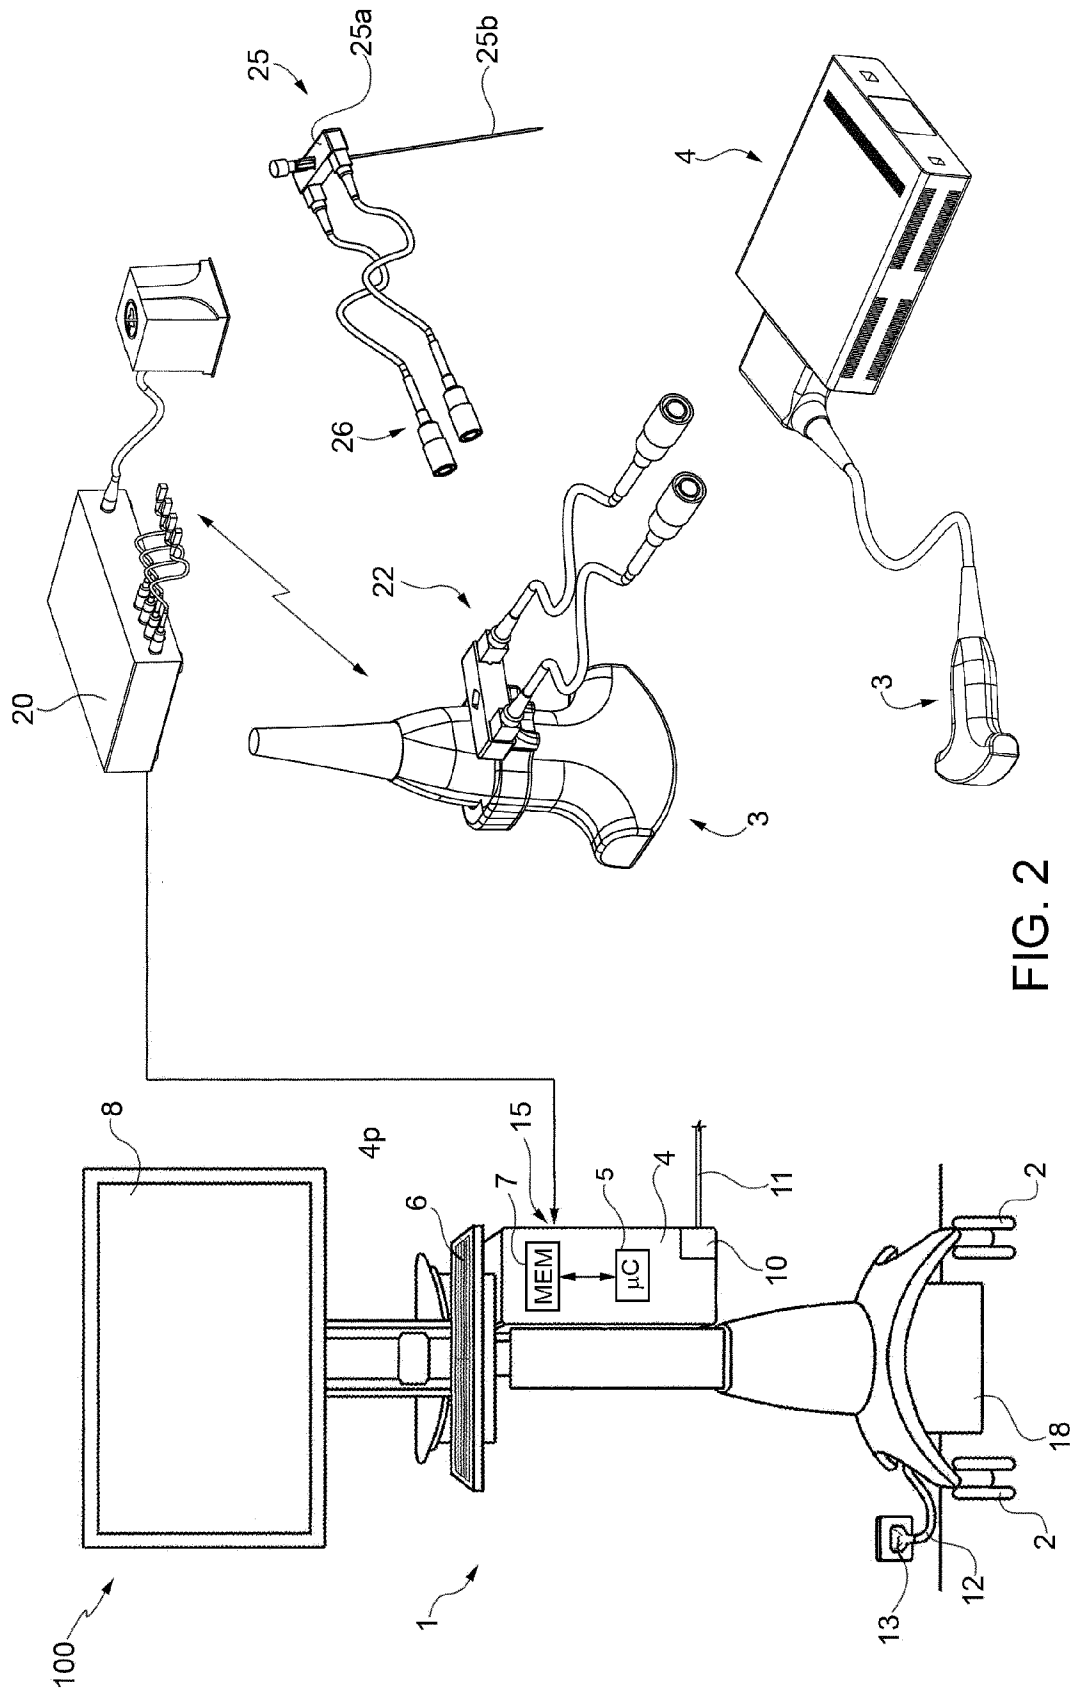


FIG. 2

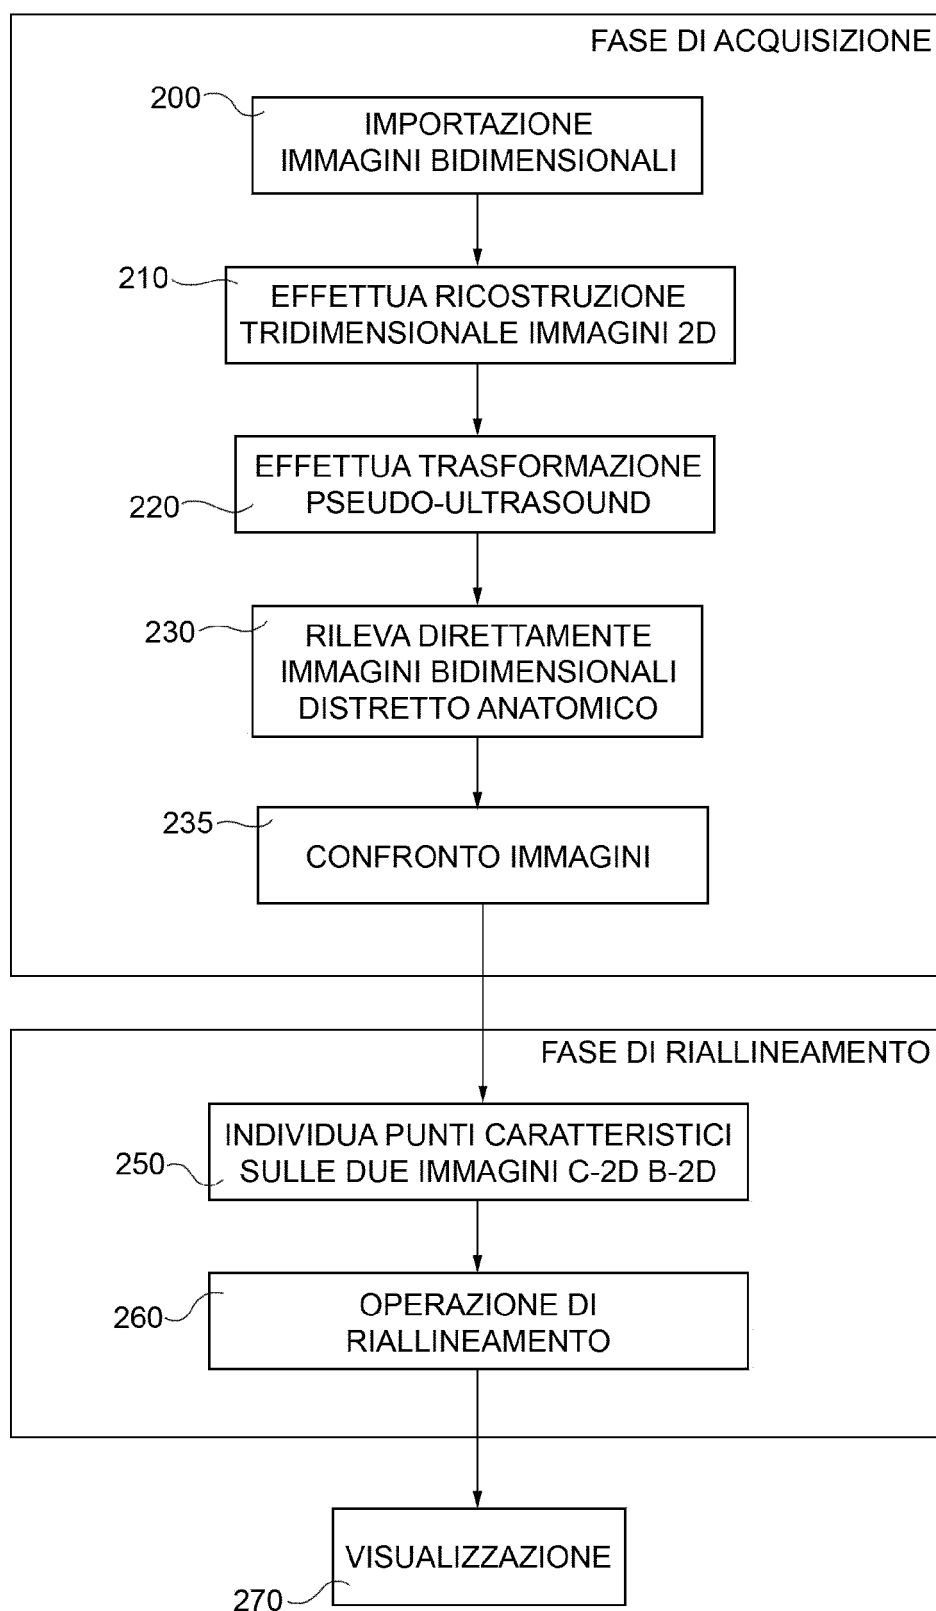


FIG. 3

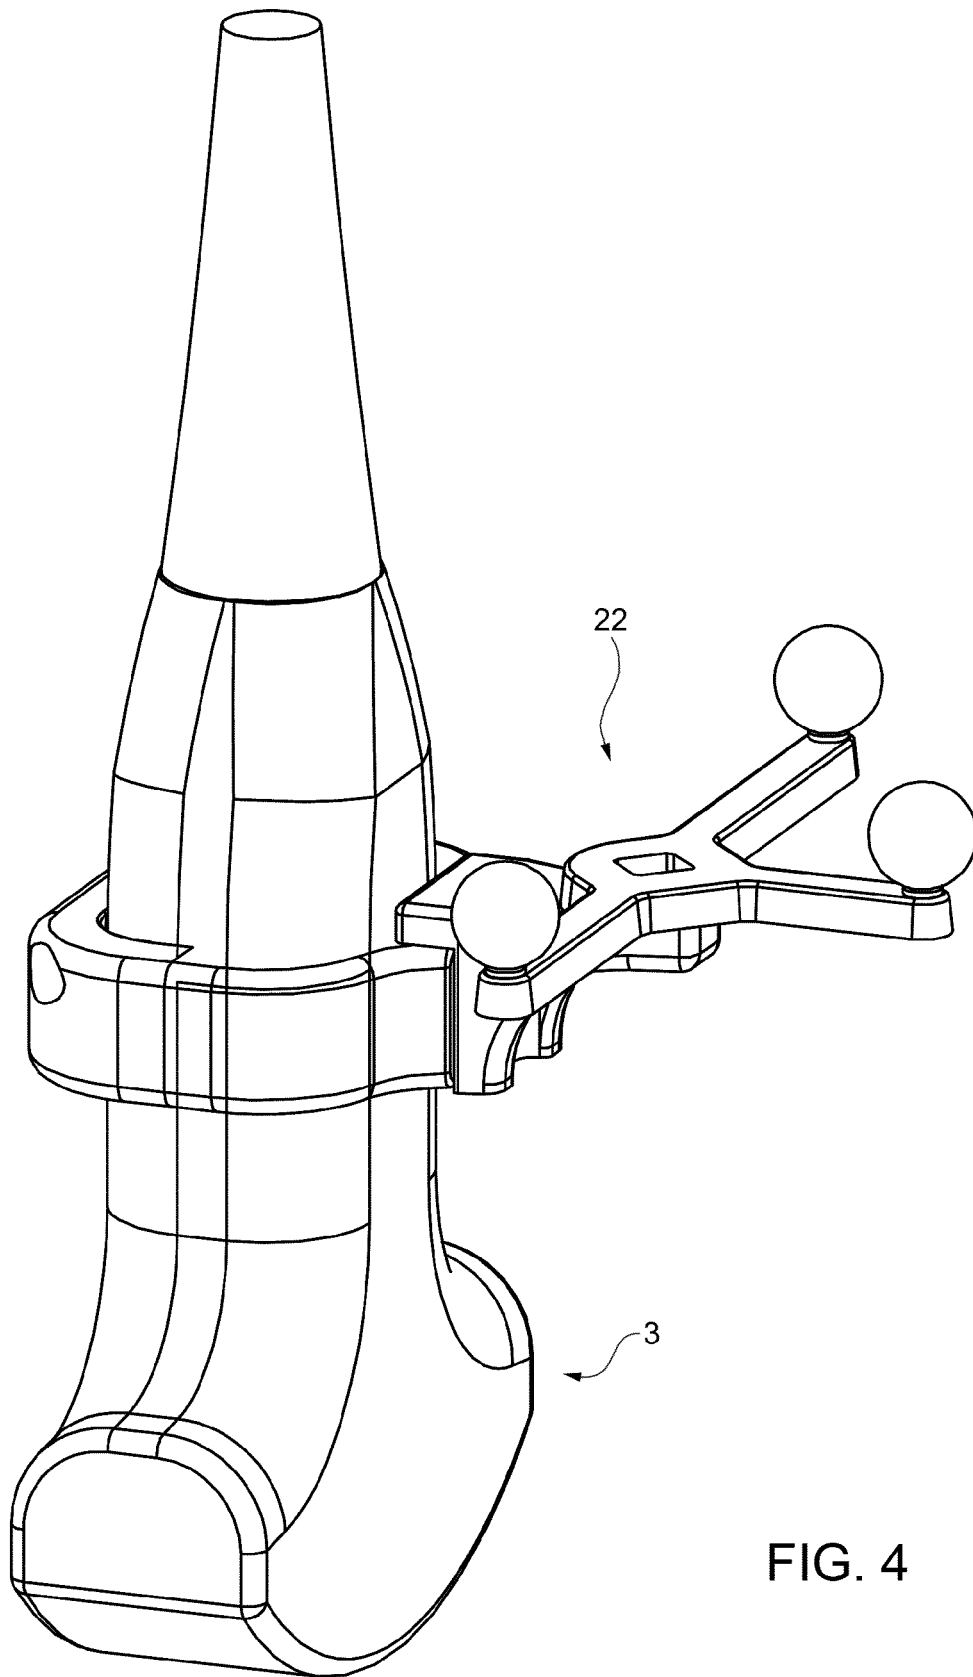


FIG. 4



## EUROPEAN SEARCH REPORT

 Application Number  
EP 14 16 4309

| DOCUMENTS CONSIDERED TO BE RELEVANT                                                                                                                                                                                                                    |                                                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                                                                                                                                                                                                                       |                                          |
|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------|
| Category                                                                                                                                                                                                                                               | Citation of document with indication, where appropriate, of relevant passages                                                                                                                                                                                                                                                                                                                                                   | Relevant to claim                                                                                                                                                                                                                                                                     | CLASSIFICATION OF THE APPLICATION (IPC)  |
| X                                                                                                                                                                                                                                                      | US 2013/144135 A1 (MAHFOUZ MOHAMED R [US] ET AL) 6 June 2013 (2013-06-06)<br>* abstract *<br>* figures 1-27 *<br>* paragraph [0053] - paragraph [0143] *<br>-----                                                                                                                                                                                                                                                               | 1-7                                                                                                                                                                                                                                                                                   | INV.<br>A61B8/00<br>A61B8/08<br>A61B6/00 |
| X                                                                                                                                                                                                                                                      | US 2006/036170 A1 (LACHAINE MARTIN [CA] ET AL) 16 February 2006 (2006-02-16)<br>* abstract *<br>* figures 1-12 *<br>* paragraph [0034] - paragraph [0079] *<br>-----                                                                                                                                                                                                                                                            | 1                                                                                                                                                                                                                                                                                     |                                          |
| X                                                                                                                                                                                                                                                      | US 2010/208963 A1 (KRUECKER JOCHEN [US] ET AL) 19 August 2010 (2010-08-19)<br>* abstract *<br>* figures 1-5 *<br>* paragraph [0022] - paragraph [0051] *<br>-----                                                                                                                                                                                                                                                               | 1                                                                                                                                                                                                                                                                                     |                                          |
| A                                                                                                                                                                                                                                                      | WEIN W ET AL: "Automatic CT-ultrasound registration for diagnostic imaging and image-guided intervention", MEDICAL IMAGE ANALYSIS, OXFORD UNIVERSITY PRESS, OXOFRD, GB, vol. 12, no. 5, 2 October 2008 (2008-10-02), pages 577-585, XP023783020, ISSN: 1361-8415, DOI: 10.1016/J.MEDIA.2008.06.006 [retrieved on 2008-06-19]<br>* abstract *<br>* figures 2-9 *<br>* Section 1. Introduction; and Section 2. Methods *<br>----- | 2-5,7                                                                                                                                                                                                                                                                                 | TECHNICAL FIELDS SEARCHED (IPC)<br>A61B  |
| A                                                                                                                                                                                                                                                      | US 2010/298704 A1 (PELISSIER LAURENT [CA] ET AL) 25 November 2010 (2010-11-25)<br>* abstract *<br>* figure 1 *<br>* paragraph [0129] - paragraph [0131] *<br>-----                                                                                                                                                                                                                                                              | 6                                                                                                                                                                                                                                                                                     |                                          |
| The present search report has been drawn up for all claims                                                                                                                                                                                             |                                                                                                                                                                                                                                                                                                                                                                                                                                 |                                                                                                                                                                                                                                                                                       |                                          |
| Place of search<br>Munich                                                                                                                                                                                                                              |                                                                                                                                                                                                                                                                                                                                                                                                                                 | Date of completion of the search<br>25 July 2014                                                                                                                                                                                                                                      | Examiner<br>Moehrs, Sascha               |
| CATEGORY OF CITED DOCUMENTS<br>X : particularly relevant if taken alone<br>Y : particularly relevant if combined with another document of the same category<br>A : technological background<br>O : non-written disclosure<br>P : intermediate document |                                                                                                                                                                                                                                                                                                                                                                                                                                 | T : theory or principle underlying the invention<br>E : earlier patent document, but published on, or after the filing date<br>D : document cited in the application<br>L : document cited for other reasons<br>.....<br>& : member of the same patent family, corresponding document |                                          |

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 14 16 4309

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.  
The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

25-07-2014

| Patent document<br>cited in search report | Publication<br>date | Patent family<br>member(s)                                                                                    | Publication<br>date                                                              |
|-------------------------------------------|---------------------|---------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------|
| US 2013144135 A1                          | 06-06-2013          | NONE                                                                                                          |                                                                                  |
| US 2006036170 A1                          | 16-02-2006          | CA 2574675 A1<br>EP 1774312 A2<br>US 2006036170 A1<br>WO 2006007716 A2                                        | 26-01-2006<br>18-04-2007<br>16-02-2006<br>26-01-2006                             |
| US 2010208963 A1                          | 19-08-2010          | CN 101681504 A<br>EP 2104919 A2<br>JP 2010515472 A<br>RU 2009124479 A<br>US 2010208963 A1<br>WO 2008065600 A2 | 24-03-2010<br>30-09-2009<br>13-05-2010<br>10-01-2011<br>19-08-2010<br>05-06-2008 |
| US 2010298704 A1                          | 25-11-2010          | US 2010298704 A1<br>US 2010298705 A1<br>WO 2010132985 A1                                                      | 25-11-2010<br>25-11-2010<br>25-11-2010                                           |

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

## REFERENCES CITED IN THE DESCRIPTION

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

### Patent documents cited in the description

- EP 09425116 A [0038]

### Non-patent literature cited in the description

- **W. WEIN et al.** Automatic CT-Ultrasound Registration for Diagnostic Imaging and Image-guided Intervention. *Medical Image Analysis*, October 2008, vol. 12 (5), 577-585 [0025]
- **J. L. DILLENSEGER et al.** Fast simulation of ultrasound images from a CT volume. *Computers in Biology and Medicine*, 2009 [0025]
- **P. LEROY et al.** Rigid Registration of Freehand 3D Ultrasound and CT-Scan Kidney Images. *International Journal of Computer Assisted Radiology and Surgery*, 2007 [0025]
- **S. GILL et al.** Group-wise registration of ultrasound to CT images of human vertebrae. *Medical Imaging*, 2009 [0025]

|                |                                                                                                    |         |            |
|----------------|----------------------------------------------------------------------------------------------------|---------|------------|
| 专利名称(译)        | 计算机辅助超声导航系统，用于在诊断和治疗操作期间提供帮助                                                                       |         |            |
| 公开(公告)号        | <a href="#">EP2818116A1</a>                                                                        | 公开(公告)日 | 2014-12-31 |
| 申请号            | EP2014164309                                                                                       | 申请日     | 2014-04-10 |
| [标]申请(专利权)人(译) | MASMEC                                                                                             |         |            |
| 申请(专利权)人(译)    | MASMEC S.P.A.                                                                                      |         |            |
| 当前申请(专利权)人(译)  | MASMEC S.P.A.                                                                                      |         |            |
| [标]发明人         | LARIZZA PIETRO<br>VINCI ANGELO MICHELE                                                             |         |            |
| 发明人            | LARIZZA, PIETRO<br>VINCI, ANGELO MICHELE                                                           |         |            |
| IPC分类号         | A61B8/00 A61B8/08 A61B6/00                                                                         |         |            |
| CPC分类号         | A61B8/4254 A61B6/5247 A61B8/4245 A61B8/4263 A61B8/4405 A61B8/463 A61B8/483 A61B8/523<br>A61B8/5261 |         |            |
| 优先权            | TO2013000527 2013-06-26 IT                                                                         |         |            |
| 其他公开文献         | EP2818116A9<br>EP2818116B1                                                                         |         |            |
| 外部链接           | <a href="#">Espacenet</a>                                                                          |         |            |

## 摘要(译)

一种计算机辅助超声成像系统（100），其中超声设备（4）设置有超声探头（3），用于捕获相关区域的多个二维超声图像。系统处理所获取的超声图像以获得三维复合超声图形重建（C），其与通过处理通过手段获得的多个二维图像而获得的三维伪超声图像（B）进行比较。X射线或磁共振技术（A）。在使用第一点测试方法的调整过程之后，或者替代地，使用第二结构方法，将图像C叠加在图像A上。

