

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
16 October 2008 (16.10.2008)

PCT

(10) International Publication Number
WO 2008/123595 A1

- (51) International Patent Classification:
A61B 8/08 (2006.01) A61B 8/06 (2006.01)
 - (21) International Application Number:
PCT/JP2008/056727
 - (22) International Filing Date: 28 March 2008 (28.03.2008)
 - (25) Filing Language: English
 - (26) Publication Language: English
 - (30) Priority Data:
60/920,639 29 March 2007 (29.03.2007) US
11/926,206 29 October 2007 (29.10.2007) US
 - (71) Applicant (for all designated States except US): **ALOKA CO., LTD.** [JP/JP]; 6-22-1, Mure, Mitaka-shi, Tokyo, 1818622 (JP).
 - (72) Inventor; and
 - (75) Inventor/Applicant (for US only): **TAMURA, Tadashi** [JP/US]; 1298 Hartford Turnpike, Unit 5H, North Haven, Connecticut, 06473 (US).
 - (74) Agents: **ISHIDA, Jun** et al.; 34-12, Kichijoji-honcho 1-chome, Musashino-shi, Tokyo, 1800004 (JP).
 - (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
 - (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
— with international search report

(54) Title: METHODS AND APPARATUS FOR ULTRASOUND IMAGING

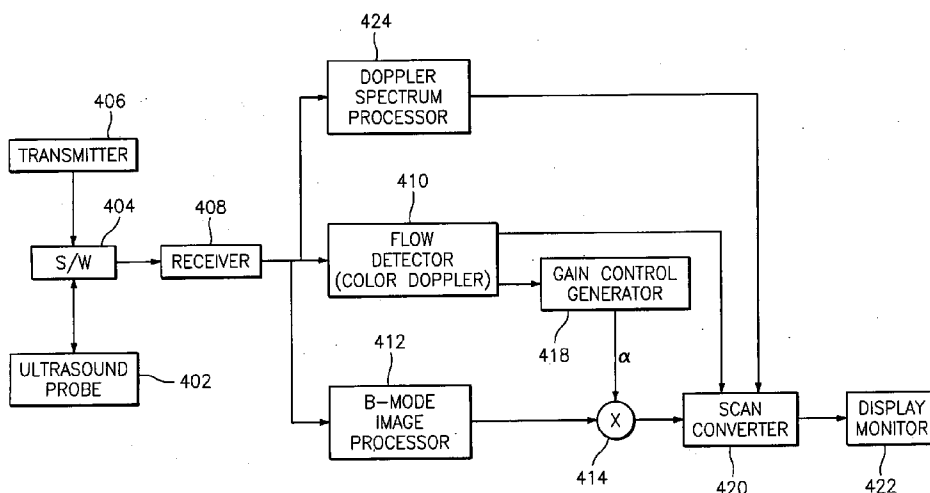


FIG. 4

(57) Abstract: Blood flow information is used to reduce noise manifest in blood vessel ultrasound B-mode images. A blood flow signal is obtained by a flow detector. After high-pass filtering, only the flow signal power in the blood vessel lumen remains, while signal power from stationary tissue region is suppressed. The flow signal component is used to calculate a flow component parameter that is used to generate a gain control signal α that reduces noise in a B-mode image.

WO 2008/123595 A1

DESCRIPTION

METHODS AND APPARATUS FOR ULTRASOUND IMAGING

5

TECHNICAL FIELD

The invention relates generally to the field of ultrasound imaging. More specifically, embodiments of the invention relate to methods and systems for reducing noise when imaging blood vessels.

10

BACKGROUND ART

Ultrasound is used to image various internal body structures such as organs like the heart and liver, blood vessels, and fetuses in pregnant women. B-mode imaging is a technique used to image blood vessels. In a vessel, blood
15 generally exhibits lower echo power than vessel walls or surrounding tissues do, resulting in high contrast. The surface layer of vessel walls, or intima, is of particular interest in diagnosing cardiovascular diseases such as arteriosclerosis, stenosis or coronary blockages. The
20 thickness of the intima is typically measured and is used in diagnosis. However, due to various causes, clutter noise usually appears in the lumen of blood vessels which makes the intima thickness measurement difficult.

25

There is a need to reduce noise present in blood vessel images.

DISCLOSURE OF THE INVENTION

The inventor has discovered that it would be desirable to have a system and method that uses blood flow information to reduce clutter noise in blood vessel B-mode images.

5 One aspect of the invention provides a method to suppress clutter noise manifest by returned ultrasound signals when imaging blood vessels by transmitting ultrasound signals to and receiving ultrasound signals from the blood vessels several times per position. The method includes
10 processing the returned ultrasound image signals to produce a B-mode image output, demodulating the returned ultrasound signals to produce Doppler signals, wall filtering the Doppler signals to only pass the flow components of the signals, calculating a flow component parameter, generating a
15 gain control signal α based on the flow component parameter, and controlling the output of the B-mode image processor with the gain control signal α wherein noise manifest in the B-mode image processor output is suppressed.

20 Another aspect of the invention provides a method to suppress clutter noise manifest by returned ultrasound signals when imaging blood vessels by transmitting ultrasound signals to and receiving ultrasound signals from the blood vessels several times per position. Methods according to this aspect of the invention include processing the returned
25 ultrasound image signals to produce a B-mode image output,

wall filtering the returned ultrasound image signals to only pass the flow components of the signals, calculating a flow component parameter, generating a gain control signal α based on the flow component parameter, and controlling the output of the B-mode image processor with the gain control signal α wherein noise manifest in the B-mode image processor output is suppressed.

Another aspect of the invention provides a system for suppressing clutter noise manifest by returned ultrasound signals when imaging blood vessels by transmitting ultrasound signals to and receiving ultrasound signals from the blood vessels several times per position. Systems according to this aspect of the invention include a receiver configured to receive the returned ultrasound image signals and output received signals, a B-mode image processor coupled to the receiver configured to output a B-mode processed image from the received signals, a Doppler flow detector coupled to the receiver configured to demodulate the returned ultrasound image signals to produce Doppler signals and having a wall filter configured to filter the Doppler signals and output only flow components of the Doppler signals, a gain control generator coupled to the Doppler flow detector configured to calculate a flow component parameter and generate a gain control signal α based on the flow components, and a signal combiner coupled to the gain control generator and the B-mode image processor, the signal combiner configured to modify the

B-mode processed image output with the gain control signal α wherein noise manifest in the B-mode processed image is suppressed.

Another aspect of the invention provides a system for
5 suppressing clutter noise manifest by returned ultrasound
signals when imaging blood vessels by transmitting ultrasound
signals to and receiving ultrasound signals from the blood
vessels several times per position. Systems according to this
aspect of the invention include a receiver configured to
10 receive the returned ultrasound image signals and output
received signals, a B-mode image processor coupled to the
receiver configured to output a B-mode processed image from
the received signals, an RF flow detector coupled to the
receiver, the flow detector having a wall filter configured
15 to filter the returned ultrasound RF signals and output only
flow components of the received signals, a gain control
generator coupled to the RF flow detector configured to
calculate a flow component parameter and generate a gain
control signal α based on the flow components, and a signal
20 combiner coupled to the gain control generator and the B-mode
image processor, the signal combiner configured to modify the
B-mode processed image output with the gain control signal α
wherein noise manifest in the B-mode processed image is
suppressed.

The details of one or more embodiments of the invention are set forth in the accompanying drawings and the description below. Other features, objects, and advantages of the invention will be apparent from the description and drawings, and from the claims.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is an exemplary B-mode image of a blood vessel exhibiting clutter noise.

FIG. 2 is an exemplary blood flow image.

10 FIG. 3 is an exemplary B-mode image after clutter noise suppression.

FIG. 4 is an exemplary system diagram of a clutter noise suppression system for B-mode images using Doppler flow processing.

15 FIG. 5 is an exemplary system diagram of a clutter noise suppression system for B-mode images using RF flow processing.

FIG. 6 is an exemplary Doppler flow detector.

FIG. 7 is an exemplary RF flow detector.

FIG. 8 is an exemplary gain control signal generator configured as a look-up table.

FIG. 9 is an exemplary gain control signal curve.

FIG. 10 is an exemplary gain control signal generator
5 configured as a look-up table

FIG. 11 is an exemplary gain control signal curve.

FIG. 12 is an exemplary gain control signal generator configured as a digital signal processor.

FIG. 13 is an exemplary gain control signal generator
10 configured as a digital signal processor.

FIG. 14 is an exemplary method for B-mode image clutter noise suppression using Doppler flow processing.

FIG. 15 is an exemplary method for B-mode image clutter noise suppression using RF flow processing.

15 BEST MODE FOR CARRYING OUT THE INVENTION

Embodiments of the invention will be described with reference to the accompanying drawing figures wherein like

numbers represent like elements throughout. Before
embodiments of the invention are explained in detail, it is
to be understood that the invention is not limited in its
application to the details of the examples set forth in the
5 following description or illustrated in the figures. The
invention is capable of other embodiments and of being
practiced or carried out in a variety of applications and in
various ways. Also, it is to be understood that the
phraseology and terminology used herein is for the purpose of
10 description and should not be regarded as limiting. The use
of "including," "comprising," or "having," and variations
thereof herein is meant to encompass the items listed
thereafter and equivalents thereof as well as additional
items. The terms "mounted," "connected," and "coupled," are
15 used broadly and encompass both direct and indirect mounting,
connecting, and coupling. Further, "connected," and "coupled"
are not restricted to physical or mechanical connections or
couplings.

It should be noted that the invention is not limited to
20 any particular software language described or that is implied
in the figures. One of ordinary skill in the art will
understand that a variety of alternative software languages
may be used for implementation of the invention. It should
also be understood that some of the components and items are
25 illustrated and described as if they were hardware elements,
as is common practice within the art. However, one of

ordinary skill in the art, and based on a reading of this detailed description, would understand that, in at least one embodiment, components in the method and system may be implemented in software or hardware.

5 Ultrasound is transmitted by an ultrasound transducer into a human body to image various organs, blood vessels, or a fetus in a pregnant woman. Scatterers in tissue scatter ultrasound and scattered ultrasound is returned to the transducer. A receive beamformer creates ultrasound beams and
10 a post processor creates an image of tissues from the amplitude of the returned ultrasound signal as a B-mode image.

 Blood vessels are often imaged, since they indicate cardiovascular conditions of patients. Intima thickness is often measured and used for diagnosis. However, images of
15 intima are often obscured by noise due to various causes. Blood flow information is usually acquired using color Doppler and spectral Doppler techniques.

 Color Doppler is a two-dimensional imaging technique commonly used for imaging blood flow by sending ultrasonic
20 waves into the blood vessel and detecting the scattered ultrasound from the moving red cells. It consists of many beams similar to B-mode image. In order to detect flow velocity, color Doppler transmits ultrasound signals several times per position to detect motion. To create a

two-dimensional flow image, the transmit position is shifted by sub-millimeters, or about the order of an ultrasound wavelength. The transmit position shifting is repeated about 100 times to cover several centimeters to create a
5 two-dimensional flow image. For a phased array transducer or a sector image format, the transmit direction is changed a small angle, for example, about 0.5-1.0 degrees. This is repeated approximately 100 times to cover about 90 degrees of a sector image. For each transmit position or direction,
10 ultrasound is transmitted several times. Received beamformed RF ultrasound signals undergo quadrature demodulation resulting in complex, Doppler I-Q signals.

The Doppler I-Q signals may contain blood flow signal components as well as stationary tissue signal components.
15 The stationary components are typically 30-40 dB greater than the blood flow components. Therefore, it is necessary to remove the stationary signal components in order to detect blood flow accurately.

A high-pass filter is applied to the received Doppler
20 signals from several transmits to obtain only flow signal components and is generally referred to as a wall filter because the filter removes vessel wall noise. The high-pass filter removes stationary signal components and passes only flow signal components. One form of the high-pass filter may
25 be a signal subtraction or 2-tap FIR where the Doppler signal

from a subsequent transmit is subtracted from the Doppler signal from a preceding transmit. The phase differences between the received Doppler I-Q signals from consecutive transmits indicate blood flow. Additionally, the power of the high-pass filtered Doppler I-Q signals indicates the existence of blood flow.

The system and method of the invention reduces clutter noise by decreasing B-mode signal amplitude using the above described blood flow signal. Even if clutter noise is present in a vessel lumen, blood flow is usually also present in the lumen at the same location. Clutter noise in blood vessels obscure intima and makes its thickness measurement difficult. A blood flow component parameter such as amplitude a , power a^2 or power raised to a power a^b , where b is a real number, may be calculated and used to generate a gain control signal α to suppress a B-mode image processor output signal at the same image position. The flow component parameters may be total or average quantities. The amount of clutter noise suppression may be proportional, or in a predetermined relationship to the flow component parameter used.

FIG. 1 shows a blood vessel 101 image output from a typical B-mode image processor with near 103 and far 105 walls. Clutter noise 107 is shown close to the near-wall 103. FIG. 2 shows a blood flow 201 image of the same vessel which is used to decrease the gain of the B-mode image shown in FIG.

1. FIG. 3 shows a resultant image with a clean vessel lumen 301.

FIG. 4 shows an ultrasound system with the invention. FIG. 14 shows a flow chart to describe the method. An
5 ultrasound signal is transmitted from the ultrasound probe 402 driven by the transmitter 406 through the transmit/receive switch 404. The receiver 408 receives the received ultrasound signal from the probe 402 through the switch 404 and processes the signal (step 1405). The
10 processed signal is coupled to a flow detector 410, a B-mode image processor 412 (step 1410) and a Doppler spectrum processor 424. The Doppler spectrum processor calculates a Doppler spectrum from the signal output by the receiver 408 and outputs the Doppler spectrum to a scan converter 420 in a
15 Doppler spectrum mode or a combination mode with either a B-mode image and/or a color flow image.

The flow detector 410 detects blood flow, and calculates and outputs a flow component parameter which may be amplitude a , power a^2 , power raised to a power a^b or a combination of
20 these values to the gain control signal generator 418. The gain control signal generator 418 generates a gain control signal α according to the flow component parameter and outputs the gain control signal α to a signal combiner 414 such as a multiplier or variable gain amplifier.

FIG. 6 shows a diagram of the Doppler flow detector 410. The Doppler flow detector includes a wall filter (*i.e.* high-pass filter) 602, a velocity calculator 604, a power calculator 606 and a variance calculator 606. The wall filter
5 receives the demodulated I-Q signals from the receiver 408 (step 1415). The high-pass filter cutoff or corner frequency may be user-adjustable and blocks low-frequency stationary tissue signal components passing only the higher-frequency flow signal components. The high-pass filter architecture may
10 be an FIR (finite impulse response) filter, an IIR (infinite impulse response) filter, a polynomial filter, a regression-line filter, or other type of architecture (step 1420). The flow signal components are coupled to the velocity calculator 604, the power calculator 606 and the variance
15 calculator 608.

The velocity calculator 604 calculates blood flow velocity which is output to a scan converter 420 which converts the velocity signal to a TV raster-scan velocity image. The velocity image is then displayed on a display
20 monitor 422 in a regular color flow mode. The variance calculator 608 calculates a variance or a turbulence indicator which is output to the scan converter 420 which converts the variance signal to a TV raster-scan variance image. The variance image is then displayed on the display
25 monitor 422 in a regular color flow mode. The power calculator 606 calculates flow component parameters signal

amplitude a , power a^2 , power raised to a power a^b and a combination of these values. The flow component parameters are generally calculated from the sampled high-pass filtered Doppler I-Q complex signals using

$$5 \quad a^2 = \sum_{i=1}^N z_i z_i^* , \quad (1)$$

where z_i is a high-pass filtered, complex Doppler signal, i may indicate an i^{th} component related to an ultrasound transmit sequence and N is the number of the high-pass filtered signal samples in discrete time. The $*$ indicates the
 10 complex conjugate. The number of filtered outputs is usually less than the number of transmit/receive signals.

The power calculator 606 may be a DSP, an FPGA, an ASIC or discrete components such as multipliers, adders, dividers and absolute calculators.

15 The other flow component parameters may be obtained from the power a^2 by

$$a = \sqrt{a^2} , \text{ or} \quad (2)$$

$$a^b = (\sqrt{a^2})^b . \quad (3)$$

Signal amplitude a and power raised to a power a^b may also be obtained by

$$a = \sum_{i=1}^N |z_i|, \text{ or} \quad (4)$$

$$a^b = \sum_{i=1}^N |z_i|^b. \quad (5)$$

- 5 The flow component parameters obtained by (4) and (5) are different than those derived by (2) and (3) because the order of processing steps are different (step 1425). The above flow component parameter calculations for amplitude a , power a^2 or power raised to a power a^b represent total values.
- 10 The total flow component parameters may be normalized by dividing each parameter value by the number of samples N to obtain average values at the cost of an extra calculation.

 The flow component parameters amplitude a , power a^2 , power raised to a power a^b or a combination of these values are coupled to the gain control generator 418 and is used to generate a gain control signal α . To increase signal-to-noise ratio (SNR), the flow component parameters may be combined into a combined flow component parameter such as $d_1 a + d_2 a^2 + \sum_i d_i a^{b(i)}$ where d_1 , d_2 and d_i are real numbers that

represent weighting factors and the i^{th} component $b(i)$ is also a real number. Combining more than one flow component parameter generally increases the signal-to-noise ratio and reduces noise that is uncorrelated. $d_1 a + d_2 a^2 + \sum_i d_i a^{b(i)}$ may be

5 calculated in the power calculator 606 and then output to the gain control generator 418 as well. The power calculator 606 may also output to the scan converter 420 in a color flow mode.

The gain control generator 418 may be, for example, a
10 digital signal processor (DSP) 1210 as shown in FIG. 12, or a look-up table (LUT) 810 as shown in FIG. 8, or an FPGA, an ASIC or discrete components such as multipliers and adders. The gain control generator 418 uses the flow component parameters as an input. FIG. 9 shows the LUT's 810 or DSP's
15 signal throughput as a response curve. If the input is small, the gain is high. If the input is large, the gain will be 0 or close to 0. The curve shown in FIG. 9 is exemplary. Other predetermined curves may be employed to suppress the signal output by the B-mode image processor 412 (step 1430). The
20 gain control generator 418 gain control signal α is output and coupled to the signal combiner 414.

The B-mode image processor 412 creates B-mode images and outputs an image to the signal combiner 414. The image is output to the scan converter 420 which converts the image

signal to a TV raster-scan image. The image is then displayed on the display monitor 422. The B-mode signal gain is controlled by the gain control signal α . For example, if the flow component parameter is large, the signal combiner's 414 gain is small, resulting in the suppression of clutter noise if present in the vessel lumen. Overall gain control removes clutter noise since blood flow exists only in the vessel lumen where clutter noise exists. If the flow component parameter is low, which may be the case in a tissue area, the signal combiner's 414 gain is large resulting in a B-mode tissue image of normal brightness. In this manner, the clutter noise, which is in the blood flow area, is reduced by the flow signal (step 1435).

In an alternate embodiment, the blood flow may be detected in the RF signal level using a cross-correlation or time-shift technique instead of using a color Doppler process. To detect flow velocity, the ultrasound signal is transmitted several times per position to detect motion. To create a two-dimensional flow image, the transmit position is shifted by sub-millimeters, or about the order of an ultrasound wavelength. The transmit position shifting is repeated about 100 times to cover several centimeters to create a two-dimensional flow image. For a phased array transducer or a sector image format, the transmit direction is changed about a small angle, for example, about 0.5-1.0 degrees. This is repeated approximately 100 times to cover about 90 degrees

of a sector image. For each transmit position or direction, ultrasound is transmitted several times. High-pass filtering is applied to the beamformed RF signal to remove tissue signals and pass blood flow signals. A blood flow component parameter such as amplitude c , power c^2 , power raised to a power c^b , where b is a real number, or a combination of these values may be calculated and used to generate a gain control signal α to suppress a B-mode image processor output signal at the same position. The flow component parameters may be total or average quantities.

FIGs. 5, 7, 10, 11 and 15 show the system and method. A transmitter 506 sends ultrasound signal to the ultrasound probe 502 through a switch 504. Ultrasound is transmitted to the human subject which may include vessels. Ultrasound is then returned to the ultrasound probe 502 which converts it to an electrical signal (step 1505). The returned ultrasound signal is coupled to a receiver 508 through the switch 504. The receiver processes the signal and outputs an RF signal to an RF flow detector 510, a B-mode image processor 512 (step 1510) and a Doppler spectrum processor 524. The Doppler spectrum processor calculates a Doppler spectrum from the signal output by the receiver 508 and outputs the Doppler spectrum to a scan converter 520 in a Doppler mode or a combination mode with either a B-mode image and/or a color flow mode. The B-mode image processor 512 processes the RF signal and outputs a B-mode image signal. The RF flow

detector 510 processes the RF signal and outputs a flow component parameter amplitude c , power c^2 , power raised to a power c^b or a combination of these values to a gain control signal generator 518.

5 FIG. 7 shows a diagram of the RF flow detector 510. The RF flow detector includes a high-pass filter 702, a velocity calculator 704, a power calculator 706 and a variance calculator 708. One form of the high-pass filter may be a signal subtraction or 2-tap FIR where the received RF signal from a subsequent transmit is subtracted from the RF signal from a preceding transmit. This performs high-pass filtering among two or more transmit sequences. The high-pass filtering among several transmits removes vessel wall noise and is referred to as a wall filter. The high-pass filter may use received RF signals from two or more transmits in higher order FIR, IIR or other filter types. The high-pass filter, whose cut-off frequency may be user-adjustable and blocks low-frequency stationary tissue signal components passing only the higher-frequency flow signal components from the RF signals received from the receiver 508 (step 1520) and is coupled to the velocity calculator 704, the power calculator 706 and the variance calculator 708.

The velocity calculator 704 calculates blood flow velocity from the high-pass filtered RF signal. The velocity is output to a scan converter 520 which converts velocity

signal to a TV raster-scan velocity image. The velocity image is then displayed on the display monitor 522 in a regular color flow mode. The variance calculator 708 calculates variance as a turbulence indicator from the high-pass filtered RF signal. The variance is output to the scan converter 520 which converts the variance signal to a TV raster-scan variance image. The variance image is then displayed on the display monitor 522 in a regular color flow mode. The power calculator 706 calculates a flow component parameter amplitude c , power c^2 , or power raised to a power c^b from the sampled RF signals using

$$c = \sum_{i=1}^N |x_i|, \quad (6)$$

$$c^2 = \sum_{i=1}^N x_i^2, \text{ and} \quad (7)$$

$$c^b = \sum_{i=1}^N |x_i|^b \quad (8)$$

where, x_i are the high-pass filtered RF signal samples and N is the number of high-pass filtered signal samples.

The power calculator 706 may be a DSP, an FPGA, an ASIC or discrete components such as multipliers, adders, dividers and absolute calculators.

Alternately, one of these values may be calculated and the other values may be obtained from the first calculated value as follows. For example, the power c^2 may be first calculated, and the amplitude c and the power raised to a power c^b obtained from the power c^2 by

$$c^2 = \sum_{i=1}^N x_i^2, \quad (9)$$

$$c = \sqrt{c^2}, \text{ and} \quad (10)$$

$$c^b = (\sqrt{c^2})^b. \quad (11)$$

The flow component parameters calculated by (10) and (11) are different from those calculated by (6) and (8) because the order of processing steps are different (step 1525). The above flow component parameter calculations for amplitude c , power c^2 or power raised to a power c^b represent total values. The total flow component parameters may be normalized by dividing each parameter value by the number of samples N to obtain average values at the cost of an extra calculation.

The gain control generator 518 receives the flow component parameters amplitude c , power c^2 , power raised to a power c^b , or a combination of these values, and generates a gain control signal α . To increase signal-to-noise ratio (SNR), the flow component parameters may be combined into a combined flow component parameter such as $d_1c + d_2c^2 + \sum_i d_i c^{b(i)}$

where d_1 , d_2 and d_i are real numbers that represent weighting factors and the i^{th} component $b(i)$ is also a real number.

Combining more than one flow component parameter generally increases the signal-to-noise ratio and reduces noise that is uncorrelated. $d_1c + d_2c^2 + \sum_i d_i c^{b(i)}$ may be calculated in the power calculator 706 and then output to the gain control generator 518 as well. The power calculator 706 may also output to the scan converter in a color flow mode.

The gain control generator 518 may be a digital signal processor DSP 1310 as shown in FIG. 13 or a look-up table (LUT) 1010 as shown in FIG. 10, or an FPGA, an ASIC or discrete components such as multipliers and adders. An example response of the DSP 1310 or LUT 1010 is shown in FIG. 11. For a small value of a flow component parameter, the gain control signal α is high while a high value may yield a gain close to 0. The curve shown in FIG. 11 is exemplary. Other predetermined curves may be employed to suppress the signal output by the B-mode image processor 512 (step 1530). The

gain control generator 518 gain control signal α is output and coupled to a signal combiner 514.

The signal combiner 514 may be a multiplier or variable gain amplifier. The signal combiner 514 multiplies the B-mode
5 image with the gain control signal α and outputs a B-mode image to the scan converter 520 which converts the image signal to an TV raster-scan image. The image is then displayed on the display monitor 522 (step 1535).

The RF flow detection system and method may use a wide
10 band ultrasound signal and therefore offer higher spatial resolution than the Doppler flow detection does.

One or more embodiments of the present invention have been described. Nevertheless, it will be understood that various modifications may be made without departing from the
15 spirit and scope of the invention. Accordingly, other embodiments are within the scope of the following claims.

CLAIMS

1. A method to suppress clutter noise manifest by returned ultrasound signals when imaging blood vessels by transmitting
5 ultrasound signals to and receiving ultrasound signals from the blood vessels several times per position comprising:
 processing the returned ultrasound image signals to produce a B-mode image output;
 demodulating the returned ultrasound signals to produce
10 Doppler signals;
 wall filtering the Doppler signals to only pass the flow components of the signals;
 calculating a flow component parameter;
 generating a gain control signal α based on the flow
15 component parameter; and
 controlling the output of the B-mode image processor with the gain control signal α wherein noise manifest in the B-mode image processor output is suppressed.
- 20 2. The method according to claim 1 wherein wall filtering further comprises receiving Doppler signals and processing the received Doppler signals using a high-pass filter response.
- 25 3. The method according to claim 1 wherein calculating the flow component parameter further comprises calculating an amplitude a from the wall filtered Doppler signals.

4. The method according to claim 1 wherein calculating the flow component parameter further comprises calculating a power a^2 from the wall filtered Doppler signals.

5 5. The method according to claim 1 wherein calculating a flow component parameter further comprises:

calculating an amplitude a , a power a^2 and a power raised to a power $a^{b(i)}$, where the power $b(i)$ is a real number, from the wall filtered Doppler signals;

10 multiplying the amplitude a , power a^2 and power raised to a power $a^{b(i)}$, with a corresponding weight d_1 , d_2 and d_i , where d_1 , d_2 and d_i the i^{th} component are real numbers; and

summing together the weighted amplitude d_1a , power d_2a^2 and power raised to a power $d_i a^{b(i)}$ as a combined flow

15 component parameter $d_1a + d_2a^2 + \sum_i d_i a^{b(i)}$.

6. The method according to claim 1 wherein the gain control signal α is a predetermined curve response based on the flow component parameter.

20

7. A method to suppress clutter noise manifest by returned ultrasound signals when imaging blood vessels by transmitting ultrasound signals to and receiving ultrasound signals from the blood vessels several times per position comprising:

25 processing the returned ultrasound image signals to produce a B-mode image output;

wall filtering the returned ultrasound image signals to only pass the flow components of the signals;

calculating a flow component parameter;

generating a gain control signal α based on the flow component parameter; and

controlling the output of the B-mode image processor with the gain control signal α wherein noise manifest in the B-mode image processor output is suppressed.

10 8. The method according to claim 7 wherein wall filtering further comprises receiving RF signals and processing the received RF signals using a high-pass filter response.

9. The method according to claim 7 wherein calculating the flow component parameter further comprises calculating an amplitude c from the wall filtered signals.

10. The method according to claim 7 wherein calculating the flow component parameter further comprises calculating a power c^2 from the wall filtered signals.

11. The method according to claim 7 wherein calculating a flow component parameter further comprises:
calculating an amplitude c , a power c^2 and a power raised to a power $c^{b(i)}$, where the power $b(i)$ is a real number, from the wall filtered signals;

multiplying the amplitude c , power c^2 and power raised to a power $c^{b(i)}$, with a corresponding weight d_1 , d_2 and d_i , where d_1 , d_2 and d_i the i^{th} component are real numbers; and

5 summing together the weighted amplitude d_1c , power d_2c^2 and power raised to a power $d_i c^{b(i)}$ as a combined flow component parameter $d_1c + d_2c^2 + \sum_i d_i c^{b(i)}$.

12. The method according to claim 7 wherein the gain control signal α is a predetermined curve response based on the flow
10 component parameter.

13. A system for suppressing clutter noise manifest by returned ultrasound signals when imaging blood vessels by transmitting ultrasound signals to and receiving ultrasound
15 signals from the blood vessels several times per position comprising:

a receiver configured to receive the returned ultrasound image signals and output received signals;

a B-mode image processor coupled to the receiver
20 configured to output a B-mode processed image from the received signals;

a Doppler flow detector coupled to the receiver configured to demodulate the returned ultrasound image signals to produce Doppler signals and having a wall filter
25 configured to filter the Doppler signals and output only flow components of the Doppler signals;

a gain control generator coupled to the Doppler flow detector configured to calculate a flow component parameter and generate a gain control signal α based on the flow components; and

5 a signal combiner coupled to the gain control generator and the B-mode image processor, the signal combiner configured to modify the B-mode processed image output with the gain control signal α wherein noise manifest in the B-mode processed image is suppressed.

10

14. The system according to claim 13 wherein the wall filter response is a high-pass filter response.

15 15. The system according to claim 13 wherein the flow component parameter is amplitude a .

16. The system according to claim 13 wherein the flow component parameter is power a^2 .

20 17. The system according to claim 13 wherein the flow component parameter is a combined flow component parameter $d_1 a + d_2 a^2 + \sum_i d_i a^{b(i)}$ comprising an amplitude a , a power a^2 and a power raised to a power $a^{b(i)}$, where the power $b(i)$ is a real number, from the wall filtered Doppler signals, where the
 25 amplitude a , power a^2 and power raised to a power $a^{b(i)}$ are multiplied with a corresponding weight d_1 , d_2 and d_i , where

d_1 , d_2 and d_i , the i^{th} component are real numbers, and summed together.

18. The system according to claim 13 wherein the gain
5 control signal α is a predetermined curve response based on the flow components.

19. A system for suppressing clutter noise manifest by
returned ultrasound signals when imaging blood vessels by
10 transmitting ultrasound signals to and receiving ultrasound signals from the blood vessels several times per position comprising:

a receiver configured to receive the returned ultrasound image signals and output received signals;

15 a B-mode image processor coupled to the receiver configured to output a B-mode processed image from the received signals;

an RF flow detector coupled to the receiver, the flow detector having a wall filter configured to filter the
20 returned ultrasound RF signals and output only flow components of the received signals;

a gain control generator coupled to the RF flow detector configured to calculate a flow component parameter and generate a gain control signal α based on the flow
25 components; and

a signal combiner coupled to the gain control generator and the B-mode image processor, the signal combiner configured to modify the B-mode processed image output with

the gain control signal α wherein noise manifest in the B-mode processed image is suppressed.

20. The system according to claim 19 wherein the wall filter
5 response is a high-pass filter response.

21. The system according to claim 19 wherein the flow component parameter is amplitude c .

10 22. The system according to claim 19 wherein the flow component parameter is power c^2 .

23. The system according to claim 19 wherein the flow component parameter is a combined flow component parameter
15 $d_1c + d_2c^2 + \sum_i d_i c^{b(i)}$ comprising an amplitude c , a power c^2 and a power raised to a power $c^{b(i)}$, where the power $b(i)$ is a real number, from the wall filtered RF signals, where the amplitude c , power c^2 and power raised to a power $c^{b(i)}$ are multiplied with a corresponding weight d_1 , d_2 and d_i , where
20 d_1 , d_2 and d_i the i^{th} component are real numbers, and summed together.

24. The system according to claim 19 wherein the gain control signal α is a predetermined curve response based on
25 the flow components.

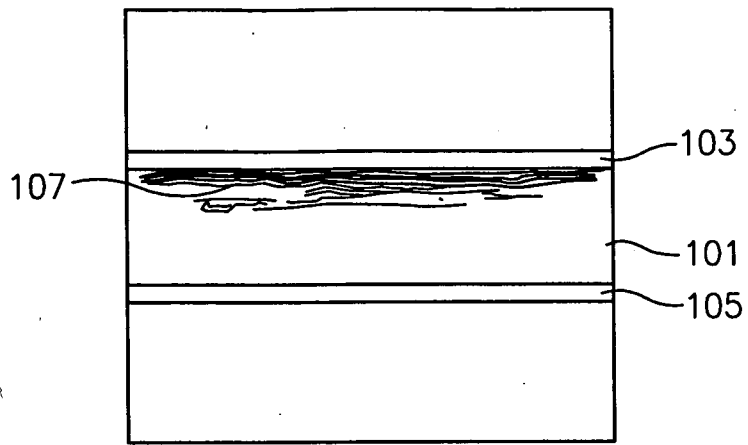


FIG. 1

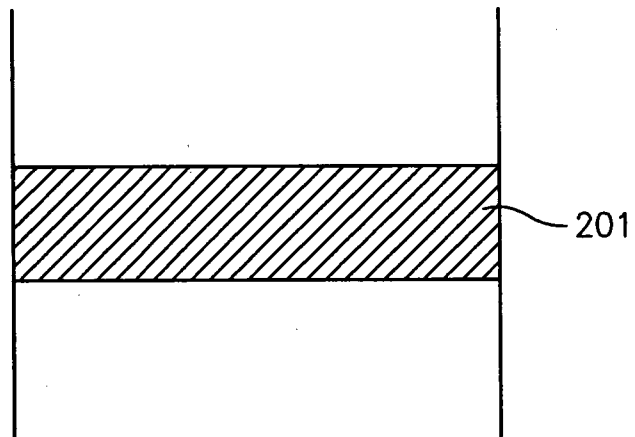


FIG. 2

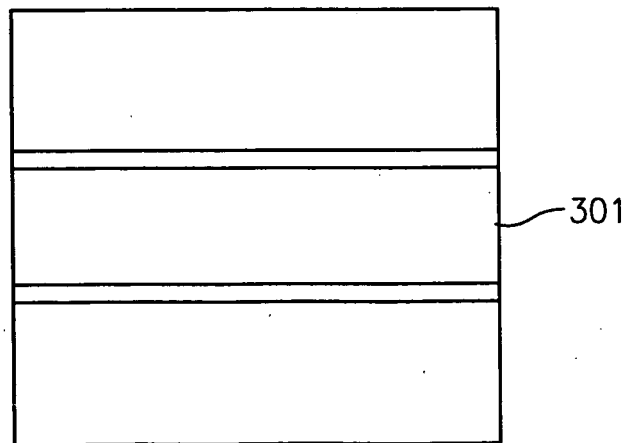


FIG. 3

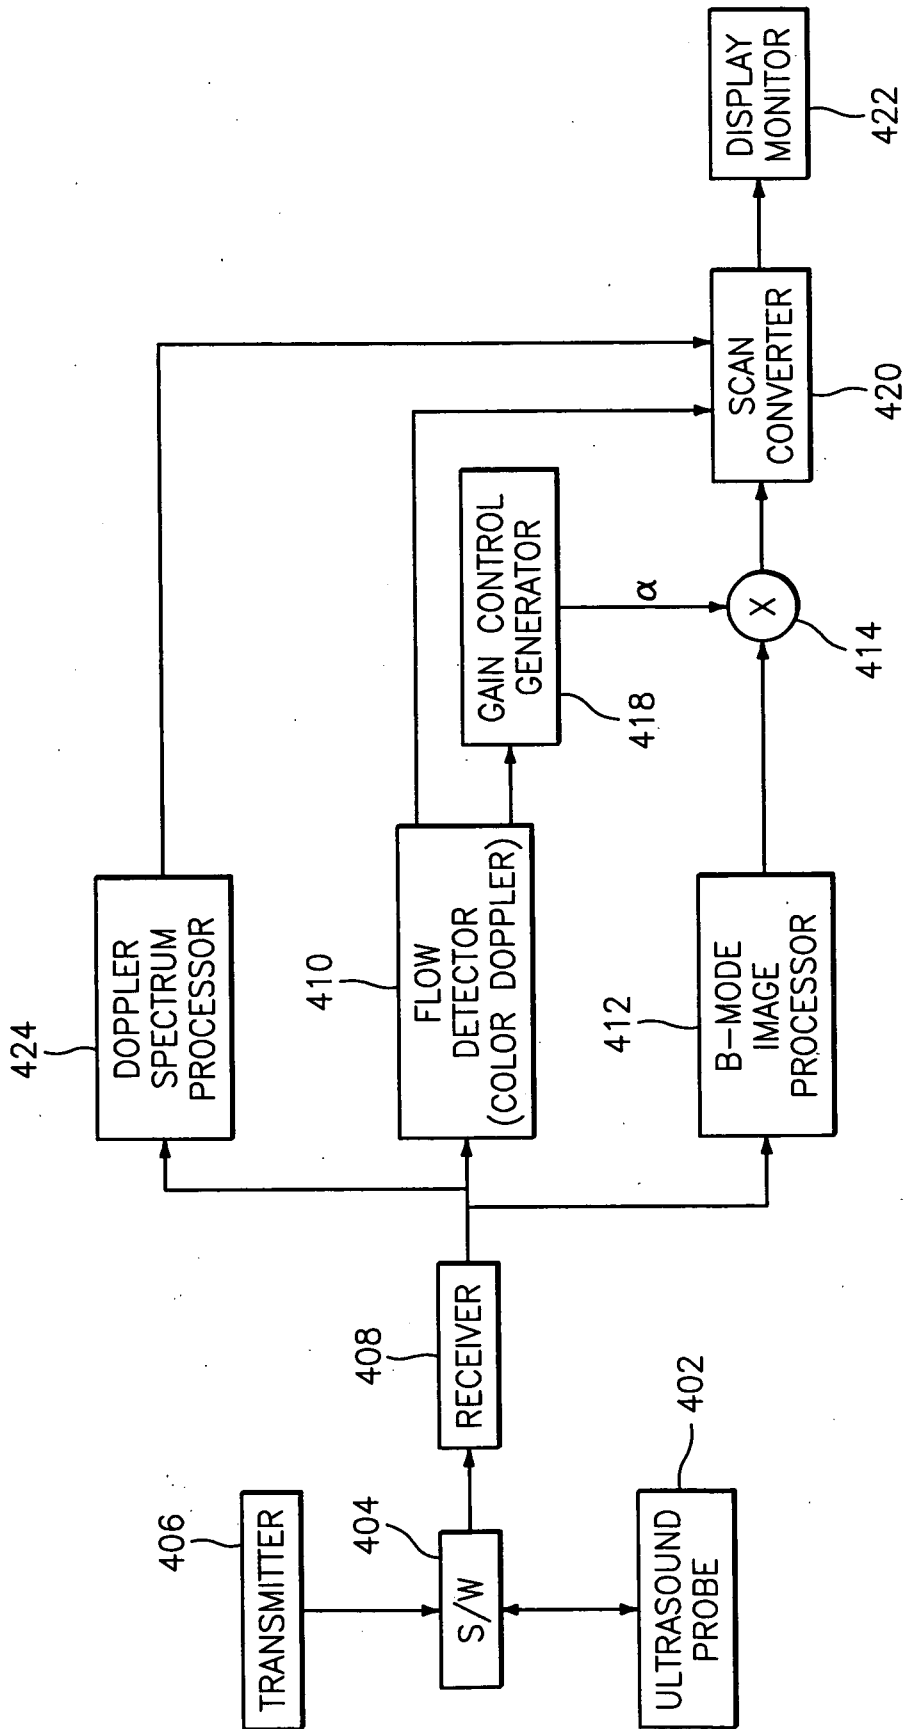


FIG. 4

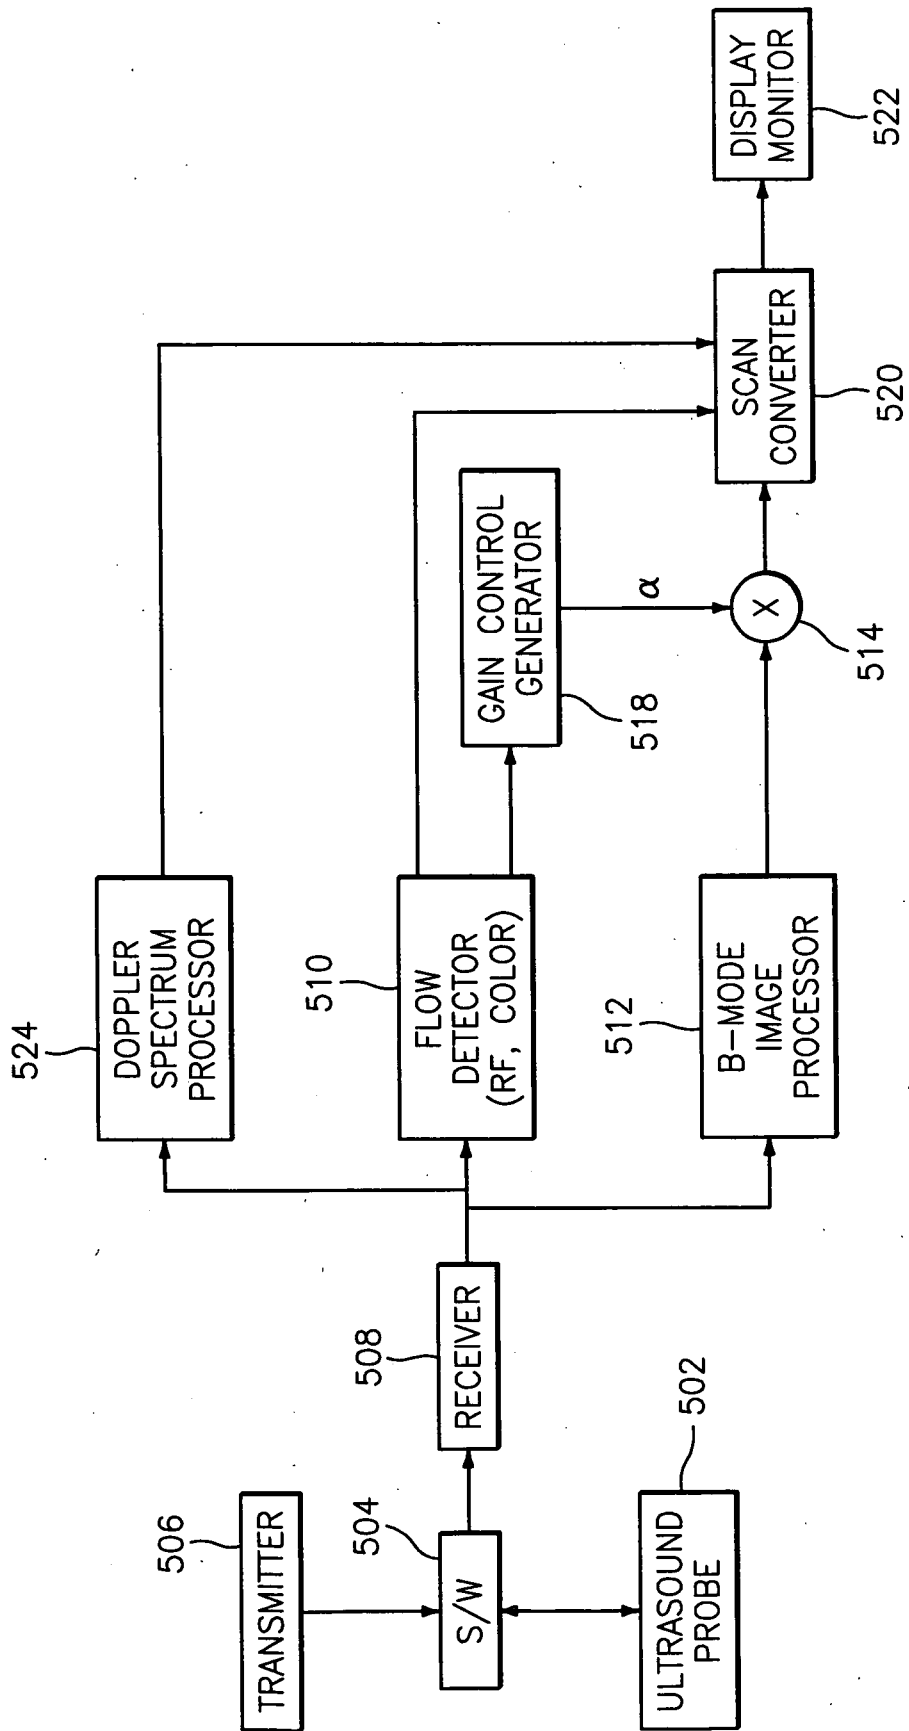


FIG. 5

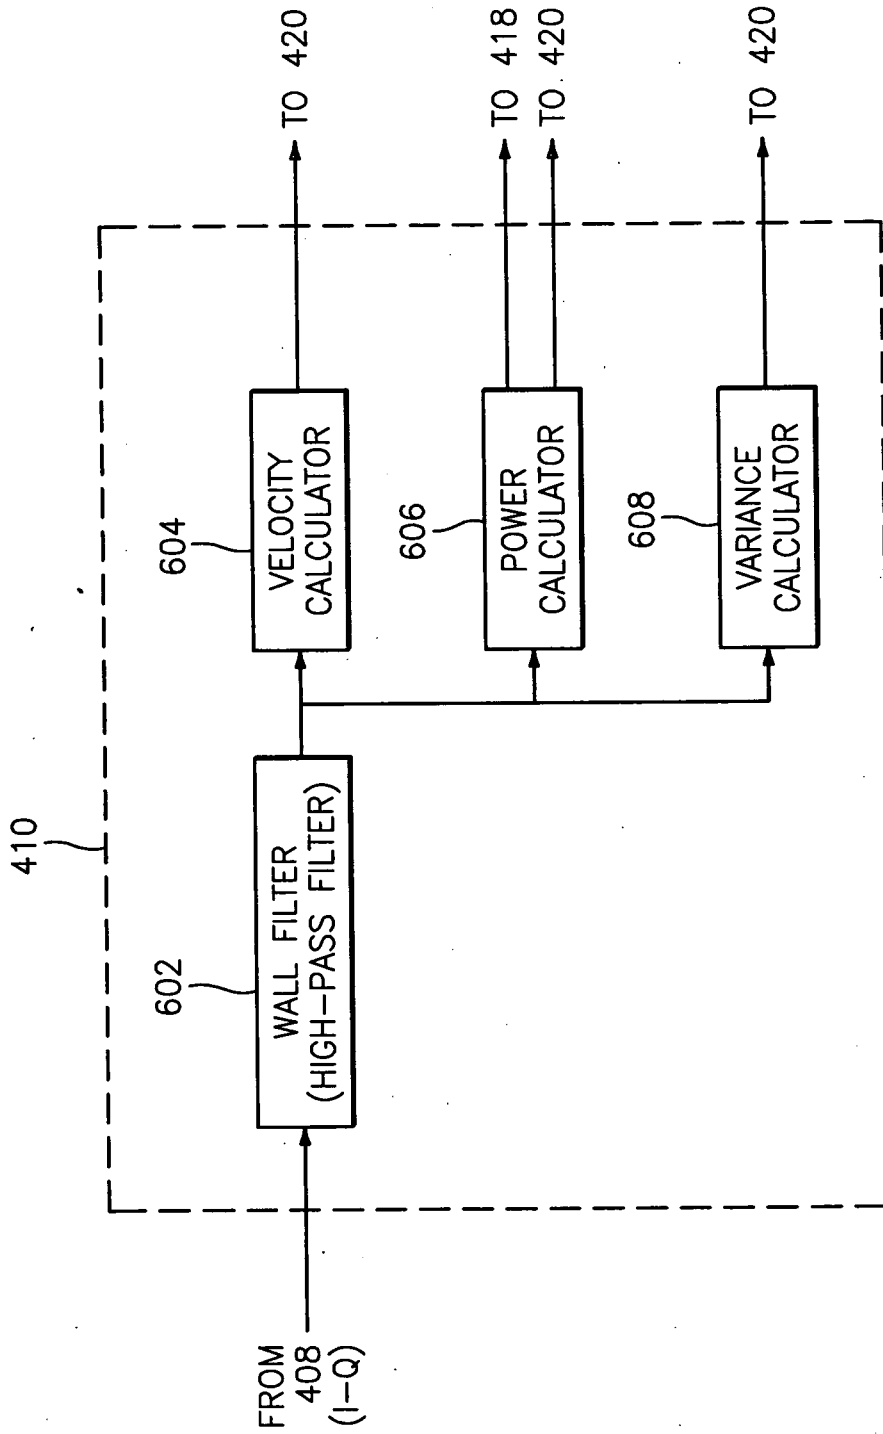


FIG. 6

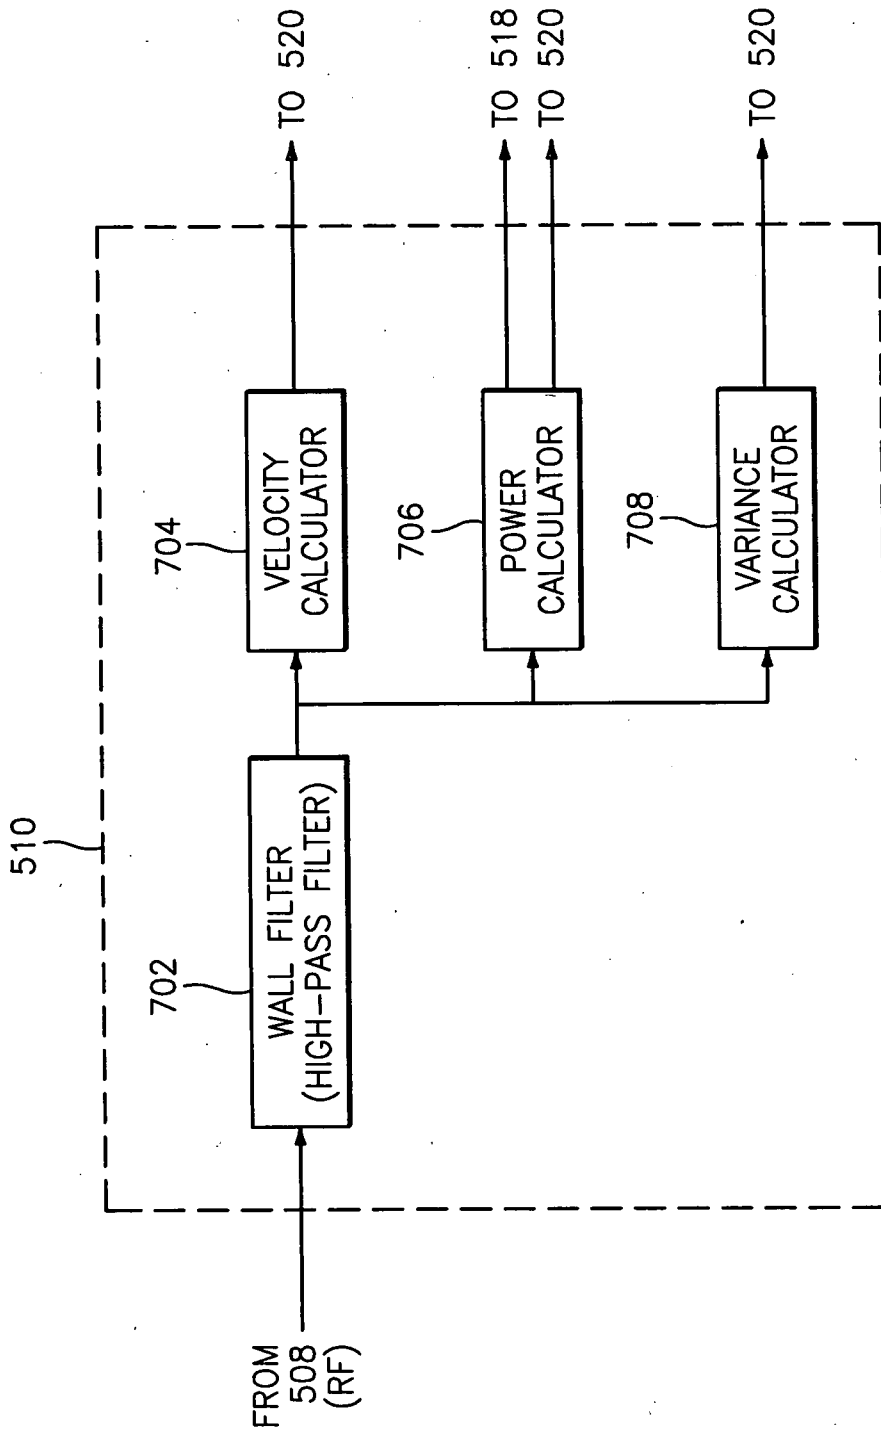


FIG. 7

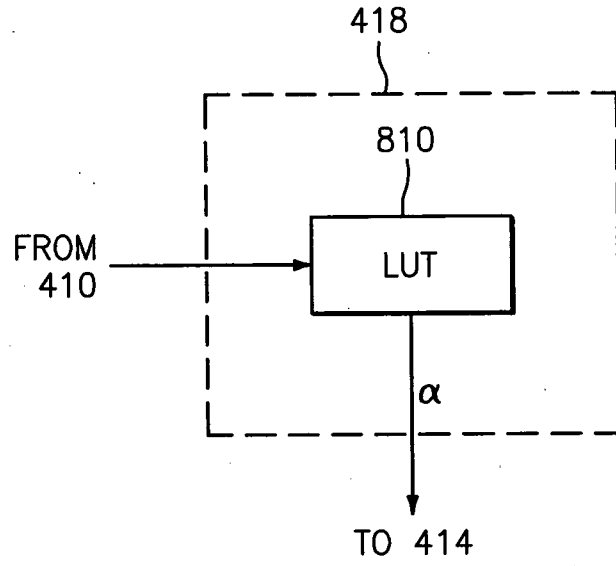


FIG. 8

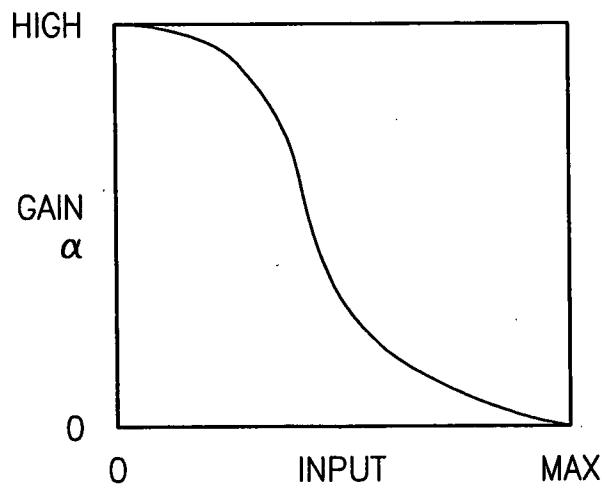


FIG. 9

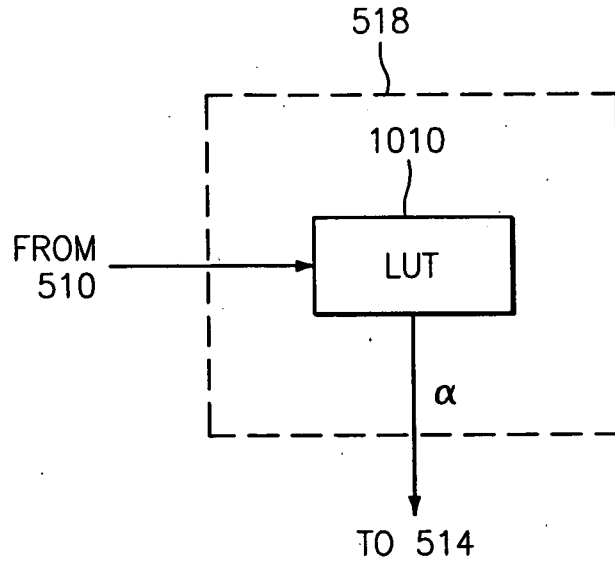


FIG. 10

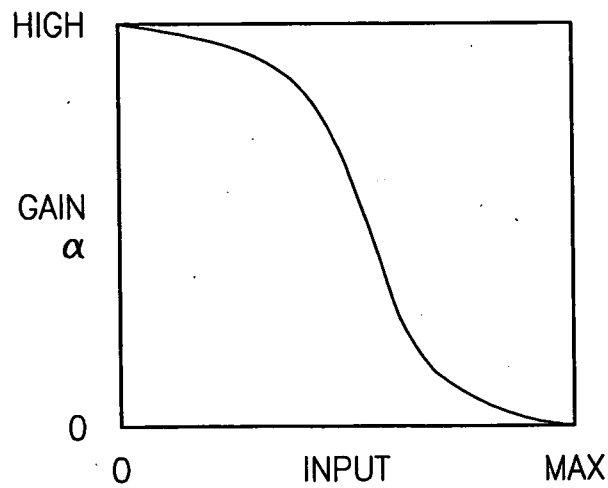


FIG. 11

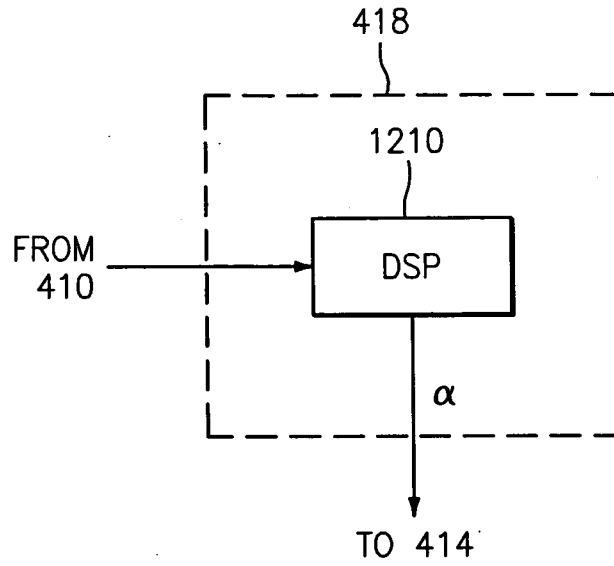


FIG. 12

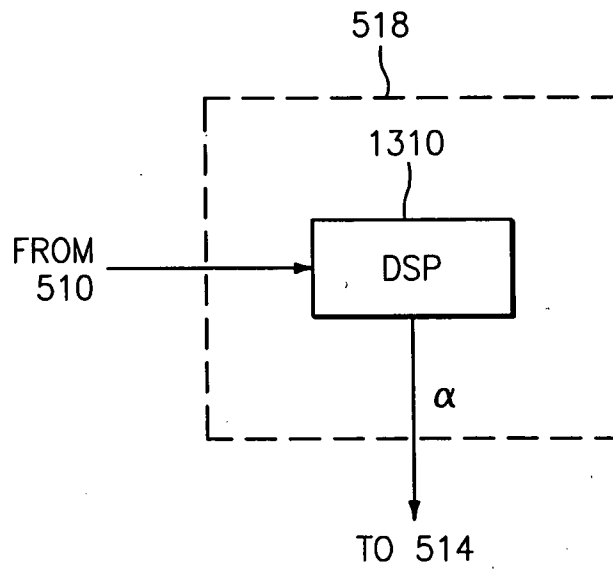
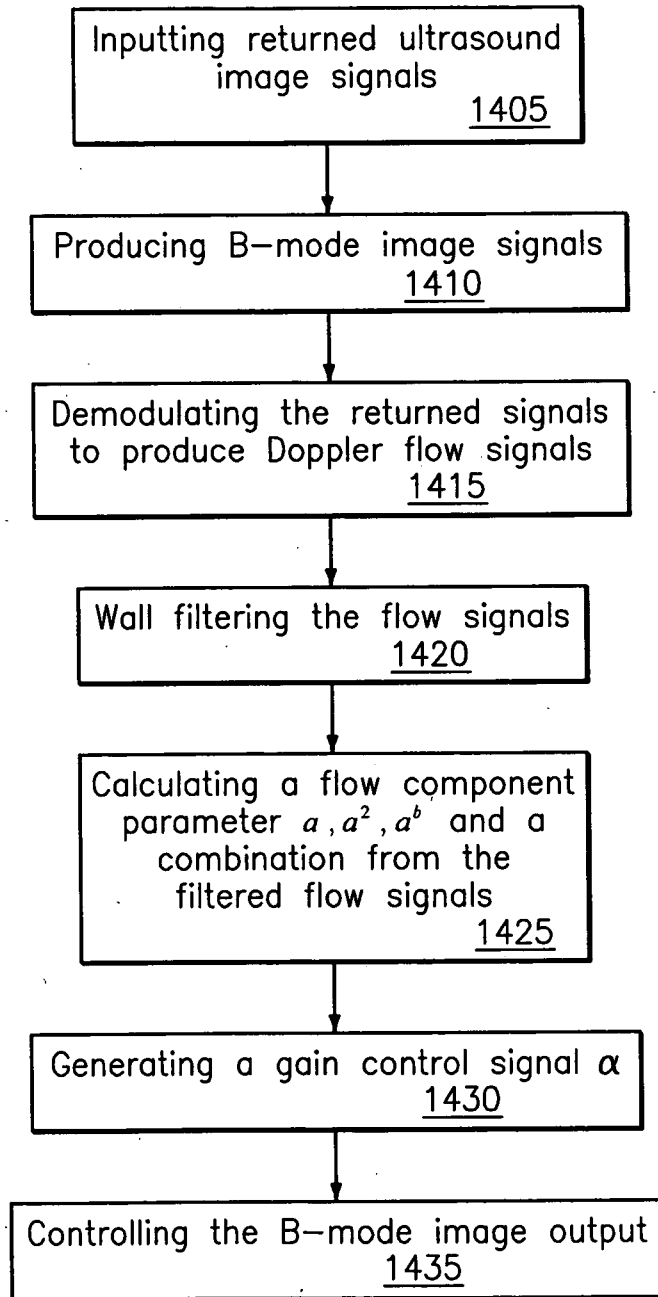
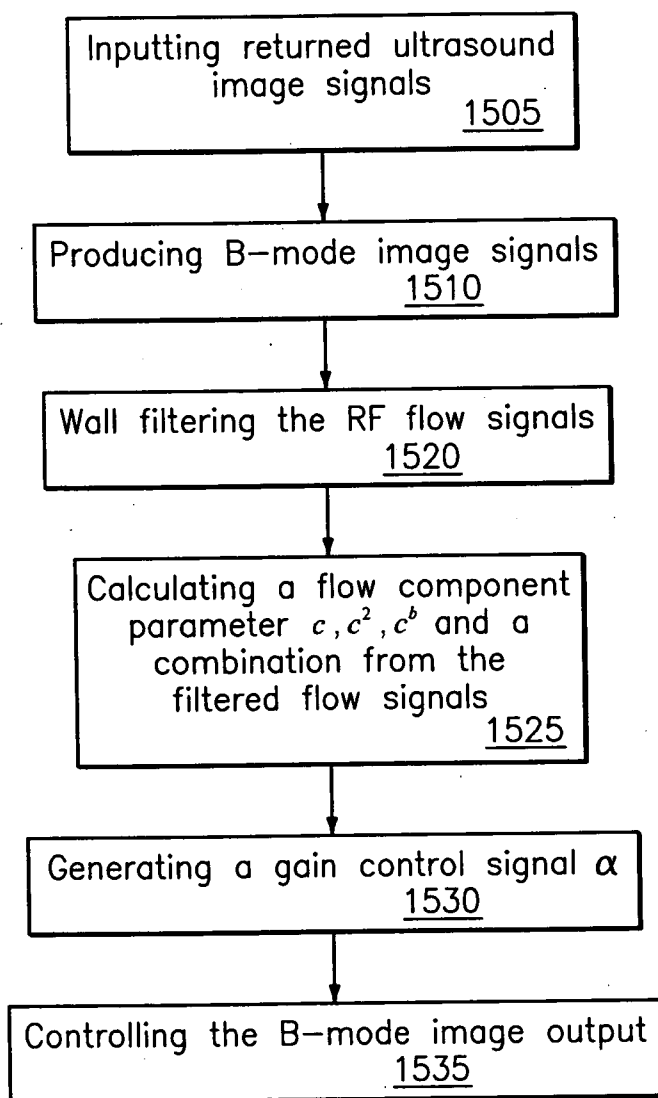


FIG. 13

**FIG. 14**

*FIG. 15*

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2008/056727

A. CLASSIFICATION OF SUBJECT MATTER Int.Cl. A61B8/08 (2006.01) i, A61B8/06 (2006.01) i According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED Minimum documentation searched (classification system followed by classification symbols) Int.Cl. A61B8/08, A61B8/06 Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched Published examined utility model applications of Japan 1922-1996 Published unexamined utility model applications of Japan 1971-2008 Registered utility model specifications of Japan 1996-2008 Published registered utility model applications of Japan 1994-2008 Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	JP 2002-34987 A (GE MEDICAL SYSTEMS GLOBAL TECHNOLOGY COMPANY LLC) Feb. 05, 2002 Paragraph [0016] to [0020]; Figure 4 and 5 (Family: none)	1-4, 13-16 6-10, 12, 18-22, 24
A		5, 11, 17, 23
X	US 2005/0240101 A1 (Makoto Kato) Oct. 27, 2005 Paragraph [0078] and [0080] & JP 3694019 B2 & WO 2004/089222 A1	1, 2, 13, 14
<input checked="" type="checkbox"/> Further documents are listed in the continuation of Box C. <input type="checkbox"/> See patent family annex.		
<p>* Special categories of cited documents:</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier application or patent but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&" document member of the same patent family</p>		
Date of the actual completion of the international search 30.06.2008		Date of mailing of the international search report 08.07.2008
Name and mailing address of the ISA/JP Japan Patent Office 3-4-3, Kasumigaseki, Chiyoda-ku, Tokyo 100-8915, Japan		Authorized officer MIGITAKA Takayuki Telephone No. +81-3-3581-1101 Ext. 3292
		20 9808

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2008/056727

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 6036643 A (Aline Laure Criton) Mar. 14, 2000 Column 3, line 23 to column 4, line 6; Figure 4 & JP 11-342130 A & DE 69934649 T & NO 992323 A	6, 12, 18, 24
Y	US 4853904 A (Patrick R. A. Pesque) Aug. 1, 1989 Column 4, line 23 to column 5, line 15; Figure 1 & JP 63-77437 A & DE 3785409 T & FR 2604081 A	7-10, 12, 19-22, 24
Y	US 6599248 B1 (Tadashi Tamura) Jul. 29, 2003 Column 5, line 14 to 27 (Family: none)	7-10, 12, 19-22, 24

专利名称(译)	用于超声成像的方法和设备		
公开(公告)号	EP2136713A4	公开(公告)日	2012-02-22
申请号	EP2008739834	申请日	2008-03-28
[标]申请(专利权)人(译)	日立阿洛卡医疗株式会社		
申请(专利权)人(译)	ALOKA CO. , LTD.		
当前申请(专利权)人(译)	ALOKA CO. , LTD.		
[标]发明人	TAMURA TADASHI		
发明人	TAMURA, TADASHI		
IPC分类号	A61B8/08 A61B8/06		
CPC分类号	G01S7/52033 A61B8/06 A61B8/13 G01S7/52077 G01S15/8981		
优先权	11/926206 2007-10-29 US 60/920639 2007-03-29 US		
其他公开文献	EP2136713A1		
外部链接	Espacenet		

摘要(译)

血流信息用于减少血管超声B模式图像中的噪声。通过流量检测器获得血流信号。在壁过滤之后，仅保留血管腔中的流动信号功率，同时抑制来自静止组织区域的信号功率。流量信号分量用于计算流量分量参数，该流量分量参数用于生成减小B模式图像中的噪声的增益控制信号 α 。