



(11) **EP 1 527 357 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**15.10.2008 Bulletin 2008/42**

(21) Application number: **03767260.7**

(22) Date of filing: **04.08.2003**

(51) Int Cl.:  
**G01S 11/14 (2006.01)**

(86) International application number:  
**PCT/US2003/024664**

(87) International publication number:  
**WO 2004/013651 (12.02.2004 Gazette 2004/07)**

(54) **SYSTEM FOR ULTRASOUND RANGING IN THE PRESENCE OF ULTRASOUND INTERFERENCE**  
**ULTRASCHALLENTFERNUNGSMESSER IN GEGENWART VON ULTRASCHALL-INTERFERENZ**  
**SYSTEME DE TELEMETRIE PAR ULTRASON EN PRESENCE DE BROUILLAGE D'ULTRASON**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PT RO SE SI SK TR**

(30) Priority: **06.08.2002 US 214441**

(43) Date of publication of application:  
**04.05.2005 Bulletin 2005/18**

(73) Proprietor: **Boston Scientific Limited**  
**St. Michael,**  
**Barbados, West Indies (BB)**

(72) Inventor: **WILLIS, N., Parker**  
**Atherton, CA 94027 (US)**

(74) Representative: **Denemeyer, John James**  
**Denemeyer & Associates S.A.**  
**55, rue des Bruyères**  
**1274 Howald (LU)**

(56) References cited:  
**US-A- 5 321 668 US-A- 5 373 482**  
**US-B1- 6 298 261**

**EP 1 527 357 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description**

## FIELD OF THE INVENTION

5 **[0001]** The invention relates generally to ultrasound ranging, and more particularly to systems for performing ultrasound ranging in the presence of ultrasound interference.

## BACKGROUND OF THE INVENTION

10 **[0002]** Ultrasound ranging is a technique for computing the distance between two ultrasound transducers. The principle of ultrasound ranging is illustrated in FIG. 1, which shows two ultrasound transducers 10,20 separated by a distance. One of the ultrasound transducers is designated as a transmitting transducer 10 and the other is designated as a receiving transducer 20. To measure the distance between the transducers 10,20, the transmitting transducer 10 transmits an ultrasound pulse 25, which is detected by the receiving transducer 20. The distance,  $d$ , between the transducers 10,20  
15 is computed as

$$d = v\tau$$

20 where  $v$  is the velocity of the ultrasound pulse 25 in the medium between the transducers 10,20 and  $\tau$  is the time of flight of the ultrasound pulse 25 in traveling from the transmitting transducer 10 to the receiving transducer 20.

**[0003]** One application of ultrasound ranging is in ultrasound positional tracking to track the position of a device within a three-dimensional (3-D) coordinate system. Referring to FIG. 2, this is accomplished by mounting one or more ranging transducers 110 on the device 115 being tracked and providing four or more reference transducers 120-1 to 120-4 that are spaced apart.

**[0004]** In this particular example, the device 115 being tracked is a catheter tip. The ranging transducer 110 acts as a receiving transducer and each of the reference transducers 120-1 to 120-4 can act both as a receiving and transmitting transducer.

30 **[0005]** To establish the 3-D coordinate system, the reference transducers 120-1 to 120-4 are sequentially excited to transmit ultrasound pulses (not shown). When each reference transducer 120-1 to 120-4 transmits an ultrasound pulse, the other reference transducers 120-1 to 120-4 detect the ultrasound pulse. The relative distances between the reference transducers 120-1 to 120-4 are then computed by performing ultrasound ranging on each of the detected ultrasound pulses. The computed distances are then triangulated to determine the relative positions between the reference transducers 120-1 to 120-4 in 3-D space. The relative positions between the reference transducers 120-1 to 120-4 are then mapped onto the 3-D coordinate system to provide a reference for tracking the position of the ranging transducer 110 in the 3-D coordinate system.

**[0006]** To track the position of the ranging transducer 110, and hence the device 115 carrying the ranging transducer 110, in the 3-D coordinate system, the reference transducers 120-1 to 120-4 are sequentially excited to transmit ultrasound pulses. When each of the reference transducers 120-1 to 120-4 transmits an ultrasound pulse, the ranging transducer 110 detects the ultrasound pulse. The distance  $d_1$ - $d_4$  between the ranging transducer 110 and each of the reference transducers 120-1 to 120-4 is computed by performing ultrasound ranging on each of the detected ultrasound pulses. The computed distances are then triangulated to determine the relative position of the ranging transducer 110 to the reference transducers 120-1 to 120-4 in 3-D space. The position of the ranging transducer 110 in the 3-D coordinate system is then determined based on the relative position of the ranging transducer 110 to the reference transducers 120-1 to 120-4 and the known positions of reference transducers 120-1 to 120-4 in the 3-D coordinate system.

45 **[0007]** An example of a tracking system using ultrasound ranging is the Realtime Position Management™ (RPM) tracking system developed commercially by Cardiac Pathways Corporation, now part of Boston Scientific Corp. The RPM system uses ultrasound ranging to track the positions of medical devices, including reference catheters, mapping catheters and ablation catheters.

**[0008]** Because ultrasound ranging relies on the transmission and detection of ultrasound pulses to measure distance, it is vulnerable to ultrasound interference from ultrasound sources, e.g., an ultrasound imager. For example, ultrasound interference may be detected by the receiving transducer 20 and misinterpreted as an ultrasound pulse from the transmitting transducer 10, producing an erroneous distance measurement.

55 **[0009]** U.S. patent No. 5,373,482 discloses a distance measuring system that generates ultrasound signals and detects echoes of the ultrasound signals to determine a distance of an external object to the measuring system. However, this distance measuring system is not capable of measuring the distance between transducers.

**[0010]** U.S. patent No. 5,321,668 discloses a distance measuring system according to the preamble of claim 1 that

generates acoustic signals from one transducer and receives the acoustic signals at another transducer to measure the distance between the transducers. However, this measuring system is susceptible to ultrasound interference from other sources.

## 5 SUMMARY OF THE INVENTION

10 **[0011]** In accordance with a first aspect of the present inventions, a distance measuring system according to claim 1 is provided. By way of nonlimiting example, the distance measuring system, in informing the distance measurements, comprises a pulse generator coupled to the first transducer for generating and transmitting transmit pulses to the first transducer, a threshold detector coupled to the second transducer for detecting receive pulses from the second detector, and measurement means (e.g., a digital counter) coupled to the pulse generator and the threshold detector. In this case, for each distance measurement, the measurement means triggers the pulse generator to generate and transmit a pulse to the first transducer, measures the elapsed time between transmission of the transmit pulse and detection of a receive pulse by the threshold detector, and generates the distance measurement based on the measured elapsed time.

15 **[0012]** The distance measuring system further comprises a filter coupled to the ultrasound ranging subsystem for filtering ultrasound interference from the plurality of distance measurements (such as, e.g., eight), and outputting a distance based on the filtered distance measurements. The distance measurement system can have various applications, including medical applications, in which case, the first and second transducers can be mounted on a catheter.

20 **[0013]** In the preferred embodiment, the filter filters the ultrasound interference by selecting one of the plurality distance measurements, in which case, the outputted distance is the selected distance measurement. Because the ultrasound interference will typically present itself as the shortest distance measurement, the selected distance measurement is preferably greater than the minimum distance measurement (such as, e.g., the maximum distance measurement), thereby filtering the ultrasound interference out.

25 **[0014]** Although the present inventions should not be so limited in its broadest aspects, the filter sequentially receives the distance measurements, and filters the ultrasound interference from the last N distance measurements. In this case, the filter may filter the last N distance measurements by selecting one of them. So that the system is more responsive to movements of the transducers, the filter can compute a distance variation of the N distance measurements, and compare the distance variation to a threshold value. The filter can then output the distance when the distance variation exceeds the threshold value, while outputting the most recent distance measurement received from the ultrasound ranging subsystem otherwise. In effect, the filtering is only accomplished when there is ultrasound interference, thereby providing more responsiveness to the distance measuring process. The distance variation computation can be accomplished in a variety of ways, including taking the difference between the maximum and minimum of the last N distance measurements, calculating the variance of the last N distance measurements, or calculating the second derivative of the last N distance measurements.

30 **[0015]** In accordance with a second aspect of the present inventions, a method for measuring the distance between two transducers comprises performing a plurality of distance measurements (e.g., eight) between the transducers. For example, the distance measurement can comprise exciting one of the transducers to transmit an ultrasound pulse, and measuring the time for the ultrasound pulse to reach the other transducer.

35 **[0016]** The method further comprises filtering ultrasound interference from the plurality of distance measurements, and outputting a distance based on the filtered distance measurements. The distance measurements can be filtered by, e.g., selecting one of the plurality distance measurements, in which case, the outputted distance will be the selected distance measurement. The selected distance measurement is preferably more than the minimum distance measurement, such as, e.g., the maximum distance measurement.

40 **[0017]** Although the present inventions should not be some limited in its broadest aspects, the distance measurements are sequentially received, and the ultrasound interference is filtered from the last N distance measurements. In this case, the last N distance measurements can be filtered by selecting one of them. So that the method is more responsive to movements of the transducers, a distance variation of the N distance measurements can be computed and compared to a threshold value. The distance can then be outputted when the distance variation exceeds the threshold value, while the most recent distance measurement received from the ultrasound ranging subsystem can be outputted otherwise, thereby providing for a more responsive method. The distance variation computation can be accomplished in a variety of ways, including taking the difference between the maximum and minimum of the last N distance measurements, calculating the variance of the last N distance measurements, or calculating the second derivative of the last N distance measurements.

## 55 BRIEF DESCRIPTION OF THE DRAWINGS

**[0018]** The drawings illustrate the design and utility of preferred embodiments of the invention, in which similar elements are referred to by common reference numerals, in which:

FIG. 1 is a diagram illustrating the principle of ultrasound ranging between two transducers.

FIG. 2 is a diagram illustrating ultrasound positional tracking using ultrasound ranging.

FIG. 3 is a functional diagram of an ultrasound ranging system.

FIG. 4 is a timeline of a transmit pulse and a received pulse used to measure the time of flight of an ultrasound pulse.

5 FIG. 5 is a diagram of the ultrasound ranging system of FIG. 3 in an environment containing a source of ultrasound interference.

FIG. 6 is a timeline depicting the arrival of ultrasound interference between the transmit pulse and the receive pulse.

FIG. 7 is a functional diagram of the ultrasound ranging system further comprising a distance filter according to one embodiment of the invention.

10 FIG. 8 is a flowchart illustrating the operation of a distance filter according to another embodiment of the invention.

FIG. 9 is a functional block diagram of an ultrasound ranging system comprising multiple transmitting transducers according to another embodiment of the invention.

FIG. 10 is a functional block diagram of an ultrasound positional tracking system according to still another embodiment of the invention.

15 FIG. 11 illustrates examples of a medical catheter and a reference catheter that can be used with the system of FIG. 10.

FIG. 12 illustrates an exemplary display image of the system of FIG. 10.

FIG. 13 is a graph illustrating the probability of a distance error with and without the filter of the invention as a function of distance between two transducers.

20 DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

**[0019]** FIG. 3 is a block diagram of an ultrasound ranging system 310 for measuring the distance between transducers 10,20. The ranging system 310 generally includes a pulse generator 320 coupled to the transmitting transducer 10, a threshold detector coupled 330 to the receiving transducer 20, and distance circuitry 340 coupled to the threshold detector 330. The pulse generator 320 may generate voltage pulses having a frequency of, e.g., 600 KHz. The threshold detector 330 detects signals from the receiving transducer 20 that are above a threshold level, e.g., a voltage level. The ranging system 310 further includes control and timing circuitry 350 coupled to the pulse generator 320, and a distance counter 360 coupled to the control and timing circuitry 350 and the distance circuitry 340. The distance counter 360 may be a digital counter driven by a clock. For ease of discussion, only one transmitting transducer 10 is shown. The more typical case of multiple transmitting transducers will be discussed later.

**[0020]** To measure the distance between the transducers 10,20, the control and timing circuitry 350 triggers the pulse generator 320 to generate and transmit a transmit pulse to the transmitting transducer 10. The transmitting transducer 10 converts the transmit pulse into an ultrasound pulse and transmits the ultrasound pulse 25. The control and timing circuitry 350 also triggers the distance counter 360 to begin counting from zero at the transmit time of the transmit pulse. The running count value of the distance counter 360 provides a measure of time from the transmission of the transmit pulse.

**[0021]** After the ultrasound pulse 25 has been transmitted, the receiving transducer 20 receives the ultrasound pulse and converts the ultrasound pulse into a receive pulse, which is detected by the threshold detector 330. Upon detection of the receive pulse, the distance circuitry 340 reads the current count value from the distance counter 360. The read count value indicates the elapsed time between the transmission of the transmit pulse and the detection of the receive pulse, which corresponds to the time of flight,  $\tau$ , of the ultrasound pulse 25 between the transducers 10,20. This is illustrated in FIG. 4, which shows a timeline of the transmit pulse and the receive pulse. The read count value also provides a distance measurement between the transducers 10,20. This is because the distance,  $d$ , between the transducers 10,20 is proportional to the time of flight,  $\tau$ , of the ultrasound pulse 25, by

$$d = v\tau$$

where  $v$  is the velocity of the ultrasound pulse 25. The distance circuitry 340 outputs the read count value as a distance measurement between the transducers 10,20.

**[0022]** In one embodiment, the distance circuitry 340 listens for the receive pulse within a time window, e.g., 100  $\mu$ .sec, after the transmit pulse has been transmitted. The time window may begin immediately or shortly after the transmit pulse has been transmitted. In determining the time of detection of the receive pulse, the distance circuitry 340 interprets the first signal that the threshold detector 330 detects within the time window as the receive pulse.

**[0023]** The operation of the ultrasound ranging system 310 in an environment containing ultrasound interference will now be described with reference to FIG. 5, in which a source 510 of ultrasound interference 525 is introduced. The source of ultrasound interference may be, e.g., an ultrasound imaging transducer. In the following discussion, it will be assumed that the ultrasound interference 525 is large enough in amplitude to be detected by the threshold detector 330.

**[0024]** When the ultrasound interference reaches the receiving transducer 20 before transmission of the transmit pulse, the distance circuitry 340 ignores the ultrasound interference. This is because the distance circuitry 340 does not listen for the receive pulse until after the transmit pulse has been transmitted.

**[0025]** FIG. 6 is a timeline illustrating the case in which the ultrasound interference reaches the receiving transducer 20 between the transmit pulse and the receive pulse. When this occurs, the threshold detector 330 detects the ultrasound interference first. As a result, the distance circuitry 340 misinterprets the detected ultrasound interference as the receive pulse. This causes the distance measurement 350 unit to prematurely read the count value from the distance counter 360. In this case, the read count value indicates the time between the transmit pulse and the detection of the ultrasound interference. As a result, the read count value corresponds to an erroneous time of flight,  $\tau_{err}$ , that is shorter than the actually time of flight,  $\tau$ , of the ultrasound pulse, as illustrated in FIG. 6. This in turn causes the distance circuitry 340 to output a distance measurement that is shorter than the actual distance between the transducers 10,20.

**[0026]** When the ultrasound interference reaches the receiving transducer 20 after the receive pulse, the distance measurement circuitry 340 ignores the ultrasound interference. This is because the threshold detector 330 detects the receive pulse first. As a result, the distance circuitry 340 correctly reads the count value at the detection of the receive pulse.

**[0027]** Of the three cases discussed above, the only case in which the ranging system 310 is affected by the ultrasound interference is when the ultrasound interference reaches the receiving transducer 20 between the transmit pulse and the receive pulse. In this case, the distance circuitry 340 outputs a distance measurement that is shorter than the actual distance between the transducers 10,20. Thus, ultrasound interference causes the ranging system 310 to measure distances that are too short. The invention exploits this property to filter out erroneous distance measurements caused by ultrasound interference, as explained further below.

**[0028]** FIG. 7 illustrates an embodiment of a system 710 for measuring the distance between transducers 10,20 further including a distance filter 715 coupled to the distance circuitry 340. In the preferred embodiment, the distance filter 715 is implemented in software, but can be implemented in firmware or hardware as well. In this embodiment, the control and timing circuitry 350 may continuously initiate distance measurements between the transducers 10,20 at regular intervals (e.g., once every 13 ms for a RPM system). Each time the control and timing circuitry 340 initiates a distance measurement, the distance circuitry 340 outputs a distance measurement to the distance filter 715. The filter 715 takes the last N distance measurements outputted by the distance circuitry 340, and outputs the maximum of the N distance measurements, where N is a positive integer (e.g., N = 8).

**[0029]** The operation of the distance filter 715 can be represented as

$$y(n) = \max[x(n), x(n-1), \dots, x(n-N)]$$

where  $y(n)$  is the most recent output of the distance filter,  $x(n)$  is the most recent distance measurement from the distance circuitry 340, and  $\max[ ]$  is a function that takes the maximum of the last N distance measurements from the distance circuitry 340 starting with the most recent distance measurement  $x(n)$ .

**[0030]** The distance filter 715 filters out erroneous distance measurements caused by ultrasound interference. This is because ultrasound interference causes the distance circuitry 340 to output distance measurements that are shorter than the actual distance between the transducers 10,20. As a result, correct distance measurements outputted by the distance circuitry 340 will be larger than erroneous distance measurements caused by ultrasound interference. Therefore, when at least one of the last N distance measurements is correct, the maximum distance measurement outputted by the distance filter 715 will be one of the correct distance measurements. The distance filter 715 only outputs a distance error when every one of the last N distance measurements from the distance circuitry 340 is in error.

**[0031]** The distance filter 715 of the invention can significantly reduce distance errors due to ultrasound interference. This can be demonstrated by assuming that the probability of a distance error from the distance circuitry 340 due to ultrasound interference is P. In this case, the probability that every one of the last N distance measurements is in error is P to the Nth power. Since the distance filter 715 outputs a distance error only when every one of the last N distance measurements is in error, the probability of a distance error from the distance filter 715 is P to the Nth power, which can be significantly smaller than P. For example, if P equals 77% and N = 8, the probability of a distance error from the distance circuitry 340 due to ultrasound interference is 77%, while the probability of a distance error from the distance filter due to ultrasound interference is 12.3%. Obviously increasing N can further reduce the probability of a distance error from the distance filter 715 due to ultrasound interference. However, increasing N may increase another type of distance error, as explained further below.

**[0032]** For the case in which the control and timing circuitry 350 initiates distance measurements at regular intervals (e.g., once every 13 milliseconds), the distance filter 715 outputs the maximum distance measurement over a finite measurement time window, M, of

$$M=N\Delta t$$

5 where  $\Delta t$  is the time between adjacent distance measurements and N is the number of distance measurements considered. For example, when  $\Delta t = 13$  ms and  $N = 8$ , the measurement time window is 104 ms. In order for the distance filter 715 to provide a good approximation of the current distance between the transducers 10,20, the distance between the transducers 10,20 should remain relatively stable within the measurement window. This ensures that the maximum distance measurement within the measurement window provides a good approximation of the current distance between the transducers 10,20. When the distance between the transducers 10,20 varies within measurement window, the maximum distance may no longer closely approximate the current distance between the transducers 10,20. For example, when the distance between the transducers 10,20 decreases within the measurement window, the maximum distance will tend to be larger than the current distance between the transducers 10,20.

10 [0033] Therefore, there is tradeoff in increasing N. Increasing N decreases distance error due to ultrasound interference, but also increases distance error due to distance variation within the measurement window by increasing the size of the measurement window.

15 [0034] One way to reduce error caused by distance variation within the measurement window is to shorten the measurement window. This may be accomplished without decreasing N, e.g., by increasing the transmit rate of the system 710 in order to provide more distance measurements within a shorter period of time. This way, distance error due to distance variation can be reduced without increasing distance error due to ultrasound interference.

20 [0035] In another embodiment, the distance filter 715 computes a distance variation within the measurement window, and compares the computed distance variation to a threshold value. The distance filter 715 outputs the maximum distance measurement only when the distance variation within the measurement window exceeds the threshold value. Otherwise, the filter 715 outputs the most recent distance measurement from the distance circuitry 340.

25 [0036] The threshold value may be determined by the maximum that the distance between the transducers 10,20 can change within the measurement window due to movement between the transducers 10,20. For example, when the receiving transducer 20 is mounted on a catheter (not shown), the maximum change in distance may be determined by the maximum distance that a physician navigates the catheter within the measurement window. The threshold value may be represented as

30

$$\text{threshold} = N\delta$$

35 where  $\delta$  represents the maximum change in distance between adjacent distance measurements and N is the number of distance measurements considered.

[0037] The operation of the distance filter 715 according to this embodiment will now be described with reference to FIG. 8. In step 810, the distance filter 715 computes a distance variation for the last N distance measurements from the distance circuitry 340. The distance variation may be computed as the difference between the maximum and minimum of the last N distance measurements. This is represented as

40

$$\text{range}(n) = \max[x(n), x(n-1), \dots, x(n-N)] - \min[x(n), x(n-1), \dots, x(n-N)]$$

45

where  $\text{range}(n)$  is the distance variation for the last N distance measurements, and  $x(n)$  is the most recent distance measurement from the distance circuitry 340. Other measures of distance variation may be used, such as computing the variance of the last N distance measurements. As another example, the second derivative of the last N distance measurements, which can be used to differentiate between rapid catheter movement and random interference can be taken. This is because rapid catheter movement, in the absence of interference, produces a distance measurement with a small second derivative, whereas random interference produces a distance measurement with a relatively large second derivative.

50 [0038] In step 820, the distance filter 715 compares the distance variation to the threshold value. If the distance variation is above the threshold value, the distance filter 715, at step 830, outputs the maximum of the last N distance measurements from the distance circuitry 340. Otherwise, at step 840, the distance filter 715 outputs the most recent distance measurement from the distance circuitry 340. The distance filter 715 repeats the steps in FIG. 8 for each subsequent distance measurement it receives from the distance circuitry 340.

55 [0039] Therefore, the distance filter 715 according to this embodiment reduces the unwanted side effects of increasing

N by only outputting the maximum distance measurement when the computed distance variation exceeds the threshold value. In other words, the distance filter 715 only applies its maximum filtering function when the distance variation is most likely due to ultrasound interference, and not due to movement between the transducers 10,20.

**[0040]** In the discussion above, the systems had one transmitting transducer. Many applications, such as ultrasound positional tracking, require multiple transmitting transducers. FIG. 9 illustrates an embodiment of the system 905, further including multiple transmitting transducers 10-1 to 10-n, where each of the transmitting transducers is coupled to a pulse generator 920-1 to 920-n. In this embodiment, the control and timing circuitry 950 sequentially initiates distance measurements between the receiving transducer 20 and each of the transmitting transducers 10-1 to 10-n.

**[0041]** In operation, the control and timing circuitry 950 sequentially triggers each one of the pulse generators 920-1 to 920-n to generate and transmit a transmit pulse to its respective transmitting transducer 10-1 to 10-n causing the transmitting transducer 10-1 to 10-n to transmit an ultrasound pulse (not shown). The transmit pulses may be spaced apart in time, e.g., 1ms, so they do not interfere within one another.

**[0042]** For each transmit pulse, the control and timing circuitry 950 triggers the distance counter 360 to begin counting from zero at the transmit time of the transmit pulse. The control and timing circuitry 950 may also send data to the distance circuitry 340 identifying the corresponding transmitting transducer 10-1 to 10-n. After the transmit pulse has been transmitted, the distance circuitry 340 listens for a receive pulse within a time window, e.g., 100  $\mu$ s. Upon detection of the receive pulse by the threshold detector 330, the distance circuitry 340 reads the current count value from the distance counter 360, which provides a distance measurement between the receiving transducer 20 and the corresponding transmitting transducer 10-1 to 10-n. The distance circuitry outputs the distance measurement to the distance filter 915. The distance circuitry 340 may also output data identifying the transmitting transducer 10-1 to 10-n corresponding to the distance measurement.

**[0043]** The distance filter 915 sequentially receives distance measurements corresponding to the distance between the ranging transducer 20 and each of the transmitting transducers 10-1 to 10-n from the distance circuitry 340. For each received distance measurement, the filter 915 identifies the corresponding transmitting transducer 10-1 to 10-n.

This may be accomplished several ways. For example, for each distance measurement, the control and timing circuitry 950 and/or the distance circuitry 340 may send data to the filter 915 identifying the corresponding transmitting transducer 10-1 to 10-n. Alternatively, the filter 915 may determine the identity of the corresponding transmitting transducer 10-1 to 10-2 according to the order in which it receives a sequence of distance measurements from the distance circuitry 340. For example, the filter 915 may assume that the first distance measurement in the sequence corresponds to transmitting transducer 10-1, the second distance measurement corresponds to transmitting transducer 10-2, and so forth.

**[0044]** In one embodiment, the distance filter 915 outputs a maximum distance for each of the transmitting transducers 10-1 to 10-n. In determining the maximum distance for each transmitting transducer 10-1 to 10-n, the filter 915 takes the maximum of the last N distance measurements for that particular transmitting transducer 10-1 to 10-n from the distance circuitry 340.

**[0045]** In another embodiment, the 915 filter also computes a distance variation for each transmitting transducer 10-1 to 10-n by computing a variation in the last N distance measurements for that particular transmitting transducer 10-1 to 10-n. The filter 915 may then compare the distance variation for each transmitting transducer 10-1 to 10-n to a threshold value. If the distance variation for a particular transmitting transducer 10-1 to 10-n is below the threshold value, then the filter 915 outputs the most recent distance measurement for that transmitting transducer 10-1 to 10-n. If the distance variation for a particular transmitting transducer 10-1 to 10-n is above the threshold value, then the filter 915 outputs the maximum of the last N distance measurements for that transmitting transducer 10-1 to 10-n.

**[0046]** Preferably, each time the filter 915 outputs a filtered distance measurement it includes data identifying the corresponding transmitting transducer 10-1 to 10-n. If implemented in software, the filter 915 is preferably embodied in several software modules--one for each transmitting transducer.

**[0047]** The invention is particularly well suited for use in ultrasound positional tracking systems to track the position of one or more devices (e.g., catheter). FIG. 10 illustrates an ultrasound positional tracking system 1005 according to an embodiment of the invention. The system 1005 includes two or more ranging transducers 1020-1 to 1020-m mounted on the medical device being tracked (not shown), and four or more reference transducers 1010-1 to 1010-n. Each of the ranging transducers 1020-1 to 1020-m acts as a receiving transducer and each of the reference transducers 1010-1 and 1010-n can act both as a receiving and transmitting transducer.

**[0048]** FIG. 11 illustrates exemplary devices on which the ranging transducers 1020-1 to 1020-m and the reference transducers 1010-1 to 1010-n can be mounted. Three ranging transducers 1020-1 to 1020-3 are mounted on a distal portion of a catheter 1110 for performing medical and/or mapping procedures within the body. The catheter 1110 may be a mapping catheter, an ablation catheter, or the like. In this example, the ranging transducers 1020-1 to 1020-m take the form of annular ultrasound transducers. Also illustrated in FIG. 11 are four reference transducers 1010-1 to 1010-4 mounted on a distal portion of a reference catheter 1120.

**[0049]** Referring back to FIG. 10, the system 1005 also includes a distance measurement subsystem 1015-1 to 1015-(n+m) coupled to each of the ranging transducers 1020-1 to 1020-m and reference transducers 1010-1 to 1010-

n, and a pulse generator 1025-1 to 1025-n coupled to each of the reference transducers 1010-1 to 1010-n. Each distance subsystem 1015-1 to 1015-(n+m) includes a threshold detector 1030-1 to 1030-(n+m), distance circuitry 1035-1 to 1035-(n+m) and a distance filter 1040-1 to 1040-(n+m) according to the invention for filtering out distance errors from the respective distance circuitry 1035-1 to 1035-(n+m). Notably, if implemented in software, the number of software modules for the distance filter 1040 will equal the product of the number of ranging transducers 1020 and the number of reference transducers 1010, i.e.,  $m \times n$  filter modules. The system 1005 further includes control and timing circuitry 1050 coupled to each of the pulse generators 1025-1 to 1025-n and a distance counter 1060 coupled to control and timing circuitry 1050 and each of the distance measurement subsystems 1015-1 to 1015-(n+m). The system 1005 also includes a triangulation circuitry 1070 for triangulating the positions of the ranging transducers 1020-1 to 1020-m and the reference transducers 1010-1 to 1010-n, a display image processor 1075 coupled to the triangulation circuitry, and a display 1080 coupled to the display image processor 1075. In the preferred embodiment, the triangulation circuitry 1070 is implemented in software, but can be implemented in firmware or hardware as well.

**[0050]** In operation, the control and timing circuitry 1050 sequentially triggers each one of the pulse generators 1025-1 to 1025-n to generate and transmit a transmit pulse to its respective reference transducer 1010-1 and 1010-n causing the reference transducer 1010-1 and 1010-n to transmit an ultrasound pulse. The transmit pulses may be spaced apart in time, e.g., 1 ms, so they do not interfere within one another.

**[0051]** For each transmit pulse, the control and timing circuitry 1050 triggers the distance counter 1060 to begin counting from zero at the transmit time of the transmit pulse. After the transmit pulse has been transmitted, each distance measurement subsystem 1015-1 to 1015-n listens for a receive pulse at its respective transducer 1020-1 to 1020-m and 1010-1 to 1010-n. Upon detection of a receive pulse by its respective threshold detector 1030-1 to 1030-(n+m), each distance circuitry 1035-1 to 1035-(n+m) reads the current count value from the distance counter, and outputs the read count value as a distance measurement to the respective distance filter 1040-1 to 1040-(n+m). Each distance filter 1040-1 to 1040-(n+m) filters out erroneous distance measurements from its respective distance circuitry 1035-1 to 1035-(n+m) due to ultrasound interference, and outputs the filtered distance measurements to the triangulation circuitry 1070. Each distance filter 1040-1 to 1040-(n+m), preferably, includes data identifying the corresponding receiving and transmitting transducer for each filtered distance measurement.

**[0052]** For each transmit pulse, the triangulation circuitry 1070 receives distance measurements between the reference transducer 1010-1 to 1010-n corresponding to the transmit pulse and each of the other reference transducers 1010-1 to 1010-n. The triangulation circuitry 1070 also receives distance measurements between the reference transducer 1010-1 to 1010-n corresponding to the transmit pulse and each of the ranging transducers 1020-1 to 1020-m.

**[0053]** The triangulation circuitry 1070 computes the relative positions between the reference transducers 1010-1 to 1010-n in 3-D space by triangulating the distance measurements between the reference transducers 1010-1 to 1010-n. The triangulation circuitry 1070 then maps the relative positions between the reference transducers 1010-1 to 1010-n onto the 3-D coordinate system to provide a reference for tracking the positions of the ranging transducers 1020-1 to 1020-m in the 3-D coordinate system. The triangulation circuitry 1070 may employ any one of a number of mapping procedures as long as the mapping procedure preserves the relative positions between the reference transducers 1010-1 to 1010-n.

**[0054]** To track the positions of the ranging transducers 1020-1 to 1020-m within the 3-D coordinate system, the triangulation circuitry 1070 triangulates the relative positions of the ranging transducers 1020-1 to 1020-m to the reference transducers 1010-1 to 1010-n by triangulating the distance measurements between the ranging transducers 1020-1 to 1020-m and the reference transducers 1010-1 to 1010-n. The triangulation circuitry 1070 then determines the positions of the ranging transducers 1020-1 to 1020-m in the 3-D coordinate system based on the relative positions of the ranging transducers 1020-1 to 1020-m to the reference transducers 1010-1 to 1010-n and the known positions of reference transducers 1010-1 to 1010-n in the 3-D coordinate system.

**[0055]** Those skilled in the art will appreciate that the filters 1040-1 to 1040-(n+m) may be integrated in the triangulation circuitry 1070. This may be done, e.g., by modifying software in the triangulation circuitry 1070 to perform the filtering functions according to the invention. In this case, the distance measurements from each distance circuitry 1040-1 to 1040-(n+m) may be outputted directly to the triangulation circuitry 1070, which performs the filtering functions according to the invention before triangulating the positions of the transducers.

**[0056]** The triangulation circuitry 1070 outputs the positions of the ranging transducers 1020-1 to 1020-m and the reference transducers 1010-1 to 1010-n in the 3-D coordinate system to the display image processor 1075. The display image processor 1075 generates an image showing the position and orientation of the device being tracked in graphical form. The display image processor 1075 may do this by plotting the positions of the ranging transducers 1020-1 to 1020-m in the 3-D coordinate system and reconstructing a graphical representation of the device onto the plotted positions based on a pre-programmed graphical model of the device. The graphical model may include information on the relative positions of the ranging transducers on the device. The image may also show the position and orientation of the reference catheter 1120 (shown in FIG. 11) in graphical form. The display image processor 1075 may do this by plotting the positions of the reference transducers 1010-1 to 1010-n in the 3-D coordinate system and reconstructing a graphical

representation of the reference catheter 1120 onto the plotted positions. The display image processor 1075 outputs the image to the display 1080, which displays the image to a physician.

[0057] Fig. 12 shows an exemplary image 1210 in which the device being tracked is a medical catheter 1110 (shown in FIG. 11). The image 1210 includes graphical reconstructions of the medical catheter 1110 and the reference catheter 1120. The graphical reconstruction of the medical catheter 1110 is positioned and orientated in the image 1210 based on the tracked positions of the ranging transducers 1020-1 to 1020-3 in the 3-D coordinate system. Similarly, the graphical reconstruction of the reference catheter 1120 is positioned and orientated in the image 1210 based on the tracked positions of the reference transducers 1010-1 to 1010-4 in the 3-D coordinate system. The 3-D coordinate 1215 system may or may not be shown in the image 1210.

[0058] Even though one device was tracked in the above example, the ultrasound positional system 1005 may be used to track multiple devices equipped with ranging transducers. In addition, the display 1080 may display the position of anatomical landmarks in the 3-D coordinate system. This may be done, e.g., by positioning a mapping catheter equipped with ranging transducers at an anatomical landmark and recording the position of the anatomical landmark in the 3-D coordinate system based on the position of the mapping catheter. The position of the anatomical landmark in the 3-D coordinate system may then be displayed and labeled on the display 1080. This enables a physician to more precisely guide devices within the body by referencing their tracked position on the display 1080 to the position of the anatomical landmark on the display 1080.

[0059] The display 1080 may also display a computer representation of body tissue in the 3-D coordinate system. This may be done, e.g., by moving a mapping catheter equipped with ranging transducers to different positions on the surface of the body tissue and recording these positions in the 3-D coordinate system. The image display processor 1075 may then reconstruct the computer representation of the body tissue in the 3-D coordinate system, e.g., by fitting an anatomical shell onto the recorded positions. The computer representation of the body tissue may then be displayed on the display 1080. This enables a physician to more precisely guide devices within the body by referencing their tracked position on the display 1080 to the computer representation of the body tissue on the display 1080. Additional details on this graphical reconstruction technique can be found in patent application serial number 09/128,304 to Willis et al., entitled, "A dynamically alterable three-dimensional graphical model of a body region."

[0060] An advantage of the ultrasound tracking system 1005 according to the invention is that the distance filters 1040-1 to 1040-(n+m) enable the tracking system 1005 to more reliably operate in an environment containing ultrasound interference. This is accomplished by filtering out distance errors due to ultrasound interference, thereby improving the accuracy of the distance measurements used to triangulate the positions of the ranging transducers 1020-1 to 1020-n and the reference transducers 1010-1 to 1010-n.

[0061] The invention is especially useful for using ultrasound tracking systems concurrently with ultrasound imaging. One advantage of using an ultrasound tracking system concurrently with ultrasound imaging is that it allows a physician to track the position of a device within a portion of the body while at the same time imaging the portion of the body using an ultrasound imager to provide additional information. Another advantage is that it allows the use of an ultrasound tracking system to track the position of a device having an ultrasound imager, e.g., an ultrasound imaging catheter.

[0062] The usefulness of the invention in using an ultrasound ranging system concurrently with ultrasound imaging will now be examined.

[0063] An ultrasound imager typically images the body by transmitting ultrasound pulses in the body and detecting the resulting echo pulses. The rate of transmission of the ultrasound pulses is constrained by two factors.

1. The distance that is to be imaged. This is because there must be enough time for the ultrasound energy to travel out to and back from the object being imaged.
2. Scattering interference. This is because the scattered energy from one ultrasound pulse must die out before the next ultrasound pulse can be transmitted.

[0064] The more rapidly the imaging transducer is pulsing, the higher the probability it will cause interference at an ultrasound tracking system. The probability of ultrasound interference occurring between two transducers of an ultrasound ranging system is

$$P = (d/v)/T$$

where d is distance between the transducers, v is the velocity of ultrasound between the transducers, and T is the time between ultrasound pulses from the interfering ultrasound imager.

[0065] In one example, an Intracardiac Echocardiography ("ICE") catheter contains an ultrasound imager that transmits at a rate of 7680 Hz, which corresponds to a time, T, of 130µs between ultrasound pulses from the imager. FIG. 13 is

a graph showing the probability of this particular ultrasound imager causing interference between two transducers of an ultrasound ranging system as a function of distance between the transducers. Without the distance filter of the invention, the probability of a distance measurement error is  $P \approx (d/v)/T$ , as given by the above equation. This is shown for  $v = 1.5 \text{ mm}/\mu\text{sec}$  and  $T = 130 \mu\text{s}$  by the curve labeled "unfiltered" in FIG. 13. The value  $v = 1.5 \text{ mm}/\mu\text{sec}$  is an approximation of the velocity of ultrasound in the body. With the distance filter of the invention, the probability of a distance measurement error is significantly reduced to  $P$  to the  $N$ th power. This is shown for  $N = 8$  by the curve labeled "filtered" in FIG. 13.

**[0066]** Those skilled in the art will appreciate that various modifications may be made to the just described preferred embodiments without departing from the scope of the invention, as defined by the claims. For example, the distance filters of the invention are not limited for use with the particular ultrasound ranging systems described in the specification, and may be used with other ultrasound ranging systems susceptible to ultrasound interference.

## Claims

1. A distance measuring system (710, 905), comprising first and second transducers (10, 20); an ultrasound ranging subsystem (310, 910) coupled to the first and second transducers (10, 20) for performing a plurality of distance measurements between the first and second transducers (10, 20), the system **characterized in that** it further comprises:

a filter (715, 915) coupled to the ultrasound ranging subsystem (310, 910) for filtering ultrasound interference from the plurality of distance measurements by selecting one of the plurality of distance measurements, and outputting the selected distance measurement.

2. The system (710, 905) of claim 1, wherein the selected distance measurement is greater than the minimum distance measurement.

3. The system (710, 905) of claim 1, wherein the selected distance measurement is the maximum distance measurement.

4. The system (710, 905) of claim 1, wherein one of the first and second transducers is mounted on a catheter.

5. The system (710, 905) of claim 1, wherein the number of distance measurements is 8.

6. The system (710, 905) of claim 1, wherein the ultrasound ranging subsystem (310, 910) further comprises:

a pulse generator (320) coupled to the first transducer (10) for generating and transmitting transmit pulses to the first transducer (10);

a threshold detector (330) coupled to the second transducer (20) for detecting receive pulses from the second transducer (20); and

measurement means (340, 350, 360) coupled to the pulse generator (320) and the threshold detector (330);

wherein, for each distance measurement, the measurement means (340, 350, 360) triggers the pulse generator (320) to generate and transmit a transmit pulse to the first transducer (10), measures the elapsed time between transmission of the transmit pulse and detection of a receive pulse by the threshold detector (330), and generates the distance measurement based on the measured elapsed time.

7. The system (710, 905) of claim 6, wherein the measurement means comprises a digital counter for measuring the elapsed time.

8. The system (710, 905) of claim 1, wherein the ultrasound ranging subsystem (310, 910) is coupled to the first and second transducers (10, 20) for sequentially performing distance measurements between the first and second transducers (10, 20); and the filter (715, 915) is coupled to the ultrasound ranging subsystem (310, 910) for sequentially receiving the distance measurements, filtering ultrasound interference from the last  $N$  distance measurements by selecting one of the last  $N$  distance measurements, and outputting the selected distance measurement.

9. The system (710, 905) of claim 8, wherein the selected distance measurement is greater than the minimum distance measurement.

10. The system (710, 905) of claim 8, wherein the selected distance measurement is the maximum distance measurement.

11. The system (710, 905) of claim 8, wherein N is 8.

12. The system (710, 905) of claim 8, wherein the filter (715, 915) computes a distance variation of the N distance measurements, compares the distance variation to a threshold value, outputs the selected distance measurement when the distance variation exceeds the threshold value, and outputs the most recent distance measurement received from the ultrasound ranging subsystem (310, 910) otherwise.

13. The system (710, 905) of claim 12, wherein the distance variation is the difference between the maximum and minimum of the last N distance measurements received from the ultrasound ranging subsystem (310, 910).

14. The system (710, 905) of claim 12, wherein the distance variation is the variance of the last N distance measurements received from the ultrasound ranging subsystem (310, 910).

15. The system (710, 905) of claim 12, wherein the distance variation is the second derivative of the last N distance measurements received from the ultrasound ranging subsystem (910, 910).

### Patentansprüche

1. Entfernungsmesssystem (710, 905), welches aufweist:

einen ersten und einen zweiten Wandler (10, 20); ein Ultraschall-Entfernungsmess-Subsystem (310, 910), das mit dem ersten und dem zweiten Wandler (10, 20) gekoppelt ist, um mehrere Entfernungsmessungen zwischen dem ersten und dem zweiten Wandler (10, 20) durchzuführen, welches System **dadurch gekennzeichnet ist, dass** es weiterhin aufweist:

ein Filter (715, 915), das mit dem Ultraschall-Entfernungsmess-Subsystem (310, 910) gekoppelt ist, zum Filtern von Ultraschall-Interferenzstörungen aus den mehreren Entfernungsmessungen durch Auswählen einer der mehreren Entfernungsmessungen und Ausgeben der ausgewählten Entfernungsmessung.

2. System (710, 905) nach Anspruch 1, bei dem die ausgewählte Entfernungsmessung größer als die minimale Entfernungsmessung ist.

3. System (710, 905) nach Anspruch 1, bei dem die ausgewählte Entfernungsmessung die maximale Entfernungsmessung ist.

4. System (710, 905) nach Anspruch 1, bei dem der erste oder der zweite Wandler an einem Katheter befestigt ist.

5. System (710, 905) nach Anspruch 1, bei dem die Anzahl von Entfernungsmessungen gleich 8 ist.

6. System (710, 905) nach Anspruch 1, bei dem das Ultraschall-Entfernungsmess-Subsystem (310, 910) weiterhin aufweist:

einen Impulsgenerator (320), der mit dem ersten Wandler (10) gekoppelt ist, um Impulse zu erzeugen und zu dem ersten Wandler (10) zu übertragen;

einen Schwellenwertdetektor (330), der mit dem zweiten Wandler (20) gekoppelt ist, um von dem zweiten Wandler (20) empfangene Impulse zu erfassen; und

eine Messvorrichtung (340, 350, 360), die mit dem Impulsgenerator (320) und dem Schwellenwertdetektor (330) gekoppelt ist;

wobei die Messvorrichtung (340, 350, 360) für jede Entfernungsmessung den Impulsgenerator (320) auslöst, um einen Übertragungsimpuls zu erzeugen und zu dem ersten Wandler (10) zu übertragen, die verstrichene Zeit zwischen der Aussendung des Übertragungsimpulses und der Erfassung eines Empfangsimpulses durch den Schwellenwertdetektor (330) misst und die Entfernungsmessung auf der Grundlage der gemessenen verstrichenen Zeit erzeugt.

## EP 1 527 357 B1

7. System (710, 905) nach Anspruch 6, bei dem die Messvorrichtung einen digitalen Zähler zum Messen der verstrichenen Zeit aufweist.
- 5 8. System (710, 905) nach Anspruch 1, bei dem das Ultraschall-Entfernungsmess-Subsystem (310, 910) mit dem ersten und dem zweiten Wandler (10, 20) gekoppelt ist, um aufeinander folgend Entfernungsmessungen zwischen dem ersten und dem zweiten Wandler (10, 20) durchzuführen; und das Filter (715, 915) mit dem Ultraschall-Entfernungsmess-Subsystem (310, 910) gekoppelt ist, um aufeinander folgend die Entfernungsmessungen zu empfangen, Ultraschall-Interferenzstörungen aus den letzten N Entfernungsmessungen auszufiltern durch Auswählen einer der letzten N Entfernungsmessungen, und die ausgewählte Entfernungsmessung auszugeben.
- 10 9. System (710, 905) nach Anspruch 8, bei dem die ausgewählte Entfernungsmessung größer als die minimale Entfernungsmessung ist.
- 15 10. System (710, 905) nach Anspruch 8, bei dem die ausgewählte Entfernungsmessung die maximale Entfernungsmessung ist.
11. System (710, 905) nach Anspruch 8, bei dem N gleich 8 ist.
- 20 12. System (710, 905) nach Anspruch 8, bei dem das Filter (715, 915) eine Entfernungsvariation der N Entfernungsmessungen berechnet, die Entfernungsvariation mit einem Schwellenwert vergleicht, die ausgewählte Entfernungsmessung ausgibt, wenn die Entfernungsvariation den Schwellenwert überschreitet, und anderenfalls die letzte von dem Ultraschall-Entfernungsmess-Subsystem (310, 910) empfangene Entfernungsmessung ausgibt.
- 25 13. System (710, 905) nach Anspruch 12, bei dem die Entfernungsvariation die Differenz zwischen der maximalen und der minimalen der letzten N Entfernungsmessungen, die von dem Ultraschall-Entfernungsmess-Subsystem (310, 910) empfangen wurden, ist.
- 30 14. System (710, 905) nach Anspruch 12, bei dem die Entfernungsvariation die Veränderlichkeit der letzten N Entfernungsmessungen, die von dem Ultraschall-Entfernungsmess-Subsystem (310, 910) empfangen wurden, ist.
15. System (710, 905) nach Anspruch 12, bei dem die Entfernungsvariation die zweite Ableitung der letzten N Entfernungsmessungen, die von dem Ultraschall-Entfernungsmess-Subsystem (310, 910) empfangen wurden, ist.

### 35 Revendications

1. Système de mesure de distance (710, 905), comprenant :
- 40 des premier et second transducteurs (10, 20) ;  
un sous-système de télémétrie par ultrasons (310, 910) couplé aux premier et second transducteurs (10, 20) pour réaliser une pluralité de mesures de distance entre les premier et second transducteurs (10, 20), le système étant **caractérisé en ce qu'il** comprend en outre :
- 45 un filtre (715, 915) couplé au sous-système de télémétrie par ultrasons (310, 910) pour filtrer une interférence ultrasonore de la pluralité de mesures de distance en sélectionnant l'une de la pluralité de mesures de distance, et pour produire en sortie la mesure de distance sélectionnée.
2. Système (710, 905) selon la revendication 1, dans lequel la mesure de distance sélectionnée est supérieure à la mesure de distance minimum.
- 50 3. Système (710, 905) selon la revendication 1, dans lequel la mesure de distance sélectionnée est la mesure de distance maximum.
4. Système (710, 905) selon la revendication 1, dans lequel l'un des premier et second transducteurs est monté sur un cathéter.
- 55 5. Système (710, 905) selon la revendication 1, dans lequel le nombre de mesures de distance est de 8.

## EP 1 527 357 B1

6. Système (710, 905) selon la revendication 1, dans lequel le sous-système de télémétrie par ultrasons (310, 910) comprend en outre :

un générateur d'impulsions (320) couplé au premier transducteur (10) pour générer et émettre des impulsions d'émission sur le premier transducteur (10) ;  
un détecteur de seuil (330) couplé au second transducteur (20) pour détecter des impulsions de réception en provenance du second transducteur (20) ; et  
un moyen de mesure (340, 350, 360) couplé au générateur d'impulsions (320) et au détecteur de seuil (330),

dans lequel, pour chaque mesure de distance, le moyen de mesure (340, 350, 360) déclenche le générateur d'impulsions (320) pour générer et émettre une impulsion d'émission sur le premier transducteur (10), mesure le temps écoulé entre une émission de l'impulsion d'émission et une détection d'une impulsion de réception par le détecteur de seuil (330), et génère la mesure de distance sur la base du temps écoulé mesuré.

7. Système (710, 905) selon la revendication 6, dans lequel le moyen de mesure comprend un compteur numérique pour mesurer le temps écoulé.

8. Système (710, 905) selon la revendication 1, dans lequel le sous-système de télémétrie par ultrasons (310, 910) est couplé aux premier et second transducteurs (10, 20) pour réaliser séquentiellement des mesures de distance entre les premier et second transducteurs (10, 20) ; et le filtre (715, 915) est couplé au sous-système de télémétrie par ultrasons (310, 910) pour recevoir séquentiellement les mesures de distance, pour filtrer une interférence ultrasonore de\* N dernières mesures de distance en sélectionnant l'une des N dernières mesures de distance et pour produire en sortie la mesure de distance sélectionnée.

9. Système (710, 905) selon la revendication 8, dans lequel la mesure de distance sélectionnée est supérieure à la mesure de distance minimum.

10. Système (710, 905) selon la revendication 8, dans lequel la mesure de distance sélectionnée est la mesure de distance maximum.

11. Système (710, 905) selon la revendication 8, dans lequel N est de 8.

12. Système (710, 905) selon la revendication 8, dans lequel le filtre (715, 915) calcule une variation de distance des N mesures de distance, compare la variation de distance à une valeur de seuil, produit en sortie la mesure de distance sélectionnée lorsque la variation de distance excède la valeur de seuil et produit en sortie la mesure de distance la plus récente reçue depuis le sous-système de télémétrie par ultrasons (310, 910) sinon.

13. Système (710, 905) selon la revendication 12, dans lequel la variation de distance est la différence entre les maximum et minimum des N dernières mesures de distance reçues depuis le sous-système de télémétrie par ultrasons (310, 910).

14. Système (710, 905) selon la revendication 12, dans lequel la variation de distance est la variance des N dernières mesures de distance reçues depuis le sous-système de télémétrie par ultrasons (310, 910).

15. Système (710, 905) selon la revendication 12, dans lequel la variation de distance est la dérivée seconde des N dernières mesures de distance reçues depuis le sous-système de télémétrie par ultrasons (310, 910).

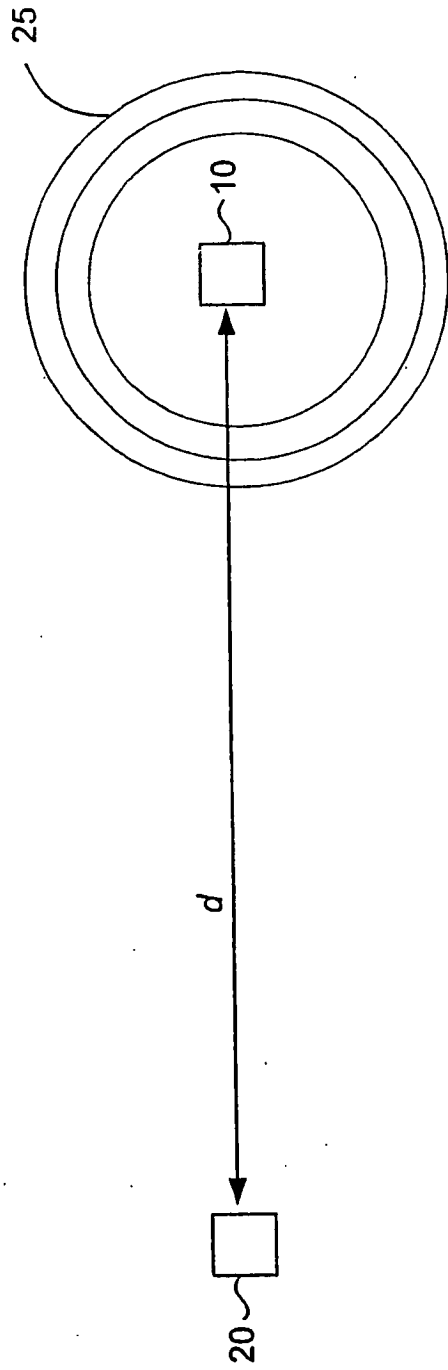


FIG. 1  
(Prior Art)

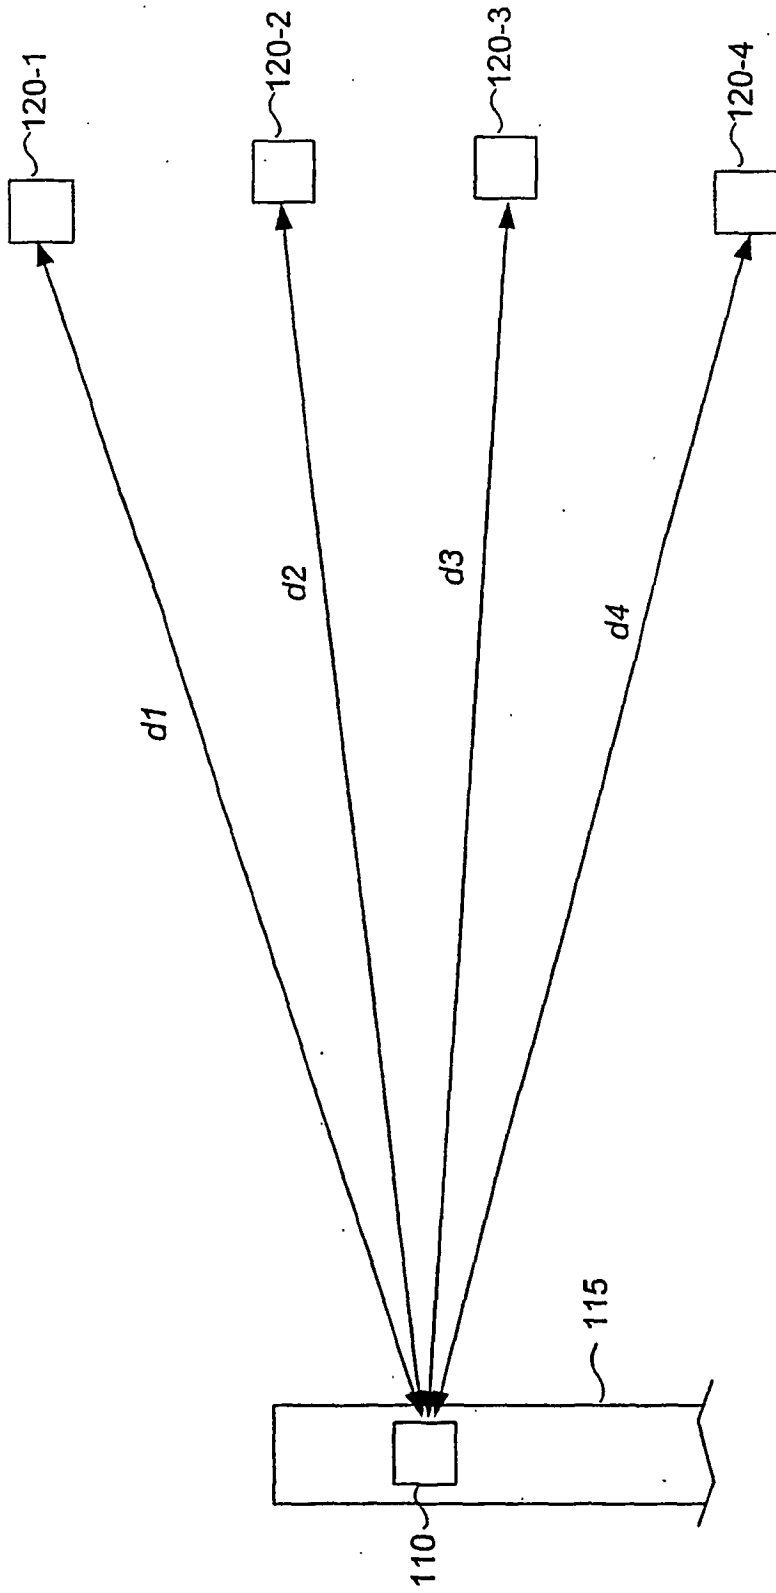


FIG. 2  
(Prior Art)

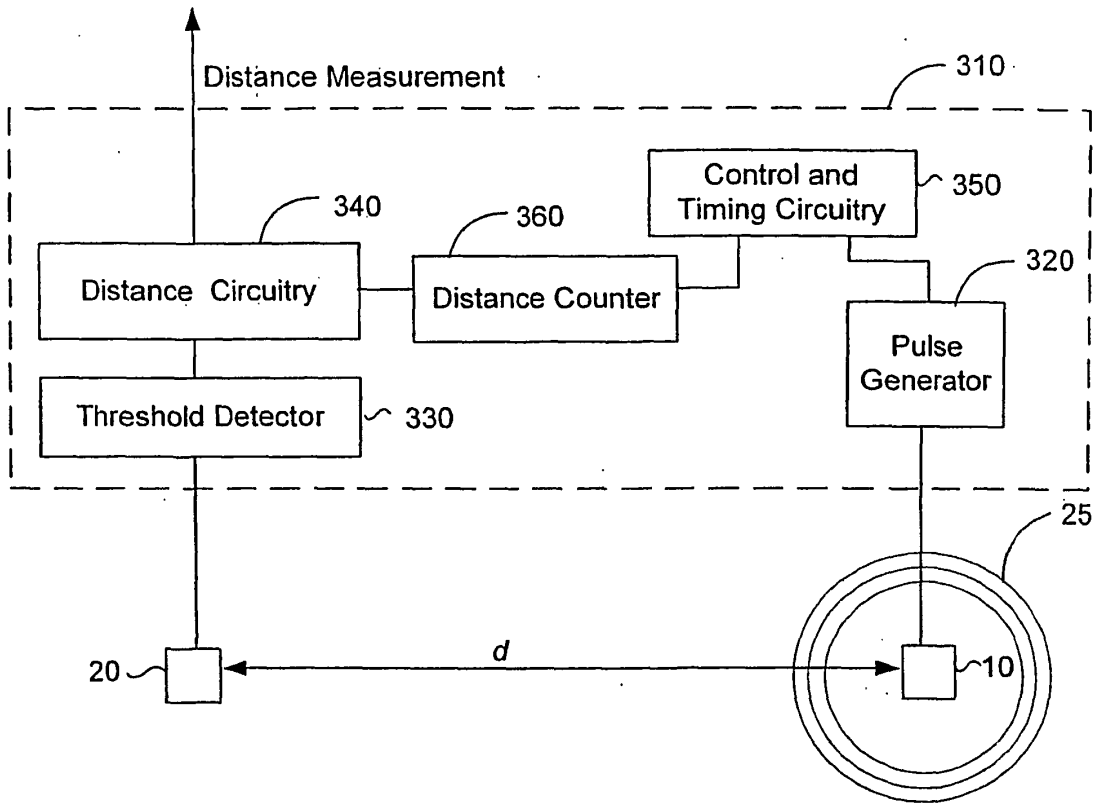


FIG. 3

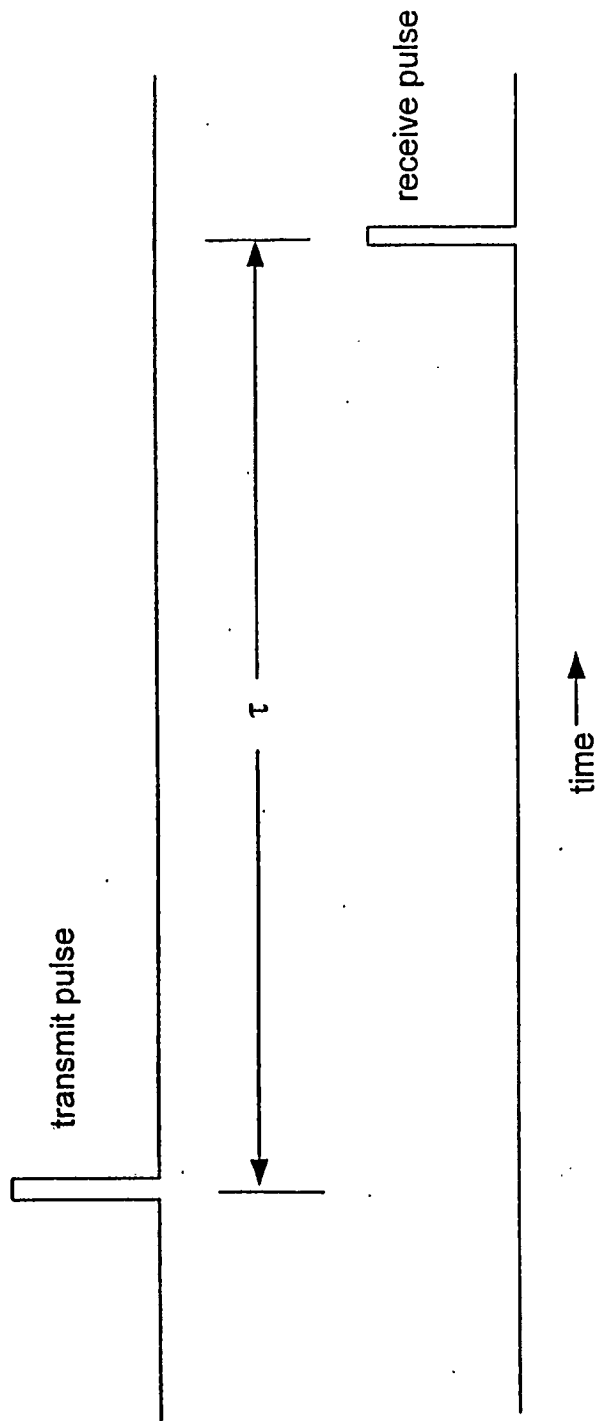


FIG. 4

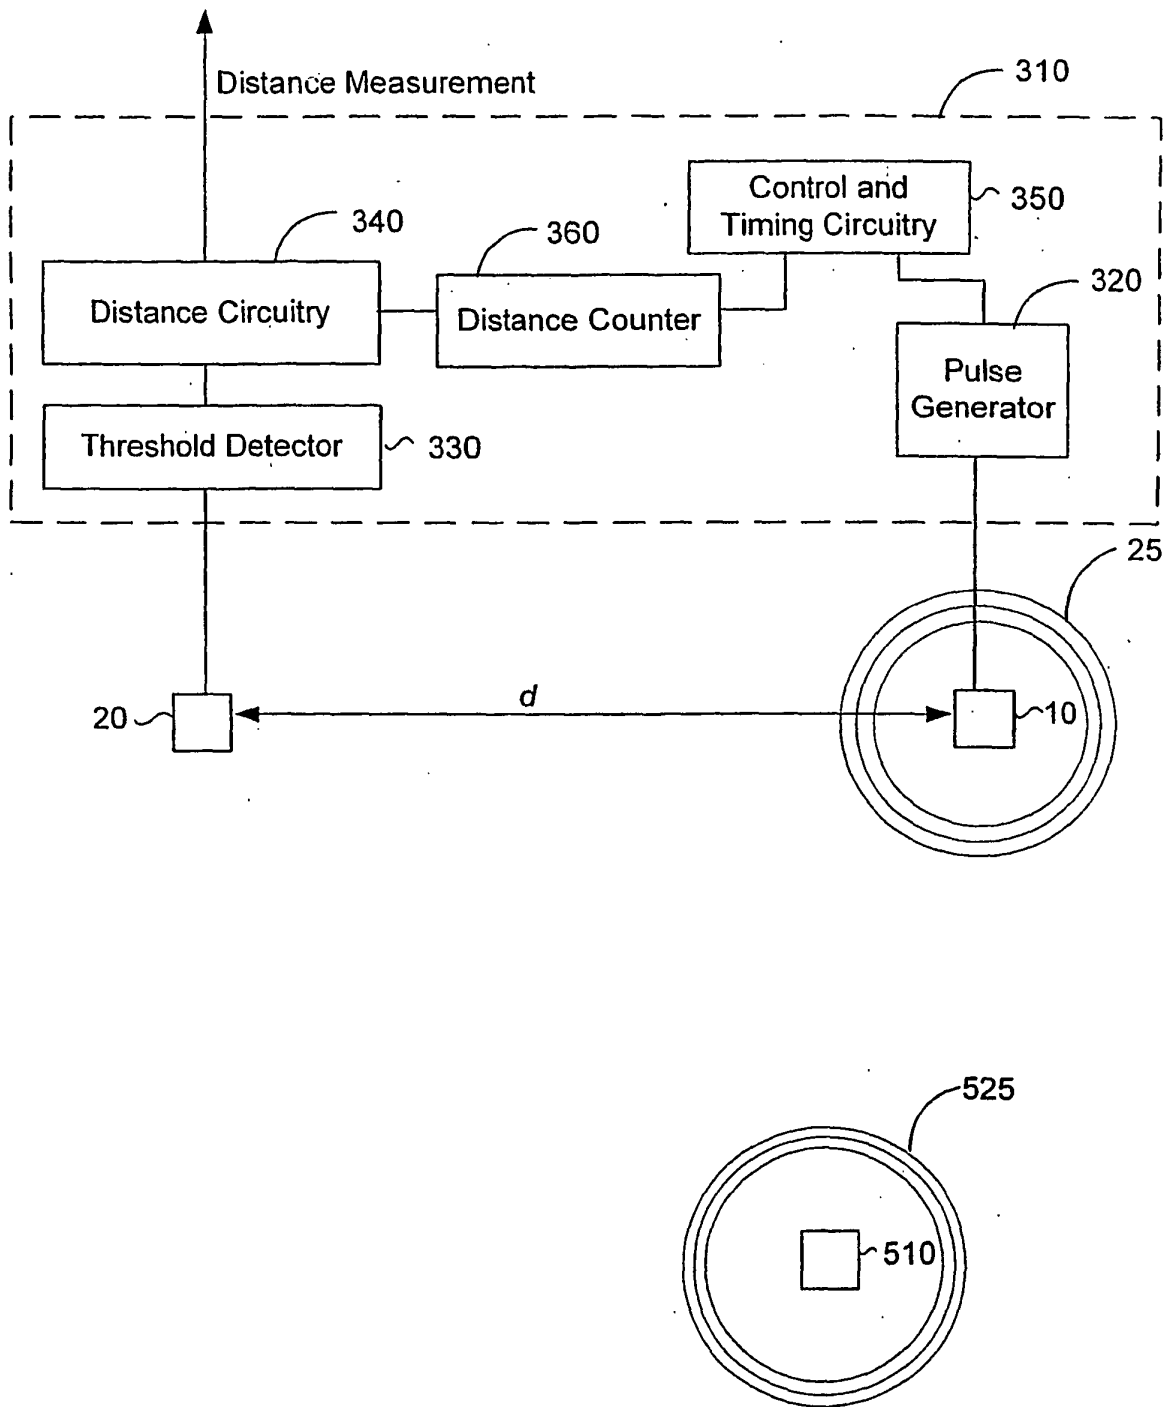


FIG. 5

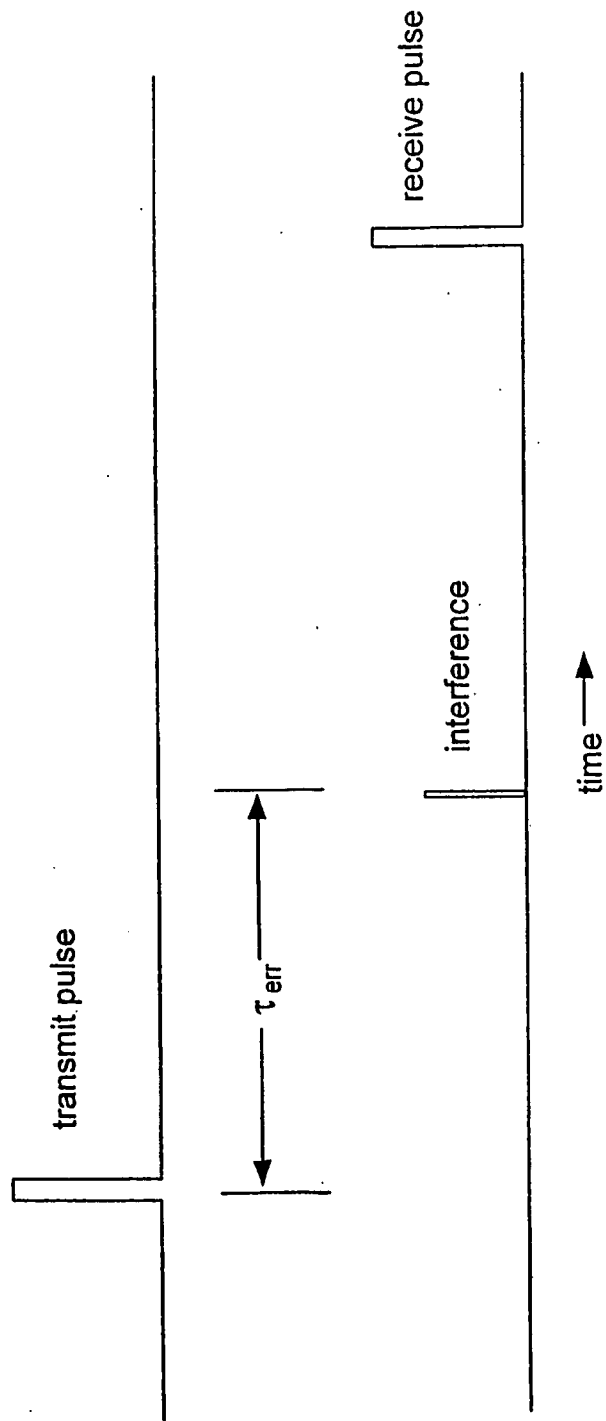


FIG. 6

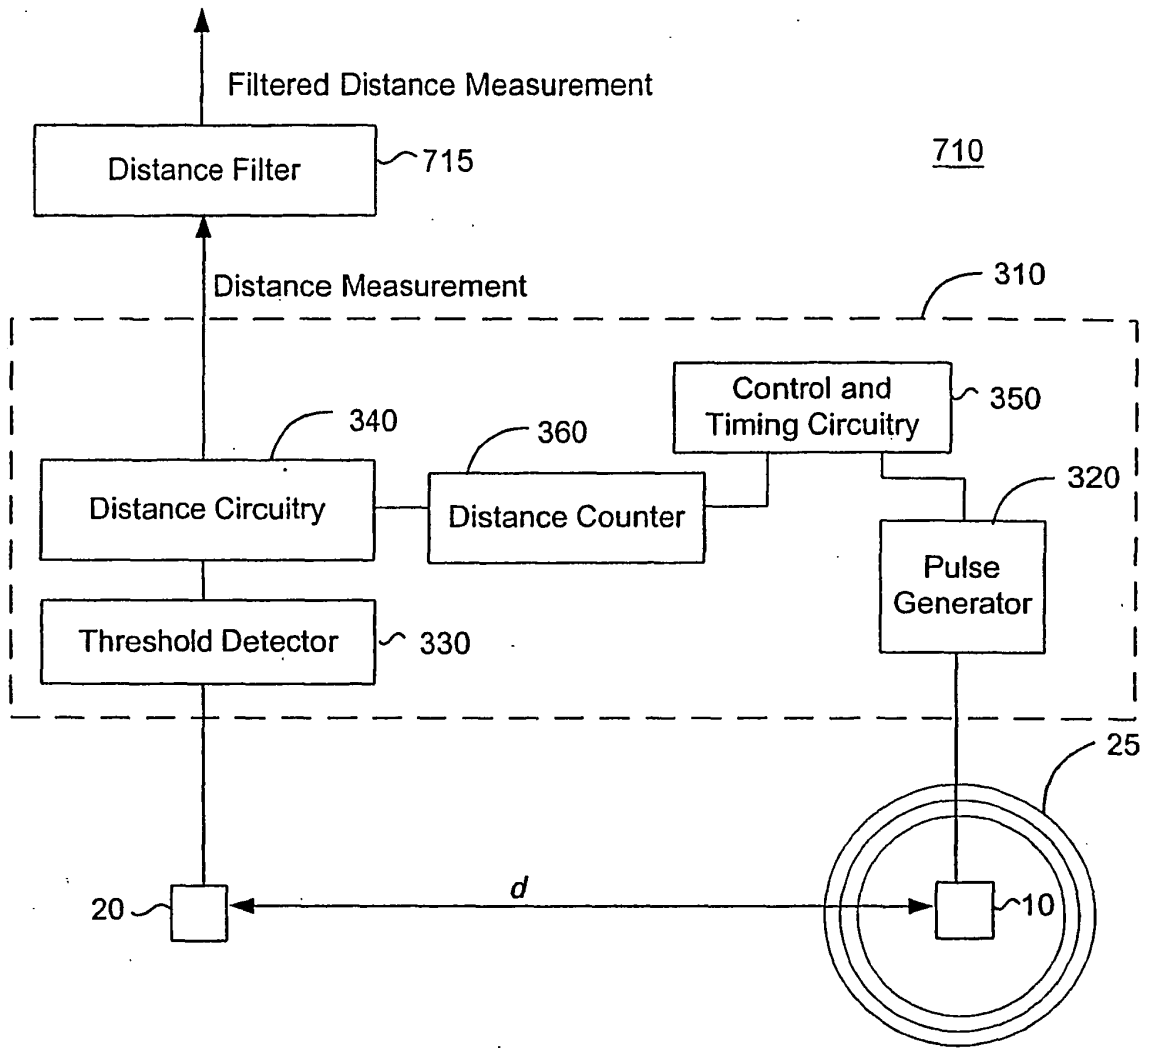


FIG. 7

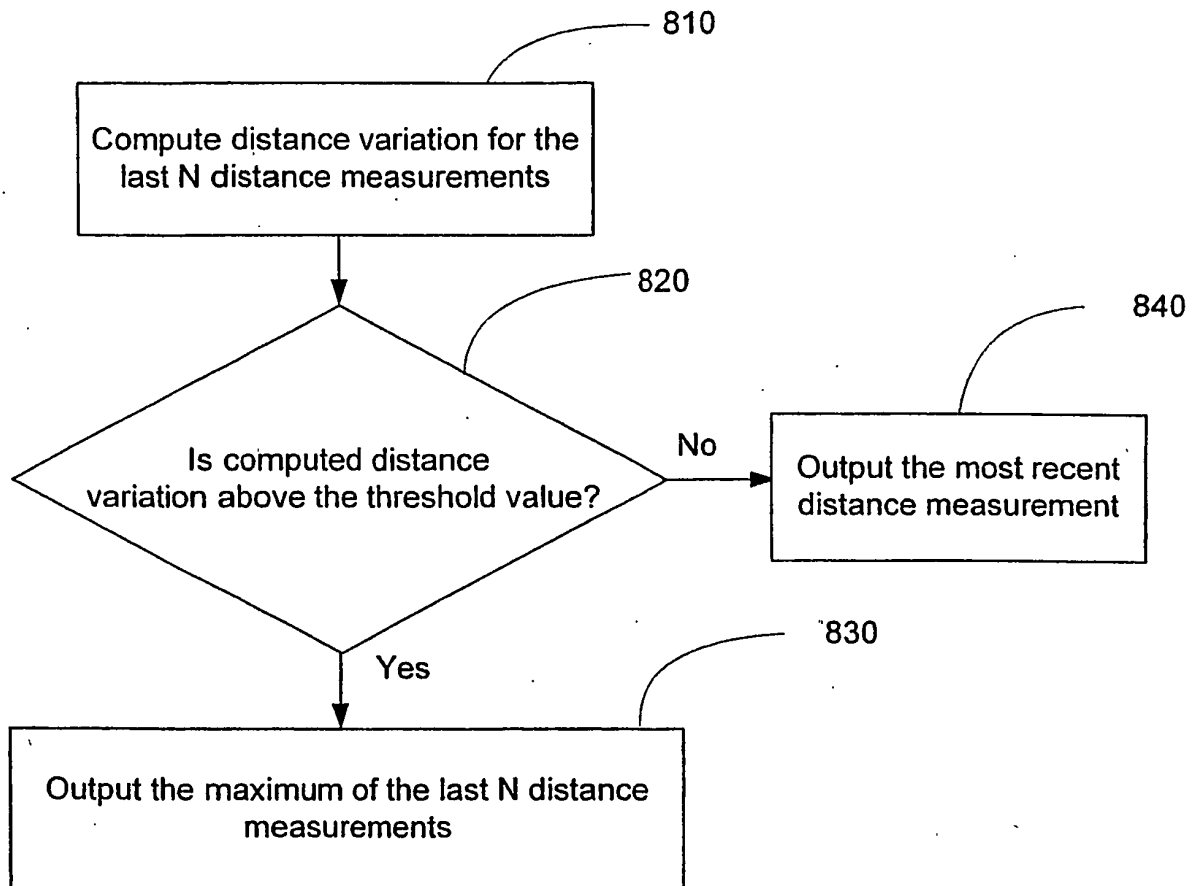


FIG. 8

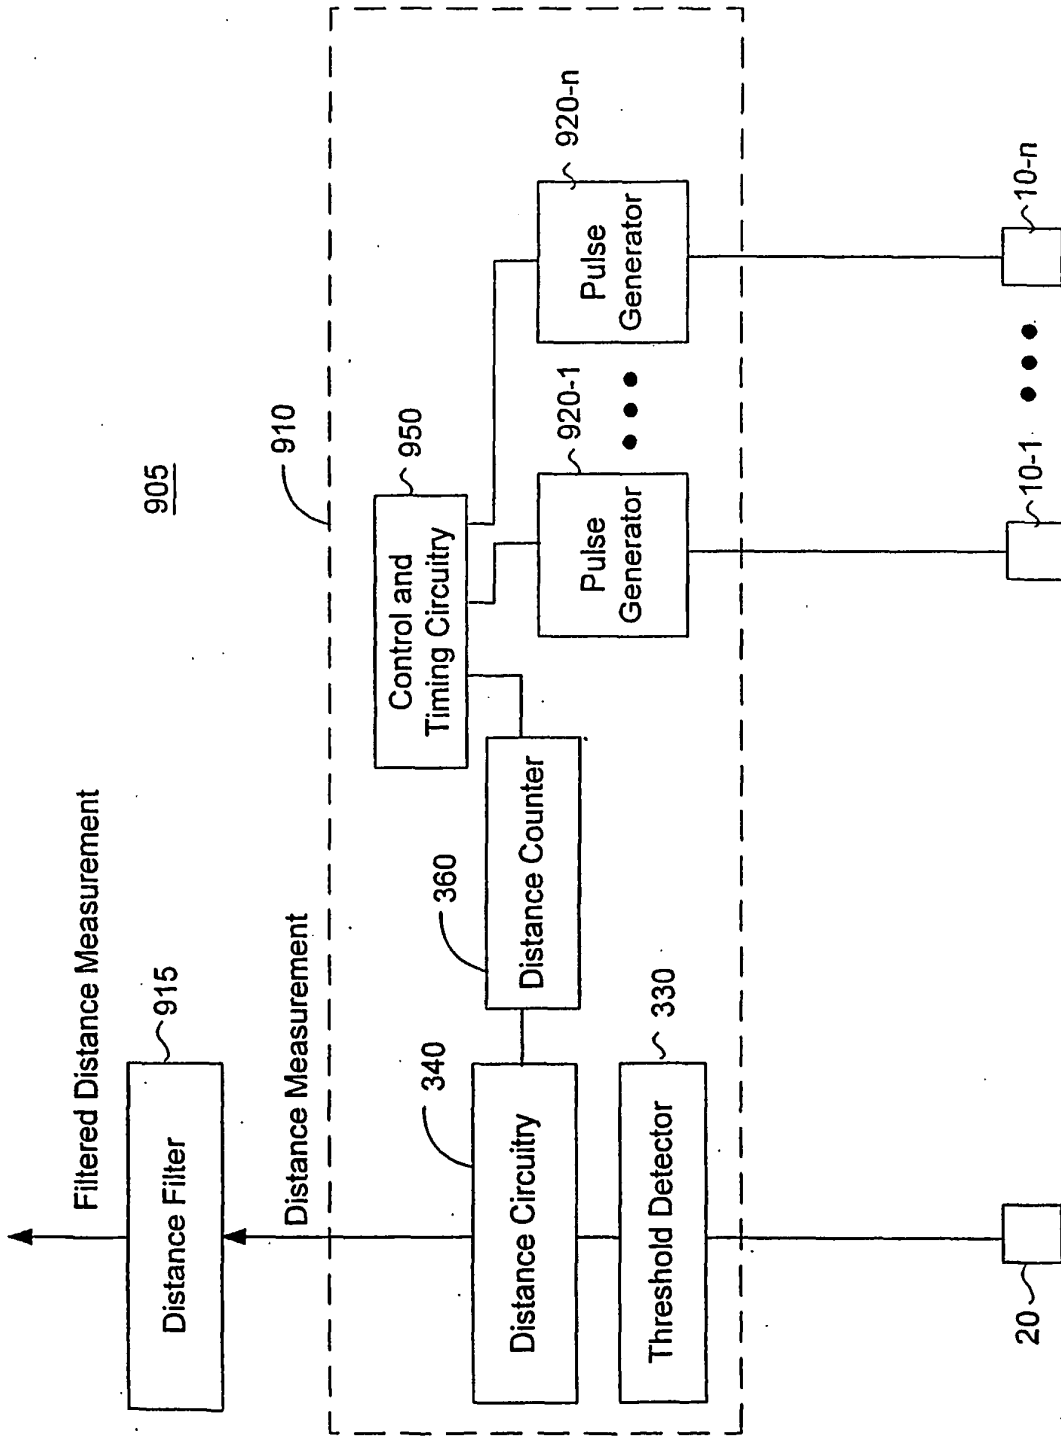


FIG. 9

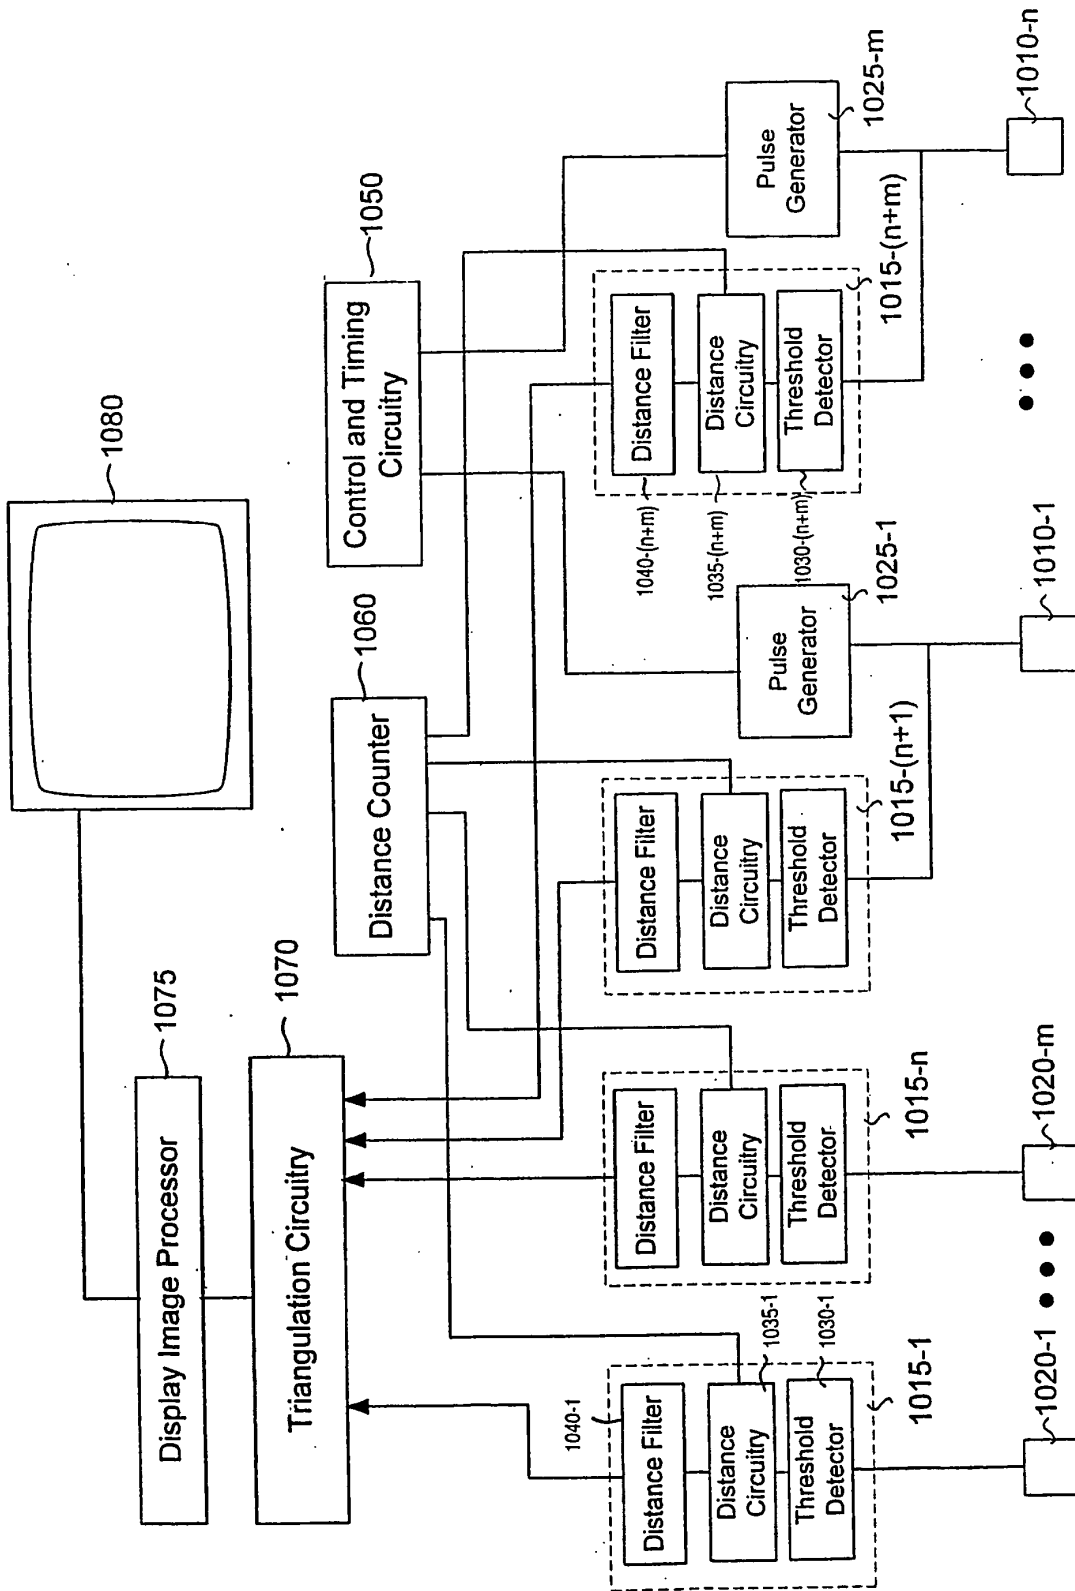


FIG. 10

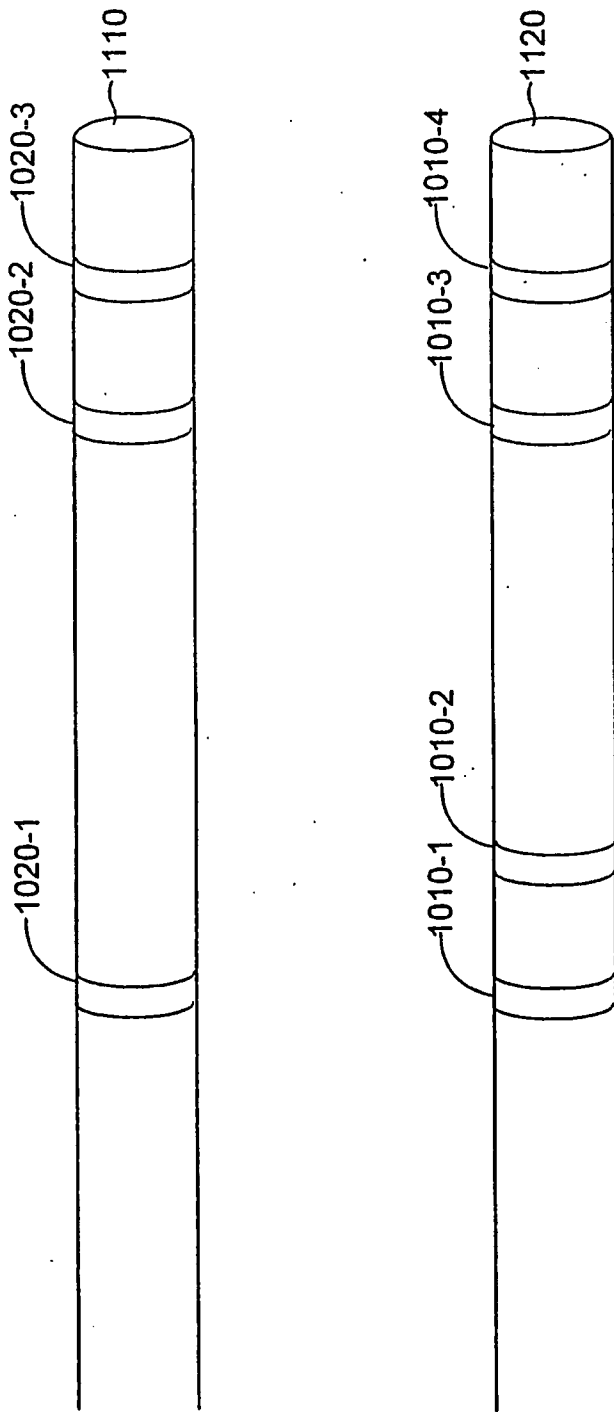


FIG. 11

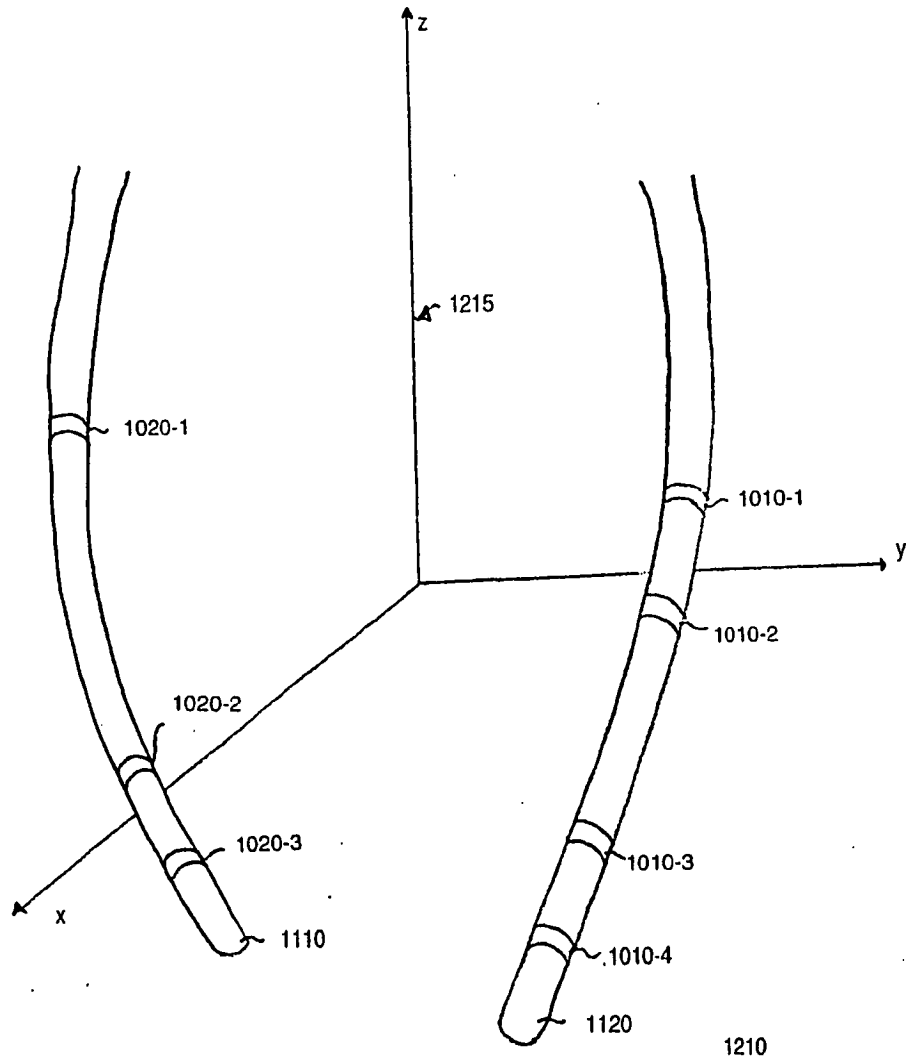


Fig. 12

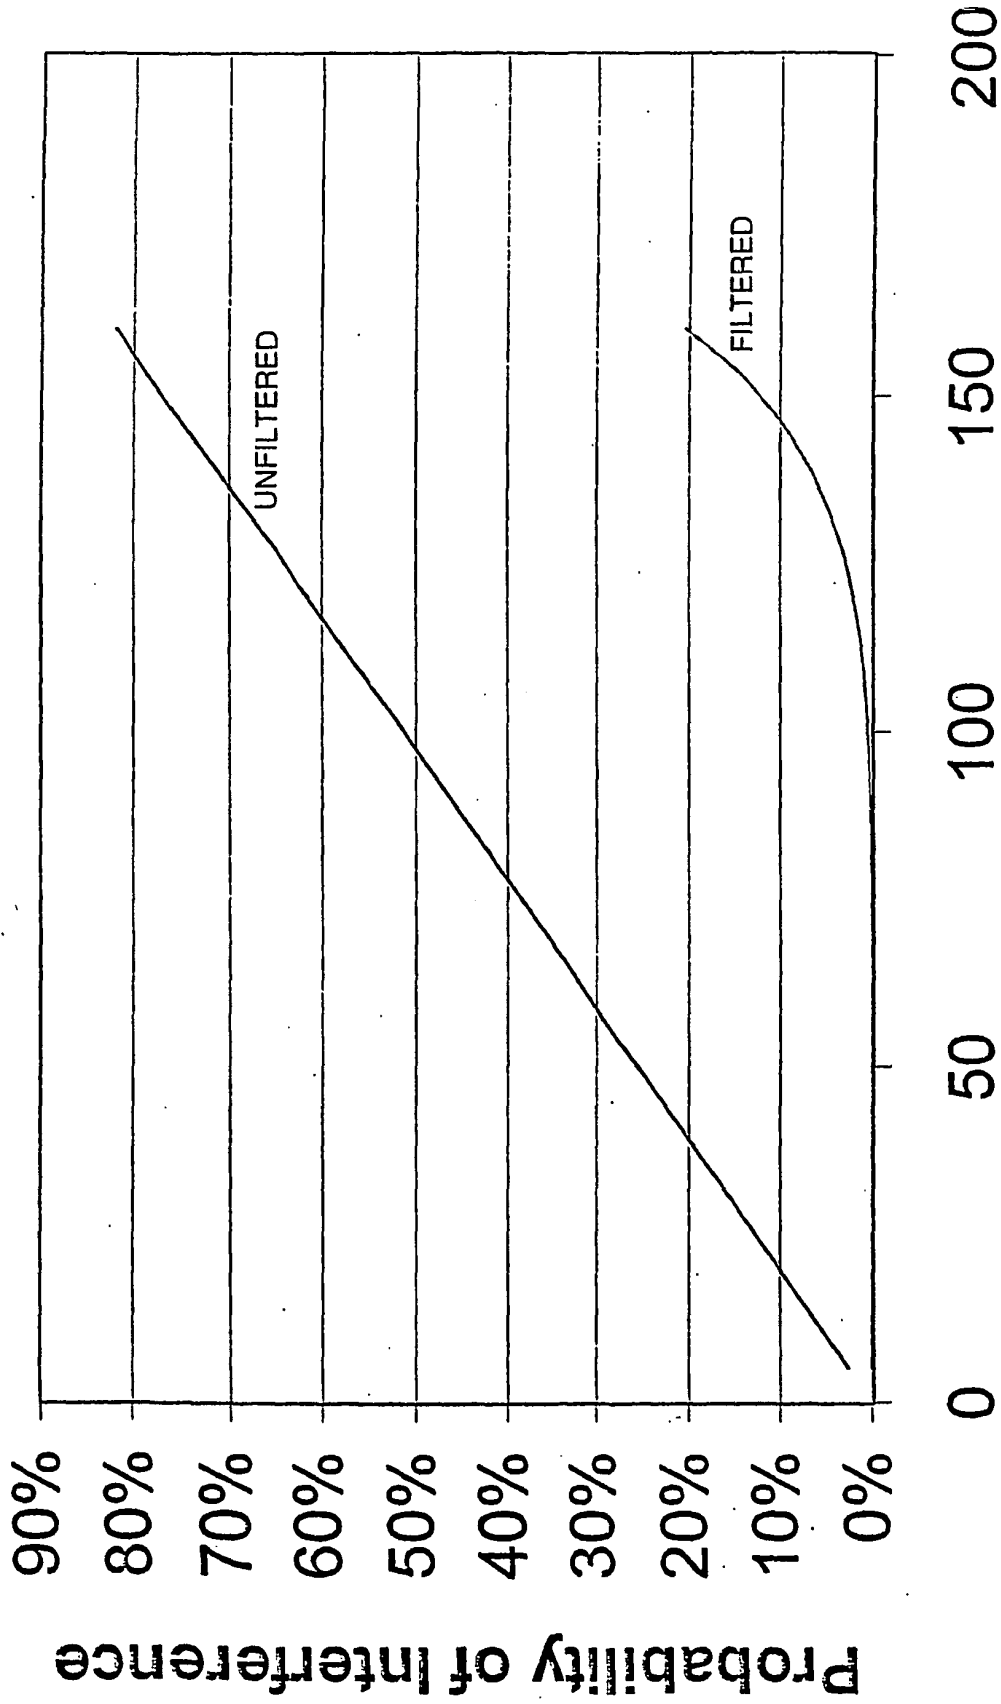


Fig. 13

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 5373482 A [0009]
- US 5321668 A [0010]

专利名称(译)	用于在存在超声干扰的情况下进行超声波测距的系		
公开(公告)号	<a href="#">EP1527357B1</a>	公开(公告)日	2008-10-15
申请号	EP2003767260	申请日	2003-08-04
[标]申请(专利权)人(译)	波士顿科学有限公司		
申请(专利权)人(译)	BOSTON SCIENTIFIC LIMITED		
当前申请(专利权)人(译)	BOSTON SCIENTIFIC LIMITED		
[标]发明人	WILLIS N PARKER		
发明人	WILLIS, N., PARKER		
IPC分类号	G01S11/14 A61B8/12 A61B8/08 G01S5/30 G01S15/10		
CPC分类号	G01S11/14 A61B5/064 A61B5/065 A61B8/0833 A61B8/0841 G01S5/30		
优先权	10/214441 2002-08-06 US		
其他公开文献	EP1527357A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

距离测量系统包括第一和第二换能器，以及耦合到第一和第二换能器的超声测距子系统，用于在第一和第二换能器之间执行多个距离测量。距离测量系统还包括耦合到超声测距子系统的滤波器，用于从多个距离测量（例如，八个）中过滤超声干扰，并基于滤波的距离测量输出距离。滤波器通过选择多个距离测量中的一个来过滤超声干扰，在这种情况下，输出的距离是所选择的距离测量。因为超声干扰通常将其自身表示为最短距离测量，所以所选距离测量优选地大于最小距离测量（例如，最大距离测量），从而将超声干扰滤除。

$$d = vt$$