

(19)



(11)

EP 2 276 409 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
30.05.2018 Bulletin 2018/22

(51) Int Cl.:
A61B 8/12 (2006.01)

(21) Application number: **09732222.6**

(86) International application number:
PCT/US2009/040914

(22) Date of filing: **17.04.2009**

(87) International publication number:
WO 2009/129438 (22.10.2009 Gazette 2009/43)

(54) INTRAVASCULAR ULTRASOUND IMAGING SYSTEMS WITH SEALED CATHETERS FILLED WITH AN ACOUSTICALLY-FAVORABLE MEDIUM AND METHODS OF MAKING

INTRAVASKULÄRE ULTRASCHALL-DARSTELLUNGSSYSTEME MIT ABGEDICHTETEN KATHETERN, DIE MIT EINEM AKUSTISCH GÜNSTIGEN MEDIUM GEFÜLLT SIND, UND HERSTELLUNGSverfahren

SYSTÈMES D'IMAGERIE ULTRASONORE INTRAVASCULAIRES AVEC DES CATHÉTERS SCÉLLÉS REMPLIS D'UN MILIEU FAVORABLE SUR LE PLAN ACOUSTIQUE ET PROCÉDÉS DE FABRICATION

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO SE SI SK TR

(72) Inventor: **SADAKA, Alain**
San Jose
CA 95120 (US)

(30) Priority: **17.04.2008 US 45904**

(74) Representative: **Vossius & Partner**
Patentanwälte Rechtsanwälte mbB
Siebertstrasse 3
81675 München (DE)

(43) Date of publication of application:
26.01.2011 Bulletin 2011/04

(73) Proprietor: **Boston Scientific Scimed, Inc.**
Maple Grove, MN 55311-1566 (US)

(56) References cited:
US-A- 4 951 677 US-A- 5 167 233
US-A- 5 331 947 US-A- 5 967 984

EP 2 276 409 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionCROSS REFERENCE TO RELATED APPLICATION

[0001] This application claims the benefit of U.S. Provisional Patent Application Serial No. 61/045,904, filed April 17, 2008, the entire contents of which is incorporated by reference.

TECHNICAL FIELD

[0002] The present invention is directed to the area of intravascular ultrasound imaging systems and methods of making the systems. The present invention is also directed to an intravascular ultrasound imaging system with a catheter having a sealed lumen filled with an acoustically-favorable medium, as well as methods of making the intravascular ultrasound systems.

BACKGROUND

[0003] Intravascular ultrasound ("IVUS") imaging systems have proven diagnostic capabilities for a variety of diseases and disorders. A known system of this kind is described, e.g. in document US 5 331 947 A. For example, IVUS imaging systems have been used as an imaging modality for diagnosing blocked blood vessels and providing information to aid medical practitioners in selecting and placing stents and other devices to restore or increase blood flow. IVUS imaging systems have been used to diagnose atheromatous plaque build-up at particular locations within blood vessels. IVUS imaging systems can be used to determine the existence of an intravascular obstruction or stenosis, as well as the nature and degree of the obstruction or stenosis. IVUS imaging systems can be used to visualize segments of a vascular system that may be difficult to visualize using other intravascular imaging techniques, such as angiography, due to, for example, movement (e.g., a beating heart) or obstruction by one or more structures (e.g., one or more blood vessels not desired to be imaged). IVUS imaging systems can be used to monitor or assess ongoing intravascular treatments, such as angiography and stent placement in real (or almost real) time. Moreover, IVUS imaging systems can be used to monitor one or more heart chambers.

[0004] IVUS imaging systems have been developed to provide a diagnostic tool for visualizing a variety of diseases or disorders. An IVUS imaging system can include a control module (with a pulse generator, an image processor, and a monitor), a catheter, and one or more transducers disposed in the catheter. The transducer-containing catheter can be positioned in a lumen or cavity within, or in proximity to, a region to be imaged, such as a blood vessel wall or patient tissue in proximity to a blood vessel wall. The pulse generator in the control module generates electrical pulses that are delivered to the one or more

transducers and transformed to acoustic pulses that are transmitted through patient tissue. Reflected pulses of the transmitted acoustic pulses are absorbed by the one or more transducers and transformed to electric pulses.

The transformed electric pulses are delivered to the image processor and converted to an image displayable on the monitor.

BRIEF SUMMARY

[0005] In one embodiment, a catheter assembly for an intravascular ultrasound system includes a catheter and an imaging core. The catheter has a longitudinal length, a distal end, and a proximal end. The catheter includes a sealable lumen extending along the longitudinal length of the catheter from the proximal end to the distal end, and a movable plunger or a movable seal in fluid communication with the lumen. The movable plunger or the movable seal provides a gas-tight seal. The movable plunger or the movable seal is configured and arranged for adjusting to changes in volume of the lumen when the lumen is filled with an acoustically-favorable medium and sealed. The imaging core is configured and arranged for inserting into the sealable lumen and for coupling to a control module.

[0006] In another embodiment, an intravascular ultrasound imaging system includes a catheter, an imaging core, and a control module. The catheter has a longitudinal length, a distal end, and a proximal end. The catheter includes a sealable lumen extending along the longitudinal length of the catheter from the proximal end to the distal end, and a movable plunger or a movable seal in fluid communication with the lumen. The movable plunger or the movable seal provides an acoustically-favorable-medium-tight seal. The movable plunger or the movable seal is configured and arranged for adjusting to changes in volume of the lumen to maintain an acoustically-favorable-medium-filled environment within the lumen when the lumen is filled with an acoustically-favorable medium and sealed. The imaging core is disposed within the lumen. The control module is coupled to the imaging core. The control module includes a pulse generator and a processor. The pulse generator and the processor are both electrically coupled to the imaging core. The pulse generator is configured and arranged for providing electric pulses to the imaging core. The processor is configured and arranged for processing received electrical pulses from the imaging core to form at least one image.

[0007] In yet another embodiment, a method for forming a catheter of an intravascular ultrasound imaging system includes degassing a sealable lumen of the catheter, filling the sealable lumen with an acoustically-favorable medium through at least one flush port, and sealing the lumen using a movable plunger or a movable seal in fluid communication with the sealable lumen. The catheter includes at least one transducer mounted to a driveshaft extending along at least a portion of a longitudinal length

of the sealable lumen. The movable plunger or the movable seal is configured and arranged to adjust to changes in volume of the lumen to maintain the substantially degassed environment in the lumen.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008] Non-limiting and non-exhaustive embodiments of the present invention are described with reference to the following drawings. In the drawings, like reference numerals refer to like parts throughout the various figures unless otherwise specified.

[0009] For a better understanding of the present invention, reference will be made to the following Detailed Description, which is to be read in association with the accompanying drawings, wherein:

FIG. 1 is a schematic view of one embodiment of an intravascular ultrasound imaging system, according to the invention;

FIG. 2 is a schematic side view of one embodiment of a catheter of an intravascular ultrasound imaging system, according to the invention;

FIG. 3 is a schematic perspective view of one embodiment of a distal end of an elongated member of the catheter shown in FIG. 2 with an imaging core disposed in a lumen in the distal end of the elongated member, according to the invention;

FIG. 4 is a schematic longitudinal cross-sectional view of one embodiment of a hub of a catheter, the hub including a movable plunger disposed in a main flush port, according to the invention;

FIG. 5A is a schematic longitudinal cross-sectional view of one embodiment of a hub with a movable seal or a movable plunger disposed in a main flush port and an open auxiliary input port, according to the invention; and

FIG. 5B is a schematic longitudinal cross-sectional view of another embodiment of a hub with a movable seal or a movable plunger disposed in a main flush port and a seal disposed in an auxiliary input port, according to the invention.

DETAILED DESCRIPTION

[0010] The present invention is directed to the area of intravascular ultrasound imaging systems and methods of making the systems. The present invention is also directed to an intravascular ultrasound imaging system with a catheter having a sealed lumen filled with an acoustically-favorable medium, as well as methods of making the catheter and intravascular ultrasound system.

[0011] Suitable intravascular ultrasound ("IVUS") imaging systems include, but are not limited to, one or more transducers disposed on a distal end of a catheter configured and arranged for percutaneous insertion into a patient. Examples of IVUS imaging systems with catheters are found in, for example, U.S. Patents Nos. 7,306,561; and 6,945,938; as well as U.S. Patent Application Publication Nos. 20060253028; 20070016054; 20070038111; 20060173350; and 20060100522, all of which are incorporated by reference.

[0012] Figure 1 illustrates schematically one embodiment of an IVUS imaging system 100. The IVUS imaging system 100 includes a catheter 102 that is coupleable to a control module 104. The control module 104 may include, for example, a processor 106, a pulse generator 108, a motor 110, and one or more displays 112. In at least some embodiments, the pulse generator 108 forms electric pulses that may be input to one or more transducers (312 in Figure 3) disposed in the catheter 102. In at least some embodiments, mechanical energy from the motor 110 may be used to drive an imaging core (306 in Figure 3) disposed in the catheter 102. In at least some embodiments, electric pulses transmitted from the one or more transducers (312 in Figure 3) may be input to the processor 106 for processing. In at least some embodiments, the processed electric pulses from the one or more transducers (312 in Figure 3) may be displayed as one or more images on the one or more displays 112. In at least some embodiments, the processor 106 may also be used to control the functioning of one or more of the other components of the control module 104. For example, the processor 106 may be used to control at least one of the frequency or duration of the electrical pulses transmitted from the pulse generator 108, the rotation rate of the imaging core (306 in Figure 3) by the motor 110, the velocity or length of the pullback of the imaging core (306 in Figure 3) by the motor 110, or one or more properties of one or more images formed on the one or more displays 112.

[0013] Figure 2 is a schematic side view of one embodiment of the catheter 102 of the IVUS imaging system (100 in Figure 1). The catheter 102 includes an elongated member 202 and a hub 204. The elongated member 202 includes a proximal end 206 and a distal end 208. In Figure 2, the proximal end 206 of the elongated member 202 is coupled to the catheter hub 204 and the distal end 208 of the elongated member is configured and arranged for percutaneous insertion into a patient. In at least some embodiments, the catheter 102 defines at least one flush port, such as flush port 210. In at least some embodiments, the flush port 210 is defined in the hub 204. In at least some embodiments, the hub 204 is configured and arranged to couple to the control module (104 in Figure 1). In some embodiments, the elongated member 202 and the hub 204 are formed as a unitary body. In other embodiments, the elongated member 202 and the catheter hub 204 are formed separately and subsequently assembled together.

[0014] Figure 3 is a schematic perspective view of one embodiment of the distal end 208 of the elongated member 202 of the catheter 102. The elongated member 202 includes a sheath 302 and a lumen 304. An imaging core 306 is disposed in the lumen 304. The imaging core 306 includes an imaging device 308 coupled to a distal end of a rotatable driveshaft 310.

[0015] The sheath 302 may be formed from any flexible, biocompatible material suitable for insertion into a patient. Examples of suitable materials include, for example, polyethylene, polyurethane, plastic, spiral-cut stainless steel, nitinol hypotube, and the like or combinations thereof.

[0016] One or more transducers 312 may be mounted to the imaging device 308 and employed to transmit and receive acoustic pulses. In a preferred embodiment (as shown in Figure 3), an array of transducers 312 are mounted to the imaging device 308. In other embodiments, a single transducer may be employed. In yet other embodiments, multiple transducers in an irregular-array may be employed. Any number of transducers 312 can be used. For example, there can be two, three, four, five, six, seven, eight, nine, ten, twelve, fifteen, sixteen, twenty, twenty-five, fifty, one hundred, five hundred, one thousand, or more transducers. As will be recognized, other numbers of transducers may also be used.

[0017] The one or more transducers 312 may be formed from one or more known materials capable of transforming applied electrical pulses to pressure distortions on the surface of the one or more transducers 312, and vice versa. Examples of suitable materials include piezoelectric ceramic materials, piezocomposite materials, piezoelectric plastics, barium titanates, lead zirconate titanates, lead metaniobates, polyvinylidene fluoride, and the like.

[0018] The pressure distortions on the surface of the one or more transducers 312 form acoustic pulses of a frequency based on the resonant frequencies of the one or more transducers 312. The resonant frequencies of the one or more transducers 312 may be affected by the size, shape, and material used to form the one or more transducers 312. The one or more transducers 312 may be formed in any shape suitable for positioning within the catheter 102 and for propagating acoustic pulses of a desired frequency in one or more selected directions. For example, transducers may be disc-shaped, block-shaped, rectangular-shaped, oval-shaped, and the like. The one or more transducers may be formed in the desired shape by any process including, for example, dicing, dice and fill, machining, microfabrication, and the like.

[0019] As an example, each of the one or more transducers 312 may include a layer of piezoelectric material sandwiched between a conductive acoustic lens and a conductive backing material formed from an acoustically absorbent material (e.g., an epoxy substrate with tungsten particles). During operation, the piezoelectric layer may be electrically excited by both the backing material

and the acoustic lens to cause the emission of acoustic pulses.

[0020] In at least some embodiments, the one or more transducers 312 can be used to form a radial cross-sectional image of a surrounding space. Thus, for example, when the one or more transducers 312 are disposed in the catheter 102 and inserted into a blood vessel of a patient, the one or more transducers 312 may be used to form an image of the walls of the blood vessel and tissue surrounding the blood vessel.

[0021] In at least some embodiments, the imaging core 306 may be rotated about a longitudinal axis of the catheter 102. As the imaging core 306 rotates, the one or more transducers 312 emit acoustic pulses in different radial directions. When an emitted acoustic pulse with sufficient energy encounters one or more medium boundaries, such as one or more tissue boundaries, a portion of the emitted acoustic pulse is reflected back to the emitting transducer as an echo pulse. Each echo pulse that reaches a transducer with sufficient energy to be detected is transformed to an electrical signal in the receiving transducer. The one or more transformed electrical signals are transmitted to the control module (104 in Figure 1) where the processor 106 processes the electrical-signal characteristics to form a displayable image of the imaged region based, at least in part, on a collection of information from each of the acoustic pulses transmitted and the echo pulses received. In at least some embodiments, the rotation of the imaging core 306 is driven by the motor 110 disposed in the control module (104 in Figure 1).

[0022] As the one or more transducers 312 rotate about the longitudinal axis of the catheter 102 emitting acoustic pulses, a plurality of images are formed that collectively form a radial cross-sectional image of a portion of the region surrounding the one or more transducers 312, such as the walls of a blood vessel of interest and the tissue surrounding the blood vessel. In at least some embodiments, the radial cross-sectional image can be displayed on one or more displays 112.

[0023] In at least some embodiments, the imaging core 306 may also move longitudinally along the blood vessel within which the catheter 102 is inserted so that a plurality of cross-sectional images may be formed along a longitudinal length of the blood vessel. In at least some embodiments, during an imaging procedure the one or more transducers 312 may be retracted (*i.e.*, pulled back) along the longitudinal length of the catheter 102. In at least some embodiments, the catheter 102 includes at least one telescoping section that can be retracted during pullback of the one or more transducers 312. In at least some embodiments, the motor 110 drives the pullback of the imaging core 306 within the catheter 102. In at least some embodiments, the motor 110 pullback distance of the imaging core is at least 5 cm. In at least some embodiments, the motor 110 pullback distance of the imaging core is at least 10 cm. In at least some embodiments, the motor 110 pullback distance of the imaging

core is at least 15 cm. In at least some embodiments, the motor 110 pullback distance of the imaging core is at least 20 cm. In at least some embodiments, the motor 110 pullback distance of the imaging core is at least 25 cm.

[0024] The quality of an image produced at different depths from the one or more transducers 312 may be affected by one or more factors including, for example, bandwidth, transducer focus, beam pattern, as well as the frequency of the acoustic pulse. The frequency of the acoustic pulse output from the one or more transducers 312 may also affect the penetration depth of the acoustic pulse output from the one or more transducers 312. In general, as the frequency of an acoustic pulse is lowered, the depth of the penetration of the acoustic pulse within patient tissue increases. In at least some embodiments, the IVUS imaging system 100 operates within a frequency range of 5MHz to 60 MHz.

[0025] In at least some embodiments, one or more conductors 314 electrically couple the transducers 312 to the control module 104 (See Figure 1). In at least some embodiments, the one or more conductors 314 extend along a longitudinal length of the rotatable driveshaft 310.

[0026] In at least some embodiments, the catheter 102 with one or more transducers 312 mounted to the distal end 208 of the imaging core 308 may be inserted percutaneously into a patient via an accessible blood vessel, such as the femoral artery, at a site remote from the selected portion of the selected region, such as a blood vessel, to be imaged. The catheter 102 may then be advanced through the blood vessels of the patient to the selected imaging site, such as a portion of a selected blood vessel.

[0027] Acoustic pulses propagating from the one or more transducers 312 propagate through the lumen of the catheter 102 before passing through the sheath 302 to the region exterior of the catheter 102, such as a blood vessel or a chamber of a heart. Likewise, echo pulses reflected back to the one or more transducers 312 from medium boundaries also propagate through the lumen of the catheter 102. Typically, air is not a desirable transmission medium and image quality may, consequently, be reduced when acoustic pulses or echo pulses are required by catheter design to propagate through air. In the MHz range, acoustic pulses may not propagate at all through air. Accordingly, it is typically advantageous, and in some cases necessary, to purge air from the lumen 304 surrounding the one or more transducers 312 prior to the performance of an imaging procedure. One technique for purging air surrounding the one or more transducers 312 is to flush the lumen 304 with an acoustically-favorable medium through which acoustic pulses more easily propagate than through air. Acoustically-favorable media may include one or more solvents such as, for example, water. An acoustically-favorable medium may include one or more solutes mixed with the one or more solvents such as, for example, one or more salts. In at least some embodiments, one or more agents may also

be added, for example, to decrease the potential advancement of corrosion or microbial growth. In at least some embodiments, an acoustically-favorable medium may include a gel, and the like. In at least some embodiments, the acoustically-favorable medium may be input through the main flush port 210. In at least some embodiments, the elongated member 202 also defines an output port 316 for outputting one or more gases.

[0028] When using a conventional IVUS imaging system, a lumen of a catheter may be flushed to remove air at the beginning of an IVUS imaging procedure. Additionally, the lumen of the catheter may also need to be flushed of air one or more additional times during the course of the IVUS imaging procedure. Unfortunately, each flushing of air from the catheter lumen can add to the amount of time it takes for a healthcare professional to perform an IVUS imaging procedure on a patient. Moreover, the use of IVUS imaging systems often results in changes in volume of the lumen. For example, the volume of the lumen may change as the lumen twists and turns around tortuous blood vessels during placement of a catheter. Additionally, during an IVUS imaging procedure the volume of a lumen may change during pullback, as the imaging core 306 moves longitudinally along a longitudinal length of the catheter 102. As discussed above, in at least some embodiments the catheter 102 may include one or more telescoping sections that retract during pullback. In at least some embodiments, the retraction of the one or more telescoping sections may change the volume of the lumen. When the volume of a lumen changes, it may be the case that an air pocket develops across a portion of the path along which an acoustic pulse or an echo pulse propagates, thereby potentially reducing the quality of the IVUS image, or even prohibiting the IVUS imaging system 100 from forming an IVUS image.

[0029] To address these issues, in at least some embodiments the catheter 102 is filled with an acoustically-favorable medium and sealed so that the acoustically-favorable medium remains in the lumen 304. By sealing the catheter 102 with an acoustically-favorable medium, it is not necessary to flush the lumen 304 of air either before or during an IVUS imaging procedure. In at least some embodiments, the catheter 102 utilizes one or more movable seals or movable plungers in fluid communication with the lumen 304. The one or more movable seals or the movable plungers adjust to changes in the internal volume of the lumen 304 to maintain the lumen 304 of the catheter 102 filled with the acoustically-favorable medium. Figure 4 is a schematic longitudinal cross-sectional view of one embodiment of the hub 204. The hub 204 includes a movable seal or a movable plunger 402 disposed in the main flush port 210. In at least some embodiments, the movable seal or the movable plunger 402 act like a piston moving up and down as the volume of the lumen 304 changes.

[0030] In at least some embodiments, the lumen 304 is degassed, filled with an acoustically-favorable medi-

um, and sealed with the movable seal or the movable plunger 402. In at least some embodiments, degassing involves generating a vacuum in the lumen 304 and then filling the lumen 304 with an acoustically-favorable medium without introducing gas into the lumen 304. For example, in at least some embodiments, air in the lumen 304 is flushed out of the main flush port 210, an acoustically-favorable medium is input to the main flush port 210, and the main flush port 210 is sealed with the movable seal or the movable plunger 402. In at least some embodiments, the lumen 304 is degassed, filled with the acoustically-favorable medium, and the main flush port 210 is sealed all in one integrated step. In at least some embodiments, the operability of the imaging core 306 may be tested prior to sealing the main flush port 210.

[0031] Once the lumen 304 is filled with the acoustically-favorable medium and the main flush port 210 is sealed, the movable seal or the movable plunger 402 moves along a longitudinal length of the main flush port 210 in a direction shown by directional arrow 404 when the volume of the lumen 304 decreases. Conversely, when the volume of the lumen 304 increases, the movable seal or the movable plunger 402 moves in a direction shown by directional arrow 406. In at least some embodiments, each seal in fluid contact with the lumen 304 is provided with a vacuum seal.

[0032] In at least some embodiments, the volume of the main flush port 210 should be sufficient to allow the movable seal or the movable plunger 402 full movement for volume changes. In at least some embodiments, the movement of the movable seal or the movable plunger 402 may be restricted to a given longitudinal movement, thereby corresponding to a given volume. For example, in at least some embodiments, one or more stops may be used to limit the longitudinal movement of the movable seal or the movable plunger 402 within the main flush port 210. In Figure 4, stops 408 and 410 are shown for limiting the movement of the movable seal or the movable plunger 402 in the direction shown by the directional arrow 404. In other embodiments, additional stops may be employed instead of, or in addition to, the stops 408 and 410 to limit the movement of the movable seal or the movable plunger 402 in the direction shown by the directional arrow 406.

[0033] In at least some embodiments, air in the lumen 304 is flushed out of the output port 316 and an acoustically-favorable medium is input to the main flush port 210. Once the air is removed from the lumen 304 and the acoustically-favorable medium is input to the main flush port 210, the output port 316 may be sealed with a fixed seal. In some embodiments, the fixed seal is made permanent, for example, by fusing the output port 316 or plugging the output port 316 with a cap and applying epoxy around the edges of the cap. In other embodiments, the fixed seal is designed to be removable. In at least some embodiments, the output port 316 is sealed with a vacuum seal. In at least some embodiments, the lumen 304 is degassed, filled with the acoustically-favo-

orable medium, and the main flush port 210 and the output port 316 are sealed all in one integrated step. In at least some embodiments, the imaging core 306 may be tested for operability prior to sealing the main flush port 210 and the output port 316.

[0034] In at least some embodiments, the catheter 102 may also define one or more auxiliary ports. For example, in at least some embodiments, the catheter 102 may define one or more auxiliary flush ports. Figure 5A is a schematic longitudinal cross-sectional view of one embodiment of the hub 204. The hub 204 defines the main flush port 210 and an auxiliary flush port 502. In Figure 5A, the movable seal or the movable plunger 402 is shown disposed in the main flush port 210 and the auxiliary flush port 502 is shown open.

[0035] In at least some embodiments, the movable seal or the movable plunger 402 may be disposed in the main flush port 210 and the auxiliary flush port 210 may be used to degas or flush the air out of the lumen 304, as described above. Once the lumen 304 is degassed and filled with an acoustically-favorable medium, the auxiliary flush port 502 may be sealed with a fixed seal (either permanent or removable), as described above. In at least some embodiments, the auxiliary flush port 502 is sealed with a vacuum seal.

[0036] Figure 5B is a schematic longitudinal cross-sectional view of one embodiment of the hub 204 with the movable seal or the movable plunger 402 disposed in the main flush port 210 and a fixed seal 504 disposed in the auxiliary flush port 502. In at least some embodiments, the movable seal or the movable plunger 402 is disposed in the auxiliary flush port 502 and the fixed seal 504 is disposed in the main flush port 210. In at least some embodiments, a plurality of auxiliary flush ports are defined by the catheter 102. In at least some embodiments, the fixed seal 504 or the movable seal or the movable plunger 402 is disposed in each of the auxiliary flush ports.

[0037] In at least some embodiments, one or more auxiliary output ports are defined in the catheter 102. In at least some embodiments, the movable seal or the movable plunger 402 is disposed in the output port 316. In at least some embodiments, the movable seal or the movable plunger 402 is disposed in one or more auxiliary output ports. In at least some embodiments, the movable seal or the movable plunger 402 is disposed in a reservoir in fluid communication with one or more of the main flush port 210, the one or more of the auxiliary flush ports 502, the output port 316, or the one or more auxiliary output ports.

Claims

1. A catheter assembly for an intravascular ultrasound system, the catheter assembly comprising:

a catheter (102) having a longitudinal length, a

distal end (208), and a proximal end (206), the catheter (102) comprising

a hub (204) comprising a flush port (210), an elongate member (202) coupled to the hub and comprising a sealable lumen (304) extending along the longitudinal length of the catheter (102) from the proximal end to the distal end, and

a movable plunger (402) or a movable seal disposed in the flush port of the hub and in fluid communication with the lumen (304), the movable plunger (402) or the movable seal providing a gas-tight seal, the movable plunger (402) or the movable seal configured and arranged for adjusting to changes in volume of the lumen (304) when the lumen (304) is filled with an acoustically-favorable medium and sealed; and

an imaging core (306) configured and arranged for inserting into the sealable lumen (304) and for coupling to a control module (104).

2. The catheter assembly of claim 1, wherein the flush port is a main flush port (210) in fluid communication with the sealable lumen (304), the main flush port (210) is configured and arranged for inputting the acoustically-favorable medium to the sealable lumen (304).
3. The catheter assembly of claim 1, further including an auxiliary flush port in fluid communication with the sealable lumen (304), the auxiliary flush port configured and arranged for inputting the acoustically-favorable medium to the sealable lumen (304).
4. The catheter assembly of claim 3, wherein the auxiliary flush port is configured and arranged to receive a fixed seal.
5. The catheter assembly of claim 3, wherein the auxiliary flush port is the flush port within which the movable plunger (402) or the movable seal is disposed.
6. The catheter assembly of claim 1, wherein the catheter (102) defines an output port in fluid communication with the sealable lumen (304), the output port configured and arranged for flushing out gas from the sealable lumen (304).
7. The catheter assembly of claim 1, wherein the catheter (102) further defines at least one auxiliary output port in fluid communication with the sealable lumen (304), the at least one auxiliary output port configured and arranged for flushing out gas from the sealable lumen (304).

5

10

15

20

25

30

35

40

45

50

55

8. The catheter assembly of claim 1, wherein the movable plunger (402) or the movable seal is disposed in a reservoir in fluid communication with the sealable lumen (304).

9. The catheter assembly of claim 1, wherein the movable plunger (402) or the movable seal provides a vacuum seal.

10. The catheter assembly of claim 1, wherein the catheter (102) further comprises at least one telescoping section.

11. The catheter assembly of claim 1, wherein the imaging core (306) comprises a rotatable driveshaft having a distal end; and an imaging device mounted to the distal end of the rotatable driveshaft, the imaging device comprising at least one transducer (312) mounted to the imaging device, the at least one transducer (312) configured and arranged for transforming applied electrical pulses to acoustic pulses and also for transforming received echo pulses to electrical pulses.

12. An intravascular ultrasound imaging system comprising:

the catheter assembly of any one of claims 1 to 3 and 6; and

a control module (104) coupled to the imaging core (306), the control module comprising

a pulse generator (108) electrically coupled to the imaging core (306), the pulse generator (108) configured and arranged for providing electric pulses to the imaging core (306), and

a processor (106) electrically coupled to the imaging core (306), the processor (106) configured and arranged for processing received electrical pulses from the imaging core (306) to form at least one image.

13. The intravascular ultrasound imaging system of claim 12, wherein the catheter (102) is sealed.

14. A method for forming the catheter (102) of claim 1, the method comprising:

degassing the sealable lumen (304) of the catheter (102) with the imaging core inserted into the sealable lumen;

filling the sealable lumen (304) with an acoustically-favorable medium through at least one flush port (210); and

sealing the lumen (304) using the movable plunger (402) or the movable seal in fluid communication with the sealable lumen (304), the

movable plunger (402) configured and arranged to adjust to changes in volume of the lumen (304) to maintain the substantially degassed environment in the lumen (304).

15. The method of claim 14, wherein sealing the lumen (304) using the movable plunger (402) or the movable seal in fluid communication with the sealable lumen (304) comprises disposing the movable plunger (402) or the movable seal in a main flush port (210).

Patentansprüche

1. Katheteranordnung für ein intravaskuläres Ultraschallsystem, wobei die Katheteranordnung aufweist:

einen Katheter (102), der eine longitudinale Länge, ein distales Ende (208) und ein proximales Ende (206) aufweist, wobei der Katheter (102) aufweist:

ein Ansatzstück (204), das einen Spülport (210) aufweist,

ein längliches Element (202), das mit dem Ansatzstück gekoppelt ist und das ein abdichtbares Lumen (304) aufweist, das sich entlang der longitudinalen Länge des Katheters (102) vom proximalen Ende zum distalen Ende erstreckt, und

einen beweglichen Kolben (402) oder eine bewegliche Dichtung, die im Spülport des Ansatzstücks angeordnet ist und mit dem Lumen (304) in Fluidverbindung steht, wobei der bewegliche Kolben (402) oder die bewegliche Dichtung eine gasdichte Abdichtung bereitstellt, der bewegliche Kolben (402) oder die bewegliche Dichtung zum Anpassen an Änderungen des Volumen des Lumens (304) konfiguriert und eingerichtet ist, wenn das Lumen (304) mit einem akustisch günstigen Medium gefüllt und abgedichtet ist; und

einen Bildgebungskern (306), der zum Einsetzen in das abdichtbare Lumen (304) und zum Koppeln mit einem Steuermodul (104) konfiguriert und eingerichtet ist.

2. Katheteranordnung nach Anspruch 1, wobei der Spülport ein Hauptspülport (210) in Fluidverbindung mit dem abdichtbaren Lumen (304) ist und der Hauptspülport (210) zum Zuführen des akustisch günstigen Mediums in das abdichtbare Lumen (304) konfiguriert und eingerichtet ist.

3. Katheteranordnung nach Anspruch 1, die ferner einen Hilfsspülport in Fluidverbindung mit dem abdichtbaren Lumen (304) aufweist, wobei der Hilfsspülport zum Zuführen des akustisch günstigen Mediums in das abdichtbare Lumen (304) konfiguriert und eingerichtet ist.

4. Katheteranordnung nach Anspruch 3, wobei der Hilfsspülport konfiguriert und eingerichtet ist, eine feste Dichtung aufzunehmen.

5. Katheteranordnung nach Anspruch 3, wobei der Hilfsspülport der Spülport ist, in dem der bewegliche Kolben (402) oder die bewegliche Dichtung angeordnet ist.

6. Katheteranordnung nach Anspruch 1, wobei der Katheter (102) einen Ausgangsport in Fluidverbindung mit dem abdichtbaren Lumen (304) definiert und der Ausgangsport zum Ausspülen von Gas aus dem abdichtbaren Lumen (304) konfiguriert und eingerichtet ist.

7. Katheteranordnung nach Anspruch 1, wobei der Katheter (102) ferner mindestens einen Hilfsausgangsport in Fluidverbindung mit dem abdichtbaren Lumen (304) definiert und der mindestens einen Hilfsausgangsport zum Ausspülen von Gas aus dem abdichtbaren Lumen (304) konfiguriert und eingerichtet ist.

8. Katheteranordnung nach Anspruch 1, wobei der bewegliche Kolben (402) oder die bewegliche Dichtung in einen Reservoir in Fluidverbindung mit dem abdichtbaren Lumen (304) angeordnet ist.

9. Katheteranordnung nach Anspruch 1, wobei der bewegliche Kolben (402) oder die bewegliche Dichtung eine Vakuumdichtung bereitstellt.

10. Katheteranordnung nach Anspruch 1, wobei der Katheter (102) ferner mindestens einen Teleskopabschnitt aufweist.

11. Katheteranordnung nach Anspruch 1, wobei der Bildgebungskern (306) aufweist:

eine drehbare Antriebswelle, die ein distales Ende aufweist; und

eine Bildgebungsvorrichtung, die an dem distalen Ende der drehbaren Antriebswelle angebracht ist, wobei die Bildgebungsvorrichtung mindestens einen Transducer (312) aufweist, der an der Bildgebungsvorrichtung angebracht ist, wobei der mindestens einen Transducer (312) zum Umwandeln angelegter elektrischer Impulse in akustische Impulse und außerdem zum Umwandeln empfangener Echoimpulse in elek-

trische Impulse konfiguriert und eingerichtet ist.

12. Intravaskuläres Ultraschallbildgebungssystem, das aufweist:

die Katheteranordnung nach einem der Ansprüche 1 bis 3 und 6; und ein Steuermodul (104), das mit dem Bildgebungskern (306) gekoppelt ist, wobei das Steuermodul aufweist:

einen Impulsgenerator (108), der mit dem Bildgebungskern (306) elektrisch gekoppelt ist, wobei der Impulsgenerator (108) zum Bereitstellen von elektrischen Impulsen an den Bildgebungskern (306) konfiguriert und eingerichtet ist, und einen Prozessor (106), der mit dem Bildgebungskern (306) elektrisch gekoppelt ist, wobei der Prozessor (106) zum Verarbeiten von empfangenen elektrischen Impulsen vom Bildgebungskern (306) konfiguriert und eingerichtet ist, um mindestens ein Bild zu bilden.

13. Intravaskuläres Ultraschallbildgebungssystem nach Anspruch 12, wobei der Katheter (102) abgedichtet ist.

14. Verfahren zum Bilden des Katheters (102) nach Anspruch 1, wobei das Verfahren aufweist:

Entgasen des abdichtbaren Lumens (304) des Katheters (102), wobei der Bildgebungskern in das abdichtbare Lumen eingesetzt ist; Füllen des abdichtbaren Lumens (304) mit einem akustisch günstigen Medium durch mindestens einen Spülport (210); und Abdichten des Lumens (304) mittels des beweglichen Kolbens (402) oder der beweglichen Dichtung in Fluidverbindung mit dem abdichtbaren Lumen (304), wobei der bewegliche Kolben (402) konfiguriert und eingerichtet ist, sich Änderungen des Volumen des Lumens (304) anzupassen, um die im Wesentlichen entgaste Umgebung im Lumen (304) aufrechtzuerhalten.

15. Verfahren nach Anspruch 14, wobei das Abdichten des Lumens (304) mittels des beweglichen Kolbens (402) oder der beweglichen Dichtung in Fluidverbindung mit dem abdichtbaren Lumen (304) ein Anordnen des beweglichen Kolbens (402) oder der beweglichen Dichtung in einem Hauptspülport (210) aufweist.

Revendications

1. Dispositif de cathéter pour un système ultrasonore intravasculaire, ledit dispositif de cathéter comprenant :

un cathéter (102) ayant une longueur longitudinale, une extrémité distale (208) et une extrémité proximale (206), ledit cathéter (102) comprenant un embout (204) avec un orifice d'écoulement (210), un élément allongé (202) relié à l'embout et présentant une lumière obturable (304) s'étendant sur la longueur longitudinale du cathéter (102) de l'extrémité proximale à l'extrémité distale, et un piston mobile (402) ou un joint mobile disposé dans l'orifice d'écoulement de l'embout et en communication fluïdique avec la lumière (304), le piston mobile (402) ou le joint mobile formant un joint étanche au gaz, le piston mobile (402) ou le joint mobile étant prévu et disposé pour s'ajuster à des variations de volume de la lumière (304) quand la lumière (304) est remplie d'un milieu acoustiquement favorable et obturée ; et un noyau d'imagerie (306) prévu et disposé pour être introduit dans la lumière obturable (304) et pour être couplé à un module de commande (104).

2. Dispositif de cathéter selon la revendication 1, où l'orifice d'écoulement est un orifice d'écoulement principal (210) en communication fluïdique avec la lumière obturable (304), ledit orifice d'écoulement principal (210) étant prévu et disposé pour l'admission du milieu acoustiquement favorable dans la lumière obturable (304).

3. Dispositif de cathéter selon la revendication 1, comprenant en outre un orifice d'écoulement secondaire en communication fluïdique avec la lumière obturable (304), ledit orifice d'écoulement secondaire étant prévu et disposé pour l'admission du milieu acoustiquement favorable dans la lumière obturable (304).

4. Dispositif de cathéter selon la revendication 3, où l'orifice d'écoulement secondaire est prévu et disposé pour recevoir une obturation fixe.

5. Dispositif de cathéter selon la revendication 3, où l'orifice d'écoulement secondaire est l'orifice d'écoulement dans lequel le piston mobile (402) ou le joint mobile est disposé.

6. Dispositif de cathéter selon la revendication 1, où le cathéter (102) définit un orifice de sortie en communication fluïdique avec la lumière obturable (304), ledit orifice de sortie étant prévu et disposé pour éva-

- cuer du gaz de la lumière obturable (304).
7. Dispositif de cathéter selon la revendication 1, où le cathéter (102) définit en outre au moins un orifice de sortie secondaire en communication fluïdique avec la lumière obturable (304), ledit au moins un orifice de sortie secondaire étant prévu et disposé pour évacuer du gaz de la lumière obturable (304). 5
8. Dispositif de cathéter selon la revendication 1, où le piston mobile (402) ou le joint mobile est disposé dans un réservoir en communication fluïdique avec la lumière obturable (304). 10
9. Dispositif de cathéter selon la revendication 1, où le piston mobile (402) ou le joint mobile assure une obturation hermétique. 15
10. Dispositif de cathéter selon la revendication 1, où le cathéter (102) comprend en outre au moins une section télescopique. 20
11. Dispositif de cathéter selon la revendication 1, où le noyau d'imagerie (306) comprend un arbre d'entraînement rotatif ayant une extrémité distale ; et un dispositif d'imagerie monté à l'extrémité distale de l'arbre d'entraînement rotatif, ledit dispositif d'imagerie comprenant au moins un transducteur (312) monté sur le dispositif d'imagerie, ledit au moins un transducteur (312) étant prévu et disposé pour transformer des impulsions électriques appliquées en impulsions acoustiques et également pour transformer des impulsions d'écho reçues en impulsions électriques. 25 30
12. Système d'imagerie ultrasonore intravasculaire, comprenant : 35
- le dispositif de cathéter selon l'une des revendications 1 à 3 et 6 ; et 40
- un module de commande (104) relié au noyau d'imagerie (306), ledit module de commande comprenant un générateur d'impulsions (108) électriquement relié au noyau d'imagerie (306), ledit générateur d'impulsions (108) étant prévu et disposé pour délivrer des impulsions électriques vers le noyau d'imagerie (306), et 45
- un processeur (106) électriquement relié au noyau d'imagerie (306), ledit processeur (106) étant prévu et disposé pour traiter des impulsions électriques reçues du noyau d'imagerie (306) pour former au moins une image. 50
13. Système d'imagerie ultrasonore intravasculaire selon la revendication 12, où le cathéter (102) est obturé. 55
14. Procédé de formation du cathéter (102) selon la re-

vendication 1, ledit procédé comprenant :

- le dégazage de la lumière obturable (304) du cathéter (102) par le noyau d'imagerie introduit dans la lumière obturable ;
- le remplissage de la lumière obturable (304) avec un milieu acoustiquement favorable par au moins un orifice d'écoulement (210) ; et
- l'obturation de la lumière (304) au moyen du piston mobile (402) ou du joint mobile en communication fluïdique avec la lumière obturable (304), le piston mobile (402) étant prévu et disposé pour s'ajuster aux variations de volume de la lumière (304) afin de maintenir l'environnement sensiblement dégazé dans la lumière (304).
15. Procédé selon la revendication 14, où l'obturation de la lumière (304) au moyen du piston mobile (402) ou du joint mobile en communication fluïdique avec la lumière obturable (304) comprend la disposition du piston mobile (402) ou du joint mobile dans un orifice d'écoulement principal (210).

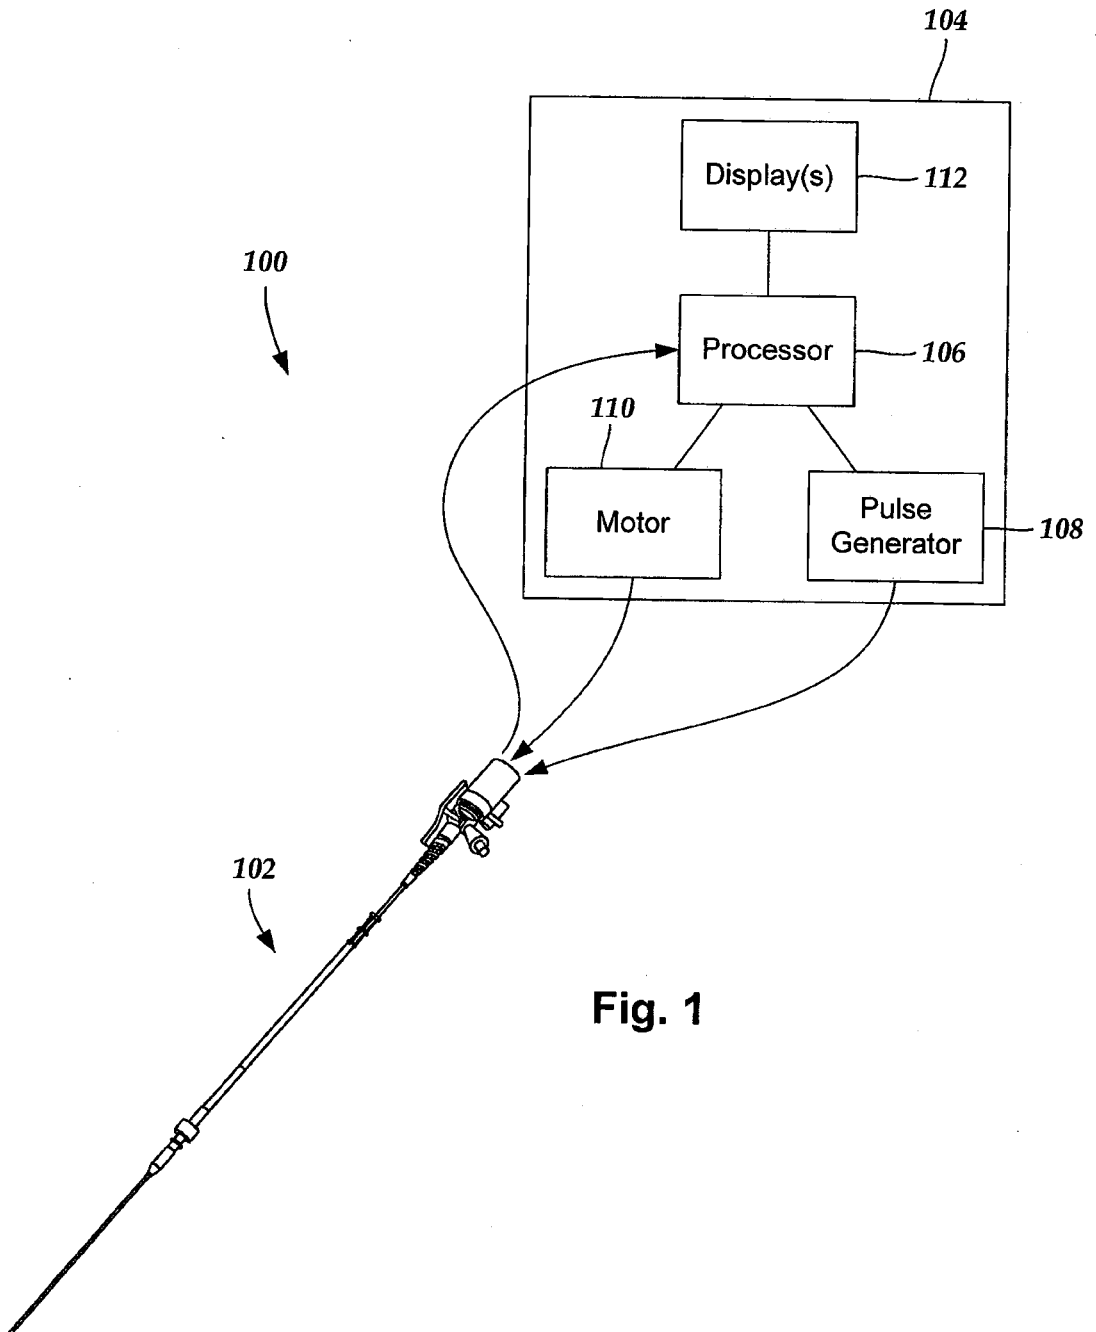


Fig. 1

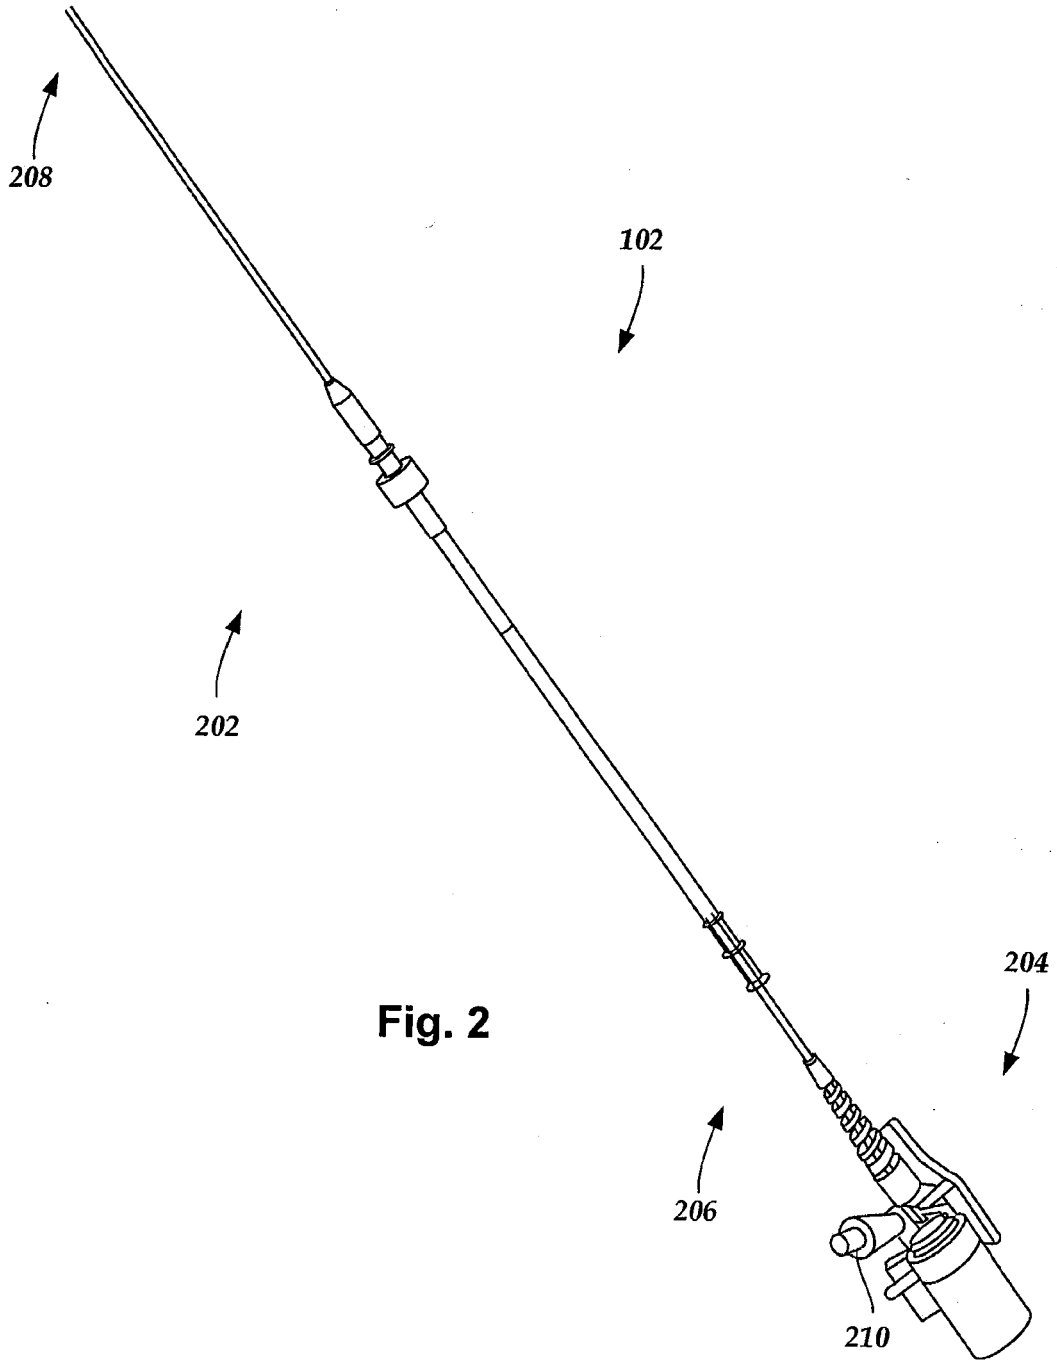


Fig. 2

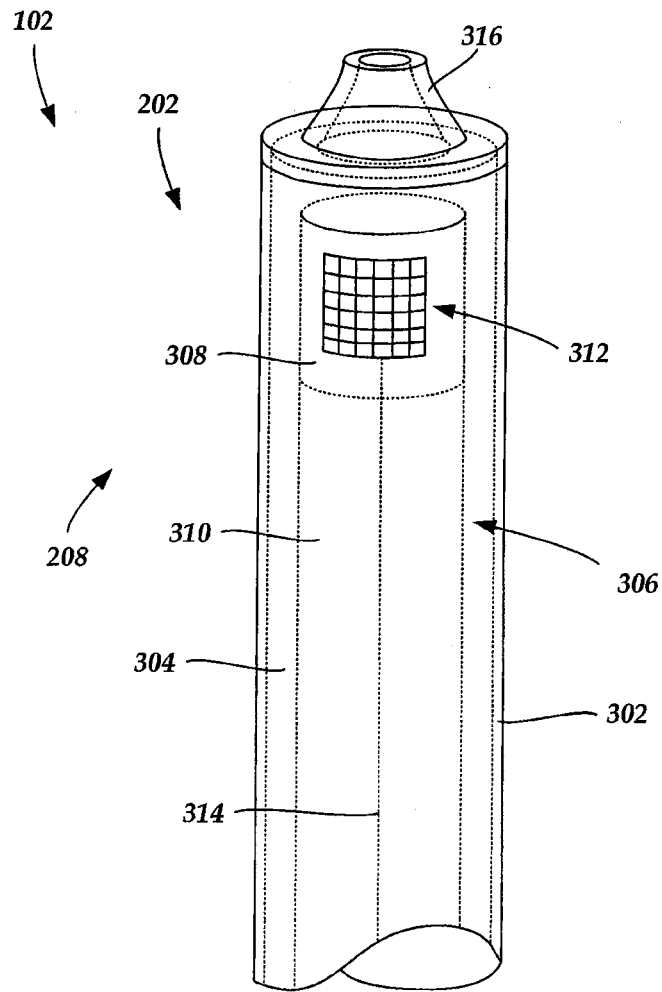


Fig. 3

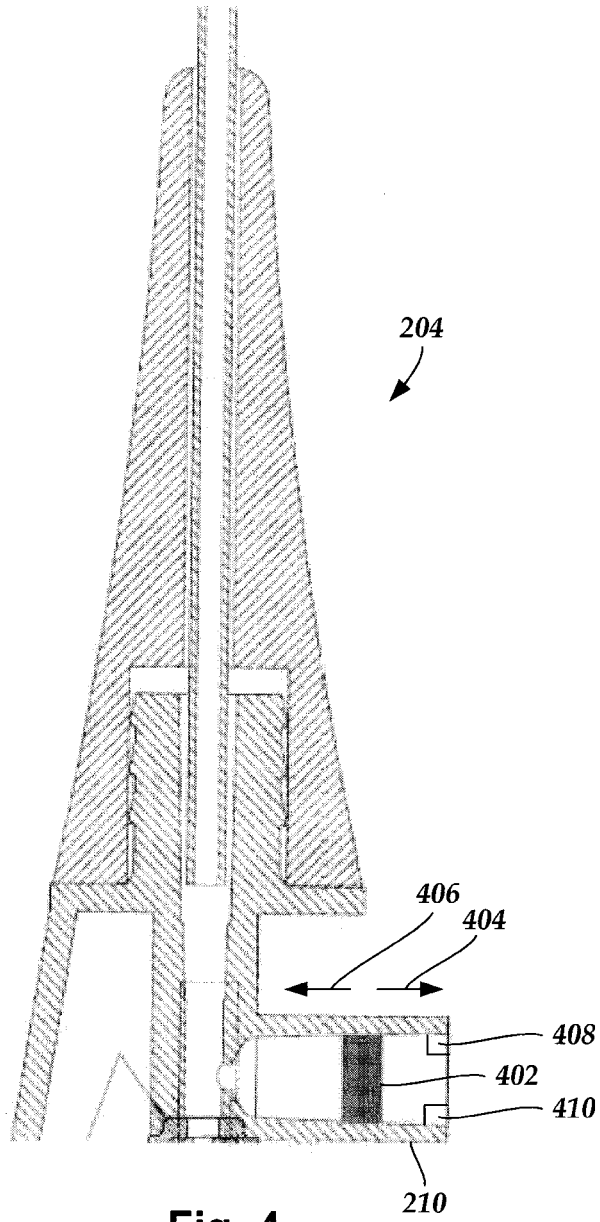


Fig. 4

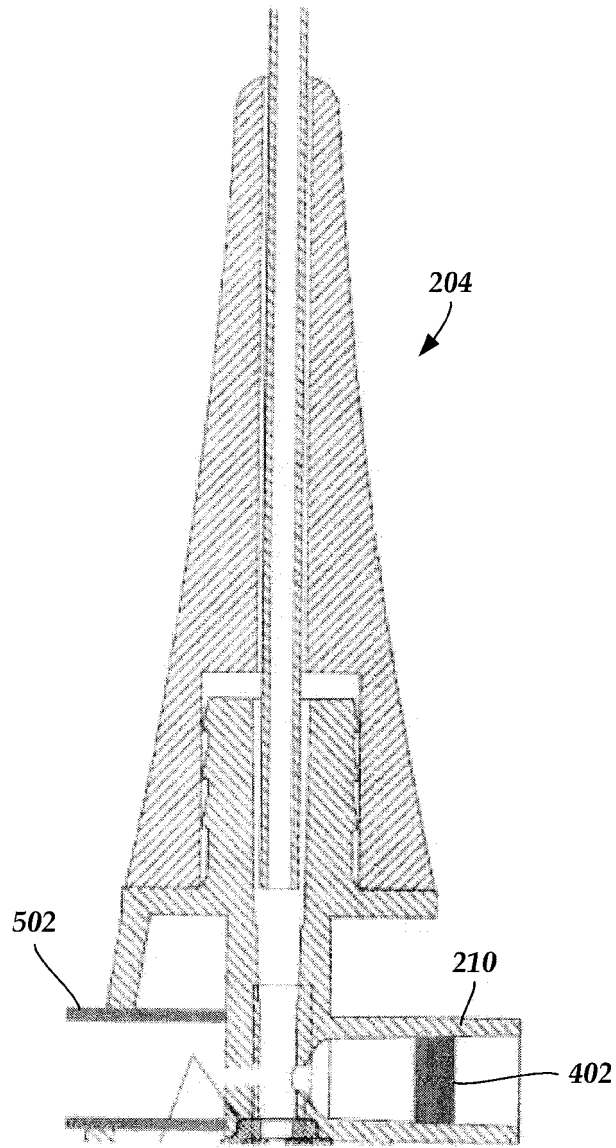


Fig. 5A

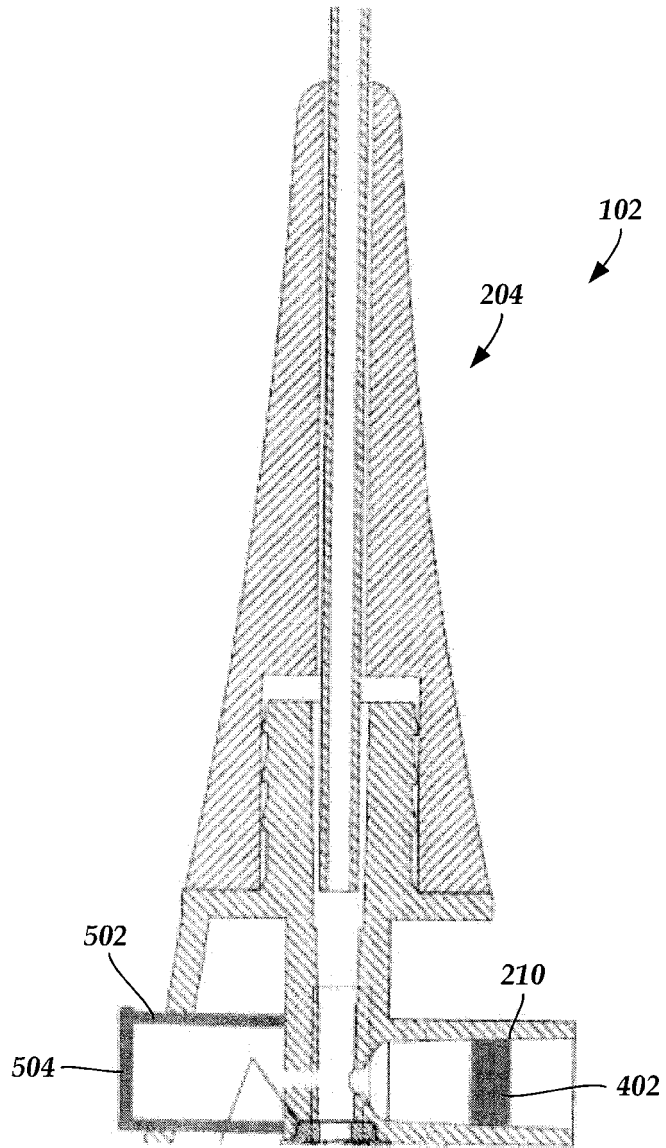


Fig. 5B

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 61045904 A [0001]
- US 5331947 A [0003]
- US 7306561 B [0011]
- US 6945938 B [0011]
- US 20060253028 A [0011]
- US 20070016054 A [0011]
- US 20070038111 A [0011]
- US 20060173350 A [0011]
- US 20060100522 A [0011]

专利名称(译)	具有填充有声学有利介质的密封导管的血管内超声成像系统以及制造和使用的方法		
公开(公告)号	EP2276409A1	公开(公告)日	2011-01-26
申请号	EP2009732222	申请日	2009-04-17
[标]申请(专利权)人(译)	波士顿科学西美德公司		
申请(专利权)人(译)	BOSTON SCIENTIFIC SCIMED , INC.		
当前申请(专利权)人(译)	BOSTON SCIENTIFIC SCIMED , INC.		
[标]发明人	SADAKA ALAIN		
发明人	SADAKA, ALAIN		
IPC分类号	A61B8/12		
CPC分类号	A61B8/0833 A61B8/12 A61B8/4281 A61B8/445		
优先权	61/045904 2008-04-17 US		
其他公开文献	EP2276409B1		
外部链接	Espacenet		

摘要(译)

用于血管内超声系统的导管组件包括导管和成像核心。导管具有纵向长度，远端和近端。导管包括沿着导管的纵向长度从近端延伸到远端的可密封内腔，以及与内腔流体连通的可移动柱塞或可移动密封件。可移动柱塞或可移动密封件提供气密密封。可移动柱塞或可移动密封件被配置和布置成当内腔填充声学上有利的介质并密封时调节内腔体积的变化。成像芯被配置和布置成用于插入可密封的内腔中并且用于耦合到控制模块。