

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
24 July 2003 (24.07.2003)

PCT

(10) International Publication Number
WO 03/060553 A2

(51) International Patent Classification⁷: **G01S 15/89**, (74) Agent: **LOTTIN, Claudine**; Internationaal Octrooibureau B.V., Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(21) International Application Number: PCT/IB02/05356

(22) International Filing Date:
11 December 2002 (11.12.2002)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
01403392.2 28 December 2001 (28.12.2001) EP

(71) Applicant (for all designated States except US): **KONINKLIJKE PHILIPS ELECTRONICS N.V.** [NL/NL]; Groenewoudseweg 1, NL-5621 BA Eindhoven (NL).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **JACOB, Marie** [FR/NL]; Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **GERARD, Olivier** [FR/NL]; Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL). **COLLER-BILLON, Antoine** [FR/NL]; Prof. Holstlaan 6, NL-5656 AA Eindhoven (NL).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with declaration under Article 17(2)(a); without abstract; title not checked by the International Searching Authority

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

WO 03/060553 A2

(54) Title: VIEWING SYSTEM HAVING MEANS FOR PROCESSING A SEQUENCE OF ULTRASOUND IMAGES FOR PERFORMING A QUANTITATIVE ESTIMATION OF A FLOW IN A BODY ORGAN

(57) Abstract:

Viewing system having means for processing a sequence of ultrasound images for performing a quantitative estimation of a flow in a body organ

FIELD OF THE INVENTION

The invention relates to a viewing system having means for processing a sequence of three-dimensional (3-D) ultrasound images for performing a quantitative estimation of a flow in a body organ. In particular, the invention relates to a medical viewing system and to an image processing method for performing an automatic quantitative estimation of the blood flow through the heart valves, and/or of the regurgitant jet, from a sequence of 3-D color flow images.

The invention particularly finds an application in the field of medical imaging in cardiology using ultrasound medical apparatus and/or viewing systems.

10

BACKGROUND OF THE INVENTION

A method for assessing mitral regurgitation is already known from the publication entitled "Hemieliptic Proximal Isovoltage Surface Area Method Modified for Clinical Application, More Accurate Quantification of Mitral Regurgitation In Doppler Echocardiography" by HIROKO FUJI *et al.*", in Japanese Circulation Journal, Vol. 65, September 2001, pages 820-826. According to this publication, the Proximal Isovoltage Surface Area (PISA) method is used for quantitative estimation of the mitral jet regurgitation. The PISA shape is chosen hemieliptic rather than hemispheric on a slit-like orifice, because the hemieliptic method is more accurate than the hemispheric method for in vitro studies. Nevertheless, the hemispheric method is used clinically because of its simplicity, whereas the hemieliptic method is difficult to approach from 3 orthogonal directions. The publication in reference presents a modified approach for use in clinical applications. A closed circuit, constant flow system was designed to simulate PISA, and various types of slit-like orifices were selected. Three orthogonal PISA radii were measured and flow rates were calculated using the original hemieliptic formula using the three orthogonal PISA radii. Flow rates were also calculated indirectly using a linear regression formula, and PISA radii from a bird's eye approach and lateral approaches (modified hemieliptic method) were compared. Flow rates that were determined using the original hemieliptic method correlated significantly with actual flow rates. Similarly, flow rates calculated using the modified hemieliptic method

correlated significantly with actual flow rates. So, the study results imply that the proposed modified hemielliptic method could be used in clinical applications.

SUMMARY OF THE INVENTION

5 The quantitative estimation of the blood flow through the heart valves, from 3D color flow image sequences, has important clinical implications for the assessment of the condition of the valves. The estimation of the importance of the regurgitant jet is an index of the severity of the valve diseases, such as the congenital malformation or the valvular insufficiency, or the lack of attachment of the chordal structures. The presence of a normal 10 regurgitation is also very often to be found in non-pathologic patients. This normal regurgitation is used to estimate the pressure in the cavities, for instance in the case of patients suffering from hypertension. Also, the study of the flow through the valve helps the diagnosis in case of a stenosis of the cardiac valves. The intracardiac blood flow is also studied in the follow-up of valve transplants comprising estimation of the residual 15 regurgitation, detection and quantification of the para-prosthetic leaks that can cause the disinsertion of the prosthesis.

Recent years have seen the introduction of a high quality imaging modality which uses the Doppler shift for the study of blood flow and tissue motion. 2-D color Doppler ultrasound technology has now reached a level of maturity. Combined with gray 20 level exam, this is the most widely used technique for assessing valve diseases. Several methods based on this 2-D image processing technique are known for estimating the severity of the regurgitation. These methods are based on measurements on the cross-sectional jet that can be the length of the jet, or its area. However, these measurements, even though they are based on the maximal demonstrable regurgitant jet, tend to underestimate the extent of the 25 jet. Scanning multiple planes only reduces this underestimation. These measurements can also vary considerably over consecutive repeated measurements, because they depend on the choice of the image plane. Moreover, the regurgitant jet can be eccentric or asymmetric, and can reverberate against the heart walls, which is the case in most severe mitral regurgitations for instance, and which does not permit of assessing the actual mitral regurgitation correctly. 30 Hence, on the one hand, the known 2-D measurements do not permit of quantifying said mitral regurgitation accurately. That is why the emergent 3-D color Doppler technique, based on the 3-D reconstruction of the color flow, is considered as the future reference method for assessing valve diseases severity. However, on the other hand, the publication by HIROKO FUJI *et alii*, in reference, which is based on geometrical assumption limited to a very strict

hemielliptic shape of the isovelocity surface of the 3D color flow of the blood issuing the mitral valve, does not permit of reaching sufficiently accurate results. This shows the need for more accurate tools to automatically quantify the severity of the regurgitation in 3-D color Doppler images.

5 The invention has for an object to provide a viewing system associated to an ultrasound examination apparatus and an image processing method for performing an automatic quantitative estimation of a flow through a body organ, from a sequence of three-dimensional (3-D) ultrasound color flow images. According to the invention, a 3-D ultrasound technique is used for acquiring a sequence of 3-D color flow images of a flow 10 through an orifice, for instance using a 3-D color Doppler technique, within an interval of time. Then, a map of isovelocity surfaces is constructed by velocity segmentation related to the blood flow at the vicinity of said orifice, issuing through the orifice, which permits of estimating both the blood velocity at a given surface and the actual volume delimited by said isovelocity surface. The peak velocity of the regurgitant jet of blood through the orifice, in 15 the opposite direction, is also measured using a pulse wave Doppler technique. These measured data permit of calculating the surface of the orifice. In particular, for estimating the severity of the mitral regurgitation through the heart valve, the Surface Of Regurgitation (SOR) can be obtained by calculations based on the real volume corresponding to the real PISA.

20 Such a viewing system is claimed in Claim 1. Particular embodiments of the viewing system, an examination apparatus associated to the viewing system and an image processing method to be carried out in the system, are claimed in dependent Claims.

BRIEF DESCRIPTION OF THE DRAWINGS

25 The invention is described hereafter in detail in reference to the following diagrammatic drawings, wherein:

FIG. 1 is a flow chart of the functions performed by the viewing system;

FIG. 2 shows a schematic drawing of the left atrium and left ventricle with a valve;

30 FIG. 3 illustrates the determination of the Surface Of Regurgitation " S.O.R";

FIG. 4 shows a diagram of an ultrasound examination apparatus having a viewing system.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

The invention relates to a viewing system for performing a quantitative estimation of a flow in a body organ. In particular, the invention relates to a medical viewing system and to an image processing method for performing an automatic quantitative estimation of the blood flow through the heart valves, and/or of the regurgitant jet, from a sequence of 3-D color flow images.

5 The method can be carried out using reconstructed or real-time 3D echocardiography, the images being formed using a trans-thoracic or a trans-esophageal probe. The method of the invention can also be applied to a sequence of 3-D images of other 10 organs of the body that can be formed by ultrasound systems or ultrasound apparatus, or by other medical imaging systems known of those skilled in the art.

15 In the example described hereafter, severity of the cardiac regurgitant jet between the left heart atrium and the left heart ventricle is assessed from a sequence of 3-D Doppler color flow images.

20 Referring to FIG.1, the ultrasound examination apparatus yields ultrasound data to the viewing system. In a step S1, the viewing system acquires a sequence of 3D ultrasound images of the heart atrium, the heart left ventricle and the mitral valve, which is located between the left atrium and the left ventricle, during an interval of time, for instance between two heart pulses. The sequence images can be acquired at a rate of 15 to 30 or 50 25 images per second, each image of the sequence being preferably associated to an instant of the cardiac cycle. Other examples of forming sequences of 3-D images of different organs may be found by operators of ultrasound apparatus or of other systems of image acquisition.

30 In a step S2, the viewing system acquires a sequence of 3D Doppler color flow velocity images of the blood flow normally issuing from the heart atrium, and entering the heart left ventricle through the mitral valve. Referring to FIG.3, when a disease of the heart does not permit the mitral valve to completely close at given heart pulse instants, then a regurgitant jet retropropagates from a small remaining orifice 3 let by the mitral valve 5 toward the atrium, in the opposite direction with respect to the normal direction of blood flow. The invention has for an object to provide a quantitative measure relative to the severity of the regurgitant jet.

In a step S3, the viewing system has segmentation means to construct 3D isovelocity surfaces from the Doppler color flow images. In case of normal functioning of the heart, each of these surfaces yields the blood velocity value in the normal direction of the blood flow, *i. e.* in the conventional blood direction from the left atrium LA to the left

ventricle LV. It is to be noted that, due to the existence of a remaining orifice 3 of the mitral valve 5, isovelocity surfaces that are inside the left ventricle LV, near said remaining orifice of mitral valve 5, concern the velocity of the blood flow that leaves the left ventricle opposite to the conventional blood direction, through said remaining orifice, and that contributes to 5 form the regurgitant jet. These isovelocity surfaces concern the velocity of an upstream flow with respect to said remaining orifice of the mitral valve that permits the existence of the regurgitant jet and with respect to the flow of said regurgitant jet. These isovelocity surfaces 6 of said upstream flow are constructed and shown in FIG.3.

Several different possible technique of segmentation may be used for 10 constructing said color flow isovelocity surfaces 6. The segmentation techniques allow to obtain surface models that are extremely near to the actual isovelocity surfaces and are not an approximation of the surfaces or an assumed geometrical shape of the surfaces, as was proposed by the state of the art. Since the isovelocity surfaces are not smooth, they cannot be estimated correctly by any assumed geometrical shape, because the assumed surface 15 constitutes a too rough approximation. The segmentation technique is applied on the Doppler blood color flow data provided by step S2.

A first segmentation technique is already disclosed by H. Delingette in the publication entitled "Simplex Meshes: a General Representation for 3D shape Reconstruction" published in the "Proceedings of the International Conference on Computer 20 Vision and Pattern Recognition (CVPR'94), 20-24 June 1994, Seattle, USA". In this paper, a physically based approach for recovering three-dimensional objects is presented. This approach is based on the geometry of "Simplex Meshes". Elastic behavior of the meshes is modeled by local stabilizing functions controlling the mean curvature through the simplex angle extracted at each vertex (node of the mesh). Those functions are viewpoint-invariant, 25 intrinsic and scale-sensitive. Unlike distortable surfaces defined on regular grids, Simplex Meshes are very adaptive structures. A refinement process for increasing the mesh resolution at highly curved or inaccurate parts is also disclosed. Operations for connecting Simplex Meshes in order to recover complex models may be performed using parts having simpler shapes. A Simplex Mesh has constant vertex connectivity. For representing 3-D surfaces, 2-D 30 Simplex Meshes, where each vertex is connected to three neighboring vertices, are used. The structure of a Simplex Mesh is dual to the structure of a triangulation as illustrated by the FIG.1 of the cited publication. It can represent all types of rotatable surface. The contour on a Simplex Mesh is defined as a closed polygonal chain consisting in neighboring vertices on the Simplex Mesh. The contour is restricted to not intersect itself. Contours are distortable

models and are handled independently of the Simplex Mesh where they are embedded. Four independent transformations are defined for achieving the whole range of possible mesh transformations. They consist in inserting or in deleting edges in a face. The description of the Simplex Mesh also comprises the definition of a Simplex Angle that generalized the 5 angle used in planar geometry; and the definition of metric parameters that describe how the vertex is located with respect to its three neighbors. The dynamic of each vertex is given by a Newtonian law of motion. The deformation implies a force that constrains the shape to be smooth and a force that constrains the mesh to be close to the 3-D data-Internal forces determine the response of a physically based model to external constraints. The internal 10 forces are expressed so that they be intrinsic viewpoint invariant and scale dependant. Similar types of constraints hold for contours. Hence, the cited publication provides a simple model for representing a 3-D object of interest. It defines the forces to be applied in order to reshape and adjust the model onto the 3-D object of interest. The "Simplex Mesh technique" is a robust segmentation technique.

15 A second possible segmentation technique is already disclosed in a publication entitled "A fast marching level set method for monotonically advancing fronts" by J. A. SETHIAN in Proc. Nat. Acad. Sci., USA, Vol. 93, pp. 1591-1595, February 1996, Applied Mathematics. According to said reference, a front, formed in a 2-D grid of potential values, is propagated using a "Fast Marching Technique" with a determination of the front points. The 20 front is a solution of a so-called Eikonal Equation. The Fast Marching Technique introduces order in the selection of the grid points and sweeps the front ahead in one pass on the 2-D image. The Fast Marching Technique comprises marching the Front outwards by freezing already visited points denoted Alive, coming from a set of points referred to as Narrow Band, and by bringing new ones denoted Far Away into said Narrow Band. The Narrow Band grid 25 points are always up-dated as those having minimal potential values in a neighboring structure denoted Min-Heap and the potential of the neighbors are further re-adjusted. Said Fast Marching technique provides one path of minimal cost joining a first end point called **Start Point** to respectively each point of the front, said front propagating until a second and final end point, called **End Point** is reached. It is interesting to note that the points of a path 30 constructed in the operation of marching the front forwards are points, which have the smallest possible potentials. Starting at the Start Point, and going forwards from one point to the next point must be at the "minimal cost". So, such a path is a path of "minimal Action", i. e. a path on which the "Sum" or the "Integral" of potentials calculated over point potentials is the smallest though strictly continuously growing as a function of the number of points

present on said path between the Start Point and the current point on the front. This Front Propagation Technique thus needs **two End-Points** between which it propagates the Front onwards and backwards. Referring to FIG.3, according to the invention, the Start Point for propagating the front is set in the substantially middle of the orifice 3. The front has two End 5 values, which are:

The value of the velocity **V** of the chosen isovelocity surface 6 of the upstream flow related to the regurgitant flow, with respect to the remaining orifice in the mitral valve 5; and

10 The value of a velocity substantially near **ZERO**, which is the velocity at the vicinity of the mitral valve 5 itself.

The system has means to provide in step S4, accurate values of the velocity **V** at the surface of a given isovelocity surface model together with the actual volume, denoted by **Vol**, delimited by the considered isovelocity surface 6. This values **V** and **Vol** are calculated from the images of the Doppler color simplified models of the Doppler color flow 15 isovelocity surfaces of said upstream flow, which are obtained from the segmentation of 3-D ultrasound Doppler color blood flow of the heart at the vicinity of the mitral valve of the heart as described for carrying out said previous step S4.

20 The system has means to perform a step S6, wherein the peak velocity of the regurgitant jet, denoted by **V_{REG}**, which is in the same direction as the velocity **V** of the isovelocity surface 6 of said upstream flow, is measured using a known technique of pulse wave Doppler.

25 Now the system has calculation means to perform a step S7 of calculating the surface, denoted by Surface Of the Regurgitant jet “**S.O.R**”, of said remaining orifice 3 of the mitral valve 5 through which the regurgitant jet is emitted. This surface is calculated through the following formula:

$$\text{SOR} = \text{Vol} \times \text{V} / \text{V}_{\text{REG}}$$

This formula yields the surface value “**S.O.R**” with the minimum of approximation since the evaluation of the volume by surface segmentation is as near as possible of the actual volume.

30 The above-described method can be applied to any estimation of a surface of an orifice through which a flow of a fluid is emitted and propagates. The direction of the flow may be the conventional direction, or opposite to the normal direction usually found for the flow of said fluid.

The above-described method can be applied without difficulty to 2-D images, which are for instance cross-sections of the 3-D images of a 3-D object. In the case of the

simplex mesh segmentation method, the 2-D segmented objects of the sequence are polygons. For a 3-D sequence of images, one might provide three orthogonal cross-section image sequences. When other segmentation methods are used, the 2-D images represent the trace of the wall of the segmented 3-D object.

5 The 3D or the 2D methods may be applied to ultrasound images as well as to X-ray images or to any other kind of image sequences.

Referring to FIG.4, a medical examination apparatus 150 comprises means for acquiring a digital image sequence, and a viewing system 120 for processing these data according to the processing steps above-described. The medical examination apparatus 10 comprises means for providing image data to the viewing system 120, which has at least one output 106 to provide image data to display and/or storage means 130, 140. The display and storage means may respectively be the screen 140 and the memory 130 of a workstation 110. Said storage means may be alternately external storage means. This image viewing system 120 may comprise a suitably programmed computer of the workstation 110, or a special 15 purpose processor having circuit means such as LUTs, Memories, Filters, Logic Operators, that are arranged to perform the functions of the method steps according to the invention. The workstation 110 may also comprise a keyboard 131 and a mouse 132. This medical examination apparatus 150 may be a standard ultrasonic apparatus. The viewing system 120 may use a computer program product having program instructions to be executed by the 20 computing means of said processing system.

CLAIMS:

1. A medical ultrasound viewing system for processing a sequence of three-dimensional (3-D) ultrasound images for performing a quantitative estimation of a flow in a body organ comprising means for performing steps of:

acquiring a sequence of 3D color flow images, of a flow in a body organ;

5 assessing the flow velocity values (V) in the 3D images,

constructing isovelocity surfaces (6) by segmentation of the flow velocity values;

computing the volume (Vol) delimited by the isovelocity surfaces (6);

and using the flow velocity value and the volume computed from a segmented surface, for 10 computing the surface of an orifice (SOR) of the organ through which the flow propagates.

2. The medical ultrasound viewing system of Claim 1, wherein the system has means for performing steps of measuring the peak velocity of a flow through the orifice (3) in the direction of said flow; and computing the surface of said orifice (SOR) through which the 15 flow propagates as a function of:

the flow velocity value (V) at an isovelocity surface (6) upstream said flow propagation with respect to said orifice (3),

the volume (Vol) computed from said segmented isovelocity surface, and

the peak velocity of the flow through the orifice (3) in the direction of the flow

20 propagation.

3. The system of Claim 2, wherein the technique of segmentation is an active mesh model technique.

25 4. The system of Claim 2, wherein the technique of segmentation is a front propagation technique, whose starting values and stopping values are the velocities at the isovelocity surface.

5. The system of one of Claims 2 to 4, wherein the formula for providing the surface of said orifice S.O.R through which the flow propagates is of the form:

$$\mathbf{SOR} = \mathbf{Vol} \times \mathbf{V} / \mathbf{V}_{\mathbf{REG}}$$

5 6. The system of Claim 5, wherein the 3D ultrasound images are acquired from the heart atrium, the heart left ventricle and the mitral valve, using blood flow color 3D imaging for assessing the mitral regurgitation, and the surface that is assessed is the surface of regurgitation of the mitral valve (SOR).

10 7. An ultrasound examination apparatus having means to acquire medical image data, having a system as claimed in one of Claims 1 to 6, having access to said medical digital image data, and processing the image data, and having means to display the processed images.

15 8. A computer program product comprising a set of instructions for carrying out the steps as claimed in one of Claims 1 to 6.

1/2

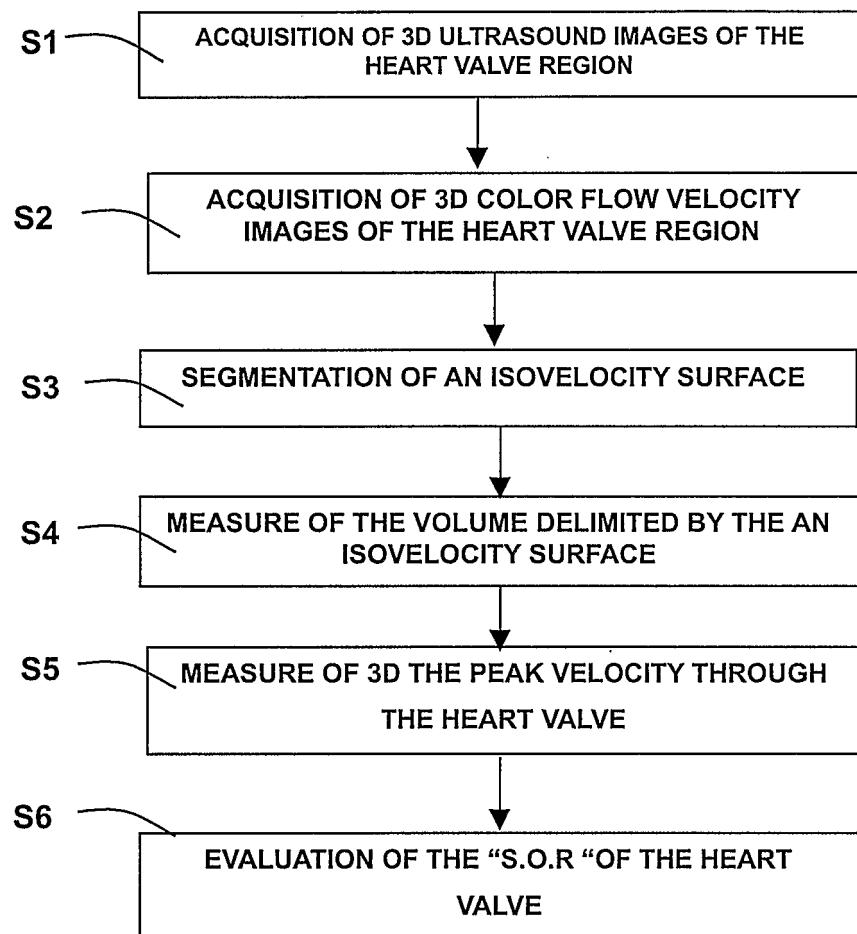


FIG.1

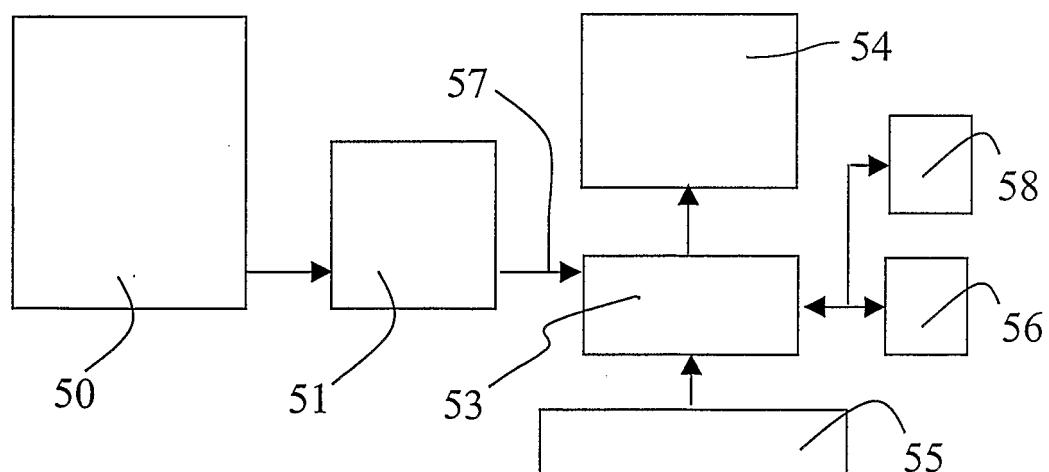


FIG.4

2/2

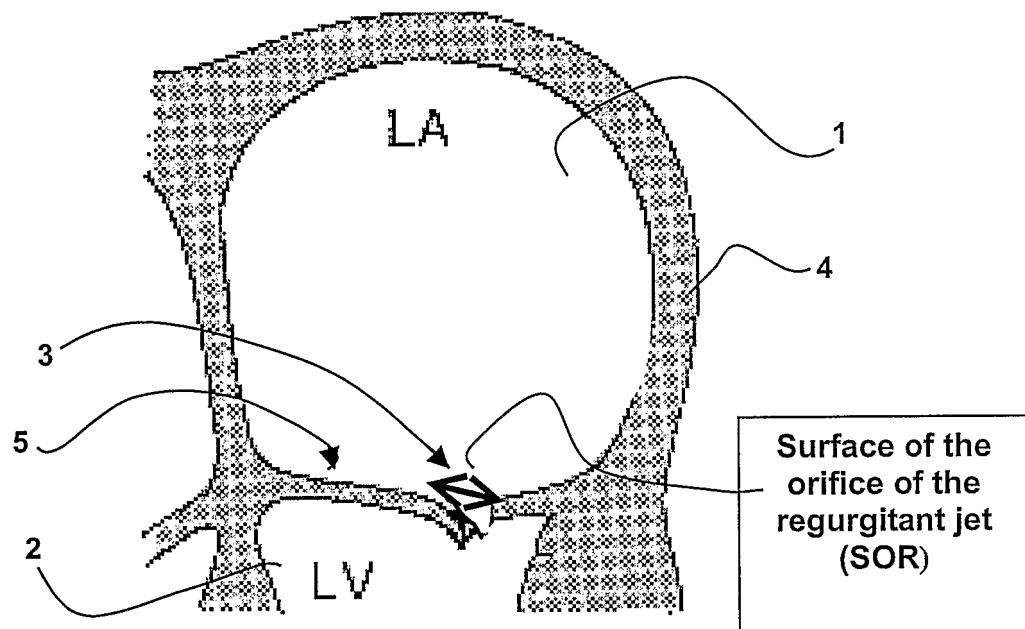


FIG.2

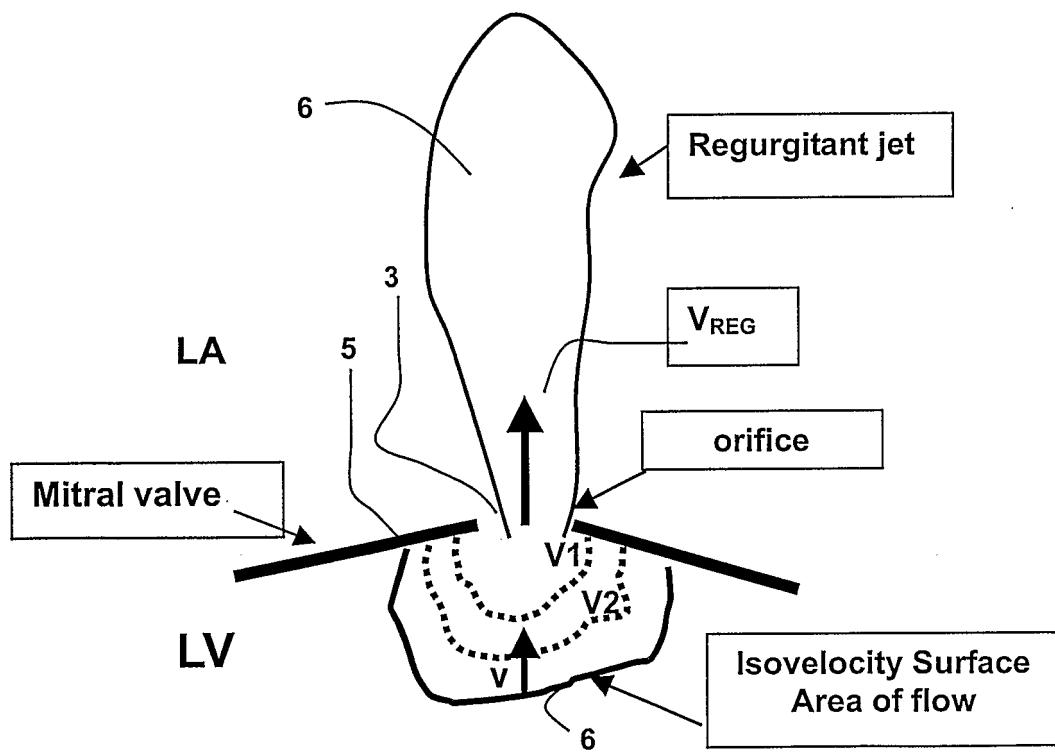


FIG.3

PCT

DECLARATION OF NON-ESTABLISHMENT OF INTERNATIONAL SEARCH REPORT

(PCT Article 17(2)(a), Rules 13ter.1(c) and Rule 39)

Applicant's or agent's file reference PHFR010197W0	IMPORTANT DECLARATION		Date of mailing(<i>day/month/year</i>) 02/07/2003
International application No. PCT/ IB 02/ 05356	International filing date(<i>day/month/year</i>) 11/12/2002	(Earliest) Priority date(<i>day/month/year</i>) 28/12/2001	
International Patent Classification (IPC) or both national classification and IPC		G01S15/89, A61B8/06	
Applicant KONINKLIJKE PHILIPS ELECTRONICS N.V.			

This International Searching Authority hereby declares, according to Article 17(2)(a), that **no international search report will be established** on the international application for the reasons indicated below

1. The subject matter of the international application relates to:
 - a. scientific theories.
 - b. mathematical theories
 - c. plant varieties.
 - d. animal varieties.
 - e. essentially biological processes for the production of plants and animals, other than microbiological processes and the products of such processes.
 - f. schemes, rules or methods of doing business.
 - g. schemes, rules or methods of performing purely mental acts.
 - h. schemes, rules or methods of playing games.
 - i. methods for treatment of the human body by surgery or therapy.
 - j. methods for treatment of the animal body by surgery or therapy.
 - k. diagnostic methods practised on the human or animal body.
 - l. mere presentations of information.
 - m. computer programs for which this International Searching Authority is not equipped to search prior art.
2. The failure of the following parts of the international application to comply with prescribed requirements prevents a meaningful search from being carried out:

the description the claims the drawings
3. The failure of the nucleotide and/or amino acid sequence listing to comply with the standard provided for in Annex C of the Administrative Instructions prevents a meaningful search from being carried out:

the written form has not been furnished or does not comply with the standard.

 the computer readable form has not been furnished or does not comply with the standard.
4. Further comments:

Name and mailing address of the International Searching Authority  European Patent Office, P.B. 5818 Patentlaan 2 NL-2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3016	Authorized officer Lucia Ertl
---	---

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 203

The present application relates to a medical ultrasound system comprising means for computing the surface (SOR) of an orifice of a human organ through which a flow propagates. According to the description (see page 7, lines 11-28), the calculation of the surface (SOR) is performed through the formula: $SOR = Vol \times (V/V_{reg})$, where Vol is the volume delimited by an isovelocity surface, V is the flow velocity at said isovelocity surface and V_{reg} is the peak velocity of the flow through the orifice. However, this equation is incorrect, because the right part has volume units and does not equal a surface. Therefore, the present application does not disclose the invention in a manner sufficiently clear and complete for the invention to be carried out by a person skilled in the art contrary to the requirements of Article 5 PCT. Consequently, no search can be carried out for the present application.

The applicant's attention is drawn to the fact that claims relating to inventions in respect of which no international search report has been established need not be the subject of an international preliminary examination (Rule 66.1(e) PCT). The applicant is advised that the EPO policy when acting as an International Preliminary Examining Authority is normally not to carry out a preliminary examination on matter which has not been searched. This is the case irrespective of whether or not the claims are amended following receipt of the search report or during any Chapter II procedure. If the application proceeds into the regional phase before the EPO, the applicant is reminded that a search may be carried out during examination before the EPO (see EPO Guideline C-VI, 8.5), should the problems which led to the Article 17(2) declaration be overcome.

专利名称(译)	观察系统具有用于处理超声图像序列的装置，用于执行对身体器官中的流动的定量估计		
公开(公告)号	EP1481261A1	公开(公告)日	2004-12-01
申请号	EP2002788346	申请日	2002-12-11
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦电子N.V.		
[标]发明人	JACOB MARIE GERARD OLIVIER COLLER BILLON ANTOINE		
发明人	JACOB, MARIE GERARD, OLIVIER COLLER-BILLON, ANTOINE		
IPC分类号	A61B8/06 A61B8/12 G01S15/89		
CPC分类号	A61B8/06 A61B8/0883 G01S15/8979 G01S15/8993		
代理机构(译)	LOTTIN , CLAUDINE		
优先权	2001403392 2001-12-28 EP		
外部链接	Espacenet		

摘要(译)

一种用于处理一系列三维 (3-D) 超声图像的医学超声观察系统，其远程执行通过身体器官的流量的定量估计，包括用于执行获取所述流的3D彩色血流图像序列的步骤的装置;评估三维图像中的流速值，通过分割流速值构建等速面 (6) ;计算由等速表面界定的体积 (Vol) ;并且使用从分段表面计算的流速值 (V) 和体积 (Vol) 来计算流动传播的器官的孔口 (3) 的表面。观察系统还包括用于执行测量通过所述孔的所述流的峰值速度 (V REG) 的步骤的装置。计算流量表面 (SOR) ，流量通过该流量传播，作为相对于所述孔口的流动传播上游的等速表面处的流速值 (V) 的函数，从所述分段的等速表面计算的体积 (Vol) ，以及通过所述孔口的流动的峰值速度。表面由下式给出：SOR = Vol。 V / V REG 。该系统可用于评估二尖瓣射流的反流表面。