



(11) EP 1 543 775 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
27.04.2011 Bulletin 2011/17

(21) Application number: **03798403.6**(22) Date of filing: **12.09.2003**

(51) Int Cl.:
A61B 8/12 (2006.01)

(86) International application number:
PCT/JP2003/011692

(87) International publication number:
WO 2004/028373 (08.04.2004 Gazette 2004/15)

(54) **ULTRASONIC DIAGNOSING SYSTEM**

ULTRASCHALLDIAGNOSESYSTEM

SYSTEME DE DIAGNOSTIC ULTRASONORE

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT RO SE SI SK TR**

(30) Priority: **27.09.2002 JP 2002283804**

(43) Date of publication of application:
22.06.2005 Bulletin 2005/25

(73) Proprietor: **Olympus Corporation
Tokyo 151-0072 (JP)**

(72) Inventor: **KAWASHIMA, Tomonao
Hachioji-shi, Tokyo 192-0045 (JP)**

(74) Representative: **von Hellfeld, Axel
Wuesthoff & Wuesthoff
Patent- und Rechtsanwälte
Schweigerstrasse 2
81541 München (DE)**

(56) References cited:

JP-A- 11 113 913	JP-A- 11 318 904
JP-A- 2000 023 980	JP-A- 2001 017 430
JP-A- 2002 143 167	JP-A- 2002 159 472
US-B1- 6 248 074	

- **PRAGER R W ET AL: "Stradx: real-time acquisition and visualization of freehand three-dimensional ultrasound" MEDICAL IMAGE ANALYSIS, OXFORDUNIVERSITY PRESS, OXFORD, GB, vol. 3, no. 2, 1998, pages 129-140, XP002199116 ISSN: 1361-8423**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Technical Field

[0001] The present invention relates to an ultrasonic diagnostic apparatus which generates a plurality of time-series radial tomographic images in the advancing and returning operation of a radial scanning ultrasonic vibrator in the body cavity of a subject.

Background Art

[0002] Japanese Unexamined Patent Application Publication No. 11-113913 discloses an ultrasonic diagnostic apparatus which has a position detector at the edge thereof and easily obtains spatial ultrasonic image data along a route by advancing and returning a general radial scanning ultrasonic probe (including an ultrasonic endoscope with an optical observing window) along a bent or inflected luminal portion so as to obtain a plurality of ultrasonic tomographic images. Various expressing methods of the spatial ultrasonic image data are examined and Japanese Unexamined Patent Application Publication No. 11-113913 discloses the expressing method with an ultrasonic three-dimensional image or a plurality of cross-sectional images which are sectioned by planes in different directions.

[0003] Further, Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766 disclose apparatuses which easily form cross-sectional images that are longitudinally sectioned by curved surfaces along an observation target such as the vein and the intestine from spatial image data and which display a guiding image indicating by which curved surface the cross-sectional image is longitudinally sectioned.

[0004] The apparatuses disclosed in Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766 have view-point setting means in the observation target included in the original image, which display a tomographic image obtained by longitudinally sectioning the image by the curved surface passing through a plurality of view points.

[0005] However, in the apparatus disclosed in Japanese Unexamined Patent Application Publication No. 11-113913, the spatial ultrasonic image data is expressed as the tomographic image obtained by sectioning the image data by a certain plane and then, the luminal portion is expressed as piecemeal images as shown in Fig. 14 and the entire luminal portion is not displayed on the screen in many cases. Because the luminal portion in the living body does not run on the specific plane. Fig. 14 shows a state of the luminal portion which partly runs on the depth side from the cross section.

[0006] Consequently, the apparatus disclosed in Japanese Unexamined Patent Application Publication No. 11-113913 has the following problems.

[0007] First problem: it is hard to clarify how the lesion is spreading along the luminal portion.

[0008] Second problem: it is hard to clarify which part in the luminal portion is scanning during the examination.

[0009] In the apparatuses disclosed in Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766, the view point upon drawing the curved surface is set after the examination, that is, after obtaining all the original images necessary for continuous viewing of the luminal portion.

[0010] Therefore, the first problem is solved after the examination. However, the apparatuses disclosed in Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766 have a drawback that the first problem is not solved in real-time during the examination. Further, the apparatuses disclosed in Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766 have a drawback that the second problem such that it is hard to clarify which part in the luminal portion is scanning during the examination (particularly, during the scanning) is still unsolved.

[0011] Incidentally, in the apparatuses disclosed in Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766, it is not considered that the examination is performed by using an ultrasonic probe which is inserted in the luminal portion in the body cavity.

[0012] Upon using the radial scanning ultrasonic probe in the body cavity, generally, the following examining method is used. That is, in general, the lesion is found during the examination and an image thereof is recorded in view of the examination efficiency and the invasion to a subject and the ultrasonic probe is sooner removed as much as possible after approximate diagnosis.

[0013] However, in the apparatuses disclosed in Japanese Unexamined Patent Application Publication Nos. 11-318884 and 2000-243766, the first and second problems are not solved during the examination, therefore, the recording of the necessary image is not clearly recognized, and the advantage to easily express the tomographic image is not obtained.

[0014] US 6,248,074 B1 discloses that an ultrasonic transducer for producing an ultrasonic tomographic image is included in a distal part of an ultrasonic endoscope to be inserted into an object of observation. A magnetic sensor for detecting a position is included in the distal part. A magnetic field generated by a magnetic field generator located near the object of observation is sensed. The position and orientation of the distal part are detected, whereby information of a position and orientation relevant to the ultrasonic tomographic image is obtained. **[0015]** The present invention is devised in consideration of the above-mentioned circumstances and it is an object of the present invention to provide an ultrasonic diagnostic apparatus which can recognize how the lesion is spreading along the luminal portion during the examination.

[0016] The present invention is devised in consideration of the above-mentioned circumstances and it is an object of the present invention to provide an ultrasonic diagnostic apparatus which can recognize how the lesion is spreading along the luminal portion during the examination.

ination and which can easily recognize which part in the luminal portion is scanned during the examination by advancing and returning the radial scanning ultrasonic probe in the body cavity.

Disclosure of Invention

[0016] The object of the present invention is achieved by an apparatus according to claim 1.

[0017] An exemplary ultrasonic diagnostic apparatus advances and returns a radial scanning ultrasonic vibrator in the body cavity of a subject and generates a plurality of time-series radial tomographic images in accordance with the advance and return. The ultrasonic diagnostic apparatus includes positional information detecting means which detects positional information of the radial scanning ultrasonic vibrator upon obtaining the radial tomographic image, and route tomographic generating means which generates a route tomographic image along a route of the advance and return of the radial scanning ultrasonic vibrator based on the positional information obtained from the positional information detecting means and the plurality of the time-series radial tomographic images.

[0018] Other features and advantages of the present invention will be obvious by the following description.

Brief Description of the Drawings

[0019]

Figs. 1 to 10 relate to the first embodiment of the present invention, Fig. 1 is a structural diagram showing the structure of an ultrasonic diagnostic apparatus, Fig. 2 is a diagram showing the structure of an edge of an ultrasonic endoscope, Fig. 3 is a flow-chart for explaining the processing flow of the ultrasonic diagnostic apparatus shown in Fig. 1, Fig. 4 is a first diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1, Fig. 5 is a second diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1, Fig. 6 is a third diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1, Fig. 7 is a fourth diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1, Fig. 8 is a fifth diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1, Fig. 9 is a sixth diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1, and Fig. 10 is a seventh diagram for explaining the operation of the ultrasonic diagnostic apparatus shown in Fig. 1.

Figs. 11 and 12 relate to the second embodiment of the present invention, Fig. 11 is a structural diagram showing the structure of an ultrasonic apparatus, and Fig. 12 is a diagram showing the structure of an edge of an ultrasonic endoscope shown in Fig. 11.

Fig. 13 is a structural diagram showing the structure of a capsule ultrasonic endoscope according to the third embodiment of the present invention.

5 Best Mode for Carrying Out the Invention

[0020] A detailed description is given of the present invention with reference to the drawings.

10 First embodiment:

[0021] Hereinbelow, a description is given of the structure and the operation of an ultrasonic diagnostic apparatus according to the first embodiment with reference to Figs. 1 to 10.

(Structure)

[0022] Referring to Fig. 1, an ultrasonic diagnostic apparatus 1 according to the first embodiment comprises an ultrasonic endoscope 2, an ultrasonic observing portion 3, a position detecting unit 4, a monitor 5, a keyboard 6, and a mouse 7. The ultrasonic endoscope 2 has an inserting portion 11 which is inserted in the body cavity of a subject, containing a flexible material, and a driving unit 14 having a motor 13 for driving an ultrasonic vibrator (which will be described later) of the inserting portion edge.

[0023] The state of the edge of the inserting portion 11 will be described with reference to Fig. 2. Referring to Fig. 2, the inserting portion 11 has, at the edge thereof, an acoustic transparent edge cap 15 which is made of a material for transmitting ultrasonic waves. The edge cap 15 has the ultrasonic vibrator 12, and the edge cap 15 is filled with a so-called acoustic medium (not shown). The ultrasonic vibrator 12 is connected to a flexible shaft 16 also made of a flexible material. The flexible shaft 16 is connected to the motor 13 in the driving unit 14.

[0024] The ultrasonic vibrator 12 is connected via a signal line (not shown) in the flexible shaft 16 to an image forming circuit (which will be described) in the ultrasonic observing portion 3 via the driving unit 14. The inserting portion 11 further has, at the edge thereof, a transmitting coil 17 with a magnetic field in space. The transmitting coil 17 is connected to a coil driving circuit (which will be described later) in the position detecting unit 4 via a signal line. The transmitting coil 17 is wound with the axes in two perpendicular directions (y- and z-axes in Fig. 2). The z-axis is the inserting direction of the ultrasonic endoscope 2, and the y-axis is vertical to the z-axis and is in parallel of the radial scanning plane (which will be described later).

[0025] Referring back to Fig. 1, the ultrasonic observing portion 3 comprises: an image forming circuit 21 which outputs a pulse-voltage excitation signal to the ultrasonic vibrator 12, performs various receiving signal processing of an echo signal from the ultrasonic vibrator 12, and forms ultrasonic image data; an image memory

22 which stores a plurality of pieces of image data; an image processing circuit 23 which performs various imaging processing of the image data; a display circuit 24 which performs D/A conversion processing of the image data and which converts the image data into an analog video signal; a three-dimensional data recording unit 25 which comprises a rigid disk or a large-capacity memory; a communication circuit 27 which communicates with the position detecting unit 4 and supplies positional and directional data to a bus 26; and an external input control circuit 29 which transmits an input from the keyboard 6 and the mouse 7 to a controller 28. The bus 26 receives and transmits a control command and data to the above circuits and the above portions. The controller 28 outputs the control command to the above circuits via the bus 26.

[0026] The position detecting unit 4 comprises: a coil driving circuit 31 which outputs a coil excitation signal to the transmitting coil 17; a plurality of receiving coils (hereinafter, referred to as receiving coils) 32 which sequentially detect the magnetic field of the transmitting coil 17 and output electric receiving signals; and a position calculating circuit 33 which outputs positional and directional data from the receiving signal outputted from the receiving coils 32.

[0027] A thick broken line shown in Fig. 1 indicates the flow of signal/image data of a radial tomographic image (which will be described later) and a route tomographic image (which will be described later), and a thin broken line indicates the flow of positional and directional data.

(Operation)

[0028] Hereinbelow, the operation of the first embodiment will be described.

[0029] The operation for forming the radial tomographic image will be described.

[0030] The ultrasonic vibrator 12 receives a pulse-voltage excitation signal from the image forming circuit 21 in the ultrasonic observing portion 3 and converts the received signal into ultrasonic beams as coarse waves of a medium. The ultrasonic beams are transmitted to the acoustic medium and the edge cap 15, and are radiated to the outside of the ultrasonic endoscope 2. Further, a reflection echo from the subject traces a route inverse to that of the ultrasonic beams and returns to the ultrasonic vibrator 12. The ultrasonic vibrator 12 converts the reflecting echo into an electric echo signal and transmits the converted signal to the image forming circuit 21 with a route inverse to that of the excitation signal.

[0031] Furthermore, while repeating the operation, the motor 13 in the driving unit 14 is rotated, thereby rotating the flexible shaft 16 and the ultrasonic vibrator 12 in the direction shown by a block arrow 18 in Fig. 2. Thus, the ultrasonic beams are sequentially radiated radially in a plane (hereinafter, referred to as a radial scanning plane) 19 in Fig. 2 vertical to the inserting portion 11 in the ultrasonic endoscope 2 and, so-called mechanical radial scanning is realized (hereinafter, simply referred to as

radial scanning).

[0032] The image forming circuit 21 performs the well-known processing of the echo signal from the ultrasonic vibrator 12, such as the envelop detection, logarithm amplification, A/D conversion, scanning conversion (processing for data on a converting polarity-coordinate system generated by the radial scanning into image data on an orthogonal-coordinate system), etc. Thus, the image forming circuit 21 forms the ultrasonic image data (hereinafter, referred to as the radial tomographic image). The radial tomographic image is outputted and is stored in the image memory 22 via the bus 26.

[0033] Next, the operation of the positional and directional data will be described.

[0034] The coil driving circuit 31 sequentially outputs the coil excitation signal to the transmitting coil 17. The transmitting coil 17 generates the magnetic coil in space. The receiving coils 32 sequentially detect the magnetic field and output electric receiving signals to the position calculating circuit 33. The position calculating circuit 33 calculates the positional and directional data based on the receiving signal and outputs the calculated data to the communication circuit 27 in the ultrasonic observing portion 3.

[0035] The positional and directional data contains data on the positions and directions of the receiving coils 32 in the transmitting coil 17. Specifically, the positional and directional data contains not only the position of the transmitting coil but also an inserting direction (z-axis in Fig. 2) of the ultrasonic endoscope and a specific direction in parallel with the radial tomographic image (y-axis in Fig. 2). The transmitting coil 17 is attached so that the y-axis in Fig. 2 is in a 12 o'clock direction of the radial tomographic image (in the upper direction displayed on the monitor) and, then, the positional and directional data includes data on the normal-line direction of the radial tomographic image (z-axis in Fig. 2) and data on the 12 o'clock direction (y-axis in Fig. 2).

[0036] The communication circuit 27 outputs the positional and directional data to the bus 26. The positional and directional data is outputted and stored in the image memory 22 via the bus 26.

[0037] The controller 28 synchronizes the radial tomographic image to the positional and directional data, correlates them, and stores them.

[0038] Next, the operation for generating the route tomographic image will mainly be described.

[0039] First, the direction of the cross-sectional plane is set. An operator normally advances and returns the (radial scanning) ultrasonic endoscope 2 in the body cavity so as to sequentially obtain a plurality of radial tomographic images, thereafter, sections the images as spatial image data by the specific plane, and observes the cross-sectional image. What is referred to as the cross-sectional plane indicates the specific plane.

[0040] According to the features of the first embodiment, the cross-sectional planes which are in parallel therewith are set for the radial tomographic images, an

intersecting line segment is obtained between the radial tomographic image and the cross-sectional plane, the intersecting line segments are combined, and thus the tomographic images (hereinafter, referred to as a route tomographic images) are generated.

[0041] Hereinbelow, a detailed description is given of the actual use of the ultrasonic diagnostic apparatus shown in Fig. 3 with reference to the flowchart.

[0042] Referring to Fig. 3, in step S1, the operator sets the direction of the cross-sectional plane. Various setting methods are considered. Preferably, an arrow index for expressing the normal-line direction of the cross-sectional plane and a plate index for schematically expressing the cross-sectional plane are stereoscopically displayed on the monitor 5, the directions of the indexes are changed by the keyboard 6 or the mouse 7, and the directions of the cross-sectional planes are sensuously recognized.

[0043] In this case, preferably, the operator can further easily recognize and set a positional relationship between the ultrasonic endoscope 2 and the receiving coils 32 by stereoscopically displaying the indexes on the coordinate system based on the direction and the position of the ultrasonic endoscope 2 at the moment of the setting or based on the directions and the positions of the fixed receiving coils 32.

[0044] The specific operation is as follows. The operator inputs the direction of the cross-sectional plane from the keyboard 6 and the mouse 7. The information on the direction is transmitted to the controller 28 via the external input control circuit 29 and then is inputted to the image processing circuit 23 as a command from the controller 28. The image processing circuit 23 performs the image processing by using the positional and directional data so as to stereoscopically display the indexes, displays the data on the monitor 5 via the display circuit 24, and sets the directions of the cross-sectional planes.

[0045] In step S2, the operator instructs the start of radial scanning.

[0046] Specifically, the operator selects various menus by using a button (not shown) on the keyboard 6 or the mouse 7, then, the image forming circuit 21 outputs an excitation signal based on a command from the controller 28, and the radial scanning starts by rotating the motor 13.

[0047] In step S3, the operator radially scans the ultrasonic endoscope 2 that is inserted in the body cavity of the subject and simultaneously starts to insert and remove (hereinafter, referred to as "manually pull out") it along the luminal portion.

[0048] In the subsequent steps, the radial tomographic images are sequentially formed by repeating the radial scanning while pulling out the ultrasonic endoscope 2. This scanning method is referred to as "manually pulling-out and scanning". Fig. 4 shows the state of the "manually pulling-out and scanning". Referring to Fig. 4, the radial tomographic images are numbered starting from one in the forming order thereof.

[0049] In step S4, the image processing circuit 21 substitutes one for a variable n provided as a counter.

[0050] In step S5, the image forming circuit 21 forms an n-th radial tomographic image and the controller 28 synchronizes the radial tomographic image to the positional and directional data, correlates them, and stores the radial tomographic image and the positional and directional data.

[0051] In step S6, the image processing circuit 23 obtains the n-th radial cross-sectional plane. Specifically, the image processing circuit 23 reads, from the image memory 22, the n-th radial tomographic image and the positional and directional data correlated therewith, and the transmitting coil 17 is arranged near the ultrasonic vibrator 12. Consequently, the transmitting coil 17 is positioned in the rotating center of the ultrasonic vibrator 12 in the n-th radial tomographic image, and the n-th cross-sectional plane is obtained.

[0052] Hereinbelow, a detailed description is given of how to obtain the n-th cross-sectional plane. Fig. 5 shows the n-th cross-sectional plane. The n-th cross-sectional plane is in the direction set in step S1 and passes through the rotating center of the n-th radial tomographic image. The single cross-sectional plane is determined for the n-th radial tomographic image. Therefore, this step is repeated by changing the variable n, each single cross-sectional plane is obtained for each of the first, second, and, ..., radial tomographic images. All of the above-obtained cross-sectional planes for the first, second, and, ..., radial tomographic images are in the direction set in step S1 and are in parallel therewith as shown in Fig. 4.

[0053] In step S7, the image processing circuit 23 obtains the intersecting line segment (n-th intersecting line segment) of the n-th radial tomographic image and the n-th cross-sectional plane. Fig. 5 shows the n-th intersecting line segment.

[0054] In step S8, in the case of n = 1, the processing jumps to step S14.

[0055] In step S9, the image processing circuit 23 interpolates image information on an (n-1)-th intersecting line segment and image information on the n-th intersecting line segment, and forms an n-th piece. Fig. 6 shows the n-th piece. Various interpolating methods are considered, for example, the interval between the intersecting lines is linearly interpolated and it is non-linearly interpolated along the route for manually pulling out.

[0056] For the convenience of a description, the intersecting line segments are thinned out and drawn in Fig. 6 and, originally, the interval between the intersecting line segments are close to each other as shown in Fig. 7.

[0057] In step S10, the image processing circuit 23 rewrites the n-th piece to the previous route tomographic images and updates the images. That is, the image processing circuit 23 forms the new route tomographic image. Fig. 6 shows the updated route tomographic image.

[0058] In step S11, the display circuit 24 generates an

image signal obtained by arranging the n-th radial tomographic image and the route tomographic image. Fig. 8 shows the image in step S11. As shown in Fig. 8, the n-th radial tomographic image is on the left and the route tomographic image is on the right. Thick lines on the n-th radial tomographic image and on the route tomographic image are markers (hereinafter, referred to as intersecting-line-segment markers) indicating the intersecting line segment obtained for forming the route tomographic image. That is, the intersecting-line-segment maker shown in Fig. 8 indicates the n-th intersecting line segment and is displayed with a color different from that of the background such as green when the background image is a monochrome one.

[0059] In step S12, the monitor 5 arranges the n-th radial tomographic image and the route tomographic image and displays them.

[0060] The monitor 5 has displayed the (n-1)-th radial tomographic image and the route tomographic image obtained by superimposing the first to (n-1)-th pieces in the previous steps and, then, the screen is updated.

[0061] In step S13, the operator instructs the end of manually pulling-out and scanning via the keyboard 6 or the mouse 7. In other steps, the processing sequence jumps to step S14.

[0062] Specifically, the operator selects various menus by a button (not shown) on the keyboard 6 or the mouse 7 and instructs the end of manually pulling-out and scanning, then, the image forming circuit 21 stops the output of the excitation signal based on the command from the controller 28, the motor 13 stops rotating, and the radial scanning ends.

[0063] In step S14, the image processing circuit 23 increments the variable n provided as the counter by 1. After that, the image processing circuit 23 jumps the processing to step S5.

[0064] As mentioned above, unless the operator instructs the end of manually pulling-out and scanning, the processing from steps S5 to S14 is repeated.

[0065] By repeating the processing from steps S5 to S14, the route tomographic image is sequentially extended in accordance with the manually pulling-out and scanning as shown in Fig. 8.

[0066] According to the first embodiment, it is characterized that the image data comprising a plurality of radial tomographic images are not sectioned by the specific plane so as to generate the tomographic planar image, but a plurality of cross-sectional planes are obtained for a plurality of radial tomographic images, the radial tomographic images are sectioned by the cross-sectional planes, a plurality of intersecting line segments are obtained, the image data on the intersecting line segment is interpolated, the route tomographic image is generated on the two-dimensional screen.

[0067] The above description has been given of the operation for generating the route tomographic image during examination, especially, during the manually pulling-out and scanning. Hereinbelow, a description is given

of the operation after the manually pulling-out and scanning.

[0068] The preparation needs the writing various data into the three-dimensional data recording unit 25 during the examination as preparation. Hereinbelow, a detailed description is given.

[0069] If the operator sets the direction of the cross-sectional plane in step S1, the controller 28 writes, to the three-dimensional data recording unit 25, a directional vector in the normal-line direction of the cross-sectional plane.

[0070] In step S6, when the image processing circuit 23 reads, from the image memory 22, the n-th radial tomographic image and the positional and directional data correlated therewith, the controller 28 correlates the n-th radial tomographic image with the positional and directional data, and writes the correlated result to the three-dimensional data recording unit 25.

[0071] With the above structure and operation, not only the operation described with reference to the flowchart shown in Fig. 3 is obtained during the manually pulling-out and scanning but also the cross-sectional planes and a plurality of continuous radial tomographic images are used after the manually pulling-out and scanning.

[0072] Next, the operation after the manually pulling-out and scanning will be described.

[0073] First, the controller 28 sequentially reads, to the image memory from the three-dimensional data recording unit 25, the radial tomographic image and the positional and directional data, starting from the first radial tomographic image.

[0074] In this case, the operator sets the cross-sectional plane similarly to the case in step S1, and the components perform the operation in steps S4 to S14. Consequently, the route tomographic image is obtained along the route for the manually pulling-out scanning upon obtaining the positional and directional data.

[0075] Further, referring to Fig. 9, the controller 28 changes the position and the direction of the intersecting line-segment marker on the route tomographic image and the intersecting-line-segment on the radial tomographic image based on the operator's instruction obtained via an arrow key (not shown) on the keyboard 6 or via the mouse 7.

[0076] The intersecting-line-segment marker on the route tomographic image can selectively be moved at the position of each intersecting line segment. For example, the intersecting-line-segment marker is in the direction shown by an arrow shown in Fig. 9.

[0077] The operator moves the intersecting-line-segment marker, in accordance therewith, the (n-1)-th, n-th, (n+1)-th, ... radial tomographic images are sequentially updated and are displayed on the left of the monitor 5.

[0078] The intersecting-line-segment marker on the n-th radial tomographic image is rotated with the rotating center of the ultrasonic vibrator 12 as a center on the radial tomographic image. For example, the rotating direction is shown by an arrow in Fig. 9.

[0079] The operator rotates the intersecting-line-segment marker, in accordance therewith, the cross-sectional plane is set again. Various methods for setting the new cross-sectional planes are considered. Hereinbelow, a detailed description is given.

[0080] For example, according to a first method, the new cross-sectional plane is vertical to the n-th radial tomographic image and passes through the intersecting-line-segment marker on the n-th radial tomographic image. In this case, although the original cross-sectional plane is not limited to be vertical to the n-th radial tomographic image, the operation of the keyboard 6 or the mouse 7 enables the cross-sectional plane to be set again to be vertical to the radial tomographic image as soon as the intersecting-line-segment marker starts to rotate on the radial tomographic image.

[0081] According to a second method, the new cross-sectional plane keeps an angle formed between the n-th radial tomographic image and the original cross-sectional plane (that is, an angle formed between the normal line of the n-th radial tomographic image and the normal line of the original cross-sectional plane), and passes through the intersecting-line-segment marker on the n-th radial tomographic image.

[0082] According to the first method, the cross-sectional plane is promptly set again vertically and thus the route tomographic image sharply changes. However, with the structure and the operation according to the second method, the sharp change can be prevented.

[0083] The operator rotates the intersecting-line-segment marker and, in accordance therewith, the new route tomographic image is sequentially updated and displayed on the right of the monitor 5.

[0084] A series of operations after the manually pulling-out and scanning is realized mainly by the operation of the image processing circuit 23 and the command from the controller 28.

[0085] The above description has given of the operation for generating the route tomographic image after the manually pulling-out and scanning. Hereinbelow, the operation for the new radial scanning after the manually pulling-out and scanning will be described.

[0086] First, the operator forms the route tomographic image and temporarily stops the radial scanning. After that, the operator performs the new radial scanning without removing the ultrasonic endoscope 2 from the subject. However, the route tomographic image is not updated in the new radial scanning.

[0087] The image processing circuit 23 obtains the intersecting line segment of the already-obtained route tomographic image and the current radial scanning plane, generates the intersecting-line-segment marker based on the position of the intersecting line segment, superimposes the intersecting-line-segment marker on the obtained route tomographic image, and displays it. This state is shown in Fig. 10. In this case, the radial tomographic image which is currently scanned is displayed on the left of the screen on the monitor 5.

(Advantages)

[0088] With the structure and operations according to the first embodiment, the (radial scanning) ultrasonic endoscope 2 is advanced and returned in the body cavity. Thus, (1) how the lesion is spreading along the luminal portion during the examination is easily understood, and (2) which part of the luminal portion is scanning during the examination is easily understood.

[0089] Further, every formation of the radial tomographic image, the cross-sectional plane and the intersecting line segment are sequentially obtained, and the route tomographic image is updated and displayed. Consequently, the coordinate conversion of the two-dimensional image is not necessary, the scale of the image processing is reduced, and the route tomographic image is generated and updated fast irrespective of during or after the examination.

[0090] The intersecting-line-segment marker is provided so that the intersecting-line-segment is expressed between the radial tomographic image and the route tomographic image. Consequently, the positional relationship is easily understood irrespective of during/after the examination.

[0091] The intersecting-line-segment marker is moved on the route tomographic image by the input means such as the keyboard and the mouse and the radial tomographic image is updated in accordance with the movement. The route tomographic image is used as a guide for searching for the radial tomographic image. The obtained radial tomographic image is easily understood which part in the bent or inflected luminal portion is scanned. Therefore, the desired tomographic image is readily obtained and the interest area such as the lesion is easily drawn and found.

[0092] Further, the intersecting-line-segment line marker is moved little by little and the radial tomographic image is updated. Thus, the connection of the organ and the shape of the vas are easily understood and the spatial positional relationship is easily clarified between the lesion and the peripheral organ.

[0093] The intersecting-line-segment marker is rotated on the radial tomographic image by the input means such as the keyboard 6 or the mouse 7 and, in accordance therewith, the route tomographic image is updated. The desired route tomographic image is readily obtained, how lesion is spreading along the luminal portion is easily and precisely understood.

[0094] The image processing circuit 23 obtains the intersecting line segment between the already-obtained radial scanning plane and the route tomographic image, and generates the intersecting-line-segment marker based on the position of the intersecting line segment. The intersecting-line-segment marker is superimposed and displayed onto the obtained route tomographic image. The operator uses the route tomographic image and the intersecting-line-segment marker as the guide of the current radial scanning plane, and the lesion is easily

drawn.

(Modification)

[0095] According to the first embodiment, the intersecting-line-segment marker is moved on the route tomographic image as shown in Fig. 8 and the radial tomographic image is updated. The intersecting-line-segment marker may be fixed and the route tomographic image may be scrolled.

[0096] During the manually pulling-out and scanning, the route tomographic image is out of the monitor screen and the route tomographic image may be scrolled so that the newest intersecting line segment is always displayed on the screen. With the above-described structure and operation, the operator easily understands which part in the living body is scanning by checking the screen.

[0097] According to the first embodiment, the intersecting-line-segment marker is rotated on the radial tomographic image and the route tomographic image is updated. However, the intersecting-line-segment marker may be fixed and the radial tomographic image may be rotated.

[0098] According to the first embodiment, the manually pulling-out and scanning is performed by pulling out the ultrasonic endoscope. On the contrary, the ultrasonic endoscope may be moved in the direction for inserting the ultrasonic endoscope deeply in the body cavity and may be advanced or returned.

[0099] According to the first embodiment, the radial tomographic image and the route tomographic image are arranged and displayed on the single monitor at the same time. However, both the images may be displayed on separate monitor and may be switched and displayed with the intersecting-line-segment marker.

[0100] According to the first embodiment, the transmitting coil 17 is arranged to the edge of the inserting portion 11 in the ultrasonic endoscope 2 and the receiving coils 32 are fixed in space. However, the reception and the transmission may be on the contrary.

[0101] According to the first embodiment, the position and the direction of the radial tomographic image are detected by using the magnetic field. However, they may be detected with the acceleration or another means.

Second embodiment:

[0102] The second embodiment is almost the same as the first embodiment, therefore, only different points are described, the same reference numerals denote the same components, and a description thereof is omitted.

[0103] Hereinbelow, a description is given of the structure and the operation of the ultrasonic diagnostic apparatus according to the second embodiment with reference to Figs. 11 and 12.

(Structure)

[0104] Referring to Fig. 11, the driving unit 14 according to the second embodiment does not have the motor.

5 However, referring to Fig. 12, the ultrasonic vibrator is cut in rectangles at the edge of the inserting portion in an ultrasonic endoscope 2a according to the second embodiment and thus a circular array (hereinafter, referred to as an ultrasonic vibrator array) 51 is aligned around the inserting axis. Ultrasonic vibrators forming the ultrasonic vibrator array 51 are connected to the image forming circuit 21 in the ultrasonic observing unit 3 via the signal lines and the driving unit 14. Other structure is the same as that according to the first embodiment.

15

(Operation)

[0105] The operation for forming the radial tomographic image is different from that according to the first embodiment.

[0106] Among the ultrasonic vibrators forming the ultrasonic vibrator array 51, a part of and a plurality of the ultrasonic vibrators receive pulse excitation signals from the image forming circuit 21 in the ultrasonic observing unit 3, and convert the signals into ultrasonic waves as coarse waves of the medium. In this case, the image forming circuit 21 delays the excitation signals so that the excitation signals reach the ultrasonic vibrators at different times. This delay operation is implemented so that a single ultrasonic beam is formed when the ultrasonic waves excited by the ultrasonic vibrators are overlapped in the subject.

[0107] The ultrasonic beam is irradiated to the outside of the ultrasonic endoscope 2a, and the reflecting echo from the subject is returned to the ultrasonic vibrator while tracing the route contrary to that of the ultrasonic beam. The ultrasonic vibrators convert the reflecting echo into electric echo signals, and transmit the converted signals to the image forming circuit 21 via the route contrary to that of the excitation signals.

[0108] Next, the image forming circuit 21 selects again a plurality of ultrasonic vibrators for forming the ultrasonic beams and transmits the excitation signal so as to execute the radial scanning by the ultrasonic beams shown 45 by an arrow in Fig. 12. Thus, the angle of the ultrasonic beams changes. By repeating the operation of the above image forming circuit 21, the so-called electric radial scanning is realized.

[0109] Other operations are the same as those according 50 to the first embodiment.

(Advantages)

[0110] According to the first embodiment, the mechanical radial scanning is used and, therefore, the deviation of the flexible shaft 16 is caused and the deviations are not uniform among a plurality of radial tomographic images, thus resulting in the deviation on the route tomo-

graphic image. Because in the normal mechanical radial scanning, the angle and the position for the rotation of the motor 13 are detected by a rotary encoder adjacent to the motor 13.

[0111] However, according to the second embodiment, the electric radial scanning is used and, consequently, the above-mentioned problem of the deviation on the route tomographic image is solved. Other advantages are the same as those according to the first embodiment.

(Modification)

[0112] The radial scanning according to the second embodiment is implemented at the entire circumference with an angle of 360° or with an angle of 270° smaller than the foregoing. Third embodiment:

The third embodiment is substantially the same as the first embodiment, therefore, only different points are described, the same reference numerals denotes the same components, and a description thereof is omitted.

(Structure and operation)

[0113] Hereinbelow, the structure and the operation of an ultrasonic diagnostic apparatus will be described according to the third embodiment with reference to Fig. 13. The entire structural diagram is the same as Fig. 11.

[0114] Referring to Fig. 13, a radial scanning ultrasonic probe according to the third embodiment uses a capsule ultrasonic endoscope (hereinafter, referred to as the capsule ultrasonic endoscope) 101 as the radial scanning ultrasonic probe.

[0115] The capsule ultrasonic endoscope 101 comprises the transmitting coil 17, the ultrasonic vibrator 12, a rigid shaft 104, an ultracompact motor 102, and a signal cable 103. Unlike the first embodiment, the driving unit 14 does not have the motor 13. In place of the motor 13 in the driving unit 14, the capsule ultrasonic endoscope 101 has the ultracompact motor 102.

[0116] The ultrasonic vibrator 12 is connected to the rigid stick shaft 104. The rigid shaft 104 is connected to the ultracompact motor 102. The ultrasonic vibrator 12 is connected to the image forming circuit 21 in the ultrasonic observing unit 3 via the driving unit 13 and a signal line 105 passing through the rigid shaft 104, the ultracompact motor 102, and the signal cable 103. The transmitting coil 17 generates the magnetic field in space and is connected to the coil driving circuit 31 in the position detecting unit 4 via the signal line 105.

[0117] Other structure and operation are the same as those according to the first embodiment.

(Advantages)

[0118] According to the first embodiment, the devia-

tions of the flexible shaft 16 are caused and the deviations are not uniform among the plurality of radial tomographic images, thus causing the problem of the deviation on the route tomographic image. Because, in the normal mechanical radial scanning, the angle and the position of the motor rotation are detected by the rotary encoder adjacent to the motor. However, according to the third embodiment, not the flexible shaft 16, but the ultracompact motor 102 and the rigid shaft 104 are arranged near the ultrasonic vibrator 12, thereby solving the problem.

[0119] Further, according to the third embodiment, the capsule ultrasonic endoscope 101 is used, thus, the examinee easily drinks the capsule, and the load thereof is reduced. Normally, the operator can not easily operate the radial scanning plane by using the capsule ultrasonic endoscope 101 and thus the observed portion of the subject is not easily recognized which part of the subject is observing. However, with the structure and the operation according to the third embodiment, the route tomographic

image is observed and thus the operator easily performs the diagnosis.

[0120] Furthermore, since the observed portion is easily recognized which part of the subject is observing without the optical observing window, the components such as the optical observing window, the CCD camera, the glass fiber, and the video signal cable are not necessary and the capsule ultrasonic endoscope 101 is reduced in size.

[0121] In addition, normally, the capsule ultrasonic endoscope 101 cannot manually be advanced and returned. However, the route tomographic image is formed while the capsule ultrasonic endoscope 101 is advanced and returned by the natural swallowing, falling, and peristaltic motions, and thus the operator observes the images. Other advantages are the same as those according to the first embodiment.

[0122] According to the present invention, various embodiments can be implemented within the wide range of the present invention. The present invention is not limited by specific embodiments, except for the following claims.

Industrial Applicability

[0123] As mentioned above, the ultrasonic diagnostic apparatus according to the present invention is advantageous as an apparatus for detecting the stretch of the observing portion in the luminal portion.

50 Claims

1. An ultrasonic diagnostic apparatus which is adapted to advance and return a radial scanning ultrasonic vibrator (12; 51) for performing radial scanning in which ultrasonic beams are sequentially radiated radially in the living body of a subject and generates a plurality of time-series radial tomographic images in accordance with the advance and return, the ultra-

sonic diagnostic apparatus comprising:

positional information detecting means (17, 32), which detects positional information of the radial scanning ultrasonic vibrator (12; 51) upon obtaining the radial tomographic image; and route tomographic generating means which generates a route tomographic image along a route of the advance and return of the radial scanning ultrasonic vibrator (12; 51) based on the positional information obtained from the positional information detecting means (17, 32) and the plurality of the time-series radial tomographic images, **characterized by**

intersecting line segment extracting means which obtains an intersecting line segment of the radial tomographic image and a respective of a plurality of parallel planes passing through the radiation center of the radially radiated ultrasonic beams, generating the radial tomographic image, wherein

the route tomographic image generating means generates each route tomographic image along the advancing and returning route based on a plurality of intersecting line segments obtained by the intersecting line segment extracting means.

2. The ultrasonic diagnostic apparatus according to Claim 1, wherein the intersecting line segment extracting means extracts the intersecting line segment for every obtained new radial tomographic image, and the route tomographic image generating means generates the route tomographic image for every extracted new intersecting line segment.

3. The ultrasonic diagnostic apparatus according to claim 1, wherein said positional information detecting means (17, 32) is configured as a positional and directional detecting means which detects positions and directions of the plurality of radial tomographic images; and wherein the route tomographic image generating means generates a route tomographic image along the advancing and returning route based on the position and the direction.

4. The ultrasonic diagnostic apparatus according to Claim 1 or 2, further comprising:

display means (3, 5) which comparably displays the radial tomographic image and the route tomographic image, wherein the display means superimposes and displays an intersecting-line-segment marker indicating the intersecting line segment on at

least one of the radial tomographic image and the route tomographic image.

5. The ultrasonic diagnostic apparatus according to Claim 4, wherein the display means (3, 5) superimposes and displays an intersecting-line-segment marker indicating the intersecting line segment on at least one of the radial tomographic image and the route tomographic image.

6. The ultrasonic diagnostic apparatus according to Claim 4 or 5, further comprising: setting means (6, 7) which sets the position of the intersecting-line-segment marker, wherein the display means (3, 5) updates and displays the radial tomographic image or the route tomographic image in conjunction with the setting of the position of the intersecting-line-segment marker.

7. The ultrasonic diagnostic apparatus according to any one of Claims 4 to 6, wherein the display means (3, 5) updates and displays the radial tomographic image or the route tomographic image in conjunction with the setting of the position of the intersecting-line-segment marker.

8. The ultrasonic diagnostic apparatus according to any one of Claims 4 to 7, wherein the intersecting line segment extracting means extracts the intersecting line segment between the already-formed route tomographic image and the radial scanning plane during the scanning, and the display means (3, 5) superimposes and displays the intersecting-line-segment marker indicating the intersecting line segment, as a guide of the radial scanning plane during the scanning, on the already-formed route tomographic image.

9. The ultrasonic diagnostic apparatus according to any one of Claims 1 to 8, wherein the radial scanning ultrasonic vibrator (12; 51) is an electric radial scanning ultrasonic vibrator.

10. The ultrasonic diagnostic apparatus according to any one of Claims 1 to 8, wherein the radial scanning ultrasonic vibrator (12; 51) is arranged in a capsule (101) inserted in the body cavity.

11. The ultrasonic diagnostic apparatus according to Claim 10, wherein the capsule has a motor (102) which rotates the ultrasonic vibrator (12).

Patentansprüche

1. Ultraschall-Diagnosevorrichtung, die zum Ausführen einer Radialabtastung einen Radialabtastungs-Ultraschallvibrator (12; 51) vorwärts und rückwärts zu bewegen vermag, wobei Ultraschallstrahlen sequentiell radial in den lebenden Körper eines Patienten gestrahlt werden, und die in Zeitserie mehrere radiale tomographische Bilder entsprechend der Vorwärts- und Rückwärtsbewegung erzeugt, wobei die Ultraschall-Diagnosevorrichtung umfasst:

ein Positionsinformations-Erfassungsmittel (17, 32), das Positionsinformation des Radialabtastungs-Ultraschallvibrators (12; 51) bei Erhalt des radialen tomographischen Bildes erfasst; und

ein Mittel zum Erzeugen eines tomographischen Routenbilds, das ein tomographisches Routenbild entlang einer Route der Vorwärts- und Rückwärtsbewegung des Radialabtastungs-Ultraschallvibrators (12; 51) erzeugt, basierend auf der von dem Positionsinformations-Erfassungsmittel (17, 32) erhaltenen Positionsinformation und den mehreren radialen tomographischen Bildern in Zeitserie, **gekennzeichnet durch**

ein Schnittliniensegment-Extraktionsmittel, das ein Schnittliniensegment des radialen tomographischen Bilds und einer betreffenden Ebene einer Vielzahl paralleler Ebenen, die **durch** das Strahlungszentrum der radial abgestrahlten, das radiale tomographische Bild erzeugenden Ultraschallstrahlen hindurchgehen, erhält, wobei

das Mittel zum Erzeugen eines tomographischen Routenbilds jedes tomographische Routenbild entlang der Vorwärts- und Rückwärtsbewegungsroute auf der Basis einer Vielzahl von dem Schnittliniensegment-Extraktionsmittel erhaltenen Schnittliniensegmente erzeugt.

2. Ultraschall-Diagnosevorrichtung nach Anspruch 1, wobei das Schnittliniensegment-Extraktionsmittel das Schnittliniensegment für jedes erhaltene neue radiale tomographische Bild extrahiert, und das Mittel zum Erzeugen eines tomographischen Routenbilds das tomographische Routenbild für jedes extrahierte neue Schnittliniensegment erzeugt.

3. Ultraschall-Diagnosevorrichtung nach Anspruch 1, wobei das Positionsinformations-Erfassungsmittel (17, 32) als ein Positions- und Richtungs-Erfassungsmittel ausgebildet ist, das Positionen und Richtungen der mehreren radialen tomographischen Bilder erfasst; und wobei das Mittel zum Erzeugen eines tomographischen Routenbilds ein tomographisches Routenbild entlang der Vorwärts- und Rückwärtsbewegungsroute basierend auf der Position und der Richtung erzeugt.

5 4. Ultraschall-Diagnosevorrichtung nach Anspruch 1 oder 2, ferner mit:

einem Anzeigemittel (3, 5), das zum Vergleich das radiale tomographische Bild und das tomographische Routenbild anzeigt, wobei das Anzeigemittel einen das Schnittliniensegment angebenden Schnittliniensegment-Markierer dem radialen tomographischen Bild und/oder dem tomographischen Routenbild überlagert und anzeigt.

5. Ultraschall-Diagnosevorrichtung nach Anspruch 4, wobei das Anzeigemittel (3, 5) einen das Schnittliniensegment angebenden Schnittliniensegment-Markierer dem radialen tomographischen Bild und/oder dem tomographischen Routenbild überlagert und anzeigt.

6. Ultraschall-Diagnosevorrichtung nach Anspruch 4 oder 5, ferner mit:

einem Einstellmittel (6, 7), das die Position des Schnittliniensegment-Markierers einstellt, wobei das Anzeigemittel (3, 5) das radiale tomographische Bild oder das tomographische Routenbild in Verbindung mit dem Einstellen der Position des Schnittliniensegment-Markierers aktualisiert und anzeigt.

35 7. Ultraschall-Diagnosevorrichtung nach einem der Ansprüche 4 bis 6, wobei das Anzeigemittel (3, 5) das radiale tomographische Bild oder das tomographische Routenbild in Verbindung mit dem Einstellen der Position des Schnittliniensegment-Markierers aktualisiert und anzeigt.

8. Ultraschall-Diagnosevorrichtung nach einem der Ansprüche 4 bis 7, wobei das Schnittliniensegment-Extraktionsmittel das Schnittliniensegment zwischen dem bereits gebildeten tomographischen Routenbild und der radialen Abtastebene während des Abtastvorgangs extrahiert, und das Anzeigemittel (3, 5) den das Schnittliniensegment angebenden Schnittliniensegment-Markierer als eine Führung der radialen Abtastebene beim Abtastvorgang dem bereits gebildeten tomographischen Routenbild überlagert und anzeigt.

50 9. Ultraschall-Diagnosevorrichtung nach einem der Ansprüche 1 bis 8, wobei der Radialabtastungs-Ultraschallvibrator (12;

51) ein elektrischer Radialabtastungs-Ultraschallvibrator ist.

10. Ultraschall-Diagnosevorrichtung nach einem der Ansprüche 1 bis 8, wobei der Radialabtastungs-Ultraschallvibrator (12; 51) in einer in den Körperhohlraum eingeführten Kapsel (101) angeordnet ist. 5

11. Ultraschall-Diagnosevorrichtung nach Anspruch 10, wobei die Kapsel einen Motor (102) aufweist, der den Ultraschallvibrator (12) dreht. 10

Revendications 15

1. Appareil de diagnostic ultrasonore qui est adapté à faire avancer et revenir un vibrateur ultrasonore à balayage radial (12; 51) pour exécuter un balayage radial dans lequel des faisceaux ultrasonores sont séquentiellement projetés radialement dans le corps vivant d'un sujet et génère une pluralité d'images tomographiques radiales en série chronologique en fonction de l'avance et du retour, l'appareil de diagnostic ultrasonore comprenant: 20

un moyen de détection d'information positionnelle (17, 32) qui détecte une information positionnelle du vibrateur ultrasonore à balayage radial (12; 51) à l'obtention de l'image tomographique radiale; et 25

un moyen de génération d'image tomographique de trajectoire qui génère une image tomographique de trajectoire sur une trajectoire d'avance et de retour du vibrateur ultrasonore à balayage radial (12; 51) sur la base de l'information positionnelle obtenue du moyen de détection d'information positionnelle (17, 32) et de la pluralité des images tomographiques radiales en série chronologique, **caractérisé par** 30

un moyen d'extraction de segment de lignes sécantes, qui obtient un segment de lignes sécantes de l'image tomographique radiale et un respectif d'une pluralité de plans parallèles passant par le centre de rayonnement des faisceaux ultrasonores projetés radialement générant l'image tomographique radiale, dans lequel le moyen de génération d'image tomographique de trajectoire génère chaque image tomographique de trajectoire sur la trajectoire d'avance et de retour sur la base d'une pluralité de segments de lignes sécantes obtenus par le moyen d'extraction de segment de lignes sécantes. 35

2. Appareil de diagnostic ultrasonore selon la revendication 1, dans lequel le moyen d'extraction de segment de lignes sécantes extrait le segment de lignes sécantes pour chaque nouvelle image tomographique radiale obtenue, et 40

le moyen de génération d'image tomographique de trajectoire génère l'image tomographique de trajectoire pour chaque nouveau segment de lignes sécantes extrait. 45

3. Appareil de diagnostic ultrasonore selon la revendication 1, dans lequel ledit moyen de détection d'information positionnelle (17, 32) est configuré comme un moyen de détection positionnel et directionnel qui détecte des positions et des directions de la pluralité d'images tomographiques radiales; et 50

dans lequel le moyen de génération d'image tomographique de trajectoire génère une image tomographique de trajectoire sur la trajectoire d'avance et de retour sur la base de la position et de la direction. 55

4. Appareil de diagnostic ultrasonore selon la revendication 1 ou 2, comprenant en outre:

un moyen d'affichage (3, 5) qui affiche de manière comparable l'image tomographique radiale et l'image tomographique de trajectoire, dans lequel le moyen d'affichage superpose et affiche un marqueur de segment de lignes sécantes indiquant le segment de lignes sécantes sur au moins l'une de l'image tomographique radiale et de l'image tomographique de trajectoire. 60

5. Appareil de diagnostic ultrasonore selon la revendication 4, dans lequel le moyen d'affichage (3, 5) superpose et affiche un marqueur de segment de lignes sécantes indiquant le segment de lignes sécantes sur au moins l'une de l'image tomographique radiale et de l'image tomographique de trajectoire. 65

6. Appareil de diagnostic ultrasonore selon la revendication 4 ou 5, comprenant en outre:

un moyen de réglage (6, 7) qui règle la position du marqueur de segment de lignes sécantes, dans lequel le moyen d'affichage (3, 5) met à jour et affiche l'image tomographique radiale ou l'image tomographique de trajectoire en conjonction avec le réglage de la position du marqueur de segment de lignes sécantes. 70

7. Appareil de diagnostic ultrasonore selon l'une quelconque des revendications 4 à 6, dans lequel le moyen d'affichage (3, 5) met à jour et affiche l'image tomographique radiale ou l'image tomographique de trajectoire en conjonction avec le réglage de la position du marqueur de segment de lignes sécantes. 75

8. Appareil de diagnostic ultrasonore selon l'une quelconque des revendications 4 à 7,
dans lequel le moyen d'extraction de segment de lignes sécantes extrait le segment de lignes sécantes entre l'image tomographique de trajectoire déjà 5
formée et le plan de balayage radial pendant le balayage, et
le moyen d'affichage (3, 5) superpose et affiche le marqueur de segment de lignes sécantes indiquant le segment de lignes sécantes, comme un guide du 10
plan de balayage radial pendant le balayage, sur l'image tomographique de trajectoire déjà formée.

9. Appareil de diagnostic ultrasonore selon l'une quelconque des revendications 1 à 8, 15
dans lequel le vibrateur ultrasonore à balayage radial (12; 51) est un vibrateur ultrasonore à balayage radial électrique.

10. Appareil de diagnostic ultrasonore selon l'une quelconque des revendications 1 à 8, 20
dans lequel le vibrateur ultrasonore à balayage radial (12; 51) est agencé dans une capsule (101) insérée dans la cavité corporelle.

11. Appareil de diagnostic ultrasonore selon la revendication 10, dans lequel la capsule a un moteur (102) qui met en rotation le vibrateur ultrasonore (12).

25

30

35

40

45

50

55

FIG.1

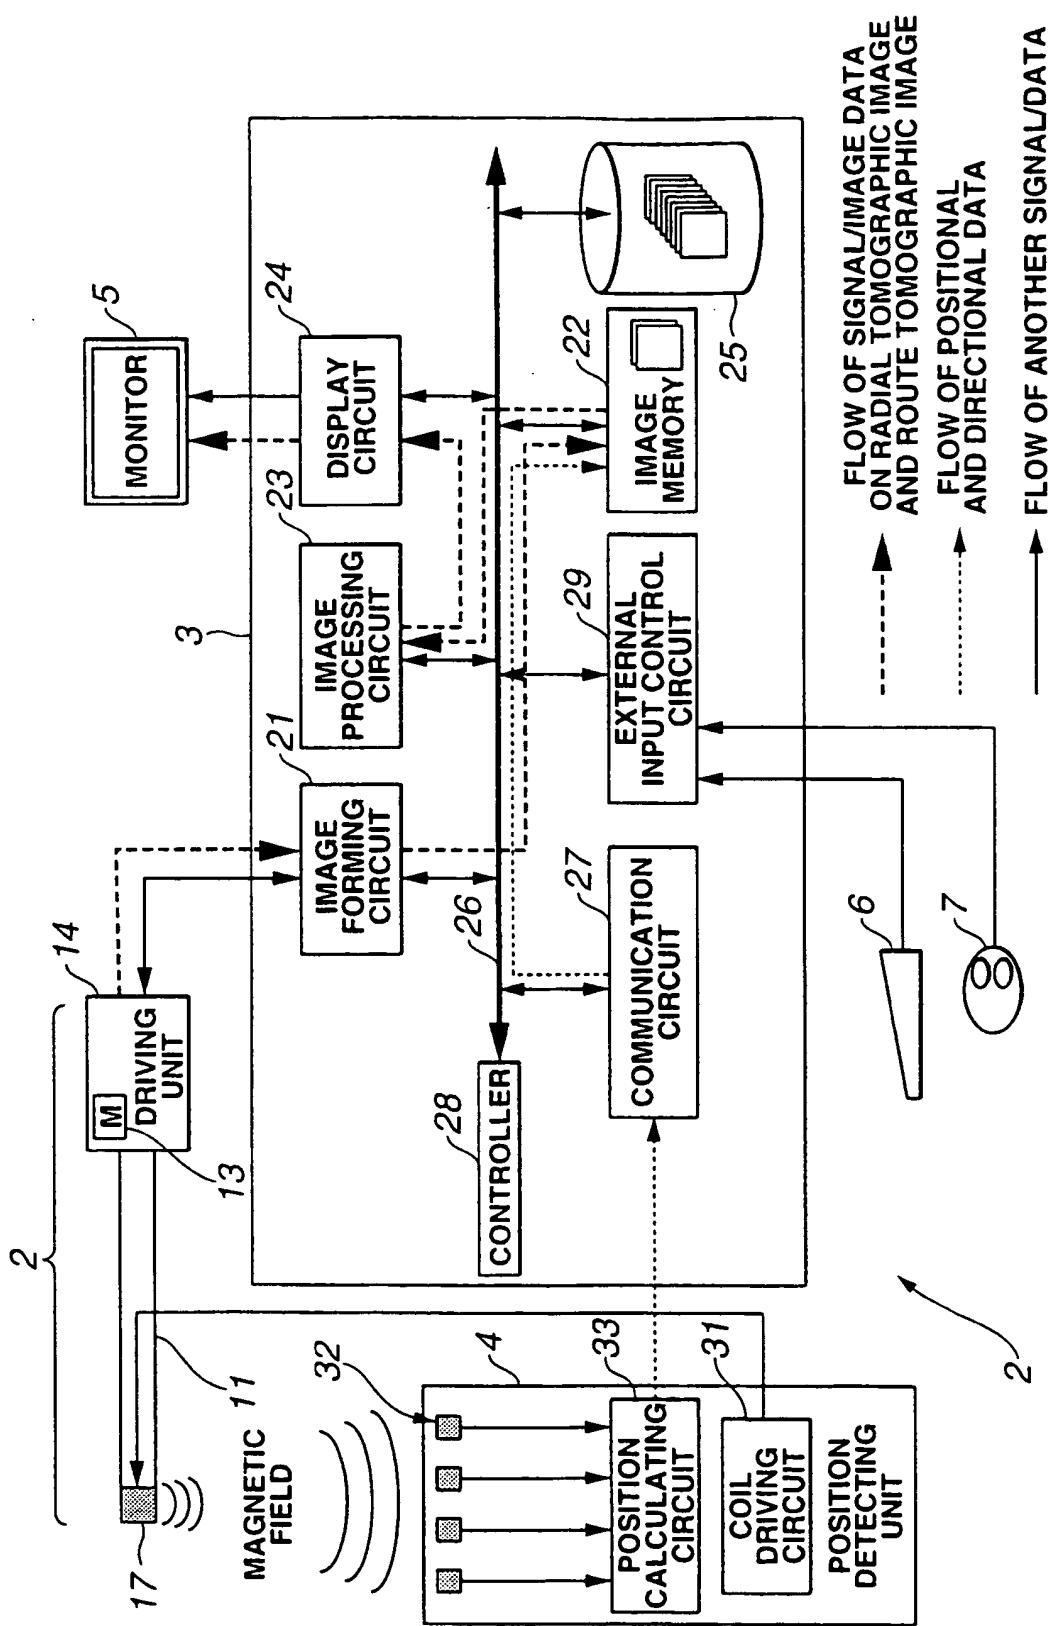


FIG.2

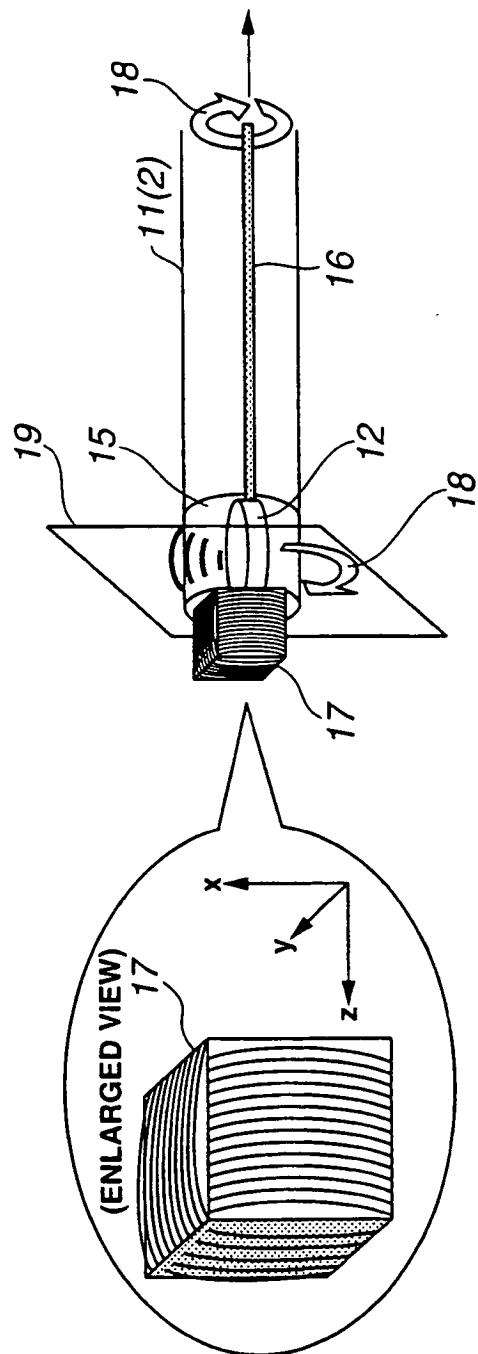


FIG.3

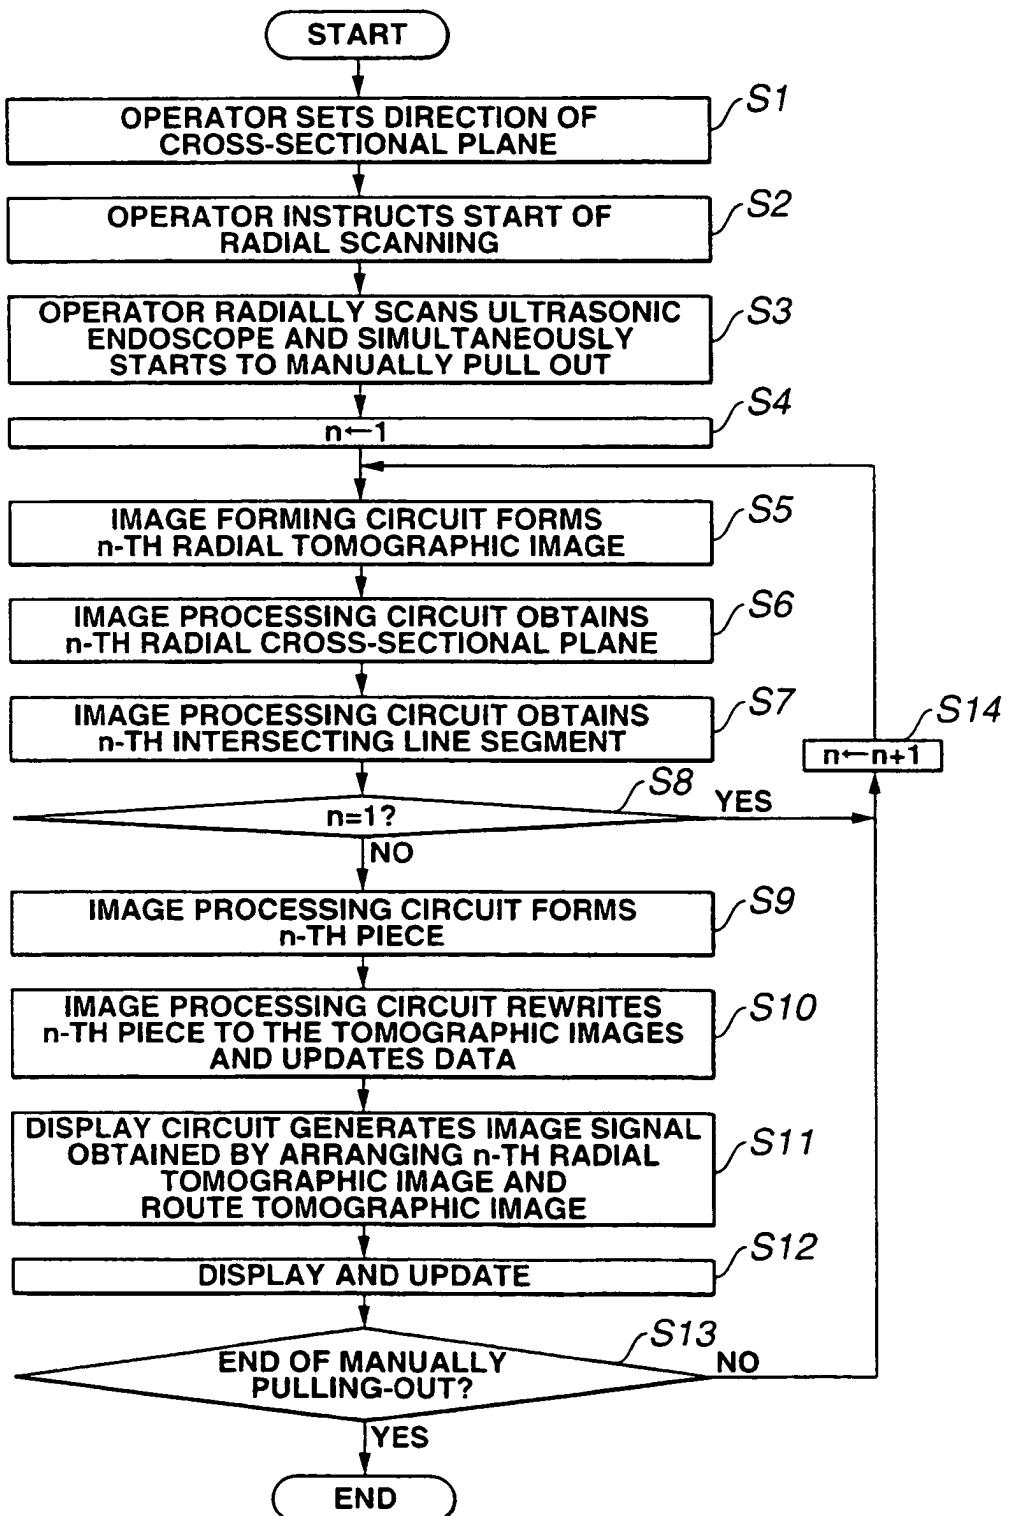


FIG.4

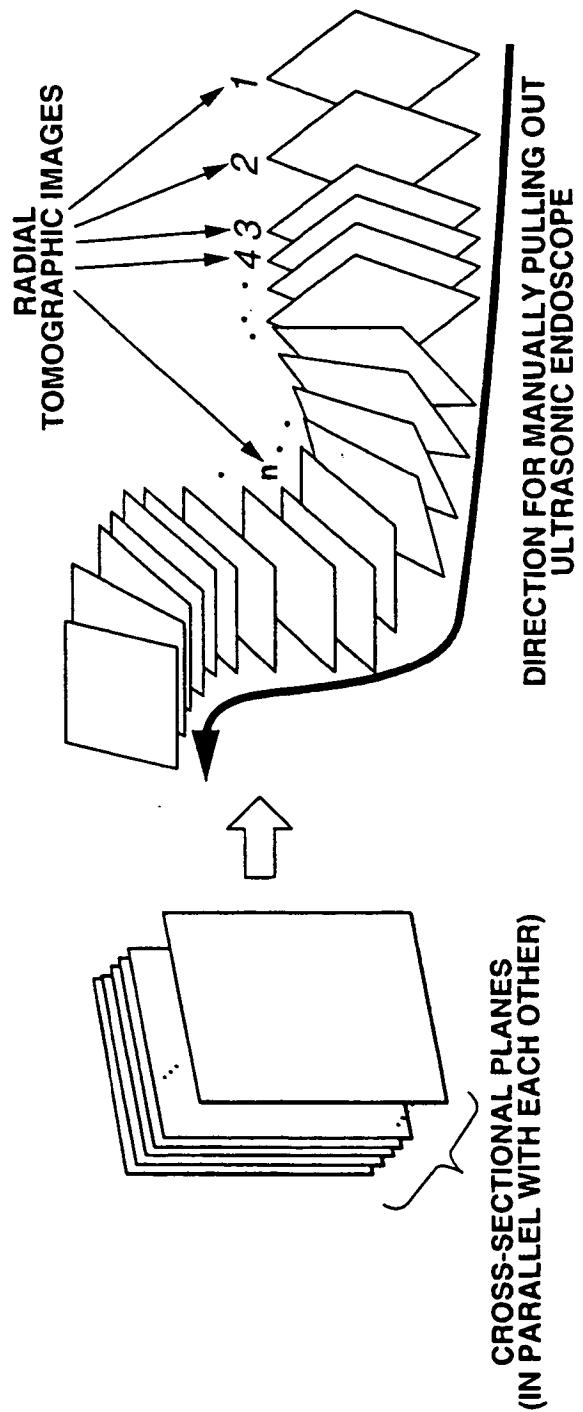


FIG. 5

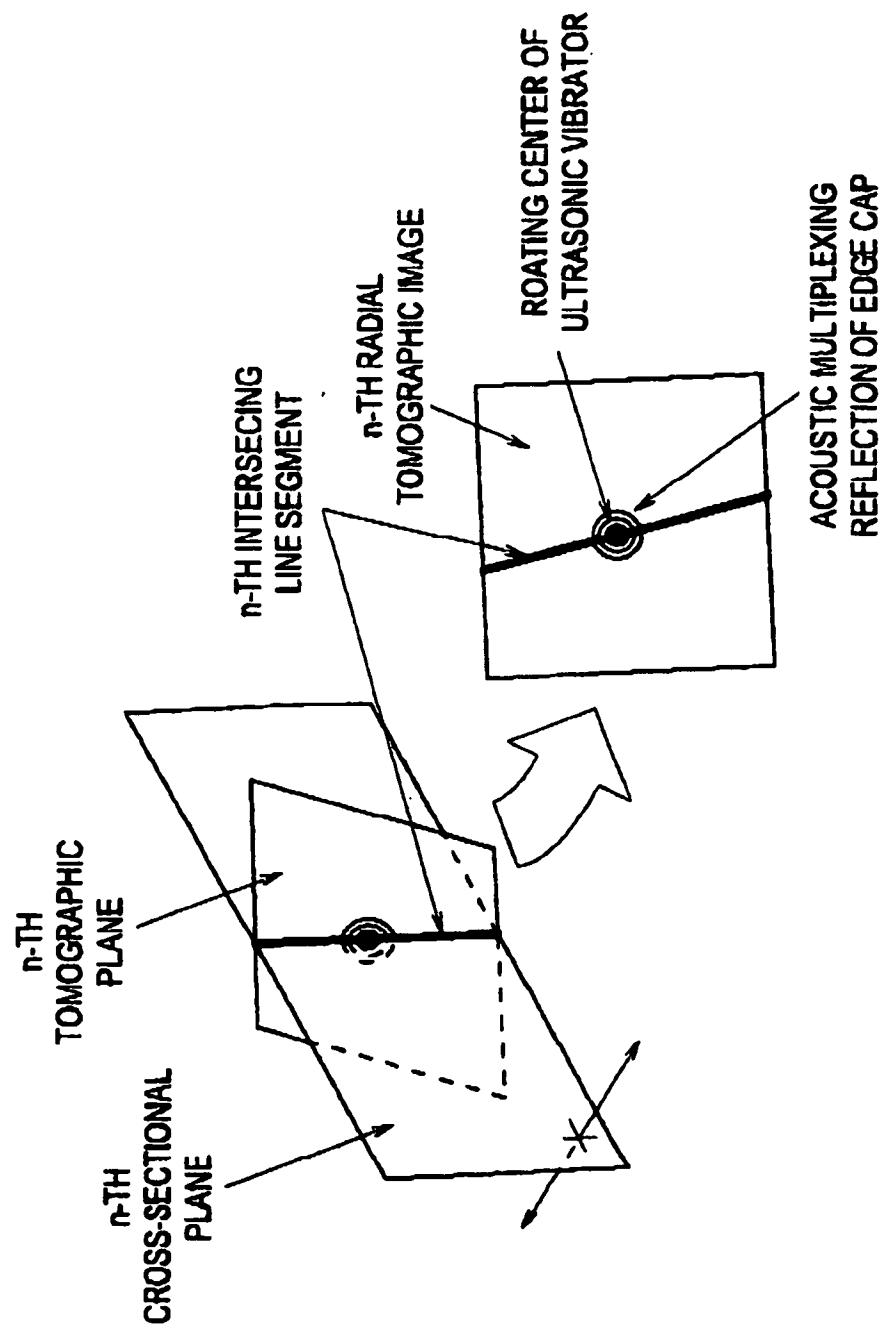


FIG.6

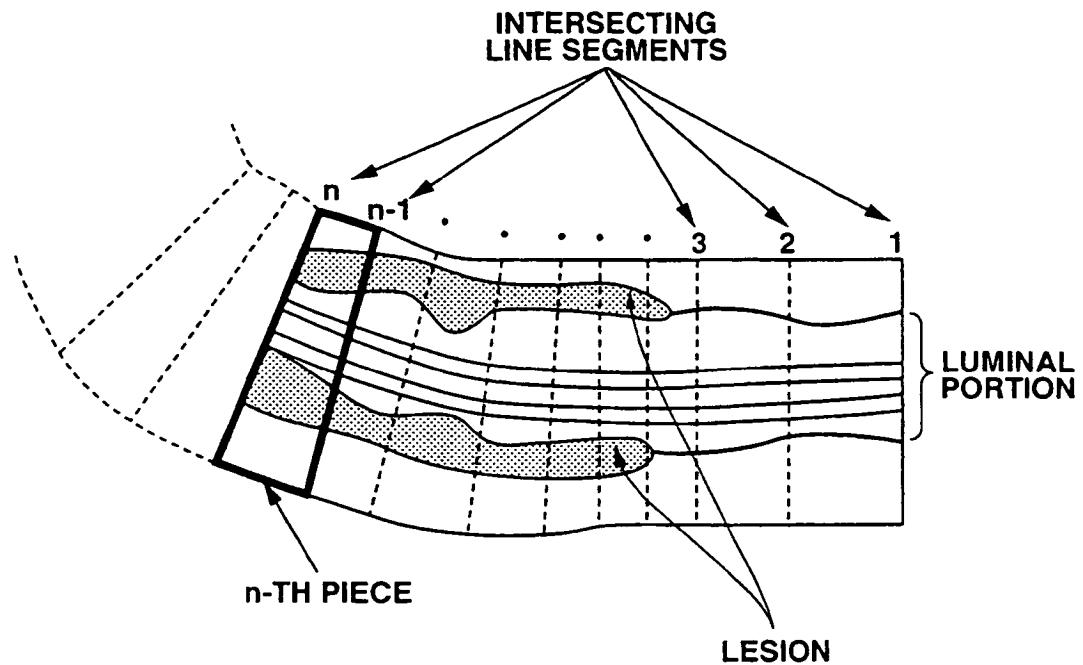


FIG.7

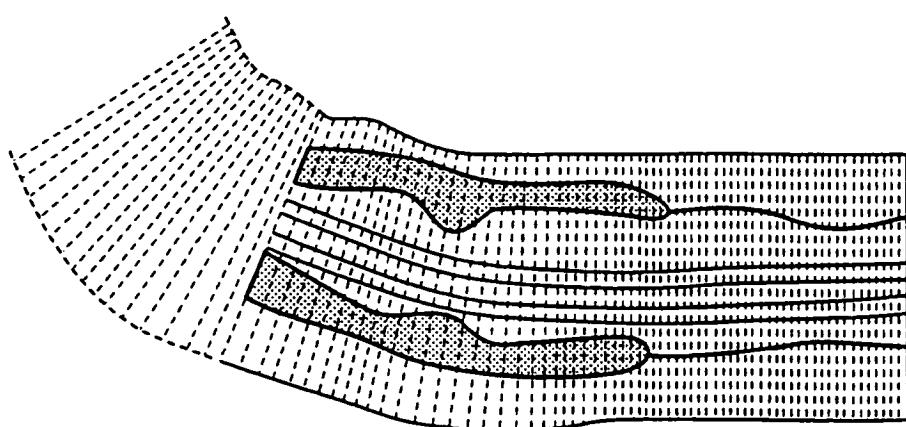


FIG.8

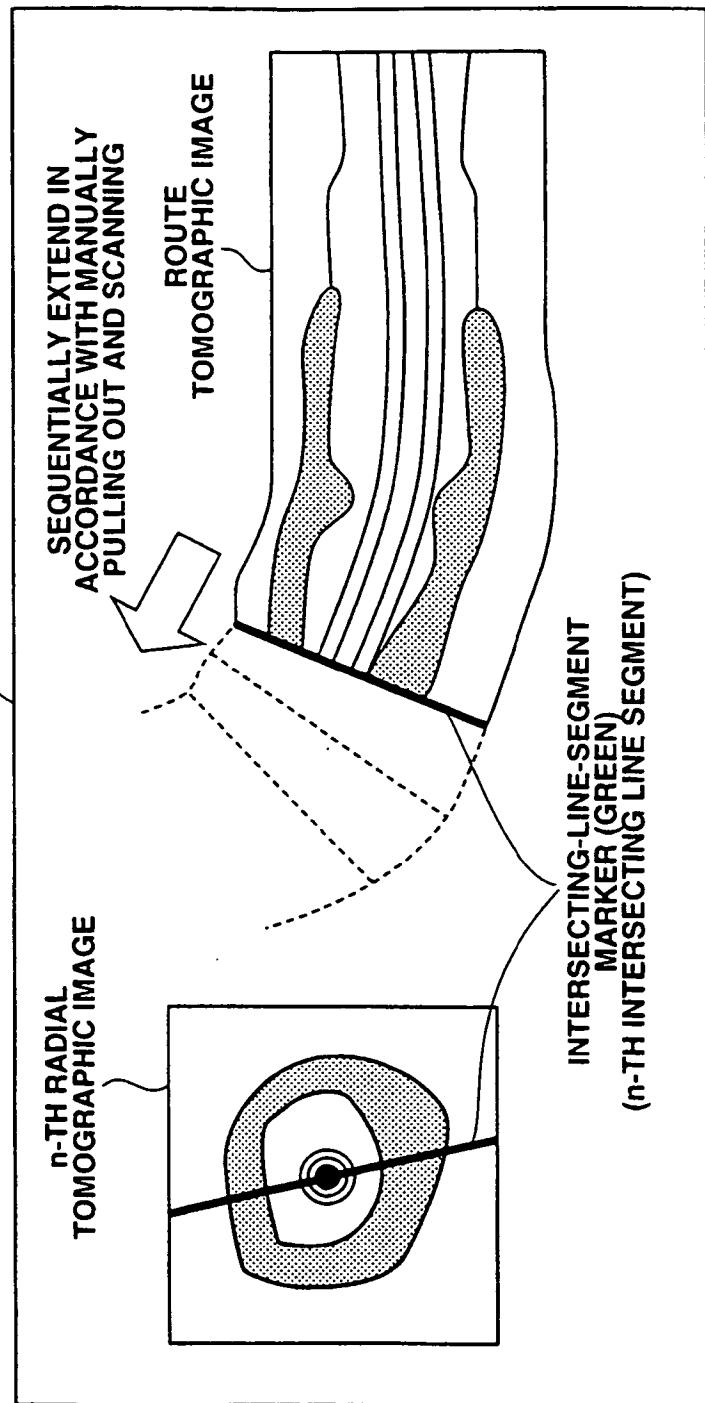


FIG.9

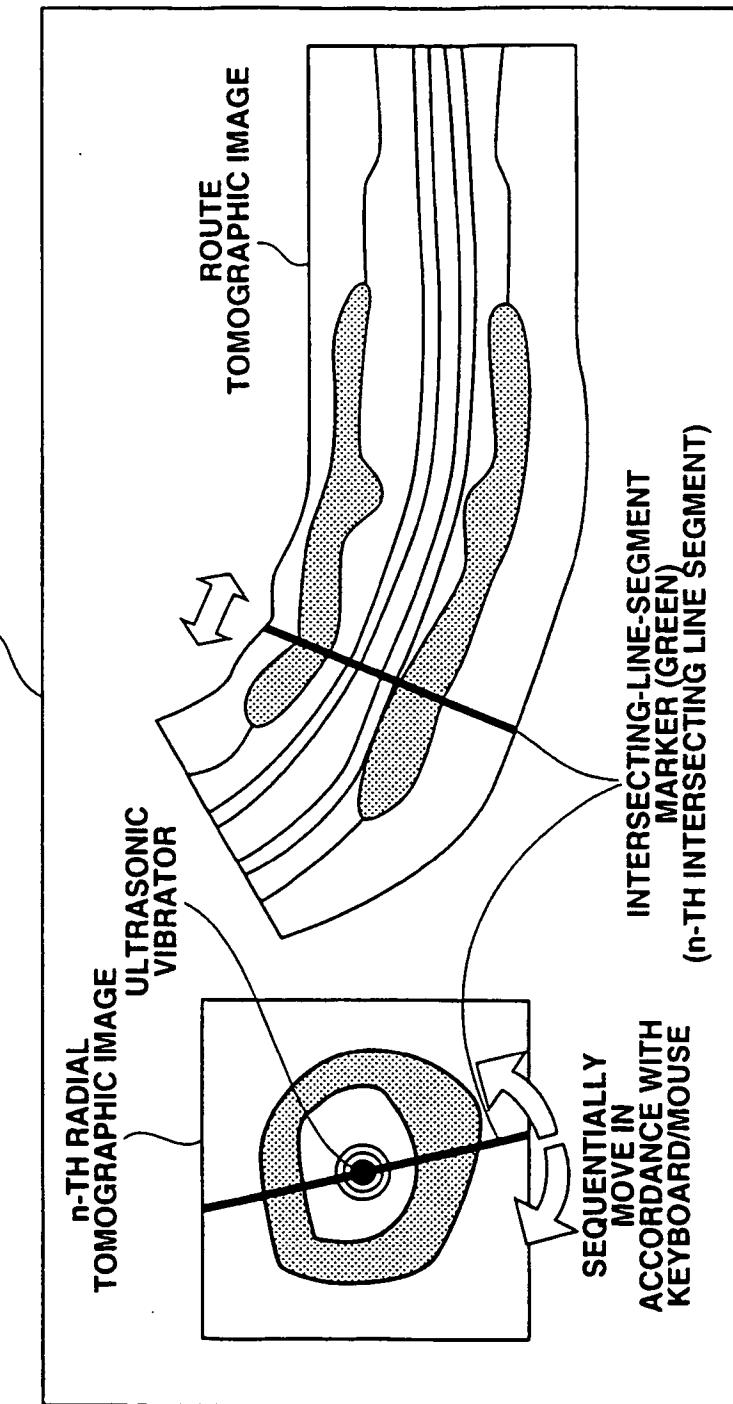


FIG.10

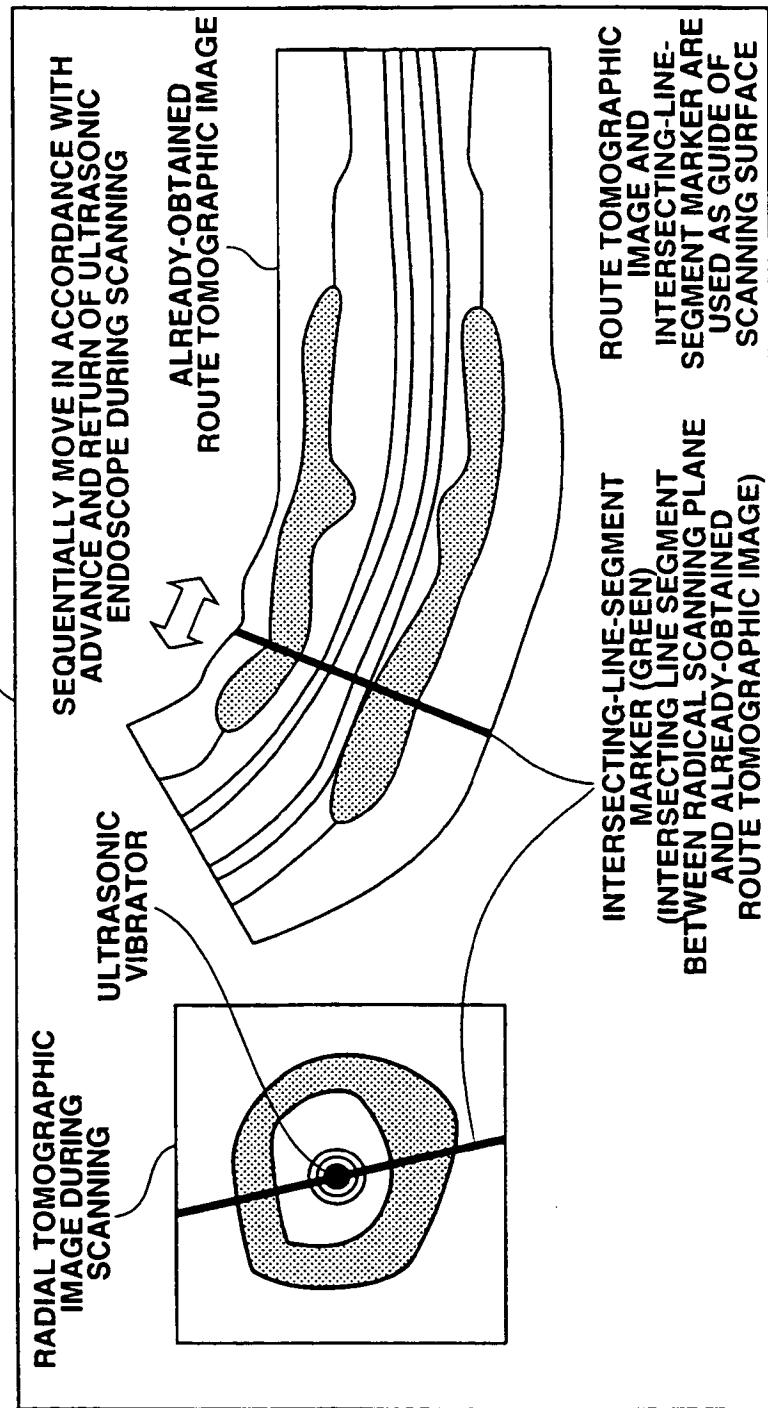


FIG.11

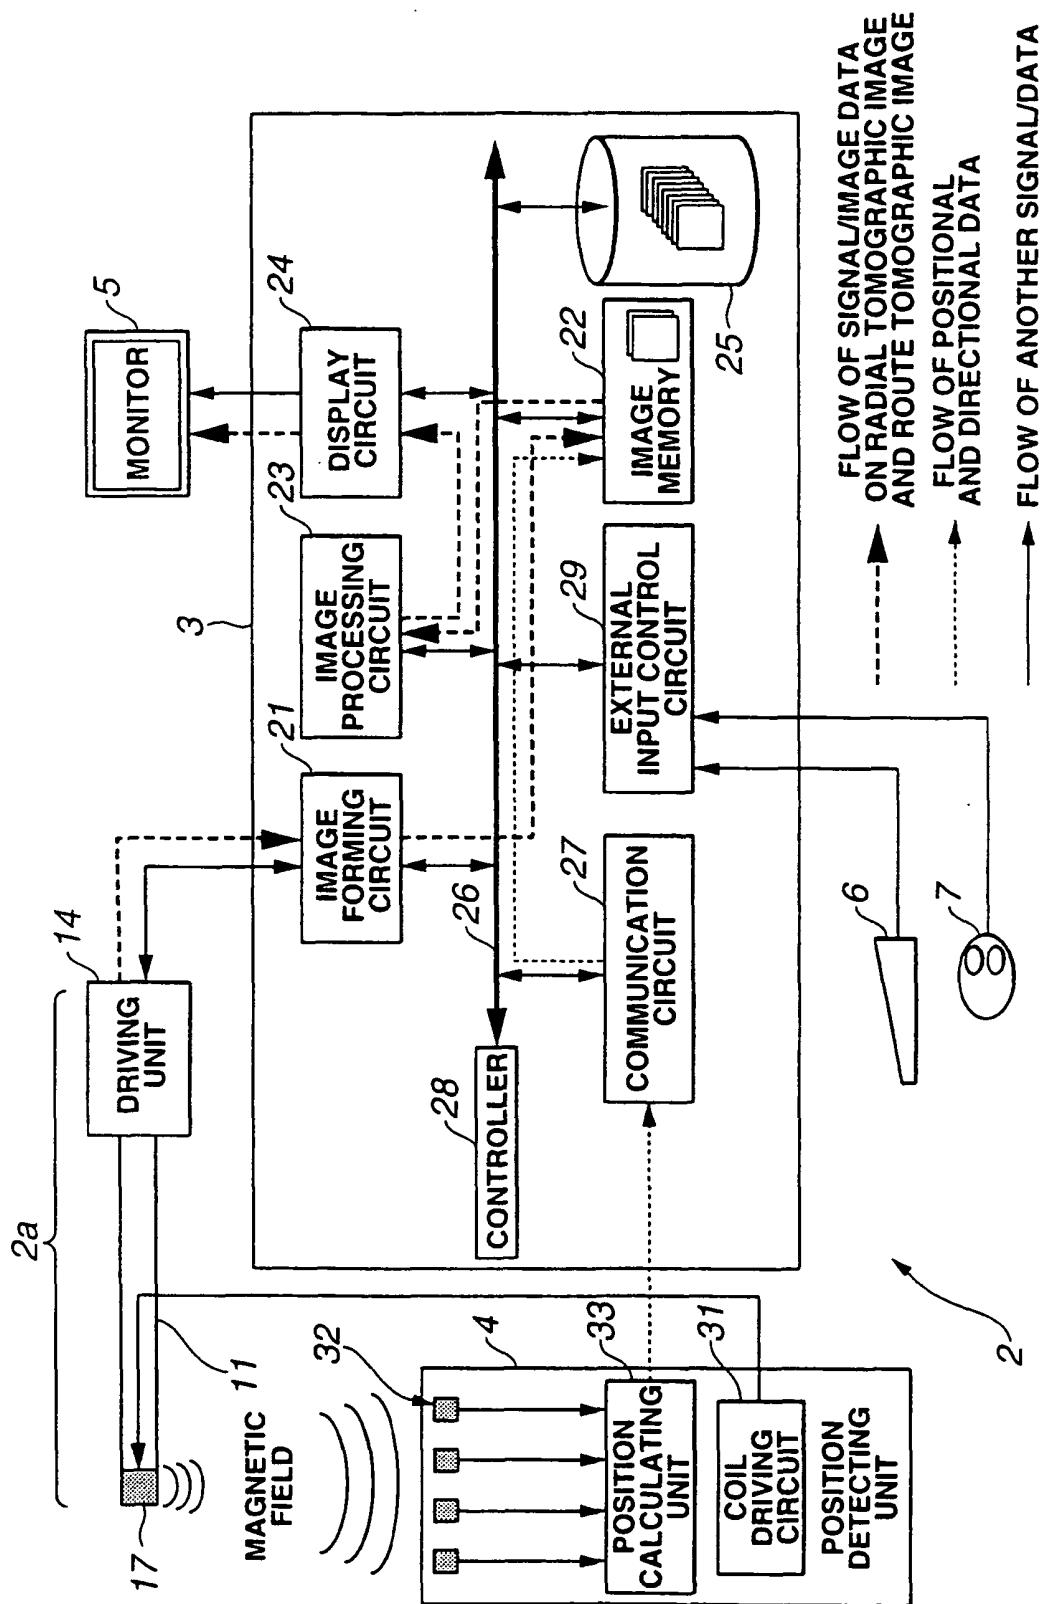


FIG.12

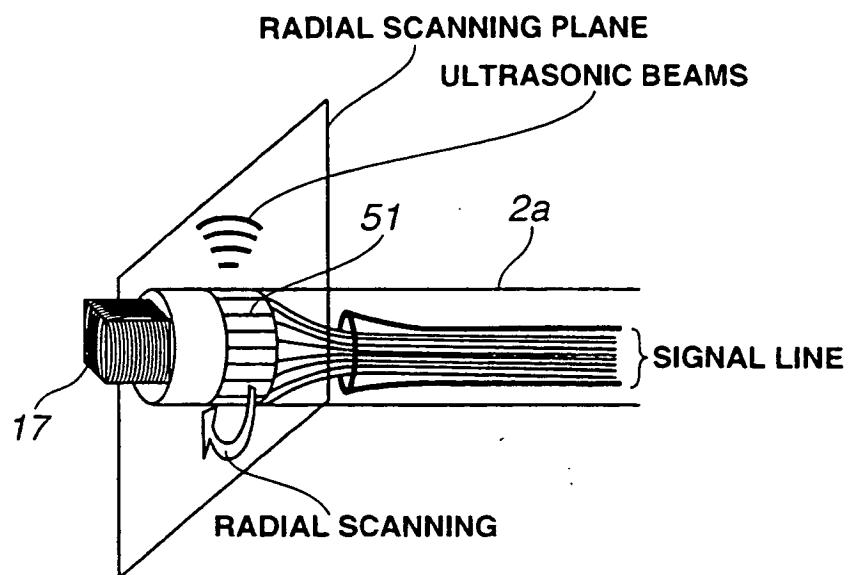


FIG.13


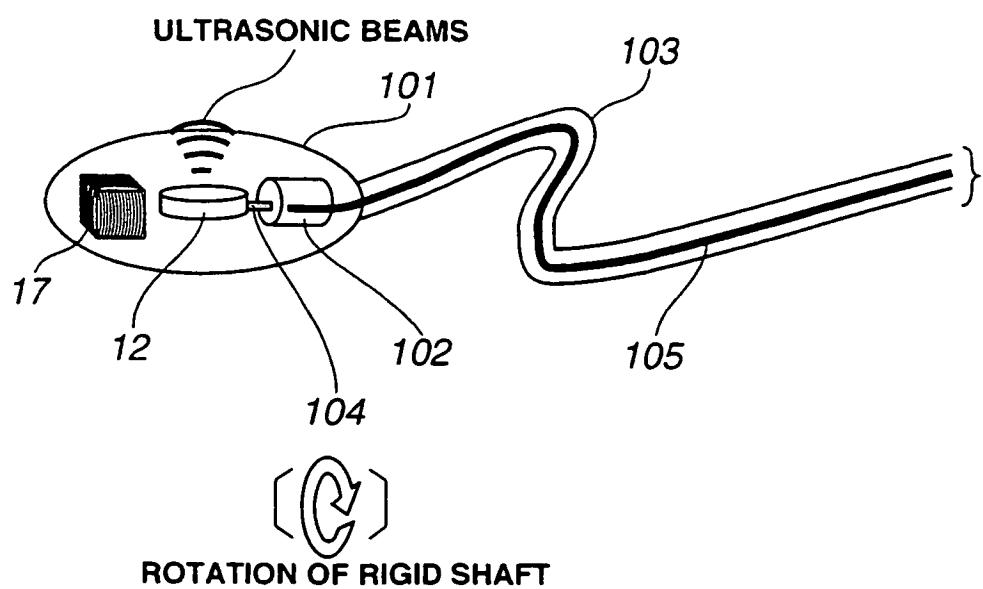


FIG.14

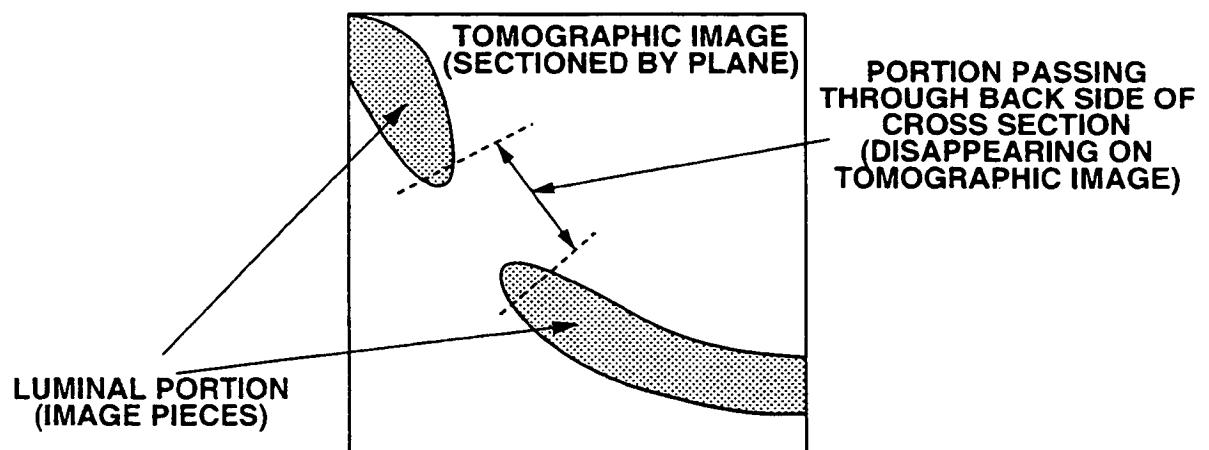

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 11113913 A [0002] [0005] [0006]
- JP 11318884 A [0003] [0004] [0009] [0010] [0011] [0013]
- JP 2000243766 A [0003] [0004] [0009] [0010] [0011] [0013]
- US 6248074 B1 [0014]

专利名称(译)	超声诊断系统		
公开(公告)号	EP1543775B1	公开(公告)日	2011-04-27
申请号	EP2003798403	申请日	2003-09-12
[标]申请(专利权)人(译)	奥林巴斯株式会社		
申请(专利权)人(译)	OLYMPUS CORPORATION		
当前申请(专利权)人(译)	OLYMPUS CORPORATION		
[标]发明人	KAWASHIMA TOMONAO		
发明人	KAWASHIMA, TOMONAO		
IPC分类号	A61B8/12 A61B8/14 G01S7/52 G01S15/89 G06T1/00		
CPC分类号	A61B8/4254 A61B8/12 A61B8/14 A61B8/145 A61B8/463 A61B8/483 A61B8/523 G01S7/52065 G01S7/52074 G01S15/8997		
优先权	2002283804 2002-09-27 JP		
其他公开文献	EP1543775A4 EP1543775A1		
外部链接	Espacenet		

摘要(译)

超声波诊断装置具有超声波内窥镜，超声波观察部分，位置检测单元，监视器，键盘和鼠标。将与其平行的横截面设置为径向断层图像，在径向断层图像和横截面之间获得交叉线段，组合交叉线段，并生成路径断层图像。通过推进和返回径向扫描超声探头，很容易识别出在检查期间病变如何沿着腔部分扩散。此外，在检查期间，可以容易地识别在管腔部分中的哪个部分是在检查期间扫描。

