

(19)



(11)

**EP 2 744 415 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**24.06.2020 Bulletin 2020/26**

(51) Int Cl.:  
**A61B 8/08 (2006.01) G06F 3/00 (2006.01)**  
**A61B 8/00 (2006.01) G06F 3/0489 (2013.01)**

(21) Application number: **12781452.3**

(86) International application number:  
**PCT/IB2012/055018**

(22) Date of filing: **21.09.2012**

(87) International publication number:  
**WO 2013/046103 (04.04.2013 Gazette 2013/14)**

(54) **ULTRASONIC DIAGNOSTIC IMAGING SYSTEM WITH CONTEXTUALLY VARIABLE CONTROL PANEL**

ULTRASCHALLDIAGNOSTIK- BILDERZEUGUNGSSYSTEM MIT EINEM KONTEXTABHÄNGIGEN BEDIENFELD

SYSTÈME D'IMAGERIE DIAGNOSTIQUE ÉCHOGRAPHIQUE AVEC PANNEAU DE COMMANDE CONTEXTUELLEMENT VARIABLE

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

(72) Inventors:  
• **CHENG, Jeanne**  
**5656 AE Eindhoven (NL)**  
• **MARK, Zsolt**  
**5656 AE Eindhoven (NL)**

(30) Priority: **29.09.2011 US 201161540586 P**

(74) Representative: **Philips Intellectual Property & Standards**  
**High Tech Campus 5**  
**5656 AE Eindhoven (NL)**

(43) Date of publication of application:  
**25.06.2014 Bulletin 2014/26**

(73) Proprietor: **Koninklijke Philips N.V.**  
**5656 AG Eindhoven (NL)**

(56) References cited:  
**EP-A1- 2 337 225 US-A1- 2009 131 793**  
**US-A1- 2009 262 085**

**EP 2 744 415 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

**[0001]** This invention relates to medical diagnostic ultrasonic imaging systems and, in particular, to ultrasound systems with control panels with controls which vary with the type of diagnostic procedure being performed.

**[0002]** Medical diagnostic ultrasound systems have control panels with many user controls for setting up and controlling the system to perform the desired imaging exam. Starting from a number of preset control parameters for a desired exam, the operator will manipulate the controls to vary the settings to those uniquely suited for the particular exam to be performed. Once the starting control parameters have been established, the exam can begin and the same and additional controls are manipulated to vary the performance of the system as the exam proceeds. For example, the operator can set the imaging mode for B mode, Doppler, or M mode. The size and angle of the image field can be changed and the frequency adjusted for fundamental or harmonic imaging. The system gain can be adjusted to more clearly distinguish anatomy at deeper depths in the body, and time gain control slides are adjusted to provide the appropriate gain over the depth of interest. Focal zones can be added and repositioned to different depths. Additional modes can be added during the exam, such as a spectral Doppler display when a Doppler gate is placed over the anatomy. A wide variety of measurements can be made of the anatomy and blood flow parameters estimated. These are but a few of the controls and adjustments available on a typical ultrasound system control panel.

**[0003]** While every ultrasound exam can require the adjustment and use of many controls on the control panel, different types of exams can require the use of a slightly different or significantly different group of controls. Thus, the control panel must contain a very large number of user controls to accommodate all the variable uses and functions of the ultrasound system. The ever-increasing number of controls has been addressed by different equipment providers in different ways. Some simply increase the number and/or density of mechanical controls on the control panel. Others augment the mechanical controls with softkey controls on the system display screen, which the user can call up and adjust and click with a computer mouse or trackball control on the control panel. Still others have employed softkey controls on a touchpanel display, which the user can manipulate and adjust manually without the need for a computer pointing device. The iU33 echocardiography system, available from Philips Healthcare of Andover, Massachusetts has all three: a fully populated mechanical control panel, softkeys on the system display screen and small touchpanels for additional user controls.

**[0004]** One approach to dealing with the large number and varying variety of controls needed for an ultrasound system is described in US Pat. 6,063,030 (Vara et al.) This patent describes a virtual control interface for an ultrasound system in which the entire control interface is

comprised of softkeys. A major portion of the display screen is devoted to the ultrasound image and a panel on the side of the screen is filled with controls which adapt to the type of and stage of an imaging exam. At the outset of the exam the side panel contains setup controls. Once the exam is underway the side panel display changes and contains controls appropriate for the type of exam. At different phases of the exam the side panel display is changed to provide controls appropriate for the particular phase of the exam. When measurements are to be made on the image, for instance, the side panel changes to display measurement controls. The user can also call up specific control sets when needed. If the user wants to annotate body markers on an anatomical model, for example, the body marker display and control panel is called up and the user annotates the graphical model, which is then saved with the results of the exam.

**[0005]** Another approach is described in US 2009131793 A1, wherein a single panel display includes a first portion configured to display an image and a second portion configured as a touch-based user interface. The touch-based user interface may be configured (dynamically changed) to display controls that may be needed to perform a particular scanning task at a time.

**[0006]** It is possible, though, for a user to become lost in the ever-changing panoply of virtual controls. A simpler, more intuitive approach to control configuration is often preferable. Moreover, some user controls are frequently used, whereas others are only needed in specific circumstances. It is further desirable for the user to have more commonly used controls readily at hand, but with the ability to call upon more specialized controls when needed. In addition, the commonly used controls should be in unvarying locations so the user can intuitively access them without having to hunt for their currently placement and location. Furthermore, these objectives should also include providing the controls needed for a particular exam while unneeded controls are removed from the user's access.

**[0007]** The invention is defined by the claims.

**[0008]** In accordance with the principles of the present invention an ultrasound system user control panel is provided in which the user controls needed for a particular ultrasound exam are available for use and unneeded controls are hidden from the user and neither available nor distracting to the user. The user controls on the control panel are in fixed physical locations on the control panel so that the user will always find a given control at the same place on the panel. In a constructed embodiment available user controls are illuminated and visible to the user and controls not necessary in the context of a current exam are darkened and invisible. All of the controls are touch actuated and located beneath a continuous surface, a dark glass plate, so that there are no crevices or projections to trap dust and acoustic gel. The continuous surface enables the control panel to be easily cleaned for patient and operator health and safety. The controls can all be turned off by a switch while the ultra-

sound system is still powered on, in which case none will be accidentally actuated when the control panel surface is being cleaned.

**[0009]** In the drawings:

FIGURE 1 illustrates a cart-borne ultrasound system of the prior art.

FIGURE 2 illustrates a portable ultrasound system constructed in accordance with the principles of the present invention.

FIGURE 3 is a block diagram of an ultrasound system constructed in accordance with the principles of the present invention.

FIGURE 4 illustrates a contextually variable ultrasound system control panel constructed in accordance with the principles of the present invention.

FIGURE 5 illustrates the control panel of FIGURE 4 when the controls have been inactivated for cleaning the control panel.

FIGURE 6 is an internal view of the control panel of FIGURE 4.

FIGURE 6a is a cross-sectional view of the control panel of FIGURES 4-6.

**[0010]** Referring first to FIGURE 1, a typical cart-borne ultrasound system of the prior art is shown. The ultrasound system includes a mainframe or chassis 60 containing most of the electronic circuitry for the system. The chassis 60 is wheel-mounted so that it can be rolled to the location in a hospital or clinic where it is to be used. An image display 62 is mounted on the chassis 60. A variety of imaging probes may be plugged into three connectors 64 on the chassis. Mounted at the front of the chassis 60 is a control panel 66 with a keyboard and controls arrayed over the surface of the control panel, by which a sonographer operates the ultrasound system and enters information about the patient or the type of examination that is being conducted. At the back of the control panel 66 of the illustrated ultrasound system is a touchscreen display 68 on which programmable softkeys are displayed for specific control functions. The sonographer selects a softkey on the touchscreen display 18 simply by touching the image of the softkey on the display. At the bottom of the touchscreen display is a row of control knobs, the functionality of which varies in accordance with the softkey labels on the touchscreen immediately above each button. At the front of the control panel is a trackball which the sonographer manipulates to indicate anatomy of the ultrasound image on the image display 62, and to steer a pointer or cursor on the screen to indicate a softkey on the display screen, which is selected by clicking a button adjacent to the trackball. Above and around the trackball are a variety of switches, buttons, and knobs which the sonographer manipulates to adjust the imaging parameters of the ultrasound system such as a signal gain knob, time gain control slide switches, and save and print buttons. The many knobs, buttons, and switches of the control panel make cleaning difficult,

as dust and acoustic gel can easily become trapped around and under the controls.

**[0011]** FIGURE 2 illustrates a portable ultrasound system of the present invention. The electronics of the ultrasound system are located in a base 80 between the wheels of the system. A central column 76 supports the control panel 40 and the image display 62 at the top of the column. The upper portion of the column 76 may be configured to move up and down with respect to the lower portion of the column so that the height of the control panel and display screen may be adjusted. The connectors for three probes are located on the lower portion of the column. The control panel has no knobs, buttons, switches or other projections but has a continuous smooth dark planar surface of plastic or preferably glass. The flat, smooth glass surface of the control panel will not trap dust, gel or debris.

**[0012]** A functional block diagram of the ultrasound system of FIGURE 2 is illustrated in FIGURE 3. The ultrasound system operates through two major subsystems, a front end acquisition subsystem 10A and a display subsystem 10B. An ultrasound probe is coupled to the acquisition subsystem to transmit ultrasound waves and receive ultrasound echo signals. The probe may do this with a linear (one-dimensional) row of transducer elements, or may use a two-dimensional matrix array of transducer elements 70 and a micro-beamformer 72 located in the probe. The micro-beamformer contains circuitry which controls the signals applied to groups of elements of the array transducer 70 and does some processing of the echo signals received by elements of each group. Micro-beamforming in the probe advantageously reduces the number of conductors in the cable between the probe and the ultrasound system and is described in US Pat. 5,997,479 (Savord et al.) and in US Pat. 6,436,048 (Pesque), and provides electronic steering of beams on transmit and receive for high frame rate real-time (live) imaging.

**[0013]** The probe is coupled to the acquisition subsystem 10A of the ultrasound system. The acquisition subsystem includes a beamform controller 74 which is responsive to controls of the control panel 40 and provides control signals to the microbeamformer 72, instructing the probe as to the timing, frequency, direction and focusing of transmit and receive beams. The beamform controller also control the beamforming of echo signals received by the acquisition subsystem by its control of analog-to-digital (A/D) converters 18 and a beamformer 20. Partially beamformed echo signals received by the probe are amplified by preamplifier and TGC (time gain control) circuitry 16 in the acquisition subsystem, then digitized by the A/D converters 18. The digitized echo signals are formed into fully steered and focused beams by a main system beamformer 20. The echo signals are processed by an image processor 22 which performs digital filtering, B mode and M mode detection, and Doppler processing, and can also perform other signal processing such as harmonic separation, speckle reduction, and oth-

er desired image signal processing.

**[0014]** The echo signals produced by the acquisition subsystem 10A are coupled to the display subsystem 10B, which processes the echo signals for display in the desired image format on the display screen 62. The echo signals are processed by an image line processor 24, which is capable of sampling the echo signals, splicing segments of beams into complete line signals, and averaging line signals for signal-to-noise improvement or flow persistence. The image lines for a 2D image are scan converted into the desired image format by a scan converter 26 which performs R-theta conversion as is known in the art. The scan converter can thus format rectilinear or sector image formats. The image is then stored in an image memory 28 from which it can be displayed on the display 62. The image in memory is also overlaid with graphics to be displayed with the image, which are generated by a graphics generator 34 which is responsive to the user control 40 so that the graphics produced are associated with the images of the display. Individual images or image sequences can be stored in a cine memory 30 during capture of image loops or sequences. Images for diagnosis can be stored on a networked image memory 128.

**[0015]** For real-time volumetric imaging the display subsystem 10B also includes a 3D image rendering processor 32 which receives image lines from the image line processor 24 for the rendering of real-time three dimensional images. The 3D images can be displayed as live (real time) 3D images on the display 38 or coupled to the image memory 128 for storage of the 3D data sets for later review and diagnosis.

**[0016]** An ECG subsystem is provided for use when it is desirable to acquire images at particular phases of the heart cycle. ECG leads 50 provide ECG signals for a QRS processor 52 which identifies the R-wave of each heartbeat. The timing of the R-wave is used to acquire images of a particular heart cycle. Images of the heart at the end diastole phase of a succession of heartbeats can be acquired by coupling the R-wave timing as a trigger signal from a trigger signal generator 54 for the beamform controller 74 and the controls of the control panel 40 used to select the desired heart phase at which heart phase-gated images are to be acquired.

**[0017]** In accordance with the principles of the present invention, the ultrasound system of FIGURES 2 and 3 contains a context-variable control panel 40 as shown in FIGURES 4, 5, 6, and 6a. The upper layer of the control panel is a flat sheet of optically transparent material. The upper layer can be formed by a sheet of plastic or other polymer, but preferably is formed by a sheet of glass 42 so as to be more resistant to scratches and more impervious to solvents that may be found in a hospital. The glass sheet 42 presents a smooth, uniform surface on the top of the control panel. The underside 44 of the glass sheet 42 is painted a dark opaque color such as black or charcoal, except in locations where control graphics are screened on the back surface. The screening is a trans-

parent or translucent color which outlines the individual control area as shown in FIGURE 4. Within the control outline is text or a graphic symbol which identifies the function controlled by the specific control. The graphics may also be adjacent to a control as shown for the Baseline, Scale/Focus, Depth and Gain controls. Capacitive foils 46 are adhesively attached to the back of the screened glass which are sensitive to the touch of an operator on the glass above a particular foil. The touch by an operator on the area of a graphically-delineated control produces a capacitive change which is sensed by the underlying foil and coupled to the control panel electronics on a printed circuit board 82 below the glass sheet 42 and foils 46. Electrical conductors between the control areas connect individual foils to circuitry on the printed circuit board, which sends a control signal to the ultrasound system electronics in response to the sensing of a touch on a control area by the system operator.

**[0018]** The glass sheet with its screened graphics and capacitive foils is adhered to a white barrier layer 48 which in turn is fastened to the printed circuit board 82 on the other side of the white barrier layer. The white barrier layer 48 contains depressions or pockets such as 92 behind the areas of specific controls. Light sources such as LEDs 94 mounted on the underlying printed circuit board extend into these depressions or pockets from below and fill a pocket with light when the LED or LEDs in the pocket are illuminated. The surrounding area of the white barrier layer contacts the painted glass plate around each control area (or the capacitive foil layer laminated to the glass plate), confining the light of the LED in the depression (light chamber) to the area of the specific control. A depression in the barrier layer 48 thus forms a diffuser frame with light chambers which distribute the light of an LED over the graphics of a specific control and pipes the light to the control graphic, while the peripheral contact with the glass plate prevents the light from the specific control from bleeding into the area of an adjacent control. In a constructed embodiment the white barrier layer is not a unitary structure but is formed of sections which fit together with gaps 98 between the sections. The capacitive foils or foil conductors extend through these gaps to electrically connect to the underlying printed circuit board 82. Technologies suitable for constructing a control panel as described herein are available from RAFI GmbH & Co. KG, Ravensburg, Germany.

**[0019]** In a constructed example, the light chambers generally include multiple LED light sources of different colors. When a control is not to be used for a specific diagnostic procedure, none of the LEDs of the control area are illuminated and the light chamber is dark, causing the control to be virtually invisible to the ultrasound system operator. If the ultrasound system is not operating in the PW or CW mode, for example, the Baseline control slider is darkened and unavailable to the operator. The operator is thus presented with only those controls which are applicable to the current ultrasound system mode or

procedure. In the constructed example, controls which are available in the current mode or procedure are illuminated by white LEDs to indicate their availability. When the operator selects a control in a particular procedure, the control is illuminated by an amber LED to indicate that it is active. For example, the operator may be conducting a diagnostic procedure in which 2D images in grayscale are being acquired, but can also acquire the 2D images with colorflow indication of blood flow. The 2D button will be illuminated in amber at this time to show that the 2D mode is in use, and the Color button is illuminated in white to indicate that colorflow imaging is available in this procedure. If the operator then selects the Color button, colorflow imaging will commence and the Color button will change to an amber color to show the selection of the colorflow function.

**[0020]** As another example, the operator may be performing 3D imaging. If it is possible to switch immediately to 2D imaging, the 2D control will be illuminated in white to indicate the availability of the 2D imaging mode, and pressing the 2D control will change the system operation immediately to 2D imaging.

**[0021]** In the constructed control panel, different controls operate differently in response to different gestures or touches. The Color control is a simple on/off button, for example. When it is touched the first time it turns amber and is on; when it is touched again it turns back to white and is off but available for subsequent use. The 2D mode is a default mode and thus the 2D control is generally amber; it is rarely white. The four controls above the 2D button in FIGURE 4, the Baseline, Scale/Focus, Depth and Gain controls, operate control functions which can be progressively increased or decreased. Repeatedly tapping the arrow at the top of the Gain control will progressively increase the gain of the signal amplifier in the system. Repeatedly tapping the arrow at the bottom of the Gain control will stepwise reduce the gain. The TGC controls to the right of the Gain control can be constructed to operate in a similar manner, or may be constructed as a series of individual lights and buttons. When the operator touches a different graphic dot on a TGC control, the touched dot will illuminate more brightly or in a different color, and the gain applied by that particular control will change in accordance with the location of the touched dot in the row of dots.

**[0022]** The touchpad 46 in the lower center of the control panel in FIGURES 4 and 6 can be operated in the manner of the trackball of a typical mechanical control panel. The operator can slide his or her finger around in the delineated touchpad area, causing a cursor or pointer on the display screen to be positionally controlled correspondingly. To select a screen function indicated by the cursor or pointer, the operator can touch one of the button areas immediately above the touchpad area, or can tap or double tap on the touchpad to select the indicated function.

**[0023]** FIGURE 4 illustrates a constructed control panel of the present invention when all of the controls are

illuminated and available. In practice, this is usually not the case. When the system operator selects an imaging mode or a specific imaging procedure or exam, as by selecting a mode or procedure from a list of selections on the display screen 62, the system will actuate and illuminate only those controls which are applicable to the selected mode or exam. Controls which have no use in the context of the selected mode or exam are not illuminated and are invisible to the operator. The operator will thus not be distracted by non-useful controls on a busy control panel. Instead, the operator's attention will be focused on only those controls which are useful for the current procedure.

**[0024]** The positions and the identified functions of the controls in the example of FIGURE 4 are fixed, both by the fixed graphics behind the glass top and the fixed positions of the illuminated diffuser regions and light pipes behind them. With specific controls being in fixed positions, an operator will quickly become familiar with their positions and access them instinctively. An operator will not have to stop and wonder where a control may have been repositioned, which is often the case with scanned softkey displays. The operator soon becomes comfortable and efficient when using the control panel with its fixed control positions.

**[0025]** FIGURE 5 illustrates the control panel of FIGURE 4 when all of the ultrasound controls have been extinguished and turned off. This may be done by the on/off control 100 shown in the upper left-hand corner of the control panel. Alternatively, all of the controls may be de-activated and extinguished by a switch located on another part of the ultrasound system, such as on the display 62. An ultrasound system control panel can frequently need cleaning after being continuously touched by an operator during a series of exams. The control panel can also be marred by acoustic gel used by the operator to provide good acoustic coupling from the probe to the patient's body. If some of the controls were active during cleaning, the act of cleaning would unavoidably actuate controls on the panel, which is undesirable. An on/off control 100 is used to de-activate all of the controls on the panel, which is visually indicated by the lack of illumination of the controls. The control panel may then be cleaned without randomly actuating control panel controls.

**[0026]** Cleaning the glass sheet forming the top of the control panel is easy and efficient, as the smooth top has no projections or crevices which trap debris and make cleaning difficult, as is the case with the typical mechanical control panel of knobs, buttons, and switches of the prior art. More comfortable and safer working conditions are thus afforded to both the operator and patient.

## 55 Claims

1. A diagnostic ultrasound system which is selectively operable in one of a plurality of operating modes for

the conduct of one of a plurality of different imaging procedures comprising:

a connector for connecting an ultrasound probe to the system for use in imaging;  
 an image display screen; and  
 a touch-sensitive user control panel (40) comprising a smooth top surface formed by a sheet of transparent material (42),  
 wherein the control panel further comprises a plurality of control graphics located on the underside (44) of the sheet at fixed positions corresponding to positions of touch-actuated user controls provided by the control panel in use, the control graphics being surrounded by a dark opaque color,  
 a barrier layer (48) below the control graphics, having pockets or depressions behind areas of each of the different user controls, the pockets or depressions defining illumination areas confined to said fixed positions of the user controls, the illumination areas containing selectively illuminated light sources (94), and an illumination controller coupled to the light sources,  
 wherein the light sources for illuminating different groups of user controls are controlled to be illuminated during different operating modes or imaging procedures in accordance with the need for the controls during a selected mode or procedure, with the illumination of unneeded user controls being extinguished such that the unneeded controls are substantially invisible to a user by reason of the dark opaque color.

2. The diagnostic ultrasound system of Claim 1, wherein the dark opaque color is black.
3. The diagnostic ultrasound system of Claim 2, wherein the sheet of transparent material further comprises a glass sheet, the control graphics being screened onto the underside of the glass sheet and being surrounded by black paint.
4. The diagnostic ultrasound system of Claim 3, further comprising a plurality of capacitive foils (46) attached to the glass sheet at locations of control graphics for the capacitive actuation of controls by a user.
5. The diagnostic ultrasound system of Claim 1, wherein each of the pockets or depressions contacts the periphery of a corresponding user control above the barrier layer to confine light in a given pocket or depression to the user control above it.
6. The diagnostic ultrasound system of Claim 5, wherein the barrier layer further comprises a diffuser frame and light pipes for the user controls.

7. The diagnostic ultrasound system of Claim 5, wherein the light sources further comprise LEDs located in the pockets or depressions.
8. The diagnostic ultrasound system of Claim 7, wherein the illumination controller further comprises a printed circuit board fastened to the barrier layer, wherein the LEDs are electrically coupled to the printed circuit board and the illumination of the LEDs is controlled by the printed circuit board.
9. The diagnostic ultrasound system of Claim 7, wherein the light sources further comprise LEDs of different colors located in the same pocket or depression, wherein the different colors are used to illuminate the user control in accordance with a state of the function of the user control.
10. The diagnostic ultrasound system of Claim 9, wherein the states of the user control is available or active.
11. The diagnostic ultrasound system of Claim 1, further comprising a switch coupled to the user control panel, wherein the switch is actuated to extinguish the illumination of substantially all of the user controls during cleaning of the top surface of the control panel.
12. The diagnostic ultrasound system of Claim 11, wherein actuation of the switch to extinguish the illumination further acts to de-activate the users controls from their control functionality.
13. The diagnostic ultrasound system of Claim 11, wherein the switch is located at a position on the ultrasound system other than the top surface of the control panel.
14. The diagnostic ultrasound system of Claim 12, wherein actuation of the switch to extinguish the illumination causes the user controls and their surrounding areas of the control panel to appear black.
15. The diagnostic ultrasound system of Claim 1, wherein one of the user controls further comprises a capacitive touchpad located forward of the center of the control panel toward a position of a user, the touch surface above the touchpad comprising the top surface of the control panel which is continuous with the touch surface of a majority of other user controls of the control panel.

#### Patentansprüche

1. Diagnostisches Ultraschallsystem, das selektiv in einer von mehreren Betriebsarten zur Durchführung eines von mehreren verschiedenen bildgebenden

Verfahren betreibbar ist, umfassend Folgendes:

einen Anschluss zur Verbindung einer Ultraschallsonde mit dem System zur Verwendung in der Bildgebung;  
einen Bildschirm; und  
ein berührungsempfindliches Benutzer-Bedienfeld (40) mit einer glatten Oberseite, die durch eine Folie aus transparentem Material (42) gebildet wird,  
wobei das Bedienfeld ferner Folgendes umfasst:

eine Vielzahl von Steuergrafiken, die auf der Unterseite (44) des Blattes an festen Positionen angeordnet sind, die den Positionen von berührungsbetätigten Benutzersteuerungen entsprechen, die durch das verwendete Bedienfeld bereitgestellt werden, wobei die Steuergrafiken von einer dunklen, undurchsichtigen Farbe umgeben sind,  
eine Sperrschicht (48) unter der Steuergrafik, die Taschen oder Vertiefungen hinter Bereichen jeder der verschiedenen Benutzersteuerungen aufweist, wobei die Taschen oder Vertiefungen Beleuchtungsbereiche definieren, die auf die festen Positionen der Benutzersteuerungen beschränkt sind, wobei die Beleuchtungsbereiche selektiv beleuchtete Lichtquellen (94) enthalten, und eine mit den Lichtquellen gekoppelte Beleuchtungssteuerung,  
wobei die Lichtquellen zur Beleuchtung verschiedener Gruppen von Benutzersteuerungen so gesteuert werden, dass sie während verschiedener Betriebsmodi oder Abbildungsverfahren entsprechend des Bedarfs der Steuerungen während eines ausgewählten Modus oder Verfahrens beleuchtet werden, wobei die Beleuchtung nicht benötigter Benutzersteuerungen so ausgelöscht wird, dass die nicht benötigten Steuerungen aufgrund der dunklen, undurchsichtigen Farbe für einen Benutzer im Wesentlichen unsichtbar sind.

2. Diagnostisches Ultraschallsystem nach Anspruch 1, wobei die dunkle, opake Farbe schwarz ist.
3. Diagnostisches Ultraschallsystem nach Anspruch 2, bei dem das Blatt aus transparentem Material ferner eine Glasplatte umfasst, wobei die Kontrollgrafiken auf die Unterseite der Glasplatte gerastert und von schwarzer Farbe umgeben sind.
4. Diagnostisches Ultraschallsystem nach Anspruch 3 ferner umfassend eine Vielzahl von kapazitiven Fo-

lien (46), die an der Glasscheibe an Stellen von Kontrollgrafiken für die kapazitive Betätigung von Bedienelementen durch einen Benutzer angebracht sind.

- 5 5. Diagnostisches Ultraschallsystem nach Anspruch 1, bei dem jede der Taschen oder Vertiefungen die Peripherie einer entsprechenden Benutzersteuerung oberhalb der Sperrschicht berührt, um das Licht in einer bestimmten Tasche oder Vertiefung auf die Benutzersteuerung darüber zu beschränken.
- 10 6. Diagnostisches Ultraschallsystem nach Anspruch 5, wobei die Sperrschicht ferner einen Diffusorrahmen und Lichtleiter für die Benutzersteuerung umfasst.
- 15 7. Diagnostisches Ultraschallsystem nach Anspruch 5, bei dem die Lichtquellen ferner aus LEDs bestehen, die sich in den Taschen oder Vertiefungen befinden.
- 20 8. Diagnostisches Ultraschallsystem nach Anspruch 7, wobei die Beleuchtungssteuerung ferner eine an der Sperrschicht befestigte Leiterplatte umfasst, wobei die LEDs elektrisch mit der Leiterplatte gekoppelt sind und die Beleuchtung der LEDs durch die Leiterplatte gesteuert wird.
- 25 9. Diagnostisches Ultraschallsystem nach Anspruch 7, wobei die Lichtquellen ferner LEDs unterschiedlicher Farben aufweisen, die sich in derselben Tasche oder Vertiefung befinden, wobei die unterschiedlichen Farben verwendet werden, um die Benutzersteuerung gemäß einem Zustand der Funktion der Benutzersteuerung zu beleuchten.
- 30 10. Diagnostisches Ultraschallsystem nach Anspruch 9, bei dem die Zustände der Benutzerkontrolle verfügbar oder aktiv sind.
- 35 11. Diagnostisches Ultraschallsystem nach Anspruch 1, ferner mit einem Schalter, der mit dem Bedienfeld des Benutzers gekoppelt ist, wobei der Schalter betätigt wird, um die Beleuchtung von im Wesentlichen allen Bedienelementen des Benutzers während der Reinigung der oberen Oberfläche des Bedienfelds auszulöschen.
- 40 12. Diagnostisches Ultraschallsystem nach Anspruch 11, bei dem die Betätigung des Schalters zum Auslösen der Beleuchtung weiterhin dazu dient, die Bedienelemente des Benutzers von ihrer Steuerfunktionalität abzuschalten.
- 45 13. Diagnostisches Ultraschallsystem nach Anspruch 11, bei dem sich der Schalter an einer anderen Stelle des Ultraschallsystems als an der Oberseite des Bedienfelds befindet.
- 50 14. Diagnostisches Ultraschallsystem nach Anspruch

12, bei dem die Betätigung des Schalters zum Auslösen der Beleuchtung dazu führt, dass die Bedienelemente des Benutzers und die sie umgebenden Bereiche des Bedienfeldes schwarz erscheinen.

15. Diagnostisches Ultraschallsystem nach Anspruch 1, bei dem eine der Benutzersteuerungen ferner ein kapazitives Berührungsfeld aufweist, das vor der Mitte des Bedienfeldes in Richtung einer Position eines Benutzers angebracht ist, wobei die Berührungsfläche über dem Berührungsfeld die obere Fläche des Bedienfeldes umfasst, die mit der Berührungsfläche einer Mehrheit anderer Benutzersteuerungen des Bedienfeldes zusammenhängend ist.

### Revendications

1. Système de diagnostic par ultrasons pouvant fonctionner sélectivement dans l'un d'une pluralité de modes de fonctionnement pour la conduite de l'une d'une pluralité de procédures d'imagerie différentes, comprenant :

un connecteur pour connecter une sonde à ultrasons au système pour une utilisation en imagerie ;

un écran d'affichage d'image ; et

un panneau de commande utilisateur (40) tactile comprenant une surface supérieure lisse formée par une feuille de matière transparente (42),

dans lequel le panneau de commande comprend en outre une pluralité de graphiques de commande situés sur une face inférieure (44) de la feuille à des positions fixes correspondant à des positions des commandes utilisateur actionnées par le toucher fournies par le panneau de commande en cours d'utilisation, les graphiques de commande étant entourés d'une couleur opaque sombre,

une couche barrière (48) au-dessous des graphiques de commande, comportant des poches ou des dépressions derrière les zones de chacune des différentes commandes utilisateur, lesdites poches ou dépressions définissant des zones d'éclairage confinées auxdites positions fixes des commandes utilisateur, lesdites zones d'éclairage contenant des sources lumineuses (94) sélectivement éclairées, et un dispositif de commande d'éclairage couplé aux sources lumineuses,

dans lequel les sources lumineuses pour éclairer différents groupes de commandes utilisateur sont commandées pour être éclairées pendant différents modes de fonctionnement ou pendant différentes procédures d'imagerie conformément au besoin des commandes pendant un

mode ou une procédure sélectionné, l'éclairage des commandes utilisateur hors d'usage étant éteint de telle sorte que les commandes hors d'usage sont pratiquement invisibles pour un utilisateur en raison de la couleur opaque sombre.

2. Système de diagnostic par ultrasons selon la revendication 1, dans lequel la couleur opaque sombre est noire.

3. Système de diagnostic par ultrasons selon la revendication 2, dans lequel la feuille de matière transparente comprend en outre une feuille de verre, les graphiques de commande étant affichés sur la face inférieure de la feuille de verre et entourés de peinture noire.

4. Système de diagnostic par ultrasons selon la revendication 3, comprenant en outre une pluralité de feuilles de métal capacitives (46) fixées à la feuille de verre à des emplacements de graphiques de commande pour l'actionnement capacitif des commandes par un utilisateur.

5. Système de diagnostic par ultrasons selon la revendication 1, dans lequel chacune des poches ou dépressions entre en contact avec la périphérie d'une commande utilisateur correspondant au-dessus de la couche barrière pour confiner la lumière dans une poche ou dépression donnée à la commande utilisateur au-dessus.

6. Système de diagnostic par ultrasons selon la revendication 5, dans lequel la couche barrière comprend en outre un cadre de diffuseur et des tubes lumineux pour les commandes utilisateur.


7. Système de diagnostic par ultrasons selon la revendication 5, dans lequel les sources lumineuses comprennent en outre des DEL situées dans les poches ou dépressions.

8. Système de diagnostic par ultrasons selon la revendication 7, dans lequel le dispositif de commande d'éclairage comprend en outre une carte de circuit imprimé fixée à la couche barrière, dans lequel les DEL sont couplées électriquement à la carte de circuit imprimé et l'éclairage des DEL est commandé par la carte de circuit imprimé.

9. Système de diagnostic par ultrasons selon la revendication 7, dans lequel les sources lumineuses comprennent

- en outre des DEL de différentes couleurs situées dans la même poche ou dépression, dans lequel les différentes couleurs sont utilisées pour éclairer la commande utilisateur conformément à un état de la fonction de la commande utilisateur. 5
10. Système de diagnostic par ultrasons selon la revendication 9, dans lequel les états de la commande utilisateur sont disponibles ou actifs. 10
11. Système de diagnostic par ultrasons selon la revendication 1, comprenant en outre un commutateur couplé au panneau de commande utilisateur, dans lequel ledit commutateur est actionné pour éteindre l'éclairage de pratiquement toutes les commandes utilisateur pendant le nettoyage de la surface supérieure du panneau de commande. 15  
20
12. Système de diagnostic par ultrasons selon la revendication 11, dans lequel l'actionnement du commutateur pour éteindre l'éclairage a en outre pour rôle de désactiver les commandes utilisateur de leur fonctionnalité de commande. 25
13. Système de diagnostic par ultrasons selon la revendication 11, dans lequel le commutateur est situé à une position sur le système à ultrasons autre que la surface supérieure du panneau de commande. 30
14. Système de diagnostic par ultrasons selon la revendication 12, dans lequel l'actionnement du commutateur pour éteindre l'éclairage fait apparaître en noir les commandes utilisateur et leurs zones environnantes du panneau de commande. 35  
40
15. Système de diagnostic par ultrasons selon la revendication 1, dans lequel l'une des commandes utilisateur comprend en outre un pavé tactile capacitif situé en avant du centre du panneau de commande vers une position d'un utilisateur, la surface tactile au-dessus du pavé tactile comprenant la surface supérieure du panneau de commande, laquelle est en continuité avec la surface tactile de la majorité des autres commandes utilisateur du panneau de commande. 45  
50

55

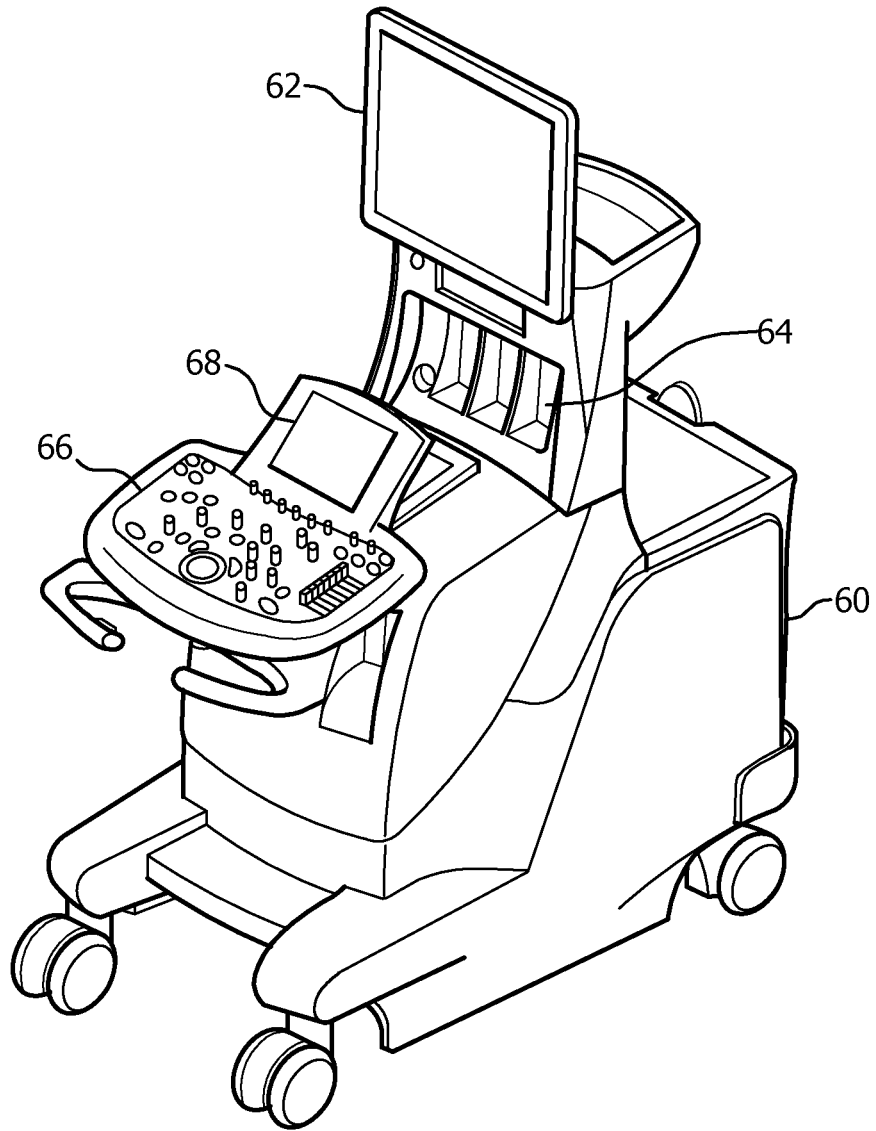

**FIG. 1**  
(Prior art)

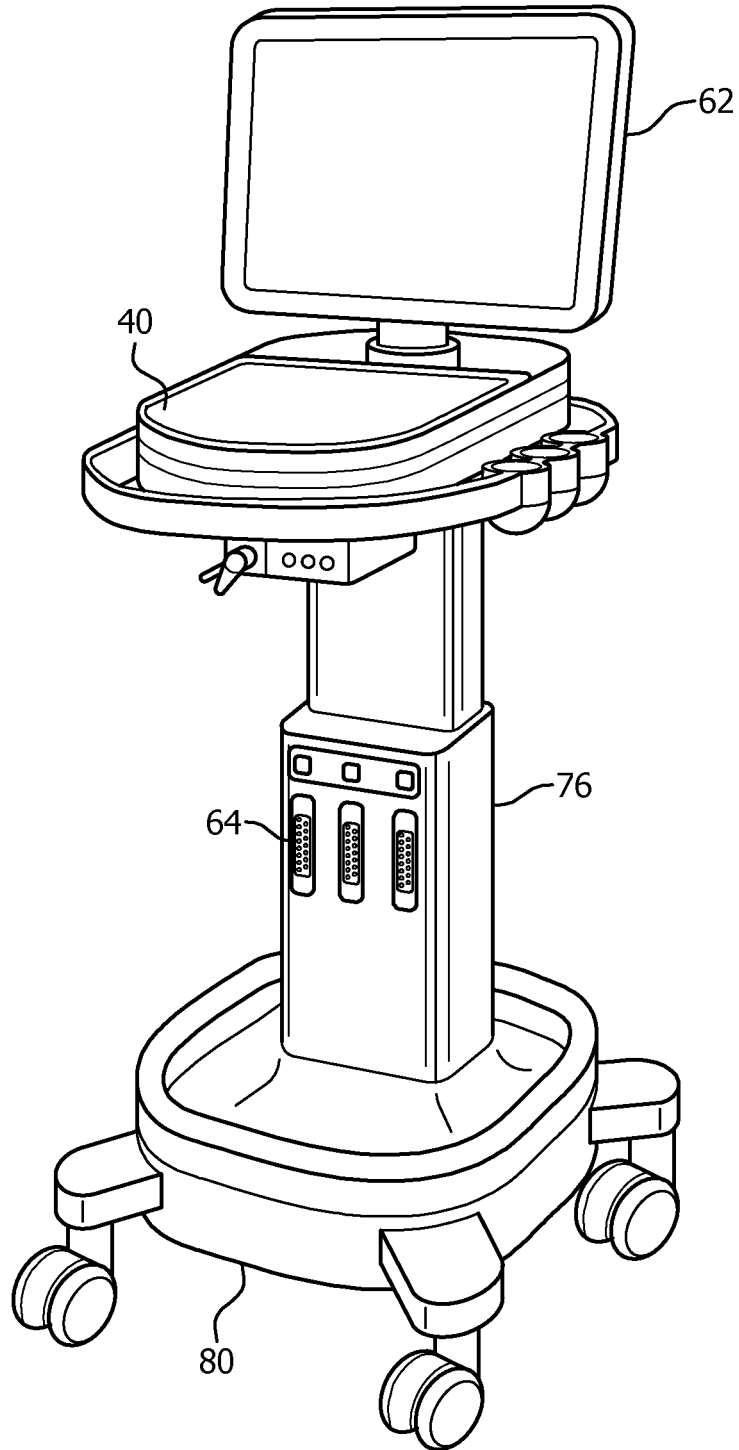


FIG. 2

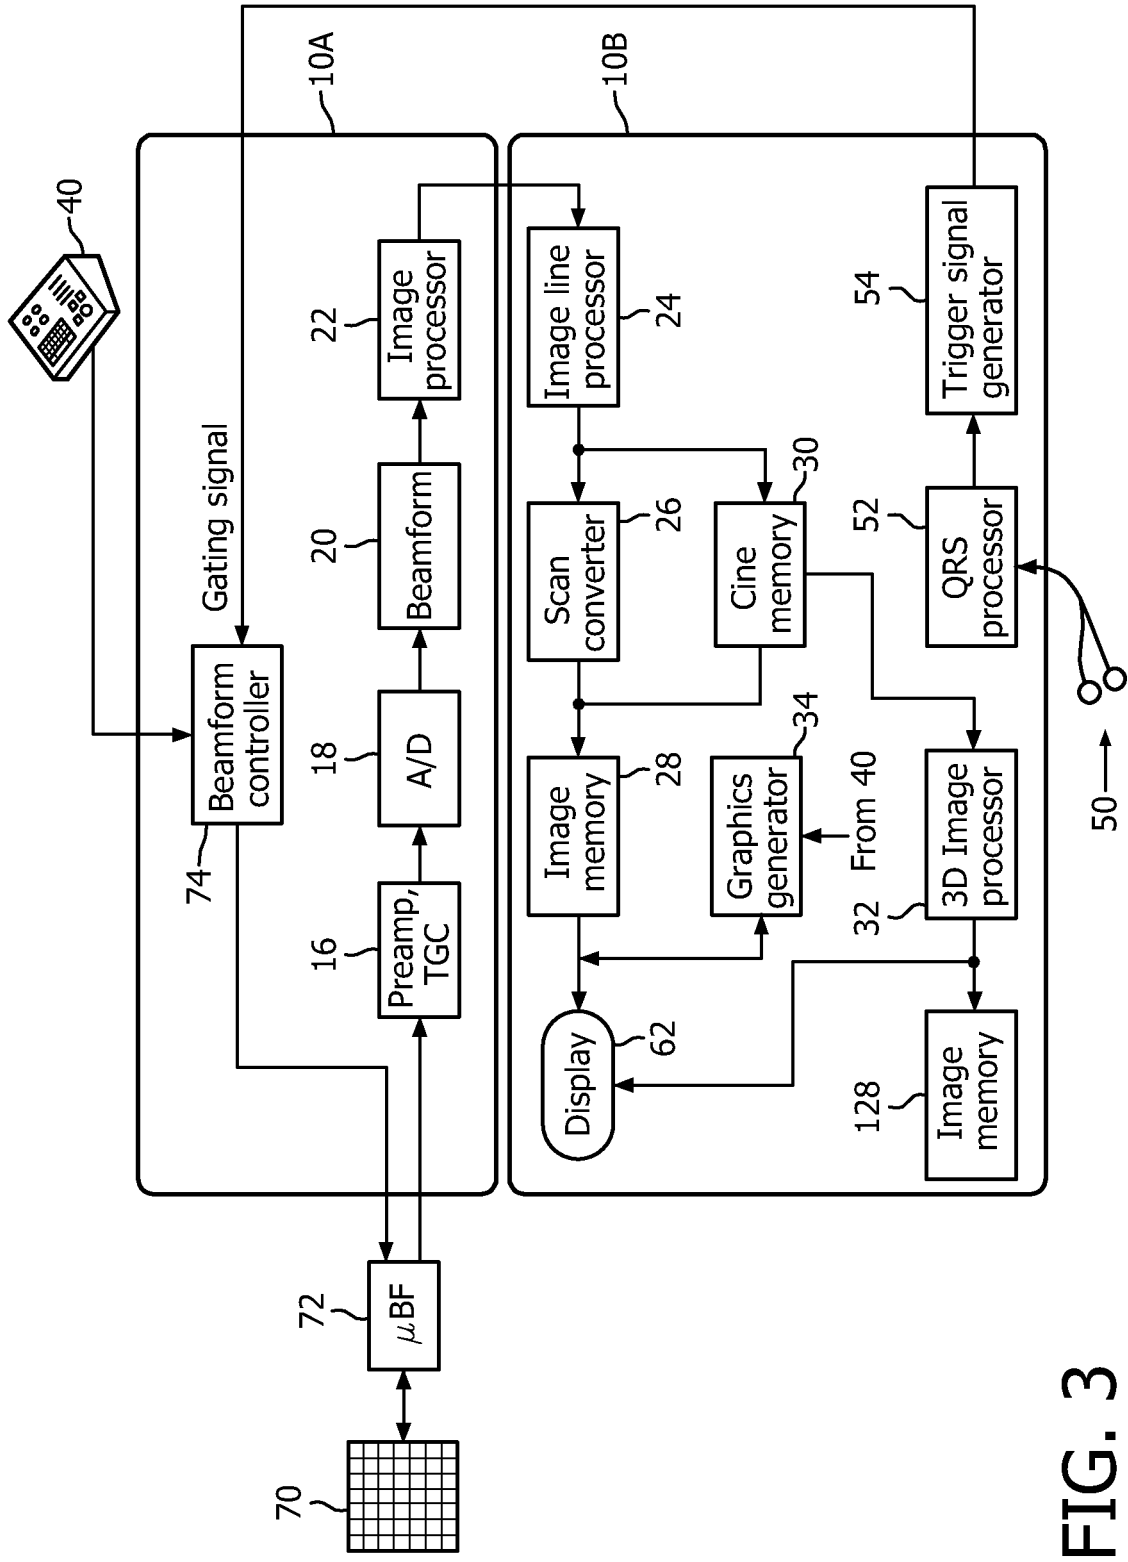


FIG. 3

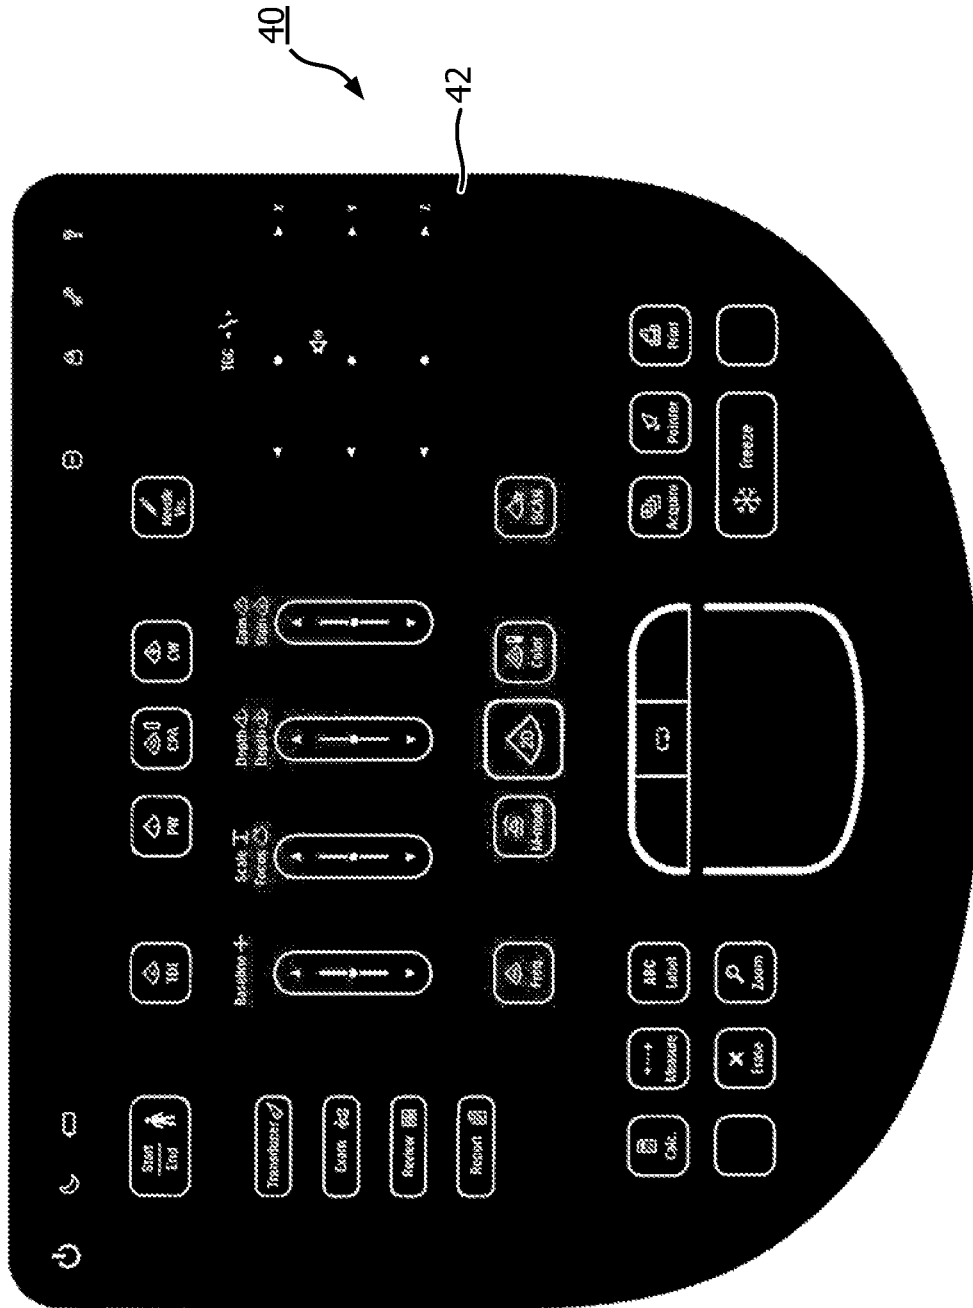


FIG. 4

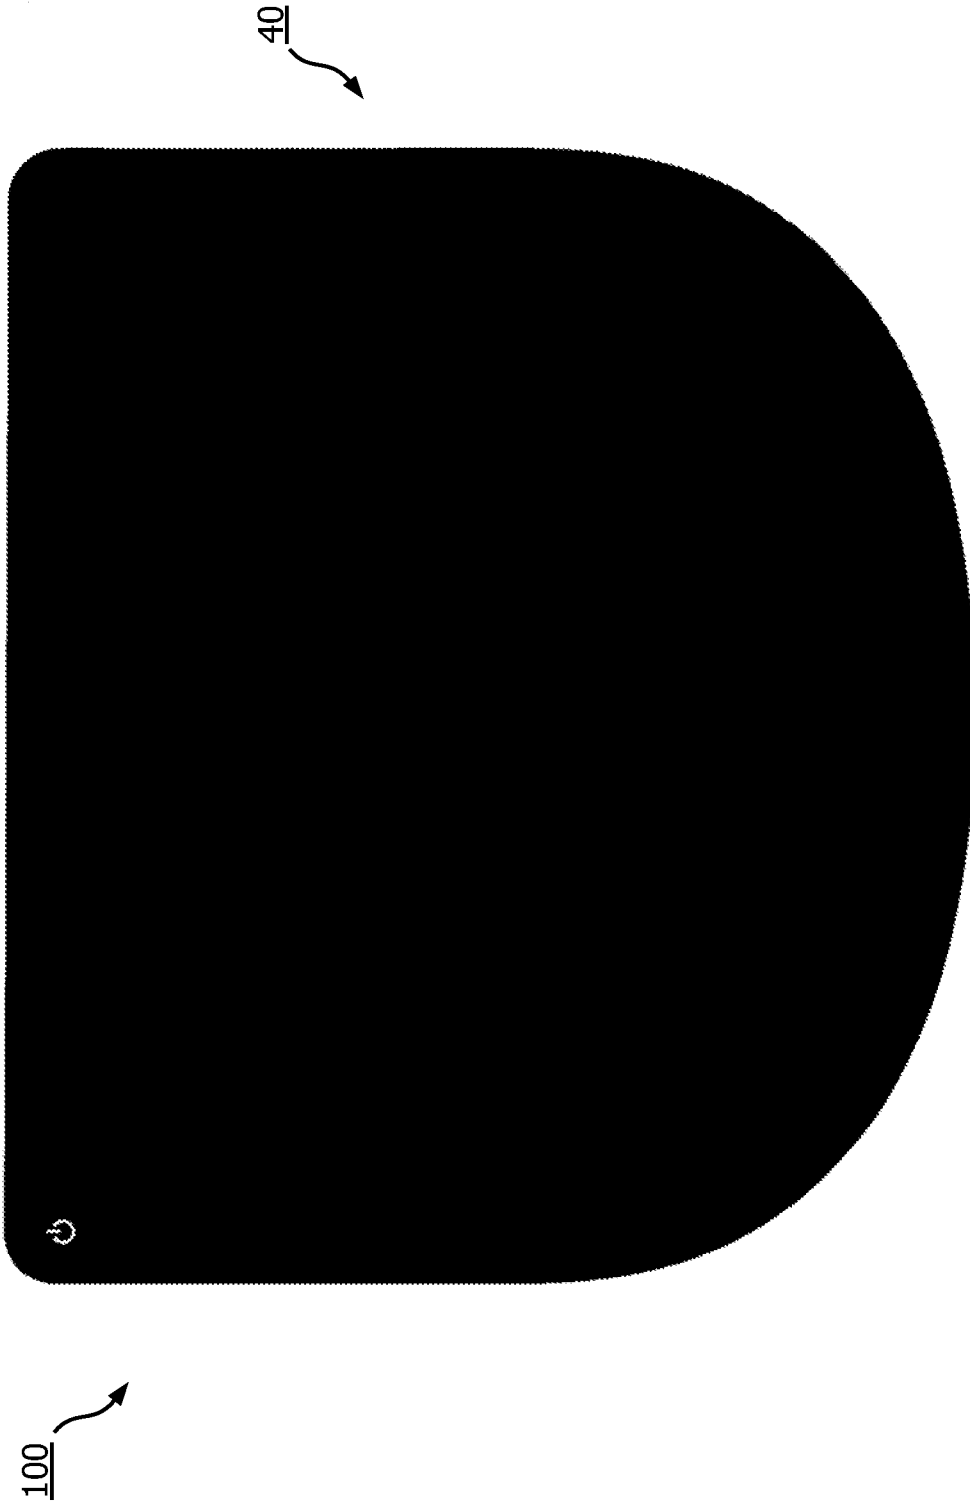


FIG. 5

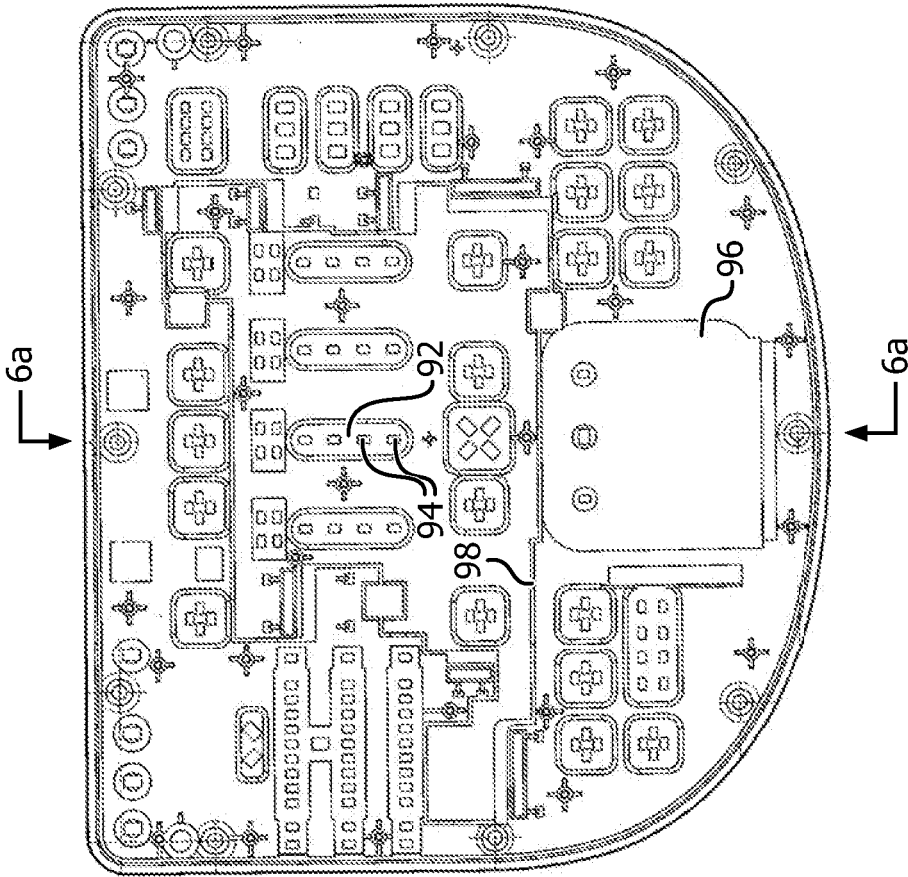
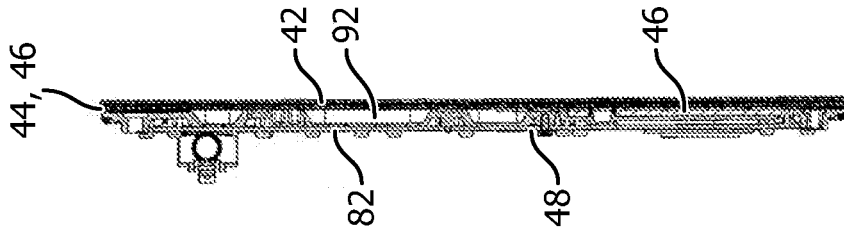


FIG. 6a

FIG. 6

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 6063030 A, Vara **[0004]**
- US 2009131793 A **[0005]**
- US 5997479 A, Savord **[0012]**
- US 6436048 B, Pesque **[0012]**

专利名称(译)	具有上下文可变控制面板的超声诊断成像系统		
公开(公告)号	<a href="#">EP2744415A1</a>	公开(公告)日	2014-06-25
申请号	EP2012781452	申请日	2012-09-21
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	CHENG JEANNE MARK ZSOLT		
发明人	CHENG, JEANNE MARK, ZSOLT		
IPC分类号	A61B8/00 G06F3/00		
CPC分类号	A61B8/4405 A61B8/4433 A61B8/4477 A61B8/462 A61B8/465 A61B8/466 A61B8/467 A61B8/483 A61B8/486 A61B8/488 A61B8/54 G06F3/044 G06F3/04895 A61B8/14 A61B8/463		
代理机构(译)	STEFFEN , THOMAS		
优先权	61/540586 2011-09-29 US		
其他公开文献	EP2744415B1		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

超声系统具有由顶部玻璃板形成的控制面板，其中控制区域图形被屏蔽在玻璃板的底表面上。电容箔贴附在屏蔽图形的上方，从而可以通过触摸屏蔽图形上方的顶部表面来电容选择用户控件。每个控制区域由扩散器框架有选择地进行背照明，其中光管固定在玻璃板下方。用于照明的LED安装在固定至扩散器框架的印刷电路板上，该印刷电路板由印刷电路板控制。根据正在执行的操作模式或成像过程的上下文来照亮不同组的用户控件，以便仅照亮所需的控件，而用户看不见不需要的控件。所有控件都可以熄灭和停用，以便可以清洁控制面板的上表面，而无需随机激活控制面板的控件。