

(19)



(11)

EP 2 901 938 A1

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
05.08.2015 Bulletin 2015/32

(51) Int Cl.:
A61B 8/00 (2006.01)

(21) Application number: **14176134.6**

(22) Date of filing: **08.07.2014**

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
 GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
 PL PT RO RS SE SI SK SM TR**
 Designated Extension States:
BA ME

(72) Inventor: **Min, Hae-kee
 Gangwon-do (KR)**

(74) Representative: **Schmid, Wolfgang
 Lorenz & Kollegen
 Patentanwälte Partnerschaftsgesellschaft mbB
 Alte Ulmer Strasse 2
 89522 Heidenheim (DE)**

(30) Priority: **29.01.2014 KR 20140011526**


(71) Applicant: **Samsung Medison Co., Ltd.
 Gangwon-do 250-870 (KR)**

(54) Ultrasonic probe and ultrasonic diagnostic apparatus including the same

(57) Provided is an ultrasonic probe including: a housing; an ultrasonic module; at least one signal line; a support barrel which is supported by the housing, in which the at least one signal line is arranged and an outer surface of which has at least one ring electrode which electrically connects the at least one signal line to the ultra-

sonic module; and a rotation barrel which is rotatable around the support barrel in one direction and supports the ultrasonic module so as to maintain an electrical contact of the ultrasonic module to the at least one ring electrode.

FIG. 5

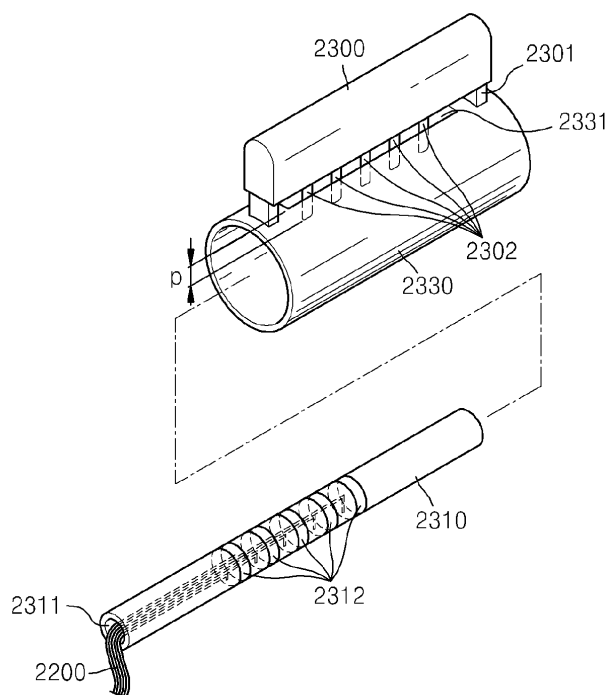

EP 2 901 938 A1

Description

RELATED APPLICATION

[0001] This application claims the benefit of Korean Patent Application No. 10-2014-0011526, filed on January 29, 2014, in the Korean Intellectual Property Office, the disclosure of which is incorporated herein in its entirety by reference.

BACKGROUND

1. Field

[0002] One or more embodiments of the present invention relate to an ultrasonic probe used for ultrasonic diagnoses and an ultrasonic diagnostic apparatus including the same.

2. Description of the Related Art

[0003] An ultrasonic diagnostic apparatus is an apparatus for diagnosing a target object by visualizing internal body parts of the target object, and acquires an image of a certain part from among the internal body parts of the target object by transmitting ultrasonic signals to the target object and receiving information via echo signals reflected from the target object.

[0004] In comparison with a diagnostic apparatus using X rays, the ultrasonic diagnostic apparatus has high stability, is capable of displaying an image on a screen in real time, and there is no possibility of radiation exposure, and thus the ultrasonic diagnostic apparatus is widely used along with other image diagnostic apparatuses.

[0005] An ultrasonic diagnostic apparatus has a probe which contacts a target object in order to examine internal body parts thereof. The probe includes an ultrasonic module which generates ultrasonic signals and transmits/receives the ultrasonic signals to/from the target object. According to various arrangements of piezoelectric vibrators forming the ultrasonic module, types of the ultrasonic probe may be classified into a linear type, a convex type, a circular type, etc. Also, the ultrasonic probe may be classified into an ultrasonic probe for acquiring a two-dimensional (2D) image and an ultrasonic probe for acquiring a three-dimensional (3D) image according to the types of the acquired images.

[0006] The ultrasonic probe for acquiring a 3D image may have a module-driving structure formed to acquire an image by reciprocating motion of an ultrasonic module within a predetermined range.

[0007] However, in the above case, because of reciprocating motion of the ultrasonic module, it is necessary to reduce movement velocity when the ultrasonic module changes its movement direction. Such velocity reduction may decrease an image processing speed of the ultrasonic diagnostic apparatus. Also, vibration and noises

may be generated while the ultrasonic module changes its movement direction.

SUMMARY

5

[0008] One or more embodiments of the present invention include an ultrasonic probe including an ultrasonic module capable of rotating at least about 360° degrees in one direction, and an ultrasonic diagnostic apparatus including the ultrasonic probe.

10

[0009] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

15

[0010] According to one or more embodiments of the present invention, an ultrasonic probe includes: a housing; an ultrasonic module arranged inside the housing; at least one signal line which transmits/receives signals to/from the ultrasonic module; a support barrel which is supported by the housing, in which the at least one signal line is arranged and an outer surface of which has at least one ring electrode which electrically connects the at least one signal line to the ultrasonic module; and a rotation barrel which is rotatable around the support barrel in one direction and supports the ultrasonic module so as to maintain an electrical contact of the ultrasonic module to the at least one ring electrode.

20

25

[0011] The ultrasonic module may be formed to be rotatable at least about 360° in one direction due to the rotation barrel.

30

[0012] The at least one ring electrode may be continuously formed along a circumference direction of the support barrel.

35

[0013] The at least one ring electrode may be a plurality of ring electrodes, and the plurality of ring electrodes may be arranged to be separated from each other along a lengthwise direction of the support barrel.

40

[0014] The ultrasonic module may further include contact electrodes protruding towards the support barrel from an inside of the rotation barrel.

45

[0015] The contact electrodes may be bent due to a contact with the at least one ring electrode.

[0016] The ultrasonic probe may further include a driving unit which rotates the rotation barrel.

50

[0017] The ultrasonic module may rotate about a rotation axis which is perpendicular to a lengthwise direction of the housing.

[0018] The ultrasonic module may further include a controller which makes the ultrasonic module transmit or receive ultrasonic signals at some of regions where the ultrasonic module rotates while the ultrasonic module rotates.

55

[0019] The ultrasonic module may rotate about a rotation axis which is parallel to lengthwise direction of the housing.

[0020] According to one or more embodiments of the present invention, an ultrasonic diagnostic apparatus includes: an ultrasonic probe which transmits ultrasonic

signals to a target object and receives echo signals reflected from the target object; an image processor which generates an ultrasonic image based on the received echo signal; and a display unit which displays the generated ultrasonic image. The ultrasonic probe includes: a housing; an ultrasonic module arranged inside the housing; at least one signal line which transmits/receives signals to/from the ultrasonic module; a support barrel which is supported by the housing, in which the at least one signal line is arranged, and an outer surface of which has at least one ring electrode which electrically connects the at least one signal line to the ultrasonic; and a rotation barrel which is rotatable around the support barrel in one direction and supports the ultrasonic module so as to maintain an electrical contact of the ultrasonic module to the at least one ring electrode.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021] These and/or other aspects will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings in which:

FIG. 1 is a block diagram of a structure of an ultrasonic diagnostic apparatus according to an embodiment of the present invention;

FIG. 2 is a schematic view of a structure of an ultrasonic probe according to an embodiment of the present invention;

FIG. 3 is a schematic view of a structure of an ultrasonic probe according to another embodiment of the present invention;

FIG. 4 is an exploded perspective view of the ultrasonic probe of FIG. 2;

FIG. 5 is an exploded perspective view showing some parts of FIG. 4;

FIG. 6A is a cross-sectional view of an ultrasonic module of FIG. 4, taken along a line VI-VI of FIG. 4; FIGS. 6B and 6C are cross-sectional views sequentially showing one-way rotation states of the ultrasonic module of FIG. 6A in one direction; and

FIG. 7 is a cross-sectional view of an ultrasonic probe according to another embodiment of the present invention.

DETAILED DESCRIPTION

[0022] In the description of the present invention, since terms used herein are defined in consideration of the functions of the present invention and commonly-used terms, they may vary according to users' intentions, practices or the advent of new technologies. In addition, terms may be arbitrarily determined by an applicant and, in this case, they may be later described in detail. Therefore, the terms used herein must be defined based on meanings thereof and contents of the entire specification.

[0023] Throughout the specification, when a portion

"includes" an element, another element may be further included, rather than excluding the existence of the other element, unless otherwise described. Also, throughout the specification, the terms such as "unit" and "module" refer a unit which processes at least one function or operation, and may be configured as hardware, software, or a combination thereof.

[0024] Throughout the specification, an "ultrasonic image" denotes an image of a target object acquired by using ultrasonic waves. Also, the target object may include a person or an animal, or some parts of a person or an animal. For example, the target object may include organs or blood vessels included in a liver, a heart, a uterus, a brain, breasts or an abdomen. Also, the target object may include a phantom, and the phantom may refer a material having a volume which approximates to a density of an organism or an effective atomic number.

[0025] Also, throughout the specification, the term "user" may be a medical expert such as a doctor, a nurse, a medical technologist and a medical imaging technologist, or a technician who fixes medical equipment, but is not limited thereto.

[0026] Reference will now be made in detail to embodiments, examples of which are illustrated in the accompanying drawings. Expressions such as "at least one of," when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

[0027] FIG. 1 is a block diagram of a structure of an ultrasonic diagnostic apparatus 1000 according to an embodiment of the present invention. The ultrasonic diagnostic apparatus 1000 may include an ultrasonic probe 2000, an ultrasonic transmitter/receiver 100, an image processor 200, a communication unit 300, a memory 400, an input device 500, and a controller 600, and each of the above-listed components may be connected via a bus 700.

[0028] The ultrasonic diagnostic apparatus 1000 may be configured as a cart-type or portable ultrasonic diagnostic apparatus. Examples of the portable ultrasonic diagnostic apparatus may include a picture archiving and communication system (PACS) viewer, a smart phone, a laptop computer, a personal digital assistant (PDA), or the like, but are not limited thereto.

[0029] The ultrasonic probe 2000 transmits ultrasonic signals to a target object 10 and receives echo signals reflected from the target object 10 according to driving signals transmitted by the ultrasonic transmitter/receiver 100. The ultrasonic probe 2000 includes transducers (not shown), and each of the transducers vibrates according to the driving signals and generates ultrasonic waves which are sound energy. Also, the ultrasonic probe 2000 may be connected to a main body of the ultrasonic diagnostic apparatus 1000 via a wired or wireless method, and the ultrasonic diagnostic apparatus 1000 may include a plurality of ultrasonic probes 2000 according to configuration types.

[0030] The transmitter 110 provides driving signals to

the ultrasonic probe 2000 and includes a pulse generator 112, a transmitting delay unit 114 and a pulser 116. The pulse generator 112 generates pulses for generating transmission ultrasonic waves according to a predetermined pulse repetition frequency (PRF), and the transmitting delay unit 114 applies a delay time for determining transmission directivity to the pulses. Each pulse to which the delay time is applied corresponds to one of piezoelectric vibrators included in the ultrasonic probe 2000. The pulser 116 is a timing corresponding to each pulse to which the delay time is applied, and transmits driving signals (or driving pulses) to the ultrasonic probe 2000.

[0031] The receiver 120 generates ultrasonic data by processing echo signals transmitted by the ultrasonic probe 2000, and may include an amplifier 122, an analog digital converter (ADC) 124, a receiving delay unit 126 and an adding unit 128. The amplifier 122 amplifies the echo signals in each of channels, and the ADC 124 AD-converts the amplified echo signals. The receiving delay unit 126 applies a delay time for determining receipt directivity to each signal which is digitally converted, and the adding unit 128 generates ultrasonic data by adding echo signals processed by the receiving delay unit 126. The receiver 120 may not include the amplifier 122, depending on configuration types. That is, when a sensitivity of the ultrasonic probe 2000 is improved or the number of bits to be processed by the ADC 124 is increased, the amplifier 122 may not be included.

[0032] The image processor 200 generates an ultrasonic image via a scan conversion process with regard to the ultrasonic data generated in the ultrasonic transmitter/receiver 100, and displays the generated ultrasonic image. The ultrasonic image may include a grayscale image, which is acquired by scanning the target object 10 in an amplitude (A) mode, a brightness (B) mode and a motion (M) mode, as well as a Doppler image, which shows the target object 10 which moves using a Doppler effect. The Doppler image may include a blood flow Doppler image (or a color Doppler image) which shows a flow of blood, a tissue Doppler image which shows movements of tissues and a spectral Doppler image which marks movement velocity of the target object 10 with a wavy form.

[0033] The B-mode processor 212 extracts B-mode components from the ultrasonic data and processes the extracted B-mode components. The image generator 220 may generate an ultrasonic image which marks an intensity of a signal with brightness based on the B-mode components extracted by the B-mode processor 212.

[0034] Likewise, the Doppler processor 214 extracts Doppler components from the ultrasonic data, and the image generator 220 may generate a Doppler image which marks movements of the target object 10 with a color or a wavy form based on the extracted Doppler components.

[0035] The image generator 220 may generate a three-dimensional (3D) image via a volume rendering process with regard to volume data or an elasticity image which

visualizes a degree of deformity of the target object 10. Furthermore, the image generator 220 may display a variety of additional information as texts or graphics on the ultrasonic image. The generated ultrasonic image may be stored in the memory 400.

[0036] The display unit 230 may display the generated ultrasonic image. The display unit 230 may display the ultrasonic image and a variety of information processed in the ultrasonic diagnostic apparatus 1000 on a screen via a graphic user interface (GUI). The ultrasonic diagnostic apparatus 1000 may include two or more display units 230, depending on configuration types.

[0037] The communication unit 300 has a wired or wireless connection with a network 30 and communicates with an external device or a server. The communication unit 300 may share data with a server 32 in a hospital or another medical apparatus 34 in the hospital which is connected to the communication unit 300 via a picture archiving and communication system (PACS). Also, the communication unit 300 may perform data communication according to digital imaging and communications in medicine (DICOM) standards.

[0038] The communication unit 300 may receive/transmit data related to a diagnosis of the target object 10, for example, an ultrasonic image, ultrasonic data, Doppler data, or the like via the network 30. Also, the communication unit 300 may receive/transmit images acquired by other medical apparatuses such as a computed tomography (CT) apparatus, a magnetic resonance imaging (MRI) apparatus and an X-ray apparatus. Furthermore, the communication unit 300 may receive information with regard to a diagnostic history, treatment schedules, etc. of the target object 10 and may use the information to diagnose the target object 10. In addition, the communication unit 300 may perform data communication with not only the server 32 or the medical apparatus 34 in the hospital but also a mobile terminal 36 of a doctor or a patient.

[0039] The communication unit 300 has a wired or wireless connection with the network 30 and may share data with the server 32, the medical apparatus 34 or the mobile terminal 36. The communication unit 300 may include one or more components which enables communication with an external device, and may include, for example, a short distance communication module 310, a wired communication module 320 and a mobile communication module 330.

[0040] The short distance communication module 310 is a module for short distance communication within a predetermined distance. Short distance communication technologies may include, but are not limited to, wireless LAN, Wi-Fi, Bluetooth, Zigbee, Wi-Fi Direct (WFD), ultra wideband (UWB), an infrared data association (IrDA), Bluetooth low energy (BLE), near field communication (NFC), etc.

[0041] The wired communication module 320 is a module for communication using electrical signals or optical signals, and wired communication technologies may in-

clude a pair cable, a coaxial cable, a fiber optic cable, Ethernet cable, etc.

[0042] The mobile communication module 330 receives/transmits wireless signals from/to at least one of a base station, an external terminal and a server. The wireless signals may include various forms of data according to receipt/transmission of voice call signals, video call signals or text/multimedia messages.

[0043] The memory 400 stores a variety of information processed in the ultrasonic diagnostic apparatus 1000. For example, the memory 400 may store medical data with regard to a diagnosis of the target object 10, for example, input/output ultrasonic data, an ultrasonic image, etc., and may also store algorithms or programs that may be executed in the ultrasonic diagnostic apparatus 1000.

[0044] The memory 400 may be configured as various storage media such as a flash memory, a hard disk and an electrically erasable and programmable random access memory (EEPROM). Also, the ultrasonic diagnostic apparatus 1000 may operate web storage or a cloud server which performs a storage function of the memory 400 on the Web.

[0045] The input device 500 denotes a medium for receiving, from a user, data which controls the ultrasonic diagnostic apparatus 1000. The input device 500 may include, but is not limited to, hardware components such as a key pad, a mouse, a touch panel, a touch screen, a track ball and a jog switch, and may further include various input media such as an electrocardiogram measurement module, a breath measurement module, a voice recognition sensor, a gesture recognition sensor, a fingerprint recognition sensor, an iris recognition sensor, a depth sensor and distance sensor.

[0046] The controller 600 generally controls operations of the ultrasonic diagnostic apparatus 1000. That is, the controller 600 may control operations among the ultrasonic probe 2000, the ultrasonic receiver/transmitter 100, the image processor 200, the communication unit 300, the memory 400 and the input device 500 of FIG. 1.

[0047] Some or all of the ultrasonic probe 2000, the ultrasonic receiver/transmitter 100, the image processor 200, the communication unit 300, the memory 400, the input device 500 and the controller 600 may operate as a software module, but the operations of some or all of the above-listed components are not limited thereto. Also, Some of the ultrasonic probe 2000, the ultrasonic receiver/transmitter 100, the image processor 200, the communication unit 300, the memory 400, the input device 500 and the controller 600 may operate as hardware. At least some of the ultrasonic receiver/transmitter 100, the image processor 200, the communication unit 300 may be included in the controller 600, but are not limited thereto.

[0048] FIG. 2 is a schematic view of a structure of the ultrasonic probe 2000 according to an embodiment of the present invention. The ultrasonic probe 2000 includes a housing 2100 and an ultrasonic module 2300 arranged

to rotate in the housing 2100.

[0049] The housing 2100 includes a handle case 2110 and a cap 2120 which is arranged at a front end of the handle case 2110 and contacts the target object 10 to be examined. The handle case 2110 fixes the cap 2120 and may have a shape which allows the user to easily grasp the handle case 2110. The cap 2120 transmits the ultrasonic signals, which are emitted from the ultrasonic module 2300 arranged in the housing 2100, to the target object 10 of FIG. 1 and may function to transmit the echo signals reflected from the target object 10 to the ultrasonic module 2300.

[0050] The ultrasonic module 2300 includes at least one transducer (not shown) and may be configured to rotate at least about 360° in one direction. That is, the ultrasonic module 2300 does not repeatedly move within a predetermined range of degrees, but may have a structure capable of rotating about 360° and more in one direction. The at least one transducer may include a piezoelectric vibrator, a sound absorption layer, an acoustic matching layer, etc. The housing 2100 includes a space where the ultrasonic module 2300 may rotate about 360° and more in one direction.

[0051] Since the ultrasonic module 2300 rotates in one direction, periodical sections for reducing movement velocity of the ultrasonic module 2300 which may appear during reciprocating motion may be removed. Thus, a decrease in the movement velocity of the ultrasonic module 2300 may be prevented. Also, vibration and noises, which are generated while the movement velocity of the ultrasonic module 2300, may be reduced.

[0052] The ultrasonic module 2300 rotates about a rotation axis. The rotation axis has a direction crossing a lengthwise direction (L) of the housing 2100, for example, a vertical direction. However, the rotation axis of the ultrasonic module 2300 is not limited thereto, and may vary according to necessity. For example, as shown in FIG. 3, the ultrasonic module may rotate about a rotation axis which is parallel to the lengthwise direction (L) of the housing 2100. In this regard, structures of the handle case 2110a and the cap 2120a of FIG. 3 may be partially different from the handle case 2110 and the cap 2120 of Fig. 2.

[0053] For transmission and receipt of the ultrasonic signals, the ultrasonic module 2300 needs to be connected to signal lines 2200 (refer to FIG. 4) which receives/transmits electrical signals from/to the receiver 120/the transmitter 110. However, when the ultrasonic module 2300 rotates about 360° and more in one direction in a state where the signal lines 2200 are directly connected to the ultrasonic module 2300, the signal lines 2200 connected to the rotating ultrasonic module 2300 are twisted due to a rotation of the ultrasonic module 2300. Also, when there are signal lines 2200, the signal lines 2200 may be twisted around each other, and twists of the signal lines 2200 may cause damage to the signal lines 2200 or to portions where the signal lines 2200 are connected to other components.

[0054] However, in the present embodiment, although the ultrasonic module 2300 rotates in one direction, a structure of connecting the ultrasonic module 2300 to the signal lines 2200, which may prevent torsion or the twists of the signal lines 2200, is provided.

[0055] FIG. 4 is an exploded perspective view of the ultrasonic probe 2000 of FIG. 2, and FIG. 5 is an exploded perspective view showing some parts of the ultrasonic probe 2000 of FIG. 4. FIG. 6A is a cross-sectional view of the ultrasonic module 2300 of FIG. 4, taken along a line VI-VI of FIG. 4, and FIGS. 6B and 6C are cross-sectional views sequentially showing one-way rotation states of the ultrasonic module 2300 of FIG. 6A in one direction.

[0056] Referring to FIGS. 4 and 5, there are the signal lines 2200, a support barrel 2310 in which the signal lines 2200 are arranged, a rotation barrel 2330 capable of rotating around the support barrel 2310, and the ultrasonic module 2300 attached to the rotation barrel 2330.

[0057] Both end portions of the support barrel 2310 are supported by support members 2111 formed on the handle case 2110. A cavity 2311 into which the signal lines 2200 may be inserted is formed in the support barrel 2310. Some part of each of the signal lines 2200 are inserted into the support barrel 2310 and other part of each of the signal lines 2200 may be connected to a connection cable 2113 by passing through an opening 2112 formed in the handle case 2110. Through the connection cable 2113, the signal lines 2200 may be connected to the transmitter 110 and the receiver 120 arranged on the main body of the ultrasonic diagnostic apparatus 1000.

[0058] Ring electrodes 2312 are arranged on an outer surface of the support barrel 2310. For example, the ring electrodes 2312 may be arranged to be separated from each other in a lengthwise direction of the support barrel 2310. The ring electrodes 2312 are connected to the signal lines 2200 inserted into the cavity 2311, respectively. The number of the ring electrodes 2312 may correspond to that of the signal lines 2200. For example, as shown in FIGS. 4 and 5, when there are five ring electrodes 2312, there may be five signal lines 2200. As another example, although not illustrated in the drawings, when there are a hundred and ninety two (192) ring electrodes 2312, the number of the signal lines 2200 may also be 192.

[0059] Each of the ring electrodes 2312 is continuously formed along a circumference direction of the support barrel 2310. Accordingly, the ring electrodes 2312 may remain in electrical contact with the ultrasonic module 2300 even though the ultrasonic module 2300 rotates in one direction. Materials of the ring electrodes 2312 may include an electrically conductive material so as to transmit electrical signals between the ultrasonic module 2300 and the signal lines 2200. A conductive material may be a metal such as copper, iron, aluminum, nickel, gold and silver. However, the conductive material is not limited thereto, and the ring electrodes 2312 may be formed of

a non-conductive material which may be generally used to transmit electrical signals.

[0060] The rotation barrel 2330 is arranged outside the support barrel 2310 and may rotate around the support barrel 2310. The rotation barrel 2330 has a hollow structure in order for the support barrel 2310 to be inserted into the rotation barrel 2330. The rotation barrel 2330 may be connected to a driving unit 2114 installed on the housing 2100, for example, to a driving motor. The driving unit 2114 may be controlled by the controller 600 of the main body of the ultrasonic diagnostic apparatus 1000. As the driving unit 2114 rotates in one direction, the rotation barrel 2330 may rotate in one direction. Rotation velocity and a rotation direction of the rotation barrel 2330 may vary according to rotation velocity and a rotation direction of the driving unit 2114, and accordingly, rotation velocity and a rotation direction of the ultrasonic module 2300 supported by the rotation barrel 2330 may vary.

[0061] In the present embodiment, a case where the driving unit 2114 is arranged outside the rotation barrel 2330 is described, but a location and a shape of the driving unit 2114 may be appropriately changed according to necessity.

[0062] The rotation barrel 2330 supports the ultrasonic module 2300. The ultrasonic module 2300 and the rotation barrel 2330 may be fixed and supported by fixtures 2301. Since the ultrasonic module 2300 remains fixed to the rotation barrel 2330, the ultrasonic module 2300 rotates when the rotation barrel 2330 rotates.

[0063] The ultrasonic module 2300 includes contact electrodes 2302 formed to contact the ring electrodes 2312. The contact electrodes 2302 may transmit/receive electrical signals to/from the signal lines 2200 through the ring electrodes 2312. Materials of the contact electrodes 2302 may include an electrically conductive material so as to transmit the electrical signals to the ring electrodes 2312. A conductive material may be a metal such as copper, iron, aluminum, nickel, gold and silver. However, the conductive material is not limited thereto, and the contact electrodes 2302 may be formed of a non-conductive material which may be generally used to transmit electrical signals.

[0064] The contact electrodes 2302 pass through a hole 2331 formed in the rotation barrel 2330 and may be arranged to protrude towards the support barrel 2310 from an inside of the rotation barrel 2330.

[0065] Referring to FIGS. 5 and 6A, the contact electrodes 2302 protruding towards the support barrel 2310 contact the ring electrodes 2312 of the support barrel 2310, and the electrical signals are transmitted between them. A protrusion length (P) of each of the contact electrodes 2302 may be greater than a gap (G) between the ring electrodes 2312 and the inside of the rotation barrel 2330. An end portion of each contact electrode 2302 may be bent due to the contact with the ring electrodes 2312.

[0066] In this state, when the rotation barrel 2330 rotates around the support barrel 2310 in one direction, for example, a counterclockwise direction, the ultrasonic

module 2300 supported by the rotation barrel 2330 rotates in the counterclockwise direction as shown in FIGS. 6B and 6C. The contact electrodes 2302 of the ultrasonic module 2300 rotate while remaining in contact with the ring electrodes 2312. Since each of the ring electrodes 2312 is continuously formed along the circumference direction of the support barrel 2310, the ring electrodes 2312 may remain in contact with the rotating contact electrodes 2302.

[0067] As described above, by forming the contact electrodes 2302 of the ultrasonic module 2300 and the ring electrodes 2200 connected to the signal lines 2200 as separate members, the signal lines 2200 may be fixed without rotation when the ultrasonic module 2300 rotates. As a result, the torsion or twists of the signal lines 2200, which occur when the ultrasonic module 2300 rotates in one direction, may be prevented.

[0068] While rotating, the ultrasonic module 2300 may be activated at some rotation regions. For example, as shown in FIG. 6A, entire rotation regions of the ultrasonic module 2300 may be classified into activation regions (ARs) where the ultrasonic module 2300 is relatively close to the target object 10 and non-activation regions (NARs) where the ultrasonic module 2300 is relatively far from the target object 10 as shown in FIGS. 6B and 6C. For example, a range of the activation regions (ARs) may be about 80° or smaller, and that of the non-activation regions (NARs) may exceed about 280°. The controller 600 may make the ultrasonic module 2300 transmit or receive the ultrasonic signals when the ultrasonic module 2300 is disposed at the activation regions (ARs). When the ultrasonic module 2300 is disposed at the non-activation regions (NARs), the controller 600 may prevent the ultrasonic module from transmitting or receiving the ultrasonic signals.

[0069] FIG. 7 is a cross-sectional view of an ultrasonic probe 2001 according to another embodiment of the present invention. FIG. 7 is a cross-sectional view showing parts of the ultrasonic probe 2001 of FIG. 3, taken along a lengthwise direction (L) of a housing 2100a of FIG. 3. The ultrasonic module 2300 may rotate about a rotation axis which has a direction parallel to the lengthwise direction (L) of the housing 2100a. Hereinafter, descriptions with regard to a configuration which is the same as that of FIG. 5 will be omitted, differences between two configurations will be described.

[0070] Referring to FIG. 7, the ultrasonic probe 2001 includes signal lines 2200, a support barrel 2310 in which the signal lines 2200 are arranged, a rotation barrel 2330 capable of rotating the support barrel 2310 and an ultrasonic module 2300 supported by the rotation barrel 2330.

[0071] The support barrel 2310 is arranged along a direction parallel to the lengthwise direction (L) of the housing 2100a. Ring electrodes 2312 are arranged outside or on the outer surface of the support barrel 2310 in order to be separated from each other in a lengthwise direction of the support barrel 2310. The lengthwise direction (L) of the housing 2100a may be parallel to that

of the support barrel 2310. Each of the signal lines 2200 may be connected to each of the ring electrodes 2312.

[0072] Each of the ring electrodes 2312 is continuously formed along a circumference direction of support barrel 2310. Accordingly, the ring electrodes 2312 may remain in electrical contact with the ultrasonic module 2300 even though the ultrasonic module 2300 rotates in one direction. Materials of the ring electrodes 2312 may include an electrically conductive material so as to transmit electrical signals to the ultrasonic module 2300 and the signal lines 2200. A conductive material may be a metal such as copper, iron, aluminum, nickel, gold and silver. However, the conductive material is not limited thereto, and the ring electrodes 2312 may be formed of a non-conductive material which may be generally used to transmit electrical signals.

[0073] The rotation barrel 2330 is arranged outside the support barrel 2310 and may rotate around the support barrel 2310. The rotation barrel 2330 has a hollow structure in order for the support barrel 2310 to be inserted into the rotation barrel 2330. The rotation barrel 2330 may be connected to a driving unit 2114 installed on the housing 2100a. Therefore, the rotation barrel 2330 rotates due to the driving unit 2114.

[0074] The ultrasonic module 2300 and the rotation barrel 2330 may be fixed and supported by fixtures 2301. Since the ultrasonic module 2300 remains fixed to the rotation barrel 2330, the ultrasonic module 2300 and the rotation barrel 2330 rotate at the same time.

[0075] The ultrasonic module 2300 includes contact electrodes 2302 formed to contact the ring electrodes 2312. The contact electrodes 2302 may transmit/receive electrical signals to/from the signal lines 2200 through the ring electrodes. Materials of the contact electrodes 2302 may include an electrically conductive material so as to transmit the electrical signals to the ring electrodes 2312. A conductive material may be a metal such as copper, iron, aluminum, nickel, gold and silver. However, the conductive material is not limited thereto, and the contact electrodes 2302 may be formed of a non-conductive material which may be generally used to transmit electrical signals.

[0076] The contact electrodes 2302 pass through the rotation barrel 2330 and may be arranged to protrude towards the support barrel 2310 from an inside of the rotation barrel 2330. The contact electrodes 2302, which protrude towards the support barrel 2310, contact the ring electrodes 2312 of the support barrel 2310, and the electrical signals are transmitted between them.

[0077] When the rotation barrel 2330 rotates around the support barrel 2310 in one direction, the ultrasonic module 2300 supported by the rotation barrel 2330 may rotate in one direction. The contact electrodes 2302 of the ultrasonic module 2300 rotate while remaining in contact with the ring electrodes 2312. Since the ring electrodes 2312 are continuously formed along the circumference direction of the support barrel 2310, the ring electrodes 2312 may remain in contact with the rotating con-

tact electrodes 2302.

[0078] As described above, by forming the contact electrodes 2302 of the ultrasonic module 2300 and the ring electrodes 2200 connected to the signal lines 2200 as separate members, the signal lines 2200 may be fixed without rotation when the ultrasonic module 2300 rotates. As a result, the torsion or twists of the signal lines 2200, which occur when the ultrasonic module 2300 rotates in one direction, may be prevented.

[0079] According to the one or more embodiments of the present invention, the ultrasonic probe and the ultrasonic diagnostic apparatus including the same include the ultrasonic module capable of rotating at least about 360° in one direction, and have a structure that prevent signal lines, which transmit signals, from being twisted despite rotation of the ultrasonic module. Thus, a speed of processing images may be improved, and also vibration and generation of noises may be prevented.

[0080] It should be understood that the exemplary embodiments described herein should be considered in a descriptive sense only and not for purposes of limitation. Descriptions of features or aspects within each embodiment should typically be considered as available for other similar features or aspects in other embodiments.

[0081] While one or more embodiments of the present invention have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope of the present invention as defined by the following claims.

Claims

1. An ultrasonic probe comprising:

- a housing;
- an ultrasonic module arranged inside the housing;
- at least one signal line which transmits/receives signals to/from the ultrasonic module;
- a support barrel which is supported by the housing, in which the at least one signal line is arranged and an outer surface of which has at least one ring electrode which electrically connects the at least one signal line to the ultrasonic module; and
- a rotation barrel which is rotatable around the support barrel in one direction and supports the ultrasonic module so as to maintain an electrical contact of the ultrasonic module to the at least one ring electrode.

2. The ultrasonic probe of claim 1, wherein the ultrasonic module is formed to be rotatable at least about 360° in one direction due to the rotation barrel.

3. The ultrasonic probe of claim 1, wherein the at least

one ring electrode is continuously formed along a circumference direction of the support barrel.

4. The ultrasonic probe of claim 1, wherein the at least one ring electrode comprises a plurality of ring electrodes, and the plurality of ring electrodes are arranged to be separated from each other along a lengthwise direction of the support barrel.

5. The ultrasonic probe of claim 1, wherein the ultrasonic module further comprises contact electrodes protruding towards the support barrel from an inside of the rotation barrel.

6. The ultrasonic probe of claim 5, wherein the contact electrodes are bent due to a contact with the at least one ring electrode.

7. The ultrasonic probe of claim 1, wherein the ultrasonic probe further comprises a driving unit which rotates the rotation barrel.

8. The ultrasonic probe of claim 1, wherein the ultrasonic module rotates about a rotation axis which is perpendicular to a lengthwise direction of the housing.

9. The ultrasonic probe of claim 8, wherein the ultrasonic module further comprises a controller which makes the ultrasonic module transmit or receive ultrasonic signals at some of regions where the ultrasonic module rotates while the ultrasonic module rotates.

10. The ultrasonic probe of claim 1, wherein the ultrasonic module rotates about a rotation axis which is parallel to lengthwise direction of the housing.

11. An ultrasonic diagnostic apparatus comprising:

- an ultrasonic probe of any preceding claim;
- an image processor which generates an ultrasonic image based on the received echo signal; and
- a display unit which displays the generated ultrasonic image.

FIG. 1

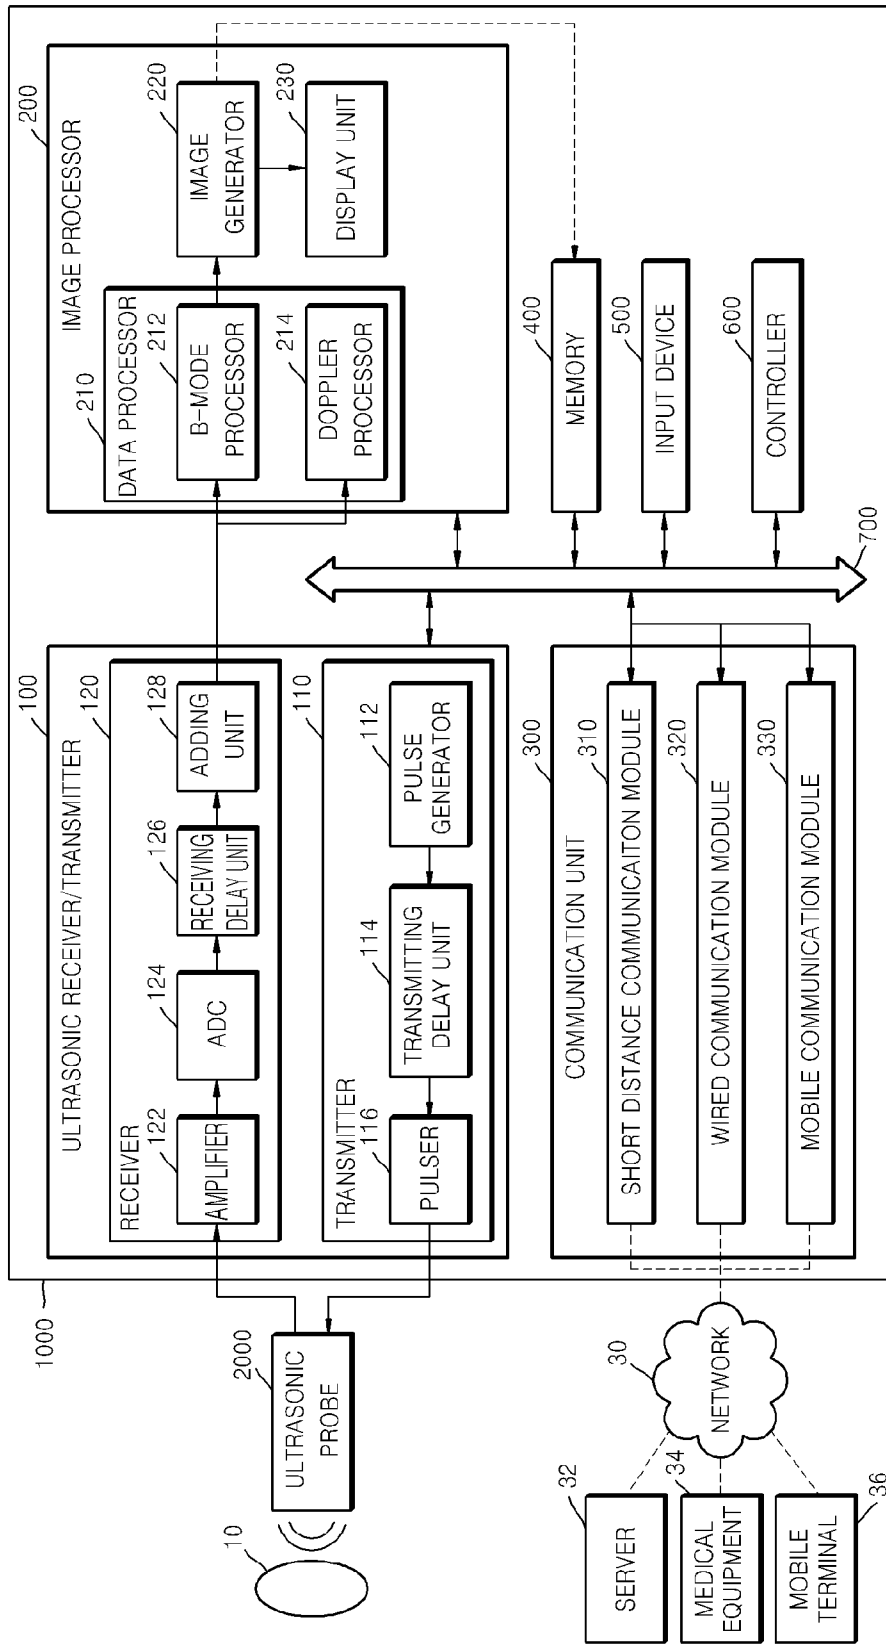


FIG. 2

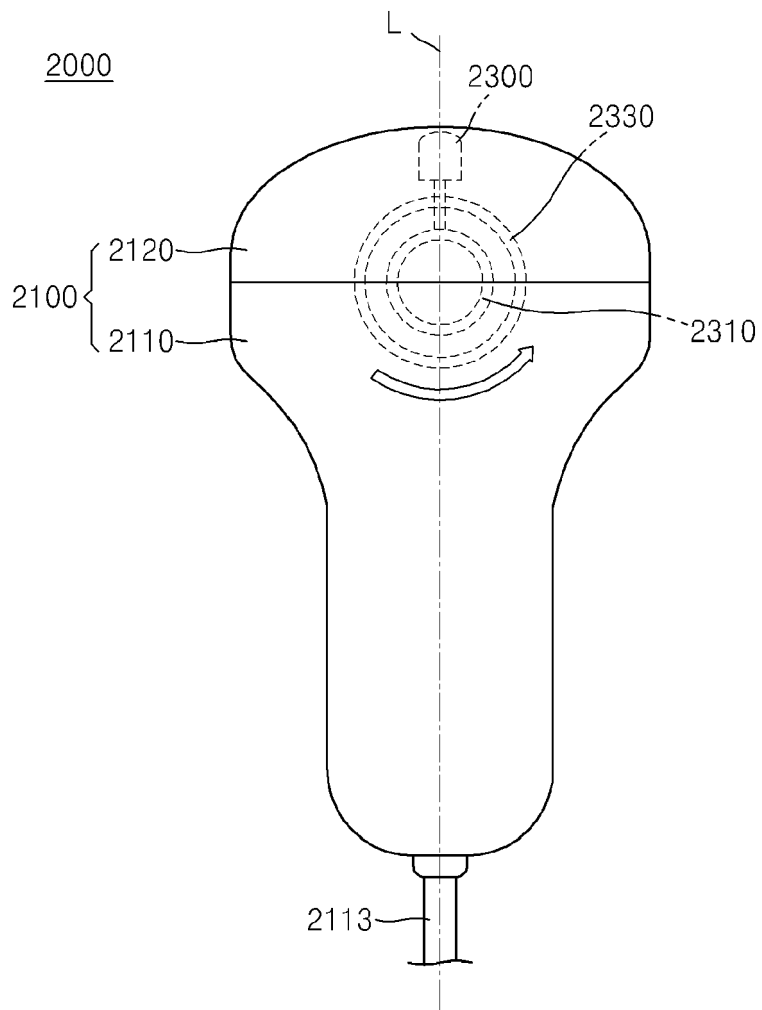


FIG. 3

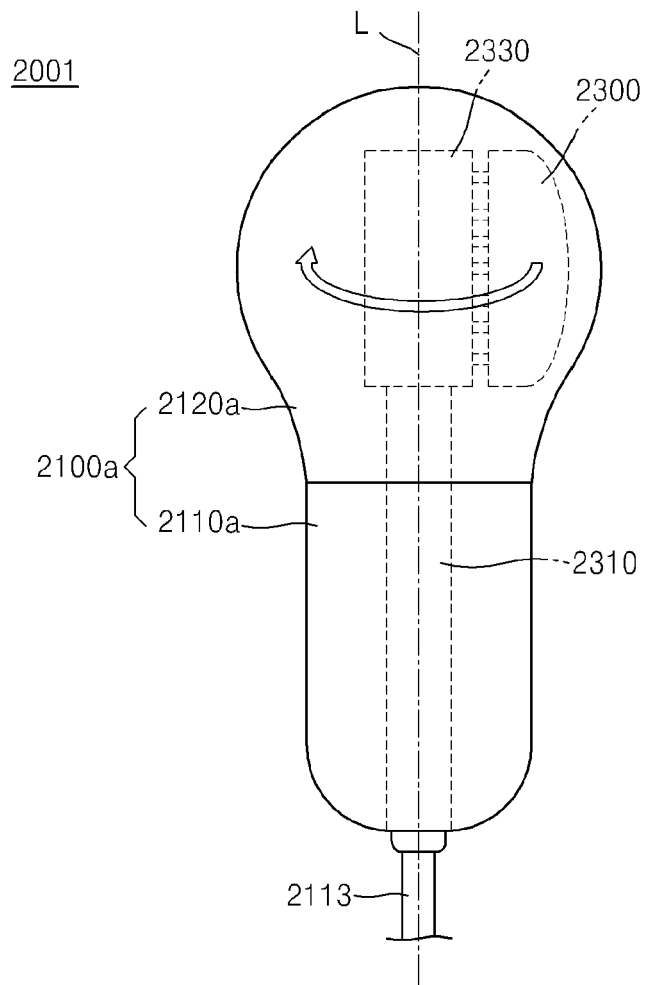


FIG. 4

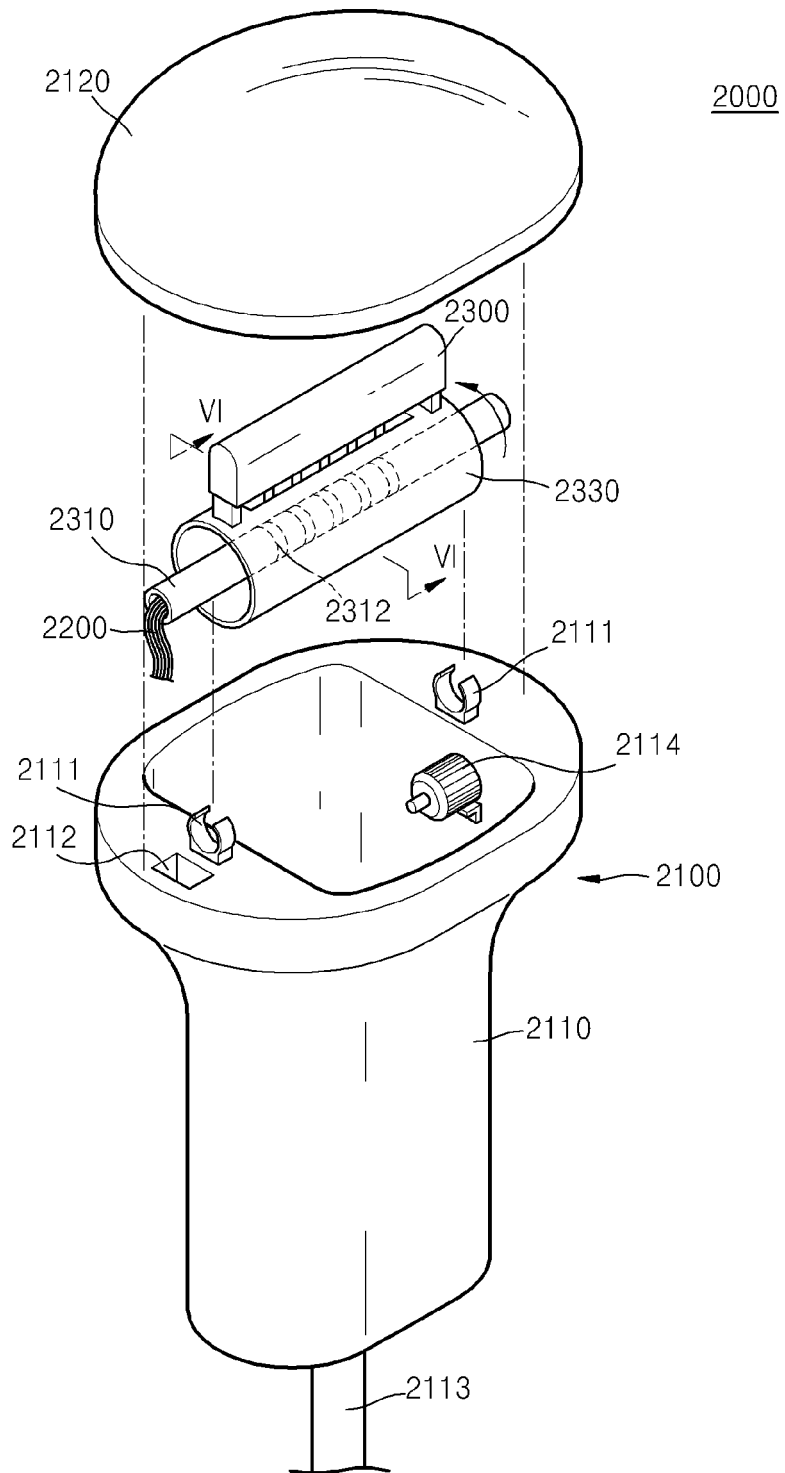


FIG. 5

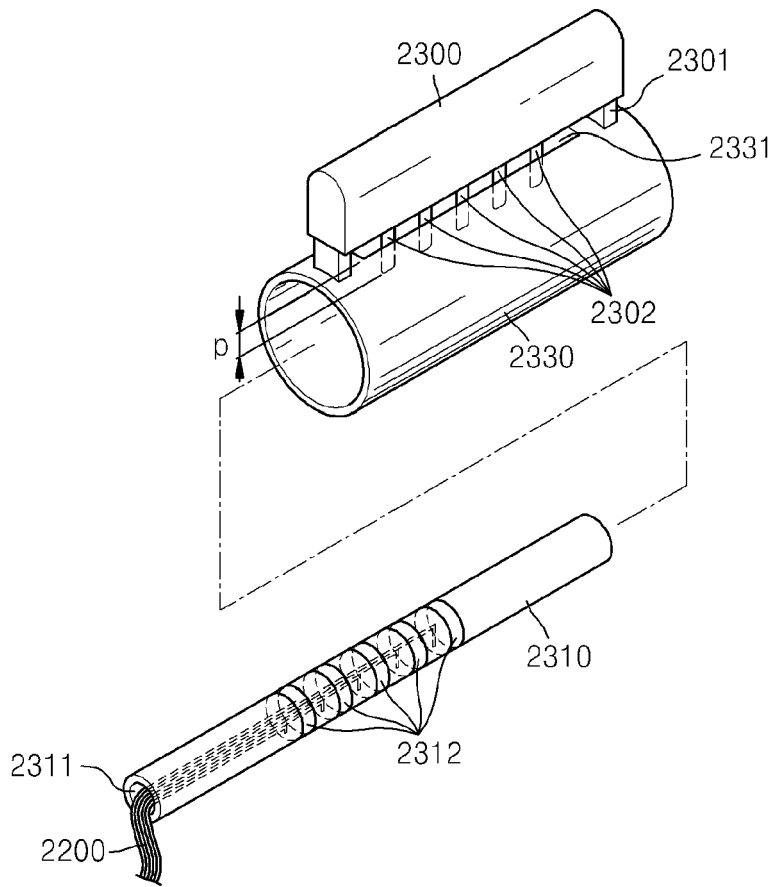


FIG. 6A

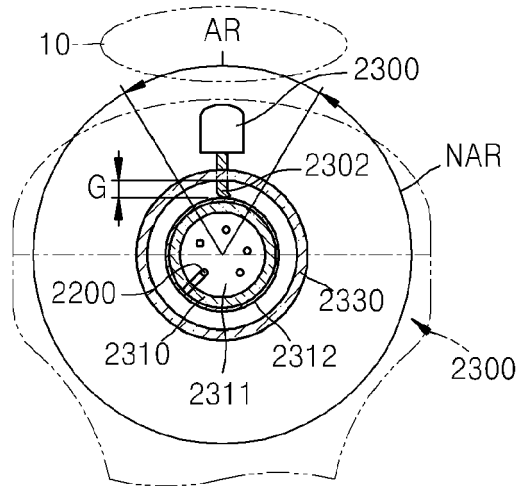


FIG. 6B

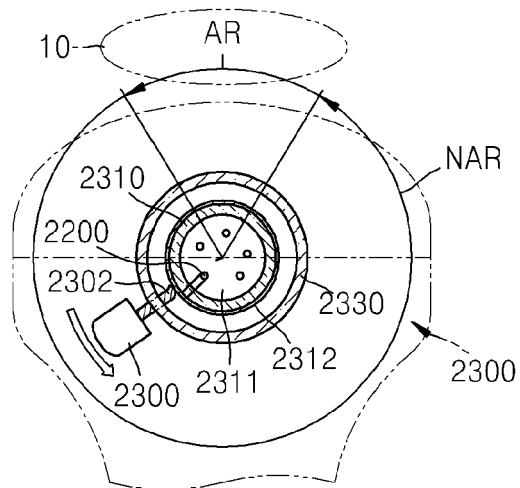


FIG. 6C


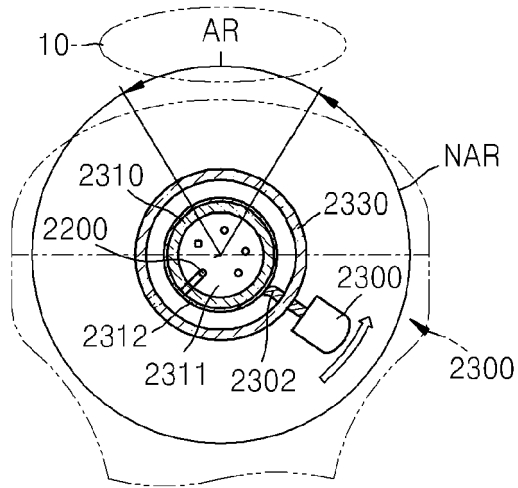


FIG. 7



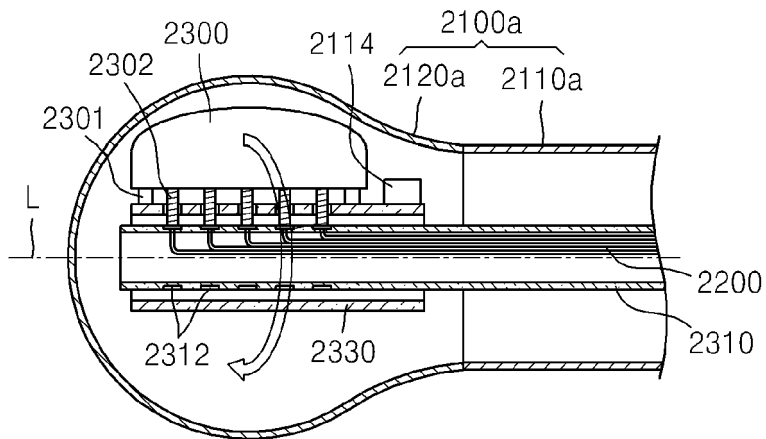

EUROPEAN SEARCH REPORT

Application Number
EP 14 17 6134

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 4 149 419 A (CONNELL JR RAYMOND S ET AL) 17 April 1979 (1979-04-17) * abstract; figures 1, 2, 5, 8 * * column 1, lines 5-9 * * page 2, lines 64-66 * * page 3, lines 5-6, 11-13 * * column 3, line 20 - column 4, line 40 * * column 5, line 5 - column 6, line 51 *	1-11	INV. A61B8/00
A	US 4 466 444 A (BABA KAZUO [JP]) 21 August 1984 (1984-08-21) * the whole document *	1-11	
A	US 4 231 373 A (WAXMAN ALBERT S ET AL) 4 November 1980 (1980-11-04) * the whole document *	1-11	
A	US 4 895 158 A (KAWABUCHI MASAMI [JP] ET AL) 23 January 1990 (1990-01-23) * the whole document *	1-11	
A	KR 2013 0132171 A (UNIV NAT CHONNAM IND FOUND [KR]) 4 December 2013 (2013-12-04) * the whole document *	1-11	TECHNICAL FIELDS SEARCHED (IPC) A61B
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 16 June 2015	Examiner Molina Silvestre, A
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

EPO FORM 1503 03.82 (F04C01)

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 14 17 6134

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

16-06-2015

10

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 4149419 A	17-04-1979	AU 4190878 A	31-05-1979
		CA 1101980 A1	26-05-1981
		DE 2851004 A1	07-06-1979
		FR 2409742 A1	22-06-1979
		GB 2008754 A	06-06-1979
		JP S5493882 A	25-07-1979
		US 4149419 A	17-04-1979

US 4466444 A	21-08-1984	DE 3275973 D1	14-05-1987
		EP 0065275 A1	24-11-1982
		JP S6334737 B2	12-07-1988
		JP S57190552 A	24-11-1982
		US 4466444 A	21-08-1984

US 4231373 A	04-11-1980	AU 544671 B2	13-06-1985
		AU 4698679 A	24-01-1980
		CA 1127750 A1	13-07-1982
		DE 2928560 A1	07-02-1980
		FR 2431811 A1	15-02-1980
		GB 2027197 A	13-02-1980
		GB 2108267 A	11-05-1983
		JP S5516687 A	05-02-1980
		NL 7904046 A	22-01-1980
		US 4231373 A	04-11-1980

US 4895158 A	23-01-1990	DE 3751117 D1	06-04-1995
		DE 3751117 T2	20-07-1995
		DE 3783281 D1	11-02-1993
		DE 3783281 T2	22-07-1993
		EP 0253268 A1	20-01-1988
		EP 0460711 A2	11-12-1991
		US 4895158 A	23-01-1990

KR 20130132171 A	04-12-2013	NONE	

45

50

55

EPO FORM P0489

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 1020140011526 [0001]

专利名称(译)	超声波探头和包括其的超声波诊断装置		
公开(公告)号	EP2901938A1	公开(公告)日	2015-08-05
申请号	EP2014176134	申请日	2014-07-08
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	MIN HAE KEE		
发明人	MIN, HAE-KEE		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4461 A61B8/466 B06B1/0622 G10K11/346 G10K11/352 G10K15/00		
代理机构(译)	SCHMID , WOLFGANG		
优先权	1020140011526 2014-01-29 KR		
其他公开文献	EP2901938B1		
外部链接	Espacenet		

摘要(译)

提供一种超声波探头，包括：壳体；超声波模块；至少一条信号线；支撑筒，由壳体支撑，其中布置有至少一个信号线，并且其外表面具有至少一个环形电极，该环形电极将至少一个信号线电连接到超声波模块；旋转筒可沿一个方向绕支撑筒旋转，并支撑超声波模块，以保持超声波模块与至少一个环形电极的电接触。

FIG. 5

