

(19)



(11)

EP 3 184 051 A2

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication:
28.06.2017 Bulletin 2017/26

(51) Int Cl.:
A61B 8/08 (2006.01) **A61B 8/06 (2006.01)**
A61B 8/00 (2006.01)

(21) Application number: **16205350.8**

(22) Date of filing: **20.12.2016**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME
Designated Validation States:
MA MD

(72) Inventors:
• **CHEN, Argon**
 105 Taipei (TW)
• **CHEN, Jia-Jiun**
 105 Taipei (TW)
• **SHEN, Yu-Han**
 105 Taipei (TW)
• **LIU, Cheng-Hsien**
 105 Taipei (TW)

(30) Priority: **23.12.2015 TW 104143257**

(74) Representative: **Sticht, Andreas**
Kraus & Weisert
Patentanwälte PartGmbH
Thomas-Wimmer-Ring 15
80539 München (DE)

(71) Applicant: **AmCad BioMed Corporation**
Taipei City 10547 (TW)

(54) **CLUSTERING, NOISE REDUCTION AND VISUALIZATION METHOD FOR DOPPLER ULTRASOUND IMAGES**

(57) The invention provides an analysis system for Doppler ultrasound image includes: a capture device, a processing device, and an output device. The capture device obtains a plurality of Doppler ultrasound images. The processing device arranges the color value in each pixel of the images based on the time domain, and obtains a reference sequence through a referencing method, furthermore performs a clustering method to obtain

a plurality of correlation coefficient values, then uses a clustering and noise reducing method to classify into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal, finally annotates the primary pulsatile signal, a secondary pulsatile signal, and a noise signal with different color values, respectively. The output device displays a plurality of visualized pulsatile ultrasound images for visualization.

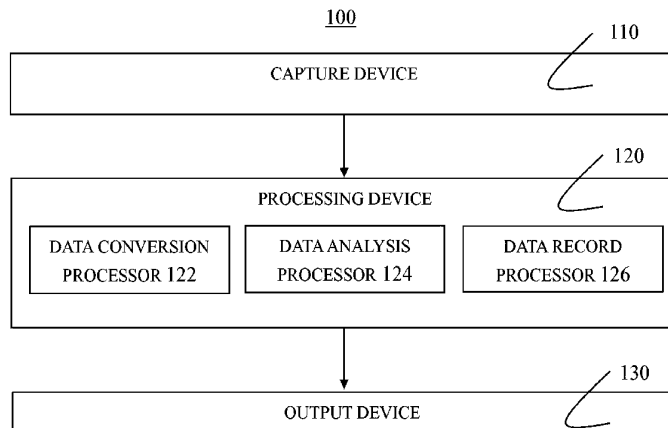


FIG. 1

EP 3 184 051 A2

Description**BACKGROUND OF THE INVENTION**5 Field of the Invention

[0001] The invention relates to a method of Doppler ultrasound images clustering, noise reduction and visualization. In particular, a method implemented in an image processing system for Doppler ultrasound images.

10 Descriptions of the Related Art

[0002] Receiving of ultrasound images may be distinguished as power Doppler ultrasound image and color Doppler ultrasound image. Power Doppler ultrasound image shows complete artery and vein image, but it does not have direction information on blood flow. Nevertheless color Doppler ultrasound image only shows indirect direction information on blood flow. Otherwise, noise in the Doppler ultrasound images caused by the motion artifacts is also a critical problem for explaining the blood flow information. Thus, some patients should keep stationary during the Doppler examination because breathing may produce motion artifacts. Additionally, there are probe motion artifacts which may be arisen by using a hand-held probe (called a transducer) which is placed directly on and moved over the patient. Therefore, it is necessary to provide a suitable noise-reduced Doppler ultrasound image for evaluating the completely pulsatile information on blood flow.

[0003] In the prior art, Taiwan Patent No. 1275,383 in and US patent No. 8,047,993 B2 disclose a non-invasive measurement method of tumor hemodynamic parameters to detect the degree of malignancy in tumors. The method comprises the steps of: using a power Doppler ultrasound unit to scan a tumor and capture sequential color images in a heartbeat cycle, and choosing an area of interest (AREA_ROI) from the images, labeling pixels reflecting signals of blood flow in the images during one heartbeat cycle to contour an area of tumor blood vessels (AREA_vessel); calculating a difference of PDVI between maximal systolic pressure and diastolic pressure during the heartbeat cycle to obtain tumor differential vascularity index (TDVI), in which PDVI is the ratio obtained by dividing pixels of AREA_vessel by total area in the section of AREA_ROI to determine the degree of malignancy by the TDVI. It can be applied to clinical diagnostic.

[0004] Furthermore, US patent No. 8,047,993 B2 discloses a method for evaluation of renal perfusion with power Doppler ultrasonography. Serial renal vascular images at different vascular areas including the whole vascular tree, interlobar, arcuate, and interlobular vessels were captured. Imaging processing software was designed to analyze the changes of power Doppler intensity of colored pixels within regions of interest (ROI). Power Doppler Vascularity index (PDVI) has been defined as the percentage of vascular perfusion within a region of interest (ROI). The renal vascular perfusion index (RVPI) was defined as the maximal power Doppler vascular index which divided by minimal power Doppler vascular index (PDVI max/PDVI min) among the serial images. The mean of weighted power Doppler vascular index (WPDVI mean) was defined as the average of the intensity of colored pixels among the ROI within the serial images. By using the RVPI and WPDVI mean, a more dynamic sense of vascular perfusion and a novel approach for the evaluation of renal vascular function in clinical practice can be provided.

[0005] However, TW 1275383, US 8,047,993 B2 and US 8,777,860 B2 do not disclose clustering methods for evaluation of pulsatile information from blood flow in a sequence of power Doppler ultrasound images and the color Doppler ultrasound images. In particular, the present invention provides a method and system to quantify and classify the color pixels in the Doppler ultrasound images into three groups, namely the primary pulsatile signal, the secondary pulsatile signal, and noise signal based on the intensity changes of each color pixel over the sequence of Doppler ultrasound images. The classified signals will be visualized with different color values. Therefore, methods and systems in this invention provide the noise-reduced pulsatile signal images for reflecting pulsatile information form blood flow in the images, which is intended for vascular pulsatility analysis.

SUMMARY OF THE INVENTION

50 **[0006]** The present invention provides a system of clustering, noise reduction and visualization for Doppler ultrasound image as defined in claim 1. The dependent claims define further embodiments. The Doppler ultrasound image processing system comprises a capture device, a processing device, and an output device, wherein the processing device further comprises a data conversion processor, a data analysis processor, and a data record processor.

[0007] The capture device obtains a plurality of Doppler ultrasound images based on a time domain, wherein each Doppler ultrasound image comprises a color value in each pixel.

[0008] The data conversion processor arranges each color value in each pixel of the Doppler ultrasound images based on the time domain to obtain a plurality of color value sequences.

[0009] The data analysis processor calculates the color value sequences through a referencing method to obtain a

reference sequence, and compares the reference sequence with each color value sequences through a clustering method to obtain a plurality of correlation coefficient values, then classifies the color value sequences into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal based on the correlation coefficient values through a clustering and noise reduction method.

5 [0010] The data record processor annotates the color values of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal to obtain a plurality of visualized pulsatile ultrasound images.

[0011] The output device is connected to the processing device for displaying the visualized pulsatile ultrasound images.

10 [0012] In an embodiment of the invention, a method as defined in claim 16 implemented in an image processing system of clustering, noise reduction and visualization for Doppler ultrasound image, which comprises: obtaining a plurality of Doppler ultrasound images based on time domain, wherein each Doppler ultrasound image comprises a color value in each pixel; and arranging each color value in each pixel of Doppler ultrasound images based on the time domain to obtain a plurality of color value sequences.

15 [0013] The method further comprises: calculating the color value sequences through a referencing method to obtain a reference sequence; comparing the reference sequence with each color value sequences through a clustering method to obtain a plurality of correlation coefficient values; using a clustering and noise reduction method to classify the color value sequences into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal based on the correlation coefficient values; and annotating the color values of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal to obtain a plurality of visualized pulsatile ultrasound images.

20 [0014] Other systems, methods, features, and advantages of the present invention will be or become apparent to one with skill in the art upon examination of following drawings and detailed description. It is intended that all such additional systems, methods, features, and advantages be included within this description, be within the scope of the present invention, and be protected by the accompanying claims.

BRIEF DESCRIPTION OF THE DRAWINGS

25 [0015] Many aspects of the disclosure can be better understood with reference to the following drawings. The components in the drawings are not necessarily to scale, emphasis instead being placed upon clearly illustrating the principles of the present invention. Moreover, in the drawings, like reference numerals designate corresponding parts throughout the several views.

30 FIG. 1 is a block diagram of this system of clustering, noise reduction and visualization method for Doppler ultrasound image in accordance with various embodiments of the present invention.

35 FIG. 2A illustrates a sequence of Doppler ultrasound images based on a time domain in accordance with various embodiments.

FIG. 2B illustrates an arrangement of a plurality of color value sequences based on a time domain in accordance with various embodiments.

40 FIG. 3 illustrates a diagram for clustering and noise reduction method in accordance with various embodiments of the present invention.

45 FIG. 4 illustrates common carotid artery and internal jugular vein in the original power Doppler ultrasound image and the corresponding visualized pulsatile ultrasound image in accordance with one embodiment of the present invention.

FIG. 5 illustrates common carotid artery and internal jugular vein in the original color Doppler ultrasound image and the corresponding visualized pulsatile ultrasound image in accordance with one embodiment of the present invention.

50 FIG. 6 illustrates renal artery and renal vein in the original power Doppler ultrasound image and the corresponding visualized pulsatile ultrasound image in accordance with one embodiment of the present invention.

55 FIG. 7 illustrates brachial artery and brachial vein of arm in the original power Doppler ultrasound image and the corresponding visualized pulsatile ultrasound image in accordance with one embodiment of the present invention.

FIG. 8 illustrates a diagram for reclassifying the color values to obtain the visualized pulsatile ultrasound image in accordance with one embodiment of the present invention.

FIG. 9 illustrates intensity change value trends of the visualized pulsatile ultrasound image in accordance with one embodiment of the present invention.

FIG. 10 is a flowchart for the method of clustering, noise reduction and visualization for Doppler ultrasound images according to various embodiments of the present invention.

DESCRIPTION OF THE PREFERRED EMBODIMENT

[0016] Having summarized various aspects of the present invention, reference will now be made in detail to the description of the disclosure as illustrated in the drawings. However, these embodiments are not intended to limit the present invention to any environment, applications, or implementations described in these embodiments. Therefore, description of these embodiments is only for purpose of illustration rather than to limit the scope of the present invention. It shall be appreciated that elements unrelated to the present invention are omitted from depiction in the following embodiments and the attached drawings.

[0017] The present invention discloses a method of clustering, noise reduction and visualization for Doppler ultrasound image. It should be noted that the method provides merely an example of the many different types of functional arrangements that may be employed to implement the operation of the various components of a system, a computer system, a multiprocessor computing device, and so forth. The execution steps of the present invention may include application specific software which may store in any portion or component of the memory including, for example, random access memory (RAM), read-only memory (ROM), hard drive, solid-state drive, magneto optical (MO), IC chip, USB flash drive, memory card, optical disc, or other memory components.

[0018] For some embodiments, the system comprises a capture device, a processing device, and an output device. The capture device is used to provide data such as image, text or control signals to the processing device such as a computer or other information appliance. The processing device performs data calculations, data comparisons, and data copying. Finally, the information from the analyzing system can be provided by the processing device and presented on the output device such as CRT monitors, LCD monitors and displays, gas plasma monitors, and televisions. The output device visually conveys text, graphics, and spectrum. Information shown on the output device is called soft copy because the information exists electronically and is displayed for a temporary period of time.

[0019] In accordance with some embodiments, the system further comprises of a storage medium and a memory. For example and without limitation, the storage medium can be a hard drive, an optical device or a remote database server coupled to a network, and storage software. The memory typically is the processor in which information is encoded, stored, and retrieved etc. The software can be stored in the memory and executed by the processing device when the computer system executes the method of clustering, noise reduction and visualization for Doppler ultrasound image.

[0020] **FIG. 1** is a block diagram of a system **100** of clustering, noise reduction and visualization method for Doppler ultrasound image in accordance with various embodiments of the present invention. The Doppler ultrasound image processing system comprises a capture device **110**, a processing device **120**, and an output device **130**. The processing device **120** includes a data conversion processor **122**, a data analysis processor **124**, and a data record processor **126**.

[0021] Please refer to **FIG. 2A** and **FIG. 2B** together. **FIG. 2A** illustrates a sequence of Doppler ultrasound images in accordance with various embodiments. **FIG. 2B** illustrates an arrangement of a plurality of color value sequences based on a time domain in accordance with various embodiments. The capture device **110** acquires a plurality of Doppler ultrasound images (I frames) **210** based on a time domain, wherein each Doppler ultrasound image comprises a color value in each pixel ($B_{j,i}$) **212**.

[0022] The data conversion processor **122** arranges the color value in each pixel ($j=1\sim J$) **212** of the Doppler ultrasound images based on the time domain ($i=1\sim I$) to obtain a plurality of color value sequences ($C_1, C_2, C_3, \dots, C_j$) **214**. Each of the color value sequences is a sequences showing intensity change of the pixels. For various embodiments, the sequence showing intensity change of the pixels (C_j) is obtained according to the following expression:

$$C_j = \{B_{j,i}\}, \quad i = 1, 2, 3, \dots, I \quad (\text{Equation 1})$$

wherein each $B_{j,i}$ of input data represents the intensity value of the j^{th} pixel at the i^{th} frame based on the definition of the intensity color map given by the original Doppler ultrasound image.

[0023] The data analysis processor **124** calculates the color value sequences through a referencing method to obtain a reference sequence (Cref). The referencing method comprises an intensity percentage method, an average standard deviation ratio method, an autocorrelation method, a hierarchical correlation method or any combination thereof.

[0024] In one embodiment, the data analysis processor **124** performs the intensity percentage method to obtain the reference sequence. The intensity percentage method comprises the steps of: arranging the color value sequences ($C_1,$

C2, C3, ...Cj) 214 according to the largest color value of each color value sequence to obtain a plurality of percentile ranks; choosing the color value sequences (j=1~J) which the percentile rank is within a predetermined rank range to obtain a reference group (R.G.); and averaging the color value sequences which the percentile rank belongs to the reference group to obtain the reference sequence. For various embodiments, the reference sequence is calculated according to the following expression:

$$C_{ref.} = \left\{ \frac{\sum_{j \in R.G.} B_{ji}}{J'} \right\}, \quad i = 1, 2, \dots, I \quad (\text{Equation 2})$$

[0025] In another embodiment, the data analysis processor **124** performs the average standard deviation ratio method to obtain the reference sequence. The average standard deviation ratio method comprises the steps of: calculating the color value in each pixel of color value sequences (j=1~J) to obtain a plurality of standard (Stdj) values; and dividing the standard (Stdj) values by an average value of the standard values (Std Avg) to obtain a plurality of average standard deviation ratio (Avg STD ratio) values. The average standard deviation ratio value is calculated according to the following expression:

$$\text{Avg STD ratio} = \frac{\text{Std}_j}{\text{Std Avg}} = \frac{\text{Std of each } C_j}{\sum_{j=1}^J \frac{\text{Std}_j}{J}}, \quad \forall j \quad (\text{Equation 3})$$

[0026] Then, the reference group is obtained by choosing the color value sequences which the averaging standard deviation ratio value is within a predetermined ration range, and the reference sequence is obtained by averaging the color value sequences from the reference group.

[0027] In another embodiment, the data analysis processor **124** performs the autocorrelation method to obtain the reference sequence. The autocorrelation method comprises the steps of: calculating each color value sequence through an autocorrelation function with a plurality of lag varieties to obtain a plurality of autocorrelation function values; and choosing a color value sequence which has the smallest autocorrelation value to obtain the reference sequence.

[0028] In another embodiment, the data analysis processor **124** performs the hierarchical correlation method to obtain the reference sequence. The hierarchical correlation method comprises the following steps of: (a) gathering the color value sequences into an ith reference sequence set, wherein an initial value of i is 1; (b) obtaining a plurality of correlation coefficient values of the ith reference sequence set by calculating each pair of the color value sequences in the ith reference sequence set through a correlation function; (c) selecting the pair of the color value sequences in the ith reference sequence set, which have a largest correlation coefficient value; (d) averaging the selected pair of the color value sequences in the ith reference sequence set to generate a new color value sequence; (e) gathering the new color value sequence and the color value sequences in the ith reference sequence set except for the selected pair of the color value sequences into a (i+1)th reference sequence set; (f) obtaining a plurality of correlation coefficient values of the (i+1)th reference sequence set by calculating each pair of the color value sequences in the (i+1)th reference sequence set through the correlation function; (g) determining whether all of the correlation coefficient values of the (i+1)th reference sequence set are less than a predetermined correlation threshold; and (h) when one of the correlation coefficient values of the (i+1)th reference sequence set is not less than the predetermined correlation threshold, setting i=i+1 and repeating steps (c), (d), (e), (f) and (g), and when the all of the correlation coefficient values of the (i+1)th reference sequence set are less than the predetermined correlation threshold, outputting the color value sequence in the (i+1)th reference sequence set which is generated by averaging a most number of the color value sequences in the first reference sequence set as a reference sequence.

[0029] For example, the data analysis processor **124** performs the hierarchical correlation method on the eight color value sequences C₁, C₂, ..., C₈ to obtain the reference sequence. First, the data analysis processor **124** gathers the eight color value sequences C₁, C₂, ..., C₈ into a 1st reference sequence set. Next, the analysis processor **124** obtains the correlation coefficient values of the 1st reference sequence set by calculating each pair of the color value sequences in the 1st reference sequence set through the correlation function. On the assumption the pair of the color value sequences (i.e., C₂ and C₃) has the largest correlation coefficient value, the analysis processor **124** selects the pair of the color value sequences (i.e., C₂ and C₃) in the 1st reference sequence set, which have the largest correlation coefficient value, and averages the color value sequences C₂ and C₃ to generate a new color value sequence C'_{2,3}. Next, the analysis processor **124** gathers C'_{2,3} and the color value sequences C₁, C₄, C₅, C₆, C₇, C₈ into a 2nd reference sequence set. Similarly, the analysis processor **124** obtains the correlation coefficient values of the 2nd reference sequence set by

calculating each pair of the color value sequences in the 2th reference sequence set through the correlation function.

[0030] Afterwards, the analysis processor **124** determines whether all of the correlation coefficient values of the 2nd reference sequence set are less than a predetermined correlation threshold. Assuming there is at least one of the correlation coefficient values of the 2nd reference sequence set is not less than the predetermined correlation threshold, the analysis processor **124** selects the pair of the color value sequences in the 2nd reference sequence set, which have a largest correlation coefficient value. Then, on the assumption the pair of the color value sequences (C_1 and $C'_{2,3}$) has the largest correlation coefficient value, the analysis processor **124** selects the pair of the color value sequences (i.e., C_1 and $C'_{2,3}$) in the 2nd reference sequence set, which have the largest correlation coefficient value, and averages the pair of the color value sequences (i.e., C_1 and $C'_{2,3}$) to generate a new color value sequence $C'_{1,2,3}$.

[0031] Next, the analysis processor **124** gathers the new color value sequence $C'_{1,2,3}$ and the color value sequences C_4, C_5, C_6, C_7, C_8 into a 3rd reference sequence set. Similarly, the analysis processor **124** obtains the correlation coefficient values of the 3rd reference sequence set by calculating each pair of the color value sequences in the 3rd reference sequence set through the correlation function, and determines whether all of the correlation coefficient values of the 3rd reference sequence set are less than a predetermined correlation threshold. Assuming there is at least one of the correlation coefficient values of the 3rd reference sequence set is not less than the predetermined correlation threshold, the analysis processor **124** selects the pair of the color value sequences in the 3rd reference sequence set, which have a largest correlation coefficient value. Then, on the assumption the pair of the color value sequences (i.e., C_5 and C_6) has the largest correlation coefficient value, the analysis processor **124** selects the pair of the color value sequences (i.e., C_5 and C_6) in the 3rd reference sequence set, which have the largest correlation coefficient value, and averages the pair of the color value sequences (i.e., C_5 and C_6) to generate a new color value sequence $C'_{5,6}$.

[0032] Next, the analysis processor **124** gathers the new color value sequence $C'_{5,6}$ and the color value sequences $C'_{1,2,3}, C_4, C_7, C_8$ into a 4th reference sequence set. Similarly, the analysis processor **124** obtains the correlation coefficient values of the 4th reference sequence set by calculating each pair of the color value sequences in the 4th reference sequence set through the correlation function, and determines whether all of the correlation coefficient values of the 4th reference sequence set are less than the predetermined correlation threshold.

[0033] On the assumption that all of the correlation coefficient values of the 4th reference sequence set are less than the predetermined correlation threshold, the analysis processor **124** outputs the color value sequence $C'_{1,2,3}$ in the 4th reference sequence set which is generated by averaging the most number (i.e., 3) of the color value sequences (i.e., C_1, C_2 and C_3) in the first reference sequence set as a reference sequence.

[0034] The data analysis processor **124** compares the reference sequence with each color value sequences through a clustering method to obtain the correlation coefficient values. The clustering method comprises a correlation grouping method, a grouping with lag-correlation method or a two-centers correlation clustering method or any combination thereof.

[0035] In an embodiment, the data analysis processor **124** performs the correlation grouping method to obtain the correlation coefficient values. The correlation grouping method comprises the step of: calculating each color value sequence with the reference sequence through a correlation function to obtain the correlation coefficient values of the color value sequences.

[0036] In another embodiment, the data analysis processor **124** performs the grouping with lag-correlation method to obtain the correlation coefficient values and the lag varieties. The grouping with lag-correlation method comprises the steps of: calculating each color value sequences with the reference sequence through a correlation function with a plurality of lag varieties to obtain a plurality of correlation coefficient values; and choosing the largest correlation coefficient value and the corresponding lag variety to obtain the correlation coefficient value and the lag variety of each color value sequence.

[0037] In another embodiment, the data analysis processor **124** performs the two-centers correlation clustering method to obtain a plurality of correlation coefficient values. The two-centers correlation clustering method comprises the following steps of: (a) gathering the color value sequences into an operation set; (b) calculating each of the color value sequences in the operation set with the reference sequence through a correlation function to obtain a plurality of temporary correlation coefficient values of the color value sequences; (c) removing the color value sequence with the smallest temporary correlation coefficient value from the operation set and assigning the smallest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence with the smallest temporary correlation coefficient value; (d) removing the color value sequence with the largest temporary correlation coefficient value and assigning the largest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence with the largest temporary correlation coefficient value; (e) updating the reference sequence by averaging the color value sequence with the largest temporary correlation coefficient value and the reference sequence; and (f) repeating steps (b), (c), (d), and (e) until all of the color value sequences are assigned with the correlation coefficient values.

[0038] For example, the data analysis processor **124** performs the two-centers correlation clustering method on the eight color value sequences C_1, C_2, \dots, C_8 to obtain the plurality of correlation coefficient values. First, the data analysis processor **124** gathers the eight color value sequences C_1, C_2, \dots, C_8 into an operation set. Next, the analysis processor **124** obtains a plurality of temporary correlation coefficient values of the color value sequences by calculating each of

the color value sequences C_1, C_2, \dots, C_8 in the operation set with the reference sequence through a correlation function. On the assumption the color value sequence C_8 has the smallest temporary correlation coefficient value and the color value sequence C_2 has the largest temporary correlation coefficient value. Thereafter, the analysis processor **124** removes the color value sequence C_8 from the operation set and assigns the smallest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_8 . Similarly, the analysis processor **124** removes the color value sequence C_2 from the operation set and assigns the largest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_2 . Afterwards, the analysis processor **124** update the reference sequence by averaging the color value sequence C_2 (which has the largest temporary correlation coefficient value) and the current reference sequence.

[0039] Next, the analysis processor **124** obtains a plurality of temporary correlation coefficient values of the color value sequences by calculating each of the color value sequences $C_1, C_3, C_4, C_5, C_6, C_7$ in the operation set with the updated reference sequence through the correlation function. On the assumption the color value sequences C_3 has the smallest temporary correlation coefficient value and the color value sequence C_1 has the largest temporary correlation coefficient value. Thereafter, the analysis processor **124** removes the color value sequence C_3 from the operation set and assigns the smallest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_3 . Similarly, the analysis processor **124** removes the color value sequence C_1 from the operation set and assigns the largest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_1 . Afterwards, the analysis processor **124** updates the reference sequence again by averaging the color value sequence C_1 (which has the largest temporary correlation coefficient value) and the current reference sequence.

[0040] Next, the analysis processor **124** obtains a plurality of temporary correlation coefficient values of the color value sequences by calculating each of the color value sequences (C_4, C_5, C_6, C_7) in the operation set with the updated reference sequence through the correlation function. On the assumption the color value sequence C_4 has the smallest temporary correlation coefficient value and the color value sequence C_7 has the largest temporary correlation coefficient value. Thereafter, the analysis processor **124** removes the color value sequences C_4 from the operation set and assigns the smallest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_4 . Similarly, the analysis processor **124** removes the color value sequence C_7 with the largest temporary correlation coefficient value from the operation set and assigns the largest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_7 .

[0041] Once again, the analysis processor **124** updates the reference sequence again by averaging the color value sequence C_7 (which has the largest temporary correlation coefficient value) and the current reference sequence. Afterwards, the analysis processor **124** obtains a plurality of temporary correlation coefficient values of the color value sequence by calculating the color value sequence (C_5, C_6) in the operation set with the updated reference sequence through the correlation function.

[0042] On the assumption the color value sequence C_6 has the smallest temporary correlation coefficient value and the color value sequence C_5 has the largest temporary correlation coefficient value. Thereafter, the analysis processor **124** removes the color value sequences C_6 from the operation set and assigns the smallest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_6 . Similarly, the analysis processor **124** removes the color value sequence C_5 from the operation set and assigns the largest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence C_5 . By the aforesaid operations all of the color value sequences (C_1, C_2, \dots, C_8) are assigned with their correlation coefficient values.

[0043] The data analysis processor **124** classifies the color value sequences into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal based on the correlation coefficient values through a clustering and noise reduction method.

[0044] FIG. 3 illustrates a diagram for clustering and noise reduction method in accordance with various embodiments of the present invention. The data analysis processor **124** performs the clustering and noise reduction method comprising the steps of: classifying the color value sequences into the primary pulsatile signal if the correlation coefficient value within a main correlation coefficient threshold **300** and the lag variety within a main lag-coefficient threshold **302, 304**; and classifying the color value sequences into the secondary pulsatile signal if the correlation coefficient values within a secondary correlation coefficient threshold **306, 308** and the lag variety within a secondary lag-coefficient threshold **310**. The data analysis processor **124** further classifies the remaining color value sequences into the noise signal.

[0045] FIG. 4 illustrates common carotid artery **402** and internal jugular vein **404** in the original power Doppler ultrasound image **400** and the visualized pulsatile ultrasound images **410** in accordance with various embodiments of the present invention. The data analysis processor **124** performs the referencing method based on the combination of the intensity percentage and the average standard methods. The data analysis processor **124** further performs the clustering method based on the correlation grouping method, and then performs the clustering and noise reduction method.

[0046] The data analysis processor **124** chooses the color value sequences which the percentile rank is within a predetermined rank range, and chooses the color value sequences which the averaging standard ration value is within a predetermined ration range to obtain the reference group, wherein the predetermined rank range is less than 5% and

predetermined ration range is less than 0.1. The data analysis processor **124** averages the color value sequences in the reference group to obtain the reference sequence.

[0047] The data analysis processor **124** classifies the color value sequences into the primary pulsatile signal **412** if the correlation coefficient value within a main correlation coefficient range, which is between 0.6 and 1.0, and classifies the color value sequences into the secondary pulsatile signal **414** if the correlation coefficient values within a secondary correlation coefficient threshold, which is between -1.0 and 0.4. The data analysis processor **124** further classifies the remaining color value sequences into the noise signal **416**.

[0048] The data record processor **126** obtains a sequence of pulsatile ultrasound images **410** by classifying the color value sequences into three groups: the primary pulsatile signal, the secondary pulsatile signal, and the noise signal. The pixels of the primary pulsatile signal **412** in the visualized pulsatile ultrasound images **410** are displayed in first color values (e.g., warm colors from yellowish to dark red). The pixels of the secondary pulsatile signal **414** in the visualized pulsatile ultrasound images **410** are display in second color values (e.g., cold colors from light cyan to dark blue). The pixels of the noise signal are display in a third color value (e.g., a white color).

[0049] **FIG. 5** illustrates common carotid artery **502** and internal jugular vein **504** in the original color Doppler ultrasound image **500** and the visualized pulsatile ultrasound image **510** in accordance with various embodiments of the present invention. The data analysis processor **124** performs the referencing method based on the combination of the intensity percentage method and the autocorrelation method. The data analysis processor **124** further performs the clustering method based on the two-centers correlation clustering method, and then performs the clustering and noise reduction method.

[0050] The data analysis processor **124** selects the plurality of color value sequences which the percentile rank is within a predetermined rank range, wherein the predetermined rank range is less than 10%. The plurality of color value sequences are calculated by the autocorrelation function calculation with lag varieties from 5 to 8. The data analysis processor **124** chooses the color value sequence which has the smallest autocorrelation function value to obtain the reference sequence.

[0051] Then, the data analysis processor **124** obtains a plurality of correlation coefficient values by calculating each color value sequence with the reference sequence through a correlation function. The data analysis processor **124** chooses the color value sequence with the smallest correlation coefficient value to obtain a minimum correlation coefficient value, and chooses the color value sequence with the largest correlation coefficient value to obtain a maximum correlation coefficient value.

[0052] The data analysis processor **124** averages the color value sequences which belong to the maximum correlation coefficient value and the reference sequence to obtain an updated reference sequence. Afterwards, the data analysis processor **124** obtains the correlation coefficient values of all color value sequence by calculate each remaining color value sequence with the updated reference sequence through the correlation function in sequence.

[0053] Furthermore, the data analysis processor **124** classifies the color value sequences into the primary pulsatile signal **512** if the correlation coefficient value within a main correlation coefficient threshold, wherein the main correlation coefficient threshold is between 0.6 and 1.0. The pixels of the primary pulsatile signal **512** in the visualized pulsatile ultrasound image are annotated by first color values (e.g., warm color values from light yellow to dark red).

[0054] The data analysis processor **124** classifies the color value sequences into the secondary pulsatile signal **514** if the correlation coefficient values within a secondary correlation coefficient threshold, wherein the secondary correlation coefficient threshold is between -1.0 and 0.4. The pixels of the secondary pulsatile signal **514** in the visualized pulsatile ultrasound image are annotated by second color values (e.g., cold color values from light cyan to dark blue).

[0055] The data analysis processor **124** classifies the remaining color value sequences into the noise signal **516** in a third color value (e.g., a white color). The data record processor **126** displays the visualized pulsatile ultrasound images **510** for visualization of the primary pulsatile signal **512**, the secondary pulsatile signal **514** and the noise signal **516** based on clustering and noise reduction methods.

[0056] **FIG. 6** illustrates renal artery **602** and renal vein **604** in the original power Doppler ultrasound image **600** and the visualized pulsatile ultrasound images **610** in accordance with various embodiments of the present invention. The data analysis processor **124** performs the referencing method based on hierarchical correlation method to obtain the reference sequence, as aforementioned. Then, the data analysis processor **124** further performs the clustering method based on correlation grouping method to obtain the correlation coefficient values of the color value sequences by calculating each color value sequence with the reference sequence through a correlation function to obtain the correlation coefficient values.

[0057] Next, the data analysis processor **124** performs the clustering and noise reduction method as follows. The data analysis processor **124** classifies the color value sequences into the primary pulsatile signal **612** if the correlation coefficient value within a main correlation coefficient threshold, e.g., the main correlation coefficient threshold is between 0.6 and 1.0. The pixels of the primary pulsatile signal **612** in the visualized pulsatile ultrasound image are annotated by first color values (e.g. warm color values from yellowish to dark red) for showing the intensity changes of pixels.

[0058] The data analysis processor **124** classifies the color value sequences into the secondary pulsatile signal **614**

if the correlation coefficient values within a secondary correlation coefficient threshold, e.g., the secondary coefficient threshold is between -1.0 to 0.2. The pixels of the secondary pulsatile signal **612** in the visualized pulsatile ultrasound image are annotated by second color values (e.g., cold color values from light cyan to dark blue) for showing the intensity changes of pixels.

5 **[0059]** The data analysis processor **124** classifies remaining color value sequences into the noise signal **616**. The data record processor **126** displays the visualized pulsatile ultrasound images **610** for visualization of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal based on clustering and noise reduction methods.

10 **[0060]** FIG. 7 illustrates brachial artery **702** and brachial vein **704** of arm in the original power Doppler ultrasound image **700** and the visualized pulsatile ultrasound image **710** in accordance with various embodiments of the present invention. The data analysis processor **124** performs the referencing method based on the combination of the intensity percentage method and the average standard deviation ratio method. The data analysis processor **124** further performs the clustering method based on the grouping with lag-correlation method, and then performs the clustering and noise reduction method.

15 **[0061]** The data analysis processor **124** arranges the color value sequences according to the largest color value of each of the color value sequences to obtain a plurality of percentile ranks. The data analysis processor **124** chooses the color value sequences which the percentile rank is within a predetermined rank range, and chooses the color value sequences which the averaging standard ration value is within a predetermined ration range to obtain the reference group, wherein the predetermined rank range is less than 5% and predetermined ration range is less than 0.1. The data analysis processor **124** averages the color value sequences in the reference group to obtain the reference sequence.

20 **[0062]** Then, the data analysis processor **124** performs the grouping with lag-correlation method to obtain the correlation coefficient values, and calculates each color value sequences with the reference sequence through a correlation function with a plurality of lag varieties to obtain a plurality of correlation coefficient values, wherein the range of the lag varieties are 0 to 8.

25 **[0063]** Furthermore, the data analysis processor **124** chooses the largest correlation coefficient value and the corresponding lag variety to obtain the correlation coefficient value and the lag variety of each color value sequence. The data analysis processor **124** classifies the color value sequences into the primary pulsatile signal **712** if the correlation coefficient value within a main correlation coefficient threshold and the lag variety within a main lag-coefficient threshold, e.g., the main correlation coefficient threshold is between -0.2 and 1.0 and the main lag-coefficient threshold is between 0 and 1. The pixels of the primary pulsatile signal **712** in the visualized pulsatile ultrasound image are annotated by first color values (e.g., warm color values from light yellow to dark red).

30 **[0064]** The data analysis processor **124** classifies the color value sequences into the secondary pulsatile signal **714** if the correlation coefficient values within a secondary correlation coefficient threshold and the lag variety within a secondary lag-coefficient threshold, e.g., the secondary correlation coefficient threshold is between -0.2 and 1.0 and the secondary lag-coefficient threshold is between 2 and 8. The pixels of the secondary pulsatile signal **714** in the visualized pulsatile ultrasound image are annotated by second color values (e.g. cold color values from light cyan to dark blue).

35 **[0065]** The data analysis processor **124** classifies remaining color value sequences into the noise signal **716**. The data record processor **126** displays the visualized pulsatile ultrasound images **710** for visualization of the primary pulsatile signal **712**, the secondary pulsatile signal **714** and the noise signal **716** based on clustering and noise reductions.

40 **[0066]** FIG. 8 illustrates a diagram for reclassifying the color values in the primary pulsatile signal and secondary pulsatile signal to obtain the visualized pulsatile ultrasound images (e.g., the visualized pulsatile ultrasound images **410** in FIG 4) in accordance with various embodiments of the present invention. For each of the visualized pulsatile ultrasound images, the data record processor **126** selects a pixel of the noise signal **806** as a center pixel of a mask region, and starts at the center pixel and follows direction of arrow to search and calculate the number of pixels in the mask region of the visualized pulsatile ultrasound image.

45 **[0067]** Then, the data record processor **126** reclassifies the noise signal (i.e. center pixel) into the primary pulsatile signals **802** if the number of primary pulsatile signals is more than that of the secondary pulsatile signals in the mask region, and reclassifies the noise signal (i.e. center pixel) into the secondary pulsatile **804** if the number of secondary pulsatile signals is more than that of the primary pulsatile signals in the mask region.

50 **[0068]** The present invention provides a method and system to classify all pixels. In theory, the pixels from actual artifact interference are more likely to have a lower intensity and a random fluctuation. Therefore, the data record processor **126** will keep these pixels in the noise group, while, the remaining pixels (i.e. the pixels with a higher intensity and a periodical fluctuation) are to be reclassified to avoid misjudgment with a higher correlation coefficient threshold.

55 **[0069]** FIG. 9 illustrates intensity value change trends of the visualized pulsatile ultrasound image in accordance with various embodiments of the present invention. As shown in Equation 4, the intensity value in each frame is expressed in percent.

$$\text{Intensity value} = \frac{\text{Sum of the normalized color values of the pixels}}{\text{the total number of the pixels}} \times 100 (\%) \quad (\text{Equation 4})$$

5 [0070] The data record processor **126** normalizes the color values of each pixel of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal in the region of interest of the visualized pulsatile ultrasound image. Then, for color values of each pixel of the primary pulsatile signal in each frame (i.e., at each capture time), the data record processor **126** calculates the average of the normalized color values to obtain the intensity value in each frame. And, for color values of each pixel of the secondary pulsatile signal in each frame, the data record processor **126**
10 calculates the average of the normalized color values to obtain the intensity value in each frame. Similarly, for color values of each pixel of the noise signal on each frame, the data record processor **126** calculates the average of the normalized color values to obtain the intensity value in each frame. Therefore, the intensity value change trends **900** of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal are obtained.

15 [0071] In an embodiment, the data record processor **126** calculates a plurality of the first similarity indices (SI_{ps}) between the intensity value change trend of the primary signal and the intensity value change trend of the secondary pulsatile signal, the second similarity indices (SI_{pn}) between the intensity value change trend of the primary signal and the intensity value change trend of the noise signal, and the third similarity indices (SI_{sn}) between the intensity value change trend of the secondary signal and the intensity value change trend of the noise signal through a correlation function with a plurality of lag varieties, chooses the largest value from the first similarity indices (SI_{ps}) to be the pulsatile similarity index (PSI), chooses the largest value from the second similarity indices (SI_{pn}) and the similarity indices (SI_{sn})
20 to be the noise similarity index (NSI), and obtains a ratio coefficient (RC) by Equation 5 to assist evaluating the efficiency of visualization through outputting the ratio coefficient (RC) by the output device **130**.

$$25 \quad RC = \frac{NSI}{PSI} = \frac{\text{Max}(SI_{pn}, SI_{sn})}{\text{Max}(SI_{ps})} \quad (\text{Equation 5})$$

30 [0072] FIG. 10 is a flowchart for the method of clustering, noise reduction and visualization for Doppler ultrasound images according to various embodiments of the present invention. It should be noted that the flowchart of FIG. 10 provides merely an example of the many different types of functional arrangements that may be employed to implement the operation of the various components of the image processing system **100** (FIG. 1). As an alternative, the flowchart of FIG. 10 may be viewed as depicting an example of steps of a method implemented in the image processing system **100** according to one or more embodiments.

35 [0073] Although the flowchart of FIG. 10 shows a specific order of execution, it should be noted that the order of execution may differ from that which is depicted. For example, the order of execution of two or more blocks may be scrambled relative to the order shown. Also, two or more blocks shown in succession in FIG. 10 may be executed concurrently or with partial concurrence. It should be noted that all such variations are within the scope of the present invention.

40 [0074] Beginning with step **S1010**, a sequence of Doppler ultrasound images (I frames) **210** based on a time domain are obtained, wherein each Doppler ultrasound image comprises a color value in each pixel ($B_{j,i}$).

[0075] In step **S1020**, each color value in each pixel of the Doppler ultrasound images are arranged based on the time domain to obtain a plurality of color value sequences.

45 [0076] In step **S1030**, a reference sequence (C_{ref}) is obtained through a referencing method. The referencing method comprises an intensity percentage method, an average standard deviation ratio method, an autocorrelation method, a hierarchical correlation method or any combination thereof.

[0077] In step **S1040**, the data analysis processor **124** compares the reference sequence with each color value sequence through a clustering method to obtain a plurality of correlation coefficient values. The clustering method comprises a correlation grouping method, a grouping with lag-correlation method, a two-centers correlation clustering method or any combination thereof.
50

[0078] In step **S1050**, the data analysis processor **124** further performs a clustering and noise reduction method to classify the color value sequences into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal based on the correlation coefficient values.

55 [0079] Finally, in step **S1060**, the data record processor **126** annotates the color value in each pixel which belong to the primary pulsatile signal, the secondary pulsatile signal, and the noise signal with different color values to obtain a plurality of visualized pulsatile ultrasound images.

[0080] In addition to the aforesaid steps, the method of clustering, noise reduction and visualization for Doppler ultrasound images of the present invention can also execute all the operations and have all the corresponding functions set

forth in all the aforesaid embodiments. How this embodiment executes these operations and has these functions will be readily appreciated by those of ordinary skill in the art based on the explanation of all the aforesaid embodiments, and thus will not be further described herein.

5 [0081] According to the above descriptions, the system and the method of clustering, noise reduction and visualization for Doppler ultrasound images of the present invention provide the Doppler ultrasound images with different colors to visually segment the primary pulsatile signal, the secondary pulsatile signal, and the noise signal in consideration that signal intensities of Doppler ultrasound images would be affected by pulsatile flow intensities of the artery and the vein. Therefore, the method and system in this invention can apply different appropriate analysis methods on different specific organs, respectively, to visualize information of the artery and the vein and reduce the noise caused by the motion artifacts to clearly present the artery and the vein, thereby improving diagnostic accuracy and efficiency.

10 [0082] It shall be appreciated that the method and system do not limit to blood signal of the specific organ and utilizes one of the clustering methods, for example, the correlation grouping method, the two-center correlation clustering method, and hierarchical correlation clustering method to obtain the Doppler ultrasound images for different organs. It should be emphasized that the above-described embodiments of the present invention are merely possible examples of implementations set forth for a clear understanding of the principles of the disclosure. Many variations and modifications may be made to the above-described embodiment(s) without departing substantially from the spirit and principles of the disclosure. All such modifications and variations are intended to be included herein within the scope of this disclosure and protected by the following claims.

20

Claims

1. A system of clustering, noise reduction and visualization for Doppler ultrasound image, comprising:

25

a capture device, being configured to obtain a plurality of Doppler ultrasound images based on a time domain, wherein each of the Doppler ultrasound image comprises a color value in each pixel;

a processing device, being connected to the capture device, and comprising:

30

a data conversion processor, being configured to arrange the color value in each pixel of the Doppler ultrasound images based on the time domain to obtain a plurality of color value sequences;

a data analysis processor, being configured to calculate the color value sequences through a referencing method to obtain a reference sequence, compare the reference sequence with each of the color value sequences through a clustering method to obtain a plurality of correlation coefficient values, and classify the color value sequences into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal based on the correlation coefficient values through a clustering and noise reduction method; and

35

a data record processor, being configured to annotate the color values of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal to obtain a plurality of visualized pulsatile ultrasound images;

40

an output device, being connected to the processing device and configured to display the visualized pulsatile ultrasound images.

2. The system of claim 1, wherein the output device provides selection of a region of interest in the visualized pulsatile ultrasound images, the data record processor obtains a plurality of intensity value change trends of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal in the region of interest of the visualized pulsatile ultrasound images by following steps:

45

normalizing the color values of each pixel of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal in the region of interest of the visualized pulsatile ultrasound image;

calculating an average of the normalized color values of the primary pulsatile signal at each capture time to obtain a plurality of intensity value of the primary signal;

50

calculating an average of the normalized color values of the secondary pulsatile signal at each capture time to obtain a plurality of intensity values of the secondary pulsatile signal; and

calculating an average of the normalized color values of the noise signal at each capture time to obtain a plurality of intensity values of the noise signal;

55

wherein the output device further displays a plurality of intensity value change trends in a chart according to the intensity values of the primary signal, the secondary pulsatile signal, and the noise signal.

3. The system of claim 2, wherein the output device calculates a plurality of first similarity indices between the intensity

value change trend of the primary pulsatile signal and the intensity value change trend of the secondary pulsatile signal, a plurality of second similarity indices between the intensity value change trend of the primary signal and the intensity value change trend of the noise signal, and a plurality of third similarity indices similarity indices between the intensity value change trend of the secondary signal and the intensity value change trend of the noise signal through a correlation function with a plurality of lag varieties, and the output device chooses a largest value from the first similarity indices to be a pulsatile similarity index, chooses the largest value from the second and third similarity indices to be the noise similarity index, and obtains a ratio coefficient by dividing the noise similarity index by the pulsatile similarity index.

4. The system of any one of claims 1-3, wherein the referencing method comprises an intensity percentage method, an average standard deviation ratio method, an autocorrelation method, a hierarchical correlation method or any combination thereof.

5. The system of claim 4, wherein the data analysis processor performs the intensity percentage method to obtain the reference sequence, and the intensity percentage method comprises the following steps of:

arranging the color value sequences according to the largest color value of each of the color value sequences to obtain a plurality of percentile ranks;
choosing the color value sequences which the percentile rank is within a predetermined rank range to obtain a reference group; and
averaging the color value sequences in the reference group to obtain the reference sequence.

6. The system of claim 4, wherein the data analysis processor performs the average standard deviation ratio method to obtain the reference sequence, and the average standard deviation ratio method comprises the following steps of:

calculating the color value in each color value sequences to obtain a plurality of standard deviation values, and then dividing by an average value of the standard deviation values to obtain a plurality of average standard deviation ratio values;
choosing the color value sequences which the averaging standard deviation ratio value is within a predetermined ratio range to obtain a reference group; and
averaging the color value sequences in the reference group to obtain the reference sequence.

7. The system of claim 4, wherein the data analysis processor performs the autocorrelation method to obtain the reference sequence, and the autocorrelation method comprises the following steps of:

calculating each color value sequence through an autocorrelation function with a plurality of lag varieties to obtain a plurality of autocorrelation coefficient values; and
choosing a color value sequence which has the smallest autocorrelation coefficient value to obtain the reference sequence.

8. The system of claim 4, wherein the data analysis processor performs the hierarchical correlation method to obtain the reference sequence, and the hierarchical correlation method comprises the following steps of:

(a) gathering the color value sequences into an i^{th} reference sequence set, wherein an initial value of i is 1;
(b) obtaining a plurality of correlation coefficient values of the i^{th} reference sequence set by calculating each pair of the color value sequences in the i^{th} reference sequence set through a correlation function;
(c) selecting the pair of the color value sequences in the i^{th} reference sequence set, which have a largest correlation coefficient value;
(d) averaging the selected pair of the color value sequences in the i^{th} reference sequence set to generate a new color value sequence;
(e) gathering the new color value sequence and the color value sequences in the i^{th} reference sequence set except for the selected pair of the color value sequences into a $(i+1)^{\text{th}}$ reference sequence set;
(f) obtaining a plurality of correlation coefficient values of the $(i+1)^{\text{th}}$ reference sequence set by calculating each pair of the color value sequences in the $(i+1)^{\text{th}}$ reference sequence set through the correlation function;
(g) determining whether all of the correlation coefficient values of the $(i+1)^{\text{th}}$ reference sequence set are less than a predetermined correlation threshold; and
(h) when one of the correlation coefficient values of the $(i+1)^{\text{th}}$ reference sequence set is not less than the predetermined correlation threshold, setting $i=i+1$ and repeating steps (c), (d), (e), (f) and (g), and when the all

of the correlation coefficient values of the $(i+1)^{\text{th}}$ reference sequence set are less than the predetermined correlation threshold, outputting the color value sequence in the $(i+1)^{\text{th}}$ reference sequence set which is generated by averaging a most number of the color value sequences in the first reference sequence set as a reference sequence.

5

9. The system of any one of claims 1-8, wherein the clustering method comprises a correlation grouping method, a grouping with lag-correlation method, a two-centers correlation clustering method or any combination thereof.

10

10. The system of claim 9, wherein the data analysis processor performs the correlation grouping method to obtain the correlation coefficient values, and the correlation grouping method comprises the following step of:

calculating each of the color value sequences with the reference sequence through a correlation function to obtain the correlation coefficient values of the color value sequences.

15

11. The system of claim 9, wherein the data analysis processor performs the two-centers correlation clustering method to obtain the correlation coefficient values, and the two-centers correlation clustering method comprises the following steps of:

20

(a) gathering the color value sequences into an operation set;

(b) calculating each of the color value sequences in the operation set with the reference sequence through a correlation function to obtain a plurality of temporary correlation coefficient values of the color value sequences;

(c) removing the color value sequence with the smallest temporary correlation coefficient value from the operation set and assigning the smallest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence with the smallest temporary correlation coefficient value;

25

(d) removing the color value sequence with the largest temporary correlation coefficient value and assigning the largest temporary correlation coefficient value to be the correlation coefficient value of the color value sequence with the largest temporary correlation coefficient value;

30

(e) updating the reference sequence by averaging the color value sequence with the largest temporary correlation coefficient value and the reference sequence; and

(f) repeating steps (b), (c), (d), and (e) until all of the color value sequences are assigned with the correlation coefficient values.

35

12. The system of claim 9, wherein the data analysis processor performs the grouping with lag-correlation method to obtain the correlation coefficient values, and the grouping with lag-correlation method comprises the following steps of:

calculating each color value sequences with the reference sequence through a correlation function with a plurality of lag varieties to obtain a plurality of correlation coefficient values;

40

choosing the largest correlation coefficient value and the corresponding lag variety to obtain the correlation coefficient value and the lag variety of each color value sequence.

45

13. The system of any one of claims 1-12, wherein the data analysis processor further compares the reference sequence with each of the color value sequences through the clustering method to obtain the correlation coefficient values and a plurality of lag varieties corresponding to the correlation coefficient values of the color value sequences and performs the clustering and noise reduction method comprising the following steps of:

classifying the color value sequences, the correlation coefficient values of which are within a main correlation coefficient threshold and the lag varieties of which are within a main lag-coefficient threshold, into the primary pulsatile signal;

50

classifying the color value sequences, the correlation coefficient values of which are within a secondary correlation coefficient threshold and the lag varieties of which are within a secondary lag-coefficient threshold, into the secondary pulsatile signal; and

55

classifying the color value sequences, the correlation coefficient values of which are not within the main correlation coefficient threshold and the secondary correlation coefficient threshold and the lag variety of which are not within the main lag-coefficient threshold and the secondary lag-coefficient threshold, into the noise signal.

14. The system of any one of claims 1-13, wherein the step of obtaining the visualized pulsatile ultrasound images executed by the data record processor comprises the following steps of:

for each of the visualized pulsatile ultrasound images:

- selecting a pixel of the noise signal as a center pixel of a mask region;
- calculating a number of pixels in the mask region;
- 5 reclassifying the noise signal into the primary pulsatile signal if the number of primary pulsatile signals is more than that of the secondary pulsatile signals in the mask region; and
- reclassifying the noise signal into the secondary pulsatile signal if the number of secondary pulsatile signals is more than that of the primary pulsatile signals in the mask region.

10 **15.** The system of any one of claims 1-14, wherein the step of obtaining the visualized pulsatile ultrasound images executed by the data record processor, further comprises the following steps of:

- annotating the pixels which belong to the primary pulsatile signal with first color values;
- annotating the pixels which belong to the secondary pulsatile signal with second color values;
- 15 annotating the pixels which belong to the noise signal with a third color value; and
- obtaining the visualized pulsatile ultrasound images.

16. A method of clustering, noise reduction and visualization for Doppler ultrasound image, comprising:

- 20 obtaining a plurality of Doppler ultrasound images based on time domain, wherein each of Doppler ultrasound images comprises a color value in each pixel;
- arranging each color value in each pixel of Doppler ultrasound images based on the time domain to obtain a plurality of color value sequences;
- calculating the color value sequences through a referencing method to obtain a reference sequence;
- 25 comparing the reference sequence with each color value sequences through a clustering method to obtain a plurality of correlation coefficient values;
- classifying the color value sequences into a primary pulsatile signal, a secondary pulsatile signal, and a noise signal based on the correlation coefficient values through a clustering and noise reduction method; and
- 30 annotating the color values of the primary pulsatile signal, the secondary pulsatile signal, and the noise signal with first color values, second color values, and a third color value, respectively, to obtain a plurality of visualized pulsatile ultrasound images.

35

40

45

50

55

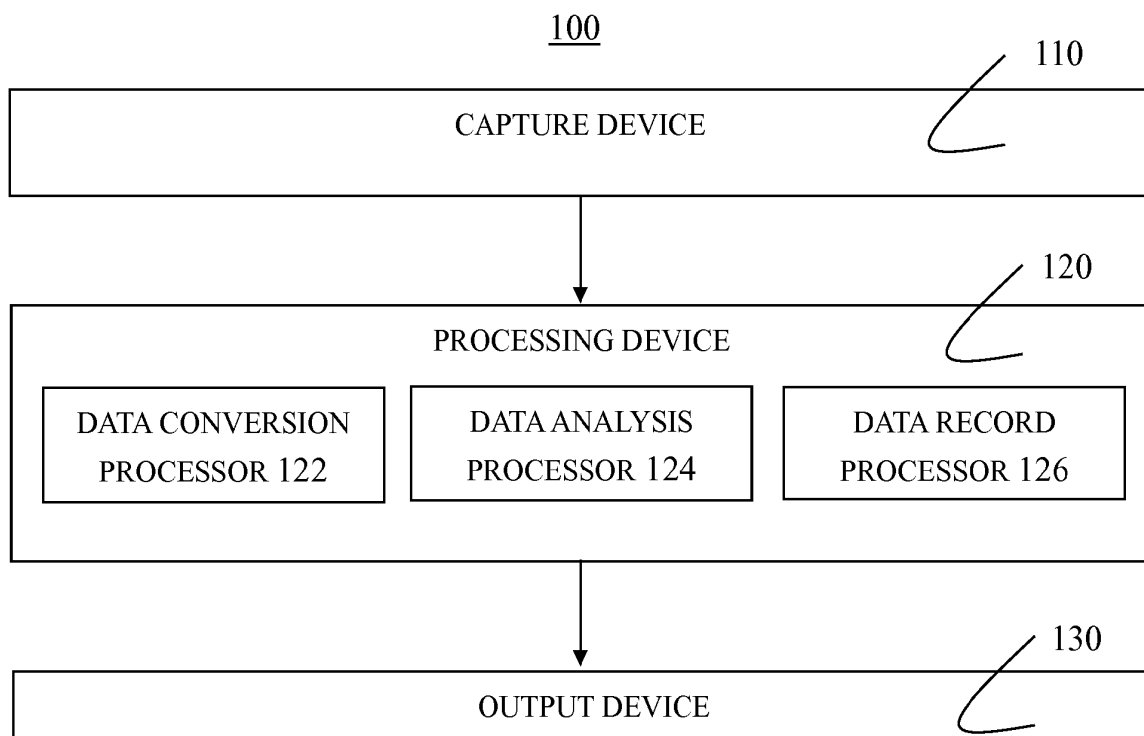


FIG. 1

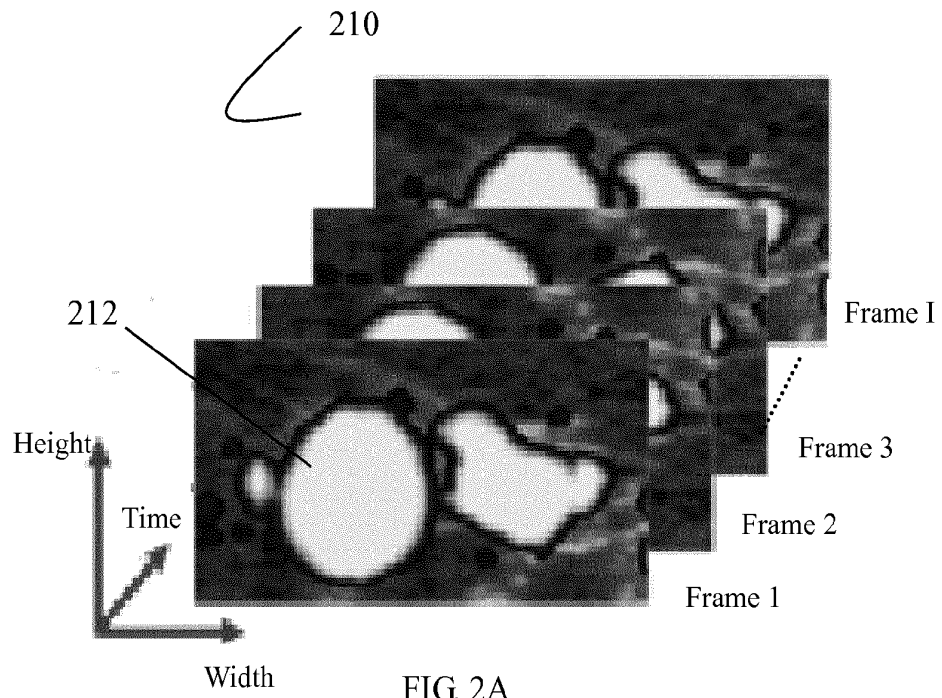


FIG. 2A

	Frame 1	Frame 2	Frame 3	Frame 4	Frame i	Frame I	
Pixel 1	$B_{1,1}$	$B_{1,2}$	$B_{1,3}$	$B_{1,4}$	$B_{1,i}$	$B_{1,I}$	C_1
Pixel 2	$B_{2,1}$	$B_{2,2}$	$B_{2,3}$	$B_{2,4}$	$B_{2,i}$	$B_{2,I}$	C_2
.....
.....
Pixel j	$B_{j,1}$	$B_{j,2}$	$B_{j,3}$	$B_{j,4}$	$B_{j,i}$	$B_{j,I}$	C_j

FIG. 2B

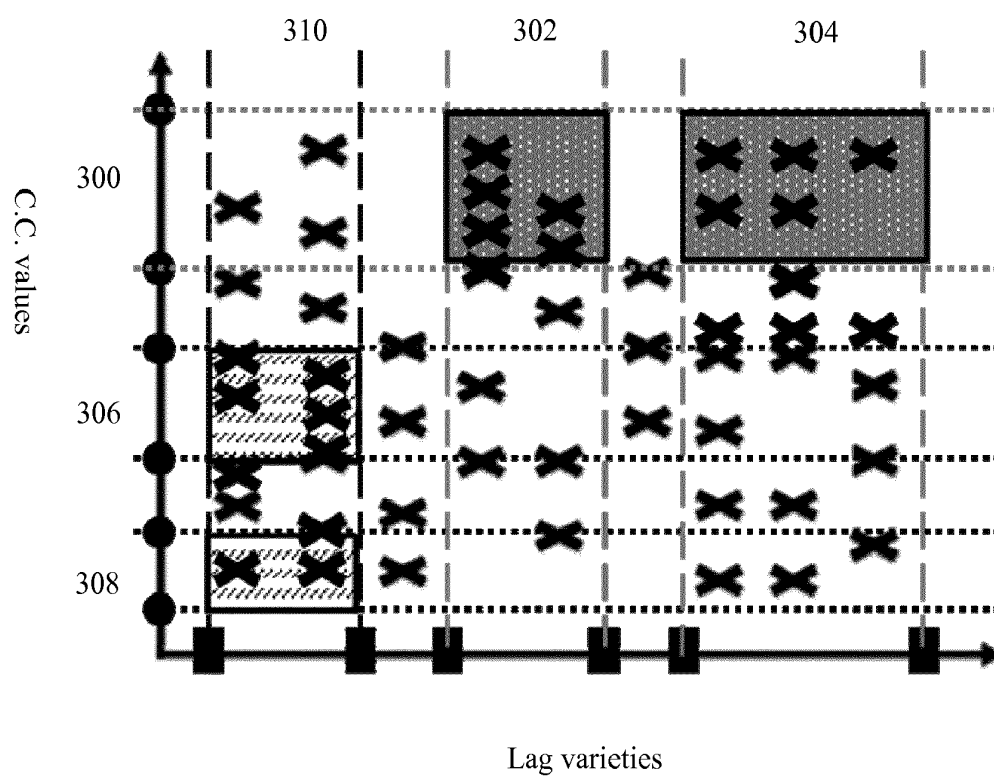


FIG. 3

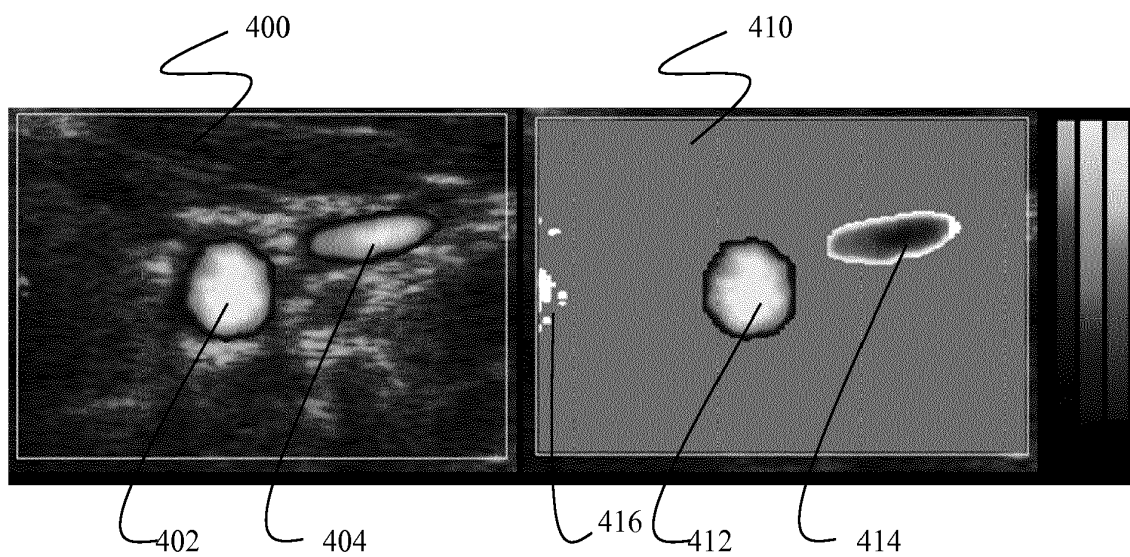


FIG. 4

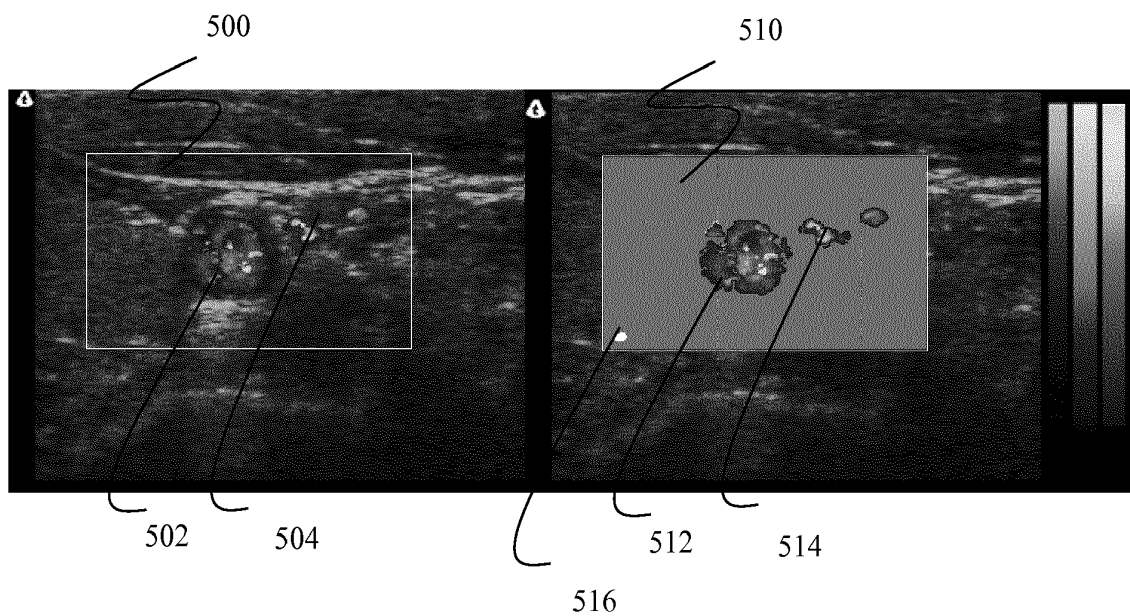


FIG. 5

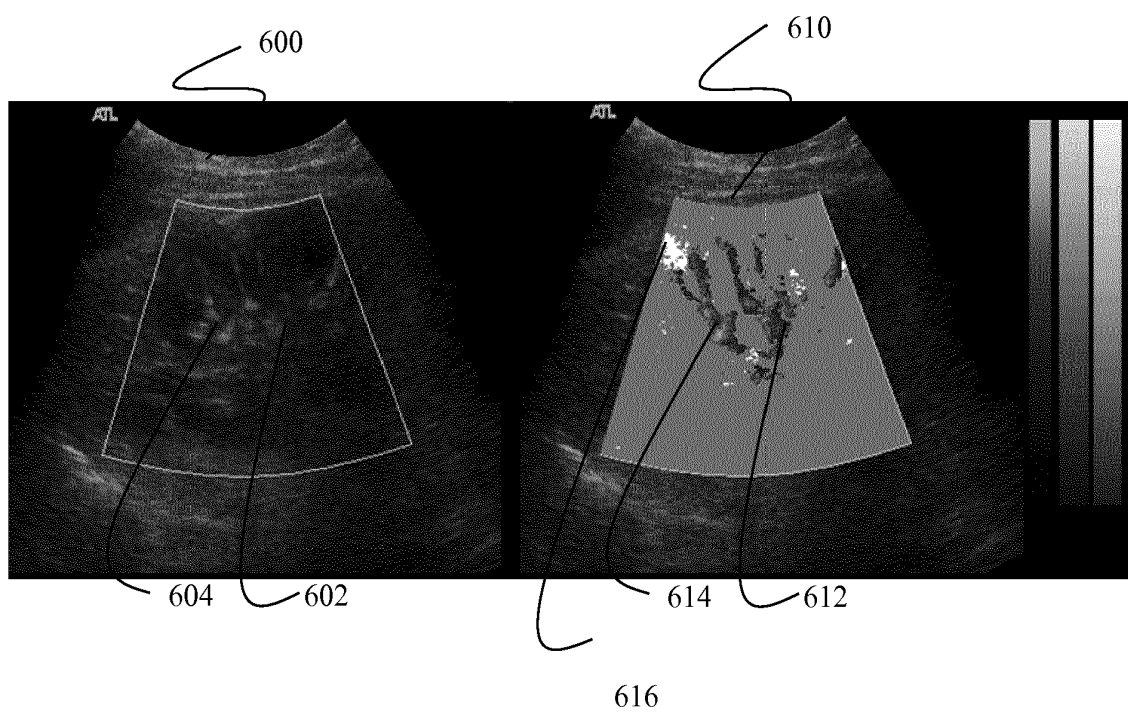


FIG. 6

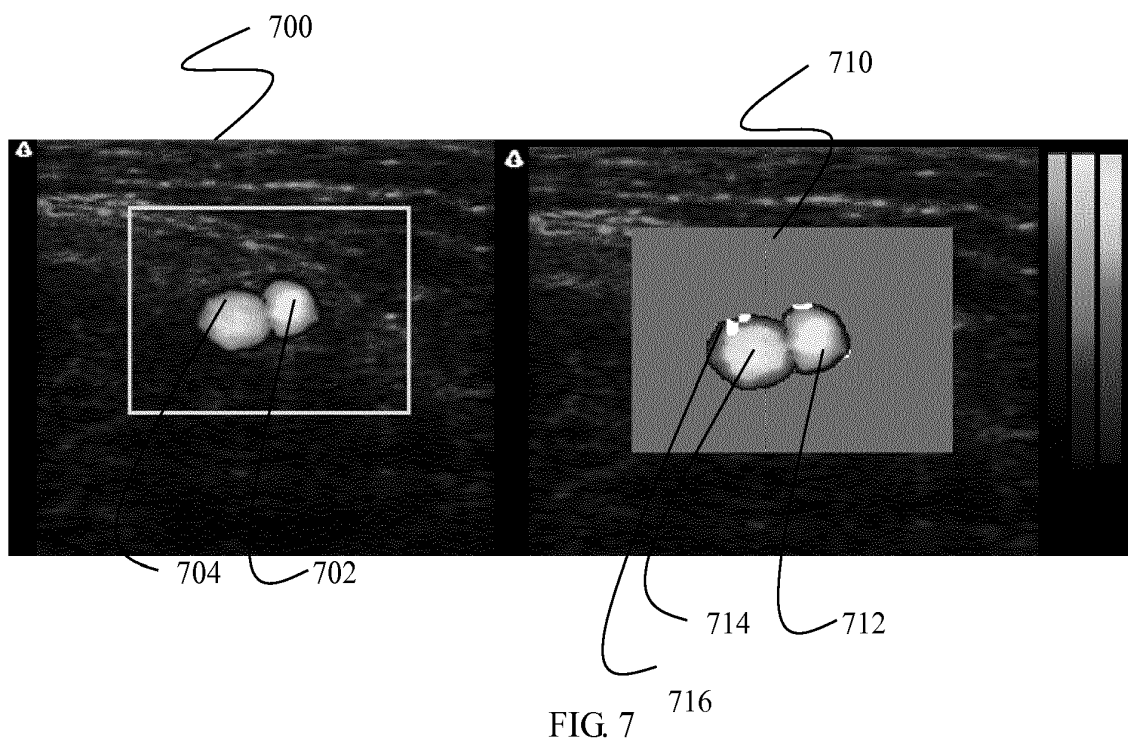


FIG. 7

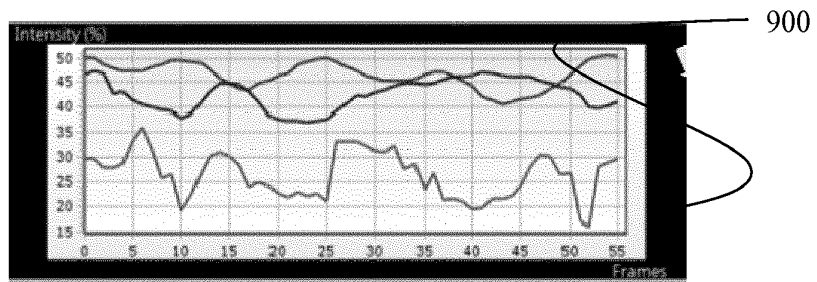


FIG. 9

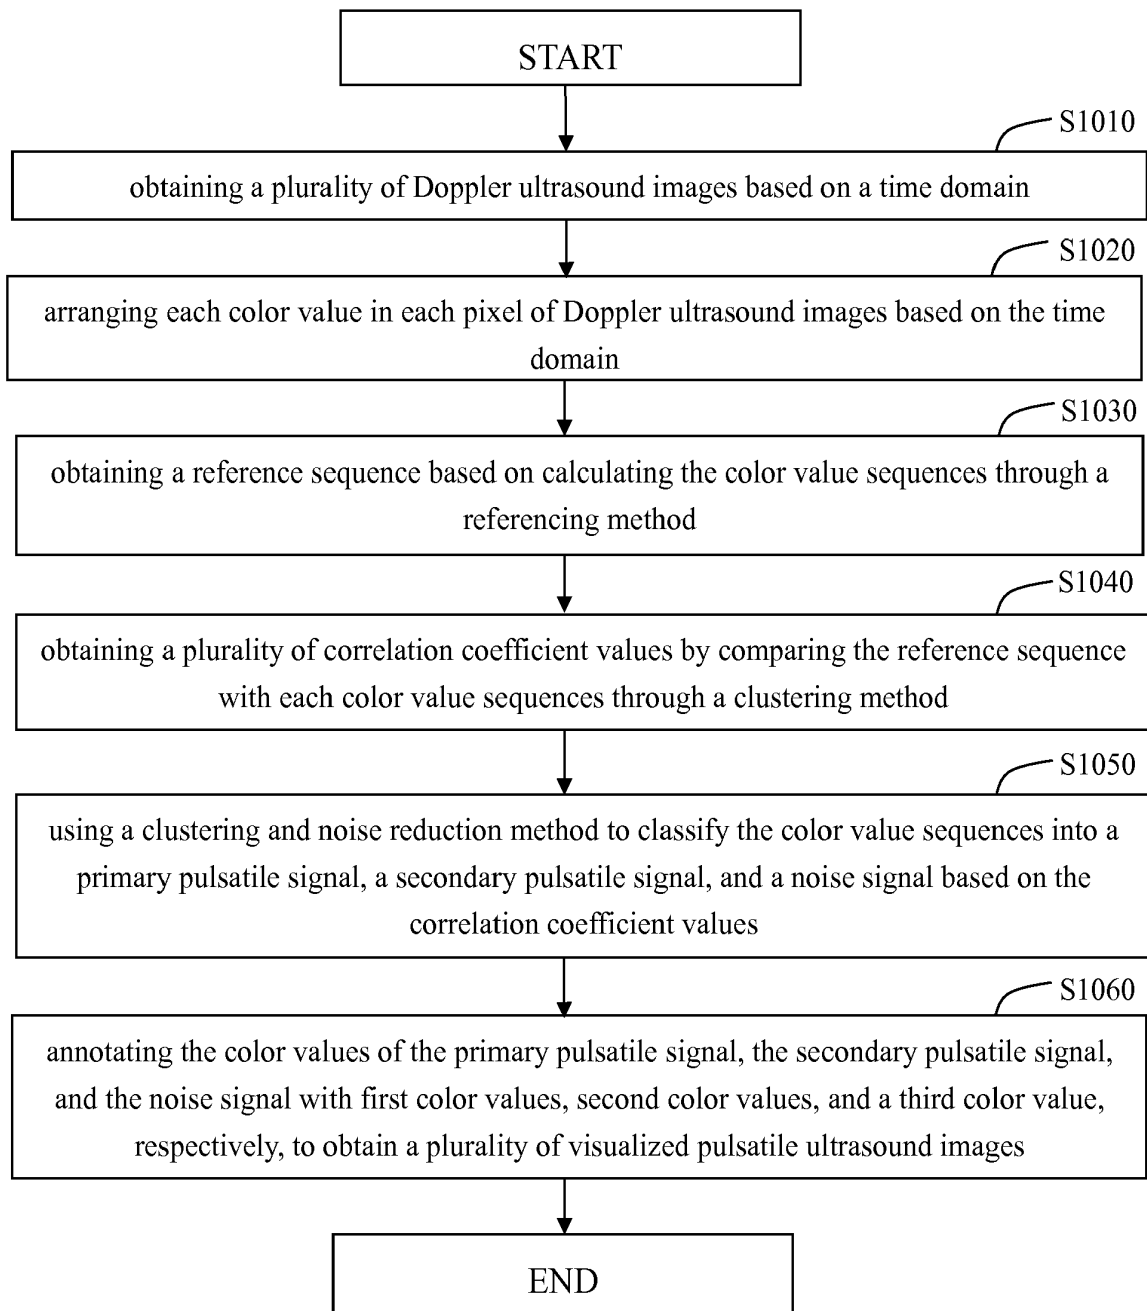


FIG. 10

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- TW 1275383 [0003] [0005]
- US 8047993 B2 [0003] [0004] [0005]
- US 8777860 B2 [0005]

专利名称(译)	多普勒超声图像的聚类，降噪和可视化方法		
公开(公告)号	EP3184051A2	公开(公告)日	2017-06-28
申请号	EP2016205350	申请日	2016-12-20
[标]申请(专利权)人(译)	美国医科华股份有限公司		
申请(专利权)人(译)	AMCAD BIOMED CORPORATION		
当前申请(专利权)人(译)	AMCAD BIOMED CORPORATION		
[标]发明人	CHEN ARGON CHEN JIA JIUN SHEN YU HAN LIU CHENG HSIEN		
发明人	CHEN, ARGON CHEN, JIA-JIUN SHEN, YU-HAN LIU, CHENG-HSIEN		
IPC分类号	A61B8/08 A61B8/06 A61B8/00		
CPC分类号	A61B8/06 A61B8/08 A61B8/0891 A61B8/463 A61B8/468 A61B8/469 A61B8/488 A61B8/5207 A61B8/5223 G01S7/52036 G01S7/52071 G01S7/52074 G01S7/52077 G01S15/8988 G16H50/30 G01S7/52053 G06K9/42 G06K9/4642 G06K9/4652 G06K9/4661 G06K9/6215 G06K9/6218 G06K9/623 G06K9/628		
优先权	104143257 2015-12-23 TW		
其他公开文献	EP3184051A3 EP3184051B1		
外部链接	Espacenet		

摘要(译)

本发明提供了一种用于多普勒超声图像的分析系统，包括：捕获装置，处理装置和输出装置。捕获装置获得多个多普勒超声图像。处理装置基于时域在图像的每个像素中排列颜色值，并通过参照方法获得参考序列，进一步执行聚类方法以获得多个相关系数值，然后使用聚类和降噪分类为主脉动信号，二次脉动信号和噪声信号的方法分别最终分别标注主脉动信号，次脉冲信号和具有不同颜色值的噪声信号。输出装置显示多个可视化的脉冲超声图像，用于可视化。

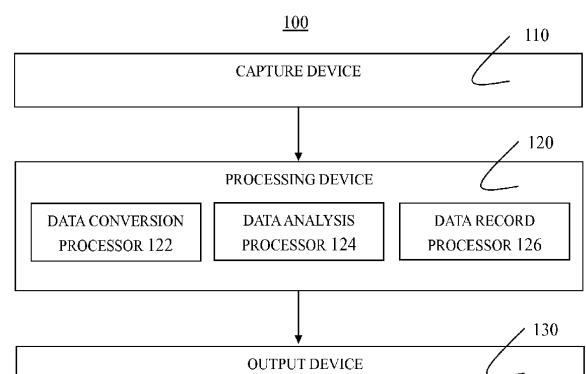


FIG. 1