

(19)



(11)

**EP 1 589 878 B1**

(12)

## EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention  
of the grant of the patent:  
**28.10.2009 Bulletin 2009/44**

(21) Application number: **04706450.6**

(22) Date of filing: **29.01.2004**

(51) Int Cl.:  
**A61B 8/00 (2006.01)**

(86) International application number:  
**PCT/US2004/002423**

(87) International publication number:  
**WO 2004/069028 (19.08.2004 Gazette 2004/34)**

(54) **SYSTEM FOR USE WITH A MODULAR APPARATUS FOR DIAGNOSTIC ULTRASOUND**

SYSTEM ZUR VERWENDUNG MIT EINEM MODULAREN GERÄT FÜR DIE  
ULTRASCHALLDIAGNOSE

SYSTEME UTILISE AVEC UN APPAREIL MODULAIRE ULTRASONORE DE DIAGNOSTIC

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR  
HU IE IT LI LU MC NL PT RO SE SI SK TR**

(30) Priority: **31.01.2003 US 356401**

(43) Date of publication of application:  
**02.11.2005 Bulletin 2005/44**

(60) Divisional application:  
**09075402.9**

(73) Proprietor: **Sonosite, Inc.**  
**Bothell, WA 98021-3904 (US)**

(72) Inventors:  
• **HOLMBERG, Randy, T.**  
**Bothell, WA 98021 (US)**

• **LITTLE, Blake, W.**  
**Bothell, WA 98021 (US)**  
• **BUNCE, Steven**  
**Sedro Woolley, WA 98284 (US)**

(74) Representative: **Jackson, Richard Eric et al**  
**Carpmaels & Ransford**  
**43-45 Bloomsbury Square**  
**London WC1A 2RA (GB)**

(56) References cited:  
**US-A1- 2002 103 435 US-A1- 2002 143 256**  
**US-A1- 2003 013 959 US-A1- 2003 013 965**  
**US-A1- 2003 013 966**

**EP 1 589 878 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description****BACKGROUND OF THE INVENTION**

5 **[0001]** The present invention relates to diagnostic ultrasound equipment. More particularly the present invention describes a modular system having a mobile core module for data processing, beamforming and system operations, and additional modules capable of connecting to the core module to provide additional features and connectivity to peripheral devices needed in diagnostic ultrasound procedures.

10 **[0002]** Modern ultrasound diagnostic systems are large, complex instruments. Today's premium ultrasound systems, while mounted in carts for portability, continue to weigh several hundred pounds. In the past, ultrasound systems such as the ADR 4000 ultrasound system, produced by Advanced Technology Laboratories, Inc., were smaller desktop units about the size of a personal computer. However such instruments lacked many of the advanced features of today's premium ultrasound systems such as color Doppler imaging and three dimensional display capabilities.

15 **[0003]** The judicious use of power and signal processing on ASIC devices has enabled smaller system to push past the feature limitations in smaller older systems that employed mechanical transducers or analog chip sets. Digital beam forming and advanced processing is now available on smaller systems such as the SonoHeart Elite, by SonoSite, Inc., and common assignee of the present invention. The success of the handheld device has spawned competitive products that are beginning to offer more advanced features. However, the use of a small handheld requires a trade off in the form of display size and battery life. Cart based units provide users with the luxury of full sized CRT monitors, as well as a host of peripheral devices at the ready. Hand held devices offer portability, but are restricted to the features built in to their chassis. Some hand held devices are offered in combination with an interface to added peripherals through a cart add on, however this increases the cost of the device and requires a user to buy specialized equipment from the manufacturer of the hand held.

25 **[0004]** Thus, there remains a need for a diagnostic ultrasound instrument which provides the advantages of light weight mobility, combined with advanced functionality traditionally restricted to larger cart based system.

**[0005]** There is also a need for a more economical diagnostic ultrasound system that will allow small users and institutions to purchase ultrasound units that have the capacity the user or institution requires without having to pay the expense of additional features the user or institution will not use.

30 **[0006]** There further remains a need for a device that is portable, and remains highly resistant to shock damage from being dropped or jostled during transport from place to place.

**BRIEF SUMMARY OF THE INVENTION**

35 **[0007]** The present invention relates to a mini-dock for connecting peripheral devices to a modular diagnostic ultrasound apparatus as claimed in claim 1.

**[0008]** Another aspect of the present invention is a docking station for connecting a plurality of peripheral devices to a modular diagnostic ultrasound apparatus as claimed in claim 8.

**[0009]** The modular diagnostic ultrasound apparatus also includes a system for diagnostic ultrasound examinations as claimed in claim 12.

**BRIEF DESCRIPTION OF THE DRAWINGS**

**[0010]** Figure 1 illustrates in block diagram form the architecture of a hand held ultrasound system.

**[0011]** Figure 1B shows a core unit module of the present invention.

45 **[0012]** Figure 1C shows a clamshell embodiment of the core unit.

**[0013]** Figure 2 shows a mini-dock style connector module.

**[0014]** Figure 3 shows a docking station style system module.

**[0015]** Figure 4 shows a mobile workstation style system module.

**[0016]** Figure 5 shows a multi-tap transducer module.

50 **[0017]** Figure 6 shows a multi station system incorporating all the modules.

**DETAILED DESCRIPTION OF THE INVENTION**

55 **[0018]** The focus of the present invention lies in a modular ultrasound system having a core module having the essential ultrasound processor functions, and a series of additional modules which, when combined with the core module, provide expanded capability and utility to the core module. The following description gives both the principle embodiment and alternative embodiments of the invention. Use of certain terms in the disclosure warrant clarification before an in depth discussion can occur.

**[0019]** The invention presented here is for an ultrasound device to be principally used for diagnostic purposes. However the term diagnostic should not be misconstrued to be read as being for non-therapeutic purposes. We use the term diagnostic to mean providing high quality imaging, as is characteristic of diagnostic imaging devices in the medical ultrasound industry. Because the present invention can provide images for use in biopsy procedures, Peripherally Inserted Central Catheter (PICC) lines and other procedures, the use of the ultrasound device herein is not purely for diagnosis of diseases. However, we specifically disclaim any use of the present invention for a purely therapeutic purpose, such as ablative ultrasound, thermal heating (as in the treatment of hypothermia) or mechanical tissue disruption, such as the generation of cavitation effects. The diagnostic ultrasound device of the present invention runs with the same power and frequency of devices used for diagnostic imaging, or therapies using diagnostic imaging - the device itself is not used as the source of therapy.

**[0020]** A focal point of the invention is the communication ability of the core module to the various other modules that comprise the system of the invention. Thus the core module has a single I/O port in its preferred embodiment sometimes referred to as the plug. The plug is a multi-pin electronic communication adaptor for matingly engaging a receptacle. The receptacle is a device with a corresponding pin set to match up the plug, and read data from the core module and sort it out to a variety of other devices that are in electronic communication with the receptacle. In alternative embodiments, there may be multiple I/O ports and a plug. The plug retains its function in all embodiments of the present invention, though electronic communication with additional module and components may be achieved through dedicated I/O ports. Any port in addition to the plug is a dedicate I/O port designed to receive input, or transmit output to a particular device. Likewise, in alternative embodiments of modules with a receptacle, there are no other I/O ports involved except the receptacle designed to mate with and communicate with the plug.

**[0021]** The core unit has a system electronics that should be understood to be the central processing core of the ultrasound device and the ultrasound engine. It can be thought of as an ultrasound motherboard. The system electronics of the core module, both in the preferred embodiment, and alternative embodiments, has the capacity to recognize and drive a group of transducer arrays such that a single core module can be connected with a plurality of transducers and perform all types of ultrasound procedures the transducers are designed for.

**[0022]** Turning now to Figure 1A, a core module 10 for an ultrasound system is illustrated having system electronics 14 allowing the core module 10 to operate as a data processing and signal processing unit for a modular ultrasound system 60. The core module 10 comprises a housing 11 having the system electronics 14 mated to an I/O connector (plug) 12. A gap space 13 exists between the system electronics 14 and housing 11 and can be filled with an impact resistant padding material, or the housing can be made to abut the system electronics to eliminate or minimize the gap space. In its simplest form the core module 10 comprises just the system electronics 14 without a power supply, transducer, video interface or user interface. The core module 10 is highly mobile and very lightweight. The core module can be easily moved from place to place and mated to a modular ultrasound system 60 having the additional components desired for performing any variety of ultrasound scans.

**[0023]** The system electronics 14 (Fig. 1B) has one or more concatenated functions (filters) and includes a transmit/receive ASIC (beamformer) which are capable of driving one or more transducer arrays (not shown). The concatenated functions are ultrasound functions for processing signals in various ways. Two examples are a QBP filter and a digital Doppler processing function. The concatenated functions are not necessarily serially linked in that they require each other to operate. Though this is true in some cases where the processing of one type of signal is needed for the handling of another (e.g. QBP can be used by both a B mode and a PW Doppler mode), it is not necessary that a circuit for color power angio is linked together with continuous wave Doppler, in this instance, the filters can operate independently. The transmit/receive ASIC also controls the active transmit and receive apertures of a transducer array and the gain of the received echo signals. Echo data received by the transmit/receive ASIC are provided to the adjacent front end ASIC, which digitizes and beamforms the echoes from the individual transducer elements into coherent scan line signals. The front end ASIC also controls the transmit waveform timing, aperture and focusing of the ultrasound beam through control signals provided for by the transmit/receive ASIC. A memory device is connected to the front end ASIC which stores data used by the beamformer.

**[0024]** The beamformed scan line signals are coupled from the front end ASIC to the adjacent digital signal processing ASIC. The digital signal processing ASIC filters the scan line signals and can provide additional features such as synthetic aperture formation, frequency compounding, Doppler processing such as power Doppler (color power angio) processing, speckle reduction, and pulse wave Doppler. Additional features such as continuous wave Doppler, can be incorporated into the system electronics if desired.

**[0025]** The ultrasound information is then coupled to the adjacent back end ASIC for scan conversion and the production of video outputs signals through the I/O port to the monitoring device attached to the core module. A memory device is coupled to the back end ASIC to provide storage used in three dimensional, 2D and power Doppler (3d CPA) imaging. The back end ASIC also adds alphanumeric information to the display such as the time, date, and patient identification. A graphics processor overlays the ultrasound image with information such as depth and focus markers and cursors. The graphics processor need not be incorporated into the core electronics system package, instead relying on a dedicated

graphics processor card integrated into a docking module 40 of the modular system 60, and receiving the necessary component information from the core module 10. The video data can be transmitted through the I/O port 12 in one of several formats including NTSC, PAL, and RGB. Frames of ultrasound images are exported to an external video memory again through the I/O port 12 coupled to the back end ASIC. The stored data can be retrieved through the system electronics using a playback mode for either live Cineloop® real time sequence or as individual stills.

**[0026]** The back end ASIC also includes the central processor for the core module. The central processor is preferably a RISC (reduced instruction set controller) processor. The RISC processor is coupled to the front end and digital signal processing ASICs to control and synchronize the processing and control functions for both the core module, and the modular system the core module may be linked into at the time. A program memory is coupled to the back end ASIC to store program data which is used by the RISC processor to operate and control the core module, and the various elements of the modular system (transducer, multi-tap connector, video data overlay features, etc.). The RISC processor is also coupled to any user interface controls connected to the modular system, the RISC processor accepts user inputs to direct and control the operations of the core module, and the modular system as illustrated, all the inputs and outputs of the system electronics are designed to go through a single I/O port 12.

**[0027]** The main system, application and control software are stored in a persistent memory device integrated directly into the system electronics. The system software, control software and application software are loaded into the system electronics processors during power up. The core module may use any number of persistent memory devices integrated into the system electronics. Each ASIC includes a separate memory core having the necessary loadable data on it that is loaded into each ASIC during the power up cycle. The main system and application software includes the essential driver and communications information for the core module to communicate with, and control, a select number of peripherals. In particular these peripherals include scan heads, preferred user I/O devices (such as keyboards, pointer devices and touch screen interface recognition), printers, VCRs, monitors and data storage devices. The entire volume of system and application software should be efficiently coded to preserve space and avoid the need for a large capacity storage device like a hard drive. Since the core module is principally desired for diagnostic ultrasound, large capacity storage devices such as hard drives should not be necessary. The omission of devices like a hard drive, power supply and other elements commonly incorporated into computers or typical hand held products allows the core module to be manufactured with the smallest foot print the technology will allow. The housing for the core module only needs to securely enclose the system electronics and the I/O port. To improve impact resistance, the system electronics can be encased in resin or epoxy.

**[0028]** Power for the core module is provided by the modular system through the I/O port, or in the alternative, through a separate I/O used as a dedicated power terminal. Although the core module preferably does not have a built in power supply, it still requires a power monitoring/regulating circuit to provide proper power to the individual components during use. An external power supply can feed energy to the core module either through the I/O port, or through a dedicated power adaptor, however the power supply "brick" must be separate from the core module.

**[0029]** In an alternative embodiment, the core module can incorporate additional hardware elements allowing the core module to operate as a stand alone device. In a first alternative embodiment, the core module 10 includes the features of previously described hand-held ultrasound systems in the form of system electronics, video out with the addition of an on board video display device 26, and a plurality of user inputs 28 in the form of a pointer, alphanumeric keypad, touch screen, programmable hot keys, and/or display control dials. This embodiment may also include speakers for audio output (not shown) and/or a direct transducer connection 24. The core module 10 now requires an internal power supply 25 in the form of a battery in order to operate as a stand alone device. This embodiment also requires either a built in or removable data storage device.

**[0030]** For ergonomic considerations, the stand alone version of the core module may be in the form of a tablet style PC or a laptop computer, as both of these designs are commonly used today and provide users with a familiar design and interface mode. In these embodiments the core module must have sufficient video capabilities to drive the video device coupled to the core module, such as an LCD device. The display output can be as low as six bit to provide sufficient color capacity to drive the core module video display, or an external display that the core module may be attached to. The display output is preferably 8 or 16 bit, but can include 24 bit RGB output. Color supporting bandwidth is necessary for some ultrasound scans that involve color display (PW, color angio) or higher definition gray scale. Where the core module 10 may be connected to a docking station 40 having an independent video processor, the data necessary for the video display need only be transmitted to the independent video processor. It is both possible and desirable in certain instances to be able to utilize both displays simultaneously, such as in the instances where more than one display is desired, or where it is necessary to check one display against the other as in a system diagnostic test.

**[0031]** In another variation on this embodiment, a form factor having the tablet or laptop configuration may include a built in handle 23. The handle 23 may be used strictly for carrying the core module 20, or it may serve as a sound chamber for speakers built into the handle. The handle may also serve as an I/O port for a dedicated connection, such as an external mouse, power adaptor or other user interface tool. In operation a user may use the handle as a wrist rest to reduce the incidence of repetitive motion syndrome while inputting information into the core module 10 through the

user interface 28.

**[0032]** No matter what user interface elements are incorporated into the core module, the principle design is still focused toward, and optimized for, using the core module with a modular system. Thus while the core module may have the features of a portable or hand-held ultrasound system, it remains primarily the core module of a larger modular system that has greater capacity for complete diagnostic ultrasound scans with a full range of peripheral devices at the ready.

**[0033]** The connection between the core module 10 and the modular system is through a receptacle module 30 or mini-dock. The receptacle module 30 connects peripheral devices to the core module 10. The receptacle module 30 comprises a receptacle housing, peripheral ports 34 and a receptacle 32. The receptacle module housing is a body designed to contain the hardware needed to provide the electronic communication between the peripheral devices and the core module 10. A plurality of peripheral device ports 34 are mounted in said receptacle housing 30, each peripheral device port is connected to one or more individual electrical connectors) for electrical communication with a receptacle 32. The receptacle 32 is designed for releasably mating with the I/O port 12 of the core module 10. Thus the core module 10 may communicate with the desired peripheral devices through the receptacle module, and visa-versa.

**[0034]** The electronic communication between said receptacle 32 and the plurality of peripheral device ports 34 can be either a pass through connection or an active connection. If the connection is active, the receptacle module 30 contains one or more active circuits. The 30 interface functions essentially as an interface converter for signals. Typically the active circuits required are analog to digital (A/D) and digital to analog (D/A) converts for video out and in. It may also perform digital-to-digital conversion (D/D) for different digital video outputs. By placing the A/D and D/A converters in the receptacle housing 30, space and weight is conserved within the core module 10. This provides a substantial weight and real estate savings in the core module 10 whether it is used as a stand alone unit, or as a central processing core for a modular system. Video A/D and D/A converters should not be needed in the core module having built in video, since the built in display should be able to use the native signal without conversion.

**[0035]** The receptacle housing may also have a latching mechanism 35 for securing itself to the core module 10. A simple latch, such as tension locking arms or hooks may be used, or an interlocking connector Like rails and grooves. A manual release of the interlocking mechanism allows for an easy release of the core module and the receptacle module. This feature may be found in another module when the receptacle module 30 is connected to either a docking station 40 or a mobile docking stand 50. The receptacle housing itself contains all the connectors needed for the core unit to interface with a wide body of peripheral devices. Examples of such connections include specialized adaptors for power 34a, printer 34b, network 34c, Ethernet 34d, RS232 adaptor 34e, S-video out 34f, VGA out 34g, composite video out 34h, sound out 34i, physio-adaptor 34j (as for an ECG measuring device), and transducer adaptor 34k. The physio port is designed for receiving input from a device that measures some physiological parameter that a user can combine with a diagnostic ultrasound scan to produce a more accurate diagnosis. Electro cardio gram (ECG) measurements are an example of such a physio-monitoring device that can be used in conjunction with the ultrasound scan. Additional controls for a full sized user interface station (keyboard, pointer, input devices) may use an additional port, or go through the Ethernet adaptor 34d or RS232 34e port. The peripheral devices are "off the shelf" materials commonly used in hospitals and ultrasound scanning environments, and the receptacle housing uses peripheral ports to match these existing technologies. However the receptacle module can be constructed and configured to communicate with virtually any device so long as the system electronics 14 has the appropriate communications protocol programmed into it. The receptacle housing may further include a surge protector (not shown) to shield the core module from electrical surges while plugged into a power supply.

**[0036]** The receptacle housing uses a plurality of electrical pins in the receptacle 32 for communication with the I/O port 12 of the core module 10. The layout of the pins varies with the intended communication the core module would need to interact with a modular system, or a series of stand alone peripherals. Further pin economy may be achieved by using the same pins for communicating to different devices through a well tinned cycle of instruction based on the system clock, such as with an I2C protocol. An example of the pin layout is as follows:

PINS 1-20	Power and ground
PINS 21-106	Digital video out
PINS 107-143	Communication links, (e.g. RS232, Ethernet, USB printer, 12C, ECG and Audio in/out.
PINS 144-200	Connection status lines, additional ground lines, and spare lines.

**[0037]** In a fourth embodiment of the present invention, a docking station 40 is designed to mate with the core module 10 through a receptacle module 30. The docking station 40 is used for connecting a plurality of peripheral devices to the core module. The docking station 40 comprising a receptacle module 30 component as described above attached to a base unit 42. The base unit 42 has a means for guiding the core module 10 into alignment with the receptacle module 30. The base 42 also preferably includes a means for securing the core module and the receptacle module into

place while connected. The means for guiding the core module into place and securing the core module into position can be the same feature. By way of example, the docking station may include a mechanical tray or cradle having an open position that the core module can be placed into, then the mechanical tray or cradle is moved to a closed position with the core module in place. The movement of the mechanical tray or cradle causes the core module to be moved into the proper position and locked into position at the same time. As long as the mechanical tray or cradle is in place, the core module cannot be removed or become misaligned. The mechanism could be a simple funnel type of guide rails that ensure the core module is Funneled into the correct orientation for proper docking. The user in this case must apply the necessary force to ensure the core module and receptacle module or docking station properly line up. An electro-mechanical device may also be used. A small motor could be used to perform the mechanical work of a person, and the motor could be activated as soon as it detects the core module in place, or by the push of a button from a user. The docking station incorporates a power supply within the base and in electronic communication with the receptacle module such that electrical power can be fed from the power supply to the core module through the receptacle module/mini-dock.

**[0038]** Alternatively the docking station may utilize a housing having a slot or aperture for slidably receiving the core module. Thus in a fashion similar to the way a VHS tape is inserted into a VCR, the core module would be placed into the docking station having a housing, and an electromechanical component would draw the core module into the housing and secure it in place. In this embodiment the housing can be either attached to the base, or incorporate the base into a single component. In this embodiment it is not possible to utilize a video display which may be incorporated into the core module, therefore it would be preferable to reinforce the internal frame of the housing to support the weight of a video display, such as a CRT, LCD or plasma display monitor.

**[0039]** In either format, the docking station would not be mobile, so the use of additional accessories that ordinarily would not be considered highly portable is logistically acceptable here. Such additional components include a larger, more ergonomically designed user interface, such as a full size QWERTY style keyboard, a pointing device such as a mouse, track ball or "joy stick." A large touch screen can also be used to allow the use of on screen hot keys and supplemental pointer device.

**[0040]** A fifth module for use with the docking station is a multi-transducer interface module 50. The multi-transducer interface module 50 has a single transducer connector 51 for mating with the docking station 40, or in the alternative with the transducer connector aperture 24 of the core module, and a plurality of transducer connector apertures 52 incorporated into the multi-tap module. In this manner the docking station 40 can have at the ready a variety of ultrasound probes, such as a neonatal probe, trans-esophageal probe, or any other probe desired to be used in a diagnostic scan. When the core module 10 is mated to the docking station 40 and powered up, the core module 10 can detect which transducers are connected to the system and select the appropriate beamformer program and data processing to match the probe. The multi-tap module 50 may incorporate either a plurality of electromechanical switches 53 to allow a user to switch between probes, or the core module 10 may contain a soft switch within its system electronics package to switch between transducers at the direction of a user.

**[0041]** Additional utility is realized in a sixth embodiment in the form of a mobile docking station 45. The mobile docking station 45 comprises a base 44 having a plurality of castors 46 wherein at least one said castor is capable of locking, a tower 48 is mounted on the base and a docking station 40 is located substantially near the top of the tower 48, the docking station 40 is capable of releasably receiving the core module 10.

**[0042]** The mobile docking station 45 can incorporate a plurality of storage bins into the tower design. The bins can be used for the storage of both peripheral devices such as a printer, data storage device and VCR, as well as peripheral equipment such as coupling gels, transducers, connecting cables and the like. The tower is preferably height adjustable and may include gas cylinders actuated by a manual trigger to raise or lower the docking station. The tower is preferably a weight balanced design to avoid imbalance of the mobile docking station either while in use, or while being moved from place to place. The tower may be any design corresponding to the weight balanced design, such as an "A" frame, "Z" frame, an inverted "T" frame, or an "I" frame. Multiple other frames are equally usable assuming the base has been weighted to compensate for the positioning of peripheral devices and accessory products that might be used in the ordinary course of the mobile docking station.

**[0043]** Similar in the design and intended use of the stationary docking station, the mobile docking station can incorporate the interface to the core module for a multi-transducer adaptor (multi-tap module) and an enhanced user interface utilizing full sized components for ease of use.

**[0044]** In another embodiment of the present invention, a system 60 is envisioned for providing enhanced diagnostic ultrasound flexibility and capacity through the use of one or more core modules 10 and a plurality of docking stations 40. The docking stations may either be desktop (stationary 40) or mobile 45 in design. In this manner, a user, such as a hospital or clinic can reduce the costs of purchasing a variety of ultrasound devices, and instead purchase a multitude of cheaper docking stations 40 or mobile docking stations 45. It can be appreciated by those who perform ultrasound scans that there is an advantage for only paying for expensive equipment such as the core module once or twice, and being able to carry that around easily and using it with cheaper docking stations or mobile docking stations. Substantial savings in capital equipment may be made in using a system of this design. The alternative embodiment of the core

module 10 which incorporates hand held functionality can then operate as a mobile or field device and then return to a docking station for operation with a plurality of peripheral devices, thus enabling the mobile unit to perform as a the processor for an ultrasound suite. The core module 10 is designed to provide complex ultrasound capabilities such as those found in large, premium devices, as well as scaled down feature sets in the event it is plugged into a dock with less capable peripherals. The core module is fairly simple in construction, yet provides the processing for as many ultrasound features as a user may desire. The core may be easily and quickly removed from one dock and inserted into another, even if the docking station is "hot" (powered).

**[0045]** Where the core module is moved from one docking station to another within system 60, the system electronics package has the capability to either automatically detect, or identify through user input, the type of ultrasound probe attached to the docking station it is being used with, and draw on the appropriate concatenated filters needed. This allows maximum flexibility and minimum user effort in the system.

## Claims

1. A mini-dock for connecting peripheral devices to a modular diagnostic ultrasound apparatus, the mini-dock comprising:
  - a receptacle housing;
  - a plurality of peripheral device ports, in or on said receptacle housing, each peripheral device port connected to one or more individual electrical connector(s), at least one peripheral device port of said plurality of peripheral device ports comprising an ultrasound transducer adapter; and
  - a receptacle for releasably mating with an I/O port of said modular diagnostic ultrasound apparatus, said receptacle in electronic communication with said plurality of peripheral device ports.
2. The mini-dock as described in claim 1, wherein the electronic communication between said receptacle and said peripheral device ports is a pass through connection.
3. The mini-dock as described in claim 1, wherein the electronic communication between said receptacle and said peripheral device ports is achieved through the use of one or more active circuits.
4. The mini-dock as described in claim 3, wherein the active circuit is a digital to analog video converter for video signal passing from the modular diagnostic ultrasound apparatus to a video device through a peripheral device port.
5. The mini-dock as described in claim 3, wherein the active circuit is an analog to digital video converter for video feed through a peripheral device port to the receptacle.
6. The mini-dock as described in claim 1, having one or more means for removably connecting the mini-dock to the modular diagnostic ultrasound apparatus.
7. The mini-dock as described in claim 1, further comprising a surge protector.
8. A docking station for connecting a plurality of peripheral devices to a modular diagnostic ultrasound apparatus, the docking station comprising:
  - a mini-dock having a housing, a receptacle, a plurality of peripheral device ports in electronic communication with the receptacle, at least one peripheral device port of said plurality of peripheral device ports comprising an ultrasound transducer adaptor;
  - a base fixedly attached to the mini-dock and having means for guiding a modular diagnostic ultrasound apparatus into alignment with said mini-dock and means for securing the modular diagnostic ultrasound apparatus to the mini-dock; and
  - a power supply incorporated within said base and in electronic communication with said mini-dock such that electrical power can be fed from the power supply to the modular ultrasound apparatus through the mini-dock.
9. The docking station as described in claim 8, wherein the base further comprises a housing having an aperture for slidably receiving said modular diagnostic ultrasound apparatus.
10. The docking station as described in claim 9, wherein said housing has a reinforced internal frame for supporting a

video display unit.

11. The docking station as described in claim 8, further comprising a plurality of user interfaces for controlling said modular diagnostic ultrasound apparatus.

12. A system for diagnostic ultrasound examinations comprising:

at least one core module having a housing, system electronics package and a I/O port; and one or more docking station capable of electronic communication with a plurality of peripheral devices, the docking station capable of releasable connection to said core module, wherein the core module is useable as an ultrasound diagnostic imaging device while docked to at least one docking station of the one or more docking station(s), and wherein all data inputs and outputs are sendable or receiveable through the docking station to or from the peripheral devices.

13. The system of claim 12, wherein the docking station is a mobile docking station.

14. The system of claim 12, wherein the one or more docking stations is a mix of mobile docking stations and desktop docking stations.

## Patentansprüche

1. Mini-Dock zum Verbinden von Peripheriegeräten mit einer modularen, diagnostischen Ultraschallvorrichtung, wobei das Mini-Dock umfasst:

ein Aufnahmegehäuse;  
eine Mehrzahl von Peripheriegeräteports bzw. -anschlüssen in oder an dem Aufnahmegehäuse, von denen jeder Peripheriegeräteport mit einem oder mehreren individuellen bzw. einzelnen elektrischen Verbindern verbunden ist, wobei zumindest ein Peripheriegeräteport der Mehrzahl von Peripheriegeräteports einen Ultraschallwandleradapter umfasst; und  
eine Aufnahme zum lösbaren Zusammenpassen mit einem I/O-Port bzw. -Anschluss der modularen, diagnostischen Ultraschallvorrichtung, wobei die Aufnahme in elektronischer Kommunikation bzw. Verbindung mit der Mehrzahl von Peripheriegeräteports ist.

2. Mini-Dock nach Anspruch 1, wobei die elektronische Kommunikation zwischen der Aufnahme und den Peripheriegeräteports eine Durchlaufverbindung ist.

3. Mini-Dock nach Anspruch 1, wobei die elektronische Kommunikation zwischen der Aufnahme und den Peripheriegeräteports durch die Verwendung einer oder mehrerer aktiver Schaltungen erreicht wird.

4. Mini-Dock nach Anspruch 3, wobei die aktive Schaltung ein Digital-Analog-Videowandler ist, um Videosignale von der modularen, diagnostischen Ultraschallvorrichtung durch einen Peripheriegeräteport an eine Videoeinrichtung zu übertragen.

5. Mini-Dock nach Anspruch 3, wobei die aktive Schaltung ein Analog-Digital-Videowandler ist, um Videos durch einen Peripheriegeräteport an die Aufnahme zu leiten.

6. Mini-Dock nach Anspruch 1, das ein oder mehrere Mittel zum lösbaren Verbinden des Mini-Docks mit der modularen, diagnostischen Ultraschallvorrichtung aufweist.

7. Mini-Dock nach Anspruch 1, ferner umfassend einen Überspannungsschutz.

8. Dockingstation zum Verbinden einer Mehrzahl von Peripheriegeräten mit einer modularen, diagnostischen Ultraschallvorrichtung, wobei die Dockingstation umfasst:

ein Mini-Dock mit einem Gehäuse, einer Aufnahme, einer Mehrzahl von Peripheriegeräteports bzw. -anschlüssen in elektronischer Kommunikation bzw. in Verbindung mit der Aufnahme, wobei zumindest ein Peripheriegeräteport der Mehrzahl von Peripheriegeräteports einen Ultraschallwandleradapter umfasst;



eine Basis, die fest an dem Mini-Dock angebracht ist und Mittel, um eine modulare, diagnostische Ultraschallvorrichtung in Ausrichtung bzw. eine Linie mit dem Dock zu bringen, und Mittel aufweist, um die modulare, diagnostische Ultraschallvorrichtung an dem Mini-Dock zu befestigen; und  
eine Leistungsversorgung, die in der Basis integriert ist und in elektronischer Kommunikation bzw. Verbindung mit dem Mini-Dock ist, so dass elektrische Leistung von der Leistungsversorgung durch das Mini-Dock an die modulare Ultraschallvorrichtung geführt werden kann.

9. Dockingstation nach Anspruch 8, wobei die Basis ferner ein Gehäuse mit einer Öffnung umfasst, um die modulare, diagnostische Ultraschallvorrichtung verschiebbar aufzunehmen.

10. Dockingstation nach Anspruch 9, wobei das Gehäuse einen verstärkten inneren Rahmen zum Tragen bzw. Stützen einer Videoanzeigeeinheit aufweist.

11. Dockingstation nach Anspruch 8, ferner umfassend eine Mehrzahl von Benutzerschnittstellen zum Steuern bzw. Regeln der modularen, diagnostischen Ultraschallvorrichtung.

12. System für diagnostische Ultraschalluntersuchungen, umfassend:

zumindest ein Kemmodul mit einem Gehäuse, einem Systemelektronik-Package bzw. -Baueinheit bzw. -Gehäuse, und einem I/O-Port bzw. -Anschluss; und  
eine oder mehrere Dockingstationen, die zur elektronischen Kommunikation bzw. Verbindung mit einer Mehrzahl von Peripheriegeräten in der Lage sind, wobei die Dockingstation zur lösbaren Verbindung mit dem Kemmodul in der Lage ist, wobei das Kemmodul als eine diagnostische Ultraschallabbildungseinrichtung verwendbar ist, während es an zumindest eine Dockingstation der einen oder mehreren Dockingstationen andockt ist, und wobei alle Dateneingaben und -ausgaben von den Peripheriegeräten durch die Dockingstation gesendet oder empfangen werden können.

13. System nach Anspruch 12, wobei die Dockingstation eine mobile Dockingstation ist.

14. System nach Anspruch 12, wobei die eine oder mehreren Dockingstationen eine Mischung aus mobilen Dockingstationen und Desktop- bzw. Tisch-Dockingstationen sind.

## Revendications

1. Mini-station d'accueil pour connecter des dispositifs périphériques à un appareil de diagnostic modulaire à ultrasons, la mini-station d'accueil comprenant :

un corps de prise ;  
une pluralité de ports d'accès pour dispositifs périphériques, dans ou sur ledit corps de prise, chaque port d'accès pour dispositif périphérique étant relié à un ou plusieurs connecteur(s) électrique(s) individuel(s), au moins un port d'accès pour dispositif périphérique parmi ladite pluralité de ports d'accès pour dispositifs périphériques comprenant un adaptateur pour transducteur à ultrasons ; et  
une prise pour se raccorder de façon amovible à un port E/S dudit appareil de diagnostic modulaire à ultrasons, ladite prise étant en communication par voie électronique avec ladite pluralité de ports d'accès pour dispositifs périphériques.

2. Mini-station d'accueil selon la revendication 1, dans laquelle la communication par voie électronique entre ladite prise et lesdits ports d'accès pour appareils périphériques est une connexion d'intercommunication.

3. Mini-station d'accueil selon la revendication 1, dans laquelle la communication par voie électronique entre ladite prise et lesdits ports d'accès pour appareils périphériques est assurée en utilisant un ou plusieurs circuit(s) actif(s).

4. Mini-station d'accueil selon la revendication 3, dans laquelle le circuit actif est un convertisseur vidéo numérique-analogique pour un signal vidéo qui transite de l'appareil de diagnostic modulaire à ultrasons à un dispositif vidéo via un port d'accès pour dispositif périphérique.

5. Mini-station d'accueil selon la revendication 3, dans laquelle le circuit actif est un convertisseur vidéo analogique-

numérique pour une source vidéo qui est raccordée via le port d'accès pour dispositif périphérique à la prise.

6. Mini-station d'accueil selon la revendication 1, pourvue d'un ou plusieurs moyen(s) permettant de raccorder de façon amovible la mini-station d'accueil à l'appareil de diagnostic modulaire à ultrasons.

7. Mini-station d'accueil selon la revendication 1, comprenant en outre une protection anti-surtension.

8. Station d'accueil pour raccorder une pluralité de dispositifs périphériques à un appareil de diagnostic modulaire à ultrasons, la station d'accueil comprenant :

une mini-station d'accueil pourvue d'un corps, d'une prise, d'une pluralité de ports d'accès pour dispositifs périphériques en communication électronique avec la prise, au moins un port d'accès pour dispositif périphérique parmi ladite pluralité de ports d'accès pour dispositifs périphériques comprenant un adaptateur pour transducteur à ultrasons ;

une base fixée de façon inamovible à la mini-station d'accueil et pourvue de moyens de guidage d'un appareil de diagnostic modulaire à ultrasons pour en garantir l'alignement avec ladite mini-station d'accueil, et de moyens de blocage de l'appareil de diagnostic modulaire à ultrasons sur la mini-station d'accueil ; et

une source d'alimentation électrique intégrée à ladite base et en communication électronique avec ladite mini-station d'accueil de telle sorte que le courant électrique peut être amené de la source d'alimentation électrique à l'appareil modulaire à ultrasons via la mini-station d'accueil.

9. Station d'accueil selon la revendication 8, dans laquelle la base comprend en outre un logement muni d'une ouverture destinée à y accueillir de façon coulissante ledit appareil de diagnostic modulaire à ultrasons.

10. Station d'accueil selon la revendication 9, dans laquelle ledit logement comporte un cadre intérieur renforcé pour supporter un terminal vidéo.

11. Station d'accueil selon la revendication 8, comprenant en outre une pluralité d'interfaces utilisateurs pour commander ledit appareil de diagnostic modulaire à ultrasons.

12. Système d'examen diagnostique par ultrasons comprenant :

au moins un module noyau doté d'un boîtier, d'un bloc système électronique et d'un port E/S ; et une ou plusieurs station(s) d'accueil capable(s) d'être reliée(s) par voie électronique à une pluralité de dispositifs périphériques, la station d'accueil pouvant être raccordée de façon amovible audit module noyau, dans lequel ledit module noyau peut être utilisé comme appareil d'imagerie diagnostique par ultrasons lorsqu'il est relié à au moins une station d'accueil parmi la ou les station(s) d'accueil, et où toutes les données en entrée et en sortie peuvent être émises ou reçues via la station d'accueil depuis ou vers les dispositifs périphériques.

13. Système selon la revendication 12, dans lequel la station d'accueil est une station d'accueil mobile.

14. Système selon la revendication 12, dans lequel la ou les station(s) d'accueil consistent en une combinaison de stations d'accueil mobiles et de stations d'accueil de bureau.

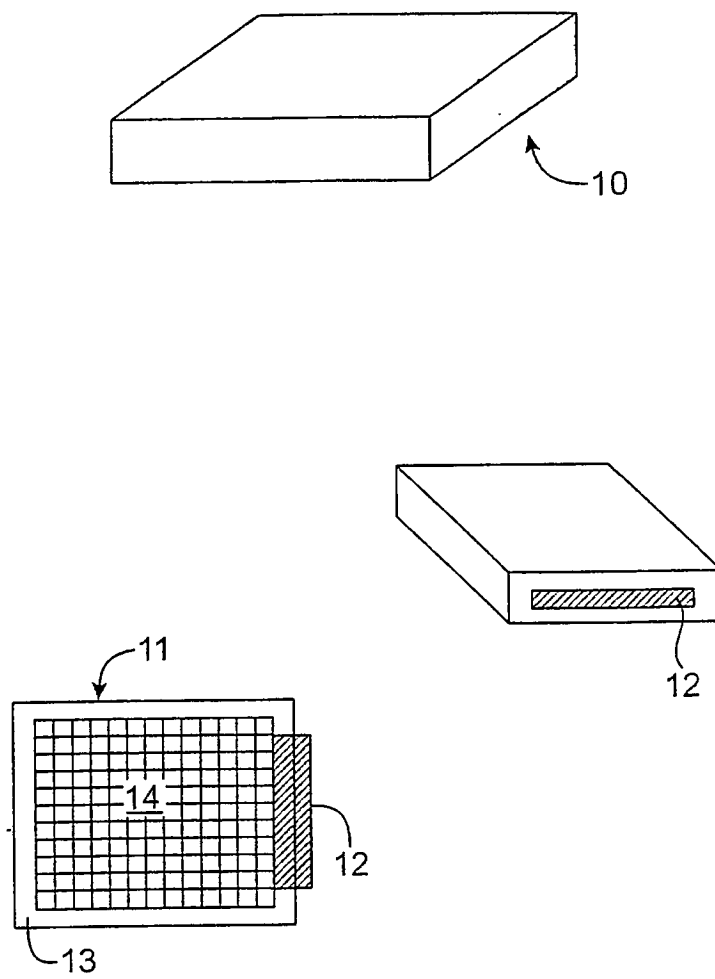


FIG. 1A

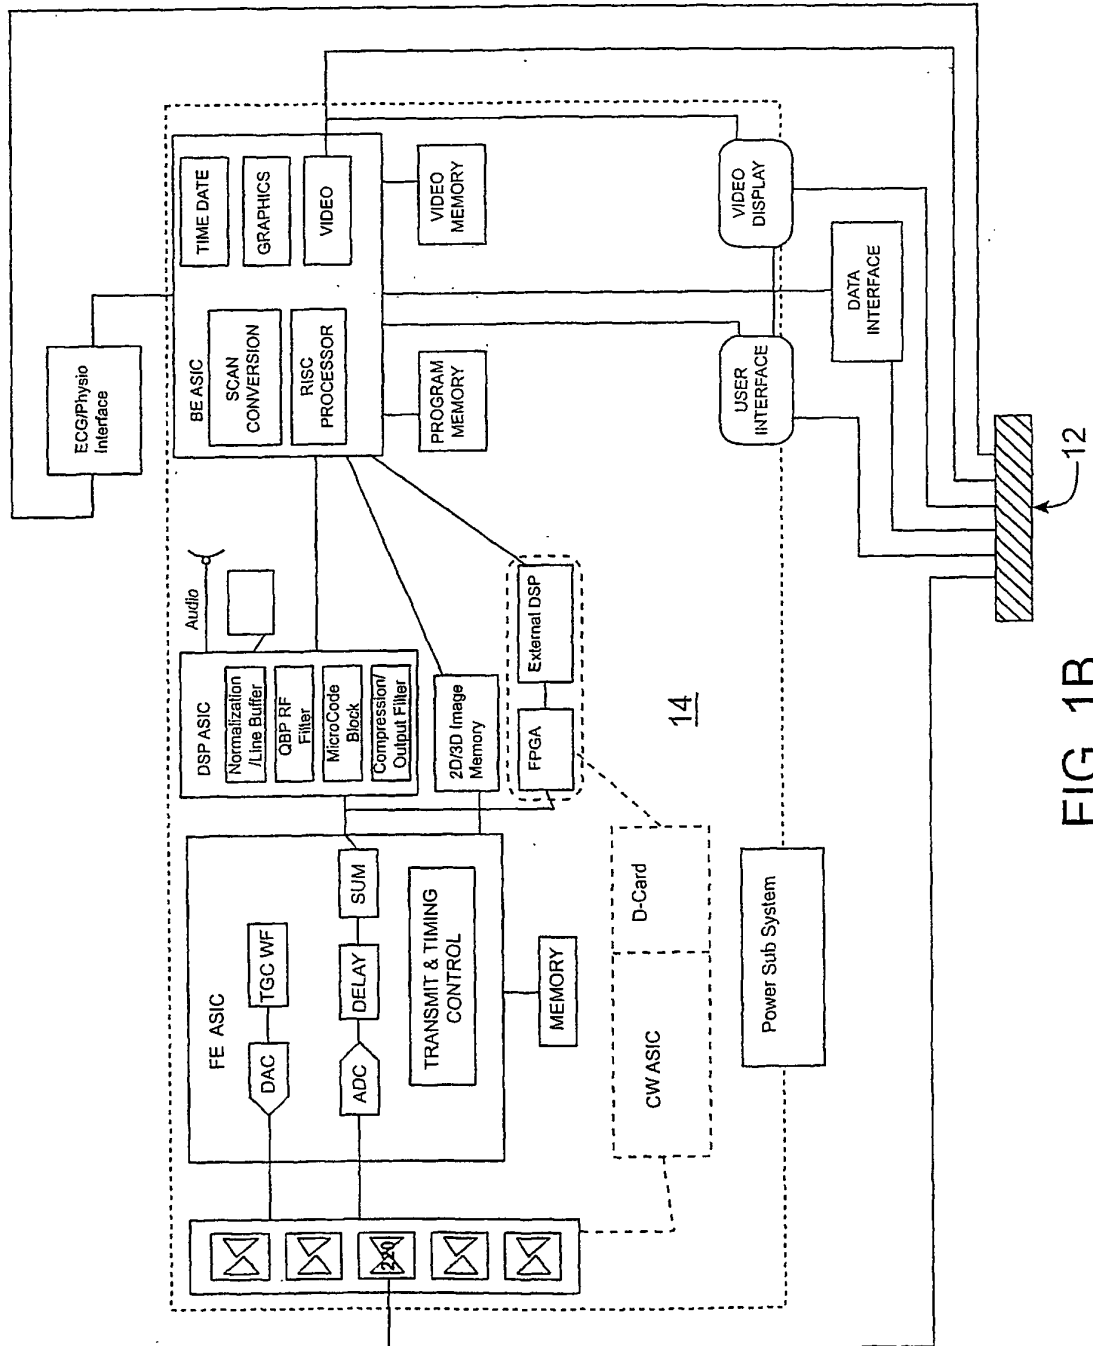


FIG. 1B

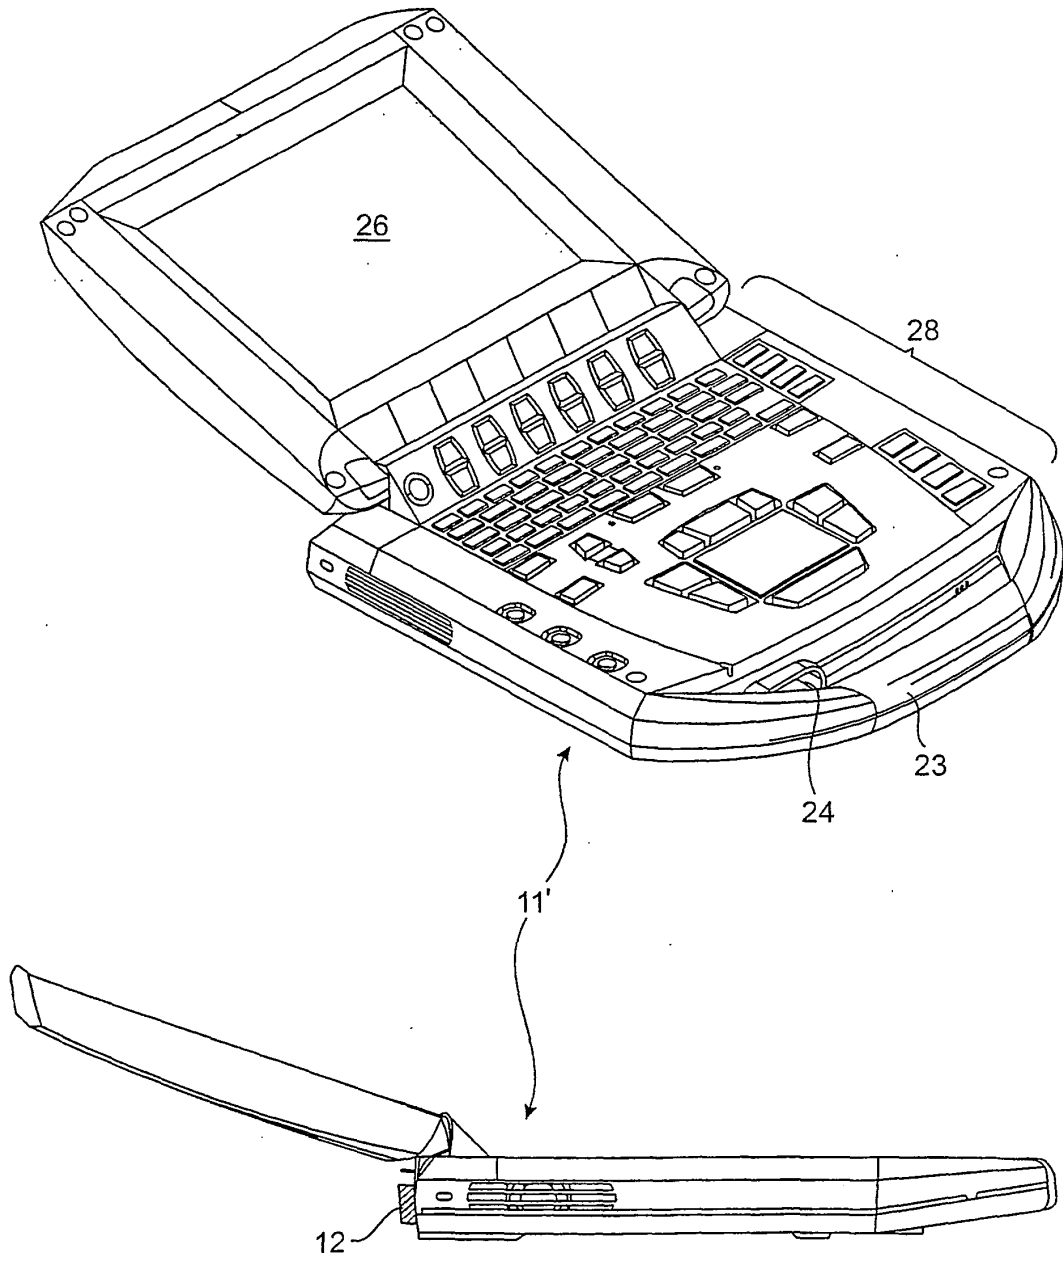


FIG. 1C

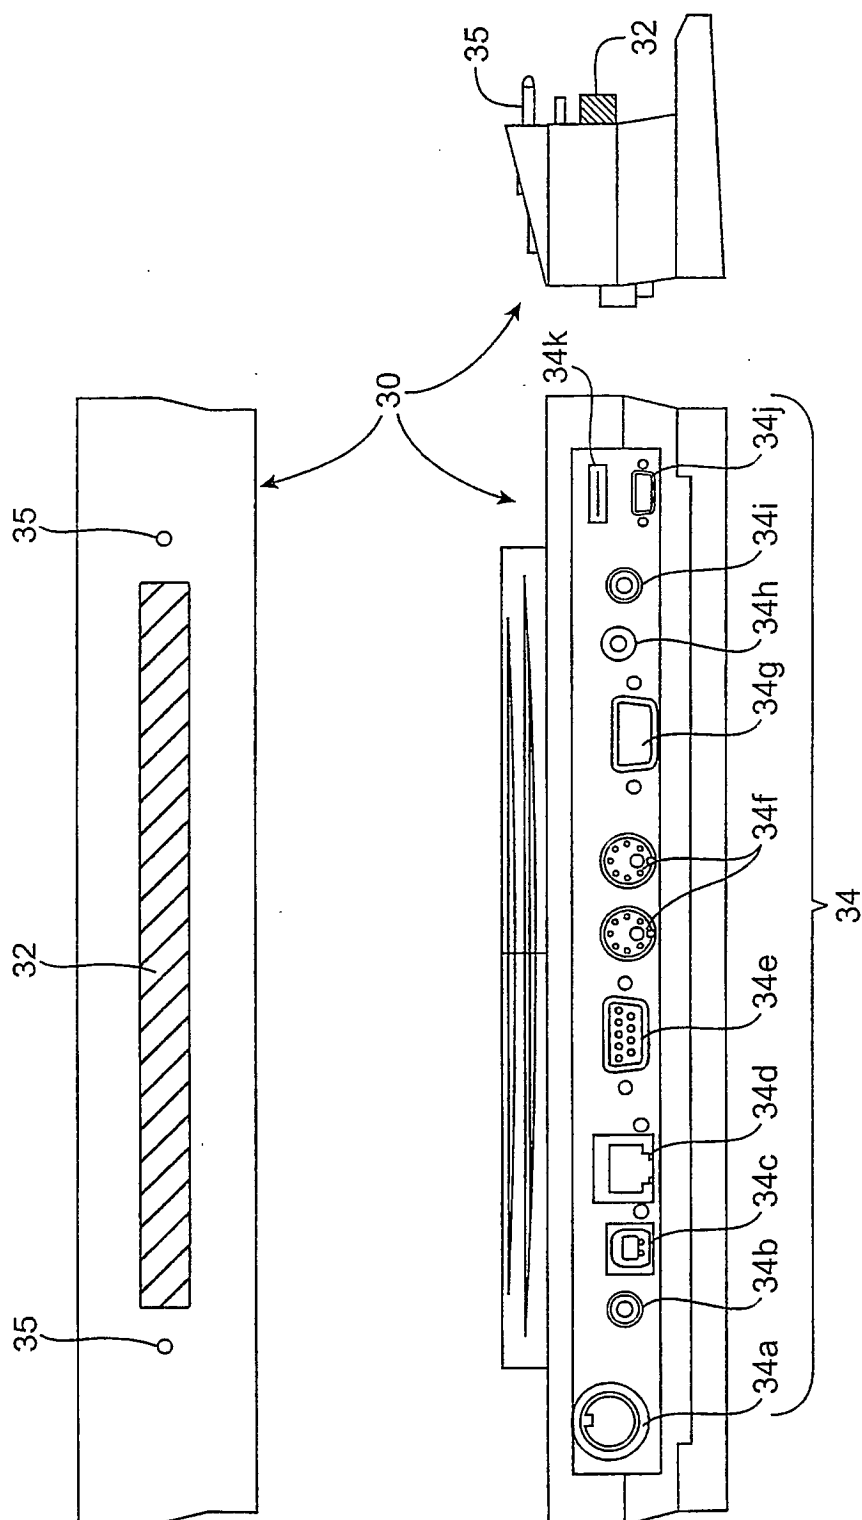


FIG. 2

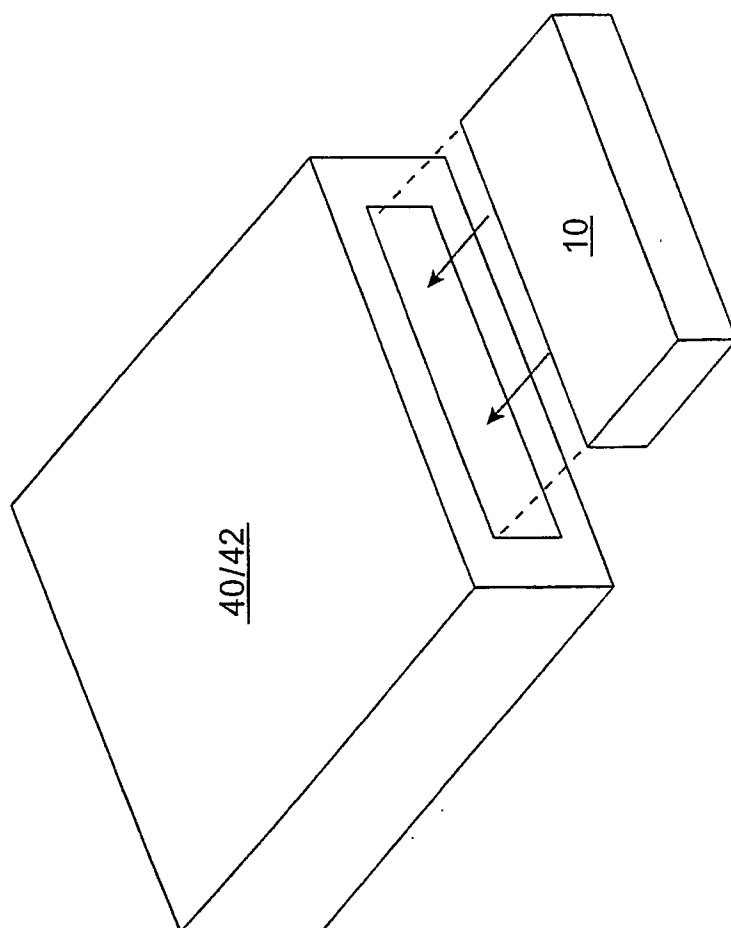


FIG. 3A

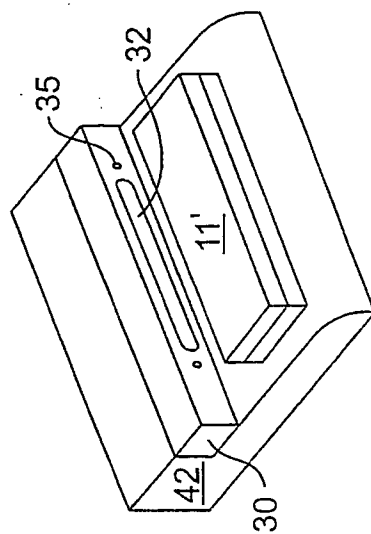


FIG. 3B

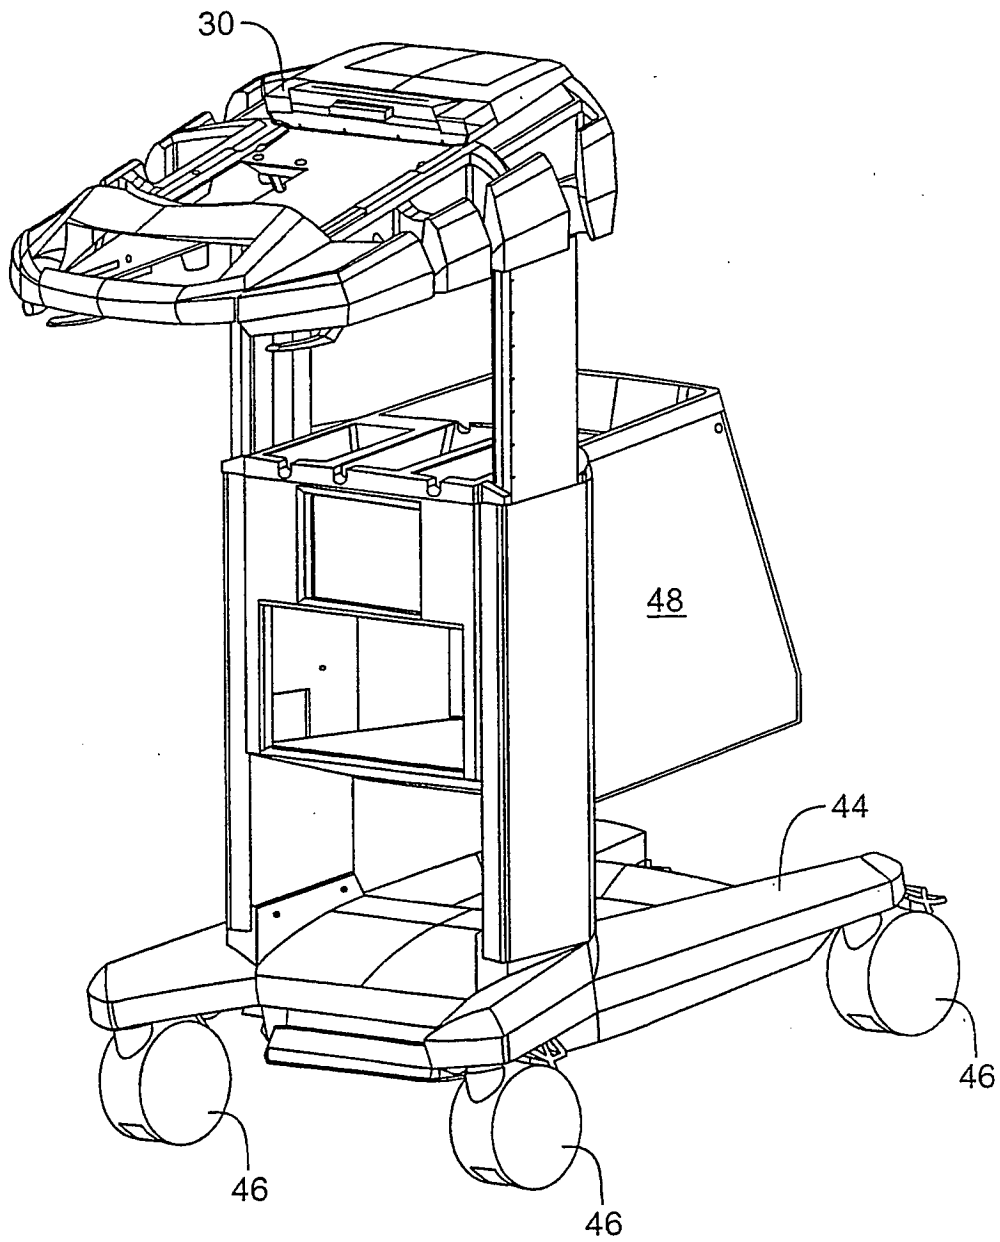


FIG. 4



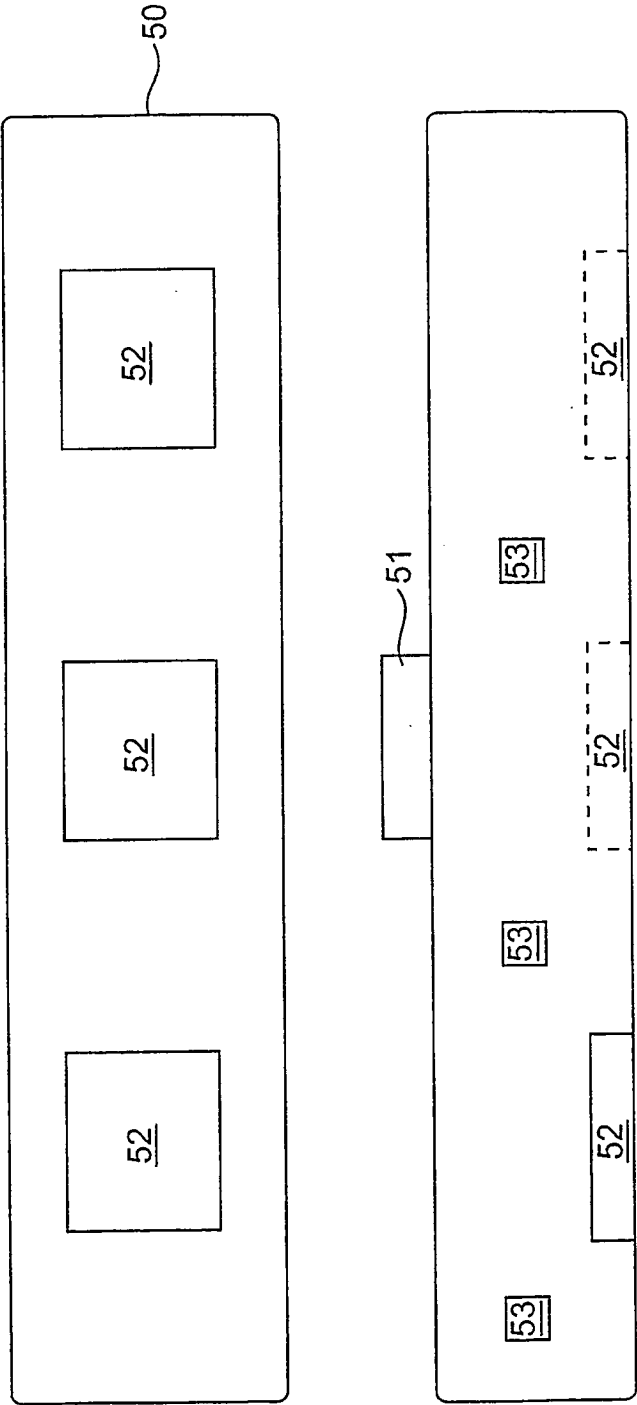


FIG. 5

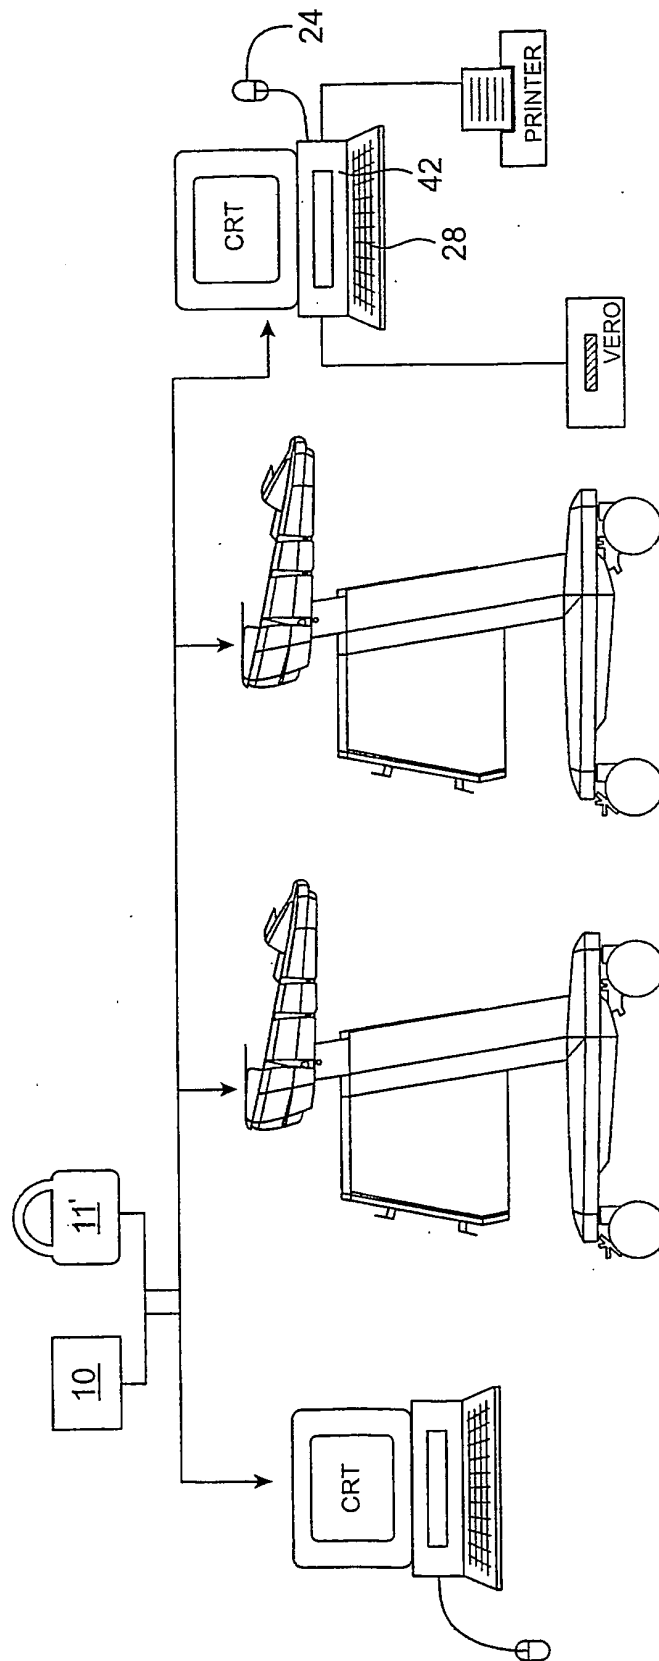


FIG. 6

专利名称(译)	用于诊断超声的模块化设备的系统		
公开(公告)号	<a href="#">EP1589878B1</a>	公开(公告)日	2009-10-28
申请号	EP2004706450	申请日	2004-01-29
[标]申请(专利权)人(译)	索诺塞特公司		
申请(专利权)人(译)	SONOSITE INC.		
当前申请(专利权)人(译)	SONOSITE INC.		
[标]发明人	HOLMBERG RANDY T LITTLE BLAKE W BUNCE STEVEN		
发明人	HOLMBERG, RANDY, T. LITTLE, BLAKE, W. BUNCE, STEVEN		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4411 A61B8/00 A61B8/4405 A61B8/4427 A61B8/4433 A61B8/56 A61B2560/0456 G01S7/52079 G01S7/52082		
优先权	10/356401 2003-01-31 US		
其他公开文献	EP1589878A2		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

本发明描述了一种与用于诊断超声的核心模块 ( 10 ) 一起使用的系统, 该系统包括至少一个核心模块 ( 10 ), 其具有壳体 ( 11 ), 系统电子组件 ( 14 ) 和 I / O 端口 ( 12 )。 ) 和与多个外围设备电子通信的一个或多个扩展坞 ( 40 ), 扩展坞 ( 40 ) 能够可释放地连接到核心模块 ( 10 )。本发明进一步详细说明了系统的各个模块化部件, 即插座连接器 ( 32 ), 扩展坞 ( 40 ), 多换能器适配器 ( 344 ) 和移动扩展坞 ( 50 )。

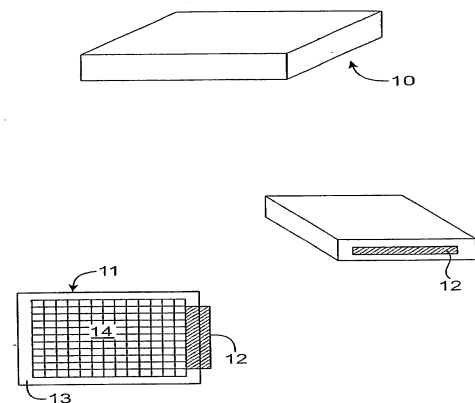


FIG. 1A