



(51) International Patent Classification:
A61B 8/00 (2006.01)

(21) International Application Number:
PCT/US2016/055649

(22) International Filing Date:
6 October 2016 (06.10.2016)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
62/238,891 8 October 2015 (08.10.2015) US

(71) Applicant: **MAYO FOUNDATION FOR MEDICAL
EDUCATION AND RESEARCH** [US/US]; 200 First
Street SE, Rochester, MN 55905 (US).

(72) Inventors: **MELLEMA, Daniel, C.**; 640 Northern
Heights Drive NE, Rochester, MN 55906 (US). **SONG,
Pengfei**; 3816 9th Street NW, Unit C, Rochester, MN
55901 (US). **URBAN, Matthew, W.**; 3634 Odyssey Drive
SW, Rochester, MN 55902 (US). **MANDUCA, Armando**;

7023 Indigo Court NW, Rochester, MN 55901 (US).
GREENLEAF, James, F.; 600 4th Street SW, Apt. 101,
Rochester, MN 55902 (US). **CHEN, Shigao**; 1605 Red-
wood Lane SW, Rochester, MN 55902 (US).

(74) Agent: **STONE, Jonathan, D.**; Quarles & Brady LLP, 411
E. Wisconsin Avenue, Milwaukee, WI 53202 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,

[Continued on next page]

(54) Title: SYSTEMS AND METHODS FOR ULTRASOUND ELASTOGRAPHY WITH CONTINUOUS TRANSDUCER VI-
BRATION

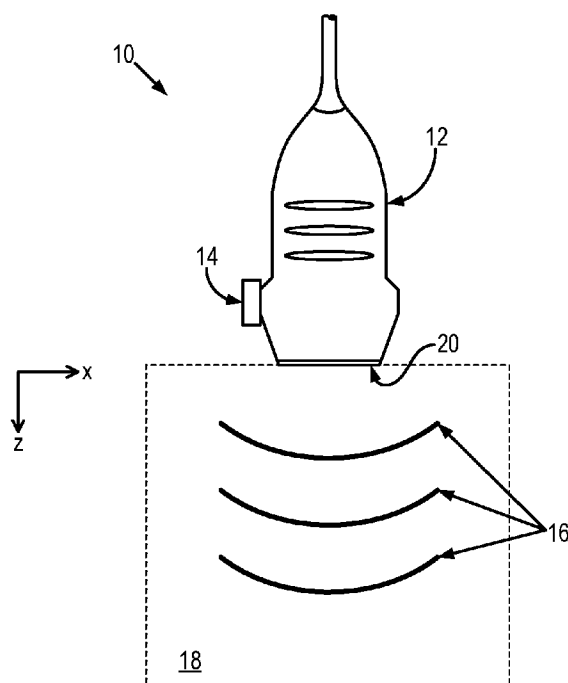


FIG. 1

(57) Abstract: Systems and methods for processing data
acquired using ultrasound elastography, in which shear
waves are generated in a subject using continuous vibra-
tion of an ultrasound transducer, are provided. The sys-
tems and methods described here can effectively remove
motion artifacts associated with vibration of the ultra-
sound transducer, and can also remove the data sampling
misalignment caused when a line-by-line imaging mode is
used to acquire data, as is done by many conventional ul-
trasound scanners. Thus, the systems and methods de-
scribed here provide techniques for transducer motion
correction and for aligning motion signals detected by
line-by-line scanning ultrasound systems.



GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ,
TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU,
TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE,
DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT,
LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE,

SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA,
GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

SYSTEMS AND METHODS FOR ULTRASOUND ELASTOGRAPHY WITH CONTINUOUS TRANSDUCER VIBRATION

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Provisional Patent Application Serial No. 62/238,891, filed on October 8, 2015, and entitled "SYSTEMS AND METHODS FOR ULTRASOUND ELASTOGRAPHY WITH CONTINUOUS TRANSDUCER VIBRATION."

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH

[0002] This invention was made with government support under DK106957 awarded by the National Institutes of Health. The government has certain rights in the invention.

BACKGROUND OF THE INVENTION

[0003] The field of the invention is systems and methods for ultrasound elastography. More particularly, the invention relates to systems and methods for processing data acquired using ultrasound elastography.

[0004] Ultrasound shear wave elastography ("SWE") has emerged as a new ultrasound imaging technique that can noninvasively and quantitatively assess tissue mechanical properties, which are strong biomarkers for the state of tissue health. Typically, in SWE shear waves are induced in tissues and the propagation of the shear waves is detected with pulse-echo ultrasound. The detection of the shear waves is then used to calculate parameters related to tissue mechanical properties, including shear wave propagation speed, dispersion (i.e., frequency dependency), shear wave attenuation, shear modulus, shear viscosity, Young's modulus, storage modulus, loss modulus, loss tangent, and mechanical relaxation time.

[0005] Conventional ultrasound SWE uses an acoustic radiation force ("ARF") to

generate shear waves in the tissue. ARF requires transmission of long-duration push pulses from the ultrasound transducer, which demands a long period of cooling time before the next transmission to avoid potential probe and tissue heating. This fundamentally limits the frame rate of ultrasound SWE (e.g., to about 1 Hz). ARF also has high power supply requirements to the ultrasound system, which makes it challenging to be implemented in mid and low-end ultrasound scanners.

[0006] To address these limitations, an ultrasound elastography technique with continuous vibration of the ultrasound transducer (e.g., the techniques described in co-pending US Provisional Application Serial No. 62/072,167). This technique generates shear waves through continuous vibration of the transducer, and detects the generated shear wave signal with the same transducer. Because this technique does not use ARF for shear wave generation, it allows for continuous high frame-rate shear wave imaging and convenient implementation with mid and low-end ultrasound systems.

[0007] The continuous vibration of the transducer, however, also introduces challenges for shear wave signal processing. One major challenge is correcting the acquired data for motion of the transducer, and another major challenge is motion signal alignment when imaging with a line-by-line scanning ultrasound system.

SUMMARY OF THE INVENTION

[0008] The present invention overcomes the aforementioned drawbacks by providing a method for measuring a mechanical property of an object using an ultrasound system having a transducer. A continuous vibration is provided to the ultrasound transducer, whereby vibration of the ultrasound transducer induces at least one shear wave in the object. Motion data are then acquired from the object using the ultrasound transducer. The motion data are indicative of the at least one shear wave

propagating within the object. A compression profile that is indicative of a deformation of the object caused by the continuous vibration of the ultrasound transducer is then estimated and used to produce corrected data by demodulating, separating, or otherwise removing the compression profile from the acquired motion data. The corrected data are then processed to calculate a mechanical property of the object.

[0009] It is another aspect of the invention to provide a method for measuring a mechanical property of an object using an ultrasound system having a transducer. A continuous and periodic vibration is provided to the ultrasound transducer, whereby vibration of the ultrasound transducer induces at least one shear wave in the object. Motion data are then acquired from the object using the ultrasound transducer. The motion data are indicative of the at least one shear wave propagating within the object, and are acquired at time points selected to mitigate motion errors attributable to deformations in the object caused by the continuous and periodic vibration. The motion data are then processed to calculate a mechanical property of the object.

[0010] It is another aspect of the invention to provide a method for measuring a mechanical property of an object using an ultrasound system having a transducer. Shear waves are induced in an object and motion data are acquired from the object using an ultrasound transducer in a pulse-echo mode. The motion data are indicative of the shear waves propagating within the object. The motion data are then corrected for errors caused by time delays between data acquisitions at different locations in the object, and the corrected data are processed to calculate a mechanical property of the object.

[0011] The foregoing and other aspects and advantages of the invention will appear from the following description. In the description, reference is made to the accompanying drawings that form a part hereof, and in which there is shown by way of illustration a preferred embodiment of the invention. Such embodiment does not

necessarily represent the full scope of the invention, however, and reference is made therefore to the claims and herein for interpreting the scope of the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] FIG. 1 is a block diagram of an example ultrasound system that implements a continuous vibration of the ultrasound transducer to induce shear waves in an object.

[0013] FIGS. 2A-2C illustrate examples of inducing shear waves and additional deformations in an object using continuous vibration of an ultrasound transducer.

[0014] FIG. 3 is a flowchart setting forth the steps of an example method for acquiring motion data in response to a continuously vibrating ultrasound transducer and correcting the acquired data for effects of the transducer vibration.

[0015] FIGS. 4A-4B illustrate examples of estimating a compression profile from k-space data generated from acquired motion data.

[0016] FIG. 5. Illustrated an example of implementing pulse-echo motion detection near peaks (circles) and valleys (squares) of a sine signal representative of a continuous transducer vibration.

[0017] FIG. 6 illustrates a schematic plot of motion signal alignment methods. The time alignment of motion detection is illustrated within zone 1. The proposed zone-to-zone alignment method is depicted for zone 2. The solid squares indicate the actual pulse echo events. The hollow circles indicate data points interpolated in time. The gray squares with dashed outlines indicate time-shifted motion signal data points based on the zone-to-zone alignment.

[0018] FIG. 7 illustrates an example of shear wave signal alignment using a phase-shift technique.

[0019] FIG. 8 illustrates a schematic plot of an aliasing correction method for low PRF, single imaging zone tissue motion detection. The upper panel shows the relationship between the actual sampling point and the sine wave signal. The lower panel shows the time-shifted sampling points that recover a non-aliasing sine signal.

[0020] FIG. 9 depicts a k-space representation of propagating shear waves and a non-propagating compression profile.

DETAILED DESCRIPTION OF THE INVENTION

[0021] Described here are systems and methods for processing data acquired using ultrasound elastography, in which shear waves are generated in a subject using continuous vibration of the ultrasound transducer. The systems and methods described here can effectively remove motion artifacts associated with vibration of the ultrasound transducer, and can also remove the data sampling misalignment caused when a line-by-line imaging mode is used to acquire data, as is done by many conventional ultrasound scanners.

[0022] Thus, the systems and methods described here provide techniques for transducer motion correction and for aligning motion signals detected by line-by-line scanning ultrasound systems.

[0023] Referring first to FIG. 1, an example system 10 for inducing shear waves in an object 20 is illustrated. In this system, the transducer 12 is mechanically vibrated by an actuator 14, which causes the transducer 12 to oscillate in the axial direction (e.g., the z-direction in FIG. 1). As one example, the actuator 14 can be a mechanical actuator, such as a voice coil actuator. As the transducer 12 moves in the axial direction, shear waves 16 are induced within the object 18. Shear waves 16 can also be produced from mode conversion of compressional waves. The produced shear waves 16 are then

detected by the same ultrasound transducer 12 operating in a pulse-echo mode to provide quantitative measurements of mechanical properties of the object.

[0024] The actuator 14 is coupled to the ultrasound transducer 12. As one example, the actuator 14 can be attached directly to the outer surface of the transducer 12. For illustration purposes, the actuator 14 is attached to one side of transducer 12 in FIG. 1. In some applications, however, it may be preferred to align the actuator co-axially with the transducer 12 so that the transducer motion is primarily axial with minimal transverse and azimuthal motions. This setup eliminates the need for a separate vibration source, and therefore allows for a convenient single-handed operation. The vibration is preferably continuous to allow continuous updating of measurements.

[0025] The ultrasound transducer 12 can be vibrated axially along the beam axis of ultrasound, or in other directions depending on the desired imaging application. The ultrasound system used for shear wave detection can be operated to detect a single A-line, multiple A-lines through parallel beam forming, or an entire 2D area or 3D volume with plane wave imaging and software beam forming, such as is done in a Verasonics® ultrasound scanner.

[0026] The continuous vibration applied to the ultrasound transducer 12 by the actuator 14 can contain multiple frequencies, and the detected shear waves can thus be processed to resolve frequency dependent properties of the object. For example, the processing may use a bandpass filter along the time dimension to select only one frequency at a time, and the subsequent processing would be identical to that as if data were collected with a single vibration frequency. Multi-frequency vibrations can speed up acquisition for dispersion analysis. With continuous vibration and continuous shear wave detection and processing, elastography measurements can be updated

continuously in a substantially real-time manner.

[0027] When the transducer 12 is vibrating in the axial direction, such as when the vibration is normal to the active surface 20 of the transducer 12, the motion of the transducer 12 will contaminate the shear wave signals detected in the object 18. This signal contamination is present because ultrasound motion detection uses the transducer 12 as a non-moving reference coordinate, but this assumption is violated when the transducer 12 is oscillating due to external vibration. Therefore, motion of the transducer 12 that is caused by the actuator 14 needs to be corrected for in order to properly measure mechanical properties from the detected shear waves.

Transducer Motion Correction

[0028] In one aspect of the disclosure, systems and methods for correcting transducer motion during continuous transducer vibration are provided. In ultrasound, measurements of tissue motion are made by comparing the time shift, τ , of ultrasound echo signals between two pulse-echo events. Because the ultrasound propagation speed, c , in soft tissues is a constant (commonly assumed to be $c = 1540$ m/s), this time shift can be converted to tissue displacement as,

$$d = \frac{c\tau}{2} \quad (1);$$

[0029] where the factor of two accounts for round trip distance in pulse-echo ultrasound detection. The mean tissue particle velocity, v , can also be calculated by,

$$v = \frac{d}{\delta} \quad (2);$$

[0030] where δ is the time interval between the two pulse-echo events. Sometimes, compounding from multiple pulse-echo events is used to form a single set of echoes to improve signal-to-noise ratio ("SNR"). In such situations, compounded pulse-

echo events may each be composed of multiple transmit-receive processes. As used herein, the term “motion” can include displacement, velocity, acceleration, and so on.

[0031] As illustrated below in FIGS. 2A–2C, and as described above, motion detection in ultrasound uses the ultrasound transducer as the reference coordinate. When vibrating the transducer itself in continuous transducer vibration, however, the transducer is in motion to produce shear waves. This has several effects. First, the reference coordinate of motion detection is moving, which adds a constant motion offset to all imaged pixels or voxels at a given time instant. Second, the transducer physically pushes on the tissue and causes a compressional deformation in the tissue. Tissue motion due to this effect changes with the location of each imaged pixel or voxel, even at the same time instance. Third, the vibrating transducer produces shear waves in tissue, which is the signal that is used to estimate tissue mechanical properties. Therefore, it is important to remove motions due to the first two effects in order to recover motions due to shear waves for accurate calculation of tissue mechanical properties.

[0032] FIG. 2A shows illustrates a uniform compression, dz , applied by an ultrasound transducer 12 at the top surface of a tissue object 18. The displacement resulting from the deformation of the tissue is dependent on both position and material properties of tissue. As an example, the black line 50 in FIG. 2B shows the change in displacement along the depth (e.g., z-direction) after compression by the continuously vibrating transducer at a time point, t_1 . The displacement is measured at a stationary reference point set at the top of the uncompressed object. Tissue compression measured by the transducer is shown as the solid grey line 52 in FIG. 2B, because the transducer surface is used as a reference coordinate here. The total tissue motion measured by the transducer, including deformation due to compression and shear

waves caused by the transducer vibration, is illustrated as the dashed line 54 in FIG. 2B.

[0033] The deformation and shear wave motion at a second time point, t_2 , are shown at FIG. 2C. In this example illustrated in FIG. 2C, the deformation 52 due to transducer compression is smaller (i.e., there is a smaller dz) and the shear wave has propagated through the medium, noted by the phase shift along the z-direction for the total motion signal 54.

[0034] Referring now to FIG. 3, flowchart is illustrated as setting forth the steps of an example method for correcting transducer motion during continuous transducer vibration. The method generally includes acquiring data from an object using a transducer that is vibrating to generate shear waves in the object while the data are being acquired from the object, as indicated at step 302. The acquired data indicate the total, observed motion in the object. After the data are acquired, a compression, or deformation, profile representative of the transducer vibration during data acquisition is estimated, as indicated at step 304. The compression profile can be estimated according to a number of different procedures, which are described below in more detail. Using the estimated compression profile, the effects of transducer motion are demodulated, separated, or otherwise removed from the acquired data, as indicated at step 306. As one example, the transducer motion can be removed from the data by subtracting the compression profile from the acquired data. From the corrected data, mechanical properties of the object can be estimated, as indicated at step 308.

Estimating the Compression Profile Using Curve Fitting

[0035] As one example method for estimating the compression profile, a curve fitting procedure can be implemented. In this approach, the compression profile can be estimated by fitting the total motion (depicted as the dashed line in FIG. 2B) to a known function. As an example, the known function can include one or more of the following:

an exponential, a polynomial, a power law, a spline, a Flamant solution, and a Boussinesq solution. In some embodiments, to account for local changes in material properties, multiple functions can be used to estimate the compression profile in multiple spatial windows at different depths. The spatial window can be a one-dimensional, two-dimensional, or three-dimensional window.

[0036] To improve the estimation of the compression profile, the measured total motion can be denoised prior to the curve-fitting procedure. As an example, denoising can be implemented using filtering or regularization methods.

[0037] The methods described here can be extended to higher-dimensional images using various approaches. In one example, the previously described fitting methods can be extended to multi-dimensional counterparts allowing for axial, lateral, and temporal estimation of the compression to be conducted for one or more frames. The term “frame” can refer to a two-dimensional (“2D”) ultrasound echo data set obtained at a given time, and multiple frames can be obtained at the same 2D plane over time. In another example, the fit is performed along a single 1D profile repeated at each lateral position, which allows for removing the effects of the transducer motion from the entire imaged frame. In other implementations, a single deformation profile can be applied to each lateral position within the image in order to further reduce the computational time. This process can also be repeated on each frame of an acquisition (i.e., applied to different time instances) to correct transducer motion from the entire acquisition over time.

[0038] In the curve-fitting example described above, transducer motion is estimated along the compression direction from a single lateral location and a single frame. Like any acquisition technique, all measurements will contain some error. As such, utilizing information from multiple spatial locations and multiple frames will

reduce random errors and provide better estimates of the true compression profile. This can be done in at least two ways.

[0039] In one method, multiple total observed motion signals measured at several adjacent lateral positions are combined using a mean, weighted mean, median, or similar technique in order to obtain a less noisy total motion measurement for curve fitting and subtraction.

[0040] In another method, the compression profile from each frame is estimated, the estimated profiles are combined into a single compression profile, and the combined profile is subtracted from each frame to remove compression effects. While each frame will be acquired at a different time point, and will compress the tissue to different degrees, it can be assumed, as a first-order approximation, that the compression profiles will be amplitude scaled versions of one another.

[0041] Thus, it is possible to normalize all of the individual compression profiles of different frames at each lateral location such that the profiles will be combined (such as using averaging) into a single compression profile for each lateral location where random noise is suppressed. The combined compression profile can be scaled by, and fit to, individual frames and then subtracted to obtain the true shear wave motion at that lateral position. The same process can be repeated for all lateral positions to obtain shear wave signals over a 2D area for further processing. Note that these two techniques are not mutually exclusive and can be used in conjunction with one another.

Estimating the Compression Profile Using Reference Data

[0042] As another example method for estimating the compression profile, a reference compression profile can be obtained and implemented. In this approach, a quasi-static compression is applied to the object and a reference compression profile is estimated by pulse-echo detection using the same ultrasound transducer. The quasi-

static compression can be achieved with manual compression or by vibrating the transducer at a frequency much lower than that typically used in shear wave imaging (e.g., 1 Hz).

[0043] It can be assumed that motions due to shear waves are negligible in this situation; thus, the measured motion profile should be due only to transducer compression. As a first-order approximation, compression profiles at different compression levels, dz , should be scaled versions of each other. Thus, one reference compression profile obtained at a single compression level should be sufficient. Alternatively, multiple compression profiles can be obtained at different compression levels, and can be scaled and combined to form a single reference compression profile with a higher signal-to-noise ratio ("SNR") using similar processes as those described above with respect to combining compression profiles for curve fitting.

[0044] The reference compression profile can be scaled, fit to the measured total tissue motion, and subtracted from the total tissue motion to obtain the true shear wave motion. The spatial and temporal averaging techniques described above with respect to curve fitting can also be used in the reference compression method to improve SNR.

Estimating the Compression Profile Using a Computational Model

[0045] As another example method for estimating the compression profile, a compression profile modeling can be implemented. In this approach, the compression profile can be obtained from finite element method ("FEM") simulation or analytical solutions. Once the modeled compression profile is known, it can be scaled, fit, and subtracted from the measured total tissue motion as described above. As a first approximation, the object can be assumed to be homogeneous. For a homogenous medium, the compression profile from a flat surface transducer should not change with the shear modulus of the medium. Therefore, a typical shear modulus, such as 1 kPa, can

be used for such modeling. For objects containing heterogeneous materials or tissues, compression profiles from homogeneous assumptions can be used to obtain the first order solution of the 2D elasticity image of the object. This image can then be used to run another FEM simulation to obtain a more accurate compression profile for better reconstruction of the true 2D elasticity image of the object.

Estimating the Compression Profile Using Adaptive Estimation

[0046] As another example method for estimating the compression profile, an adaptive estimation method can be implemented. In this approach, the compression profile can be estimated by applying spatial mean, weighted mean, median or similar techniques to the measured total motion in a series of small spatial windows along the depth axis (i.e., the z-axis). The spatial window can be a one-dimensional, two-dimensional, or three-dimensional window. It is contemplated that shear waves will be cyclic over the depth direction and will diminish when applying the averaging process. Thus, after the averaging process it is contemplated that the compression profile will remain. Similar to the curve fitting method described above, these adaptive methods can incorporate information from multiple spatial locations and temporal instances to increase the accuracy and precision of the estimated compression profile. This can be done by applying either multidimensional convolution techniques with specialized kernels, such as Gaussian or Laplacian kernels, or other multidimensional filters, such as median or bilateral filters.

Removing the Compression Profile in k-Space

[0047] In some situations it is not necessary to estimate the compression, but instead the compression can be directly decoupled from the shear waves. If multiple frames are acquired across the full motion path of the transducer, such that motion is

obtained in both the depth direction (e.g., z-direction) and lateral direction (e.g., x-direction) at multiple time points (e.g., frames), the propagating shear wave signal can be separated from the compression. This can be done by utilizing the differences in the k-space representation of propagating waves and non-propagating motion.

[0048] As shown in FIG. 9, for a wave propagating in the depth direction (e.g., the z-axis), the spectral representation in the k-space k_z -f plane (where k_z denotes the wavenumber in the depth direction and f denotes the temporal frequency) will contain two conjugate symmetric peaks 90, 92. The first peak 90 is located at the point corresponding to the positive wavenumber and temporal frequency of the signal, and the second peak 92 is radially symmetric to the first and is located at the point corresponding to the negative wavenumber and negative temporal frequency. Thus, the k-space representation of the propagating signal will occur in non-adjacent quadrants of the k_z -f plane, and is not conjugate symmetric across the k_z -axis. Given that, as a first-order approximation, the compression profile will be amplitude scaled, but non-propagating, the spectral information 94 associated with the compression profile in k-space will be conjugate symmetric across the k_z -axis. A representation of the k-space for a propagating wave and non-propagating compression is shown in FIG. 9.

[0049] Because the compression profile is conjugate symmetric across the k_z -axis, while the propagating waves do not share this same property, the shear waves can be decoupled from the compression by utilizing this difference in symmetry. One method to accomplish this is to represent each point in k-space as $k(f_M, k_{zN})$, where f_M and k_{zN} represent one of the temporal frequencies and wavenumber pairs defining a single point in k-space. The complex conjugate of $k(f_M, -k_{zN})$ can be added to all points, $k(f_M, k_{zN})$, defined in k-space, and the shear wave motion can then be recovered by applying the inverse Fourier transform on the k-space data. To restore the wave

propagation the quadrants that did not originally contain the shear wave signal can be attenuated or set to zero before applying the inverse Fourier transform. While this method was described here for waves propagating in 1D space and 1D time, it will be appreciated by those skilled in the art that this method can be readily extended to 2D space, 3D space, and so on.

Estimating the Compression Profile from k-Space

[0050] As another example method for estimating the compression profile, the compression profile can be estimated from k-space. In this approach, a Fourier transform is applied along the depth direction (e.g., the z-axis) of the observed signal, $u(z)$, at a given frame to obtain the frequency domain representation $U(k_z)$. This frequency domain representation can be referred to as k-space. For a given pixel in k-space with coordinate k_z , the distance to the origin of k-space is representative of the spatial frequency of that pixel.

[0051] It can be assumed that the compression profile is slowly increasing and smooth. Thus, the deformation signal in k-space will also retain smoothness. However, the k-space components of the shear wave will be at distinct points in k-space corresponding to the wavelength in image space. This results in increased amplitudes at one or more values of k_z associated with the frequencies of those shear wave components. When the k-space combined spectrum of the compression and shear wave signals are evaluated together, the spectrum will be smoothly varying with one or more amplitude discontinuities due to the shear wave motion signal. By removing the k-space components corresponding to the shear wave signal through the use of mean, weighted mean, median, or other filtering methods, an estimate of the frequency components corresponding to the compression profile can be obtained. The estimated compression profile can be produced by performing an inverse Fourier transform to convert the k-

space signal back to image space. The spatial averaging or frame averaging approaches described above can be used to improve the SNR of the compression profile estimation. Alternatively, this method can be extended to higher dimensions when using 2D/3D spatial region and/or including temporal dimension by using multiple frames.

[0052] This process is generally illustrated in FIG. 4A, where a sinusoidal shear wave signal has been added to a compression profile simulated using a FEM simulation of an elastic material (black dots). Using the Fourier transform to convert to k-space, the resulting spectrum has a single frequency component corresponding to the shear wave at 50 m^{-1} (FIG. 4B, solid line). Applying a sliding median filter with 10 m^{-1} sliding window (applied from $10\text{--}200 \text{ m}^{-1}$) leads to the filtered spectra (FIG. 4B, dashed with dots). The filtered spectrum has no peak corresponding to the shear wave signal, and when transformed back to image space provides an estimate of the compression profile due to transducer motion (FIG. 4A, solid line).

Ultrasound Detection at Peaks or Valleys of Sine Wave

[0053] In some embodiments, the compression profile is not estimated, but rather the data acquisition is altered to minimize the effects of the transducer motion. Particularly, for a transducer vibrating sinusoidally, pulse-echo detection made at time instances near the peaks or valleys of the sine signal may suppress tissue deformation due to the transducer compression.

[0054] As shown in FIG. 5, when the two pulse echo events of motion detection are made at times t_1 and t_2 symmetric to the peak of the sine wave (i.e., the time from t_1 to the peak of the sine wave is equal to the time from the peak of the sine wave to t_2), the transducer will be at the same compression position, dz , at both times t_1 and t_2 . By acquiring data at these times, tissue deformation is not detected because the pulse-echo only detects relative motion between times t_1 and t_2 . As a result, only propagating shear

waves are detected using this acquisition.

[0055] Similarly, detection at valleys of the sine wave (the squares in FIG. 5) can also be implemented to suppress tissue deformation due to transducer compression. The method is valid for different time intervals between the pulse echo events, as long as they are placed symmetric to the peak or valley of the sine wave. However, because the detected motion is an averaged motion between these two pulse echo events, the time interval, $\Delta t = t_2 - t_1$, should not be too large in order to provide sufficient time resolution for shear wave detection. Note that the sine signal is periodic; therefore, detection events at one or more whole cycles apart from t_2 , such as t_3 in FIG. 5, are identical to the detection event at t_2 . This allows more flexibility in pulse-echo timing.

[0056] In the cases where detections do not occur when the transducer is at the same position, it is possible to obtain an image with the effects of transducer motion minimized. This can be done by utilizing other detections to recover or estimate the motion when the detections were symmetric about the peak or valley of the motion profile. This can be performed using interpolation, parametric fitting, or phase shifting methods.

Using a Motion Sensor to Measure Transducer Motion

[0057] As another example method for estimating the compression profile, the compression profile can be estimated from data acquired with motion sensors that are coupled to or integrated with the ultrasound transducer. In this approach, motion sensors for measuring acceleration, velocity, displacement, and so on can be coupled to or integrated within the ultrasound transducer to measure its vibration. This approach provides certain additional advantages. As one example, the vibration response of the transducer may have a phase delay compared to the sine signal that is used to drive the

actuator that vibrates the transducer. In these instances, a sensor measuring the motion of the transducer can provide accurate synchronization for ultrasound detection at the peaks or valleys of the sine wave as described above. As another example, the transducer motion measured by motion sensors may be used to properly scale the deformation profiles in the motion subtraction methods described above. Thus, it is contemplated that using motion sensors to measure the motion of the transducer can be used alone or in combination with the methods described above.

[0058] As an alternative to using a motion sensor, the motion of a stationary target detected by the moving transducer can also be used to estimate the position of the transducer, and to improve the accuracy of synchronization for ultrasound detection at the peaks or valleys of the sine wave as described above. As an example, the stationary target can be a non-moving bone or a tissue target at a deep position (where shear waves are fully attenuated) in the field of view of the transducer.

Correction of Time Delay in Ultrasound Motion Detection

[0059] In another aspect of the disclosure, systems and methods for correcting time delays in ultrasound motion detection are provided. After shear waves are generated in tissues, the shear waves can be detected using pulse-echo motion detection, as described above. To produce a 2D image of mechanical properties of tissue, simultaneous detection of tissue motion over a large 2D area with high temporal resolution is desired. This can be achieved by "plane wave" imagers, where echoes from every pixel within the 2D detection area can be reconstructed from a single transmission of a plane ultrasound wave.

[0060] However, most commercial ultrasound scanners do not use plane wave imaging, but instead still use a sequential line-by-line scanning approach, where

multiple pulse-echo events are required to cover a 2D detection area. Line-by-line scanners thus have a significantly lower imaging frame rate than plane wave imagers. In addition, with line-by-line scanners, the time delay between each imaging line within the 2D imaging area needs to be accounted for in order to correctly calculate the mechanical properties of tissues from detected shear waves. Several techniques for addressing this challenge for detecting shear waves with line-by-line scanners are described below.

[0061] As shown in FIG. 6, a transducer 12 implemented in a line-by-line scanner can be operated to sequentially and periodically fire detection beams in a first zone of the transducer 12 (e.g., zone 1) following an order,

$$V_1 \rightarrow V_2 \rightarrow V_3 \rightarrow \dots V_N \rightarrow V_1 \rightarrow V_2 \rightarrow \dots V_N$$

[0062] where V is the imaging vector each containing n imaging A-lines that can be parallel beamformed during one pulse-echo event; N is the total number of imaging vectors within each imaging zone; and M is the number of pulse-echo events acquired at each imaging vector position. The solid black squares in FIG. 6 represent the time instances of pulse-echo events, and the number next to each black square indicates the time sequence of each pulse-echo event.

[0063] Assuming that the pulse repetition frequency for the pulse-echo events is PRF_0 , then the upper limit of PRF_0 is controlled by the imaging depth. The effective pulse repetition frequency at each vector is,

$$PRF_e = \frac{PRF_0}{N} \quad (3);$$

[0064] It is often desirable to maintain a high PRF_e , such as 1 kHz; therefore, N should be small enough to sustain a high PRF_e . Reducing the number of imaging

vectors, however, will reduce the size of each zone; thus, with smaller values of N , multiple zones may be required to cover a large 2D detection area.

[0065] As shown in FIG. 6, the sequential tracking proceeds to another zone (e.g., zone 2) of the transducer 12 after all of the M samples have been collected for each vector in the preceding zone (e.g., zone 1). The same tracking sequence is repeated until all of the M samples have been collected for each vector in zone 2. Detection events for zone 2 are also represented by the black solid squares under zone 2. This process can be repeated until data in all zones are collected.

[0066] There are two problems with motion signals detected using the sequential tracking method as shown in FIG. 6. First, the detection events are not aligned in time within each zone. Second, there is a time delay,

$$\Delta t = \frac{N \cdot M}{PRF_0} \quad (4);$$

[0067] between temporally adjacent zones (e.g., zone 1 and zone 2). As explained above, proper calculation of tissue mechanical properties requires that motion signals over the entire 2D imaging area should have the same time grid (i.e., should be time aligned).

[0068] Methods for aligning shear wave signals within each zone, such as the time interpolation described in co-pending US Provisional Patent Application Serial No. 62/072,167, can be used to correct for non-aligned motion signals. In time interpolation, echoes from each vector over different pulse-echo events are first used to calculate tissue motion, which includes motion due to shear waves and deformation from transducer compression. Therefore, in time interpolation techniques, tissue motion is measured at the black solid squares. Interpolation in time at each vector position (indicated as white circles in zone 1 of FIG. 6) can align tissue motion signal

within each zone.

Motion Signal Alignment: Phase Shift Signal to a Common Time Grid

[0069] As one example, motion signals can be aligned to a common time grid by applying appropriate phase shifts to the misaligned motion signals. Because tissue motion is a sine wave of known frequency, it allows additional methods to align the motion signal. Assume tissue motion, M_1 , detected by vector V_1 in zone 1 as,

$$M_1(t) = D_1 \cdot e^{j\omega t} \quad (5);$$

[0070] where D_1 is the motion amplitude at vector V_1 , and ω is the frequency of continuous vibration from the ultrasound transducer. The tissue motion detected by vector V_{N+1} in zone 2 will be,

$$M_{N+1}(t) = D_{N+1} \cdot e^{j\omega \left(t + \frac{N \cdot M}{PRF_0} \right)} \quad (6);$$

[0071] where D_{N+1} is the motion amplitude at vector V_{N+1} , and $(N \cdot M)/PRF_0$ is the time delay between vector V_1 and V_{N+1} . A phase shift of $\exp(j\omega((N \cdot M)/PRF_0))$ can be applied to the signal in Eqn. (6) so that the time is aligned with that in Eqn. (5),

$$D_{N+1} \cdot e^{j\omega \left(t + \frac{N \cdot M}{PRF_0} \right)} \cdot e^{-j\omega \left(\frac{N \cdot M}{PRF_0} \right)} = D_{N+1} \cdot e^{j\omega t} \quad (7).$$

[0072] This phase shift method can be used to align vectors within each zone, and to align vectors across zones.

[0073] An example of the zone-to-zone time alignment method described above is shown in FIG. 7. In this example, a 50 Hz continuous vibration was used to produce continuous shear waves inside a tissue-mimicking homogeneous phantom. The PRF_e for shear wave detection was 500 Hz, the parallel beamforming capability was 4, total number of imaging vectors was 64, the number of imaging zones was 2, and the number

of temporal samples for each vector was 24. Before alignment, the zone-to-zone discontinuity of the shear wave signal along the lateral dimension can be seen. After within-zone alignment by time interpolation, the sequential tracking delay within each imaging zone was corrected, as can be seen by careful observations of the slope of the shear wave signal. However, the zone-to-zone discontinuity still exists, as predicted in Eqn. (6). After zone-to-zone time alignment, it can be seen that the zone-to-zone discontinuity was successfully removed (i.e., a continuous vibration can be clearly appreciated across different imaging zones).

Motion Signal Alignment: Parametric Fitting

[0074] As another example of aligning motion signals, the detected tissue motion at a given pixel over multiple time points (frames) can be fit to a sine time function to estimate the amplitude and phase of the sine wave signal as a function of time. Once the amplitude and phase of the sine time-function is known, motion signals at any time point can be calculated. The amplitude and phase parameters of the sine signal at each pixel can thus be estimated, and the motion signal at all pixels at a commonly aligned time grid can then be calculated. This method can be used to time-align pixels detected with different vectors within each zone or across zones.

Motion Signal Alignment: Synchronization Using 2π shift of the Sine Motion Signal

[0075] As yet another example, motion signals can be aligned based on the cyclic nature of tissue motions produced by continuous sinusoidal vibration of the transducer. In these instances, the motion signal at each spatial location is temporally repeated with a period of T . The period, T , is determined by the angular frequency, ω , of the continuous vibration,

$$T = \frac{2\pi}{\omega} \quad (8);$$

[0076] therefore, the sine motion signal repeats itself over a phase difference of 2π , or a time period of T . The motion signals from two imaging zones can thus be time-aligned by careful design of the time delay, Δt , in FIG. 6, such that,

$$\Delta t = k \cdot T = k \cdot \frac{2\pi}{\omega} \text{ for } k = 1, 2, 3, \dots \quad (9).$$

[0077] Thus, by selecting the time delay according to Eqn. (9), the motion signals from different imaging zones are “automatically” aligned without the need of further time alignment.

[0078] Based on Eqns. (4) and (9), the vibration frequency, ω ; the detection PRF_0 ; the number of temporal samples, M ; and the number of imaging vectors within each zone, N , can all be fine-tuned to fulfill the condition described in Eqn. (9).

[0079] Alternatively, a “wait time,” ε , can be added between the detection zones such that,

$$\Delta t = \frac{N \cdot M}{PRF_0} + \varepsilon \quad (10).$$

[0080] As a result, the wait time, ε , can be conveniently adjusted to meet the requirement of Eqn. (9), or, the detection events for each zone can be initiated by an external trigger signal that is synchronized to a fixed phase over different cycles of the sine vibration signal. Note that within-zone alignment is still necessary to remove the time-delay induced by within-zone sequential tracking.

Motion Signal Alignment: Within Zone Processing

[0081] As can be seen in FIG. 7, after within-zone alignment, tissue motion signals within each imaging zone are aligned and ready to be used for calculation of mechanical properties. In some instances, however, instead of aligning motion signals across different imaging zones, tissue mechanical properties can be calculated within

each individual zone, and then the estimates from different zones can be combined into a final map. In this way, discontinuities of the motion signal across zones would not matter. If there are small discontinuities in the final mechanical property map between zones, a spatial filter (e.g., a median filter) can be used to smooth the final mechanical property map. This approach is suitable for continuous transducer vibration shear waves because the primary shear wave propagation direction is top-to-bottom, away from the transducer. This propagation direction is primarily within zone with little across-zone propagation, and thus makes calculation of tissue mechanical properties within each zone feasible.

Motion Signal Alignment: Single Imaging Zone Detection

[0082] Another solution to the motion signal alignment problem is to avoid using multiple imaging zones (i.e., to use only a single imaging zone). Using a single imaging zone generally requires a large number of imaging vectors (i.e., a large value of N) to cover a sufficiently large imaging area. The challenge of this approach, however, is that the PRF_e will be too low if N is very large. Low PRF_e can be problematic in terms of causing aliasing, especially for transient and broadband shear waves produced by acoustic radiation force.

[0083] However, for continuous tissue motion produced by transducer vibration, the aliasing can be corrected for by taking advantage of the cyclic nature of the sine wave used to drive the continuous vibration of the transducer. As illustrated in FIG. 8, the detection PRF_e and the vibration frequency, ω , can be carefully selected such that by shifting the pulse-echo events (represented as circles in FIG. 8) by integer multiple numbers of sine cycles, the non-aliased motion signal can be reconstructed.

[0084] In the example shown in FIG. 8, $PRF_e = 0.8\omega/2\pi$, which causes aliasing.

By shifting data samples 2, 3, 4, and 5 by one cycle, two cycles, three cycles, and four cycles, respectively, the original sine signal can be reconstructed without aliasing. This can be done for each imaging vector within the single imaging zone to obtain non-aliased shear wave signals. After this step, additional time alignments across different vectors, as described above, can then be used to account for delays among vectors.

[0085] After correcting for effects of transducer motion (e.g., using the methods described above) and time delay in ultrasound pulse-echo motion detection, 2D shear wave signals at a common time grid can be used to calculate mechanical properties of tissue using standard elastography processing methods, such as Local Frequency Estimation ("LFE"), time-of-flight, direct inversion, and other methods.

[0086] It is assumed that the ultrasound transducer is vibrating at a single frequency in the examples given above. The methods described here can also be readily extended to situations where the continuous transducer vibration contains multiple sinusoidal frequencies, or a chirp signal. As such, mechanical properties can be measured over multiple frequencies.

[0087] The techniques above have been described for 2D elastography imaging using a 1D-linear ultrasound array transducer. These techniques are also applicable to single element, 1D curved array, 1.5D array, 1.75D array, and 2D array transducers. For single element transducers, the methods can be scaled down to 1D elastography. For 2D arrays, the methods can be extended to 3D elastography imaging. The correction of transducer motion and delay in ultrasound motion detection can also be combined together. The methods described here can also be used for measuring mechanical properties of tissues and non-tissue materials such as polymers.

[0088] The present invention has been described in terms of one or more preferred embodiments, and it should be appreciated that many equivalents,

alternatives, variations, and modifications, aside from those expressly stated, are possible and within the scope of the invention.

CLAIMS

1. A method for measuring a mechanical property of an object using an ultrasound system having a transducer, the steps of the method comprising:
 - (a) providing a continuous vibration to the ultrasound transducer, whereby vibration of the ultrasound transducer induces at least one shear wave in the object;
 - (b) acquiring motion data from the object using the ultrasound transducer, wherein the motion data are indicative of the at least one shear wave propagating within the object;
 - (c) estimating a compression profile indicative of a deformation of the object caused by the continuous vibration of the ultrasound transducer;
 - (d) producing corrected data by separating the compression profile from the acquired motion data; and
 - (e) processing the corrected data to calculate a mechanical property of the object.
2. The method as recited in claim 1, wherein the compression profile is estimated by fitting the acquired motion data to a function that approximates the deformation of the object caused by the continuous vibration of the ultrasound transducer.
3. The method as recited in claim 2, wherein the function is based on at least one of an exponential, a polynomial, a power law, a spline, a Flamant solution, or a Boussinesq solution.

4. The method as recited in claim 1, wherein the compression profile is estimated by providing reference data indicative of the deformation of the object caused by the continuous vibration of the ultrasound transducer.

5. The method as recited in claim 4, wherein the reference data represents a quasi-static compression of the object.

6. The method as recited in claim 1, wherein the compression profile is estimated by a numerical simulation of deformations of a simulated object caused by continuous vibrations.

7. The method as recited in claim 1, wherein the compression profile is estimated by adaptively estimating the compression profile from the acquired motion data.

8. The method as recited in claim 1, wherein the compression profile is estimated by Fourier transforming the motion data to k-space, identifying spectral information associated with the compression profile in k-space, and Fourier transforming the identified spectral information to produce the estimate of the compression profile.

9. The method as recited in claim 1, wherein step (c) includes Fourier transforming the acquired motion data to produce k-space data having spectral information indicative of the compression profile, and wherein step (d) includes

identifying spectral information in the k-space data not indicative of the compression profile and Fourier transforming the identified spectral information to produce the corrected data.

10. The method as recited in claim 1, wherein the compression profile is estimated by a motion sensor coupled to the ultrasound transducer.

11. The method as recited in claim 1, wherein the compression profile is removed from the motion data by subtracting the estimated compression profile from the motion data.

12. A method for measuring a mechanical property of an object using an ultrasound system having a transducer, the steps of the method comprising:

- (a) providing a continuous and periodic vibration to the ultrasound transducer, whereby vibration of the ultrasound transducer induces at least one shear wave in the object;
- (b) acquiring motion data from the object using the ultrasound transducer, wherein the motion data are indicative of the at least one shear wave propagating within the object and wherein the motion data are acquired at time points selected to mitigate motion errors attributable to deformations in the object caused by the continuous and periodic vibration; and
- (c) processing the motion data to calculate a mechanical property of the object.

13. The method as recited in claim 12, wherein the motion data are acquired at time points that are symmetric about at least one of a peak or a valley in the continuous and periodic vibration.

14. The method as recited in claim 13, wherein the time points are

15. The method as recited in claim 12, wherein the time points are selected based on data representative of the continuous and periodic vibration that is received from a motion sensor coupled to the ultrasound transducer.

16. The method as recited in claim 12, wherein the time points are selected based on data representative of the continuous and periodic vibration that is received by detection of motion from a position of a stationary target.

17. A method for measuring a mechanical property of an object using an ultrasound system having an ultrasound transducer, the steps of the method comprising:

- (a) providing a continuous vibration to the ultrasound transducer, whereby vibration of the ultrasound transducer induces at least one shear wave in the object;
- (b) acquiring motion data from the object using the ultrasound transducer in a pulse-echo mode, wherein the motion data are indicative of the shear waves propagating within the object;
- (c) correcting the motion data for errors caused by time delays between data acquisitions at different locations in the object; and

- (d) processing the corrected data to calculate a mechanical property of the object.

18. The method as recited in claim 17, wherein correcting the motion data includes shifting signals in the motion data detected at the different locations to a common time grid using at least one of time interpolation, phase shifts based on a sine function, parametric fitting, and a 2π -shift of a sine function.

19. The method as recited in claim 17, wherein step (b) includes acquiring motion data using multiple detection zones of the ultrasound transducer, and wherein step (c) includes at least one of correcting for time delays within each detection zone or correcting time delays across different detection zones.

20. The method as recited in claim 1, 12, or 17, wherein the ultrasound transducer is at least one of a single element transducer, a 1-dimensional array transducer, 1.5-dimensional array transducer, 1.75-dimensional array transducer, and 2-dimensional array transducer.

21. The method as recited in claim 1, 12, or 17, wherein acquiring the motion data includes performing a data acquisition over at least one of one, two, or three spatial dimensions.

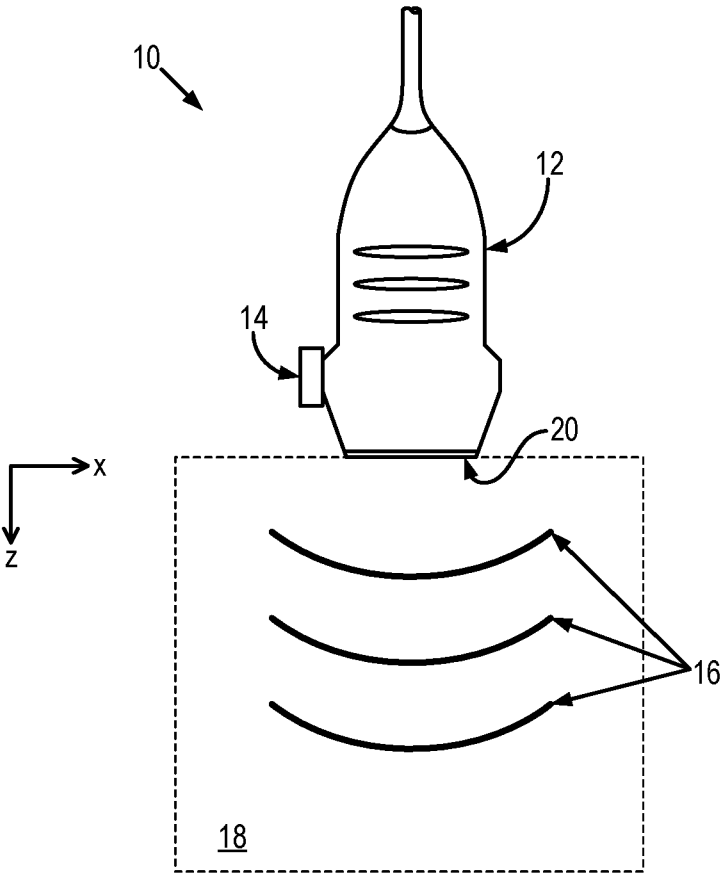


FIG. 1

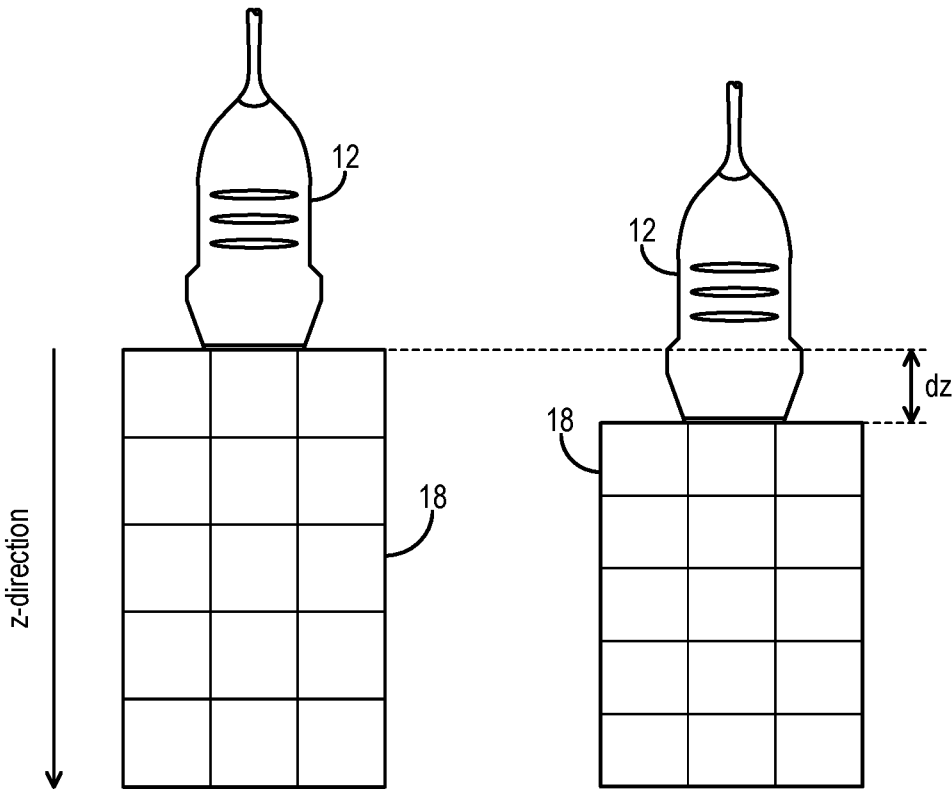


FIG. 2A

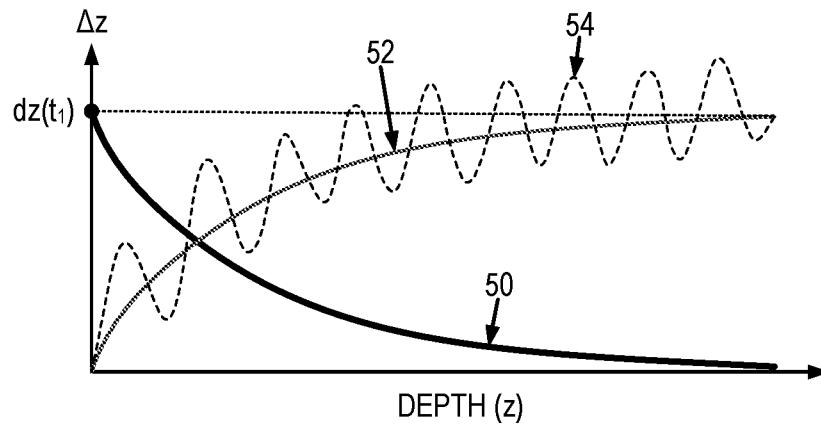


FIG. 2B

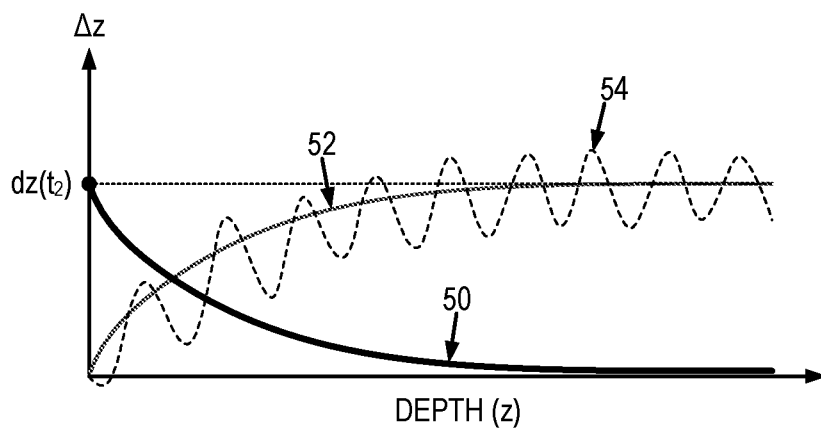


FIG. 2C

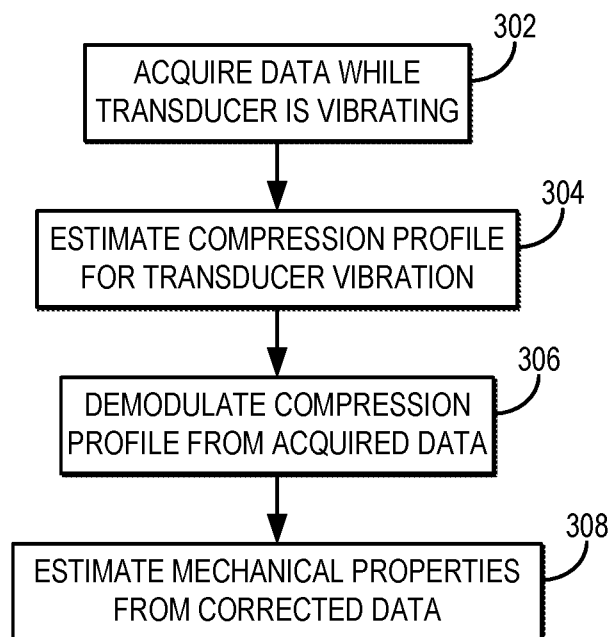


FIG. 3

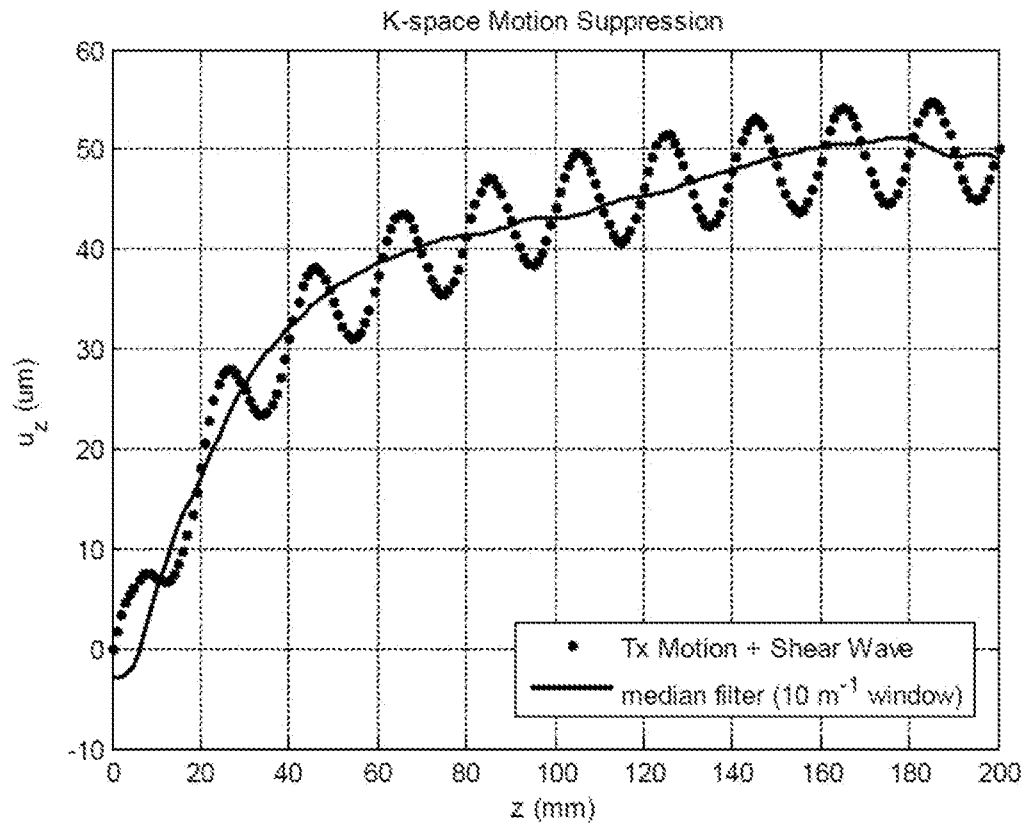


FIG. 4A

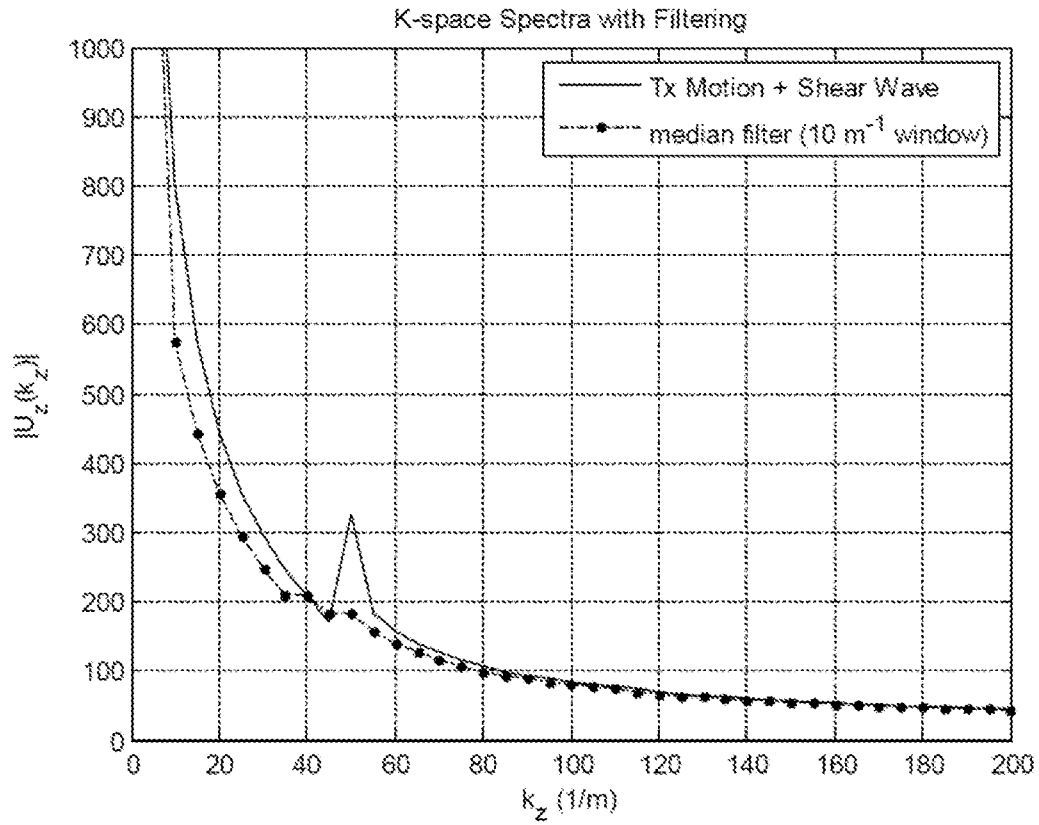


FIG. 4B

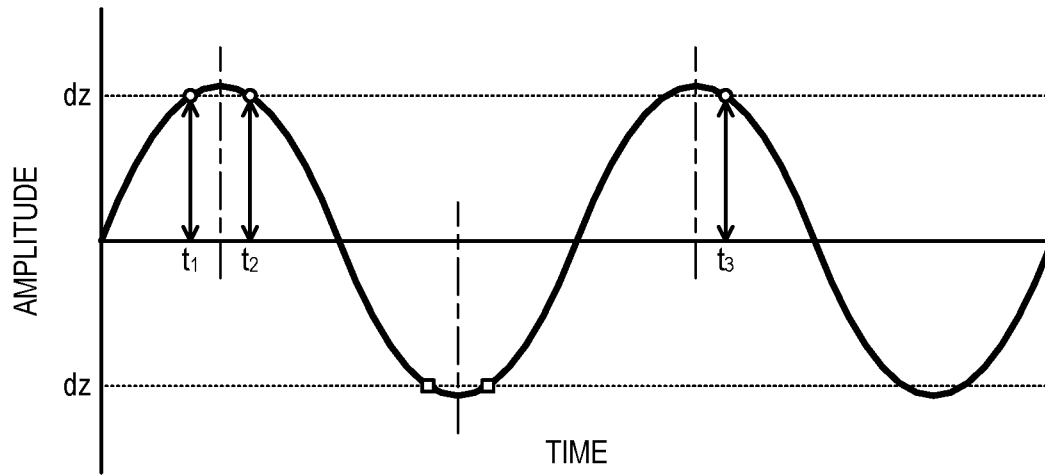


FIG. 5

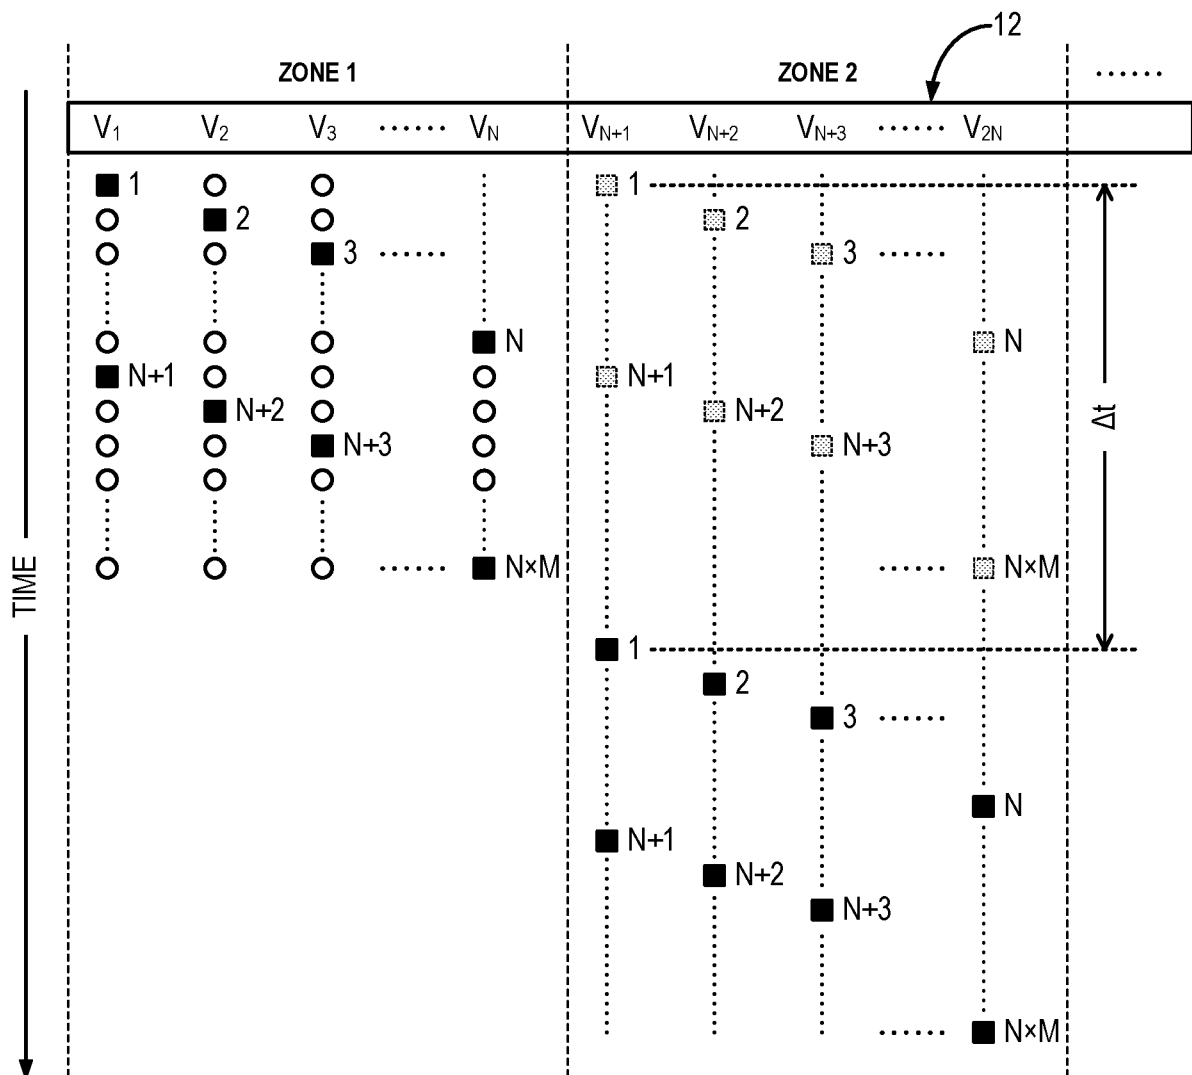


FIG. 6

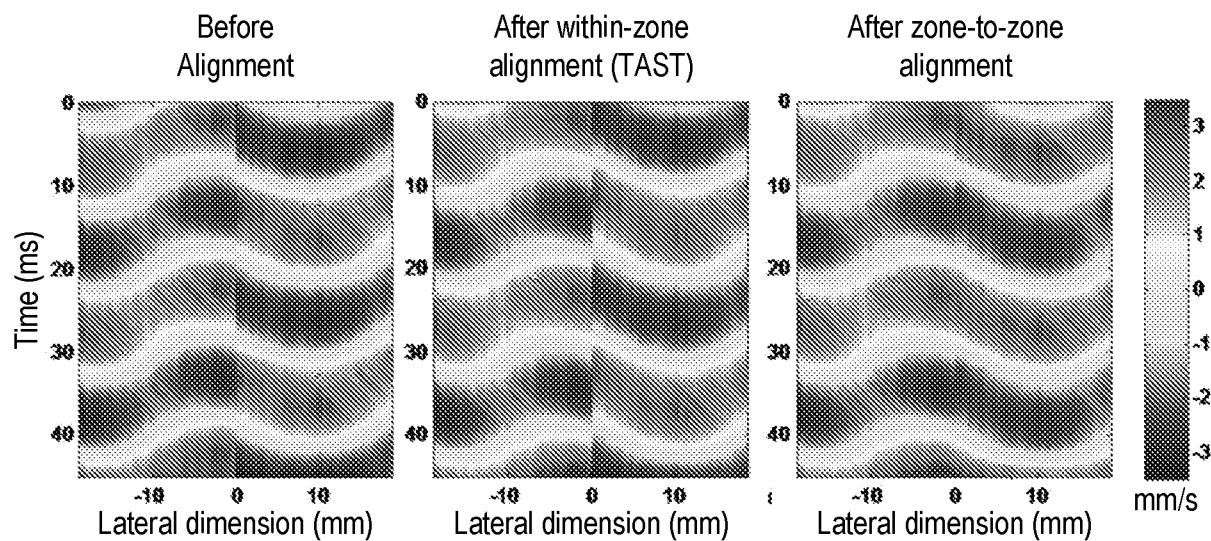


FIG. 7

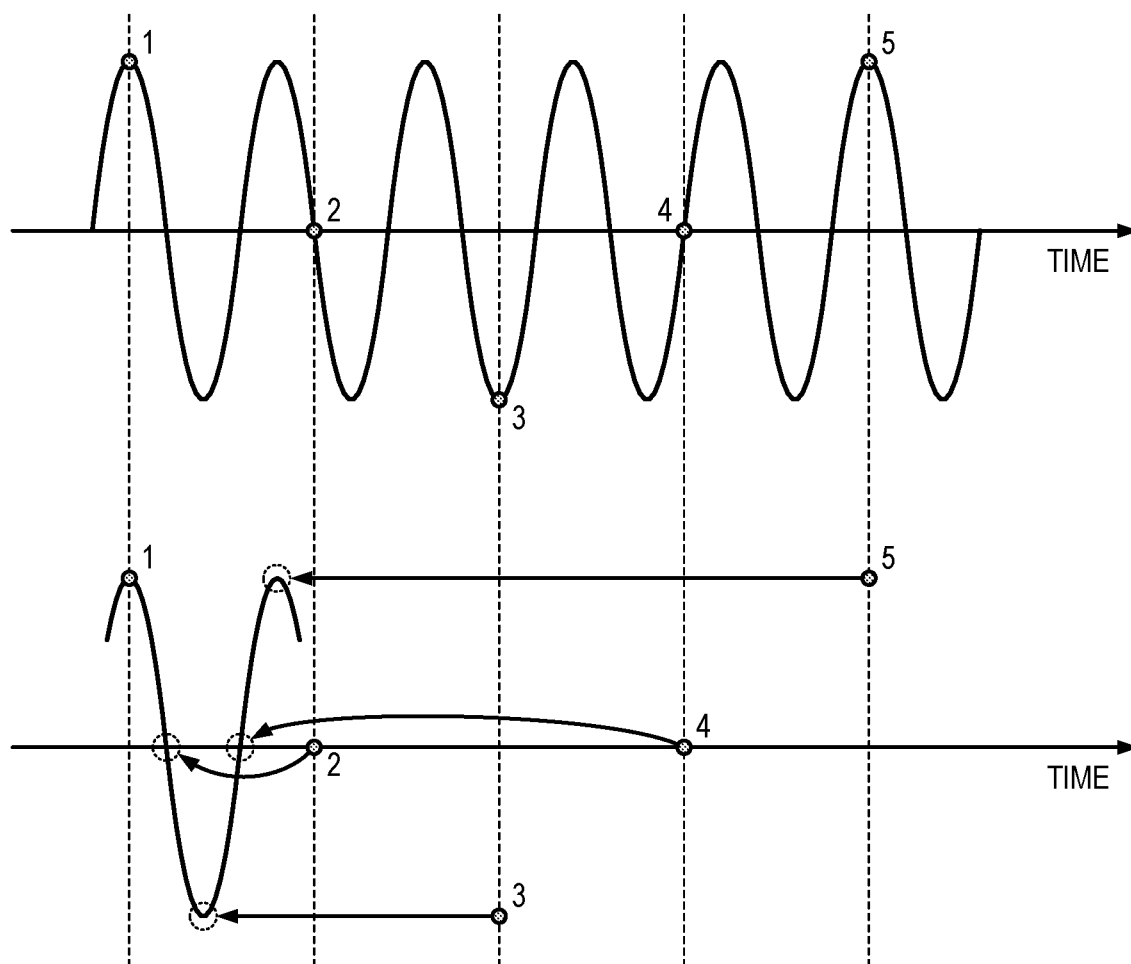


FIG. 8

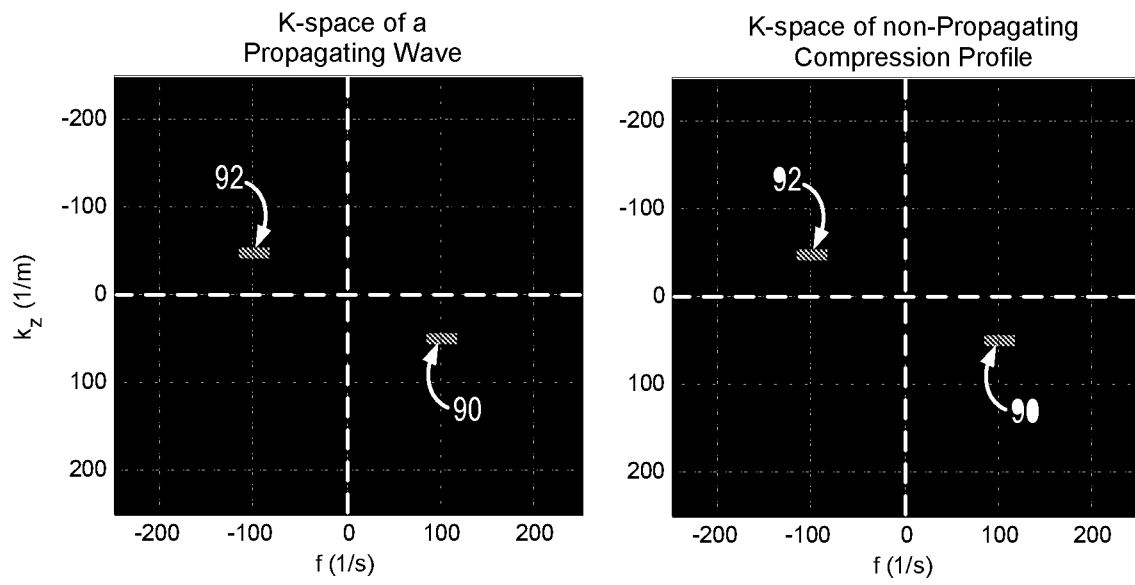


FIG. 9

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US 16/55649

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 8/00 (2016.01)

CPC - A61B 8/4444, A61B 8/485, G01S 7/52022

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8) - A61B 8/00 (2016.01)

CPC - A61B8/4444, A61B8/485, G01S7/52022

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
IPC(8) - A61B 8/00 (2016.01); CPC - A61B8/4444, A61B8/485, G01S7/52022, G01S7/52042, G01S7/52077, A61B8/5207; USPC - 600/438, 73/579

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

Electronic Database Searched: PatBase, Google Scholar/Patents

Search Terms Used: mechanical property, ultrasound/ultrasonic, transducer, compression, shear wave, deformation, motion, vibration, propagation

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y --- A	US 2012/0226158 A1 (Greenleaf et al.) 06 September 2012 (06.09.2012), entire document, especially para. [0011], [0023], [0024], [0040]	1, 6, 7-10, 12-18, 20, 21 ----- 2-5, 11, 19
Y --- A	US 2007/0093716 A1 (Radulescu) 26 April 2007 (26.04.2007), entire document, especially para. [0022], [0039], [0050]	1, 6, 7-10, 20/(1), 21/(1) ----- 2-5, 11
Y --- A	US 2005/0267695 A1 (German) 01 December 2005 (01.12.2005), entire document, especially para. [0078], [0503], [0510], [0511]	12-18, 20/(12,17), 21/(12,17) ----- 19
Y	US 2012/0215101 A1 (Maleke et al.) 23 August 2012 (23.08.2012), entire document, especially para. [0006], [0007], [0046], [0050]	8, 9
A	US 7,975,555 B2 (Zhuang et al.) 12 July 2011 (12.07.2011), entire document	1-21
A	US 2009/0182234 A1 (Perrey et al.) 16 July 2009 (16.07.2009), entire document	1-21

☐ Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

07 December 2016

Date of mailing of the international search report

25 JAN 2017

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774

专利名称(译)	具有连续换能器振动的超声弹性成像系统和方法		
公开(公告)号	EP3359047A4	公开(公告)日	2019-10-09
申请号	EP2016854283	申请日	2016-10-06
[标]申请(专利权)人(译)	梅约医学教育与研究基金会		
申请(专利权)人(译)	梅奥基金会的医学教育和研究		
当前申请(专利权)人(译)	Mayo医学教育与研究基金会		
[标]发明人	MELLEMA DANIEL C SONG PENGFEI URBAN MATTHEW W MANDUCA ARMANDO GREENLEAF JAMES F CHEN SHIGAO		
发明人	MELLEMA, DANIEL C. SONG, PENGFEI URBAN, MATTHEW W. MANDUCA, ARMANDO GREENLEAF, JAMES F. CHEN, SHIGAO		
IPC分类号	A61B8/00		
优先权	62/238891 2015-10-08 US		
其他公开文献	EP3359047A1		
外部链接	Espacenet		

摘要(译)

提供了用于处理使用超声弹性成像获取的数据的系统和方法，其中使用超声换能器的连续振动在对象中产生切波。此处描述的系统和方法可以有效地消除与超声换能器的振动相关的运动伪像，并且还可以消除在使用逐行成像模式获取数据时引起的数据采样未对准，就像许多常规超声所做的那样扫描仪。因此，这里描述的系统和方法提供了用于换能器运动校正和用于对准由逐行扫描超声系统检测到的运动信号的技术。