



(11) **EP 1 621 897 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
01.02.2006 Bulletin 2006/05

(51) Int Cl.:
G01S 7/52 (2006.01) A61B 8/00 (2006.01)
G10K 11/34 (2006.01)

(21) Application number: **04017837.8**

(22) Date of filing: **28.07.2004**

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PL PT RO SE SI SK TR
Designated Extension States:
AL HR LT LV MK

(71) Applicant: **MEDISON CO., LTD.**
Kangwon-do 250-870 (KR)

(72) Inventors:
• **An Kim, Cheol**
Guseong-eup
Yongin-si
Gyeonggi-do449-939 (KR)


• **Gye, Sang Bum**
Seoul 138-916 (KR)
• **The other inventors have agreed to waive their entitlement to designation.**

(74) Representative: **Schmid, Wolfgang**
Lorenz & Kollegen
Patent- und Rechtsanwaltskanzlei
Alte Ulmer Strasse 2
D-89522 Heidenheim (DE)

(54) **Ultrasound imaging apparatus having a function of selecting transmit focal points and method thereof**

(57) The present invention relates to an ultrasound imaging apparatus having a function of selecting transmit focal points and method thereof, in which an operator may select at least one transmit focal point, allowing for transmit-focusing ultrasound signals upon the selected focal point to create an ultrasound image of a target object. The ultrasound imaging apparatus includes an ultrasound transducer array, a pulse generator, a controller, a database, an input device, an analog-to-digital converter (ADC), a beam former, a signal processor, and a display device. The method for ultrasound imaging comprises the steps of: a) transmitting to a target object ultrasound signals in accordance with a predetermined initial time-delay profile; b) receiving and processing the reflected ultrasound signals from the target object to create an ultrasound image of the target object; c) displaying the created ultrasound image to allow an operator to select at least one region of interest within the displayed ultrasound image; d) in response to the operator's selection, detecting coordinates of the selected region of interest; e) determining at least one transmit focal point corresponding to the detected coordinates of the selected region of interest; f) determining at least one new time-delay profile based on each of the transmit focal points; and g) transmitting the ultrasound signals in accordance with the new time-delay profile to the target object; h) receiving and processing the reflected ultrasound signals off the target object to create an updated ultrasound image of the target object.

Fig. 4

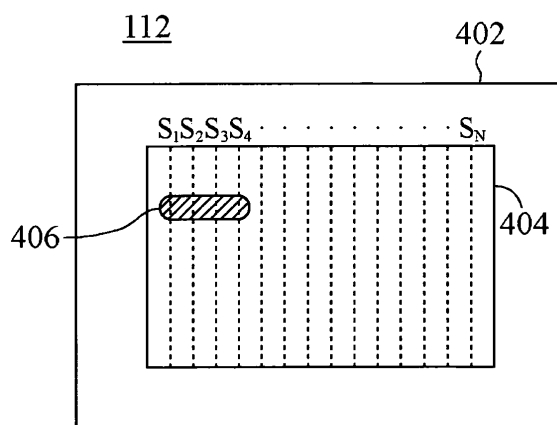

Description

[0001] The present invention relates to the field of ultrasound imaging, and more particularly, to an ultrasound imaging apparatus having a function of selecting transmit focal points and method thereof, in which an operator may select at least one transmit focal point.

[0002] In a diagnostic ultrasound system, "ultrasound-focusing" has to be performed for detailed observation of a desired part of an ultrasound image. This ultrasound-focusing involves "transmit-focusing," which is to be performed while the ultrasound signals are transmitted to a target object, and "receive-focusing," which is to be performed while the reflected ultrasound signals from the target object are received. The receive-focusing, which is to focus the ultrasound signals for all the pixels on a screen where the ultrasound image is to be displayed, has been widely used in the art of the present invention.

[0003] Unlike the receive-focusing, transmit-focusing, however, cannot be performed for each point on the target object corresponding to each of all the pixels on the screen where the ultrasound image is to be displayed, and is usually performed only for the transmit focal points predetermined by a manufacturer of the diagnostic ultrasound system. Accordingly, when an operator wants to choose particular transmit focal points on the target object, he may select transmit focal points, which are adjacent to the desired points, among the several predetermined transmit focal points via a switch or button on a input device in the diagnostic ultrasound system. Thus, in a conventional diagnostic ultrasound system, the problem is that the operator cannot transmit-focus the ultrasound signals exactly upon the desired points on the target object.

[0004] Referring to Fig. 3, which illustrates an example of a conventional input interface for transmit focal points, the conventional diagnostic ultrasound system has input interface 302 for transmit focal points, which enables the operator to input the transmit focal points, as shown in Fig. 3. Although scan-lines 308 shown in Fig. 3 are not actually displayed on display region 304 for the ultrasound image, they are shown to illustratively represent the relationship between the scan-lines and the transmit focal points to be displayed in region 304. As is well known, in order to create an ultrasound image, scan conversion of the ultrasound image data obtained on scan-lines 308 in Fig. 3 must be performed to convert it into data that can be displayed on the corresponding pixel within display region 304. Since this scan conversion process would be readily understood by those skilled in the art, we omit detailed description of this for the convenience of description herein.

[0005] While the operator observes the ultrasound image being currently displayed on display region 304, he may select the predetermined transmit-focal points, e.g., such as the points on the intersection between scan-lines 308 and transmit-focusing lines 312 or 314, which are

adjacent to the desired point for ultrasound transmit-focusing. Then, the ultrasound image may be obtained by transmit-focusing the ultrasound signals upon the selected transmit focal points. As shown in Fig. 3, however, the conventional diagnostic ultrasound system cannot provide the function of selecting transmit focal points only in the region of interest within the ultrasound image, which is being observed by the operator. So the operator has no choice but to select the predetermined transmit focal points on every scan-line 308 of the ultrasound image. Accordingly, in the conventional diagnostic ultrasound system, the frame rate of the ultrasound image may be reduced because the ultrasound signals are transmit-focused on every point on the intersection between scan-lines 308 and the transmit-focusing line selected by an operator.

[0006] Therefore, a need exists for an apparatus and method for creating an ultrasound image by transmit-focusing the ultrasound signals only upon the transmit focal points selected by the operator while observing the ultrasound image of the target object currently being displayed, to improve signal processing rate and thus obtain a high frame rate of the ultrasound image.

[0007] It is, therefore, an object of the present invention to provide an ultrasound imaging apparatus having a function of selecting transmit focal points and method thereof, in which an operator may select at least one transmit focal point while observing an ultrasound image of a target object being currently displayed, allowing for transmit-focusing ultrasound signals only upon the selected transmit focal point in order to create an ultrasound image at a high frame rate.

In accordance with one aspect of the present invention, an ultrasound imaging apparatus is provided, which comprises: means for storing a plurality of time-delay profiles; means for selecting one of the stored plurality of time-delay profiles; means for generating a plurality of pulse signals according to the selected time-delay profile; means for producing, transmitting ultrasound signals corresponding to each of the plurality of pulse signals to a target object, and receiving the ultrasound signal reflected from the target object; means for processing the reflected ultrasound signals to create an ultrasound image of the target object; and means for displaying the created ultrasound image to allow an operator to select at least one region of interest within the displayed ultrasound image, and in response to the operator's selection, detecting coordinates of the selected region of interest, wherein the means for selecting determines at least one transmit focal point corresponding to the detected coordinates of the selected region of interest, and selects at least one new time-delay profile among the stored plurality of time-delay profiles based on each of the transmit focal points.

[0008] In accordance with another aspect of the present invention, a method for ultrasound imaging is provided, wherein the method comprises the steps of: a) transmitting to a target object ultrasound signals in ac-

c) displaying the created ultrasound image to allow an operator to select at least one region of interest within the displayed ultrasound image; d) in response to the operator's selection, detecting coordinates of the selected region of interest; e) determining at least one transmit focal point corresponding to the detected coordinates of the selected region of interest; f) determining at least one new time-delay profile based on each of the transmit focal points; and g) transmitting the ultrasound signals in accordance with the new time-delay profile to the target object; h) receiving and processing the reflected ultrasound signals from the target object to create an updated ultrasound image of the target object.

[0009] The above and other objects and features in accordance with the present invention will become apparent from the following descriptions of preferred embodiments given in conjunction with the accompanying drawings, in which:

Fig. 1 is a schematic block diagram of an apparatus for creating an ultrasound image by transmit-focusing ultrasound signals upon at least one transmit focal point selected by an operator according to the present invention.

Fig. 2 is a flow diagram illustrating a method for creating the ultrasound image by transmit-focusing the ultrasound signals upon at least one transmit focal point selected by the operator according to the present invention

Fig. 3 illustrates an example of an input interface for use in inputting the transmit focal points, which is provided in a conventional ultrasound imaging system.

Fig. 4 illustrates an example of a selection interface for use in selecting the transmit focal points, which is provided in the input device shown in Fig. 1.

[0010] Referring to Fig. 1, a schematic block diagram of an ultrasound imaging apparatus allowing selection of transmit focal points is illustrated according to the present invention. As shown in Fig. 1, ultrasound imaging apparatus 100 includes ultrasound transducer array 102, pulse generator 106, controller 108, database 110, input device 112, analog-to-digital converter (ADC) 114, beam former 116, signal processor 118, display device 120, and further includes cables 104 that couples ultrasound transducer array 102 to pulse generator 106 and ADC 114. According to the present invention, selecting a region of interest within an ultrasound image, which is currently being observed by an operator, is essentially the same as selecting a transmit focal point where ultrasound signals are to be transmit-focused. In this context, it should be appreciated and interpreted that the terms "selection of a region of interest" and "selection of a transmit focal point" have substantially the same meanings in the

description below.

[0011] Input device 112 enables the operator to select the region of interest within the ultrasound image of a target object, which was created and is being currently displayed by ultrasound imaging apparatus 100, and detects the selected region of interest. Input device 112, for example, provides a selection interface for the transmit focal points, such as shown in Fig. 4. The operator may select region of interest 406 using his finger or a separate selection tool (e.g., a stylus), while observing the ultrasound image being currently displayed. Input device 112 may be implemented by a normal touch screen to allow the operator to select the region of interest just by touching a desired point within the ultrasound image with his finger or a stylus, as described above. Then, input device 112 detects the location of selected region of interest 406 within region 404. Because the procedure for detecting the location at input device 112 is apparent to those skilled in the art, the description thereof will be omitted. It should be appreciated that a plurality of regions of interest may be provided, even though only one region of interest 406 is shown in Fig. 4, which is merely illustrative. Further, although a plurality of scan-lines S_1 - S_n are illustrated in region 404 of selection interface 402 for transmit focal points, these are shown merely for the convenience of description, as mentioned above with reference to Fig. 3.

[0012] Referring again to Fig. 1, controller 108 is coupled to input device 112, database 110, and signal processor 118, and determines the scan-lines, which are included within region of interest 406 selected by the operator via input device 112 (refer to Fig. 4), and the transmit focal points on the scan-lines. As shown in Fig. 5, if controller 108 determines that scan-lines S_1 - S_4 are included within selected region of interest 406 based on the information on the scan-lines transmitted from signal processor 118, it then selects transmit focal points P_1 - P_8 on scan-lines S_1 - S_4 . In this case, scan-lines S_5 - S_n are not subject to selection since they are not included within selected region of interest 406. Although the number of the transmit focal points on each of the scan-lines is fixed to two (2) herein for the purpose of illustration, the number may be changed in consideration of the frame rate of an ultrasound image to be obtained.

[0013] Next, controller 108 determines time-delay profiles, each of which corresponds to each of determined transmit focal points P_1 - P_8 , respectively. At that time, controller 108 may retrieve the time-delay profiles from database 110, which stores the corresponding time-delay profiles for all transmit focal points selectable within the ultrasound image being currently observed by the operator, and provide them to pulse generator 106. It will be readily understood by those skilled in the art that if the controller operates at a high speed, then the controller may directly calculate the time-delay profiles corresponding to each of determined transmit focal points P_1 - P_8 , respectively, without using the time-delay profiles already stored in database 110.

[0014] Based on the time-delay profiles provided from controller 108, pulse generator 106 generates pulses to produce ultrasound signals according to each of the time-delay profiles, and then transmits them to transducer array 102.

[0015] Transducer array 102 is coupled to pulse generator 106 through cable 104, and produces the ultrasound signals according to the determined time-delay profiles, in response to the pulses transmitted from pulse generator 106. Then, transducer array 102 transmit-focuses and transmits the ultrasound signals.

[0016] The ultrasound signals reflected from the target object are received at transducer array 102, formed into an ultrasound image of the target object via ADC 114, beam former 116, and signal processor 118, and then displayed in display device 120, as is well known. At that time, signal processor 118 performs scan conversion to convert the ultrasound image into a suitable format for displaying the image on display device 120, and transmit the information acquired during the scan conversion process to controller 198 so that controller 108 may determine the scan-lines included within the region of interest.

[0017] Signal processor 118 may process the reflected ultrasound signals sequentially, which correspond to each of scan-lines S_1 - S_4 respectively, wherein scan-lines S_1 - S_4 include determined transmit focal points P_1 - P_8 . Alternatively, signal processor 118 may process the reflected ultrasound signals in a "scan-line interleaving" mode in order to increase the frame rate of the ultrasound image to be created. Specifically, in order to generate one frame of the image data, signal processor 118 first processes the reflected ultrasound signals corresponding to the transmit focal points on scan-lines S_1 and S_3 , and then processes the reflected ultrasound signals corresponding to the transmit focal points on scan-lines S_2 and S_4 . Then, by combining the output produced as a result of both of the above processes to organize one full frame image data, signal processor 118 can create the ultrasound image without reducing the overall frame rate. Alternatively, signal processor 118 may create the ultrasound image in a "transmit-focal point interleaving" mode. In this mode, the reflected ultrasound signals are processed such that the reflected ultrasound signals, for example, corresponding to transmit focal points P_1 , P_3 , P_5 , and P_7 are processed sequentially at first, and then the reflected ultrasound signals corresponding to transmit focal points P_2 , P_4 , P_6 , and P_8 are processed sequentially thereafter. According to the process in this mode, the necessity of processing all the reflected ultrasound signals corresponding to the transmit focal points on each of the scan-lines sequentially may be eliminated.

[0018] Although input device 112 and display device 120 are illustrated separately herein as shown in Fig. 1, it will be readily understood by those skilled in the art that these may be constructed as one unit.

[0019] Referring to Fig. 2, a flow diagram is shown

which illustrates a method for creating an ultrasound image by transmit-focusing the ultrasound signals on the transmit focal points selected by the operator according to the present invention. First, in step S202, the ultrasound image is displayed on display device 120 and region 404 of input display 112, which is created using the ultrasound signals that are produced according to an initial predetermined time-delay profile selected by controller 108 from among a plurality of time-delay profiles stored in database 110. In step S204, input device 112 detects region of interest 406 selected by the operator via selection interface 402 for use in selecting transmit focal points such as shown in Fig. 4.

[0020] In step S206, input device 112 determines whether the operator selects another region of interest. If so, then the process returns to step S204. On the other hand, if it is determined that the operator does not select another region of interest, or if it is determined that the selection process of the region of interest is completed, the process proceeds to step S208.

[0021] In step S208, controller 108 determines scan-lines included within the selected region of interest and at least one transmit focal point on the respective scan-lines based on information on scan-lines transmitted from signal processor 118 and information on the selected region transmitted from input device 112. As described above, the information on the selected region of interest include coordinates of the selected region of interest within region 404, and the information on scan-lines represent a relationship between pixels in region 404 and the scan-lines, which may be acquired during the scan conversion process at signal processor 118.

[0022] In step S210, controller 108 selects at least one new time-delay profile from among the plurality of time-delay profiles stored in database 110 in order to transmit-focus the ultrasound signals on the selected transmit focal point. Alternatively, controller 108 may directly calculate the new time-delay profile directly, as described above.

[0023] In step S212, controller 108 provides the new time-delay profile, which may be selected or calculated as mentioned above, to pulse generator 106. Pulse generator 106 generates pulses to produce the ultrasound signals according to the time-delay profile, and then transmits them to transducer array 102 via cable 104. Transducer array 102 produces the ultrasound signals according to the new time-delay profile, in response to the pulses transmitted from pulse generator 106 and transmit them to the target object.

[0024] In step S214, ADC 114 receives the ultrasound signals, which are reflected from the target object, from transducer array 102 via cable 104. The reflected ultrasound signals are then transmitted to signal processor 118 via ADC 114 and beam former 116. Signal processor 118 creates an updated ultrasound image by processing the reflected ultrasound signals. At that time, signal processor 118 may process the reflected ultrasound signals in the "scan-line interleaving" mode, or alternatively, in

the "transmit focal point interleaving" mode in order to increase the frame rate of the ultrasound image to be created, as described above.

[0025] As mentioned above, according to the present invention, the operator may select any transmit focal points within the region of interest, while observing the ultrasound image currently displayed, and obtain the transmit-focused ultrasound image without reducing the overall frame rate of the image of the target object. This is achieved by transmit-focusing the ultrasound signals only upon the transmit focal points on each scan-line that the operator selected.

[0026] While the present invention has been shown and described with respect to a preferred embodiment, those skilled in the art will recognize that various changes and modifications may be made without departing from the scope of the invention as defined in the appended claims.

Claims

1. An ultrasound imaging apparatus, which allows selection of transmit focal points, the apparatus comprising:

means for storing a plurality of time-delay profiles;
 means for selecting one of the stored plurality of time-delay profiles;
 means for generating a plurality of pulse signals according to the selected time-delay profile;
 means for producing and transmitting ultrasound signals corresponding to each of the plurality of pulse signals to a target object, and receiving the ultrasound signal reflected from the target object;
 means for processing the reflected ultrasound signals to create an ultrasound image of the target object; and
 means for displaying the created ultrasound image to allow selection of at least one region of interest within the displayed ultrasound image, and detecting coordinates of the selected region of interest,

wherein the means for selecting determines at least one transmit focal point corresponding to the detected coordinates of the selected region of interest, and selects at least one new time-delay profile from among the stored plurality of time-delay profiles based on each of the transmit focal points.

2. The apparatus of Claim 1, wherein the means for processing include a scan conversion portion to convert the ultrasound image into a format for displaying in the display region, and wherein the scan conversion portion provides information on the scan-lines

to the means for selecting, which is obtained during the conversion of the format of the ultrasound image.

3. The apparatus of Claim 1, wherein the means for detecting includes a touch screen.
4. The apparatus of Claim 1, wherein the means for processing processes the reflected ultrasound signals either in a scan-line interleaving mode or in a transmit focal point interleaving mode to create an updated ultrasound image.
5. The apparatus of Claim 1, wherein the means for detecting includes a separate display device for displaying the ultrasound image and the updated ultrasound image.
6. The apparatus of Claim 1, wherein the means for selecting builds the new time-delay profile.
7. A method for ultrasound imaging, comprising the steps of:

a) transmitting to a target object ultrasound signals in accordance with a predetermined initial time-delay profile;
 b) receiving and processing the reflected ultrasound signals from the target object to create an ultrasound image of the target object;
 c) displaying the created ultrasound image to allow selection of at least one region of interest within the displayed ultrasound image;
 d) detecting coordinates of the selected region of interest;
 e) determining at least one transmit focal point corresponding to the detected coordinates of the selected region of interest;
 f) determining at least one new time-delay profile based on each of the transmit focal points; and
 g) transmitting the ultrasound signals in accordance with the new time-delay profile to the target object;
 h) receiving and processing the reflected ultrasound signals from the target object to create an updated ultrasound image of the target object.

8. The method of Claim 7, wherein the step (h) processes the reflected ultrasound signal either in a scan-line interleaving mode or in a transmit focal point interleaving mode to create the updated ultrasound image.

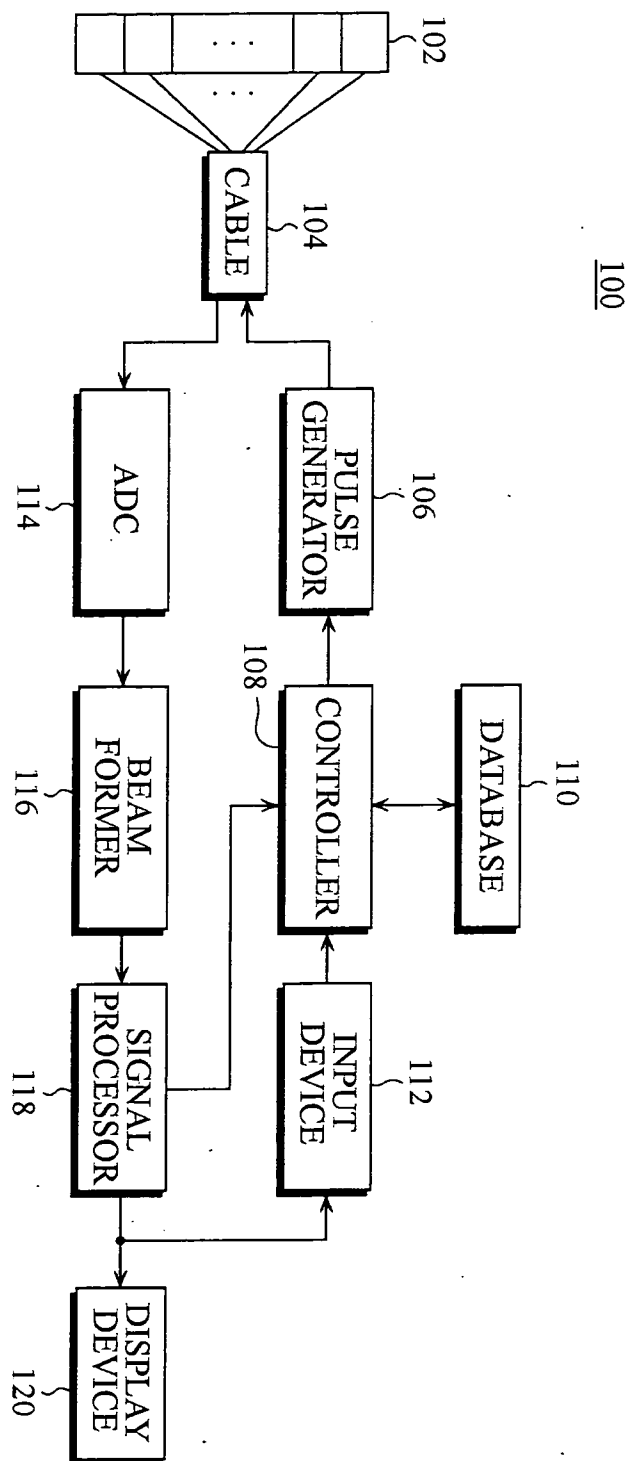


Fig. 1

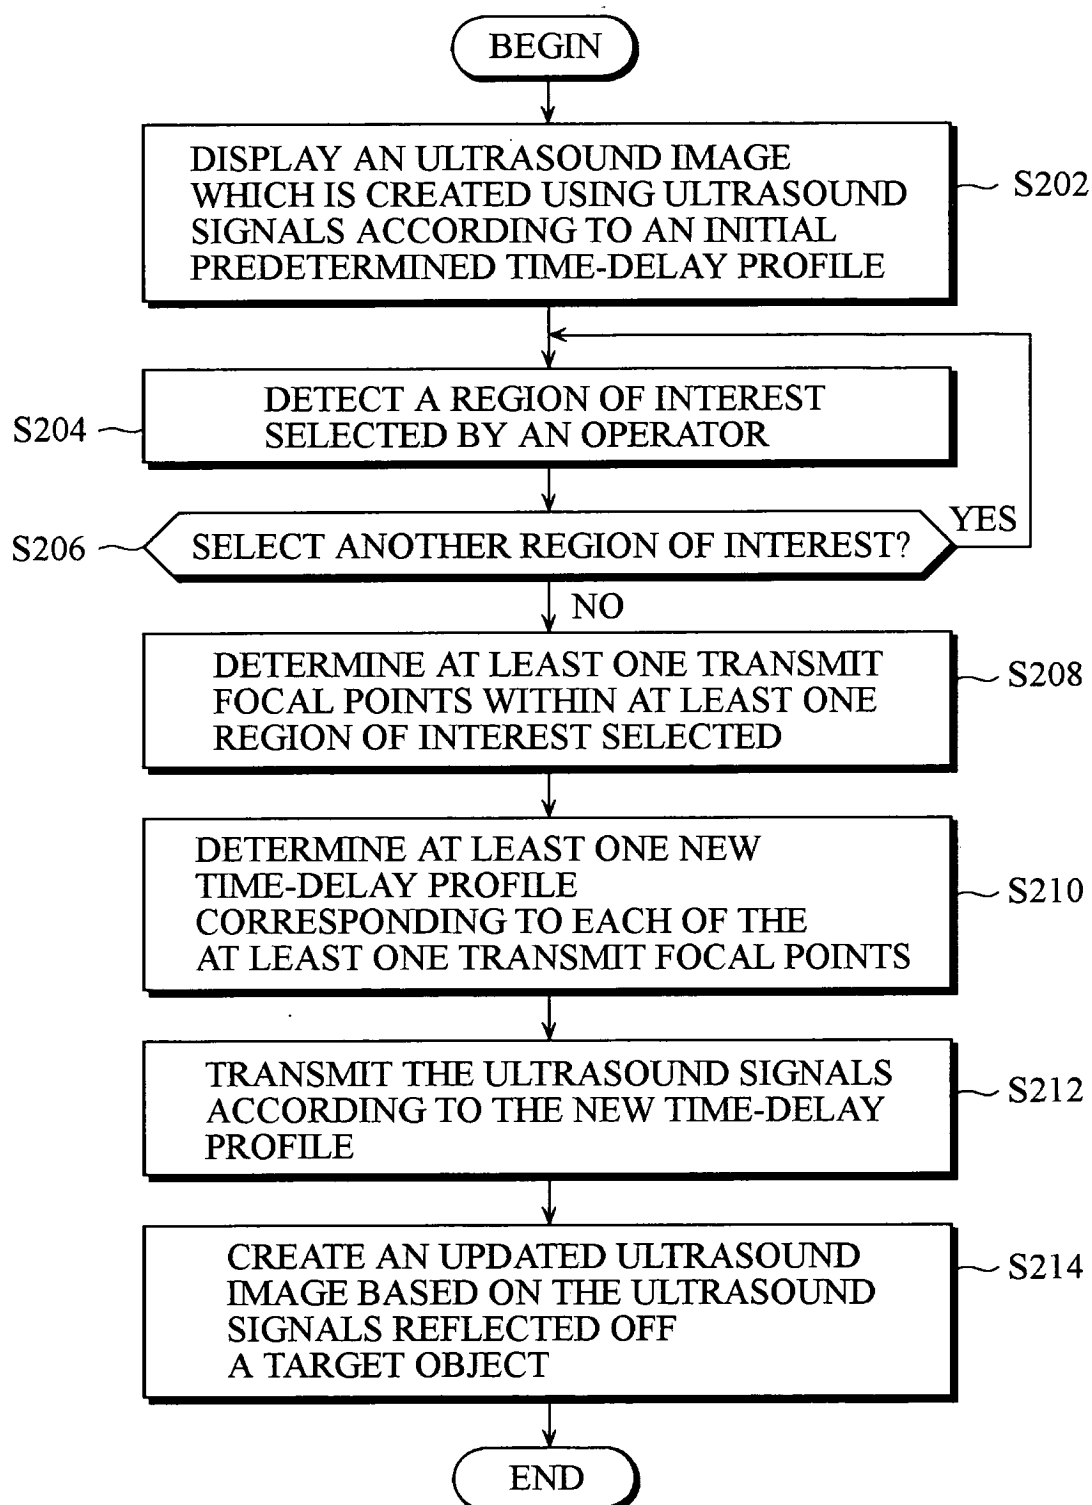
Fig. 2

Fig. 3

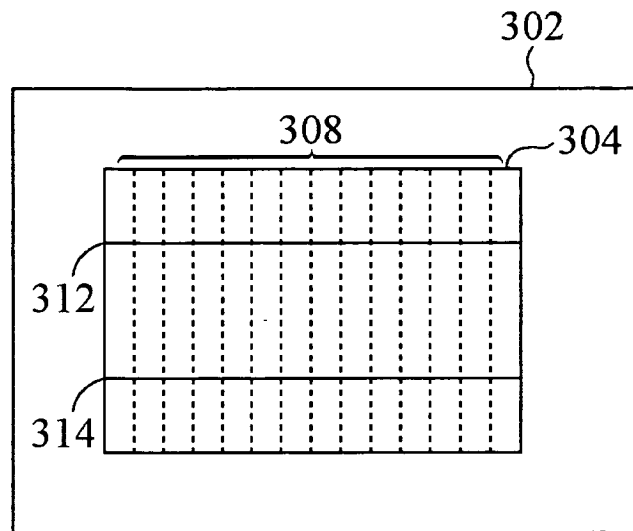


Fig. 4


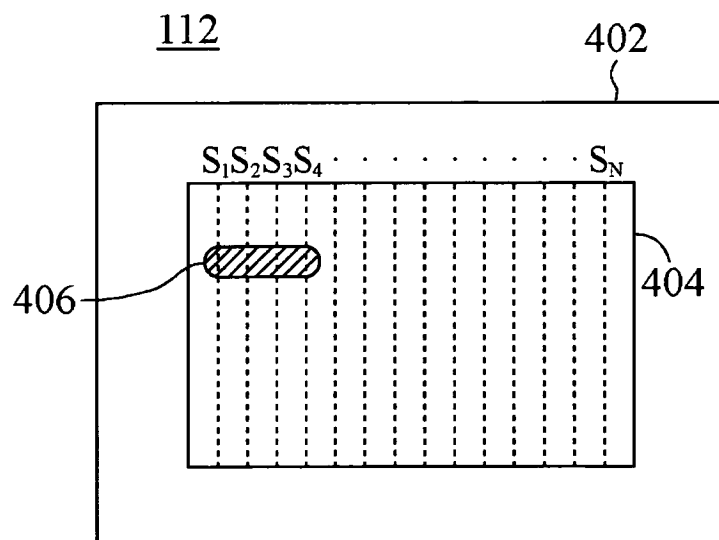


Fig. 5

406



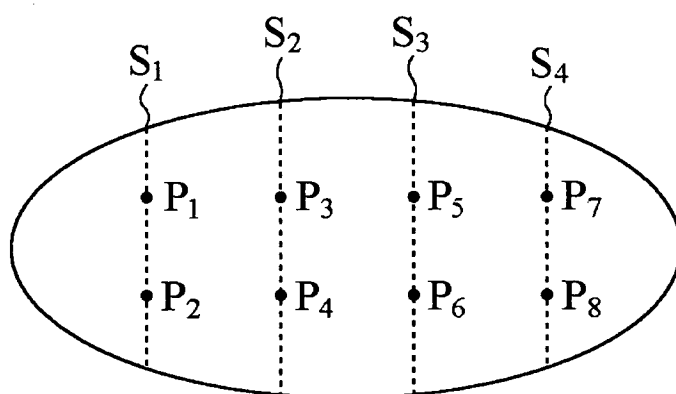

European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 04 01 7837

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
X	US 6 544 179 B1 (OLSSON LARS JONAS ET AL) 8 April 2003 (2003-04-08)	1-3,5-7	G01S7/52 A61B8/00 G10K11/34
Y	* column 1, line 29 - column 7, line 67; figures 1,4-6,8,10,11 *	4,8	
Y	----- US 6 315 723 B1 (COOLEY CLIFFORD R ET AL) 13 November 2001 (2001-11-13) * abstract * * column 9, line 28 - column 10, line 34; figures 2,11 *	4,8	
X	----- US 6 217 516 B1 (BROCK-FISHER GEORGE A ET AL) 17 April 2001 (2001-04-17) * column 2, line 49 - column 6, line 29; figures 1-4 *	1,2,5-7	
A	----- US 5 357 962 A (GREEN PHILIP S) 25 October 1994 (1994-10-25) * column 3, line 29 - column 6, line 63; figures 1,2 *	1,2,6,7	
A	----- US 5 072 735 A (OKAZAKI TAKAHISA ET AL) 17 December 1991 (1991-12-17) * column 3, line 60 - column 6, line 2; figures 1,3A,4A *	1,2,7	TECHNICAL FIELDS SEARCHED (Int.Cl.7) G01S A61B G10K
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 6 December 2004	Examiner Artikis, T
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

2
EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 04 01 7837

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

06-12-2004

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
US 6544179	B1	08-04-2003	EP	1458294 A1		22-09-2004
			WO	03051202 A1		26-06-2003

US 6315723	B1	13-11-2001	NONE			

US 6217516	B1	17-04-2001	NONE			

US 5357962	A	25-10-1994	CA	2128887 A1		05-08-1993
			EP	0624254 A1		17-11-1994
			JP	7503321 T		06-04-1995
			WO	9315415 A1		05-08-1993

US 5072735	A	17-12-1991	JP	2004351 A		09-01-1990
			JP	2604007 B2		23-04-1997
			JP	2004352 A		09-01-1990
			JP	1926923 C		25-04-1995
			JP	2004353 A		09-01-1990
			JP	6053122 B		20-07-1994
			JP	1926924 C		25-04-1995
			JP	2004354 A		09-01-1990
			JP	6053123 B		20-07-1994

专利名称(译)	具有选择发射焦点功能的超声成像设备及其方法		
公开(公告)号	EP1621897A1	公开(公告)日	2006-02-01
申请号	EP2004017837	申请日	2004-07-28
申请(专利权)人(译)	MEDISON CO. , LTD.		
当前申请(专利权)人(译)	MEDISON CO. , LTD.		
[标]发明人	AN KIM CHEOL GYE SANG BUM		
发明人	AN KIM, CHEOL GYE, SANG BUM		
IPC分类号	G01S7/52 A61B8/00 G10K11/34		
CPC分类号	A61B8/14 A61B8/461 A61B8/467 A61B8/469 G01S7/5202 G01S7/52046 G01S7/5206 G01S7/52071 G10K11/346		
优先权	10/901201 2004-07-29 US		
其他公开文献	EP1621897B1 EP1621897A8		
外部链接	Espacenet		

摘要(译)

本发明涉及一种具有选择发送焦点的功能的超声成像设备及其方法，其中操作者可以选择至少一个发送焦点，允许在所选择的焦点上发送聚焦超声信号以产生超声图像。超声成像设备包括超声换能器阵列，脉冲发生器，控制器，数据库，输入装置，模数转换器（ADC），波束形成器，信号处理器和显示装置。用于超声成像的方法包括以下步骤：a）根据预定的初始时间延迟分布向目标对象发送超声信号；b）接收并处理来自目标对象的反射的超声信号，以创建目标对象的超声图像；c）显示所创建的超声图像以允许操作者选择所显示的超声图像内的至少一个感兴趣区域；d）响应于操作者的选择，检测所选择的感兴趣区域的坐标；e）确定与所选择的感兴趣区域的检测到的坐标相对应的至少一个发射焦点；f）基于每个所述发送焦点确定至少一个新的时间延迟分布；以及g）根据所述新的时间延迟分布向所述目标对象发射所述超声波信号；h）接收和处理离开目标对象的反射的超声信号，以创建目标对象的更新的超声图像。

Fig. 4

