

(19)



(11)

EP 2 870 917 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
28.06.2017 Bulletin 2017/26

(51) Int Cl.:
A61B 8/00 (2006.01)

(21) Application number: **14157985.4**

(22) Date of filing: **06.03.2014**

(54) **Support apparatus of ultrasound probe, handsfree ultrasound probe including the support apparatus, and method of operating the support apparatus**

Trägervorrichtung für Ultraschallsonde, freihändige Ultraschallsonde mit der Trägervorrichtung und Verfahren zum Betrieb der Trägervorrichtung

Appareil de support de sonde à ultrasons, sonde à ultrasons mains libres comprenant ledit appareil et procédé de fonctionnement de ce dernier

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **06.11.2013 KR 20130134355**

(43) Date of publication of application:
13.05.2015 Bulletin 2015/20

(73) Proprietor: **Samsung Medison Co., Ltd.
Gangwon-do 250-870 (KR)**

(72) Inventors:
• **Yoon, Jeong-un
Gangwon-do (KR)**

- **Jo, Jae-moon
Gangwon-do (KR)**
- **Kim, Jong-sik
Gangwon-do (KR)**
- **Jin, Gil-ju
Gangwon-do (KR)**

(74) Representative: **Lorenz, Markus
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft mbB
Alte Ulmer Straße 2
89522 Heidenheim (DE)**

(56) References cited:
**JP-A- 2006 230 913 JP-A- 2008 061 894
US-A1- 2004 087 851 US-A1- 2010 174 189
US-A1- 2012 296 216**

EP 2 870 917 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND

1. Field

[0001] One or more embodiments of the present invention relate to a support apparatus of an ultrasound probe, a handsfree ultrasound probe including the support apparatus, and a method of operating the support apparatus.

2. Description of the Related Art

[0002] An ultrasound apparatus, a magnetic resonance imaging (MRI) apparatus, a computed tomography (CT) apparatus, an X-ray apparatus, etc. may be used as medical devices for obtaining a medical image of a body. By reason of a resolution of the medical image or a size of the medical device, these apparatuses may photograph a part of the body or an overall part of the body. The overall part of the body may be photographed at a time or the part of the body may be photographed in several times and then photographed images may be combined into one image to obtain a combined image of the whole part of the body.

[0003] An ultrasound diagnosis apparatus includes an ultrasound probe that transmits and receives ultrasound, a signal processing apparatus that performs signal processing on the received ultrasound, and a display apparatus that displays an ultrasound image.

[0004] The ultrasound probe that a user who is a doctor is holding by his/her hand contacts a target object such as a patient body, transmits ultrasound to the target object, and receives an echo signal of the ultrasound. However, although a user needs to fix the ultrasound probe to the target object when more closely diagnosing a specific part of the target object, it is difficult to fix the ultrasound probe more than a predetermined period of time due to a weight of the ultrasound probe.

[0005] In the JP 2008 061894 an ultrasonic probe system is equipped with an ultrasonic probe, a probe adapter having a suction port, and a suction apparatus. The suction port is installed on the periphery of the ultrasonic wave transmitting/receiving surface of the ultrasonic probe. By sucking the mamma or air in a vicinity of the mamma from the suction port, the contact property between the ultrasonic wave transmitting/receiving surface and the mamma is made better.

[0006] The JP 2006 230913 A discloses a probe being stuck to the body surface of a subject with a sticking device. The sticking device is provided with a sucker member, a storage body and a pump. The sucker member has an approximate plate shape and adsorbed to the body surface of the subject by changing the pressure in its inside. The storage body is fixed to the inside of the sucker member and exposes a transmitting/receiving surface of the ultrasonic wave of the probe to store the

probe. The pump is detachably attached to a check valve of the sucker member and sucks the air inside the sucker member as necessary. The sucking member is adsorbed to the body surface by being sucked the air so that the probe retained inside the sucker member is stuck to the body surface.

SUMMARY

[0007] One or more embodiments of the present invention include a support apparatus of an ultrasound probe that a user may not hold by his/her hand during a diagnosis, a handsfree ultrasound probe including the support apparatus, and a method of operating the support apparatus.

[0008] One or more embodiments of the present invention include a support apparatus of an ultrasound probe capable of remotely controlling a movement of the ultrasound probe, a handsfree ultrasound probe including the support apparatus, and a method of operating the support apparatus.

[0009] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0010] According to one or more embodiments of the present invention, a support apparatus of an ultrasonic probe is provided in claim 1, the support apparatus including: a housing including an accommodation unit capable of accommodating an ultrasound probe and an adhesion unit capable of contacting a target object; and a first control unit for controlling an adhesive force with respect to the target object of the adhesion unit according to whether a user touches at least one of the ultrasound probe and the housing.

[0011] The first control unit controls the adhesive force to be smaller than a first reference value if a user touch is detected, and controls the adhesive force to be greater than the first reference value if the user touch is not detected.

[0012] The support apparatus further includes: a second control unit for controlling a movement of the ultrasound probe according to whether the user touches at least one of the ultrasound probe and the housing.

[0013] The second control unit includes an actuator that is capable of moving such that the actuator contacts the ultrasound probe or is spaced apart from the ultrasound probe.

[0014] The actuator moves the ultrasound probe in correspondence to a user command used to move the ultrasound probe if the user touch is not detected, and the user command is input.

[0015] The adhesive force when a user touch is detected may be smaller than that when the user touch is not detected.

[0016] The first control unit may be capable of adjusting an intensity of the adhesive force at steps.

[0017] The first control unit may control the adhesive

force by using an amount of air between the adhesion unit and the target object.

[0018] The first control unit may include a vacuum pump that adjusts the amount of air.

[0019] The actuator may be spaced apart from the ultrasound probe such that the ultrasound probe moves if the user touch is detected, and fix the ultrasound probe if the user touch is not detected.

[0020] The actuator may move at a trace of a protocol that is previously stored in correspondence to the user command.

[0021] The user command may be remotely input.

[0022] The first control unit may receive whether the user touches at least one of the ultrasound probe and the housing from a sensor disposed in at least one of the ultrasound probe and the housing.

[0023] The sensor may include at least one of a touch sensor, a temperature sensor, a button sensor, a light sensor, and a pressure sensor.

[0024] The ultrasound probe may be detached from the accommodation unit.

[0025] According to one or more embodiments of the present invention, a handsfree ultrasound probe including: an ultrasound probe for irradiating ultrasound to a target object and receiving an echo signal of the ultrasound; an accommodation unit for accommodating the ultrasound probe; and an adhesion unit for contacting the target object.

[0026] The handsfree ultrasound probe may further include: a first control unit for controlling an adhesive force with respect to the target object of the adhesion unit according to whether a user touches the handsfree ultrasound probe.

[0027] The first control unit may control the adhesive force when a user touch is not detected to be greater smaller than that when the user touch is detected.

[0028] According to one or more embodiments of the present invention, a method of operating an ultrasound probe is provided in claim 10, the method including: detecting whether a user touches the ultrasound probe; and controlling an adhesive force of the ultrasound probe with respect to a target object to be smaller than a first reference value if it is detected that the user touches the ultrasound probe.

[0029] The method further includes: controlling the adhesive force of the handsfree ultrasound probe with respect to the target object to be greater than the first reference value if it is not detected that the user touches the handsfree ultrasound probe.

BRIEF DESCRIPTION OF THE DRAWINGS

[0030] These and/or other aspects will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings in which:

FIG. 1 is a schematic block diagram of a handsfree

ultrasound probe according to an embodiment of the present invention;

FIG. 2 is a block diagram of an ultrasound probe shown in FIG. 1;

FIG. 3 is a block diagram of a support apparatus shown in FIG. 1;

FIG. 4A illustrates an external appearance of the support apparatus shown in FIG. 1;

FIG. 4B illustrates an internal appearance of the support apparatus shown in FIG. 1;

FIG. 5 is a schematic block diagram of a handsfree ultrasound probe according to another embodiment of the present invention;

FIG. 6 is a block diagram of a support apparatus of an ultrasound probe according to another embodiment of the present invention;

FIG. 7 illustrates an internal appearance of the support apparatus shown in FIG. 6;

FIG. 8 is a block diagram of a support apparatus of an ultrasound probe according to another embodiment of the present invention;

FIGS. 9A through 9C illustrate examples of a user command used to move a handsfree ultrasound probe according to embodiments of the present invention;

FIG. 10 illustrates an external appearance of a handsfree ultrasound probe according to another embodiment of the present invention; and

FIG. 11 is a flowchart of a method of operating a handsfree ultrasound probe according to an embodiment of the present invention.

DETAILED DESCRIPTION

[0031] Reference will now be made in detail to embodiments, examples of which are illustrated in the accompanying drawings, wherein like reference numerals refer to the like elements throughout, and redundant explanations are omitted. In this regard, the present embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein. Accordingly, the embodiments are merely described below, by referring to the figures, to explain aspects of the present description. Expressions such as "at least one of," when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

[0032] Throughout the specification, a term 'target object' may include a person, animal, or a part of a person or animal. For example, the target object may include organs such as the liver, the heart, the womb, the brain, the breast, the abdominal region, etc., or a blood vessel. Throughout the specification, a "user" may be a medical expert including a doctor, a nurse, a medical laboratory technologist, a medical image expert, a technician repairing medical equipments, or the like.

[0033] FIG. 1 is a schematic block diagram of a handsfree ultrasound probe 100 according to an embodiment

of the present invention. FIG. 2 is a block diagram of an ultrasound probe 200 shown in FIG. 1. FIG. 3 is a block diagram of a support apparatus 300 shown in FIG. 1. FIG. 4A illustrates an external appearance of the support apparatus 300 shown in FIG. 1. FIG. 4B illustrates an internal appearance of the support apparatus 300 shown in FIG. 1.

[0034] Referring to FIG. 1, the handsfree ultrasound probe 100 includes the ultrasound probe 200 that photographs a target object by using ultrasound to generate an ultrasound image and the support apparatus 300 that supports the ultrasound probe 200 to contact the target object.

[0035] The ultrasound probe 200 transmits ultrasound to the target object and receives an echo signal of the ultrasound from the target object. The ultrasound probe 200 may include a transmission unit 220, a transducer 240, and a receiving unit 260 as shown in FIG. 2.

[0036] The transmission unit 220 provides the transducer 240 with a driving signal. The transmission unit 220 may include a pulse generation unit 222, a transmission delay unit 224, and a pulser 226.

[0037] The pulse generation unit 222 generates rate pulses for forming transmission ultrasound according to a predetermined pulse repetition frequency (PRF). The transmission delay unit 224 applies delay time to the rate pulses generated by the pulse generation unit 222 to determine a transmission directionality. The rate pulses to which the delay time is applied respectively correspond to a plurality of unit devices included in the transducer 240. The pulser 226 applies the driving signal (or a driving pulse) to the transducer 240 at timing corresponding to each of the rate pulses to which the delay time is applied. The unit devices may be in a one-dimensional array or a two-dimensional array.

[0038] The transducer 240 sends the ultrasound to the target object according to the driving signal provided by the transmission unit 220 and receives the echo signal of the ultrasound reflected from the target object. The transducer 240 may include a plurality of unit devices that convert an electrical signal into acoustic energy (or vice versa). The unit devices may be in a one-dimensional array or a two-dimensional array.

[0039] The transducer 240 may be implemented as a piezoelectric micromachined ultrasonic (pMUT) that inter-converts the ultrasound and the electrical signal by using a change in pressure while vibrating, a capacitive MUT (cMUT) that inter-converts the ultrasound and the electrical signal by using a change in capacitance, a magnetic MUT (mMUT) that inter-converts the ultrasound and the electrical signal by using a change in a magnetic field, an optical ultrasound detector that inter-converts the ultrasound and the electrical signal by using a change in an optical characteristic, etc.

[0040] The receiving unit 260 may generate ultrasound data by processing signals received from the transducer 240, and include an amplifier 262, an analogue digital converter (ADC) 264, a receiving delay unit 266, and a

summing unit 268.

[0041] The amplifier 262 amplifies the signals received from the transducer 240. The ADC 264 AD-converts the amplified signals. The receiving delay unit 266 applies a delay time used to determine a reception directionality to the digitally converted signals. The summing unit 268 generates the ultrasound data by summing signals processed by the receiving delay unit 266. A reflective component may be emphasized from a direction determined by the reception directionality according to the summing performed by the summing unit 268.

[0042] Although the ultrasound probe 200 necessarily includes the transducer 240, some elements of the transmission unit 220 and the receiving unit 260 may be included in another apparatus. For example, the ultrasound probe 200 may not include the summing unit 268 of the receiving unit 260.

[0043] The support apparatus 300 may include a housing 310 that forms an external appearance thereof and a first control unit 320 that controls an adhesive force with respect to a target object of the housing 310 according to whether the user touches at least one of the ultrasound probe 200 and the housing 310.

[0044] The housing 310 may include an accommodation unit 312 that is capable of accommodating the ultrasound probe 200 and an adhesion unit 314 that is capable of being adhered to the target object. The ultrasound probe 200 may be detachable from the accommodation unit 312. The accommodation unit 312 may be formed as a hole that passes through the housing 310 so that the ultrasound probe 200 may contact the target object but is not limited thereto. The accommodation unit 312 may be a groove formed inside the housing 310 or may be a space between a coverer 316 and the adhesion unit 314 of the housing 310.

[0045] The adhesion unit 314 may be a floor surface of the housing 310 to contact the target object. When the accommodation unit 312 is formed as the hole or the groove, the adhesion unit 314 may be disposed to surround the accommodation unit 312. When the accommodation unit 312 is a space inside the housing 310, the adhesion unit 314 may be the whole floor surface of the housing 310. The adhesion unit 314 may be formed of an elastic material. A shape of the adhesion unit 314 may be slightly changed according to an adhesive force with respect to the target object.

[0046] The first control unit 320 controls the adhesive force with respect to the target object of the adhesion unit 314 according to whether the user touches at least one of the ultrasound probe 200 and the housing 310. For example, if it is detected that the user touches at least one of the ultrasound probe 200 and the housing 310, the first control unit 320 controls the adhesive force to be smaller than a first reference value, and, if it is not detected that the user touches at least one of the ultrasound probe 200 and the housing 310, the first control unit 320 controls the adhesive force to be greater than the first reference value. That is, the adhesive force with respect

to the target object when a user touch is detected is smaller than that when the user touch is not detected. When the user touches the ultrasound probe 200 or the housing 310, since the adhesive force with respect to the target object is weak, the handsfree ultrasound probe 100 may freely move. When the user does not touch the ultrasound probe 200 or the housing 310, since the adhesive force with respect to the target object is strong, the handsfree ultrasound probe 100 may contact the target object.

[0047] The first control unit 30 may control an intensity of the adhesive force by using an amount of air between the adhesion unit 314 and the target object. For example, the first control unit 320 may include a vacuum pump capable of adjusting the amount of air. That is, the first control unit 320 may control the adhesive force to be stronger by reducing the amount of air between the adhesion unit 314 and the target object and may control the adhesive force to be weaker by increasing the amount of air between the adhesion unit 314 and the target object. The first control unit 320 may be disposed inside the housing 310 but is not limited thereto. The first control unit 320 may be disposed on the cover 316.

[0048] In addition, the first control unit 320 may adjust the intensity of the adhesive force at plural steps. For example, if the user touch is not detected, the first control unit 320 controls the adhesive force to be greater than the first reference value, and, if the user touch is detected, when an angle movement of the ultrasound probe 200 is detected, the first control unit 320 controls the adhesive force to be smaller than the first reference value and to be greater than a second reference value. When the user touch is detected, if a rectilinear movement (for example, a movement in a normal line direction or a tangent line direction with respect to the target object) of the ultrasound probe 200 is detected, the first control unit 320 controls the adhesive force to be smaller than the second reference value. The first control unit 320 may include elements in addition to the vacuum pump. For example, the first control unit 320 may be a motor that applies a pressure to contact the adhesion unit 314 to the target object or that separates the adhesion unit 314 from the target object.

[0049] Since the adhesive force with respect to the target object differs according to whether there is the user touch as described above, the user does not need to place the handsfree ultrasound probe 100 in a specific portion of the target object and hold the handsfree ultrasound probe 100. Thus, a pain in an arm that is like to occur by operating the ultrasound probe 200 may be reduced. The user may operate another function of an ultrasound diagnosis apparatus without using his/her hand to fix the ultrasound probe 200, thereby conveniently operating the ultrasound diagnosis apparatus. Furthermore, the handsfree ultrasound probe 100 may photograph an image with respect to a specific region of the target object for a predetermined period of time without shaking, and thus the user may accurately diagnose the specific region.

[0050] FIG. 5 is a schematic block diagram of the handsfree ultrasound probe 100 according to another embodiment of the present invention. Referring to FIG. 5, the handsfree ultrasound probe 100 may further include a sensor 330 that detects a user touch with respect to at least one of the ultrasound probe 200 and the housing 310 of the support apparatus 300. The sensor 330 may be at least one of a touch sensor, a temperature sensor, a button sensor, a light sensor, and a pressure sensor. The sensor 330 may be disposed in the ultrasound probe 200 or in the housing 310 of the support apparatus 300. If the sensor 330 is disposed in the ultrasound probe 200, the sensor 330 may be electrically connected to the first control unit 320 when the ultrasound probe 200 is accommodated in the accommodation unit 312 of the support apparatus 300. Thus, a detection result of the sensor 330 may be applied to the first control unit 320.

[0051] FIG. 6 is a block diagram of the support apparatus 300 of the ultrasound probe 200 according to another embodiment of the present invention. FIG. 7 illustrates an internal appearance of the support apparatus 300 shown in FIG. 6. Compared to the support apparatus 300 shown in FIG. 3, the support apparatus 300 shown in FIG. 6 may further include a second control unit 340 that controls a movement of the ultrasound probe 200 according to whether a user touch is detected. The second control unit 340 may include an actuator that is capable of moving such that the actuator may contact the ultrasound probe 200 or may be spaced apart from the ultrasound probe 200. The actuator may be spaced apart from the ultrasound probe 200 such that the ultrasound probe 200 may move if the user touch is detected. The actuator may contact and fix the ultrasound probe 200 if the user touch is not detected.

[0052] The second control unit 340 may control a movement of the ultrasound probe 200 according to a protocol that is previously stored. FIG. 8 is a block diagram of the support apparatus 300 of the ultrasound probe 200 according to another embodiment of the present invention. Compared to the support apparatus 300 shown in FIG. 7, the support apparatus 300 shown in FIG. 8 may further include a communication unit 350 that is capable of communicating with an external device. The external device may be a portable terminal as an apparatus capable of inputting a user command. If the ultrasound probe 200 is installed in the accommodation unit 312, the first control unit 320 controls an adhesive force of the adhesion unit 314 to be smaller than a first reference value, and the second control unit 340 fixes the ultrasound probe 200. If a user touch is not detected, the first control unit 320 controls the adhesive force of the adhesion unit 314 to be greater than the first reference value. In addition, if the user touch is not detected, and a user command used to move the ultrasound probe 200 is input through the communication unit 350, the second control unit 340 may move the ultrasound probe 200 according to the user command. The user command may be re-

motely input. That is, the user command may be input via wireless communication. The second control unit 340 may move the ultrasound probe 200 at one or more degrees of freedom.

[0053] Furthermore, if the user command is a movement command according to a protocol that is previous stored. For example, a movement trace of the ultrasound probe 200 may be previously stored according to a type (liver, abdomen, etc.) of a target object that is to be photographed. If a user command used to select the type of the target object is input, the second control unit 340 may move the ultrasound probe 200 to a movement trace corresponding to a selected type of the target object. The communication unit 350 is disposed in the support apparatus 300 in FIG. 7 but is not limited thereto. The communication unit 350 may be disposed in the ultrasound probe 200, and, when the ultrasound probe 200 is accommodated in the accommodation unit 312, may be electrically connected to the second control unit 340.

[0054] FIGS. 9A through 9C illustrate examples of a user command used to move the handsfree ultrasound probe 100 according to embodiments of the present invention.

[0055] Referring to FIG. 9A, after contacting the handsfree ultrasound probe 100 to a target object, a user may move the ultrasound probe 200 at one or more degrees of freedom while holding the ultrasound probe 200.

[0056] Alternatively, the user ends touching the handsfree ultrasound probe 100 while contacting the handsfree ultrasound probe 100 to the target object. Referring to FIG. 9B, a user control apparatus, for example, a portable terminal, may be used to control a movement of the ultrasound probe 200. Since a gyro sensor, an acceleration sensor, etc. are embedded in the portable terminal, if the user moves the portable terminal at one or more degrees of freedom, a movement of the portable terminal is transmitted to the handsfree ultrasound probe 100, and the ultrasound probe 200 may move in correspondence to the movement of the portable terminal.

[0057] Alternatively, referring to FIG. 9C, an icon 910 used to control a movement of the ultrasound probe 200 may be disposed in the user control apparatus. The user may control the movement of the ultrasound probe 200 by using the icon 910.

[0058] FIG. 10 illustrates an external appearance of the handsfree ultrasound probe 100 according to another embodiment of the present invention. Referring to FIG. 10, the housing 310 of the support apparatus 300 may be configured as the adhesion unit 314 and the cover 316, and the ultrasound probe 200 may be disposed in an inner space between the adhesion unit 314 and the cover 316. The ultrasound probe 200 may further include a wireless communication unit (not shown) that is capable of communicating with an external device (for example, a signal processing apparatus). Thus, the wireless communication unit may communicate data according to the digital imaging and communication in medicine (DICOM) standard.

[0059] FIG. 11 is a flowchart of a method of operating the handsfree ultrasound probe 100 according to an embodiment of the present invention. Referring to FIG. 11, the sensor 330 detects whether a user touches the handsfree ultrasound probe 100 (operation S1110). The sensor 330 may be disposed in the ultrasound probe 200 or in the support apparatus 300. The sensor 330 may be a touch sensor that is capable of detecting a user touch but is not limited thereto. The sensor 330 may be one of a temperature sensor, a button sensor, a light sensor, and a pressure sensor.

[0060] If a user touch is detected (operation S1110-Y), the first control unit 320 may control an adhesive force of the handsfree ultrasound probe 100 with respect to a target object to be smaller than a first reference value (operation S1120). Thus, the user may separate the handsfree ultrasound probe 100 from the target object.

[0061] If the user touch is not detected (operation S1110-N), the first control unit 320 may control the adhesive force of the handsfree ultrasound probe 100 with respect to the target object to be greater than the first reference value (operation S1130). Thus, the user may fix the handsfree ultrasound probe 100 to the target object without touching the handsfree ultrasound probe 100 so that the handsfree ultrasound probe 100 may continuously irradiate ultrasound to a specific region of the target object. Alternatively, the user may remotely move the ultrasound probe 200 and photograph an ultrasound image while contacting the ultrasound probe 200 to the target object. For example, if the user touch is not detected, and a user command used to move the ultrasound probe 200 is input, the second control unit 340 may move the ultrasound probe 200 in correspondence to the user command.

[0062] As described above, according to the one or more of the above embodiments of the present invention, a user may not hold an ultrasound probe during a diagnosis, thereby increasing a user convenience.

[0063] The ultrasound probe moves according to a protocol that is previous stored, thereby more accurately photographing an ultrasound image.

[0064] It should be understood that the exemplary embodiments described therein should be considered in a descriptive sense only and not for purposes of limitation. Descriptions of features or aspects within each embodiment should typically be considered as available for other similar features or aspects in other embodiments.

[0065] While one or more embodiments of the present invention have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the scope of the present invention as defined by the following claims.

Claims

1. A support apparatus (300) of an ultrasonic probe

(200), the support apparatus (300) comprising:

a housing (310) comprising an accommodation unit (312) capable of accommodating the ultrasound probe (200) and an adhesion unit (314) capable of contacting a target object; and
 a first control unit (320) configured to control an adhesive force of the adhesion unit (314) being adhered to the target object according to whether a user touches at least one of the ultrasound probe (200) and the housing (310);
 a second control unit (340) configured to control a movement of the ultrasound probe (200) according to whether the user touches at least one of the ultrasound probe (200) and the housing (310);
 wherein the first control unit (320) is configured to control the adhesive force to be smaller than a first reference value when a user touch is detected and to control the adhesive force to be greater than the first reference value when a user touch is not detected;
 wherein the second control unit (340) comprises an actuator that is capable of moving such that the actuator contacts the ultrasound probe (200) or is spaced apart from the ultrasound probe (200); and
 wherein the actuator is configured, when a user touch is not detected, to move the ultrasound probe (200) in correspondence to a user command to move the ultrasound probe (200).

2. The support apparatus (300) of claim 1, wherein the adhesive force when a user touch is detected is smaller than that when the user touch is not detected.
3. The support apparatus (300) of claims 1 or 2, wherein the first control unit (320) is capable of adjusting an intensity of the adhesive force at steps.
4. The support apparatus (300) any one of claims 1 to 3, wherein the first control unit (320) is configured to control the adhesive force by using an amount of air between the adhesion unit (314) and the target object.
5. The support apparatus (300) of claim 4, wherein the first control unit (320) comprises a vacuum pump that adjusts the amount of air.
6. The support apparatus (300) of claim 1, wherein the actuator is spaced apart from the ultrasound probe (200) such that the ultrasound probe (200) moves if the user touch is detected, and fixes the ultrasound probe (200) if the user touch is not detected.
7. The support apparatus (300) of claim 1, wherein the actuator is configured to move at a trace of a protocol

that is previously stored in correspondence to the user command.

8. The support apparatus (300) any one of claim 1 to 7, wherein the first control unit (320) is configured to receive whether the user touches at least one of the ultrasound probe (200) and the housing (310) from a sensor (330) disposed in at least one of the ultrasound probe (200) and the housing (310).
9. The support apparatus (300) any one of claim 1 to 8, wherein the ultrasound probe (200) is detachable from the accommodation unit.
10. A method of operating an ultrasound probe (100) with the support apparatus according to claim 1, the method comprising:

detecting whether a user touches the ultrasound probe (100);
 controlling an adhesive force of the adhesion unit (314) being adhered to the target object to be smaller than the first reference value when it is detected that the user touches the ultrasound probe (100) or
 to be greater than the first reference value when it is not detected that the user touches the ultrasound probe (100); and
 when it is not detected that the user touches the ultrasound probe (100),
 controlling a movement of the ultrasound probe (200) in correspondence to a user command used to move the ultrasound probe (200).

Patentansprüche

1. Trägervorrichtung (300) für eine Ultraschallsonde (200), wobei die Trägervorrichtung (300) folgendes aufweist:

ein Gehäuse (310), das eine Aufnahmeeinheit (312), die in der Lage ist, die Ultraschallsonde (200) aufzunehmen, und eine Adhäsionseinheit (314), die in der Lage ist, ein Zielobjekt zu kontaktieren, aufweist;
 eine erste Steuereinheit (320), die dafür vorgesehen ist, eine Adhäsivkraft der Adhäsionseinheit (314), die an dem Zielobjekt anhaftet, in Abhängigkeit davon zu steuern, ob ein Benutzer wenigstens eines der Ultraschallsonde (200) oder des Gehäuses (310) berührt;
 eine zweite Steuereinheit (340), die dafür vorgesehen ist, eine Bewegung der Ultraschallsonde (200) in Abhängigkeit davon zu steuern, ob der Nutzer wenigstens eines der Ultraschallsonde (200) oder des Gehäuses (310) berührt;
 wobei die erste Steuereinheit (320) dafür vorge-

- sehen ist, die Adhäsivkraft so zu steuern, dass sie kleiner als ein erster Referenzwert ist, wenn eine Berührung durch den Nutzer detektiert wird, und die Adhäsivkraft so zu steuern, dass sie größer als der erste Referenzwert ist, wenn eine Berührung durch den Nutzer nicht detektiert wird;
- wobei die zweite Steuereinheit (340) einen Aktuator aufweist, der in der Lage ist, sich so zu bewegen, dass der Aktuator die Ultraschallsonde (200) berührt oder von der Ultraschallsonde (200) entfernt angeordnet ist; und
- wobei der Aktuator dafür vorgesehen ist, die Ultraschallsonde (200), wenn eine Berührung durch den Nutzer nicht detektiert wird, in Übereinstimmung mit einem Befehl des Benutzers zu bewegen, um die Ultraschallsonde (200) zu bewegen.
2. Trägervorrichtung (300) nach Anspruch 1, wobei die Adhäsivkraft, wenn eine Berührung durch den Nutzer detektiert wird, kleiner ist als diejenige, wenn eine Berührung durch den Benutzer nicht detektiert wird.
 3. Trägervorrichtung (300) nach Anspruch 1 oder 2, wobei die erste Steuereinheit (320) dazu in der Lage ist, eine Intensität der Adhäsivkraft schrittweise einzustellen.
 4. Trägervorrichtung (300) nach einem der Ansprüche 1 bis 3, wobei die erste Steuereinheit (320) dafür vorgesehen ist, die Adhäsivkraft durch Verwenden einer Menge von Luft zwischen der Adhäsionseinheit (314) und dem Zielobjekt zu steuern.
 5. Trägervorrichtung (300) nach Anspruch 4, wobei die erste Steuereinheit (320) eine Vakuumpumpe aufweist, die die Menge an Luft einstellt.
 6. Trägervorrichtung (300) nach Anspruch 1, wobei der Aktuator von der Ultraschallsonde (200) derart beabstandet ist, dass die Ultraschallsonde (200) sich bewegt, wenn eine Berührung durch den Benutzer detektiert wird, und die Ultraschallsonde (200) befestigt, wenn die Berührung durch den Benutzer nicht detektiert wird.
 7. Trägervorrichtung (300) nach Anspruch 1, wobei der Aktuator dafür vorgesehen ist, sich in einer Spur eines Protokolls zu bewegen, das zuvor in Übereinstimmung mit dem Befehl des Benutzers gespeichert ist.
 8. Trägervorrichtung (300) nach einem der Ansprüche 1 bis 7, wobei die erste Steuereinheit (320) dafür vorgesehen ist, zu empfangen, ob der Benutzer wenigstens eines der Ultraschallsonde (200) oder des Gehäuses (310) berührt, und zwar von einem Sen-

sor (330), der in wenigstens einem der Ultraschallsonde (200) oder des Gehäuses (310) angeordnet ist.

9. Trägervorrichtung (300) nach einem der Ansprüche 1 bis 8, wobei die Ultraschallsonde (200) von der Aufnahmeeinheit abnehmbar ist.
10. Verfahren zum Betreiben einer Ultraschallsonde (100) mit der Trägervorrichtung nach Anspruch 1, wobei das Verfahren folgendes aufweist:

Detektieren, ob ein Benutzer die Ultraschallsonde (100) berührt;

Steuern einer Adhäsivkraft der Adhäsionseinheit (314), die an dem Zielobjekt anhaftet, derart, dass sie kleiner als der erste Referenzwert ist, wenn detektiert wird, dass der Benutzer die Ultraschallsonde (100) berührt, oder

dass sie größer als der erste Referenzwert ist, wenn nicht detektiert wird, dass der Benutzer die Ultraschallsonde (100) berührt; und

wenn nicht detektiert wird, dass der Benutzer die Ultraschallsonde (100) berührt,

Steuern einer Bewegung der Ultraschallsonde (200) in Übereinstimmung mit einem Befehl des Benutzers, um die Ultraschallsonde (200) zu bewegen.

Revendications

1. Appareil support (300) d'une sonde ultrasonique (200), l'appareil support (300) comportant :
 - un boîtier (310) comportant une unité d'accommodation (312) capable d'accommoder la sonde ultrasonique (200) et une unité d'adhésion (314) capable de contacter un objet cible ; et
 - une première unité de commande (320) agencée pour commander une force d'adhésion de l'unité d'adhésion (314) qui adhère à l'objet cible selon qu'un utilisateur touche au moins l'un parmi la sonde ultrasonique (200) et le boîtier (310) ;
 - une seconde unité de commande (340) agencée pour commander un mouvement de la sonde (200) selon que l'utilisateur touche au moins l'un parmi la sonde ultrasonique (200) et le boîtier (310) ;
 - dans lequel la première unité de commande (320) est agencée pour commander la force d'adhésion pour qu'elle soit inférieure à une première valeur de référence lorsqu'un toucher de l'utilisateur est détecté et pour commander la force adhésive pour qu'elle soit supérieure à la première valeur de référence, lorsqu'un toucher de l'utilisateur n'est pas détecté ;

- dans lequel la seconde unité de commande (340) comporte un actuateur capable de se déplacer de telle manière que l'actuateur contacte la sonde ultrasonique (200) ou est écartée de la sonde ultrasonique (200) ; et ; 5
- dans lequel l'actuateur est configuré, lorsqu'un toucher de l'utilisateur n'est pas détecté, pour déplacer la sonde ultrasonique (200) en correspondance avec une commande d'un utilisateur, pour déplacer la sonde ultrasonique (200). 10
2. Appareil support (300) selon la revendication 1, dans lequel, lorsqu'un toucher d'utilisateur est détecté, la force adhésive correspondante est inférieure à celle appliquée lorsqu'un toucher d'utilisateur n'est pas détecté. 15
 3. Appareil support (300) selon les revendications 1 ou 2, dans lequel la première unité de commande (320) est capable d'ajuster par paliers, l'intensité de la force adhésive. 20
 4. Appareil support (300) selon l'une des revendications 1 à 3, dans lequel la première unité de commande (320) est agencée pour commander la force adhésive en utilisant une quantité d'air entre l'unité d'adhésion (314) et l'objet cible. 25
 5. Appareil support (300) selon la revendication 4, dans lequel la première unité de commande (320) comporte une pompe à vide qui ajuste la quantité d'air. 30
 6. Appareil support (300) selon la revendication 1, dans lequel l'actuateur est espacé de la sonde ultrasonique (200), de telle manière que la sonde ultrasonique (200) se déplace si le toucher de l'utilisateur est détecté, et fixe la sonde ultrasonique (200) si le toucher de l'utilisateur n'est pas détecté. 35
 7. Appareil support (300) selon la revendication 1, dans lequel l'actuateur est configuré pour se déplacer sur une trajectoire du protocole qui a été mémorisée précédemment en rapport avec la commande de l'utilisateur. 40
 8. Appareil support (300) selon l'une des revendications 1 à 7, dans lequel la première unité de commande (320) est agencée pour recevoir si l'utilisateur touche au moins l'un parmi la sonde ultrasonique (200) et le boîtier (310) d'un capteur (330) disposé dans au moins l'un parmi la sonde ultrasonique (200) et le boîtier (310). 45
 9. Appareil support (300) selon l'une des revendications 1 à 8, dans lequel la sonde ultrasonique (200) est détachable de l'unité d'accommodation. 50
 10. Méthode opératoire d'une sonde ultrasonique (100) 55

ayant un appareil de support, selon la revendication 1, la méthode consistant à :

détecter si un utilisateur touche la sonde ultrasonique (100);

commander une force d'adhésion de l'unité d'adhésion (314) qui adhère à l'objet cible, pour être inférieure à une première valeur de référence lorsqu'il est constaté que l'utilisateur touche la sonde ultrasonique (100) ou pour être supérieure à la première valeur de référence lorsqu'il n'est pas détecté que l'utilisateur touche la sonde ultrasonique (100) ; et

lorsqu'il n'est pas détecté que l'utilisateur touche la sonde ultrasonique (100), commander un mouvement de la sonde ultrasonique (200) en correspondance avec une commande de l'utilisateur pour déplacer la sonde ultrasonique (200).

FIG. 1

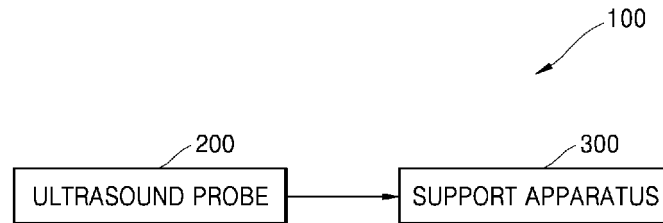


FIG. 2

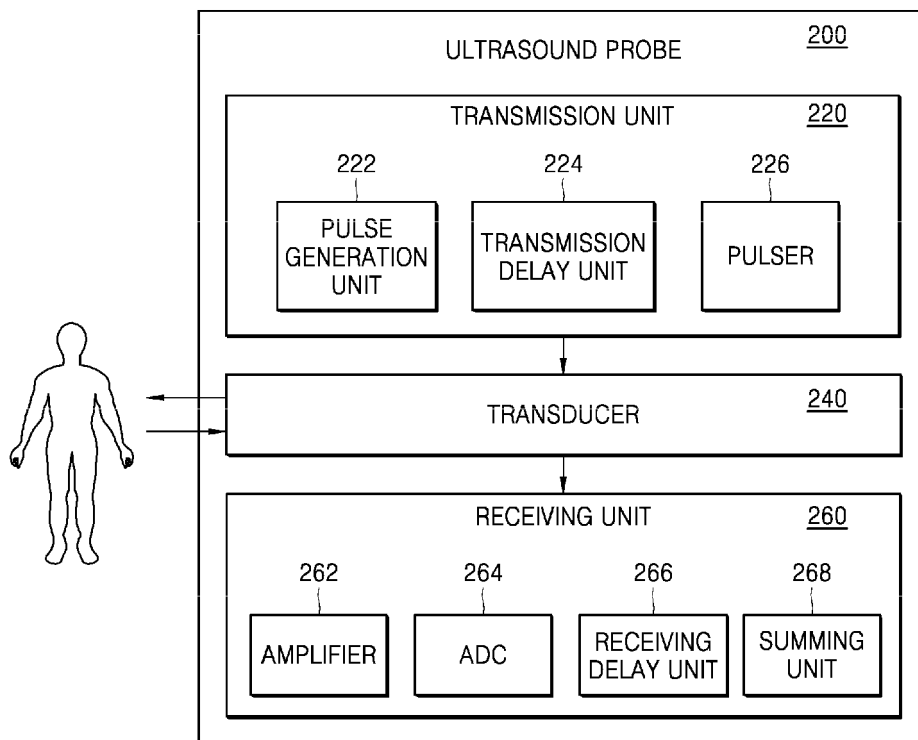


FIG. 3

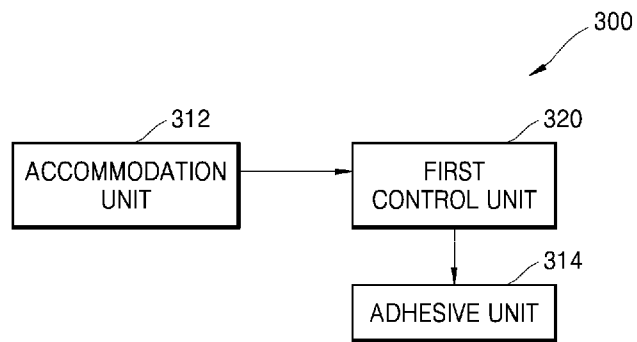


FIG. 4A

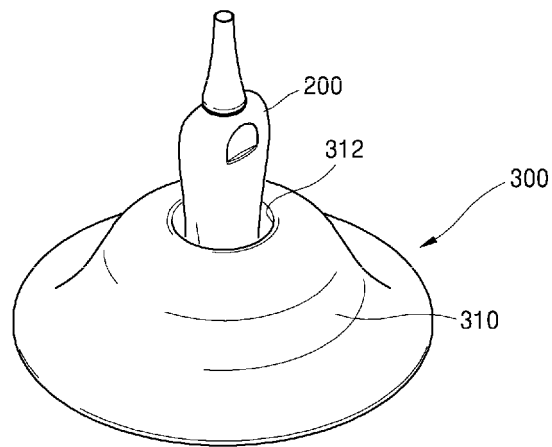


FIG. 4B

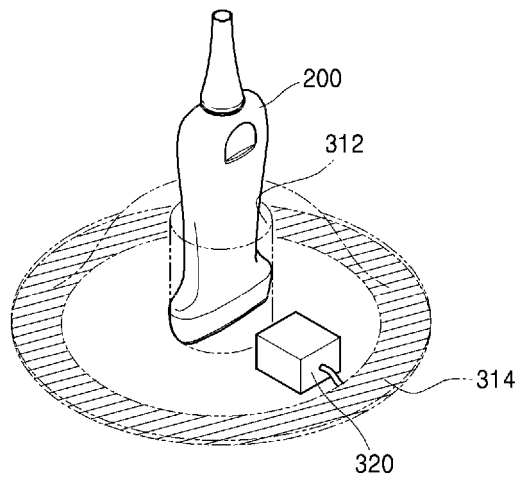


FIG. 5

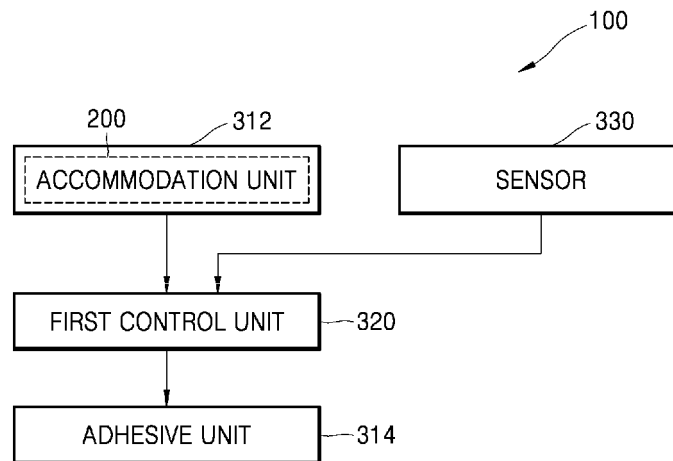


FIG. 6

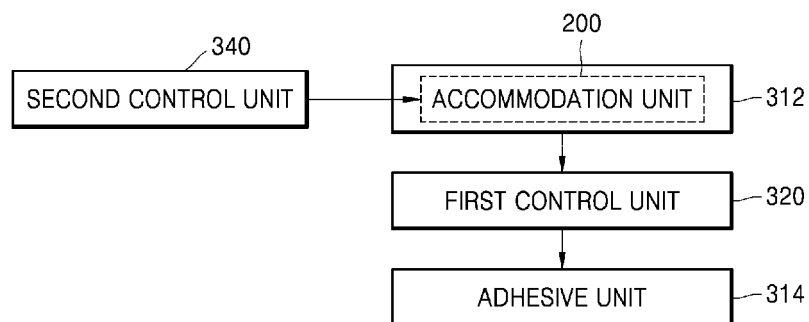


FIG. 7

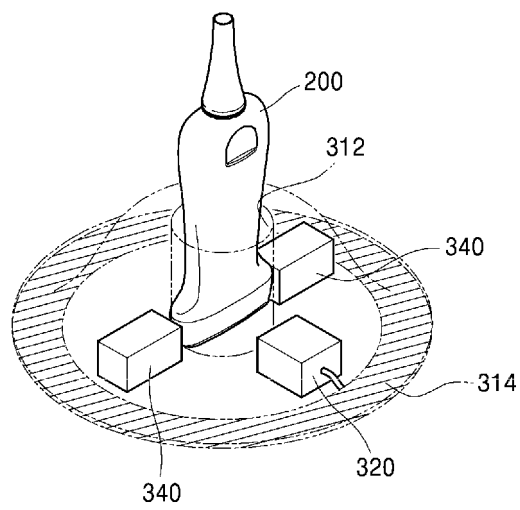


FIG. 8

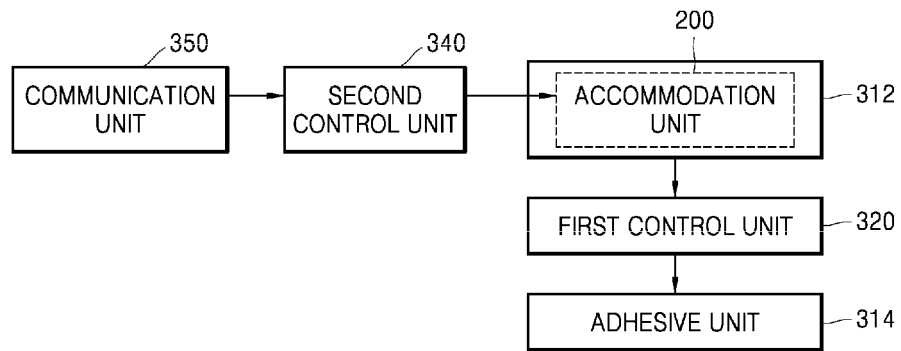


FIG. 9A

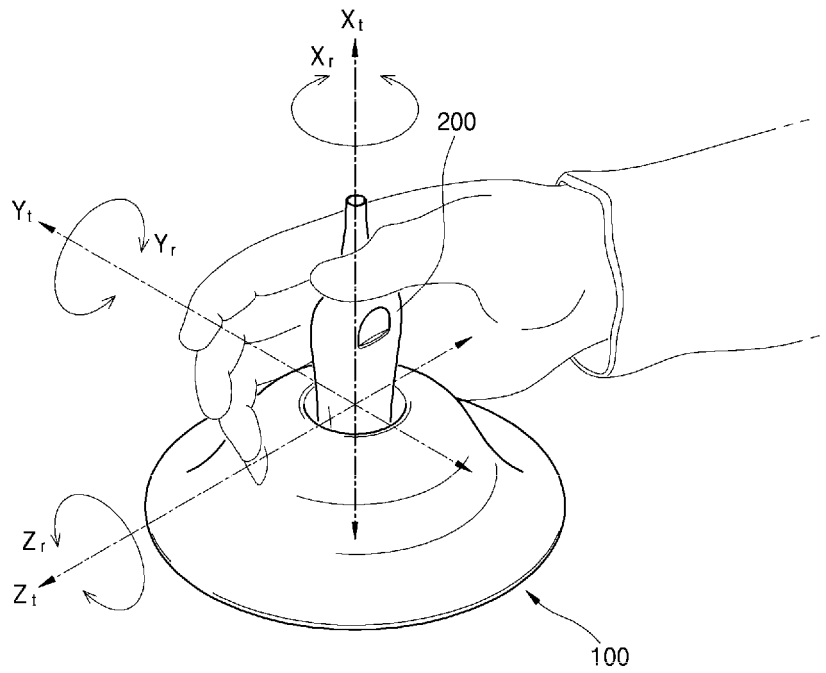


FIG. 9B

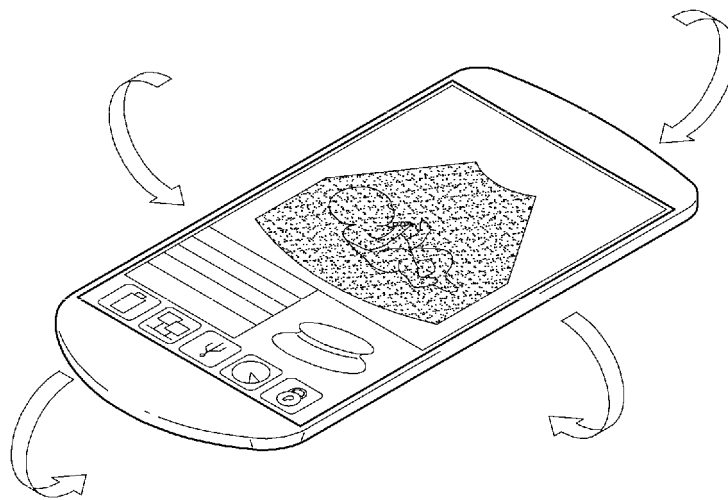


FIG. 9C

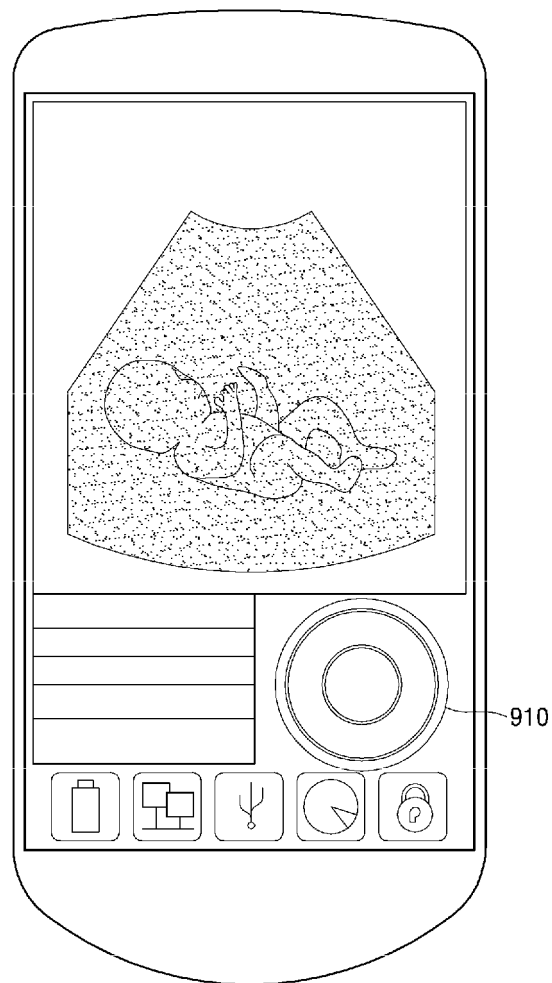


FIG. 10


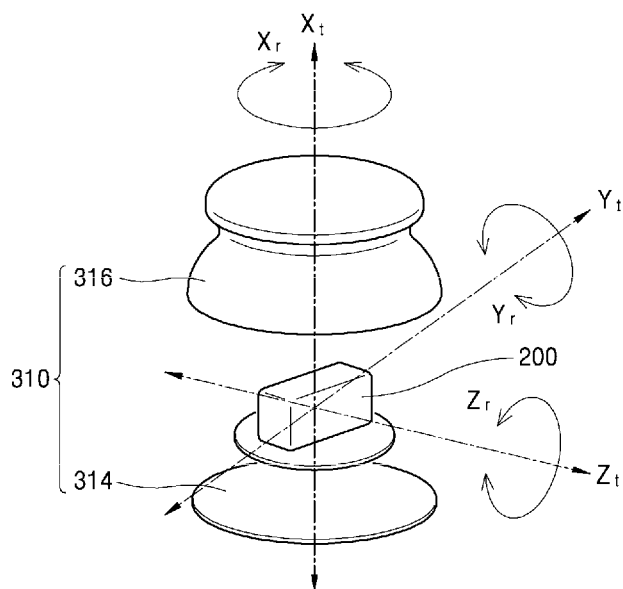


FIG. 11

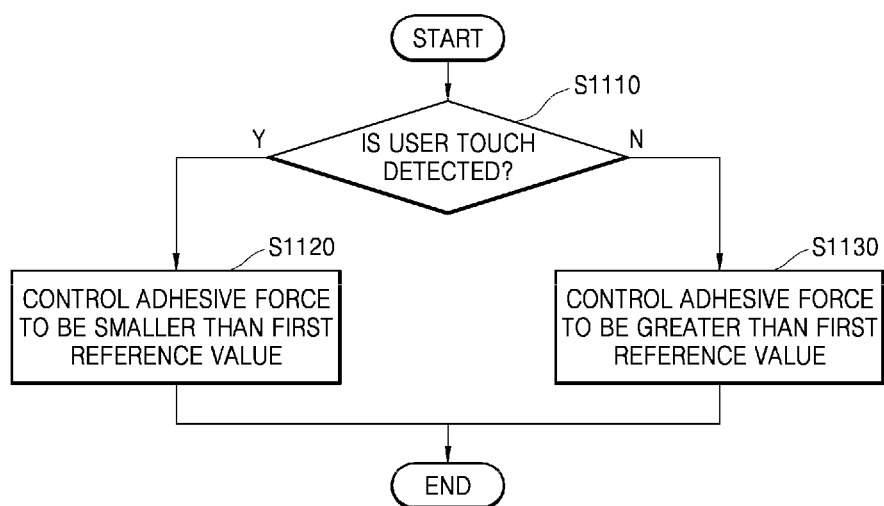

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2008061894 A [0005]
- JP 2006230913 A [0006]

专利名称(译)	超声波探头的支撑装置，包括支撑装置的免提超声波探头，以及操作支撑装置的方法		
公开(公告)号	EP2870917B1	公开(公告)日	2017-06-28
申请号	EP2014157985	申请日	2014-03-06
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	YOON JEONG UN JO JAE MOON KIM JONG SIK JIN GIL JU		
发明人	YOON, JEONG-UN JO, JAE-MOON KIM, JONG-SIK JIN, GIL-JU		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4209 A61B8/4236 A61B8/4427 A61B8/4444 A61B8/467 A61B8/54		
代理机构(译)	LORENZ , MARKUS		
优先权	1020130134355 2013-11-06 KR		
其他公开文献	EP2870917A1		
外部链接	Espacenet		

摘要(译)

一种超声波探头的支撑装置，包括该支撑装置的免提超声波探头，以及操作该支撑装置的方法。支撑装置包括：壳体，包括能够容纳超声探头的容纳单元和能够接触目标物体的粘附单元；第一控制单元，用于根据用户是否接触超声波探头和壳体中的至少一个来控制相对于粘附单元的目标物体的粘合力。

FIG. 1




FIG. 2

