



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
13.06.2012 Bulletin 2012/24

(51) Int Cl.:
A61B 8/06 (2006.01)

(21) Application number: **11191707.6**

(22) Date of filing: **02.12.2011**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(30) Priority: **07.12.2010 KR 20100123899**

(71) Applicant: **Samsung Medison Co., Ltd.**
Nam-myun
Hongchun-gun
Kangwon do 250-875 (KR)

(72) Inventors:
• **Kim, Sung Hee**
135-851 Seoul (KR)
• **Lee, Suk Jin**
135-851 Seoul (KR)


(74) Representative: **Schmid, Wolfgang**
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft
Alte Ulmer Strasse 2
89522 Heidenheim (DE)

(54) **Providing additional information corresponding to change of blood flow with a time in ultrasound system**

(57) There are provided embodiments for providing additional information. In one embodiment, an ultrasound system (100) comprises: an ultrasound data acquisition unit (120) configured to acquire first ultrasound data and second ultrasound data corresponding to a living body; and a processing unit (130) configured to form a brightness mode image based on the first ultrasound data, set

at least one sample volume on the brightness mode image, and form blood flow information corresponding to blood flow in the living body based on the second ultrasound data corresponding to the at least one sample volume, the processing unit being further configured to form additional information corresponding to a change of the blood flow with a time based on the blood flow information.

FIG. 1

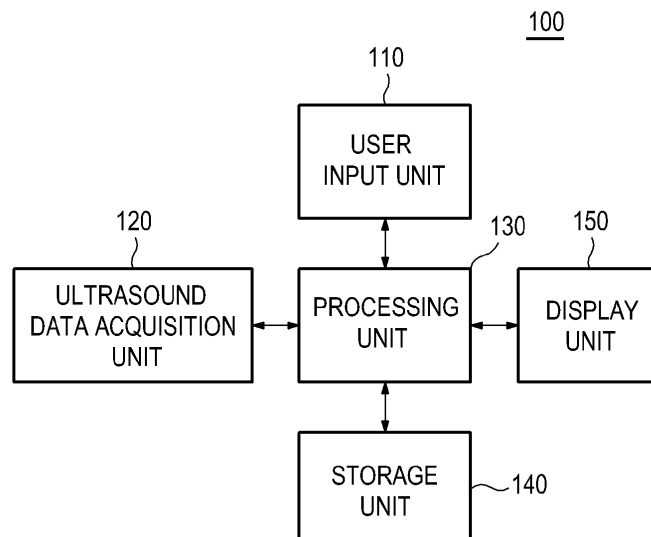

Description

CROSS-REFERENCE TO RELATED APPLICATION

[0001] The present application claims priority from Korean Patent Application No. 10-2010-0123899 filed on December 7, 2010.

TECHNICAL FIELD

[0002] The present disclosure generally relates to ultrasound systems, and more particularly to providing additional information corresponding to a change of blood flow with a time in an ultrasound system.

BACKGROUND

[0003] An ultrasound system has become an important and popular diagnostic tool since it has a wide range of applications. Specifically, due to its non-invasive and non-destructive nature, the ultrasound system has been extensively used in the medical profession. Modern high-performance ultrasound systems and techniques are commonly used to produce two-dimensional or three-dimensional ultrasound images of internal features of a target object (e.g., human organs).

[0004] The ultrasound system may provide ultrasound images of various modes including a brightness mode (B mode) image representing reflection coefficients of the ultrasound signals reflected from a target object of a living body with a 2D (two-dimensional) image, a Doppler mode (D mode) image representing speed of a moving target object with spectral Doppler by using a Doppler effect, a color Doppler mode (C mode) image representing speed of a moving target object with colors by using the Doppler effect, and an elastic mode (E mode) image representing mechanical characteristics of tissues object before and after applying a pressure thereto. Particularly, the ultrasound system may transmit and receive ultrasound signals to and from the living body to thereby form Doppler signals corresponding to a sample volume, which is set on a B mode image. The ultrasound system may further form the D mode image (i.e., Doppler spectrum image) that represents the speed of the moving target object such as blood flow, heart, etc. with Doppler spectrums based on the Doppler signals.

[0005] The ultrasound system may provide the Doppler spectrum image only based on the blood flow information. Thus, it is required to provide additional information corresponding to a change of the blood flow with a time to enhance the convenience of a user.

SUMMARY

[0006] There are provided embodiments for providing additional information corresponding to a change of blood flow with a time in an ultrasound system.

[0007] In one embodiment, by way of non-limiting ex-

ample, an ultrasound system comprises: an ultrasound data acquisition unit configured to acquire first ultrasound data and second ultrasound data corresponding to a living body; and a processing unit configured to form a brightness mode image based on the first ultrasound data, set at least one sample volume on the brightness mode image, and form blood flow information corresponding to blood flow in the living body based on the second ultrasound data corresponding to the at least one sample volume, the processing unit being further configured to form additional information corresponding to a change of the blood flow with a time based on the blood flow information.

[0008] In another embodiment, there is provided a method of providing additional information, comprising: a) acquiring first ultrasound data corresponding to a living body; b) forming a brightness mode image based on the first ultrasound data; c) setting at least one sample volume on the brightness mode image; d) acquiring second ultrasound data corresponding to the at least one sample volume; e) forming blood flow information corresponding to blood flow in the living body based on the second ultrasound data corresponding to the at least one sample volume; and f) forming additional information corresponding to a change of the blood flow with a time based on the blood flow information.

[0009] This summary is provided to introduce a selection of concepts in a simplified form that are further described below in the Detailed Description. This Summary is not intended to identify key or essential features of the claimed subject matter, nor is it intended to be used in determining the scope of the claimed subject matter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010]

FIG 1 is a block diagram showing an illustrative embodiment of an ultrasound system.

FIG 2 is a schematic diagram showing an example of a brightness mode image and a sample volume. FIG 3 is a block diagram showing an illustrative embodiment of an ultrasound data acquisition unit.

FIG 4 is a flow chart showing a process of forming a Doppler spectrum image and additional information.

FIG 5 is a schematic diagram showing an example of the additional information.

FIG 6 is a schematic diagram showing another example of the additional information.

FIG 7 is a schematic diagram showing yet another example of the additional information.

DETAILED DESCRIPTION

[0011] A detailed description may be provided with reference to the accompanying drawings. One of ordinary skill in the art may realize that the following description

is illustrative only and is not in any way limiting.

[0012] Referring to FIG 1, an ultrasound system 100 in accordance with an illustrative embodiment is shown. As depicted therein, the ultrasound system 100 includes a user input unit 110.

[0013] The user input unit 110 is configured to receive input information. In the embodiment, the input information includes sample volume setting information for setting a sample volume SV on a brightness mode image BI, as shown in FIG 2. However, it should be noted herein that the input information may not be limited thereto. In FIG 2, reference numeral BV represents a blood vessel. The user input unit 110 includes a control panel, a trackball, a mouse, a keyboard and the like.

[0014] The ultrasound system 100 further includes an ultrasound data acquisition unit 120. The ultrasound acquisition unit 120 is configured to transmit ultrasound signals to a living body. The living body includes target objects (e.g., blood flow, a heart, etc.). The ultrasound acquisition unit 120 may be further configured to receive ultrasound signals (i.e., ultrasound echo signals) from the living body to acquire ultrasound data. FIG 3 is a block diagram showing an illustrative embodiment of the ultrasound data acquisition unit. Referring to FIG 3, the ultrasound data acquisition unit 120 includes an ultrasound probe 310.

[0015] The ultrasound probe 310 includes a plurality of transducer elements (not shown) for reciprocally converting between ultrasound signals and electrical signals. The ultrasound probe 310 is configured to transmit the ultrasound signals to the living body. The ultrasound probe 310 is further configured to receive the ultrasound echo signals from the living body to output received signals. The received signals are analog signals. The ultrasound probe 310 includes a convex probe, a linear probe and the like.

[0016] The ultrasound data acquisition unit 120 further includes a transmitting section 320. The transmitting section 320 is configured to control the transmission of the ultrasound signals. The transmitting section 320 is further configured to generate electrical signals ("transmitting signals") for obtaining an ultrasound image in consideration of the elements and focusing points. The transmitting section 320 includes a transmitting signal generating section (not shown), a transmitting delay information memory (not shown), a transmitting beam former (not shown) and the like.

[0017] In the embodiment, the transmitting section 320 generates first transmitting signals for obtaining the brightness mode image BI. Thus, the ultrasound probe 310 converts the first transmitting signals into the ultrasound signals, transmits the ultrasound signals to the living body and receives the ultrasound echo signals from the living body to thereby output first received signals. The transmitting section 320 further generates second transmitting signals for obtaining a Doppler spectrum image corresponding to the sample volume SV. Thus, the ultrasound probe 310 converts the second transmitting

signals into the ultrasound signals, transmits the ultrasound signals to the living body and receives the ultrasound echo signals from the living body to thereby output second received signals.

[0018] The ultrasound data acquisition unit 120 further includes a receiving section 330. The receiving section 330 is configured to convert the received signals into digital signals. The receiving section 330 is further configured to apply delays to the digital signals in consideration of the elements and the focusing points to thereby output digital receive-focused signals. The receiving section 330 includes an analog-to-digital converter (not shown), a receiving delay time information memory (not shown), a receiving beam former (not shown) and the like.

[0019] In the embodiment, the receiving section 330 converts the first received signals provided from the ultrasound probe 310 into first digital signals. The receiving section 330 further applies delays to the first digital signals in consideration of the elements and the focusing points to thereby output first digital receive-focused signals. The receiving section 330 further converts the second received signals provided from the ultrasound probe 310 into second digital signals. The receiving section 330 further applies delays to the second digital signals in consideration of the elements and the focusing points to thereby output second digital receive-focused signals.

[0020] The ultrasound data acquisition unit 120 further includes an ultrasound data forming section 340. The ultrasound data forming section 340 is configured to form ultrasound data corresponding to the ultrasound image based on the digital receive-focused signals provided from the receiving section 330. The ultrasound data forming section 340 is further configured to perform a signal process (e.g., gain control, etc) upon the digital receive-focused signals.

[0021] In the embodiment, the ultrasound data forming section 340 forms first ultrasound data corresponding to the brightness mode image BI based on the first digital receive-focused signals provided from the receiving section 330. The first ultrasound data include radio frequency data. However, it should be noted herein that the first ultrasound data may not be limited thereto. The ultrasound data forming section 340 further forms second ultrasound data corresponding to the sample volume SV (i.e., Doppler spectrum image) based on the second digital receive-focused signals provided from the receiving section 330. The second ultrasound data include the radio frequency data or in-phase/quadrature data. However, it should be noted herein that the second ultrasound data may not be limited thereto.

[0022] Referring back to FIG 1, the ultrasound system 100 further includes a processing unit 130 in communication with the user input unit 110 and the ultrasound data acquisition unit 120. The processing unit 130 includes a central processing unit, a microprocessor, a graphic processing unit and the like.

[0023] FIG 4 is a flow chart showing a process of forming additional information. The processing unit 130 is

configure to form the brightness mode image BI based on the first ultrasound data provided from the ultrasound data acquisition unit 120, at step S402 in FIG 4. The brightness mode image BI is displayed on a display unit 150. Thus, the user sets the sample volume SV on the brightness mode image BI by using the user input unit 110.

[0024] The processing unit 130 is configured to set the sample volume SV on the brightness mode image BI as shown in FIG 2, based on the input information provided from the user input unit 110, at step S404 in FIG. 4. Thus, the ultrasound data acquisition unit 120 acquires the second ultrasound data corresponding to the sample volume SV.

[0025] The processing unit 130 is configured to form information (hereinafter, "blood flow information") corresponding to a moving target object (i.e., blood flow) in the living body based on the second ultrasound data provided from the ultrasound data acquisition unit 120, at step S406 in FIG 4. In the embodiment, the blood flow information includes blood flow velocity information, blood flow rate information, blood flow velocity distribution information and the like. The methods of forming the blood flow information are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0026] The processing unit 130 is configured to form the Doppler spectrum image based on the blood flow information, at step S408 in FIG 4. The methods of forming the Doppler spectrum image are well known in the art. Thus, they have not been described in detail so as not to unnecessarily obscure the present invention.

[0027] The processing unit 130 is configured to form additional information based on the blood flow information, at step S410 in FIG 4. The additional information is information for representing a change of the blood flow with a time.

[0028] As one example, the processing unit 130 forms a color map CM as the additional information based on the blood flow information, as shown in FIG 5. The color map CM is formed by mapping a plurality of blood flow velocities (i.e., height of Doppler spectrum) to colors.

[0029] As another example, the processing unit 130 forms a color Doppler spectrum image PWI as the additional information based on the blood flow information, as shown in FIG 5. The color Doppler spectrum image PWI is formed by mapping the colors corresponding to the color map CM to the Doppler spectrum image. That is, the color Doppler spectrum image PWI is formed by applying the colors corresponding to the blood flow velocities to pixels of the Doppler spectrum image.

[0030] As yet another example, the processing unit 130 forms a color blood flow velocity image CI as the additional information based on the blood flow information, as shown in FIG 5. The color blood flow velocity image CI is formed by mapping the blood flow velocity to the color. That is, the color blood flow velocity image CI is formed by mapping the blood flow velocity corre-

sponding to current blood flow information to the color.

[0031] Although it is described that the processing unit 130 forms the color map, the color Doppler spectrum image or the color blood flow velocity image, the processing unit 130 forms at least one of the color map, the color Doppler spectrum image and the color blood flow velocity image.

[0032] As yet another example, the processing unit 130 applies transparency corresponding to the blood flow rate to at least one of the color map, the color Doppler spectrum image and the color blood flow velocity image as the additional information, based on the blood flow information. That is, the processing unit 130 applies the transparency to the colors corresponding to the blood flow velocities based on the blood flow rate.

[0033] As yet another example, the processing unit 130 forms a blood flow velocity distribution image 610 as the additional information based on the blood flow information, as shown in FIG 6. The blood flow velocity distribution image 610 is an image for representing blood flow velocity distribution based on distribution of spots (i.e., width of Doppler spectrum).

[0034] As yet another example, the processing unit 130 forms numeric information corresponding to the blood flow velocity and variance as the additional information based on the blood flow information.

[0035] Although it is described that the processing unit 130 forms the Doppler spectrum image with the additional information based on the blood flow information, the processing unit 130 forms the additional information based on the blood flow information.

[0036] Also, although it is described that the sample volume SV is set on the brightness mode image BI and the additional information corresponding to the sample volume is provided, at least one sample volume (e.g., two sample volumes SV_1 , SV_2 as shown in FIG 7) is set on the brightness mode image BI and the additional information (e.g., color Doppler spectrum images PWI_1 , PWI_2 , color blood flow images CI_1 , CI_2 and the like) corresponding to each of the sample volumes SV_1 , SV_2 .

[0037] Referring back to FIG 1, the ultrasound system 100 further includes a storage unit 140. The storage unit 140 stores the ultrasound data (i.e., first ultrasound data and second ultrasound data) acquired by the ultrasound data acquisition unit 120. The storage unit 140 further stores the input information received by the user input unit 110.

[0038] The ultrasound system 100 further includes the display unit 150. The display unit 150 is configured to display the brightness mode image BI formed by the processing unit 130. The display unit 150 is further configured to display the Doppler spectrum image formed by the processing unit 130. The display unit 150 is further configured to display the additional information formed by the processing unit 130.

[0039] Although embodiments have been described with reference to a number of illustrative embodiments thereof, it should be understood that numerous other

modifications and embodiments can be devised by those skilled in the art that will fall within the scope of the principles of this disclosure. More particularly, numerous variations and modifications are possible in the component parts and/or arrangements of the subject combination arrangement within the scope of the disclosure, the drawings and the appended claims. In addition to variations and modifications in the component parts and/or arrangements, alternative uses will also be apparent to those skilled in the art.

Claims

1. An ultrasound system, comprising:

an ultrasound data acquisition unit configured to acquire first ultrasound data and second ultrasound data corresponding to a living body; and

a processing unit configured to form a brightness mode image based on the first ultrasound data, set at least one sample volume on the brightness mode image and form blood flow information corresponding to blood flow in the living body based on the second ultrasound data corresponding to the at least one sample volume, the processing unit being further configured to form additional information corresponding to a change of the blood flow with a time based on the blood flow information.

2. The ultrasound system of Claim 1, wherein the blood flow information includes blood flow velocity information, blood flow rate information and blood flow velocity distribution information.

3. The ultrasound system of Claim 1, wherein the processing unit is configured to form at least one of a color map for mapping blood flow velocities to colors, a color blood flow velocity image for mapping a blood flow velocity to a color and a color Doppler spectrum image for mapping blood flow velocities to colors as the additional information based on the blood flow information.

4. The ultrasound system of Claim 4, wherein the color blood flow velocity image is displayed on the at least one sample volume.

5. The ultrasound system of Claim 1, wherein the processing unit is configured to apply transparency to at least one of a color map, a color Doppler spectrum image and a color blood flow velocity image as the additional information based on the blood flow information.

6. The ultrasound system of Claim 1, wherein the

processing unit is configured to form a blood flow velocity distribution for representing blood flow velocity distribution corresponding to distribution of spots as the additional information based on the blood flow information.

7. The ultrasound system of Claim 1, wherein the processing unit is configured to form numeric information corresponding to blood flow velocity and variance as the additional information based on the blood flow information.

8. A method of providing additional information, comprising:

- a) acquiring first ultrasound data corresponding to a living body;
- b) forming a brightness mode image based on the first ultrasound data;
- c) setting at least one sample volume on the brightness mode image;
- d) acquiring second ultrasound data corresponding to the at least one sample volume;
- e) forming blood flow information corresponding to blood flow in the living body based on the second ultrasound data corresponding to the at least one sample volume; and
- f) forming additional information corresponding to a change of the blood flow with a time based on the blood flow information.

9. The method of Claim 8, wherein the blood flow information includes blood flow velocity information, blood flow rate information and blood flow velocity distribution information.

10. The method of Claim 8, wherein the step f) comprises:

- forming at least one of a color map for mapping blood flow velocities to colors,
- a color blood flow velocity image for mapping a blood flow velocity to a color and a color Doppler spectrum image for mapping blood flow velocities to colors as the additional information based on the blood flow information.

11. The method of Claim 10, wherein the color blood flow velocity image is displayed on the at least one sample volume.

12. The method of Claim 8, wherein the step f) comprises:

- applying transparency to at least one of a color map, a color Doppler spectrum image and a color blood flow velocity image as the additional information base on the blood flow information.

13. The method of Claim 8, wherein the step f) comprises:

forming a blood flow velocity distribution for representing blood flow velocity distribution corresponding to distribution of spots as the additional information based on the blood flow information. 5

14. The method of Claim 8, wherein the step f) comprises: 10

forming numeric information corresponding to blood flow velocity and variance as the additional information based on the blood flow information. 15

20

25

30

35

40

45

50

55

FIG. 1

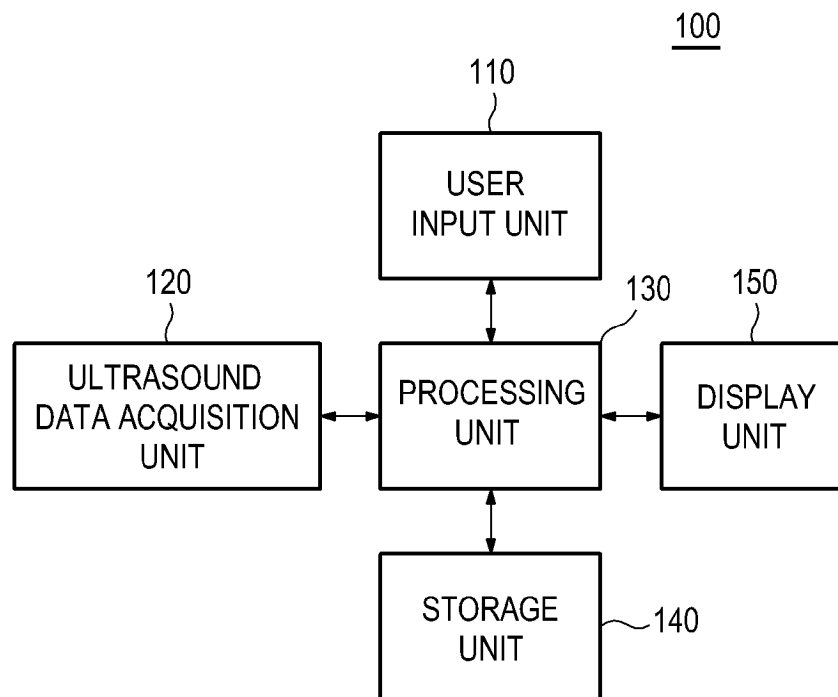


FIG. 2

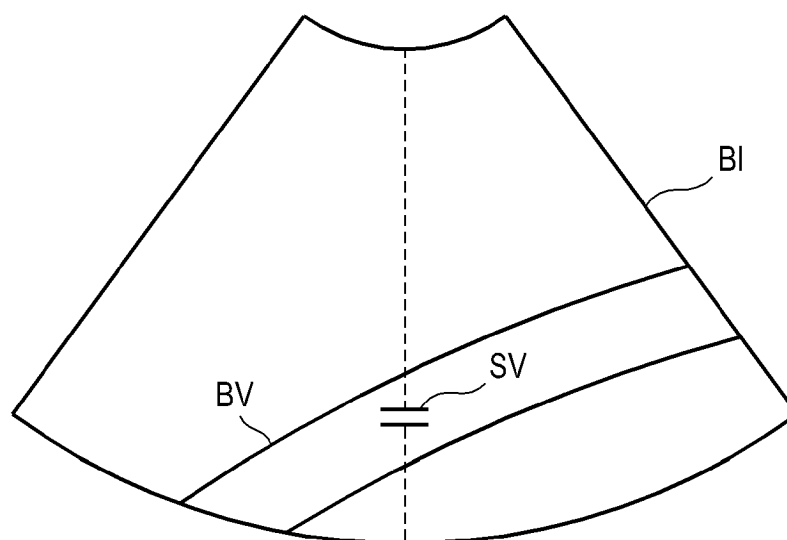


FIG. 3

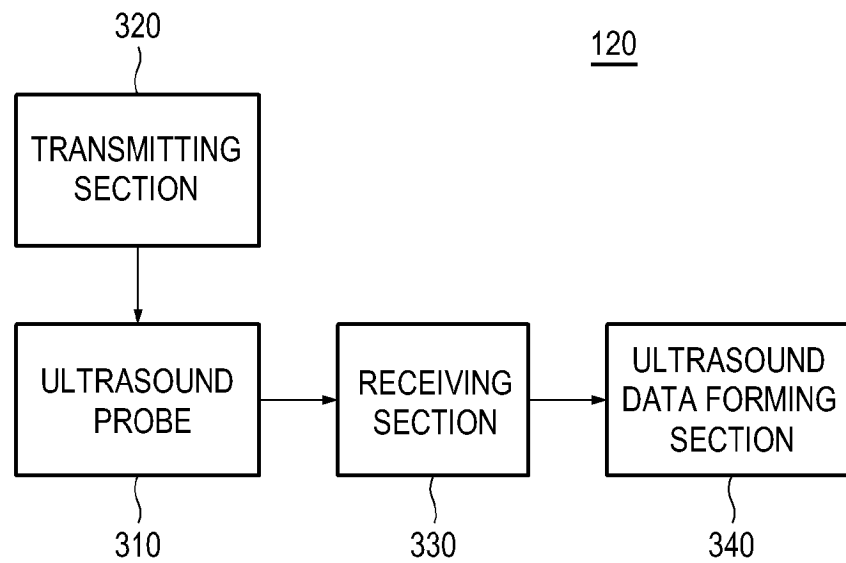


FIG. 4

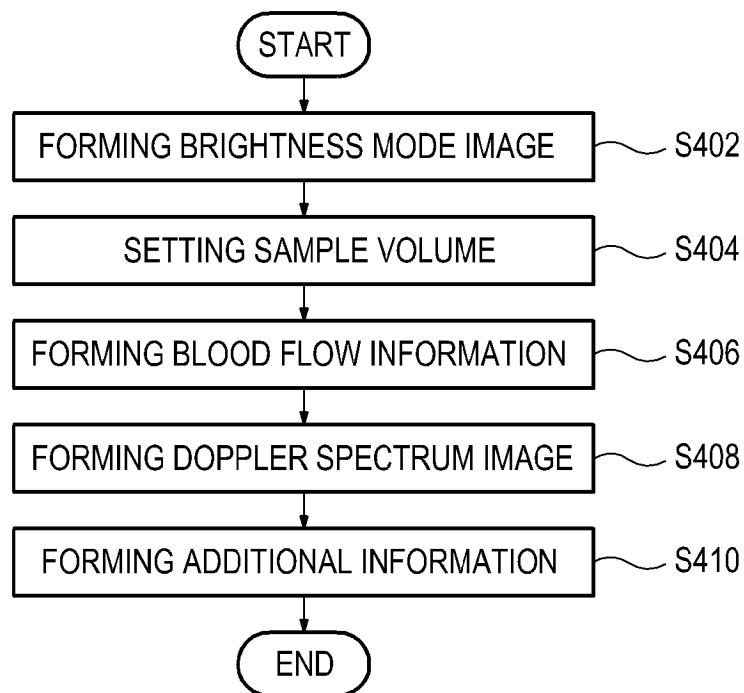


FIG. 5

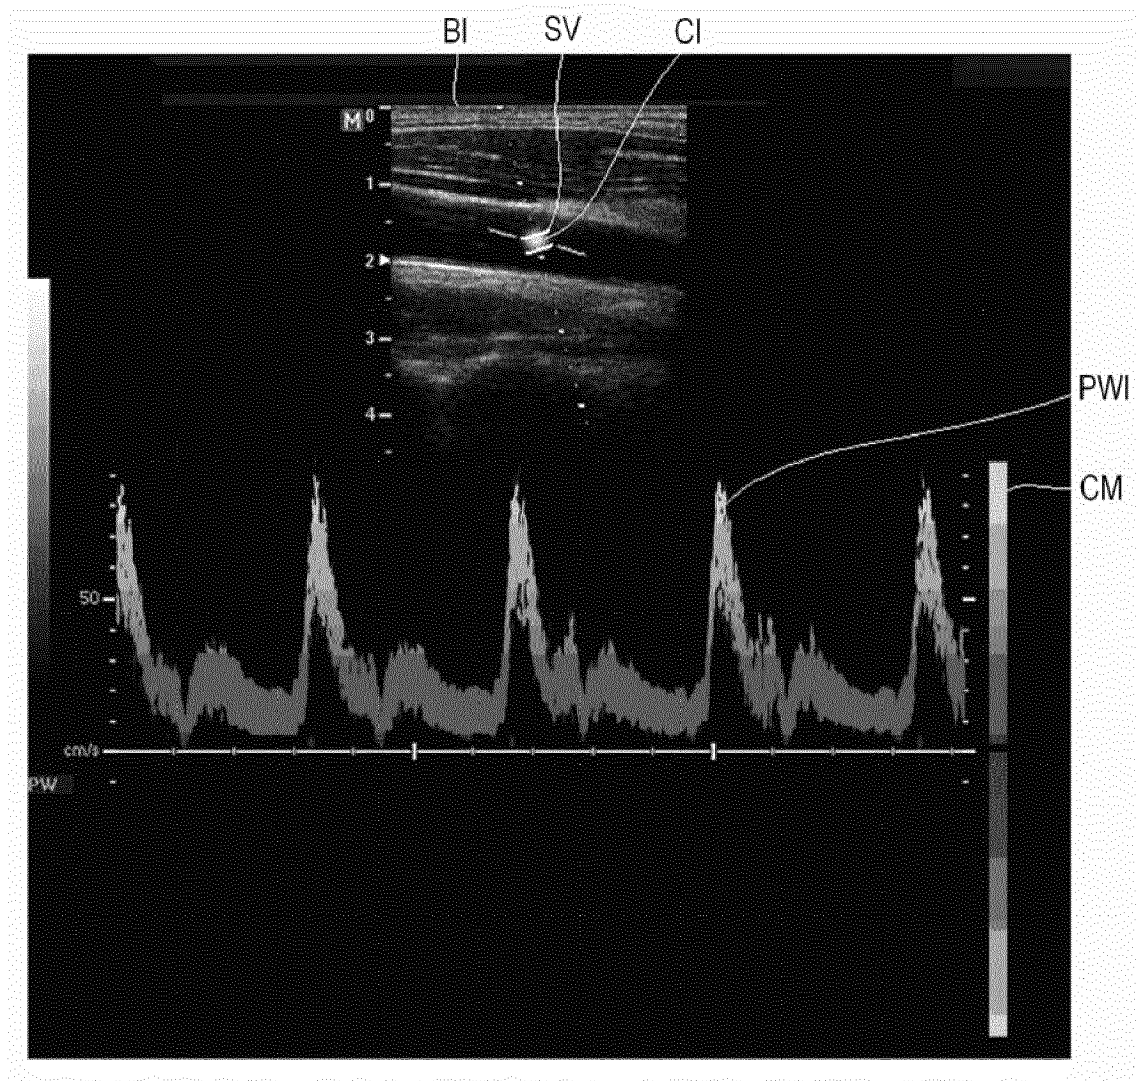


FIG. 6


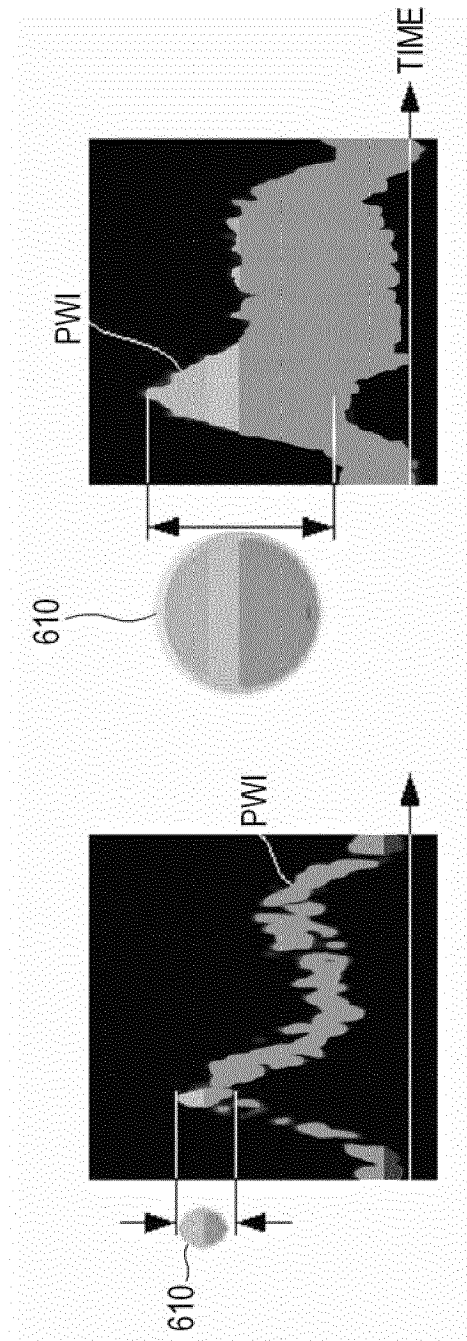


FIG. 7



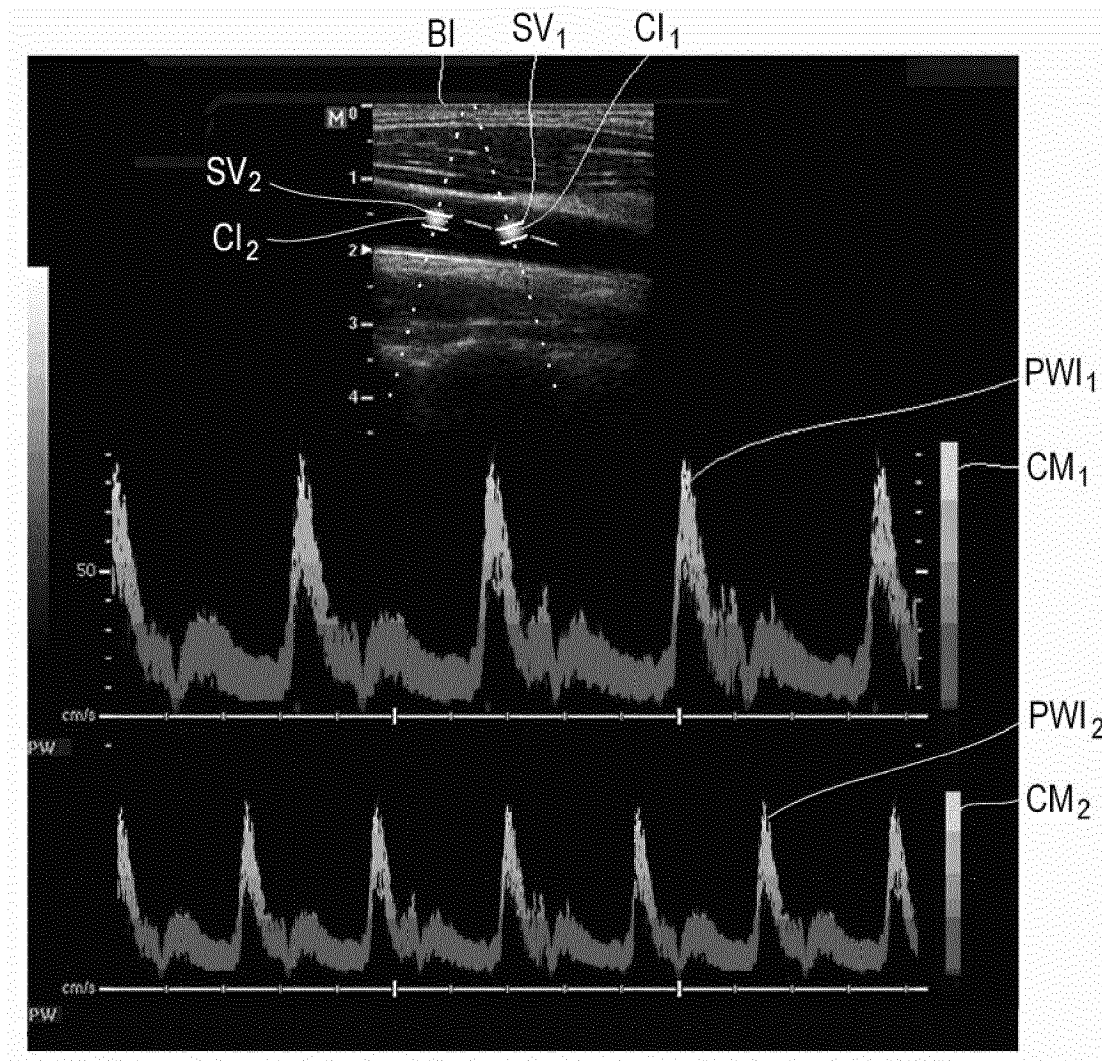

EUROPEAN SEARCH REPORT

Application Number
EP 11 19 1707

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	EP 1 977 694 A1 (MEDISON CO LTD [KR]) 8 October 2008 (2008-10-08)	1-3, 7-10,14	INV. A61B8/06
Y	* paragraphs [0001], [0011] - [0021]; claims; figures *	4-6, 11-13	
Y	----- US 5 709 211 A (MACHIDA ETSURO [JP]) 20 January 1998 (1998-01-20)	4,11	
A	* column 7, line 16 - column 8, line 14; claims; figures *	1-3, 5-10, 12-14	
Y	----- US 6 077 226 A (WASHBURN MICHAEL JOSEPH [US] ET AL) 20 June 2000 (2000-06-20)	5,12	
A	* column 2, line 65 - column 3, line 46; claims; figures * * column 4, line 19 - column 6, line 53 * * column 8, line 33 - line 57 *	1-4, 6-11,13, 14	
Y	----- US 2006/241458 A1 (HAYASHI TETSUYA [JP] ET AL) 26 October 2006 (2006-10-26)	6,13	TECHNICAL FIELDS SEARCHED (IPC) A61B
A	* paragraphs [0005] - [0009]; claims; figures *	1-5, 7-12,14	
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 7 March 2012	Examiner Mundakapadam, S
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

 2
EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 11 19 1707

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

07-03-2012

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 1977694	A1	08-10-2008	EP 1977694 A1	08-10-2008
			JP 2008253784 A	23-10-2008
			KR 20080090888 A	09-10-2008
			US 2008249411 A1	09-10-2008

US 5709211	A	20-01-1998	JP 3514553 B2	31-03-2004
			JP 9010211 A	14-01-1997
			US 5709211 A	20-01-1998

US 6077226	A	20-06-2000	DE 60025438 T2	07-09-2006
			EP 1041395 A2	04-10-2000
			JP 2000300562 A	31-10-2000
			US 6077226 A	20-06-2000
			US 6500122 B1	31-12-2002

US 2006241458	A1	26-10-2006	CN 1826082 A	30-08-2006
			JP 4610011 B2	12-01-2011
			US 2006241458 A1	26-10-2006
			WO 2005006987 A1	27-01-2005

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 1020100123899 [0001]

专利名称(译)	在超声系统中提供与血流变化相对应的附加信息		
公开(公告)号	EP2462872A1	公开(公告)日	2012-06-13
申请号	EP2011191707	申请日	2011-12-02
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	KIM SUNG HEE LEE SUK JIN		
发明人	KIM, SUNG HEE LEE, SUK JIN		
IPC分类号	A61B8/06		
代理机构(译)	SCHMID , WOLFGANG		
优先权	1020100123899 2010-12-07 KR		
其他公开文献	EP2462872B1		
外部链接	Espacenet		

摘要(译)

提供了用于提供附加信息的实施例。在一个实施例中，超声系统（100）包括：超声数据获取单元（120），被配置为获取对应于活体的第一超声数据和第二超声数据；处理单元（130），用于基于所述第一超声数据形成亮度模式图像，在所述亮度模式图像上设置至少一个样本体积，并基于所述第二超声波形成与所述生物体内的血流对应的血流信息对应于所述至少一个样本体积的超声数据，所述处理单元还被配置为基于所述血流信息形成与血流变化相对应的附加信息。

