



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
02.07.2014 Bulletin 2014/27

(51) Int Cl.:
A61B 8/08 (2006.01) A61B 8/00 (2006.01)

(21) Application number: **13194203.9**

(22) Date of filing: **25.11.2013**

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(72) Inventor: **Yoo, Jun Sang**
Suwon-Si, Gyeonggi-Do (KR)

(74) Representative: **Schmid, Wolfgang**
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft
Alte Ulmer Strasse 2
89522 Heidenheim (DE)

(30) Priority: **28.12.2012 KR 20120156147**


(71) Applicant: **Samsung Medison Co., Ltd.**
Gangwon-do 250-870 (KR)

(54) **Ultrasound system and method of controlling the same**

(57) An ultrasound diagnosis apparatus and a method of controlling the same is provided. The apparatus haptically outputs a bio-signal or a movement signal of a target object so that a state of the target object can be felt through tactile sense. The ultrasound diagnosis apparatus includes a signal acquisitioner that acquires an

ultrasound signal of a target object, and a signal generator that generates a bio-signal or movement signal of the target object from the ultrasound signal. A signal converter converts the bio-signal or movement signal of the target object into a sensory signal, and a signal transmitter transmits the sensory signal to a haptic device.

FIG. 2

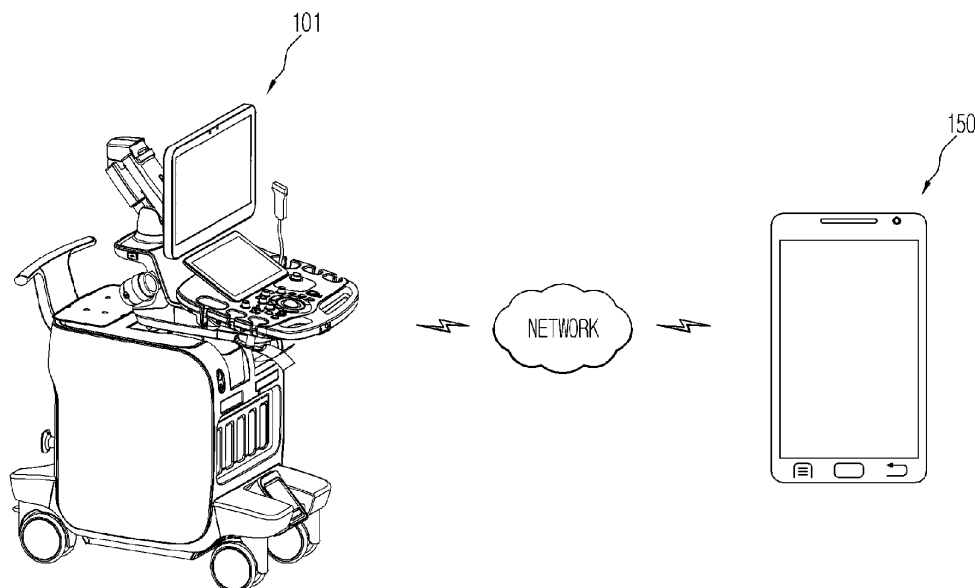

Description

TECHNICAL FIELD

[0001] The present disclosure relates to an ultrasound system to convert an ultrasound signal acquired from a target object into a sensory signal to output the sensory signal, and a method of controlling the ultrasound system.

BACKGROUND

[0002] An ultrasound diagnosis apparatus has been extensively used in the medical field to acquire internal information of a target object due to its non-invasive and nondestructive nature. In particular, the ultrasound diagnosis apparatus may image a state of a fetus to show the image to a pregnant woman or may allow the pregnant woman to listen to the heartbeat of the fetus as a sound using a Doppler signal. A state of the fetus may be diagnosed. Further, the pregnant woman may have a moving experience and develop a bond with the fetus.

[0003] Such a service for providing a sensory output of the state of the fetus is valuable to pregnant women, and thus, there is a need to develop various technologies for providing a haptic output of the state of the fetus as well as an auditory or visual output of the state of the fetus.

SUMMARY

[0004] An aspect of the present disclosure provides an ultrasound system and a method of controlling the same, which convert a bio-signal or a movement signal of a target object into a sensory signal including visual, auditory, and haptic signals to output the sensory signal, and thus, a state of the target object may experience through various senses.

[0005] Additional aspects of the disclosure will be set forth in part in the description which follows and, in part, will be obvious from the description, or may be learned by practice of the disclosure.

[0006] In accordance with an exemplary embodiment of the present disclosure, an ultrasound system includes a signal acquisitioner to acquire an ultrasound signal of a target object. A signal generator generates a bio-signal or a movement signal of the target object from the ultrasound signal. A signal converter converts the bio-signal or the movement signal of the target object into a sensory signal, and a signal transmitter transmits the sensory signal to a haptic device.

[0007] The sensory signal may include a haptic signal.

[0008] The sensory signal may further include an auditory signal.

[0009] The signal transmitter may transmit, as a visual signal, the ultrasound signal and the bio-signal or the movement signal to the haptic device.

[0010] The bio-signal may be a heartbeat signal, and the signal converter may convert the bio-signal of the

target object into a digital signal having signal characteristics of the bio-signal and may convert a pulse signal into the sensory signal.

[0011] The bio-signal may be a heartbeat signal, and the signal converter may convert the bio-signal or the movement signal of the target object into the sensory signal with different intensities according to an intensity of the bio-signal.

[0012] The bio-signal may be a heartbeat signal, and the signal converter may convert the bio-signal or movement signal of the target object into the sensory signal with different output times according to an intensity of the bio-signal.

[0013] The signal generator may generate the movement signal of the target object using a tracking algorithm.

[0014] The ultrasound system may further include an input to set a movement recognition target and a reference line.

[0015] The signal generator may generate the movement signal based on a relationship between the movement recognition target and the reference line.

[0016] The signal generator may generate the movement signal when the movement recognition target and the reference line approach each other such that a distance there between is equal to or less than a preset distance.

[0017] The ultrasound system may further include the haptic device to receive the sensory signal transmitted from the signal transmitter and to haptically and audibly output the sensory signal.

[0018] The ultrasound system may further include an input to set a response sensitivity of the haptic device with respect to the bio-signal or movement signal of the target object.

[0019] The ultrasound system may further include a signal storage to store the sensory signal, wherein the sensory signal stored in the signal storage may be loaded and transmitted to the haptic device through the signal transmitter.

[0020] The haptic device may include a signal receiver to receive the sensory signal from the signal transmitter, a signal storage to store the sensory signal, and an actuator driven according to the sensory signal when the sensory signal stored in the signal storage is loaded.

[0021] In accordance with another aspect of the present disclosure, a method of controlling an ultrasound system includes acquiring an ultrasound signal of a target object and generating a bio-signal or movement signal of the target object from the ultrasound signal. The bio-signal or movement signal of the target object is converted into a sensory signal, and the sensory signal is transmitted to a haptic device.

[0022] The converting of the bio-signal of the target object into the sensory signal may include converting the bio-signal of the target object into a pulse signal, and converting the pulse signal into the sensory signal.

[0023] The bio-signal may be a heartbeat signal, and the converting of the bio-signal of the target object into

the sensory signal may include converting the bio-signal of the target object into the sensory signal with different intensities according to an intensity of the bio-signal.

[0024] The bio-signal may be a heartbeat signal, and the converting of the bio-signal of the target object into the sensory signal may include converting the bio-signal of the target object into the sensory signal with different output times according to an intensity of the bio-signal.

[0025] The generating of the movement signal of the target object may include generating the movement signal of the target object using a tracking algorithm.

[0026] The method may further include setting a movement recognition target and a reference line in order to generate the movement signal of the target object.

[0027] The generating of the movement signal of the target object may include generating the movement signal based on a relationship between the movement recognition target and the reference line.

[0028] The generating of the movement signal of the target object may include generating the movement signal when the movement recognition target and the reference line approach each other such that a distance there between is equal to or less than a preset distance.

[0029] The method may further include receiving the sensory signal through the haptic device and haptically and audibly outputting the sensory signal.

[0030] The method may further include setting a response sensitivity of the haptic device with respect to the bio-signal or movement signal of the target object.

[0031] The method may further include storing the sensory signal, wherein the transmitting of the sensory signal to the haptic device may include loading the sensory signal and transmitting the sensory signal to the haptic device.

[0032] The receiving the sensory signal through the haptic device and the haptically and audibly outputting the sensory signal may include storing the sensory signal, and driving an actuator according to the sensory signal when the sensory signal is loaded.

BRIEF DESCRIPTION OF THE DRAWINGS

[0033] These and/or other aspects of the disclosure will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings.

FIG. 1 is a control block diagram of an ultrasound system according to an embodiment of the present disclosure.

FIG. 2 is a diagram showing an external appearance of an overall structure of an ultrasound system according to an embodiment of the present disclosure.

FIG. 3 is a control block diagram showing a structure of a signal acquisitioner.

FIG. 4 is a diagram showing a fetal heartbeat signal generated by a signal generator.

FIG. 5A is a diagram showing a pulse signal based on a fetal heartbeat signal.

FIG. 5B is a diagram showing a haptic signal converted from a pulse signal.

FIG. 6A is a graph showing a signal with vibration, intensity of which varies according to an intensity of a heartbeat signal.

FIG. 6B is a graph showing a signal with vibration, a period of time of which varies according to an intensity of a heartbeat signal.

FIG. 7 is a control block diagram of an ultrasound system that further includes an input and a display.

FIGS. 8A and 8B are diagrams related to generation of a fetal movement signal.

FIG. 9 is a control block diagram of the ultrasound system to store and load a bio-signal or movement signal of a target object.

FIG. 10 is a flowchart of a method of controlling an ultrasound system, according to an embodiment of the present disclosure.

FIG. 11 is a flowchart of a method of controlling an ultrasound system to express fetal movement using a tracking algorithm and a collision detection algorithm.

DETAILED DESCRIPTION

[0034] Reference will now be made in detail to embodiments of the present disclosure, examples of which are illustrated in the accompanying drawings.

[0035] FIG. 1 is a control block diagram of an ultrasound system 100 according to an embodiment of the present disclosure and FIG. 2 is a diagram showing an external appearance of an overall structure of the ultrasound system 100 according to an embodiment of the present disclosure.

[0036] Referring to FIG. 1, the ultrasound system 100 includes a signal acquisitioner 110 to acquire an ultrasound signal of a target object, and a signal generator 120 to generate a bio-signal or movement signal of the target object from the ultrasound signal. A signal converter 130 converts the bio-signal or movement signal of the target object into a sensory signal, and a signal transmitter 140 transmits the sensory signal to a haptic device 150. A haptic device 150 implements the transmitted sensory signal in a sensory form. Here, the sensory signal may include a haptic signal and may further include an

auditory signal or visual signal as necessary.

[0037] The signal acquisitioner 110, the signal generator 120, the signal converter 130, and the signal transmitter 140 may be included in an ultrasound diagnosis apparatus 101. Thus, referring to FIG. 2, the haptic device 150 is connected to the ultrasound diagnosis apparatus 101 through a wireless or wired network to receive the haptic signal.

[0038] The haptic device 150 includes a signal receiver 151 to receive the haptic signal and an actuator 153 driven according to the received haptic signal. The haptic device 150 may be a device realized by adding a haptic function to a portable device such as a portable phone or a separate device to provide haptic feedback. Thus, the haptic device 150 may be any device to provide haptic feedback by driving the transmitted haptic signal, and thus, a type thereof is not particularly limited.

[0039] FIG. 3 is a control block diagram showing a structure of the signal acquisition unit 110. Referring to FIG. 3, the signal acquisitioner 110 includes a transmission signal generator 111 to generate a transmission signal to be transmitted to the target object. An ultrasound probe 112 receives the transmission signal from the transmission signal generator 111, converts the transmission signal into an ultrasound signal, and transmits and receives the ultrasound signal to and from the target object. A beam former 113 receives an ultrasound echo signal from the ultrasound probe 112 to generate a receiving focus signal.

[0040] The ultrasound probe 112 includes a plurality of transducers to interconvert the ultrasound signal and an electrical signal, and a driver to drive a transducer to swing. The driver may be a stepping motor for control of a rotation angle. When the transmission signal is transmitted from the transmission signal generator 111, the transducer converts the transmitted transmission signal into an ultrasound signal to transmit the ultrasound signal to the target object and receives an ultrasound echo signal reflected by the target object to generate a receiving signal. In this case, the receiving signal is an analog signal.

[0041] In detail, the ultrasound probe 112 appropriately delays an input time of pulses to each transducer to transmit focused ultrasound beams to the target object along a transmission scan line. Ultrasound echo signals reflected by the target object are input to each transducer at different receiving times and each transducer outputs the input ultrasound echo signals.

[0042] When the ultrasound probe 112 transmits ultrasound waves, the beam former 113 adjusts driving timing of each transducer of the ultrasound probe 112 to focus the ultrasound waves at a specific location. When the receiving signal is transmitted from the ultrasound probe 112, the beam former 113 converts the analog receiving signal into a digital signal. In addition, the beam former 113 focuses the digital signal to generate the receiving focus signal in consideration of a position and focusing point of the transducer. Hereinafter, the ultrasound signal

according to the above-described embodiment may be the receiving focus signal output from the beam former 113 or an ultrasound image signal on which an imaging process is performed in order to image the target object.

[0043] The signal generator 120 generates the bio-signal or movement signal of the target object from the ultrasound signal of the target object. Generation of the bio-signal of the target object will be described with regard to an embodiment of the present disclosure.

[0044] FIG. 4 is a diagram showing a fetal heartbeat signal generated by the signal generator 120.

[0045] There are various bio-signals of the target object. For example, when the target object is a fetus, the bio-signal may be a heartbeat signal. In this case, Doppler Effect may be used in order to generate the fetal heartbeat signal from an ultrasound signal. Ultrasound waves irradiated from the ultrasound probe 112 into a human body collide with a moving object inside the human body and are reflected back to the ultrasound probe 112. The irradiated ultrasound waves and the reflected ultrasound waves have different frequencies. Such frequency change is called Doppler shift, and a phenomenon in which the Doppler shift occurs refers to the

[0046] Doppler Effect.

[0047] In detail, ultrasound waves irradiated from the ultrasound probe 112 into the abdomen of a pregnant woman are reflected by a tissue, which moves in synchronization with fetal heartbeat of a heart wall, a blood vessel wall, blood, or the like, back to the ultrasound probe 112, and the frequency of the reflected ultrasound waves is shifted. Thus, the signal generator 120 may extract a signal, the frequency of which is shifted, from the ultrasound signal to generate the fetal heartbeat signal shown in FIG. 4.

[0048] FIG. 5A is a diagram showing a pulse signal based on the fetal heartbeat signal and FIG. 5B is a diagram showing a haptic signal converted from the pulse signal.

[0049] The signal converter 130 converts the heartbeat signal of FIG. 4 into the haptic signal. Referring back to FIG. 4, the fetal heartbeat signal has periodicity according to ventricular systole. Thus, the signal converter 130 may generate a simple digital signal shown in FIG. 5A, for example, a pulse signal based on ventricular systole indicated in the heartbeat signal. The digital signal contains the characteristics of the heartbeat signal.

[0050] In addition, the signal converter 130 generates the haptic signal shown in FIG. 5B based on the generated pulse signal. The haptic signal is a signal to drive the haptic device 150 to vibrate or provide haptic feedback. The signal transmitter 140 transmits the haptic signal to the haptic device 150 through a wired or wireless network. In addition, the haptic signal is used to provide haptic feedback through the haptic device 150.

[0051] The haptic sense may include all senses obtained from external mechanical, thermal, chemical, and electric stimuli applied to skin, muscle, tendon, and joint of a human body and may be classified into tactile sense

and kinesthetic sense.

[0052] The tactile sense is the sense of touch where the geometric shape, roughness, temperature, and slip of a contact surface are recognized via sense of the skin spread in or around the knuckle, palm, or the like. The kinesthetic sense is the sense of touch where total contact force, flexibility, weight, or the like is recognized via proprioception of bone and joint as well as muscle of the fingers, wrists, arms, or the like.

[0053] As an example, when the haptic device 150 vibrates according to the haptic signal shown in FIG. 5B, a user may feel the fetal heartbeat through the vibration.

[0054] The haptic device 150 may provide other feedback such as visual and auditory feedback together with the haptic feedback. To this end, the signal converter 130 may convert the heartbeat signal that is a bio-signal into an auditory signal and may transmit the converted auditory signal to the haptic device 150 through the signal transmitter 140. In addition, the haptic device 150 may output fetal heartbeat sound through a speaker.

[0055] In addition, the ultrasound signal, that is, a fetus image signal acquired by the signal acquisitioner 110 may also be transmitted to the haptic device 150 through the signal transmitter 140. The haptic device 150 may visually output the transmitted fetus image signal. In addition, a Doppler signal generated by the signal generator 120 may also be transmitted to the haptic device 150 through the signal transmitter 140 and may be output in the form of graph through a display. In this regard, when the Doppler signal is output together with the fetus image signal, the image shown in FIG. 4A may be output through the haptic device 150. However, embodiments of the present disclosure are not limited thereto, and any visual signal related to a state of the fetus may be output through the haptic device 150.

[0056] FIG. 6A is a graph showing a signal with vibration, the intensity of which varies according to an intensity of a heartbeat signal. FIG. 6B is a graph showing a signal with vibration, a period of time of which varies according to an intensity of a heartbeat signal.

[0057] The haptic signal of FIG. 5B indicates only a period of a fetal heartbeat signal. In an ultrasound system according to an embodiment of the present disclosure, the intensity of the fetal heartbeat as well as a period of the fetal heartbeat may be haptically expressed. As an example, the intensity of the vibration signal may vary according to the intensity of the fetal heartbeat signal, as shown in FIG. 6A. Thus, the haptic device 150 outputs the vibration signal, the intensity of which is increased as the intensity of the fetal heartbeat is increased.

[0058] As another example, a period of time when vibration occurs may vary according to the intensity of the fetal heartbeat signal, as shown in FIG. 6B. Thus, the haptic device 150 outputs the vibration signal, a period of time of which is increased as the intensity of the fetal heartbeat is increased.

[0059] The haptic device 150 may express the fetal heartbeat through kinesthetic sense as well as haptic

sense such as the aforementioned vibration. As an example, the haptic device 150 may adopt a method in which liquid is concentrated on a specific location of the haptic device 150 to expand. In this regard, the fetal heartbeat may be expressed by repeating expansion and contraction according to the haptic signal shown in FIG. 5B. The location where liquid is concentrated may be a location within a user's reach, a heart location of a fetus image displayed on a display of the haptic device 150, or an arbitrary location determined by the user.

[0060] In addition, it may be possible to express only a period of the fetal heartbeat according to the signal shown in FIG. 5B, to express liquid with different expansion degrees according to the intensity of the fetal heartbeat using the signal shown in FIG. 6A, or to express liquid with different expansion times according to the intensity of the fetal heartbeat using the signal shown in FIG. 6B.

[0061] As described above, an auditory signal may also be output through the haptic device 150. In this regard, the fetal heartbeat may be audibly expressed, that is, may be expressed as a sound together with haptic sense. In this case, the sound with different intensities or different output times may be expressed according to the intensity of the fetal heartbeat.

[0062] The embodiments described with reference to FIGS. 4 through 6 relate to an ultrasound system to express fetal heartbeat through senses such as haptic sense or the like when a target object is a fetus. Hereinafter, an ultrasound system to express movement of a fetus (i.e., fetal movement) through senses such as haptic sense or the like will be described.

[0063] FIG. 7 is a control block diagram of an ultrasound system that further includes an input 160 and a display 170, and FIGS. 8A and 8B are diagrams related to generation of a fetal movement signal.

[0064] Referring to FIG. 7, the ultrasound system 100 described with reference to FIG. 1 may further include the input 160 to receive a user's command related to signal generation, and the display 170 displays an internal image of a target object. The signal generator 120 may generate the fetal movement signal. To this end, for example, a tracking algorithm or a collision detection algorithm may be used.

[0065] The ultrasound signal acquired by the signal acquisitioner 110 may include a two-dimensional or three-dimensional ultrasound signal of the fetus. As shown in FIG. 8A, when the fetus ultrasound signal acquired by the signal acquisitioner 110 is output through the display 170, the user sets a reference line and a movement recognition target through the input 160. The input 160 may be implemented as a keyboard, a trackball, a mouse, a touch panel, or the like. When the display 170 is implanted as a touchscreen, the touchscreen may perform functions of both the display 170 and the input 160.

[0066] The input 160 and the display 170 may be included in the ultrasound diagnosis apparatus 101 or the haptic device 150, or may be included in each of the

ultrasound diagnosis apparatus 101 and the haptic device 150.

[0067] The signal generator 120 may recognize movement of the movement recognition target in real time using a tracking algorithm such as particle tracking, Kalman tracking, Blob detection, or the like.

[0068] In addition, the signal generator 120 determines whether a relationship between the reference line and the movement recognition target satisfies a preset condition. Here, the preset condition is a condition to determine whether the movement recognition target moves based on the reference line. For example, a case in which the reference line and the movement recognition target approach each other such that a distance there between may be equal to or less than a preset distance, or a case in which the movement recognition target reaches the reference line may be set as a condition for generation of a haptic signal.

[0069] For example, in the latter case, when movement of the movement recognition target is tracked in real time, if the movement recognition target reaches, that is, collides with the reference line, as shown in FIG. 8B, the signal generator 120 generates a movement signal indicating the fetal movement and the signal converter 130 converts the movement signal into the haptic signal such as a vibration signal and transmits the haptic signal to the haptic device 150 through the signal transmitter 140.

[0070] The signal converter 130 may convert the fetal movement signal into an auditory signal and transmit the auditory signal to the haptic device 150 through the signal transmitter 140. In this case, the auditory signal may be a signal indicating collision of the movement recognition target with the reference line or other signals from which the fetal movement may be detected.

[0071] In addition, a fetus ultrasound image or a fetal movement image shown in FIGS. 8A and 8B may also be transmitted to the haptic device 150 and may be visually output through a display of the haptic device 150.

[0072] FIG. 9 is a control block diagram of the ultrasound system 100 to store and load a bio-signal or movement signal of a target object.

[0073] The ultrasound system 100 according to an embodiment of the present disclosure may store the bio-signal or the movement signal of the target object and may reload and output the bio-signal or movement signal as necessary. The ultrasound system 100 may further include a signal storage 180 to store a sensory signal converted by a signal converter 130, and the haptic device 150 may further include a signal storage 152 to store the sensory signal transmitted thereto.

[0074] The user may store the fetus ultrasound image and sensory signal acquired during diagnosis of a pregnant woman in the signal storage 180. When the user wants to recheck a state of the fetus or the pregnant woman wants to re-feel the fetal movement, the user may load and output the fetus ultrasound image and sensory signal.

[0075] In addition, when the haptic device 150 is im-

plemented as a portable device such as a portable phone, the pregnant woman may receive the fetus ultrasound image and the sensory signal from the ultrasound diagnosis apparatus 101 and store the fetus ultrasound image and the sensory signal in the signal storage 152, and then load the fetus ultrasound image and the sensory signal and allow the sensory signal to be output through tactile sense such as vibration or the like through the haptic device 150 whenever she wants to feel the fetal movement.

[0076] As another method of haptically outputting movement of the target object, a movement oscillation wave is output along the movement of the target object. When this method is used, the haptic signal may be output such that vibration may flow along the movement of the target object.

[0077] In detail, when the target object is a fetus, if the fetus ultrasound image acquired by the signal acquisitioner 110 and the haptic signal generated by the signal converter 130 are transmitted to the haptic device 150, the fetus ultrasound image is displayed on the display 170 included in the haptic device 150 and the haptic signal is output as the movement oscillation wave in synchronization with the fetal movement of the fetus ultrasound image displayed on the display 170. That is, the vibration output through the display 170 may flow on a surface of the display 170 in synchronization with the fetal movement. In this case, the pregnant woman may more dynamically feel the fetal movement.

[0078] Response sensitivity may be set through the input 160 and refers to a degree by which the haptic device 150 responds to the bio-signal or movement signal of the target object. When the response sensitivity is set low, haptic sense is output low, and when the response sensitivity is set high, the haptic sense is output high.

[0079] In addition, it may be possible to determine a location of the target object where the bio-signal is generated, through the input 160. For example, when a fetal heartbeat signal is generated using the Doppler Effect, the location of the fetus heart may be automatically set by determining a location where frequency shift occurs, or alternatively, the user may directly set the location of the fetus heart through the input 160 by viewing the fetus ultrasound image.

[0080] In the above-described embodiments of the present disclosure, the signal converter 130 is included in the ultrasound diagnosis apparatus 101, which is merely an embodiment of the present. Alternatively, the signal converter 130 may be included in the haptic device 150. In this case, when the signal generator 120 generates the bio-signal or movement signal of the fetus and transmits the bio-signal or movement signal to the haptic device 150, the haptic device 150 may convert the bio-signal or movement signal into a sensory signal, such as, a haptic signal, a visual signal, an auditory signal, and the like.

[0081] Hereinafter, a method of controlling an ultrasound system will be described with regard to an embod-

iment of the present disclosure with reference to a flow-chart.

[0082] FIG. 10 is a flowchart of a method of controlling an ultrasound system, according to an embodiment of the present disclosure. For detailed description, in an embodiment of the present disclosure, a case in which a target object is a fetus will be described.

[0083] Referring to FIG. 10, an ultrasound signal of the fetus is acquired (311). The ultrasound signal may be acquired using a general method of acquiring an ultrasound signal by bringing an ultrasound probe into contact with the abdomen of a pregnant woman.

[0084] A fetal heartbeat signal or a movement signal is generated from the acquired ultrasound signal (312). The fetal heartbeat signal may be generated using the Doppler Effect. In this regard, the fetal heartbeat signal may be generated by extracting a signal, the frequency of which is shifted, from the ultrasound signal. The fetal movement signal will be described below.

[0085] In addition, the fetal heartbeat signal or the movement signal is converted into a sensory signal (313). When the heartbeat signal is converted, the heartbeat signal is converted into a simple signal such as a pulse signal. Then, the pulse signal may be converted into the sensory signal. The sensory signal may be a haptic signal such as vibration or may include the haptic signal and a visual signal or an auditory signal. In addition, the sensory signal may be stored, and then, may be loaded and transmitted to a haptic device as necessary.

[0086] When the converted haptic signal is transmitted to the haptic device (314), an actuator of the haptic device operates according to the sensory signal (315). For example, when the sensory signal is a haptic signal and the haptic device is a device that vibrates according to the haptic signal, the haptic device may vibrate according to the operation of the actuator, and a user may feel fetal heartbeat or fetal movement through the vibration.

[0087] As another example, the fetal heartbeat may be expressed by concentrating liquid on a specific location of the haptic device and repeating expansion and contraction according to the haptic signal.

[0088] If the sensory signal further includes a visual signal or an auditory signal, the visual signal may be output through a display included in the haptic device or the auditory signal may be output through a speaker. The visual signal may be a Doppler signal that is expressed in the form of fetus image signal or graph and the auditory signal may indicate heartbeat as a sound.

[0089] In this case, the user may set a response sensitivity. In addition, the haptic device may adjust an intensity of the sensory signal according to the set response sensitivity and may output the sensory signal. The sensory signal transmitted to the haptic device may be stored in the haptic device, and then, may be loaded to drive the actuator as necessary.

[0090] FIG. 11 is a flowchart of a method of controlling an ultrasound system to express fetal movement using a tracking algorithm and a collision detection algorithm.

Referring to FIG. 11, a reference line for recognition of movement and a movement recognition target, movement of which is to be recognized are set (321). An ultrasound image of a target object may be displayed, and a user may set the desired reference line and movement recognition target on the displayed ultrasound image. In this case, a display for displaying the ultrasound image and an input used for user setting may be included in the ultrasound diagnosis apparatus or may be included in the haptic device.

[0091] When the setting is completed, movement of the set target object is tracked in real time (322). The movement of the movement recognition target may be tracked using a tracking algorithm such as particle tracking, Kalman tracking, Blob detection, or the like.

[0092] A haptic signal is generated based on a relationship between the reference line and the movement recognition target (323). As an example, when the relationship between the reference line and the movement recognition target satisfies a preset condition, a signal indicating that the movement recognition target moves, that is, a movement signal may be generated. The preset condition is a condition to determine whether the movement recognition target moves based on the reference line. For example, a case in which the reference line and the movement recognition target approach each other such that a distance there between may be equal to or less than a preset distance, or a case in which the movement recognition target reaches the reference line may be set as a condition for generation of the movement signal. In addition, the movement signal is converted into the haptic signal.

[0093] When the haptic signal is transmitted to the haptic device (324), the actuator of the haptic device operates according to the haptic signal (326). For example, when the haptic device is a device that vibrates according to the haptic signal, the haptic device may vibrate according to the operation of the actuator, and the user may feel fetal movement through the vibration.

[0094] The fetal movement signal may be converted into an auditory signal and may be transmitted to the haptic device 150 through the signal transmitter 140. Here, the auditory signal may be a signal indicating collision of the movement recognition target with the reference line or other sounds via which fetal movement may be detected. In addition, a fetus ultrasound image or a fetal movement image may also be transmitted to the haptic device 150 or may be visually output through a display of the haptic device 150.

[0095] As is apparent from the above description, a state of a target object may be felt through various senses such as visual, auditory, and haptic senses. In particular, when the target object is a fetus, a pregnant woman may feel fetal heartbeat or fetal movement through various senses such as visual, auditory, and haptic senses, thereby increasing the link between the fetus and the pregnant woman. In addition, fetal heartbeat or fetal movement may be implemented in a place such as a

home rather than a hospital.

[0096] Although a few embodiments of the present disclosure have been shown and described, it would be appreciated by those skilled in the art that changes may be made in these embodiments without departing from the principles and spirit of the disclosure, the scope of which is defined in the claims and their equivalents.

Claims

1. An ultrasound system comprising:

a signal acquisition unit to acquire an ultrasound signal of a target object;
a signal generation unit to generate a bio-signal or movement signal of the target object from the ultrasound signal;
a signal conversion unit to convert the bio-signal or movement signal of the target object into a sensory signal; and
a signal transmission unit to transmit the sensory signal to a haptic device.

2. The ultrasound system according to claim 1, wherein the sensory signal comprises a haptic signal or an auditory signal.

3. The ultrasound system according to claim 2, wherein the signal transmission unit transmits, as a visual signal, the ultrasound signal and the bio-signal or the movement signal to the haptic device.

4. The ultrasound system according to claim 2 wherein the signal conversion unit converts the bio-signal of the target object into a pulse signal and converts the pulse signal into the haptic signal and the auditory signal.

5. The ultrasound system according to claim 2, wherein the bio-signal is a heartbeat signal, and wherein the signal conversion unit converts the bio-signal or movement signal of the target object into the haptic signal and the auditory signal with different intensities according to intensity of the bio-signal or output times according to intensity of the bio-signal.

7. The ultrasound system according to claim 2, wherein the signal generation unit generates a movement signal of the target object using a tracking algorithm, and further comprising an input unit to set a movement recognition target and a reference line.

8. The ultrasound system according to claim 7, wherein the signal generation unit generates a movement signal based on a relationship between the movement recognition target and the reference

line, and

wherein the signal generation unit generates the movement signal when the movement recognition target and the reference line approach each other such that a distance there between is equal to or less than a preset distance.

9. The ultrasound system according to claim 3, further comprising a haptic device to receive the sensory signal transmitted from the signal transmission unit and to haptically and audibly output the sensory signal.

10. The ultrasound system according to claim 9, wherein the haptic device visually outputs the ultrasound signal and the bio-signal or the movement signal.

11. The ultrasound system according to claim 10, further comprising an input unit to set response sensitivity of the haptic device with respect to the bio-signal or movement signal of the target object.

12. The ultrasound system according to claim 1, further comprising a storage unit to store the sensory signal, wherein the sensory signal stored in the storage unit is loaded and transmitted to the haptic device through the signal transmission unit.

13. The ultrasound system according to claim 9, wherein the haptic device comprises:

a signal receiving unit to receive the sensory signal from the signal transmission unit;
a storage unit to store the sensory signal; and
an actuator driven according to the sensory signal when the sensory signal stored in the storage unit is loaded.

14. A method of controlling an ultrasound system, the method comprising:

acquiring an ultrasound signal of a target object;
generating a bio-signal or movement signal of the target object from the ultrasound signal;
converting the bio-signal or movement signal of the target object into a sensory signal; and
transmitting the sensory signal to a haptic device.

15. The method according to claim 14, wherein the sensory signal comprises a haptic signal or an auditory signal.

FIG. 1

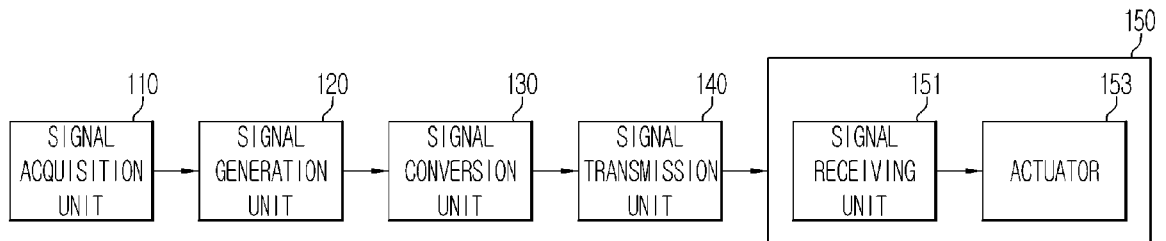


FIG. 2

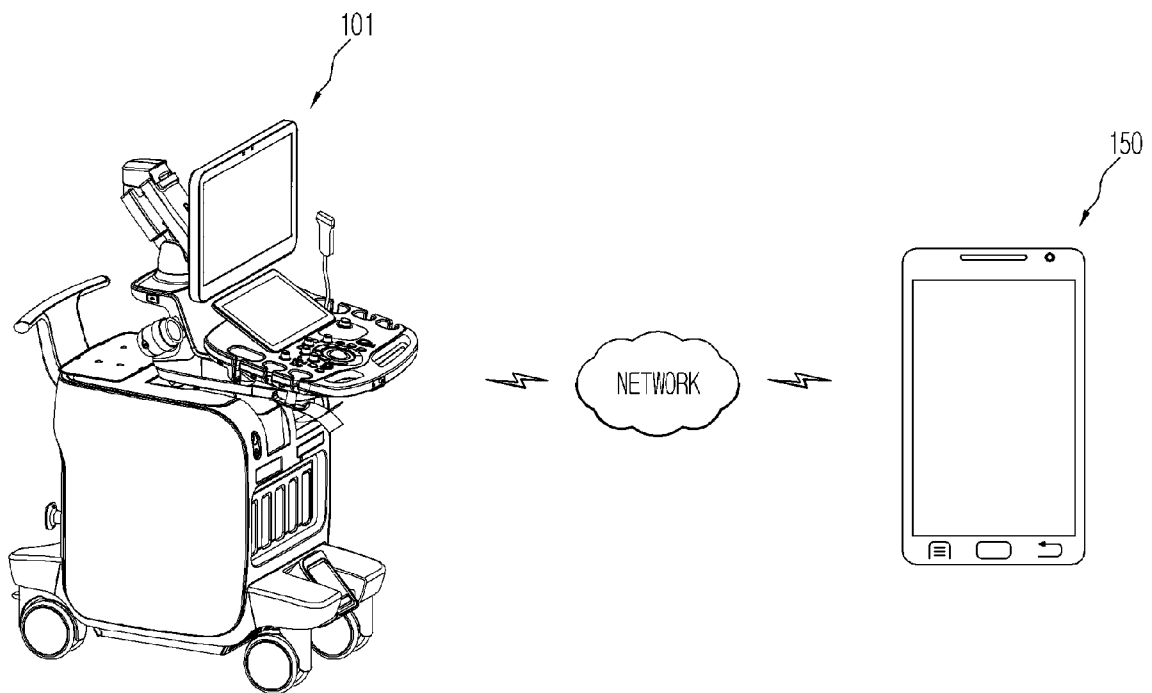


FIG. 3

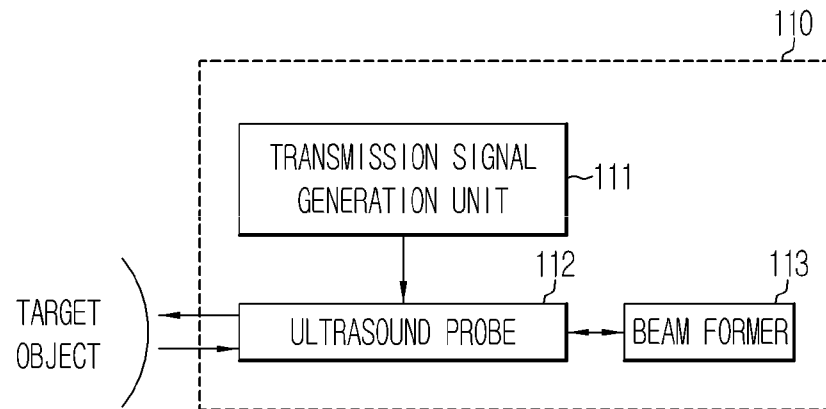


FIG. 4

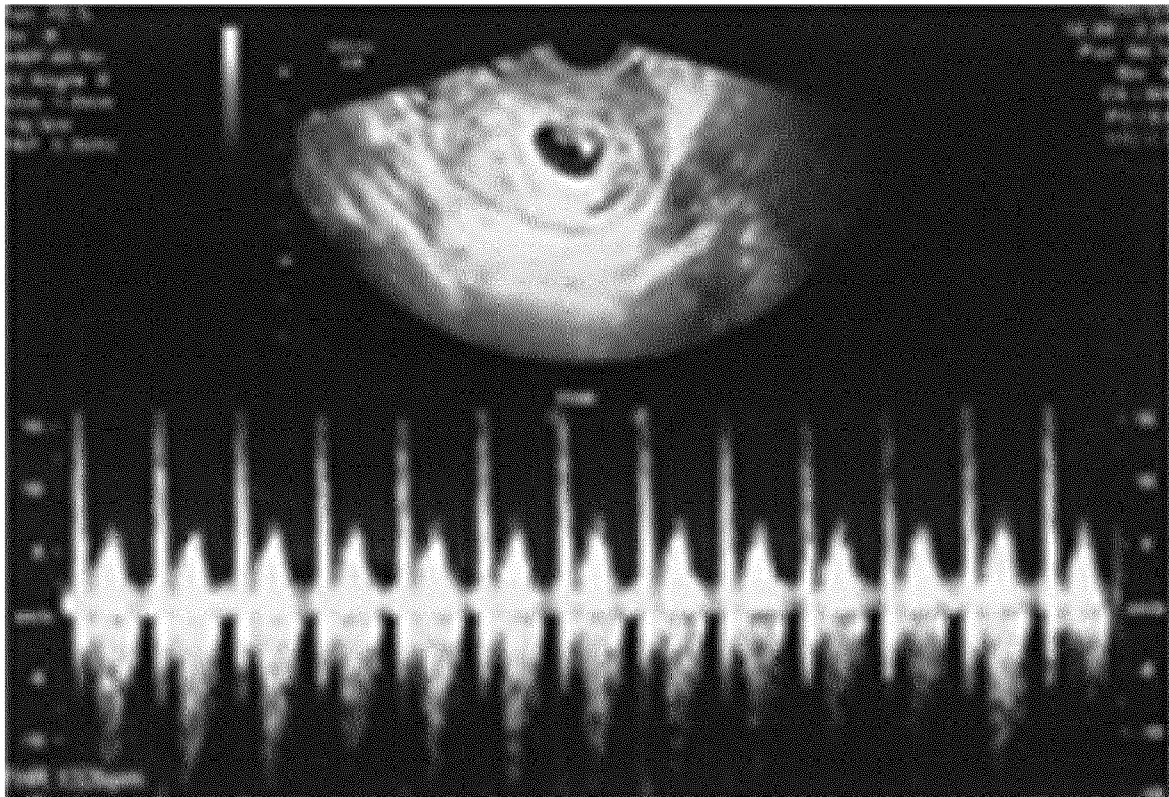


FIG. 5A

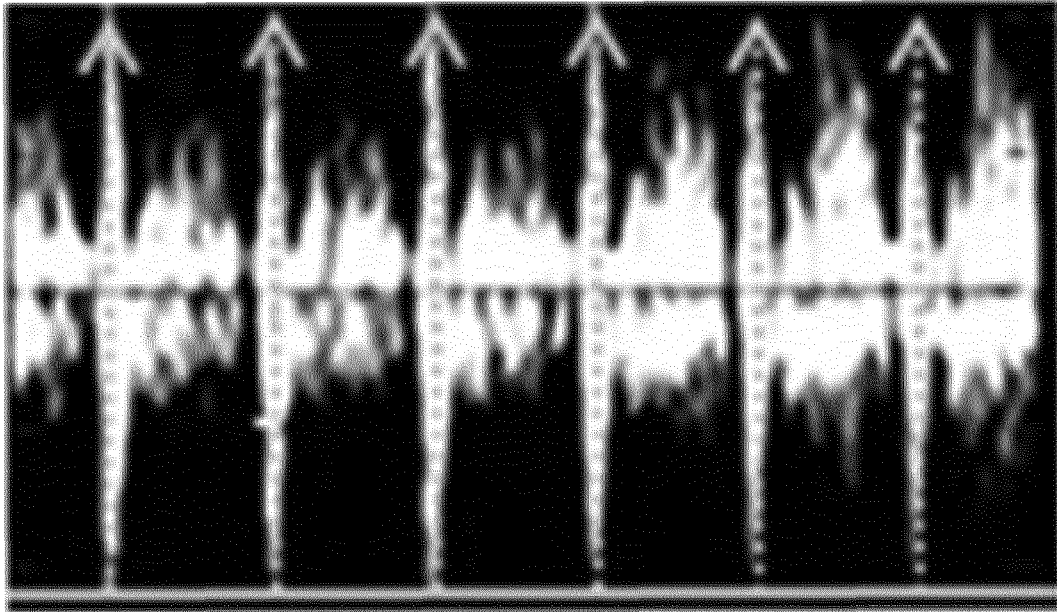


FIG. 5B

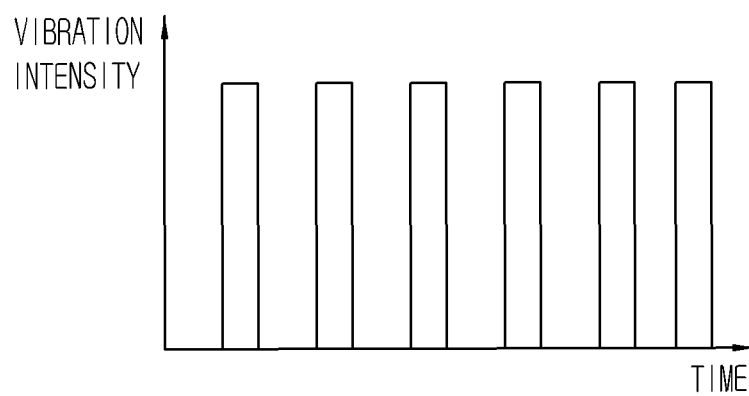


FIG. 6A

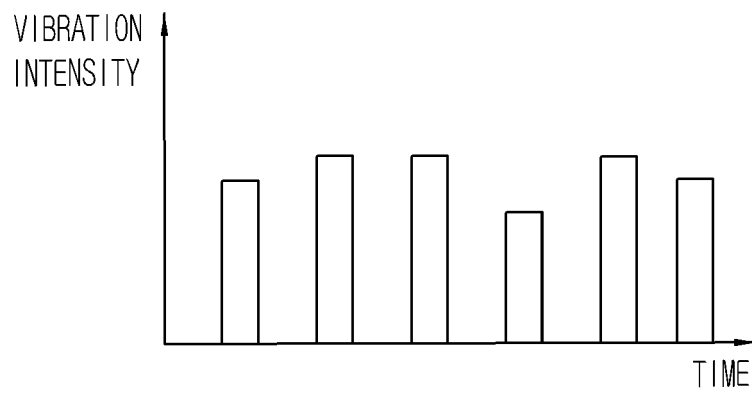


FIG. 6B

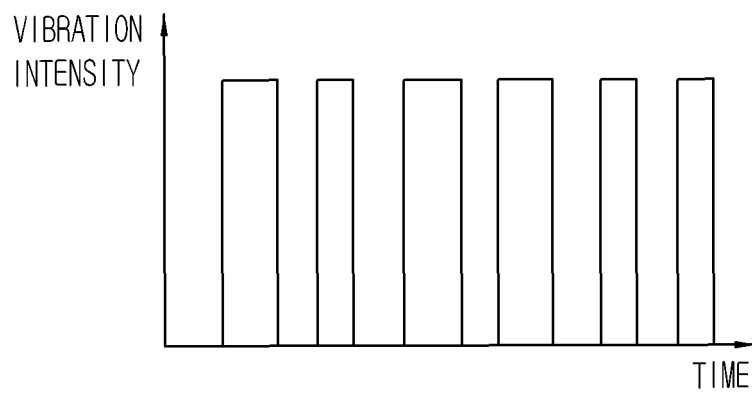


FIG. 7

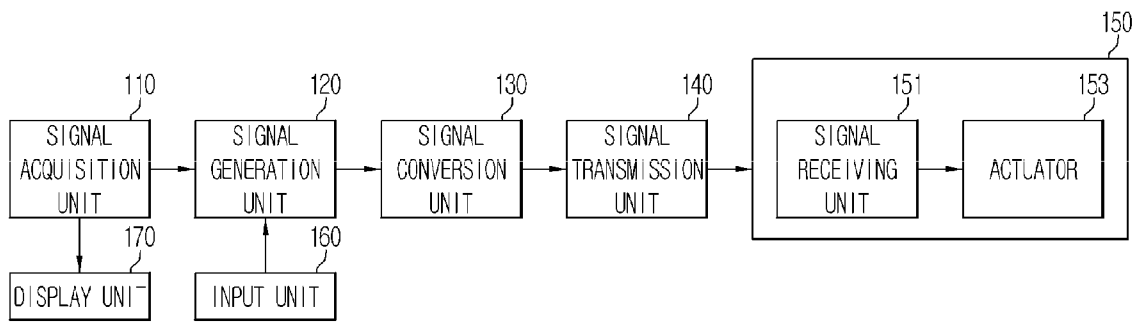


FIG. 8A

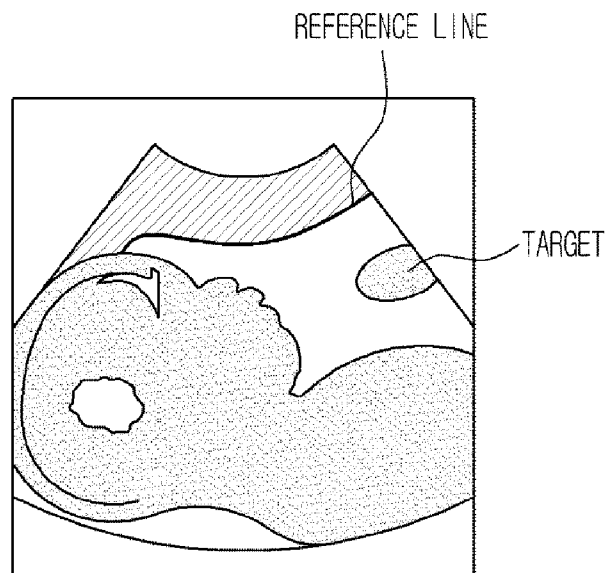


FIG. 8B

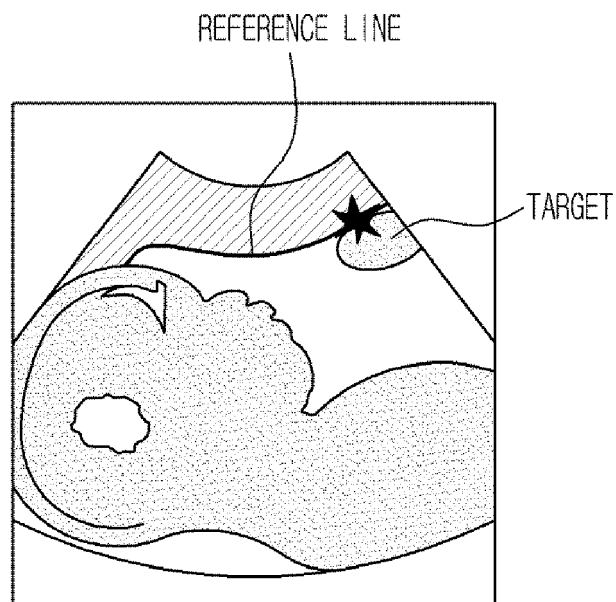


FIG. 9

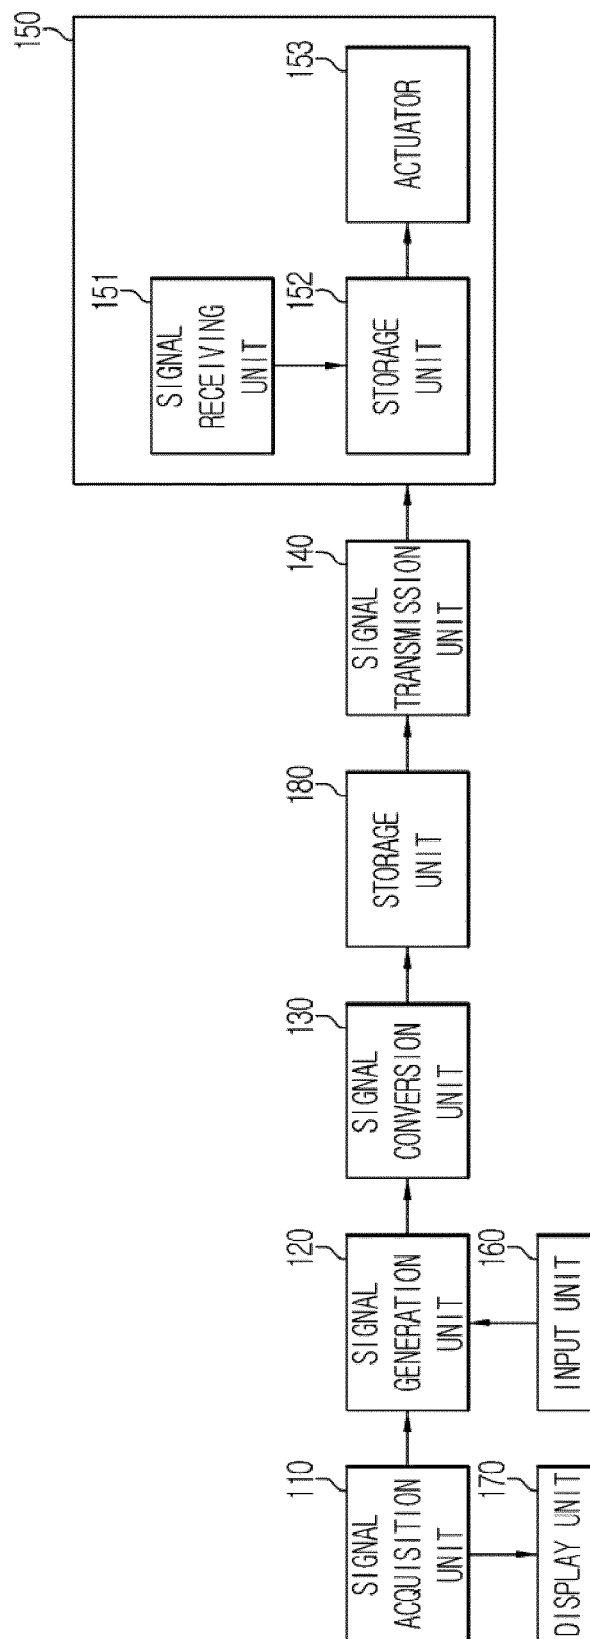


FIG. 10


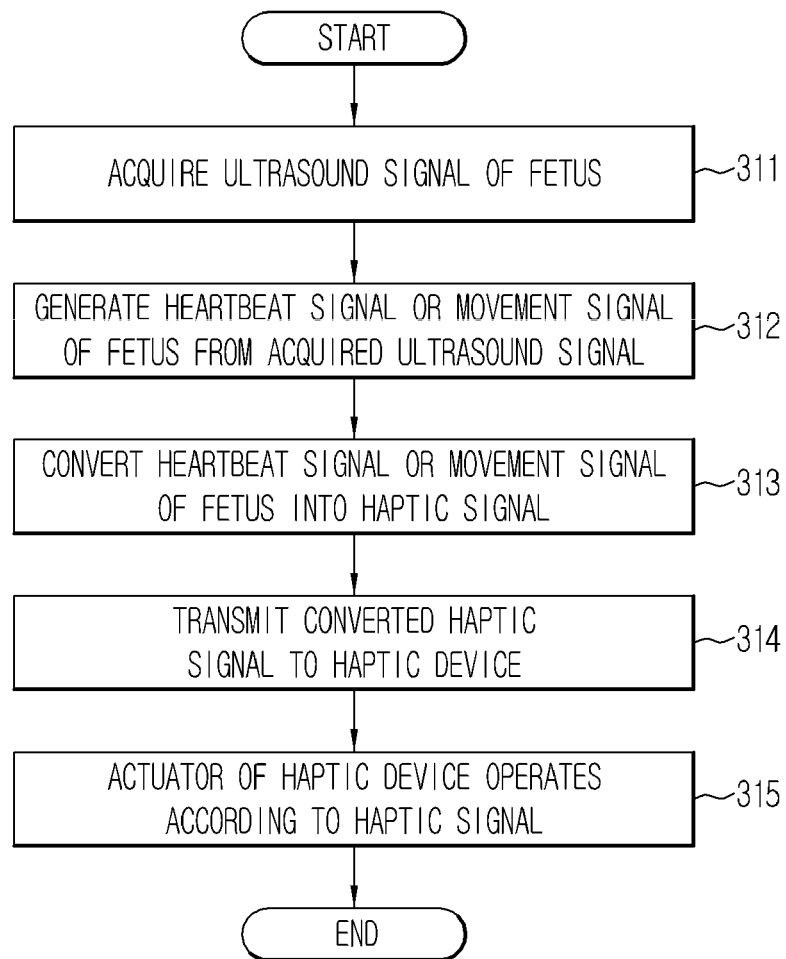


FIG. 11



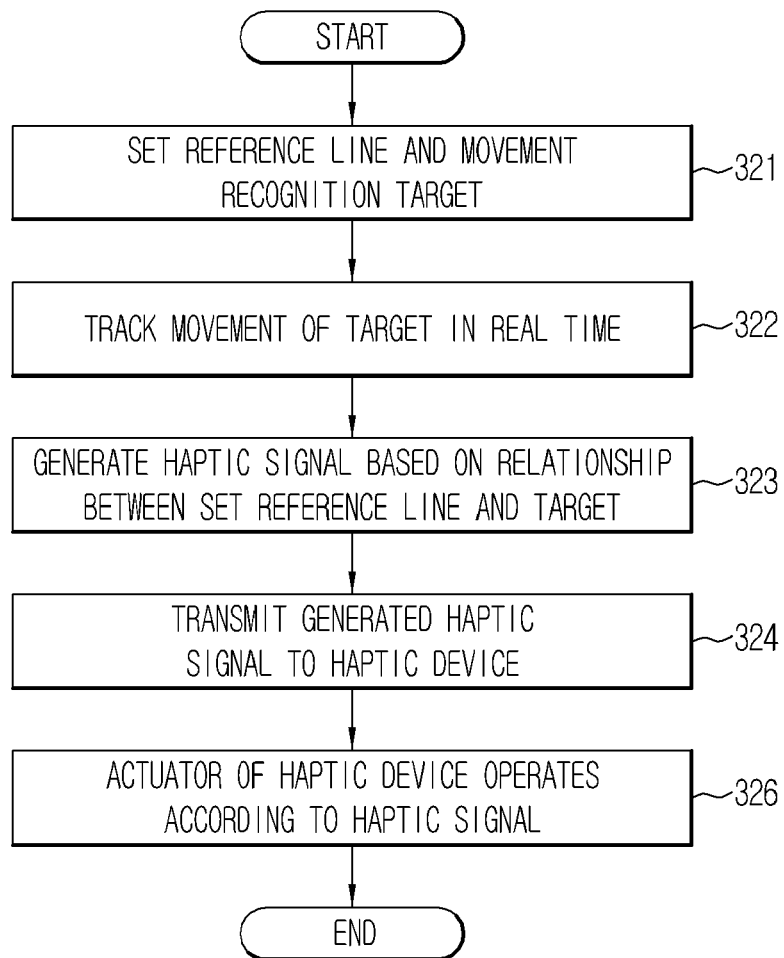

EUROPEAN SEARCH REPORT

Application Number
EP 13 19 4203

5

10

15

20

25

30

35

40

45

50

55

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	WO 2005/110236 A1 (MATERNUS PARTNERS LTD [US]; WATSON RICHARD L JR [US]) 24 November 2005 (2005-11-24) * figures 6,7,14 *	1,2,4,5,9,11-15	INV. A61B8/08 A61B8/00
X	US 2010/274145 A1 (TUPIN JR JOE PAUL [US] ET AL) 28 October 2010 (2010-10-28) * paragraphs [0061], [0089]; figures 1,6 *	1,2,7-9,14,15	
X	US 2005/124878 A1 (SHARONY REUVEN [IL]) 9 June 2005 (2005-06-09) * paragraph [0025] - paragraph [0032]; figure 1 *	1-3,7-10,14,15	
X	US 4 413 629 A (DURLEY III BENTON A [US]) 8 November 1983 (1983-11-08) * column 4; figure 1 *	1,2,14,15	
			TECHNICAL FIELDS SEARCHED (IPC)
			A61B
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 28 February 2014	Examiner Koprinarov, Ivaylo
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

2

EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 13 19 4203

5

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

28-02-2014

10

15

20

25

30

35

40

45

50

55

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2005110236 A1	24-11-2005	CA 2569409 A1	24-11-2005
		EP 1750587 A1	14-02-2007
		WO 2005110236 A1	24-11-2005

US 2010274145 A1	28-10-2010	CN 102421371 A	18-04-2012
		EP 2421442 A2	29-02-2012
		JP 2012524627 A	18-10-2012
		US 2010274145 A1	28-10-2010
		US 2012041281 A1	16-02-2012
		WO 2010124117 A2	28-10-2010

US 2005124878 A1	09-06-2005	AU 2002317454 A1	21-01-2003
		US 2005124878 A1	09-06-2005
		WO 03003899 A2	16-01-2003

US 4413629 A	08-11-1983	EP 0118417 A1	19-09-1984
		US 4413629 A	08-11-1983
		WO 8303750 A1	10-11-1983

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

专利名称(译)	超声系统及其控制方法		
公开(公告)号	EP2749229A1	公开(公告)日	2014-07-02
申请号	EP2013194203	申请日	2013-11-25
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	YOO JUN SANG		
发明人	YOO, JUN SANG		
IPC分类号	A61B8/08 A61B8/00 A61B8/02		
CPC分类号	A61B8/0866 A61B8/02 A61B8/46 A61B8/462 A61B8/463 A61B8/488 A61B8/565		
代理机构(译)	SCHMID , WOLFGANG		
审查员(译)	KOPRINAROV , IVAYLO		
优先权	1020120156147 2012-12-28 KR		
其他公开文献	EP2749229B1		
外部链接	Espacenet		

摘要(译)

提供了一种超声诊断设备及其控制方法。该装置触觉地输出目标物体的生物信号或运动信号，从而可以通过触觉感觉到目标物体的状态。超声诊断设备包括：信号获取器，其获取目标对象的超声信号；以及信号发生器，其从超声信号生成目标对象的生物信号或运动信号。信号转换器将目标对象的生物信号或运动信号转换为传感信号，并且信号发送器将传感信号发送到触觉设备。

FIG. 2

