



(12) **EUROPEAN PATENT APPLICATION**
published in accordance with Art. 153(4) EPC

(43) Date of publication:
16.03.2016 Bulletin 2016/11

(51) Int Cl.:
A61B 8/12 (2006.01)

(21) Application number: **14850702.3**

(86) International application number:
PCT/JP2014/075599

(22) Date of filing: **26.09.2014**

(87) International publication number:
WO 2015/050050 (09.04.2015 Gazette 2015/14)

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR
Designated Extension States:
BA ME

(72) Inventor: **OKUNO, Yoshiyuki**
Tokyo 151-0072 (JP)

(74) Representative: **Gunzelmann, Rainer**
Wuesthoff & Wuesthoff
Patentanwälte PartG mbB
Schweigerstraße 2
81541 München (DE)

(30) Priority: **01.10.2013 JP 2013206593**


(71) Applicant: **OLYMPUS CORPORATION**
Shibuya-ku
Tokyo 151-0072 (JP)

(54) **ULTRASONIC ENDOSCOPE SYSTEM AND COMMUNICATION METHOD THEREFOR**

(57) An ultrasound endoscope system includes: an ultrasound endoscope including an identification section that stores endoscope state information; a video processor including a first read-out section that reads out the endoscope state information in the identification section in the ultrasound endoscope; an ultrasound observation apparatus including a second read-out section that reads out endoscope state information obtained by a communication section for observation apparatus; and a control section that compares the endoscope state information

obtained by the first read-out section in the video processor and the endoscope state information obtained by the second read-out section in the ultrasound observation apparatus, and performs control for establishing wireless communication between the ultrasound endoscope and the ultrasound observation apparatus only when the endoscope state information obtained by the first read-out section and the endoscope state information obtained by the second read-out section match with each other.

FIG. 1

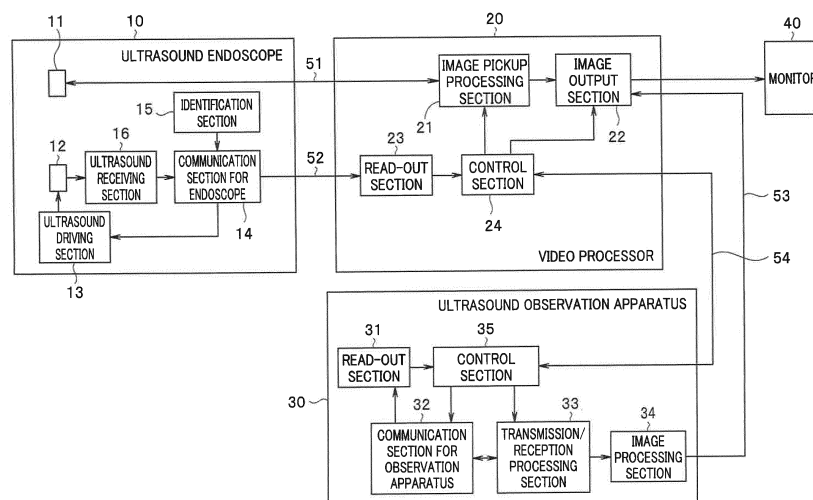

Description

Technical Field

[0001] The present invention relates to an ultrasound endoscope system, connection of which is simplified, and a communication system of the ultrasound endoscope system.

Background Art

[0002] An ultrasound endoscope is capable of outputting an endoscopic image (optical image) obtained by an image pickup device and an ultrasound image obtained by an ultrasound transducer. Output from the ultrasound endoscope is fed to a video processor that processes an optical image, thereby enabling an endoscopic image to be displayed on a monitor. Further, output from the ultrasound endoscope is fed to an ultrasound observation apparatus that processes an ultrasound image, thereby enabling an ultrasound image to be displayed on the monitor. Furthermore, the ultrasound endoscope is connected to both of the video processor and the ultrasound observation apparatus, thereby enabling patient information to be commoditized in the video processor and the ultrasound observation apparatus. Therefore, the examination status for each patient with the use of the endoscopic image and the ultrasound image can be collectively managed. As a result, decision from multifaceted viewpoint is possible in determining a diagnosis policy, which is useful at the time of making diagnosis.

[0003] That is, the video processor and the ultrasound observation apparatus, both of which are connected with the ultrasound endoscope, share setting information and the images each other, thereby capable of managing the examination status in an integrated fashion. For the purpose of such information sharing, the ultrasound endoscope and the respective apparatuses are connected to each other with cables and the like.

[0004] However, the ultrasound endoscope is required to be cleaned after having been used for diagnosis, and at the time of cleaning, the cables used for connecting the ultrasound endoscope with the video processor and the ultrasound observation apparatus have to be removed. Thus, before and after the cleaning processing, the cables connecting the ultrasound endoscope with the video processor and the ultrasound observation apparatus have to be attached to and detached from the ultrasound endoscope, which requires a troublesome operation for an operator.

[0005] Note that Japanese Patent No. 4908897 (hereinafter, referred to as Document 1) proposes a technique of performing wireless communication with an ultrasound probe in an ultrasound observation apparatus for body surface. In the proposal in Document 1, the section that communicates ultrasound signals is configured to be wireless, to eliminate attaching and detaching operations of the cable that connects the section and the ultrasound

observation apparatus, which reduces efforts.

[0006] However, in the proposal in Document 1, the ultrasound probe and the ultrasound observation apparatus are connected to each other on a one-to-one basis, and connection on a one-to-many basis as in the ultrasound endoscope is not taken into consideration. Therefore, even if connection utilizing the proposal in Document 1 is performed, information is not shared in the video processor and the ultrasound observation apparatus, and it is impossible to collectively manage the examination status with the use of endoscopic images and ultrasound images for each patient.

[0007] An object of the present invention is to provide an ultrasound endoscope system capable of reducing efforts in connection operation by establishing wireless communication, and establishing connection among an ultrasound endoscope, a video processor, and an ultrasound observation apparatus, to enable information sharing in these apparatuses, and also provide a communication method of the ultrasound endoscope system.

Disclosure of Invention

Means for Solving the Problem

[0008] An ultrasound endoscope system according to the present invention is an ultrasound endoscope system including: an ultrasound endoscope that is capable of performing optical observation; a video processor for optical observation; and an ultrasound observation apparatus for ultrasound observation, the ultrasound endoscope including: an image pickup section; an ultrasound transducer; an identification section that stores endoscope state information; and a communication section for endoscope that wirelessly transmits and receives an ultrasound signal and the endoscope state information, the video processor including: an optical image processing section that processes an optical image obtained by the image pickup section of the ultrasound endoscope; and a first read-out section that reads out the endoscope state information in the identification section in the ultrasound endoscope, and the ultrasound observation apparatus including: a transmission/reception section that is capable of transmitting and receiving the ultrasound signal; a communication section for observation apparatus that communicates with the communication section for endoscope in the ultrasound endoscope, and transmits and receives the ultrasound signal and the endoscope state information; an ultrasound image processing section that generates an image based on the ultrasound signal obtained by the communication section for observation apparatus; and a second read-out section that reads out the endoscope state information obtained by the communication section for ultrasound observation apparatus, the ultrasound endoscope system further including a control section that compares the endoscope state information obtained by the first read-out section in the video processor and the endoscope state information

obtained by the second read-out section in the ultrasound observation apparatus, and establishes wireless connection between the ultrasound endoscope and the ultrasound observation apparatus only when the endoscope state information obtained by the first read-out section and the endoscope state information obtained by the second read-out section match with each other.

[0009] Furthermore, a communication method of an ultrasound endoscope system according to the present invention is a communication method of an ultrasound endoscope system including an ultrasound endoscope that is capable of performing optical observation; a video processor for optical observation; and an ultrasound observation apparatus for ultrasound observation, the method including: a step in which a first read-out section in the video processor connected to the ultrasound endoscope reads out endoscope state information stored in an identification section in the ultrasound endoscope; a step in which a communication section for observation apparatus in the ultrasound observation apparatus wirelessly communicates with a communication section for endoscope in the ultrasound endoscope and receives the endoscope state information; and a step in which a control section cross-checks the endoscope state information received by the video processor and the endoscope state information received by the communication section for observation apparatus against each other, to perform determination of matching of the pieces of endoscope state information, and performs control for establishing communication between the ultrasound endoscope and the ultrasound observation apparatus when determining that the pieces of endoscope state information match with each other.

Brief Description of the Drawings

[0010]

FIG. 1 is a block diagram for showing an ultrasound endoscope system according to a first embodiment of the present invention.

FIG. 2 is a flowchart for describing an operation in the first embodiment.

FIG. 3 is a block diagram showing a second embodiment of the present invention.

FIG. 4 is a block diagram showing a third embodiment of the present invention.

FIG. 5 is a flowchart for describing an operation in the third embodiment.

Best Mode for Carrying Out the Invention

[0011] Hereinafter, embodiments of the present invention will be described with reference to drawings.

(First Embodiment)

[0012] FIG. 1 is a block diagram showing an ultrasound

endoscope system according to the first embodiment of the present invention. The present embodiment enables the ultrasound endoscope and the ultrasound observation apparatus to be connected to each other by wireless communication.

[0013] In FIG. 1, an ultrasound endoscope 10 and a video processor 20 can be connected to each other with a cable 51. The cable 51 includes, on each of the both ends thereof, a connector not shown, and the connectors are connected respectively with the ultrasound endoscope 10 and the video processor 20, to allow the ultrasound endoscope 10 and the video processor 20 to be connected to each other in detachable manner through the cable 51. On the other hand, the ultrasound endoscope 10 and the ultrasound observation apparatus 30 are connected to each other by wireless communication as described later.

[0014] The ultrasound endoscope 10 includes an image pickup section 11 that obtains optical images. The image pickup section 11 is constituted of a CCD, a CMOS sensor, or the like, and configured to photoelectrically convert an optical image from an object and output the photoelectrically converted optical image as an endoscopic image. The endoscopic image outputted from the image pickup section 11 is fed to an image pickup processing section 21 of the video processor 20 through the cable 51.

[0015] The image pickup processing section 21 of the video processor 20 is controlled by a control section 24, to drive and control the image pickup section 11 of the ultrasound endoscope 10 and output the endoscopic image from the image pickup section 11 to an image output section 22. The image output section 22 is controlled by the control section 24, to perform a predetermined image signal processing on the endoscopic image and output the endoscopic image subjected to the image signal processing to the monitor 40.

[0016] In addition, the image output section 22 receives the ultrasound image from an image processing section 34 in the ultrasound observation apparatus 30 to be described later, through a communication line 53. The image output section 22 is capable of outputting the endoscopic image and the ultrasound image independently to the monitor 40, and also capable of combining the endoscopic image and the ultrasound image, to output the combined image to the monitor 40. The monitor 40 is configured to display the inputted image on a display screen, not shown.

[0017] The ultrasound endoscope 10 includes a transducer 12 for transmitting and receiving ultrasound, an ultrasound driving section 13, and an ultrasound receiving section 16. The ultrasound driving section 13 drives the transducer 12 based on control information fed from a communication section for endoscope 14. The transducer 12 is driven by the ultrasound driving section 13, to repeatedly transmit ultrasound pulses into a living body and receive echoes of the ultrasound pulses reflected from inside of the living body. The ultrasound receiving

section 16 processes a received signal received by the transducer 12, to transmit the processed signal to the communication section for endoscope 14.

[0018] In addition, the ultrasound endoscope 10 is provided with an identification section 15 which stores endoscope-specific information. The identification section 15 is configured to output the endoscope-specific information to the communication section for endoscope 14. The communication section for endoscope 14 is configured to be able to read out the endoscope-specific information stored in the identification section 15 and output the read-out information to a read-out section 23 in the video processor 20 through a cable 52. Note that, the cable 52 is capable of detachably connecting the ultrasound endoscope 10 and the video processor 20 to each other through the use of a connector, not shown. In addition, the cable 51 and the cable 52 may be a common cable. The endoscope-specific information may be transmitted via a connector, not shown, of the cable 52, instead of the cable 51.

[0019] The read-out section 23 of the video processor 20 reads out the endoscope-specific information transmitted from the communication section for endoscope 14 of the ultrasound endoscope 10, to output the read-out information to the control section 24. The control section 24 controls the respective sections in the video processor 20, and communicates with a control section 35 of the ultrasound observation apparatus 30 to be described later, through a communication line 54. That is, the video processor 20 and the ultrasound observation apparatus 30 communicate with each other by wire communication through the communication lines 53, 54. When the ultrasound endoscope 10 is cleaned, the video processor 20 and the ultrasound observation apparatus 30 may remain connected to each other through the communication lines 53, 54.

[0020] In the present embodiment, the ultrasound observation apparatus 30 is provided with a communication section for observation apparatus 32. The communication section for endoscope 14 of the ultrasound endoscope 10 and the communication section for observation apparatus 32 have a wireless communication function, and are capable of communicating wirelessly with each other.

[0021] The communication section for endoscope 14 receives information related to ultrasound driving from the ultrasound observation apparatus 30, and transmits the received signal, which has been received by the transducer 12 and then fed from the ultrasound receiving section 16, to the ultrasound observation apparatus 30. Furthermore, the communication section for endoscope 14 reads out the endoscope-specific information stored in the identification section 15, and transmits the read-out information to the ultrasound observation apparatus 30 by wireless communication.

[0022] A transmission/reception processing section 33 of the ultrasound observation apparatus 30 is controlled by the control section 35, to perform transmission/recep-

tion processing for the ultrasound observation apparatus 30. The communication section for observation apparatus 32 is controlled by the transmission/reception processing section 33, to receive an ultrasound image and transmit the information for ultrasound driving, which has been fed from the control section 35, to the ultrasound endoscope 10. The communication section for observation apparatus 32 outputs the received ultrasound image to the image processing section 34 through the transmission/reception processing section 33.

[0023] The image processing section 34 performs predetermined image signal processing on the inputted ultrasound image. The transmission/reception processing section 33 is controlled by the control section 35, to enable the ultrasound image subjected to the image processing in the image processing section 34 to be transmitted to the image output section 22 of the video processor 20 through the communication line 53.

[0024] In addition, the communication section for observation apparatus 32 is controlled by the transmission/reception processing section 33, to receive endoscope-specific information. A read-out section 31 reads out the endoscope-specific information, which has been received by the communication section for observation apparatus 32, to output the read-out information to the control section 35.

[0025] The control section 35 determines whether or not the communication is appropriately established between the ultrasound observation apparatus 30 and the ultrasound endoscope 10 by using the endoscope-specific information which has been read out by the read-out section 31. That is, the control section 35 of the ultrasound observation apparatus 30 and the control section 24 of the video processor 20 communicate with each other through the communication line 54, to cross-check the endoscope-specific information read out from the read-out section 31 and the endoscope-specific information read out from the read-out section 23 against each other. Based on the cross-check, the control sections 24 and 35 determine whether the wire connection and the wireless connection are normally established, that is, determine whether communication between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the ultrasound observation apparatus 30 is established wirelessly.

[0026] When determining that the wireless communication has been established between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the ultrasound observation apparatus 30, the control section 35 shares information with the control section 24 and controls the transmission/reception processing section 33 to cause the transmission/reception processing section 33 to transmit the ultrasound image to the video processor 20.

[0027] Next, the operation in the present embodiment thus configured will be described with reference to the flowchart in FIG. 2. The left side in FIG. 2 shows the operation of the ultrasound observation apparatus 30,

the right side in FIG. 2 shows the operation of the video processor 20, and each of the dashed-line arrows shows communication.

[0028] The video processor 20 determines whether or not the ultrasound endoscope 10 is connected in step S1. When the ultrasound endoscope 10 is connected to the video processor 20 with the cable 51, the read-out section 23 in the video processor 20 reads out the endoscope-specific information stored in the identification section 15 from the communication section for endoscope 14 through the cable 52 (step S2). The read-out section 23 outputs the read-out endoscope-specific information to the control section 24. The control section 24 performs communication with the control section 35 in the ultrasound observation apparatus 30 through the communication line 54, and transfers the endoscope-specific information read out by the read-out section 23 to the control section 35 (step S3).

[0029] On the other hand, in the ultrasound observation apparatus 30, the communication section for observation apparatus 32 tries to establish communication with the communication section for endoscope 14 in the ultrasound endoscope 10, and when the communication is enabled, the communication section for observation apparatus 32 obtains the endoscope-specific information stored in the identification section 15. The read-out section 31 reads out the endoscope-specific information from the communication section for observation apparatus 32, to output the read-out information to the control section 35 (step S11).

[0030] The control section 35 cross-checks the endoscope-specific information transmitted from the video processor 20 through the communication line 54 and the endoscope-specific information obtained by the communication section for observation 23 by wireless communication against each other, to determine whether the transmitted endoscope-specific information and the obtained endoscope-specific information match with each other (step S12). As a result of the cross-check, when determining that the pieces of information match with each other, the control section 35 determines that wireless communication is established between the ultrasound observation apparatus and the ultrasound endoscope 10 connected to the video processor 20 through the wire.

[0031] In this case, the control section 35 performs setting required for transmission and reception on the ultrasound endoscope 10 in step S13. That is, the control section 35 causes setting parameters for transmission and reception to be transmitted to the communication section for endoscope 14 through the communication section for observation apparatus 32, to set a state in which the ultrasound image can be transmitted and received between the ultrasound endoscope 10 and the ultrasound observation apparatus. Thus, the ultrasound image is transmitted from the ultrasound endoscope 10 to the ultrasound observation apparatus 30 by wireless communication.

[0032] In addition, the control section 35 notifies the control section 24 in the video processor 20 that the ultrasound endoscope 10 has been recognized in the ultrasound observation apparatus 30, through the communication line 54 (step S14). Based on the notification, the video processor 20 recognizes that wireless communication is established between the ultrasound endoscope 10 connected thereto through the wire and the ultrasound observation apparatus 30, and shares information with the ultrasound observation apparatus 30.

[0033] When the video processor 20 is brought into a mode for displaying an ultrasound image, the video processor 20 performs image control for displaying the ultrasound image from the ultrasound observation apparatus 30 on the monitor 40. That is, communication is performed between the control sections 24 and 35, and the control section 35 causes the transmission/reception processing section 33 to transmit the ultrasound image obtained from the ultrasound endoscope 10. The image processing section 34 outputs the ultrasound image to the image output section 22 through the communication line 53. The image output section 22 is controlled by the control section 24, to transmit the ultrasound image received through the communication line 53 to the monitor 40 and cause the monitor to display the ultrasound image.

[0034] Note that, in this case, the endoscopic image obtained by the image pickup processing section 21 and the ultrasound image from the ultrasound observation apparatus 30 can be transmitted to the monitor 40 and displayed independently or simultaneously on the monitor 40.

[0035] In addition, as a result of the cross-check in the step S12 in FIG. 2, when determining that the endoscope-specific information from the video processor 20 and the endoscope-specific information obtained by the communication section for observation 23 via wireless communication do not match with each other, the control section 35 proceeds the processing to step S15. In this case, the control section 35 does not transmit the information necessary for transmission and reception to the ultrasound endoscope 10. In addition, the control section 35 outputs a notification indicating that the ultrasound endoscope, which is a wireless communication partner, is a non-compliant device to the control section 24 in the video processor 20. In this case, the control section 24 causes the monitor 40 to display an indication showing that the ultrasound endoscope 10 connected to the video processor 20 through the wire and the endoscope 10 which establishes a communication with the ultrasound observation apparatus 30 are different ultrasound endoscopes, to notify the operator that communication is not established between the ultrasound endoscope 10 and the ultrasound observation apparatus 30.

[0036] Thus, in the present embodiment, cross-check of the pieces of obtained endoscope-specific information is performed between the video processor connected to the ultrasound endoscope through the wire and the ultrasound observation apparatus connected to the ultra-

sound endoscope via wireless communication, to confirm whether the ultrasound endoscope connected to the video processor through the wire is the same as the ultrasound endoscope connected to the ultrasound observation apparatus via wireless communication. That is, even in the case where the method of establishing communication wirelessly between the ultrasound observation apparatus and the ultrasound endoscope is employed, the ultrasound observation apparatus connected to the video processor can be surely connected to the ultrasound endoscope via wireless communication. That is, the ultrasound endoscope and the ultrasound observation apparatus can be easily connected to each other, which enables a system performance for enabling switching between the endoscopic image and the ultrasound image to be ensured. In addition, confirmation of the communication establishment enables information sharing between the video processor and the ultrasound observation apparatus. As a result, the endoscopic image and the ultrasound image for the same one patient can be displayed and recorded while unifying the management of these images.

[0037] In addition, in FIG. 2, the processing in the step S 13 and the processing in the step S14 are performed sequentially. However, these processings may be performed simultaneously.

[0038] Furthermore, in FIG. 2, the endoscope-specific information is transferred to the ultrasound observation apparatus 30 to determine the matching of the pieces of endoscope-specific information in the ultrasound observation apparatus 30. However, without the transmission of the endoscope-specific information to the ultrasound observation apparatus 30, when the video processor 20 reads out the endoscope-specific information, the ultrasound observation apparatus 30 may read out the endoscope-specific information to transfer the read-out endoscope-specific information to the video processor 20, and the video processor 20 may determine the matching of the pieces of read-out endoscope-specific information, and display an image indicating the result of the matching on the monitor.

(Second Embodiment)

[0039] FIG. 3 is a block diagram showing the second embodiment of the present invention. In FIG. 3, the constituent elements same as those in FIG. 1 are attached with the same reference signs and descriptions thereof will be omitted. In the present embodiment, output to the monitor 40 is performed by an ultrasound observation apparatus 37.

[0040] The ultrasound observation apparatus 37 in the present embodiment is different from the ultrasound observation apparatus 30 in FIG. 1 in that an image processing section 36 is used instead of the image processing section 34. In the present embodiment, the image output section 22 of the video processor 20 outputs an endoscopic image to the image processing section 36 of the

ultrasound observation apparatus 37 through the communication line 53.

[0041] The image processing section 36 performs predetermined image signal processing on the ultrasound image received from the ultrasound endoscope 10 by the communication section for observation apparatus 32, to output the processed ultrasound image to the monitor 40, and is capable of outputting the endoscopic image, which has been inputted from the image output section 22 through the communication line 53, to the monitor 40. In addition, the image processing section 36 is also capable of combining the endoscopic image and the ultrasound image, to output the combined image to the monitor 40. The control section 35 communicates with the control section 24 to control the output of the endoscopic image and the ultrasound image to the monitor 40.

[0042] Also in the present embodiment thus configured, the process for performing communication between the video processor 20 connected to the ultrasound endoscope 10 through the wire and the ultrasound observation apparatus 37, to cross-check the pieces of endoscope-specific information, and establishing connection via wireless communication between the ultrasound endoscope 10 and the ultrasound observation apparatus 37 is the same as that in the first embodiment.

[0043] In the present embodiment, the control section 35 in the ultrasound observation apparatus 37 performs the control for outputting the endoscopic image and the ultrasound image obtained by operating the ultrasound endoscope 10 to the monitor 40. The control section 35 causes the endoscopic image transmitted from the video processor 20 and the ultrasound image obtained from the ultrasound endoscope 10 by the communication section for observation apparatus 32 via wireless communication to be displayed on the monitor 40 by switching these images or to be displayed on the monitor simultaneously.

[0044] Other working and effects are the same as those in the first embodiment.

(Third Embodiment)

[0045] FIG. 4 is a block diagram showing the third embodiment of the present invention. In FIG. 4, the constituent elements same as those in FIG. 1 are attached with the same reference signs and descriptions thereof will be omitted. An ultrasound endoscope system according to the present embodiment employs a display apparatus 60 including a control section 61, instead of the monitor 40. In the first and second embodiments, the control section 24 in the video processor 20 and the control section 35 in the ultrasound observation apparatus 30 are configured to determine the establishment of the communication with the ultrasound endoscope 10. In contrast, in the present embodiment, a control section provided in another part of the ultrasound endoscope system is configured to determine the establishment of the communication with the ultrasound endoscope 10. FIG. 4 shows

an example in which the control section 61 provided in the display apparatus 60 determines the establishment of the communication.

[0046] The control section 24 communicates with the control section 61 in the display apparatus 60 via a communication line 54V, and the control section 35 communicates with the control section 61 in the display apparatus 60 via a communication line 54U. In addition, the image output section 22 supplies an endoscopic image to the display apparatus 60 through a communication line 53V and the image processing section 34 supplies an ultrasound image to the display apparatus 60 through a communication line 53U.

[0047] The endoscopic image and the ultrasound image are inputted to the display apparatus 60. The display apparatus 60 is controlled by the control section 61 and configured to be able to selectively or simultaneously display these inputted images on a display screen, not shown.

[0048] The control section 61 in the display apparatus 60 receives the endoscope-specific information, which has been read out by the read-out section 23, from the control section 24, and receives the endoscope-specific information, which has been read out by the read-out section 31, from the control section 35. The control section 61 cross-checks these pieces of endoscope-specific information against each other, to determine whether or not the wire connection and the wireless connection are normally established, that is, determines whether or not the communication is established wirelessly between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the ultrasound observation apparatus 30.

[0049] When determining that the wireless communication has been established between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the ultrasound observation apparatus 30, the control section 61 causes the control sections 24 and 35 to share information. Furthermore, the display mode is specified by the control sections 24 and 35, and the control section 61 causes the endoscopic image and the ultrasound image to be displayed selectively or simultaneously on the display screen in the specified display mode.

[0050] Next, the operation in the present embodiment thus configured will be described with reference to the flowchart in FIG. 5. In FIG. 5, the same processing steps as those in FIG. 2 are attached with the same reference signs and descriptions thereof will be omitted. In FIG. 5, the operation of the ultrasound observation apparatus 30 is shown on the left side, the operation of the display apparatus 60 is shown in the center, and the operation of the video processor 20 is shown on the right side, and each of the dashed-line arrows shows communication.

[0051] When the video processor 20 reads out the endoscopic-specific information stored in the identification section 15 from the communication section for endoscope 14, through the cable 52 (step S2), the control

section 24 notifies the control section 35 in the ultrasound observation apparatus 30 that the endoscope-specific information has been read out, through the display apparatus 60. In response to the notification, the ultrasound observation apparatus 30 communicates with the ultrasound endoscope 10 through the communication section for observation apparatus 32, to obtain the endoscope-specific information. The read-out section 31 reads out the endoscope-specific information from the communication section for observation apparatus 32 (step S31), and outputs the read-out information to the control section 35.

[0052] In the present embodiment, the control section 24 in the video processor 20 transfers the endoscope-specific information obtained by the read-out section 23 to the display apparatus 60 through the communication line 54V (step S21), and the control section 35 in the ultrasound observation apparatus 30 transfers the endoscope-specific information read out by the read-out section 31 to the display apparatus 60 through the communication line 54U (step S31).

[0053] The control section 61 of the display apparatus 60 cross-checks the endoscope-specific information transferred from the video processor 20 and the endoscope-specific information transferred from the ultrasound observation apparatus 30 against each other, to determine match or mismatch of the pieces of endoscope-specific information (step S41). Furthermore, when determining that the pieces of endoscope-specific information match with each other, the control section 61 generates information indicating the match (match information) in step S42 (step S42). When determining that the pieces of endoscope-specific information do not match with each other, the control section 61 generates information indicating the mismatch (mismatch information) in step S43 (step S43). The control section 61 outputs the match information or the mismatch information to the control sections 24 and 35 through the communication lines 54V and 54U (step S44).

[0054] The control section 24 in the video processor 20 determines whether the received information is the match information or the mismatch information (step S22). When determining that the received information is the match information, the control section 24 recognizes that communication has been established between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the ultrasound observation apparatus 30 (step S23). Furthermore, when determining that the received information is the mismatch information, the control section 24 recognizes that communication is not established between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the ultrasound observation apparatus 30 (step S24).

[0055] The control section 35 in the ultrasound observation apparatus 30 determines whether the received information is the match information or the mismatch information in step S32. When determining that the received information is the match information, the control section

35 recognizes that wireless communication has been established between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the communication section for observation apparatus 32 (step S33). In this case, the control section 35 performs setting required for transmission and reception on the ultrasound endoscope in step S 13.

[0056] Furthermore, when determining that the received information is the mismatch information, the control sections 35 recognizes that wireless communication is not established between the ultrasound endoscope 10 connected to the video processor 20 through the wire and the communication section for observation apparatus 32, the control section 35 does not transmit the information required for transmission and reception to the ultrasound endoscope 10.

[0057] When recognizing that communication has been established, the control section 24 in the video processor 20 and the control section 35 in the ultrasound observation apparatus 30 output the endoscopic image and the ultrasound image, respectively, to the display apparatus 60 through the communication lines 53V and 53U. In response to this, the display apparatus 60 displays one of or both of the endoscopic image and the ultrasound image according to the display mode.

[0058] When the control section 61 of the display apparatus 60 generates the mismatch information, the control section 61 causes the display screen to display an indication that the ultrasound endoscope as the partner of wireless communication with the ultrasound observation apparatus 30 is a non-compliant device and the ultrasound endoscope 10 connected to the video processor 20 through the wire is different from the ultrasound endoscope 10 which establishes communication with the ultrasound observation apparatus 30. Note that, when the communication has been established, the control section 61 may display an indication of the establishment of communication on the display screen.

[0059] Thus, also in the present embodiment, it is possible to obtain the same effects as those in the first embodiment.

[0060] Note that, in the above-described embodiments, one video processor 20 and one ultrasound observation apparatus 30 are provided, but a plurality of video processors 20 and a plurality of ultrasound observation apparatuses 30 may be connected to the one display apparatus 60. However, the communication lines and the image communication lines to be connected to the display apparatus 60 have to be a pair for the respective processors and ultrasound observation apparatuses. In the above-described embodiments, description has been made on the example in which the information indicating whether or not the communication is established is displayed on the monitor or the display apparatus. However, a display section made of LCD, LED, or the like may be provided in the ultrasound endoscope system and the information may be displayed on the display section.

[0061] The present invention is not limited to the embodiments as they are described above, and can be embodied in the practical stage by modifying constituent elements within a range without departing from the gist of the invention. In addition, various inventions can be formed by appropriately combining the plurality of constituent elements disclosed in the above-described embodiments. For example, some of all constituent elements disclosed in the embodiments may be deleted. Furthermore, constituent elements shown in different embodiments may be appropriately combined.

[0062] The present application is filed claiming the priority of Japanese Patent Application No. 2013-206593 filed in Japan on October 1, 2013, and the above described disclosure is incorporated by reference in the present description, claims, and drawings.

Claims

1. An ultrasound endoscope system comprising: an ultrasound endoscope that is capable of performing optical observation; a video processor for optical observation; and an ultrasound observation apparatus for ultrasound observation,
the ultrasound endoscope comprising:

an image pickup section;
an ultrasound transducer;
an identification section that stores endoscope state information; and
a communication section for endoscope that wirelessly transmits and receives an ultrasound signal and the endoscope state information,

the video processor comprising:

an optical image processing section that processes an optical image obtained by the image pickup section of the ultrasound endoscope; and
a first read-out section that reads out the endoscope state information in the identification section in the ultrasound endoscope, and

the ultrasound observation apparatus comprising:

a transmission/reception section that is capable of transmitting and receiving the ultrasound signal;
a communication section for observation apparatus that communicates with the communication section for endoscope in the ultrasound endoscope, and transmits and receives the ultrasound signal and the endoscope state information;
an ultrasound image processing section that generates an image based on the ultrasound signal obtained by the communication section

for observation apparatus; and
a second read-out section that reads out the endoscope state information obtained by the communication section for ultrasound observation apparatus,

the ultrasound endoscope system further comprising a control section that compares the endoscope state information obtained by the first read-out section in the video processor and the endoscope state information obtained by the second read-out section in the ultrasound observation apparatus, and establishes wireless connection between the ultrasound endoscope and the ultrasound observation apparatus only when the endoscope state information obtained by the first read-out section and the endoscope state information obtained by the second read-out section match with each other.

2. The ultrasound endoscope system according to claim 1, wherein the endoscope state information also includes identification information of the ultrasound endoscope.

3. The ultrasound endoscope system according to claim 1, further comprising:

a display apparatus configured to be connected to one of the video processor and the ultrasound observation apparatus; and
an image communication line that connects the optical image processing section and the ultrasound image processing section,
wherein one of the optical image processing section and the ultrasound image processing section which are connected to each other with the image communication line obtains image information from another of the optical image processing section and the ultrasound image processing section, to cause both of an optical image and an ultrasound image to be displayed in a switchable manner by the display apparatus.

4. The ultrasound endoscope system according to claim 1, further comprising,
a display apparatus including the control section connected to at least the one video processor and at least the one ultrasound observation apparatus, wherein the display apparatus includes:

an image input section that can receive respective images outputted from the video processor and the ultrasound observation apparatus; and
an endoscope information input section that receives the endoscope state information outputted from the first read-out section in the video processor and the endoscope state information outputted from the second read-out section in

the ultrasound observation apparatus, and

the control section compares the plurality of pieces of endoscope state information, which are inputted to the control section through the endoscope information input section, with each other, and only when the plurality of pieces of endoscope state information match with each other, the control section gives an instruction for establishing wireless connection between the ultrasound endoscope and the ultrasound observation apparatus and performs control for switchably displaying images outputted from the video processor and the ultrasound observation apparatus between which the pieces of endoscope state information match with each other.

5. The ultrasound endoscope system according to claim 3 or 4, wherein the display apparatus displays a state of communication establishment on a display screen when communication is established between the ultrasound endoscope and the ultrasound observation apparatus.

6. The ultrasound endoscope system according to any one of claims 1 to 5, wherein the ultrasound endoscope includes a display section that displays a state of communication establishment when communication is established between the ultrasound endoscope and the ultrasound observation apparatus.

7. A communication method of an ultrasound endoscope system comprising an ultrasound endoscope that is capable of performing optical observation; a video processor for optical observation; and an ultrasound observation apparatus for ultrasound observation, the method comprising:

a step in which a first read-out section in the video processor connected to the ultrasound endoscope reads out endoscope state information stored in an identification section in the ultrasound endoscope;

a step in which a communication section for observation apparatus in the ultrasound observation apparatus wirelessly communicates with a communication section for endoscope in the ultrasound endoscope and receives the endoscope state information; and

a step in which a control section cross-checks the endoscope state information received by the video processor and the endoscope state information received by the communication section for observation apparatus against each other, to perform determination of matching of the pieces of endoscope state information, and performs control for establishing communication between the ultrasound endoscope and the ultrasound observation apparatus when determining that

the pieces of endoscope state information
match with each other.

5

10

15

20

25

30

35

40

45

50

55

FIG. 1

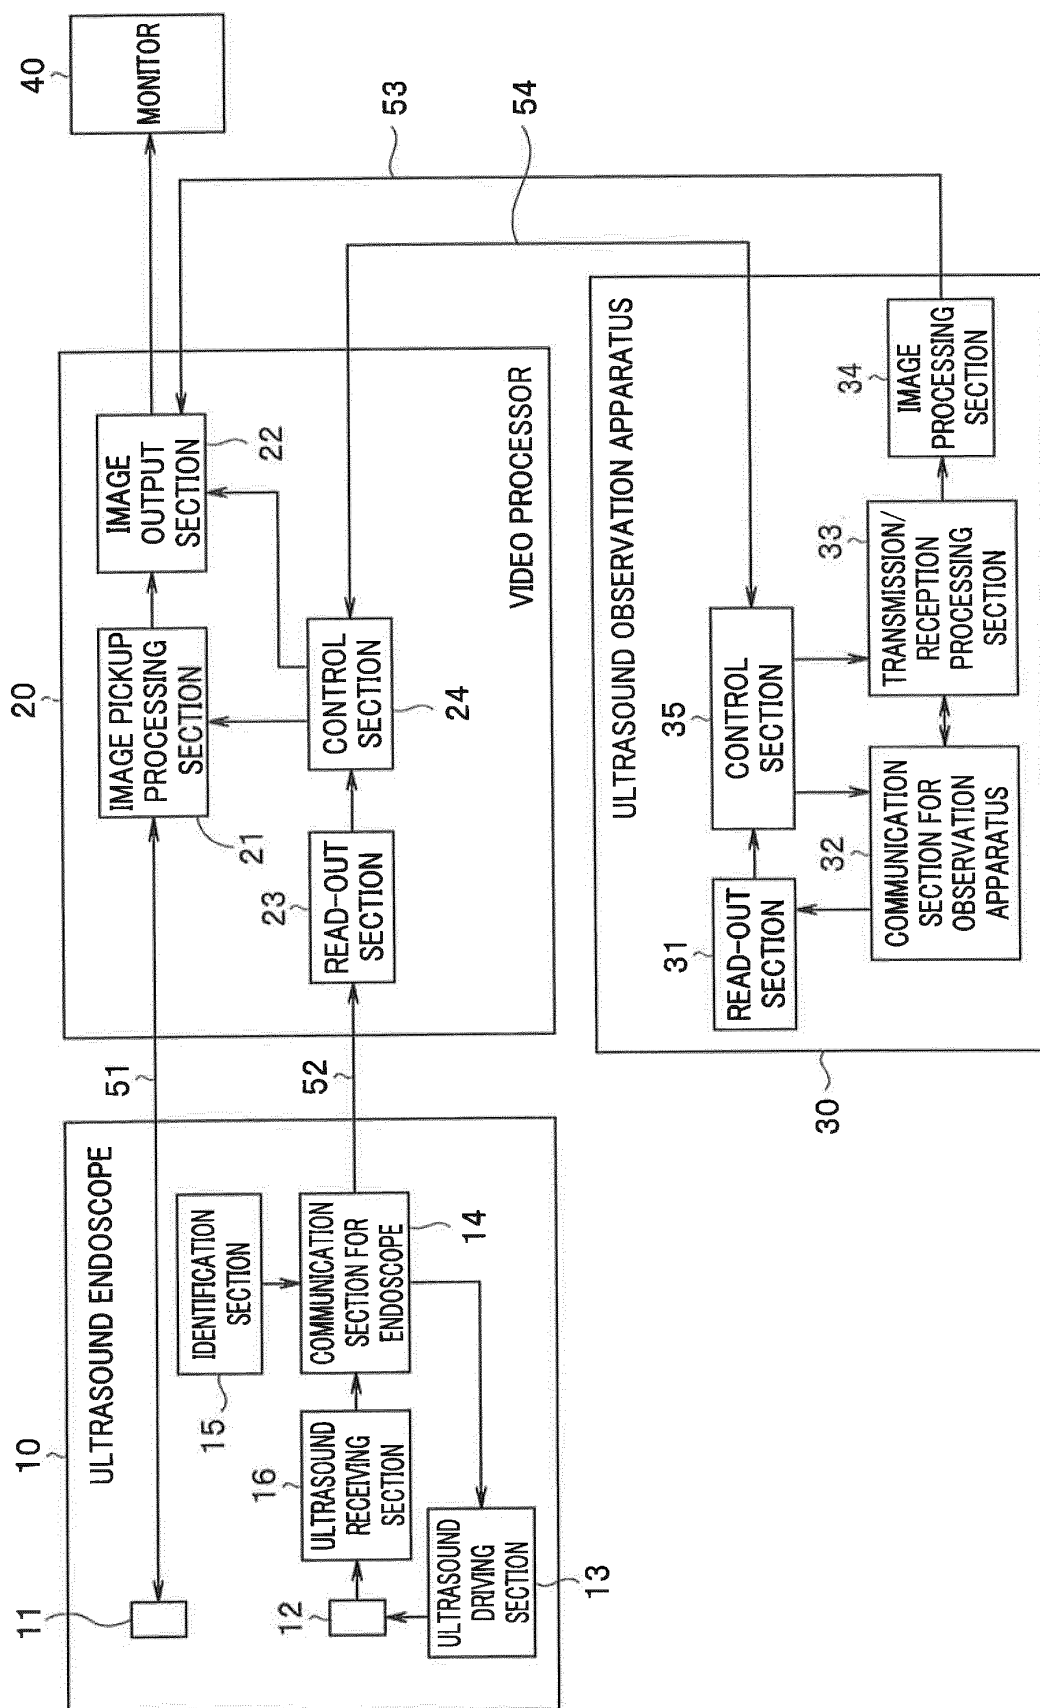


FIG. 2

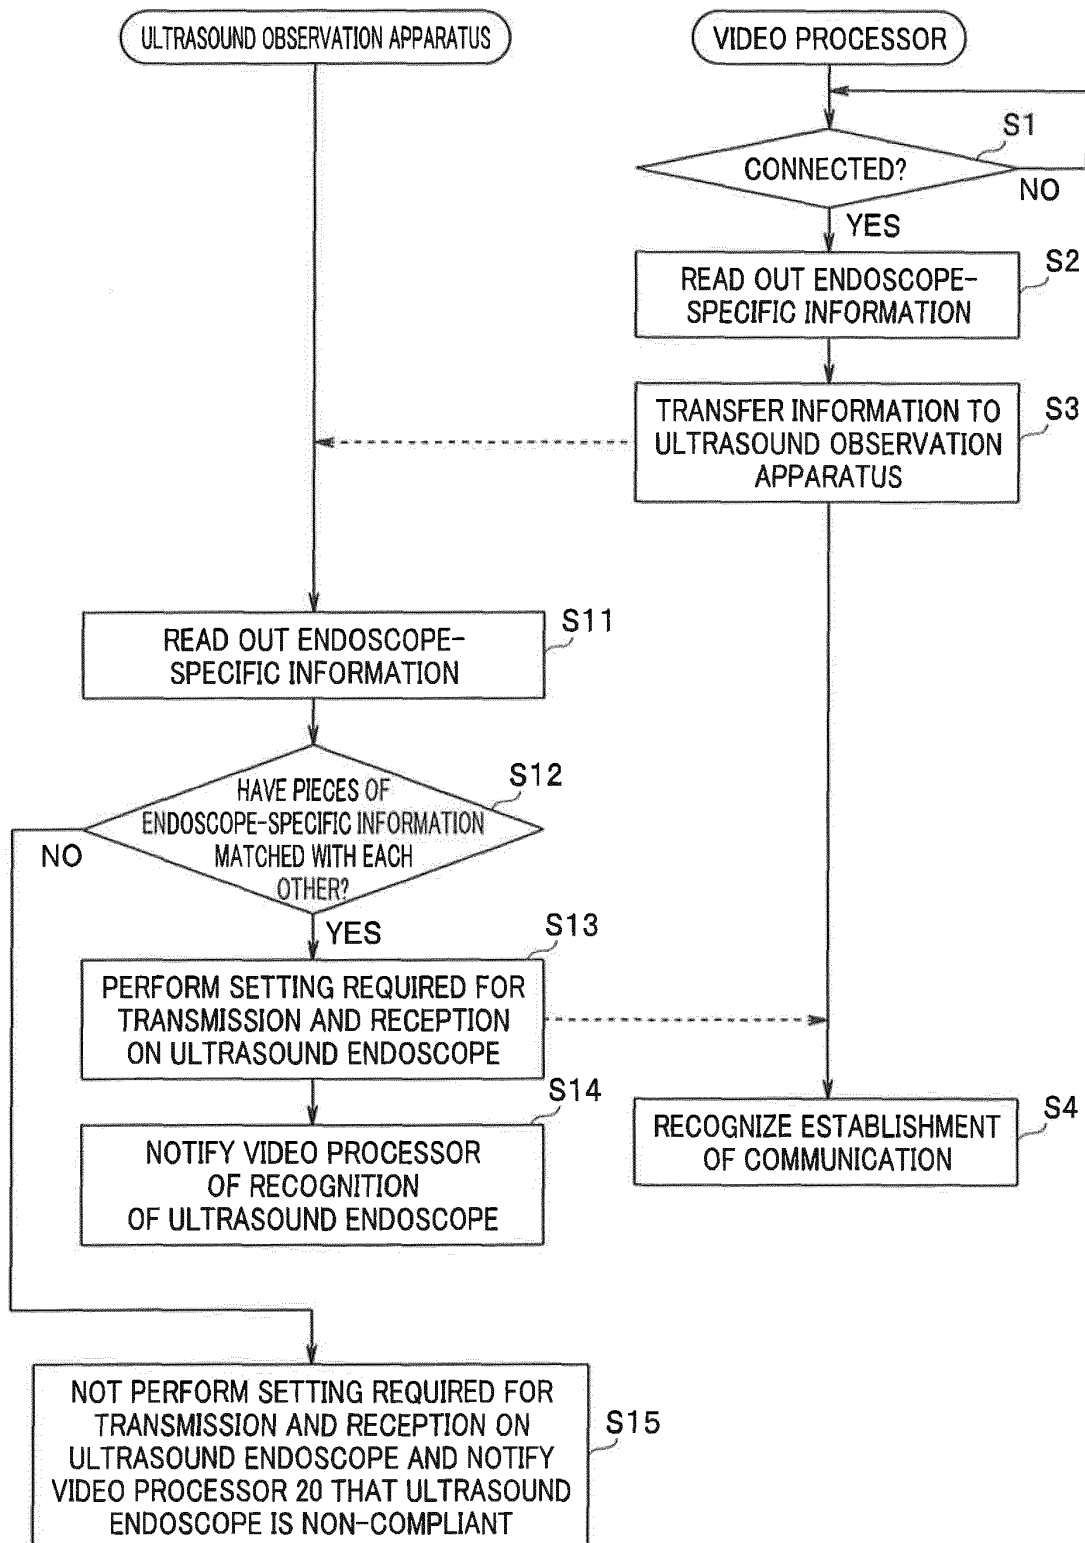


FIG. 3

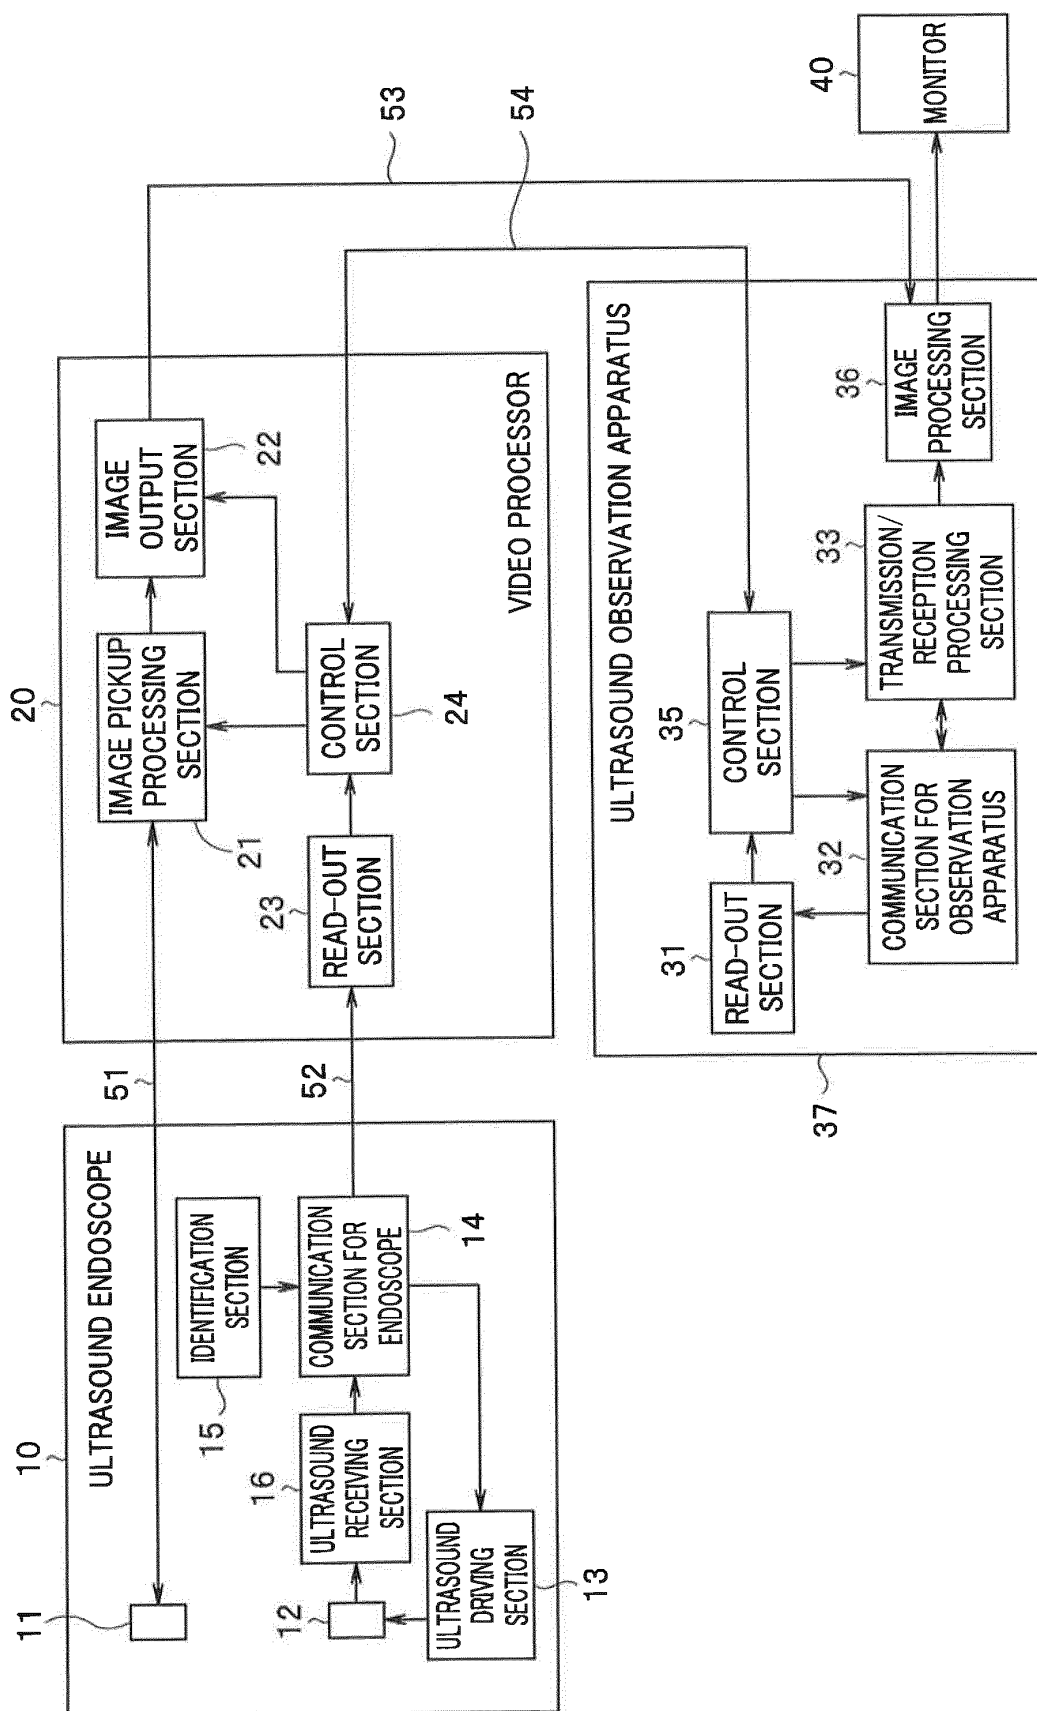


FIG. 4


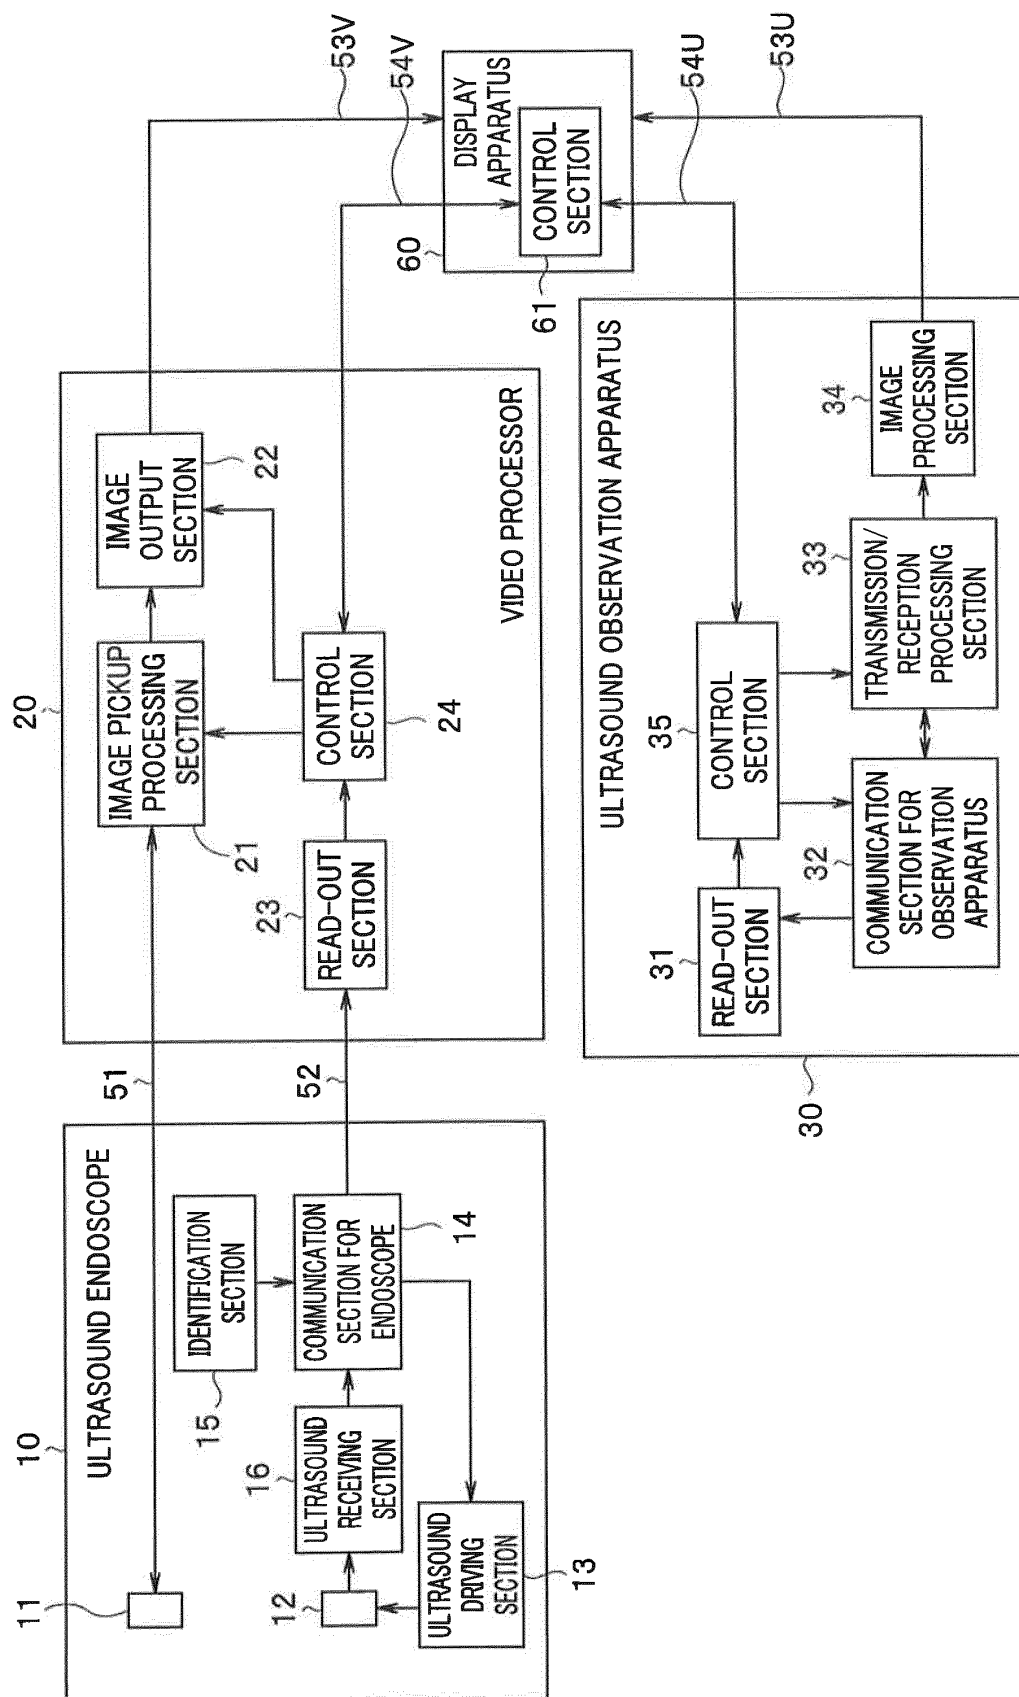


FIG. 5

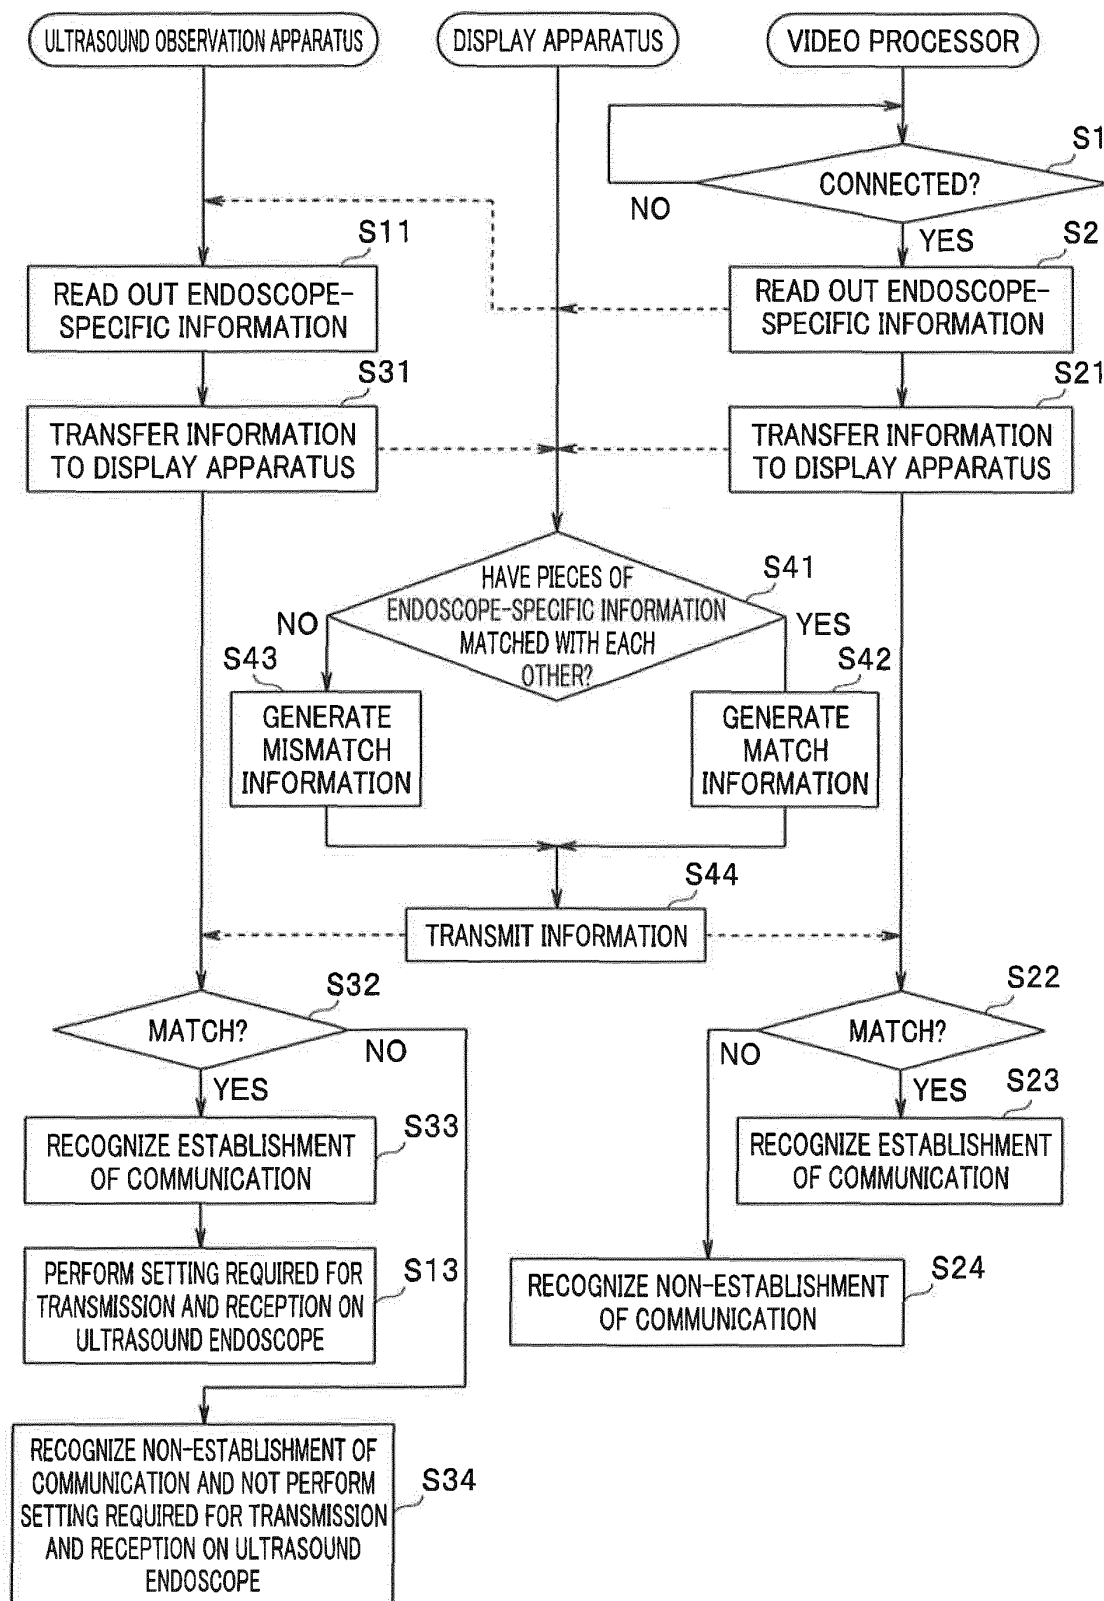

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2014/075599

A. CLASSIFICATION OF SUBJECT MATTER

A61B8/12(2006.01) i

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B8/12

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Jitsuyo Shinan Koho 1922-1996 Jitsuyo Shinan Toroku Koho 1996-2014

Kokai Jitsuyo Shinan Koho 1971-2014 Toroku Jitsuyo Shinan Koho 1994-2014

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	JP 2008-253525 A (Olympus Medical Systems Corp.), 23 October 2008 (23.10.2008), entire text; all drawings & US 2008/0249361 A1 & EP 1977695 A1 & JP 5064868 B2	1-7
A	JP 2006-334169 A (Fujifilm Holdings Corp.), 14 December 2006 (14.12.2006), entire text; all drawings & US 2006/0276687 A1 & EP 1728463 A1 & JP 4727302 B2	1-7
A	JP 4908897 B2 (Hitachi Aloka Medical, Ltd.), 04 April 2012 (04.04.2012), entire text; all drawings & JP 2007-275087 A	1-7

☐ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

14 October, 2014 (14.10.14)

Date of mailing of the international search report

28 October, 2014 (28.10.14)

Name and mailing address of the ISA/
Japanese Patent Office

Authorized officer

Facsimile No.

Telephone No.

Form PCT/ISA/210 (second sheet) (July 2009)

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 4908897 B [0005]
- JP 2013206593 A [0062]

专利名称(译)	超声波内窥镜系统及其通信方法		
公开(公告)号	EP2995258A4	公开(公告)日	2017-03-01
申请号	EP2014850702	申请日	2014-09-26
[标]申请(专利权)人(译)	奥林巴斯株式会社		
申请(专利权)人(译)	OLYMPUS CORPORATION		
当前申请(专利权)人(译)	OLYMPUS CORPORATION		
[标]发明人	OKUNO YOSHIYUKI		
发明人	OKUNO, YOSHIYUKI		
IPC分类号	A61B8/12		
CPC分类号	A61B8/12 A61B8/4438 A61B8/445 A61B8/4472 A61B8/54 A61B8/565 A61B1/00009 A61B1/00055 A61B1/04 A61B8/4416 A61B8/463		
优先权	2013206593 2013-10-01 JP		
其他公开文献	EP2995258A1		
外部链接	Espacenet		

摘要(译)

超声波内窥镜系统具备：超声波内窥镜，其具有存储内窥镜状态信息的识别部；视频处理器，其包括：第一读出部，其读出所述超声波内窥镜中的所述识别部中的所述内窥镜状态信息；超声波观测装置，包括：第二读出部，读出由观察装置用通信部获得的内窥镜状态信息；以及控制部，其将所述视频处理器中的所述第一读取部获得的所述内窥镜状态信息与所述超声波观测装置中的所述第二读取部获得的内窥镜状态信息进行比较，仅在由所述第一读取部取得的所述内窥镜状态信息与由所述第二读取部取得的所述内窥镜状态信息一致的情况下，判断为所述超声波内窥镜和所述超声波观察装置。