

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
5 November 2009 (05.11.2009)

(10) International Publication Number
WO 2009/134720 A1

(51) International Patent Classification:

A61B 8/00 (2006.01)

Penn Center, 1635 Market Street, Philadelphia, PA 19103-2212 (US).

(21) International Application Number:

PCT/US2009/041831

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(22) International Filing Date:

27 April 2009 (27.04.2009)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

12/111,387 29 April 2008 (29.04.2008) US

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(71) Applicant (for all designated States except US): **CIVCO MEDICAL INSTRUMENTS CO., INC.** [US/US]; 102 Highway 1S, Kalona, IA 52247 (US).

(72) Inventor; and


(75) Inventor/Applicant (for US only): **CERMAK, Craig, J.** [US/US]; 3215 130th Street, Riverside, IA 52327 (US).

(74) Agent: **STEIN, Barry, A.; CAESAR, RIVISE, BERNSTEIN, COHEN & POKOTILOW**, 11th Floor, Seven

[Continued on next page]

(54) Title: BRACKET FOR MOUNTING AT LEAST ONE POSITION DETECTING SENSOR ON AN ULTRASONIC PROBE

Fig. 1

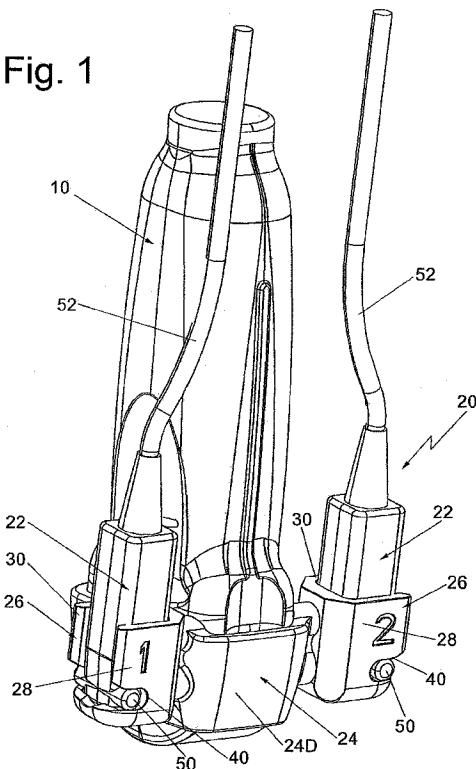

(57) Abstract: A bracket (20) for use on an ultrasound transducer (10) to releasably mount at least one 3D tracking sensor (22) on the transducer. Each sensor has a pair of axially aligned pins (50) projecting outward from its body. The bracket includes at least one socket (26) having a pair of spaced-apart wall portions (28,30), each of which includes a slot (40) arranged to receive a respective one of the pins of the sensor when the sensor is in a first position. From this position the sensor's body can be rotated to a second position, whereupon the spaced apart wall portions releasably engage (snap-fit about) a portion of the body of the sensor (22) to deter the accidental displacement of the sensor with respect to the transducer.



Declarations under Rule 4.17:

- *as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))* — *with international search report (Art. 21(3))*

Published:

**BRACKET FOR MOUNTING AT LEAST ONE
POSITION DETECTING SENSOR ON AN ULTRASONIC PROBE
SPECIFICATION**

CROSS-REFERENCE TO RELATED APPLICATIONS

5 This PCT application claims the benefit of U.S. Utility Application Serial No. 12/111,387 filed on April 29, 2008, entitled BRACKET FOR MOUNTING AT LEAST ONE POSITIONING DETECTING SENSOR ON AN ULTRASONIC PROBE and whose entire disclosure is incorporated by reference herein.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR

10 **DEVELOPMENT**

“Not Applicable”

INCORPORATION-BY-REFERENCE OF MATERIAL

SUBMITTED ON A COMPACT DISK

“Not Applicable”

15 **FIELD OF THE INVENTION**

This invention relates generally to medical devices and more particularly to devices for releasably mounting at least one sensor of a 3D tracking system on a ultrasound transducer or other hand-held medical instrument.

BACKGROUND OF THE INVENTION

20 Ultrasound has received widespread acceptance as a useful diagnostic tool by providing an image of the internal area of inquiry by emission of very high frequency sound waves from a transducer (commonly called a “probe”) placed in contact with the patient's skin adjacent that area of inquiry. Repeated arrays of ultrasonic beams scan that area and are reflected back to the transducer, where the beams are received and the data transmitted to a processing device. A processing unit, to which the probe is connected, analyzes the information and composes a picture for display on an associated monitor screen. For some applications the determination of the precise position or location of the probe with respect to the patient's body is desirable, e.g., to correlate the ultrasonic image to other scans, such as CT scans.

30 So-called “3D tracking” systems are commercially available and disclosed in the patent literature for enabling one to readily determine the 3D position of an instrument, such as a medical device, by determining location, orientation, and/or positioning information relative to some coordinate system. For example, Ascension Technology Corporation makes 3D position and orientation tracking devices suitable for various medical applications, e.g., to

navigating, localize, and guide medical instruments for image-guided procedures. Other manufacturers/suppliers of 3D tracking systems include Polhemus, Inc. Northern Digital Inc. and Medtronic, Inc.

Typically 3D tracking systems use the attenuation of oriented electromagnetic signals 5 to determine the absolute position and orientation of a sensor, relative to a source, e.g., a DC magnetic field generator. The source and the sensor are connected via cables to an electronics module, which contains a microcomputer and associated electronics of the system. The source typically includes three orthogonal coils that are pulsed in rotation, one after another. Each pulse transmits a radio frequency electromagnetic signal that is detected 10 by the sensor. The sensor also contains three orthogonal coils, which measure the strength of the signal from the current source coil. By using the known pulse strength at the source and the known attenuation of the strength with distance, the position and orientation of the sensor coils can be calculated by the system via triangulation techniques.

Utilizing device location or 3D tracking systems with ultrasonic probes can be 15 accomplished by permanently mounting the sensor(s) on the probe or by building such sensor(s) into the probe. However, this approach may not be desirable if the probe is also intended to be used in applications wherein its position need not be determined, since the inclusion of such sensor(s) permanently on or in the probe will likely increase the cost and complexity of the probe. Moreover, such an approach may not be suitable to retrofit existing 20 ultrasonic probes. Thus, the use of some releasable mounting system is deemed to be the better approach for providing an ultrasonic probe with means for determining its position with respect to the patient's body.

As will be appreciated by those skilled in the art, the prior art includes various brackets for releasable mounting devices on an ultrasonic probe. Such brackets are commonly 25 used to support biopsy needle guides and the like. Examples of such brackets are disclosed in United States Letters Patent Nos.: 5,052,396 (Wedel et al.), 5,076,269 (Arenson et al.), 5,623,931 (Wung et al.), 5,758,650 (Miller et al.), 5,941,889 (Cermak), 6,379,307 (Filly et al.), and 7087,024 (Pruter). My prior United States Letters Patent No. 5,941,889 (Cermak) discloses and claims a multiple angle disposable needle guide system for use in guiding 30 needles into selected locations of a patient relative to an ultrasonic probe or some other medical instrument imaging sensor.

While such brackets are suitable for their intended purposes, they are not designed for mounting one or more position sensors thereon. Accordingly, a need exists for such a

bracket. Moreover, that bracket should be constructed so that the sensor(s) when mounted thereon will be resistant to accidental displacement, but can be readily removed and/or mounted when desired. This invention addresses those needs.

All references cited herein are incorporated herein by reference in their entireties.

5

SUMMARY OF THE INVENTION

In accordance with one aspect of this invention there is provided a bracket for use with an ultrasound transducer to releasably mount at least one sensor of a location/tracking system on the transducer. The at least one sensor has a body including an opposed pair of wall portions. The bracket comprises a member arranged to be releasably mounted on the
10 transducer and includes at least one socket therein. The at least one socket has a pair of spaced-apart wall portions. The at least one socket and the at least one sensor are arranged to be coupled together via cooperating pins and slots to enable the at least one sensor to be oriented in a first position for insertion between the spaced-apart walls of the at least one socket to introduce said pins into respective ones of said slots so that the at least one sensor
15 may be rotated to a second or locked position within the at least one socket. When the sensor is in the locked position, the wall portions of the at least one socket releasably engage, e.g., snap-fit, about a portion of the sensor to deter accidental displacement of the sensor with respect to the transducer.

In accordance with one exemplary embodiment of the bracket of this invention each
20 of the wall portions of the at least one socket includes a slot and the pins project from the opposed wall portions of the at least one sensor and are axially aligned.

In accordance with another aspect of this invention there is provided the combination
25 of a bracket and at least one sensor of a location/tracking system. The bracket and sensor are arranged for enabling the location of an ultrasound transducer to be determined. The sensor forms a part of a location/tracking system. The bracket comprises a member arranged to be releasably mounted on the transducer and includes at least one socket in it. The at least one socket has a pair of spaced-apart wall portions. The at least one socket and the at least one sensor are arranged to be coupled together via cooperating pins and slots to enable the at least one sensor to be oriented in a first position for insertion between the spaced-apart walls of the
30 at least one socket to introduce said pins into respective ones of said slots so that the at least one sensor may be rotated to a second or locked position within the at least one socket. When the at least one sensor is in the locked position, the wall portions of the at least one

socket releasably engage, e.g., snap-fit, about a portion of the at least one sensor to deter accidental displacement of the at least one sensor with respect to the transducer.

DESCRIPTION OF THE DRAWING

Fig. 1 is an isometric view of a portion of an ultrasonic probe having one exemplary embodiment of a bracket constructed in accordance with one aspect of this invention for supporting up to two position-locating sensors on the probe, so that those sensors are resistant to accidental displacement;

Fig. 2A is an side elevation view showing the sensor in an orientation wherein it is juxtaposed opposite a socket portion of a bracket like shown in Fig. 1 so that a sensor is ready for mounting therein;

Fig. 2B is an side elevation view, similar to Fig. 2A, showing the sensor at an initial position within the socket;

Fig. 2C is a side elevation view, similar to Figs. 2A and 2B, but showing the sensor at its final or locked position within the socket, wherein it is resistant to accidental displacement;

Fig. 3 is an isometric view of the exemplary sensor shown in Figs. 2A - 2C;

Fig. 4 is an exploded isometric view of the various components making up the embodiment of the bracket shown in Fig. 1;

Fig. 5 is an isometric view of an alternative embodiment of a bracket constructed in accordance with this invention, the bracket of this embodiment including a fixed-angle biopsy needle guide assembly;

Fig. 6 is an isometric view similar to Fig. 5, but showing still another embodiment of a bracket constructed in accordance with this invention, the bracket of this embodiment including an adjustable angle biopsy needle guide assembly.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

Referring now to the various figures of the drawing wherein like reference characters refer to like parts, there is shown in Fig. 1 a bracket 20 for use with an ultrasound transducer 10 to releasably mount one or more sensors 22 of a location sensing system, e.g., a 3D tracking system, such as available from Ascension Technology Corporation, or any other manufacturers of such systems. In the interest of drawing simplicity and brevity the other components of the locating sensing system are not shown. It should be pointed out at this juncture that subject invention can make use of any kinds of sensors for any kinds of 3D tracking systems whether based on electromagnetic, acoustic, mechanical, or optical

technology. As such, the subject invention does not require any particular construction for the sensor, except that the body or housing of the sensor should be constructed to include a feature to be described shortly that ensures that when the sensor is in a locked position it is resistant to accidental displacement. In the exemplary embodiments shown and described 5 herein such features comprise a pair of pins. However, other arrangements can be used as well.

The bracket 20 basically comprises a body portion 24 supporting one or more sockets 26. The details of the body portion 24 will be described later. Suffice for now to state that the body portion is arranged to be releasably mount the bracket 20 on the transducer 10. Each 10 socket 26 is, in turn, arranged to releasably mount a respective one of the sensors 22 of the location sensing system. In the embodiment shown in Fig. 1, two such sensors 22 are shown mounted in respective sockets of the bracket 20 in their operative or locked position (i.e., a position wherein they are resistant to accidental displacement). It should be pointed out at this juncture that the bracket of the subject invention can be constructed to accommodate 15 more than two sensors or only one sensor, depending upon the application.

The transducer 10 can be of any conventional or non-conventional construction and may be an ultrasonic transducer or any other hand-holdable probe or device for use with any type of scanning system where the position and orientation of the probe or device is desired to be determined. As best seen in Figs. 1 and 4, the body portion 24 basically comprises a 20 ring-like member which is arranged to snap-fit about a portion of the periphery of the probe 10, e.g., about the lower or distal portion of the probe as shown in Fig. 1. A sterilized cover (not shown) may be interposed between the probe and the bracket 20. In the exemplary embodiment shown, the ring-like body portion 24 is an integral member, e.g., a molded component formed of any suitable material, e.g., plastic, and includes four sidewall portions, 25 namely, a left sidewall portion 24A, a right sidewall portion 24B, a front wall portion 24C and a rear wall portion 24D. In the exemplary embodiment of Fig. 1 two sockets 26 are mounted on the body portion 24. In particular, one socket 26 is mounted on the left sidewall portion 24A while the other socket 26 is mounted on the right sidewall portion 24A. The mounting of the sockets on their respective sidewalls is accomplished by use of respective 30 pairs of threaded fastener 28 as shown clearly in Fig. 4. These fasteners are arranged to extend through respective holes (to be described later) in the sockets for receipt in respective holes (also to be described later) in bosses (also to be described later) formed on the respective sidewalls of the ring-like body member 24.

The details of the sockets 26 will now be described with reference to Fig. 4. As can be seen therein each socket 26 is a generally U-shaped member, e.g., an integral molded component formed of any suitable material, e.g., plastic. Each socket 26 basically comprises a member having a pair of opposed sidewalls 28 and 30, a back wall 32 that bridges the sidewalls 28 and 30 along their full length and a front wall 34 that bridges the bottom ends of the sidewalls 28 and 30. The free end of each of the sidewalls 28 and 30 is in the form of a slight cam surface lip or flange 36. The contiguous walls 28, 30, 32 and 34 define an internal cavity 38 which is arranged for receipt of the body of the sensor 26. The cavity 38 has a longitudinal (e.g., vertical in Fig. 4) axis 38A. The entrance to the cavity 38 is the gap 5 between the cam surface flanges 36 of the sidewalls 28 and 30. The gap extends generally parallel to the longitudinal axis 38A of the socket's cavity. It is through this gap that the sensor is introduced into the cavity 38.

Each of the sidewalls 28 and 30 includes a horizontally oriented slot 40. Each slot 40 is located immediately above the front wall 34 where the front wall meets the sidewall in 15 which the slot is located. The innermost end of each slot 40 is semicircular in shape and of a predetermined radius to accommodate a respective pin (to be described later) of the sensor 22. The back wall 32 of each socket 26 includes a pair of openings 42 through which the heretofore mentioned fasteners 28 extend for mounting the socket on the ring-like body member 24. As mentioned earlier the ring-like body member includes a pair of bosses and 20 associated holes to receive the fasteners. In particular a pair of bosses 44 projects outward from the outer surface of the sidewall portion 24A of the body portion 24, while a similar pair of bosses 44 projects outward from the outer surface of the sidewall portion 24B. A hole 46 extends through each of the bosses 44. It is in the hole 46 that a portion of and associated fastener 28 resides to secure the socket 26 to the ring-like body member 24.

25 The details of the sensors 22 will now be described with reference to Figs. 1 and 3. To that end, each sensor 22 basically comprises an elongated body 48 having a longitudinal axis 48A. The sensor's body may be formed of any suitable material, e.g., a molded plastic, and houses the components (not shown) making up the sensor.

As mentioned earlier, each sensor includes a pair of pins for cooperation with the 30 sockets to render the sensor resistant to accidental displacement from that socket when the sensor is in the locked position. Those pins are designated by the reference number 50 and are best seen in Fig. 3. The pins 50 are axially aligned pins project outward from a lower portion of sensor's body 48 perpendicularly to its longitudinal axis 48A. A cable 52 projects

outward from the upper end of the sensor for connection to the associated component of the 3D tracking system. In the exemplary embodiments shown herein the sensor's body is of a generally parallelepiped shape. However, other elongated shapes, e.g., cylindrical, oval, hexagonal, etc., can clearly be utilized for the sensor. Each of the axially aligned pins has an 5 outside diameter just slightly less than the width of the slots 40 in the sidewalls 28 and 30 of the sockets 26 so that the pins 50 can be inserted therein for ultimate residence at the semi-circular inner end of the slot 40. In order to facilitate the entry of the pins into the slots the entry to each of the slots 40 is flared or chamfered slightly as best seen in Figs. 2A – 2C.

The manner of mounting each sensor into its respective socket will now be described 10 with reference to Figs. 2A – 2C. To that end, the sensor 22 is oriented at a first position so that its lower end is juxtaposed opposite the socket 26 and wherein its longitudinal axis 48A is at an angle of approximately 80 degrees to the longitudinal axis 38A of the socket's cavity as shown in Fig. 2A. The probe is then moved towards the socket so that its pins 50 enter into the respective slots 40 in the sidewalls 28 and 30 as shown in Fig. 2B until the pins reach the 15 semi-circular ends of those slots. The sensor is then rotated upward, i.e., towards the longitudinal axis 38A of the socket using the pins 50 as the pivot axis. This action causes the body 48 of the sensor to enter into the gap between the cam ends 36 of the sidewalls 28 and 30, whereupon those sidewalls flex apart slightly to allow the body 48 of the sensor to pass therebetween. When the longitudinal axis 48A of the sensor's body 48 is in a second position 20 that is parallel to the longitudinal axis 38A of the socket, the body portion of the sensor will be fully within the socket, whereupon the sidewalls 28 and 30 snap back into place thereby locking the sensor in the cavity of the socket. This second position is the heretofore mentioned locked position, wherein the sensor is resistant to accidental displacement with respect to the bracket. In particular, the cam flanges on the ends of the sidewalls 28 and 30 25 will prevent lateral displacement of the probe, while the residence of the pins 50 within the slots 40 will prevent longitudinal displacement, e.g., displacement which could occur if the sensor's cable is accidentally pulled.

Notwithstanding the above, dismounting of any sensor can be readily accomplished when desired by merely pivoting the sensor 22 in the counter-clockwise direction, i.e., away 30 from the longitudinal axis 38A of the socket, from its locked position shown in Fig. 2C, whereupon the body 48 of the sensor passes through the gap between the cam surfaces 36 on the ends of the sidewalls 28 and 30. Continued rotation of the sensor 22 in that rotational direction with respect to the socket 26 will bring it to the orientation wherein its longitudinal

axis 48A is at an angle of approximately 80 degrees to the longitudinal axis 38A of the socket. When the sensor is in this orientation (such as shown in Fig. 2B), the sensor can be pulled laterally away from the socket, like shown in Fig. 2A, thereby dismounting it from the bracket. It should be pointed out that the acute angle of 80 degrees at which the sensor body
5 is oriented to introduce its pins 50 into the slots 40 to either mount the sensor or dismount the sensor is merely exemplary. Thus, the bracket of the subject invention can be constructed so that the entry angle of the sensor is at whatever angle is desired, e.g., perpendicular or at some acute angle less than 90 degrees.

Each sensor 22 may be mounted in or dismounted from each socket 26 in the same
10 manner as described above. Moreover, while the embodiment of the bracket 20 shown in Fig. 1 includes two sockets, each identified with respective indicia, i.e., the number "1" embossed on the sidewall 28 of one socket and the number "2" embossed on the sidewall 28 of the other socket, to permit up to two sensors to be used at one time, that is not obligatory. Thus, only one sensor may be mounted on the bracket at any one time for some procedure
15 and that sensor may be mounted within either socket #1 or socket #2.

In Fig. 5 there is shown a second embodiment of a bracket 20' constructed in accordance with this invention. The bracket 20' is identical in construction to bracket 20 except that it includes a conventional biopsy needle guide assembly 100 mounted on the rear wall 24D. The needle guide can be of any desired construction. In this embodiment the
20 needle guide is a fixed angle needle guide, i.e., a guide wherein the angle that the biopsy needle is introduced into the patient's body via the transducer is a fixed, predetermined angle.

In Fig. 6 there is shown a third embodiment of a bracket 20'' constructed in accordance with this invention. The bracket 20'' is identical in construction to bracket 20' except that it includes an adjustable angle biopsy needle guide assembly 200 mounted on the
25 rear wall 24D. The adjustable needle guide assembly 200 is preferably constructed in accordance with the teachings of my aforementioned United States Patent No. 5,941,889, which as mentioned above is incorporated by reference herein, so that the biopsy needle can be introduced into the patient's body from any one of several predetermined angles. Other adjustable needle guides can be used in lieu of that adjustable needle guide.

It should be pointed out at this juncture, that while the exemplary preferred embodiments disclosed above make use of the projecting pins being located on the sensor, it is contemplated that the pins form a portion of the sockets, e.g., extend inward into the cavity 38 from respective sidewalls 28 and 30, in which case the body 48 of the sensor would have
30

to include appropriately configured slots or recesses to enable the pins of the socket to be received therein so that the sensor can be pivoted from an initial position to a locked position and vice versa.

Without further elaboration the foregoing will so fully illustrate my invention that
5 others may, by applying current or future knowledge, adopt the same for use under various conditions of service.

CLAIMS

I claim:

1. A bracket for use with an ultrasound transducer to releasably mount at least one sensor of a location sensing system on the transducer, said at least one sensor having a body including an opposed pair of wall portions, said bracket comprising a member arranged to be releasably mounted on the transducer and including at least one socket therein, said at least one socket having a pair of spaced-apart wall portions, said at least one socket and said at least one sensor being arranged to be coupled together via cooperating pins and slots to enable said at least one sensor to be oriented in a first position for insertion between said spaced-apart walls of said at least one socket to introduce said pins into respective ones of said slots so that said at least one sensor may be rotated to a second position within said at least one socket, whereupon said wall portions releasably engage a portion of said at least one sensor to deter accidental displacement of said at least one sensor with respect to the transducer.
2. The bracket of Claim 1 wherein said pins project from said opposed wall portions of said at least one sensor and are axially aligned, and wherein each of said wall portions of said at least one socket includes a slot, said slots of said at least one socket being arranged for receipt of respective ones of said pins of said at least one sensor.
3. The bracket of Claim 2 wherein said at least one sensor comprises an elongated body having a longitudinal axis and wherein said axially aligned pins project outward from a lower portion of said body perpendicular to said longitudinal axis.
4. The bracket of Claim 3 wherein said at least one socket includes a longitudinal axis and wherein the longitudinal axis of said at least one sensor is oriented parallel to said longitudinal axis of said at least one socket when said at least one sensor is in the second position.
5. The bracket of Claim 4 wherein the longitudinal axis of said at least one sensor is oriented at an acute angle to said longitudinal axis of said at least one socket when said at least one sensor is in said first position.
6. The bracket of Claim 1 wherein said wall portions snap fit about portions of said at least one sensor.
7. The bracket of claim 4 wherein said wall portions snap fit about portions of said at least one sensor.

8. The bracket of Claim 1 wherein said bracket includes a ring-like member for encircling a portion of the transducer to releasably mount said bracket thereon.

9. In combination a bracket for use with an ultrasound transducer to releasably mount at least one sensor of a location sensing system on the transducer, said at least one sensor having a body including an opposed pair of wall portions, said bracket comprising a member arranged to be releasably mounted on the transducer and including at least one socket therein, said at least one socket having a pair of spaced-apart wall portions, said at least one socket and said at least one sensor being arranged to be coupled together via cooperating pins and slots to enable said at least one sensor to be oriented in a first position for insertion between said spaced-apart walls of said at least one socket to introduce said pins into respective ones of said slots so that said at least one sensor may be rotated to a second position within said at least one socket, whereupon said wall portions releasably engage a portion of said at least one sensor to deter accidental displacement of said at least one sensor with respect to the transducer.

10. The combination of Claim 9 wherein said pins project from said opposed wall portions of said at least one sensor and are axially aligned, and wherein each of said wall portions of said at least one socket includes a slot, said slots of said at least one socket being arranged for receipt of respective ones of said pins of said at least one sensor.

11. The combination of Claim 10 wherein said sensor comprises an elongated body having a longitudinal axis and wherein said axially aligned pins project outward from a lower portion of said body perpendicular to said longitudinal axis.

12. The combination of Claim 11 wherein said at least one socket includes a longitudinal axis and wherein said longitudinal axis of said at least one sensor is oriented parallel to said longitudinal axis of said at least one socket when said at least one sensor is in said second position.

13. The combination of Claim 12 wherein the longitudinal axis of said at least one sensor is oriented at an acute angle to said longitudinal axis of said at least one socket when said at least one sensor is in said first position.


14. The combination of Claim 9 wherein said wall portions snap fit about portions of said at least one sensor.

15. The combination of Claim 10 wherein said wall portions snap fit about portions of said at least one sensor.

16. The combination of Claim 9 wherein said bracket includes a ring-like member for encircling a portion of the transducer to releasably mount said bracket thereon.

1/4

Fig. 1

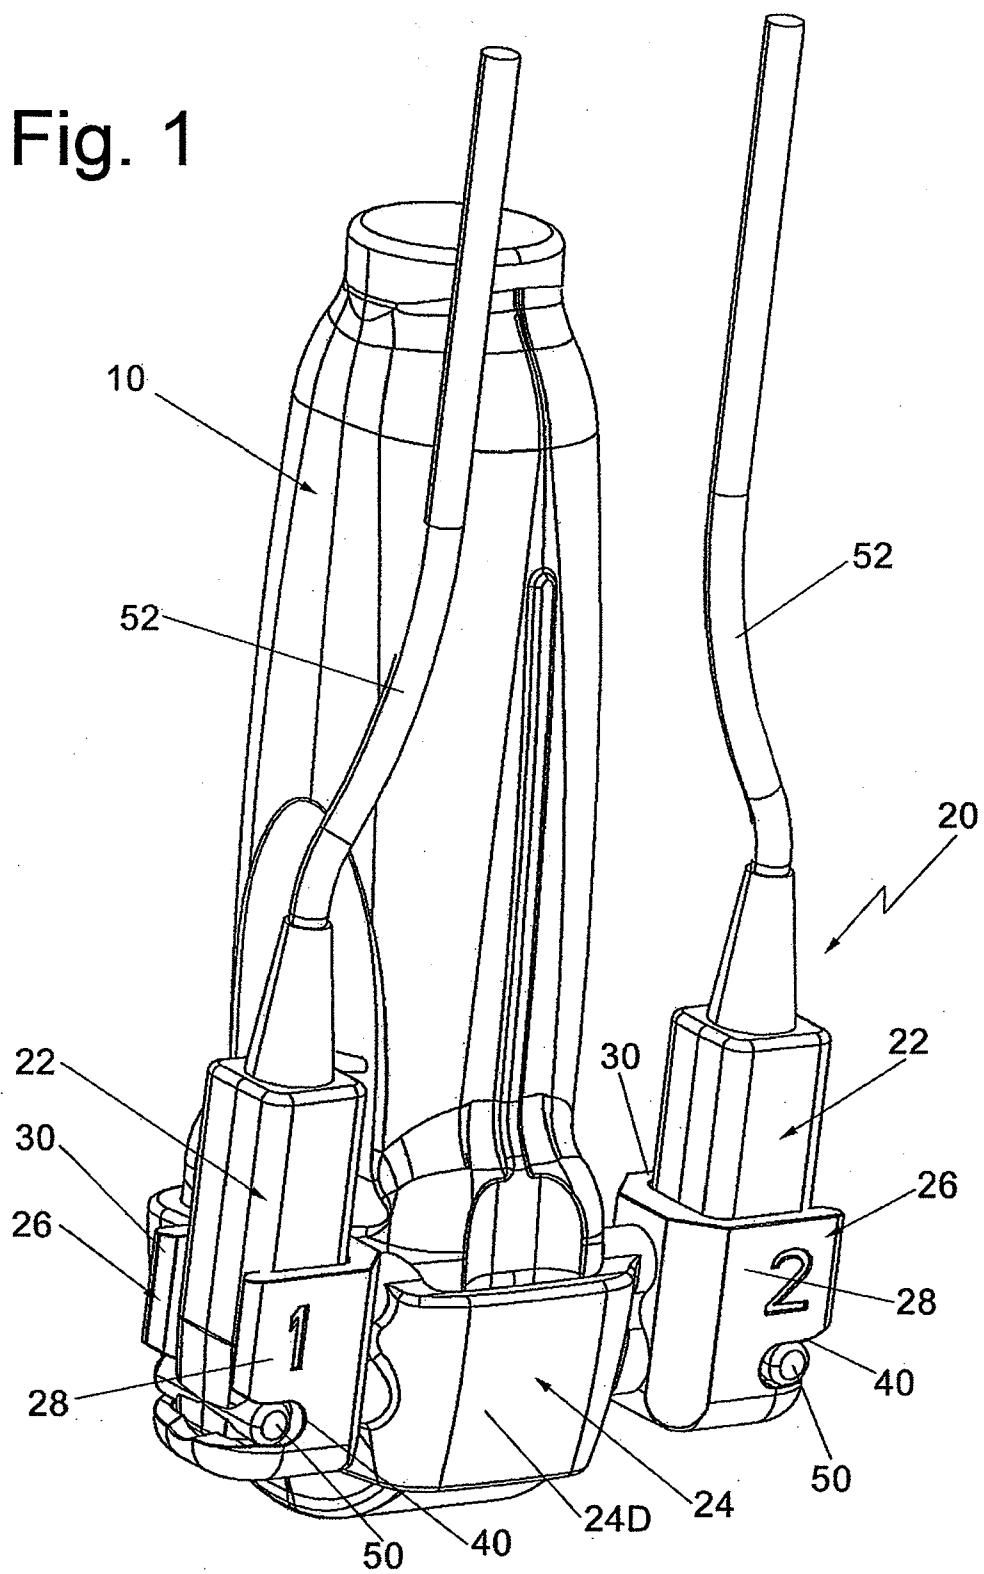

2/4

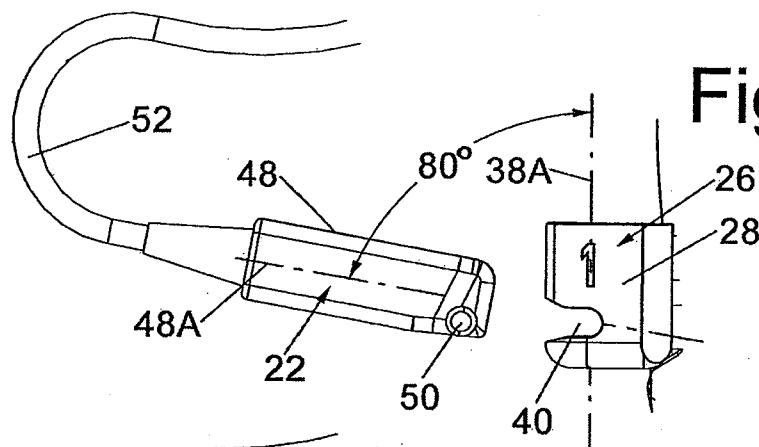


Fig. 2A

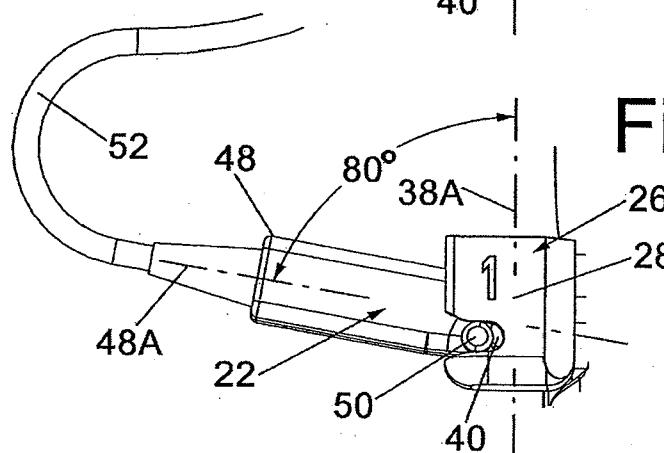


Fig. 2B

Fig. 2C

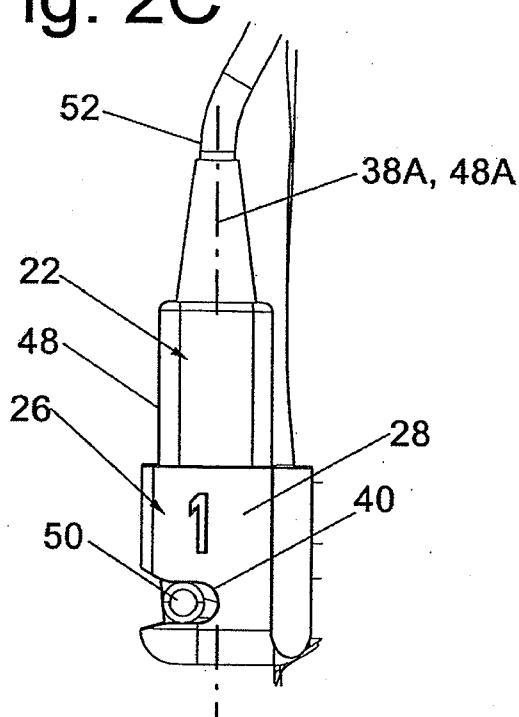


Fig. 3

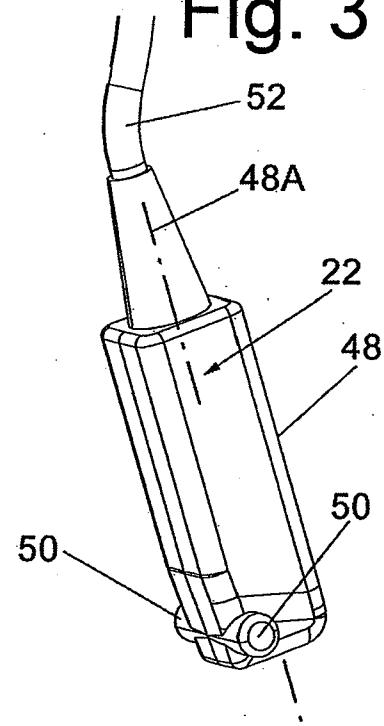


Fig. 4



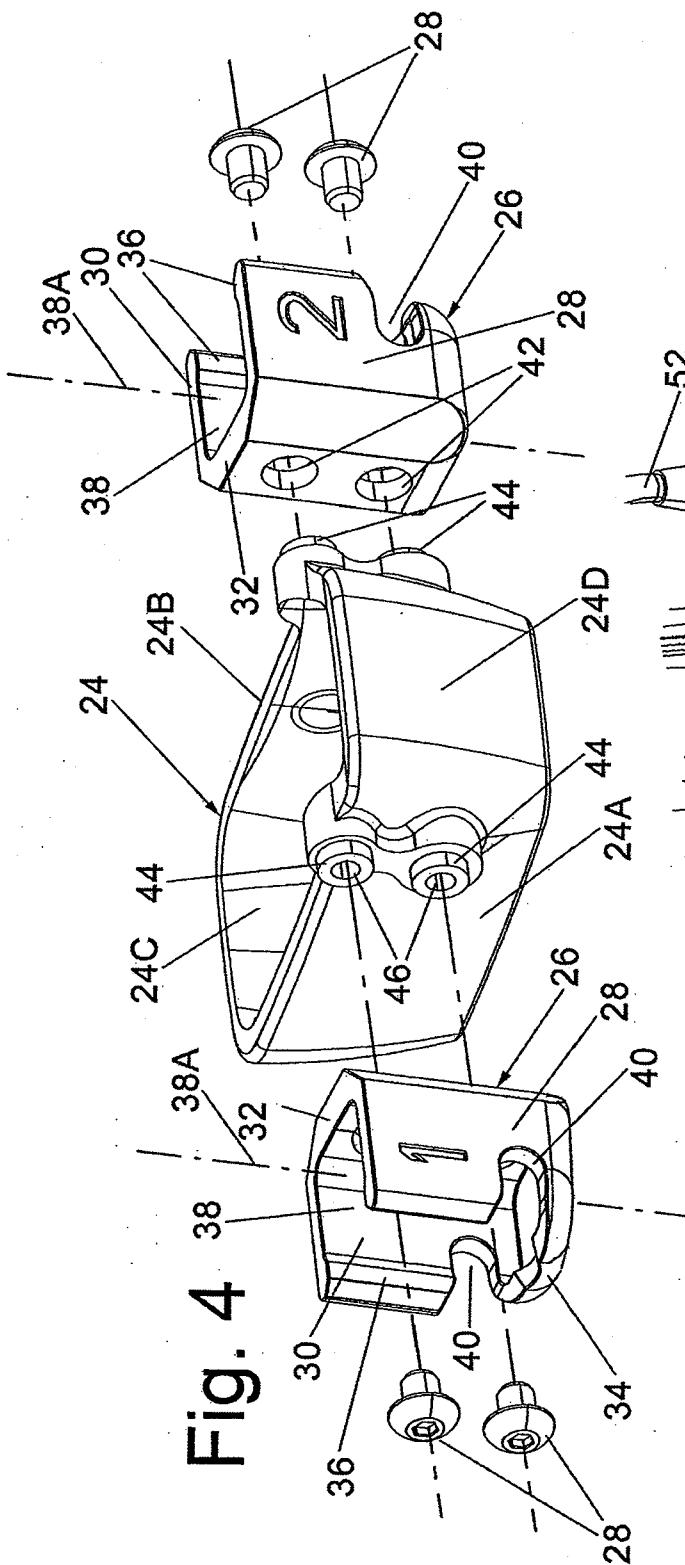


Fig. 5

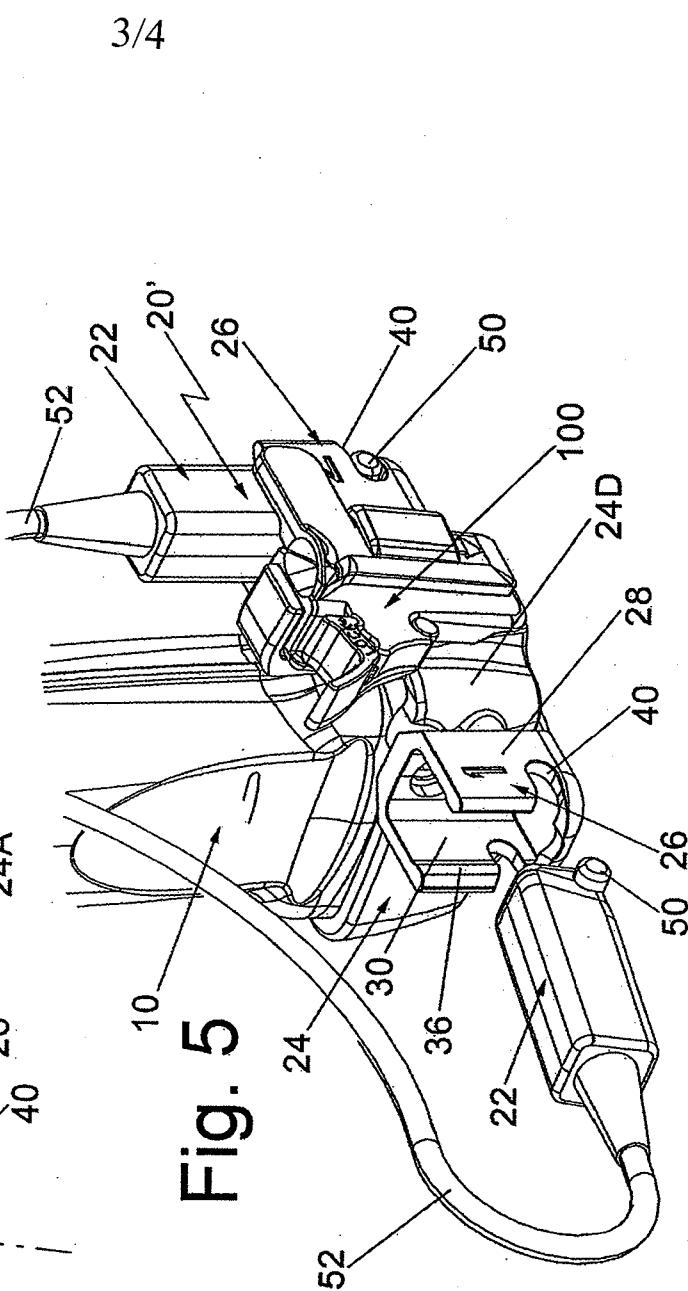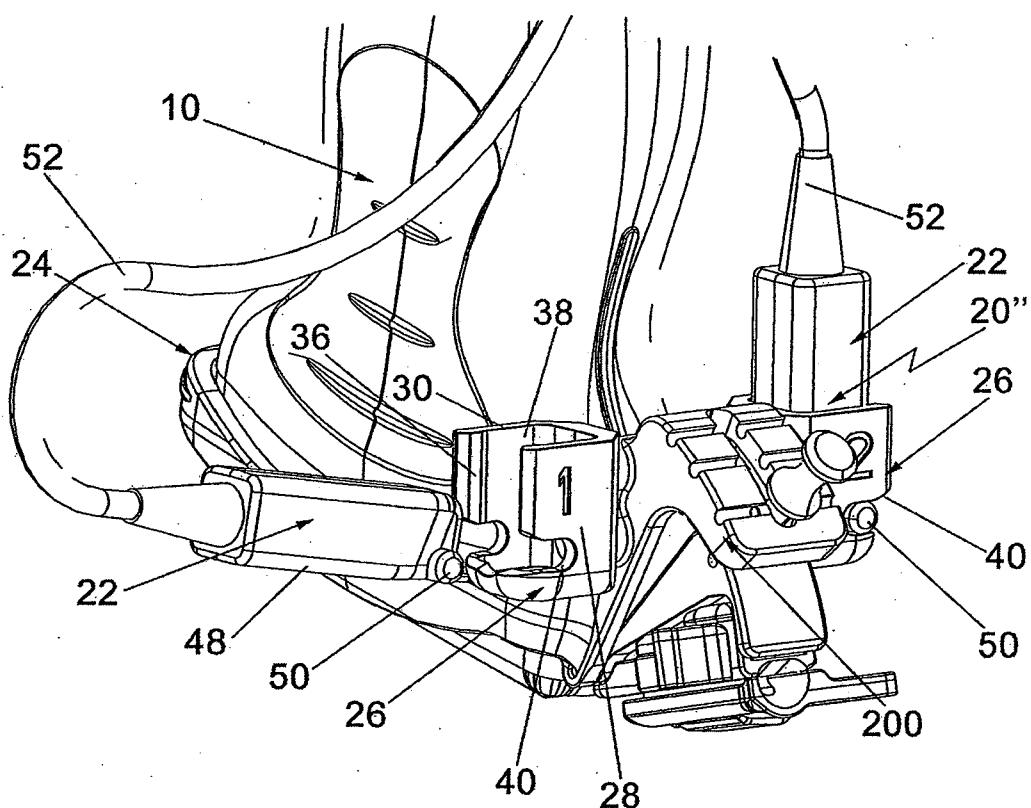

4/4

Fig. 6

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2009/041831

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61B8/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2006/072124 A1 (SMETAK EDWARD C [US] ET AL SMETAK EDWARD CHARLES [US] ET AL) 6 April 2006 (2006-04-06) paragraph [0064]; figure 3	1-5, 8-13,16
Y	US 6 190 395 B1 (WILLIAMS THOMAS R [US]) 20 February 2001 (2001-02-20) column 7, lines 3-64; figure 2	1-5, 8-13,16
A	US 2005/096536 A1 (PETERSON THOMAS H [US]) 5 May 2005 (2005-05-05) paragraph [0025]	6,7,14, 15
A	WO 96/10958 A (SIEMENS MEDICAL SYSTEMS INC [US]) 18 April 1996 (1996-04-18) page 5	6,7,14, 15
		-/-

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search

22 July 2009

Date of mailing of the international search report

30/07/2009

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Anscombe, Marcel

INTERNATIONAL SEARCH REPORT

International application No PCT/US2009/041831

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
P,A	EP 1 935 365 A (DEPUY PRODUCTS INC [US]) 25 June 2008 (2008-06-25) paragraph [0038] -----	6,7,14, 15
A	US 2004/230200 A1 (PETERSON THOMAS HERBERT [US]) 18 November 2004 (2004-11-18) paragraphs [0024], [0029] -----	6,7,14, 15
A	US 6 332 891 B1 (HIMES DAVID M [US]) 25 December 2001 (2001-12-25) column 11, lines 23-27 -----	6,7,14, 15
A	US 2007/167817 A1 (HUANG SHANZHI [CN] ET AL) 19 July 2007 (2007-07-19) paragraphs [0008], [0042] -----	6,7,14, 15
A	US 2004/049111 A1 (HIROOKA KENJI [JP] ET AL) 11 March 2004 (2004-03-11) paragraphs [0262], [0263] -----	1,9
A	US 4 896 673 A (ROSE FREEMAN H [US] ET AL) 30 January 1990 (1990-01-30) column 6, line 58 - column 7, line 5 -----	1,9
A	EP 1 491 158 A (ZIMMER TECH INC [US]) 29 December 2004 (2004-12-29) figure 5b -----	1,9
P,A	EP 1 932 477 A (HITACHI MEDICAL CORP [JP]) 18 June 2008 (2008-06-18) the whole document -----	1,9
P,A	US 2008/262356 A1 (CHALANA VIKRAM [US] ET AL) 23 October 2008 (2008-10-23) the whole document -----	1,9

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/US2009/041831	
---	--

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
US 2006072124	A1	06-04-2006	CA	2521796 A1		01-04-2006
US 6190395	B1	20-02-2001	NONE			
US 2005096536	A1	05-05-2005	DE	102004053684 A1		02-06-2005
			FR	2861830 A1		06-05-2005
WO 9610958	A	18-04-1996	DE	69509402 D1		02-06-1999
			DE	69509402 T2		28-10-1999
			EP	0785755 A2		30-07-1997
			US	5623931 A		29-04-1997
EP 1935365	A	25-06-2008	US	2008177173 A1		24-07-2008
US 2004230200	A1	18-11-2004	US	2006084946 A1		20-04-2006
US 6332891	B1	25-12-2001	NONE			
US 2007167817	A1	19-07-2007	CN	1985769 A		27-06-2007
US 2004049111	A1	11-03-2004	NONE			
US 4896673	A	30-01-1990	NONE			
EP 1491158	A	29-12-2004	AU	2004202764 A1		13-01-2005
			CA	2467532 A1		24-12-2004
			JP	2005013737 A		20-01-2005
			US	2004267242 A1		30-12-2004
EP 1932477	A	18-06-2008	CN	101193594 A		04-06-2008
			WO	2007040172 A1		12-04-2007
US 2008262356	A1	23-10-2008	NONE			

专利名称(译)	用于在超声波探头上安装至少一个位置检测传感器的支架		
公开(公告)号	EP2293722A1	公开(公告)日	2011-03-16
申请号	EP2009739522	申请日	2009-04-27
申请(专利权)人(译)	CIVCO医疗器械CO. , INC.		
当前申请(专利权)人(译)	CIVCO医疗器械CO. , INC.		
[标]发明人	CERMAK CRAIG J		
发明人	CERMAK, CRAIG, J.		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4254 A61B8/4245 A61B8/4281 A61B2017/00477		
优先权	12/111387 2008-04-29 US		
其他公开文献	EP2293722B1		
外部链接	Espacenet		

摘要(译)

一种支架 (20)，用于超声换能器 (10) 上，以将至少一个3D跟踪传感器 (22) 可释放地安装在换能器上。每个传感器具有一对轴向对齐的销 (50)，其从主体向外突出。支架包括至少一个插座 (26)，插座 (26) 具有一对间隔开的壁部分 (28,30)，每个壁部分包括一个槽 (40)，当传感器位于传感器时，该槽设置成接收传感器的相应一个销。在第一个位置。从该位置，传感器的主体可以旋转到第二位置，于是间隔开的壁部分可释放地接合 (卡扣配合) 传感器 (22) 的主体的一部分，以阻止传感器相对于传感器的意外移位。换能器。