




- (51) **International Patent Classification:**  
G01N 29/24 (2006.01) H04R 17/00 (2006.01)  
A61B 8/00 (2006.01)
- (21) **International Application Number:**  
PCT/KR2013/003439
- (22) **International Filing Date:**  
23 April 2013 (23.04.2013)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**  
10-2012-0041904 23 April 2012 (23.04.2012) KR
- (71) **Applicant:** HEALCERION CO., LTD. [KR/KR]; 409, 72, Digital-ro 26-gil, Guro-gu, Seoul 152-801 (KR).
- (72) **Inventors:** RYU, Jeong Won; 402, 14, Gasan-ro 5-gil, Geumcheon-gu, Seoul 153-801 (KR). CHOUNG, You Chan; 101-1405, 47, Seoreung-ro 21-gil, Eunpyeong-gu, Seoul 122-807 (KR).
- (74) **Agent:** YOON, Jae Seung; 7th Floor, Deokcheon Bldg., 718-10 Yeoksam-dong, Gangnam-gu, Seoul 135-080 (KR).


- (81) **Designated States** (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) **Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Published:**  
— with international search report (Art. 21(3))

(54) **Title:** MOBILE ULTRASOUND DIAGNOSIS PROBE APPARATUS FOR USING TWO-DIMENSION ARRAY DATA, MOBILE ULTRASOUND DIAGNOSIS SYSTEM USING THE SAME

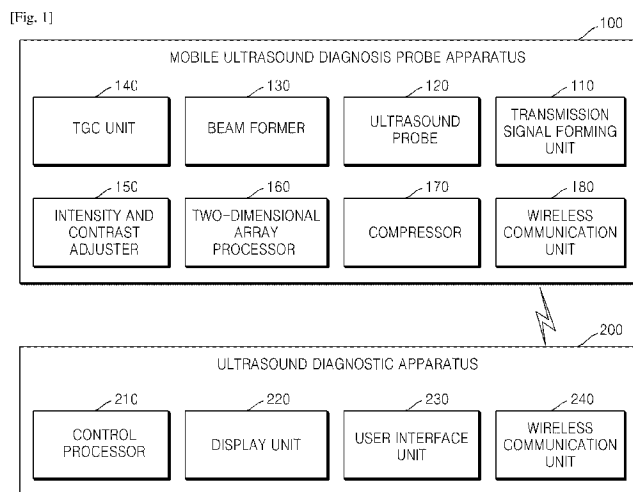

(57) **Abstract:** Provided is a mobile ultrasound diagnosis probe apparatus including a transmission signal forming unit forming a transmission signal for obtaining a frame of an ultrasound image, an ultrasound probe transducing the transmission signal of the transmission signal forming unit into an ultrasound signal, transmitting the ultrasound signal to an object, and obtaining analog ultrasound data reflected from the object, a two-dimensional array processor adjacently arranging the obtained analog ultrasound data compensated with respect to time gains thereof and adjusted with respect to intensity and contrast thereof for each ultrasound vector to be processed into two-dimensional array ultrasound data, a compressor compressing the two-dimensional array ultrasound data adjacently arranged for each ultrasound vector, and a wireless communication unit wirelessly transmitting the compressed two-dimensional array ultrasound data to an ultrasound diagnostic apparatus.



## Description

### **Title of Invention: MOBILE ULTRASOUND DIAGNOSIS PROBE APPARATUS FOR USING TWO-DIMENSION ARRAY DATA, MOBILE ULTRASOUND DIAGNOSIS SYSTEM USING THE SAME**

#### **Technical Field**

- [1] The present invention relates to a mobile ultrasound diagnosis probe apparatus and a mobile ultrasound diagnosis system using the same, and more particularly, to a mobile ultrasound diagnosis probe apparatus processing ultrasound data obtained from an object into two-dimensional array data and compressing and wirelessly transmitting the two-dimensional array data and a mobile ultrasound diagnosis system using the apparatus.

#### **Background Art**

- [2] Since having noninvasive and nondestructive properties, ultrasound diagnosis systems are generally used in the medical field to obtain information of the inside of an object. Since surgical operations of directly incising and observing objects are unnecessary and high-resolution images of internal organizations of objects may be provided to doctors, ultrasound diagnosis systems are very importantly used in the medical field.
- [3] Generally, an ultrasound system includes an ultrasound probe, a beam former, a data processor, a scan transducer, and a display unit. The ultrasound probe transmits an ultrasound signal to an object and forms a reception signal by receiving a reflected ultrasound signal, that is, an ultrasound echo signal. The ultrasound probe includes at least one transducer element operating to transduce an ultrasound signal and an electric signal into one another. The beam former analog/digital-transduces the reception signal provided from the ultrasound probe, delays a time of a digital signal considering a position and a focusing point of each transducer element, and forms ultrasound data, that is, radio frequency (RF) data by summing the time-delayed digital signals up. The data processor performs various data processes with respect to ultrasound data, which are necessary for forming an ultrasound image. The scan transducer scan-transduces the processed ultrasound data to be displayed on a display area of the display unit. The display unit displays the scan-transduced ultrasound data as an ultrasound image on a screen.
- [4] Typically, data processing such as a time gain compensation (TGC) process, a plurality of finite impulse response (FIR) filtering processes, a plurality of decimation

processes, an in-phase/quadrature-phase (I/Q) data forming process, and a compression process and a scan transducing process are sequentially performed. Due thereto, not only a lot of time is consumed to process a large amount of ultrasound data but also a frame rate is deteriorated.

[5]

## **Disclosure of Invention**

### **Technical Problem**

[6] The present invention provides a mobile ultrasound diagnosis probe apparatus processing ultrasound data obtained from an object into two-dimensional array data and compressing and wirelessly transmitting the two-dimensional array data and a mobile ultrasound diagnosis system using the apparatus.

### **Solution to Problem**

[7] To achieve these and other advantages and in accordance with the purpose of the present invention, as embodied and broadly described, there is provided a

[8] According to another aspect of the present invention, there is provided mobile ultrasound diagnosis probe apparatus including a transmission signal forming unit forming a transmission signal for obtaining a frame of an ultrasound image, an ultrasound probe transducing the transmission signal of the transmission signal forming unit into an ultrasound signal, transmitting the ultrasound signal to an object, and obtaining analog ultrasound data reflected from the object, a two-dimensional array processor adjacently arranging the obtained analog ultrasound data compensated with respect to time gains thereof and adjusted with respect to intensity and contrast thereof for each ultrasound vector to be processed into two-dimensional array ultrasound data, a compressor compressing the two-dimensional array ultrasound data adjacently arranged for each ultrasound vector, and a wireless communication unit wirelessly transmitting the compressed two-dimensional array ultrasound data to an ultrasound diagnostic apparatus.

[9] The two-dimensional array processor may arrange received ultrasound vectors in a serial stream to be adjacent for each ultrasound vector unit lengthwise to be processed into the two-dimensional array ultrasound data.

[10] The mobile ultrasound diagnosis probe apparatus may further include a beam former generating digitalized ultrasound data by using the analog ultrasound data obtained from the ultrasound probe, a time gain compensation (TGC) unit compensating the digitalized ultrasound data with time gains, and an intensity and contrast adjuster adjusting intensity and contrast of the ultrasound image.

[11] The mobile ultrasound diagnosis probe apparatus may further include a TGC unit compensating the analog ultrasound data obtained from the ultrasound probe with time

gains, a beam former generating digitalized ultrasound data by using the ultrasound data compensated with time gains, and an intensity and contrast adjuster adjusting intensity and contrast of the ultrasound image.

[12] The beam former may include M number of arrays whose size is N when using M number of ultrasounds for one ultrasound image frame and performing N times of sampling each ultrasound that is reflected from the object and returns. The TGC unit may compensate the ultrasound data according to a TGC table.

[13] The intensity and contrast adjuster may adjust an intensity value of a certain value or less to 0 and may adjust an intensity value of a certain value or more to a maximum value. The intensity and contrast adjuster may adjust a contrast value of a certain value or less to 0 and may adjust a contrast value of a certain value or more to a maximum value.

[14] The two-dimensional array processor may generate two-dimensional ultrasound data including  $N \times M$  arrays when using M number of ultrasounds for one ultrasound image frame and performing N times of sampling each ultrasound that is reflected from the object and returns.

[15] The wireless communication unit may include short-distance wireless communication by using one of Bluetooth, a wireless universal serial bus (USB), a wireless local area network (LAN), wireless fidelity (WiFi), Zigbee, and infrared data association (IrDA).

[16] According to another aspect of the present invention, there is provided a mobile ultrasound diagnostic system including a mobile ultrasound diagnosis probe apparatus, which is portable, digital-processes ultrasound data obtained from an object, compensates the digitalized ultrasound data with time gains, adjusts intensity and contrast of the ultrasound data, processes the ultrasound data into two-dimensional array ultrasound data by adjacently arranging for each ultrasound vector, compresses the two-dimensional array ultrasound data, and wirelessly transmits the two-dimensional array ultrasound data, and an ultrasound diagnostic apparatus, which receives the two-dimensional array ultrasound data from the mobile ultrasound diagnosis probe apparatus and generates ultrasound image data for diagnosis by releasing compression of the two-dimensional array ultrasound data.

[17] The mobile ultrasound diagnosis probe apparatus may arrange received ultrasound vectors in a serial stream to be adjacent for each ultrasound vector unit lengthwise to be processed into the two-dimensional array ultrasound data.

[18] The ultrasound diagnostic apparatus may determine an ultrasound measurement depth according to an input of a user and may transmit a parameter for adjusting time gains and a parameter for adjusting the intensity and the contrast to the mobile ultrasound diagnosis probe apparatus.

[19] The ultrasound diagnostic apparatus may transmit dummy data for automatically measuring a wireless communication environment and for determining the size of transmission data to the mobile ultrasound diagnosis probe apparatus, and the mobile ultrasound diagnosis probe apparatus may receive the dummy data from the ultrasound diagnostic apparatus, may calculate an available band of wireless communication currently used by measuring an amount of time used to receive the dummy data, and may determine the size of data to be wirelessly transmitted, according to the available band.

[20]

### **Advantageous Effects of Invention**

[21] According to the present invention, According to the present invention, since a throughput of processing ultrasound data may be more reduced than processing image data by time gain compensation, intensity and contrast adjustment, and two-dimensional array data processing operation in a mobile ultrasound diagnosis probe apparatus, programs operated in an ultrasound diagnostic apparatus may be simplified and consumption of resources such as a memory and a central processing unit (CPU). In addition, the ultrasound diagnostic apparatus may be applied to a mobile device having relatively low specifications.

### **Brief Description of Drawings**

[22] FIG. 1 is a block view illustrating a mobile ultrasound diagnosis system according to an embodiment of the present invention;

[23] FIG. 2 is a view illustrating a transmitting ultrasound vector of an ultrasound probe according to an embodiment of the present invention;

[24] FIG. 3 is a view illustrating ultrasound data when M number of ultrasounds are used and N times of samplings are performed;

[25] FIG. 4 is a view illustrating a time gain compensation operation according to an embodiment of the present invention;

[26] FIG. 5 is a view illustrating intensity adjustment according to an embodiment of the present invention;

[27] FIG. 6 is a view illustrating contrast adjustment according to an embodiment of the present invention;

[28] FIG. 7 is a view illustrating two-dimensional arrangement according to an embodiment of the present invention;

[29] FIGS. 8 to 10 are views illustrating a two-dimensional arrangement process according to an embodiment of the present invention; and

[30] FIGS. 11 to 14 are views illustrating a two-dimensional arrangement process according to another embodiment of the present invention.

[31]

### **Best Mode for Carrying out the Invention**

[32] Hereinafter, the embodiments of the present invention will be described in detail with reference to the attached drawings. The following embodiments are provided as examples to fully convey the spirits of the present invention to a person skilled in the art. Accordingly, the present invention is not limited to the embodiments described below and may be embodied in other forms. Also, in the drawings, a width, a length, and a thickness of an element may be exaggerated for convenience of description. Like reference numerals designate like elements throughout.

[33] FIG. 1 is a block view illustrating a mobile ultrasound diagnosis system according to an embodiment of the present invention.

[34] Referring to FIG. 1, the ultrasound diagnosis system may include a mobile ultrasound diagnosis probe apparatus 100 and an ultrasound diagnostic apparatus 200.

[35] The mobile ultrasound diagnosis apparatus 100 may include a transmission signal forming unit 110, an ultrasound probe 120 including a plurality of transducer elements, a beam former 130, a time gain compensation (TGC) unit 140, an intensity and contrast adjuster 150, a two-dimensional array processor 160, a compressor 170, and a wireless communication unit 180.

[36] The transmission signal forming unit 110 forms a plurality of transmission signal for obtaining a frame of an ultrasound image by considering the transducer elements of the ultrasound probe 120 and a focusing point. The frame is formed of a plurality of scan lines. Also, the ultrasound image may include a brightness mode (B-mode) image in which a reflection coefficient of an ultrasound echo signal reflected from an object is shown as a two-dimensional image, a Doppler mode (D-mode) image in which the velocity of a moving object is shown as a Doppler spectrum by using a Doppler effect, a color mode (C-mode) image in which the velocity of a moving object and a scatterer are shown in color by using the Doppler effect, an elastic mode (E-mode) image in which a difference between mechanical responses of a medium when applying stress to an object or not is shown as an image, and a three-dimensional mode (3D-mode) image in which a reflection coefficient of an ultrasound echo signal reflected from an object is shown as a 3D image.

[37] The ultrasound probe 120, as shown in FIG. 2, transduces the transmission signal provided from the transmission signal forming unit 110 into an ultrasound signal and transmit the ultrasound signal to an object. The ultrasound probe 120 receives the ultrasound echo signal reflected from the object and forms a reception signal. The ultrasound probe 120 forms a plurality of reception signals by repetitively performing transmission and reception of the ultrasound signals by using the plurality of

transmission signals. In this case, since having vector data, the ultrasound signals transmitted and received by the ultrasound probe 120 are designated as ultrasound vectors. For example, ultrasound vectors transmitted from the ultrasound probe 120 to a human body are designated as transmission ultrasound vectors, and ultrasound vectors echoed from the human body to the ultrasound probe 120 are designated as reception ultrasound vectors.

[38] In the present embodiment, the ultrasound probe 120 may be embodied as a convex probe, a linear probe, a 3D dimensional probe, a trapezoidal probe, and an intravascular ultrasound (IVUS) probe.

[39] The beam former 130 analog/digital-transduces the plurality of reception signals provided from the ultrasound probe 120 and generates digitalized ultrasound data. In addition, the beam former 130, considering the transducer elements of the ultrasound probe 120 and the focusing point, receives and focuses a plurality of digital-transduced reception signals and forms a plurality of digital reception focusing beams. In the present embodiment, the beam former 130, to improve the speed of processing reception signals, may be embodied as a field programmable gate array (FPGA) or an application specific integrated circuit (ASIC).

[40] The digitalized ultrasound data, as shown in FIG. 3, are data stored as an array capable of being shown as intensity values in the ultrasound image. The size of the array is determined according to the number of sampling ultrasounds that are reflected by the human body and return. The number of the arrays for each ultrasound image may be determined according to the number of ultrasound used to form each ultrasound image. When M number of ultrasounds are used for each ultrasound image and N times of sampling each ultrasound that is reflected by the human body and returns are performed, M number of arrays whose size if N may be generated.

[41] The TGC unit 140, as shown in FIG. 3, compensates time gains of the digitalized ultrasound data.

[42] Since ultrasound is absorbed in the human body due to properties thereof, ultrasound reflected by a deeper position and returns later is reduced in size because a greater loss of energy occurs. In the same human body, the size of ultrasound data reflected by the deeper position is relatively smaller. Accordingly, it is necessary to compensate with a greater value in proportion to a time for being reflected and returning. When using the ultrasound data array whose size is N, a compensation value is determined by generating a time gain compensation table having the same size and is added to an ultrasound data array value.

[43] The intensity and contrast adjuster 150 adjusts the intensity and the contrast of the ultrasound image. When the intensity and contrast adjuster 150 lowers an intensity value, an intensity value of a certain value or less is changed into 0. When the intensity and

contrast adjuster 150 makes an intensity value higher, an intensity value or a certain value or more is changed into a maximum value.

[44] Accordingly, referring to FIGs. 5 and 6, an intensity value smaller than a is adjusted into 0 when the intensity value is lowered by intensity value adjustment of the intensity and contrast adjuster 150 and an intensity value greater than b is adjusted into the maximum value.

[45] The intensity and contrast adjuster 150 may adjust the contrast of the ultrasound image. When the intensity and contrast adjuster 150 adjusts the contrast, the contrast in an intensity area having the importance in the ultrasound image is emphasized and other areas may be made as 0 or the maximum value.

[46] Accordingly, when the intensity and contrast adjuster 150 adjusts the contrast, as shown in FIG. 5, a contrast difference increases while the intensity value exists within a range from a to b, is changed into 0 while being smaller than a, and is changed into the maximum value while being greater than b.

[47] According to the operations of the TGC unit 140 and the intensity and contrast adjuster 150, the ultrasound data may be changed into 0 or the maximum value. Accordingly, when the same values are more generated, efficiency of a subsequent compression process becomes higher.

[48] As described above, the ultrasound data are processed and wirelessly transmitted by the TGC unit 140 and the intensity and contrast adjuster 150, thereby simplifying a program operated in the ultrasound diagnostic apparatus 200 and reducing consumption of resources such as a memory and a CPU. The ultrasound diagnostic apparatus 200 may be applied to a mobile device whose specifications are relatively low.

[49] The two-dimensional array processor 160 processes the ultrasound data whose time gains are compensated and intensity and contrast are adjusted into two-dimensional array ultrasound data. The two-dimensional array processor 160 may form a two-dimensional array by adjacently arranging received ultrasound vectors echoed from the human body.

[50] The two-dimensional array processor 160 may arrange the reception ultrasound vectors echoed from the human body, for example, adjacently lengthwise, instead of forming an image by collecting the reception ultrasound vectors. The two-dimensional array processor 160 provides the compressor 170 the respective reception ultrasound vectors adjacently arranged, to be compressed.

[51] The reception ultrasound vectors echoed from the human body are processed by the two-dimensional array processor 160 to be adjacently arranged instead of being collected to form an image in such a way that continuity of image patterns is increased and additionally the size of data becomes smaller relatively to image data. When the

size of data to be processed becomes smaller, data to be processed in a compression process performed by the compressor 170 may be reduced as that.

[52] FIGS. 8 and 10 are views illustrating a two-dimensional arrangement process according to an embodiment of the present invention.

[53] Referring to FIG. 8, the ultrasound probe 120 sequentially sends a first transmission ultrasound vector and a second transmission ultrasound vector to a human body. A reference numeral 10 indicates transmission ultrasound vectors. In addition, the ultrasound probe 120 receives a first reception ultrasound vector and a second reception ultrasound vector echoed from the human body. A reference numeral 20 indicates reception ultrasound vectors. The two-dimensional array processor 160 arranges the echoed first reception ultrasound vector and second reception ultrasound vector to be adjacent to each other lengthwise.

[54] Referring to FIG. 9, the ultrasound probe 120 sends a third transmission ultrasound vector to the human body. In addition, the ultrasound probe 120 receives a third reception ultrasound vector echoed from the human body. The two-dimensional array processor 160 arranges the third reception ultrasound vector to be adjacent to the second reception ultrasound vector lengthwise.

[55] Referring to FIG. 10, the ultrasound probe 120 sequentially emits an Mth transmission ultrasound vector to the human body. In addition, the ultrasound probe 120 receives an Mth reception ultrasound vector echoed from the human body. The two-dimensional array processor 160 arranges the Mth reception ultrasound vector to be adjacent to an M-1th reception ultrasound vector lengthwise.

[56] In a modified example, the beam former 130 may include a two-dimensional array processing function and may generate an array for storing initial ultrasound data as a two-dimensional array.

[57] A reason of applying the two-dimensional array is to compress data with a high compression rate. When ultrasound are compressed into a stream type in which one dimensional arrays are sequentially disposed, since compression is performed by using before and after values in order, a compression rate thereof is not high. For example, the compression rate may have a size of 60% of an original as an average. However, when image compression technology is used by two-dimensionally arranging using the two-dimensional array processor 160, since it is possible to use all peripheral values, compression into a size of 30% of the original may be performed in the case of lossless compression. When applying loss compression such as JPEG method, a different becomes greater.

[58] The compressor 170 compresses ultrasound data to be transmitted to the ultrasound diagnostic apparatus 200. To effectively using a limited band under a wireless communication environment, compression is needed. The compressor 170 compresses the

two-dimensional array data generated by the two-dimensional array processor 160. Accordingly, the compressor 170 may increase a compression rate by using the image compression technology instead of data compression. The compressor 170 may use both lossless compression and loss compression according to purpose of use and a wireless communication method.

- [59] The wireless communication unit 180 wirelessly transmits data compressed by the compressor 170 to the ultrasound diagnostic apparatus 200.
- [60] The wireless communication unit 180 may include, for example, short-distance wireless communication by using one of Bluetooth, a wireless universal serial bus (USB), a wireless local area network (LAN), wireless fidelity (WiFi), Zigbee, and infrared data association (IrDA).
- [61] The ultrasound diagnostic apparatus 200 has a wireless communication function and a display unit and may include various devices capable of operating application programs. For example, there may be a personal computer, a smart phone, a tablet type device, a pad type device, and personal digital assistants.
- [62] The ultrasound diagnostic apparatus 200 may include a control processor 210, a display unit 220, a user interface unit 230, and a wireless communication unit 240.
- [63] The control processor 210 receives ultrasound data from the mobile ultrasound diagnosis probe apparatus 100 via the wireless communication unit 240. The control processor 210 releases compression of the received ultrasound data by using the same method as that used by the mobile ultrasound diagnosis probe apparatus 100 and obtains two-dimensional array data. The control processor 210 generates an ultrasound image available to be displayed on a screen of the display unit 220 by using the released two-dimensional array data. The control processor 210 determines the size of the ultrasound image by considering the size of the screen of the display unit 220.
- [64] The control processor 210 may receive an input of a user via the user interface unit 230 and may forward the input to the mobile ultrasound diagnosis probe apparatus 100 by using wireless communication.
- [65] The control processor 210 determines, according to the input of the user, an ultrasound measurement depth, a parameter used by the TGC unit 140, and a degree of adjustment of the intensity and contrast adjuster 150.
- [66] The control processor 210 may determine whether to automatically measure a wireless communication environment and may determine the size of transmission data. The control processor 210 transmits dummy data having a certain size to the mobile ultrasound diagnosis probe apparatus 100.
- [67] Accordingly, the wireless communication unit 180 of the mobile ultrasound diagnosis probe apparatus 100 receives the dummy data from the ultrasound diagnostic apparatus 200 and calculates an available band of wireless communication currently

used by measuring an amount of time used for receiving the dummy data.

[68] The wireless communication unit 180 of the mobile ultrasound diagnosis probe apparatus 100 determines the size of data to be wirelessly transmitted, according to the available band. When the band is smaller, a rate of frames to be transmitted becomes reduced.

[69] While the present invention has been particularly shown and described with reference to exemplary embodiments thereof, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope of the present invention as defined by the following claims.

[70] For example, in the present embodiment, it has been described that a transmission signal of a transmission signal forming unit in an ultrasound probe is transduced into an ultrasound signal and transmitted to an object, analog ultrasound data reflected from the object are obtained, and digitalized ultrasound data is generated by a beam former using the obtained analog ultrasound data and compensated with respect to time gains by a TGC unit. However, the present invention is not limited thereto. In another modified example, a transmission signal of a transmission signal forming unit in an ultrasound probe is transduced into an ultrasound signal and transmitted to an object, analog ultrasound data reflected from the object are obtained, the obtained analog ultrasound data are compensated with respect to time gains by a TGC unit, and digitalized ultrasound data may be generated by a beam former using the analog ultrasound data compensated with respect to the time gains.

[71]

### **Sequence Listing Free Text**

[72] 100: a mobile ultrasound diagnosis probe apparatus

[73] 110: a transmission signal forming unit

[74] 120: an ultrasound probe

[75] 130: a beam former

[76] 140: a time gain compensation (TGC) unit

[77] 150: an intensity and contrast adjuster

[78] 160: a two-dimensional array processor

[79] 170: a compressor

[80] 180: a wireless communication unit

[81] 200: an ultrasound diagnostic apparatus

[82] 210: a control processor

[83] 220: a display unit

[84] 230: a user interface unit

[85] 240: a wireless communication unit

## Claims

- [Claim 1] A mobile ultrasound diagnosis probe apparatus comprising:  
a transmission signal forming unit forming a transmission signal for obtaining a frame of an ultrasound image;  
an ultrasound probe transducing the transmission signal of the transmission signal forming unit into an ultrasound signal, transmitting the ultrasound signal to an object, and obtaining analog ultrasound data reflected from the object;  
a two-dimensional array processor adjacently arranging the obtained analog ultrasound data compensated with respect to time gains thereof and adjusted with respect to intensity and contrast thereof for each ultrasound vector to be processed into two-dimensional array ultrasound data;  
a compressor compressing the two-dimensional array ultrasound data adjacently arranged for each ultrasound vector; and  
a wireless communication unit wirelessly transmitting the compressed two-dimensional array ultrasound data to an ultrasound diagnostic apparatus.
- [Claim 2] The apparatus of claim 1, wherein the two-dimensional array processor arranges received ultrasound vectors in a serial stream to be adjacent for each ultrasound vector unit lengthwise to be processed into the two-dimensional array ultrasound data.
- [Claim 3] The apparatus of claim 1, further comprising:  
a beam former generating digitalized ultrasound data by using the analog ultrasound data obtained from the ultrasound probe;  
a time gain compensation (TGC) unit compensating the digitalized ultrasound data with time gains; and  
an intensity and contrast adjuster adjusting intensity and contrast of the ultrasound image.
- [Claim 4] The apparatus of claim 1, further comprising:  
a TGC unit compensating the analog ultrasound data obtained from the ultrasound probe with time gains;  
a beam former generating digitalized ultrasound data by using the ultrasound data compensated with time gains; and  
an intensity and contrast adjuster adjusting intensity and contrast of the ultrasound image.
- [Claim 5] The apparatus according to any one of claims 3 and 4, wherein the

beam former generates ultrasound data comprising M number of arrays whose size is N when using M number of ultrasounds for one ultrasound image frame and performing N times of sampling each ultrasound that is reflected from the object and returns.

[Claim 6] The apparatus according to any one of claims 3 and 4, wherein the TGC unit compensates the ultrasound data according to a TGC table.

[Claim 7] The apparatus according to any one of claims 3 and 4, wherein the intensity and contrast adjuster adjusts an intensity value of a certain value or less to 0 and adjusts an intensity value of a certain value or more to a maximum value.

[Claim 8] The apparatus according to any one of claims 3 and 4, wherein the intensity and contrast adjuster adjusts a contrast value of a certain value or less to 0 and adjusts a contrast value of a certain value or more to a maximum value.

[Claim 9] The apparatus of claim 1, wherein the two-dimensional array processor generates two-dimensional ultrasound data comprising  $N \times M$  arrays when using M number of ultrasounds for one ultrasound image frame and performing N times of sampling each ultrasound that is reflected from the object and returns.

[Claim 10] The apparatus of claim 1, wherein the wireless communication unit comprises short-distance wireless communication by using one of Bluetooth, a wireless universal serial bus (USB), a wireless local area network (LAN), wireless fidelity (WiFi), Zigbee, and infrared data association (IrDA).

[Claim 11] A mobile ultrasound diagnostic system comprising:  
a mobile ultrasound diagnosis probe apparatus, which is portable, digital-processes ultrasound data obtained from an object, compensates the digitalized ultrasound data with time gains, adjusts intensity and contrast of the ultrasound data, processes the ultrasound data into two-dimensional array ultrasound data by adjacently arranging for each ultrasound vector, compresses the two-dimensional array ultrasound data, and wirelessly transmits the two-dimensional array ultrasound data, and an ultrasound diagnostic apparatus, which receives the two-dimensional array ultrasound data from the mobile ultrasound diagnosis probe apparatus and generates ultrasound image data for diagnosis by releasing compression of the two-dimensional array ultrasound data.

[Claim 12] The system of claim 11, wherein the mobile ultrasound diagnosis probe apparatus arranges received ultrasound vectors in a serial stream to be

adjacent for each ultrasound vector unit lengthwise to be processed into the two-dimensional array ultrasound data.


[Claim 13]

The system of claim 11, wherein the ultrasound diagnostic apparatus determines an ultrasound measurement depth according to an input of a user and transmits a parameter for adjusting time gains and a parameter for adjusting the intensity and the contrast to the mobile ultrasound diagnosis probe apparatus.


[Claim 14]

The system of claim 11, wherein the ultrasound diagnostic apparatus transmits dummy data for automatically measuring a wireless communication environment and for determining the size of transmission data to the mobile ultrasound diagnosis probe apparatus, and wherein the mobile ultrasound diagnosis probe apparatus receives the dummy data from the ultrasound diagnostic apparatus, calculates an available band of wireless communication currently used by measuring an amount of time used to receive the dummy data, and determines the size of data to be wirelessly transmitted, according to the available band.


[Fig. 1]

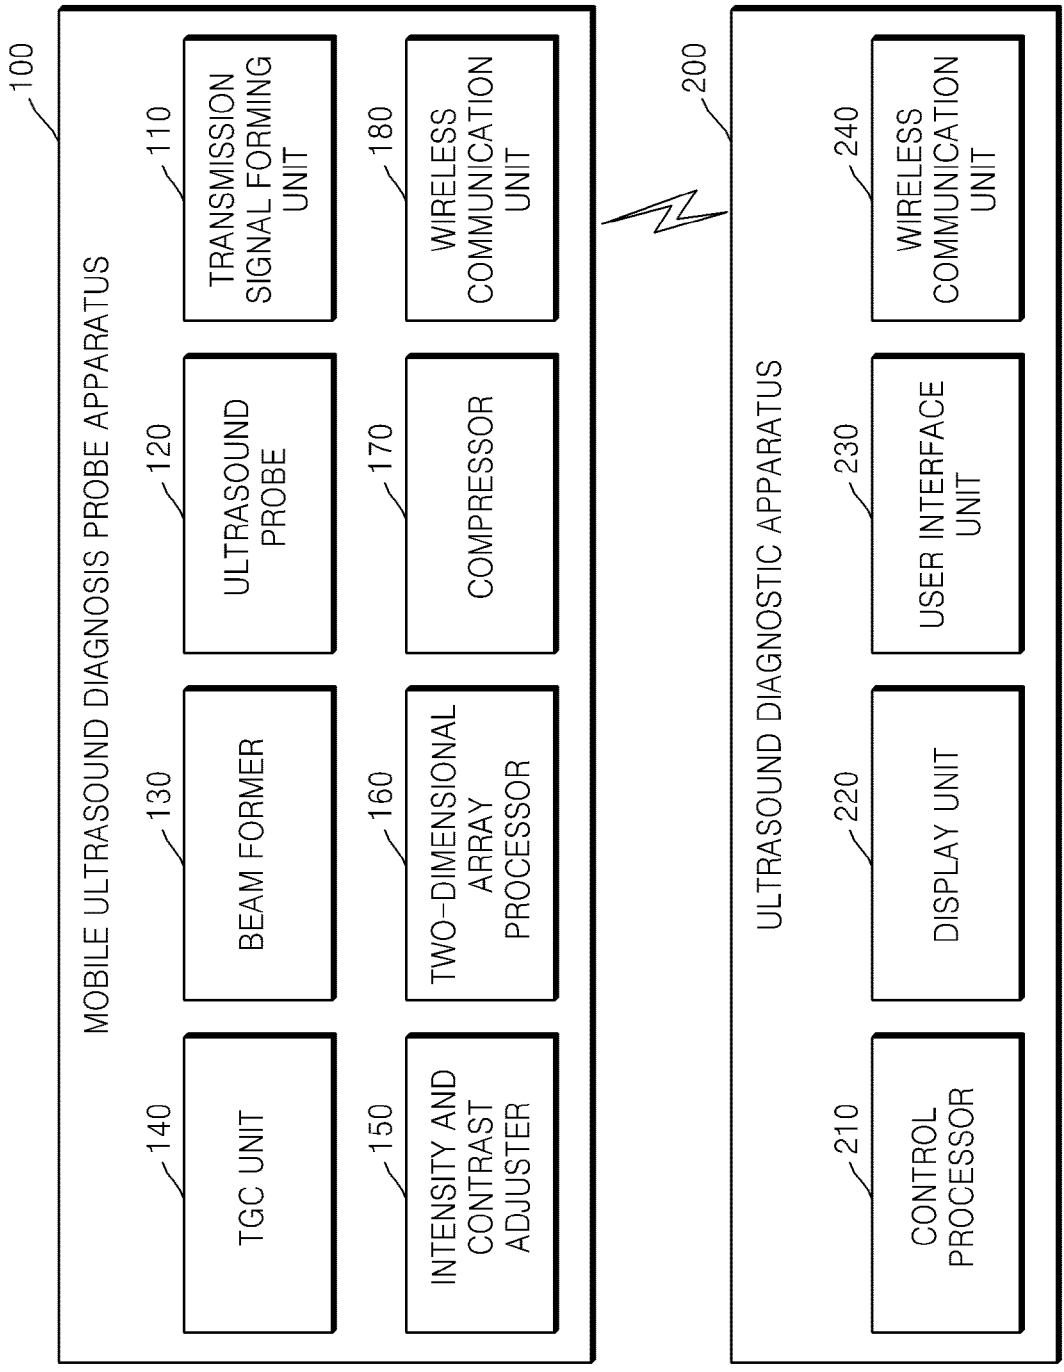

[Fig. 2]

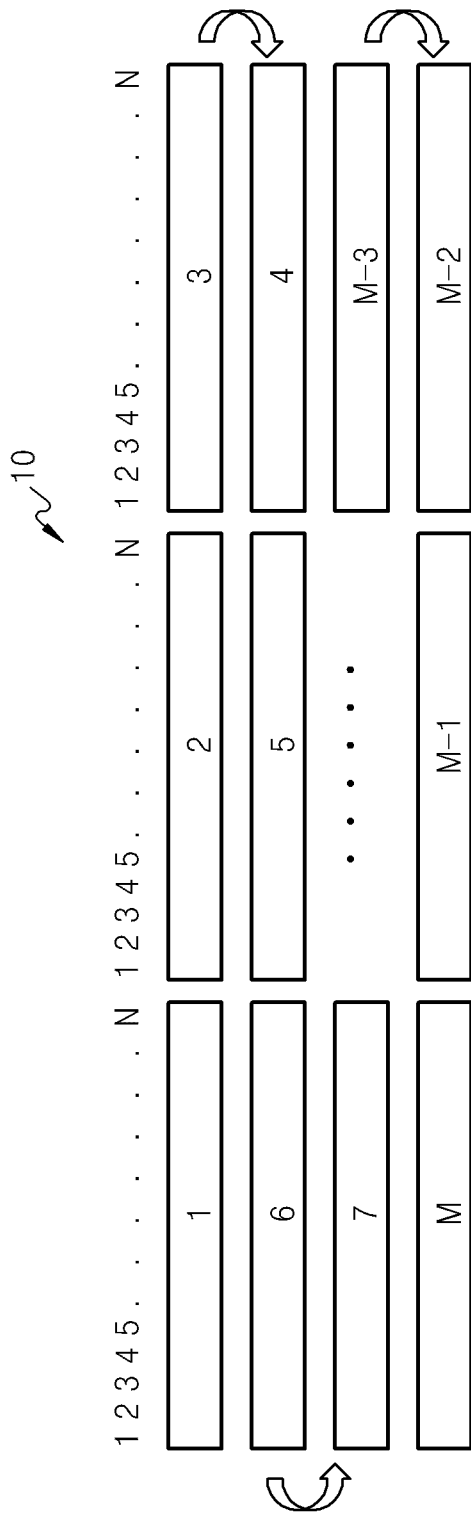



[Fig. 3]

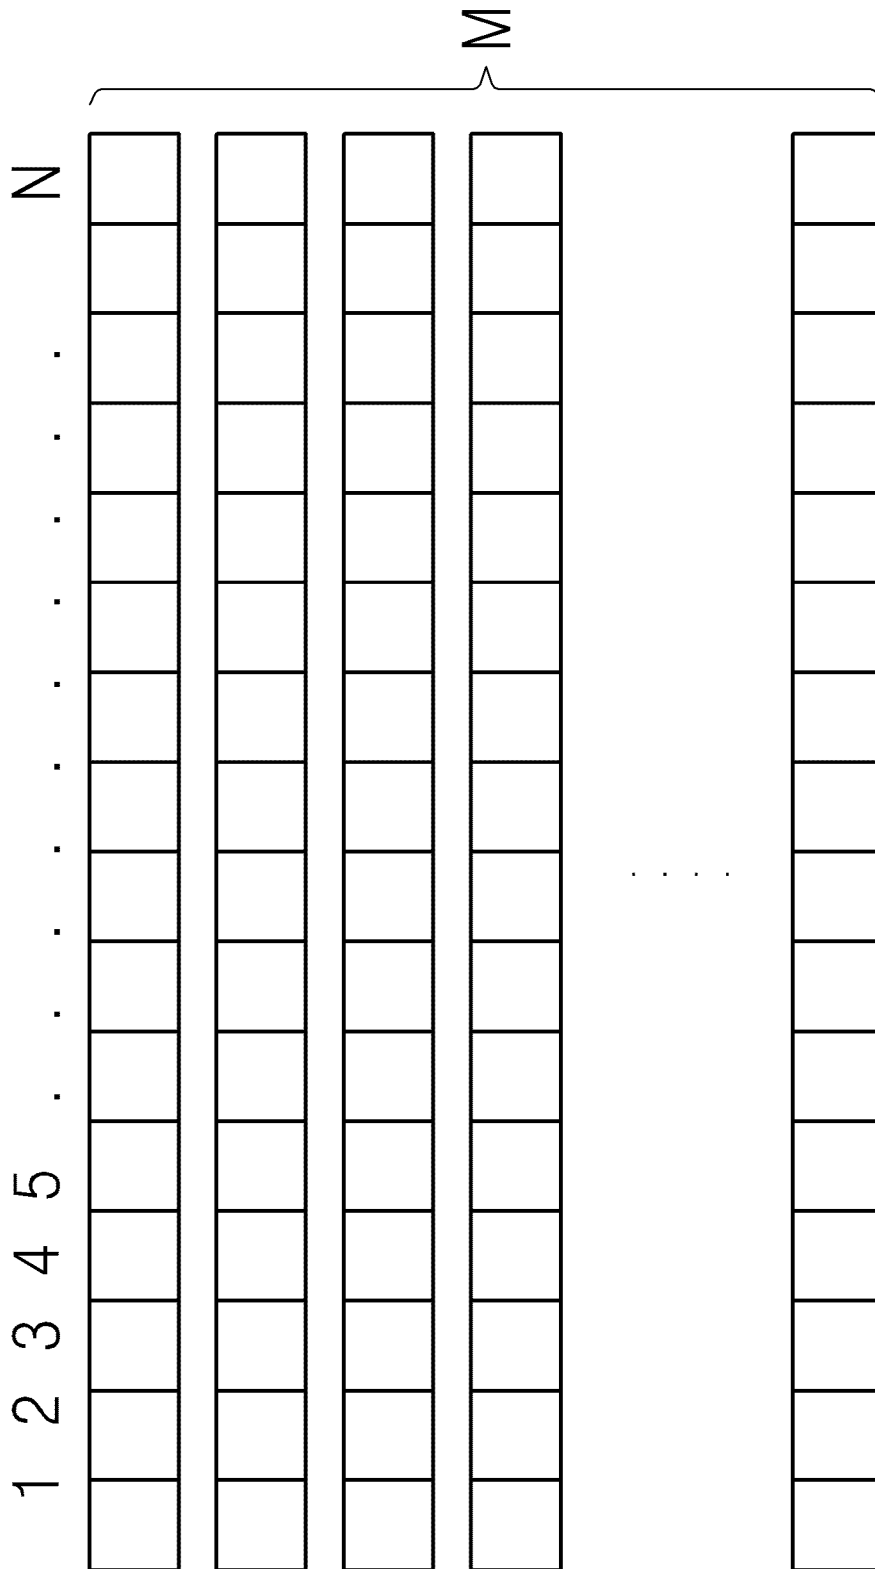


[Fig. 4]

	1	2	3	4	5	6	...	N-5	N-4	N-3	N-2	N-1	N
ULTRASOUND DATA	100	100	100	95	95	90	...	40	35	35	30	30	30
	+												
TGC TABLE	0	0	0	5	5	10	...	60	65	65	70	70	70
	+												
COMPENSATION DATA	100	100	100	100	100	100	...	100	100	100	100	100	100


[Fig. 5]

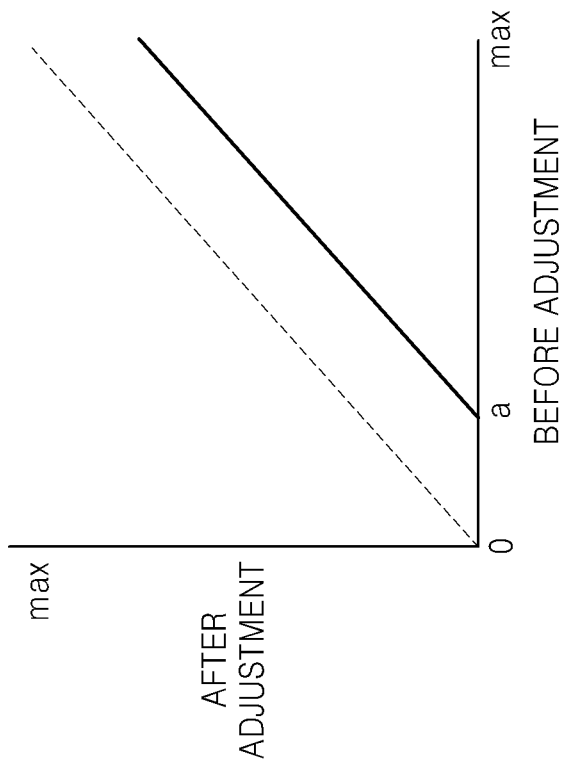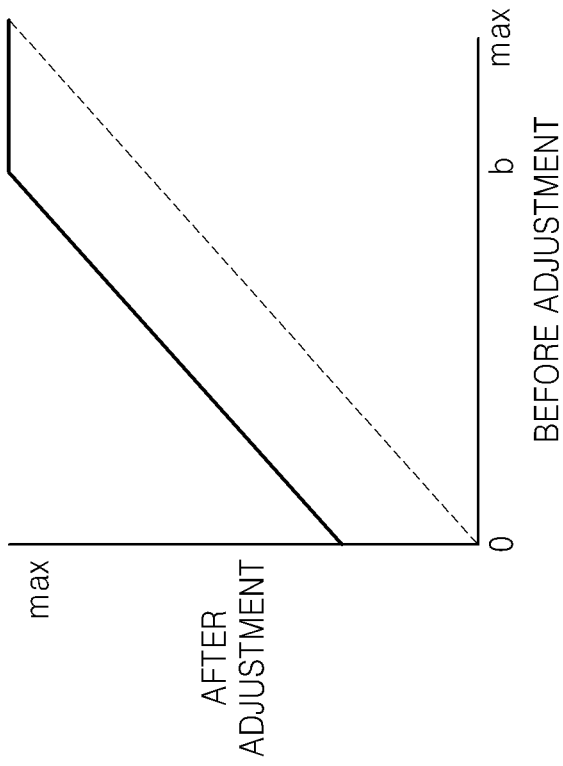



[Fig. 6]

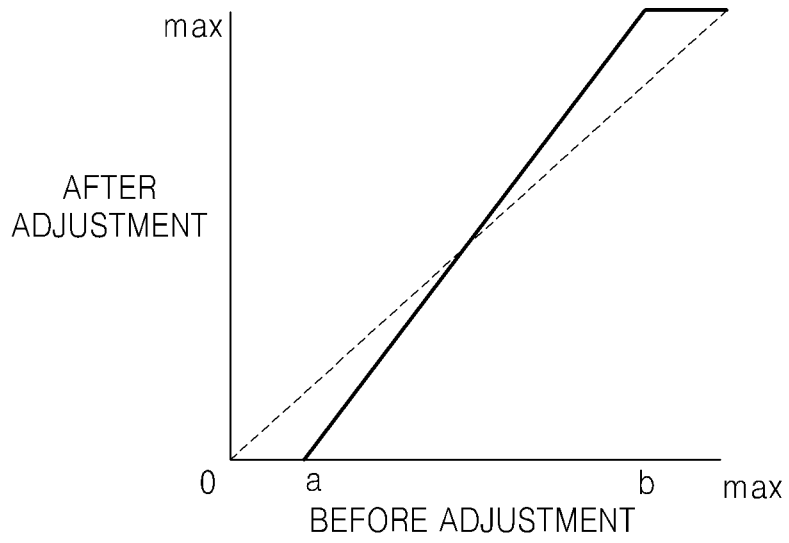


[Fig. 7]

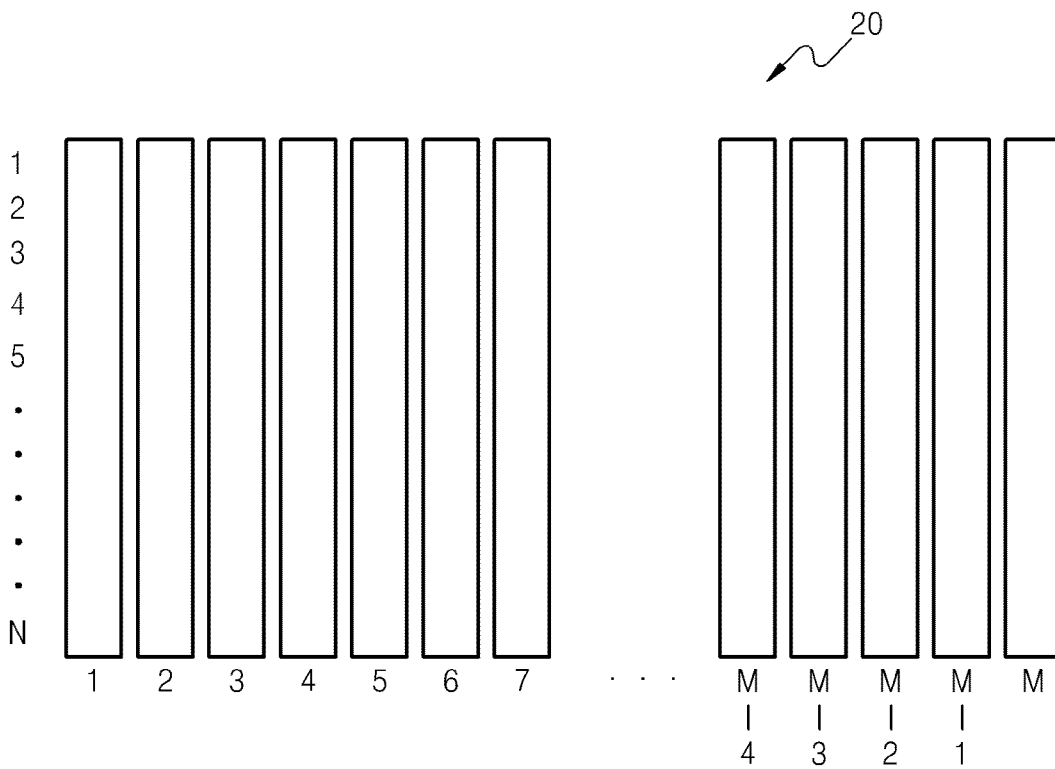


[Fig. 8]

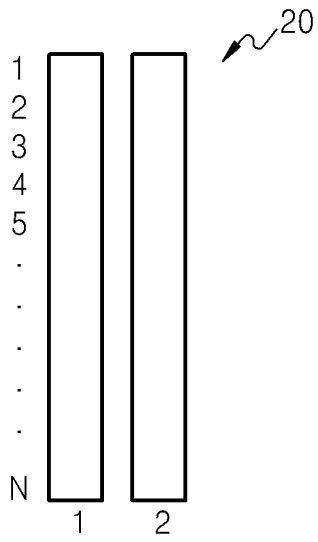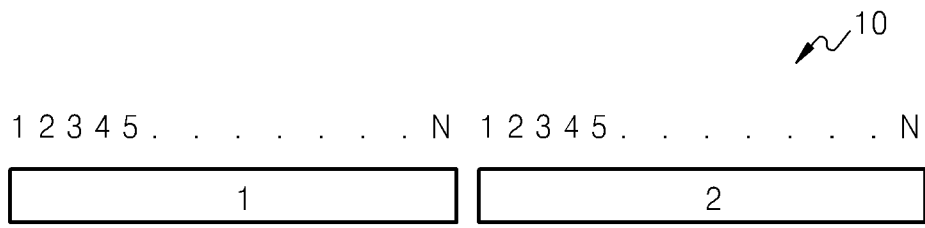


[Fig. 9]

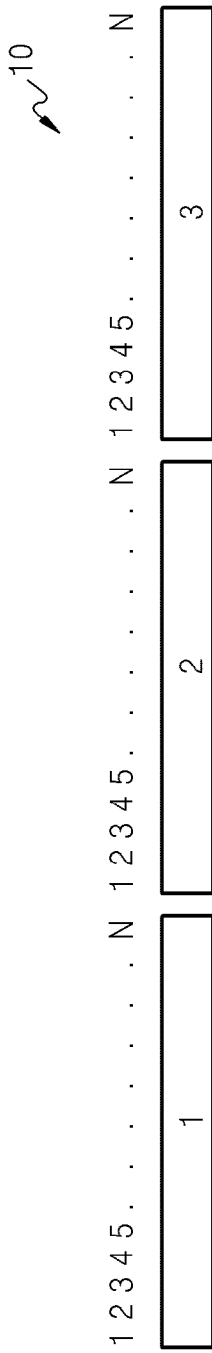


20

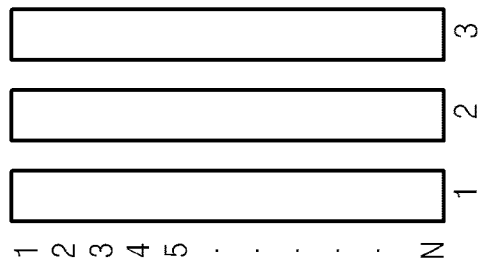


[Fig. 10]

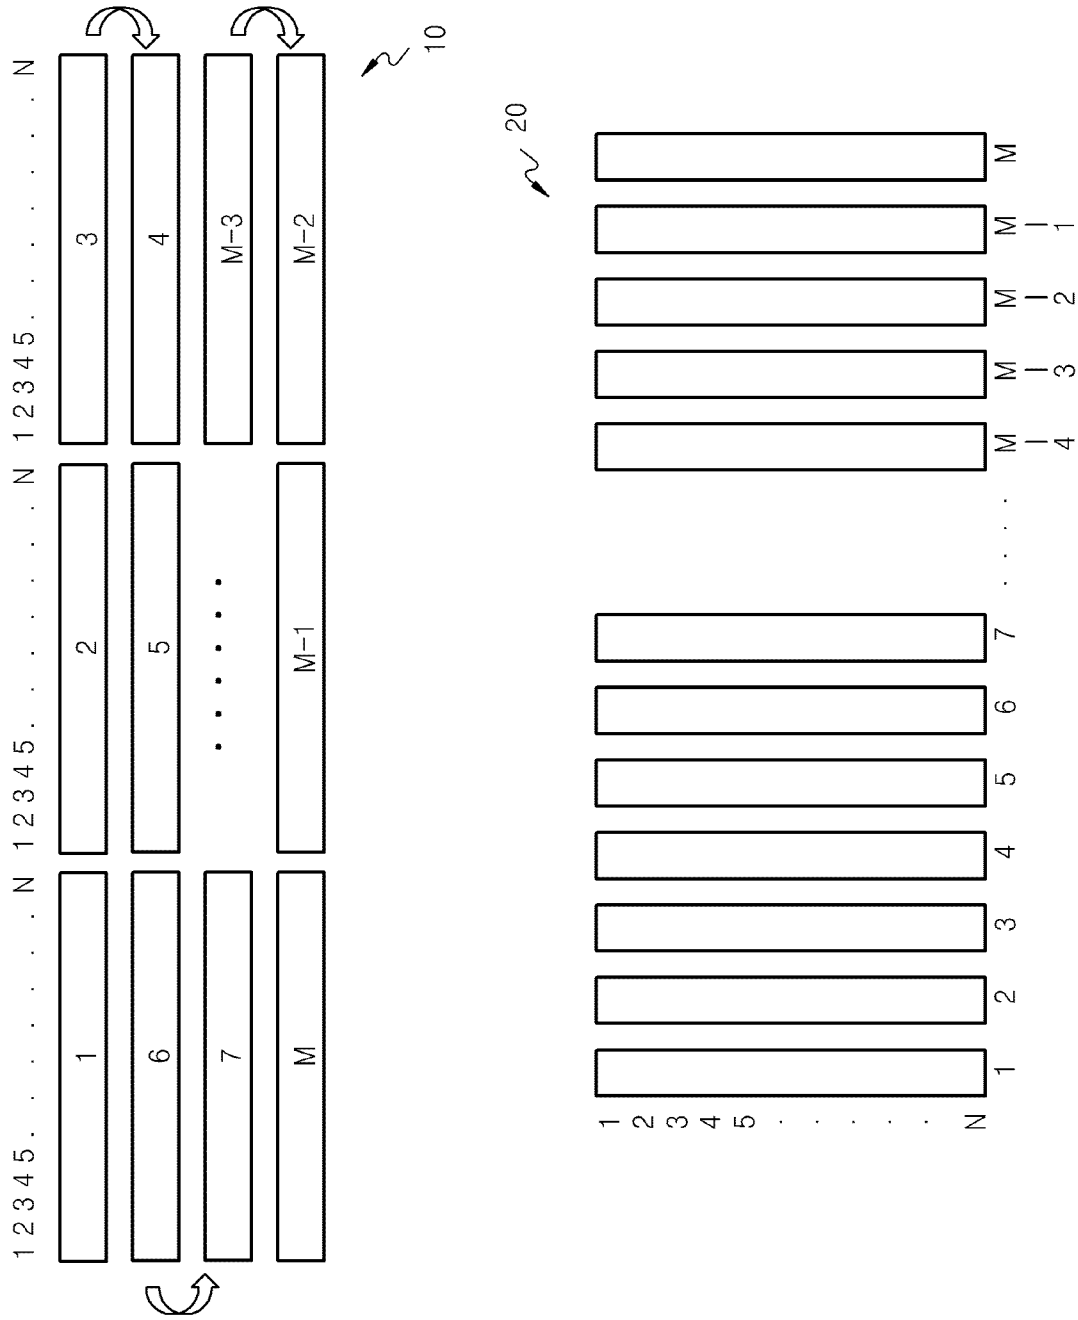


[Fig. 11]

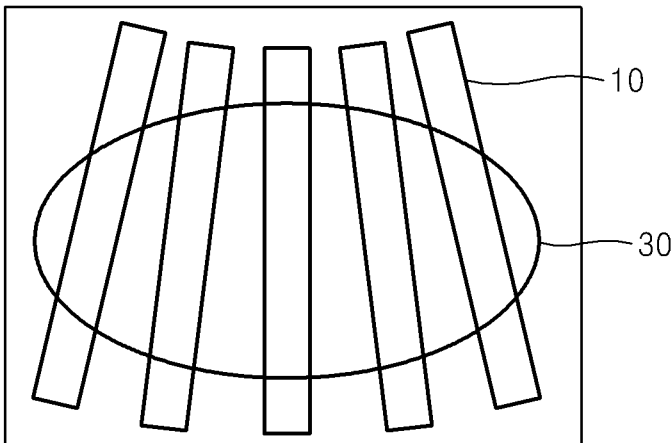


[Fig. 12]

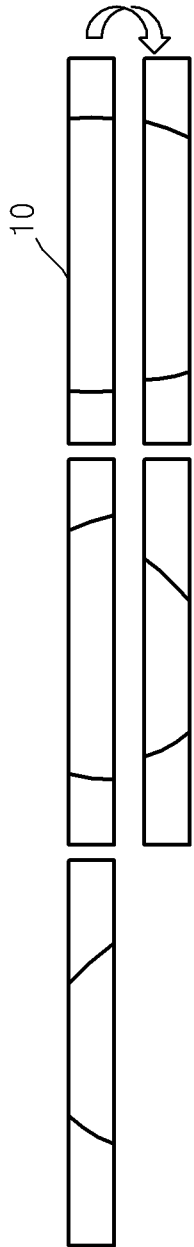

[Fig. 13]

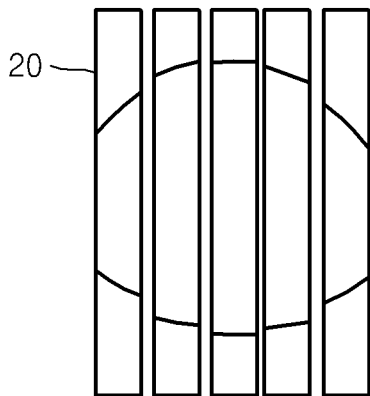

[Fig. 14]

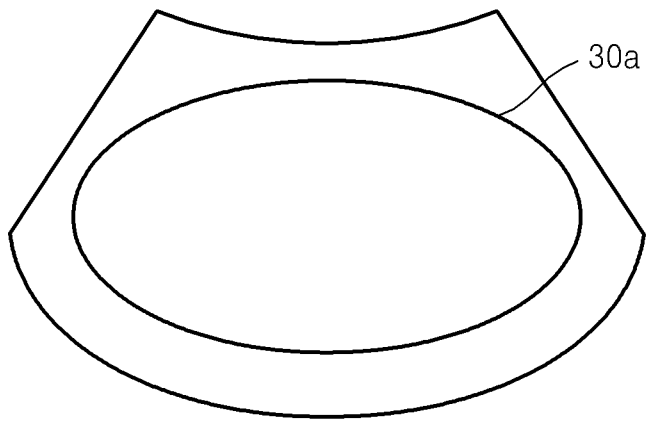

**A. CLASSIFICATION OF SUBJECT MATTER****G01N 29/24(2006.01)i, A61B 8/00(2006.01)i, H04R 17/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)

G01N 29/24; G01N 29/22; A61B 8/00; G01N 29/04; H04R 17/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models  
Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) &amp; Keywords: ultrasound, mobile, probe, compress, array and similar terms.

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 05904652 A (GILBERT JEFFREY et al.) 18 May 1999 See column 7 and figures 1 - 4.	1-14
A	US 04669314 A (MAGRANE; MARK G.) 02 June 1987 See claim 1 and figure 1.	1-14
A	JP 2002-257803 A (FUJI PHOTO FILM CO., LTD.) 11 September 2002 See claim 1 and figures 1 - 7.	1-14



Further documents are listed in the continuation of Box C.



See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

23 July 2013 (23.07.2013)

Date of mailing of the international search report

**23 July 2013 (23.07.2013)**

Name and mailing address of the ISA/KR

Korean Intellectual Property Office  
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City,  
302-701, Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

KIM Yoon Sun

Telephone No. +82-42-481-8420



## INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

**PCT/KR2013/003439**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 05904652 A	18/05/1999	AU 1996-63446 B2	24/12/1998
		AU 1998-69373 B2	24/01/2002
		AU 1998-70976 B2	13/12/2001
		AU 2000-56331 A1	09/01/2001
		AU 2002-327270 A8	03/03/2003
		AU 2003-233395 A8	29/09/2003
		CA 2279291 A1	06/08/1998
		CA 2375525 A1	28/12/2000
		CN1189217 A0	29/07/1998
		CN1242079 A0	19/01/2000
		CN1260070 A0	12/07/2000
		CN1361871 A0	31/07/2002
		EP 0835458 A2	22/09/2004
		EP 0949976 B1	16/07/2003
		EP 0956611 A2	23/06/2004
		EP 1194791 A1	10/04/2002
		EP 1353195 A3	14/04/2004
		EP 1370888 A2	17/12/2003
		JP 11-508461A	27/07/1999
		JP 2001-507794A	12/06/2001
		JP 2001-511250A	07/08/2001
		JP 2003-506172A	18/02/2003
		JP 2004-530463A	07/10/2004
		JP 2007-325937A	20/12/2007
		JP 2009-183720A	20/08/2009
		JP 2011-087949A	06/05/2011
		JP 2012-110740A	14/06/2012
		KR 10-0508276 B1	17/08/2005
		KR 10-1999-0028651 A	15/04/1999
		KR 10-2000-0070742 A	25/11/2000
		KR 10-2002-0014822 A	25/02/2002
		TW381226 A	01/02/2000
		TW447215 A	21/07/2001
		TW447215 B	21/07/2001
		TW521522 B	21/02/2003
		TW537885 B	21/06/2003
US 05590658 A	07/01/1997		
US 05690114 A	25/11/1997		
US 05839442 A	24/11/1998		
US 05964709 A	12/10/1999		
US 06111816 A	29/08/2000		
US 2002-0064093 A1	30/05/2002		
US 2002-0067359 A1	06/06/2002		
US 2002-0071345 A1	13/06/2002		
US 2002-0080683 A1	27/06/2002		
US 2002-0120193 A1	29/08/2002		
US 2002-012289 A1	31/01/2002		
US 2003-0028113 A1	06/02/2003		
US 2003-0073894 A1	17/04/2003		

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/KR2013/003439**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 2003-0176787 A1	18/09/2003
		US 2004-0015079 A1	22/01/2004
		US 2005-0018540 A1	27/01/2005
		US 6248073 B1	19/06/2001
		US 6292433 B1	18/09/2001
		US 6379304 B1	30/04/2002
		US 6530887 B1	11/03/2003
		US 6552964 B2	22/04/2003
		US 6669633 B2	30/12/2003
		US 6671227 B2	30/12/2003
		US 6721235 B2	13/04/2004
		US 6783493 B2	31/08/2004
		US 6842401 B2	11/01/2005
		US 6869401 B2	22/03/2005
		US 6969352 B2	29/11/2005
		WO 00-79300 A1	28/12/2000
		WO 02-068992 A3	17/04/2003
		WO 03-009276 A2	30/01/2003
		WO 03-079038 A2	25/09/2003
		WO 2003-079038 A3	26/02/2004
		WO 97-01768 A2	16/01/1997
		WO 98-28631 A2	02/07/1998
		WO 98-34294 A2	06/08/1998
US 04669314 A	02/06/1987	EP 0224014 A1	03/06/1987
		JP 62-116279A	27/05/1987
		KR 10-1987-0004387 A	09/05/1987
JP 2002-257803 A	11/09/2002	US 2002-0117004 A1	29/08/2002
		US 6640633 B2	04/11/2003

专利名称(译)	用于使用二维阵列数据的移动超声诊断探针设备，使用相同的移动超声诊断系统		
公开(公告)号	<a href="#">EP2841936A1</a>	公开(公告)日	2015-03-04
申请号	EP2013781415	申请日	2013-04-23
[标]申请(专利权)人(译)	和赛仑有限公司		
申请(专利权)人(译)	HEALCERION CO. , LTD.		
当前申请(专利权)人(译)	HEALCERION CO. , LTD.		
[标]发明人	RYU JEONG WON CHOUNG YOU CHAN		
发明人	RYU, JEONG WON CHOUNG, YOU CHAN		
IPC分类号	G01N29/24 A61B8/00 H04R17/00 G01S7/52		
CPC分类号	A61B8/4472 G01N29/0645 G01N29/0654 G01N29/226 G01S7/003 G01S7/52034 G01S7/5205 G01S7/5208 A61B8/14 A61B8/4427 A61B8/4488 A61B8/5207 A61B8/5269 A61B8/56		
优先权	1020120041904 2012-04-23 KR		
其他公开文献	EP2841936A4		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

提供一种移动超声诊断探针装置，包括：发送信号形成单元，形成用于获得超声图像的帧的发送信号；超声探头，将发送信号形成单元的发送信号转换为超声信号，将超声信号发送到一个物体，并且获得从物体反射的模拟超声数据，二维阵列处理器相邻地布置所获得的关于其时间增益补偿的模拟超声数据，并针对要处理的每个超声矢量针对其强度和对比度进行调整。二维阵列超声数据，压缩为每个超声矢量相邻布置的二维阵列超声数据的压缩器，以及将压缩的二维阵列超声数据无线发送到超声诊断设备的无线通信单元。