

(19)



(11)

EP 1 683 486 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
19.08.2009 Bulletin 2009/34

(51) Int Cl.:
A61B 8/06 (2006.01) A61B 8/00 (2006.01)

(21) Application number: **04792506.0**

(86) International application number:
PCT/JP2004/015289

(22) Date of filing: **15.10.2004**

(87) International publication number:
WO 2005/037104 (28.04.2005 Gazette 2005/17)

(54) **ULTRASONIC DOPPLER BLOOD FLOW MEASURING DEVICE**

ULTRASCHALL-DOPPLER-BLUTFLUSSMESSGERÄT

DISPOSITIF DE MESURE DU DEBIT SANGUIN PAR DOPPLER ULTRASONS

(84) Designated Contracting States:
DE FR GB

(72) Inventor: **HAGIWARA, Hisashi**
. (JP)

(30) Priority: **17.10.2003 JP 2003358059**

(74) Representative: **Hössle Kudlek & Partner**
Patentanwälte
Postfach 10 23 38
70019 Stuttgart (DE)

(43) Date of publication of application:
26.07.2006 Bulletin 2006/30

(73) Proprietor: **Panasonic Corporation**
Kadoma-shi
Osaka 571-8501 (JP)

(56) References cited:
JP-A- 5 095 948 JP-A- 5 212 032
JP-A- 10 099 332 JP-A- 2000 126 179
JP-A- 2000 126 179 US-A- 6 077 226
US-B1- 6 547 731 US-B1- 6 599 248

EP 1 683 486 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

TECHNICAL FIELD

5 **[0001]** The present invention relates to an ultrasonic Doppler blood flow measuring device which measures blood flow within a biological body by using the Doppler phenomenon of ultrasonic waves and performs image display regarding the measured results, in the medical field, and more particularly, relates to an ultrasonic Doppler blood flow measuring device for showing, by color display, an image according to the blood flow rate data generated by the aliasing phenomenon.

10 BACKGROUND ART

[0002] Conventionally, an ultrasonic Doppler blood flow measuring device (color flow device), which enables measurement of blood flow distribution and blood flow velocity within a biological body by using the Doppler phenomenon of ultrasonic waves and displays the blood flow velocity, in correspondence to a predetermined color, by superimposing a black and white, two-dimensional cross-sectional image therewith, is known.

15 **[0003]** Fig. 5 is a block diagram of an example of a configuration of an ultrasonic Doppler blood flow measuring device according to prior art. The ultrasonic Doppler blood flow measuring device has a probe 2 for performing transmission and reception of ultrasonic waves to a biological body. An ultrasonic pulse is irradiated from a transmitting unit 1 to the blood flowing within the biological body, and the probe 2 again receives an echo of the ultrasonic pulse reflected by the blood. The echo of the ultrasonic pulse is converted into an electrical signal by the probe 2 and supplied to a receiving unit 3. After digitalization or beamforming by the receiving unit 3, the signal is phase-detected by a phase detecting unit 4 and becomes a Doppler-shift signal comprising information on the Doppler-shift due to blood flow.

20 **[0004]** The Doppler-shift signal is supplied from the phase detecting unit 4 to a wall filter 5. In wall filter 5, signals from unnecessary tissues which are low-frequency signal components are removed, and furthermore, in a velocity calculating unit 6, blood flow information, such as blood flow velocity data, blood echo intensity data, blood flow velocity variance data, and the like, is determined based on the signal subsequent to processing by the wall filter 5. This blood flow information is smoothing-processed by a filter 7, supplied to a digital scan Converter (DSC) 8, and coordinate-converted into a shape adhering to ultrasonic scanning.

25 **[0005]** In addition, a B-mode image (ultrasonic cross-sectional image) signal (B-mode signal) is supplied from an envelope detecting unit 9 to DSC 8, in the same way, and the DSC 8 not only coordinate-converts the supplied image data into a shape adhering to ultrasonic scanning, but also combines B-mode signal and blood flow information and shows a two-dimensional blood flow image on a monitor 10.

30 **[0006]** The blood flow velocity data comprised in the blood flow information is data which has a possibility of generating an aliasing phenomenon based on the Nyquist theorem. With regards to this measurement of blood flow velocity data having this aliasing, a method, for example, for performing filter processing with an arbitrary order after determining aliasing and performing corrections is disclosed in the following Patent Document 1 as a method for filter processing in filter 7.

Patent Document 1: Japanese Patent Application Publication No. 4-161146 (Heisei)

35 United States Patent 6,077,226 discloses an apparatus for adjusting the shape of a region of interest in a frame of imaging date in response to an operator-actuated change in the depth of the region of interest, and particularly discloses a signal processing change for one type of ultra sound imaging system, comprising wall filters which are high pass filters being applied to each down range position across "firings", i.e. in "slow time".

Document US- 5 860 930 discloses an energy weighted parameter spatial/temporal filter as described in the preamble of claim 1.

45

DISCLOSURE OF THE INVENTION

PROBLEMS TO BE SOLVED BY THE INVENTION

50 **[0007]** However, in the filter processing method for blood flow velocity data disclosed in Patent Document 1, the aliasing determination method and the aliasing correction method are complicated, and this is problematic in that, in order to actualize this filter processing method, a complicated hardware configuration is required.

[0008] In light of the foregoing problems, an object of the present invention is to provide an ultrasonic Doppler blood flow measuring device which actualizes the filtering of blood flow velocity data having aliasing and performing a screen display of blood flow velocity which changes smoothly, spatially and temporally.

55

MEANS FOR SOLVING THE PROBLEM

5 **[0009]** In order to achieve the foregoing object, the ultrasonic Doppler blood flow measuring device of the present invention has a blood flow velocity filter means for performing filter processing in order to calculate the blood flow velocity value of the blood within a subject biological body from the echo signals of ultrasonic pulse transmitted to the subject biological body, wherein
the blood flow velocity filter means comprises:

- 10 a difference calculating means for subtracting the focus point blood flow velocity value of an arbitrary focus point from the blood flow velocity value supplied to the blood flow velocity filter means and calculating the difference value thereof;
a filter means for performing filter processing on the difference values; and
an addition processing means for adding the focus point blood flow velocity value to the filter processing result from the filter means.

15 According to this configuration, it becomes possible to perform filter processing of blood flow velocity data which has aliasing by only common filter means and common addition and subtraction means, and a smooth image display of blood flow velocity can be actualized.

20 **[0010]** Furthermore, the ultrasonic Doppler blood flow measuring device of the present invention is configured such that the difference calculating means calculates the difference value of consecutive point blood flow velocity value of a point which is spatially consecutive to the arbitrary focus point and the arbitrary focus point blood flow velocity value. According to this configuration, when performing an image display of the blood flow velocity of the blood flowing within the subject biological body, it becomes possible to reduce spatial random noise within one image frame and a smooth image display of blood flow velocity can be actualized.

25 **[0011]** Furthermore, the ultrasonic Doppler blood flow measuring device of the present invention is configured such that the difference calculating means calculates the difference value of the blood flow velocity value which is temporally consecutive to the arbitrary focus point and the arbitrary focus point blood flow velocity value.

30 According to this configuration, when performing an image display of the blood flow velocity of the blood flowing within the subject biological body, it becomes possible to reduce temporal random noise between a plurality of image frames and a smooth image display of blood flow velocity can be actualized.

ADVANTAGEOUS EFFECTS OF THE INVENTION

35 **[0012]** The ultrasonic Doppler blood flow measuring device of the present invention has a blood flow velocity filter means for performing filter processing to calculate the blood flow velocity value of the blood flowing within the subject biological body from the echo signals of the ultrasonic pulse transmitted to the subject biological body, wherein the blood flow velocity filter means comprises a difference calculating means for subtracting the focus point blood flow velocity value of an arbitrary focus point from the blood flow velocity value supplied to the blood flow velocity filter means and calculates the difference value thereof, a filter means for performing filter processing on the difference value,
40 an addition processing means for adding the focus point blood flow velocity value to the filter processing result from the filter means, and has an effect, wherein the filter processing of blood flow velocity data which has aliasing is preformed by only common filter means and common addition and subtraction means, and a smooth image display of blood flow velocity is actualized.

45 BRIEF DESCRIPTION OF THE DRAWINGS

[0013]

50 [Fig. 1] A block diagram showing a configuration of an ultrasonic Doppler blood flow measuring device according to a first embodiment of the present invention.

[Fig. 2] A block diagram showing a detailed configuration of a spatial filter of the ultrasonic Doppler blood flow measuring device according to the first embodiment of the present invention.

[Fig. 3] A block diagram showing a configuration of an ultrasonic Doppler blood flow measuring device according to a second embodiment of the present invention.

55 [Fig. 4] A block diagram showing a detailed configuration of a frame filter of the ultrasonic Doppler blood flow measuring device according to the second embodiment of the present invention.

[Fig. 5] A block diagram showing one example of a configuration of an ultrasonic Doppler blood flow measuring device according to prior art.

BEST MODE FOR CARRYING OUT THE INVENTION

[0014] An ultrasonic Doppler blood flow measuring device according to first and second embodiments of the present invention is described hereafter, with reference to the drawings.

[First Embodiment]

[0015] First, the first embodiment of the present invention is described. Fig. 1 is a block diagram showing a configuration of an ultrasonic Doppler blood flow measuring device according to the first embodiment of the present invention. The ultrasonic Doppler blood flow measuring device shown in Fig. 1 comprises a transmitting unit 1, a probe 2, a receiving unit 3, a phase detecting unit 4, a wall filter 5, a velocity calculating unit 6, a digital scan converter (DSC) 8, an envelope detecting unit 9, and a monitor 10. Although the ultrasonic Doppler blood flow measuring device shown in Fig. 1 has almost the same configuration as the ultrasonic Doppler blood flow measuring device shown in Fig. 5, a spatial filter 20 is provided in place of the filter 7. In the ultrasonic Doppler blood flow measuring device shown in Fig. 1, the constituent elements excluding the spatial filter 20 are the same as the constituent elements of the conventional ultrasonic Doppler blood flow measuring device shown in Fig. 5, the same reference numbers are cited and explanations of operations are omitted, as well.

[0016] Fig. 2 is a block diagram showing a detailed configuration of the spatial filter of the ultrasonic Doppler blood flow measuring device according to the first embodiment of the present invention. The spatial filter 20 shown in Fig. 2 comprises latches 21, 22, and 23 which can hold data, adders 24, 25, 28, and 29 which can add or subtract two data, and multipliers 26 and 27 which can multiply two data. The adders 24 and 25 comprise a pre-processing unit (difference calculating unit) 41, the multipliers 26 and 27 and the adder 28 comprise a filtering unit 42, and the adder 29 comprises a post-processing unit (addition processing unit) 43.

[0017] The connection configuration of respective constituent elements within the spatial filter 20 shown in Fig. 2 and the flow of data are described hereafter. Latches 21, 22, and 23 are placed in order to hold data (blood flow velocity value) of a plurality of focus points spatially consecutive in the sound ray direction of the ultrasonic waves. The input signal (blood flow velocity value) D31 of the blood flow information from the velocity calculating unit 6 is provided to the latch 21. This input signal D31 includes data on an arbitrary focus point, namely, when measuring, the input signal (consecutive point blood flow velocity value) D31 of focus points spatially consecutive in the sound ray direction of the ultrasonic waves is provided continuously, and the input signal D31 from the velocity calculating unit 6 is provided continuously to the latch 21. When the input signal D31 is provided from the velocity calculating unit 6, the latch 21 holds the input signal D31 and provides the held data (for example, data of the previous focus point) D32 to the latch 22 and the adder 24, as well.

[0018] When data D32 provided from the latch 21 is provided, the latch 22 also holds this data D32 and provides the held data (for example, data of the previous focus point) D33 to the latch 23 and the adder 24, 25, and 29, as well. Furthermore, when data D33 provided from the latch 22 is provided, the latch 23 also holds this data D33 and provides the held data D34 to the adder 25. In this way, data D32, D33, and D34 of spatially consecutive focus points are output to the pre-processing unit 41 at the same timing from the latches 21, 22, and 23, respectively.

[0019] In addition, between the latches 21, 22, and 23 and the adders 24 and 25, the output of the latch 21 is connected to the input on the addition side of the adder 24, the output of the latch 22 is connected to the input of the subtraction sides of the adder 24 and 25, respectively, and the output of the latch 23 is connected to the input on the addition side of the adder 25. In this way, the adder 24 receives data D32 from the addition side and data D33 from the subtraction side, respectively, performs calculation, and outputs the result of subtracting data D33 from data D32 to the multiplier 26 as data D35. In addition, the adder 25 receives data D34 from the addition side and data D33 from the subtraction side, respectively, performs calculation, and outputs the result of subtracting data D33 from data D34 to the multiplier 27 as data D36.

[0020] The multipliers 26 and 27 multiply the provided data by the filter coefficients set respectively to the provided data and outputs the results. Therefore, the multiplier 26 multiplies filter coefficient k_1 and data D35 provided from the adder 24 and outputs data D37, and the multiplier 27 multiplies filter coefficient k_3 and data D36 provided from the adder 25 and outputs data D38. The adder 28 receives data D37 and D38 from the multipliers 26 and 27, adds these data, and outputs the added result to the adder 29 as data D39. Then, the adder 29 receives data D33 from the latch 22 and data D39 from the adder 28, respectively, adds these data, and outputs the added result to the DSC 8 as data D40.

[0021] The spatial filter 20 according to the present embodiment is a one-dimensional filter and a second order filter (a filter having two filter coefficients). In other words, in the present embodiment, the consecutive point blood flow velocity value (data D32 and D34), which is consecutively before and after the focus point, is subtracted from the focus sample data D33 of the focus point and data D35 and D36, wherein focus sample data D33 is the origin (in other words, 0), are created by the pre-processing unit 41 composed of adders 24 and 25, with the focus point as data (focus sample data or focus point blood flow velocity value) D33 which is output from the latch 22.

[0022] The pre-processing unit 41, the filtering unit 42, and the post-processing unit 43 operate as a second order FIR (Finite duration Impulse Response) filter, by the combination thereof. The filter operation of the present invention is described using equations. If output data D40 is expressed using respective data in Fig. 2,

[0023]

[Equation 1]

$$D40 = D39 + D33$$

$$D40 = D37 + D38 + D33$$

$$D40 = k1 * D35 + k3 * D36 + D33$$

$$D40 = k1 * (D32 - D33) + k3 * (D34 - D33) + D33$$

$$D40 = k1 * D32 + (1 - k1 - k3) * D33 + k3 * D34 \dots \text{Equation 1}$$

[0024] From equation 1, Fig. 2 can be considered a second order FIR filter having the following transfer function H(z).

[0025]

[Equation 2]

$$H(z) = k1 + (1 - k1 - k3) z^{-1} + k3z^{-2} \dots \text{Equation 2}$$

[0026] Here, z^{-n} is an operator indicating the lag element of n column.

This FIR filter is given low-pass filter characteristics in order to eliminate random noise having high-frequency component. Therefore, as the second order FIR filter, it is preferable that all coefficients are positive numbers,

[0027] and are set to:

[0028]

[Equation 3]

$$0 < k1, 0 < k3, \text{ and } k1 + k3 < 1 \dots \text{Equation 3}$$

[0029] In addition, the adders 24 and 25 perform, for example, a fixed decimal point calculation, the output data format is the same as the input data format, and the carry bit of the addition result is omitted (ignored). For example, if the input has an 8-bit 2's complement format, the output also has an 8-bit 2's complement format. Thus, data D35 is calculated as the difference value of data D32 and focus sample data D33, under the condition that the velocity difference between data is a smaller velocity difference than the velocity difference which causes aliasing. Similarly, data D36 is calculated as the difference value of data D34 and focus sample data D33, under the condition that the velocity difference between data is a smaller velocity difference than the velocity difference which causes aliasing.

[0030] By the foregoing processing, it becomes possible to perform filter calculation of the consecutive point blood flow value (three data D32, D33, and D34) provided to the second order FIR filter, with one data among these as the focus sample data (for example, data D33), under the assumption that the velocity difference between the blood flow velocity value of the focus sample data and the blood flow velocity data of other data is a smaller velocity difference than the velocity difference which causes aliasing. Therefore, at the same time (within the same image), after the difference value of an arbitrary center pixel is filter processed, it becomes possible to, again, add data on the arbitrary center pixel and obtain data on the desired blood flow velocity value, and spatial random noise can be reduced. Although the foregoing

first embodiment was an example actualizing a one-dimensional second order filter, it is possible make an extension to a one-dimensional and two-dimensional, high-order filter, in the same way.

5 [0031] As described above, according to the ultrasonic Doppler blood flow measuring device according to the first embodiment of the present invention, by providing the spatial filter 20 having the pre-processing unit 41 for performing subtraction with the focus sample data D33 as the origin and the filtering unit 42 for performing filter processing on all provided data, and the post-processing unit 43 for adding the focus sample data D33 to the output data D39 after filter processing by the filtering unit 42, it becomes possible to perform filter processing of blood flow velocity data (consecutive point blood flow velocity value) which are spatially consecutive in the sound ray direction of the ultrasonic waves, without being influenced by aliasing, and a spatially smooth blood flow velocity image can be provided.

10 [Second Embodiment]

15 [0032] Next, a second embodiment of the present invention is described. Fig. 3 is a block diagram showing a configuration of the ultrasonic Doppler blood flow measuring device according to the second embodiment of the present invention. The ultrasonic Doppler blood flow measuring device according to the second embodiment of the present invention shown in Fig. 3 differs in that a frame filter 50 is provided in place of the spatial filter 20, held by the ultrasonic Doppler blood flow measuring device according to the first embodiment of the present invention. In the ultrasonic Doppler blood flow measuring device shown in Fig. 3, the constituent elements excluding the frame filter 50 are the same as the constituent elements of the conventional ultrasonic Doppler blood flow measuring devices shown in Fig. 1 and Fig. 5, the same reference numbers are cited and explanations of operations are omitted, as well.

20 [0033] Fig. 4 is a block diagram showing a detailed configuration of the frame filter of the ultrasonic Doppler blood flow measuring device according to the second embodiment of the present invention. The frame filter 50 shown in this Fig. 4 differs in that, in comparison with the spatial filter 20 shown in Fig. 2, frame memories 52 and 53 are provided in place of latches 22 and 23. In the frame filter 50 shown in Fig. 4, the constituent elements excluding the frame memories 52 and 53 are the same as the constituent elements of the spatial filter 20 shown in Fig. 2, the same reference numbers are cited and explanations of operations are omitted, as well.

25 [0034] The connection configuration of respective constituent elements within the frame filter 50 shown in Fig. 4 and the flow of data are described. The input signal D61 of the blood flow information from the velocity calculating unit 6 is provided to the latch 21. This input signal 61 includes data on an arbitrary focus point, namely, when measuring, the input signal (blood flow velocity value) D61 of focus points which are consecutive in the sound ray direction of the ultrasonic waves is provided continuously, and the input signal D61 from the velocity calculating unit 6 is provided continuously to the latch 21. When the input signal D61 is provided from the velocity calculating unit 6, the latch 21 holds the input signal D61 and provides the held data (for example, data of the previous focus point) D62 to the frame memory 52 and the adder 24, as well.

30 [0035] After the input signal D61 of the blood flow information from the velocity calculating unit 6 is provided to the latch 21, the signal is further provided to the frame memory 52 as data D62. The frame memory 52 holds data D62 provided from the latch 21 and outputs data D63 of the one frame prior thereto in the same region, as well. In addition, the frame memory 53 similarly holds data D63 output from the frame memory 52 and outputs data D64 of the one frame prior thereto in the same region (two frames before data D62), as well. Thus, data D62, D63, and D64 of the same region within temporally consecutive frames (in other words, blood flow velocity values temporally consecutive to the arbitrary focus point) are output to the pre-processing unit 41 at the same timing from the latch 21 and the frame memories 52 and 53, respectively. In this case, data D63 is used as the focus sample data (focus point blood flow velocity value), and the same processing as that in the foregoing first embodiment is performed in the pre-processing unit 41, the filtering unit 42, and the post-processing unit 43.

35 [0036] By the foregoing processing, it becomes possible to perform filter calculation of the three data, D62, D63, and D64, provided to the second order FIR filter, with one data among these as the focus sample data (for example, data D63), under the assumption that the velocity difference between the blood flow velocity value of the focus sample data and the blood flow velocity data of other data is a smaller velocity difference than the velocity difference which causes aliasing. Therefore, after the difference value of data on the blood flow velocity value at an arbitrary time and the data on the blood flow velocity value which is temporally prior and subsequent thereto is filter processed, in the same region, it becomes possible to, again, add data on the blood flow velocity value at a predetermined time and obtain data on the desired blood flow velocity value, and temporal random noise between a plurality of temporally consecutive images can be reduced.

40 [0037] As described above, according to the ultrasonic Doppler blood flow measuring device according to the second embodiment of the present invention, by providing the frame filter 50 having the pre-processing unit 41 for performing subtraction with the focus sample data D63 as the origin and the filtering unit 42 for performing filter processing on all provided data, and the post-processing unit 43 for adding the focus sample data D63 to the output data after filter processing by the filtering unit 42, it becomes possible to perform filter processing of blood flow velocity data (blood flow

velocity value temporally consecutive to arbitrary focus point) which are temporally consecutive in the same region in the sound ray direction of the ultrasonic waves, without being influenced by aliasing, and a temporally smooth blood flow velocity image can be provided. Although the foregoing second embodiment was an example actualizing a second order frame filter, it is possible make an extension to a filter of a higher order, in the same way.

[0038] Although the frame filter 50 is provided between the velocity calculating unit 6 and the DSC 8 in the foregoing second embodiment, it can be provided between the DSC 8 and the monitor 10, as well. In addition, although the ultrasonic Doppler blood flow measuring device having the spatial filter 20 was described in the first embodiment and the ultrasonic Doppler blood flow measuring device having the frame filter 50 was described in the second embodiment, separately, it is also possible to provide both the spatial filter 20 and the frame filter 50 within the ultrasonic Doppler blood flow measuring device. Furthermore, although the spatial filter 20 and the frame filter 50 are configured by hardware in the first and second embodiments, the filter processing performed by these filters can also be actualized by software programs.

INDUSTRIAL APPLICABILITY

[0039] The ultrasonic Doppler blood flow measuring device according to the present invention can actualize filtering of blood flow velocity data having aliasing by a simple, small-scale algorithm and perform image display of blood flow velocity which changes smoothly, spatially or temporally, and in the medical field, can be applied to technology for measuring the blood flow within a biological body using the Doppler phenomenon of the ultrasonic waves and performing image display related to this measured result, as well as, in particular, applied to technology for color-displaying image of blood flow velocity data generated by the aliasing phenomenon.

Claims

1. An ultrasonic Doppler blood flow measuring device having:

a transmitting means (1) for irradiating an ultrasonic pulse into a subject biological body via a probe;
 a receiving means (3) for receiving an echo of the ultrasonic pulse reflected by blood flowing within the subject biological body;
 a phase detecting means (4) for phase-detecting a signal of the echo of the ultrasonic pulse to acquire a Doppler-shift signal including information on Doppler-shift due to blood flow;
 a wall filter (5) for removing low-frequency signal components from the Doppler-shift signal;
 a velocity calculating means (6) for calculating a blood flow velocity value of the blood within the subject biological body based on a signal outputted from the wall filter; and
 a blood flow velocity filter means (20) for performing filter processing, on the blood flow velocity value;
characterized in that
 the blood flow velocity filter means (20) comprises:

a difference calculating means (41) for subtracting a focus point blood flow velocity value of an arbitrary focus point from the blood flow velocity value supplied to the blood flow velocity filter means and calculating a difference value thereof;
 a filter means for performing filter (42) processing on the difference value; and
 an addition processing means (43) for adding the focus point blood flow velocity value to a filter processing result from the filter means.

2. The ultrasonic Doppler blood flow measuring device according to claim 1, wherein said difference calculating means calculates the difference value of the consecutive point blood flow velocity value of a point which is spatially consecutive to said arbitrary focus point and said arbitrary focus point blood flow velocity value.

3. The ultrasonic Doppler blood flow measuring device according to claim 1, wherein said difference calculating means calculates the difference value of the blood flow velocity value which is temporally consecutive to said arbitrary focus point and said arbitrary focus point blood flow velocity value.

Patentansprüche

1. Ultraschall-Doppler-Blutflussmessgerät mit:

EP 1 683 486 B1

einem Übertragungsmittel (1) zum Aussenden eines Ultraschall-Pulses in einen untersuchten biologischen Körper einer Versuchs- bzw. Messperson mittels einer Sonde,
einem Empfangsmittel (3) zum Empfangen eines Echos des Ultraschall-Pulses, der durch innerhalb des untersuchten biologischen Körpers fließendes Blut reflektiert wird,
5 einem Phasendetektierungsmittel (4) zur Phasenerkennung eines Signals des Echos des Ultraschall-Pulses, um ein Doppler-Verschiebungssignal zu erhalten, das Informationen über eine durch den Blutfluss verursachte Doppler-Verschiebung umfasst,
einem Wallfilter bzw. Hochpassfilter (5) zur Entfernung von niederfrequenten Signalkomponenten aus dem Doppler-Verschiebungssignal,
10 einem Geschwindigkeitsberechnungsmittel (6) zur Berechnung eines Blutflussgeschwindigkeitswerts des Blutes innerhalb des untersuchten biologischen Körpers, der auf einem von dem Wandfilter ausgegebenen Signal basiert, und
einem Blutflussgeschwindigkeits-Filtermittel (20) zur Durchführung einer Filterung des Blutflussgeschwindigkeitswertes,

dadurch gekennzeichnet, dass

das Blutflussgeschwindigkeits-Filtermittel (20) folgende Komponenten umfasst:

ein Differenzberechnungsmittel (41) zum Subtrahieren eines Messpunkt-Blutflussgeschwindigkeitswertes eines beliebigen Beobachtungs- bzw. Messpunktes von dem Blutflussgeschwindigkeitswert, der dem Blutflussgeschwindigkeits-Filtermittel bereitgestellt wird, und Berechnen eines Differenzwertes hieraus,
20 ein Filtermittel zur Durchführung einer Filterung (42) des Differenzwertes, und
ein Additionsdurchführungsmittel (43) zum Addieren des Messpunkt-Blutflussgeschwindigkeitswertes zu einem Filterungsergebnis des Filtermittels.

- 25 **2.** Ultraschall-Doppler-Blutflussmessgerät nach Anspruch 1, wobei das Differenzberechnungsmittel den Differenzwert des nachfolgenden Punkt-Blutflussgeschwindigkeitswertes eines räumlich nachfolgend zu dem beliebigen Messpunkt angeordneten Punktes und des beliebigen Messpunkt-Blutflussgeschwindigkeitswertes berechnet.
- 30 **3.** Ultraschall-Doppler-Blutflussmessgerät nach Anspruch 1, wobei das Differenzberechnungsmittel den Differenzwert des Blutflussgeschwindigkeitswertes, der zeitlich nachfolgend zu dem beliebigen Messpunkt ist, und dem beliebigen Messpunkt-Blutflussgeschwindigkeitswert berechnet.

Revendications

- 35 **1.** Appareil de mesure de débit sanguin à ultrasons avec effet Doppler, comprenant :

un moyen émetteur (1) pour envoyer une impulsion ultrasonore dans un corps biologique étudié via une sonde ;
un moyen récepteur (3) pour recevoir un écho de l'impulsion ultrasonore réfléchi par le sang qui s'écoule dans
40 le corps biologique étudié ;
un moyen de détection de phase (4) pour détecter la phase d'un signal de l'écho de l'impulsion ultrasonore pour acquérir un signal de décalage Doppler qui inclut des informations sur le décalage Doppler dû à l'écoulement sanguin ;
un filtre passe-haut ou filtre de wall (5) pour supprimer les composantes à basse fréquence depuis le signal de décalage Doppler ;
45 un moyen de calcul de vitesse (6) pour calculer une valeur de vitesse de l'écoulement sanguin du sang à l'intérieur du corps biologique étudié en se basant sur un signal délivré depuis le filtre de wall ; et
un moyen de filtrage de vitesse de l'écoulement sanguin (20) pour effectuer un traitement de filtrage sur la valeur de vitesse de l'écoulement sanguin ;

caractérisé en ce que

le moyen de filtrage de vitesse de l'écoulement sanguin (20) comprend :

un moyen de calcul de différence (41) pour soustraire une valeur de vitesse de l'écoulement sanguin en un point focal arbitraire depuis la valeur de vitesse de l'écoulement sanguin fournie au moyen de filtrage de vitesse
55 de l'écoulement sanguin et pour calculer une valeur de différence de ces vitesses ;
un moyen de filtrage pour exécuter un traitement de filtrage (42) sur la valeur de différence ; et
un moyen de traitement additif (43) pour ajouter la valeur de vitesse de l'écoulement sanguin au point focal à

EP 1 683 486 B1

un résultat de traitement de filtrage des moyens de filtrage.

- 5
2. Appareil de mesure de débit sanguin à ultrasons avec effet Doppler selon la revendication 1, dans lequel ledit moyen de calcul de différence calcule la valeur de différence de la valeur de vitesse de débit sanguin consécutif en un point qui est consécutif dans l'espace dudit point focal arbitraire, et ladite valeur de vitesse de l'écoulement sanguin au point focal arbitraire.
- 10
3. Appareil de mesure de débit sanguin à ultrasons avec effet Doppler selon la revendication 1, dans lequel ledit moyen de calcul de différence calcule la valeur de différence de la valeur de vitesse de débit sanguin qui est consécutive dans le temps par rapport audit point focal arbitraire, et ladite valeur de vitesse de l'écoulement sanguin au point focal arbitraire.

15

20

25

30

35

40

45

50

55

FIG. 1

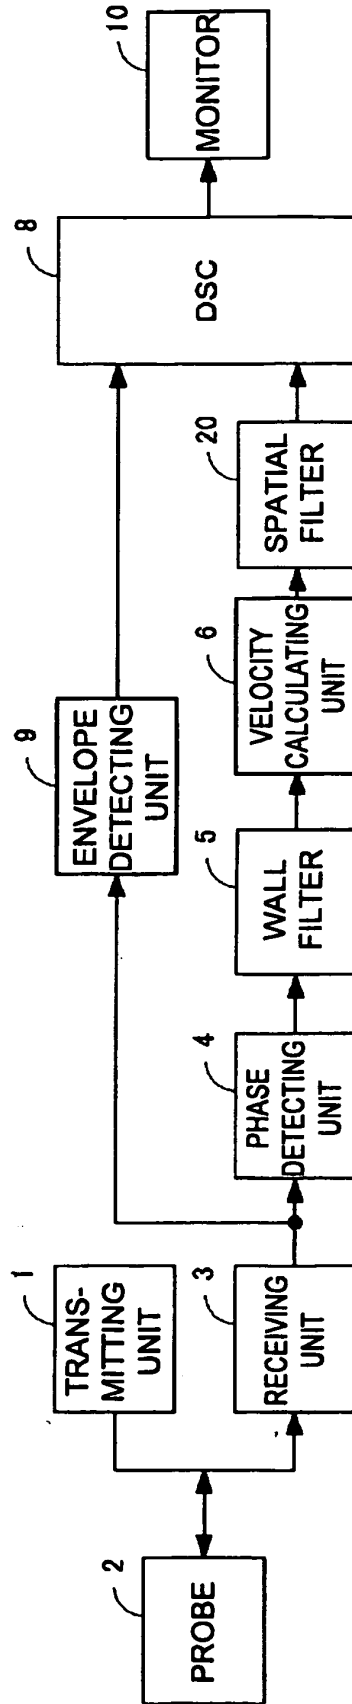


FIG. 2

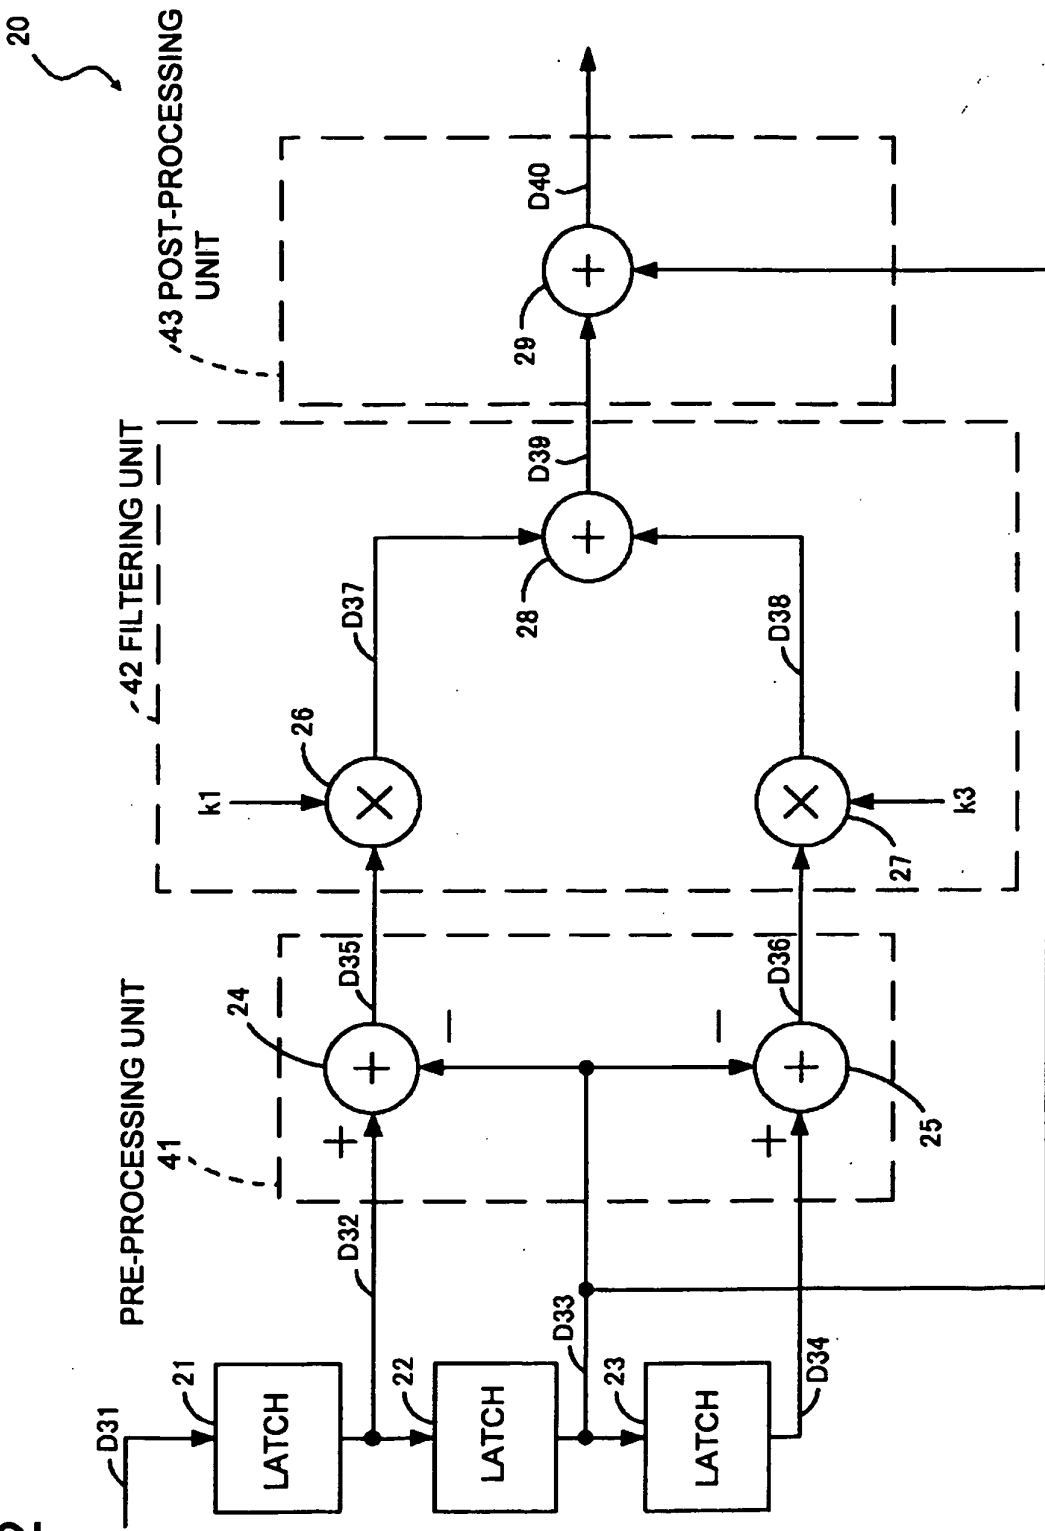
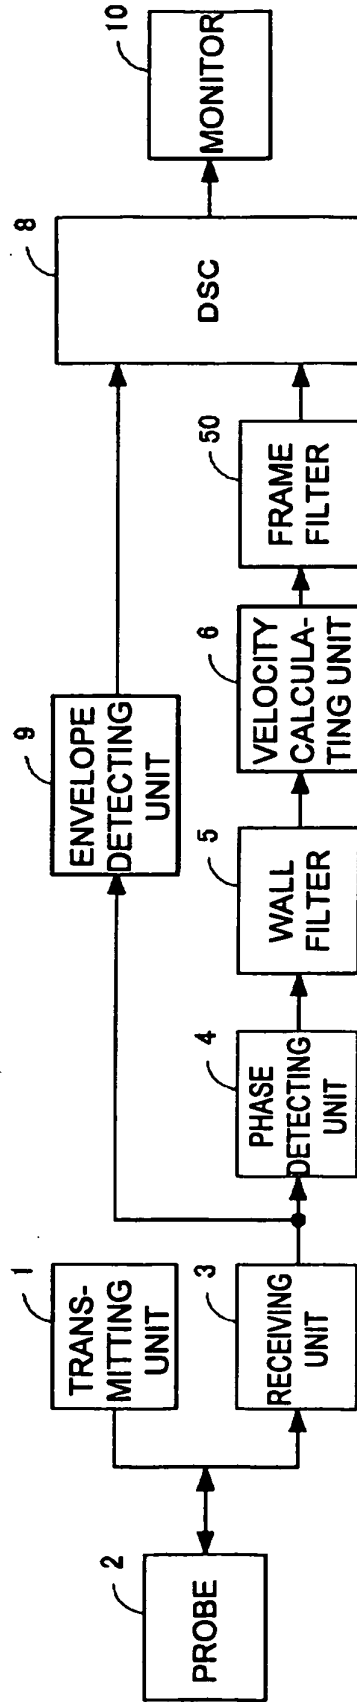


FIG. 3




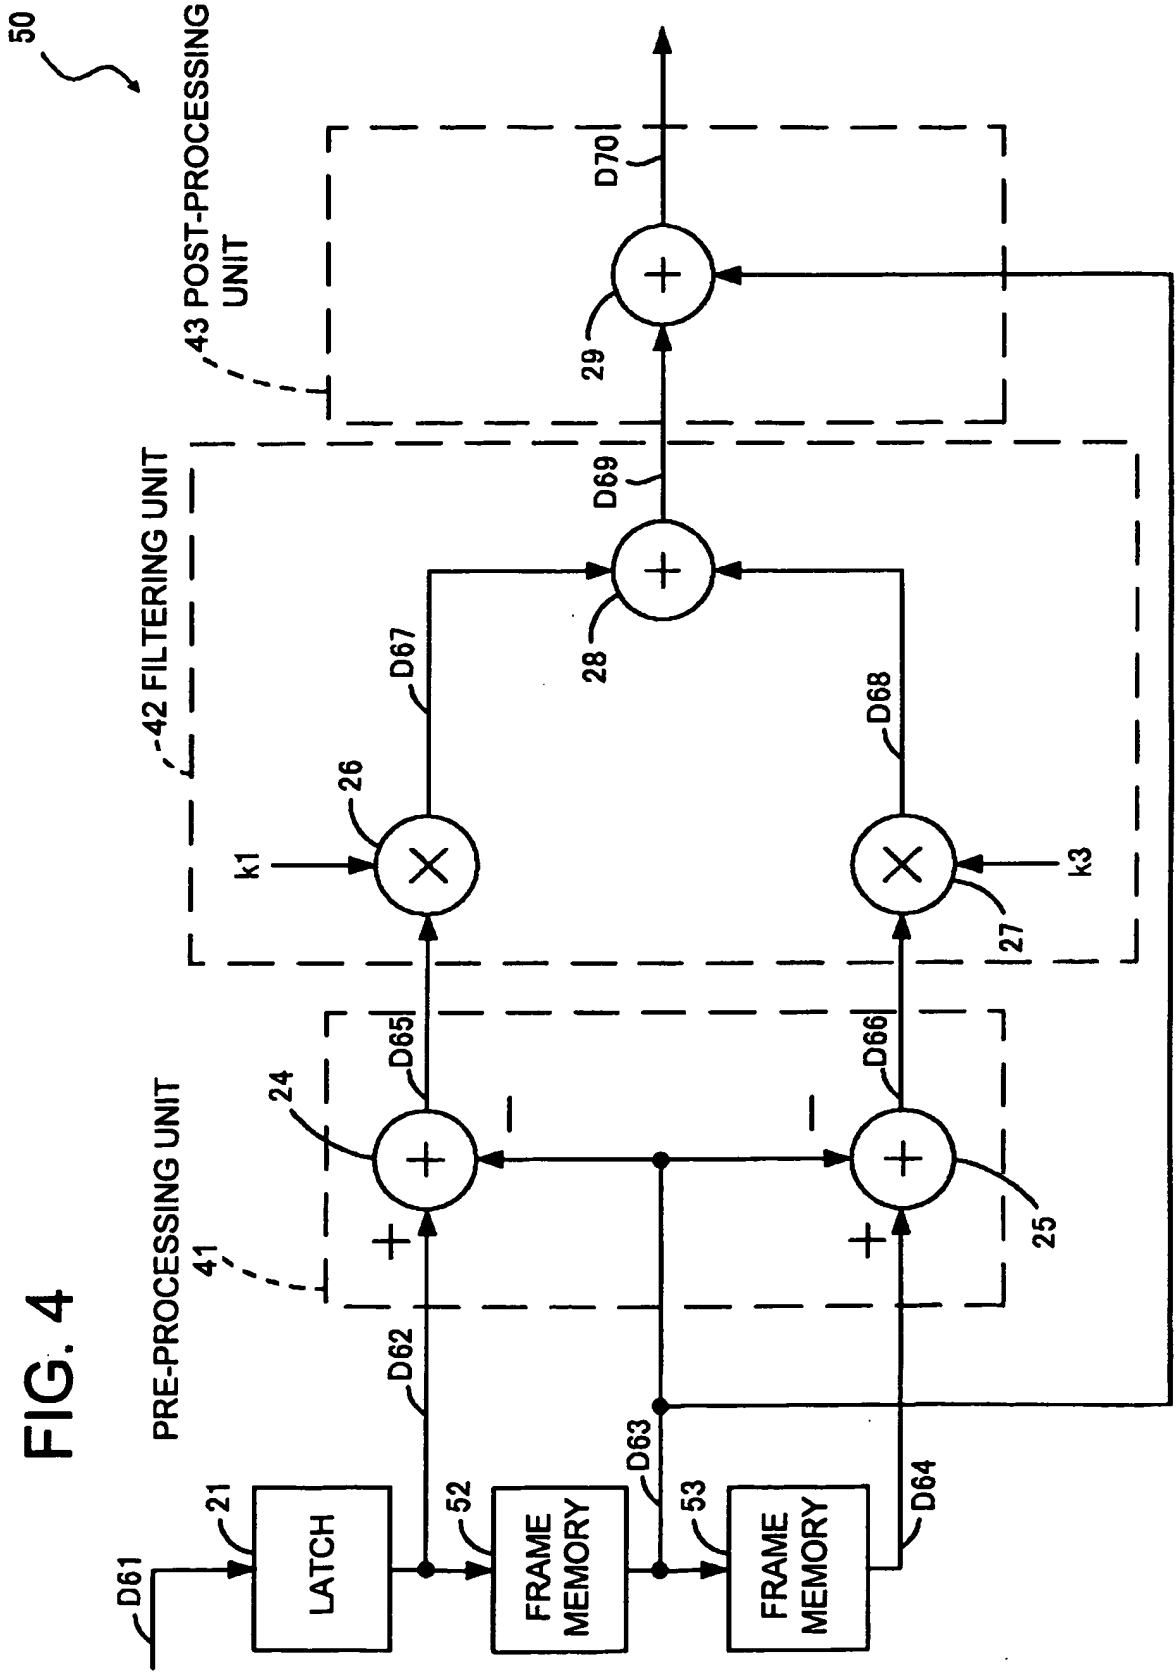


FIG. 4

FIG. 5 PRIOR ART

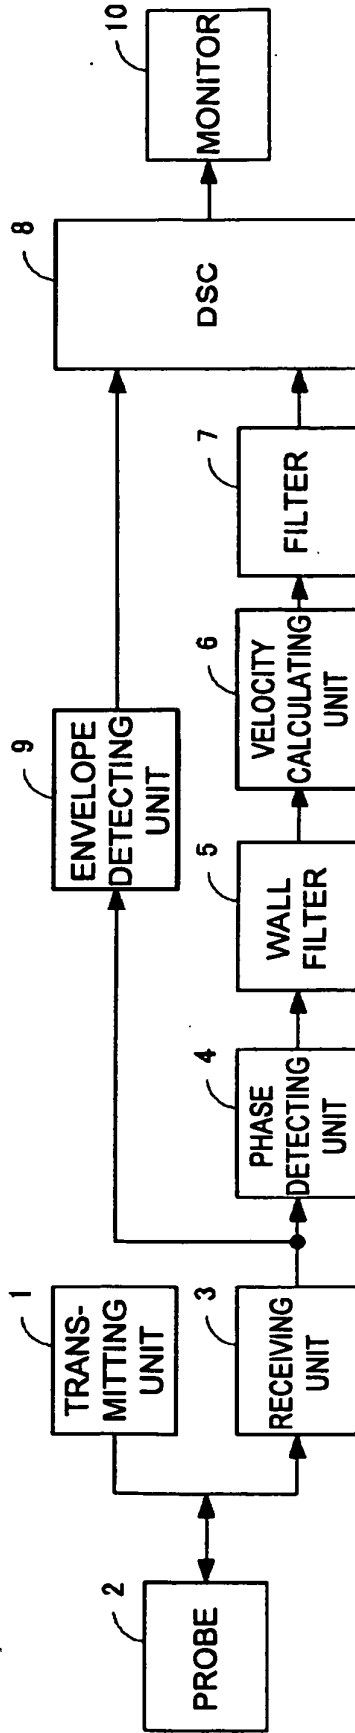

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 4161146 A [0006]
- US 6077226 A [0006]
- US 5860930 A [0006]

专利名称(译)	超声多普勒血流测量装置		
公开(公告)号	EP1683486A4	公开(公告)日	2008-04-16
申请号	EP2004792506	申请日	2004-10-15
申请(专利权)人(译)	松下电器产业有限公司.		
当前申请(专利权)人(译)	松下电器产业有限公司.		
[标]发明人	HAGIWARA HISASHI		
发明人	HAGIWARA, HISASHI		
IPC分类号	A61B8/06 A61B8/00		
CPC分类号	A61B8/06 G01S15/8981		
优先权	2003358059 2003-10-17 JP		
其他公开文献	EP1683486A1 EP1683486B1		
外部链接	Espacenet		

摘要(译)

公开了一种用于仅通过共同的滤波处理装置和共同的加法和减法装置进行混叠的血流速度数据的滤波处理和实现平滑血流速度的图像显示的技术。根据该技术，当使用超声波多普勒方法执行对象生物体内血液的血流速度的图像显示时，任意焦点的数据D33的差值和空间先前和后续的数据D32和D34在预处理单元（差值计算单元）41中计算该焦点。然后，在滤波单元42中，在对这些差值执行滤波处理之后，滤波处理之后的数据D39和任意焦点的数据D33在这样的情况下，可以在速度差小于由混叠现象产生的速度差的假设下进行滤波处理，并且对血液进行滤波处理。可以在不受混叠影响的情况下执行超声波的声线方向上的流速值。

