



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
14.04.2010 Bulletin 2010/15

(51) Int Cl.:
A61B 8/00 (2006.01)

(21) Application number: **09170532.7**

(22) Date of filing: **17.09.2009**

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL
PT RO SE SI SK SM TR**

(30) Priority: **08.10.2008 KR 20080098576**

(71) Applicant: **MEDISON CO., LTD.**
Kangwon-do 250-870 (KR)

(72) Inventor: **Song, Jung Sik**
135-851, Seoul (KR)


(74) Representative: **Schmid, Wolfgang**
Lorenz & Kollegen
Patentanwälte Partnerschaftsgesellschaft
Alte Ulmer Straße 2
89522 Heidenheim (DE)

(54) **Ultrasound System with Control Panel Adjustable in Height Through Contact**

(57) Disclosed herein is an ultrasound system which has a control panel (10) adjustable in height through contact. The ultrasound system includes the control panel (10), a power transmission device (20) adjusting a height

of the control panel (10), a contact detection unit (30) detecting contact and generating a selection signal, and a controller (40) controlling the power transmission device (20) according to the selection signal.

Fig. 1

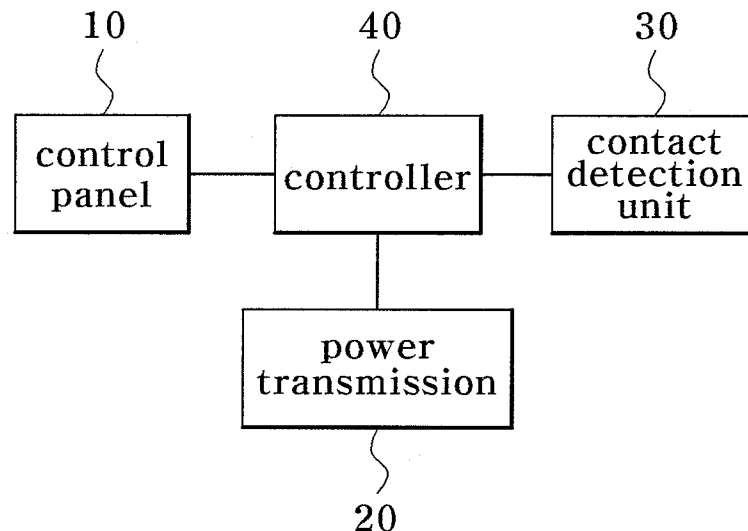

Description

BACKGROUND OF THE INVENTION

1. Field of the Invention

[0001] The present invention relates to an ultrasound system and, more particularly, to an ultrasound system that allows a user to adjust the height of a control panel with a contact detection unit detecting contact of the user and a power transmission device capable of performing a brake operation with electric power.

2. Description of the Related Art

[0002] Generally, an ultrasound system refers to a non-invasive apparatus that irradiates an ultrasound signal from a surface of a patient body towards a target internal organ within the body surface and obtains an image of a monolayer or blood flow in soft tissue from information in the reflected ultrasound signal (ultrasound echo-signal). The ultrasound system has been widely used for diagnosis of the heart, the abdomen, the urinary organs, and in obstetrics and gynecology due to its various merits such as a small size, a low price, real-time image display, and high stability through elimination of any radiation exposure, as compared with other image diagnostic systems, such as X-ray diagnostic systems, computerized tomography scanners (CT scanners), magnetic resonance imagers (MRIs), nuclear medicine diagnostic apparatuses, and the like.

[0003] Particularly, a conventional ultrasound system includes a control panel, through which a user can select measurement modes and functions, and optimize an ultrasound image displayed on a screen of a display unit. The control panel includes a touch screen which displays menus for optimizing an ultrasound image displayed on the screen of the display unit and provides a function of selecting the menus displayed thereon, a track ball which is used to move a cursor displayed on the screen of the display unit and provides a function of searching images from Cine-images, a keyboard which is used to input text and provides short cuts according to the measurement modes, and the like.

[0004] Here, it should be noted that the above description is not given for illustration of a conventional technique to which the present invention pertains, but for understanding of the background of the present invention.

[0005] A conventional ultrasound system includes a mechanical manipulating device such as a lever to adjust the height of the control panel. With this configuration, when a user adjusts the height of the control panel during ultrasound diagnosis, the conventional ultrasound system requires the user to halt diagnosis and manually adjust the height of the control panel with the lever, thereby providing inconvenience to the user. Therefore, there is a need for an improved ultrasound system that overcomes such a problem.

SUMMARY OF THE INVENTION

[0006] The present invention is conceived to solve the problem of the conventional technique as described above, and an aspect of the present invention is to provide an ultrasound system that allows a user to adjust the height of a control panel using a contact detection unit detecting contact of the user and a power transmission device capable of performing a brake operation with electric power, thereby improving user convenience in ultrasound diagnosis with the ultrasound system.

[0007] According to an aspect of the present invention, an ultrasound system having a control panel adjustable in height through contact is provided. The ultrasound system includes the control panel; a power transmission device adjusting a height of the control panel; a contact detection unit detecting contact and generating a selection signal; and a controller controlling the power transmission device according to the selection signal.

[0008] The contact detection unit may be mounted on a handle of the control panel.

[0009] The contact detection unit may include a light emitting diode (LED) which displays a contact state of a user with the contact detection unit.

[0010] The contact detection unit may include at least one of a pressure sensor, an electrostatic capacity sensor, and a temperature sensor.

[0011] The selection signal may be classified according to a contact period of time with the contact detection unit.

[0012] The power transmission device may include a brake driven by electric power.

[0013] The ultrasound system may further include an operation display unit displaying an operating state of the power transmission device according to an output from the controller.

[0014] The operation display unit may include at least one of an LED, a speaker, and a display.

[0015] As apparent from the above description, the ultrasound system according to an embodiment of the present invention allows a user to adjust the height of the control panel using the contact detection unit detecting contact of the user and the power transmission device capable of performing a brake operation with electric power, thereby improving user convenience in ultrasound diagnosis with the ultrasound system.

[0016] Further, the ultrasound system according to another embodiment of the present invention allows a user to more easily check and determine an operating state and an operation start time of the power transmission device through the operation display unit, so that the user can adjust the height of the control panel more conveniently.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] The above and other aspects, features and advantages of the present invention will become apparent

from the following description of exemplary embodiments given in conjunction with the accompanying drawings, in which:

- Fig. 1 is a block diagram of an ultrasound system according to an exemplary embodiment of the present invention;
- Fig. 2 is a block diagram of an ultrasound system including an operation display unit according to an exemplary embodiment of the present invention;
- Fig. 3 is a perspective view of an ultrasound system with a control panel adjustable in height through contact according to an exemplary embodiment of the present invention; and
- Fig. 4 shows a contact detection unit according to an exemplary embodiment of the present invention.

DETAILED DESCRIPTION OF THE EMBODIMENT

[0018] Exemplary embodiments of the present invention will now be described in detail with reference to the accompanying drawings hereinafter. It should be noted that the drawings are not to precise scale and may be exaggerated in thickness of lines or size of components for descriptive convenience and clarity only. Furthermore, terms used herein are defined by taking functions of the present invention into account and can be changed according to the custom or intention of users or operators. Therefore, definition of the terms should be made according to overall disclosures set forth herein.

[0019] Fig. 1 is a block diagram of an ultrasound system according to an exemplary embodiment of the present invention.

[0020] As shown in Fig. 1, the ultrasound system according to the embodiment of the invention includes a control panel 10, a power transmission device 20, a contact detection unit 30, and a controller 40.

[0021] Operation of the ultrasound system with the control panel adjustable in height through contact according to the embodiment of the invention will be described in detail.

[0022] When a user holds the contact detection unit 30 to adjust the height of the control panel 10 during ultrasound diagnosis with the ultrasound system, the contact detection unit 30 detects contact of the user and generates a selection signal.

[0023] Here, the contact detection unit 30 includes at least one of a pressure sensor, an electrostatic capacity sensor and a temperature sensor, and generates the selection signal after detecting the contact of the user via the respective sensors.

[0024] The selection signal may be classified according to a contact period of time of the user. For example, when the user holds the contact detection unit 30 for a predetermined period of time or more, the contact detection unit 30 may generate a selection signal which in-

structs operation of the power transmission device 20. The predetermined period of time may be 1 or 2 seconds.

[0025] When the selection signal is generated, the controller 40 receives the selection signal and controls the power transmission device 20 in response to the selection signal. Then, the power transmission device 20 adjusts the height of the control panel 10 according to the control of the control panel 40.

[0026] The power transmission device 20 may include a brake driven by electric power. For example, the power transmission device 20 includes an electric brake which can be turned-on/off by electric power, so that, when a user holds the contact detection unit 30 for a predetermined period of time or more, the power transmission device 20 releases the brake according to the control of the controller 40 to allow the user to adjust the height of the control panel 10. When the user stops contacting the contact detection unit 30, the power transmission device 20 operates the brake according to the control of the controller 40 to allow the control panel 10 to be secured at a desired height.

[0027] According to one embodiment of the invention, the contact detection unit 30 may be mounted on a handle of the control panel 10 and may include an LED to display a contact state between a user and the contact detection unit 30.

[0028] Fig. 2 is a block diagram of an ultrasound system including an operation display unit according to an exemplary embodiment of the present invention.

[0029] Operation of the ultrasound system including the operation display unit 50 will be described in detail with reference to Fig. 2. As described above, the controller 40 receives a selection signal and controls the power transmission device 20 according to the received selection signal.

[0030] When the controller 40 outputs a control signal, the operation display unit 50 displays an operation state of the power transmission device 20 according to the control signal output from the controller 40.

[0031] The operation display unit 50 may include at least one of an LED 51, a speaker 52, and a display 53.

[0032] For example, if the LED 51 is used, the LED 51 emits blue light when a user contacts the contact detection unit 30 for a predetermined period of time or more to release the brake of the power transmission device 20, and emits red light when the user stop contacting the contact detection unit 30 to operate the brake of the power transmission device 20.

[0033] Similarly, if the speaker 52 is used, the speaker 52 generates a long beep sound and a short beep sound according to an output from the controller 40 when the brake of the power transmission device 20 is released and operated, respectively, thereby allowing the user to easily recognize the operation state of the power transmission device 20.

[0034] Further, if the display 53 is used, the display 53 displays associated words, figures or the like according to an output from the controller 40 when the brake of the

power transmission device 20 is released and operated, respectively.

[0035] When one or more of the LED 51, the speaker 52 and the display 53 are used not individually but cooperatively, a user can more easily recognize the operation state of the power transmission device 20.

[0036] Fig. 3 is a perspective view of an ultrasound system with a control panel adjustable in height through contact according to an exemplary embodiment of the present invention.

[0037] As shown in Fig. 3, a user can adjust the height of the control panel 10 by touching the contact detection unit 30 mounted on the handle of the control panel 10, as described above. The user can easily recognize an operation state of the power transmission device 20 through the LED 51, the speaker 52 or the display 53 which constitutes the operation display unit 50.

[0038] Fig. 4 shows a contact detection unit according to an exemplary embodiment of the present invention.

[0039] As shown in Fig. 4, the contact detection unit 30 may include an LED 31, on which a contact state between a user and the contact detection unit 30 can be displayed. For example, the LED 31 emits yellow light while the user contacts the contact detection unit 30, and emits red-orange light when the user stops contacting the contact detection unit 30, thereby making it easy for the user to judge whether the contact between the user and the contact detection unit 30 is sufficiently carried out.

[0040] As such, the ultrasound system according to one embodiment of the present invention allows a user to adjust the height of a control panel using a contact detection unit detecting contact of the user and a power transmission device capable of performing a brake operation with electric power, thereby improving user convenience in ultrasound diagnosis with the ultrasound system.

[0041] Further, the ultrasound system according to another embodiment of the present invention allows a user to more easily check and determine an operating state and an operation start time of the power transmission device through an operation display unit, so that the user can adjust the height of the control panel more conveniently.

[0042] Although the present invention has been described with reference to the embodiments, it will be apparent to those skilled in the art that the embodiments are given by way of illustration only, and that various modifications and equivalent embodiments can be made without departing from the spirit and scope of the present invention. Accordingly, the scope of the present invention should be limited only by the accompanying claims.

Claims

1. An ultrasound system having a control panel (10) adjustable in height through contact, **characterized in that** the ultrasound system comprises:

the control panel (10);

a power transmission device (20) adjusting a height of the control panel (10);

a contact detection unit (30) detecting contact and generating a selection signal; and

a controller (40) controlling the power transmission device (20) according to the selection signal.

2. The ultrasound system according to claim 1, **characterized in that** the contact detection unit (30) is mounted on a handle of the control panel (10).

3. The ultrasound system according to claim 1, **characterized in that** the contact detection unit (30) comprises a light emitting diode (LED) (31) displaying a contact state of a user with the contact detection unit (30).

4. The ultrasound system according to claim 1, **characterized in that** the contact detection unit (30) comprises at least one of a pressure sensor, an electrostatic capacity sensor, and a temperature sensor.

5. The ultrasound system according to claim 1, **characterized in that** the selection signal is classified according to a contact period of time with the contact detection unit (30).

6. The ultrasound system according to claim 1, **characterized in that** the power transmission device (20) comprises a brake driven by electric power.

7. The ultrasound system according to claim 1, **characterized in that** the ultrasound system further comprises:

an operation display unit (50) displaying an operating state of the power transmission device (20) according to an output from the controller (10).

8. The ultrasound system according to claim 7, **characterized in that** the operation display unit (50) is at least one of an LED (51), a speaker (52), and a display (53).

Fig. 1

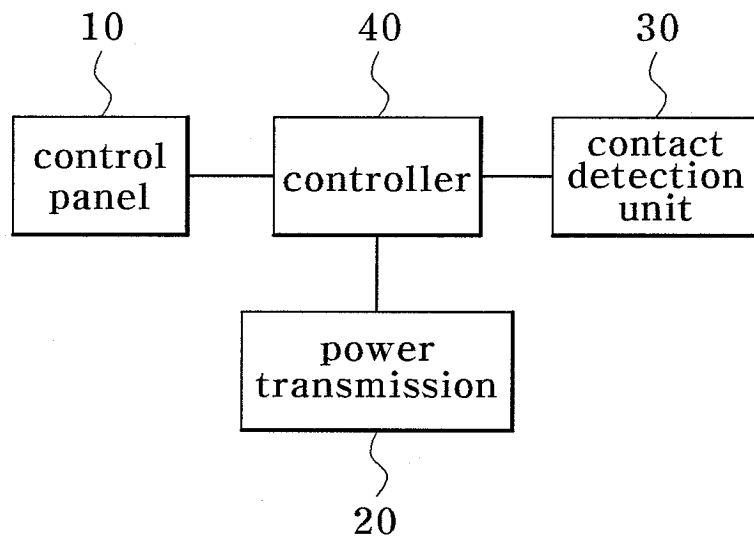


Fig. 2

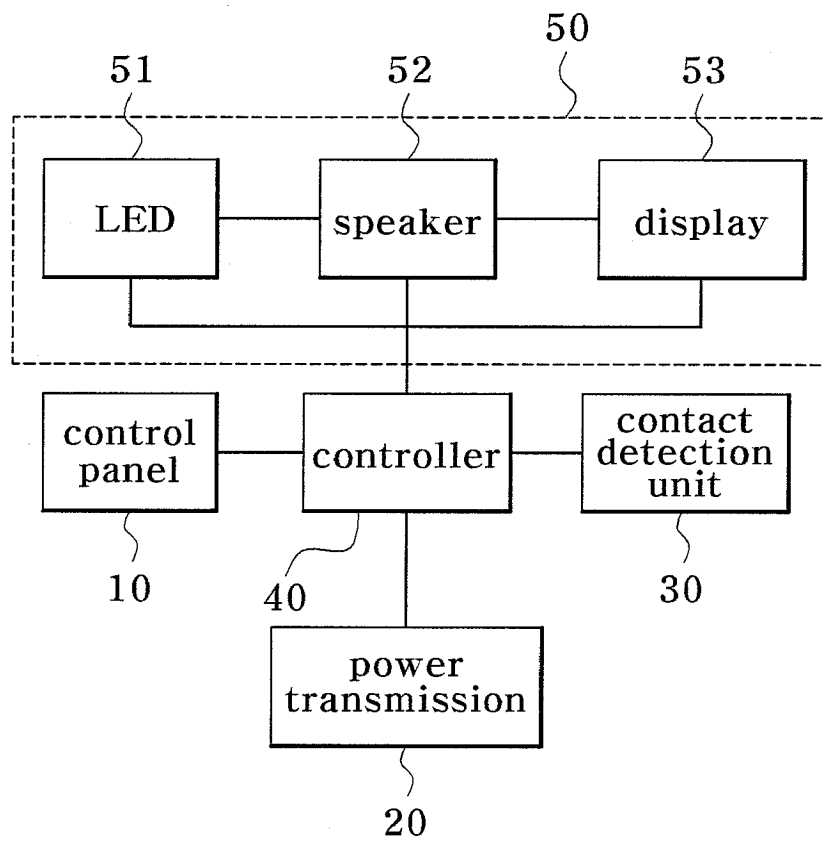


Fig. 3


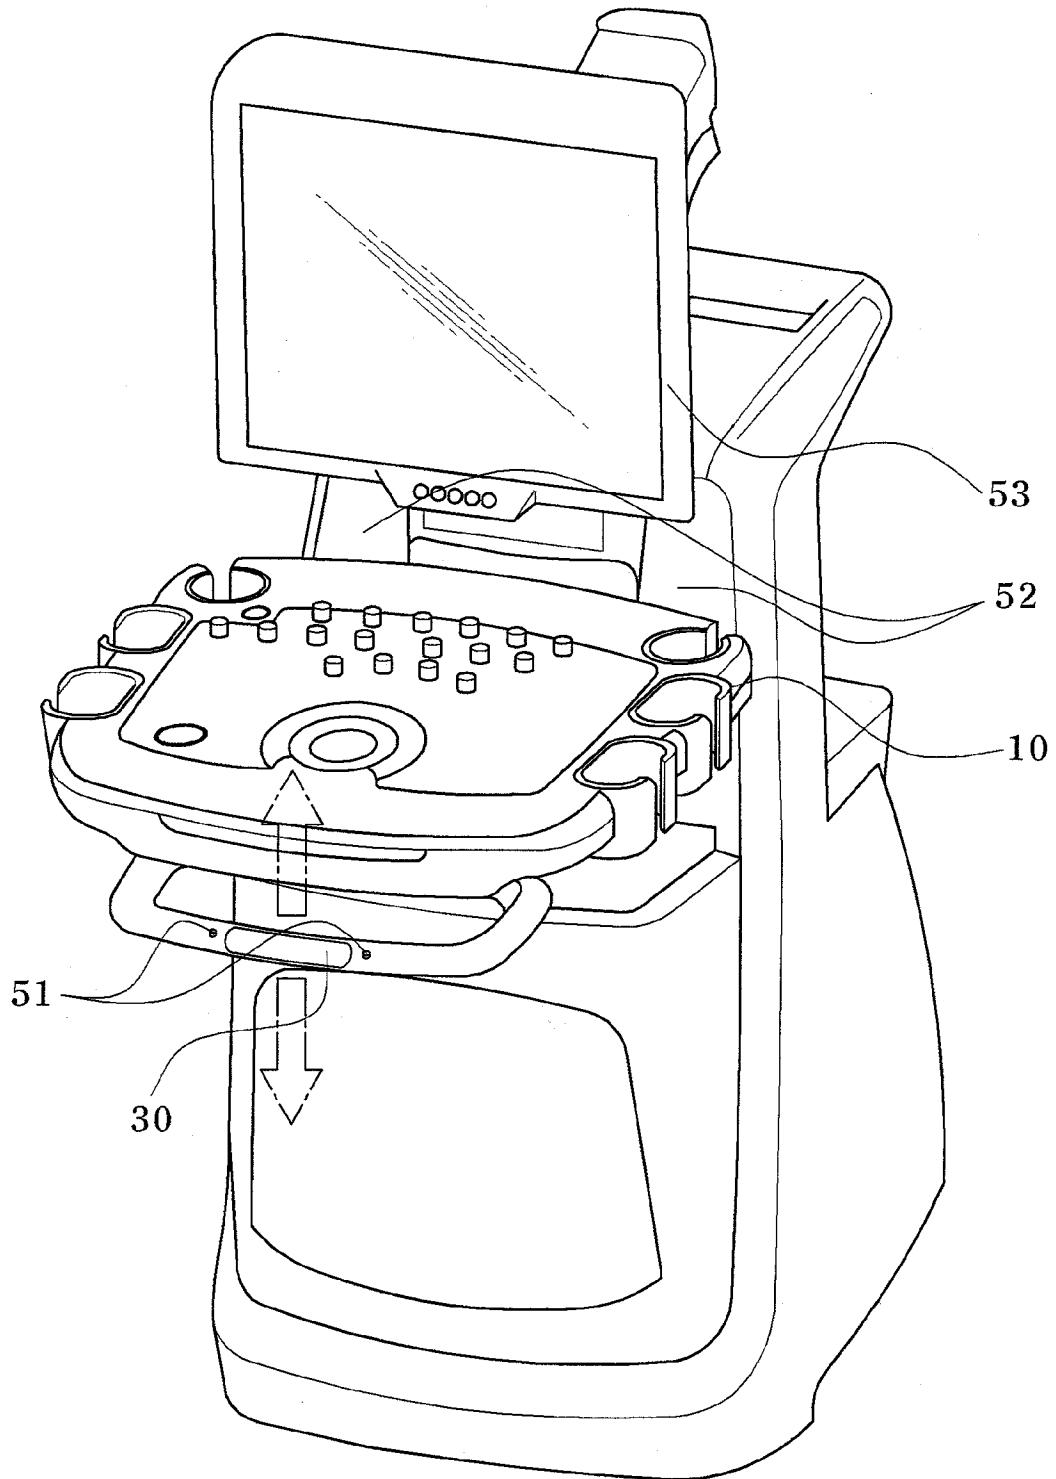


Fig. 4



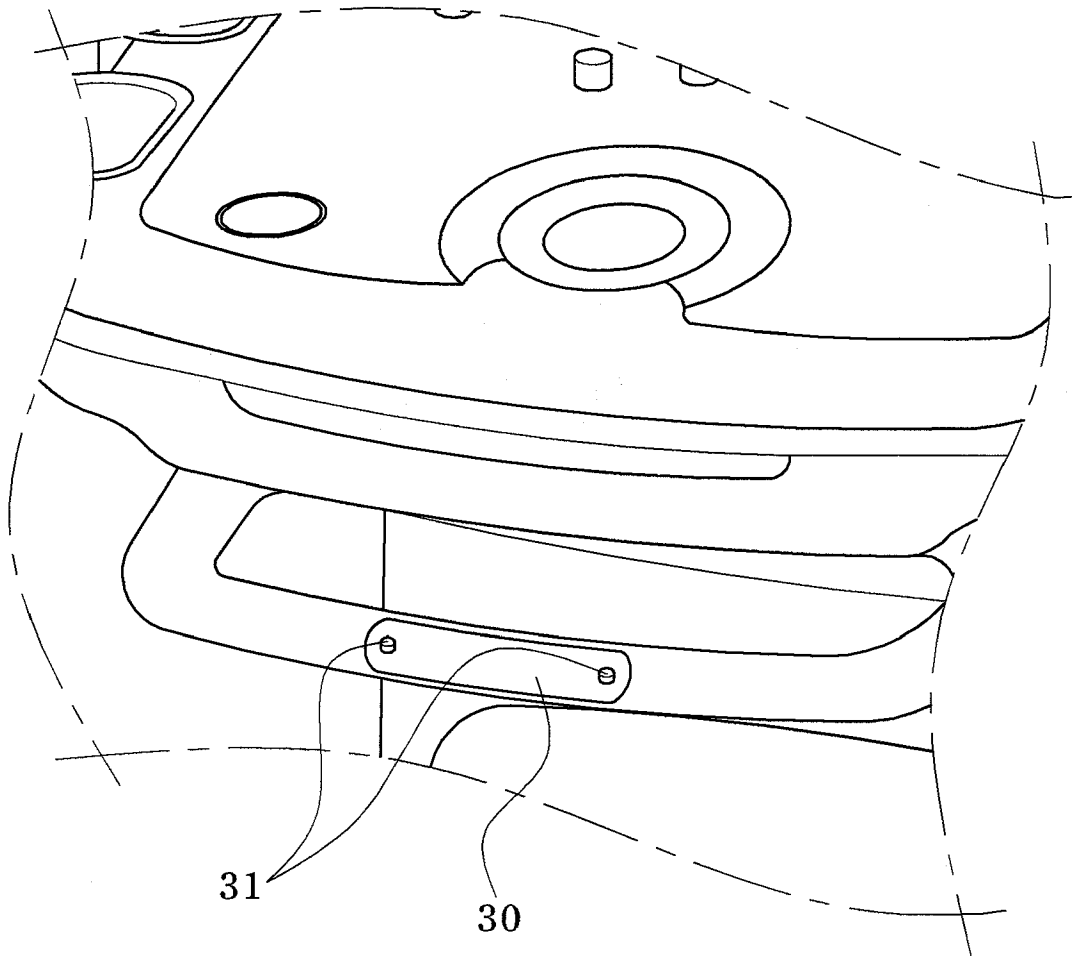

EUROPEAN SEARCH REPORT

Application Number
EP 09 17 0532

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 2004/085715 A1 (BIDWELL DEAN JEFFREY [US] ET AL) 6 May 2004 (2004-05-06)	1,4-6	INV. A61B8/00
Y	* paragraph [0052]; figure 8 *	2-3,7-8	
Y	WO 2006/111874 A2 (KONINKL PHILIPS ELECTRONICS NV [NL]; POLAND MCKEE DUNN [US]) 26 October 2006 (2006-10-26) * page 9, lines 13,24-29; figures 2,3 *	2	
A	US 2008/035030 A1 (HORTON GEORGE [GB]) 14 February 2008 (2008-02-14) * paragraphs [0045], [0047] *	2	
A	US 5 398 622 A (LUBINSKAS ROBERT B [US] ET AL) 21 March 1995 (1995-03-21) * column 5, lines 40,45,46; figure 2 * * column 8, lines 3,11 *	2,6	
Y	EP 1 749 689 A1 (CNH OESTERREICH GMBH [AT]) 7 February 2007 (2007-02-07)	3,7-8	
A	* paragraphs [0019], [0020]; figure 1 *	6	
A	EP 0 313 369 A2 (DIMATIC LIMITED [GB]) 26 April 1989 (1989-04-26) * column 12, lines 27-29,35-38 *	3,8	
A	US 2005/059892 A1 (DUBOIS ELIZABETH [US] ET AL) 17 March 2005 (2005-03-17) * paragraph [0041]; figure 3 *	6	
A	US 2007/225690 A1 (SEKIGUCHI KIYOSHI [JP] ET AL) 27 September 2007 (2007-09-27) * paragraph [0002]; figure 5 *	7-8	
The present search report has been drawn up for all claims			TECHNICAL FIELDS SEARCHED (IPC)
			A61B
Place of search		Date of completion of the search	Examiner
The Hague		19 January 2010	Visser, Rogier
CATEGORY OF CITED DOCUMENTS			
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	

 1
EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 09 17 0532

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

19-01-2010

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2004085715 A1	06-05-2004	US 6683784 B1	27-01-2004
WO 2006111874 A2	26-10-2006	JP 2008536555 T	11-09-2008
US 2008035030 A1	14-02-2008	CA 2612629 A1	12-01-2006
		EP 1773156 A1	18-04-2007
		WO 2006003406 A1	12-01-2006
US 5398622 A	21-03-1995	NONE	
EP 1749689 A1	07-02-2007	GB 2428770 A	07-02-2007
EP 0313369 A2	26-04-1989	AP 72 A	25-02-1990
		AU 2399788 A	04-05-1989
		BE 1002402 A5	29-01-1991
		IL 88018 A	12-12-1991
		ZA 8805545 A	26-04-1989
US 2005059892 A1	17-03-2005	NONE	
US 2007225690 A1	27-09-2007	JP 2007175231 A	12-07-2007

专利名称(译)	控制面板超声系统可通过接触高度调节		
公开(公告)号	EP2174595A1	公开(公告)日	2010-04-14
申请号	EP2009170532	申请日	2009-09-17
申请(专利权)人(译)	MEDISON CO. , LTD.		
当前申请(专利权)人(译)	MEDISON CO. , LTD.		
[标]发明人	SONG JUNG SIK		
发明人	SONG, JUNG SIK		
IPC分类号	A61B8/00		
CPC分类号	A61B8/00 A61B8/461 A61B8/467		
代理机构(译)	SCHMID , WOLFGANG		
优先权	1020080098576 2008-10-08 KR		
外部链接	Espacenet		

摘要(译)

本文公开了一种超声系统，其具有通过接触可调节高度的控制面板（10）。超声系统包括控制面板（10），调节控制面板（10）的高度的电力传输装置（20），检测接触并产生选择信号的接触检测单元（30），以及控制器（40）根据选择信号控制电力传输设备（20）。

Fig. 1

