

(19)



(11)

EP 2 575 624 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
26.04.2017 Bulletin 2017/17

(51) Int Cl.:
A61B 8/00 (2006.01)

(21) Application number: **11719285.6**

(86) International application number:
PCT/EP2011/057868

(22) Date of filing: **16.05.2011**

(87) International publication number:
WO 2011/147704 (01.12.2011 Gazette 2011/48)

(54) **Ultrasound coupling liquid and container**

Ultraschallkupplungsflüssigkeit und Behälter

Liquide et conteneur de couplage à ultrasons

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

• **PECHOUX, Thierry**
F-75019 Paris (FR)

(30) Priority: **25.05.2010 EP 10163725**

(74) Representative: **Hepp Wenger Ryffel AG**
Friedtalweg 5
9500 Wil (CH)

(43) Date of publication of application:
10.04.2013 Bulletin 2013/15

(56) References cited:
WO-A1-2010/016789 WO-A2-2006/032059
JP-A- 2 092 343 US-A- 4 641 362
US-A- 4 886 068 US-A- 5 078 149
US-A- 6 126 619 US-B1- 6 432 069
US-B1- 6 626 855

(73) Proprietor: **Theraclion SA**
92240 Malakoff (FR)

(72) Inventors:
• **BROCARDO, Roberta**
F-75013 Paris (FR)

EP 2 575 624 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] This invention relates to a coupling liquid for ultrasound imaging or treatment according to claim 1 as well as to a container filled with a coupling liquid according to claim 7.

[0002] The use of ultrasound is known for imaging purposes. But ultrasound may also be used for therapeutic purposes, either for the destruction of concretions by mechanical effect or in order to create lesions in tissue by thermal effect.

[0003] In both cases, use of a coupling liquid between the ultrasound transducer and the skin of the patient is advantageous. The coupling liquid ensures proper transmission of ultrasound waves from the ultrasound transducer to the skin. The coupling liquid may be applied directly on the skin, thus forming a bridging layer between the skin and the ultrasound transducer. Such a direct application is mostly used with imaging transducers. Alternatively, the coupling liquid may be contained in a balloon-like cover member affixed on an ultrasound transducer. Such a configuration is mostly used with high intensity focused ultrasound (HIFU) transducers, where the coupling liquid additionally serves as cooling liquid to both cool the transducer and the skin. The coupling liquid is advantageously being constantly cycled through additional cooling means, such as a heat exchanger.

[0004] Known coupling liquids are mostly water based hydrogels. Known gelling agents are mostly polymers, for example polyurethanes, polyols and the like.

[0005] One major problem with coupling liquids is that when high ultrasound energies are used, e.g. in a HIFU treatment, bubbles are formed in the liquid by a cavitation effect. Such bubbles may cause problems when additional ultrasound imaging is used to monitor the treatment and/or to position the focal point of the ultrasound waves.

[0006] Japanese patent application 2 92343 discloses a coupling product for ultrasound imaging formed by a matrix of porous material like polyurethane which contains an aqueous gel such as polyvinylpyrrolidone.

[0007] US 5,078,149 describes an ultrasound coupling product having a recipient containing a polymer gel. The recipient may be attached to the tip of an ultrasound probe to serve as coupling member. The polymer is integrally crosslinked with the recipient.

[0008] Such coupling products have the disadvantage that they are not pumpable and thus may not provide any cooling to the ultrasound transducer or the skin.

[0009] US 6,432,069 discloses an aqueous coupling liquid comprising a hydrophilic polymer, preferably polyvinylpyrrolidone. The polymer is present in an amount of between 10 and 50 g/L. The liquid is specifically optimized for the use in high energy ultrasound applications, like HIFU treatment, since almost no bubbles are formed due to the cavitation effect. Moreover, as the viscosity of the liquid is below $2 \cdot 10^{-4}$ Pa·s it is readily pumpable and may thus also act as cooling liquid. For this purpose, the coupling liquid is constantly pumped through a cover member covering an ultrasound transducer.

[0010] US 4 886 068 A discloses an ultrasound coupling liquid agent of low viscosity which comprises at least one aqueous solution selected from an aqueous ethyl alcohol solution and an aqueous glycerine solution.

However, at the boundary between the coupling liquid and the cover member and/or skin of the patient, a certain amount of ultrasound waves are reflected due to the different refraction indexes of the materials. Moreover, as some of the used polymers are of organic nature, bacterial and algal growth might occur, thus making a sterilization of the liquid necessary. It is an objective of the present invention to overcome the disadvantages of the known coupling liquids and especially to provide an ultrasound coupling liquid leading to less reflection of the ultrasound waves and which is not prone to bacterial or algal growth. This problem is solved with a coupling liquid according to claim 1.

[0011] A "hydrophilic polymer" as understood herein means a polymer which has a sufficient affinity to water as to dissolve therein or to form a gel with it. Suitable examples of hydrophilic polymers are: acrylic polymers, poly(vinyl alcohol), cellulose derivatives, gelatine, gums such as e.g. guar or agaragar, poly(ethylene oxide), polyvinylpyrrolidone or mixtures thereof.

[0012] Preferably, the coupling liquid comprises a single hydrophilic polymer. Polymers with an average molecular mass in the range of between 30,000 and 70,000 present at a low concentration, such as between 10 and 50 g/L allow the production of hydrogels having a relatively low viscosity, preferably between $1 \cdot 10^{-4}$ Pa·s and $2 \cdot 10^{-4}$ Pa·s at 20°C. Such a viscosity allows the hydrogel to be readily pumped and thus used in a liquid circuit with a cooling unit.

[0013] Further, the coupling liquid comprises at least one alcohol with a carbon chain of 1 to 7 carbon atoms. The carbon chain may be branched or unbranched. Preferably the alcohol is selected from ethanol, butanol, propanol, isopropanol, pentanol, hexanol, heptanol or mixtures thereof. More preferably, the at least one alcohol is a primary alcohol.

[0014] Surprisingly, addition of an alcohol to a coupling liquid comprising a hydrophilic polymer was found to considerably reduce the reflection of ultrasound waves at the boundary between the coupling liquid and the skin and/or a cover member covering an ultrasound transducer. Moreover, reduction of the refractive index between the coupling liquid and the skin and/or the cover member shifts the focal point of the ultrasound waves deeper into the body. An additional effect is that bacterial and/or algal growth is hindered by the alcohol. Another additional effect is that the freezing point of the coolant is lowered with the addition of alcohol. Whereas the low temperature of known cooling fluids is limited to 0°C, the coolant according to the invention can be cooled to less than 0°C yielding a potentially better efficiency. For example

adding 5.5% ethanol lowers the freezing point to -2°C.

[0015] The at least one alcohol is present in a concentration of 3% to 45% by weight of the total weight of the coupling liquid, preferably 5 to 20%. The amount of ultrasound wave reflections is reduced when the alcohol concentration is in this range.

5 [0016] Most preferably the at least one alcohol is present in a concentration of 5% by weight of the total weight of the coupling liquid. This concentration was found to be the optimal concentration for a coupling fluid used with high energy ultrasound, especially with HIFU treatment.

[0017] The at least one alcohol is preferably selected from a group comprising of ethanol, propanol, isopropanol and/or benzyl alcohol. These alcohols have good antibacterial and antifungal properties. Thus, the coupling liquid does not need to be sterilized before packaging or use.

10 [0018] The hydrophilic polymer preferably is or comprises polyvinylpyrrolidone. Polyvinylpyrrolidone has about the same acoustic and absorption characteristics as water, thereby allowing the use of varying concentrations of polyvinylpyrrolidone with only minor changes in the overall characteristics of the solution.

[0019] These low attenuation and/or acoustic absorption characteristics of the coupling liquid ensure that a major portion of the ultrasound waves are effectively transmitted towards the skin rather than being absorbed by the coupling liquid.

15 [0020] The polyvinylpyrrolidone used in the present invention most preferably has an average molecular mass of 58,000, like e.g. polyvinylpyrrolidone available under the trademark Plasdone® K-29/32 (ISC Corp., USA).

[0021] Most preferably, the hydrophilic polymer is present in an amount of between 1% and 5% weight/volume of the coupling liquid. This allows obtaining a hydrogel with a viscosity which is sufficiently low to render the gel pumpable. The viscosity of the coupling liquid according to the present invention preferably is between $1 \cdot 10^{-4}$ Pa·s and $2 \cdot 10^{-4}$ Pa·s at 20°C, more preferably between $1.2 \cdot 10^{-4}$ Pa·s and $1.6 \cdot 10^{-4}$ Pa·s at 20°C.

20 [0022] Another objective of the present invention is to provide a container for a coupling fluid which is easy to integrate in a cooling system of an ultrasound device and which is protected from bacterial and fungal growth. This problem is solved by a container as claimed in claim 6.

25 [0023] The container according to the present invention has an outer wall with a high thermal conductivity defining a cavity filled with an ultrasound coupling liquid comprising a preservative. The ultrasound coupling liquid is a coupling liquid according to the present invention.

[0024] As "high thermal conductivity" as understood herein is a heat conductivity of more than 1000 W/K per m² of wall surface. This allows for a good heat transfer from the container to the cooling system, thereby allowing efficient temperature reduction in the coolant.

30 [0025] The wall preferably has a tensile strength of more than 30 N/mm². This avoids rupture of the container wall during handling, storage and/or transportation.

[0026] A container with a thin wall may not be sterilized by heat since the wall would not be able to withstand the internal pressure changes caused by the expansion of the liquid enclosed, and thus would be prone to bursting. A thin wall container may also be more prone to deformation due to softening of the wall material when heated. Sterilizing methods other than heat, such as gamma exposure or ethylene oxide (ETO) gas are also prone to modifying the material of the container walls or of the coupling liquid itself. The presence of a preservative in the coupling liquid eliminates the sterilization step, since growth of bacteria or fungi will be hindered. This allows the production of coupling liquid containers under non-sterile conditions, thereby lowering the production costs quite considerably.

35 [0027] For ease of use of an ultrasound device, especially in the field of HIFU treatment, it is important that the coupling liquid may be easily introduced into a liquid cooling cycle. By providing a container with a wall with a high thermal conductivity according to the present invention, it is possible to place the container onto or into cooling means, such as between two cooling plates or into a cooling bath. A high heat conductivity of the wall thus allows an effective heat transfer between the coupling liquid within the container and the cooling means. Hence, it is not necessary to remove the coupling liquid from the container and to fill it into a cooling system.

40 [0028] The preservative comprised in the coupling fluid filled in the container according to the present invention may be any suitable preservative hindering the growth of microorganisms, especially bacteria and fungi, as long as the acoustic properties are preserved or improved. The preservative comprised in the coupling liquid is an alcohol. The coupling liquid is a coupling liquid as described in the present invention comprising a hydrophilic polymer and an alcohol having a branched or unbranched carbon chain with 1 to 7 carbon atoms.

45 [0029] Preferably, the wall has a thickness of less than 0.5mm, more preferably less than 0.25mm, most preferably less than 0.125mm. Reducing the thickness of the wall will increase the thermal conductivity across the wall and hence the heat exchange between the coupling liquid inside the container and a cooling means. Reduction of the thickness of the wall the values indicated above even allows the wall to comprise or be made of a material which has a low thermal conductivity.

50 [0030] Reducing the thickness of the wall will also render it more flexible thus allowing for a quicker and better distribution of any pressure peak applied on the wall. This reduces the risk that the wall is locally ripped apart by such a pressure peak.

[0031] The wall preferably is made of or comprises a polymeric material.

[0032] Polymeric materials are readily available and cheap. Furthermore, there are many techniques known in the art to impart a specific shape to a polymeric material, like injection moulding, extruding, punching as well as vacuum or heat forming. This greatly facilitates the production process of a container according to the present invention.

[0033] Most preferably, the thin wall is made of or comprises poly(vinyl chloride). Use of poly(vinyl chloride) allows the manufacture of containers having very thin walls. Moreover, poly(vinyl chloride) can be handled easily and does not require special disposal after use.

[0034] Preferably, the container additionally comprises means to bring the cavity in fluid connection with an ultrasound probe head. Said means preferably comprise at least one tube. By the connection means, it is possible to integrate the container into a liquid circuit of an ultrasound device. For example, the coupling liquid may be constantly cycled by means of a pump from the container to the ultrasound probe head. Since the container has a thin outer wall, it may be placed on or inside a cooling means, such that the coupling liquid may additionally serve as cooling liquid.

[0035] Additionally, the container is airtight. By airtight is understood that no gas exchange between the cavity of the container and the atmosphere outside of the container is possible. This additionally reduces the probability of contamination of the coupling liquid with any microorganisms. Of course, once the container is connected with an ultrasound device or is opened for the withdrawal of liquid, it may no longer be airtight. Preferably, connection of the container with an ultrasound device is configured in such a way as to keep the entire liquid circuit airtight.

[0036] The container preferably comprises at least one frame element defining the geometrical shape of the container in one plane and two wall elements, wherein said two wall elements are fixed over said frame element thereby forming the cavity in between said two wall elements.

[0037] The frame element preferably is of rectangular shape. But the frame member may also be of any other suitable shape, such as circular. The frame element may also comprise additional elements, such as protrusions and/or recesses for additional functions, such as handholds and/or fixation means. The frame element preferably is more rigid than the outer walls, thus imparting some stability to the container in the plane of the frame element. Two wall elements are fixed over the frame element, one on either side of the frame element. Between the wall elements, the cavity is thus formed. The wall elements may be fixed to the frame element by gluing or welding.

Alternatively the container may comprise more than one frame element, such as two, three or more frame elements. Preferably, if the container comprises more than one frame element, the frame elements are fixed one above the other, e.g. by welding or gluing. This additionally reinforces the stability of the container in the plane of the frame elements.

The frame elements preferably comprise or are made of the same material as the wall elements. Alternatively, the frame elements may comprise or be made of another material as the wall elements.

The container preferably additionally comprises an identification means, preferably an RFID tag. The identification means may enable to retrieve information about the coupling liquid in the container, such as e.g. batch serial number, production date, kit serial number or even last date of use.

[0038] Another objective is to provide a method of use of an ultrasound device with improved acoustic qualities.

In the method of use of an ultrasound device, preferably a HIFU device, a container filled with a coupling liquid comprising a preservative, preferably according to the present invention, is brought in fluid connection with the ultrasound transducer. The container may be brought in fluid connection via connection means, preferably comprised with the container. Preferably the container is brought in fluid connection with the ultrasound device by means of at least one tube, preferably a flexible tube.

[0039] This invention further relates to the use of a coupling liquid of the present invention for a treatment with ultrasound, preferably with high intensity focused ultrasound.

[0040] Another object of the present invention is to provide an ultrasound device comprising fixation means to reversibly connect a container of the present invention to the ultrasound device. The fixation means most preferably are in the form of an adaptor member which is connected to a container. Most preferably, the adaptor member is a separate device of the ultrasound device, which is insertable in a receptacle provided on the ultrasound device. Alternatively, the adaptor device may also be provided as unitary part of the ultrasound device.

The container filled with a coupling liquid is a container according to the present invention.

[0041] Additional aspects and details of the present invention will be apparent from the following description of figures and examples.

Fig. 1: Diagram showing the difference in speed of sound in a coupling liquid with alcohol compared to a coupling liquid without alcohol;

Fig. 2: An exploded view of an embodiment of a coupling liquid container according to the present invention;

Fig. 3: The coupling liquid container of Fig. 2 viewed from different sides;

Fig. 4: Schematic representation of a preferred method of manufacturing of a coupling liquid according to the present invention;

Fig. 5: Fixation means for fixing a container of the present invention to an ultrasound device;

Fig. 6: An ultrasound device comprising connection and cooling means for a container according to the present invention.

[0042] Figure 1 shows the difference in the speed of sound at various temperatures between a coupling liquid comprising 10% w/v of polyvinylpyrrolidone in water, shown as line B, compared to a coupling liquid additionally comprising 5% by weight of ethanol, shown as line A. As can readily be seen, the addition of alcohol increases the speed of sound in the coupling medium.

[0043] Additionally, the reflection coefficient of the ultrasound waves between the liquid and the skin or cover member decreases, thus allowing increased transmission of the sound waves from the liquid into the tissues of a patient. Exemplary values for different physical characteristics of a coupling liquid of the present invention compared to a coupling liquid without alcohol and with plain water are shown in table 1:

Table 1

	Water	Coupling liquid	Coupling liquid with 5% ethanol
Density ρ [g/cm ³]	1	1.006	0.9935
Impedance Z [MRay]	1,457	1,465	1,482
Reflection coefficient R of sound on cover member made of silicon	12*10 ⁻⁴	9,85*10 ⁻⁴	6,64*10 ⁻⁴

[0044] The development of bacterial contamination was tested both for a coupling medium comprising 10% weight by volume polyvinylpyrrolidone in water as well as a coupling liquid additionally comprising 5% by weight of ethanol. Further, a coupling liquid comprising alcohol was inoculated with a bacterial culture of *Pseudomonas aeruginosa* at 80 CFU/100mL. The coupling liquid probes were filled in a pouch container excluding any air and the pouches were stored for 5 months at room temperature. Samples of the liquid were taken and incubated for 3 days at 22°C ± 2°C. After this time, bacterial contamination was determined. The results are shown on table 2:

Table 2

Container	Ethanol	Innoculation	Contamination after 1,5 mts	Contamination after 5 mts
1	-	-	overgrown	500000 UFC/mL
2	-	-	overgrown	740000 UFC/mL
3	-	-	overgrown	570000 UFC/mL
A	5%	-	1 CFU/100mL	0 CFU/100mL
B	5%	-	0 CFU/100mL	0 CFU/100mL
C	5%	-	0 CFU/100mL	0 CFU/100mL
D	5%	80 CFU/100 mL	34 CFU/100 mL	0 CFU/100mL
E	5%	80 CFU/100 mL	40 CFU/100 mL	0 CFU/100mL
F	5%	80 CFU/100 mL	58 CFU/100 mL	0 CFU/100mL

[0045] As can be seen, addition of an alcohol with a carbon chain of 1 to 7 carbon atoms, in this case ethanol, hinders bacterial growth in a coupling liquid. Even if the coupling liquid was not manufactured under aseptic conditions and therefore contains low levels of bacterial contamination, overgrowing of the liquid by bacteria can be avoided by addition of ethanol.

[0046] In a test, the focal point of an imaging transducer was shifted from 11mm to 13.7mm from the tip of the probe using a coupling liquid with 5% ethanol.

[0047] Figure 2 shows an exemplary embodiment of a container of the present invention in exploded view. The container 10 comprises a first frame element 1 and a second frame element 2. In this embodiment, the frame elements 1,2 are generally of rectangular shape. On both sides of the frame elements 1,2 two wall elements 3,4 are affixed. Preferably, the frame elements 1,2 provide passages 11 for the insertion of tubes 5,6 into the cavity formed between the two walls 3,4. Identification means 7, exemplarily shown as RFID chip, may be inserted between the two frame elements 1,2. Between the walls 12 a cavity is formed.

[0048] Figure 3a shows a top view of an assembled container 10. Both wall elements 3,4 are fixed on the frame elements 1,2. This creates a border 8 at the edges of the wall elements 3,4. Wall elements 3,4 may be affixed to frame elements 1,2 by means of gluing or plastic welding. Frame elements 1,2 are also fixed together by means of gluing or plastic welding. Between the wall elements 3,4 cavity 9 is formed. Tubes 5,6 are inserted into cavity 9 through passages 11. By means of the tubes 5,6 the container 10 may be connected to an ultrasound device or to a liquid circuit of an ultrasound device.

[0049] Figures 3b and 3c are side and front views, respectively, of the assembled container 10 as shown on figure 3a. Both wall elements 3,4 have a height H_w . The overall height H of the container 10 is the sum of the height H_w of the two wall elements 3,4 and the thickness of both frame elements 1,2. The height H_w of the wall elements 3,4 is a maximal height. If the walls 12 are flexible and the cavity 9 is not completely filled, then the walls 12 may not extend to their full height H_w .

[0050] Both the frame elements 1,2 and the wall elements 3,4 are made of a polymeric material, preferably poly(vinyl chloride). Alternative embodiments may also provide for a container where the frame elements 1,2 comprise or are made of another material than the wall elements 3,4.

[0051] The thickness of the wall elements 3,4 and hence of the walls 12 preferably is 0.1mm. The frame elements 1,2 are preferably thicker than the wall elements 3,4. Preferably, thickness of the frame elements 1,2 is between 0.1mm and 1.5mm, more preferably between 0.2mm and 1mm. Most preferably, the frame elements 1,2 are 0.25mm thick.

[0052] The cavity 9 preferably has a width W_c in the range of 90mm to 150mm, more preferably of 100mm to 125mm. Most preferably width W_c is 110mm. The length L_c of cavity 9 is in the range of 180mm to 250mm, more preferably of 200mm to 225mm. Most preferably, the length L_c is 210mm.

[0053] The width of the container W is preferably in the range of 120mm to 180mm, more preferably of 140mm to 160mm. Most preferably width W is 150mm. The length of the container L preferably is in the range of 250mm to 350mm, more preferably of 280mm to 320mm. Most preferably, length L is 295mm.

[0054] Height H_w of the wall elements 3,4 preferably is in the range of 5mm to 20mm, more preferably of between 10mm to 15mm, most preferably height H_w is 12mm.

[0055] The height H of the container 10 when filled is preferably in the range of 12mm to 50mm, more preferably of between 20mm and 35mm, most preferably the height H of container 10 is 22mm.

[0056] The total volume of the cavity 9 of container 10 most preferably is 500mL.

[0057] Figure 4 shows a preferred method of manufacturing of a coupling liquid according to the present invention. In a first mixing step 19, an alcohol 15 is added to a powder of a hydrophilic polymer 16. Preferably, alcohol 15 is ethanol and polymer 16 is polyvinylpyrrolidone. The amount used may vary depending on the wanted characteristics of the coupling liquid. Preferably, 10 grams of a polyvinylpyrrolidone, preferably with an average molecular weight of about 58,000, e.g. as available under the name PLASDONE K29-32 (ISP Corp.), are dissolved in 50 grams of ethanol in the first mixing step 19. This solution is then mixed with water, preferably purified or distilled water in a second mixing step 20. The amount of water should be chosen such as to yield 1 litre of coupling liquid 18. Alternatively, additional compounds may be added to the coupling liquid 18 during any of the manufacturing steps, e.g. in first mixing step 19. Exemplarily, 1ml of a 0.2% solution of a dye, preferably methylene blue, may be added. Depending on the desired characteristics of the coupling liquid 18, any suitable compound may be additionally added to the coupling liquid 18.

[0058] Figures 5a and 5b exemplarily show fixation means to fix a container 10 to an ultrasound device. The fixation means preferably are in the form of an adaptor element 20 having a base member 22 and a lid member 21 which is pivotably coupled to the base member 22. Figure 5a shows the adaptor member 20 in an open state. The base member 22 is configured such that a container 10 may be inserted between the outer walls of the member. For ease of handling, the adaptor member 20 may further comprise a handle 24. Additionally, the base member 22 comprises at least one fixation means 23 to reversibly secure lid member 21 to base member 22 in a closed state. Such a closed state is shown in figure 5b. By pivoting lid member 21 back onto the base member 22, the container 10 is securely connected in the adaptor member 20, preferably through clamping of the border 8 of the container 10 between the lid member 21 and the base member 22. The lid member 21 is secured to the base member 22 by means of fixation means 23. The fixation means 23 may be of any suitable form and configuration, such as screws, pins or a form fit connection. Both the base member 22 and the lid member 21 are configured in such a way as to allow connection means, here shown as tubes 5,6, to be freely connected e.g. to a probe head.

[0059] Figure 6 is a representation of an ultrasound device 25 comprising cooling and/or connection means for the container 10. In this example, the cooling means are provided within the ultrasound device 25. Adaptor member 20 with

a container 10 mounted therein is inserted in a receptacle 30 provided on the ultrasound device 25. The cooling means are arranged in such a way as to provide optimal cooling of the container 10 once inserted in the receptacle 30. The ultrasound device 25 preferably further comprises an ultrasound probe head 26, a pivot arm 27 as well as input/output means, such as screen 28. Most preferably, the ultrasound probe head is covered by a cover member 29. In a special embodiment, container 10 and cover member 29 are comprised in a kit. Cover member 29 and the container 10 may then be brought in fluid connection by means of tubes or the like. Further, the ultrasound device may comprise at least one pump to allow cycling of the coupling liquid between the container 10 and the cover member 29.

Claims

1. An ultrasound coupling liquid comprising:
 - a. a liquid aqueous solution of at least one hydrophilic polymer having an average molecular mass of between 30,000 and 70,000
 - b. at least one alcohol with a carbon chain of 1 to 7 carbon atoms to reduce the reflection of ultrasound waves at a boundary between the ultrasound coupling liquid and skin and/or a cover member covering an ultrasound transducer, wherein the at least one alcohol is present in a concentration of 3% to 45% by weight, preferably 5% to 20% by weight.
2. The ultrasound coupling liquid as claimed in claim 1, **characterized in that** the at least one alcohol is present in a concentration of 5% by weight.
3. The ultrasound coupling liquid as claimed in any of claims 1 to 2, **characterized in that** the at least one alcohol is selected from a group comprising ethanol, propanol isopropanol, benzyl alcohol.
4. The ultrasound coupling liquid as claimed in any of claims 1 to 3, **characterized in that** the hydrophilic polymer is or comprises polyvinylpyrrolidone.
5. The ultrasound coupling liquid as claimed in any of claims 1 to 4, **characterized in that** the hydrophilic polymer is present in an amount of between 1% and 5% w/v.
6. A container (10) with an outer wall (12) with a high thermal conductivity defining a cavity (9) filled with an ultrasound coupling liquid according to any of claims 1 to 5, **characterized in that** the container (10) is airtight.
7. The container according to claim 6, **characterized in that** the outer wall (12) has a thickness of less than 0.5mm, preferably less than 0.25mm, most preferably less than 0.125mm.
8. The container according to either of claim 6 or 7, **characterized in that** the outer wall (12) is made of or comprises a plastic material, preferably poly(vinyl chloride) and/or an elastomeric material.
9. The container according to any of claims 6 to 8, **characterized in that** the container (10) additionally comprises means to bring the cavity in fluid connection with an ultrasound probe head, said means preferably comprising at least one tube (5,6).
10. The container according to any of claims 6 to 9, **characterized in that** the container (10) comprises at least one frame element (1,2) defining the geometrical shape of the container in one plane and two wall elements (3,4) comprising the outer wall (12), wherein said two wall elements (3,4) are fixed over said frame element (1,2) thereby forming the cavity (9) in between said two wall elements (3,4).
11. The container according to any of claims 6 to 10, **characterized in that** said container (10) additionally comprises an identification means (7), preferably an RFID tag.
12. Ultrasound device (25) comprising cooling means and/or connection means, preferably in the form of an adaptor element (20), connected to a coupling liquid container (10) as claimed in any of claims 6 to 11.
13. Kit comprising a container (10) according to any of claims 6 to 11 and a cover member (29) for an ultrasound transducer, preferably comprising connection means to bring said cover member in fluid connection with said con-

tainer.

Patentansprüche

5

1. Ultraschallkopplungsflüssigkeit, umfassend:

10

- a. eine flüssige wässrige Lösung wenigstens eines hydrophilen Polymers mit einer mittleren Molekülmasse von zwischen 30.000 und 70.000,
- b. wenigstens einen Alkohol mit einer Kohlenstoffkette mit 1 bis 7 Kohlenstoffatomen zum Verringern der Reflexion von Ultraschallwellen an einer Grenze zwischen der Ultraschallkopplungsflüssigkeit und Haut und/oder einem Abdeckelement, das einen Ultraschallwandler abdeckt,

15

wobei der wenigstens eine Alkohol in einer Konzentration von 3 Gew.-% bis 45 Gew.-%, vorzugsweise 5 Gew.-% bis 20 Gew.-%, vorhanden ist.

2. Ultraschallkopplungsflüssigkeit gemäß Anspruch 1, **dadurch gekennzeichnet, dass** der wenigstens eine Alkohol in einer Konzentration von 5 Gew.-% vorhanden ist.

20

3. Ultraschallkopplungsflüssigkeit gemäß einem der Ansprüche 1 bis 2, **dadurch gekennzeichnet, dass** der wenigstens eine Alkohol ausgewählt ist aus einer Gruppe umfassend Ethanol, Propanol, Isopropanol, Benzylalkohol.

25

4. Ultraschallkopplungsflüssigkeit gemäß einem der Ansprüche 1 bis 3, **dadurch gekennzeichnet, dass** das hydrophile Polymer Polyvinylpyrrolidon ist oder umfasst.

5. Ultraschallkopplungsflüssigkeit gemäß einem der Ansprüche 1 bis 4, **dadurch gekennzeichnet, dass** das hydrophile Polymer in einer Menge von zwischen 1 % und 5 % w/v vorhanden ist.

30

6. Behälter (10) mit einer Außenwand (12) mit einer hohen Wärmeleitfähigkeit, die einen Hohlraum (9) definiert, der mit einer Ultraschallkopplungsflüssigkeit gemäß einem der Ansprüche 1 bis 5 gefüllt ist, **dadurch gekennzeichnet, dass** der Behälter (10) luftdicht ist.

35

7. Behälter gemäß Anspruch 6, **dadurch gekennzeichnet, dass** die Außenwand (12) eine Dicke von weniger als 0,5 mm aufweist, vorzugsweise weniger als 0,25 mm, höchst bevorzugt weniger als 0,125 mm.

8. Behälter gemäß einem von Anspruch 6 oder 7, **dadurch gekennzeichnet, dass** die Außenwand (12) aus einem Kunststoffmaterial, vorzugsweise Poly(vinylchlorid), und/oder einem Elastomermaterial besteht oder es umfasst.

40

9. Behälter gemäß einem der Ansprüche 6 bis 8, **dadurch gekennzeichnet, dass** der Behälter (10) zusätzlich Einrichtungen umfasst, um den Hohlraum in Fluidverbindung mit einem Ultraschall-Sondenkopf zu bringen, wobei die Einrichtungen vorzugsweise wenigstens ein Rohr (5, 6) umfassen.

45

10. Behälter gemäß einem der Ansprüche 6 bis 9, **dadurch gekennzeichnet, dass** der Behälter (10) wenigstens ein Rahmenelement (1, 2) umfasst, das die geometrische Form des Behälters in einer Ebene definiert, und zwei Wandelemente (3, 4), die die Außenwand (12) umfassen, wobei die beiden Wandelemente (3, 4) über dem Rahmenelement (1, 2) befestigt sind und dadurch den Hohlraum (9) zwischen den beiden Wandelementen (3, 4) bilden.

50

11. Behälter gemäß einem der Ansprüche 6 bis 10, **dadurch gekennzeichnet, dass** der Behälter (10) zusätzlich eine Identifikationseinrichtung (7), vorzugsweise ein RFID-Tag, umfasst.

12. Ultraschallvorrichtung (25), umfassend Kühleinrichtungen und/oder Verbindungseinrichtungen, vorzugsweise in der Form eines Adapterelements (20), verbunden mit einem Kopplungsflüssigkeitsbehälter (10) gemäß einem der Ansprüche 6 bis 11.

55

13. Kit, umfassend einen Behälter (10) gemäß einem der Ansprüche 6 bis 11 und ein Abdeckelement (29) für einen Ultraschallwandler, vorzugsweise umfassend Verbindungseinrichtungen, um das Abdeckelement in Fluidverbindung mit dem Behälter zu bringen.

Revendications

1. Liquide de couplage d'ultrasons comprenant :
- 5 a. une solution aqueuse liquide d'au moins un polymère hydrophile ayant une masse moléculaire moyenne comprise entre 30 000 et 70 000
b. au moins un alcool avec une chaîne de carbone de 1 à 7 atomes de carbone pour réduire la réflexion d'ondes ultrasonores à une limite entre le liquide de couplage d'ultrasons et la peau et/ou un élément de couverture recouvrant un transducteur d'ultrasons,
- 10 dans lequel l'au moins un alcool est présent à une concentration de 3 % à 45 % en poids, de préférence 5 % à 20 % en poids.
2. Liquide de couplage d'ultrasons selon la revendication 1, **caractérisé en ce que** l'au moins un alcool est présent à une concentration de 5 % en poids.
3. Liquide de couplage d'ultrasons selon l'une quelconque des revendications 1 à 2, **caractérisé en ce que** l'au moins un alcool est choisi dans un groupe comprenant l'éthanol, le propanol, l'isopropanol, l'alcool benzylique.
- 20 4. Liquide de couplage d'ultrasons selon l'une quelconque des revendications 1 à 3, **caractérisé en ce que** le polymère hydrophile est ou comprend de la polyvinylpyrrolidone.
5. Liquide de couplage d'ultrasons selon l'une quelconque des revendications 1 à 4, **caractérisé en ce que** le polymère hydrophile est présent dans une quantité comprise entre 1 % et 5 % p/v.
- 25 6. Récipient (10) comportant une paroi externe (12) ayant une conductivité thermique élevée définissant une cavité (9) remplie d'un liquide de couplage d'ultrasons selon l'une quelconque des revendications 1 à 5, **caractérisé en ce que** le récipient (10) est étanche à l'air.
- 30 7. Récipient selon la revendication 6, **caractérisé en ce que** la paroi externe (12) a une épaisseur inférieure à 0,5 mm, de préférence inférieure à 0,25 mm, de manière préférée entre toutes inférieure à 0,125 mm.
8. Récipient selon la revendication 6 ou 7, **caractérisé en ce que** la paroi externe (12) est constituée de ou comprend une matière plastique, de préférence le poly(chlorure de vinyle) et/ou un matériau élastomère.
- 35 9. Récipient selon l'une quelconque des revendications 6 à 8, **caractérisé en ce que** le récipient (10) comprend en outre des moyens pour placer la cavité en raccordement fluïdique avec une tête de sonde à ultrasons, lesdits moyens comprenant de préférence au moins un tube (5,6).
- 40 10. Récipient selon l'une quelconque des revendications 6 à 9, **caractérisé en ce que** le récipient (10) comprend au moins un élément de cadre (1,2) définissant la forme géométrique du récipient dans un plan et deux éléments de paroi (3,4) comprenant la paroi externe (12), lesdits deux éléments de paroi (3,4) étant fixes, sur ledit élément de cadre (1,2) de manière à former la cavité (9) entre lesdits deux éléments de paroi (3,4).
- 45 11. Récipient selon l'une quelconque des revendications 6 à 10, **caractérisé en ce que** ledit récipient (10) comprend en outre un moyen d'identification (7), de préférence une étiquette RFID.
12. Dispositif à ultrasons (25) comprenant des moyens de refroidissement et/ou des moyens de connexion, de préférence sous la forme d'un élément d'adaptateur (20), reliés à un récipient de liquide de couplage (10) selon l'une quelconque des revendications 6 à 11.
- 50 13. Kit comprenant un récipient (10) selon l'une quelconque des revendications 6 à 11 et un élément de couverture (29) pour un transducteur à ultrasons, comprenant de préférence des moyens de connexion pour placer ledit élément de couverture en raccordement fluïdique avec ledit récipient.
- 55

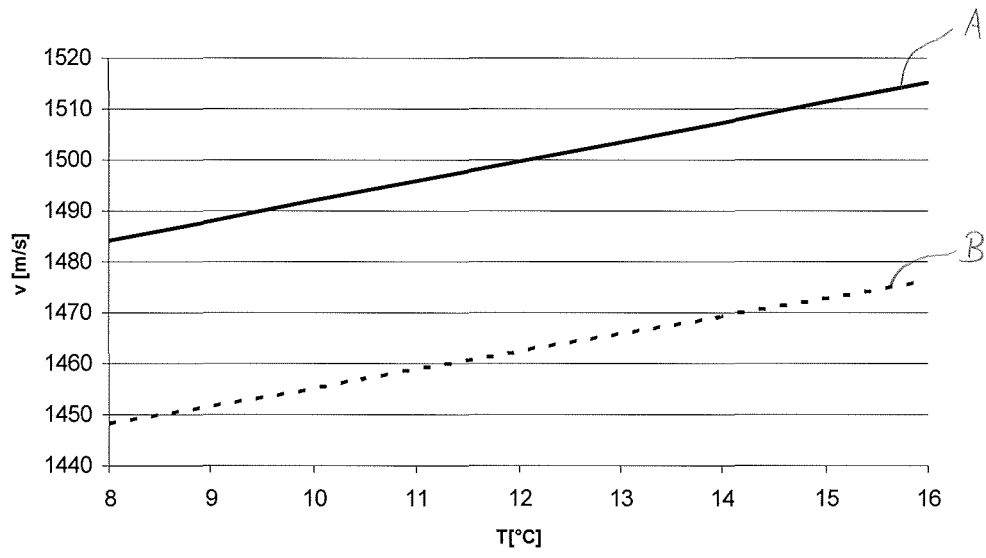


Fig. 1

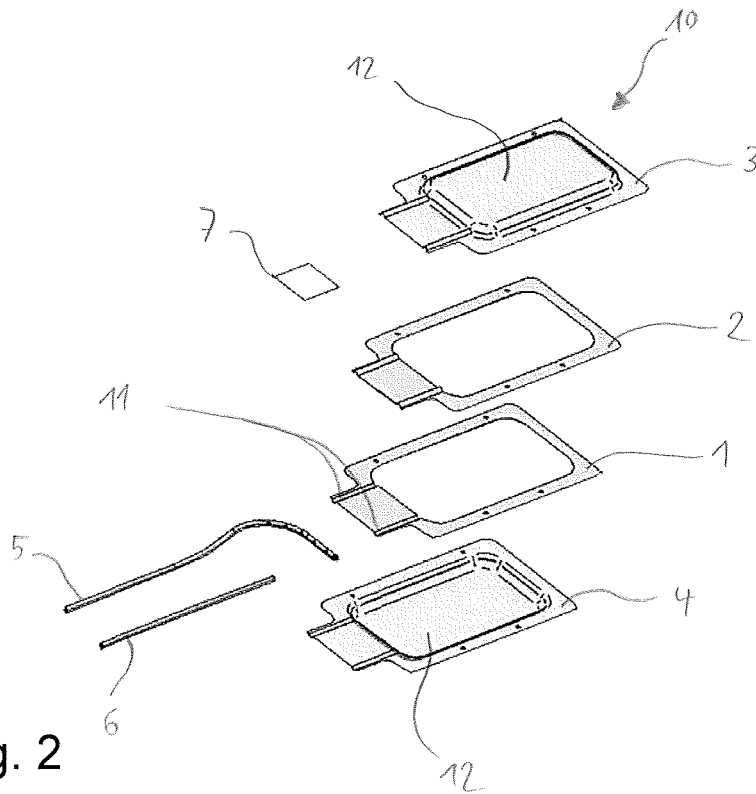


Fig. 2

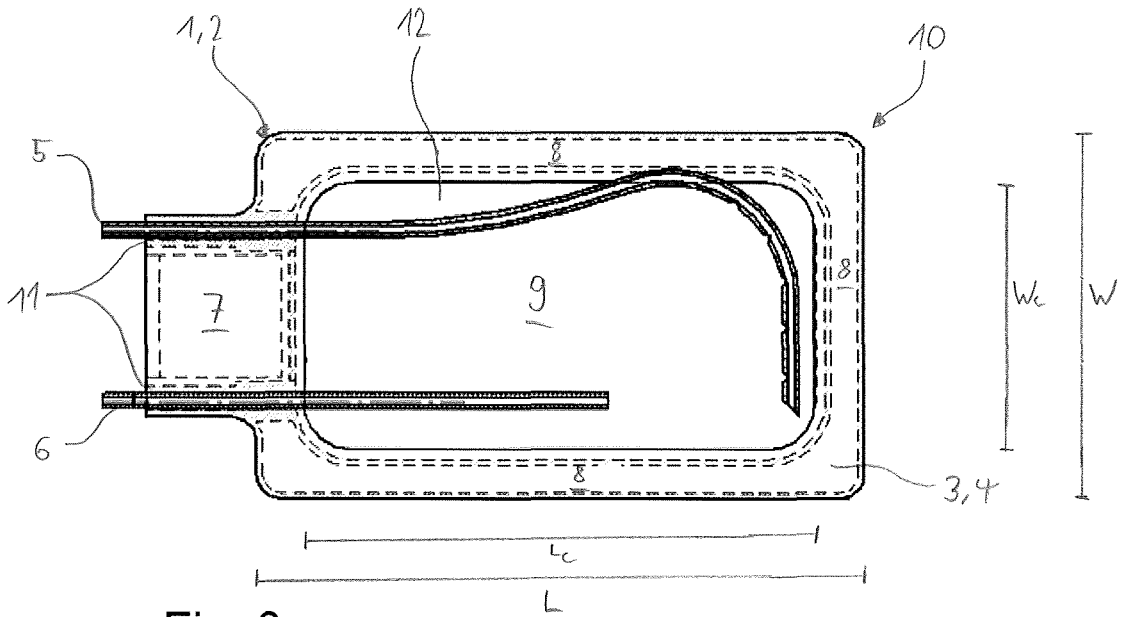


Fig. 3a

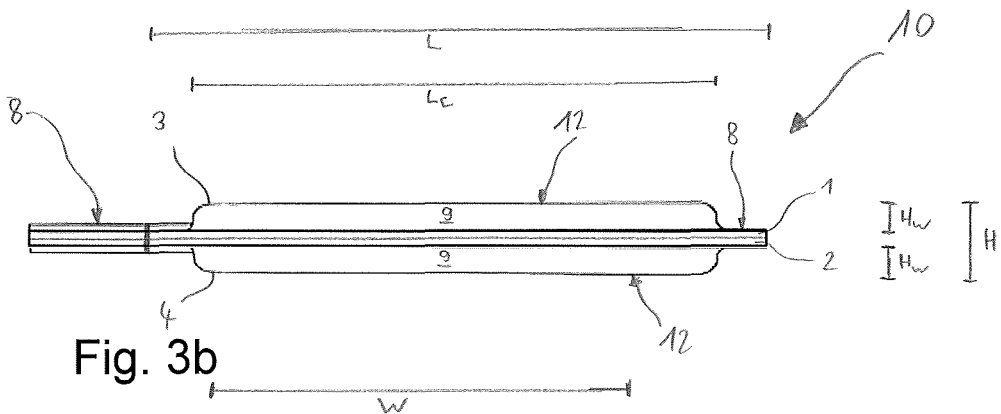


Fig. 3b

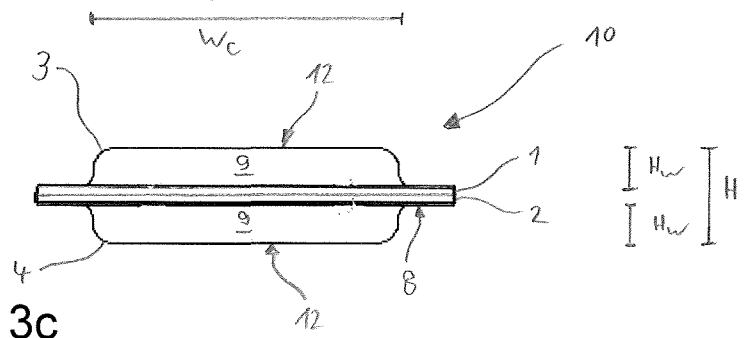


Fig. 3c

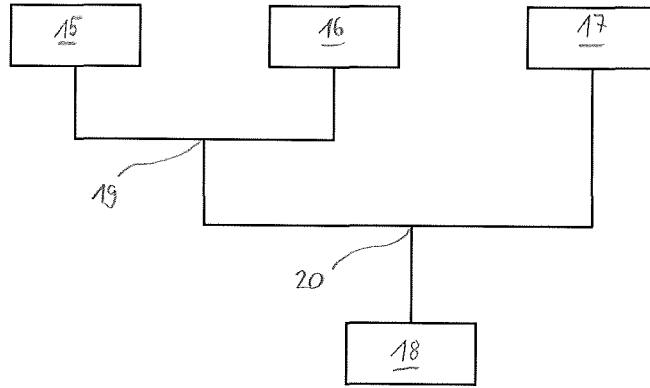


Fig. 4

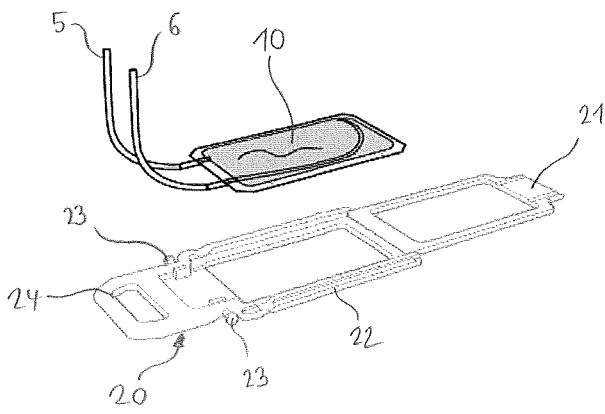


Fig. 5a

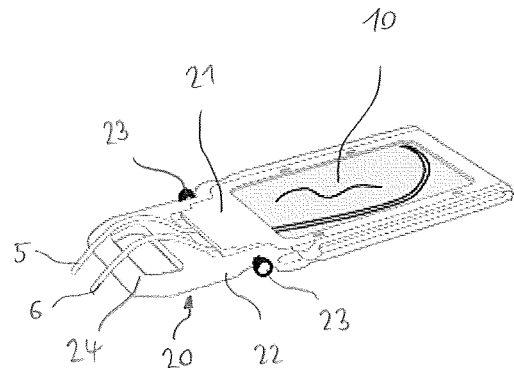


Fig. 5b

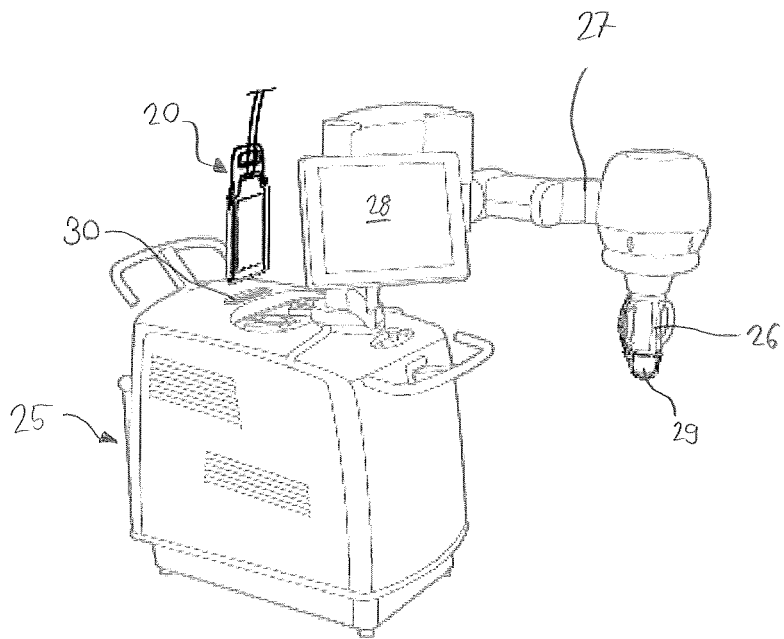


Fig. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- JP 2092343 A [0006]
- US 5078149 A [0007]
- US 6432069 B [0009]
- US 4886068 A [0010]

专利名称(译)	超声波耦合液体和容器		
公开(公告)号	EP2575624B1	公开(公告)日	2017-04-26
申请号	EP2011719285	申请日	2011-05-16
[标]申请(专利权)人(译)	泰拉克利昂公司		
申请(专利权)人(译)	THERACLION SAS		
当前申请(专利权)人(译)	THERACLION SA		
[标]发明人	BROCARDO ROBERTA PECHOUX THIERRY		
发明人	BROCARDO, ROBERTA PECHOUX, THIERRY		
IPC分类号	A61B8/00		
CPC分类号	A61L31/048 A61B8/4281 A61B8/546 A61J1/00 A61J1/1475 A61N7/02 B65D1/00		
优先权	2010163725 2010-05-25 EP		
其他公开文献	EP2575624A1		
外部链接	Espacenet		

摘要(译)

本发明涉及一种用于超声装置的耦合液，优选高强度聚焦超声（HIFU）。偶联液包含至少一种平均分子量为30,000至70,000的亲水性聚合物和至少一种碳链为1至7个碳的醇的液体水溶液。还公开了一种用于具有薄壁的超声耦合液体的容器（10）。

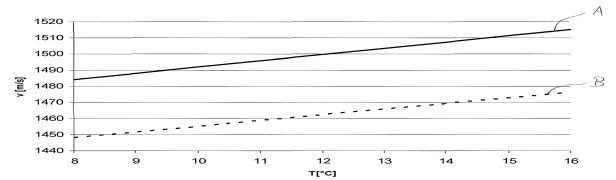


Fig. 1

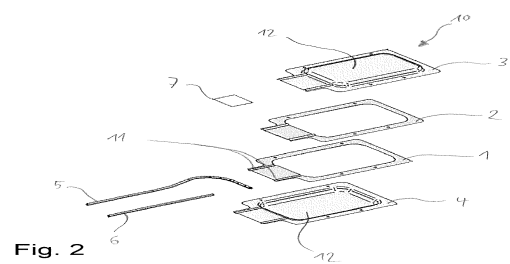


Fig. 2