

(19)



(11)

**EP 2 575 966 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**16.12.2015 Bulletin 2015/51**

(51) Int Cl.:  
**A61N 7/00 (2006.01) G01N 29/34 (2006.01)**  
**A61B 8/00 (2006.01)**

(21) Application number: **11727791.3**

(86) International application number:  
**PCT/IB2011/052255**

(22) Date of filing: **24.05.2011**

(87) International publication number:  
**WO 2011/148314 (01.12.2011 Gazette 2011/48)**

(54) **ULTRASOUND TRANSDUCER FOR SELECTIVELY GENERATING ULTRASOUND WAVES AND HEAT**

ULTRASCHALLWANDLER ZUR SELEKTIVEN ERZEUGUNG VON ULTRASCHALLWELLEN UND WÄRME

TRANSDUCTEUR À ULTRASONNS POUR LA GÉNÉRATION SÉLECTIVE D'ONDES ULTRASONORES ET DE CHALEUR

(84) Designated Contracting States:  
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR**

(74) Representative: **Kroeze, Johannes Antonius Philips**  
**Intellectual Property & Standards**  
**P.O. Box 220**  
**5600 AE Eindhoven (NL)**

(30) Priority: **27.05.2010 EP 10164111**

(43) Date of publication of application:  
**10.04.2013 Bulletin 2013/15**

(56) References cited:  
**WO-A1-2011/071703 WO-A1-2011/075227**  
**WO-A1-2011/092683 WO-A1-2011/128693**  
**WO-A2-2008/070580 WO-A2-2009/095894**  
**US-A- 5 522 869 US-A- 5 601 526**  
**US-A1- 2004 082 857 US-A1- 2006 084 891**  
**US-A1- 2006 206 105 US-A1- 2006 253 026**  
**US-B1- 6 334 846**

(73) Proprietor: **Koninklijke Philips N.V.**  
**5656 AE Eindhoven (NL)**

(72) Inventors:  
• **VAN HEESCH, Christianus Martinus**  
**5656 AE Eindhoven (NL)**  
• **KOLESNYCHENKO, Aleksey**  
**5656 AE Eindhoven (NL)**

**EP 2 575 966 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

**Description**

## FIELD OF THE INVENTION

**[0001]** The invention relates to the field of ultrasound transducers, and in particular to ultrasound transducers for selectively generating ultrasound waves and heat for use in analysis and/or diagnostics.

## BACKGROUND OF THE INVENTION

**[0002]** Since long, ultrasound is used in the field of medical treatment. Recently, ultrasonic transducers, in particular high intensity focused ultrasound transducers, have been used for inducing lesions in tissue for therapeutic cancer treatment. Tissue lesion or tissue destruction is caused by cavitation effects of high intensity ultrasonic waves. This cavitation effect is linked to the formation of microscopic vapor bubbles in a region, where the pressure of liquid falls below its vapor pressure. When these bubbles collapse, energy is released leading to the destruction of neighboring tissue.

**[0003]** US 5,601,526 describes a method and an apparatus for performing therapy using ultrasound for tissue disruption by means of cavitation and thermal effects. This document is concerned with providing a solution allowing a lesion in tissue to be treated, which is strictly limited to the focus point of the treatment device, and limiting or avoiding effects due to heat spreading around the focus point, with cavitation phenomena being limited exclusively to the focal point or to the focal region. For this, two types of ultrasonic waves are employed, one producing predominantly a thermal effect on the tissue, the other producing predominantly a cavitation effect on the tissue. Here, heating in the tissue occurs due to absorption of ultrasonic energy by frictional damping.

**[0004]** WO 2009/095894 A2 discloses an apparatus and a method for treating adipose tissue located beneath a patient's skin. The apparatus includes a single sonotrode and an ultrasound transducer operative to induce longitudinal and/or transversal ultrasound vibrations in at least a portion of the sonotrode. The apparatus provides a "cold" or "transverse" mode where ultrasound energy delivered to the patient is primarily energy of transverse ultrasound waves, and a "hot" or "longitudinal" mode where ultrasound energy delivered to the patient is primarily energy of longitudinal ultrasound waves. The longitudinal waves may be useful for 'pre-heating' tissue of the patient before delivering the transverse waves.

**[0005]** Also in analysis and diagnostics, ultrasound is more and more employed. For instance, the detection of infectious pathogens for prevention, early diagnosis and treatment of infectious diseases are based on the analysis of intracellular components, e.g. nucleic acids or specific molecules, of viruses or cells in a sample. Thus, one of the processing steps before analyzing the components is cell-lysis (cell breaking). Cell-lysis can be induced by means of high intensity focused ultrasound

waves that generate cavitations in the sample. Upon implosion of these cavitations, enough energy is released to destroy the membranes of bacteria, viruses and cells and release their intracellular components.

**[0006]** Moreover, working with cells or small organisms involves a thorough control of environmental conditions, such as temperature. Temperature has wide influence, for instance, on the metabolism and the reproduction cycle of bacteria and cells. Hence, for most biological applications, temperature control is required. Yet, the space for adding more components to an experimental setup, such as heating means, is extremely limited, and in particular, since the trend is to minimize the sample volume for saving material costs and for accelerating the procedures. Therefore, a compact setup design is desirable.

**[0007]** However, when heating is performed due to ultrasonic energy absorption of a high intensity focused ultrasonic beam, the sample may be unintentionally influenced or sensitive components in a sample, such as membranes, may be damaged by local pressure and/or temperature peaks in the sample. In particular, it may be required to heat the sample before ultrasonic treatment without exposing the sample to acoustic pressure waves in order to get neat results. Thus, in diagnostics and analysis, it is often required to heat a sample without potentially manipulating or damaging it. Therefore, ways for gently heating a sample in a controlled way have to be found, being at the same time cost saving, space saving, easy to control and sufficiently fast.

## SUMMARY OF THE INVENTION

**[0008]** Hence, it is an object of the invention to provide heating means for an ultrasonic application setup, capable of heating a sample gently and fast and being cost and space saving.

**[0009]** The object is solved by the features of the independent claims. The basic idea of the invention is based on the finding that an ultrasound transducer can be driven at several drive frequencies, whereof usually only the lowest one efficiently generates ultrasonic waves. At other frequencies, almost no ultrasonic intensity is emitted; instead the transducer itself heats up. Therefore, it is proposed to use an ultrasound transducer for selectively providing ultrasound and heat to a sample. For this, an ultrasound transducer is used that can be operated at different frequencies. For ultrasound application, the ultrasound transducer is operated at a main frequency, at which ultrasonic waves are generated very efficiently. For heating, the ultrasound transducer is operated at an alternative frequency, at which the transducer heats up.

**[0010]** Preferably, the main and alternative frequencies are resonance frequencies of the ultrasound transducer or close to those. The frequency, at which ultrasonic waves are most efficiently generated, is the main resonance frequency, while at other resonance frequencies; much less ultrasonic energy is emitted. Using res-

onance frequencies as driving frequencies, the supplied electrical energy is most efficiently transformed by the ultrasound transducer. However, it may not always be advantageous to use the exact resonance frequency, but rather a frequency close to it. The frequency, at which the ultrasound transducer is driven, may be adjustable by means of a control unit. It is then preferable that a user interface is provided, so that a user can select certain frequencies and adjust also other experimental parameters, e.g. intensity of emitted ultrasound, set-point temperature or heating rate.

**[0011]** In one exemplary embodiment, the main frequency for generating ultrasonic waves is lower than at least one of the alternative frequencies used for heating. In particular, the main frequency may be the lowest resonance frequency of the ultrasound transducer. It is preferred that high intensity ultrasonic waves can be generated at the main frequency. In one embodiment, these high intensity ultrasonic waves are capable of creating cavitations in a sample or in a liquid medium. By means of cavitations, lysis of cells, bacteria, virus capsules or membrane compartments may be induced. Preferably, the ultrasound transducer only generates ultrasound waves of sufficiently high intensity, when it is driven at the main frequency. Alternatively, the main frequency may represent the frequency, at which the highest intensity of ultrasonic waves is generated. In another example, the ultrasound intensity emitted at at least one of the alternative frequencies is much lower than the ultrasound intensity emitted at the main frequency. By these means, the alternative frequency can be used for heating without employing stress by acoustic pressure waves.

**[0012]** In one embodiment, at least one of the alternative frequencies is more efficient with respect to heating than the main frequency. Heat may be produced in the ultrasound transducer due to electric power absorption of the ultrasound transducer at one or more of the alternative resonance frequencies. Preferably, driving the ultrasound transducer at one of the alternative frequencies can be adjusted for heating such that either no ultrasonic waves are generated at all or at least none capable of creating cavitation effects. The heating characteristics, e.g. rate of temperature increase or maximum temperature, may vary among the alternative frequencies of the ultrasound transducer. Therefore, preferably, an appropriate alternative frequency can be selected by a user among the plurality of alternative frequencies, e.g. depending on the maximum temperature to be reached or on the desired rate of temperature increase. The heating characteristics of the alternative frequencies may be stored in some storing means and may be indicated to the user.

**[0013]** In a further embodiment, the ultrasound transducer is capable of being driven simultaneously at at least two frequencies or is capable of switching continuously between frequencies. Thus, the ultrasound transducer may be driven at the main as well as at one of the alternative frequencies, so that the sample may be heated,

while high intensity ultrasonic waves are induced. Therefore, it is preferred that the main frequency and at least one of the alternative frequencies suitable for heating are drivable independently from each other. This is to say that all parameters of driving the ultrasound transducer, e.g. intensity, period, interval, amplitude, coordinates of focus point etc., can be adjusted for each frequency separately. Possibly, this can be realized by using an ultrasound transducer having several separate piezoelectric elements or the like.

**[0014]** In another embodiment of the invention, a system for sample analysis is proposed. The system comprises at least one sample holder and at least one ultrasound transducer, wherein the ultrasound transducer corresponds to any of the above-mentioned embodiments. The ultrasound transducer is adapted to be heat-conductively coupled to a sample inserted in the sample holder. The system further comprises a control unit for controlling the ultrasound transducer. The control unit is adapted to control the ultrasound transducer at the main frequency for generating ultrasound waves that are to be coupled into the sample, and at one of the alternative frequencies for generating heat in the ultrasound transducer due to electric power absorption of the ultrasound transducer, wherein the heat is to be used for heating the sample due to conduction of heat generated in the ultrasound transducer. The sample analysis may include DNA diagnostics, detection of infectious pathogens and/or diagnosis and treatment of infectious diseases. For this, the system may comprise all conventional components for performing these tasks, for instance a microcontroller or computer, display means, analysis means, a control unit, a microscope and so on. Preferably, the inventive system maybe incorporated in an existing set-up, e.g. in a lab-on-a-chip system.

**[0015]** In a preferred embodiment, the system also comprises temperature control and/or temperature sensing means. Instead of temperature sensing means, however, also an ultrasound transducer maybe used that is capable of measuring the sample temperature based on sound velocity measurements. It may moreover be useful to employ a feedback cycle for the temperature control. In addition, the sample holder is preferably designed such that it is able to provide good heat conduction between the ultrasound transducer and the sample. In this regard, also heat conductive paste or the like may be employed. At the same time, of course, good acoustic coupling should be provided. By these means, it can be ensured, that the generated ultrasonic waves as well as the generated heat can be coupled into the sample without considerable loss.

**[0016]** In a further embodiment of the invention, a method for sample analysis is proposed. This method comprises the steps of controlling an ultrasound transducer at a main frequency for efficiently generating ultrasonic waves and/or at one of at least one alternative frequency for heating a sample. Preferably, this method is used for operating an ultrasound transducer according

to one of the above-described embodiments. The ultrasound transducer is adapted to be heat-conductively coupled to a sample. The ultrasound transducer is operated at the main frequency for generating ultrasound waves that are to be coupled into the sample, and at one of the alternative frequencies for generating heat in the ultrasound transducer due to electric power absorption of the ultrasound transducer, wherein the heat is used for heating the sample due to conduction of heat generated in the ultrasound transducer. In one embodiment, almost no ultrasonic waves are produced, when driving the ultrasound transducer at at least one of the alternative frequencies. Moreover, heating should be performable simultaneously to ultrasound wave generation. Thus, it should be possible to drive the ultrasound transducer simultaneously at at least two different frequencies, i.e. at the main frequency and one alternative frequency. In addition, it is preferred that the temperature of the sample is controlled and/or monitored. Possibly, also a feedback cycle for controlling the temperature of the sample is realized.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0017]** These and other aspects of the invention will be apparent from and elucidated with reference to the embodiments described hereinafter and illustrated by the drawings.

- Fig. 1A shows an exemplary impedance spectrum of an exemplary ultrasound transducer;
- Fig. 1B displays the ultrasound intensity emitted by the ultrasound transducer in dependency on the driving frequencies; and
- Fig. 2 is a schematic view of a system for sample analysis according to the invention.

#### DETAILED DESCRIPTION OF EMBODIMENTS

**[0018]** For enabling heating as well as treating with ultrasound, an ultrasound transducer is used that can be driven at at least two different frequencies. One of these frequencies should be adapted for the efficient generation of ultrasonic waves, whereas the other frequency should result in heating up the ultrasound transducer, almost without generation of ultrasonic waves. Various types of ultrasonic transducers maybe employed, such as piezoelectric ultrasound transducers or capacitive micro-machined ultrasound transducers. Preferably, high intensity focused ultrasound transducers (HIFU-transducers) are employed that are able to focus the ultrasonic beam to a small focal region in a sample. It is also preferred to use resonance frequencies for driving the ultrasound transducer, in order to ensure a favorable transformation ratio of input electrical energy to output energy. However, in some cases, it may be preferable to use frequencies close to a resonance frequency, multitudes of a resonance frequency or the like. Hence, instead of

resonance frequencies, also other driving frequencies may be used.

**[0019]** Usually, an ultrasound transducer efficiently generates ultrasonic waves only at its main resonance frequency. At other alternative resonance frequencies, much less or almost no ultrasonic waves are generated. In fig. 1A, an exemplary impedance spectrum of an ultrasound transducer is shown. The ultrasound transducer has several resonance frequencies, e.g. the main resonance frequency centered at about 1.7 MHz, and alternative resonance frequencies centered at about 2.17 MHz and 2.86 MHz (arrows). The main resonance frequency is a fundamental vibration mode of a piezo-electric element of the ultrasound transducer. These alternative resonance frequencies can represent bending modes of the piezo-electric element or higher harmonics. At these frequencies, the ultrasound transducer heats up quickly.

**[0020]** Around 1.9 MHz, the impedance increases and fluctuates a lot, as shown in fig. 1A. This is due to the method of measuring the impedance and a result of electrical reflections and resonances. Due to the high impedance, a lot of electric signal is reflected back to the amplifier resulting in this kind of artifacts in the measurement.

**[0021]** At an impedance about 50 Ohm (dashed line), all electrical equipment works optimal with no electrical reflection. When the impedance of the ultrasound transducer is 50 Ohm (e.g. at 1.52 MHz), the ultrasound transducer does not heat up as fast as at resonance frequencies, 'proving' the heating is due to the resonance, not due to electric power. The main resonance frequency at 1.7 MHz is at 50 Ohm as well.

**[0022]** Furthermore, fig. 1B shows an exemplary relation of emitted ultrasound intensity and driving frequency of the ultrasound transducer. Thus, the ultrasound transducer predominantly emits ultrasound waves at its main resonance frequency, in this example at 1.7 MHz. At all other frequencies, much less ultrasonic intensity is emitted, but the absorbed electrical energy is merely transformed into heat in the ultrasound transducer.

**[0023]** According to the invention, the ultrasound transducer can be controlled to operate at an ultrasound generating main frequency and at a heat generating alternative frequency. Hence, the transducer may be selectively used to apply acoustic pressure waves to the sample or as a heating plate for heating the sample. Usually, the main frequency is lower than most of the alternative frequencies. If resonance frequencies are used, it may even be the lowest resonance frequency. At the main frequency, the ultrasound transducer should be capable to produce high intensity ultrasonic waves for creating cavitations, which induce bacteria or cell lysis in the sample. In contrast, the ultrasound intensity generated by driving the ultrasound transducer at one of the alternative frequencies should be much lower and preferably insufficient for inducing cavitation effects.

**[0024]** The parameters of the ultrasound transducer

may be adjustable. This may be performed by the user via a user interface or pre-programmed by a control unit. In particular, coordinates of a focus point, intensity, frequency, amplitude, etc. maybe adjusted. Furthermore, it may be selected to apply ultrasonic pulses, with adjustable pulse width, period and intervals. If the ultrasound transducer is drivable in more than one alternative frequency, the alternative frequencies may differ in their heating characteristics with respect to ultrasound generation, heating velocity and achievable maximum temperature. Therefore, the alternative frequencies should be selectable according to the requirements of different applications.

**[0025]** In a preferred embodiment, the ultrasound transducer can be driven at two different frequencies simultaneously and independently. Thus, heating and ultrasound generation can be performed at the same time. For instance, this can be achieved with a transducer comprising at least two ultrasound-generating elements, e.g. two piezoelectric elements. One of these elements may be operable at least at the main frequency and capable of generating ultrasound waves, while the other may be operable at one or more alternative frequencies for generating heat. Preferably, the elements are adjustable independently from each other.

**[0026]** In fig. 2, an example of a system for sample analysis is shown. The system comprises an ultrasound transducer 10 and a sample holder 30 for holding a sample 20. The sample holder 30 is adapted to receive a sample 20 comprised in a Petri dish, a test tube, a slide, or the like. The ultrasound transducer 10 is arranged such that ultrasonic waves as well as heat can efficiently be coupled into the sample 20. In order to improve ultrasonic or thermal conduction, heat conductive paste or ultrasound gel can be used.

**[0027]** In a preferred embodiment, the system further comprises a control unit 40 and a temperature sensor 50. The temperature sensor 50 can be any kind of temperature sensing means and is arranged close to or within the sample 20. In order to further reduce the size of the setup, the ultrasound transducer 10 may also be capable of measuring the sample temperature. For instance, this can be done by measuring the speed of sound in a liquid sample, since the speed of sound in a fluid strongly depends on the temperature of the fluid. The ultrasound transducer 10 may additionally be used for analyzing, e.g. for determining the density or consistency of the sample 20. Moreover, the system may be combined with a microscope 60 in order to image the sample 20 using fluorescence and/or reflected light microscopy.

**[0028]** Preferably, a sample 20 can be heated from 20°C room temperature to 95°C within less than two minutes. The heating process may be adjusted by controlling heating cycles at at least one selected alternative frequency, by adjusting intervals between heating cycles, a cycle period or the intensity. Possibly, the transducer 10 can be simultaneously driven at several alternative frequencies for heating, so that also the spectrum of driv-

ing frequencies can be adjusted. The heating process may be controlled by the control unit 40 based on data provided by the temperature sensor 50 for regulating the sample temperature in a kind of feedback cycle.

**[0029]** The system may additionally comprise a computer or microcontroller, display means, a memory for storing setup data or measurement data, user interfaces and the like. The system may also be integrated in a general analysis or diagnostic system, for example in a microscopic or other imaging setup, in a lab-on-a-chip system or in a microfluidic system.

**[0030]** By using an ultrasound transducer not only for generating ultrasound waves, but also for other functions, in particular for heating, the setup of an analysis/diagnosis system and the number of setup components may be reduced, thus reducing costs.

### Claims

1. A method for sample analysis employing an ultrasound transducer (10) that is adapted to be heat-conductively coupled to a sample (20), comprising:
  - controlling the ultrasound transducer (10) that is capable of being operated at at least two frequencies including a main frequency and at least one alternative frequency, wherein the ultrasound transducer (10) is operated at the main frequency for generating ultrasound waves that are to be coupled into the sample (20); and
  - at one of the alternative frequencies for generating heat in the ultrasound transducer (10) due to electric power absorption of the ultrasound transducer (10), wherein the heat is used for heating the sample (20) due to conduction of heat generated in the ultrasound transducer (10).
2. The method of claim 1, wherein the main frequency and the alternative frequency are resonance frequencies of the ultrasound transducer (10).
3. The method of claim 1 or 2, wherein when driving the ultrasound transducer (10) at at least one of the alternative frequencies, less ultrasound intensity is generated than when driving the ultrasound transducer (10) at the main frequency.
4. The method according to one of the preceding claims, wherein the ultrasound intensity generated when driving the ultrasound transducer (10) at at least one of the alternative frequencies is not sufficient for generating cavitations in the sample (20).
5. The method according to one of the preceding claims, wherein high intensity ultrasound waves gen-

erated at the main frequency are capable of creating cavitations in the sample (20).

6. The method according to one of the preceding claims, wherein at least one of the alternative frequencies is more efficient in producing heat than the main frequency. 5
7. The method according to one of the preceding claims, wherein at least one of the alternative frequencies adapted for heating is higher than the main frequency. 10
8. The method according to one of the preceding claims, wherein temperature of the sample (20) is monitored and/or controlled. 15
9. The method according to one of the preceding claims, wherein the ultrasound transducer (10) is capable of being operated simultaneously and/or alternating in the main frequency and in at least one of the alternative frequencies. 20
10. The method according to one of the preceding claims, wherein the sample (20) is inserted in a sample holder (30) and the ultrasound transducer (10) is adapted to be heat-conductively coupled to the sample (20) inserted in the sample holder (30). 25
11. A system for sample analysis, comprising: 30
  - at least one sample holder (30);
  - at least one ultrasound transducer (10) that is adapted to be heat-conductively coupled to a sample (20) inserted in the sample holder (30); and 35
  - a control unit (40) for controlling the ultrasound transducer (10) that is capable of being operated at at least two frequencies including a main frequency and at least one alternative frequency, wherein the control unit (40) is adapted to control the ultrasound transducer (10) 40
    - at the main frequency for generating ultrasound waves that are to be coupled into the sample (20); and
    - at one of the alternative frequencies for generating heat in the ultrasound transducer (10) due to electric power absorption of the ultrasound transducer (10), wherein the heat is to be used for heating the sample (20) due to conduction of heat generated in the ultrasound transducer (10). 45
12. The system of claim 11, wherein the ultrasound transducer (10) is capable of inducing bacteria and/or cell lysis in a sample (20), when driven at the main frequency, and of heating the sample (20) due to conduction of heat generated in the ultrasound 55

transducer (10), when driven at the alternative frequency.

13. The system of claim 11 or 12, wherein the ultrasound transducer (10) is capable of being driven simultaneously and/or alternating at at least two frequencies. 5
14. The system of claims 11-13, wherein the ultrasound transducer (10) comprises at least two elements, whereof one is operable at the main frequency for generating ultrasound waves and the other is operable at at least one of the alternative frequencies for generating heat in the ultrasound transducer (10). 10

### Patentansprüche

1. Ein Verfahren zur Probenanalyse, unter Verwendung eines Ultraschallwandlers (10), der als wärmeleitfähig gekoppelt an eine Probe (20) adaptiert ist, und Folgendes aufweist: 20

Steuerung des Ultraschallwandlers (10), der mit mindestens zwei Frequenzen betrieben werden kann, einschließlich einer Hauptfrequenz und mindestens einer Alternativfrequenz, wobei der Ultraschallwandler (10) mit der Hauptfrequenz zur Erzeugung von Ultraschallwellen, die in die Probe (20) einzukoppeln sind, betrieben wird; und mit einer der Alternativfrequenzen für die Erzeugung von Wärme im Ultraschallwandler (10), durch elektrische Energieaufnahme des Ultraschallwandlers (10), wobei die Wärme zum Erhitzen der Probe (20) durch die Leitung der im Ultraschallwandler (10) erzeugten Wärme verwendet wird, betrieben wird.

2. Verfahren nach Anspruch 1, wobei die Hauptfrequenz und die Alternativfrequenz Resonanzfrequenzen des Ultraschallwandlers (10) sind. 40
3. Verfahren nach Anspruch 1 oder 2, wobei beim Betrieb des Ultraschallwandlers (10) mit mindestens einer der Alternativfrequenzen, weniger Ultraschallintensität erzeugt wird, als beim Betrieb des Ultraschallwandlers (10) mit der Hauptfrequenz. 45
4. Verfahren nach einem der vorhergehenden Ansprüche, wobei die im Betrieb des Ultraschallwandlers (10) mit mindestens einer der Alternativfrequenzen erzeugte Ultraschallintensität für die Erzeugung von Kavitationen in der Probe (20) nicht ausreichend ist. 50
5. Verfahren nach einem der vorhergehenden Ansprüche, wobei die mit der Hauptfrequenz erzeugten hochintensiven Ultraschallwellen Kavitationen in der 55

Probe (20) erzeugen können.

6. Verfahren nach einem der vorhergehenden Ansprüche, wobei mindestens eine der Alternativfrequenzen effizienter in der Erzeugung von Wärme ist als die Hauptfrequenz.
7. Verfahren nach einem der vorhergehenden Ansprüche, wobei mindestens eine der Alternativfrequenzen, die für das Erhitzen adaptiert ist, höher ist als die Hauptfrequenz.
8. Verfahren nach einem der vorhergehenden Ansprüche, wobei die Temperatur der Probe (20) überwacht und/oder kontrolliert wird.
9. Verfahren nach einem der vorhergehenden Ansprüche, wobei der Ultraschallwandler (10) simultan und/oder alternierend mit der Hauptfrequenz und mit mindestens einer der Alternativfrequenzen betrieben werden kann.
10. Verfahren nach einem der vorhergehenden Ansprüche, wobei die Probe (20) in einen Probenhalter (30) gesetzt wird und der Ultraschallwandler (10) als wärmeleitfähig gekoppelt an die in den Probenhalter (30) gesetzte Probe (20) adaptiert ist.
11. Ein System zur Probenanalyse, das Folgendes umfasst:
- mindestens einen Probenhalter (30);  
 mindestens einen Ultraschallwandler (10), der als wärmeleitfähig gekoppelt an die in den Probenhalter (30) gesetzte Probe (20) adaptiert ist; und  
 eine Kontrolleinheit (40) zur Kontrolle des Ultraschallwandlers (10), der mit mindestens zwei Frequenzen betrieben werden kann, einschließlich einer Hauptfrequenz und mindestens einer Alternativfrequenz, wobei die Kontrolleinheit (40) für die Kontrolle des Ultraschallwandlers (10) adaptiert ist  
 mit der Hauptfrequenz zur Erzeugung von Ultraschallwellen, die in die Probe (20) eingekoppelt werden; und  
 mit einer der Alternativfrequenzen zur Erzeugung von Wärme im Ultraschallwandler (10) durch elektrische Energieaufnahme des Ultraschallwandlers (10), wobei die Wärme zum Erhitzen der Probe (20) durch die Leitung der im Ultraschallwandler (10) erzeugten Wärme verwendet wird.
12. Das System nach Anspruch 11, wobei der Ultraschallwandler (10) Bakterien und/oder Zellyse in eine Probe (20), wenn im Betrieb mit der Hauptfrequenz, induzieren und die Probe (20) durch die im

Ultraschallwandler (10) erzeugte Wärmeleitung, wenn im Betrieb mit der Alternativfrequenz, erhitzen kann.

- 5 13. Das System nach Anspruch 11 oder 12, wobei der Ultraschallwandler (10) simultan und/oder alternierend mit mindestens zwei Frequenzen betrieben werden kann.
- 10 14. Das System nach den Ansprüchen 11-13, wobei der Ultraschallwandler (10) mindestens zwei Elemente aufweist, von denen eines mit der Hauptfrequenz betrieben werden kann, um Ultraschallwellen zu erzeugen, und das andere mit mindestens einer der Alternativfrequenzen betrieben werden kann, um Wärme im Ultraschallwandler (10) zu erzeugen.
- 15

### Revendications

1. Procédé pour analyse d'échantillon en utilisant un transducteur ultrasonore (10) qui est adapté pour être couplé de façon conductrice de chaleur à un échantillon (20), comprenant :
- la commande du transducteur ultrasonore (10) qui est capable d'être mis en fonctionnement à au moins deux fréquences incluant une fréquence principale et au moins une fréquence alternative,  
 dans lequel le transducteur ultrasonore (10) est mis en fonctionnement à la fréquence principale pour générer des ondes ultrasonores qui sont destinées à être couplées dans l'échantillon (20) ; et  
 à une des fréquences alternatives pour générer de la chaleur dans le transducteur ultrasonore (10) en raison de l'absorption d'énergie électrique du transducteur ultrasonore (10), dans lequel la chaleur est utilisée pour chauffer l'échantillon (20) en raison de la conduction de chaleur générée dans le transducteur ultrasonore (10).
2. Procédé selon la revendication 1, dans lequel la fréquence principale et la fréquence alternative sont des fréquences de résonance du transducteur ultrasonore (10).
3. Procédé selon la revendication 1 ou 2, dans lequel, lors de l'excitation du transducteur ultrasonore (10) à au moins une des fréquences alternatives, moins d'intensité ultrasonore est générée que lors de l'excitation du transducteur ultrasonore (10) à la fréquence principale.
4. Procédé selon l'une des revendications précédentes, dans lequel l'intensité ultrasonore générée lors de l'excitation du transducteur ultrasonore (10) à au

- moins une des fréquences alternatives n'est pas suffisante pour générer des cavitations dans l'échantillon (20).
5. Procédé selon l'une des revendications précédentes, dans lequel des ondes ultrasonores de haute intensité générées à la fréquence principale sont capables de créer des cavitations dans l'échantillon (20). 5
6. Procédé selon l'une des revendications précédentes, dans lequel au moins une des fréquences alternatives est plus efficace dans la production de chaleur que la fréquence principale. 10
7. Procédé selon l'une des revendications précédentes, dans lequel au moins une des fréquences alternatives adaptées pour chauffer est plus élevée que la fréquence principale. 15
8. Procédé selon l'une des revendications précédentes, dans lequel la température de l'échantillon (20) est surveillée et/ou contrôlée. 20
9. Procédé selon l'une des revendications précédentes, dans lequel le transducteur ultrasonore (10) est capable d'être mis en fonctionnement simultanément et/ou en alternance dans la fréquence principale et dans au moins une des fréquences alternatives. 25
10. Procédé selon l'une des revendications précédentes, dans lequel l'échantillon (20) est inséré dans un organe de retenue d'échantillon (30) et le transducteur ultrasonore (10) est adapté pour être couplé de façon conductrice de chaleur à l'échantillon (20) inséré dans l'organe de retenue d'échantillon (30). 30
11. Système pour analyse d'échantillon, comprenant : 35
- 40
- au moins un organe de retenue d'échantillon (30) ;
- au moins un transducteur ultrasonore (10) qui est adapté pour être couplé de façon conductrice de chaleur à un échantillon (20) inséré dans l'organe de retenue d'échantillon (30) ; et 45
- une unité de commande (40) pour commander le transducteur ultrasonore (10) qui est capable d'être mis en fonctionnement à au moins deux fréquences incluant une fréquence principale et au moins une fréquence alternative, dans lequel l'unité de commande (40) est adaptée pour commander le transducteur ultrasonore (10) 50
- à la fréquence principale pour générer des ondes ultrasonores qui sont destinées à être couplées dans l'échantillon (20) ; et 55
- à une des fréquences alternatives pour générer de la chaleur dans le transducteur ultrasonore (10) en raison d'absorption d'énergie électrique du transducteur ultrasonore (10), dans lequel la chaleur est destinée à être utilisée pour chauffer l'échantillon (20) en raison de conduction de chaleur générée dans le transducteur ultrasonore (10).
12. Système selon la revendication 11, dans lequel le transducteur ultrasonore (10) est capable d'entraîner la lyse de bactérie et/ou de cellule dans un échantillon (20), lorsqu'il est excité à la fréquence principale, et de chauffer l'échantillon (20) en raison de conduction de chaleur générée dans le transducteur ultrasonore (10), lorsqu'il est excité à la fréquence alternative.
13. Système selon la revendication 11 ou 12, dans lequel le transducteur ultrasonore (10) est capable d'être excité simultanément et/ou en alternance à au moins deux fréquences.
14. Système selon les revendications 11 à 13, dans lequel le transducteur ultrasonore (10) comprend au moins deux éléments, dont un peut être mis en fonctionnement à la fréquence principale pour générer des ondes ultrasonores et l'autre peut être mis en fonctionnement à au moins une des fréquences alternatives pour générer de la chaleur dans le transducteur ultrasonore (10).

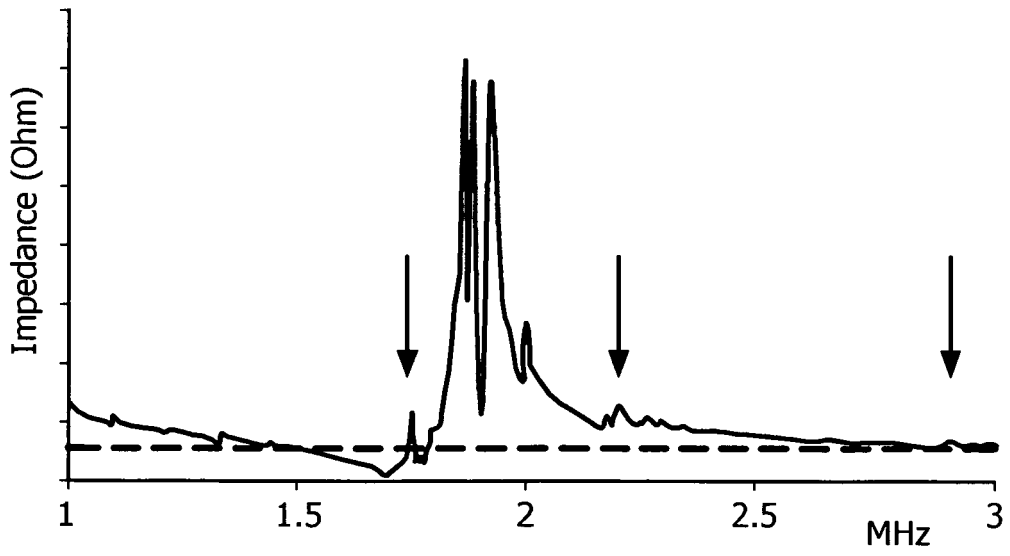


FIG. 1A

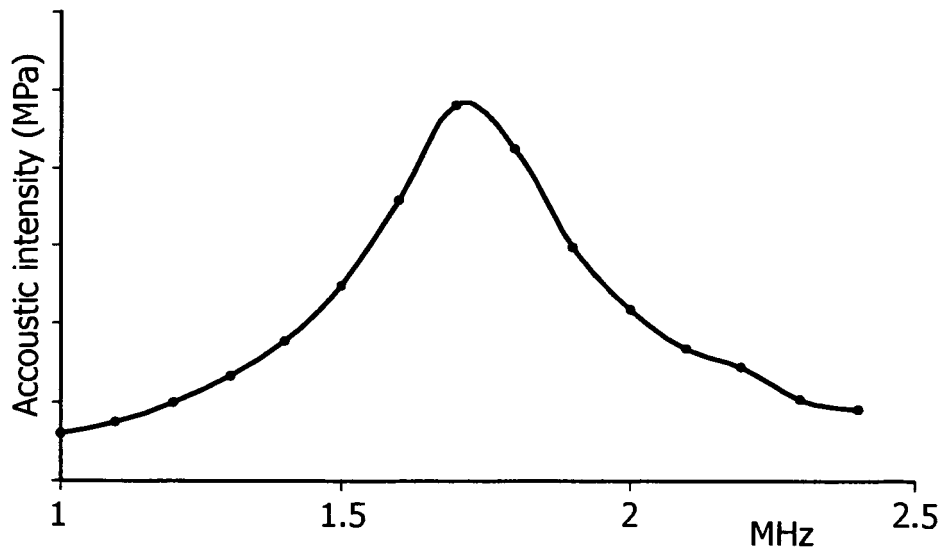


FIG. 1B

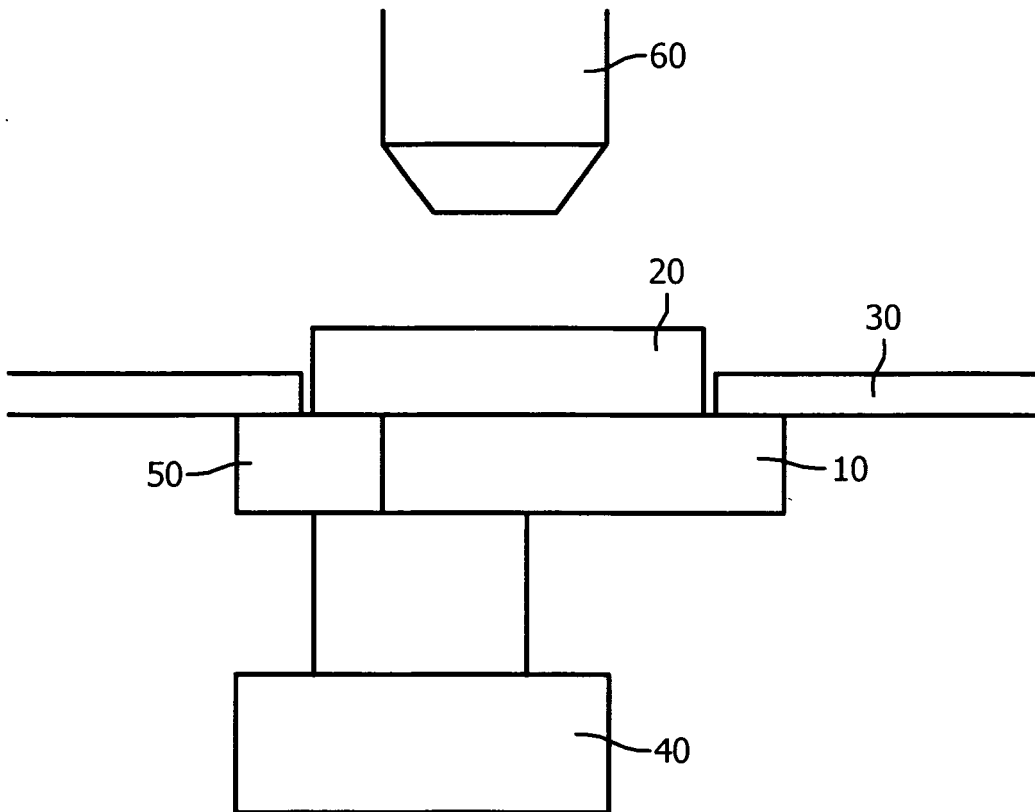


FIG. 2

**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- US 5601526 A [0003]
- WO 2009095894 A2 [0004]

专利名称(译)	超声换能器，用于选择性地产生超声波和热量		
公开(公告)号	<a href="#">EP2575966B1</a>	公开(公告)日	2015-12-16
申请号	EP2011727791	申请日	2011-05-24
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	VAN HEESCH CHRISTIANUS MARTINUS KOLESNYCHENKO ALEKSEY		
发明人	VAN HEESCH, CHRISTIANUS MARTINUS KOLESNYCHENKO, ALEKSEY		
IPC分类号	A61N7/00 G01N29/34 A61B8/00		
CPC分类号	A61N7/022 A61B8/00 A61N7/02 A61N2007/0039 A61N2007/0073 G01N29/34		
代理机构(译)	kroeze antonius , 约翰		
优先权	2010164111 2010-05-27 EP		
其他公开文献	EP2575966A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

为了提供用于超声波施加装置的加热装置，适用于平稳和快速地加热样品 ( 20 ) 并节省成本和空间，能够以包括主频率的多个频率驱动的超声波换能器 ( 10 ) 超声波和至少一个替代频率，在所述替代频率几乎不产生超声波，提出了一种包括这样的超声换能器 ( 10 ) 的用于样本分析的系统以及一种用于控制这种超声换能器 ( 10 ) 的方法，其中超声换能器 ( 10 ) 被驱动为用于产生超声波的主频率或用于在超声波换能器 ( 10 ) 中产生热的交替频率，如果样品 ( 20 ) 被加热的话。

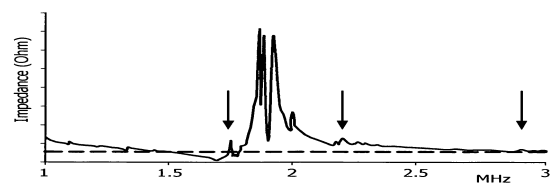


FIG. 1A

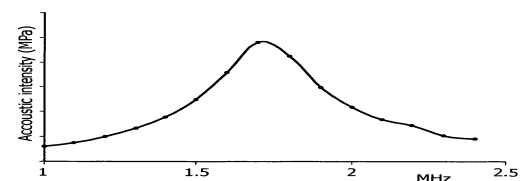


FIG. 1B