



(11) **EP 2 581 044 A2**

(12) **EUROPEAN PATENT APPLICATION**
published in accordance with Art. 153(4) EPC

(43) Date of publication:
17.04.2013 Bulletin 2013/16

(51) Int Cl.:
A61B 8/14 (2006.01) **G06F 3/048** (2013.01)
G06F 3/03 (2006.01)

(21) Application number: **11795899.1**

(86) International application number:
PCT/KR2011/003763

(22) Date of filing: **23.05.2011**

(87) International publication number:
WO 2011/159033 (22.12.2011 Gazette 2011/51)

(84) Designated Contracting States:
**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(72) Inventors:
• **JO, Dong Min**
Seoul 120-762 (KR)
• **PARK, Jin Yong**
Seoul 137-776 (KR)

(30) Priority: **14.06.2010 KR 20100055906**

(71) Applicant: **Alpinion Medical Systems Co., Ltd.**
Hwaseong-si, Gyeonggi-do 445-380 (KR)

(74) Representative: **Neobard, William John et al**
Kilburn & Strobe
20 Red Lion Street
London WC1R 4PJ (GB)

(54) **ULTRASONIC DIAGNOSIS DEVICE, GRAPHIC ENVIRONMENT CONTROL DEVICE FOR USE THEREIN, AND CONTROL METHOD THEREFOR**

(57) An ultrasonic diagnostic apparatus, a graphic environment control device for use therein, and a control method therefor are provided. The ultrasonic diagnostic apparatus includes: a touch panel for detecting an operator's touch position; a display for displaying images in response to ultrasonic waves radiated from a probe and

reflections of the ultrasonic waves; and a graphic control unit for displaying an input panel layout corresponding to the touch panel on the display, selecting a position on the input panel layout corresponding to a touch position detected by the touch panel, and performing a control operation corresponding to the position selected on the input panel layout.

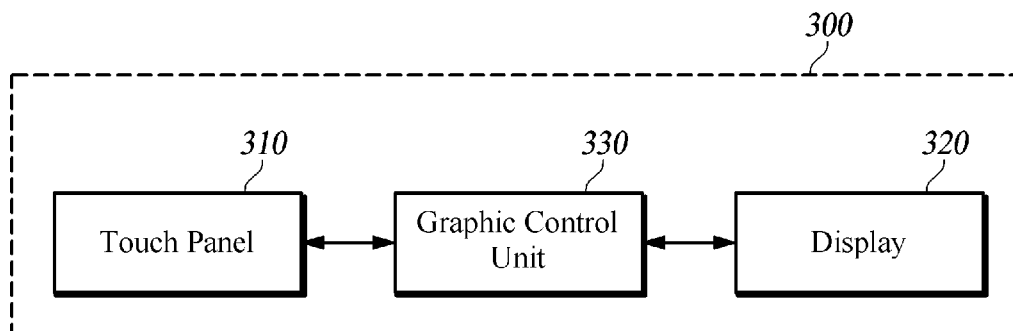


FIG. 3

Description

[Technical Field]

[0001] The present disclosure relates in some embodiments to an ultrasonic diagnostic apparatus, a graphic environment control device for use therein and a control method therefor. More particularly, the present disclosure relates to an ultrasonic diagnostic apparatus, a graphic environment control device for use therein and a control method therefor, wherein an operator is relieved from the need to move arm positions between the control panel and touch screen for each manipulation of the ultrasonic diagnostic apparatus as well as the need for constant visual attention switches between the touch screen and display.

[Background]

[0002] The statements in this section merely provide background information related to the present disclosure and may not constitute prior art.

[0003] An ultrasonic diagnostic equipment or ultrasonic diagnostic apparatus is a type of an inspection apparatus that irradiates ultrasonic wave on an inspection site of an object (for example, human body), detects a time difference between the irradiated ultrasonic wave and rebound echo reflected from the interior of the object, converts the detected time difference to a distance by using an electronic circuit, and images the inspection site of the object. The ultrasonic wave used in the ultrasonic diagnostic apparatus is harmless to humans. Therefore, the ultrasonic diagnostic apparatus is particularly useful for medical purposes and is widely used for detection of foreign substance inside human body, determination of the degree of damage, and monitoring a tumor or fetus.

[0004] FIG. 1 is a diagram for showing one example of a conventional ultrasonic diagnostic apparatus. Referring to FIG. 1, an ultrasonic diagnostic apparatus 100 is typically implemented in a transportable construction and includes a body 110, a control panel 120 and a display 130. The body 110 is mounted with an electronic circuit and a module for executing various control functions. The control panel 120 is provided with an input device, such as a keyboard, a switch, and a track ball, to allow an operator to input commands required for ultrasonic diagnosis. The display 130 performs signal processing on an ultrasonic wave irradiated through a probe and an echo, and displays the resultant image.

[0005] On the other hand, as digital electronic technologies have recently developed, the functions and inspection capability of ultrasonic diagnostic apparatuses have greatly enhanced. In order to sufficiently utilize such enhanced functions, it became necessary to extend an input device used and manipulated by an operator. However, there is a limitation to extending the control panel 120 alone by way of hardware, and a new function for separate manipulation guidance became necessary so as to

allow an operator to appropriately manipulate a complicated input device.

[0006] For this purpose, a touch screen 140 is provided for displaying additional graphic environment for manipulation and input of the operator independently of the display 130, and guiding an operator to appropriately manipulate an input device and input commands for different situations.

[0007] Generally, as shown in FIG. 1, the touch screen 140 is installed between the control panel 120 and the display 130. The touch screen 140 also serves to execute a screen function of displaying graphic environment for input and manipulation of an operator as well as a touch panel function of recognizing an operator touch point corresponding to the displayed graphic environment and executing an additional function and a control operation.

[0008] Since the touch screen 140 is typically implemented with a liquid crystal display (LCD) for displaying the graphic environment, it needs to maintain a predetermined tilt angle as shown in FIG. 2, considering the angle of the line of sight of the operator. Therefore, the control panel 120 and touch screen 140 inevitably have different installation angles from each other. However, in many cases, the control panel 120 and the touch screen 140 are alternately operated in order for the user to manipulate the ultrasonic diagnostic apparatus 100. Therefore, the operator needs to move arm positions for each manipulation of the ultrasonic diagnostic apparatus 100.

[0009] In addition, since the display 130 and the touch screen 140 of the conventional ultrasonic diagnostic apparatus 100 are located at different positions, the operator needs to alternately switch visual attention between the display 130 and touch screen 140 in the manipulation of the ultrasonic diagnostic apparatus 100.

[Disclosure]

[Technical Problem]

[0010] Therefore, the present disclosure is directed to providing an ultrasonic diagnostic apparatus, a graphic environment control device for use therein and a control method therefor, wherein an operator is relieved from the need to move arm positions between the control panel and touch screen for each manipulation of the ultrasonic diagnostic apparatus as well as the need for constant visual attention switches between the touch screen and display.

[Summary]

[0011] An embodiment of the present disclosure provides an ultrasonic diagnostic apparatus including: a touch panel for detecting a touch position; a display for displaying images in response to ultrasonic waves radiated from a probe and reflections of the ultrasonic waves; and a graphic control unit for displaying an input panel layout corresponding to the touch panel on the display,

selecting a position on the input panel layout corresponding to the touch position detected by the touch panel, and performing a control operation corresponding to the position selected on the input panel.

[0012] The touch panel may be installed on the same plane as a control panel in which one or more of a keyboard, a switch, and a track ball are installed.

[0013] The graphic control unit may adjust one or more of position, size, and rotation of the input panel displayed within the display in response to a selection from a user.

[0014] Another embodiment of the present disclosure provides a graphic environment control device for controlling graphic environment displayed on a display of an ultrasonic diagnostic apparatus, including: an input panel layout display unit for displaying an input panel layout corresponding to a touch panel on the display; a touch position calculation unit for calculating a touch position corresponding to a touch on the touch panel; a screen position determining unit for determining a position corresponding to a calculated touch position within the input panel layout; and a control execution unit for executing a control function corresponding to a determined position.

[0015] The graphic environment control device may further include an input display unit for indicating on the display that the position is determined.

[0016] The input panel layout display unit may display selection menus for a plurality of different varieties of the input panel layout, and displays an input panel layout corresponding to a menu selected by a user from among the displayed selection menus.

[0017] The input panel layout display unit may display selection menus for one or more of position adjustment, size adjustment, and rotation adjustment of the input panel layout, and display the input panel layout with one or more of position, size and rotation adjusted in response to a selected menu from among displayed selection menus by a user.

[0018] Yet another embodiment of the present disclosure provides a graphic environment control method for controlling graphic environment displayed on a display of an ultrasonic diagnostic apparatus, including: displaying an input panel layout corresponding to a touch panel on the display; calculating a touch position corresponding to a touch detected on the touch panel; determining a position corresponding to a calculated touch position within the input panel layout; and executing a control function corresponding to a determined position.

[0019] The graphic environment control method may further include indicating the determined position on the display.

[0020] The process of displaying the input panel layout may include displaying selection menus for a plurality of different varieties of the input panel layout, and displaying an input panel layout corresponding to a selected menu from among the displayed selection menus by a user.

[0021] The process of displaying the input panel layout may include displaying selection menus for one or more

of position adjustment, size adjustment, and rotation adjustment of the input panel layout, and displaying the input panel layout with one or more of position, size and rotation adjusted in response to a selected menu from among the displayed selection menus by a user.

[Advantageous Effects]

[0022] According to the present disclosure as described above, an operator is relieved from the need to move arm positions between the control panel and touch screen for each manipulation of the ultrasonic diagnostic apparatus as well as the need for constant visual attention switches between the touch screen and display and thereby the operator's convenience is enhanced with the ultrasonic diagnostic apparatus.

[Description of Drawings]

[0023] FIG. 1 is a diagram showing one example of a conventional ultrasonic diagnostic apparatus;

[0024] FIG. 2 is a diagram for describing a touch screen of FIG. 1;

[0025] FIG. 3 is a schematic diagram showing a configuration of an ultrasonic diagnostic apparatus according to an embodiment of the present disclosure;

[0026] FIG. 4 is a schematic diagram showing one example of a graphic environment control device according to an embodiment of the present disclosure;

[0027] FIG. 5 is a flow diagram showing a graphic environment control method that is performed by the graphic environment control device of FIG. 4; and

[0028] FIG. 6 is a diagram showing one example of a display screen that is realized by the graphic environment control device of FIG. 4.

[Detailed Description]

[0029] Hereinafter, embodiments of the present disclosure will be described in detail with reference to the accompanying drawings. In the following description, like reference numerals designate like elements although they are shown in different drawings. Further, in the following description of the present embodiments, a detailed description of known functions and configurations incorporated herein will be omitted for the purpose of clarity.

[0030] Additionally, in describing the components of the present disclosure, there may be terms used like first, second, A, B, (a), and (b). These are solely for the purpose of differentiating one component from the other but not to imply or suggest the substances, order or sequence of the components. If a component were described as 'connected', 'coupled', or 'linked' to another component, they may mean the components are not only directly 'connected', 'coupled', or 'linked' but also are indirectly 'connected', 'coupled', or 'linked' via a third component.

[0031] FIG. 3 is a schematic diagram showing a configuration of an ultrasonic diagnostic apparatus according to an embodiment of the present disclosure. Referring to FIG. 3, the ultrasonic diagnostic apparatus 300 according to the embodiment of the present disclosure includes a touch panel 310, a display 320, and a graphic control unit 330.

[0032] The touch panel 310 is an input device for detecting an operator touch position and includes a touch pad. The touch panel 310 used herein dispenses with a screen display function as an output device, and is conceptually different from a touch screen having a screen display function. Therefore, the touch panel 310 need not consider the angle of the line of sight of the operator, and may be installed on the same plane as the control panel 120 (see FIG. 1) in which one or more of a keyboard, a switch, and a track ball are installed. Since the touch panel and touch pad used in the embodiment of the present disclosure are conventionally available components, detailed description thereof will be omitted.

[0033] The display 320 displays images corresponding to an ultrasonic wave irradiated through a probe and an echo thereof.

[0034] The graphic control unit 330 displays an input panel layout corresponding to the touch panel 310 within the screen of the display 320, selects a point of the input panel correspondingly to a touch position detected through the touch panel 310, and performs control corresponding to the selected point of the input panel. In addition, the graphic control unit 330 may be configured to adjust one or more of the position, size, and rotation of the input panel displayed within the screen of the display 320 according to an operator's selection. The configuration and operation of the graphic control unit 330 may be realized by a graphic environment control device 400 of FIG. 4.

[0035] FIG. 4 is a schematic diagram showing one example of a graphic environment control device according to an embodiment of the present disclosure. The graphic environment control device 400 may operate as the graphic control unit 330 of FIG. 3. For this purpose, the graphic environment control device 400 may include an input panel layout display 410, a touch position calculation unit 420, a position determining unit 430, an input display unit 440, and a control execution unit 450.

[0036] The input panel layout display unit 410 displays the input panel layout corresponding to the touch panel 310 on the display 320. In addition, the input panel layout display unit 410 may include a plurality of different varieties of the input panel layout. In this case, the input panel layout display unit 410 may display a selection menu for each input panel layout on the display 320, and display an input panel layout corresponding to a menu selected by the operator on the display 320. The plurality of input panel layouts may be provided with representations of displayed input panels corresponding to each of the various functions when input and manipulation are performed on the functions by using the touch panel 310.

[0037] In addition, the input panel layout display unit 410 may display a selection menu for one or more of position adjustment, size adjustment, and rotation adjustment of the input panel, and display one or more of the adjusted position, size and rotation of the input panel corresponding to a menu selected by the operator.

[0038] The touch position calculation unit 420 calculates a touch position corresponding to an operator's touch with the touch panel 310. The method for calculating the touch position corresponding to the touch with the touch panel 310 adopts a known technique, and detailed description thereof will be omitted.

[0039] The position determining unit 430 determines a position corresponding to the touch position calculated by the touch position calculation unit 420 in the input panel layout. In this case, when the operator shifts the touch position across the touch panel 310, an arrow or cursor is adapted to follow suit thereafter in the input panel layout on the display 320. When the operator double-clicks the touch panel 310 at the touch position, its corresponding position may be recognized as determined.

[0040] When the position corresponding to the touch position is selected by the position determining unit 430, the input display unit 440 may indicate the selection of the position on the display 320. For example, when the operator double-clicks the touch panel 310 at the touch position while watching the position displayed on the display 320, the input display unit 440 may indicate the selection of the position by expressing the position in a distinctive color. The above-described displaying method of the input display unit 440 is merely exemplary, and various modifications may be made to the displaying method.

[0041] The control execution unit 450 executes a control function corresponding to the determined position. For this purpose, the control execution unit 450 may store different functions matchingly with each position of the input panel layout, and execute a function corresponding to the position selected by the position determining unit 430.

[0042] FIG. 5 is a flow diagram showing a graphic environment control method that is performed by the graphic environment control device of FIG. 4. The function and operation of the graphic environment control device 400 according to the embodiment of the present disclosure will be described in detail with reference to FIG. 5.

[0043] As shown in FIG. 6, the input panel layout display unit 410 displays an input panel layout 610 corresponding to the touch panel 310 on a screen 600 of the display 320 (S501). The input panel layout display unit 410 may include a plurality of input panel layouts divided by functions, display selection menus 620 for the input panel layouts on the display 320, and display an input panel layout corresponding to a menu, selected by the operator among the displayed selection menus, on the display 320. FIG. 6 shows a case where an input panel layout corresponding to a selection menu 1 is displayed among selection menus 1 to 4.

[0044] In addition, the input panel layout display unit 410 may display a selection menu for one or more of position adjustment, size adjustment, and rotation adjustment of the input panel, and display the input panel with one or more of the position, size and rotation adjusted corresponding to a menu selected by the operator. For example, the position of the input panel layout may be shifted by locating the position at the lateral side of the input panel layout 610 and dragging the lateral side in a vertical direction, or the size of the input panel may be adjusted by locating the position at the edge of the input panel layout 610 and dragging the edge in a diagonal direction. In addition, the input panel may be rotated by rotation in a state that the position is fixed in the input panel layout 610.

[0045] The touch position calculation unit 420 calculates a touch position corresponding to an operator's touch with the touch panel 310 (S503). The method for calculating the touch position corresponding to the touch with the touch panel 310 adopts prior art technique, and detailed description thereof will be omitted.

[0046] The position determining unit 430 determined in the input panel layout a position corresponding to the touch position calculated by the touch position calculation unit 420 (S505). In this case, when the operator shifts the touch position across the touch panel 310, an arrow or cursor is implemented to follow suit thereafter in the input panel layout on the display 320. When the operator double-clicks the touch position of the touch panel 310, the position corresponding to the touch position may be recognized as determined.

[0047] When the position corresponding to the touch position is determined by the position determining unit 430, the input display unit 440 may display the determination of the corresponding screen position on the display 320 (S507). For example, when the operator double-clicks the touch position of the touch panel 310 while watching the screen position displayed on the display 320, the input display unit 440 may display the determination of the position by expressing the position in a distinctive color.

[0048] The control execution unit 450 executes a control function corresponding to the determined position (S509). For this purpose, the control execution unit 450 may store different functions matchingly with each position of the input panel layout.

[0049] As described above, the touch panel can be installed on the same plane as the control panel. Therefore, by displaying the input panel layout on the display, the operator is relieved from the need to move between different tilt angles during the manipulation of the ultrasonic diagnostic apparatus as well as the need for constant visual attention switches between different displays.

[0050] In the description above, although all of the components of the embodiments of the present disclosure may have been explained as assembled or operatively connected as a unit, the present disclosure is not intended to limit itself to such embodiments. Rather, with-

in the objective scope of the present disclosure, the respective components may be selectively and operatively combined in any numbers. Every one of the components may be also implemented by itself in hardware while the respective ones can be combined in part or as a whole selectively and implemented in a computer program having program modules for executing functions of the hardware equivalents. Codes or code segments to constitute such a program may be easily deduced by a person skilled in the art. The computer program may be stored in computer readable media, which in operation can realize the embodiments of the present disclosure. As the computer readable media, the candidates include magnetic recording media, optical recording media, and carrier wave media.

[0051] In addition, terms like 'include', 'comprise', and 'have' should be interpreted in default as inclusive or open rather than exclusive or closed unless expressly defined to the contrary. All the terms that are technical, scientific or otherwise agree with the meanings as understood by a person skilled in the art unless defined to the contrary. Common terms as found in dictionaries should be interpreted in the context of the related technical writings not too ideally or impractically unless the present disclosure expressly defines them so.

[0052] Although exemplary embodiments of the present disclosure have been described for illustrative purposes, those skilled in the art will appreciate that various modifications, additions and substitutions are possible, without departing from essential characteristics of the disclosure. Therefore, exemplary embodiments of the present disclosure have not been described for limiting purposes. Accordingly, the scope of the disclosure is not to be limited by the above embodiments but by the claims and the equivalents thereof.

CROSS-REFERENCE TO RELATED APPLICATION

[0053] If applicable, this application claims priority under 35 U.S.C §119(a) of Patent Application No. 10-2010-0055906, filed on June 14, 2010 in Korea, the entire content of which is incorporated herein by reference. In addition, this non-provisional application claims priority in countries, other than the U.S., with the same reason based on the Korean Patent Application, the entire content of which is hereby incorporated by reference.

Claims

1. An ultrasonic diagnostic apparatus comprising:

a touch panel for detecting a touch position;
a display for displaying images in response to ultrasonic waves radiated from a probe and reflections of the ultrasonic waves; and
a graphic control unit for displaying an input panel layout corresponding to the touch panel on

- the display, selecting a position on the input panel layout corresponding to the touch position detected by the touch panel, and performing a control operation corresponding to the position selected on the input panel layout. 5
2. The ultrasonic diagnostic apparatus of claim 1, wherein the touch panel is installed on the same plane as a control panel in which one or more of a keyboard, a switch, and a track ball are installed. 10
 3. The ultrasonic diagnostic apparatus of claim 1, wherein the graphic control unit adjusts one or more of position, size, and rotation of the input panel displayed within the display in response to a selection from a user. 15
 4. A graphic environment control device for controlling graphic environment displayed on a display of an ultrasonic diagnostic apparatus, the graphic environment control device comprising: 20
 - an input panel layout display unit for displaying an input panel layout corresponding to a touch panel on the display; 25
 - a touch position calculation unit for calculating a touch position corresponding to a touch on the touch panel;
 - a screen position determining unit for determining a position corresponding to a calculated touch position within the input panel layout; and 30
 - a control execution unit for executing a control function corresponding to a determined position.
 5. The graphic environment control device of claim 4, further comprising an input display unit for indicating on the display that the position is determined. 35
 6. The graphic environment control device of claim 4, wherein the input panel layout display unit displays selection menus for a plurality of different varieties of the input panel layout, and displays an input panel layout corresponding to a menu selected by a user from among displayed selection menus. 40
 7. The graphic environment control device of claim 4, wherein the input panel layout display unit displays selection menus for one or more of position adjustment, size adjustment, and rotation adjustment of the input panel layout, and displays the input panel layout with one or more of position, size and rotation adjusted in response to a selected menu from among displayed selection menus by a user. 45 50
 8. A graphic environment control method for controlling graphic environment displayed on a display of an ultrasonic diagnostic apparatus, the graphic environment control method comprising: 55
 - displaying an input panel layout corresponding to a touch panel on the display;
 - calculating a touch position corresponding to a touch detected on the touch panel;
 - determining a position corresponding to a calculated touch position within the input panel layout; and
 - executing a control function corresponding to a determined position.
 9. The graphic environment control method of claim 8, further comprising indicating the determined position on the display.
 10. The graphic environment control method of claim 8, wherein the process of displaying the input panel layout comprises displaying selection menus for a plurality of different varieties of the input panel layout, and displaying an input panel layout corresponding to a selected menu from among displayed selection menus by a user.
 11. The graphic environment control method of claim 8, wherein the process of displaying the input panel layout comprises displaying selection menus for one or more of position adjustment, size adjustment, and rotation adjustment of the input panel layout, and displaying the input panel layout with one or more of position, size and rotation adjusted in response to a selected menu from among displayed selection menus by a user.

100

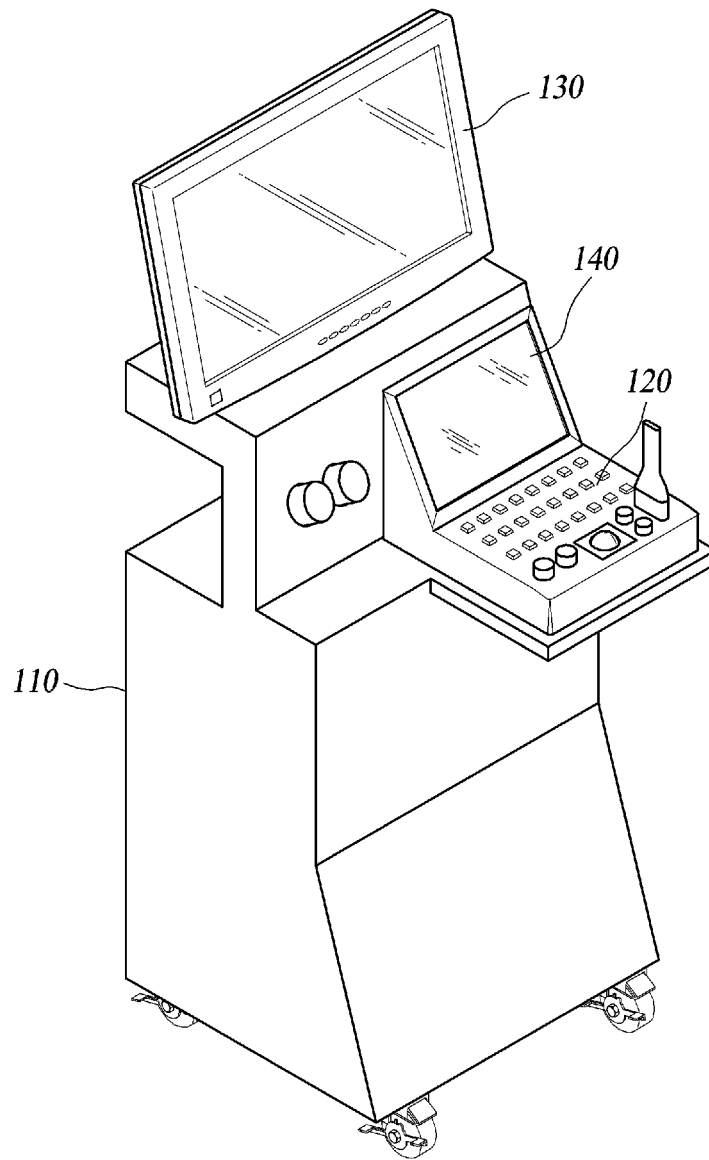


FIG. 1

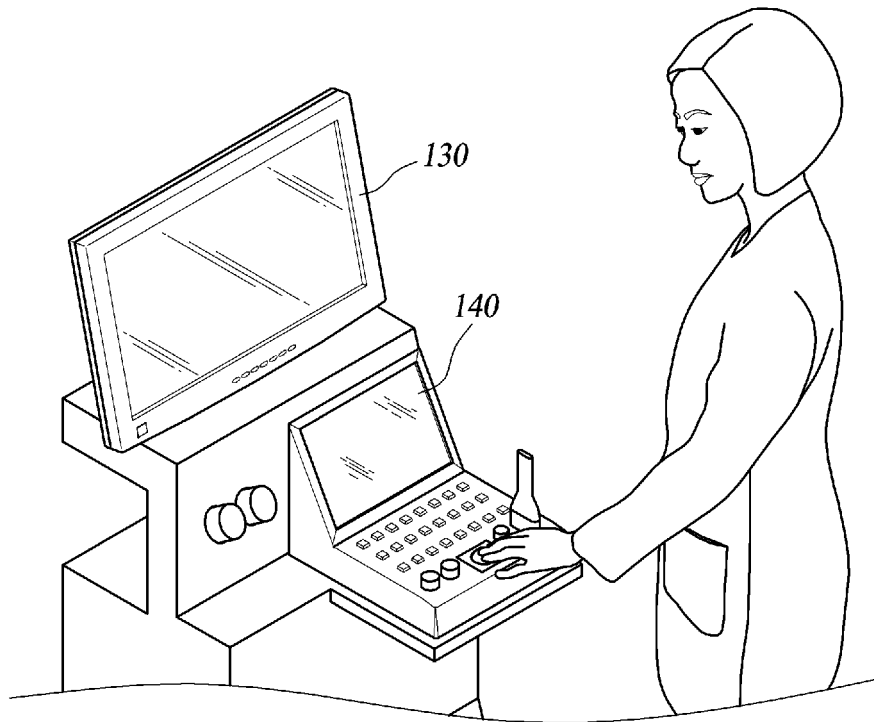


FIG. 2

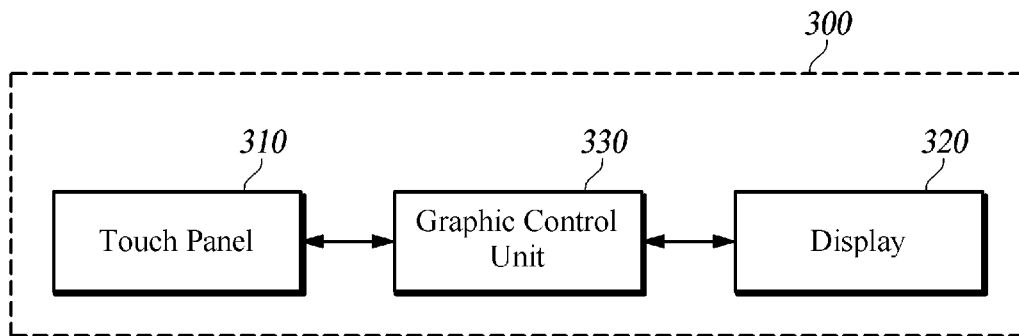


FIG. 3

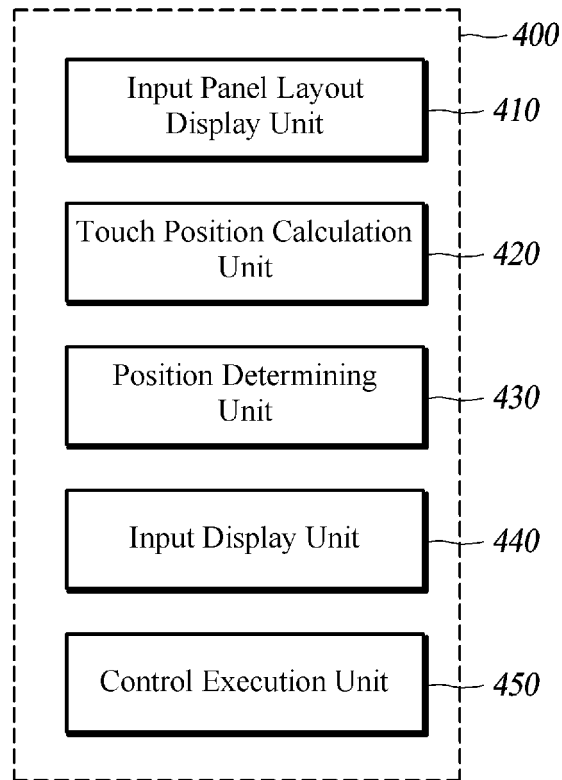
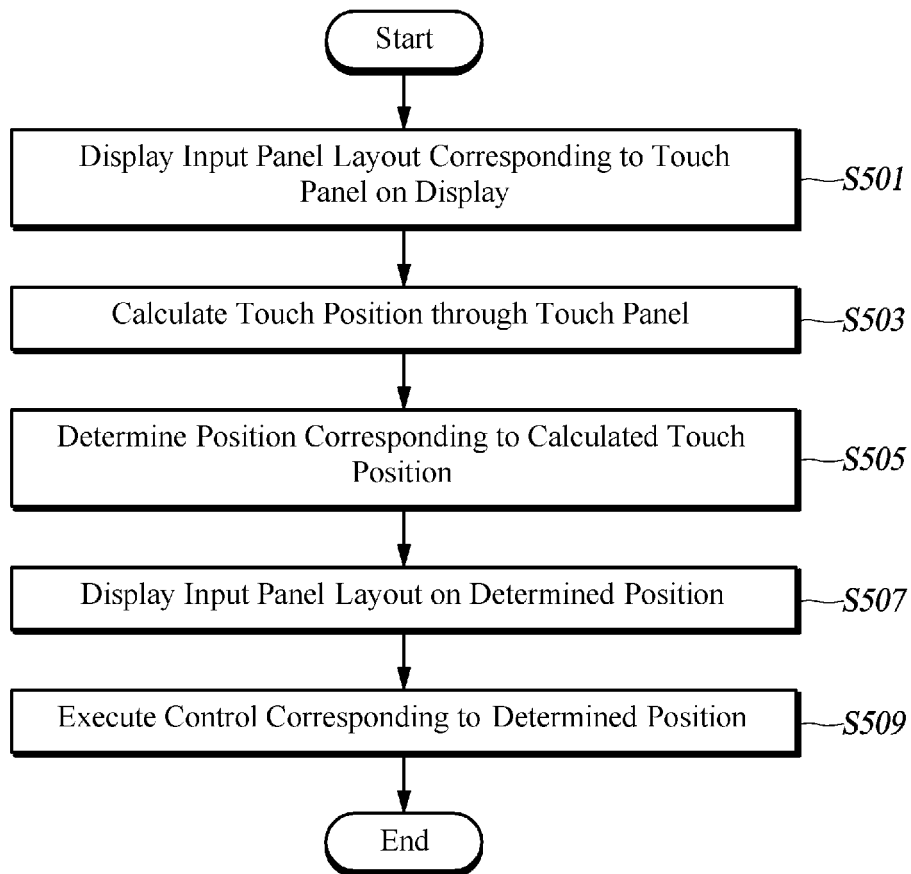


FIG. 4

**FIG. 5**

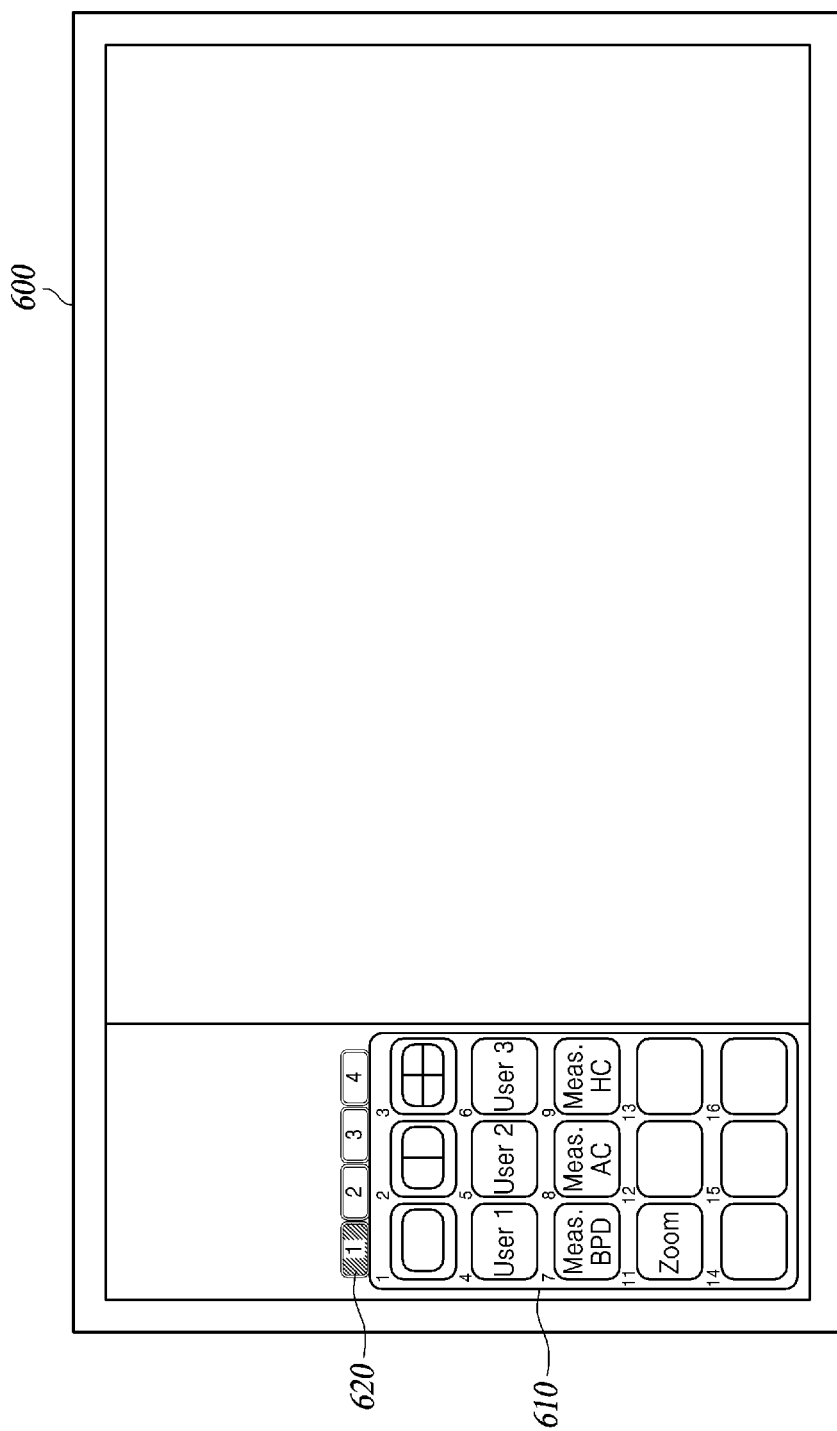


FIG. 6

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- KR 1020100055906 [0053]

专利名称(译)	超声波诊断装置，其中使用的图形环境控制装置及其控制方法		
公开(公告)号	EP2581044A2	公开(公告)日	2013-04-17
申请号	EP2011795899	申请日	2011-05-23
[标]申请(专利权)人(译)	爱飞纽医疗机械贸易有限公司		
申请(专利权)人(译)	ALPINION MEDICAL SYSTEMS CO., LTD.		
当前申请(专利权)人(译)	ALPINION MEDICAL SYSTEMS CO., LTD.		
[标]发明人	JO DONG MIN PARK JIN YONG		
发明人	JO, DONG MIN PARK, JIN YONG		
IPC分类号	A61B8/14 G06F3/048 G06F3/03		
CPC分类号	G06F3/0484 A61B8/4405 A61B8/461 A61B8/464 A61B8/465 A61B8/467		
优先权	1020100055906 2010-06-14 KR		
其他公开文献	EP2581044A4		
外部链接	Espacenet		

摘要(译)

本发明提供一种超声波诊断装置，其中使用的图形环境控制装置及其控制方法。超声波诊断装置包括：触摸面板，用于检测操作者的触摸位置；显示器，用于响应从探头辐射的超声波和超声波的反射显示图像；图形控制单元，用于在显示器上显示与触摸面板对应的输入面板布局，选择与触摸面板检测到的触摸位置对应的输入面板布局上的位置，并执行与在触摸面板上选择的位置对应的控制操作。输入面板布局。

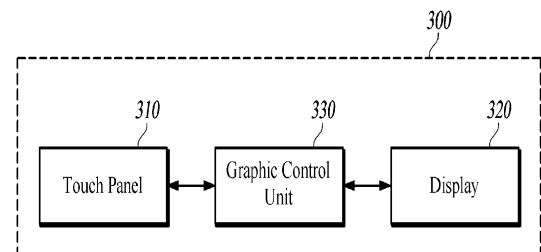


FIG. 3