



(12) **EUROPEAN PATENT APPLICATION**  
published in accordance with Art. 158(3) EPC

(43) Date of publication:  
**19.01.2005 Bulletin 2005/03**

(51) Int Cl.<sup>7</sup>: **A61B 8/12**

(21) Application number: **03746424.5**

(86) International application number:  
**PCT/JP2003/004287**

(22) Date of filing: **03.04.2003**

(87) International publication number:  
**WO 2003/086196 (23.10.2003 Gazette 2003/43)**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR  
HU IE IT LI LU MC NL PT RO SE SI SK TR**

- **ITO, Takashi**  
**Abiko-shi, Chiba 270-1132 (JP)**
- **IZUMI, Mikio**  
**Soka-shi, Saitama 340-0022 (JP)**

(30) Priority: **17.04.2002 JP 2002114333**

(71) Applicant: **Hitachi Medical Corporation**  
**Tokyo 101-0047 (JP)**

(74) Representative: **Strehl Schübel-Hopf & Partner**  
**Maximilianstrasse 54**  
**80538 München (DE)**


(72) Inventors:  
• **YAGI, Tomoyuki**  
**Kashiwa-shi, Chiba 277-0803 (JP)**

(54) **ULTRASONIC PROBE IN BODY CAVITY**

(57) To miniaturize a probe, increase the channel number, and improve flexibility of flexible section, an ultrasound probe includes transducer unit 1 having a plurality of channels arranged for transmitting and receiving an ultrasound wave, and flexible circuit board 2 connect-

ed to the respective channels of transducer unit 1 in which a signal line for supplying a transmission signal and extracting a reception signal to/from transducer unit 1 is provided, wherein flexible circuit board 2 forms at least two channel blocks made by dividing the plurality of channels and spirally wound individually.

**Fig.1**

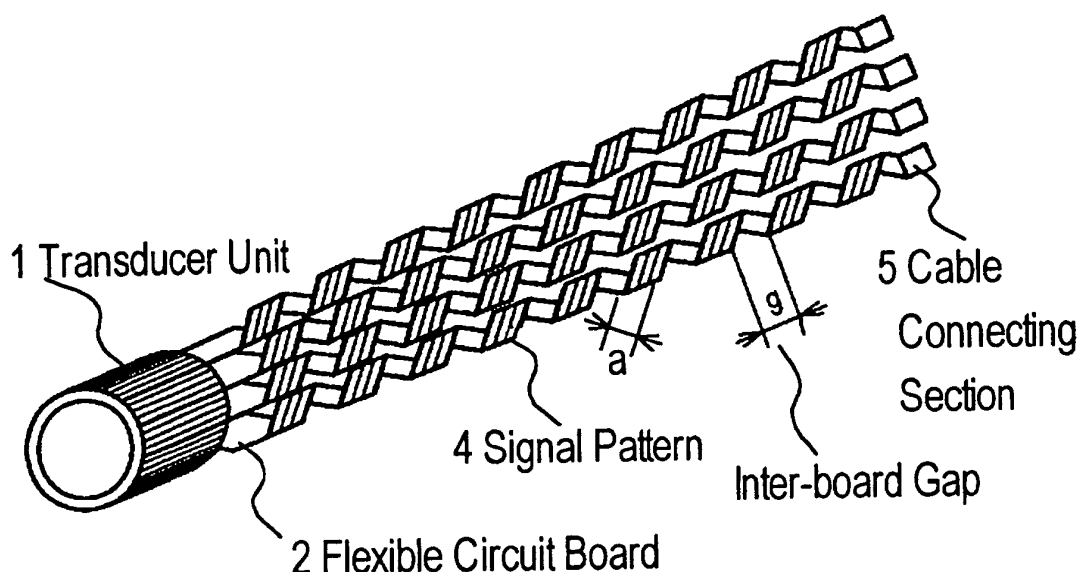

## Description

### Technical Field

**[0001]** The present invention relates to an intracavitary ultrasound probe for inserting the probe inside a body cavity of an object to be examined and scanning an ultrasound beam.

### Background of the Invention

**[0002]** An intracavitary ultrasound probe is designed to observe an esophageal wall, an intestinal wall, and the like from inside by inserting the probe inside the human body from a mouth, an anus, and the like of a human body. Accordingly, a flexible section which can be freely bent along a complicated shape of tubular organ such as an intestinal canal is variously devised as mentioned below.

**[0003]** First, as disclosed in Japanese Patent Publication No.2790253 (first conventional technique), an ultrasound probe of electronic scan type includes an ultrasound transducer group in which a transducer array for transmitting and receiving ultrasound are arranged into a plurality of transducers and a flexible print circuit board formed in a longitudinal direction of the transducers at a predetermined angle relative to the ultrasound transducer group, in which an electrode extraction lead for acquiring a signal from each ultrasound transducer of the ultrasound transducer group is formed on one end.

**[0004]** As shown in Fig.4(a), the print circuit board is formed so that a section in which the ultrasound transducer group is arranged is rectangular, and an electrode extracting section joined with the rectangular section is formed so that a surface electrode pattern is inclined at a certain angle relative to a longitudinal direction of the ultrasound transducer group. At the same time, an outer shape of the print circuit is carved out, inclining at a certain angle similar to the pattern. A portion of circuit board on which the ultrasound transducer group is mounted has adhering sections at both ends, and an adhering section is also provided on one end of the print circuit board on which the electrode pattern is formed. When the print circuit is made into a cylindrical shape and the respective adhering sections are adhered with a bond, the electrode pattern is spirally formed and a gap made between the adhering sections of the print circuit board is also formed spirally. With this construction, the print circuit board can be bent without broken.

**[0005]** Further, as mentioned in Fig.8(a) of the above patent document, the print circuit board divides the ultrasound transducer group into blocks, and the electrode extracting section of the print circuit board is lead in directions of  $\theta$ ,  $-\theta$ ,  $\theta$ ,  $-\theta$ , ... in turn at each block. By thus forming the ultrasound transducer group and the print circuit board into a cylindrical shape, the print circuit board is constructed in a meshed pattern. The end

connected with a lead wire is a little shifted so that the position of a land attached with the lead wire does not overlap with a land of other print circuit board in weaving the print circuit board. Further, the end connected with the lead wire is provided with an adhering section for adhering each of print circuit boards. The print circuit board being one undivided plate can be made more flexible by forming it into the meshed pattern.

**[0006]** Next, as disclosed in Japanese Unexamined Utility Model Patent Publication No.Hei.5-13408 (second conventional technique), an ultrasound sensor is mounted at the end of a flexible body, and a signal from the ultrasound sensor is transmitted to a cable on the end by a flexible print circuit (FPC). The FPC is provided with a plurality of slits in its longitudinal direction and wound in its width direction. A coil spring connected to a GND of the ultrasound sensor surrounds it.

**[0007]** However, according to the first conventional technique, the print circuit board is formed as one plate. Even in the example of block division, the print circuit boards are adhered to each other and substantially made into one plate.

**[0008]** Since the print circuit board is thus formed as one plate, the range of flexibility of the intracavitary probe is limited by stiffness of the print circuit board when it is inserted into the object's body cavity, and due to this limitation of flexibility the intracavitary probe cannot be sufficiently bent along a complicatedly curving tubular organ in some cases. Accordingly, there is a possibility that a part of the intracavitary ultrasound probe touch a wall of the tubular organ to cause pain to the object, which has not been considered.

**[0009]** Further, according to the second conventional technique, the plurality of slits are provided on the FPC in the longitudinal direction and surrounded with coil spring 7, which occupies extra space. Therefore, it has been an obstacle to the needs of miniaturizing the probe, increasing the number of channels, and improving flexibility of the flexible section.

**[0010]** Moreover, an ultrasound apparatus is used not only independently for diagnosis but also with a treatment device. For example, treatment is conducted by irradiating a strong ultrasound to cauterize a cancer cell. When the ultrasound diagnostic apparatus according to the present invention is used with an electronic device like the treatment device, it is also necessary to take into consideration to deal with a noise infiltrating from the electronic device into the ultrasound probe.

### Summary of the Invention

**[0011]** The present invention is done in consideration of the above. A first object thereof is to provide an ultrasound probe, which is miniaturized and in which the number of channels is increased, and the flexibility of a flexible section is improved.

**[0012]** Further, a second object of the present invention is to provide an ultrasound probe made in consid-

eration of dealing with a noise.

**[0013]** Further, a third object of the present invention is to provide an ultrasound probe in which wires of the ultrasound probe are not disrupted and broken when the probe is bent, and which is easy to insert into and pull out from the body cavity.

**[0014]** The first object is achieved by constructing an ultrasound probe including transducers for transmitting and receiving an ultrasound having an array of a plurality of channels respectively located at several adjacent positions and a flexible circuit board connected to the respective channels of those transducers and on which a signal line for transmitting a transmission signal and extracting a reception signal to/from the transducers is printed in a longitudinal direction of the transducer with a predetermined angle, wherein at least two channel blocks are formed on the flexible circuit board by dividing the plurality of channels, and the respective channel blocks are spirally wound.

**[0015]** Further, the second object is achieved by constructing an ultrasound probe in which the above two or more channel blocks formed on the flexible circuit board are surrounded with an insulating material and a first shield material, or with an insulating material evaporated on its surface one of a layer of metallic powder of gold, silver, copper, brass, aluminum, and the like or a combination thereof. Further, the second object also can be achieved by arranging a single second shield material for covering an outer circumference of the bundled channel blocks of the flexible circuit board. And further, it also can be achieved more effectively by constructing an ultrasound probe in which each channel block formed on the flexible circuit board are covered with an insulating material and a first shield material, or with an insulating material evaporated on its surface a layer of metallic powder of gold, silver, copper, brass, aluminum, and the like or a combination thereof, and further arranging a second single shield material or protective material, or an insulating material evaporated on its surface a layer of metallic powder for covering the outer circumference of the bundled channel blocks of the flexible circuit board.

**[0016]** The third object is achieved by providing either a protection material or a second shield material for covering two or more channel blocks bundled on the flexible circuit board, whereby the channel blocks are not disrupted. Further, handling is improved by making the protection layer using flexible material, and the probe becomes easy to grip and operation becomes easy for an operator by providing the stiff section and the flexible section.

#### Brief Description of Drawings

**[0017]** Fig. 1 is a diagram showing the state that a part of a flexible circuit board of an ultrasound probe according to the present invention is spirally wound. Fig. 2 is a diagram showing a transducer unit of the intracavitary

ultrasound probe, a flexible circuit board to which slits are made, and a joint unit of cable according to present invention. Fig. 3 is a diagram showing the bending state of the flexible intracavitary probe containing the flexible circuit board. Fig. 4 is a diagram showing a positional relation among a flexible tube used as a protection material for containing the flexible circuit board and the like and a plurality of flexible circuit boards. Fig. 5 is a schematic diagram showing the bending state of the flexible circuit board extending from the portion connected with the transducer. Fig. 6 is a diagram showing an example of application of the present invention to a convex type ultrasound probe. Fig. 7 is a diagram showing an example of application of the present invention to a transesophageal ultrasound probe. Fig. 8 is a diagram showing an example of application of the present invention to an abdominal ultrasound probe. Fig. 9 is a diagram showing the state that the flexible circuit board is covered with a resin tube used as an insulating material. Fig. 10 is a diagram showing the state of the flexible circuit board formed as a duplex circuit board. Fig. 11 is a diagram showing an example of covering each flexible circuit board with a first shield material. Fig. 12 is a diagram showing a first shield material and a flexible circuit board inserted into the flexible tube used as a protection layer containing parts of Fig. 11, in which the first and second shield materials are electrically connected.

#### Best Mode for Carrying Out the Invention

**[0018]** Hereinafter, embodiments of the present invention will be described in detail with reference to the accompanying drawings.

**[0019]** First, an intracavitary ultrasound probe called radial type is taken as an example. Fig. 2 is a diagram showing a connecting relation among a transducer unit, a flexible circuit board, and a cable of the radial type intracavitary ultrasound probe.

**[0020]** Transducer unit 1 is formed so that a transducer element corresponds with each of a plurality of close positions of transmission and reception (hereinafter referred to as "channel"). One end of flexible circuit board 2 is connected to each channel of the transducer elements, and the other end has a cable connecting section 5 so that a signal line can be connected to a cable for transmission and reception. On this flexible circuit board 2, signal pattern 4 is formed so that a signal can be transmitted and received between transducer unit 1 and cable connecting section 5, and each signal pattern 4 is electrically insulated. Further, flexible circuit board 2 is not formed by one circuit board but formed so that a part of all channels is bundled into blocks divided by slit 3. Further, it is preferable to provide a ground so as to sandwich signal pattern 4 because crosstalk in signal transmission can be thereby prevented.

**[0021]** Further, each divided portion of flexible circuit board 2 is spirally wound at angle  $\theta$  relative to transducer unit 1. However, because the flexible circuit board is

flexible, the angle is not exactly determined but has a certain range. Accordingly, the slit may be formed roughly at angle  $\theta$ .

**[0022]** Next, Fig.1 is a diagram showing the state of the spirally wound flexible circuit board of the intracavitary ultrasound probe according to the present invention.

**[0023]** As shown in the figure, transducer unit 1 is rolled and fixed. It may be fixed not only by adhesion but also by setting it in a formwork and the like. Flexible circuit board 2 is spirally wound at intervals of gap  $g$ . At this time, gap  $g$  is determined depending on the extent of bending the body covering flexible circuit board 2. Here, the principle thereof will be described with reference to Fig.3. Fig.3 is a diagram showing the principle for calculating gap  $g$ . When it is hypothesized that the body is bent so as to draw an arc, given that the radius is  $R$ , the diameter of the body is  $d$ , and the width of one flexible circuit board is  $a$  (see Fig.1), gap  $g$  is calculated by formula (1).

$$g = a \cdot d/R \quad (1)$$

**[0024]** A process of deriving this formula will be described. When the flexible section is bent at  $\theta^\circ$ , in Fig. 3 the length of inner arc CD of the flexible section bent to the maximum is  $2\pi R \theta / 360$ , and the length of outer arc AB of the flexible section bent to the maximum is  $2\pi (R+d) \theta / 360$ . Accordingly, a difference between outer and inner arcs is  $2\pi d \theta / 360$ . Here, number  $n$  of spiral portions in the flexible section (winding number) is calculated by dividing  $2\pi R \theta / 360$  being the length of inner arc of the flexible portion bent to the maximum by width  $a$  of the flexible circuit board, the result being  $2\pi R \theta / 360a$ . Gap  $g$  is the number obtained by dividing the difference between the arcs of the outer and inner flexible section by the winding number of the flexible circuit board, which is expressed as  $g=ad/R$ . Meanwhile, a relation between width  $a$  of the flexible circuit board and gap  $g$  is  $a \geq g$ .

**[0025]** In this manner, gap  $g$  of flexible circuit board 2 is determined, and flexible circuit board 2 is arranged in a body referred to as a flexible tube made of synthetic resin, synthetic rubber, or the like on the basis of its division number as shown in a cross sectional view of Fig. 4. Fig.4 is a diagram showing a relation of arrangement between the flexible tube and a plurality of flexible circuit boards contained therein. Fig.4(a) shows an example of the flexible circuit board divided into two, each of which is spirally wound. Fig.4(b) shows an example of division into three, Fig.4(c) shows an example of division into four, and Fig.4(d) shows an example of division into five. When the circuit board is divided into six or more, close-packed arrangement is formed.

**[0026]** Next, how the flexible circuit board is bent will be described. Fig.5 is a diagram showing modes of the flexible circuit board from an extraction point (point con-

nected with elements) to a flexible section. The flexible circuit board is contracted as shown in Fig.5(a) when it does not have to be bent. When it has to be bent, it can be bent as shown in Fig.5(c) since it has an extensible structure shown in Fig.5(b).

**[0027]** Meanwhile, the intracavitary ultrasound probe includes a convex type, a transesophageal type, and an abdominal type in addition to the radial type, examples of application of which will be mentioned.

**[0028]** Fig.6 is a diagram showing an example of application of the present invention to the convex type ultrasound probe, Fig.7 is a diagram showing an example of application of the present invention to the transesophageal ultrasound probe, and Fig.8 is a diagram showing an example of application of the present invention to the abdominal ultrasound probe. The radial type has an FOV in a cross sectional direction of the inner surface of a tubular organ. On the other hand, the convex type has a rectangular FOV with respect to an inner wall. As shown in the figure, many of transesophageal type have, e.g. a circular FOV as shown in Fig.7, or a polygonal FOV. Although the abdominal type also has a rectangular FOV similar to that of the convex type, it is not inserted into an object to be examined along the tubular organ but inserted into a hole punched on a body surface of the object. Since the probe is difficult to handle if the portion gripped by the object is flexible tube 8, it is made as hard section 12.

**[0029]** Further, as shown in Fig.9(a), each of the flexible circuit boards may be individually covered with resin tube 13 so as to react to bending stress. A cross-sectional view of the body covered with resin tube 13 is arranged as shown in Fig.9(b), which shows an example of division into five.

**[0030]** Further, the flexible circuit board is constructed by duplex print circuit boards as shown in Fig.10, in which a signal line is connected with one layer and GND layer 14 is provided over the other layer. Since a pattern of signal line can be integrated on the signal line layer, this construction is effective in increasing the number of channel and resolving crosstalk. Fig.10(b) is a cross sectional view of the body in which the duplex flexible circuit boards are arranged, which shows an example of division into five.

**[0031]** According to the above described embodiment, the limitation of the flexible range of the flexible circuit board (print circuit board) existing in the state that the flexible circuit board is made as one plate is released, the degree of flexibility is properly ensured, and miniaturizing of the probe and increase of the channel number are enabled since a coil spring is not used.

**[0032]** Further, the channels of the flexible circuit board may be divided equally or unequally.

**[0033]** Further, since the value of gap is properly determined, a signal line inside the flexible circuit board does not easily broken.

**[0034]** Further, it is needless to say that the present invention may be applied to a combination of various

modes of a flexible circuit board covered with a resin tube, that formed by two or more multiple layers of pattern, and the like.

**[0035]** Next, an embodiment of dealing with shield will be described.

**[0036]** Fig. 11 and Fig. 12 show examples of structure of an FPC covered with a shield material.

**[0037]** First, as shown in Fig. 11, transducer unit 1 is made into a cylindrical shape, and each section 2 of the FPC divided by slits is processed into a spiral shape. Each section of FPC 2 is insulated with resin tube 13 being an insulating material. The outside of resin tube 13 is attached with first shield material 20, such as a conductive tape. The shield material is made of conductive spiral tube or cross tube having high flexibility and high shield effect.

**[0038]** Next, as shown in Fig. 12, a set of the FPC assembled in Fig. 11 is contained within flexible tube 8 being a protection material via second shield material 21 covering the outside of cable. Second shield material 21 may be made of the same material as first shield material 20, or a braided shield used in a coaxial cable. Because both first shield material 20 and second shield material 21 are made of conductive material, they are electrically connected by arranging them so as to touch each other. By connecting first shield material 20 and second shield material 21, shield efficiency is further improved in this construction.

**[0039]** Further, instead of using the above first shield material, metallic powder of gold, silver, copper, brass, aluminum, and the like may be evaporated onto the surface of the resin tube being a insulating material which protects the spiral flexible circuit board.

**[0040]** It is also possible to arrange only second shield material 21 or the protection material, or both of them on the outer circumference of the bundled sections spirally wound of the above flexible circuit board without interposition of the insulating material and first shield material 20. In this case, by evaporating metallic powder of gold, silver, copper, brass, aluminum, or the like onto the surface of the protection material used as insulating material, the protection material serve as the second shield material.

**[0041]** Further, although a detailed description is omitted, it is needless to say that the present invention is applicable to every kind of intracavitary ultrasound probe including the convex type ultrasound probe mentioned in Fig. 6 and an ultrasound probe mentioned in Fig. 7.

**[0042]** As described above, by constructing an ultrasound probe so as to install a shield on a spiral flexible circuit board using a material having a shield effect, it becomes possible to shut off an electromagnetic wave noise affecting an ultrasound image generated by other electronic devices and medical devices used at the same time when a signal is extracted from a transducer to an ultrasound probe, whereby a clear ultrasound image can be provided.

## Claims

1. An ultrasound probe comprising: transducers for transmitting and receiving an ultrasound respectively located in correspondence with adjacent positions of transmission and reception; and a one- or two-layer flexible circuit board located in correspondence with the positions of transmission and reception, in which signal lines for supplying a transmission signal and extracting a reception signal to/from the positions are installed in a longitudinal direction of the transducers at a predetermined angle, wherein the flexible circuit board has slits dividing signal lines at each of the positions at the predetermined angle, and each section of the flexible circuit board divided by the slits are spirally wound.
2. An ultrasound probe according to claim 1, wherein a member is provided around each section spirally wound of the flexible circuit board.
3. An ultrasound probe according to claim 2, wherein the member is an insulating material covering a circumference of each section of the flexible circuit board and a first shield material, or an insulating material to which a layer of metallic powder is evaporated, covering the circumference of each part .
4. An ultrasound probe according to claim 2, wherein the member is a single second shield material or a protection material covering an outer circumference of bundled sections of the flexible circuit board, or a protection material to which a layer of metallic powder is evaporated on its surface.
5. An ultrasound probe according to claim 3, wherein the member includes a single second shield material or a protection material covering the outer circumference of bundled sections of the flexible circuit board, or a protection material to which a layer of metallic powder is evaporated on its surface.
6. An ultrasound probe according to claim 4, wherein the protection material is a flexible tube.
7. An ultrasound probe according to claim 4 or 5, wherein the protection material covers the outer circumference of bundled sections of the flexible circuit board, which has a stiff section and a flexible section.
8. An ultrasound probe according to claim 3, wherein the member includes a single second shield material covering the outer circumference of bundled sections of the flexible circuit board and a protection material installed inside or outside the second shield material, or a protection material to which a layer of metallic powder is evaporated on its sur-

face.

9. An ultrasound probe according to claim 2, wherein a signal line is provided on one layer of the two-layer flexible circuit board, and a ground line is provided on the other layer. 5

10

15

20

25

30

35

40

45

50

55

Fig.1

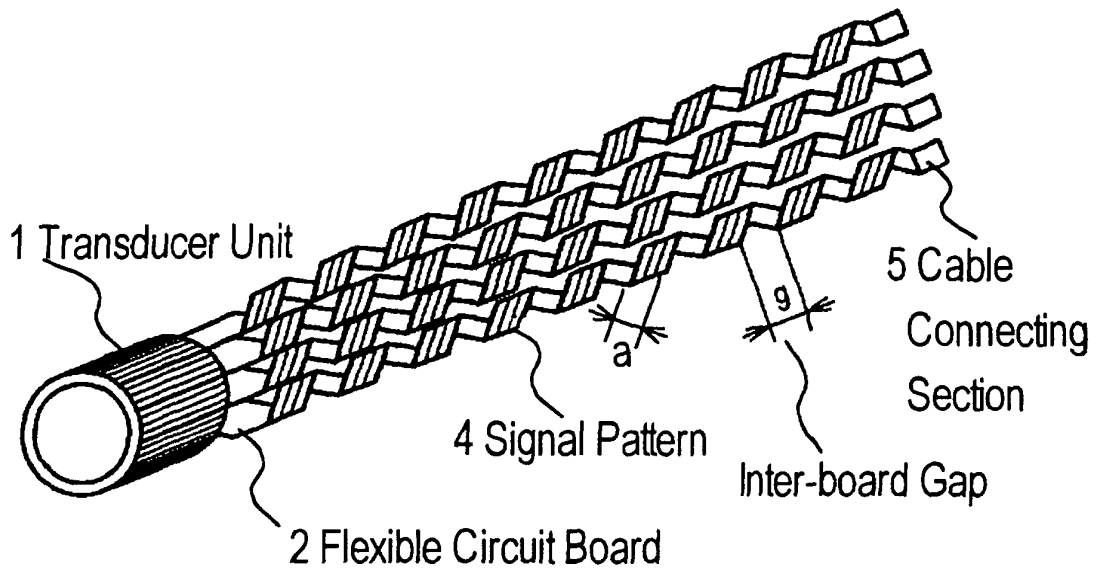


Fig.2

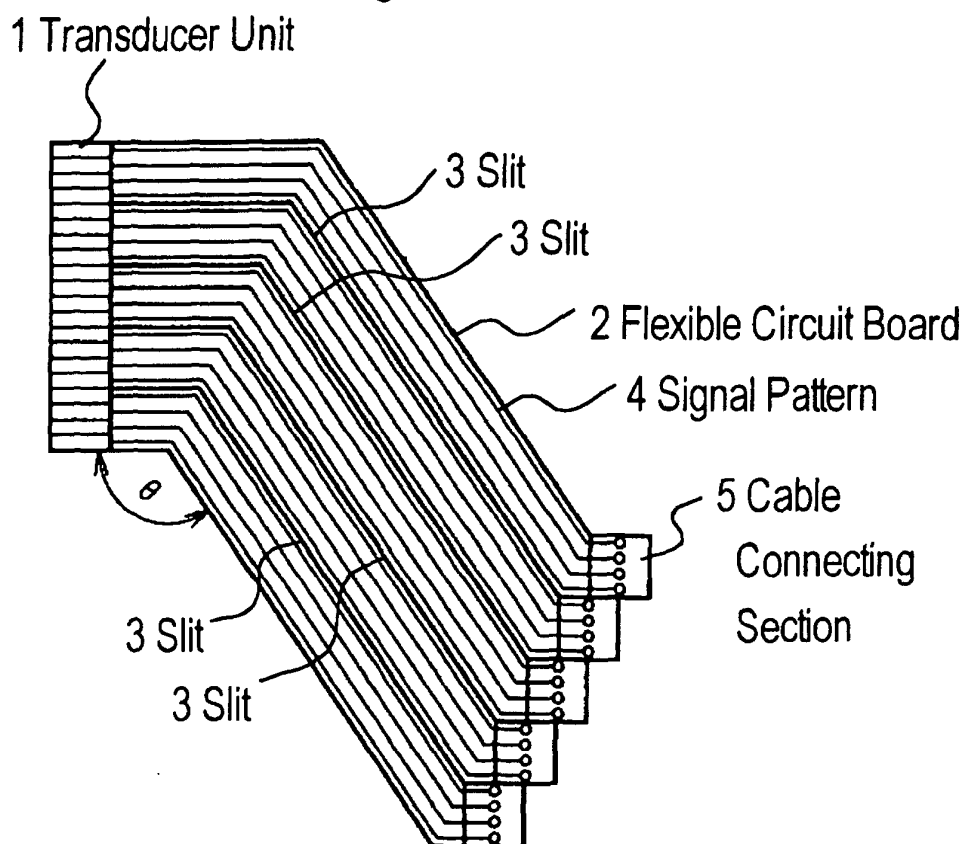


Fig.3

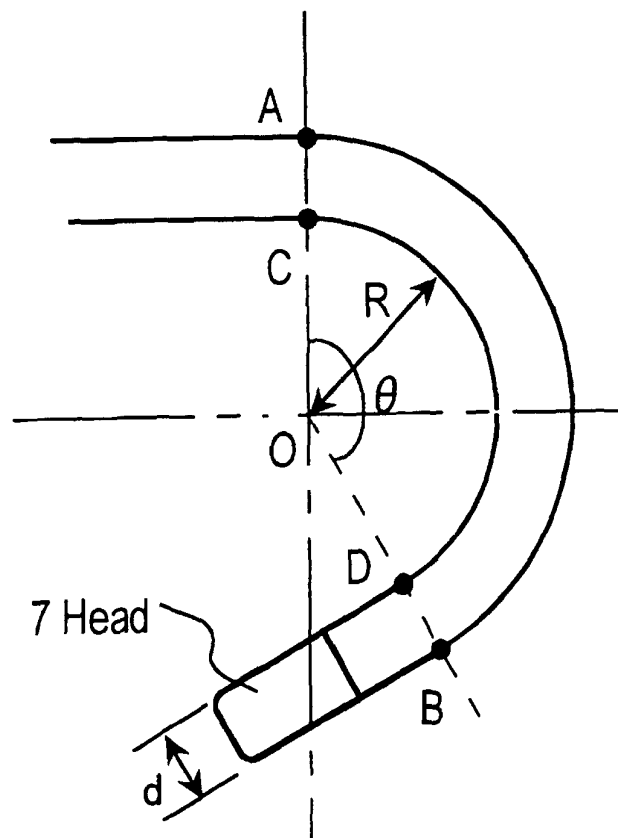




Fig.4(a)

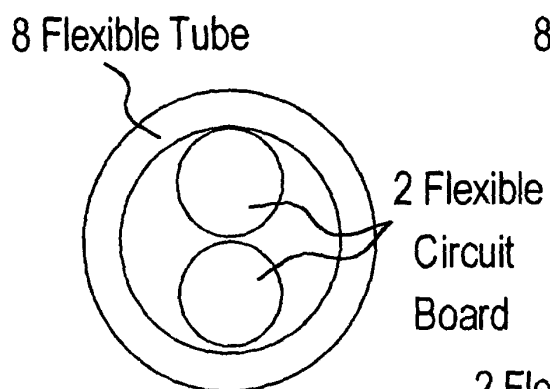


Fig.4(b)

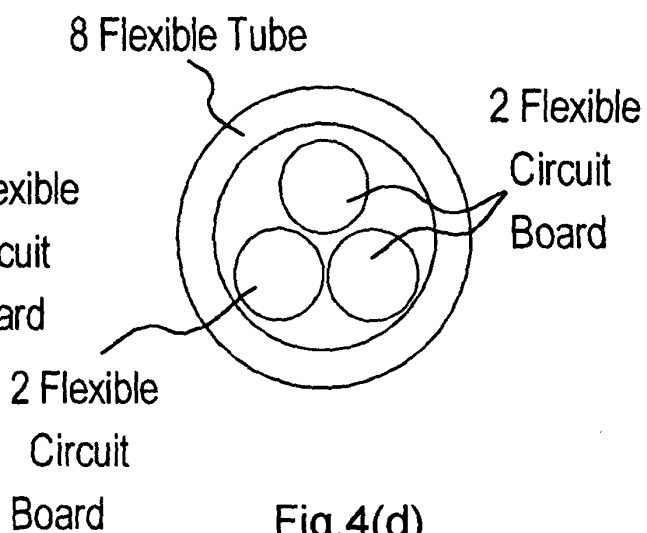


Fig.4(c)

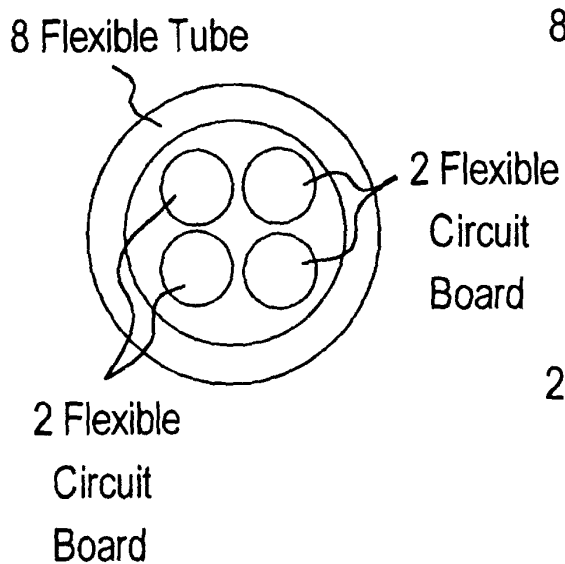


Fig.4(d)

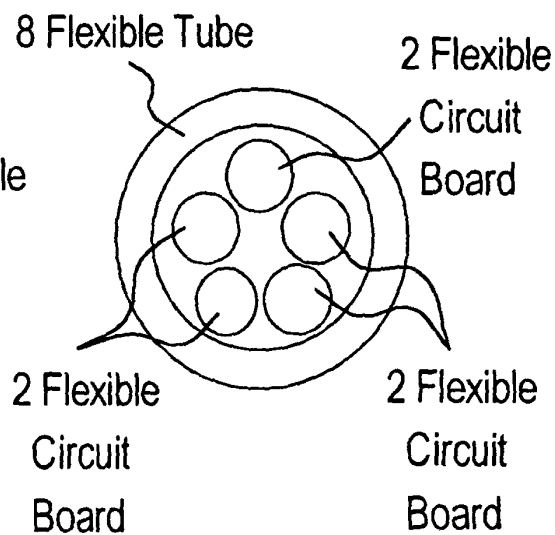


Fig.5(a)

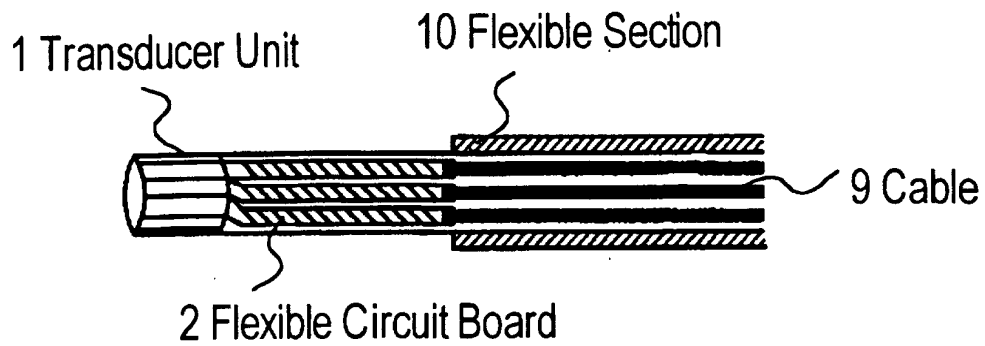


Fig.5(b)

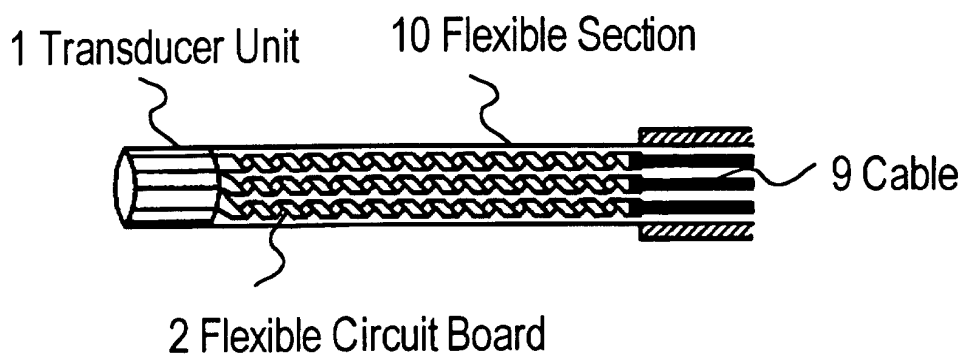


Fig.5(c)

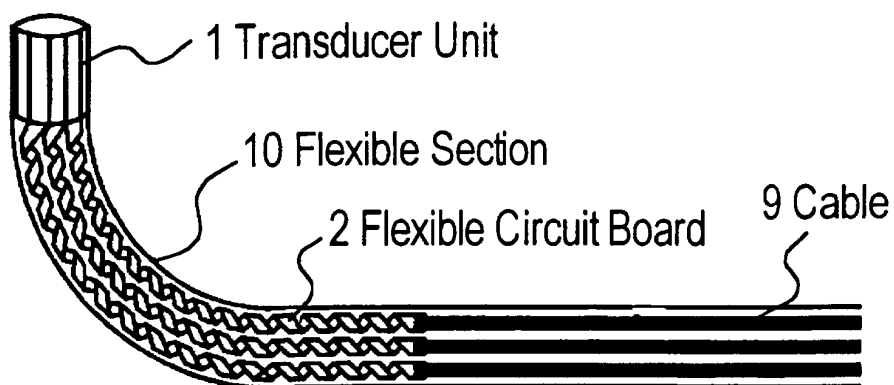


Fig.6

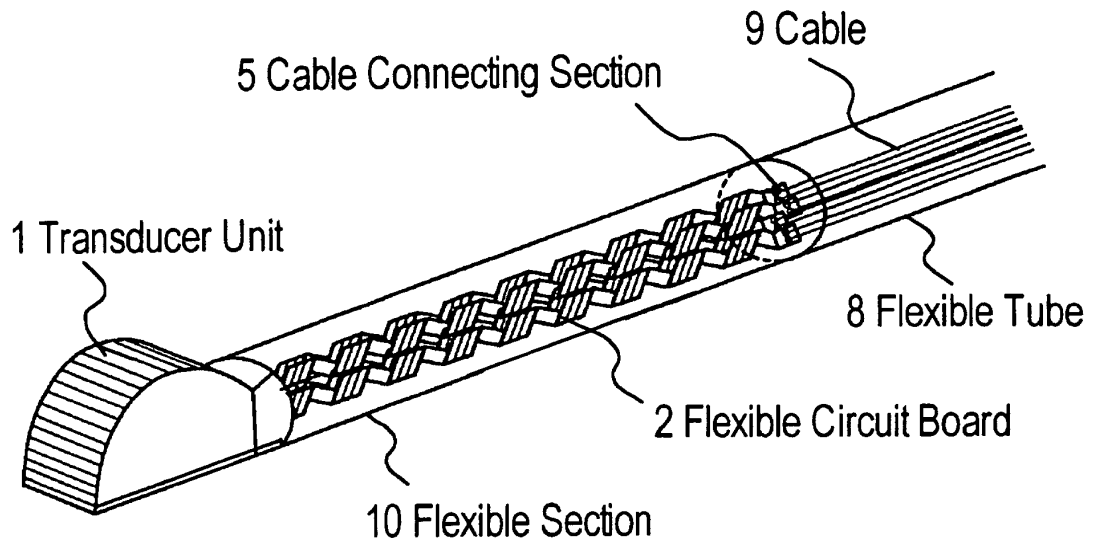


Fig.7

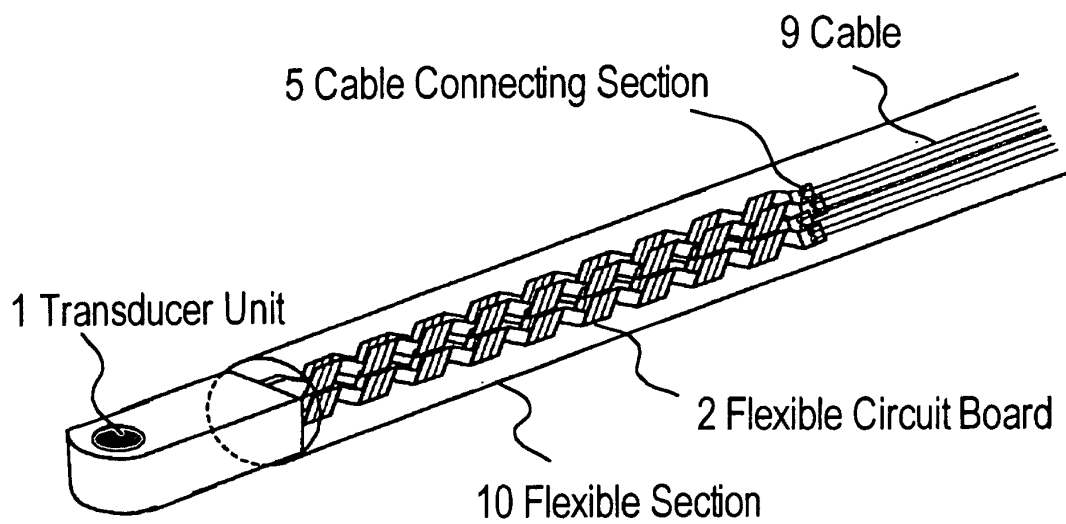


Fig.8

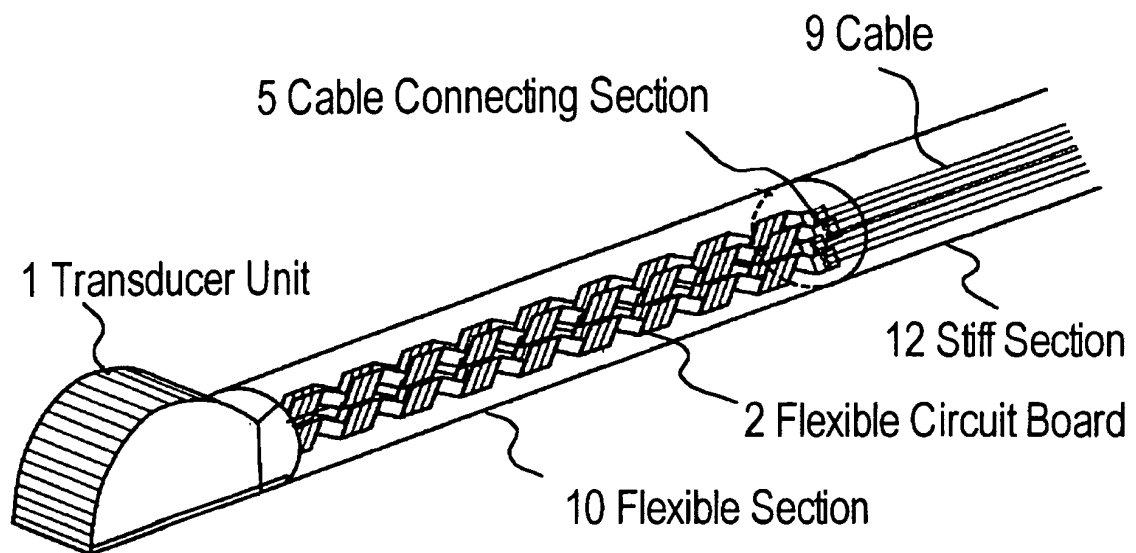


Fig.9(a)

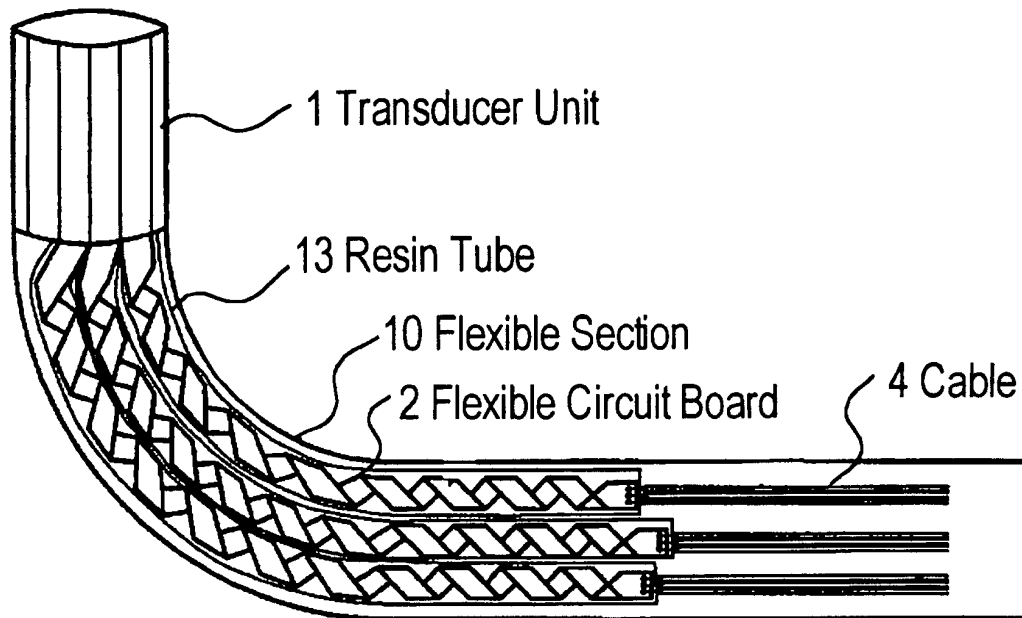


Fig.9(b)

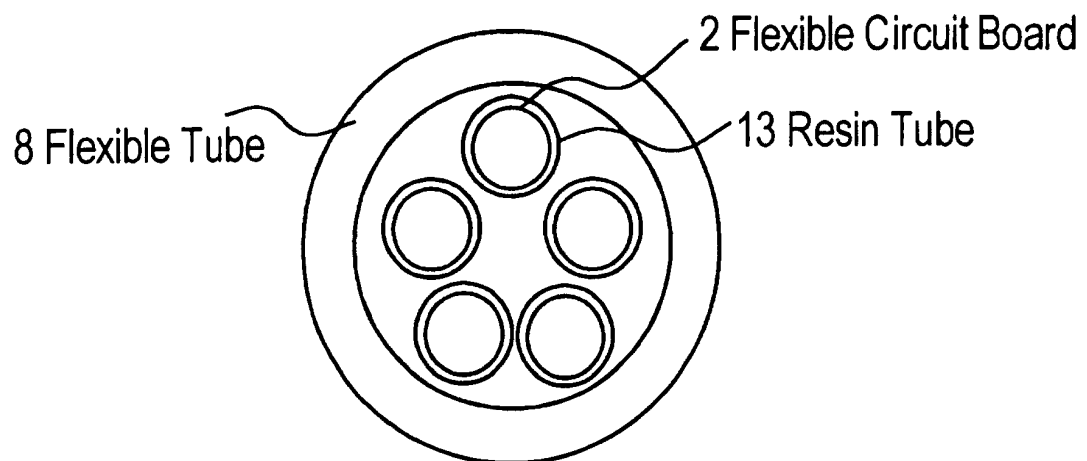


Fig.10(a)

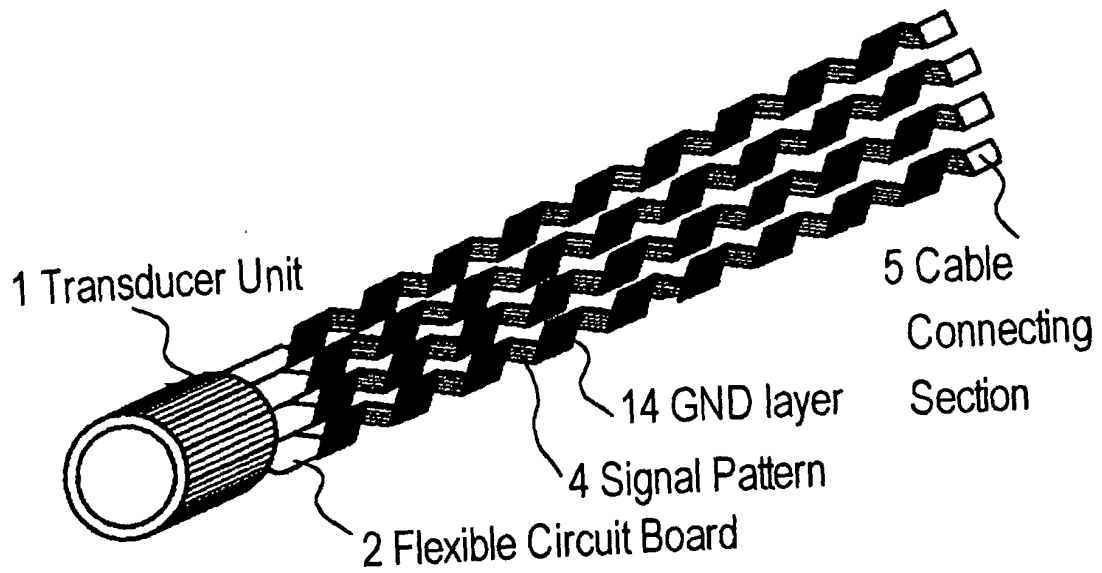


Fig.10(b)

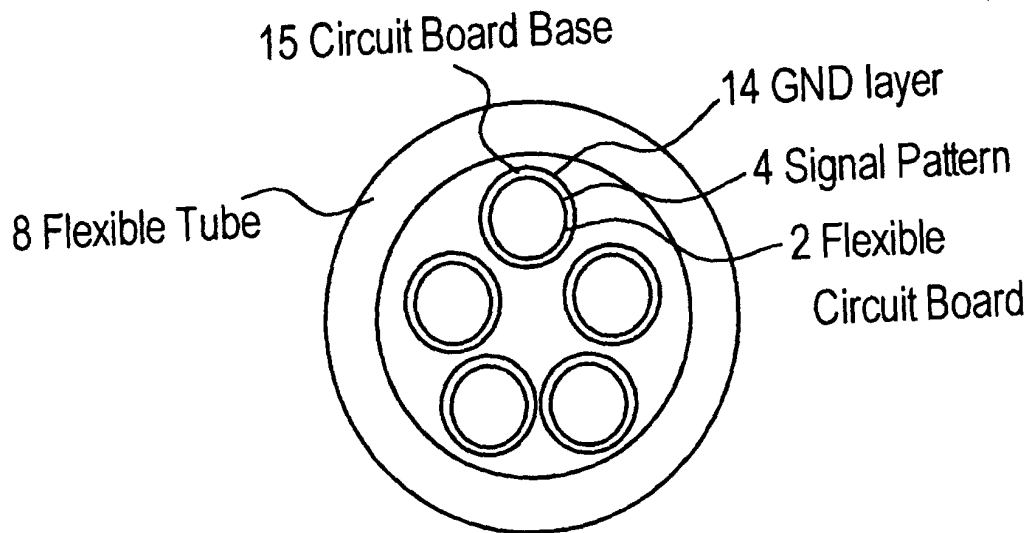


Fig.11


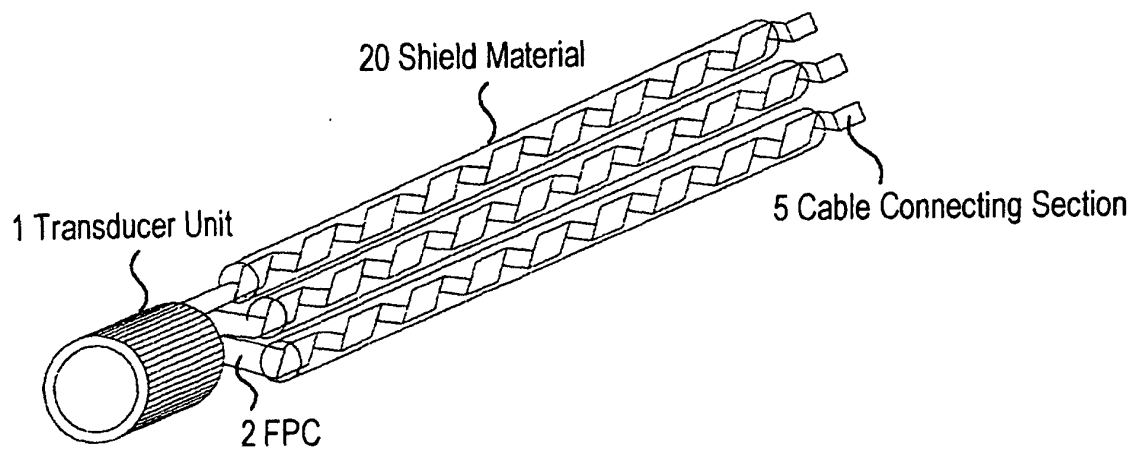


Fig.12

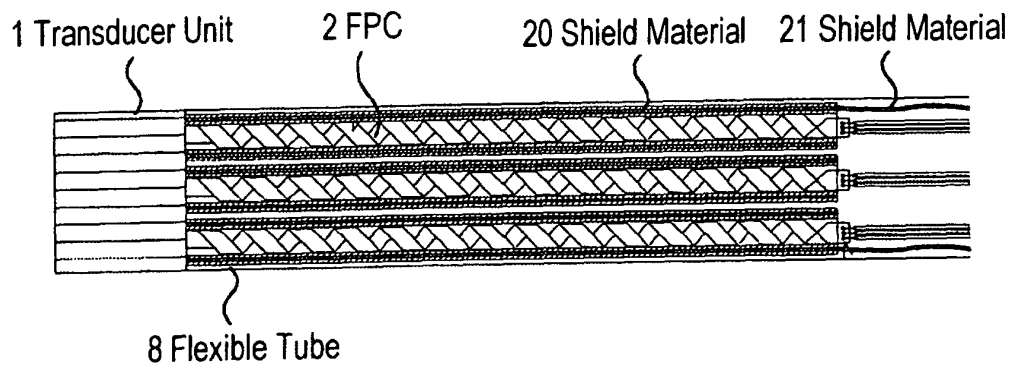

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP03/04287

A. CLASSIFICATION OF SUBJECT MATTER  
Int.Cl<sup>7</sup> A61B8/12

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

Int.Cl<sup>7</sup> A61B8/00-8/15, A61B1/00-1/32

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Jitsuyo Shinan Koho 1922-1996 Toroku Jitsuyo Shinan Koho 1994-2003  
Kokai Jitsuyo Shinan Koho 1971-2003 Jitsuyo Shinan Toroku Koho 1996-2003

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y A	JP 2-271843 A (Olympus Optical Co., Ltd.), 06 November, 1990 (06.11.90), Full text; all drawings (Family: none)	1-2, 4-9 3
Y A	JP 11-305143 A (Toshiba Corp.), 05 November, 1999 (05.11.99), Full text; all drawings (Family: none)	1-2, 4-9 3
Y A	CD-ROM of the specification and drawings annexed to the request of Japanese Utility Model Application No. 61854/1991 (Laid-open No. 13408/1993) (Yokogawa Medical Systems, Ltd.), 23 February, 1993 (23.02.93), Full text; all drawings (Family: none)	1-2, 4-9 3

☒ Further documents are listed in the continuation of Box C.

☐ See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not  
considered to be of particular relevance  
"E" earlier document but published on or after the international filing  
date  
"L" document which may throw doubts on priority claim(s) or which is  
cited to establish the publication date of another citation or other  
special reason (as specified)  
"O" document referring to an oral disclosure, use, exhibition or other  
means  
"P" document published prior to the international filing date but later  
than the priority date claimed

"T" later document published after the international filing date or  
priority date and not in conflict with the application but cited to  
understand the principle or theory underlying the invention  
"X" document of particular relevance; the claimed invention cannot be  
considered novel or cannot be considered to involve an inventive  
step when the document is taken alone  
"Y" document of particular relevance; the claimed invention cannot be  
considered to involve an inventive step when the document is  
combined with one or more other such documents, such  
combination being obvious to a person skilled in the art  
"&" document member of the same patent family

Date of the actual completion of the international search  
30 April, 2003 (30.04.03)

Date of mailing of the international search report  
20 May, 2003 (20.05.03)

Name and mailing address of the ISA/  
Japanese Patent Office

Authorized officer

Facsimile No.

Telephone No.



## INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP03/04287

## C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y A	JP 2001-224590 A (Matsushita Electric Industrial Co., Ltd.), 21 August, 2001 (21.08.01), Full text; all drawings (Family: none)	4-8 1-3,9
Y A	JP 7-116168 A (Terumo Corp.), 09 May, 1995 (09.05.95), Full text; all drawings (Family: none)	4-8 1-3,9
Y A	Microfilm of the specification and drawings annexed to the request of Japanese Utility Model Application No. 27183/1986 (Laid-open No. 140451/1987) (Fujitsu Ltd.), 04 September, 1987 (04.09.87), Full text; all drawings (Family: none)	9 1-8
A	JP 62-272222 A (Olympus Optical Co., Ltd.), 26 November, 1987 (26.11.87), Full text; all drawings (Family: none)	1-9

Form PCT/ISA/210 (continuation of second sheet) (July 1998)

专利名称(译)	超声探头在体腔内		
公开(公告)号	<a href="#">EP1498071A1</a>	公开(公告)日	2005-01-19
申请号	EP2003746424	申请日	2003-04-03
[标]申请(专利权)人(译)	株式会社日立医药		
申请(专利权)人(译)	日立医疗器械股份有限公司		
当前申请(专利权)人(译)	日立医疗器械股份有限公司		
[标]发明人	YAGI TOMOYUKI ITO TAKASHI IZUMI MIKIO		
发明人	YAGI, TOMOYUKI ITO, TAKASHI IZUMI, MIKIO		
IPC分类号	A61B8/12 B06B1/06 G01N29/22 G01N29/24		
CPC分类号	B06B1/0622 A61B8/12 A61B8/445 A61B8/4483 A61B2562/222 G01N29/225 G01N29/2487 H01R12/594 H01R12/63 H01R2201/12		
优先权	2002114333 2002-04-17 JP		
其他公开文献	EP1498071B1 EP1498071A4		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

为了使探头小型化，增加通道数，并提高柔性部分的灵活性，超声探头包括具有多个用于发送和接收超声波的通道的换能器单元1，以及连接到换能器的各个通道的柔性电路板2单元1，其中提供了用于提供发送信号并向/从换能器单元1提取接收信号的信号线，其中柔性电路板2形成至少两个通过划分多个通道并单独螺旋缠绕而形成的通道块。

Fig.1

