

(19)



Europäisches Patentamt

European Patent Office

Office européen des brevets

(11)



EP 1 602 331 A1

(12)

EUROPEAN PATENT APPLICATION

published in accordance with Art. 158(3) EPC

(43) Date of publication:

07.12.2005 Bulletin 2005/49

(51) Int Cl. 7: **A61B 8/00**

(21) Application number: 04715496.8

(86) International application number:
PCT/JP2004/002387

(22) Date of filing: 27.02.2004

(87) International publication number:
WO 2004/075753 (10.09.2004 Gazette 2004/37)

(84) Designated Contracting States:

AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT RO SE SI SK TR

Designated Extension States:

AL LT LV MK

(30) Priority: 27.02.2003 JP 2003052038

(71) Applicant: HITACHI MEDICAL CORPORATION
Tokyo 101-0047 (JP)

(72) Inventors:

- KONDO, Toshiro
Sanuki-shi, Kagawa 7692402 (JP)
- OSAWA, Takaya
Kitakatsushima-gun, Saitama 3450025 (JP)


(74) Representative: Strehl Schübel-Hopf & Partner
Maximilianstrasse 54
80538 München (DE)

(54) ULTRASONIC PROBE

(57) An ultrasound probe obtained by arranging, on a backing 10, a plurality of transducers each of which comprising a piezoelectric transducer 20, an acoustic lens 40, and an acoustic matching layer provided be-

tween the piezoelectric transducer 20 and the acoustic lens 40, the acoustic matching layer containing a fibrous material, and the direction of fibers in the fibrous material being perpendicular to the direction of sound waves.

Fig. 5

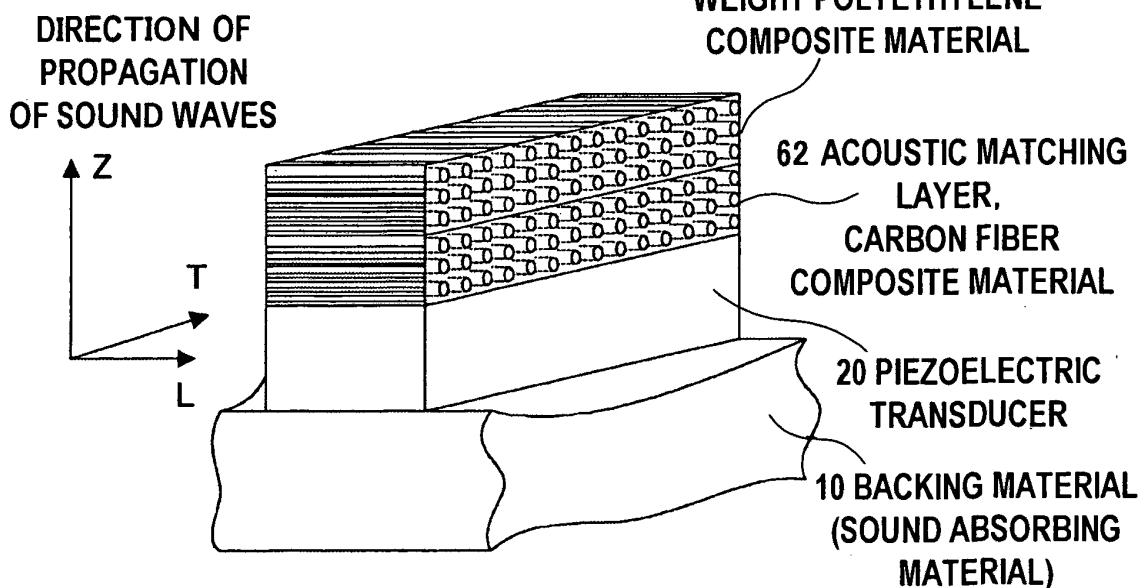

Description

Technical Field

5 [0001] This invention relates to a probe in an ultrasound diagnostic apparatus and, particularly, to a transducer in an electronic scanning probe.

Background Art

10 [0002] A probe in an electronic scanning ultrasonic diagnostic apparatus that transmits and receives ultrasonic waves has heretofore been constituted by arranging, on a backing material, a plurality of transducers each of which comprising a piezoelectric transducer, an acoustic lens, and an acoustic matching layer provided between the piezoelectric transducer and the acoustic lens.

15 [0003] In this probe, a transducer of a narrow width having the acoustic matching layer vibrates accompanied, however, by a deformation in the direction of thickness, by a deformation in the direction of width and, hence, by a reduction in the conversion efficiency in the direction of thickness. Further, since the vibration in the direction of width interferes with the vibration in the direction of thickness, the surface of the transducer goes out of vibration of a uniform amplitude deteriorating the image of the ultrasonic diagnostic equipment.

20 [0004] A probe obtained by arranging the vibrators that have a fibrous material dispersed in the acoustic matching layer has been disclosed in JP-A-10-75953. However, this fibrous material is used for realizing a low heat conduction, and the direction of fiber has not been set by taking the Young's modulus of the fiber and the Poisson's ratio into consideration. Therefore, the above problem cannot be solved by the above prior art.

Disclosure of the Invention

25 [0005] This invention is concerned with an ultrasound probe obtained by arranging, on a backing, a plurality of transducers each of which comprising a piezoelectric transducer, an acoustic lens, and an acoustic matching layer provided between the piezoelectric transducer and the acoustic lens, the acoustic matching layer containing a fibrous material, and the direction of fibers in the fibrous material being perpendicular to the direction of sound waves.

30 Brief Description of the Drawings

[0006]

35 Fig. 1 is a view illustrating the internal structure of an ultrasound probe according to the present invention;
 Fig. 2 is a diagram illustrating a propagation model of sound waves of the probe;
 Fig. 3 is a diagram illustrating a model of an equivalent circuit of a passage through which the sound waves propagate from the piezoelectric transducer in the probe to the human body;
 Fig. 4 is a view illustrating, in detail, the internal structure of an ultrasound probe according to the invention;
 40 Fig. 5 is a view illustrating a first embodiment of the invention;
 Fig. 6 is a view illustrating the characteristics of a composite material including a fibrous material of the invention;
 Fig. 7 is a diagram illustrating the characteristics of a composite material including the fibrous material of the invention;
 Fig. 8 is a diagram illustrating the effect of the invention;
 45 Fig. 9 is a view illustrating a second embodiment of the invention;
 Fig. 10 is a view illustrating a third embodiment of the invention;
 Fig. 11 is a view illustrating a fourth embodiment of the invention; and
 Fig. 12 is a diagram illustrating an ultrasonic apparatus as a whole.

50 Best Mode for Carrying Out the Invention

[0007] Referring to Fig. 1, there are arranged many slender and rod-like piezoelectric transducers 20 having a narrow width made of PZT on a sound-absorbing (backing) material 10, which are covered with an acoustic lens 40 of a shape arcuately swelling outward in a direction at right angles with the direction of arrangement thereof and with an acoustic matching layer 31 and an acoustic matching layer 32 that are provided between the transducers 20 and the acoustic lens 40. Lead wires 50 are connected to the electrodes of the vibrators.

[0008] The PZT has been extensively used as a piezoelectric transducer of the ultrasonic probe. Acoustic impedances of the PZT and the living body or water of $Z_0 = 35 \times 10^6$ [kg/m² • s] and $Z_M = 1.5 \times 10^6$ [kg/m² • s], respectively.

There is a large difference between these values. From the standpoint of impedance matching, the matching cannot be quite accomplished if the PZT is brought into contact with the living body. Therefore, the acoustic matching layers 31 and 32 are provided on the front surface of the transducer to bring the acoustic impedance of the transducer 20 into match with the acoustic impedance of the living body. This enables the vibration of the transducer 20 to be efficiently propagated into the living body.

[0009] The epoxy and the polyurethane used for the acoustic matching layers 31 and 32 have acoustic impedances of 2 to 3 [MRayl]. Since the living body has an acoustic impedance of 1.5 [MRayl], it is most desired to use the epoxy or the polyurethane on the upper surface of the acoustic matching layer of the two-layer constitution. As the lower layer of the acoustic matching layer, it is necessary to use a material having an acoustic impedance lying between that of the vibrator and that of the upper layer of the acoustic matching layer. Therefore, a powder of a substance having a relatively large density is mixed into the epoxy or polyurethane resin to adjust the value that meets the lower surface of the acoustic matching layer.

[0010] The reflection coefficient R on the interface between the PZT and the living body is given by the formula (1) like the case of an electric circuit,

$$R = \frac{|Z_M - Z_0|}{|Z_M + Z_0|} \quad (1)$$

[0011] In an electric circuit, it is a practice to insert a $\lambda/4$ matching circuit in the circuit. Here, λ is a wavelength of signals that propagate. A matching layer for propagating ultrasonic waves of the probe will now be considered based on a model shown in Fig. 2. Fig. 3 shows its equivalent circuit. Z_0 , Z_1 , Z_2 and Z_M denote acoustic impedances of the piezoelectric vibrator, the matching layer (1), the matching layer (2) and the human body.

[0012] Z_0 and Z_M have been given. Optimum values of characteristic impedances Z_1 and Z_2 can be determined by calculation by using a coaxial cable put between a signal source and a receiving end to minimize the reflection at the terminals of the coaxial cable having characteristic impedances Z_1 and Z_2 ("REVISED HANDBOOK OF ULTRASONIC EQUIPMENT FOR MEDICAL USE" compiled by the, Foundation, Japanese Industrial Association of Electronic Machines, published by Corona Co., January 20, 1997, pp. 29-30). Table 1 shows optimum acoustic impedances of the acoustic matching layer of a thickness of $1/4$ wavelength.

Table 1:

Optimum acoustic impedances of $1/4$ wavelength acoustic matching layer.						
Acoustic impedance of piezoelectric vibrator	Acoustic impedance Z_i of matching layer					Acoustic impedance Z_M of human body
	1	2	3	4	5	
34	4.25	/	/	/	/	1.5
	8.92	2.34	/	/	/	
	14.79	4.24	1.85	/	/	
	20.55	7.51	2.74	1.66	/	
	25.26	12.01	4.46	2.12	1.58	

(Note): Unit is all by $\times 10$ [kg/m² · s]

[0013] An optimum method of designing the probe using the equivalent circuit is based on a wave equation of sound waves by taking into consideration only the sound waves that propagate in the longitudinal direction. It is presumed that no deformation in the transverse direction occurs in the matching layer.

[0014] The backing material 10 is provided on the back surface of the ultrasound transducer, so that ultrasonic waves coming out from the back surface will not return back to the surface of the transducer, and is made of a material which attenuates the ultrasonic waves to a large degree.

[0015] Fig. 4 is a view illustrating the probe in detail. The piezoelectric transducer 20 exists on the backing member 10, and the acoustic matching layers 31, 32 are provided on the piezoelectric transducer 20. There exists a small gap among the vibrators which are each constituted by the piezoelectric transducer 20, acoustic matching layers 31, 32,

and acoustic lens.

[0016] Here, described below in detail as a first embodiment is the structure of a probe using a composite material as the matching layers. Fig. 5 illustrates a transducer in this probe. The transducer is constituted by two matching layers and a piezoelectric transducer. A fibrous material is contained in the two matching layers. The direction of fibers of the fibrous material is perpendicular to the direction of propagation of sound waves and is, further, perpendicular to the lengthwise direction of the transducer. The transducers of this structure are arranged in many number on the backing material 10 thereby to constitute an array-type probe. Concretely, the matching layer 61 uses a composite material of a carbon fiber and an epoxy base material which contains a tungsten powder. The matching layer 62 uses a composite material of a polyurethane base material and an ultrahigh molecular weight polyethylene fiber. The composite material used for either of these matching layers have densities and Young's moduli in a direction in which the ultrasonic waves propagate, which can be adjusted to be nearly the same as those of the base materials and, hence, their acoustic impedances can be adjusted to assume nearly the same values. The Young's moduli become very large values in the direction of fiber contributing greatly to improving the characteristics of the probe.

[0017] Next, described below in detail are the contents of the matching layers. Fig. 6(a) is a one-direction reinforcing plate obtained by arranging the fibers in the same direction. This material is symmetrical on the LZ plane, on the TZ plane or on the LT plane. Here, the axes L, T and Z are referred to as anisotropic main axes (elastic main axes, principal axes), which in Fig. 6 (a) are referred to as orthotropy in which the main axes are meeting each other at right angles.

[0018] When a stress σ_L is exerted in a direction L in Fig. 6 (b), the strain are given by the formulas (2),

$$20 \quad \varepsilon_T = \frac{V_{LT}\sigma_L}{E_L}, \quad \varepsilon_L = \frac{\sigma_T}{E_L}. \quad (2)$$

25 where E_L is a Young's modulus when pulled in the direction L, and v_{LT} is a Poisson's ratio representing the ratio of contraction in the direction T when pulled in the direction L. Similarly, when a stress σ_T is exerted in the direction T in Fig. 6(b), the strain are given by the formulas (3),

$$30 \quad \varepsilon_T = \frac{\sigma_T}{E_T}, \quad \varepsilon_L = \frac{V_{TL} - \sigma_T}{E_T} \quad (3)$$

[0019] On the other hand, a relationship of the formula (4) holds between the shearing stress and the shearing strain,

$$35 \quad \gamma_{LT} = \frac{\tau_{LT}}{G_{LT}} \quad (4)$$

[0020] Therefore, when a combined stress acts as shown in Fig. 6(b), a relationship between the stress and the strain can be expressed by a matrix of the formula (5),

$$40 \quad \begin{bmatrix} \varepsilon_L \\ \varepsilon_T \\ \gamma_{LT} \end{bmatrix} = \begin{bmatrix} 1/E_L & -v_{TL}/E_T & 0 \\ -v_{LT}/E_L & 1/E_T & 0 \\ 0 & 0 & 1/G_{LT} \end{bmatrix} \begin{bmatrix} \sigma_L \\ \sigma_T \\ \tau_{LT} \end{bmatrix} \quad (5)$$

[0021] This is the Hooke's law of an ortho-anisotropic thin plate related to the axes LT.

55 [0022] The isotropic material has two independent elastic constants, but there are appearing five constants E_L , E_T , v_{LT} , v_{TL} and G_{LT} in the formula (5). However, a relationship of the formula (6) called (Betti) reciprocal theorem has been theoretically verified, and the ortho-anisotropic thin plate has four independent elastic constants.

$$\frac{v_{LT}}{E_l} = \frac{v_{TL}}{E_T} \quad (6)$$

5 [0023] These are called basic elastic constants. The elastic constants can be estimated to some extent from the properties of the fibers and the base materials, and are derived from a model that is considered as described below.

10 [0024] The fiber usually has a circular shape in cross section and is surrounded by the base material. Here, as shown in Fig. 7, the fiber and the base material are collected separately. When pulled in the direction L, this material is elongated like when a bundle of springs that elongate little and springs that elongate much is pulled, and the following formula (7) will be derived as a result of simple calculation,

$$E_L = E_f V_f + E_m (1 - V_f) \quad (7)$$

15 where E_f and E_m are Young's moduli of the fiber and the mother member, and V_f is a volume content of the fiber.

[0025] The fiber and the mother member arranged in parallel in the direction L are called parallel model which is shown in Fig. 7.

[0026] Next, when pulled in the direction T in Fig. 6, the material becomes analogous to the connection of a strong spring of the length V_f and a weak spring of the length $(1 - V_f)$ as expressed by the formula (8),

$$\frac{1}{E_T} = \frac{V_f}{E_f} + \frac{1 - V_f}{E_m} \quad (8)$$

25 [0027] Based upon the idea of the above series and parallel models, the Poisson's ratio v_{LT} and the shearing elastic coefficient G_{LT} can be found from the formulas (9) and (10),

$$v_{LT} = v_f V_f + v_m (1 - V_f) \quad (9)$$

$$\frac{1}{G_{LT}} = \frac{V_f}{G_f} + \frac{1 - V_f}{G_m} \quad (10)$$

30 [0028] The above idea is called a strength-of-material method in the microscopic elasticity. The above formula (7) is called the composite rule (of modulus of elasticity)(M. Domoto, R. Yamamoto, "Composite Materials", published by the University of Tokyo, April 15, 1993, pp. 39-45).

35 [0029] Tables 3 and 4 show physical properties of the carbon fiber and of an ultrahigh molecular weight polyethylene fiber used for a composite material (a catalogue of carbon fibers of Toyo Rayon Co. , material No. 2 , revised 17 . 4 . 40 1, and Dieniema catalog A1703K of Toyo Boseki Co.).

Table 3:

Examples Properties of a carbon fiber.					
Name		Tensile modulus of elasticity		Fiber dia.	Density
Grade		Tensile Modulus		Filament Dia.	Density
		Tonf/mm ²	Gpa	Micrometer	g/cm ³
HTA	-W05K	24.0	235	7.0	1.76
IM600	-6K	29.0	285	5.0	1.80
UM46	-12K	44.5	435	4.7	1.82
UM68	-12K	66.0	650	4.1	1.97

Table 4:

Physical properties of an ultrahigh molecular weight polyethylene fiber.				
Grade	Mod. of elasticity		Filament dia.	Density
	(cN/dtex)	(Gpa)	(μm)	(g/cm3)
SK60	880 - 1230	88 - 123	12	0.97
SK71	1230 -	123 -	12	0.97

[0030] Table 5 shows physical properties of an epoxy resin used as the mother member (Asahi Amidas Co./"Plastics" Compiling Dpt., "Plastics Data Book", published by Kogyo Chosakai Publishing Co., December 1, 1999, p. 267).

Table 5:

Mechanical properties of a bisphenol epoxy resin cured with various curing agents.				
Composition		Liquid epoxy resin (epoxy equivalent: 180 -190)		
Properties	Standards	Polyamine	Amine adduct	Polyamide
Specific gravity (kg/cm ³)	VSM77109	1.15 - 1.20	1.15 - 1.20	1.1 - 1.2
Mod. of elasticity (kg/mm ²) [Gpa]	VSM77111	350 - 400 [3.43 - 3.92]	350 - 400 [3.43 - 3.92]	340 - 390 [3.33-3.82]

Araldite GY250 of Chiba Co. was used.

[0031] The polyurethane used for the matching layers has a tensile modulus of elasticity of 0.88 [kgf/mm²]. The carbon fiber or the ultrahigh molecular weight polyethylene has a modulus of elasticity (Young's modulus) which is different by at least not less than 22 times from that of the epoxy resin or the polyurethane used as the mother member. The carbon fiber having the greatest modulus of elasticity is different by about 200 times from the modulus of elasticity of the epoxy resin. The kind of the fiber can be arbitrarily selected by the manufacturer depending upon the use.

[0032] In an ordinary composite material, the content of the fiber is up to 50% (H. Morimoto, "Plastic Frontier Composite Materials", published by Kobunshi Kankokai, October 5, 1998, pp. 133-134).

[0033] In the formula (7), therefore, if it is presumed that $V_f = 0.6$, there holds $E_f/E_m > 20$ to 200 as described above, from which it is considered that $E_f \gg E_m$. In the composite material, therefore, the approximation can be made such that,

$$E_L \doteq E_f V_f \quad (11)$$

[0034] It can therefore be so considered that E_L is almost dependent upon the physical properties of the fiber. From the formula (8), on the other hand, E_T can be given by the following formula,

$$E_T = \frac{1}{\frac{V_f}{E_f} + \frac{1-V_f}{E_m}} \quad (12)$$

[0035] In the formula (12), too, $V_f = 0.2$ to 0.4 and $E_f \gg E_m$ and, hence, there holds $V_f/E_f \ll (1 - V_f/E_m)$. Therefore, E_T is given by the formula (13),

$$E_T \doteq \frac{E_m}{(1 - V_f)} \quad (13)$$

[0036] It can therefore be so considered that E_T is almost dependent upon the physical properties of the base material.

[0037] From the formula (6), the Poisson's ratio ν_{TL} that represents the ratio of elongation of the composite material in the direction of fiber (direction L) by compressing it in the direction (direction T) perpendicular to the direction of fiber is given by the following formula (14),

$$v_{TL} = v_{LT} \frac{E_T}{E_L} \quad (14)$$

5 [0038] where v_{LT} is the Poisson's ratio of the composite material of when it is compressed in the direction of fiber. In a typical carbon fiber composite material as shown in Table 6, $v_{LT} = 0.3$ (H. Morimoto, "Frontier Composite Materials", published by Kobunshi Kankokai (Kyoto), October 5, 1998, p. 135).

Table 6:

Compressive modulus of elasticity, Poisson's ratio and density ²¹⁾ of the carbon fiber composite materials depending upon the kind of carbon fibers.				
	Standard type	Highly strong type	Highly elastic type	Ultra-highly elastic type
Compressive modulus of elasticity, 0°C, kgf/mm ² (Gpa)	15400 (152)	14700 (145)	17430 (172)	31.5 (314)
Poisson's ratio	0.3	0.3	0.27	0.3
Density g/cm ³	1.58	1.61	1.59	1.83
(Note) (1) Constitution: CF/epoxy (60 to 65 vol%) H. Morimoto: Frontier Composite Material, Kobunshi Kankokai (Kyoto) 1998, p. 135 (2) Kind: Tensile modulus of elasticity of carbon fiber Standard type (23100 to 23800 kgf/mm ²) Highly strong type (24500 to 31500 kgf/mm ²) Highly elastic type (35000 to 38500 kgf/mm ²)				

30 [0039] From Table 3, further, the Young's modulus E_L of the composite material may be $E_L \approx 150$ to 300 [GPa]. If it is considered that E_T is close to the Young's modulus of the epoxy resin of the mother member, then, $E_T \approx 6$ [GPa] from Table 4. Therefore, $v_{TL} = 0.3 \times (6/150)$ to $0.3 \times (6/300) = 0.012$ to 0.006 which is a very small value.

35 [0040] Next, the carbon fiber composite material is studied, and, by similarly making reference to Tables 3 and 4, the composite material of the ultrahigh molecular weight polyethylene fiber and the base material of polyurethane also yields the values of $v_{LT} = 0.45$, $E_T \approx 1$ [GPa], $E_L \approx 120$ [GPa], and $v_{TL} \approx 0.45 \times (1/120) \approx 0.0038$ which is a very small value.

40 [0041] In the conventional matching layer without using the fibrous material as shown in Fig. 8a, the sound waves propagate in a direction perpendicular to the direction of propagation of the sound waves. In this embodiment, on the other hand, the matching layer provided in the vibrator of the array-type probe is constituted of an ortho-anisotropic material in which the sound wave properties in a direction perpendicular to the direction of propagation of sound waves are greatly different from the sound wave properties in the direction of travel of sound waves. As shown in Fig. 8b, therefore, the acoustic impedance can be matched in the direction of propagation of sound waves, and the sound waves propagating in a direction perpendicular to the direction of travel is not coupled by the vibration in the transverse direction of the transducer. Namely, the acoustic matching layer is deformed chiefly in the direction of thickness, and the conversion efficiency can be improved in the direction of thickness. Further, the vibration in the direction of width is prevented from interfering with the vibration in the direction of thickness, and the surface of the vibrator vibrates maintaining a uniform amplitude, making it possible to improve the quality of the image of an ultrasonic diagnostic apparatus.

45 [0042] Next, described below is a method of producing the matching layer. First, the bundle-like fibrous material is roll-pressed and is elongated. At the time of elongating the fibrous material, a resin such as an epoxy or a polyurethane is poured into the fibrous material. The resin infiltrates among the fibers, and a plate-like composite material without space or gap is constituted as shown in Fig. 5. The plate-like composite material is overlapped on the piezoelectric vibrator and the backing material, and is adhered thereto. The laminated composite material is cut maintaining a predetermined distance by using a wire saw or the like.

50 [0043] Further, the fibrous material and the resin are mixed together in advance, and the mixed material is pushed into a plate having a plurality of holes perforated therein permitting the passage of the fibrous material. The fibrous material in the mixed material pushed therein passes through the holes like rods. The fibrous material that has passed through is buried in a resin on the opposite side of the plate and is solidified therein. The plate-like composite material is overlapped on the piezoelectric vibrator and the backing material, and is adhered thereto. The thus laminated composite material is cut maintaining a predetermined distance by using a wire saw or the like. The transducer shown in

Fig. 5 is produced by the above-mentioned production method.

[0044] Next, described below in detail as a second embodiment is the structure of the probe using the composite material as the matching layers. Fig. 9 illustrates a transducer in this probe. A fibrous material is contained in the two matching layers. What makes a difference from the first embodiment is that the direction of fibers of the fibrous material in the matching layers 71, 72 is perpendicular to the direction of propagation of sound waves and is in parallel with the lengthwise direction of the transducer. Upon setting the direction of fibers to be in the lengthwise direction of the transducer, the length of the fibers can be lengthened. In this embodiment, therefore, the strength increases in the lengthwise direction.

[0045] Next, described below in detail as a third embodiment is the structure of the probe using the composite material as the matching layers. Fig. 10 illustrates a transducer in this probe. A fibrous material is contained in the two matching layers. What makes a difference from the first and second embodiments is that the direction of fiber of the fibrous material in the matching layers 81, 82 is perpendicular to the direction of propagation of sound waves and is aslant in the lengthwise direction of the transducer. Upon setting the direction of fibers of the matching layers to be aslant in the lengthwise direction of the transducer, the strength increases in both the short-axis direction and the lengthwise direction.

[0046] Next, described below in detail as a fourth embodiment is the structure of the probe using the composite material as the matching layers. Described below in detail is the structure of the probe using the composite material as the matching layers. Fig. 11 illustrates a transducer in this probe. A fibrous material is contained in the two matching layers. What makes a difference from the first, second and third embodiments is that the directions of fibers of the fibrous materials in the matching layers 91 and 92 are different from each other. In this embodiment, the directions of fibers in the two matching layers are differed from each other enabling the strength to increase in both the short-axis direction and in the lengthwise direction depending upon the layers.

[0047] What is common in these embodiments is that the direction of fibers of the fibrous material in the matching layers is perpendicular to the direction of propagation of sound waves. It is therefore allowed to decrease the sound waves propagating in a direction perpendicular to the direction of propagation of sound waves and to decrease the vibration in the transverse direction.

[0048] In the foregoing were described a plurality of acoustic matching layers all containing the fibrous material. However, the fibrous material may be contained in only either one of the acoustic matching layers. Further, through the plurality of acoustic matching layers were described above, only one acoustic matching layer may be applied to the probe.

[0049] Fig. 12 is a block diagram illustrating the whole constitution of the ultrasonic diagnostic apparatus using the ultrasound probe constituted according to the invention. Namely, the ultrasonic diagnostic apparatus comprises an ultrasound probe 100 for transmitting ultrasonic waves to, and receiving ultrasonic waves from, a sample, an ultrasonic beam-forming unit 101 which drives the ultrasound probe 100 to transmit ultrasonic waves and processes the reflected echo signals received by the ultrasound probe 100 to form an ultrasonic beam, an image processing unit 102 that receives signals from the ultrasonic beam-forming unit 101 and constitutes an ultrasonic image, and a display unit 103 that receives image signals from the image processing unit 102 to display an image, wherein the ultrasound probe 100 is the one in which there are provided the transducers of any one of Figs. 5, 9, 10 and 11. In this case, the conversion efficiency is improved in the direction of thickness, and the vibration in the direction of width is prevented from interfering with the vibration in the direction of thickness realizing an ultrasonic diagnostic apparatus featuring improved image quality.

Claims

1. An ultrasound probe obtained by arranging, on a backing, a plurality of transducers each of which comprising a piezoelectric transducer, an acoustic lens, and an acoustic matching layer provided between said piezoelectric transducer and said acoustic lens, said acoustic matching layer containing a fibrous material, and the direction of fibers in said fibrous material being perpendicular to the direction of sound waves.
2. An ultrasound probe according to claim 1, wherein the direction of fibers in said fibrous material is perpendicular to the lengthwise direction of said transducer.
3. An ultrasonic probe according to claim 1, wherein the direction of fibers in said fibrous material is in parallel with the lengthwise direction of said transducer.
4. An ultrasound probe according to claim 1, wherein the direction of fibers in said fibrous material is aslant in the lengthwise direction of said transducer.

5. An ultrasound probe according to claim 1, wherein the Young's modulus of said fibrous material in the direction of fibers is greater than the Young's modulus of the mother member in said acoustic matching layer.
6. An ultrasound probe according to claim 1, wherein said acoustic matching layer comprises a first acoustic matching layer joined to said acoustic lens and a second acoustic matching layer provided between said first acoustic matching layer and said backing material.
- 10 7. An ultrasound probe according to claim 6, wherein the direction of fibers in the fibrous material of said first acoustic matching layer and the direction of fibers in the fibrous material of said second acoustic matching layer, are perpendicular to each other.
- 15 8. An ultrasound probe according to claim 6, wherein the acoustic impedance of said first acoustic matching layer is lower than the acoustic impedance of said second acoustic matching layer.
9. An ultrasound probe according to claim 6, wherein said first acoustic matching layer is a polyethylene composite material, and said second acoustic matching layer is a carbon fiber composite material.
- 20 10. An ultrasound diagnostic equipment comprising an ultrasound probe of claim 1, an ultrasonic beam-forming unit which drives said ultrasound probe to transmit ultrasonic waves and processes the reflected echo signals received by said ultrasound probe to form an ultrasonic beam, an image processing unit that receives signals from said ultrasonic beam-forming unit and constitutes an ultrasonic image, and a display unit that receives image signals from said image processing unit to display an image.

25

30

35

40

45

50

55

Fig. 1

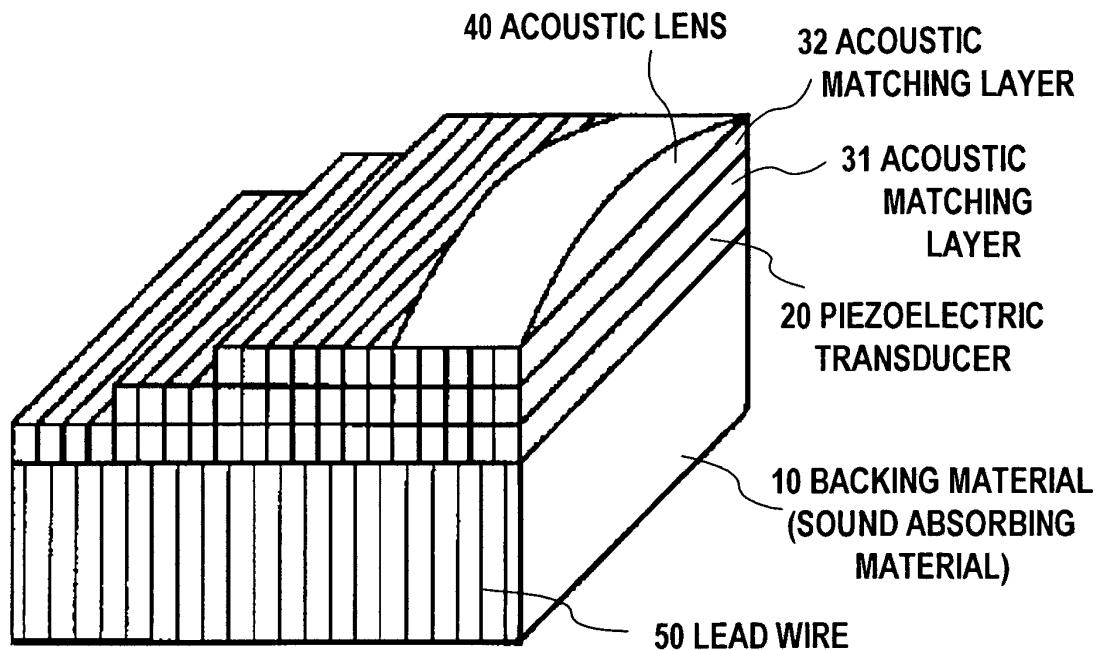


Fig. 2

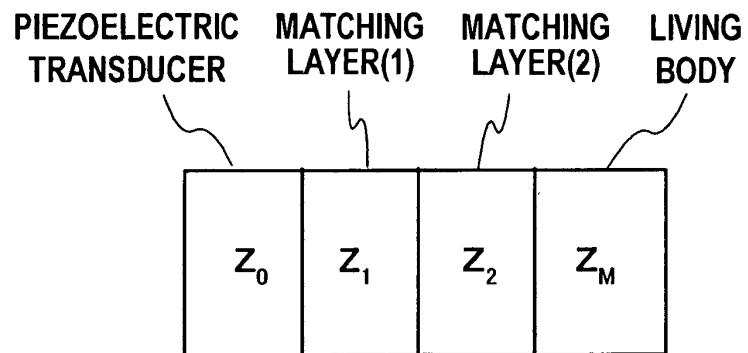


Fig. 3

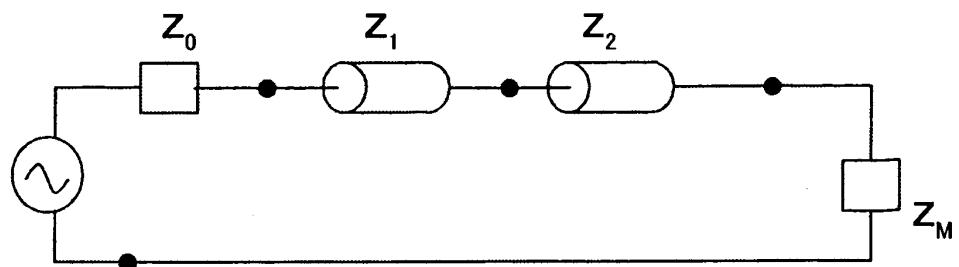


Fig. 4

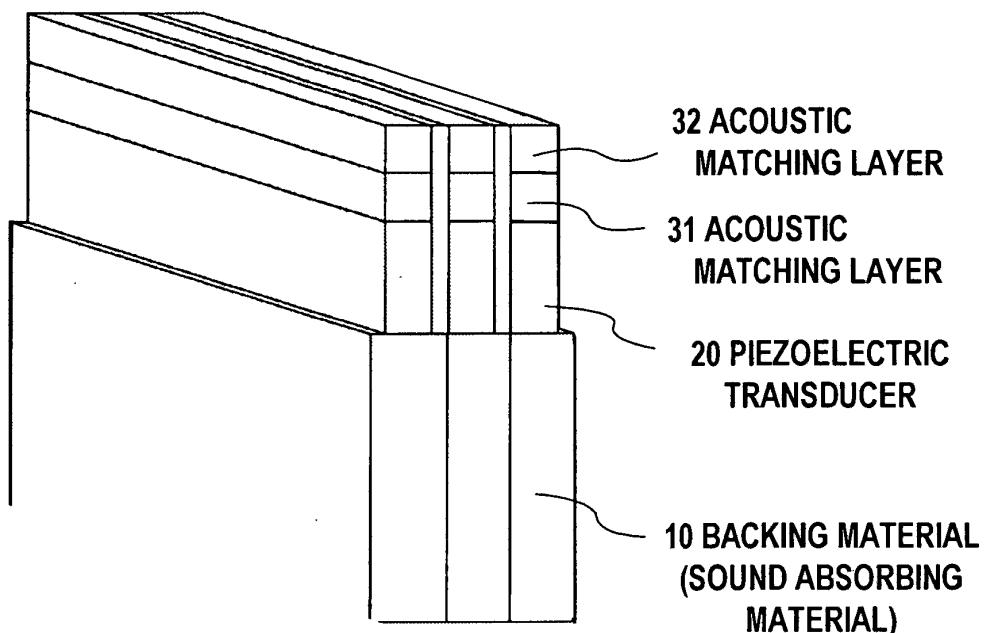


Fig. 5

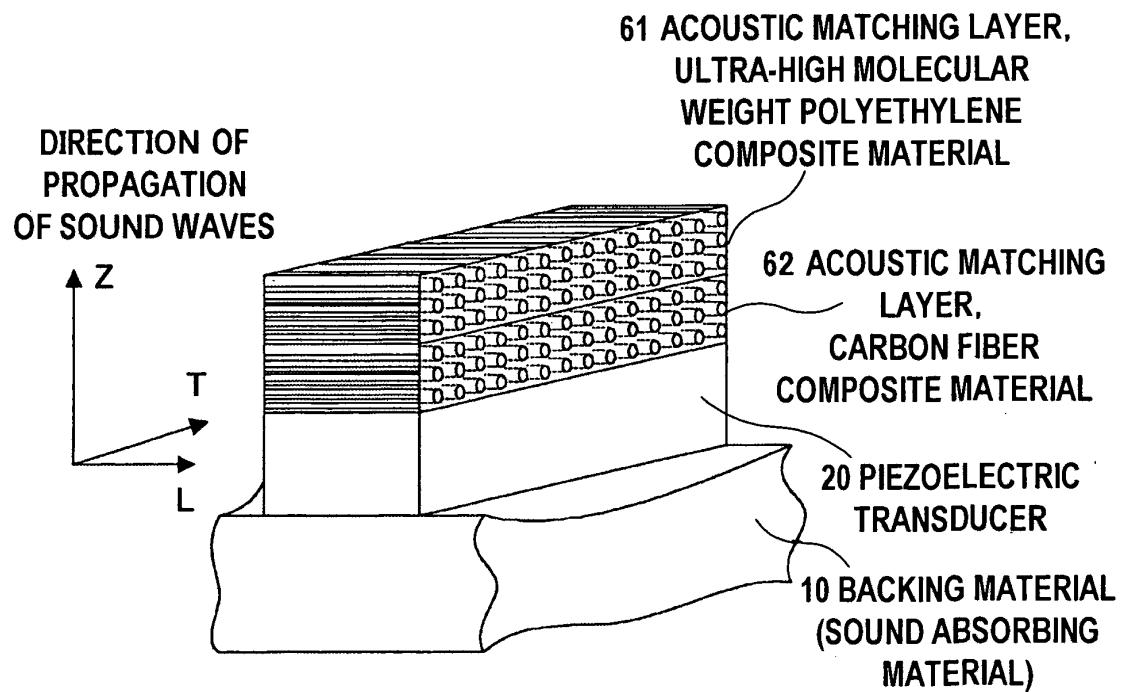


Fig. 6a

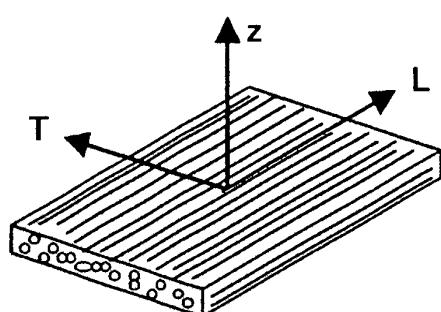


Fig. 6b

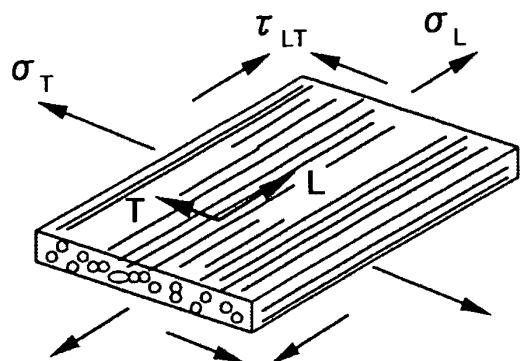


Fig. 7

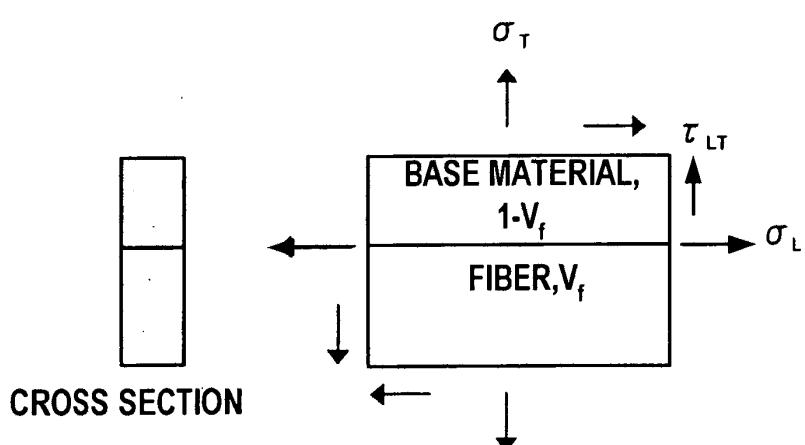


Fig. 8a

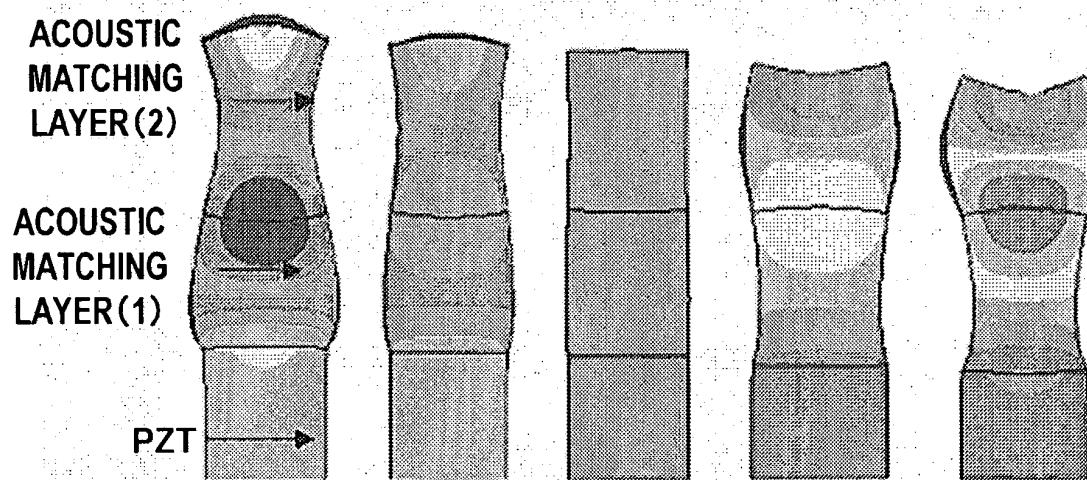


Fig. 8b

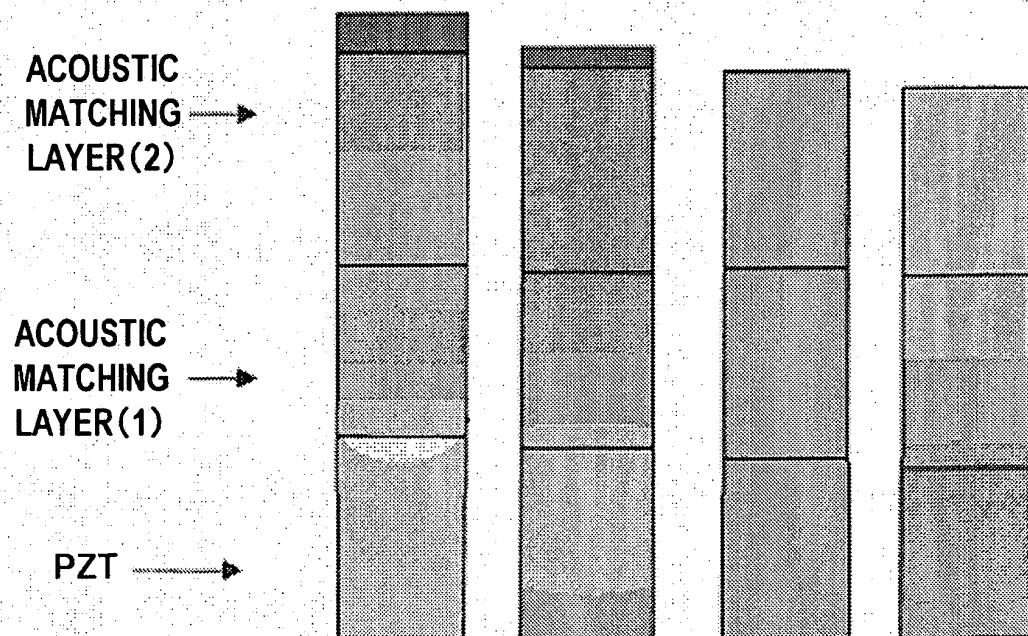


Fig. 9

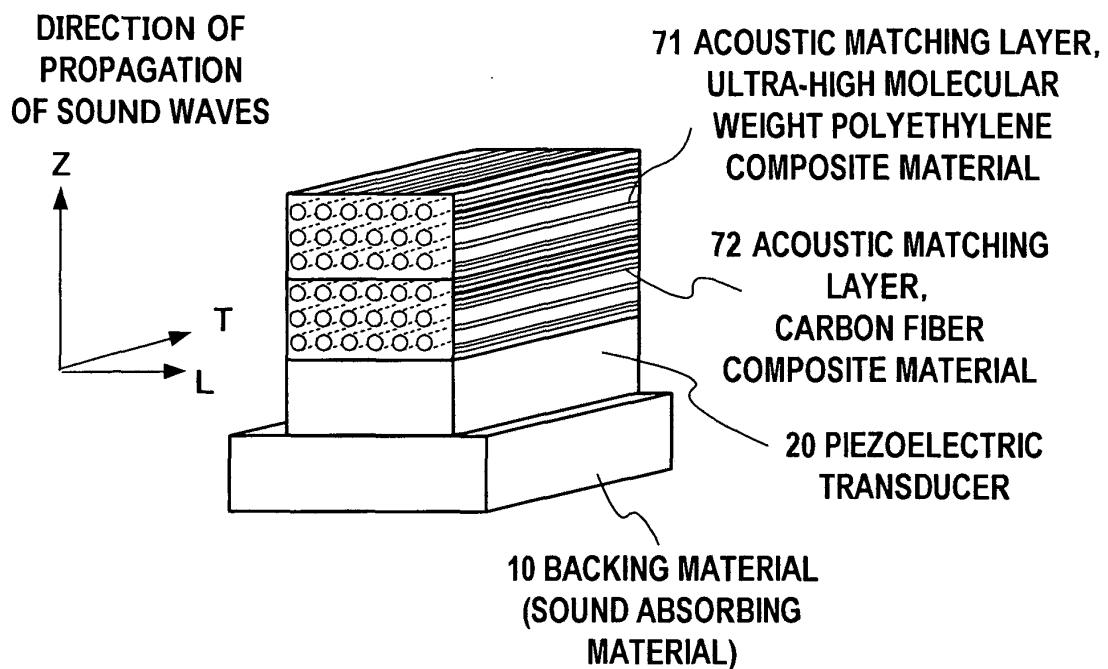


Fig. 10

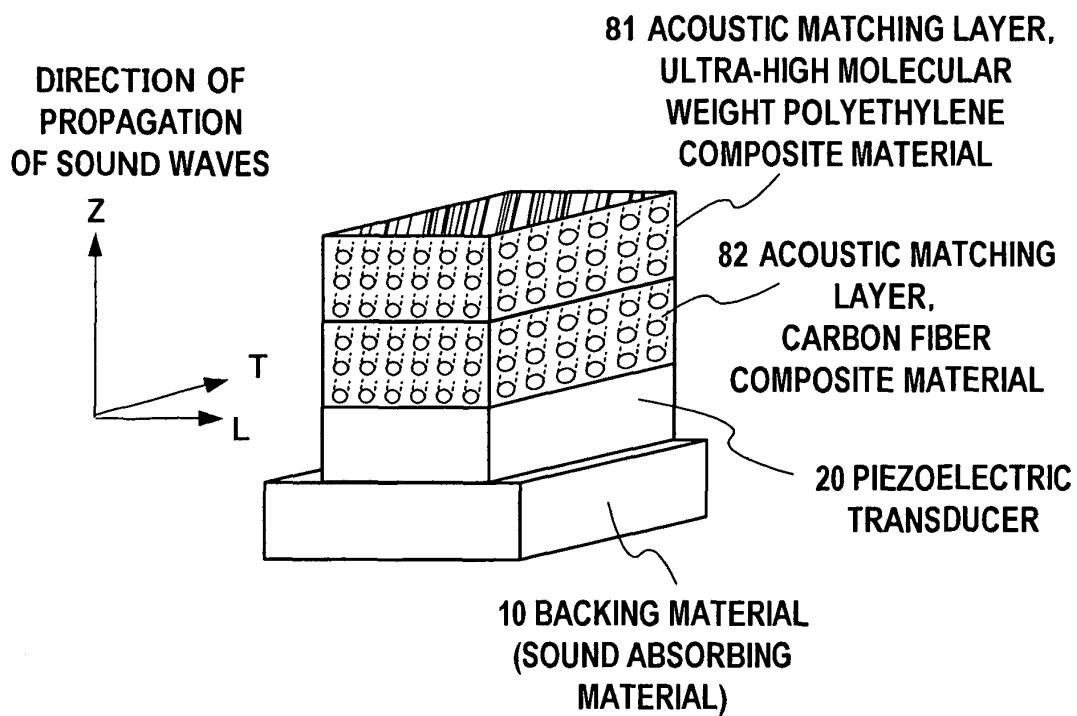


Fig. 11


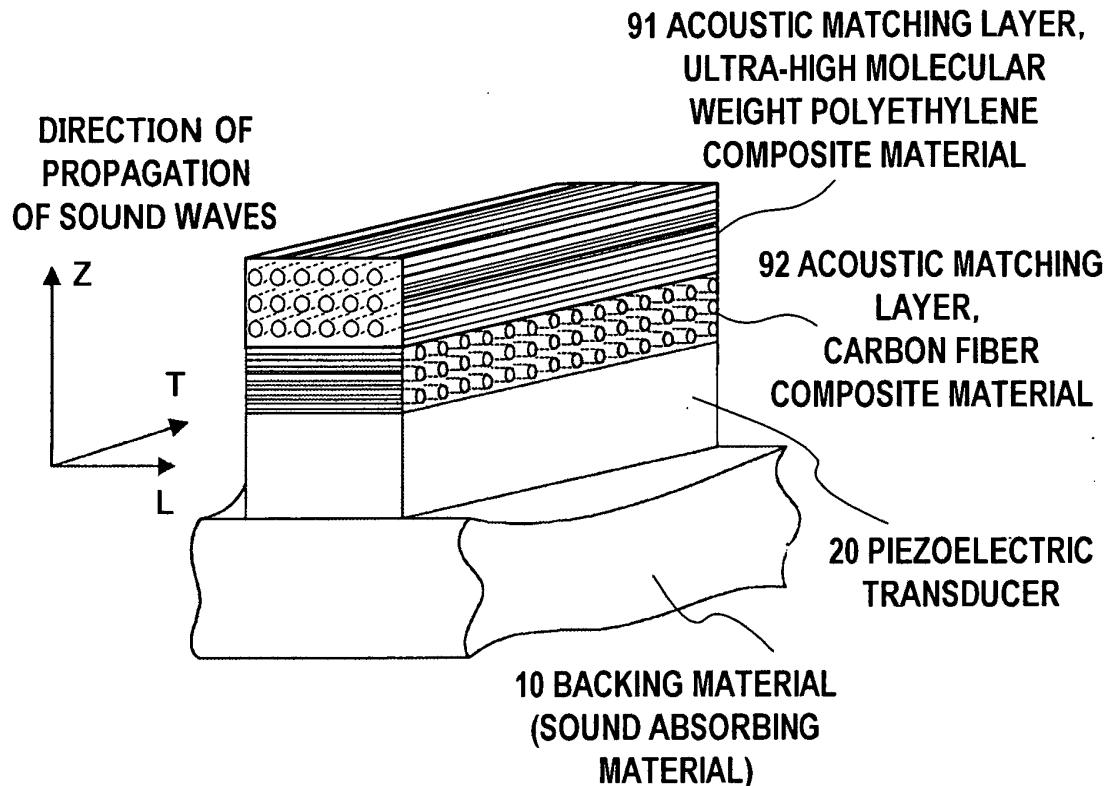


Fig. 12

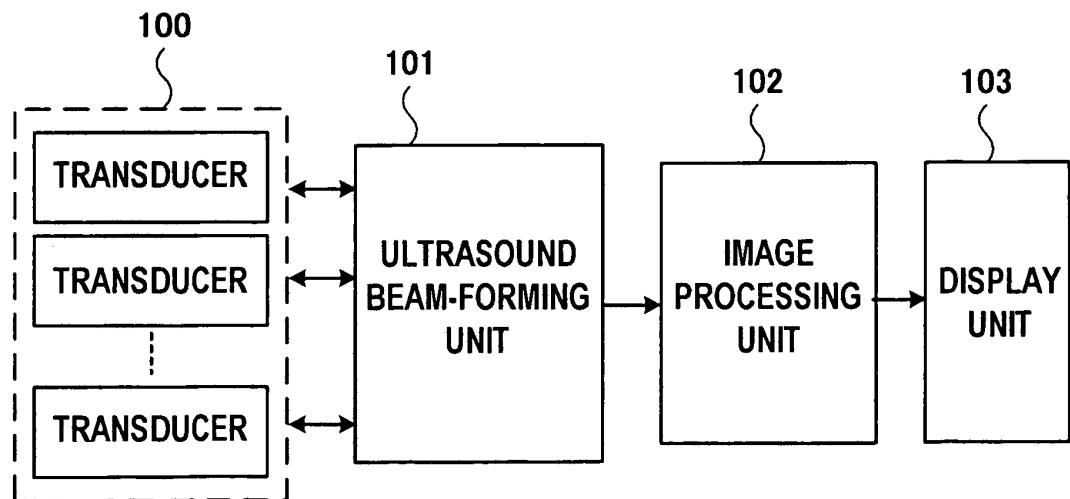

INTERNATIONAL SEARCH REPORT

International application No.
PCT/JP2004/002387

A. CLASSIFICATION OF SUBJECT MATTER
Int.Cl⁷ A61B8/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
Int.Cl⁷ A61B8/00-8/15

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
Jitsuyo Shinan Koho 1922-1996 Toroku Jitsuyo Shinan Koho 1994-2004
Kokai Jitsuyo Shinan Koho 1971-2004 Jitsuyo Shinan Toroku Koho 1996-2004

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
PATENT FILE (PATOLIS), UTILITY MODEL FILE (PATOLIS)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	JP 10-56694 A (Toshiba Corp.), 24 February, 1998 (24.02.98), Full text; all drawings (Family: none)	1-10
Y	JP 2001-309495 A (Kazumasa ONISHI), 02 November, 2001 (02.11.01), Full text; all drawings (Family: none)	1-10
A	JP 2002-247696 A (Olympus Optical Co., Ltd.), 30 August, 2002 (30.08.02), Full text; all drawings & US 2002/0156373 A1	1-10

Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:	
"A"	document defining the general state of the art which is not considered to be of particular relevance
"E"	earlier document but published on or after the international filing date
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
"O"	document referring to an oral disclosure, use, exhibition or other means
"P"	document published prior to the international filing date but later than the priority date claimed
"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"&"	document member of the same patent family

Date of the actual completion of the international search 18 March, 2004 (18.03.04)	Date of mailing of the international search report 30 March, 2004 (30.03.04)
Name and mailing address of the ISA/ Japanese Patent Office	Authorized officer
Facsimile No.	Telephone No.

Form PCT/ISA/210 (second sheet) (July 1998)

INTERNATIONAL SEARCH REPORT

International application No. PCT/JP2004/002387
--

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	JP 10-75953 A (Aloka Co., Ltd.), 24 March, 1998 (24.03.98), Full text; all drawings (Family: none)	1-10
A	JP 7-284198 A (Yoshiro TOMIKAWA), 27 October, 1995 (27.10.95), Full text; all drawings (Family: none)	1-10
A	JP 1-119199 A (Siemens AG.), 11 May, 1989 (11.05.89), Full text; all drawings & EP 0308931 A2 & US 4907207 A & DE 3732412 A1	1-10

Form PCT/ISA/210 (continuation of second sheet) (July 1998)

专利名称(译)	超声波探头		
公开(公告)号	EP1602331A1	公开(公告)日	2005-12-07
申请号	EP2004715496	申请日	2004-02-27
[标]申请(专利权)人(译)	株式会社日立医药		
申请(专利权)人(译)	日立医疗器械股份有限公司		
当前申请(专利权)人(译)	日立医疗器械股份有限公司		
[标]发明人	KONDO TOSHIRO OSAWA TAKAYA		
发明人	KONDO, TOSHIRO OSAWA, TAKAYA		
IPC分类号	A61B8/00 A61B8/14 G01N29/24 G10K11/02 H04R17/00		
CPC分类号	G10K11/02 A61B8/00 A61B8/4455		
优先权	2003052038 2003-02-27 JP		
其他公开文献	EP1602331A4		
外部链接	Espacenet		

摘要(译)

通过在背衬10上布置多个换能器而获得的超声探头，每个换能器包括压电换能器20，声透镜40和设置在压电换能器20和声透镜40之间的声匹配层，声匹配包含纤维材料的层，并且纤维材料中的纤维方向垂直于声波的方向。

Fig. 5

