



US010184826B2

(12) **United States Patent**
Li et al.

(10) **Patent No.:** **US 10,184,826 B2**
(45) **Date of Patent:** **Jan. 22, 2019**

(54) **IMAGING SYSTEM FOR GENERATING VIBRATION REGION CAUSED BY ULTRASOUND WAVE THEREBY TO OBTAIN OPTICALLY-SECTIONED IMAGES**

(2013.01); *G01N 21/4795* (2013.01); *G01N 21/49* (2013.01); *G01N 29/00* (2013.01); *G01N 2021/479* (2013.01)

(71) Applicant: **NATIONAL TAIWAN UNIVERSITY, Taipei (TW)**

(58) **Field of Classification Search**
CPC A61B 8/485; A61B 5/0097; A61B 5/0095; A61B 5/0082; G01H 9/00; G01H 9/008; G01H 9/002; G01N 29/041; G01N 29/043; G01S 15/8972

(72) Inventors: **Pai-Chi Li, Taipei (TW); Pei-Yu Chao, Taipei (TW)**

See application file for complete search history.

(73) Assignee: **NATIONAL TAIWAN UNIVERSITY, Taipei (TW)**

(56) **References Cited**

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

U.S. PATENT DOCUMENTS

5,212,667 A * 5/1993 Tomlinson, Jr. A61B 5/0059
367/11
5,293,873 A * 3/1994 Fang A61B 5/0091
600/437

(21) Appl. No.: **15/642,022**

(Continued)

(22) Filed: **Jul. 5, 2017**

Primary Examiner — Michael P LaPage

(65) **Prior Publication Data**

US 2018/0235474 A1 Aug. 23, 2018

(74) Attorney, Agent, or Firm — Muncy, Geissler, Olds & Lowe, P.C.

(30) **Foreign Application Priority Data**

Feb. 21, 2017 (TW) 106105747 A

(57) **ABSTRACT**


(51) **Int. Cl.**
G01H 9/00 (2006.01)
A61B 5/00 (2006.01)
A61B 8/00 (2006.01)
A61B 8/08 (2006.01)
G01N 21/49 (2006.01)

An imaging system is configured for generating vibration region caused by ultrasound wave thereby to obtain a plurality of optically-sectioned images. In the imaging system, a stage is operable to be moved along a plurality of scanning imaging positions, and applied to deposit an object with at least one scattering material. When the object receives an ultrasound wave, a shear wave is generated to displace the scattering material thereby to form a vibration region. A laser generating device is configured to transmit a laser beam, which penetrates the vibration region to form a speckle pattern and focused at a focusing position. An optical imaging device is set at the focusing position to receive the laser beam to generate a plurality of scanning optically-sectioned images with respect to the scanning imaging positions.

(Continued)

(52) **U.S. Cl.**
CPC *G01H 9/008* (2013.01); *A61B 5/0082* (2013.01); *A61B 5/0097* (2013.01); *A61B 8/4444* (2013.01); *A61B 8/485* (2013.01); *G01N 21/1717* (2013.01); *G01N 21/45*

4 Claims, 4 Drawing Sheets

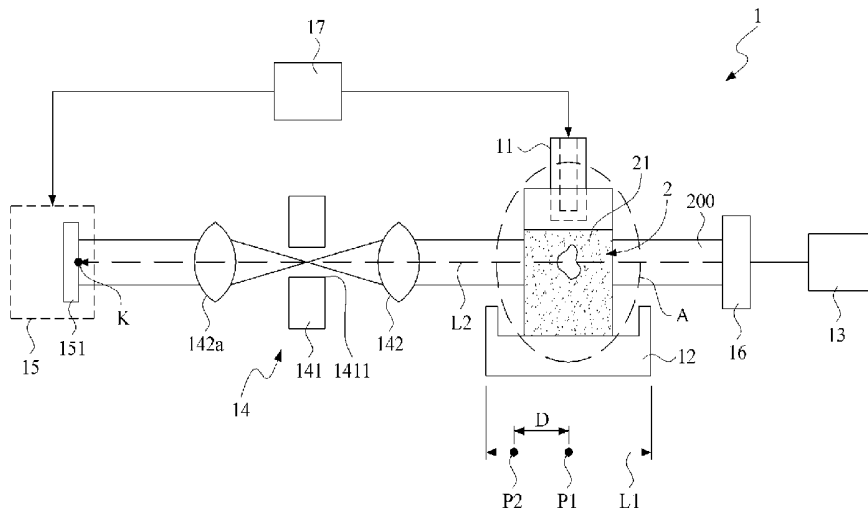

- (51) **Int. Cl.**
G01N 29/00 (2006.01)
G01N 21/17 (2006.01)
G01N 21/45 (2006.01)
G01N 21/47 (2006.01)

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,041,248 A * 3/2000 Wang G01N 21/4795
 600/407
 2004/0127782 A1 * 7/2004 Sfez A61B 5/0048
 600/407
 2007/0187632 A1 * 8/2007 Igarashi A61B 5/0048
 250/559.36
 2010/0125205 A1 * 5/2010 Park A61B 5/0095
 600/443
 2012/0182561 A1 * 7/2012 Masumura A61B 5/0095
 356/601
 2014/0009808 A1 * 1/2014 Wang G02F 1/33
 359/10
 2014/0081102 A1 * 3/2014 Baym A61B 5/0097
 600/328
 2014/0114188 A1 * 4/2014 Sangawa G01S 15/8972
 600/437
 2015/0029819 A1 * 1/2015 Yacoubian G01N 21/171
 367/7
 2018/0140279 A1 * 5/2018 Perrey A61B 8/485

* cited by examiner

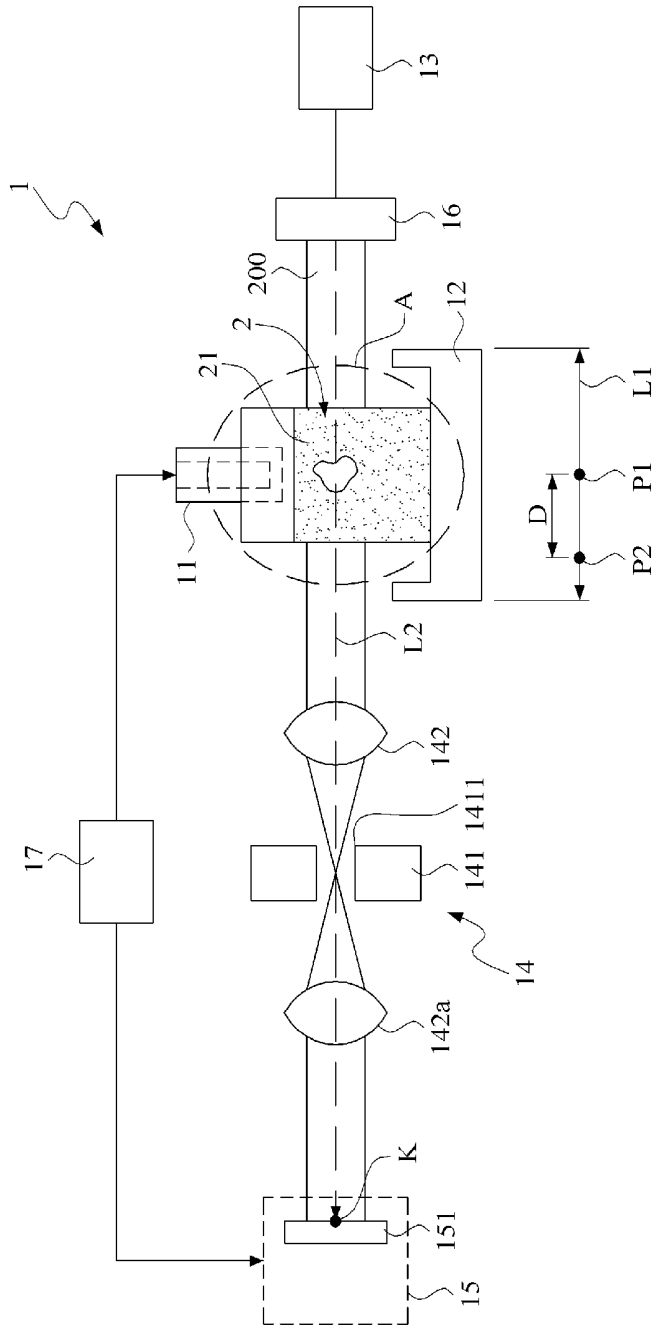


FIG. 1

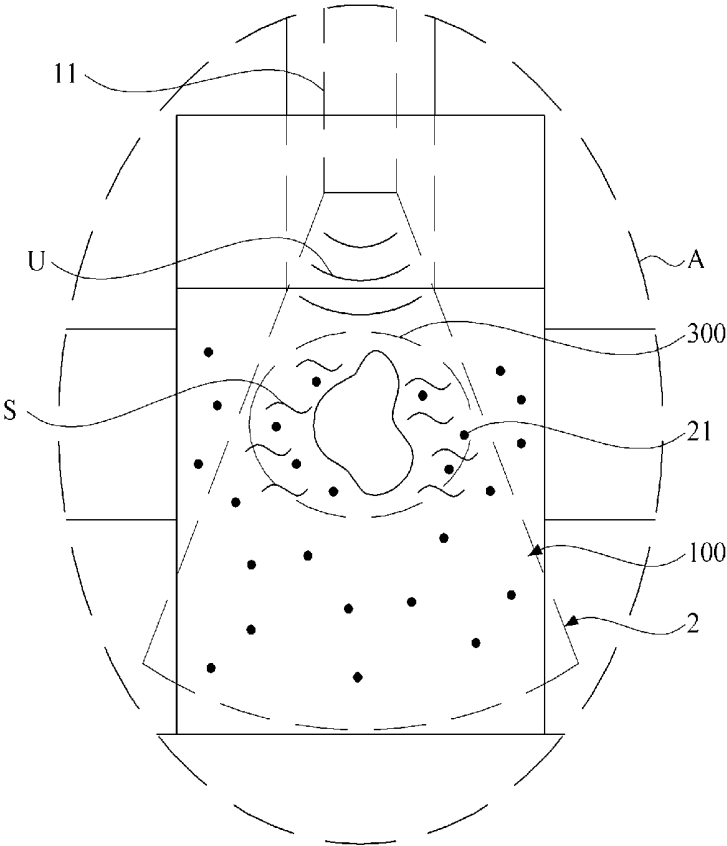


FIG.1A

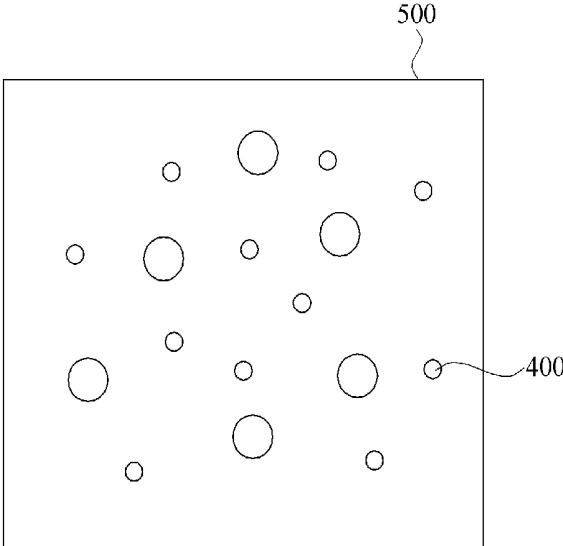


FIG. 2

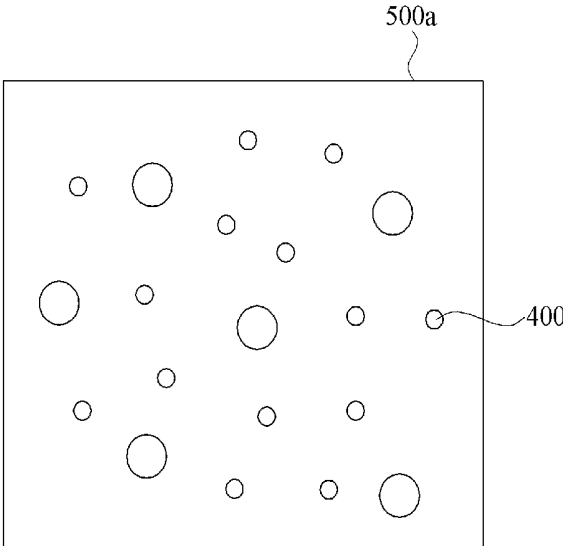


FIG. 3

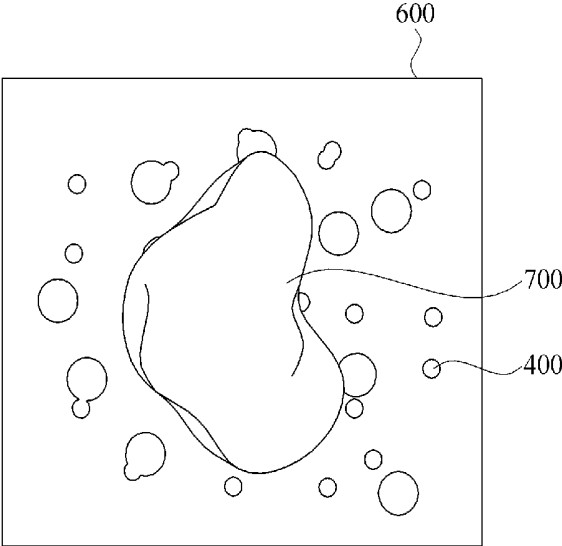


FIG. 4

**IMAGING SYSTEM FOR GENERATING
VIBRATION REGION CAUSED BY
ULTRASOUND WAVE THEREBY TO OBTAIN
OPTICALLY-SECTIONED IMAGES**

This application claims the benefit of Taiwan Patent Application Serial No. 106105747, filed Feb. 21, 2017, the subject matter of which is incorporated herein by reference.

BACKGROUND OF INVENTION

1. Field of the Invention

The present invention is related to an imaging system for generating vibration region caused by ultrasound wave to obtain optically-sectioned images, and more particularly is related to an imaging system for generating vibration region caused by ultrasound wave to obtain optically-sectioned images and processing these images to generate the elasticity image.

2. Description of the Prior Art

With the development of technologies, the improvement of medical technologies may increase the lifespan of humans. In many diseases, such as cancer, stiff nodules were formed in the biological tissue. For this reason, palpation was widely used in clinical physical examinations for sensing the degree and distribution of the stiffness of biological tissues. However, the palpation technique is highly relied on the experience of the doctor or the physician and the probability of using such technique for discovering early stage of a disease may be low. Therefore, there is a need for improving the sensitivity and specificity of the stiffness-sensing technique for accurately identifying the pathological region.

During past decades, there has been an intensive development of noninvasive imaging techniques for characterizing the stiffness of biological tissue. These techniques, such as non-invasive elasticity imaging based on ultrasound, have been exploited in numerous clinical applications, including the detection of prostate cancer, breast cancer, and the staging of liver fibrosis.

However, the imaging sensitivity and resolution of the current imaging techniques still require improvements in order to provide better contrast and distinguishable elasticity imaging result. Thus, there exist the needs to improve the conventional technology.

SUMMARY OF THE INVENTION

The common problem of the conventional elasticity imaging techniques is that the imaging resolution is still relatively poor, and elasticity distribution of the tissue may not be accurately reconstructed. Accordingly, an imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images is provided in the present invention, which uses the ultrasound wave to generate a vibration region on the object to be detected, moves the object along a plurality of scanning imaging positions to generate images corresponds to the scanning imaging positions, and processes these images to generate the elasticity image so as to achieve three-dimensional elasticity detection by using the optically-sectioned images.

Accordingly, the main objective of the present invention is to provide an imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of

optically-sectioned images. The imaging system comprises an ultrasound device, a translational stage, a laser generating device, an optical focusing device, and an optical imaging device. The ultrasound device is utilized for transmitting an ultrasound wave onto an investigating region within the object. The translational stage is at least partially located in the investigating region and is operable to be moved to a plurality of scanning imaging positions on a moving path. The translational stage is utilized for carrying and locating an object contains at least one scattering material. When the ultrasound wave is delivered into the object, a shear wave is generated in the object to vibrate at least one scattering material so as to form a vibration region in the object. The laser generating device is utilized for transmitting a laser beam along a beam propagation path. When the laser beam penetrates the object contains at least one scattering material, and onto the optical imaging device, at least one speckle pattern is imaged. The optical focusing device is located on the beam propagation path to focus the laser beam, which penetrated the object, at a focusing position, and an aperture is used to partially block the light from out-of-focusing position. The optical imaging device is set at the focusing position to receive the laser beam so as to generate a plurality of scanning optically-sectioned images corresponding to the scanning imaging positions, wherein at least one of the scanning optically-sectioned images shows the at least one speckle pattern. The optical imaging device may contain processing unit for reconstructing the elasticity image of the object from plurality of scanning optically-sectioned images.

In accordance with an embodiment of the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images of the present invention, the reduced scattering coefficient of the scattering material is required to be greater than 0.2 cm^{-1} . The aperture of the optical focusing device has a plurality of hole diameters, which can be used for adjusting the required interval between the scanning positions.

In accordance with an embodiment of the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images of the present invention, the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images further comprises a beam expansion device. The beam expansion device is located on the beam propagation path between the laser generating device and the translational stage, for expanding the illumination region of the laser beam. The beam expansion device is a combination of a concave lens and a convex lens. In addition, the optical focusing device comprises an aperture stop and at least two lenses. The aperture on the aperture stop partially allows the light beam to pass. The at least two lenses are located on the either side of the aperture stop along the beam propagation path, for adjusting the focusing position.

In accordance with an embodiment of the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images of the present invention, the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images further comprises a control device, which is electrically connected to the ultrasound device and the optical imaging device, for controlling the driving sequence for ultrasound device to transmit the ultrasound wave and optical imaging device to record optical image of the object, so as to adjust the effective frame rate of the imaging system. If the effective frame rate is high,

the propagation speed of the shear wave can be accurately detected such that the error in the stiffness estimation of the high elasticity object can be reduced.

By using the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images provided in the present invention, which uses the ultrasound wave to generate the vibration region on the object to be detected, moves the object along a plurality of scanning imaging positions to generate images corresponding to the scanning imaging positions, and processes these images to generate the elasticity image, thereby, the elasticity distribution of the object can be reconstructed effectively by using the sectioned images. The ability to detect stiff nodule accurately is helpful and convenient for both research and practical applications.

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention will now be specified with reference to its preferred embodiment illustrated in the drawings, in which:

FIG. 1 is a schematic view of an imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images in accordance with a preferred embodiment of the present invention.

FIG. 1A is a partially enlarged view of FIG. 1.

FIG. 2 and FIG. 3 are schematic views of the scanning optically-sectioned images in accordance with a preferred embodiment of the present invention.

FIG. 4 is a schematic view of the elasticity image in accordance with a preferred embodiment of the present invention.

DESCRIPTION OF THE PREFERRED EMBODIMENT

There are various embodiments of the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images provided in accordance with the present invention, which are not repeated hereby. Only one preferred embodiment is mentioned in the following paragraph as an example.

Please refer to FIG. 1 and FIG. 1A, wherein FIG. 1 is a schematic view of an imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images in accordance with a preferred embodiment of the present invention, and FIG. 1A is a partially enlarged view of FIG. 1.

As shown, the imaging system 1 for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images in accordance with a preferred embodiment of the present invention (hereinafter the "imaging system") comprises an ultrasound device 11, a translational stage 12, a laser generating device 13, an optical focusing device 14, an optical imaging device 15, and a beam expansion device 16.

The ultrasound device 11 can be an existing ultrasound probe, which is utilized for transmitting an ultrasound wave U to an investigating region 100. The investigating region 100 is defined as the combination of the spaces to which the ultrasound wave can be transmitted. Concretely speaking, the aforementioned space is the depth of field of the ultrasound device, which includes the focusing point of the ultrasound device. The investigating region is the space where acoustic radiation force is induced from the transmitted ultrasound wave, which thereby generates a shear wave.

The translational stage 12 is at least partially located in the range of the investigating region 100. The translational stage 12 is operable to be moved to a plurality of scanning imaging positions P1 and P2 on a moving path L1, and is utilized for carrying and locating an object 2 to be detected which includes at least one scattering material 21. In accordance with a preferred embodiment of the present invention, the object 2 can be placed in a transparent container (the container can be omitted in other embodiments, and the transparent container can be made from glass or acrylic), and the object 2 to be detected can be any biological tissue or 3D cell culture structure, and the reduced scattering coefficient of the scattering material 21 (such as the light scattering particles), which causes the object to be semitransparent, is required to be greater than 0.2 cm^{-1} for producing the necessary speckle pattern. In the preferred embodiment of the present invention, the reduced scattering coefficient is 0.97 cm^{-1} as an example. It should be mentioned that the reduced scattering coefficient of the container should be smaller than that of the scattering material 21, however, if the thickness of the container is ranged between 1 and 2 millimeters, the reduced scattering coefficient of the scattering material 21 is not limited to the aforementioned value. In addition, a moving path L1 along the X-axis is provided in the present preferred embodiment as an example, the moving path can be expanded to include 2D or 3D movement.

In addition, if the object 2 is a 3D cell culture structure, the object 2 is required to be in solid phase for allowing the shear wave to propagate therein. The ingredient of the object may be the biological hydrogel or extracellular matrix gel (i.e. Matrigel and collagen), and the biological tissue or cells to be cultured are placed in the extracellular matrix gel.

The laser generating device 13 can be any existing device that can generate and transmit laser beams, and is utilized for transmitting a laser beam 200 along a beam propagation path L2. The optical focusing device 14 has an aperture 1411 located on the beam propagation path L2. Concretely speaking, the optical focusing device 14 in accordance with the preferred embodiment of the present invention includes a aperture stop 141 and at least two lenses 142 and 142a, the aperture stop 141 has the aforementioned aperture, and the two lenses 142 and 142a are located on the beam propagation path L2.

The optical imaging device 15 is located on the beam propagation path L2. The optical imaging device 15 may include the optical lenses, optical sensing unit 151 (i.e. charge-coupled device (CCD), the complementary metal-oxide-semiconductor (CMOS) or any existing optical sensor), and the image processor depends on the design in practice.

The beam expansion device 16 is located on the beam propagation path L2 between the translational stage 12 and the laser generating device 13. The beam expansion device 16 can be a combination of a concave lens and a convex lens, a combination of two convex lenses, or a diffuser, depends on the design in practice. The beam expansion device 16 is utilized for expanding the coverage of the laser beam 200.

Please refer to FIG. 1 to FIG. 4, wherein FIG. 2 and FIG. 3 are schematic views of the scanning optically-sectioned images in accordance with a preferred embodiment of the present invention, and FIG. 4 is a schematic view of the elasticity image in accordance with a preferred embodiment of the present invention.

As shown, when the object 2 to be detected receives the ultrasound wave U, a shear wave S is generated in the object 2 to vibrate the at least one scattering material 21 so as to

form a vibration region **200** in the object **2**. In the vibration region **200**, the shear wave **S** may cause the scattering particles in the object to displace and change the refractive index of the object. The laser beam **200** propagating along the beam propagation path **L2** may generate at least one a speckle pattern **400** after penetrating the vibration region **300** (as shown in FIG. 2 and FIG. 3), and the laser beam **200** is then focused at a focusing location **K** on the beam propagation path **L2** after the laser beam **200** penetrating the vibration region **300** and the aperture **1411** in a serial. The aforementioned optical sensing unit **151** is located at the focusing position **K**.

In the present preferred embodiment, the laser beam **200** penetrates the vibration region **300**, the lens **142**, the aperture **1411**, and the lens **142a**, and consequently focused at the focusing position **K**. The position of the lenses **142** and the **142a** can be used for adjusting the focusing position **K**. In addition, the aperture **1411** can be used for shielding the unwanted illumination (i.e., the unwanted portion of the expanded laser beam **200** is shielded), adjusting the thickness of the focusing plane. In the present preferred embodiment, the aperture **1411** has been adjusted in advance to show a fixed hole diameter and also a fixed focusing plane.

The optical imaging device **15** is set at the focusing position **K** to receive the laser beam **200** so as to generate a plurality of scanning optically-sectioned images **500** and **500a** corresponding to the scanning imaging positions **P1** and **P2**. For example, for the scanning imaging position **P1**, the optical imaging device **15** receives the scanning optically-sectioned image **500**, for the scanning imaging position **P2**, the optical imaging device receives the scanning optically-sectioned image **500a**, and at least one of these scanning optically-sectioned images shows the at least one speckle pattern **400**.

The optical imaging device **15** may process these scanning optically-sectioned images **500** and **500a** to form a 3D elasticity image **600**. Concretely speaking, the optical imaging device **15** may process the scanning optically-sectioned images **500** and **500a** as two 2D elasticity images then recombine the scanning optically-sectioned images **500** and **500a** to rebuild the 3D elasticity image. The elasticity image **600** includes the speckle pattern **400** and the image **700** of the object (such as the integration of the background image and the image of the object to be detected). It should be also noted that the images shown in FIG. 2 to FIG. 4 are merely the schematic views.

It should be also mentioned that although only two scanning optically-sectioned images **500**, **500a** and two scanning imaging positions **P1**, **P2** are mentioned in the present preferred embodiment, but in practice, more scanning optically-sectioned images and scanning imaging positions can be used, and thus the present invention is not so restricted.

In addition, transmission of the shear wave **S** may cause displacement of scattering particles in the object **2** to be detected. When the laser beam **200** passes through the vibration region **300**, phase of the laser beam would be changed, which resulted in a change of the interference pattern (i.e. the speckle pattern). The image formed by the optical imaging device **15** would show the changed in the interference pattern as local blurring. Therefore, the wave front of the shear wave **S** can be detected by measuring the spatial blurring of the speckle pattern **400**. The time difference between the shear wave **S** wave front at any two locations along the shear wave **S** propagation path can be

used to yield the velocity of the shear wave **S**, and the velocity of the shear wave **S** is related to the elasticity of the object **2**.

In addition, in the present preferred embodiment, a scanning gap **D** is the distance between the neighboring scanning imaging positions **P1** and **P2**, the aperture **1411** of optical focusing device **14** has a plurality of hole diameters (i.e. the aperture **1411** is operable to be expanded or shrunk), thereby the scanning gap **D** can be adjusted according to the size of the hole diameters. For example, by using a small hole diameter with a small scanning gap **D**, the precision of the estimated propagation speed of the shear wave **S** can be enhanced. In addition, a smaller hole diameter of the aperture **1411** may increase the size of the speckle pattern **400** and block the multi-scattering light waves exiting from the object **2**, so as to enhance the contrast and clarity of the speckle pattern **400** in the scanning optically-sectioned images **500** and **500a**.

In addition, the imaging system **1** may also include a control device **17**, which is electrically connected to the ultrasound device **11** and the optical imaging device **15**, and is also electrically connected to the translational stage **12**. The control device **17** can be used for controlling the time sequence, for example, when the translational stage **12** is moved to a certain position, the control device **17** would control the driving sequence for the ultrasound device **11** to transmit the ultrasound wave **U** and also control the driving sequence of the optical imaging device **15**, such as control the optical imaging device **15** to acquire **N** images, such that, the optical imaging device **15** may identify the condition of the shear wave **S** propagated on the image focusing plane according to the aforementioned **N** images, and then the control device **17** may control the translational stage **12** to move to the next position and repeat the aforementioned steps.

In accordance with another embodiment of the present invention, for example, after the translational stage **2** is moved to the scanning imaging position **P1**, the control device **17** controls the ultrasound device **11** to transmit the ultrasound wave **U**, and controls the optical imaging device **15** to take a real-time image. Thereafter, the control device **17** will control the ultrasound device **11** to transmit the ultrasound wave **U** again, and controls the optical imaging device **15** to acquire another real-time image after a time delay. The aforementioned process can be repeated for different scanning imaging position. Therefore, the control device **17** is utilized for controlling whether the cycle of the ultrasound wave **U** transmitted by the ultrasound device **11** is synchronized with the imaging cycle or not, which depends on the need in practice, and the wave speed of the shear wave **S** can be calculated thereby. It should be noted that the control device **17** may also control the exposure time of the optical imaging device **15**.

For example, after the control device **17** triggers the ultrasound device **11**, the control device **17** may wait for 100 microseconds before sending the triggering signal to the optical imaging device **15**, and the optical imaging device **15** would take the image showing the condition after the shear wave **S** has been propagated for 100 microseconds, i.e. the position of the shear wave **S** wave front after the shear wave **S** has been induced and propagated for 100 microseconds. The propagation of the shear wave **S** can be fully detected by modulating the delay time between two trigger signals. If the adjustable interval of the delay time is 100 microseconds, the effective imaging frame rate of the shear wave **S** would be 10000 frames/second.

In conclusion, by using the imaging system for generating vibration region caused by ultrasound wave to obtain a plurality of optically-sectioned images provided in the present invention, 3D elasticity image can be reconstructed by utilizing technical features of the laser generating device, the translational stage, the optical focusing device, and the optical imaging device. In addition, because the optical scanning system is used, the contrast of the elasticity image and the sensitivity can be effectively enhanced.

While the present invention has been particularly shown and described with reference to a preferred embodiment, it will be understood by those skilled in the art that various changes in form and detail may be without departing from the spirit and scope of the present invention.

What is claimed is:

1. An imaging system configured for generating a vibration region caused by an ultrasound wave to obtain a plurality of optically-sectioned images, comprising:

- an ultrasound device, utilized for transmitting an ultrasound wave to an investigating region;
- a translational stage, at least partially located in the investigating region, operable to be moved to a plurality of scanning imaging positions on a moving path, and being utilized for locating an object with at least one scattering material, wherein when the object receives the ultrasound wave, a shear wave is generated in the object to vibrate the at least one scattering material so as to form a vibration region in the object;
- a laser generating device, utilized for transmitting a laser beam along a beam propagation path to have the laser beam penetrate the vibration region to form at least one speckle pattern; an optical focusing device, having an aperture on the beam propagation path, to focus the laser beam which penetrated the object at a focusing

position on the beam propagation path after penetrating the vibration region and the aperture; and

an optical imaging device, set at the focusing position to receive the laser beam so as to generate a plurality of scanning optically-sectioned images with respective to the scanning imaging positions and process the scanning optically-sectioned images as 2D elasticity images and combine the 2D elasticity images to build a 3D elasticity image, wherein at least one of the scanning optically-sectioned images shows the at least one speckle pattern;

wherein the optical imaging device comprises an optical lens, an optical sensing unit and an image processor; and

wherein a scanning gap is located between the neighboring scanning imaging positions, the aperture of the optical focusing device is set with a plurality of hole diameters, and the scanning gap is adjusted according to the hole diameters.

2. The imaging system of claim 1, further comprising a beam expansion device, which is located on the beam propagation path between the translational stage and the laser generating device, for expanding illumination region of the laser beam.

3. The imaging system of claim 2, wherein the beam expansion device is a combination of a concave lens and a convex lens.

4. The imaging system of claim 1, wherein the optical focusing device comprises:

- an aperture stop, containing an aperture that partially allows the laser beam to pass; and
- at least two lenses, located on the beam propagation path of the two sides of the aperture stop, for adjusting the focusing position.

* * * * *

专利名称(译)	用于产生由超声波引起的振动区域从而获得光学截面图像的成像系统		
公开(公告)号	US10184826	公开(公告)日	2019-01-22
申请号	US15/642022	申请日	2017-07-05
[标]申请(专利权)人(译)	国立台湾大学		
申请(专利权)人(译)	国立台湾大学		
当前申请(专利权)人(译)	国立台湾大学		
[标]发明人	LI PAI CHI CHAO PEI YU		
发明人	LI, PAI-CHI CHAO, PEI-YU		
IPC分类号	G01H9/00 A61B8/08 A61B8/00 A61B5/00 G01N21/49 G01N21/47 G01N29/00 G01N21/17 G01N21/45		
CPC分类号	G01H9/008 A61B5/0082 A61B5/0097 A61B8/4444 A61B8/485 G01N21/45 G01N21/4795 G01N21/49 G01N29/00 G01N21/1717 G01N2021/479 G01N29/2418		
优先权	106105747 2017-02-21 TW		
其他公开文献	US20180235474A1		
外部链接	Espacenet		

摘要(译)

成像系统被配置用于产生由超声波引起的振动区域，从而获得多个光学截面图像。在成像系统中，台可操作以沿多个扫描成像位置移动，并施加以用至少一种散射材料沉积物体。当物体接收超声波时，产生剪切波以移动散射材料从而形成振动区域。激光产生装置被配置为透射激光束，该激光束穿透振动区域以形成散斑图案并聚焦在聚焦位置。将光学成像装置设置在聚焦位置以接收激光束，以产生相对于扫描成像位置的多个扫描光学截面图像。

